



US00D638545S

(12) **United States Design Patent**
Okawa et al.

(10) **Patent No.:** **US D638,545 S**
(45) **Date of Patent:** **** May 24, 2011**

(54) **MEDICAL IMMUNOASSAY DEVICE**

(75) Inventors: **Aya Okawa**, Tokyo (JP); **Makoto Isozaki**, Tokyo (JP)

(73) Assignee: **Fujifilm Corporation**, Tokyo (JP)

(**) Term: **14 Years**

(21) Appl. No.: **29/375,896**

(22) Filed: **Sep. 29, 2010**

(30) **Foreign Application Priority Data**

Mar. 31, 2010 (JP) 2010-008019

(51) **LOC (9) Cl.** **24-01**

(52) **U.S. Cl.** **D24/186**

(58) **Field of Classification Search** D10/81;
D24/107, 169, 185–186, 216, 232, 233; 73/864.01,
73/864.12; 134/21, 22.11, 24, 26–27, 169 R;
422/62–64, 99, 100; 436/47, 49, 179, 180;
600/300, 301, 368, 372, 481, 529, 544, 554,
600/561

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D330,596 S * 10/1992 Frenkel et al. D24/186
D334,237 S * 3/1993 Collister et al. D10/81
D339,636 S * 9/1993 Uchiyama D24/185
D381,756 S * 7/1997 Ohnuma et al. D24/231
D400,673 S * 11/1998 Kheiri et al. D24/107
D404,140 S * 1/1999 Meguro D24/232

D406,901 S * 3/1999 Ditterline et al. D24/231
D467,349 S * 12/2002 Niedbala et al. D24/232
D471,642 S * 3/2003 Alden et al. D24/232
D491,272 S * 6/2004 Alden et al. D24/216
D527,464 S * 8/2006 Ina et al. D24/232
D535,403 S * 1/2007 Isozaki et al. D24/232
D573,051 S * 7/2008 Alden et al. D10/81
D588,276 S * 3/2009 Isozaki et al. D24/232
D607,569 S * 1/2010 Yukikado et al. D24/186

* cited by examiner

Primary Examiner — T. Chase Nelson

Assistant Examiner — Mark Cavanna

(74) *Attorney, Agent, or Firm* — Young & Thompson

(57) **CLAIM**

The ornamental design for a medical immunoassay device, as shown and described.

DESCRIPTION

FIG. 1 is a top, front and side perspective view of a medical immunoassay device showing our new design;

FIG. 2 is a front elevational view thereof;

FIG. 3 is a rear elevational view thereof;

FIG. 4 is a top plan view thereof;

FIG. 5 is a bottom plan view thereof;



FIG. 6 is a left side elevational view thereof;

FIG. 7 is a right side elevational view thereof; and,

FIG. 8 is a top, front and side perspective view thereof, with a cover in an opened position.

The broken lines are included for the purpose of illustrating portions of the medical immunoassay device that form no part of the claimed design.

1 Claim, 6 Drawing Sheets

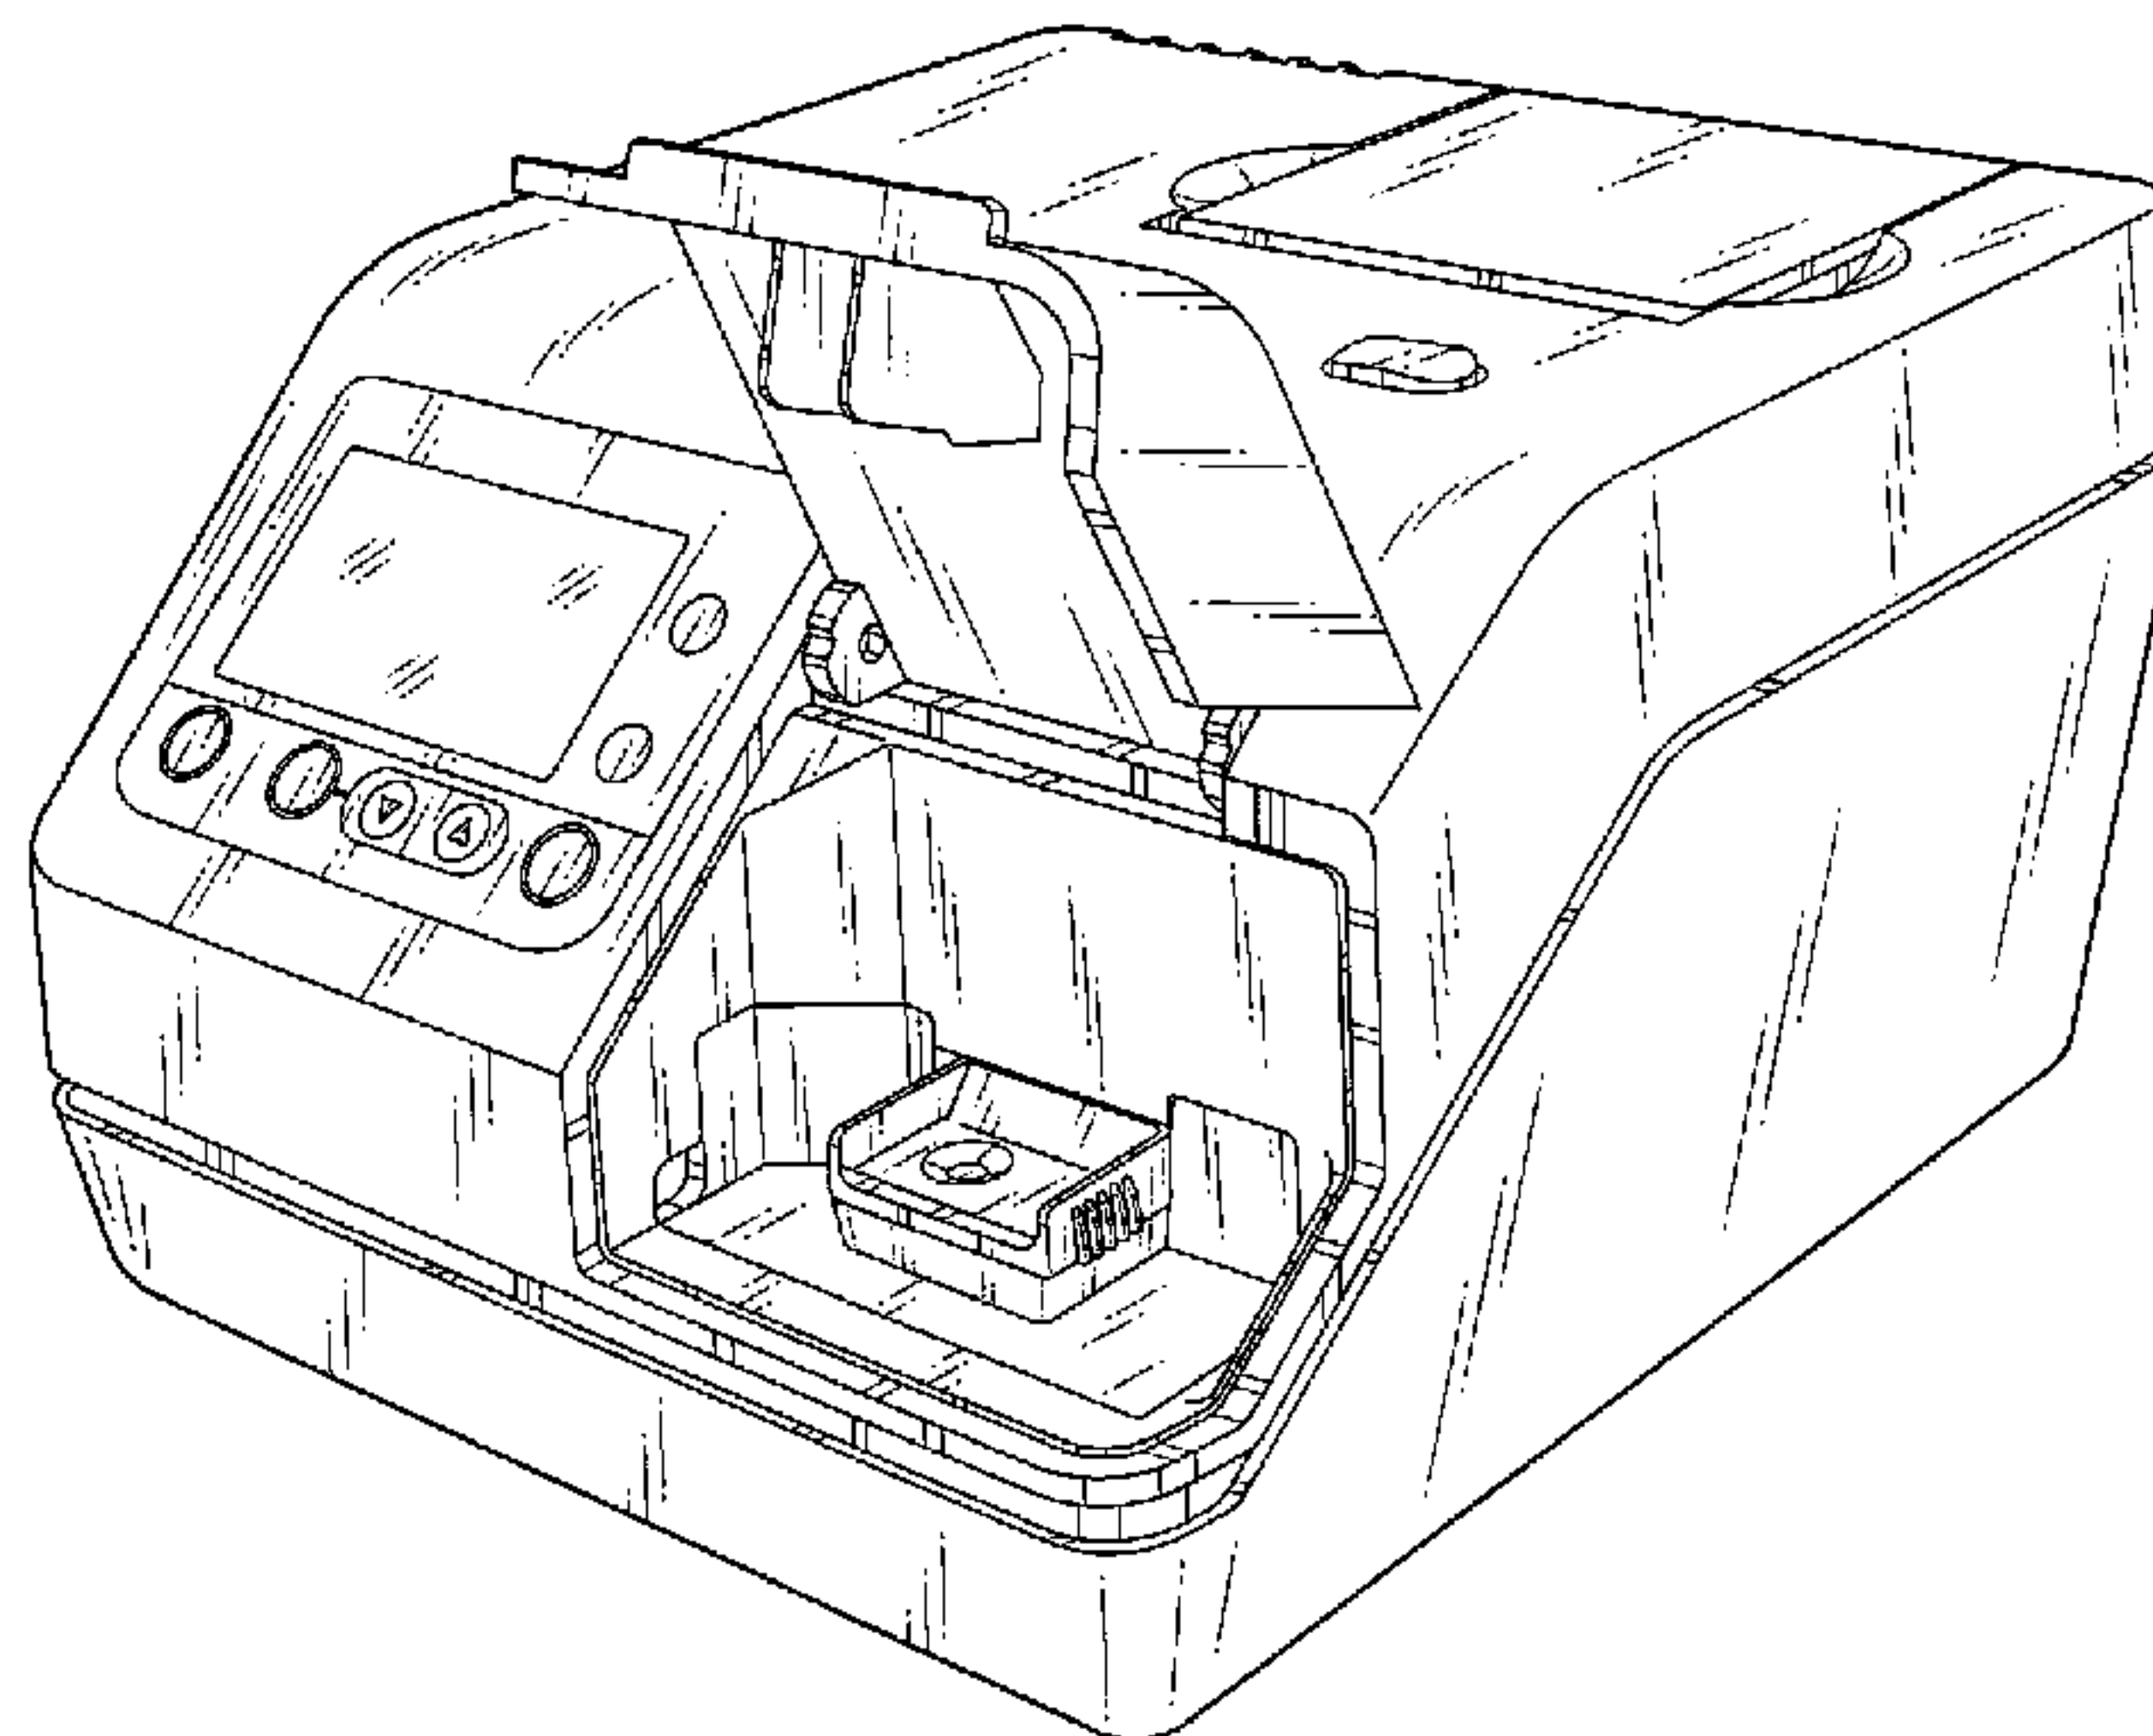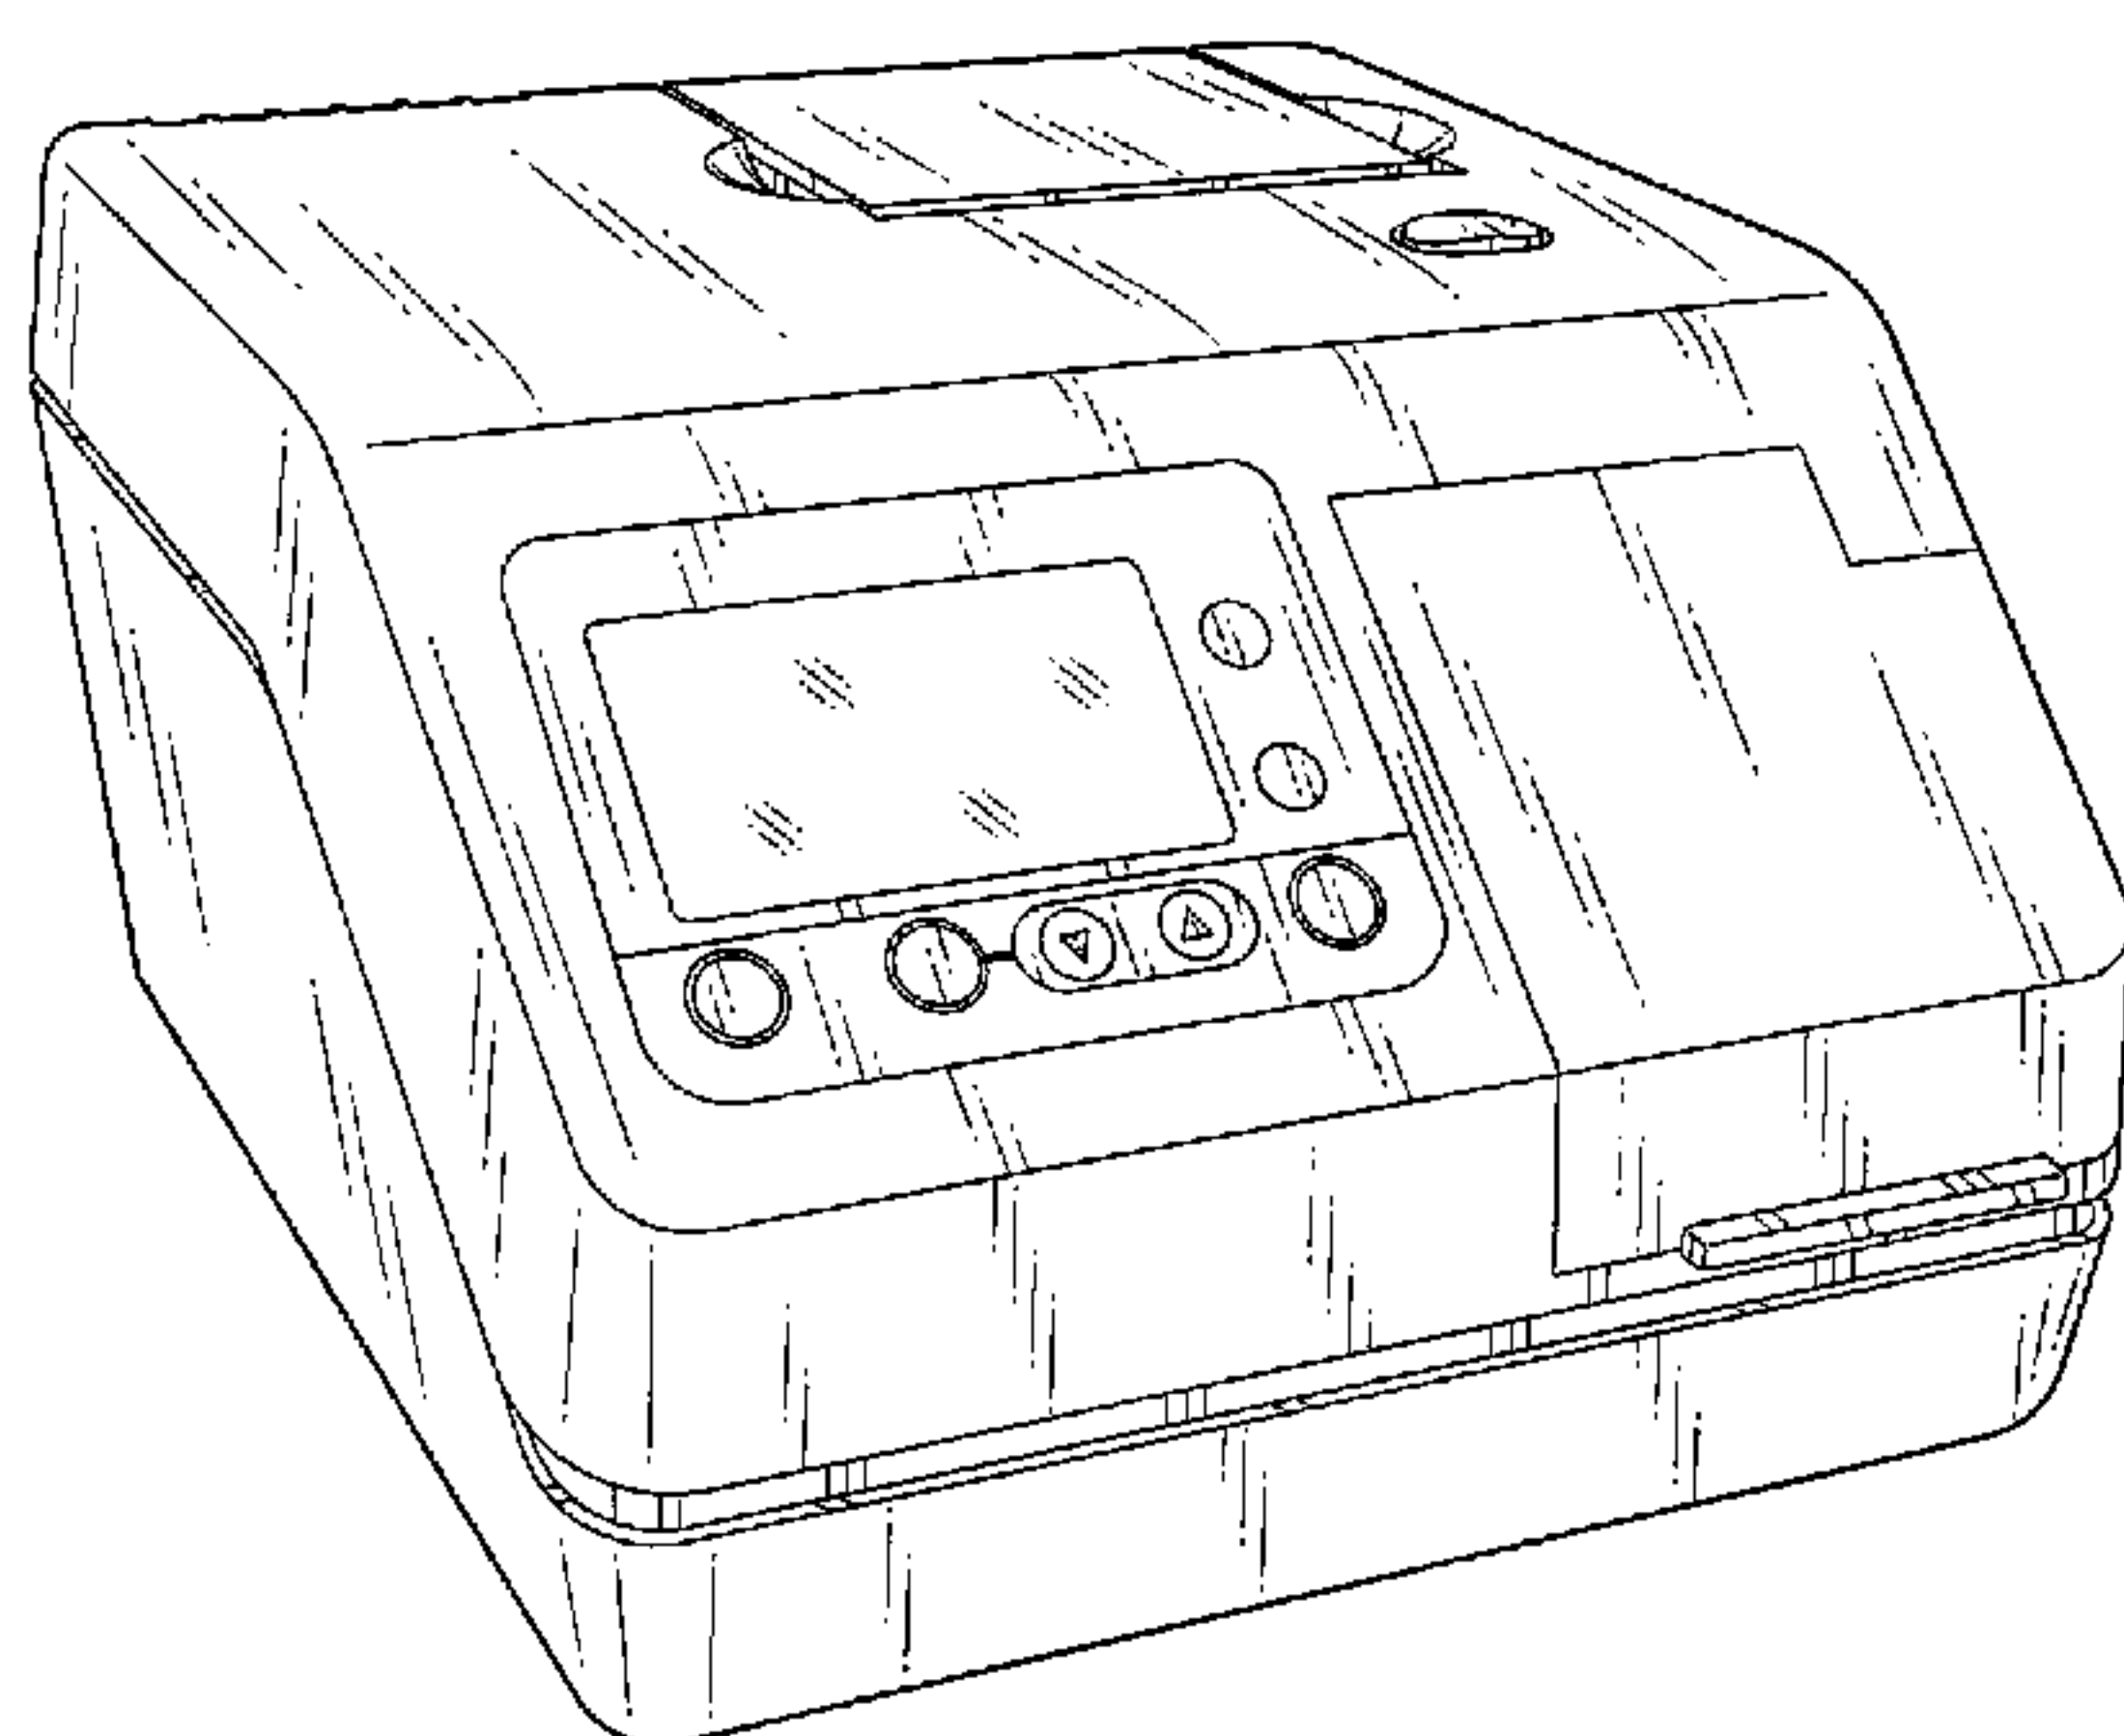

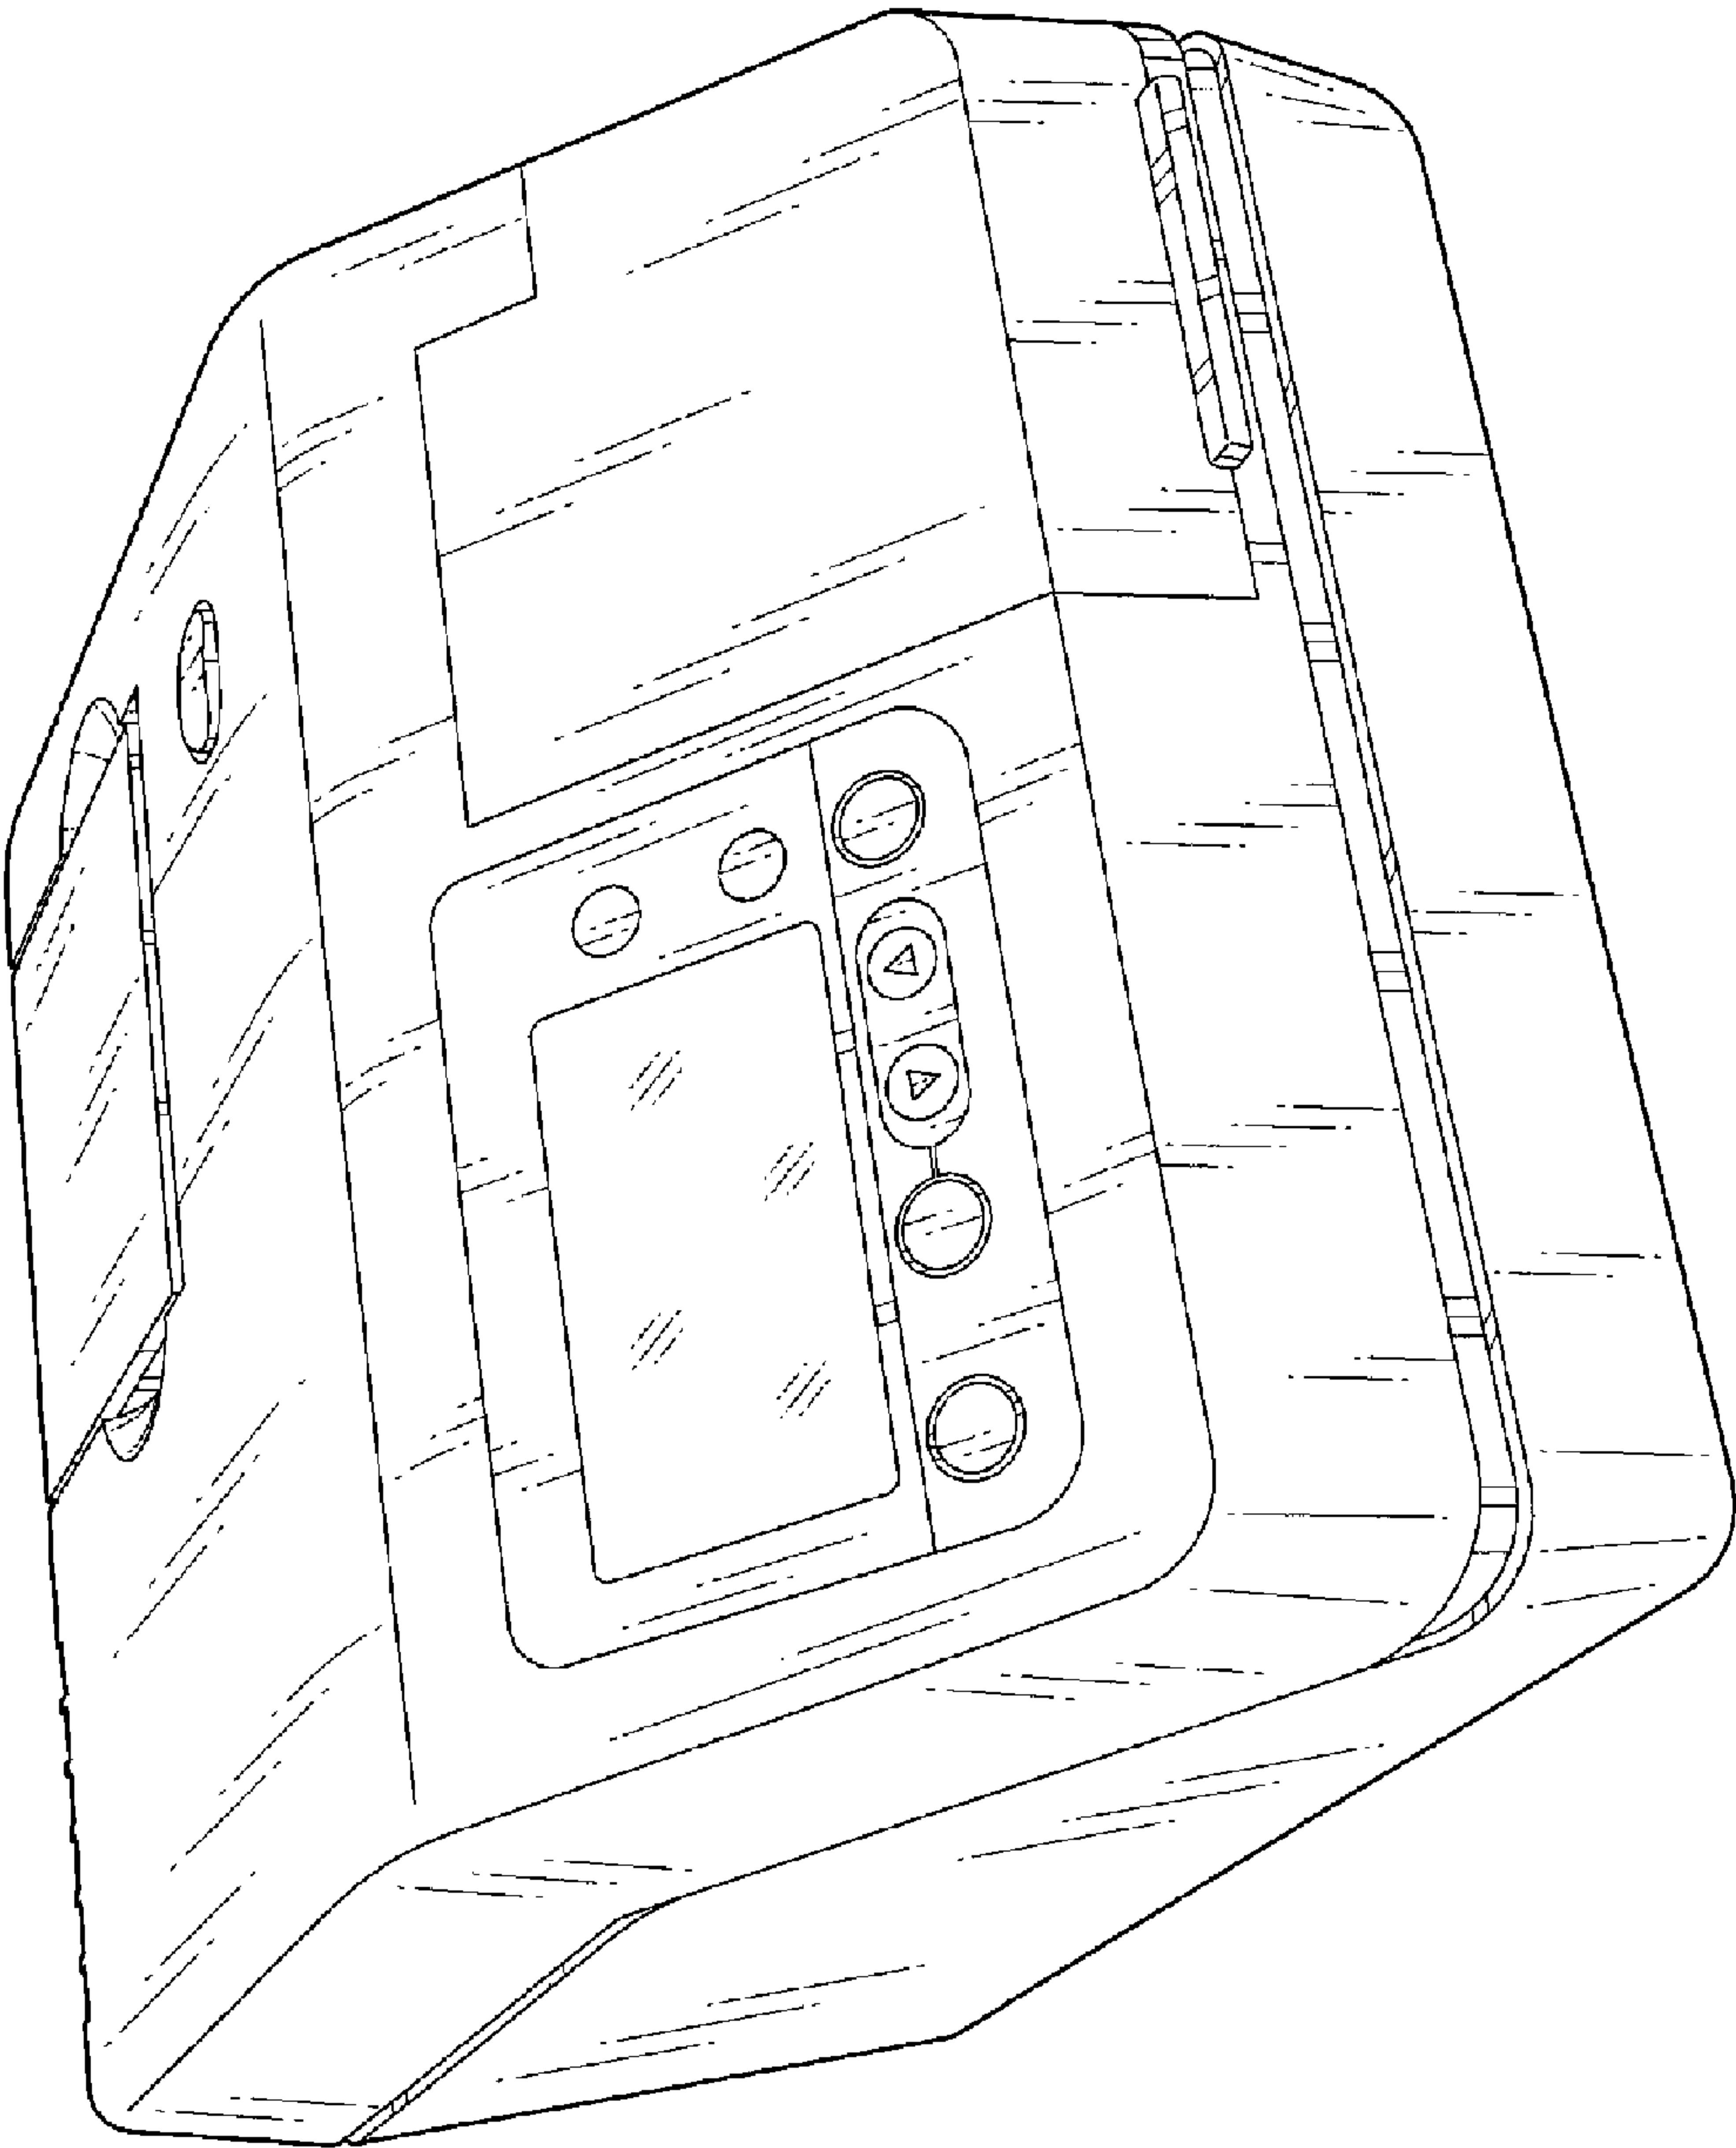


FIG.1

FIG.2

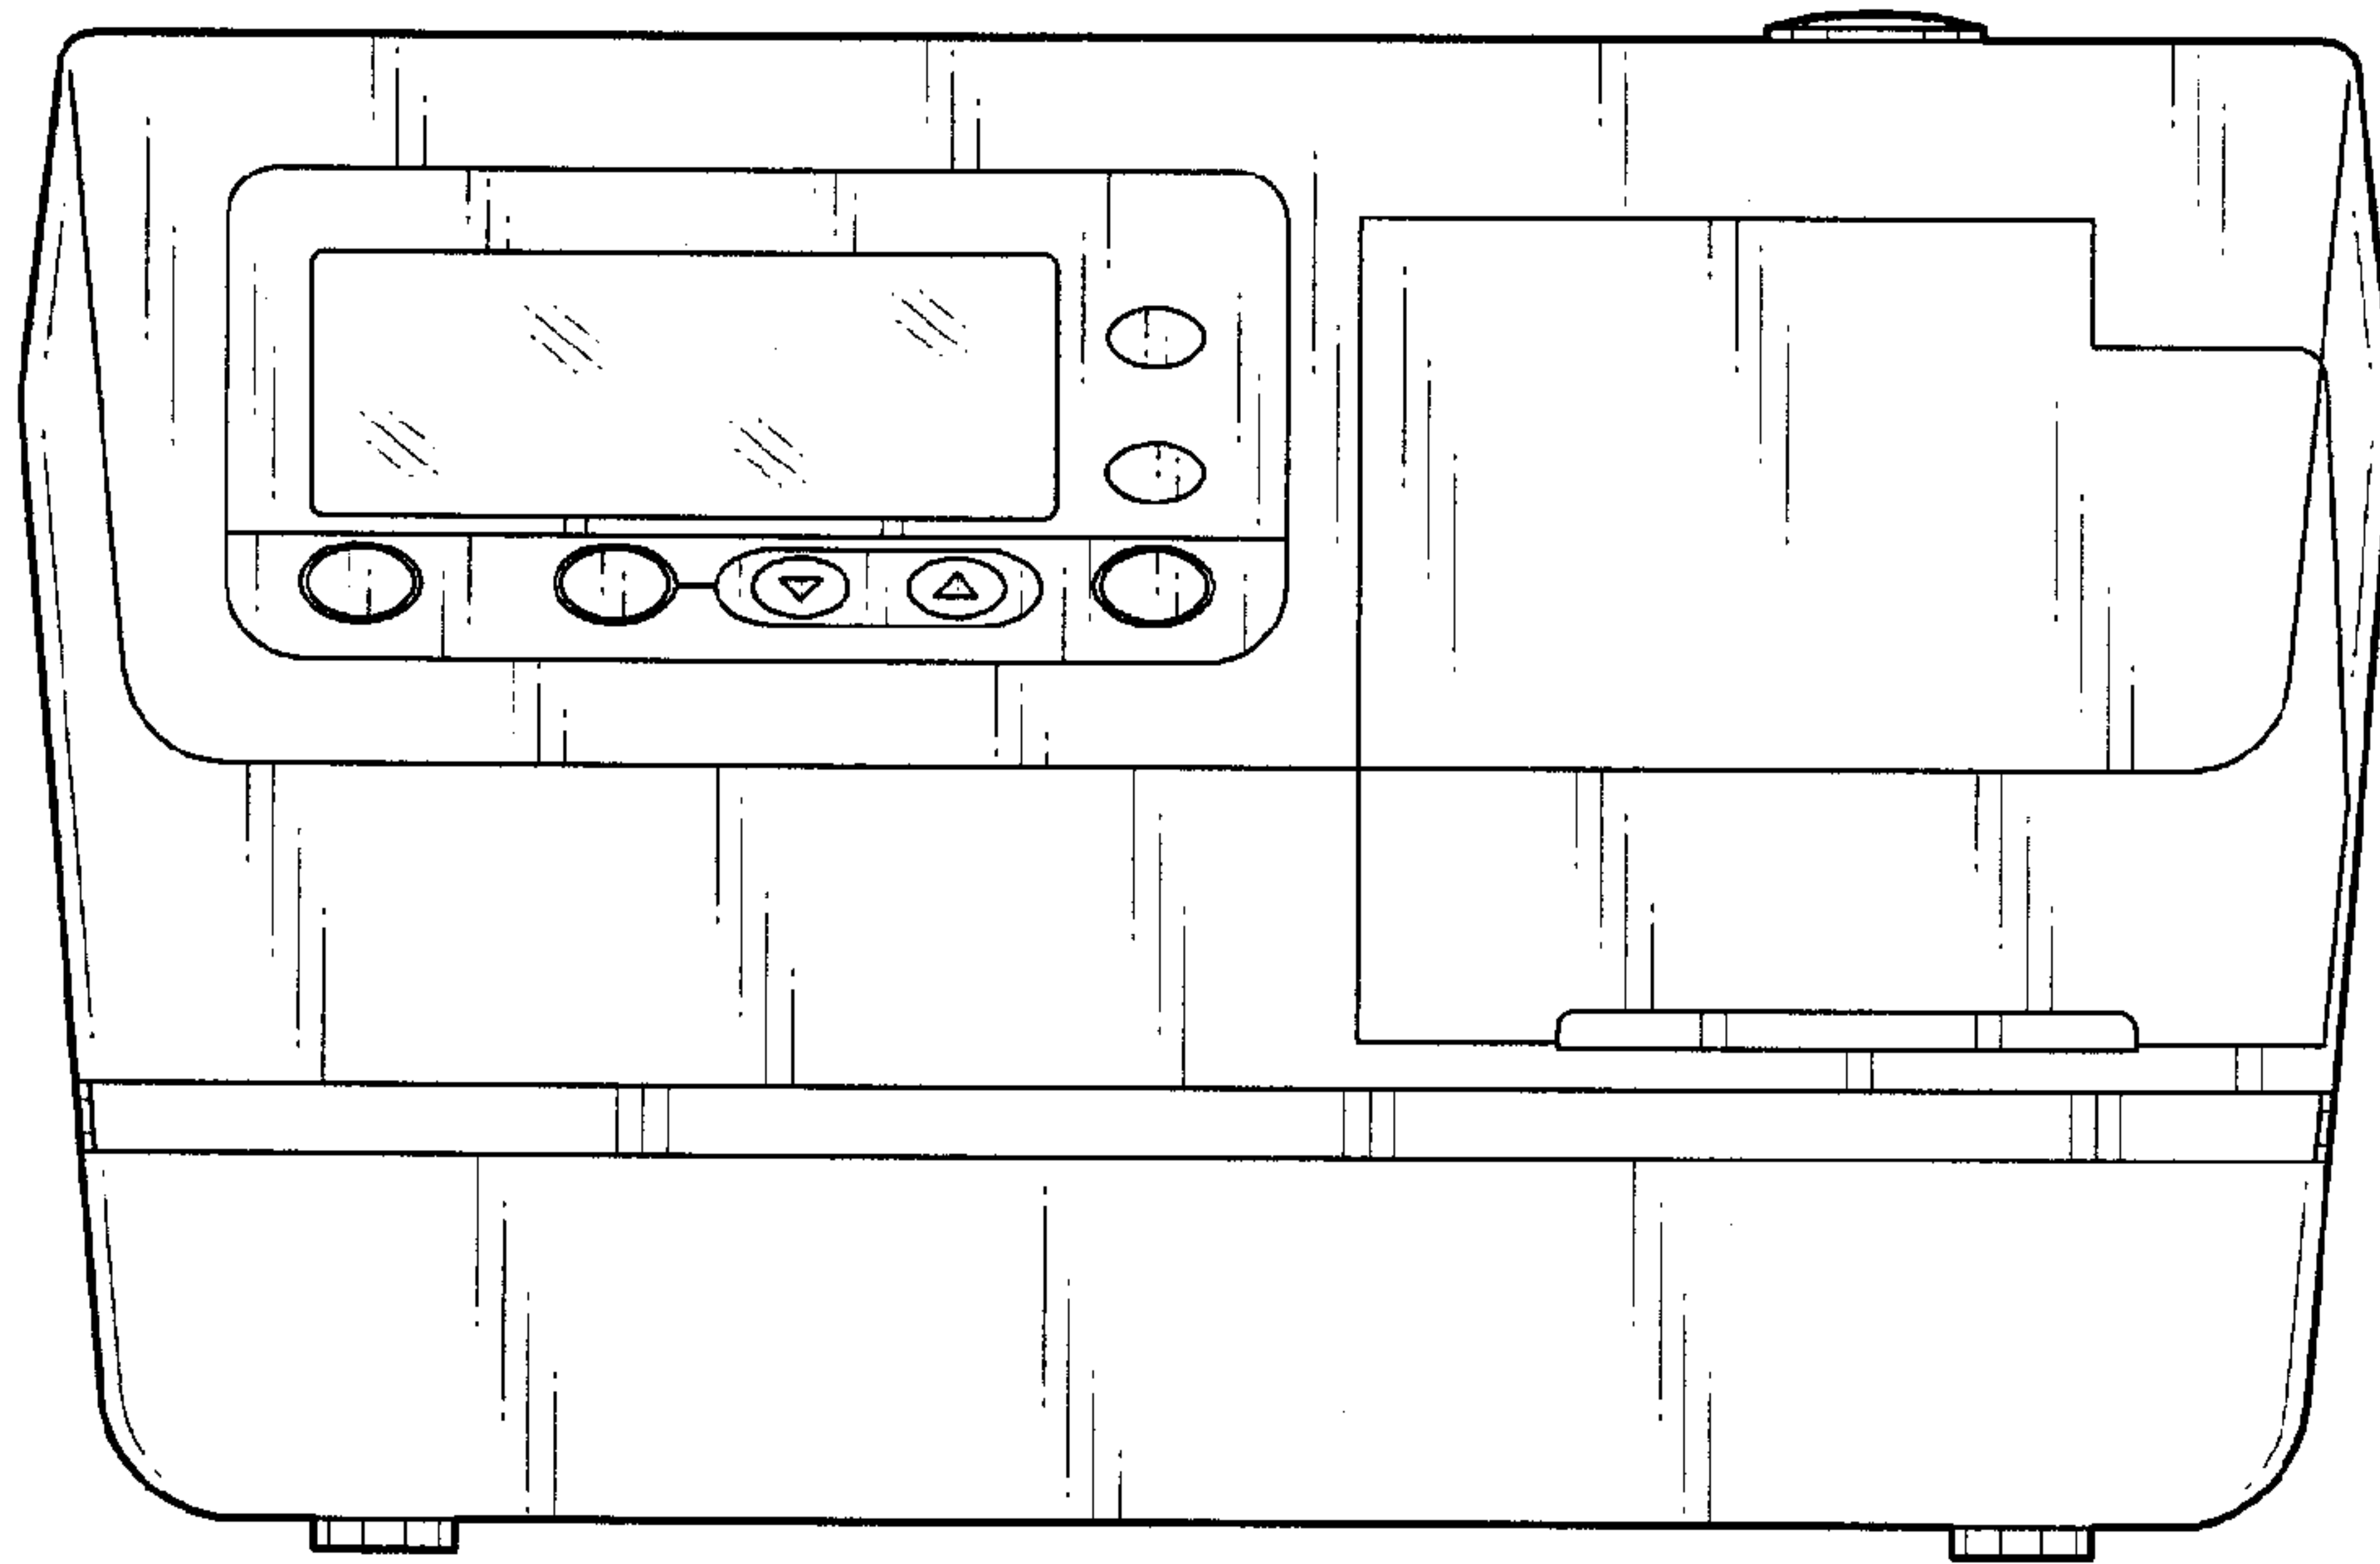


FIG.3

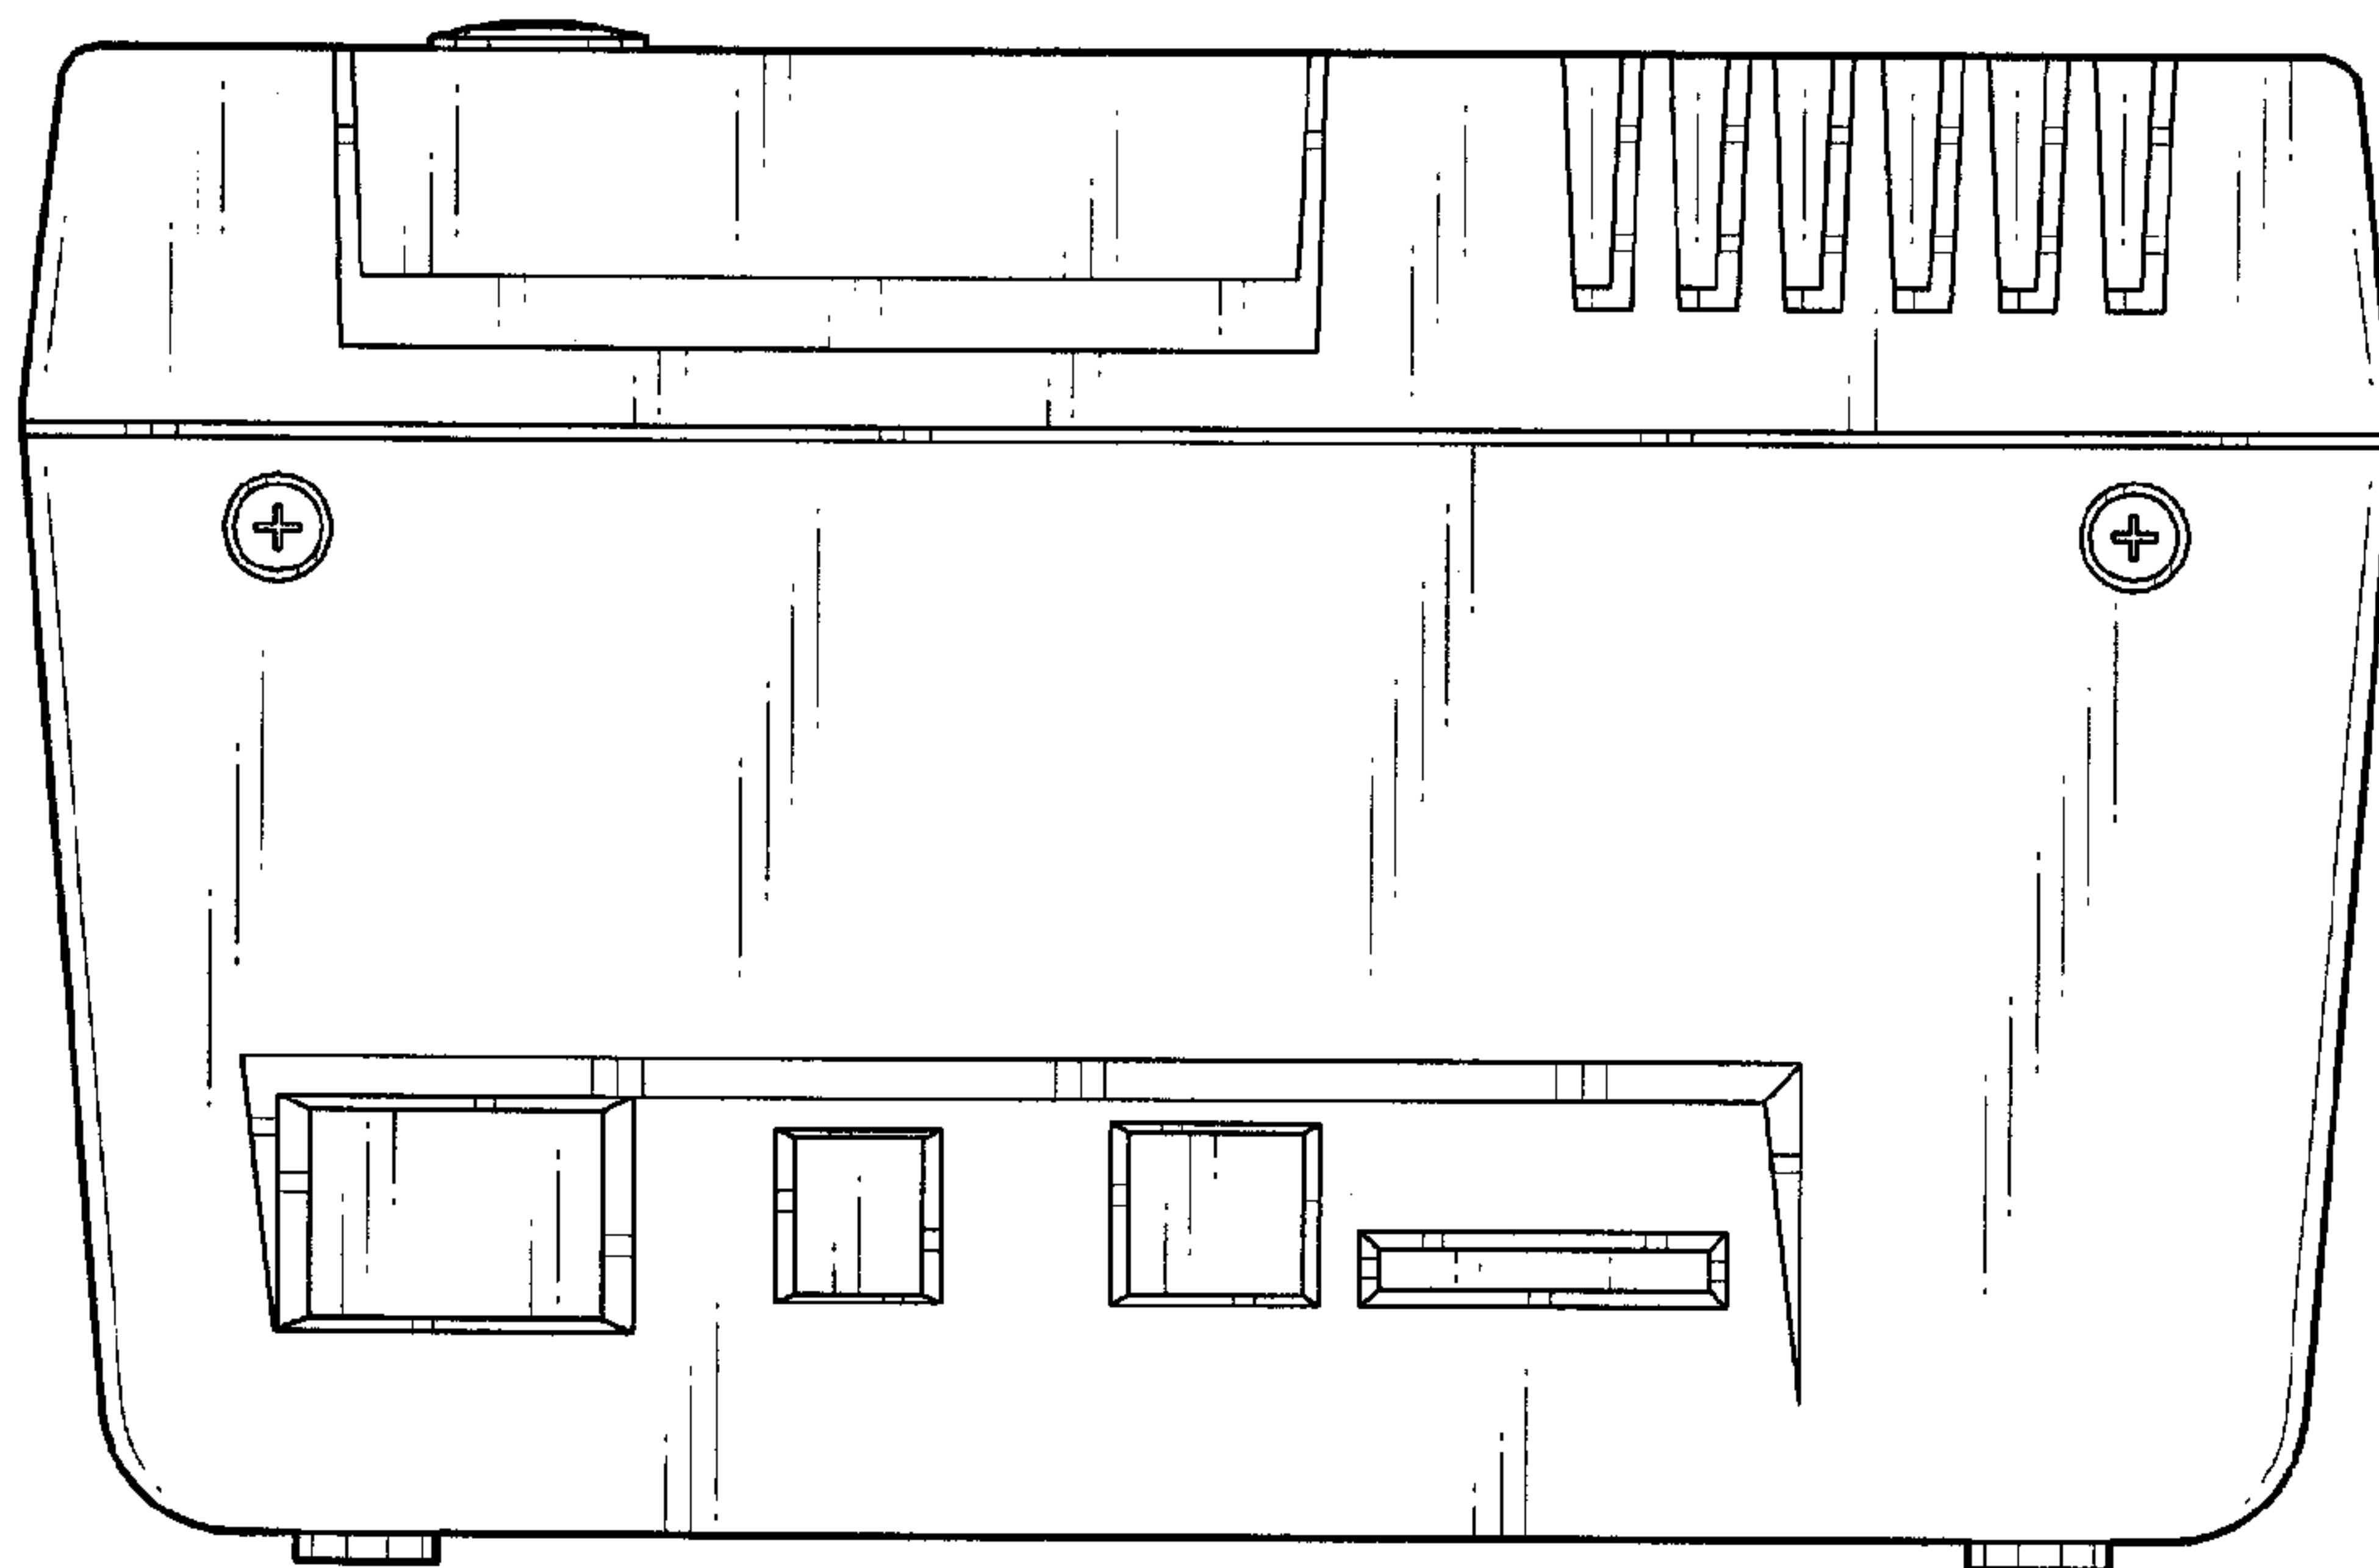


FIG.4

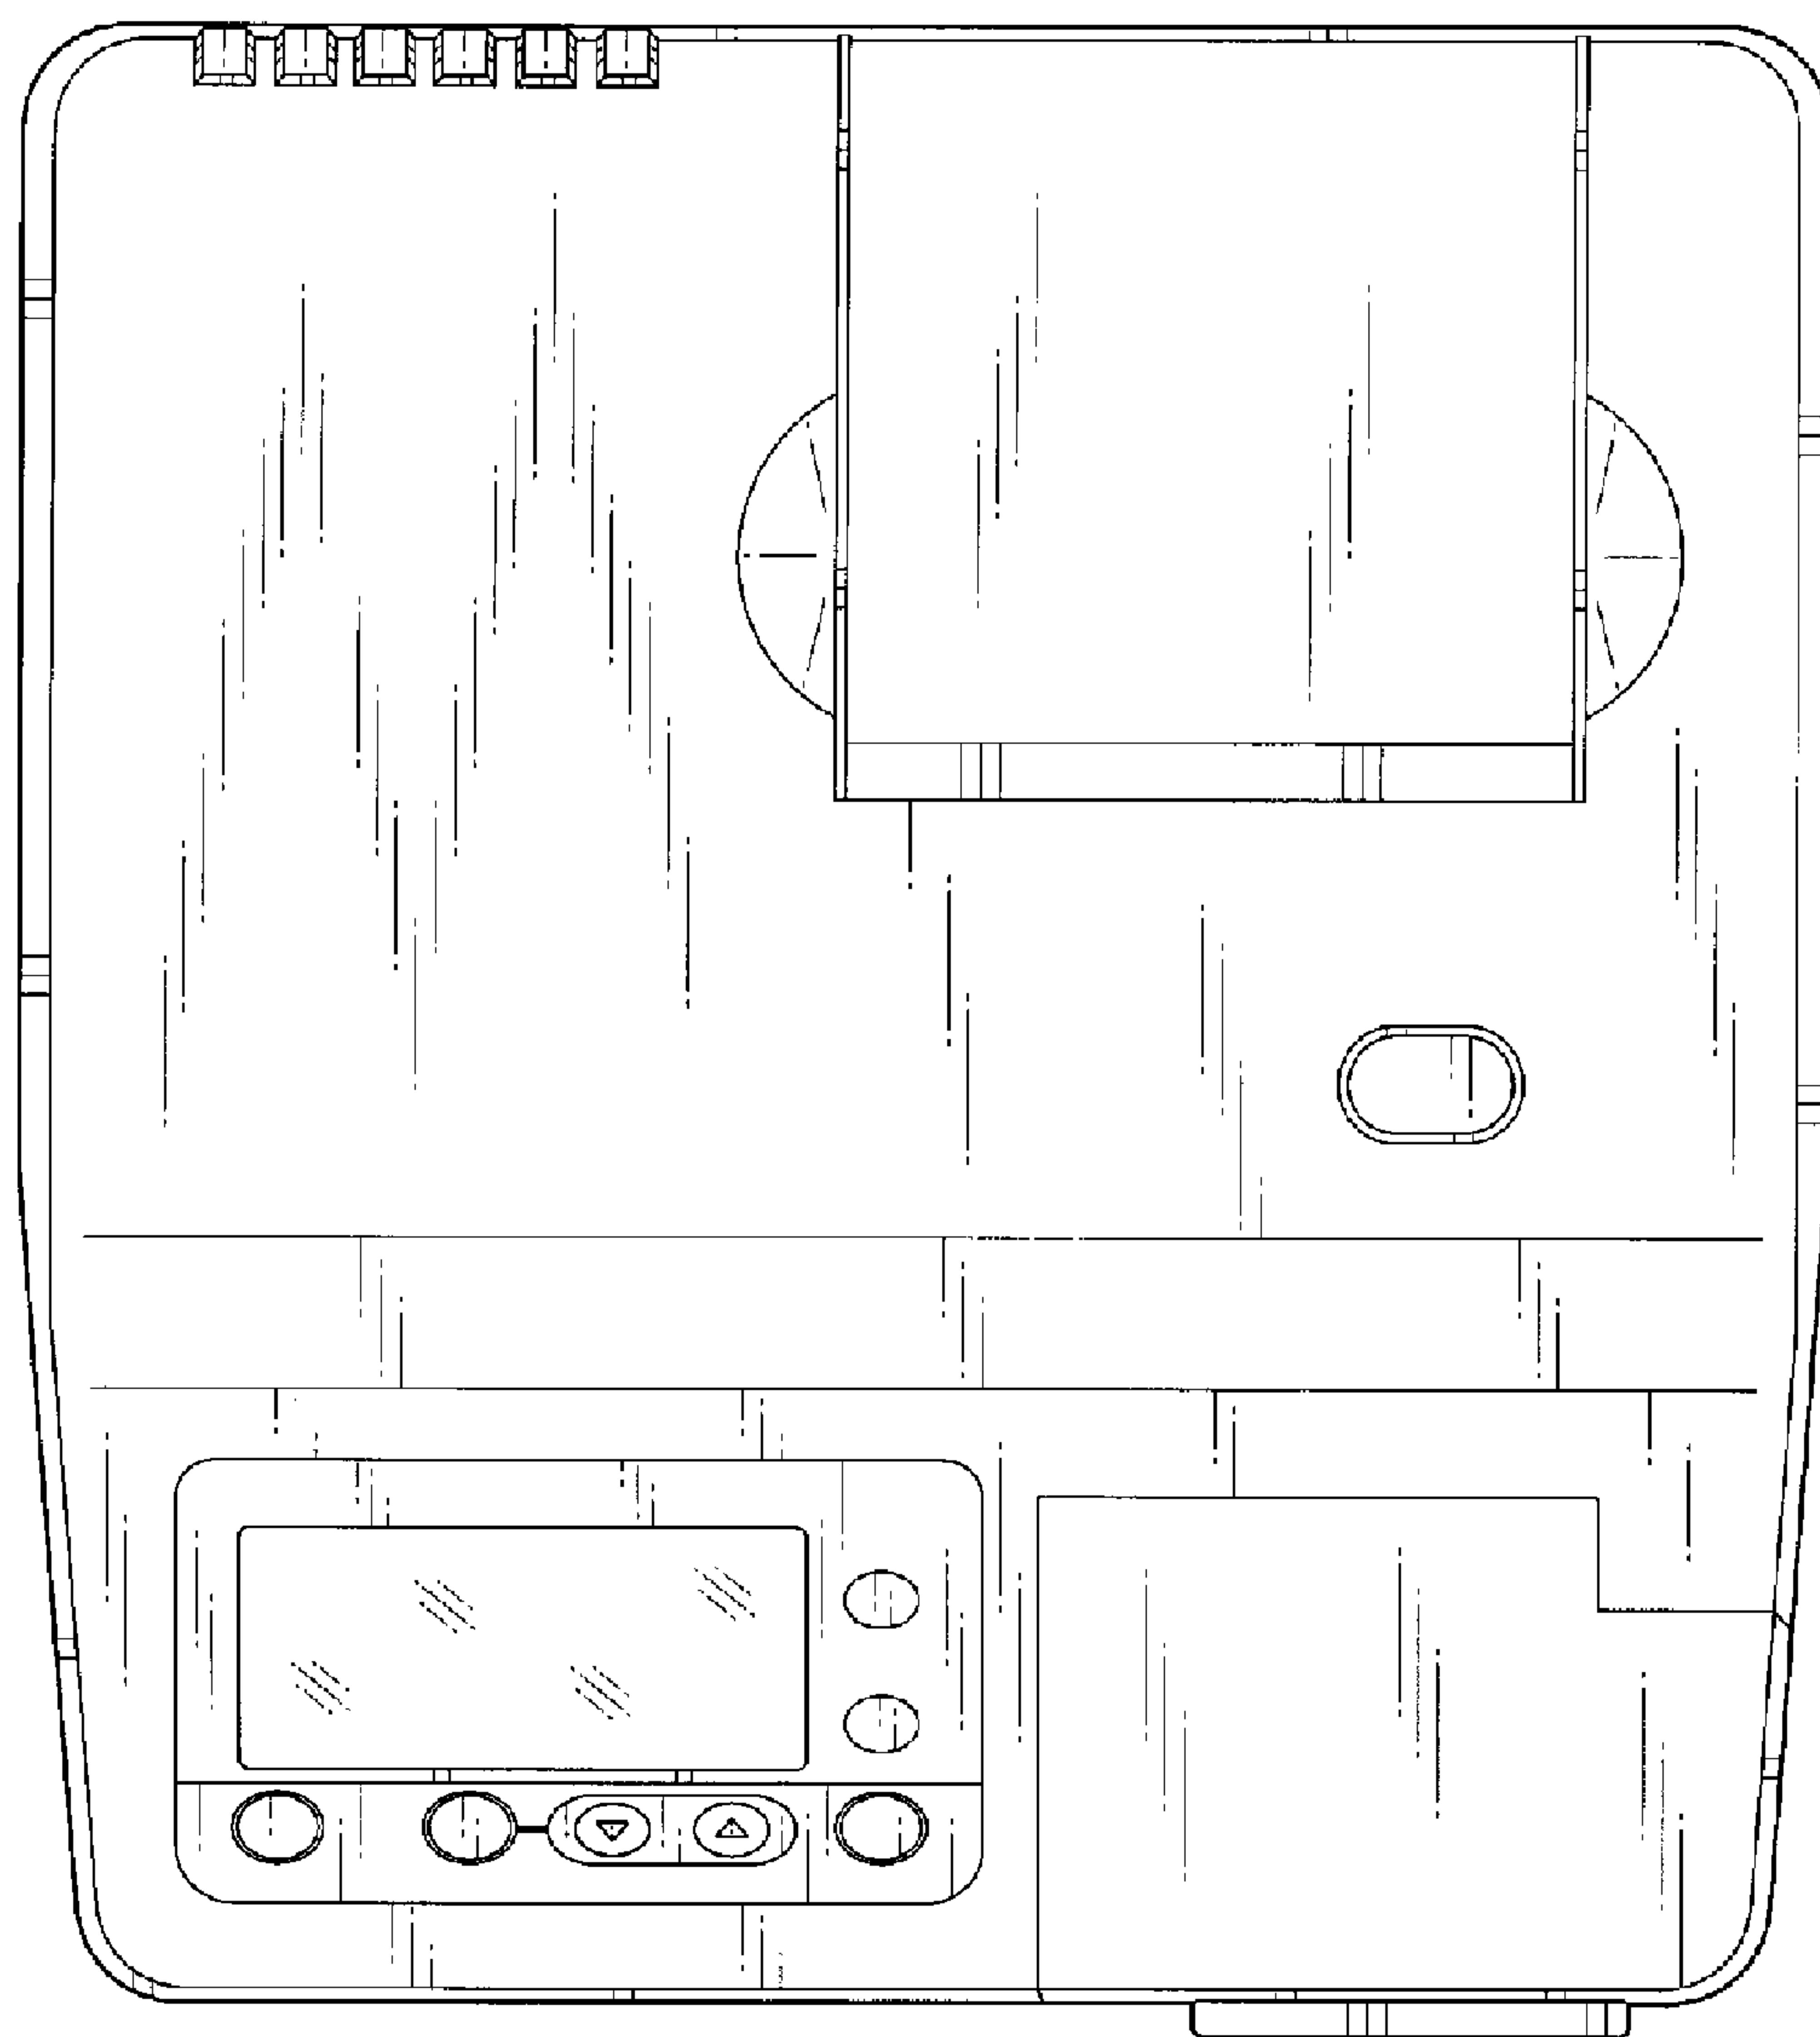


FIG.5

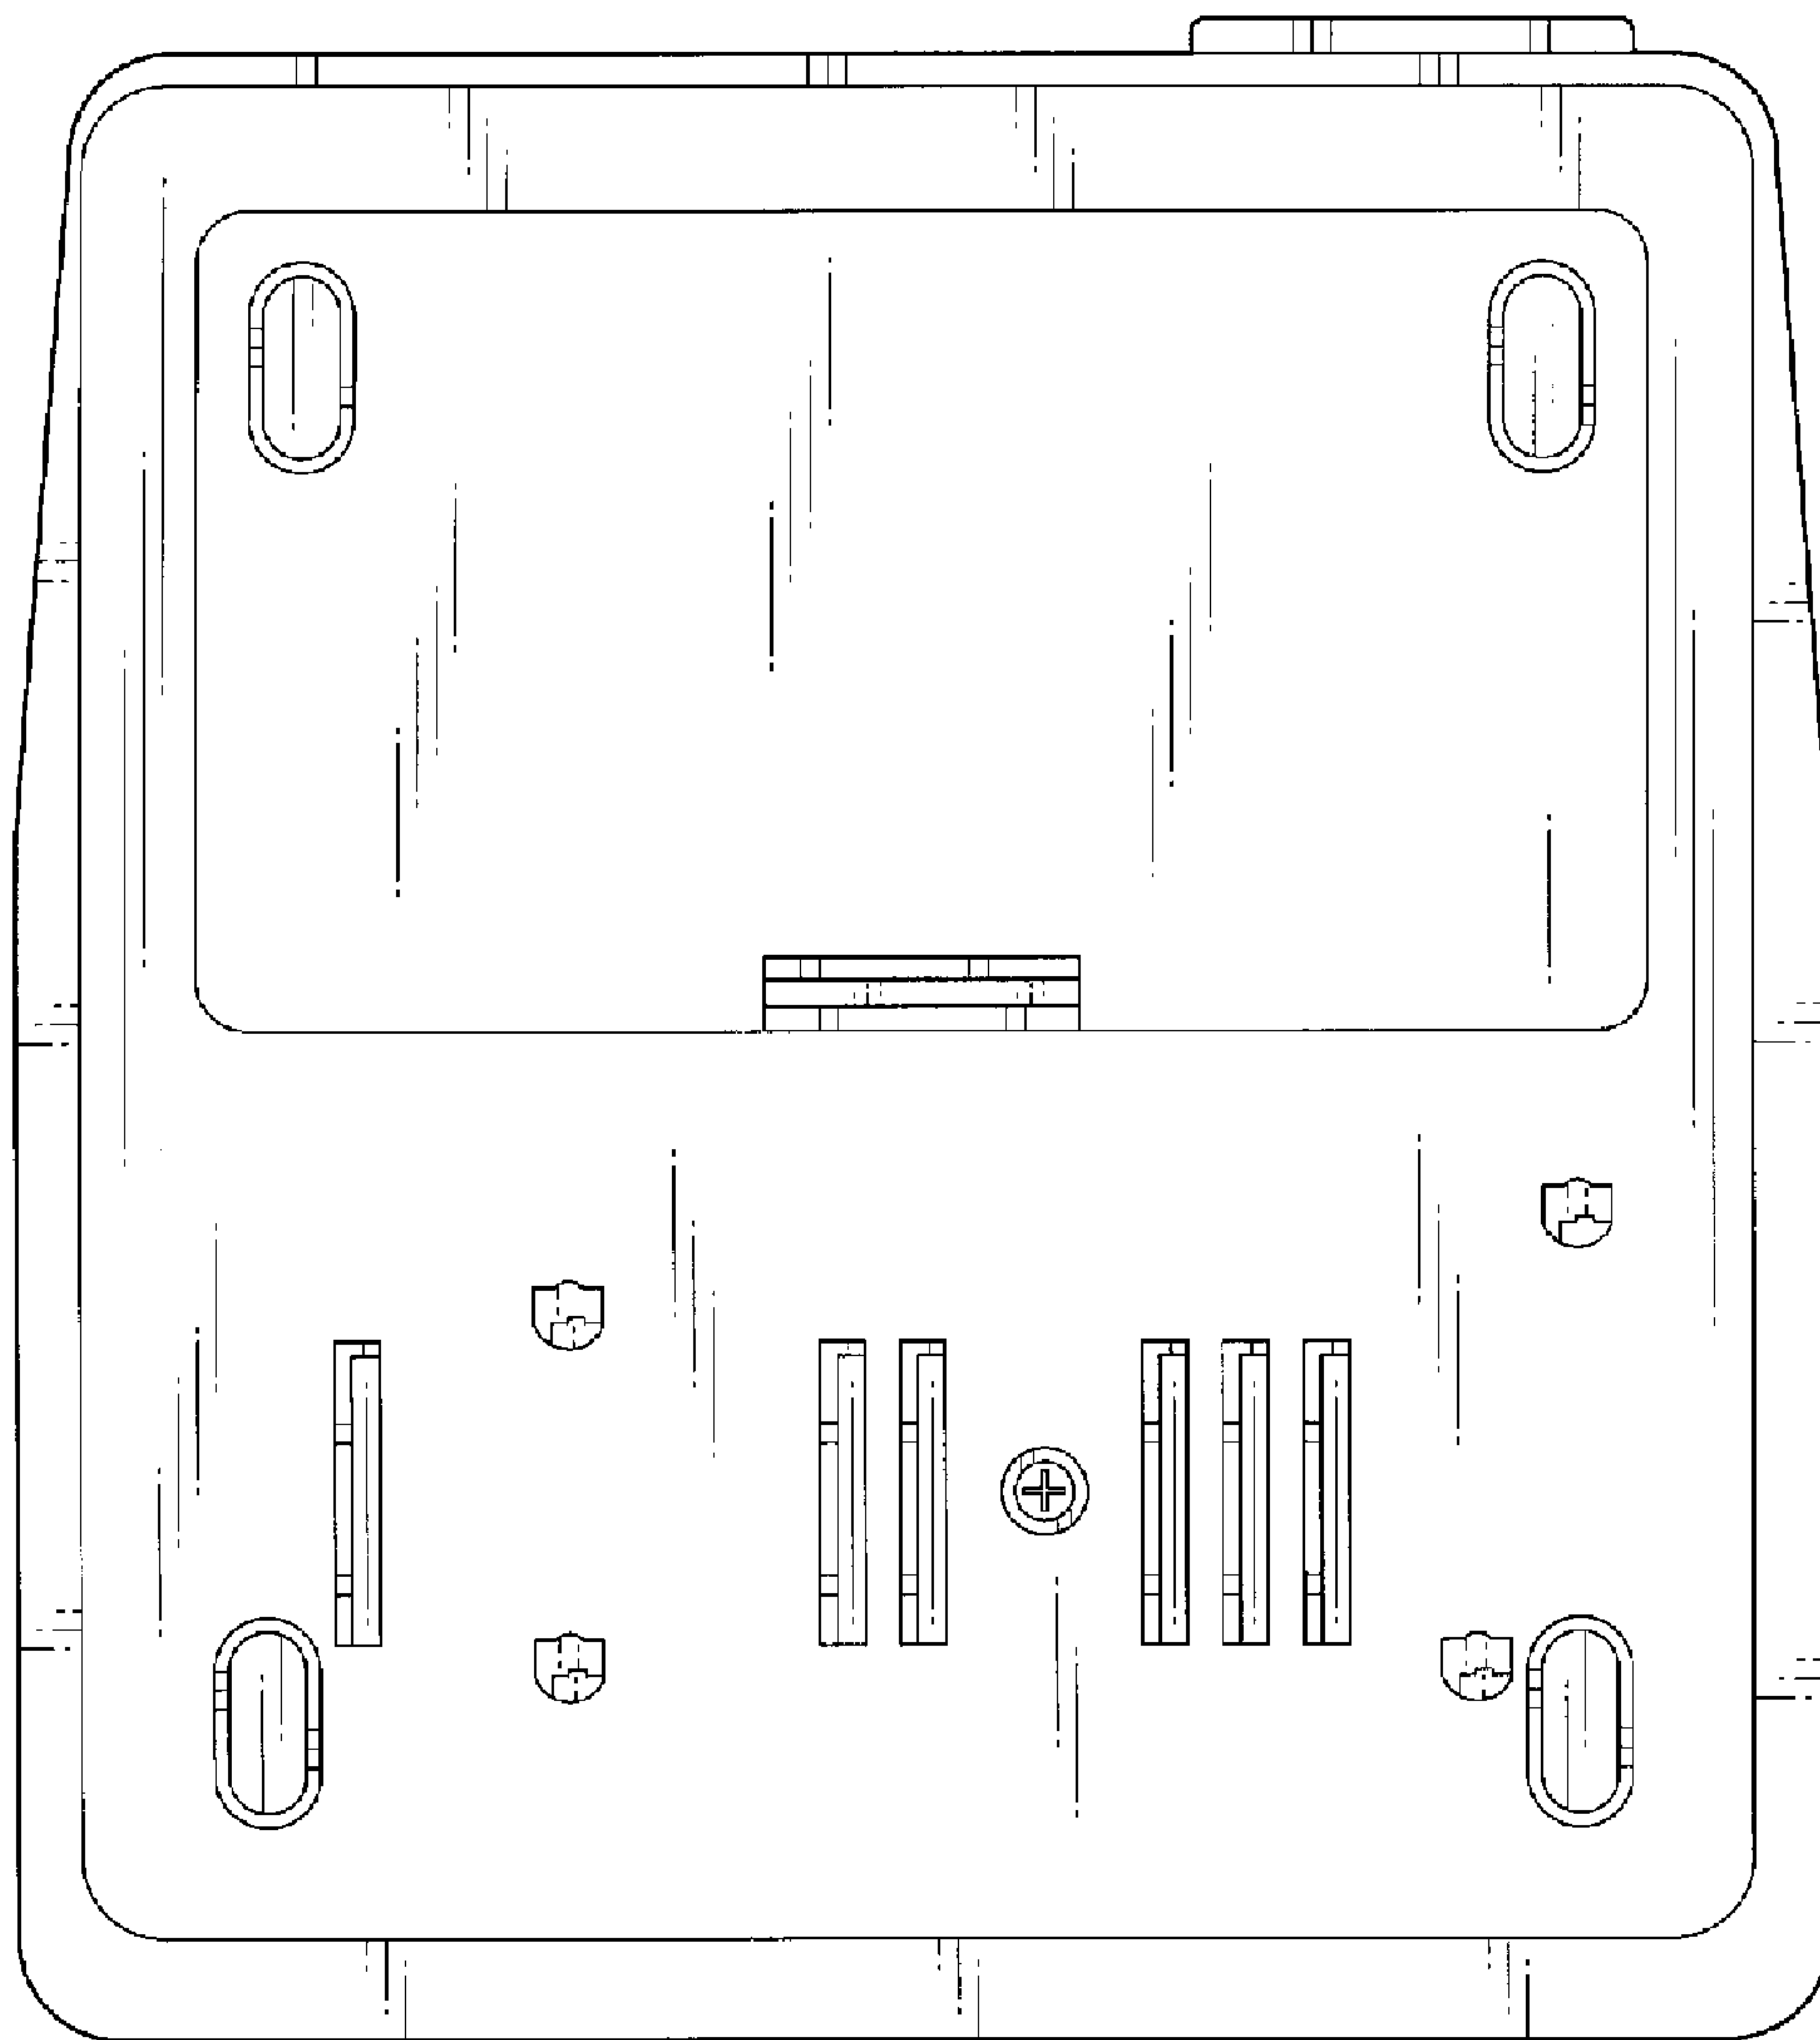


FIG.6

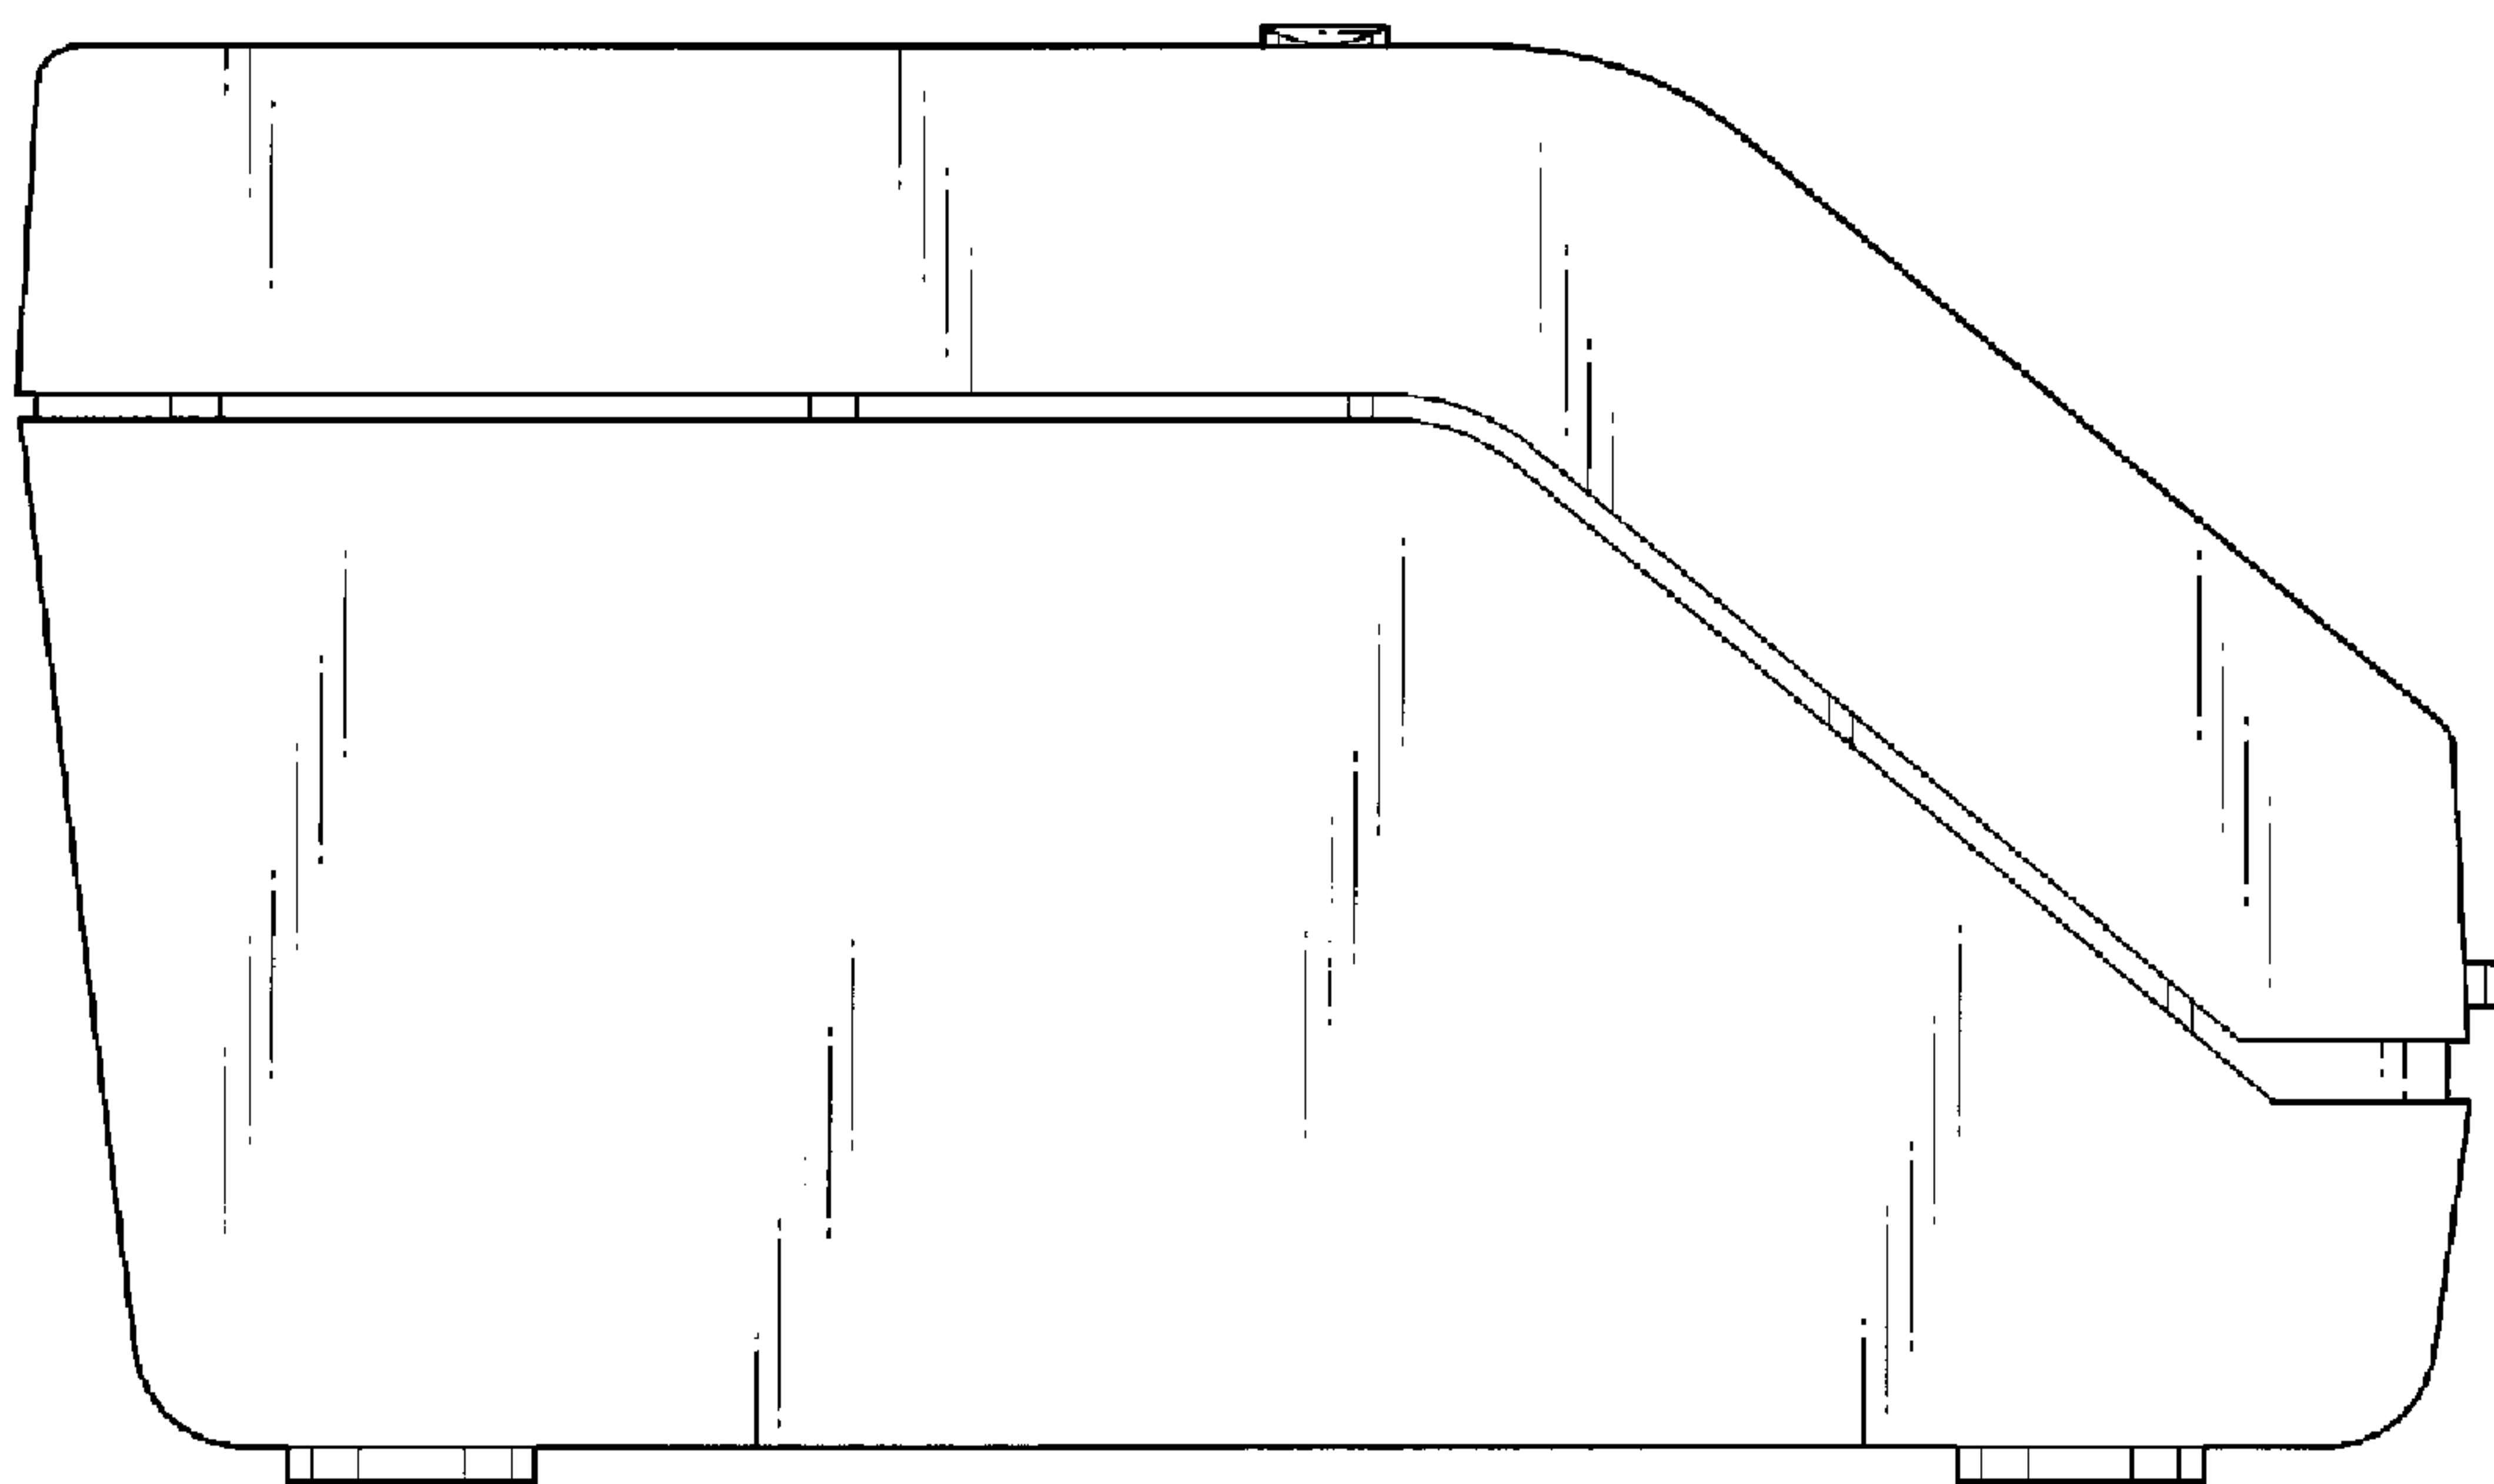
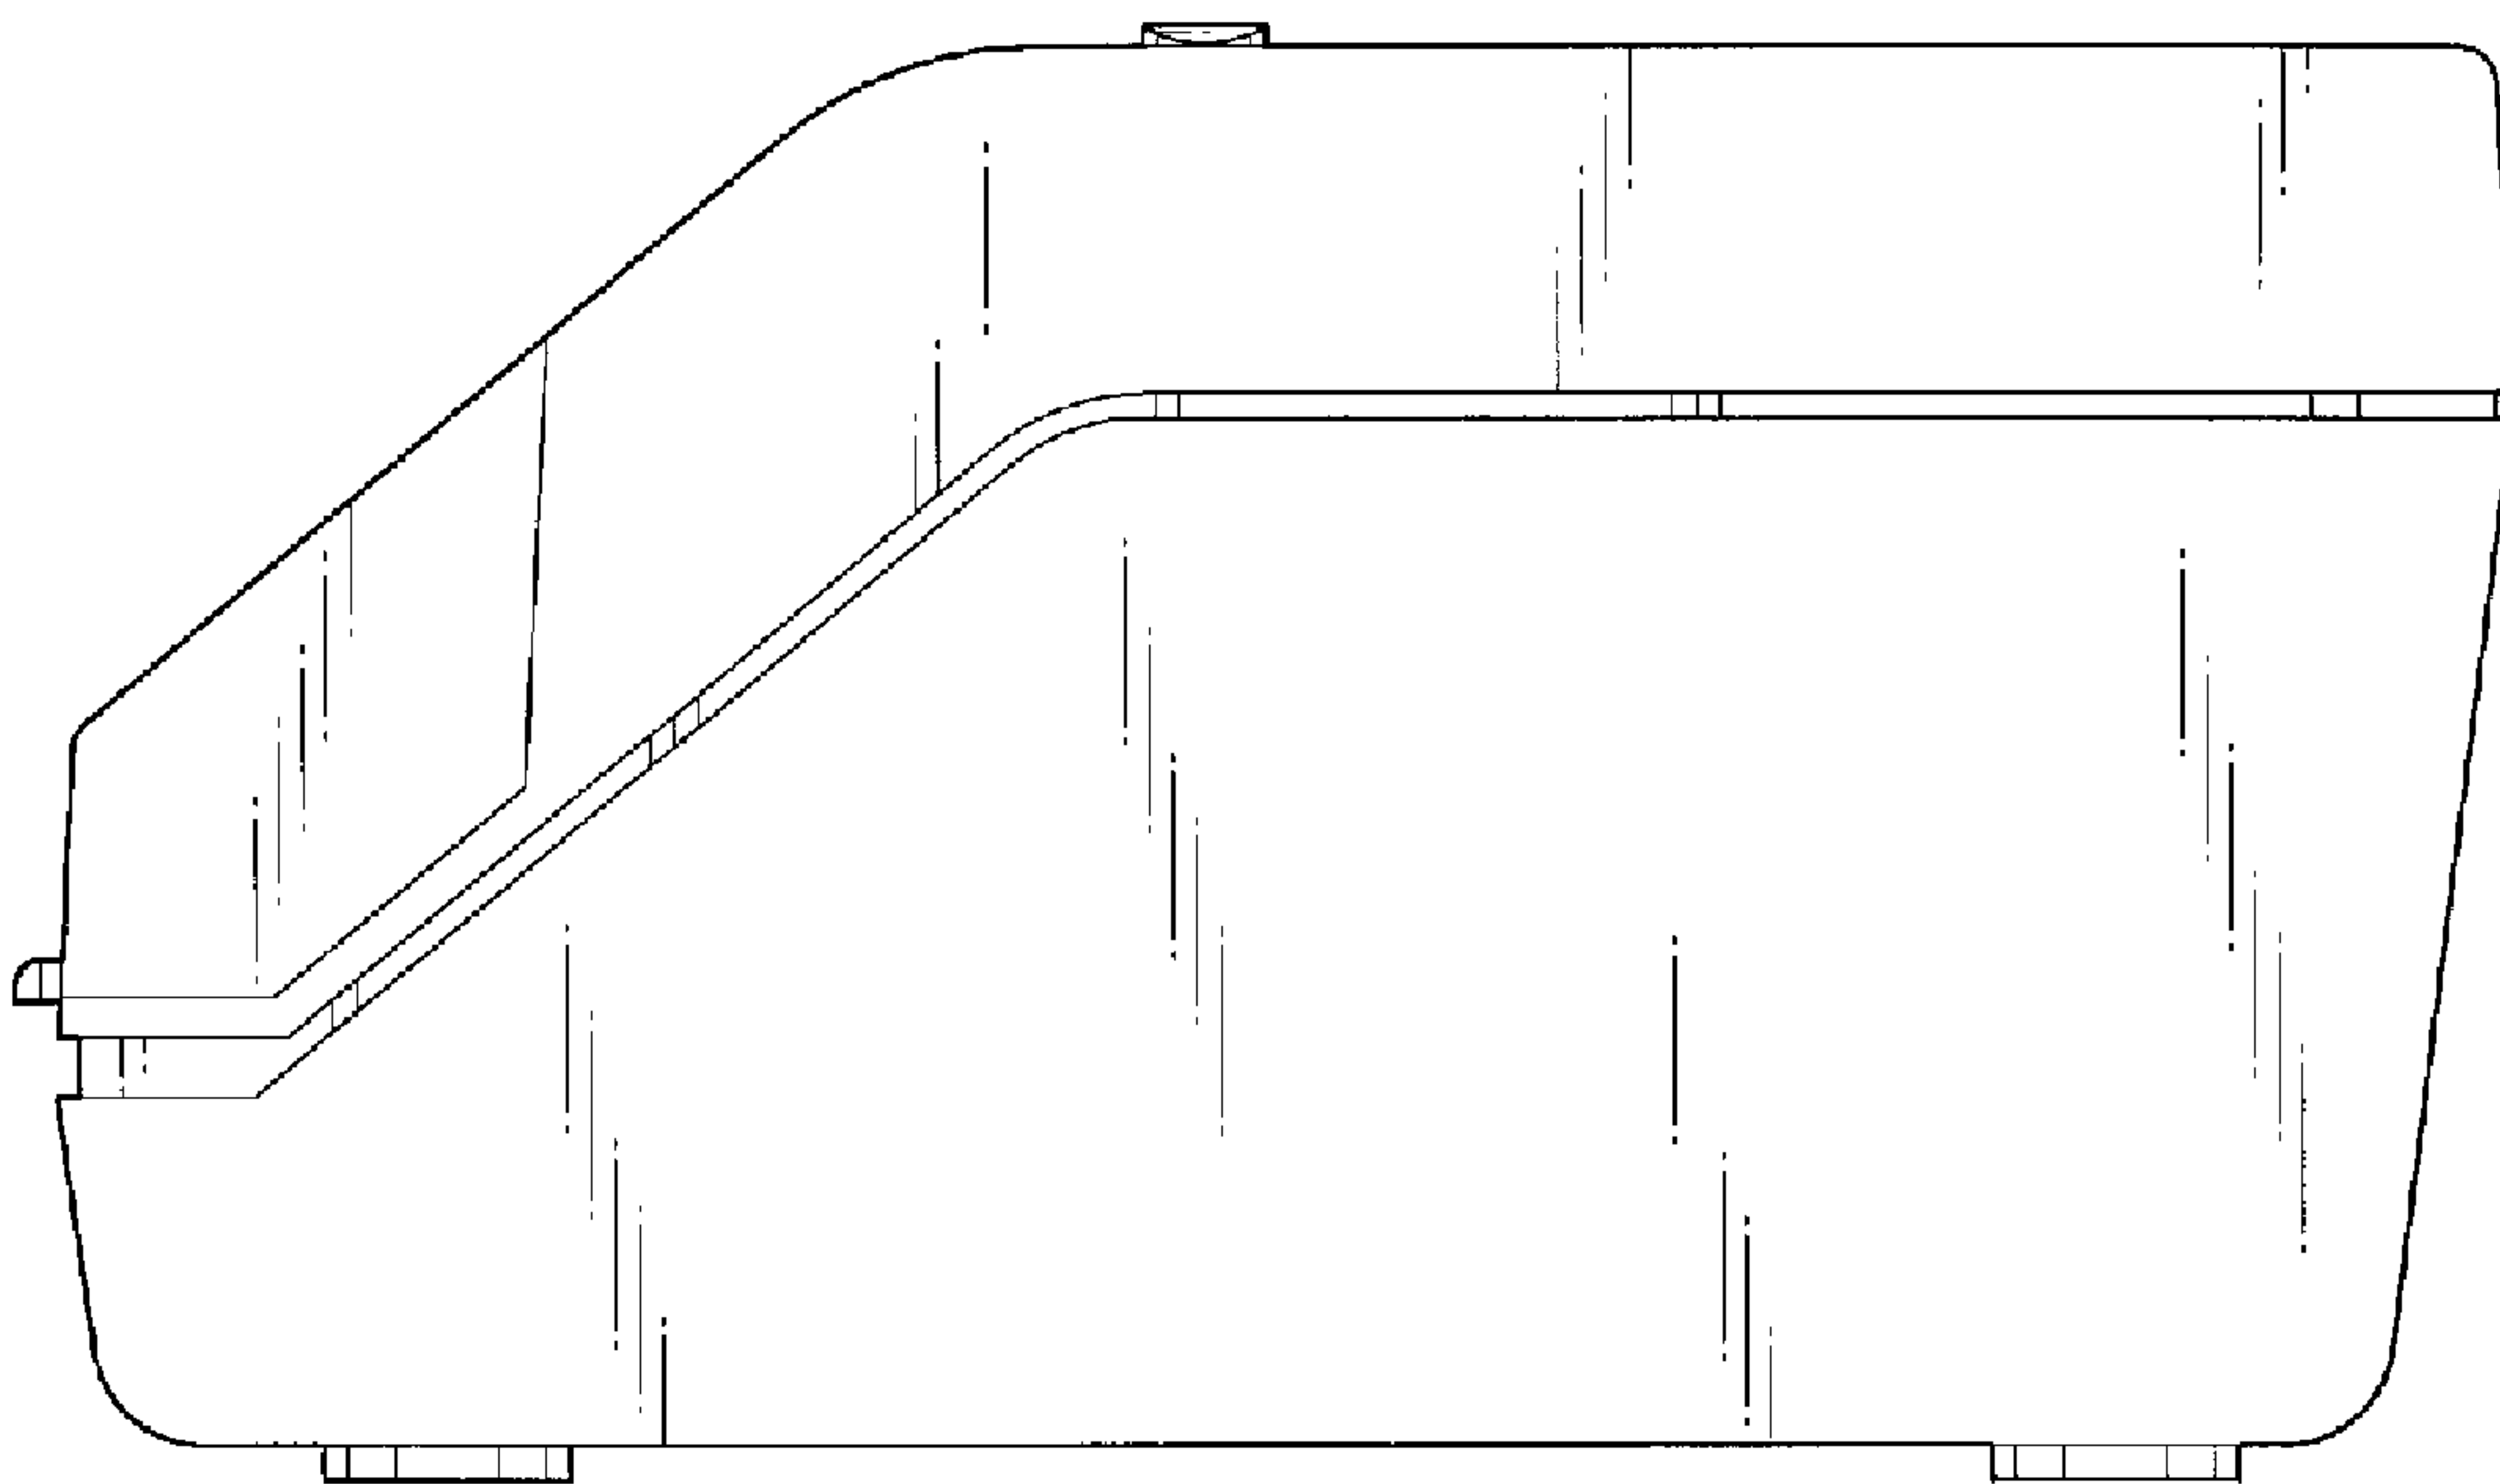


FIG.7



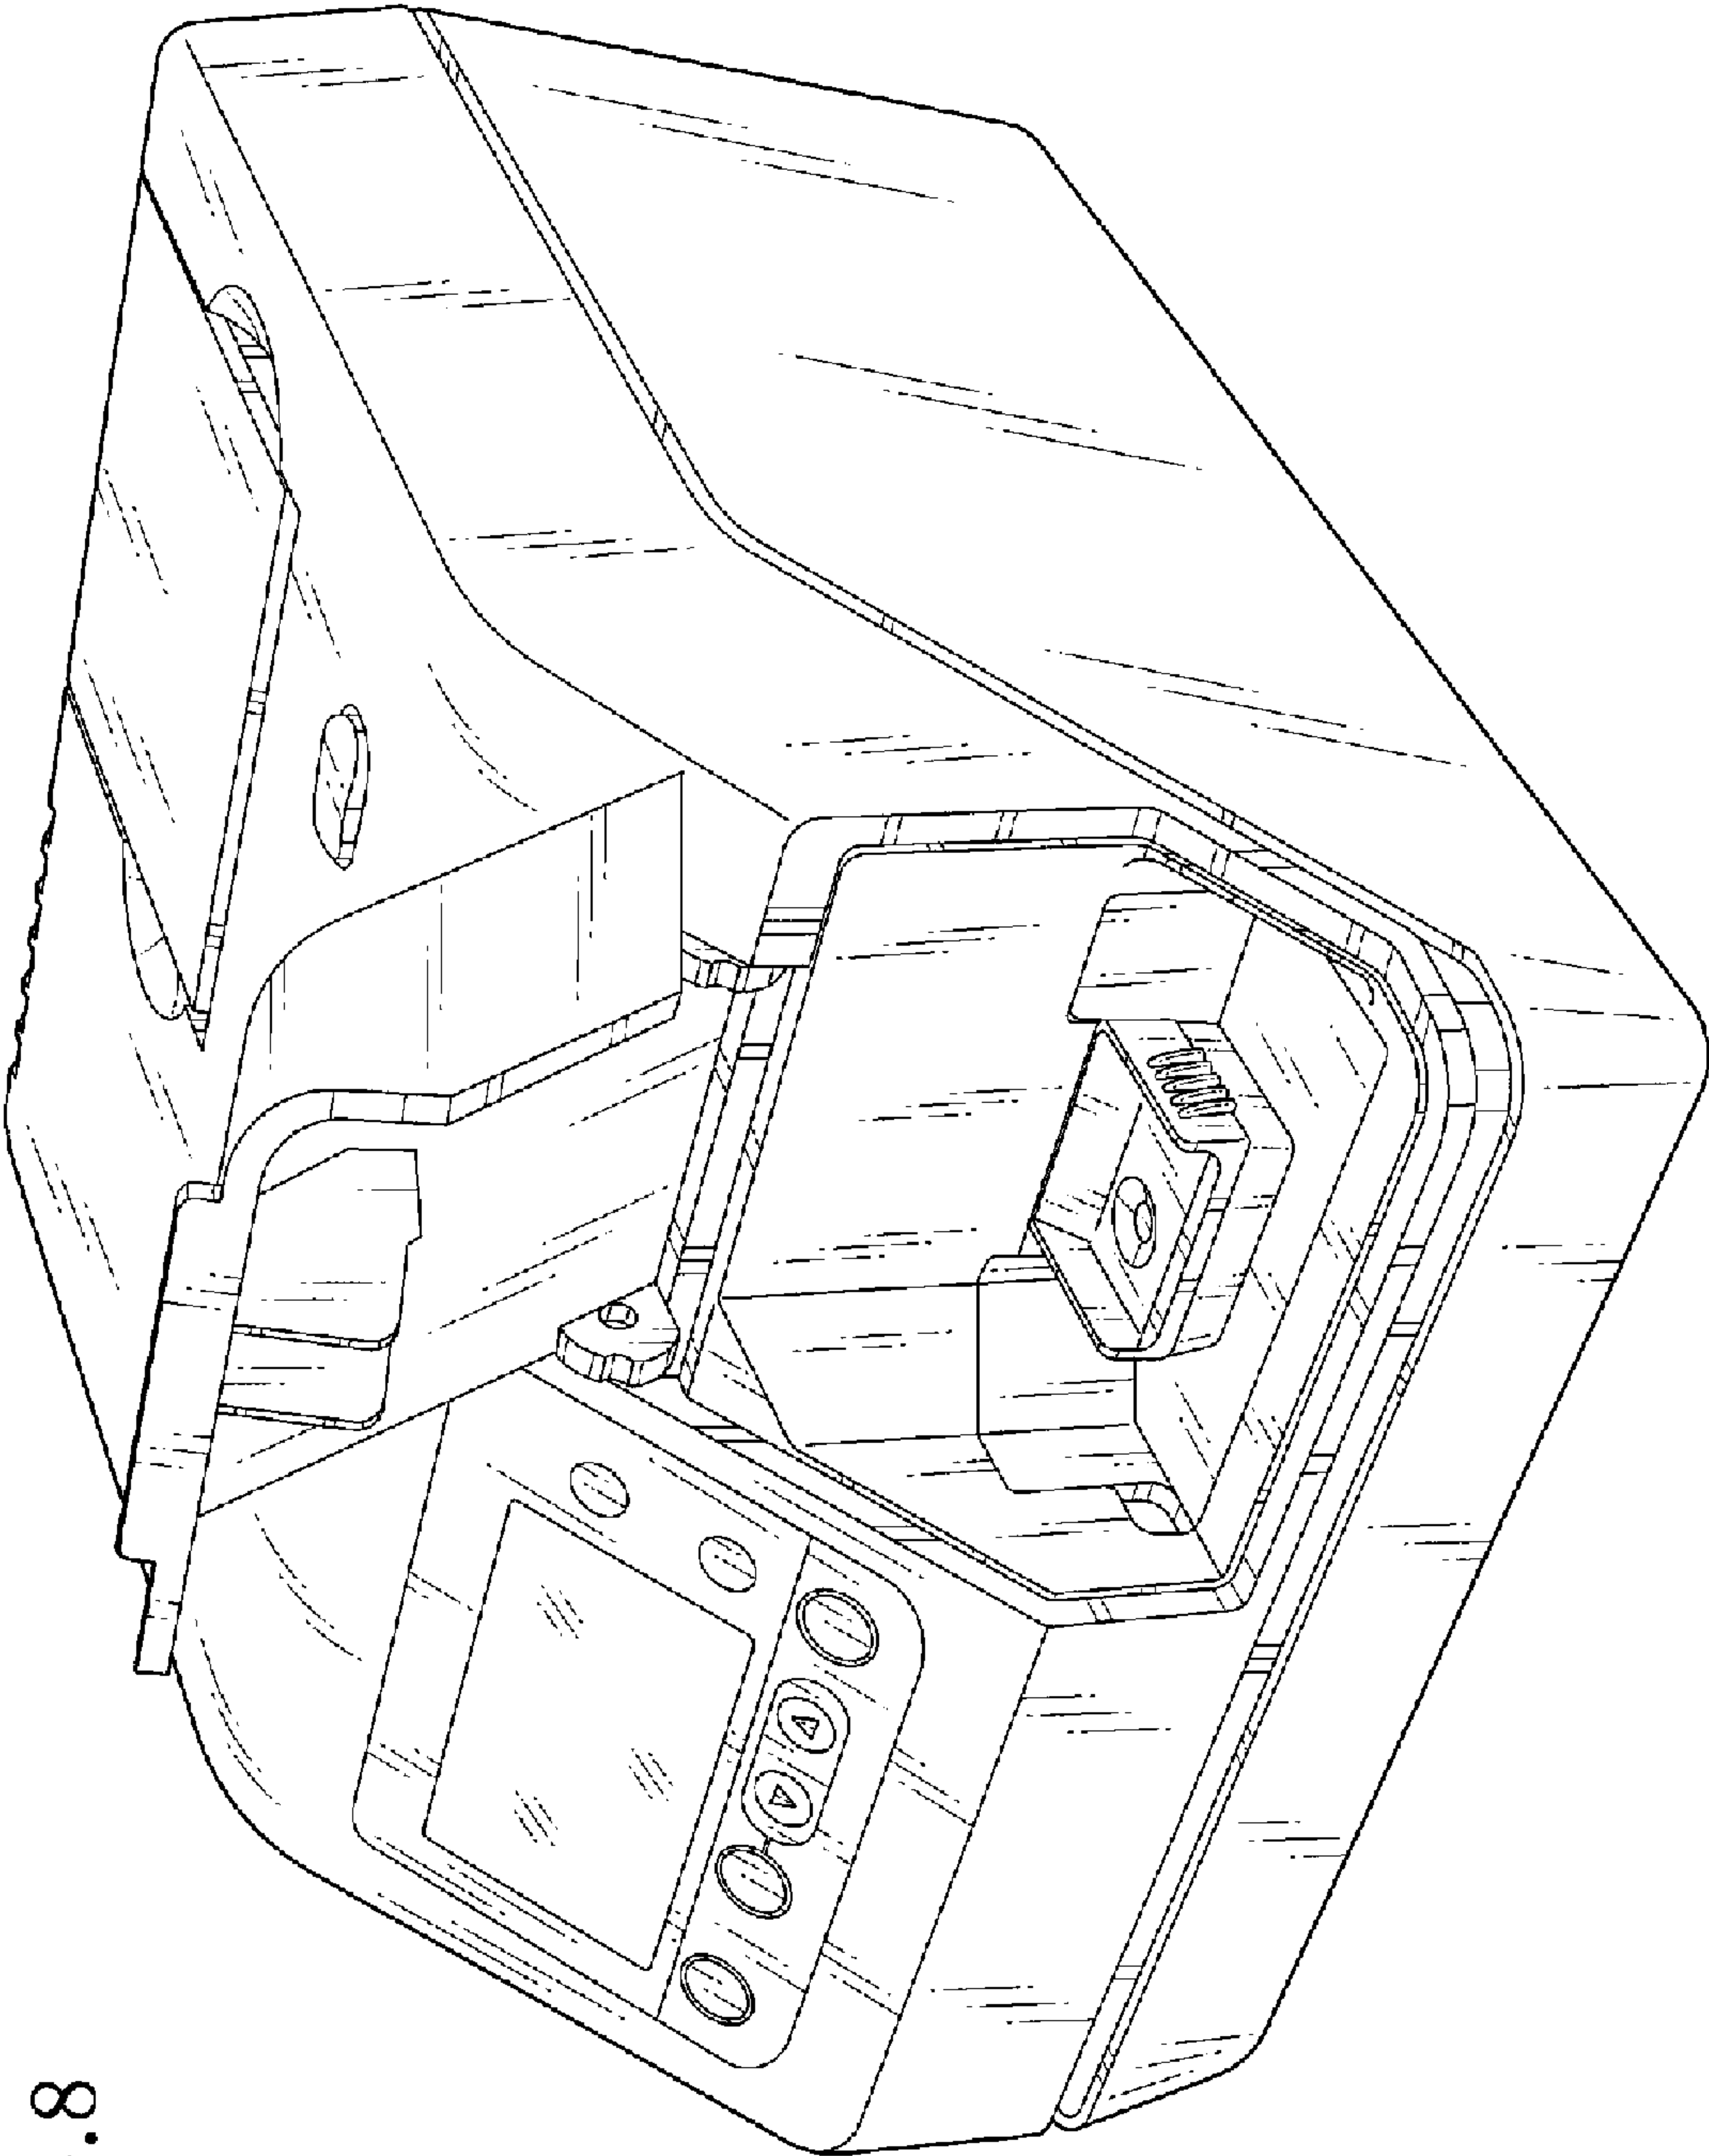


FIG. 8