



US00D639957S

(12) **United States Design Patent**  
**Pauschitz**

(10) **Patent No.:** **US D639,957 S**

(45) **Date of Patent:** **\*\* Jun. 14, 2011**

(54) **BLOOD GLUCOSE METER**

(75) Inventor: **Christoph Pauschitz**, Vienna (AT)

(73) Assignee: **MED TRUST Handelsgesellschaft  
m.b.H.**, Marz (AT)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/347,393**

(22) Filed: **Dec. 22, 2009**

(30) **Foreign Application Priority Data**

Jun. 26, 2009 (EM) ..... 001150288-0001

Jun. 26, 2009 (EM) ..... 001150288-0002

(51) **LOC (9) Cl.** ..... **24-01**

(52) **U.S. Cl.** ..... **D24/169**

(58) **Field of Classification Search** ..... D24/164-169,  
D24/107, 186, 187; D10/46, 78, 81; 435/14,  
435/287.1; 422/56, 58, 68.1; 600/316, 322,  
600/365, 368; D14/488-490

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D446,582 S \* 8/2001 Hayakawa ..... D24/165  
D469,107 S \* 1/2003 Miller et al. .... D14/488  
6,781,921 B2 \* 8/2004 Markart ..... 368/10

D504,516 S \* 4/2005 Yamazaki ..... D24/186  
D523,555 S \* 6/2006 Loerwald et al. .... D24/146  
D585,314 S \* 1/2009 Schvetz ..... D10/78  
7,514,040 B2 \* 4/2009 Wu et al. .... 422/68.1  
D610,688 S \* 2/2010 Donars et al. .... D24/169  
D611,489 S \* 3/2010 Bell et al. .... D14/486  
2008/0294024 A1 \* 11/2008 Cosentino et al. .... 600/309  
2008/0312555 A1 \* 12/2008 Boecker ..... 600/583  
2009/0240129 A1 \* 9/2009 Ginsberg ..... 600/365  
2009/0326445 A1 \* 12/2009 Graskov et al. .... 604/67  
2010/0331650 A1 \* 12/2010 Batman et al. .... 600/365

\* cited by examiner

*Primary Examiner* — T. Chase Nelson

*Assistant Examiner* — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Dennison, Schultz &  
MacDonald; George H. Spencer

(57) **CLAIM**

The ornamental design for a blood glucose meter, as shown  
and described.

**DESCRIPTION**


FIG. 1 is a front elevational view showing my new design of  
a blood glucose meter.

FIG. 2 is a perspective view showing the front, top and one  
side view thereof; and,

FIG. 3 is a rear elevation view thereof.

The portions of the blood glucose meter shown in broken  
lines form no part of the claimed design.

**1 Claim, 2 Drawing Sheets**

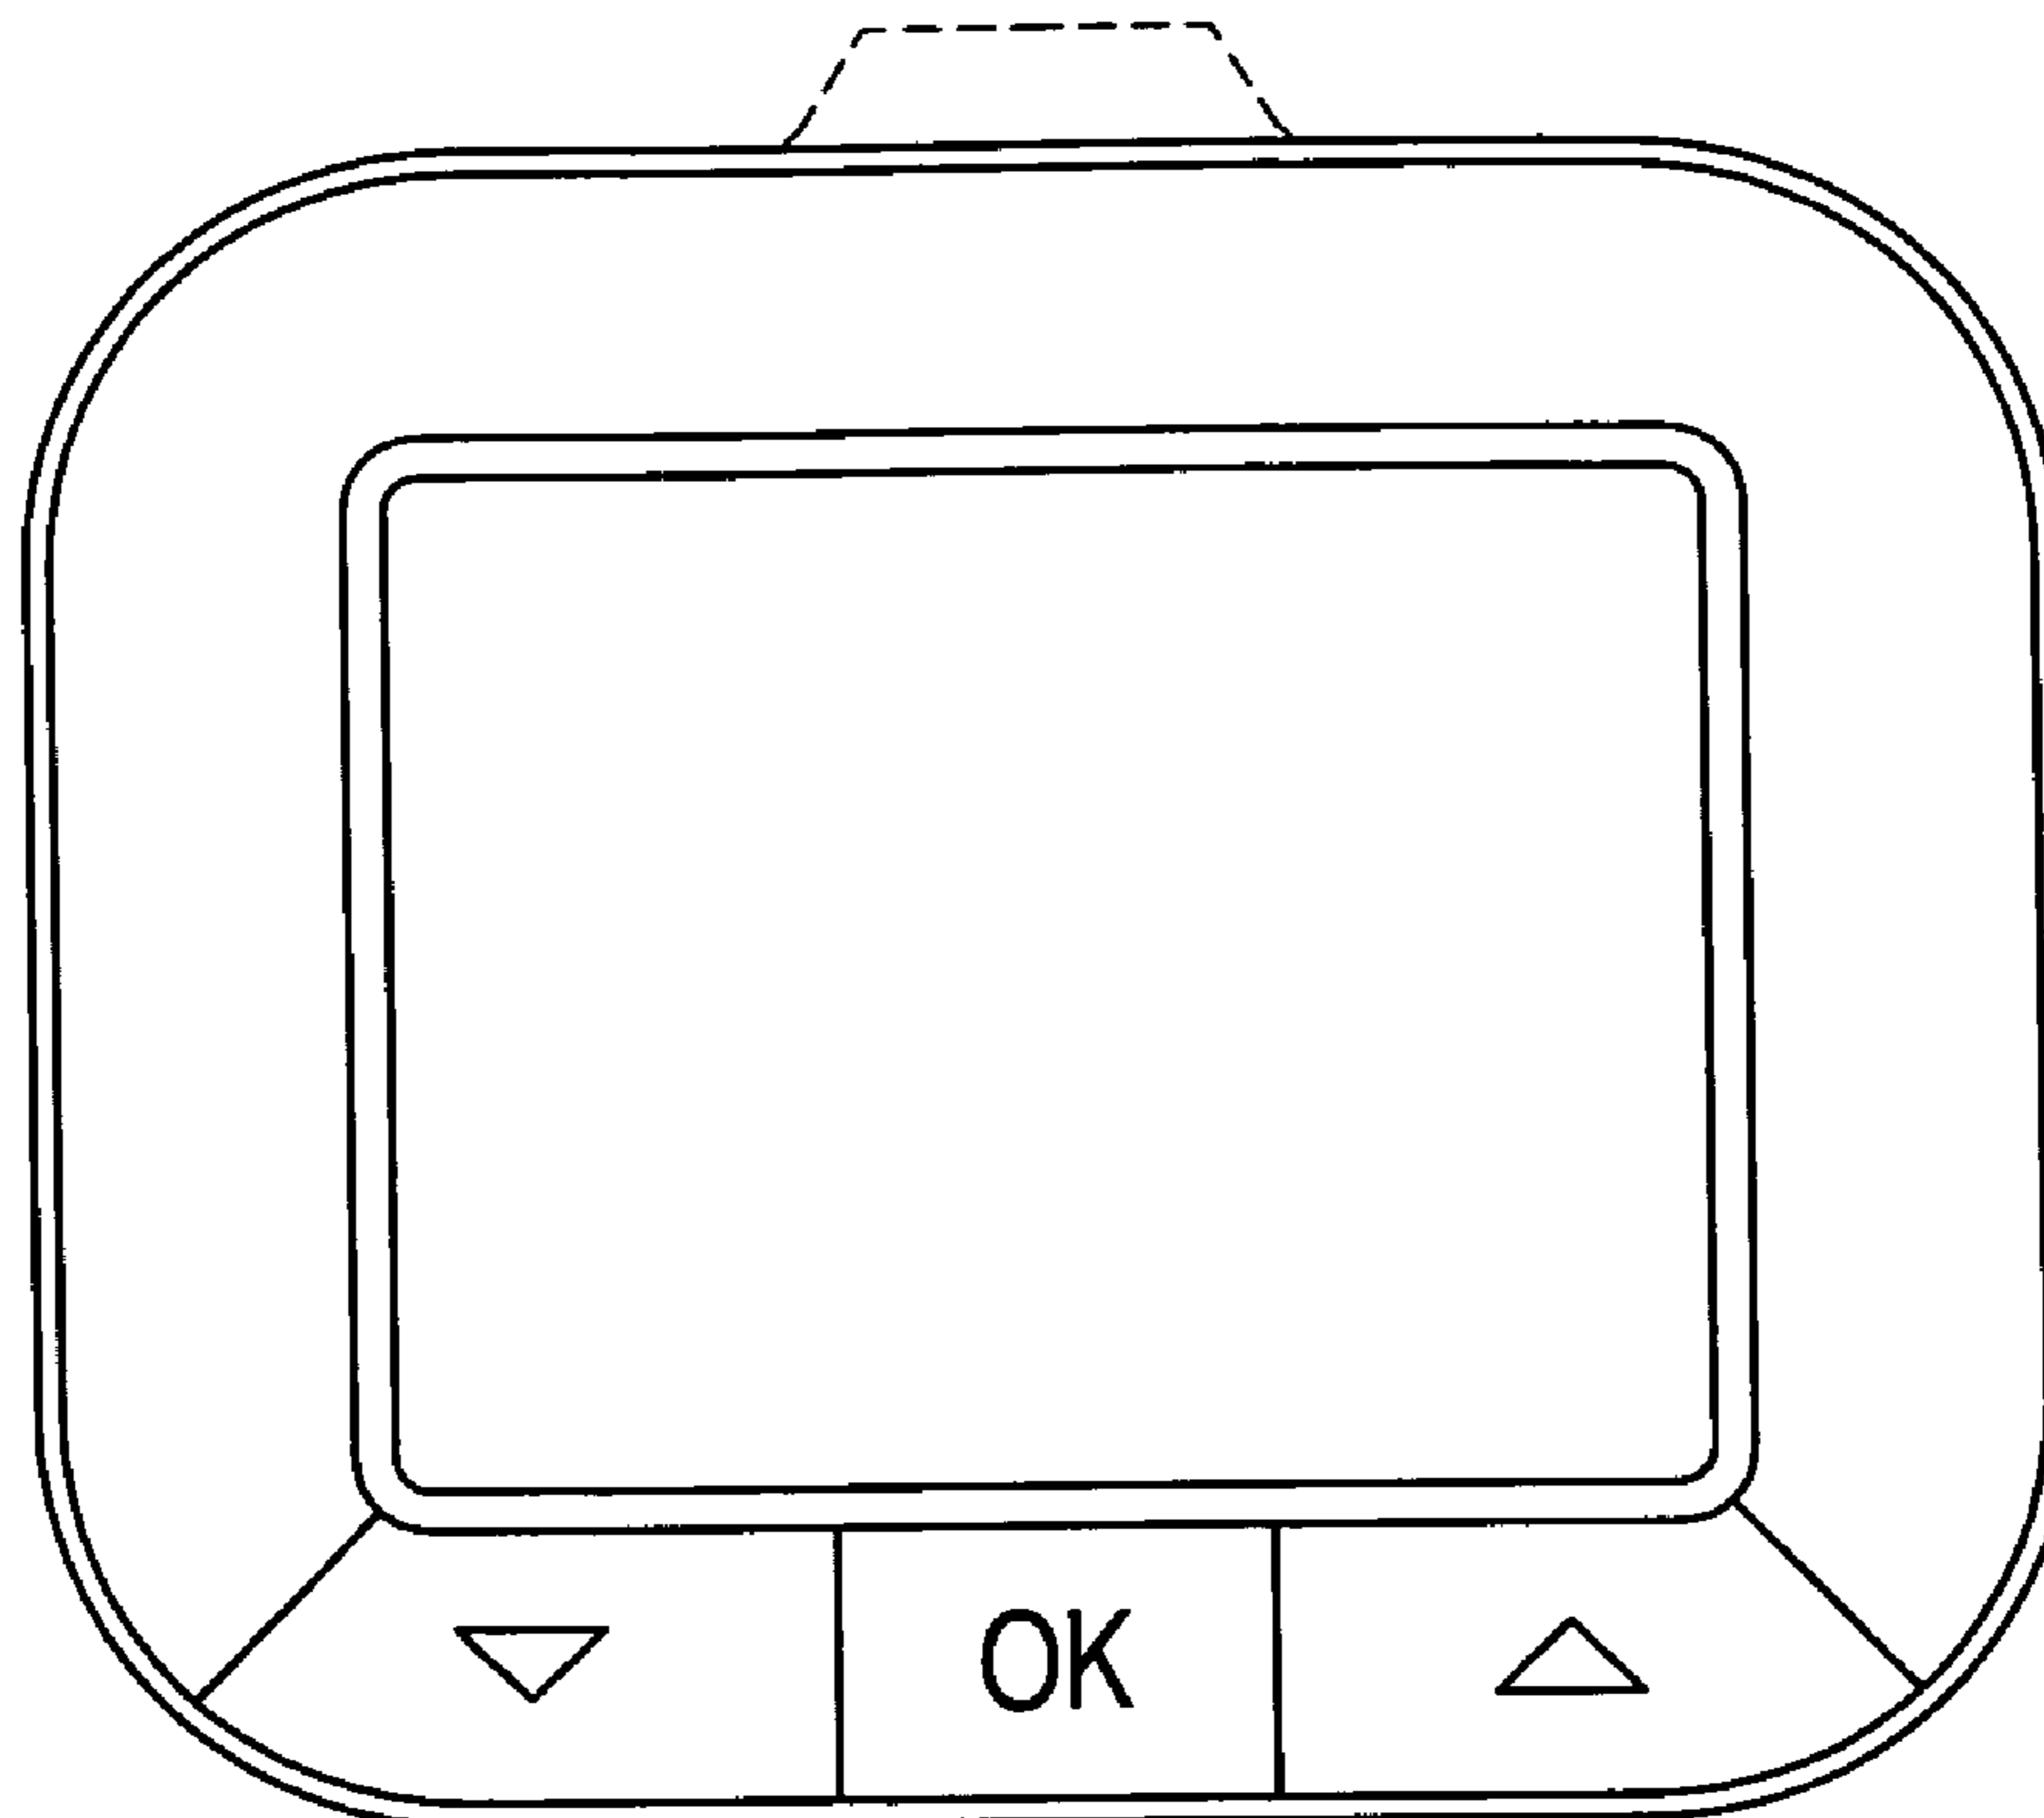

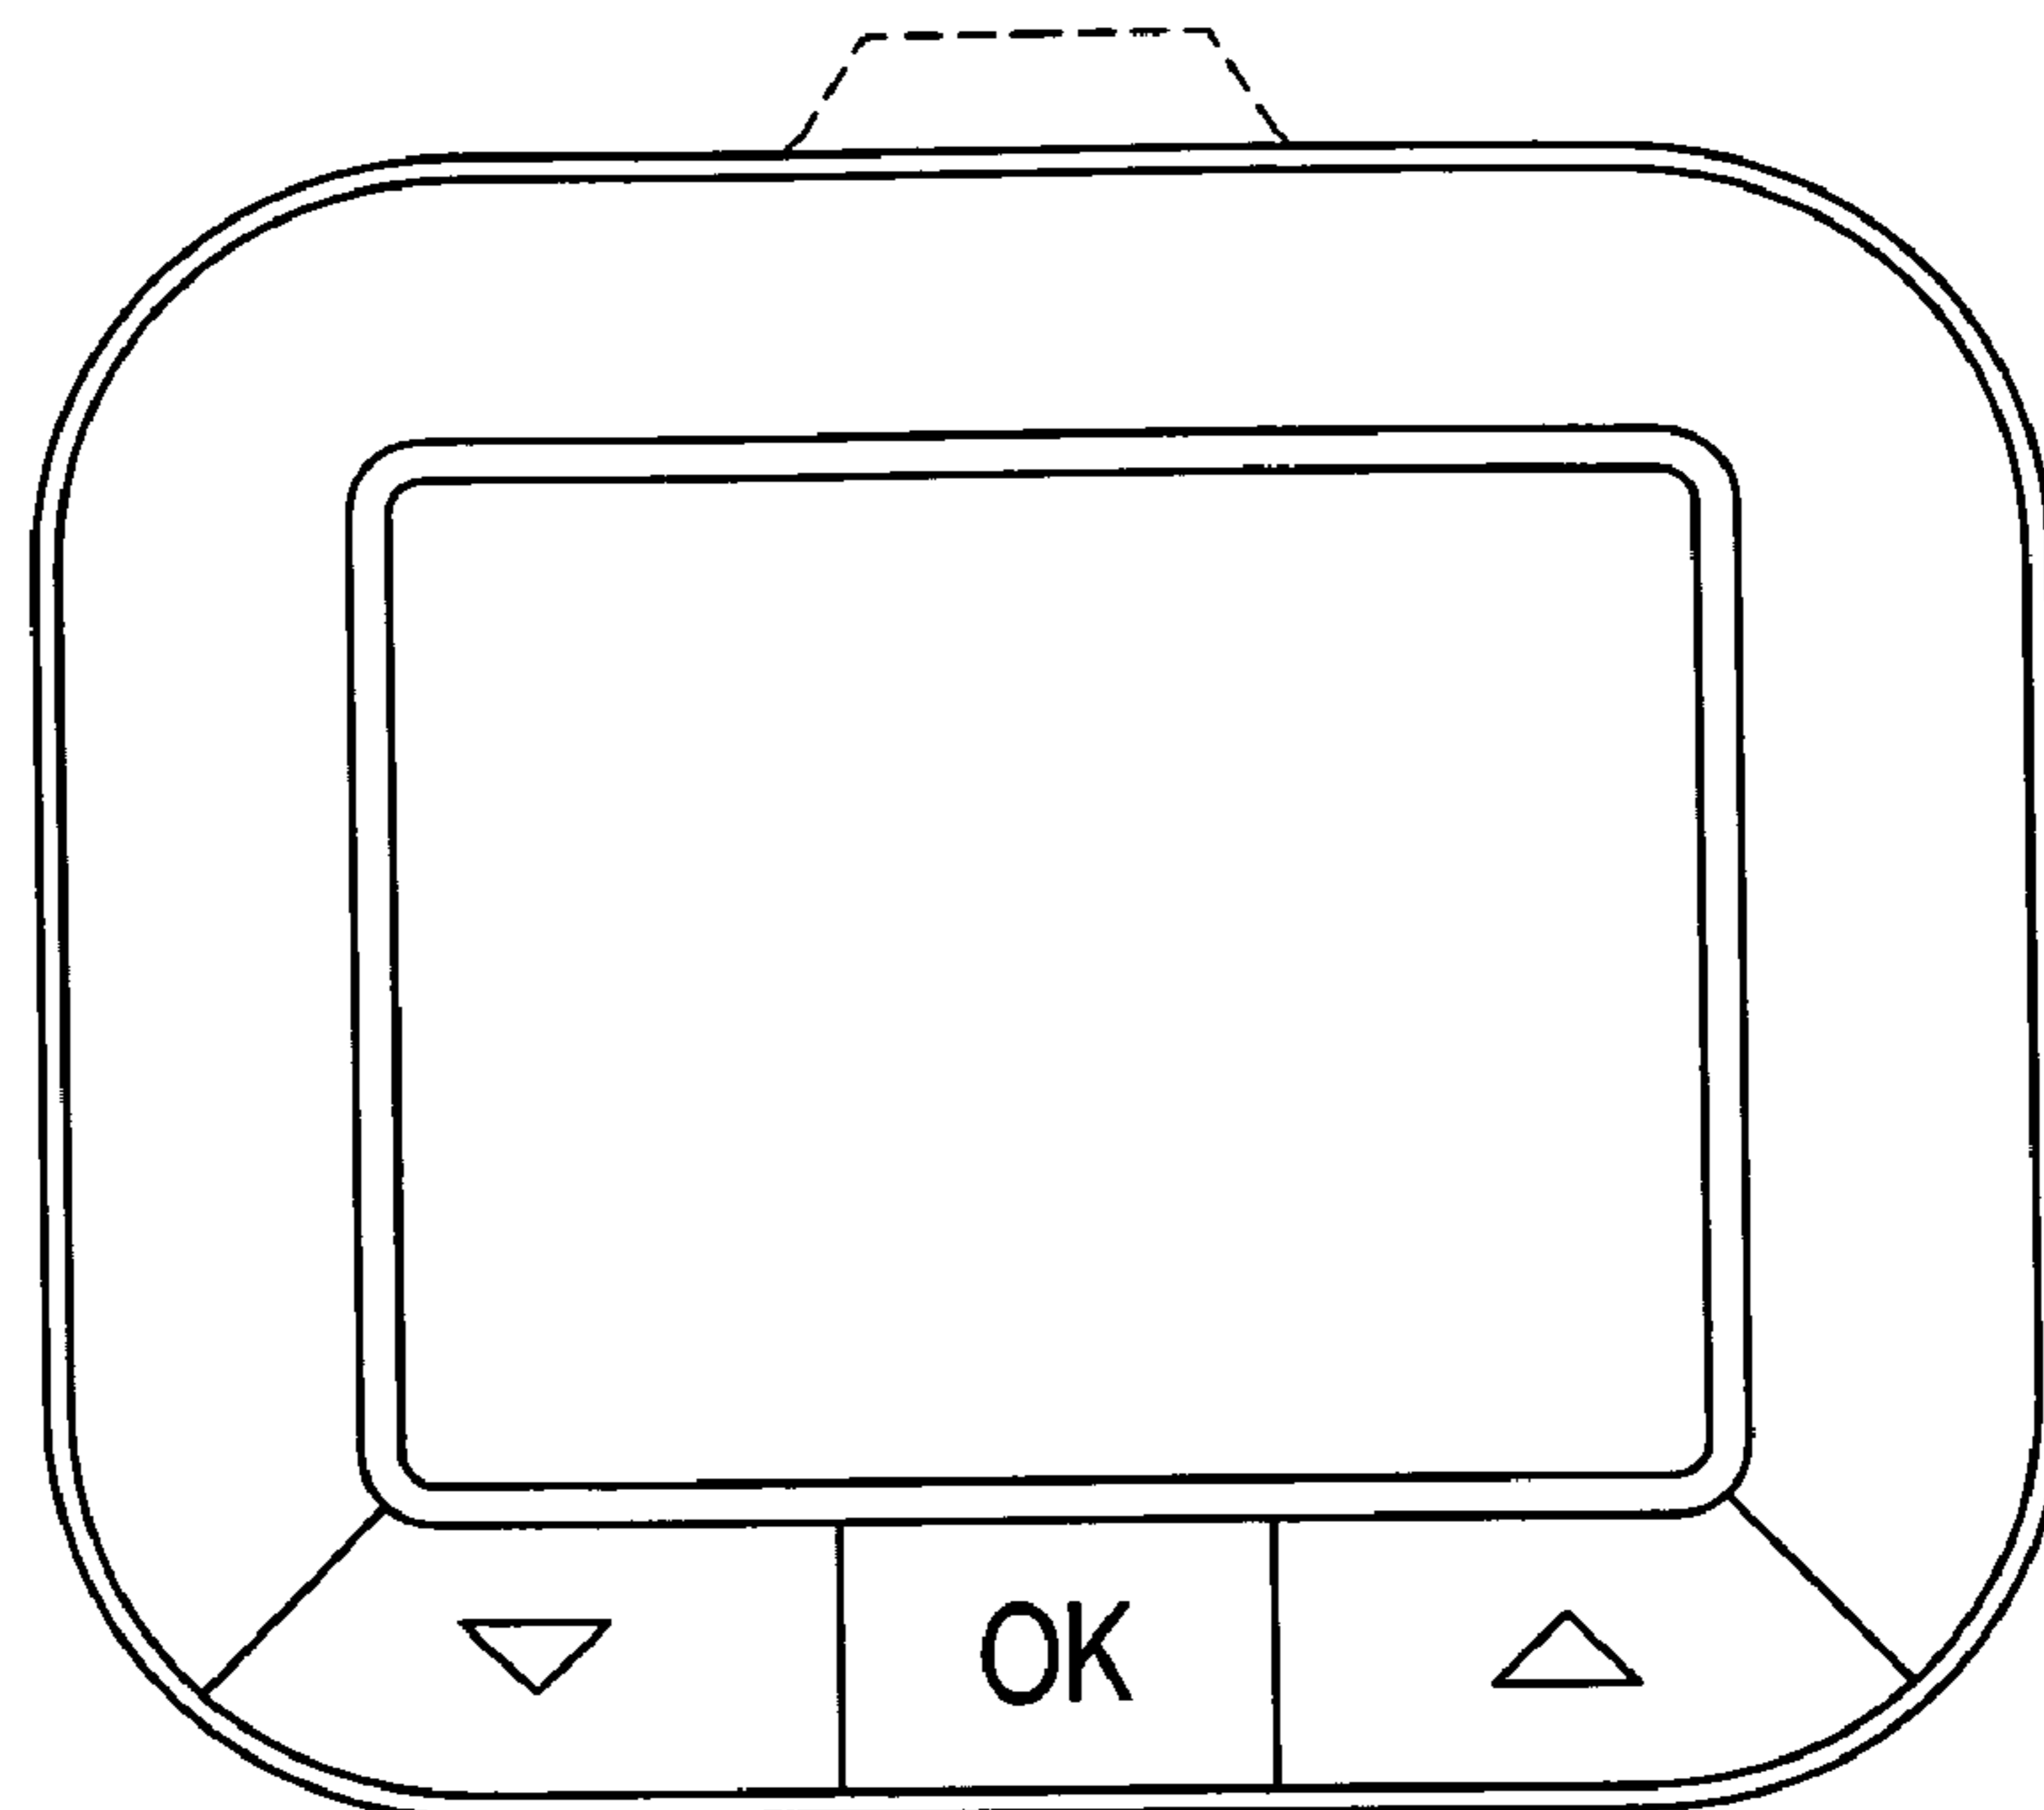


FIG. 1

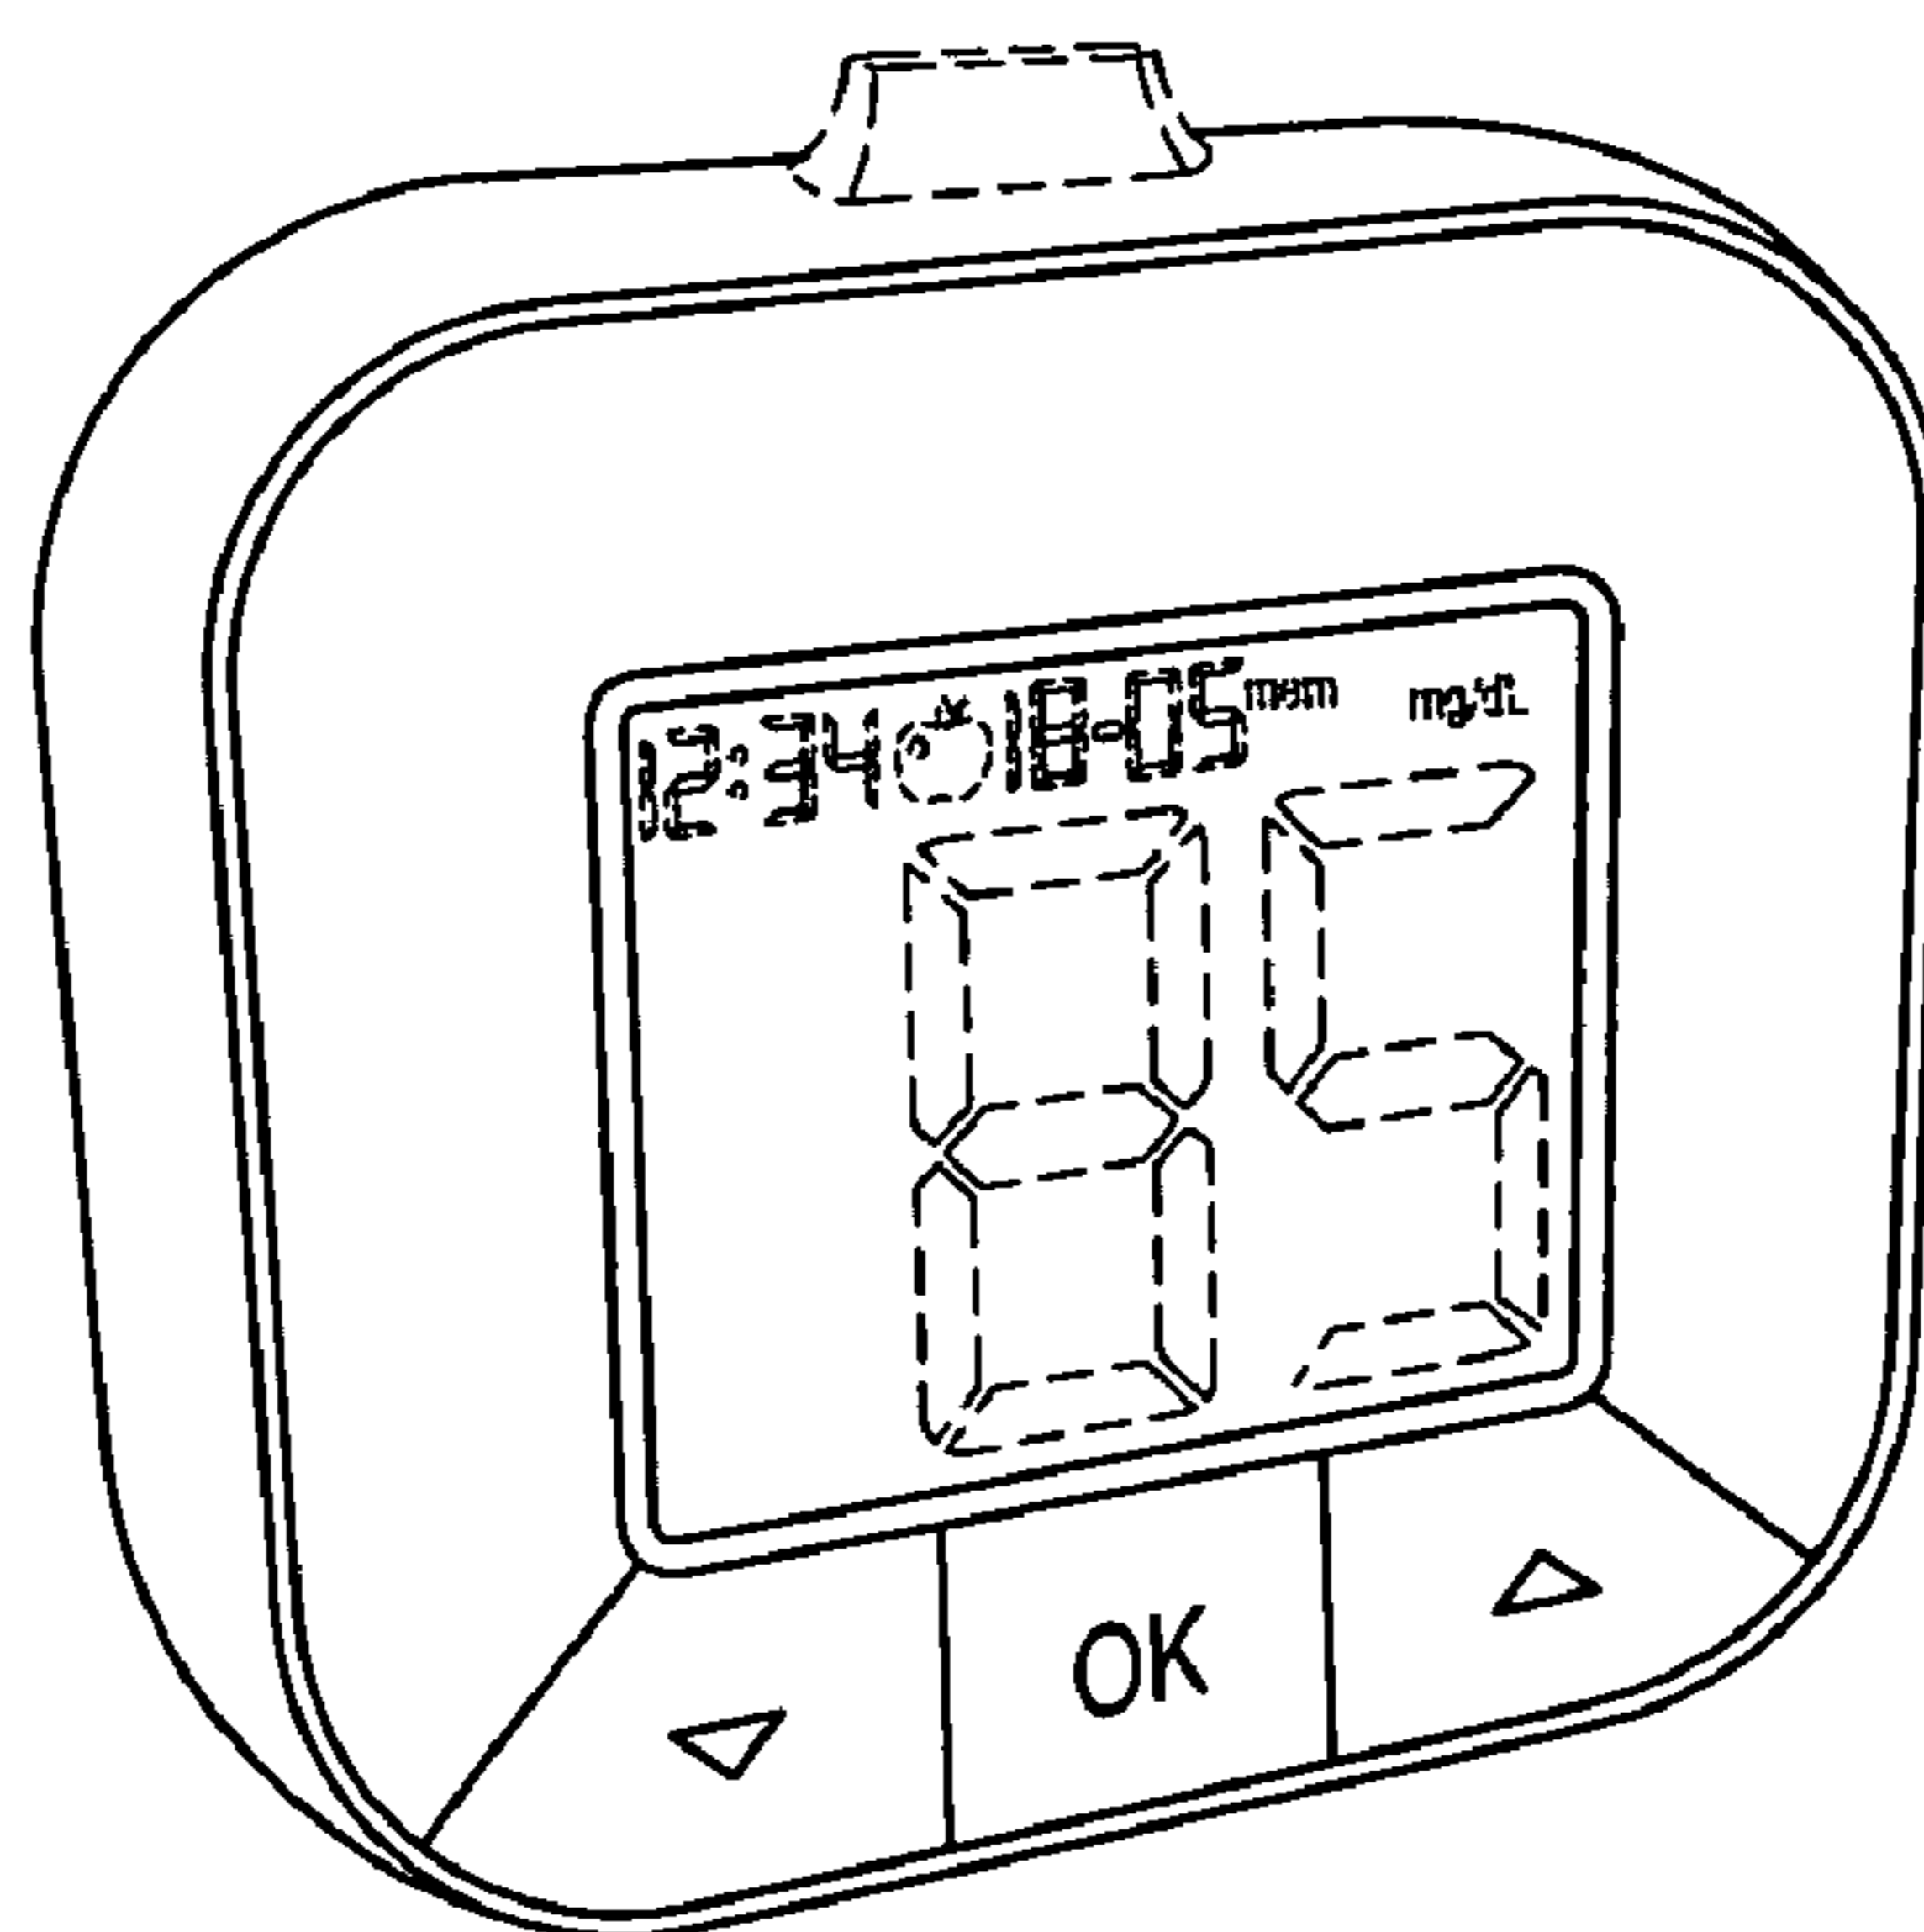


FIG. 2

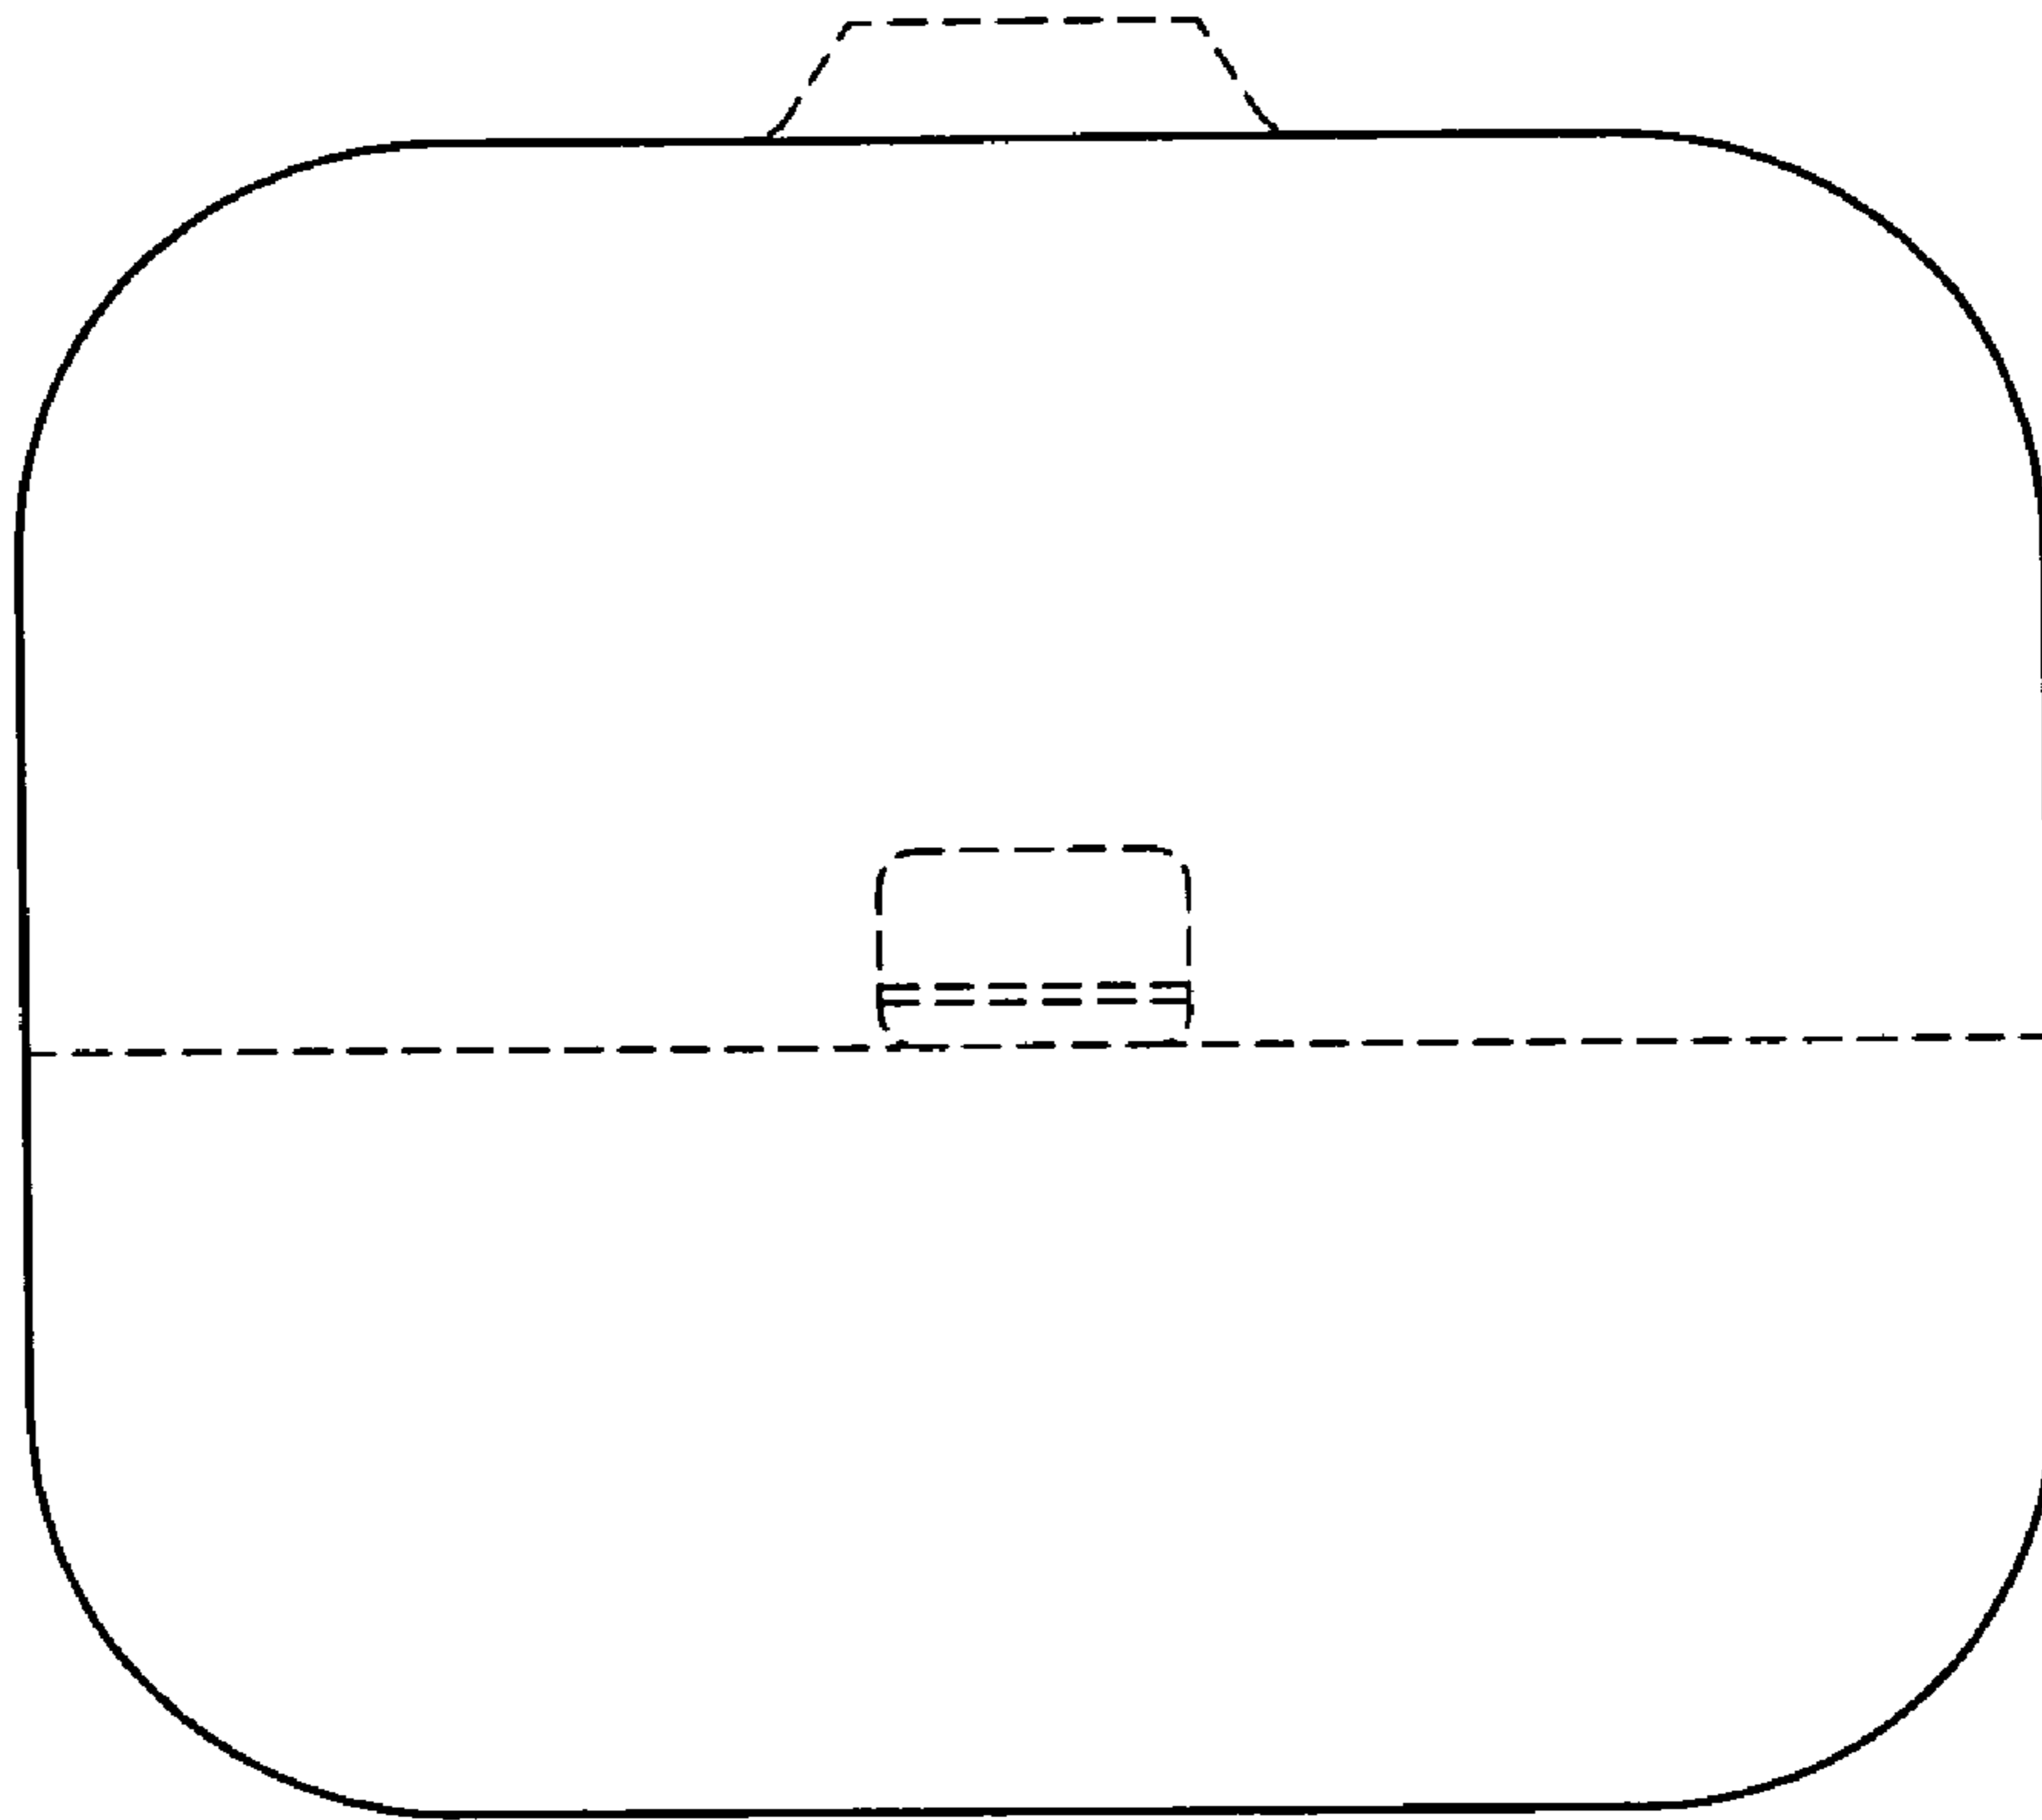


FIG. 3