



US00D640377S

(12) **United States Design Patent**  
**Amano et al.**

(10) **Patent No.:** **US D640,377 S**  
(45) **Date of Patent:** **\*\* Jun. 21, 2011**

(54) **CONTROLLER FOR MEDICAL APPARATUS**

(75) Inventors: **Hirotohi Amano**, Tachikawa (JP);  
**Kenji Tajima**, Hachioji (JP); **Takao Tabata**, Hachioji (JP)

(73) Assignee: **Olympus Medical Systems Corp.**,  
Tokyo (JP)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/377,049**

(22) Filed: **Oct. 15, 2010**

**Related U.S. Application Data**

(62) Division of application No. 29/329,853, filed on Dec. 22, 2008, now Pat. No. Des. 626,224.

(30) **Foreign Application Priority Data**

Jul. 4, 2008 (JP) ..... 2008-017303  
Jul. 4, 2008 (JP) ..... 2008-017304  
Jul. 4, 2008 (JP) ..... 2008-017305  
Jul. 4, 2008 (JP) ..... 2008-017306  
Sep. 5, 2008 (JP) ..... 2008-022913

(51) **LOC (9) Cl.** ..... **24-02**

(52) **U.S. Cl.** ..... **D24/138; D24/107; D24/144**

(58) **Field of Classification Search** ..... D24/107,  
D24/138, 144, 170, 186; D10/46, 78, 81,  
D10/103, 122, 124, 125, 108; D13/173,  
D13/177, 171, 174; D16/235, 219; 600/132,  
600/300, 301, 481, 178, 180, 182

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D243,115 S \* 1/1977 Ziegler et al. .... D24/138  
D247,251 S \* 2/1978 Napoli ..... D24/186  
D250,480 S \* 12/1978 Wettermann et al. .... D24/170  
D317,136 S \* 5/1991 Kulikowski et al. .... D10/108  
D323,894 S \* 2/1992 Rosati et al. .... D24/186

D340,769 S \* 10/1993 Bloom et al. .... D24/186  
D348,623 S \* 7/1994 Coronato et al. .... D10/108  
D349,340 S \* 8/1994 Snoke et al. .... D24/138  
D349,343 S \* 8/1994 Hannon et al. .... D24/170  
D376,207 S \* 12/1996 Buczek et al. .... D24/138  
D378,200 S \* 2/1997 Doppelt et al. .... D10/108  
D412,977 S \* 8/1999 Hayamizu ..... D24/107  
D534,654 S \* 1/2007 Hayamizu ..... D24/138  
D565,513 S \* 4/2008 Biondo et al. .... D13/174  
D598,100 S \* 8/2009 Tanaka ..... D24/138  
D626,224 S \* 10/2010 Amano et al. .... D24/138

\* cited by examiner

*Primary Examiner* — Ian Simmons

*Assistant Examiner* — Wan Laymon

(74) *Attorney, Agent, or Firm* — Holtz, Holtz, Goodman & Chick, PC

(57) **CLAIM**



The ornamental design for a controller for medical apparatus, as shown and described.

**DESCRIPTION**

FIG. 1 is a front, right side and top perspective view of a controller for medical apparatus, showing our new design; FIG. 2 is an enlarged front elevational view thereof; FIG. 3 is an enlarged rear elevational view thereof; FIG. 4 is an enlarged top plan view thereof; FIG. 5 is an enlarged bottom plan view thereof; FIG. 6 is an enlarged right side elevational view thereof; FIG. 7 is an enlarged left side elevational view thereof; and, FIG. 8 is an enlarged fragmentary perspective view of the portion thereof surrounded by box 8 in FIG. 1, showing the power button part.

The broken lines immediately adjacent to the shaded areas and the claimed areas in the views represent the boundaries of the design while all other broken lines are included for the purpose of illustrating environmental structure and form no part of the claimed design. The stippling is used in the drawings to differentiate between the stippled and unstippled areas.

**1 Claim, 6 Drawing Sheets**

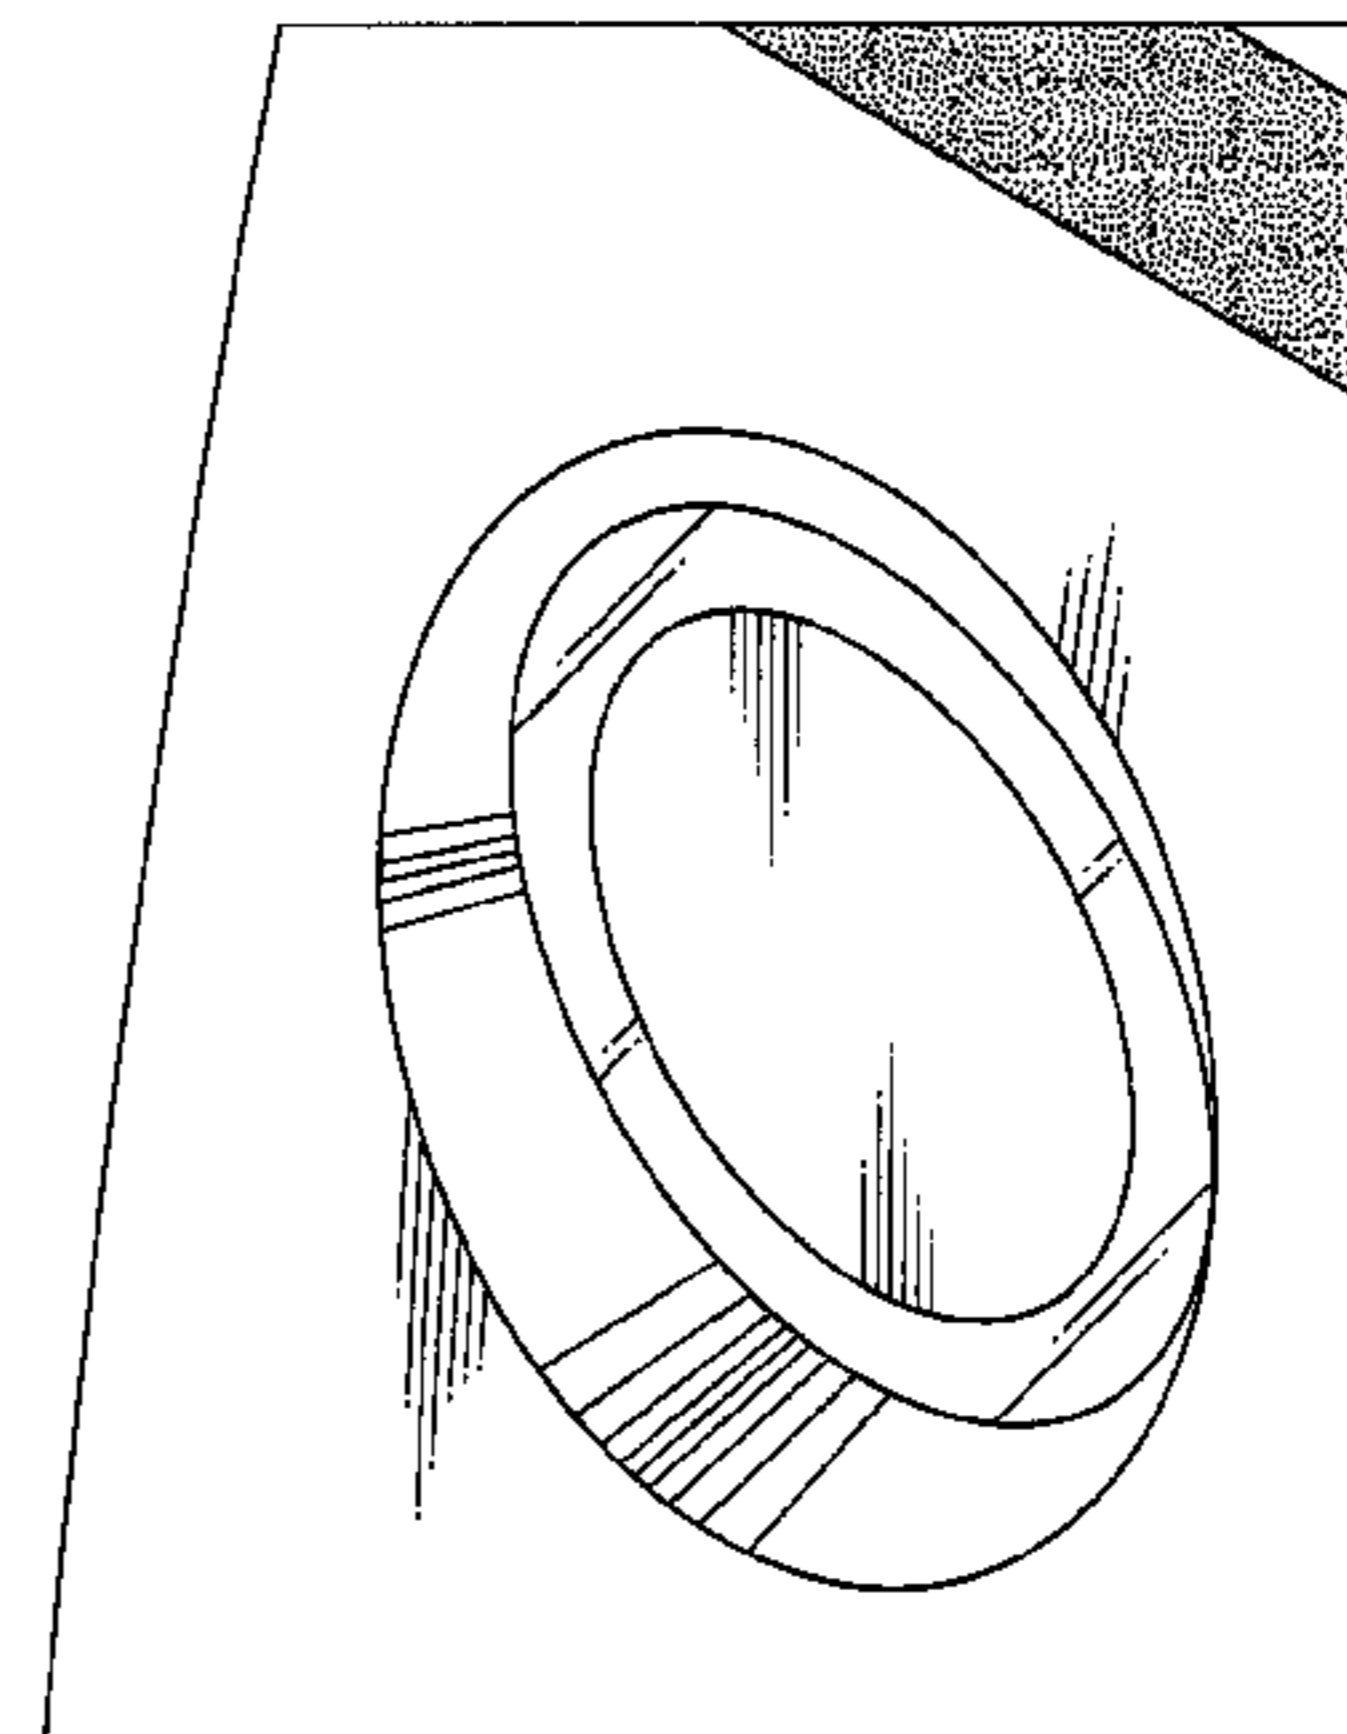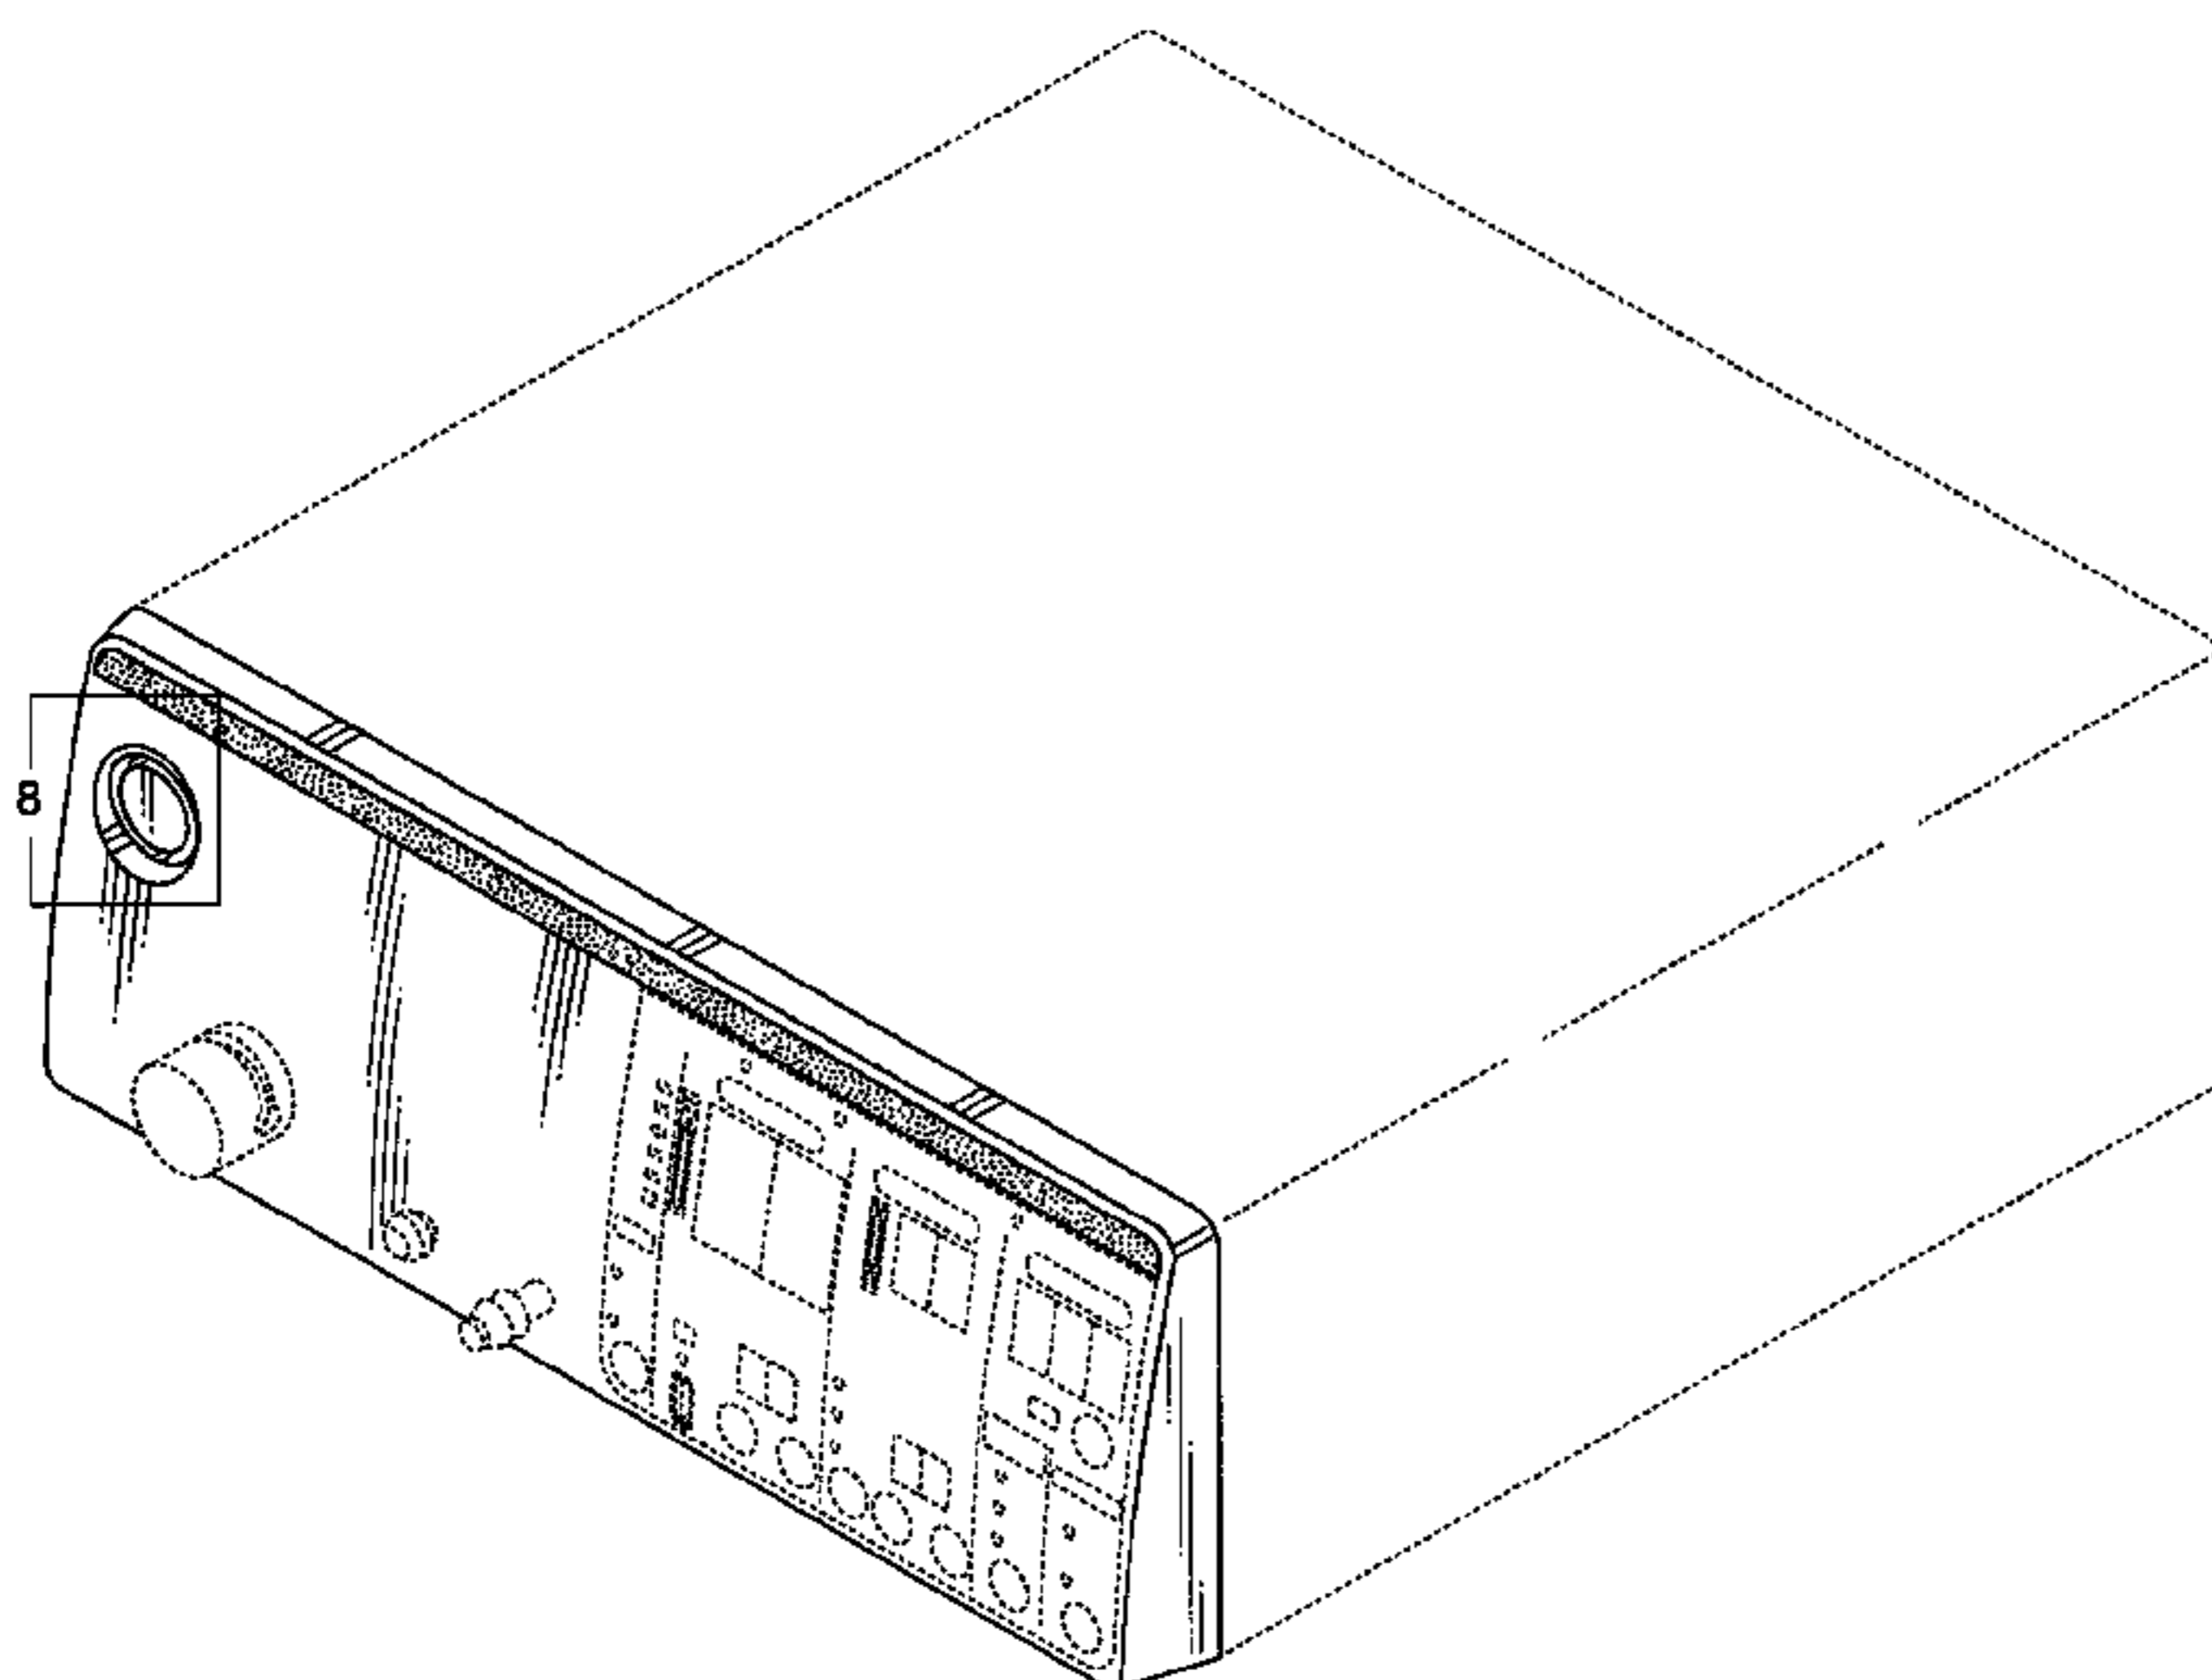

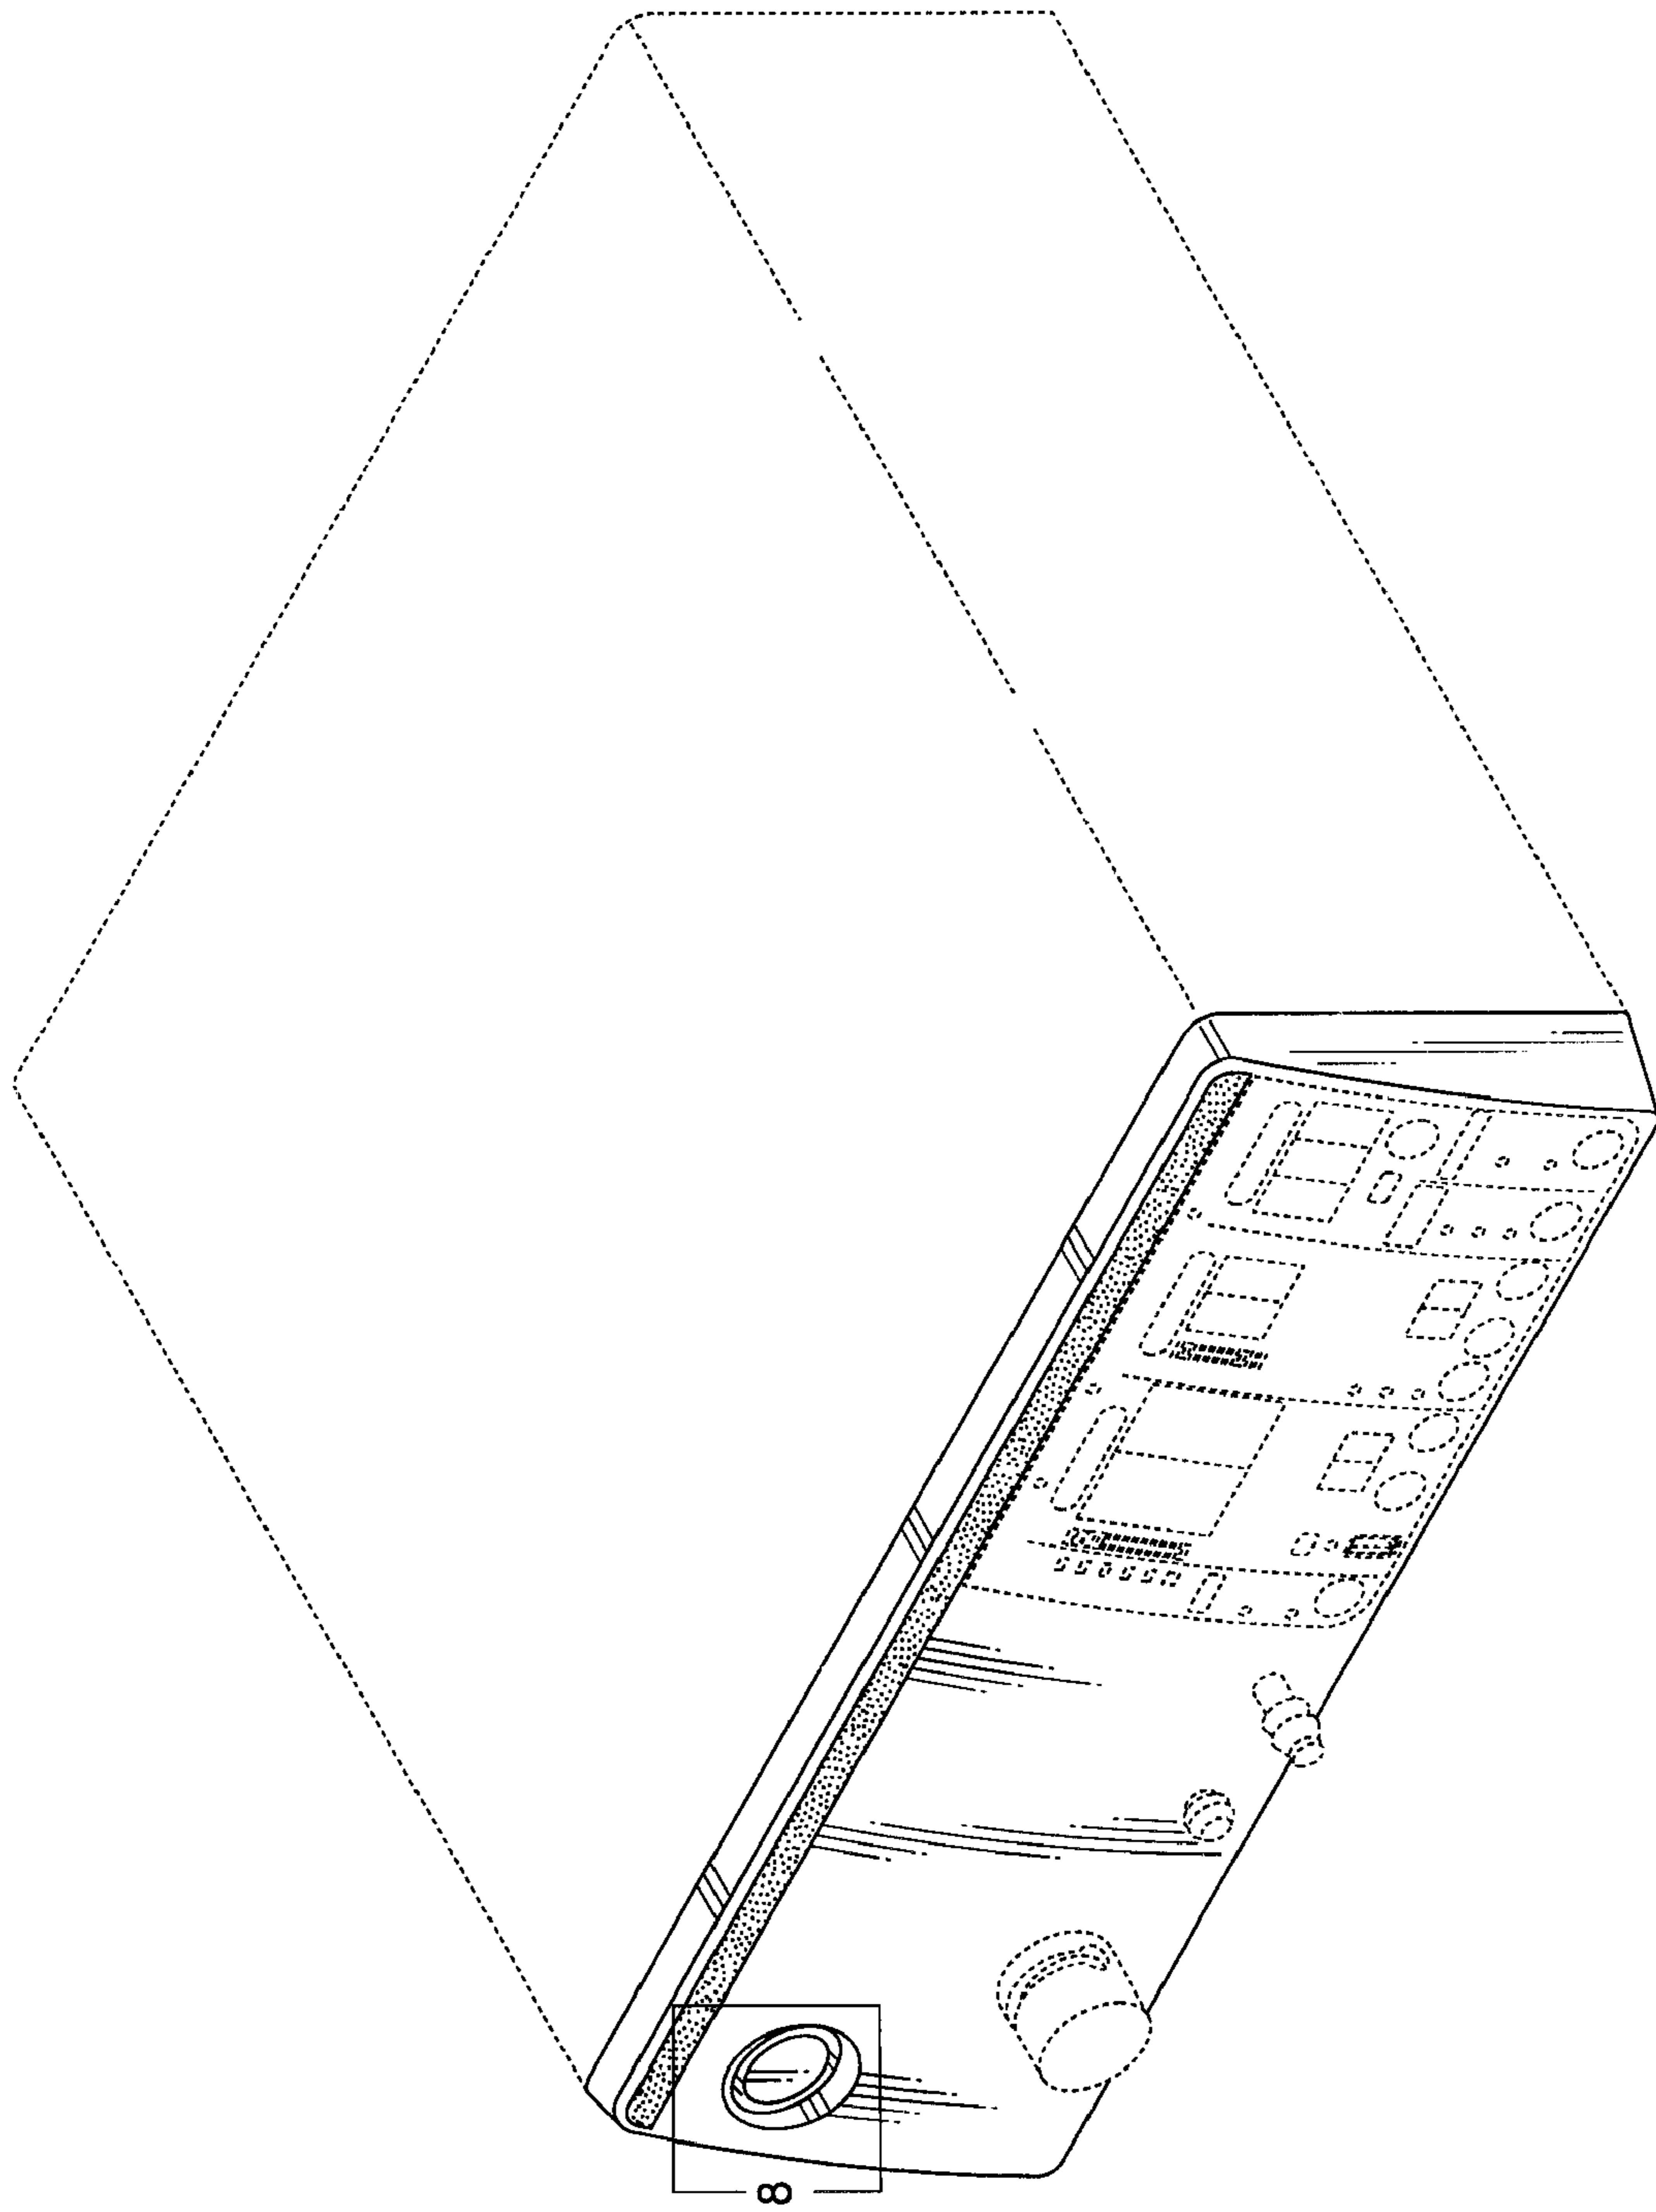


FIG.1

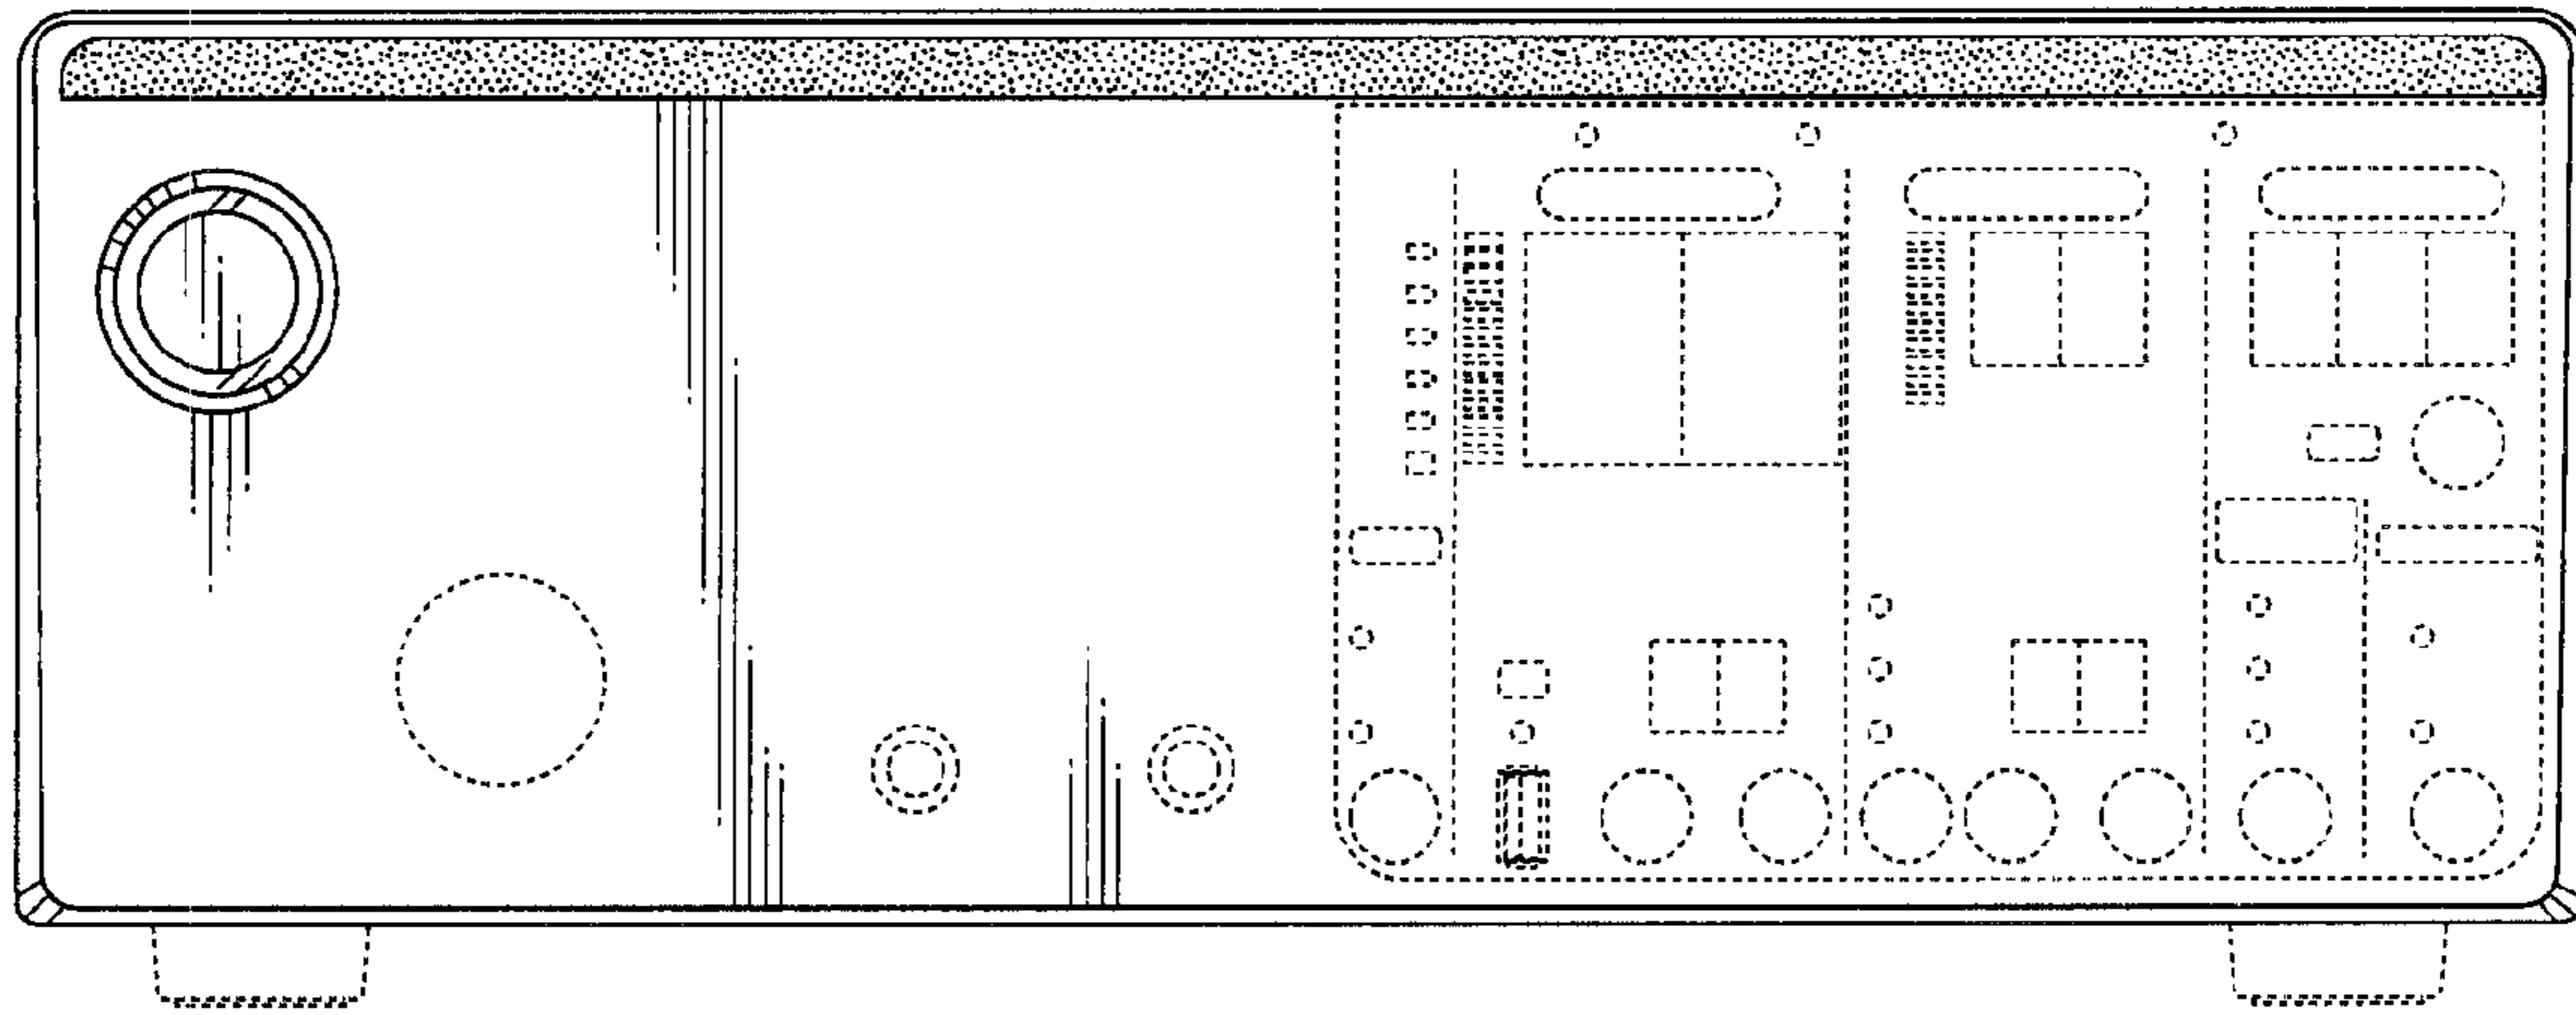


FIG.2

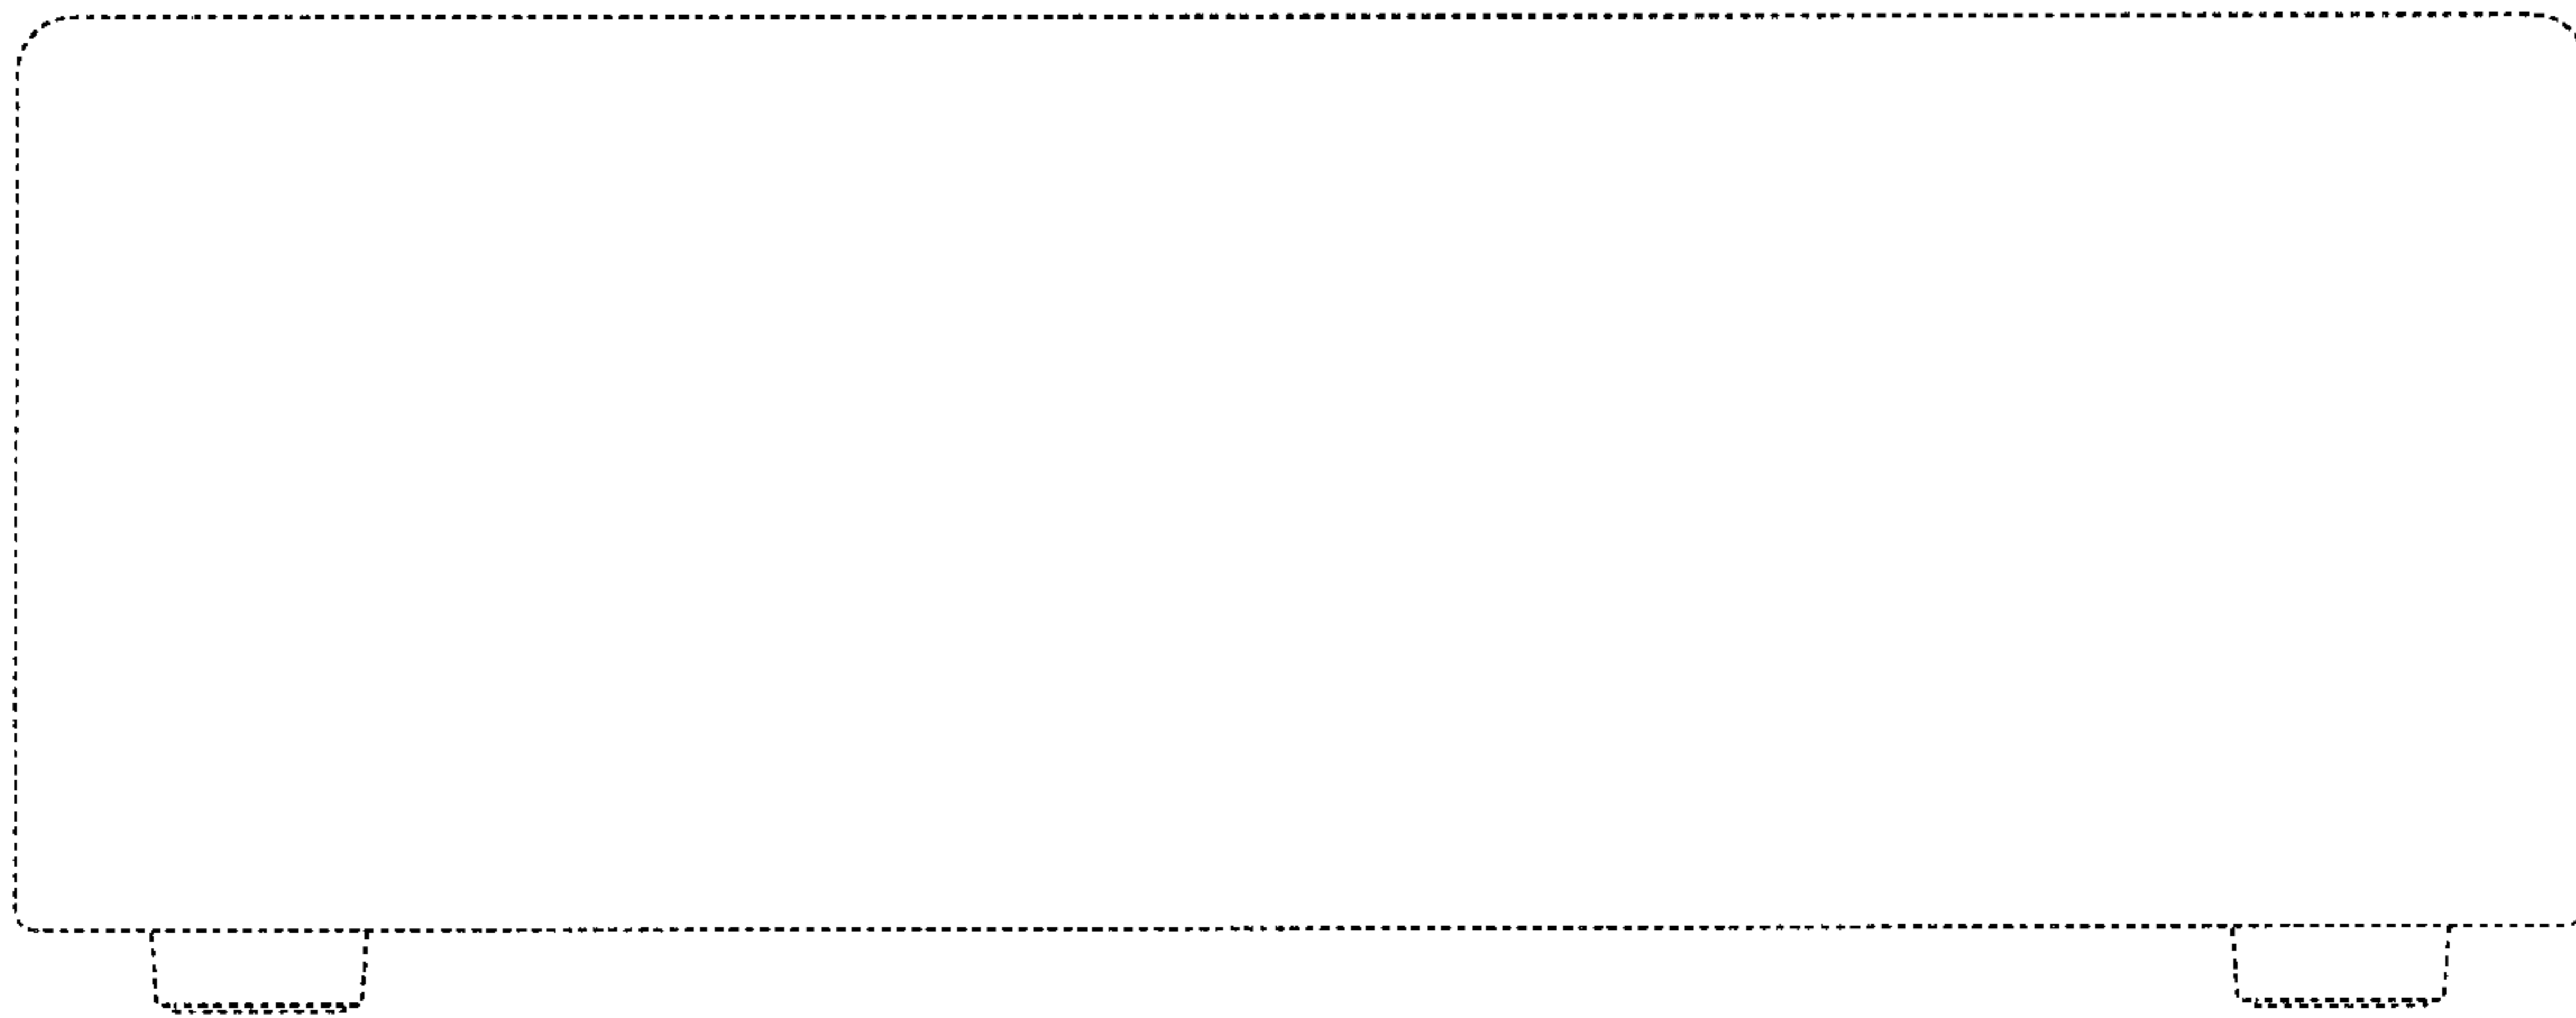


FIG.3

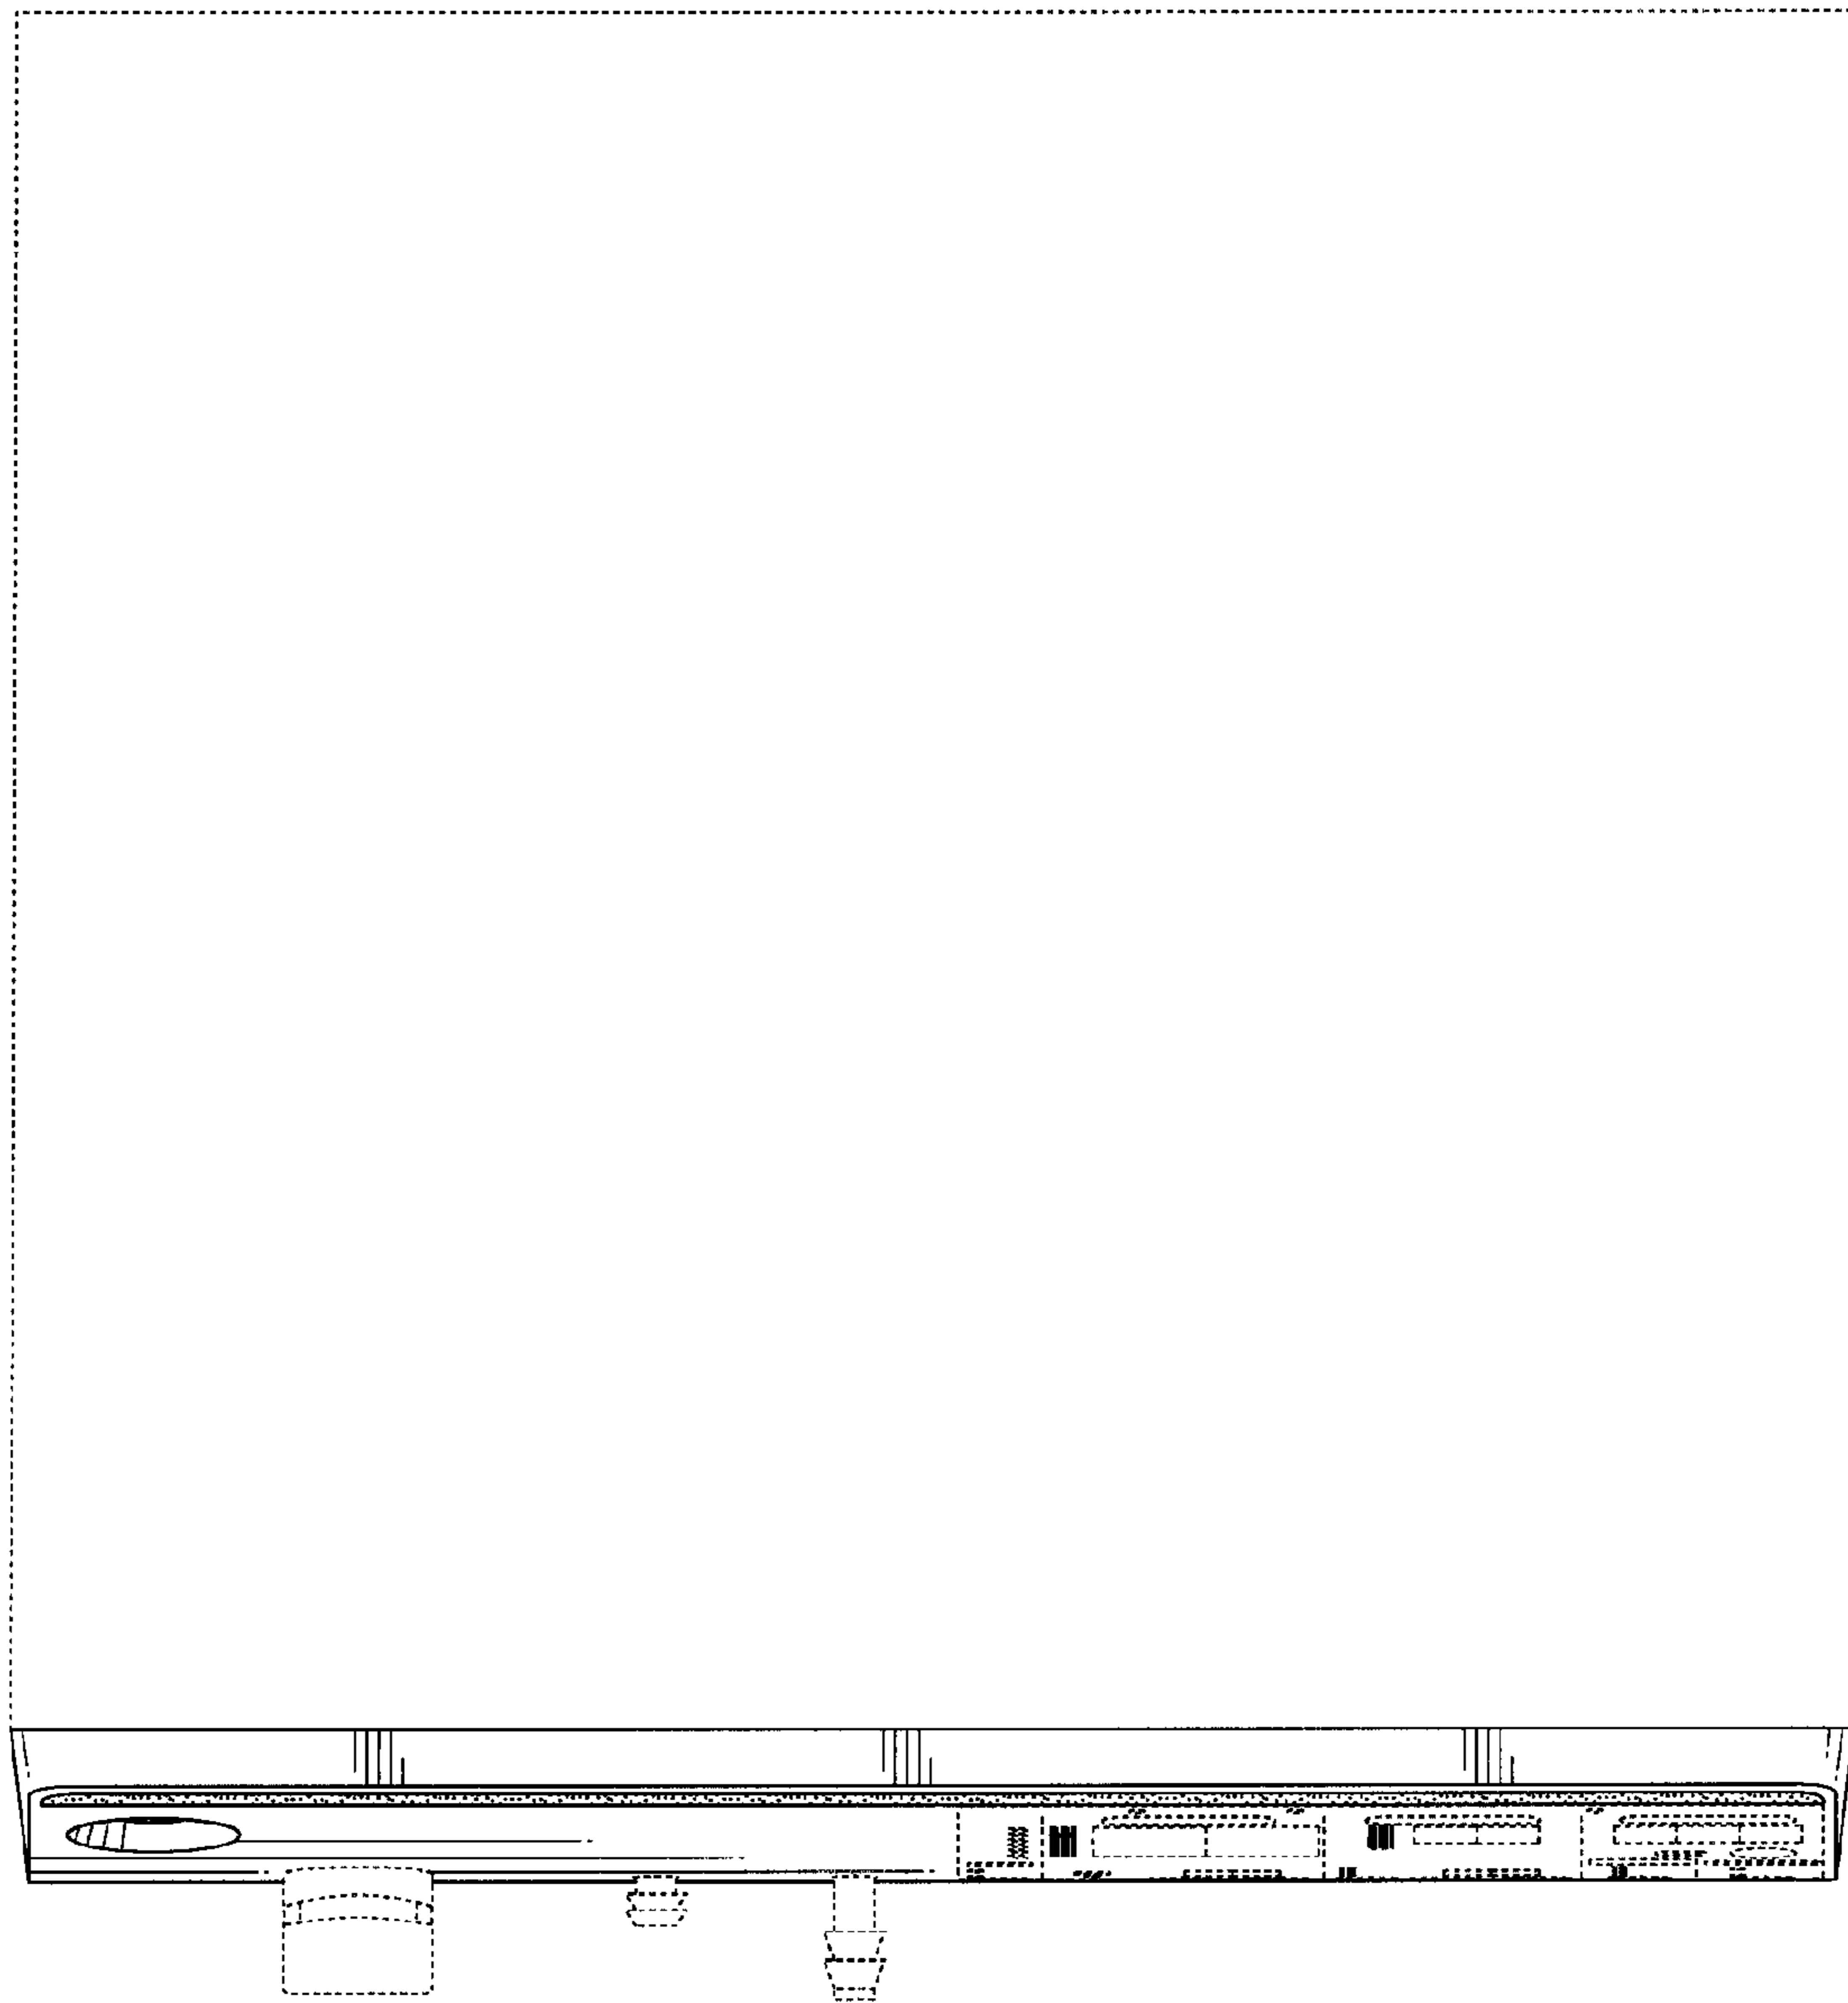


FIG. 4

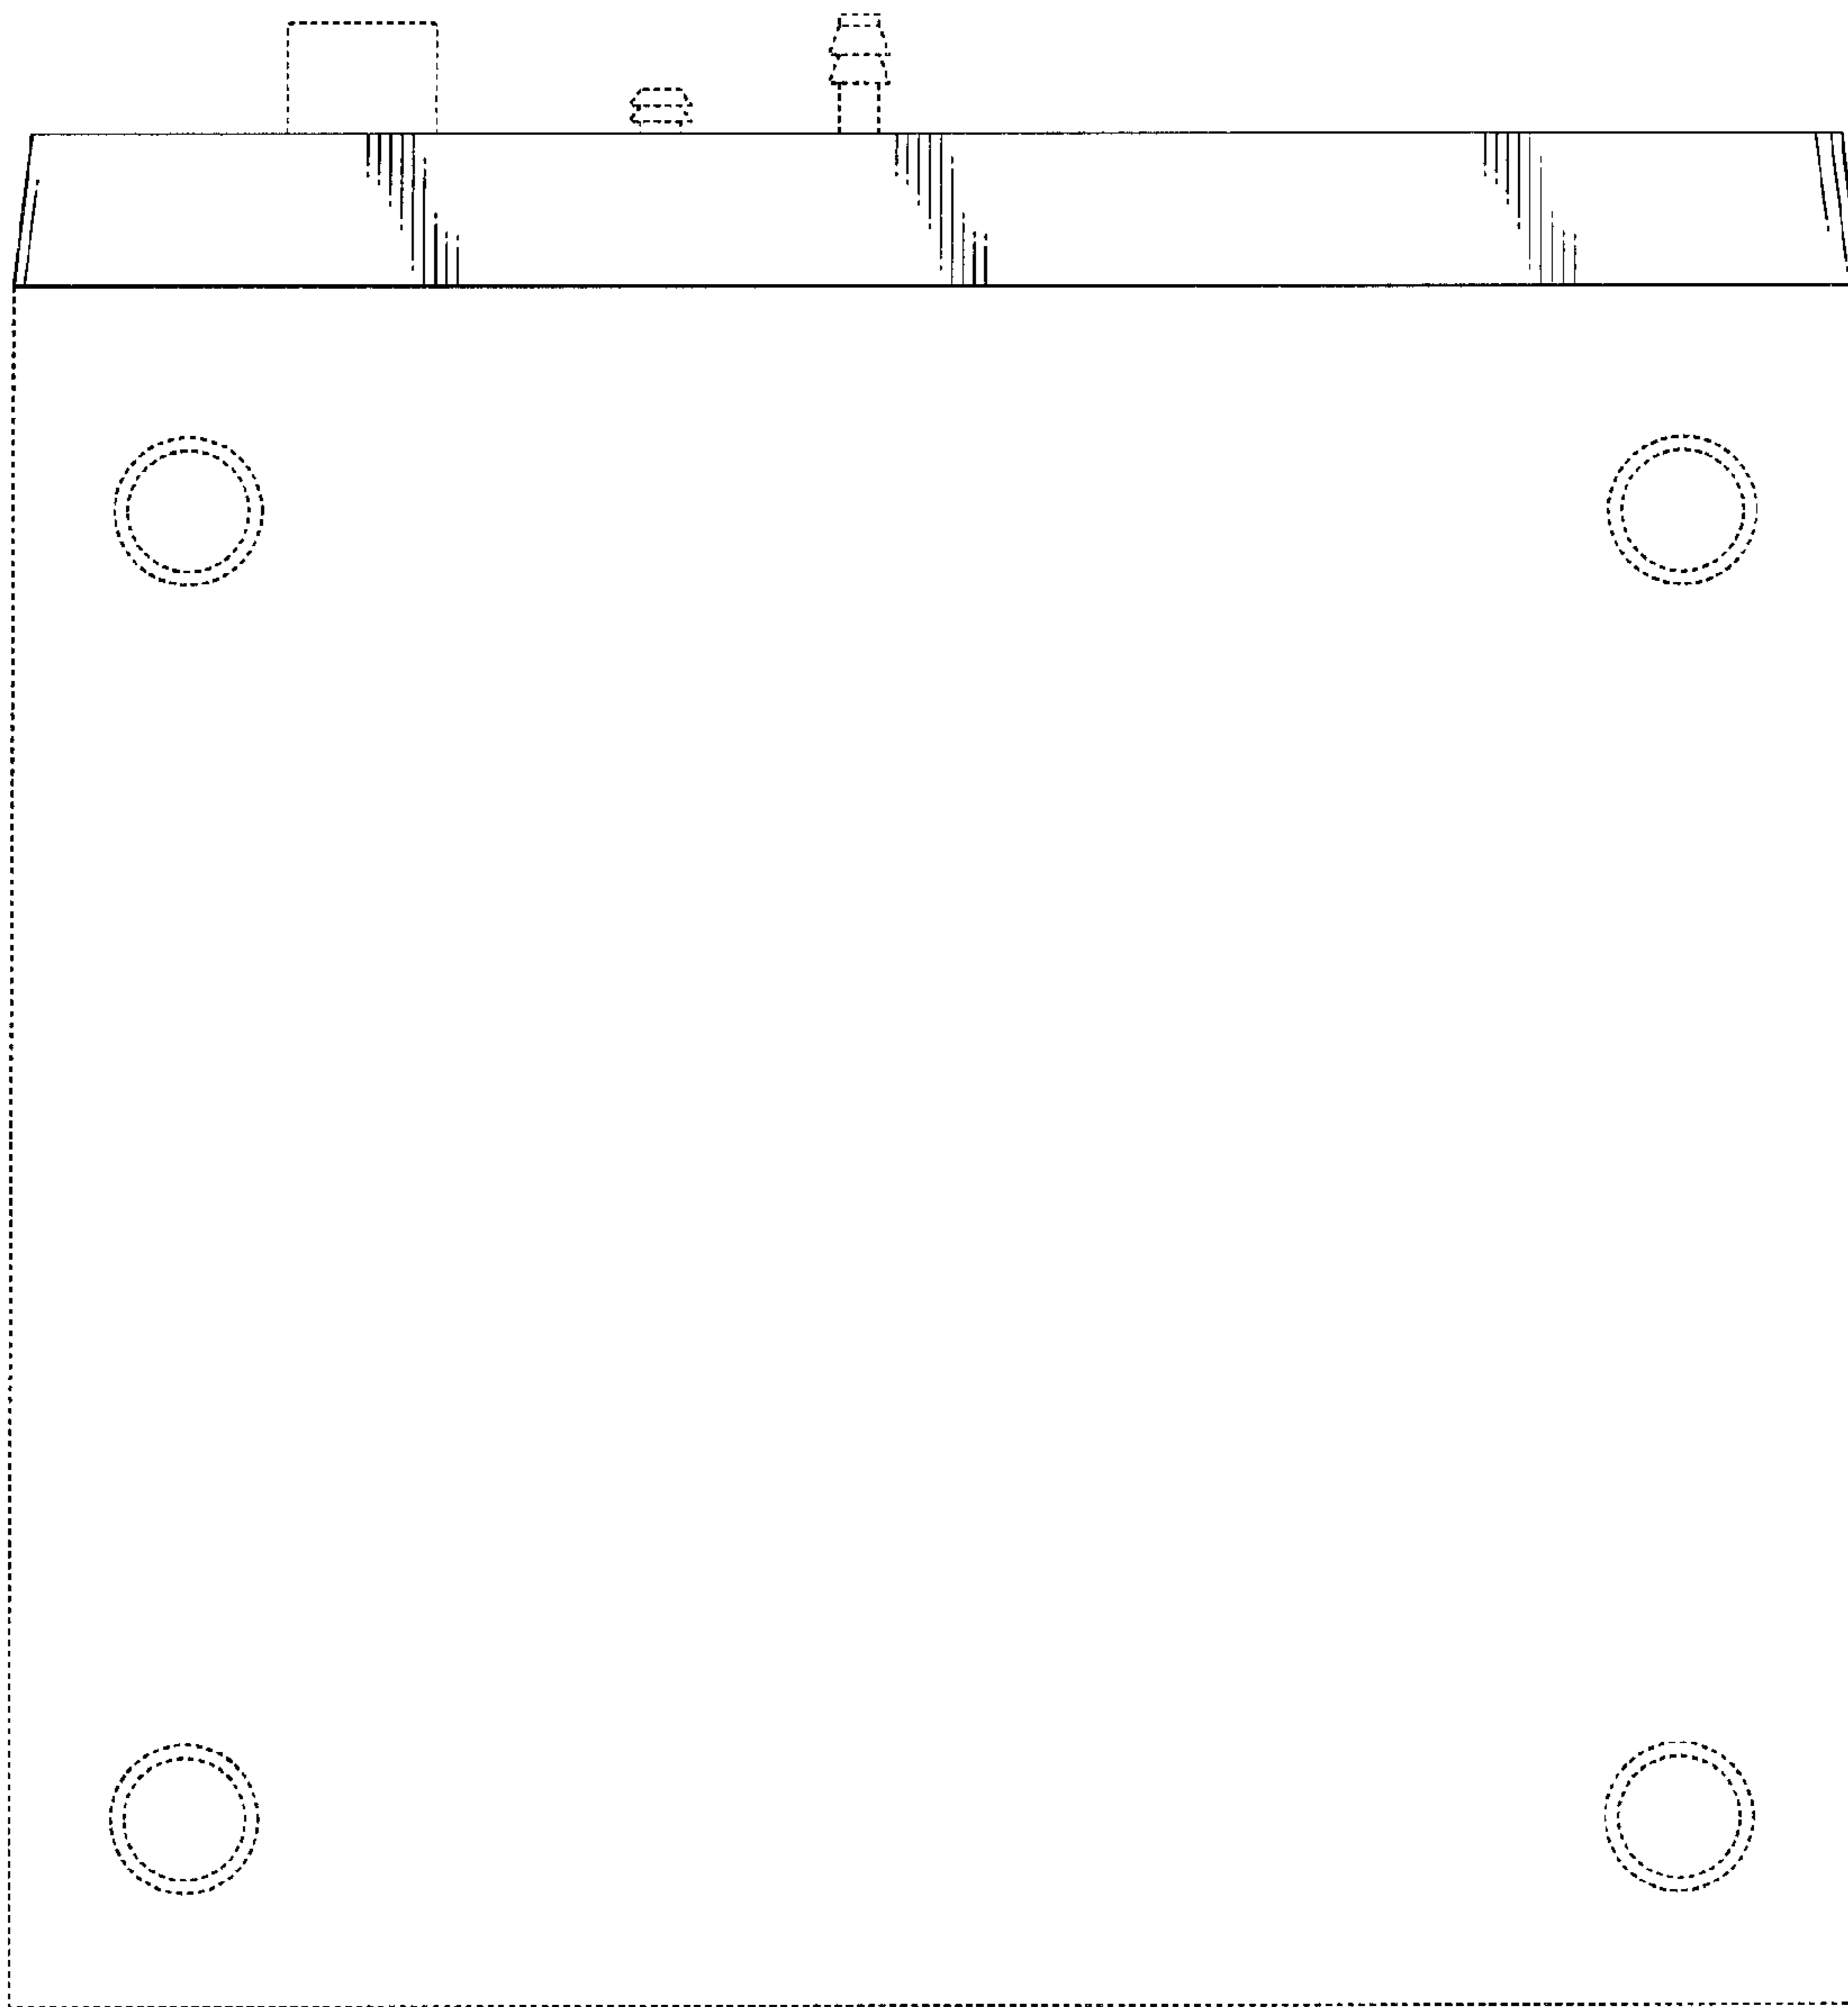


FIG.5

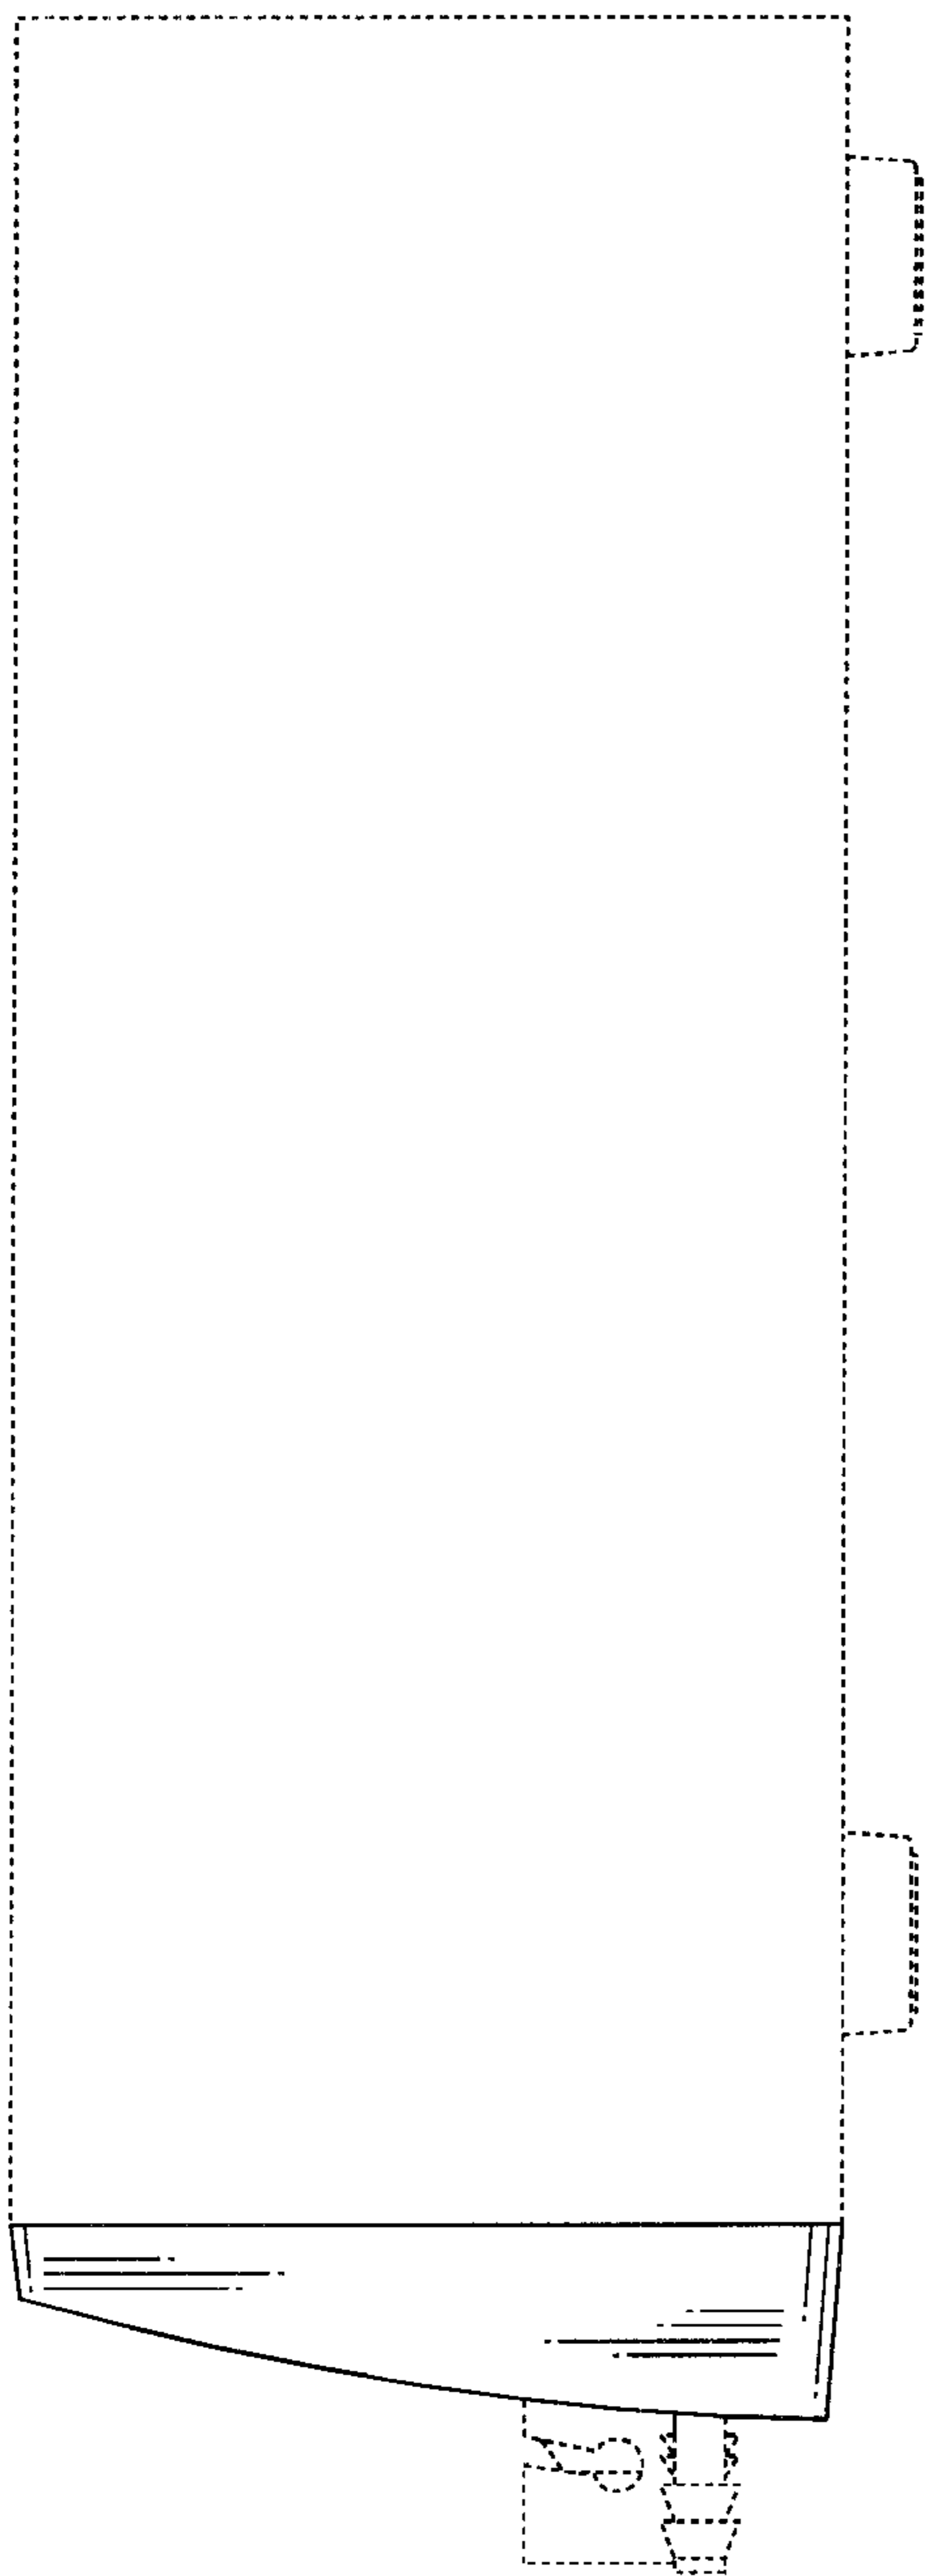


FIG. 6

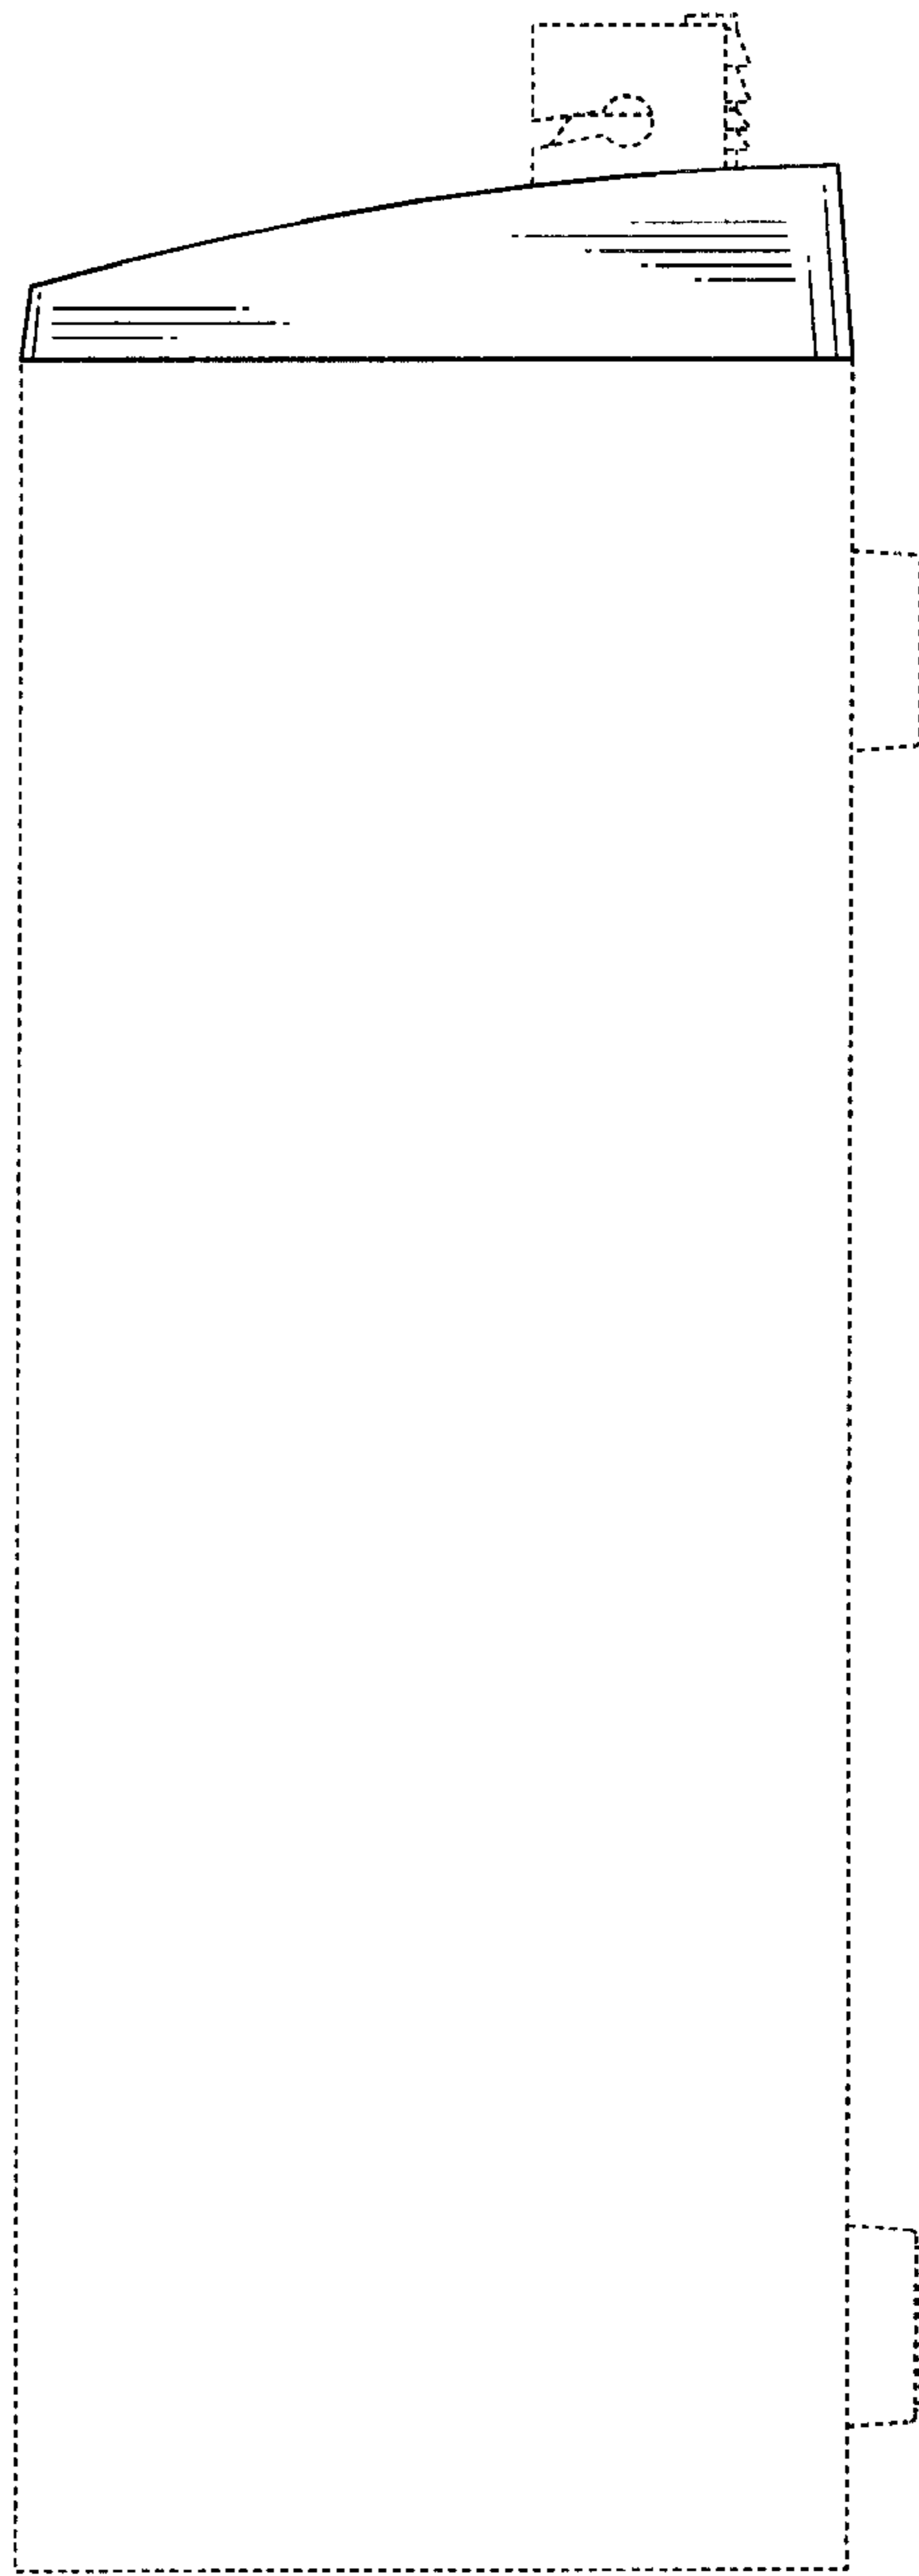


FIG. 7

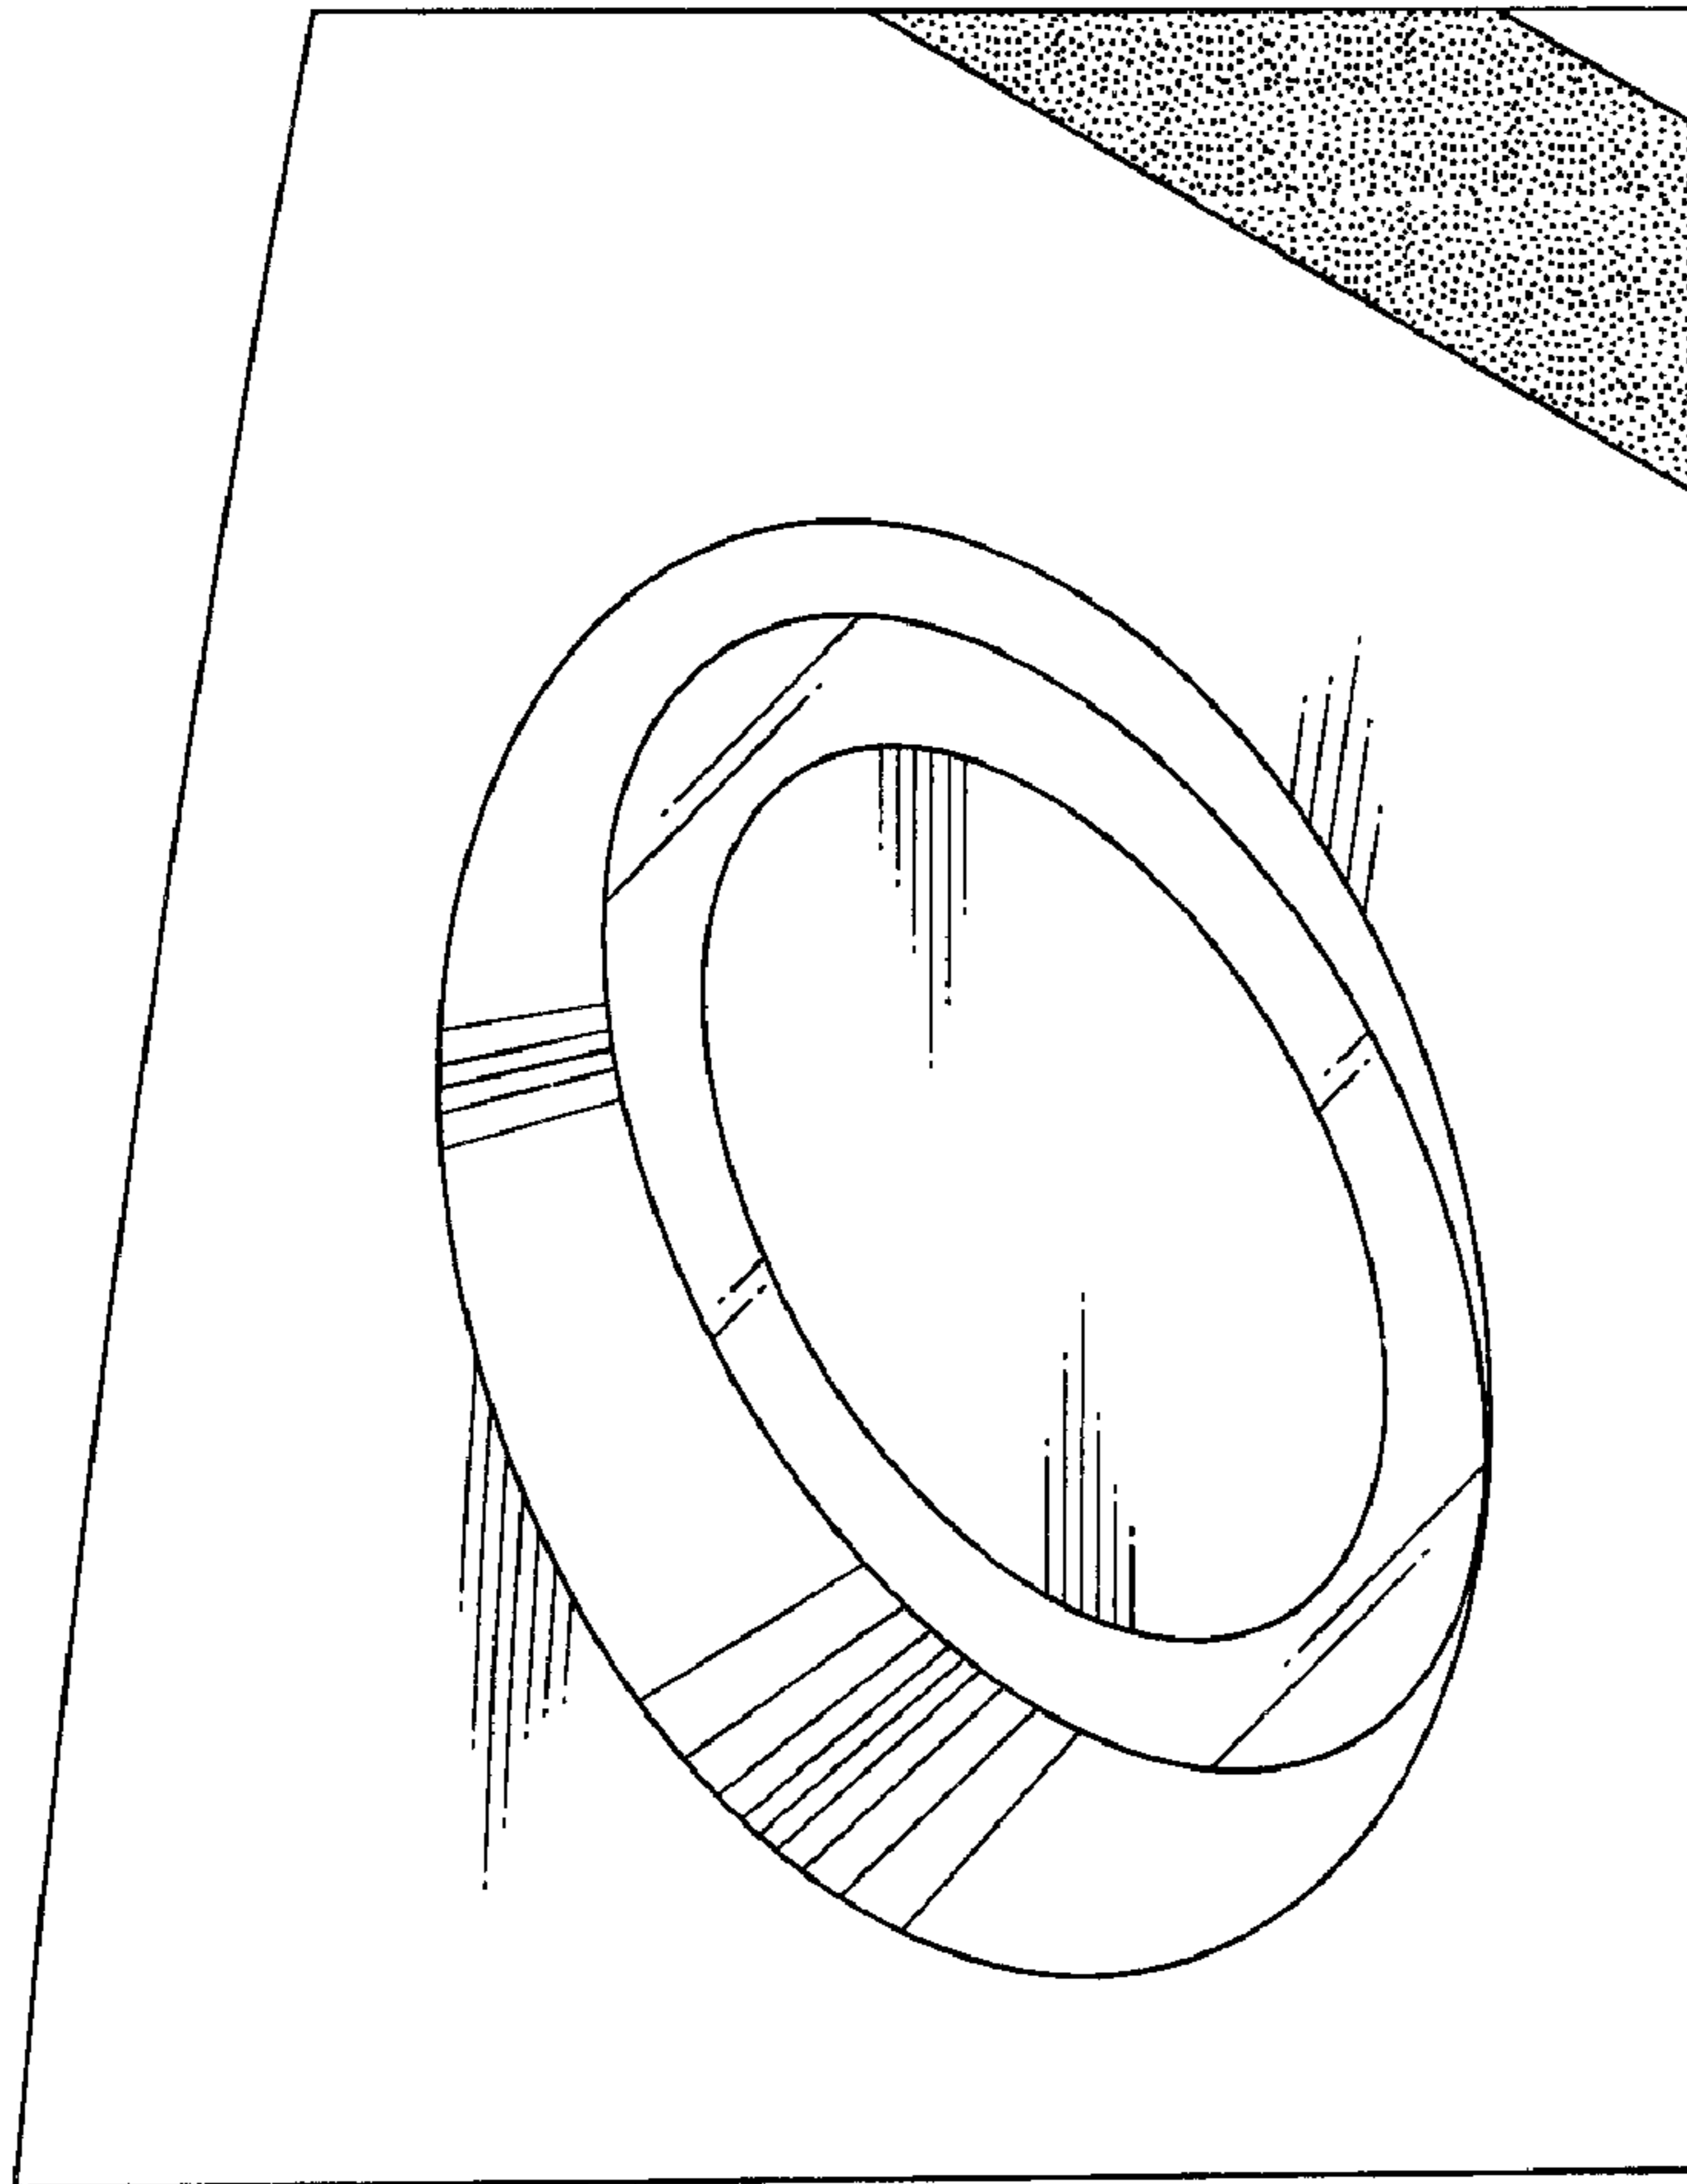


FIG.8