



US00D641472S

(12) **United States Design Patent**  
**Sonoi et al.**

(10) **Patent No.:** **US D641,472 S**

(45) **Date of Patent:** **\*\* \*Jul. 12, 2011**

(54) **DENTAL ROTARY INSTRUMENT**

(75) Inventors: **Shuji Sonoi**, Kyoto (JP); **Osamu Asao**,  
Kyoto (JP); **Masako Shigezawa**, Kyoto  
(JP)

(73) Assignee: **Shofu Inc.**, Kyoto-shi (JP)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/341,373**

(22) Filed: **Aug. 4, 2009**

(30) **Foreign Application Priority Data**

Feb. 4, 2009 (JP) ..... 2009-002285  
Feb. 4, 2009 (JP) ..... 2009-002286  
Feb. 4, 2009 (JP) ..... 2009-002287

(51) **LOC (9) Cl.** ..... **24-02**

(52) **U.S. Cl.** ..... **D24/152**

(58) **Field of Classification Search** ..... D24/152;  
D8/107, 83, 16, 88, 89, 397; D28/65; 606/80;  
417/420, 11; 433/141, 102; 385/176  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D144,607 S \* 5/1946 Charters ..... D24/152  
4,325,606 A \* 4/1982 Ikuno et al. .... 385/76  
4,751,922 A \* 6/1988 DiPietropolo ..... 606/80  
5,122,134 A \* 6/1992 Borzone et al. .... 606/80  
5,499,984 A \* 3/1996 Steiner et al. .... 606/80  
5,947,730 A \* 9/1999 Kaldestad ..... 433/102  
6,258,093 B1 \* 7/2001 Edwards et al. .... 606/80  
6,439,885 B2 \* 8/2002 Antler ..... 433/142

6,520,774 B1 \* 2/2003 Mays ..... 433/102  
7,367,804 B2 \* 5/2008 Lewis ..... 433/141  
D588,270 S \* 3/2009 Hickok ..... D24/152  
D595,850 S \* 7/2009 Koch ..... D24/152  
7,708,767 B2 \* 5/2010 Contiliano et al. .... 606/301  
2005/0186534 A1 \* 8/2005 Roane ..... 433/102  
2010/0248182 A1 \* 9/2010 Sonoi et al. .... 433/166

**FOREIGN PATENT DOCUMENTS**

EM 000968722-0005 \* 9/2008

**OTHER PUBLICATIONS**

German Registered Community Design No. 000679204-0001, Registered Feb. 9, 2007.

\* cited by examiner

*Primary Examiner* — Ian Simmons

*Assistant Examiner* — Wan Laymon

(74) *Attorney, Agent, or Firm* — Oliff & Berridge, PLC

(57) **CLAIM**

The ornamental design for dental rotary instrument, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of a dental rotary instrument showing our new design;

FIG. 2 is a front view thereof, the rear view being identical to the front view;


FIG. 3 is a right-side view thereof, the left-side view being identical to the right-side view;

FIG. 4 is an enlarged top view thereof;

FIG. 5 is an enlarged bottom view thereof; and,

FIG. 6 is an enlarged cross-sectional view thereof taken along the line 6—6 of FIG. 2.

**1 Claim, 2 Drawing Sheets**

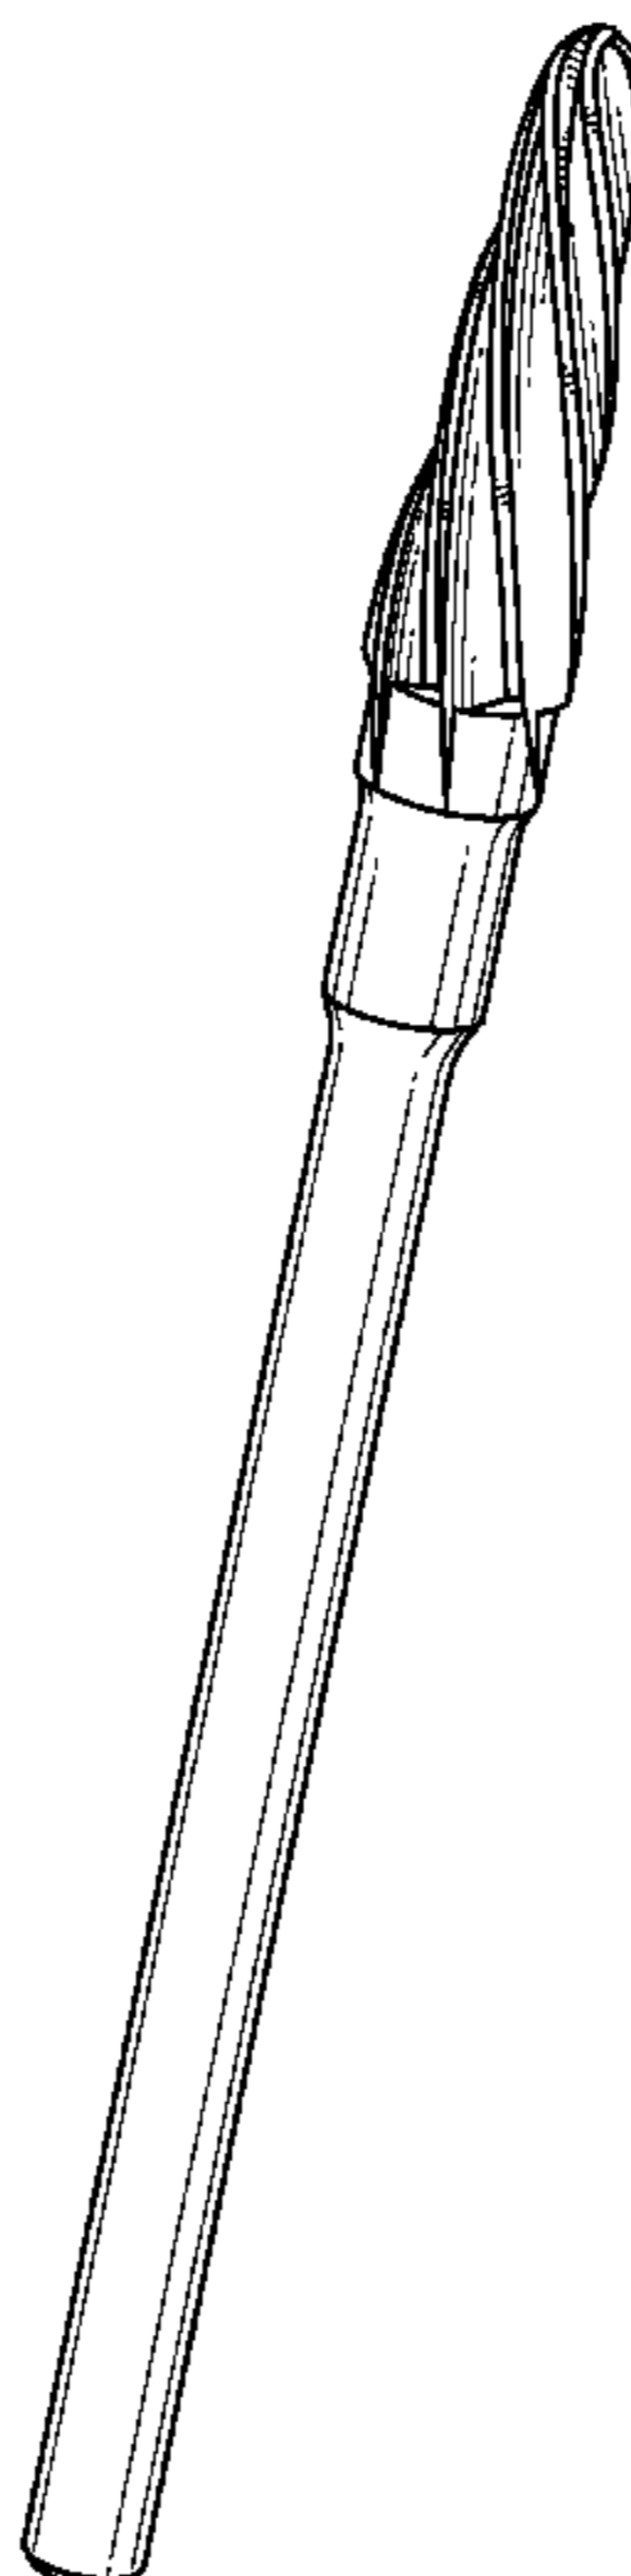

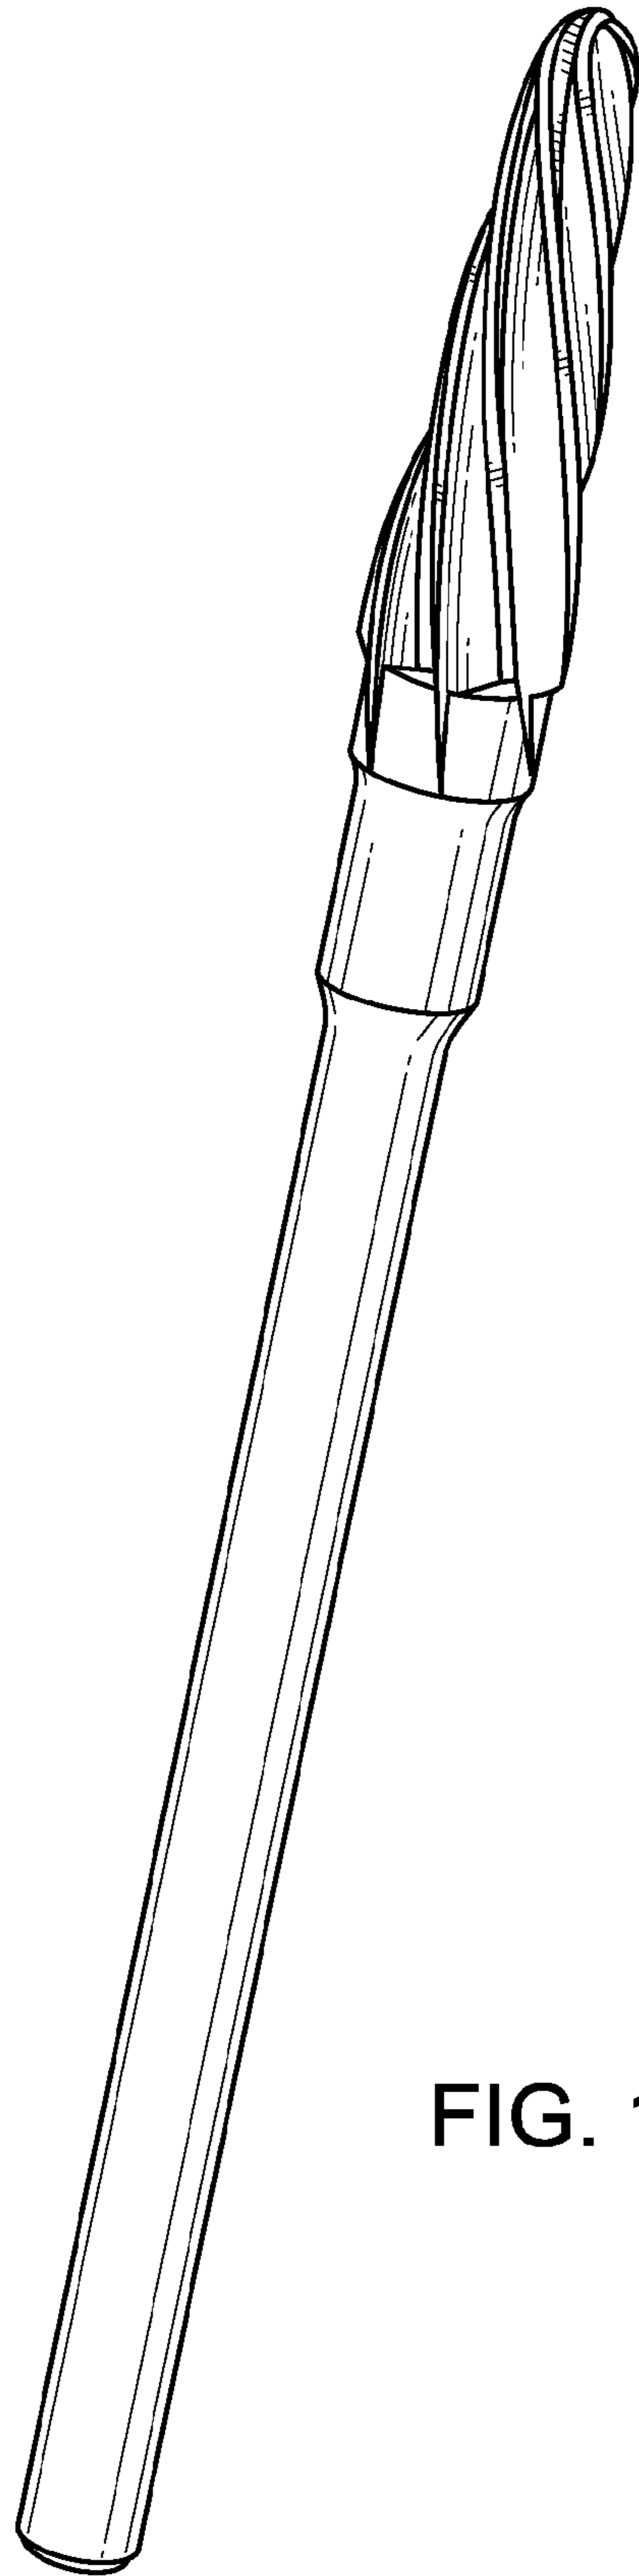


FIG. 1

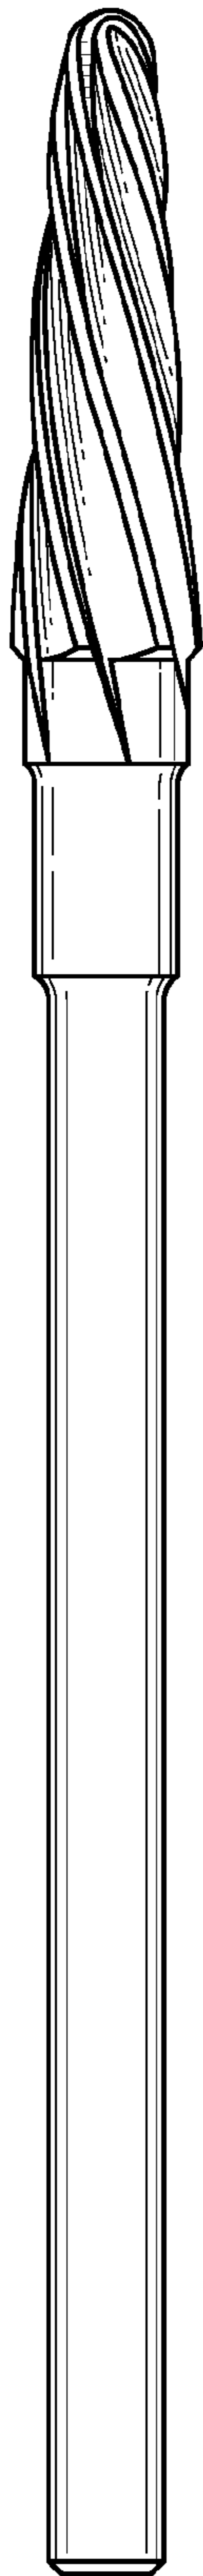


FIG. 3

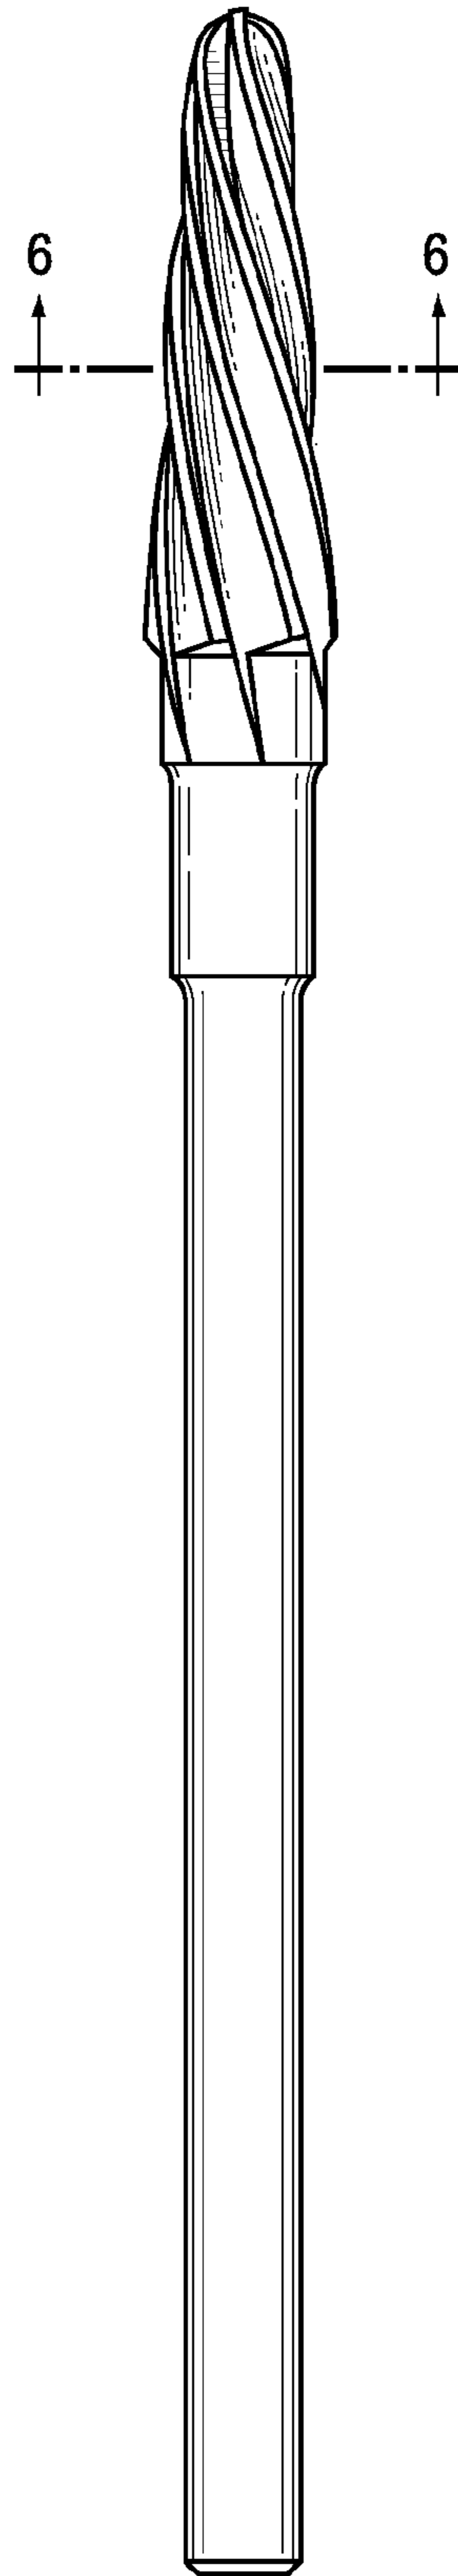


FIG. 2

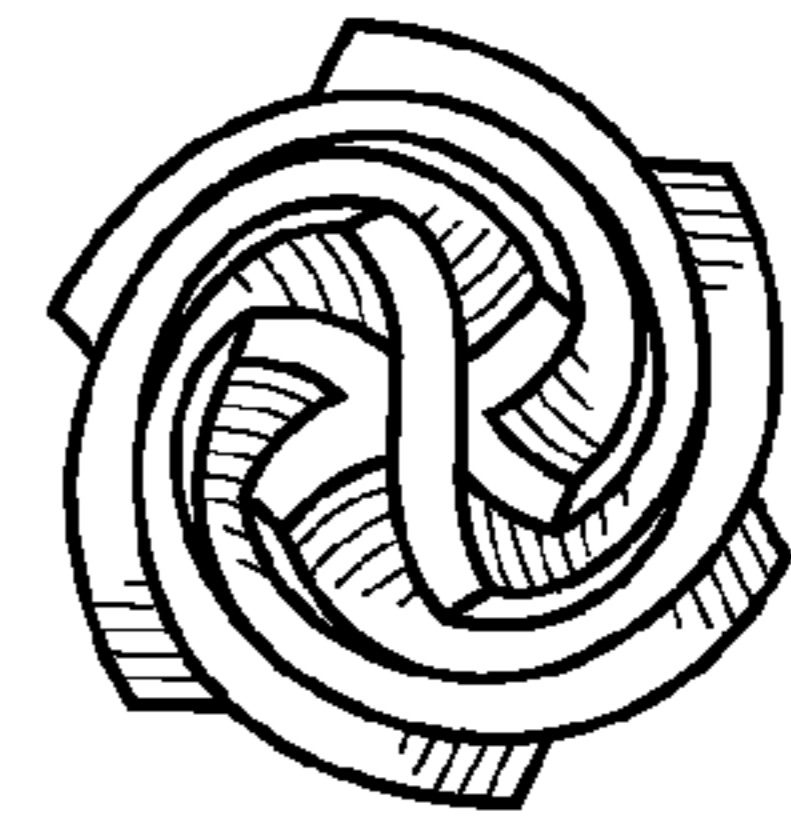


FIG. 4

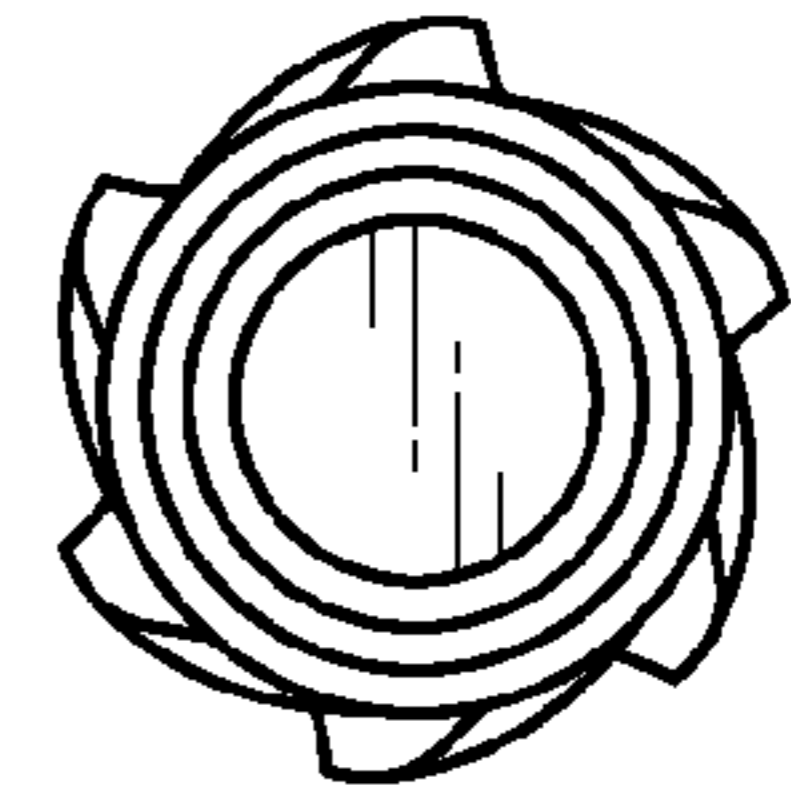


FIG. 5

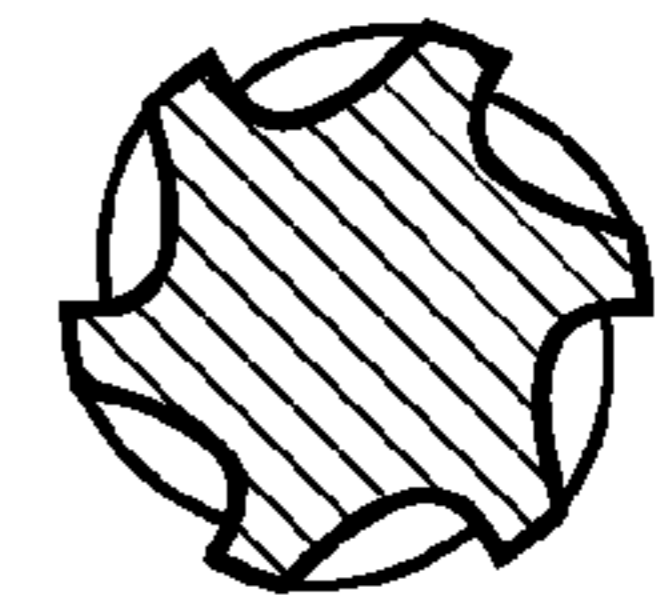


FIG. 6