



US00D645147S

(12) **United States Design Patent**  
**Ruf**

(10) **Patent No.:** **US D645,147 S**

(45) **Date of Patent:** **\*\* Sep. 13, 2011**

(54) **SAFETY LANCET**

(75) Inventor: **Christopher J. Ruf**, Marietta, GA (US)

(73) Assignee: **Facet Technologies, LLC**, Kennesaw, GA (US)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/378,921**

(22) Filed: **Nov. 11, 2010**

(51) **LOC (9) Cl.** ..... **24-02**

(52) **U.S. Cl.** ..... **D24/147**

(58) **Field of Classification Search** ..... D24/133,  
D24/130, 113, 114, 146-147; 600/385, 573,  
600/583; 606/167, 172, 181-185; 210/453  
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,449,529	A	5/1984	Burns et al.	
4,616,649	A	10/1986	Burns	
4,624,253	A	11/1986	Burns	
5,106,379	A	4/1992	Leap	
D336,335	S *	6/1993	Poulsen	..... D24/147
5,356,420	A	10/1994	Czernecki et al.	
5,366,469	A	11/1994	Steg et al.	
5,397,334	A	3/1995	Schenk et al.	
5,421,347	A	6/1995	Enstrom	
5,439,473	A	8/1995	Jorgensen	

(Continued)

FOREIGN PATENT DOCUMENTS

WO 2006004664 A1 1/2006

OTHER PUBLICATIONS

Microtainer Contact-Activated Lancets; at least as early as Nov. 10, 2009.

(Continued)

*Primary Examiner* — Ian Simmons

*Assistant Examiner* — Carissa C Fitts

(74) *Attorney, Agent, or Firm* — Gardner Groff Greenwald & Villanueva, PC

(57) **CLAIM**

The ornamental design for a safety lancet, substantially as shown and described.

**DESCRIPTION**

FIG. 1 is a first perspective view of a safety lancet according to the design.

FIG. 2 is a second perspective view of the safety lancet of FIG. 1.

FIG. 3 is a first side view of the safety lancet of FIG. 1.

FIG. 4 is a second side view of the safety lancet of FIG. 1.

FIG. 5 is a first end view of the safety lancet of FIG. 1.

FIG. 6 is a second end view of the safety lancet of FIG. 1.

FIG. 7 is a top view of the safety lancet of FIG. 1.

FIG. 8 is a bottom view of the safety lancet of FIG. 1.

FIG. 9 is a first perspective view of the safety lancet of FIG. 1, in a second state having a cap portion removed.

FIG. 10 is a second perspective view of the safety lancet of FIG. 1 with the cap removed.

FIG. 11 is a first side view of the safety lancet of FIG. 1 with the cap removed.

FIG. 12 is a second side view of the safety lancet of FIG. 1 with the cap removed.

FIG. 13 is a first end view of the safety lancet of FIG. 1 with the cap removed.


FIG. 14 is a second end view of the safety lancet of FIG. 1 with the cap removed.

FIG. 15 is a top view of the safety lancet of FIG. 1 with the cap removed; and,

FIG. 16 is a bottom view of the safety lancet of FIG. 1 with the cap removed.

Portions shown in broken lines are for illustrative purposes only and form no part of the claimed design.

**1 Claim, 10 Drawing Sheets**

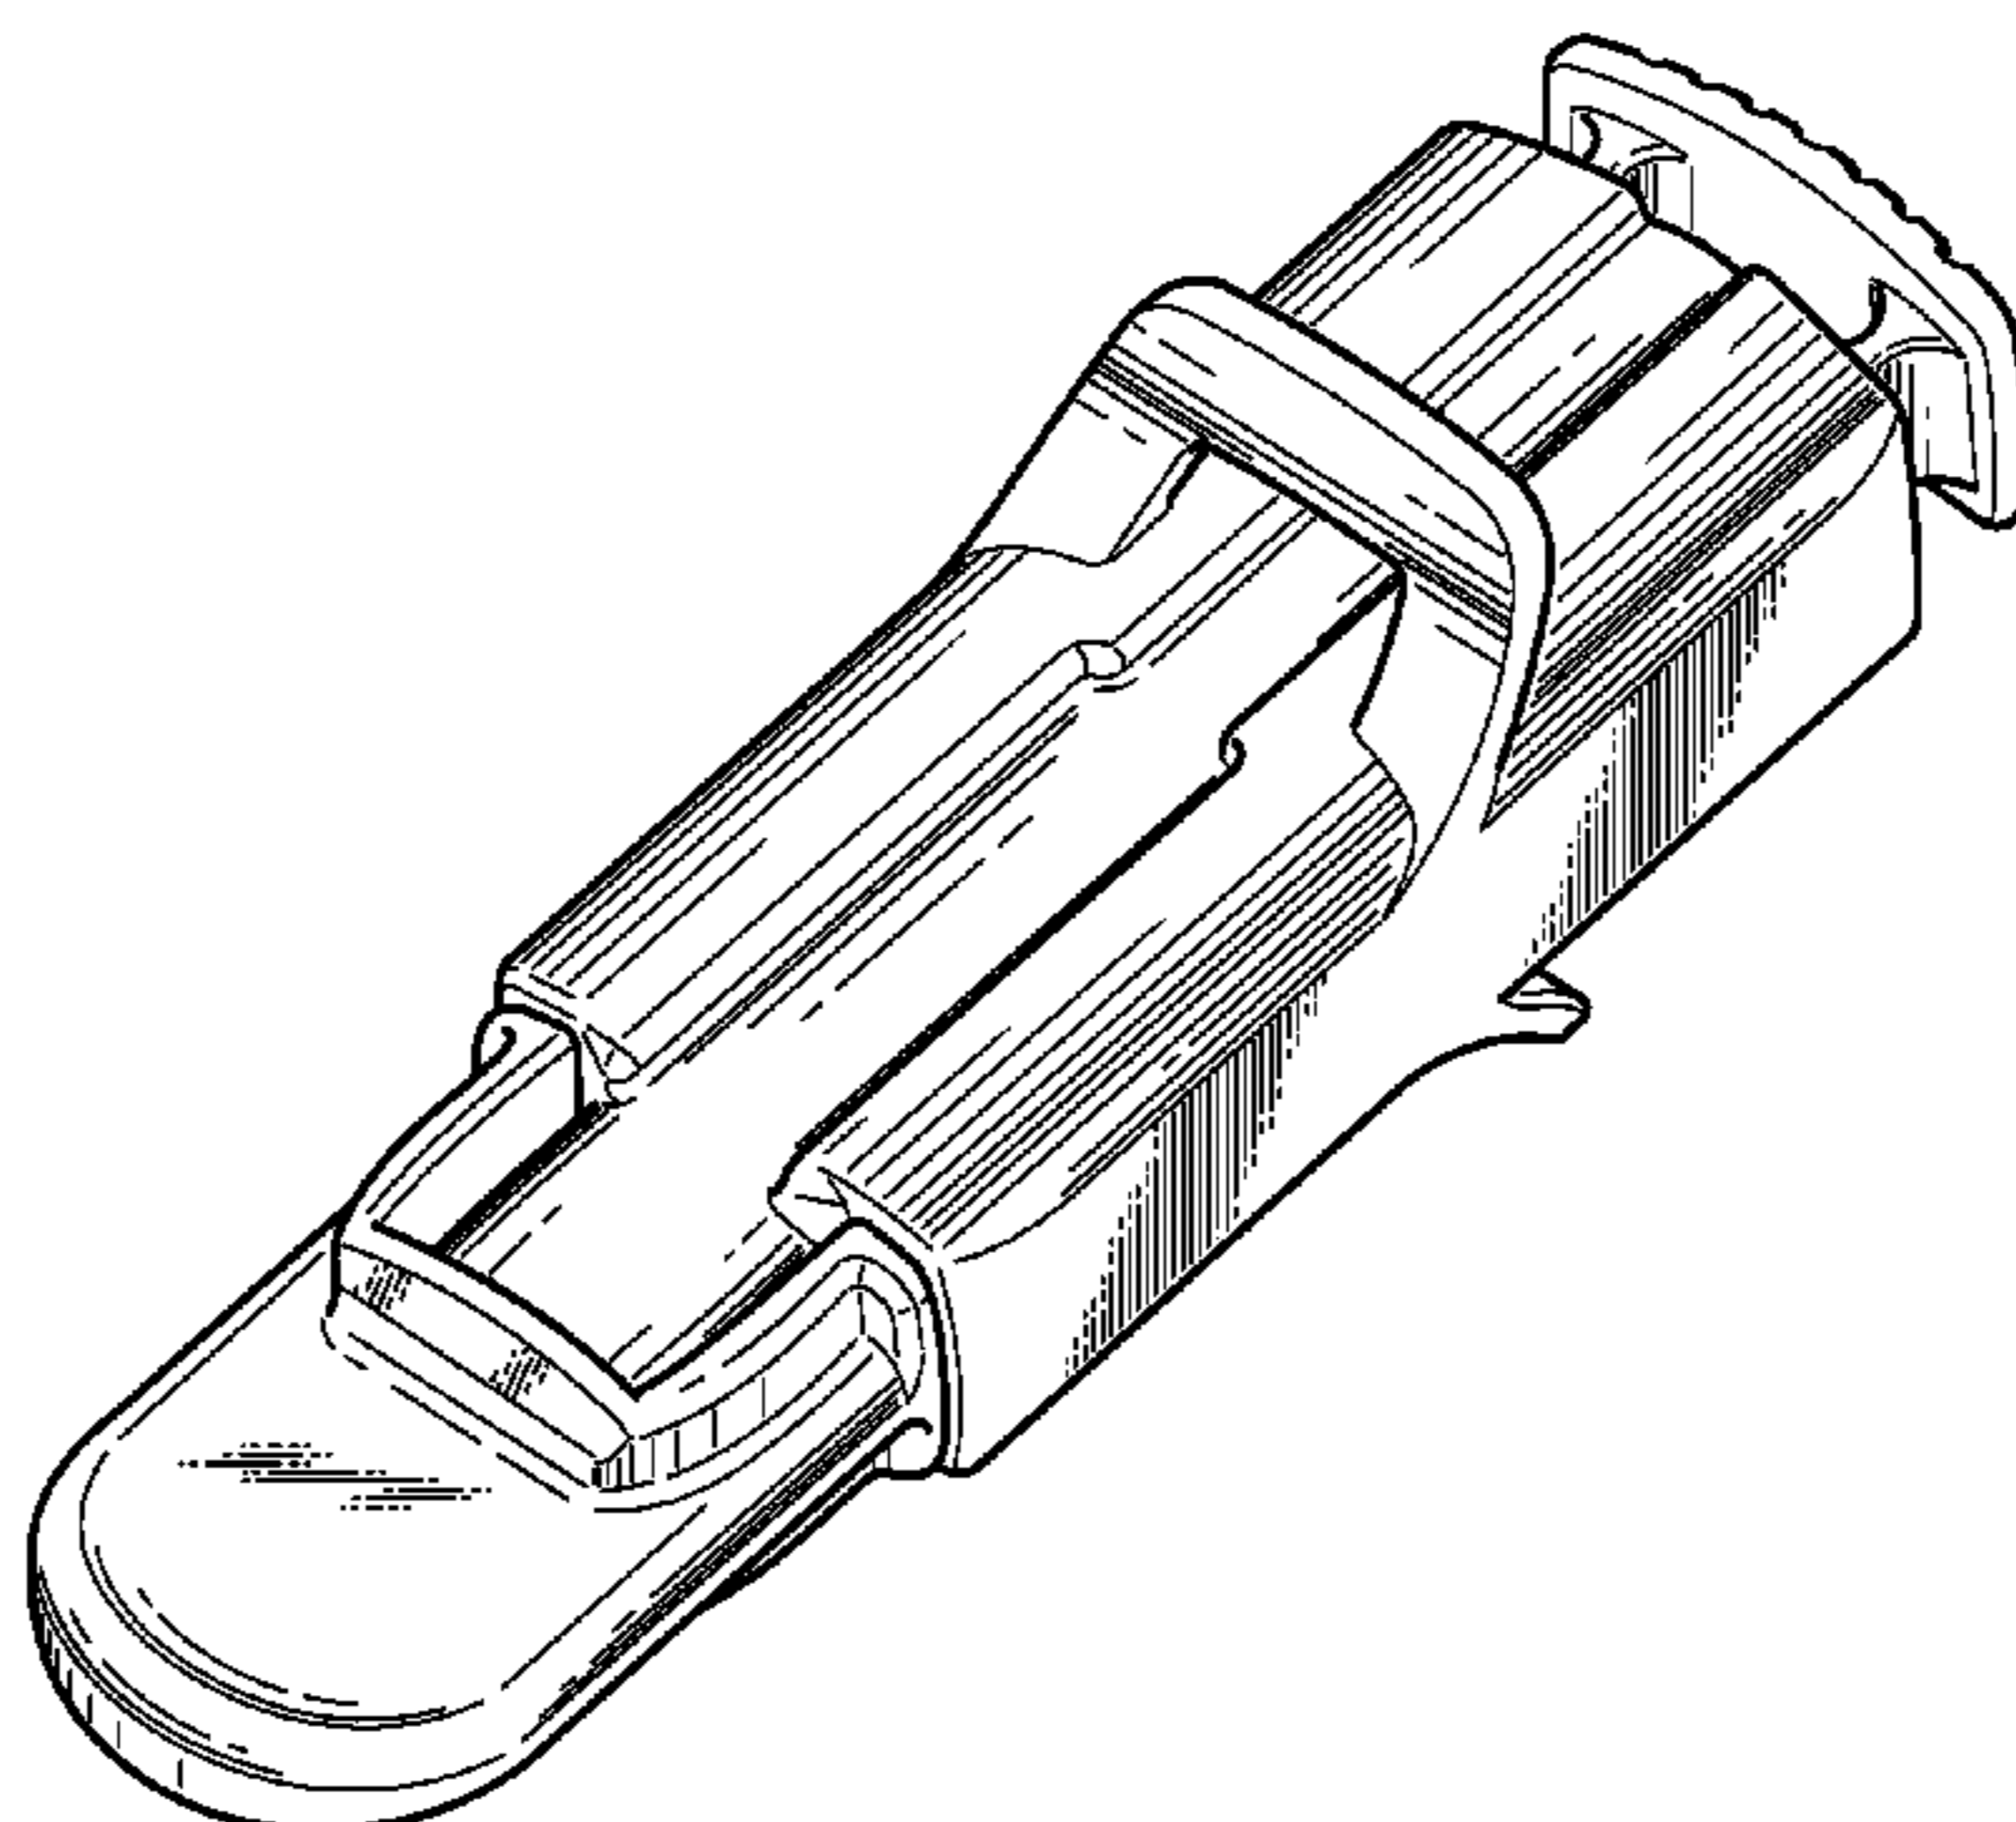

U.S. PATENT DOCUMENTS


D374,284	S *	10/1996	Stone et al. ....	D24/145
D374,285	S *	10/1996	DeFonzo et al. ....	D24/145
D376,649	S *	12/1996	Kim .....	D24/147
5,628,765	A	5/1997	Morita	
5,954,738	A *	9/1999	LeVaughn et al. ....	606/181
6,248,120	B1	6/2001	Wyszogrodzki	
6,613,064	B2	9/2003	Rutynowski et al.	
6,997,936	B2	2/2006	Marshall	
7,322,997	B2	1/2008	Shi	
7,357,808	B2	4/2008	Kennedy	
D621,044	S *	8/2010	Trissel et al. ....	D24/147
D628,293	S *	11/2010	Ruf .....	D24/146
2006/0052809	A1	3/2006	Karbowniczek et al.	
2008/0082117	A1 *	4/2008	Ruf .....	606/182

OTHER PUBLICATIONS


Medlance Plus Lancets; at least as early as Nov. 11, 2009.  
 Medlance Lancets; at least as early as Nov. 10, 2009.  
 Safe-T Pro Lancet; at least as early as Nov. 10, 2009.  
 Acti-Lance Lancets; at least as early as Nov. 10, 2009.  
 MediSafe SOLO Lancet; at least as early as Nov. 10, 2009.  
 Safe-T-Pro Uno Lancet; at least as early as Nov. 10, 2009.  
 Haemolance Plus Lancets; at least as early as Nov. 10, 2009.  
 Haemolance Lancets; at least as early as Nov. 10, 2009.  
 Prolance Lancets; at least as early as Nov. 10, 2009.  
 Unistik 2 Lancets; at least as early as Nov. 10, 2009.  
 Unistik 3 Lancets; at least as early as Nov. 10, 2009.  
 Surgilance Safety Lancets; at least as early as Nov. 10, 2009.  
 Safe-T-Pro Plus Lancet; at least as early as Nov. 10, 2009.

Single-Let Lancet; at least as early as Nov. 10, 2009.  
 Carelet Lancets; at least as early as Nov. 10, 2009.  
 BD Safety Flow Lancets; at least as early as Nov. 10, 2009.  
 EZ-Lance Lancets; at least as early as Nov. 10, 2009.  
 Monolettor Safety Lancets; at least as early as Nov. 11, 2009.  
 SteriLance PA Lancets; at least as early as Nov. 10, 2009.  
 SteriLance AD Lancets; at least as early as Nov. 10, 2009.  
 SteriLance BA Lancets; at least as early as Nov. 10, 2009.  
 Safelance Lancets; at least as early as Nov. 10, 2009.  
 Fingerpit Lancet; at least as early as Nov. 10, 2009.  
 Misawa Lancet; at least as early as Nov. 10, 2009.  
 Bullseye Safety Lancets; at least as early as Nov. 10, 2009.  
 Al-Pit Lancet; at least as early as Nov. 10, 2009.  
 Stat-Let Auto Lancets; at least as early as Nov. 10, 2009.  
 Auto Lancets; at least as early as Nov. 10, 2009.  
 Gentle-let 1 Lancet; at least as early as Nov. 10, 2009.  
 Single Stick Lancet; at least as early as Nov. 10, 2009.  
 Simplet Lancet; at least as early as Nov. 10, 2009.  
 EZ-Let Lancets; at least as early as Nov. 10, 2009.  
 Lite-Stik Safety Lancet; at least as early as Nov. 10, 2009.  
 Safelet Lancet; at least as early as Nov. 10, 2009.  
 Worldlet Lancet; at least as early as Nov. 10, 2009.  
 FUTUMEDS Safety Lancet; at least as early as Nov. 10, 2009.  
 Medsun Safety Lancet; at least as early as Nov. 10, 2009.  
 Ningbo Medsun Medical; at least as early as Nov. 10, 2009.  
 Suzhou Zhenwu Medical Sutures & Suture Needles; at least as early as Nov. 10, 2009.


\* cited by examiner

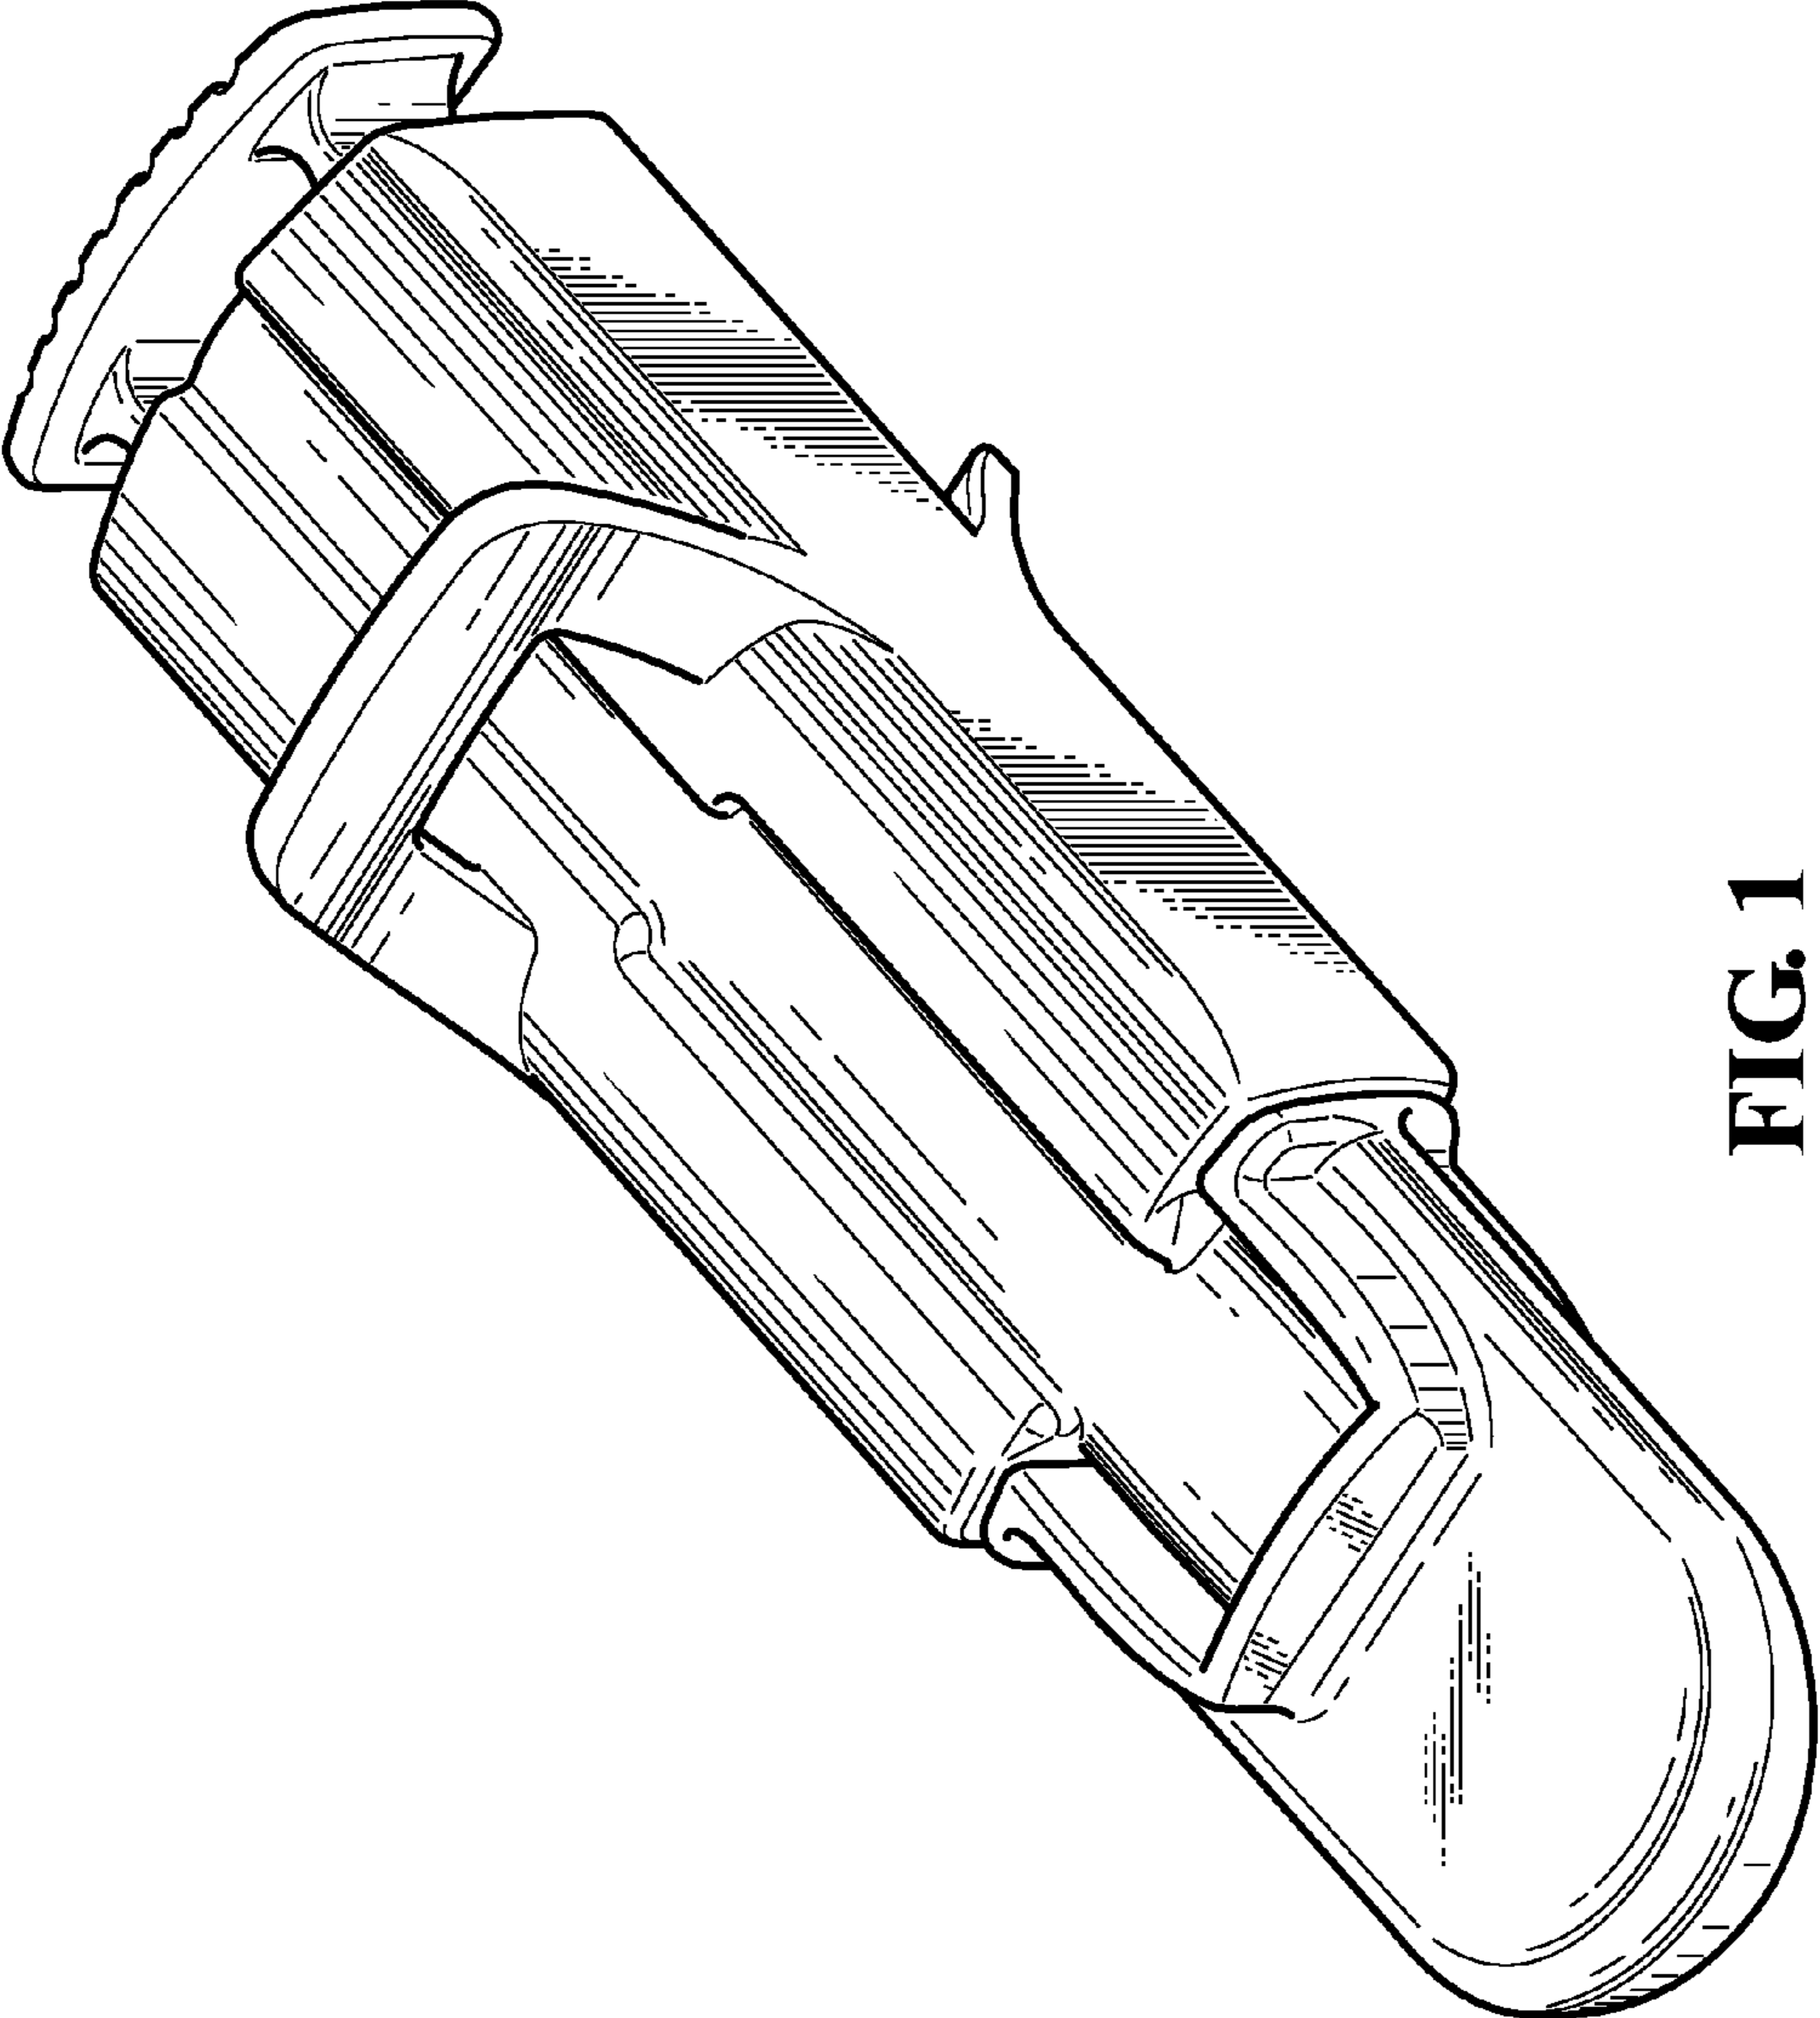


**FIG. 1**

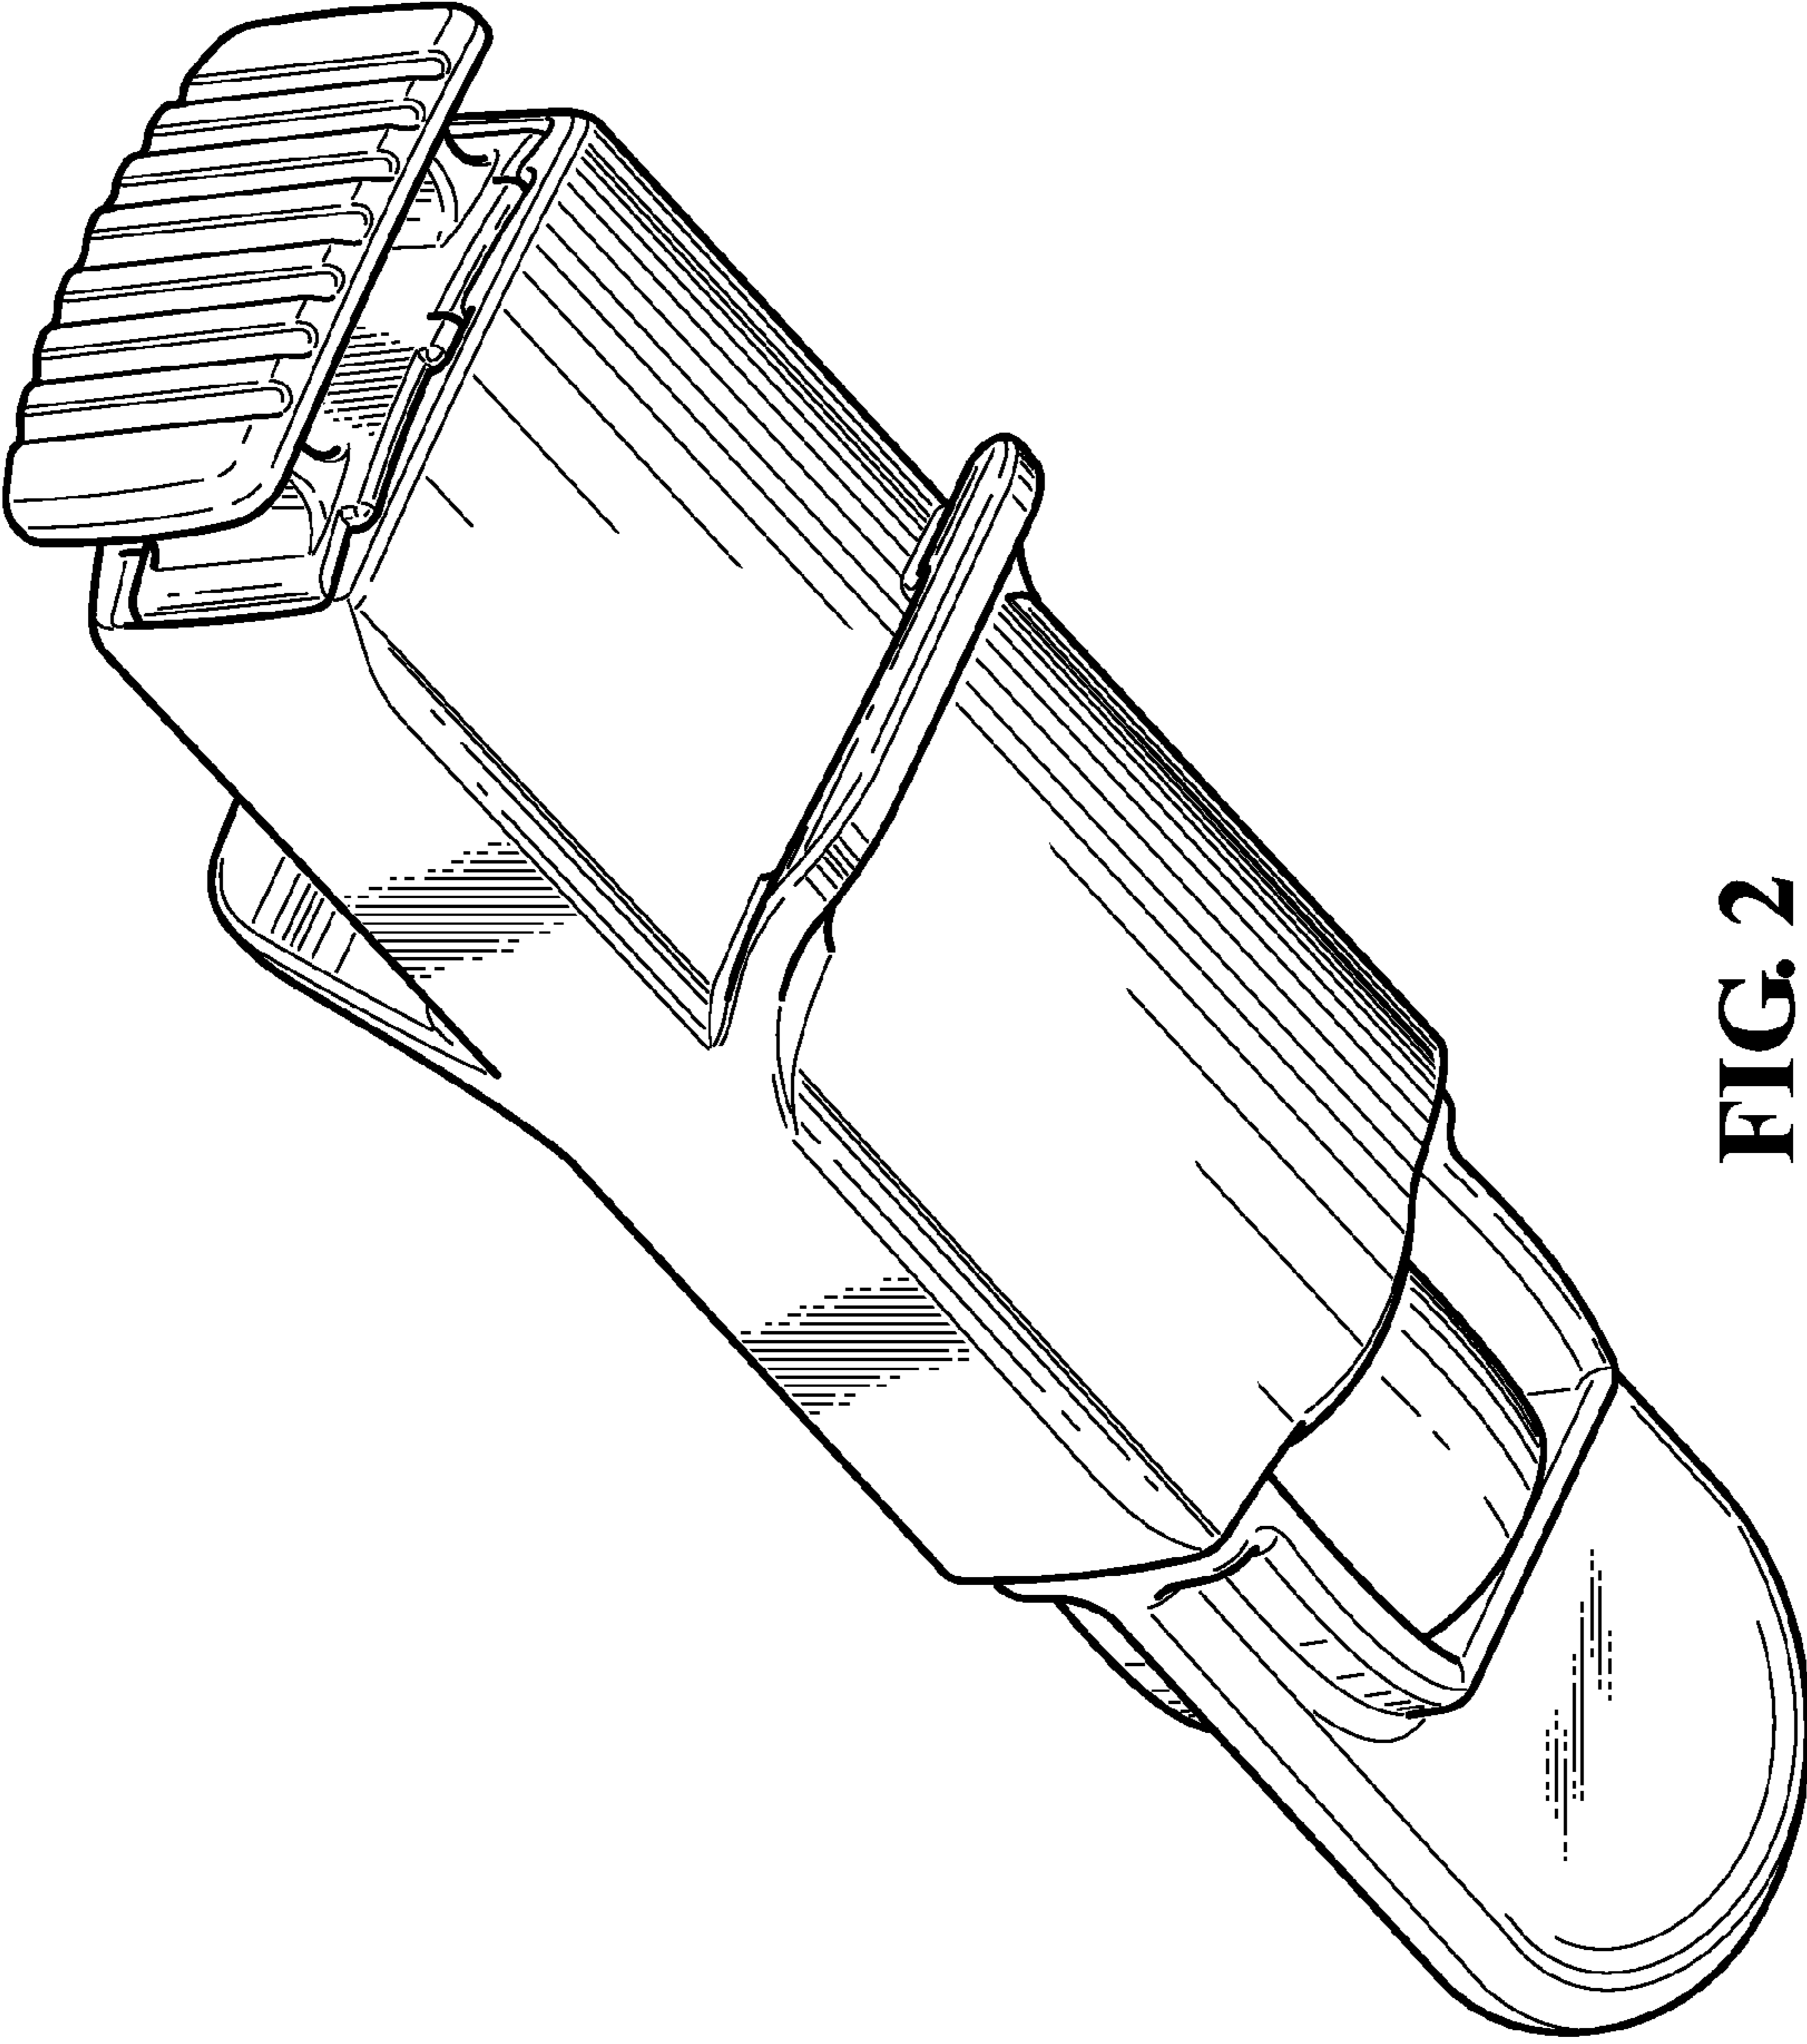


**FIG. 2**

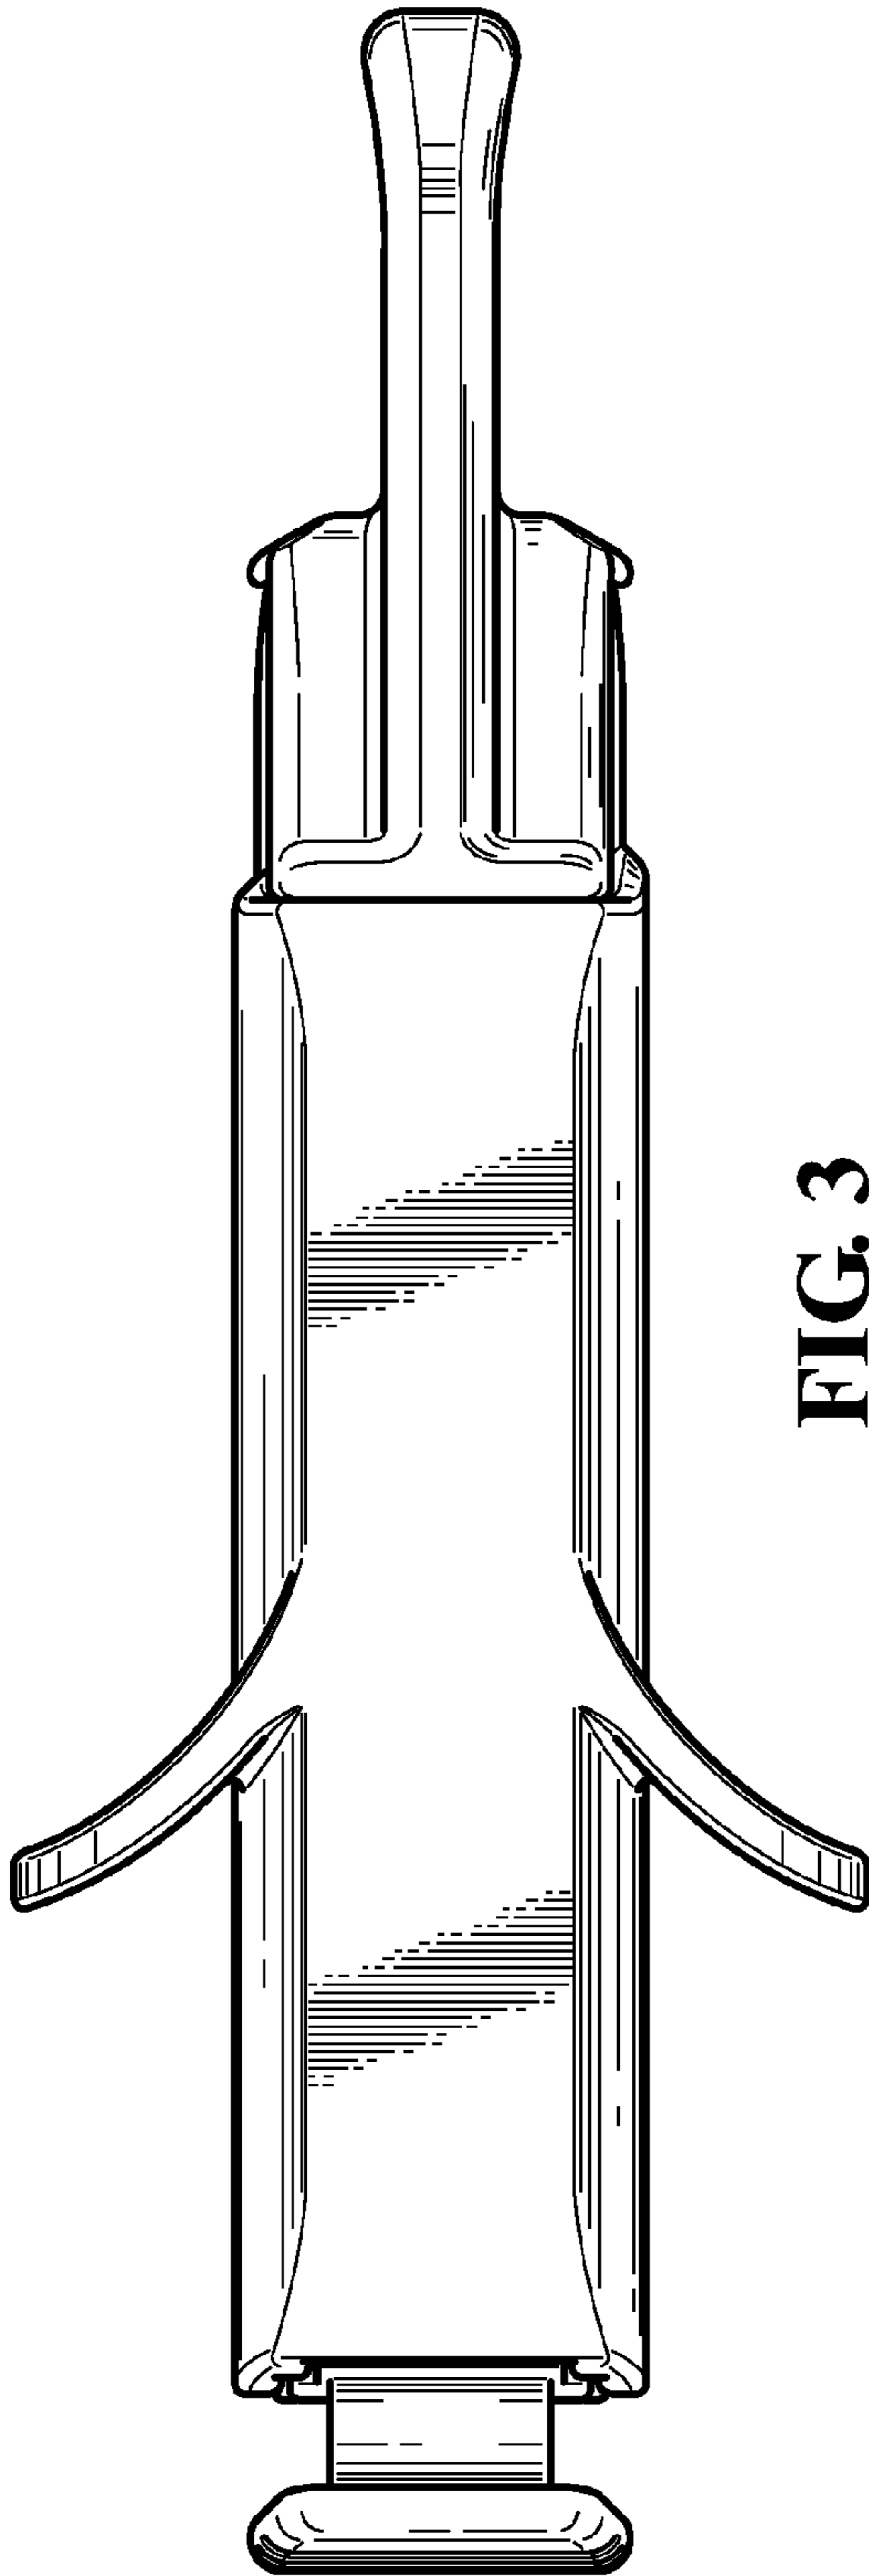


**FIG. 3**

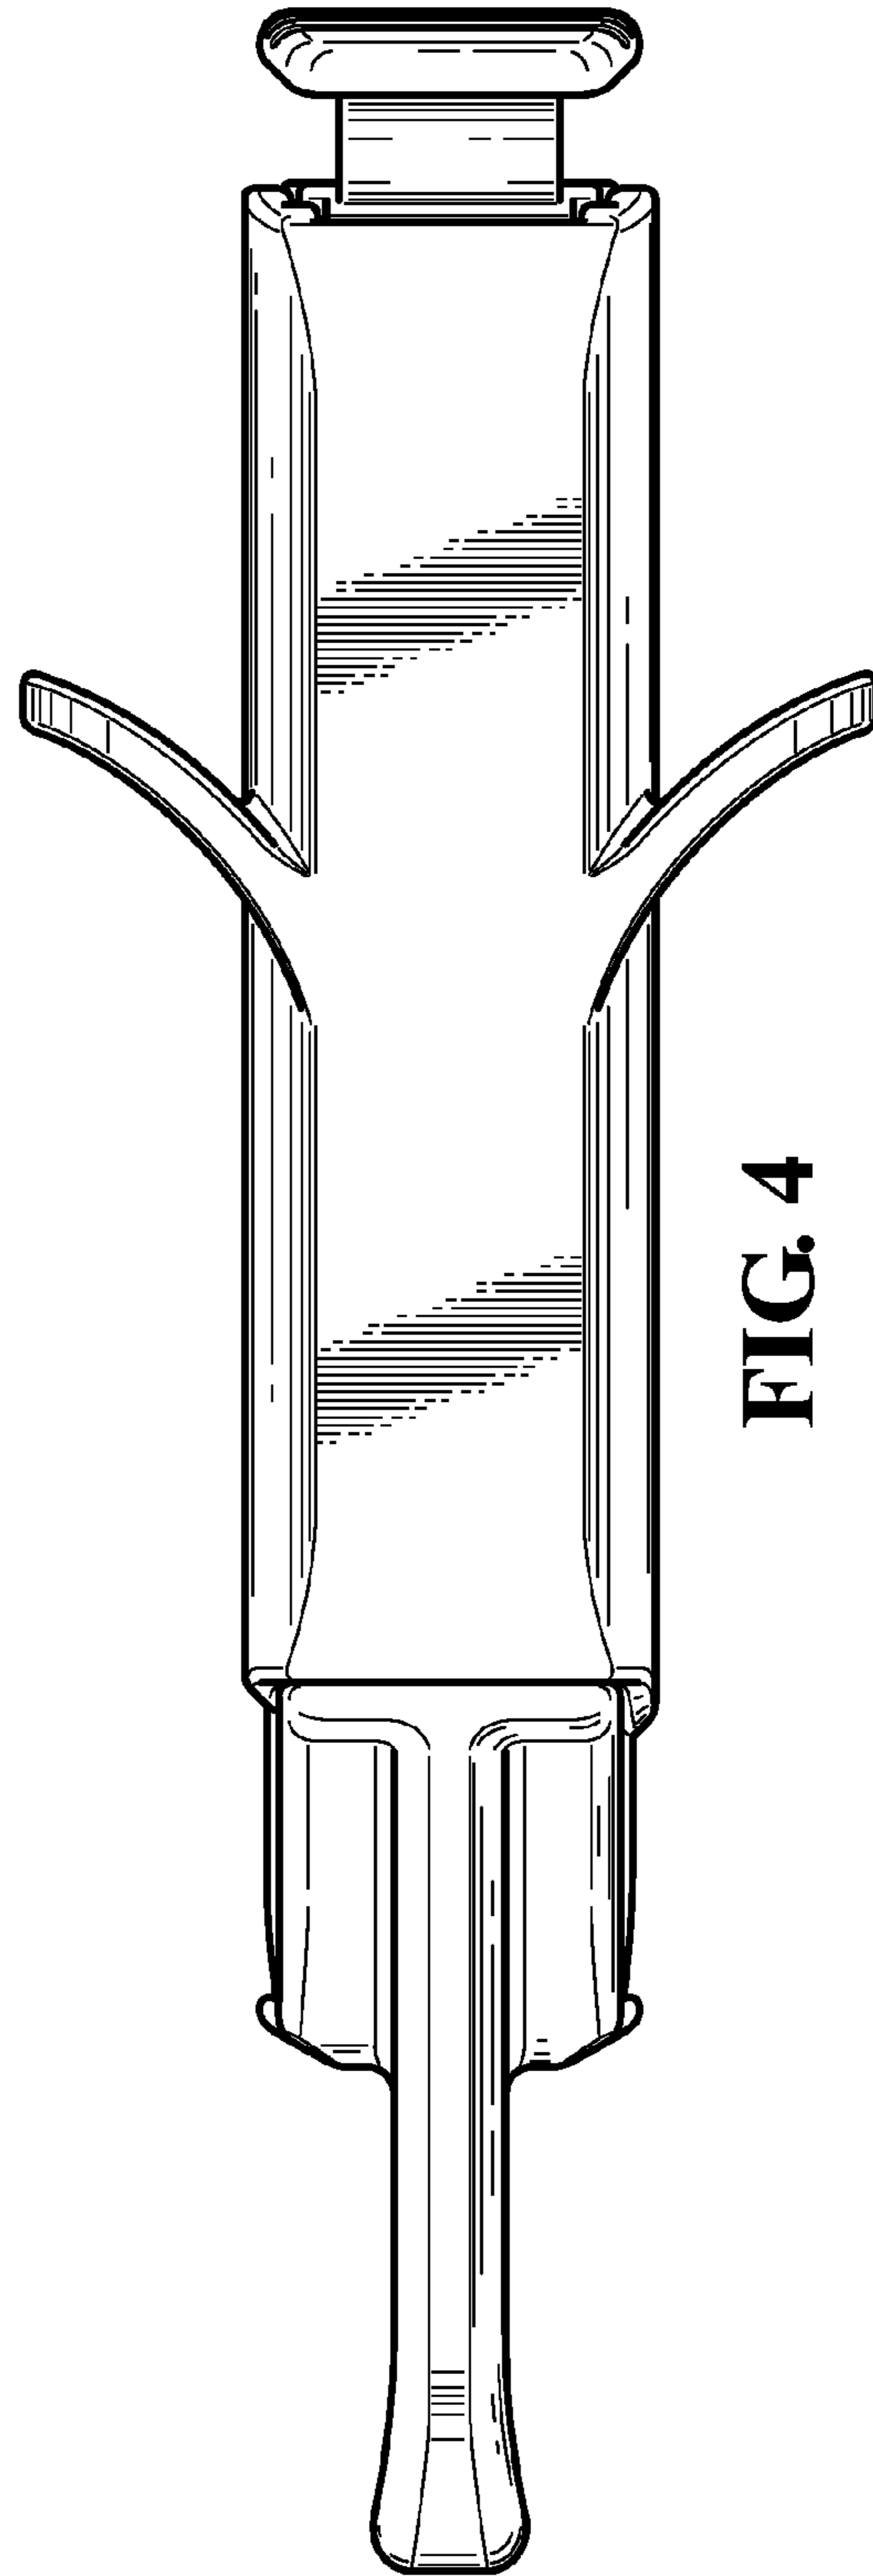

**FIG. 4**

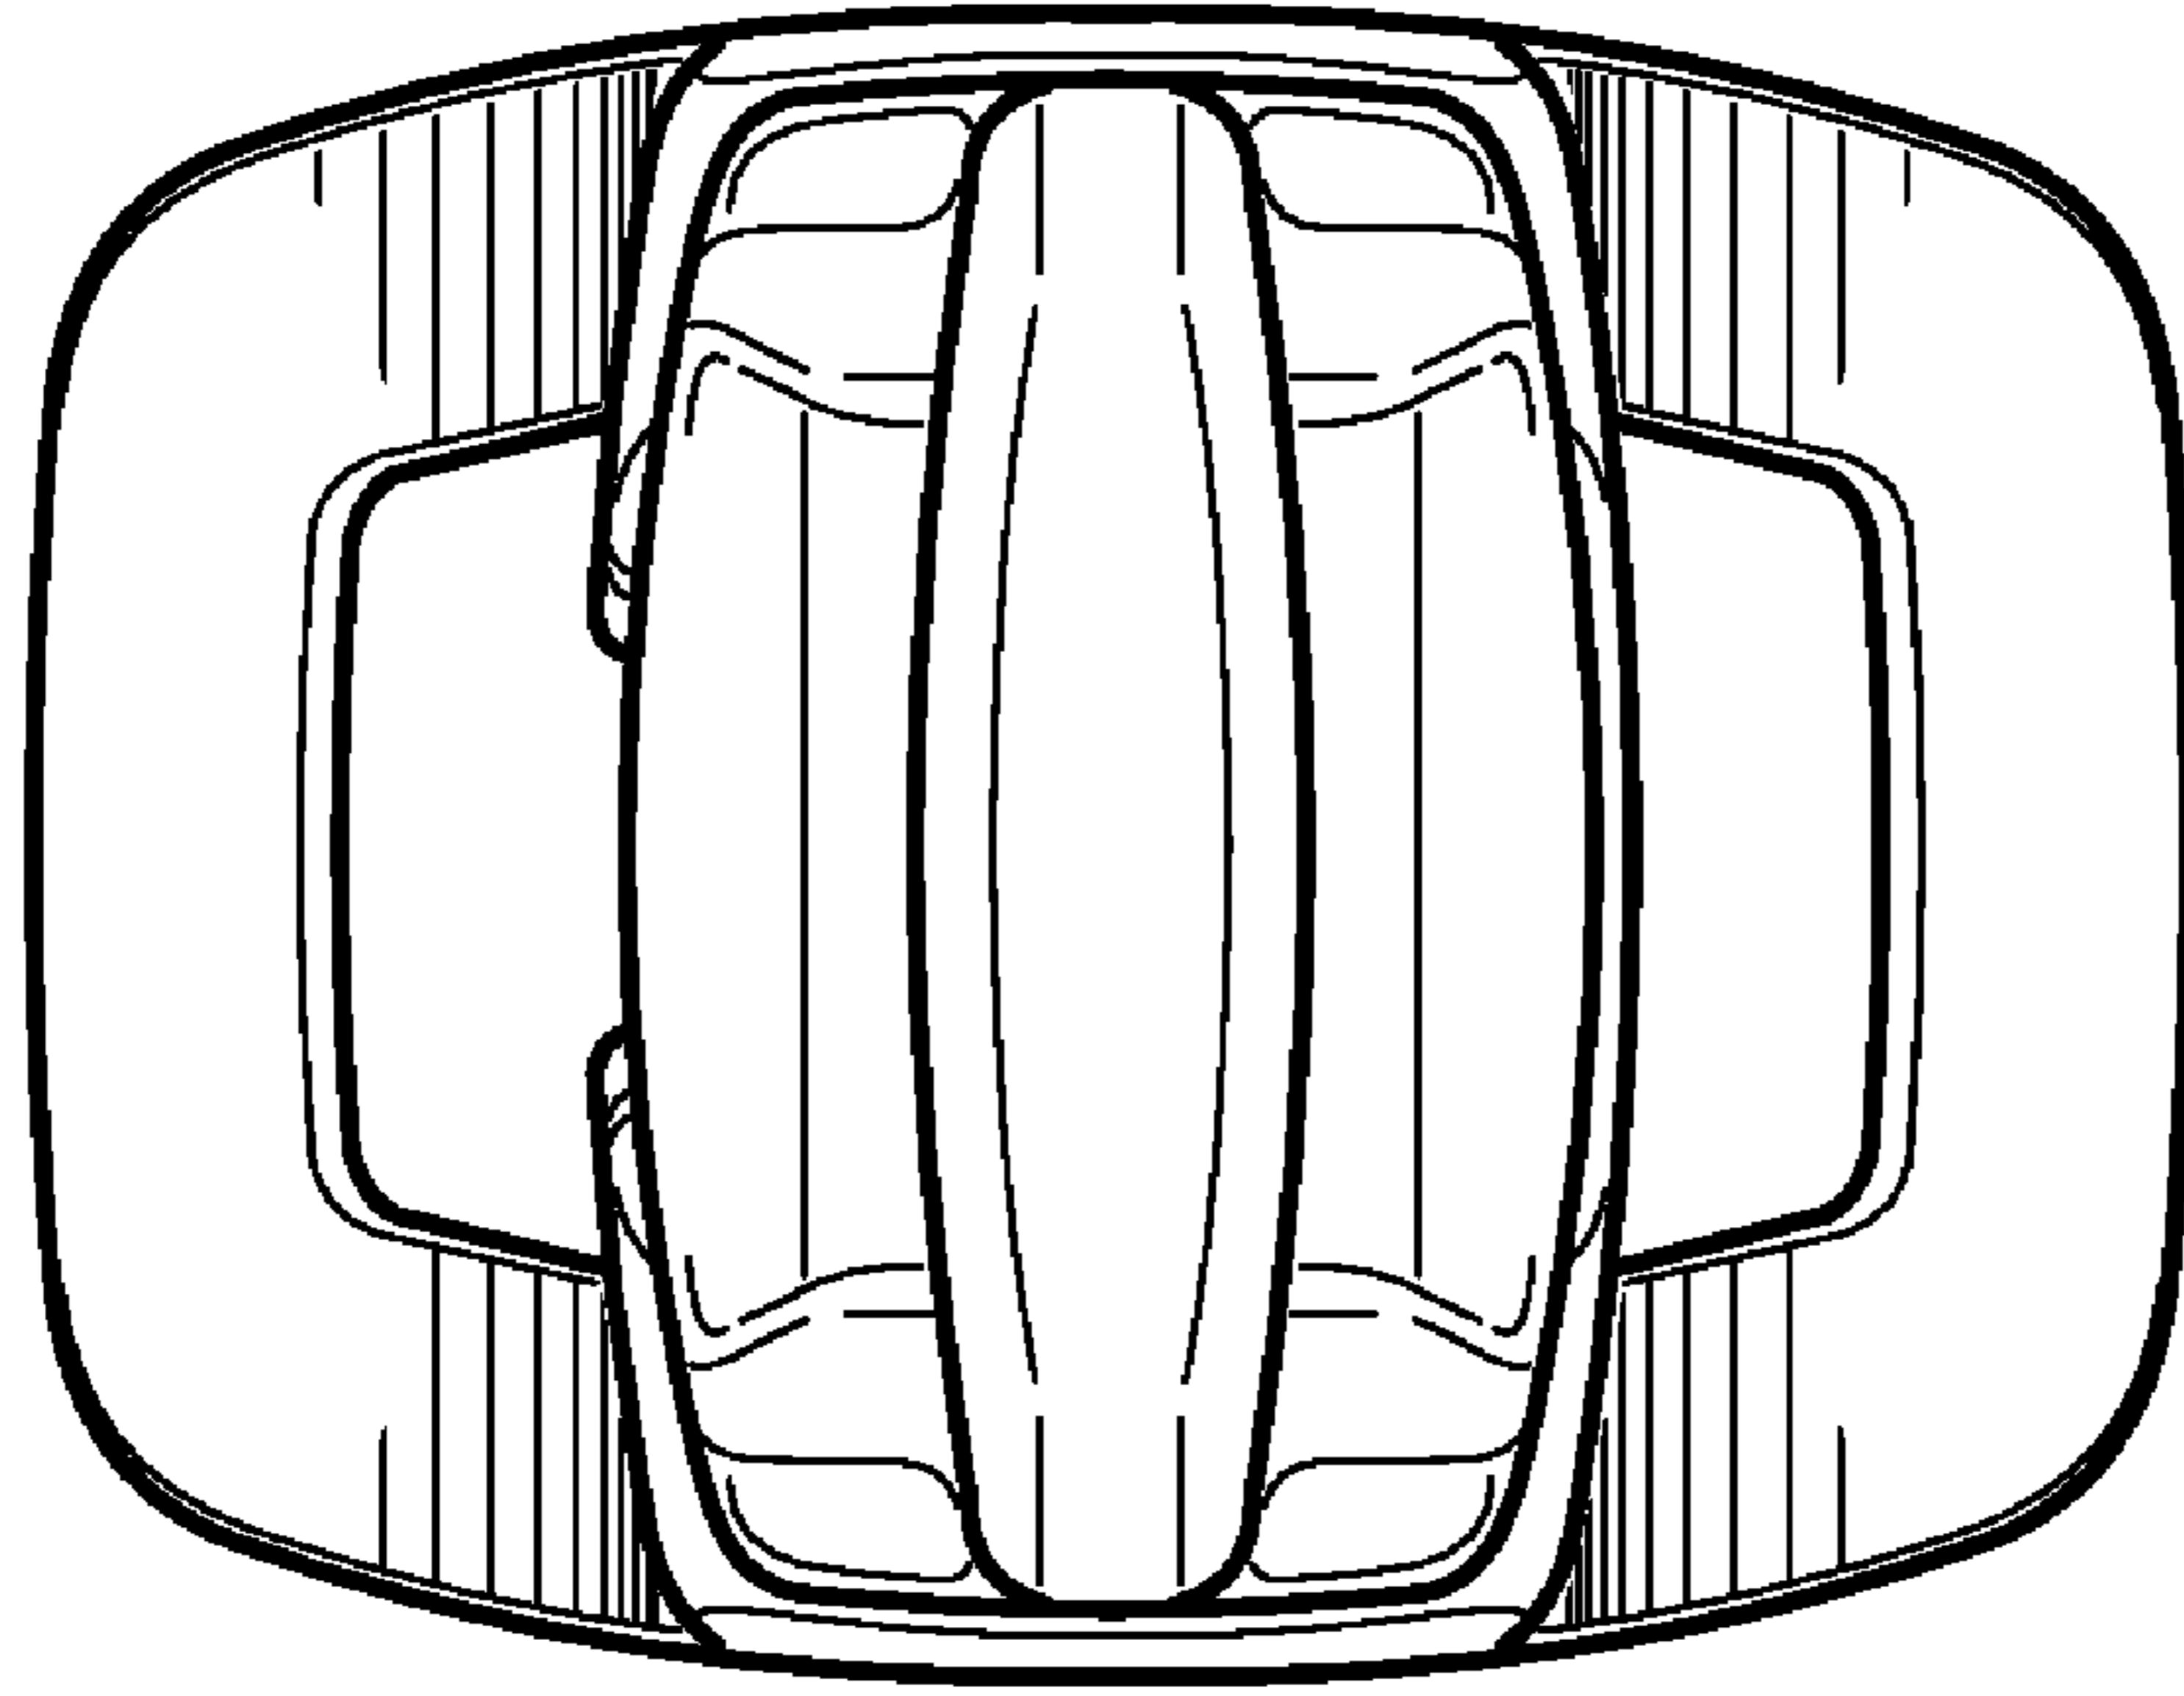

**FIG. 6**

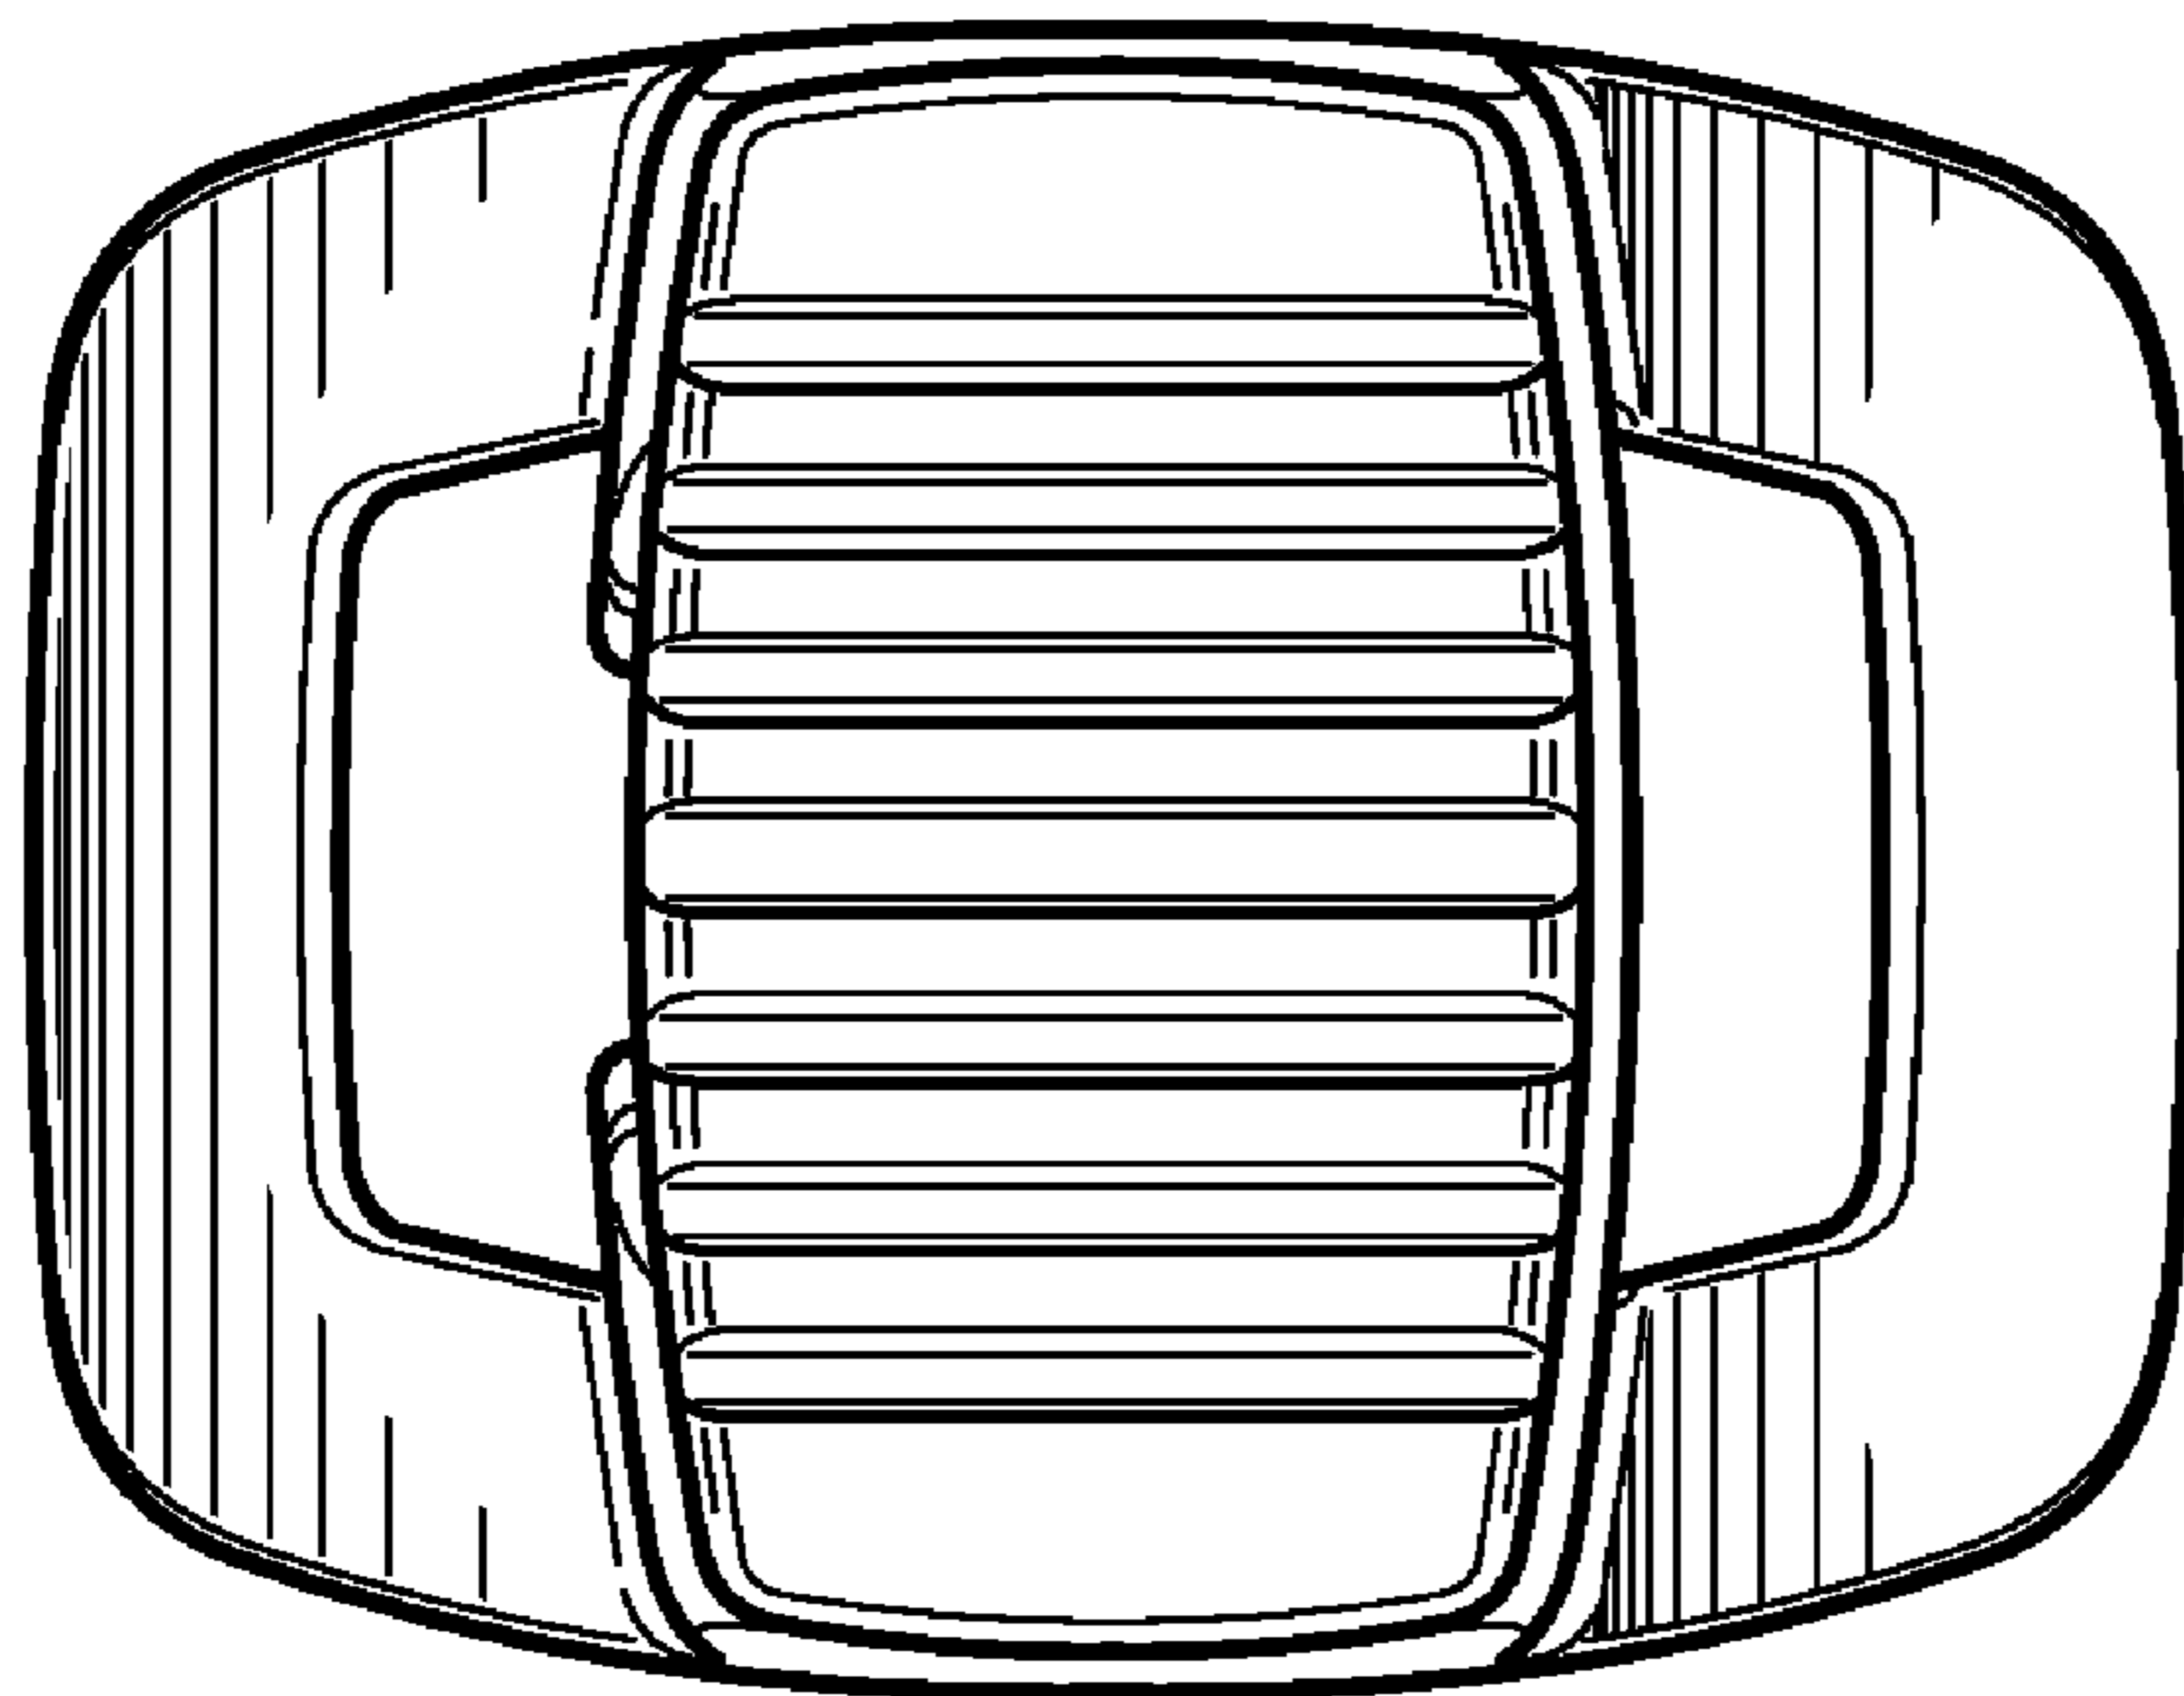

**FIG. 5**

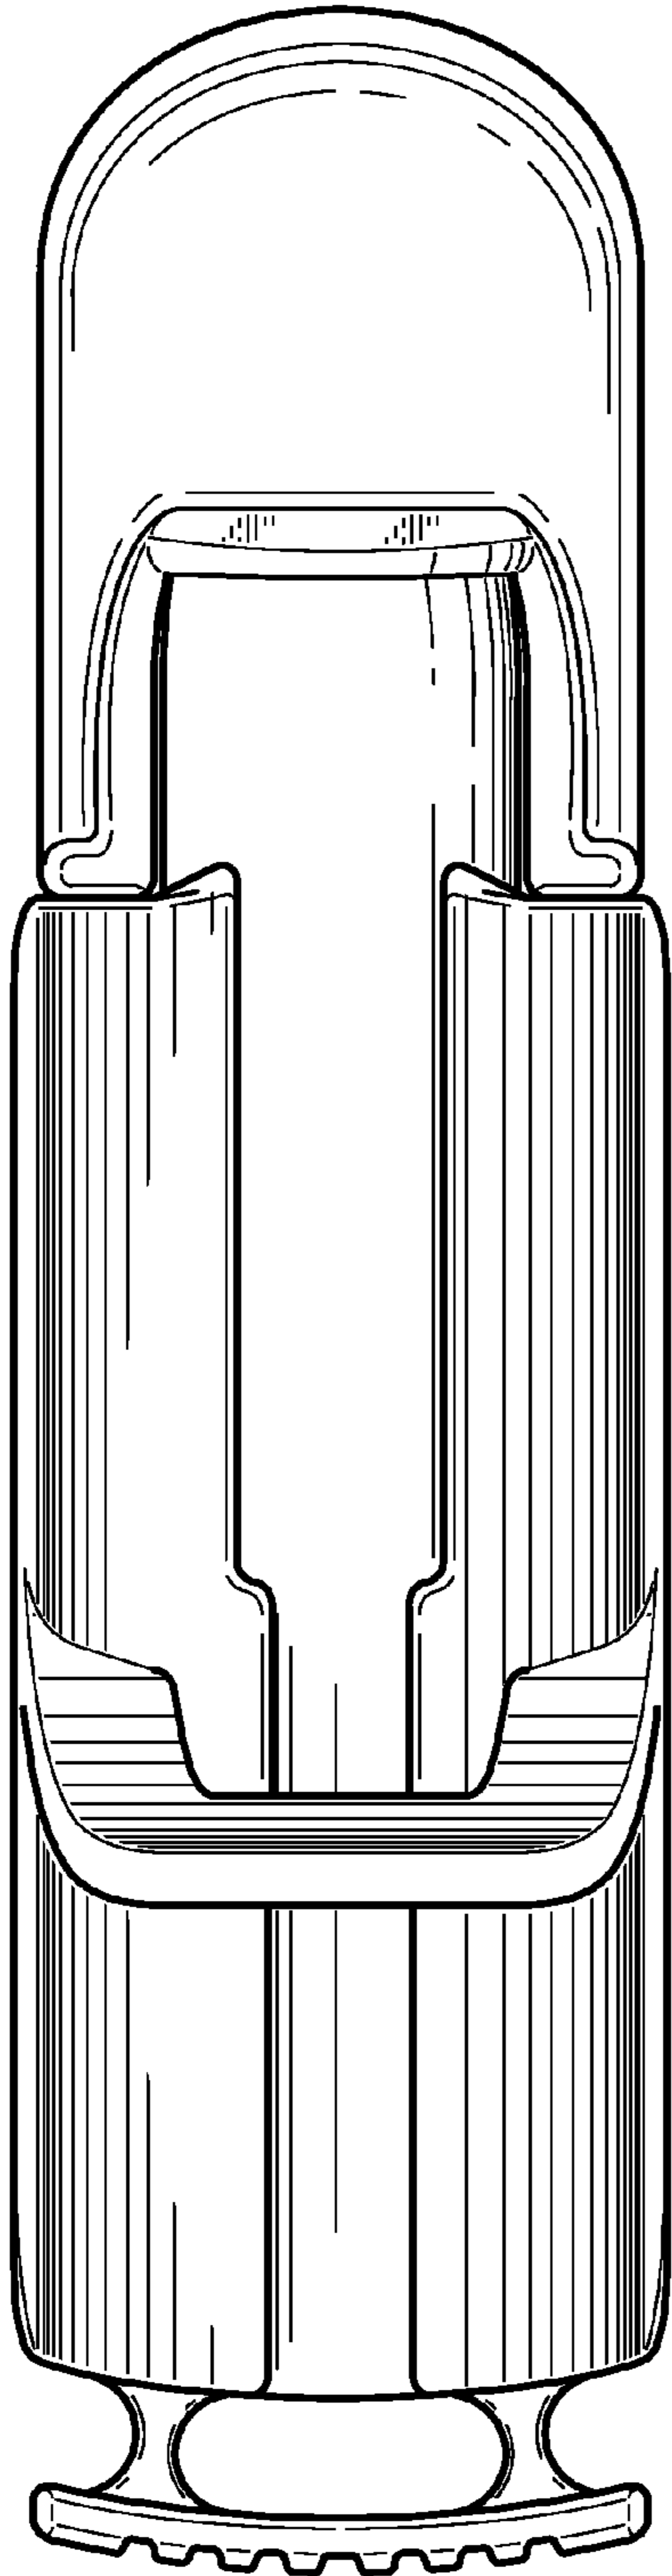


FIG. 7



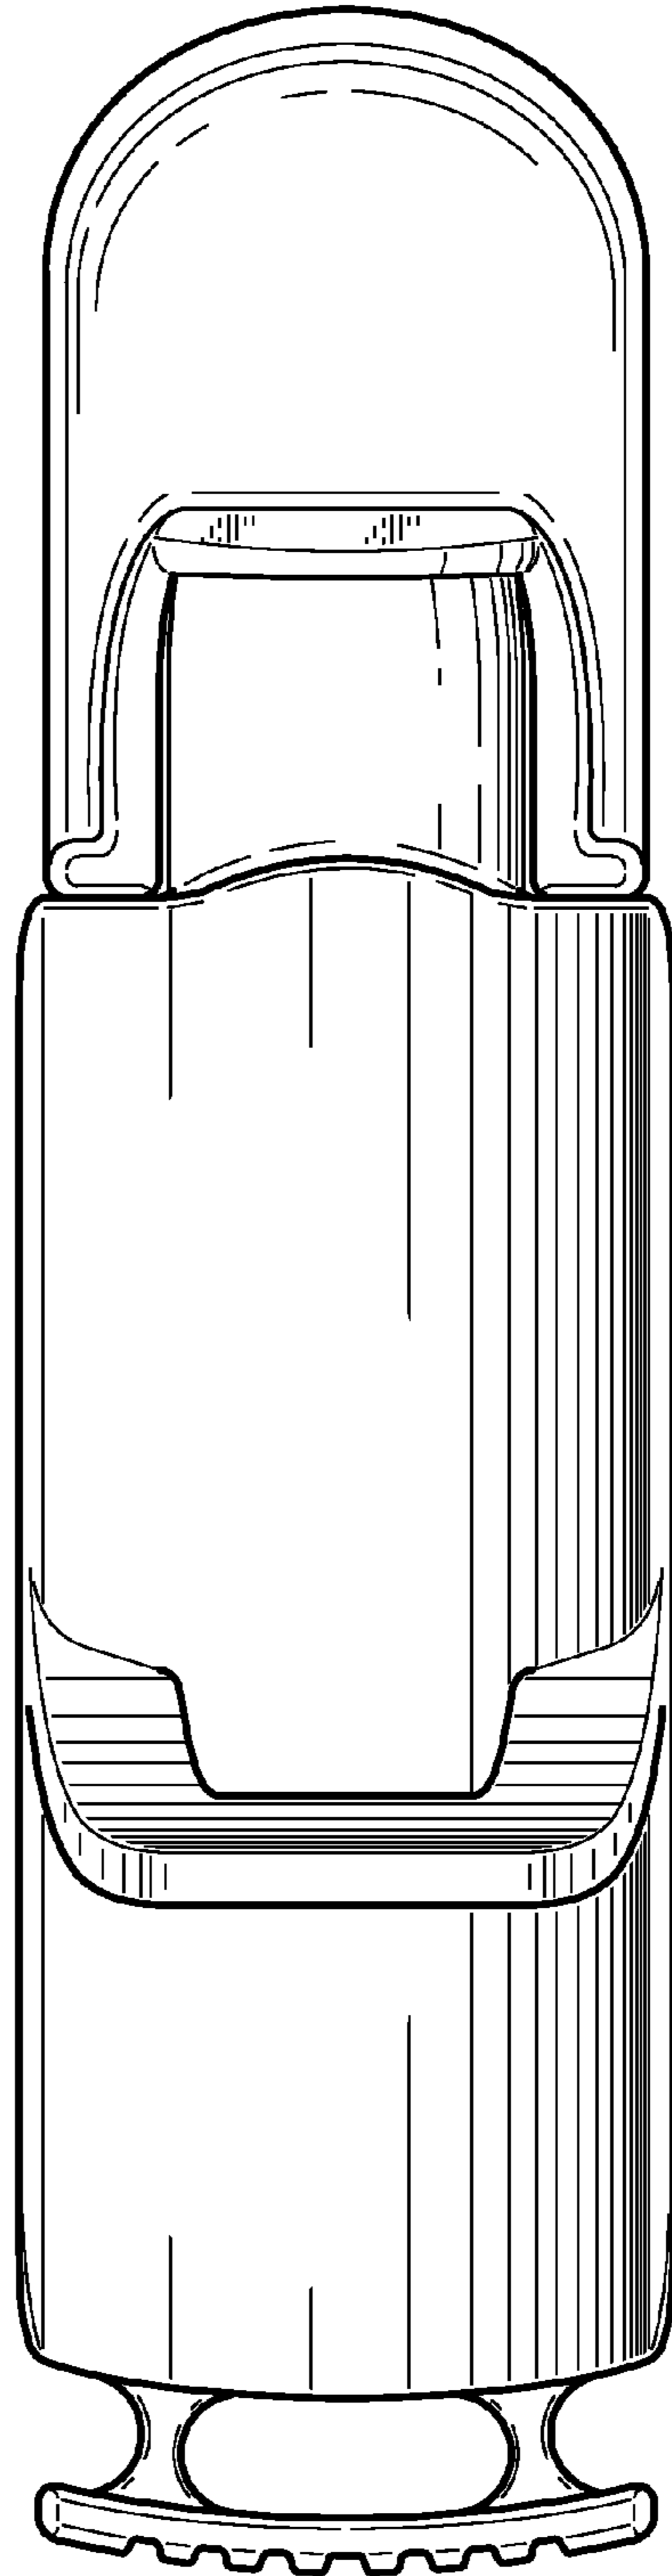


FIG. 8



**FIG. 9**

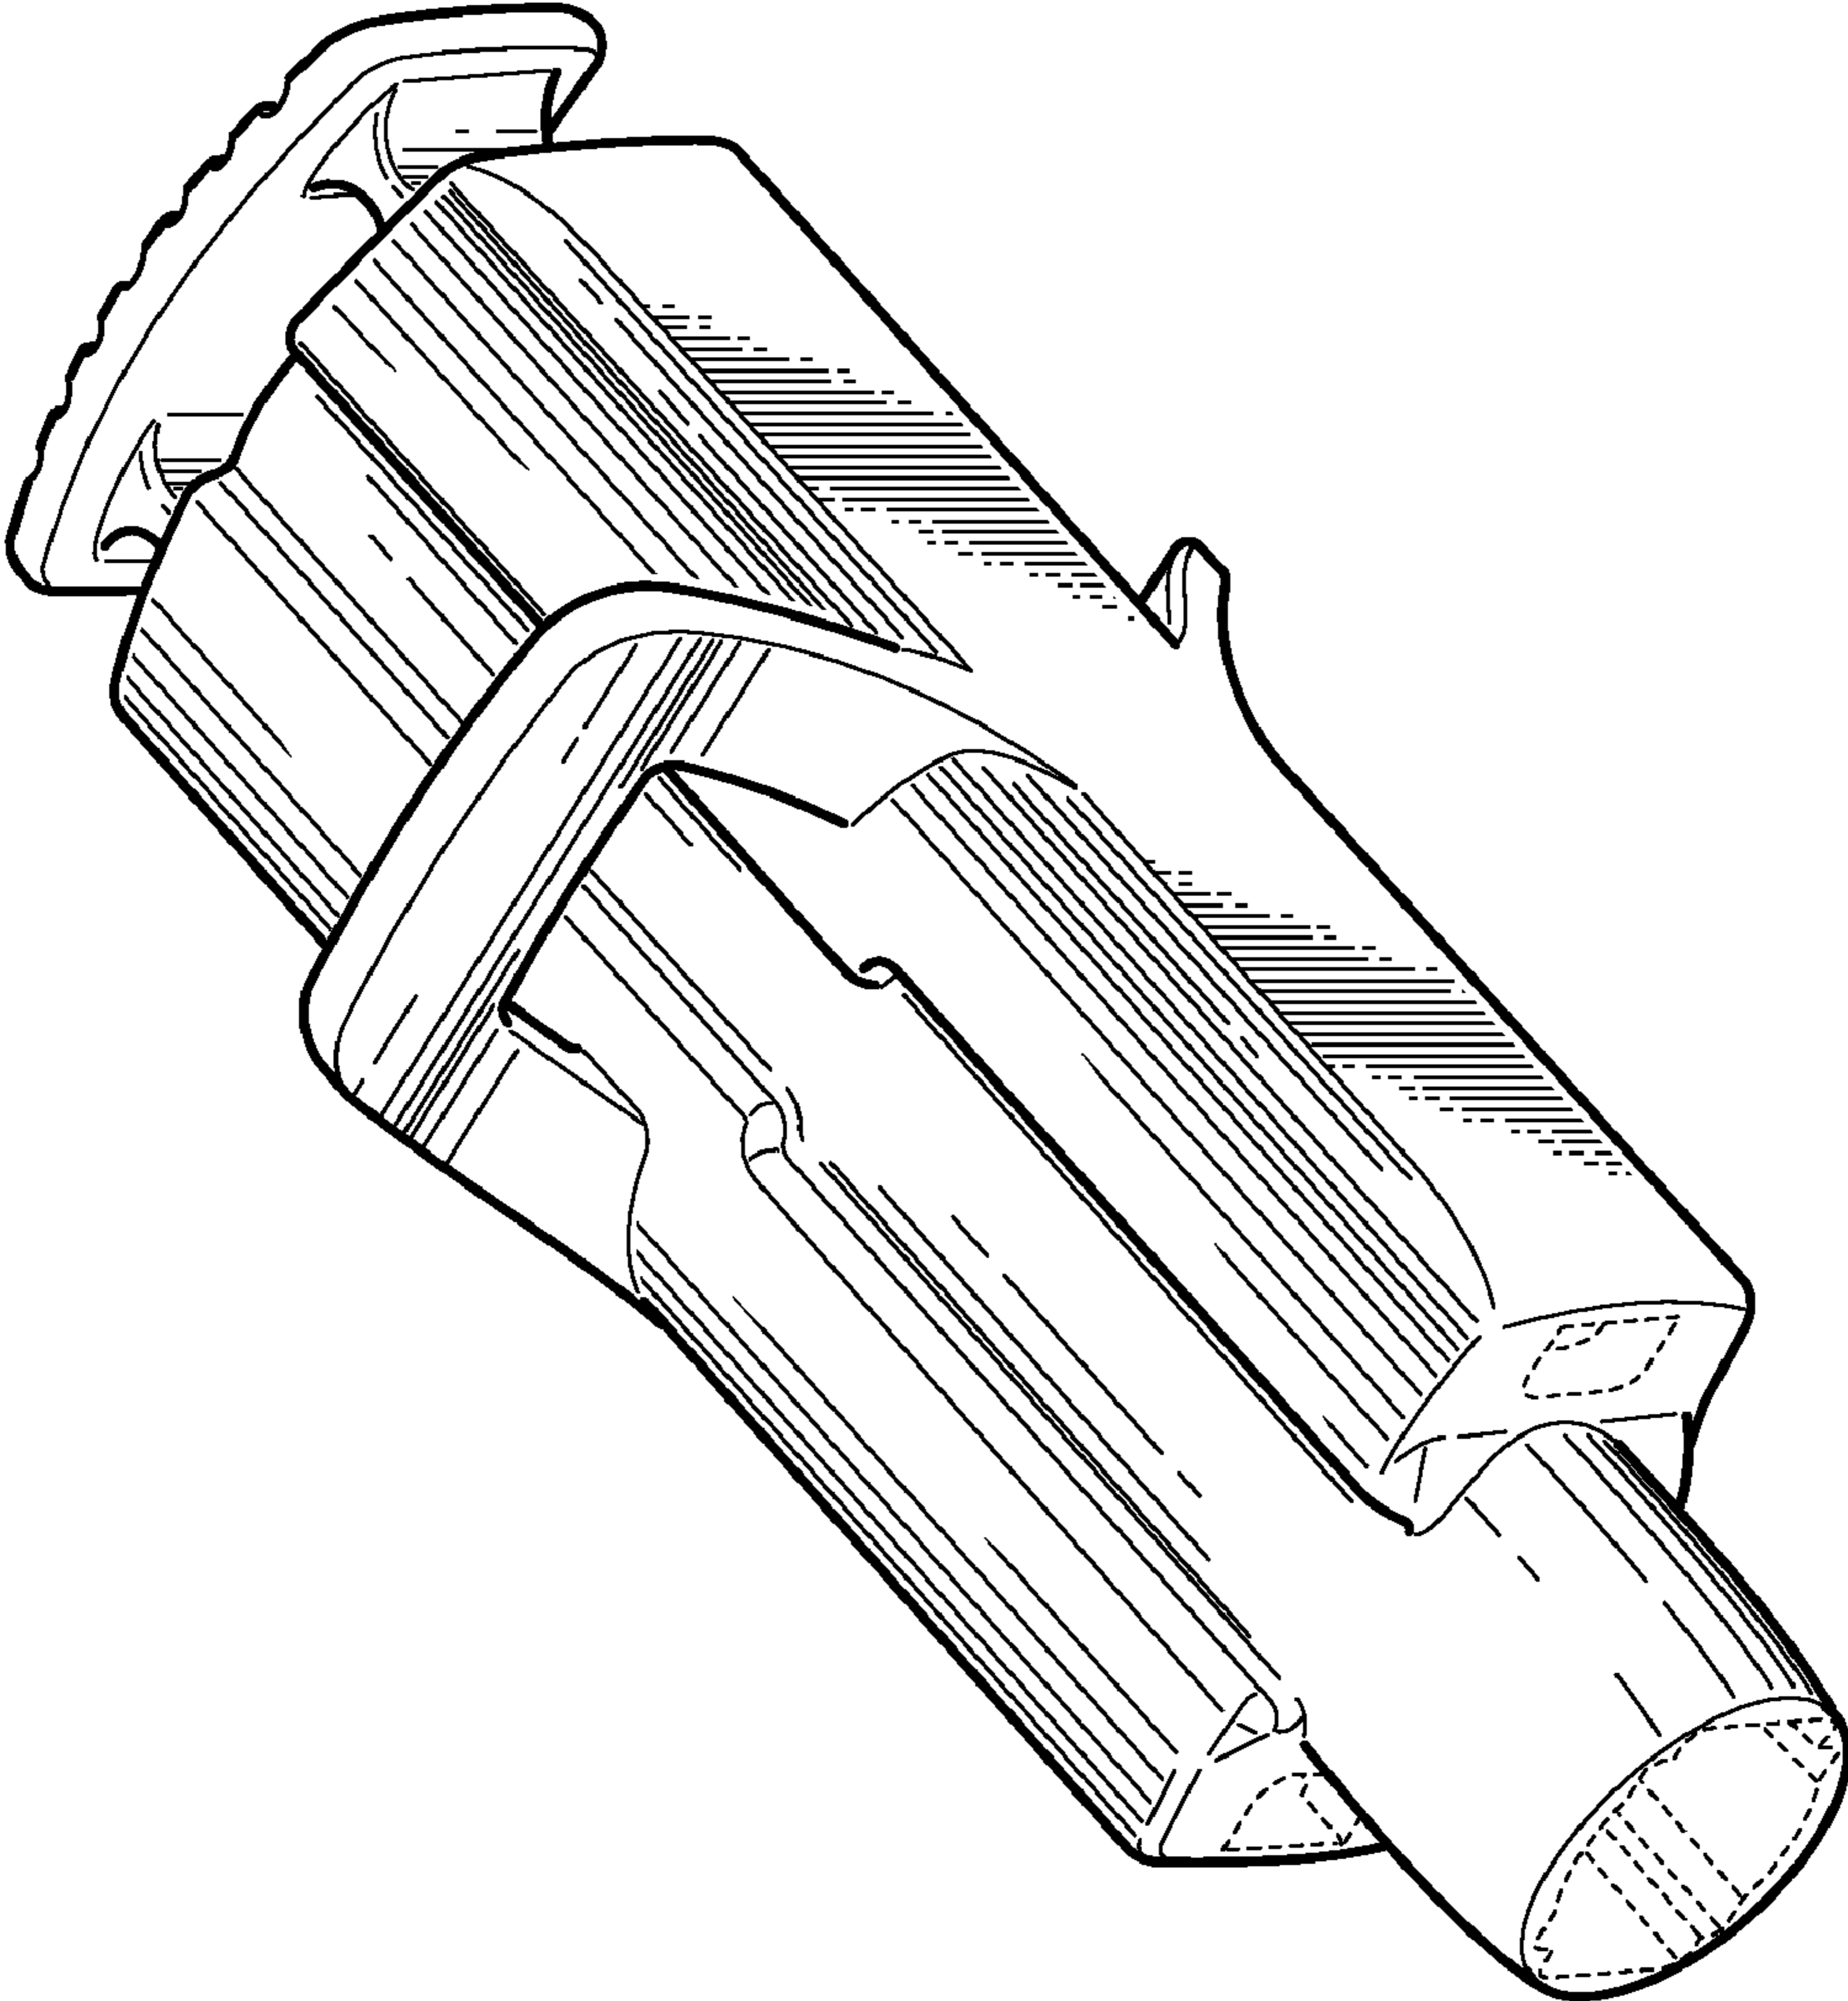

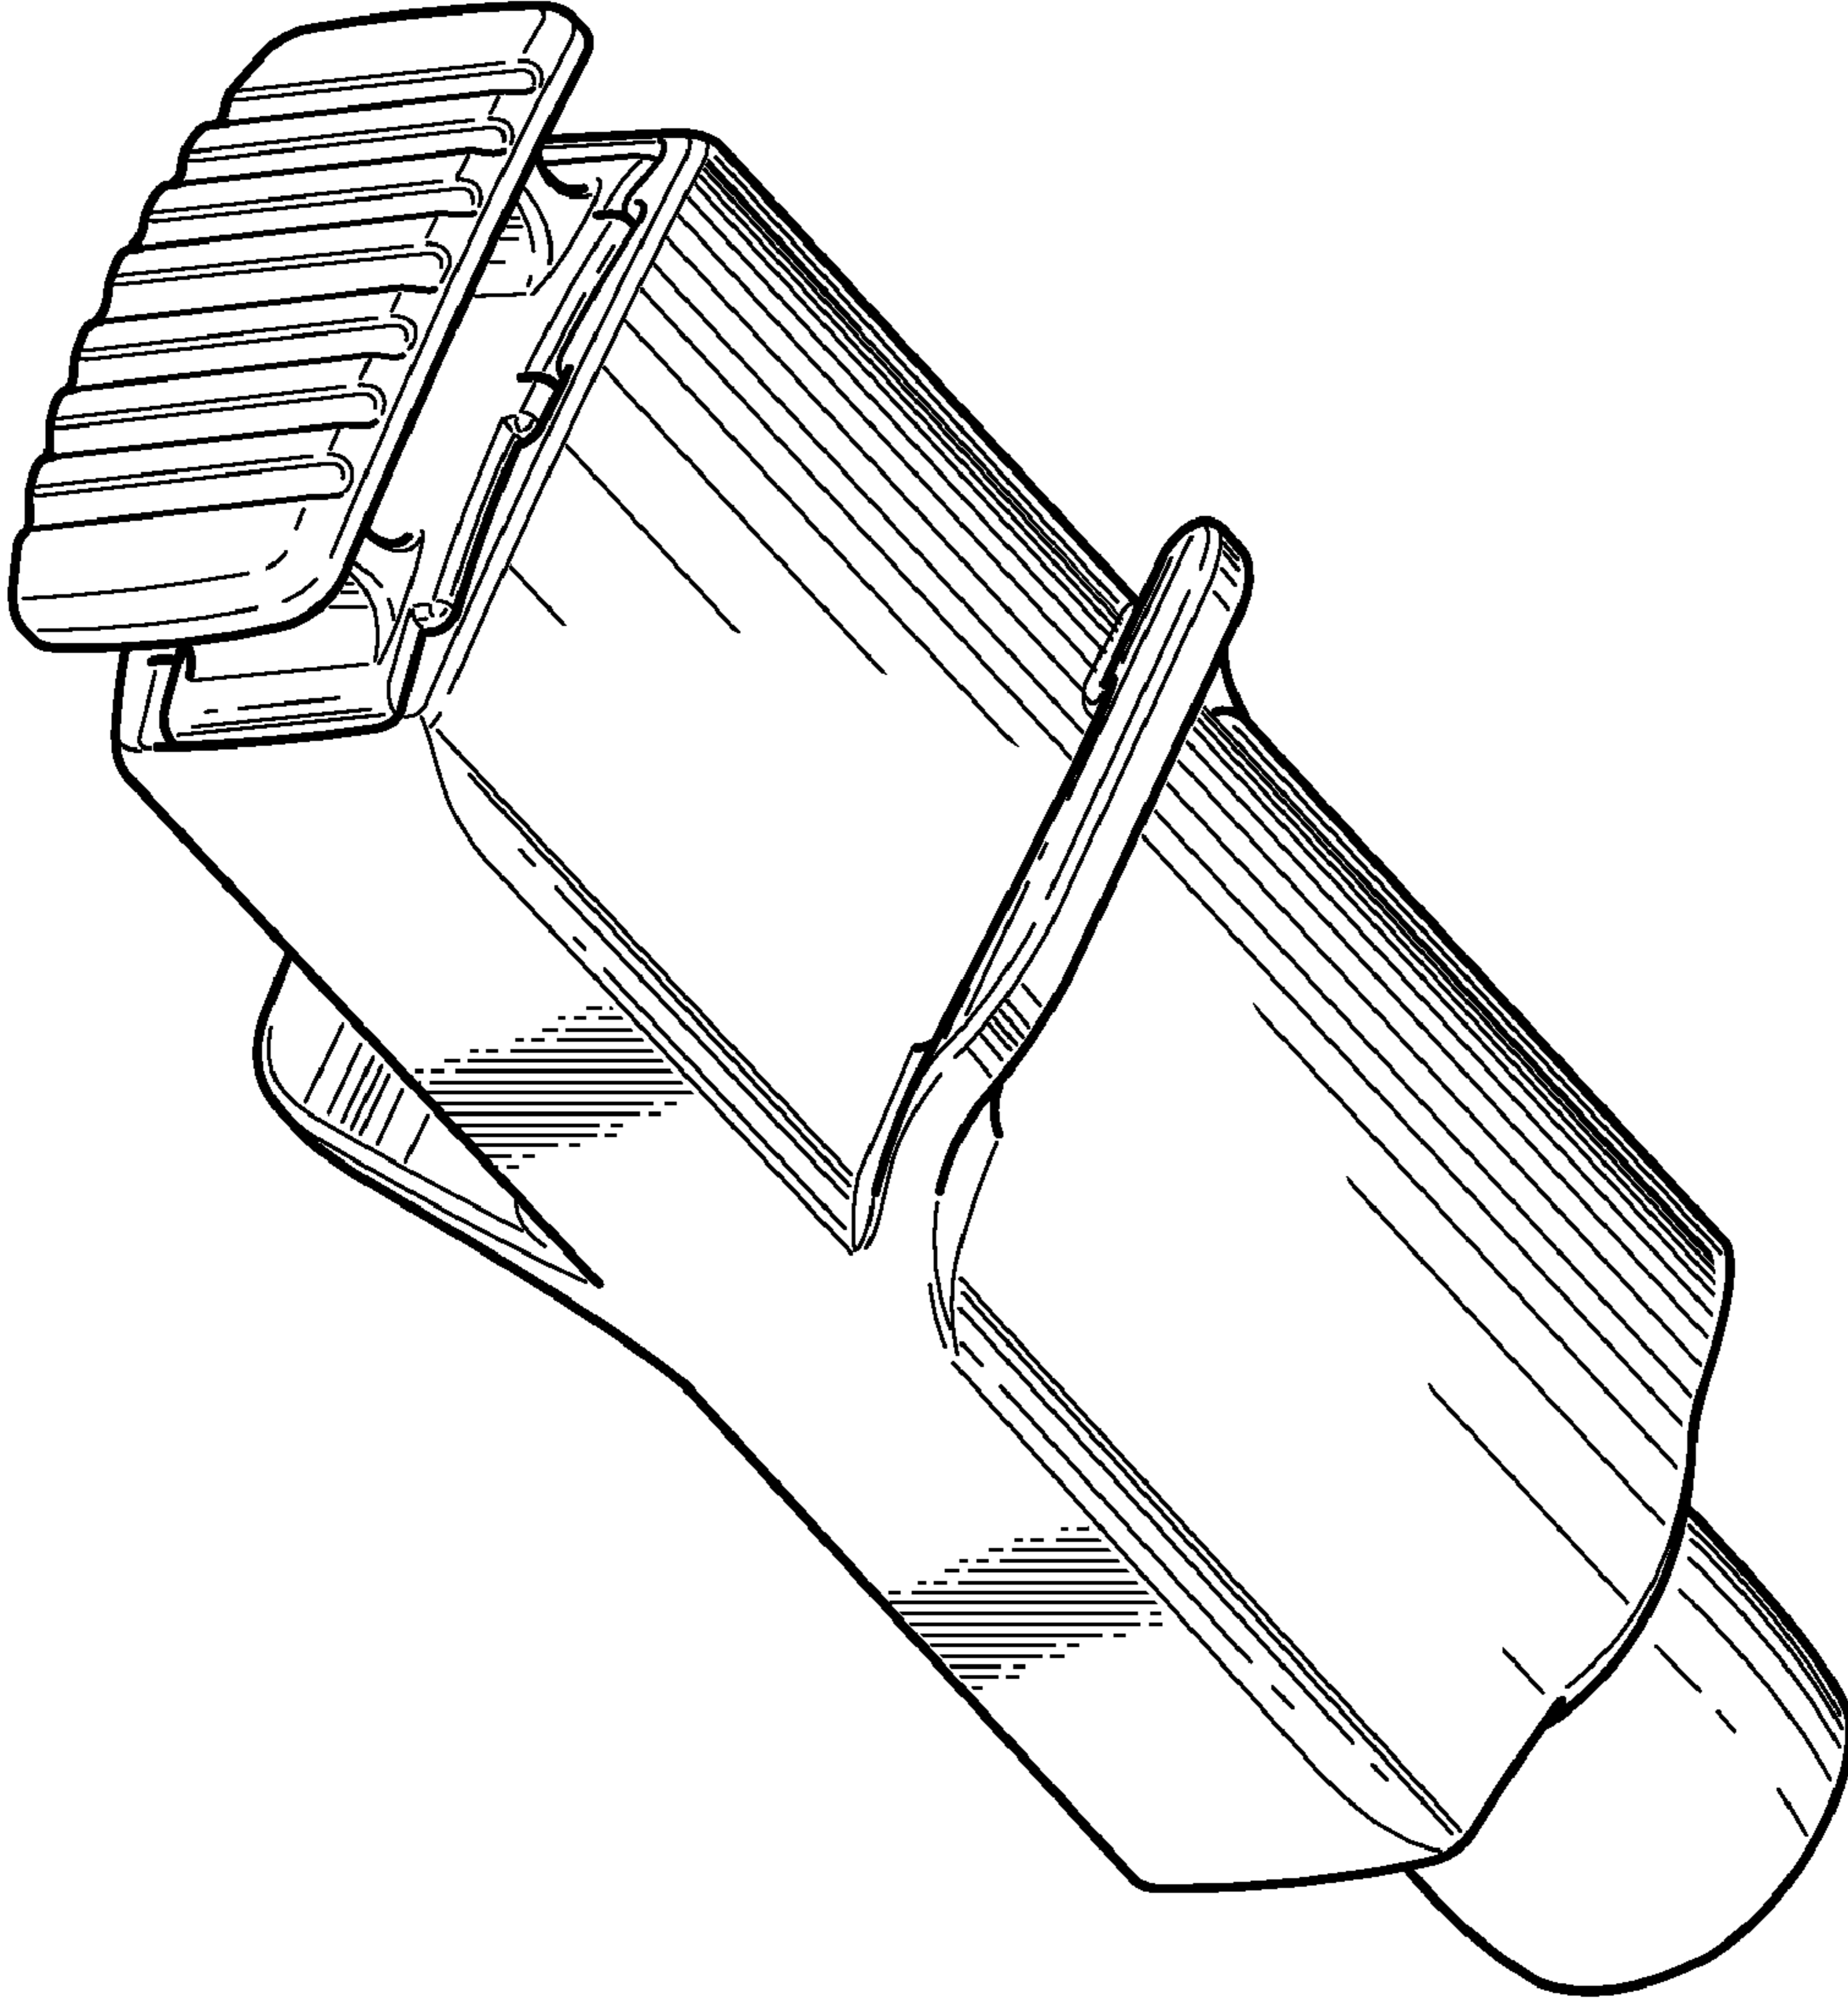

**FIG. 10**

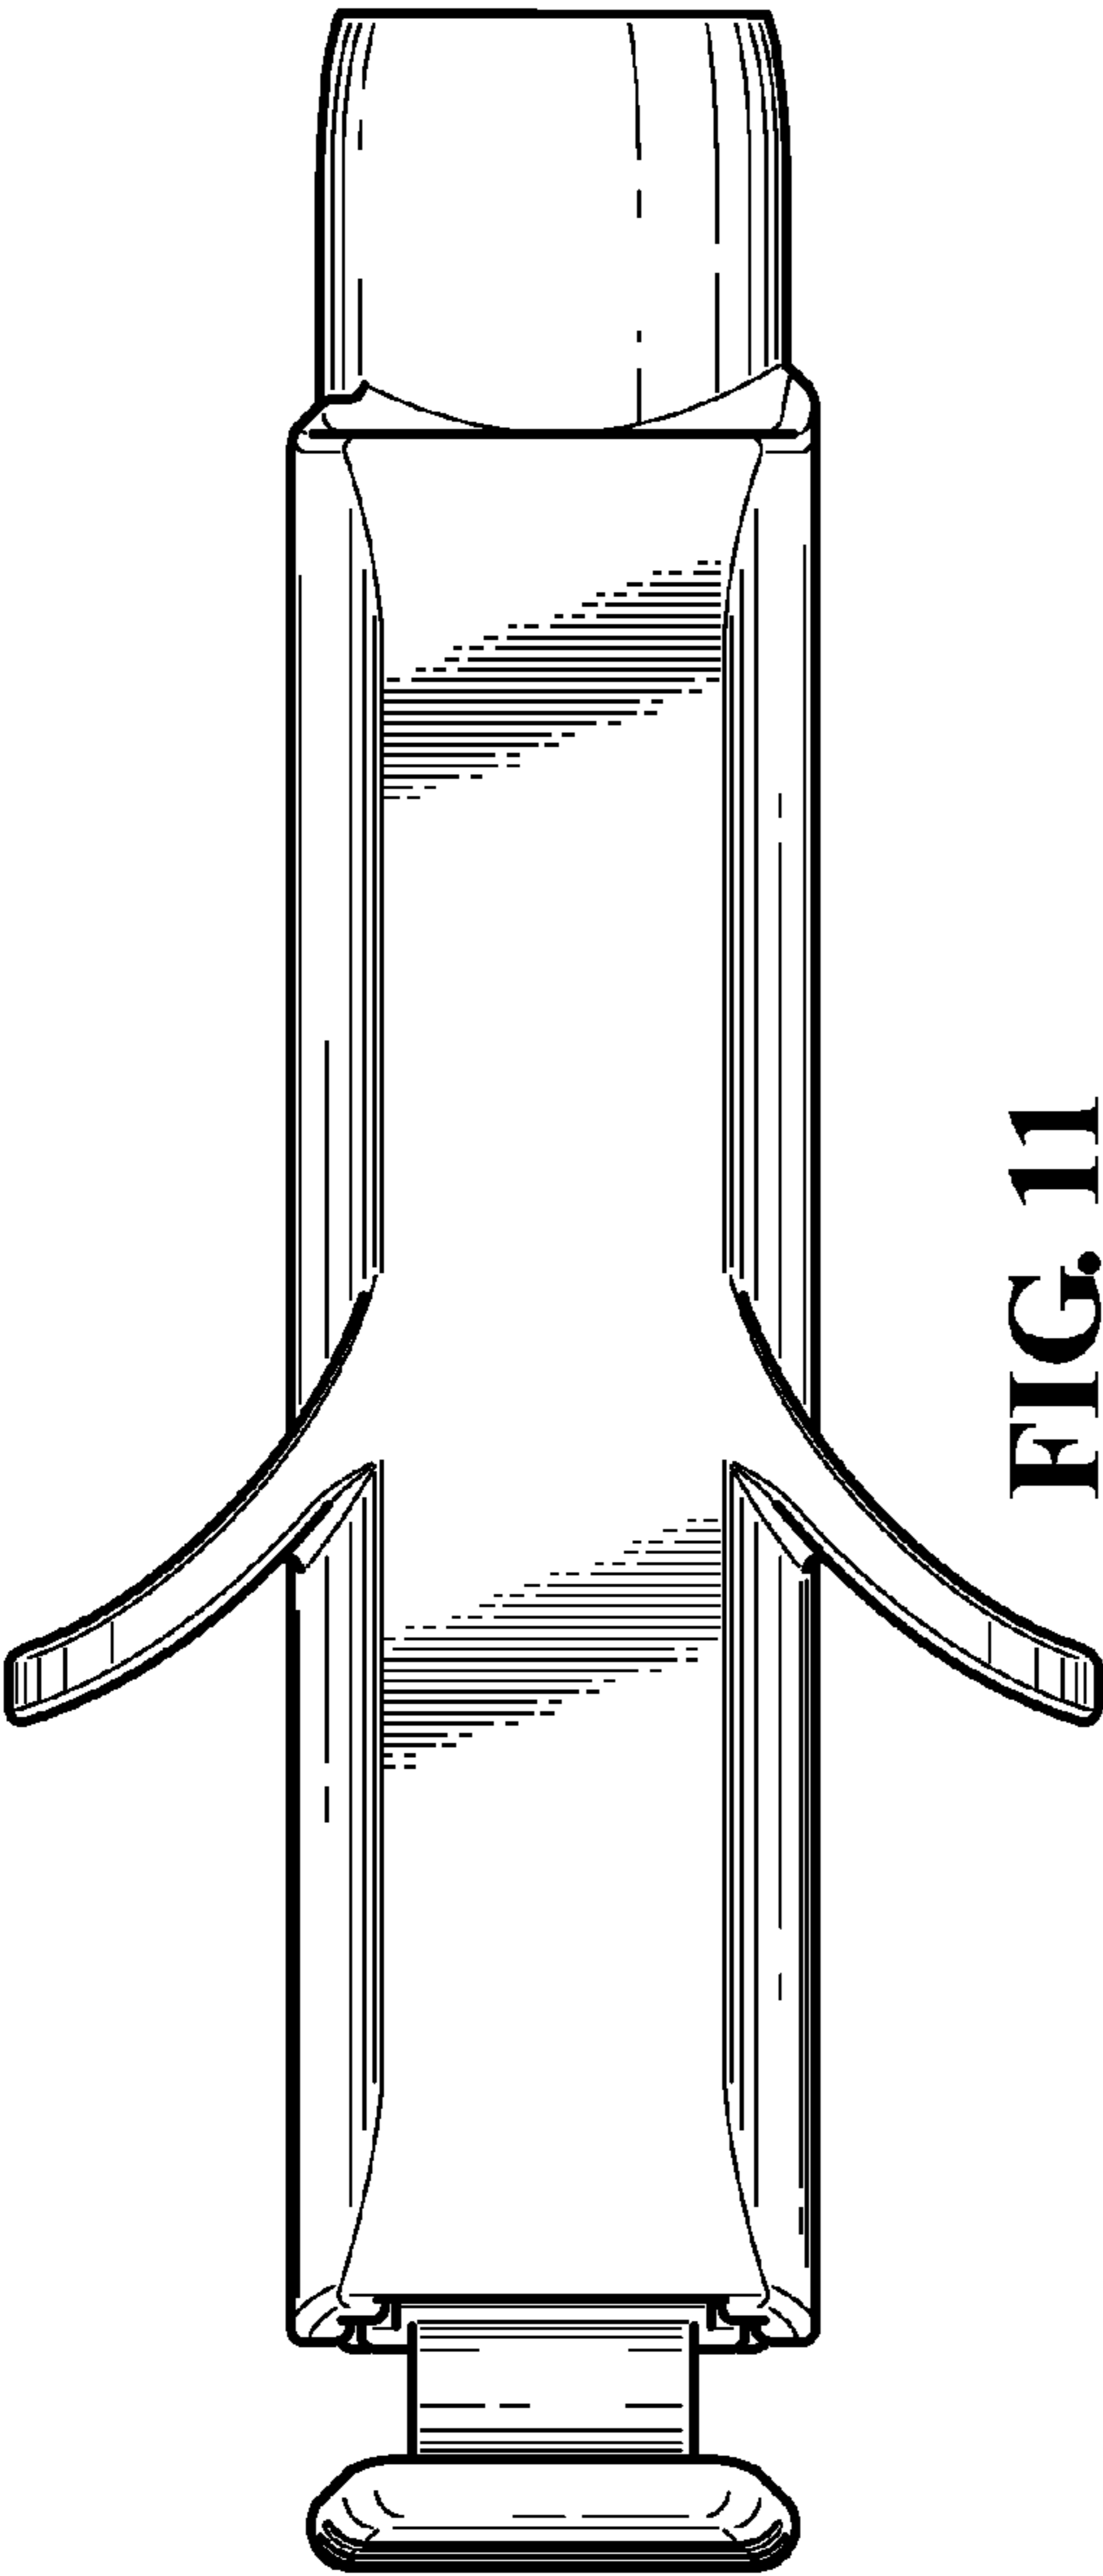


FIG. 11

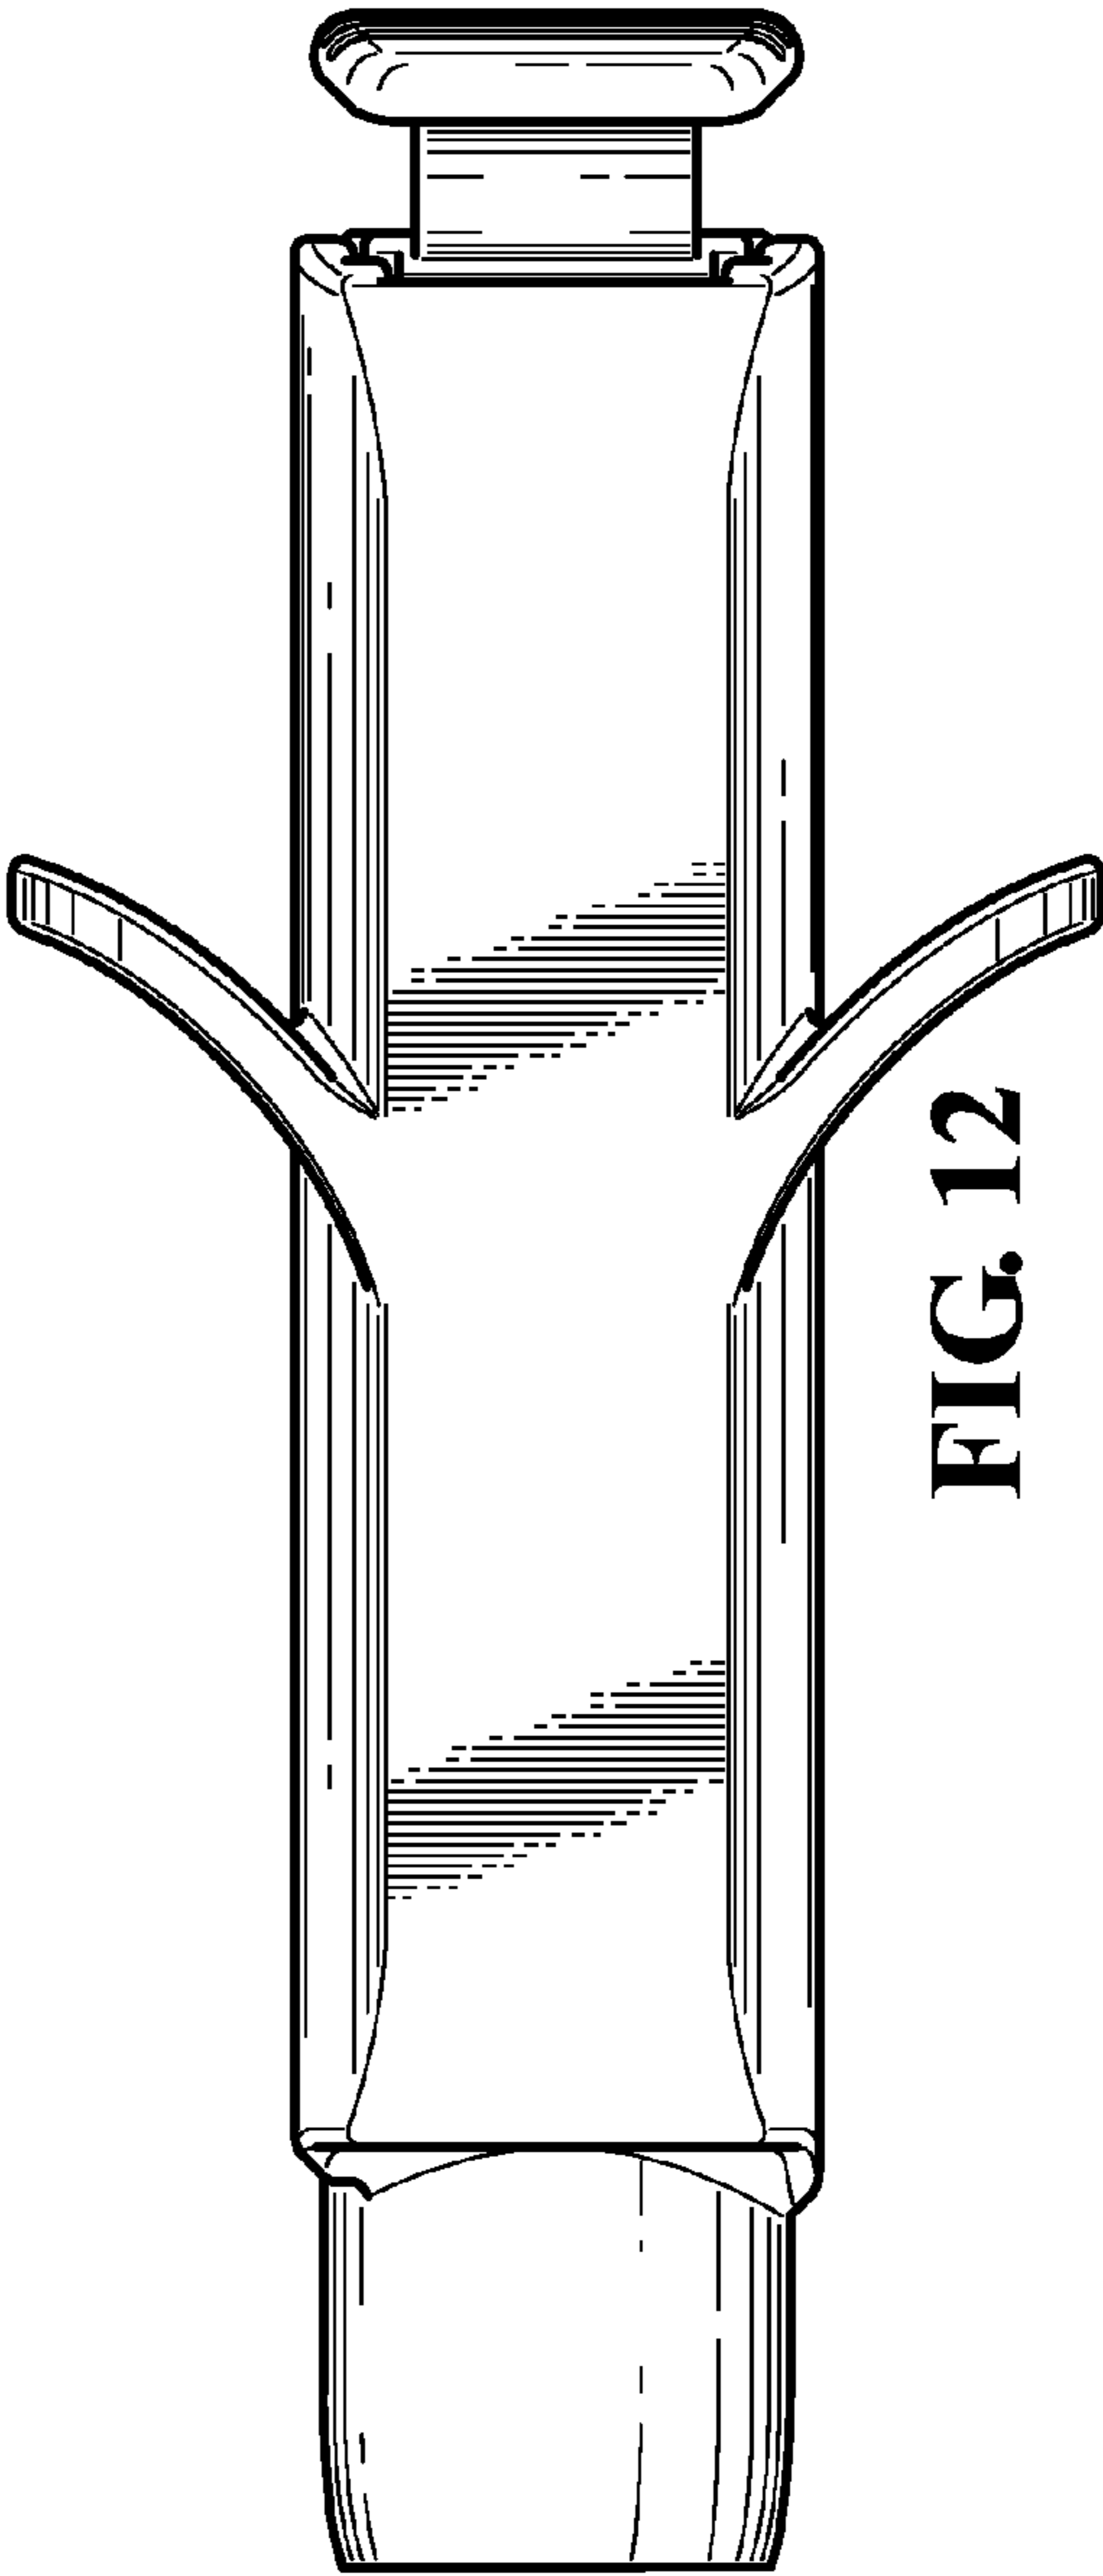


FIG. 12

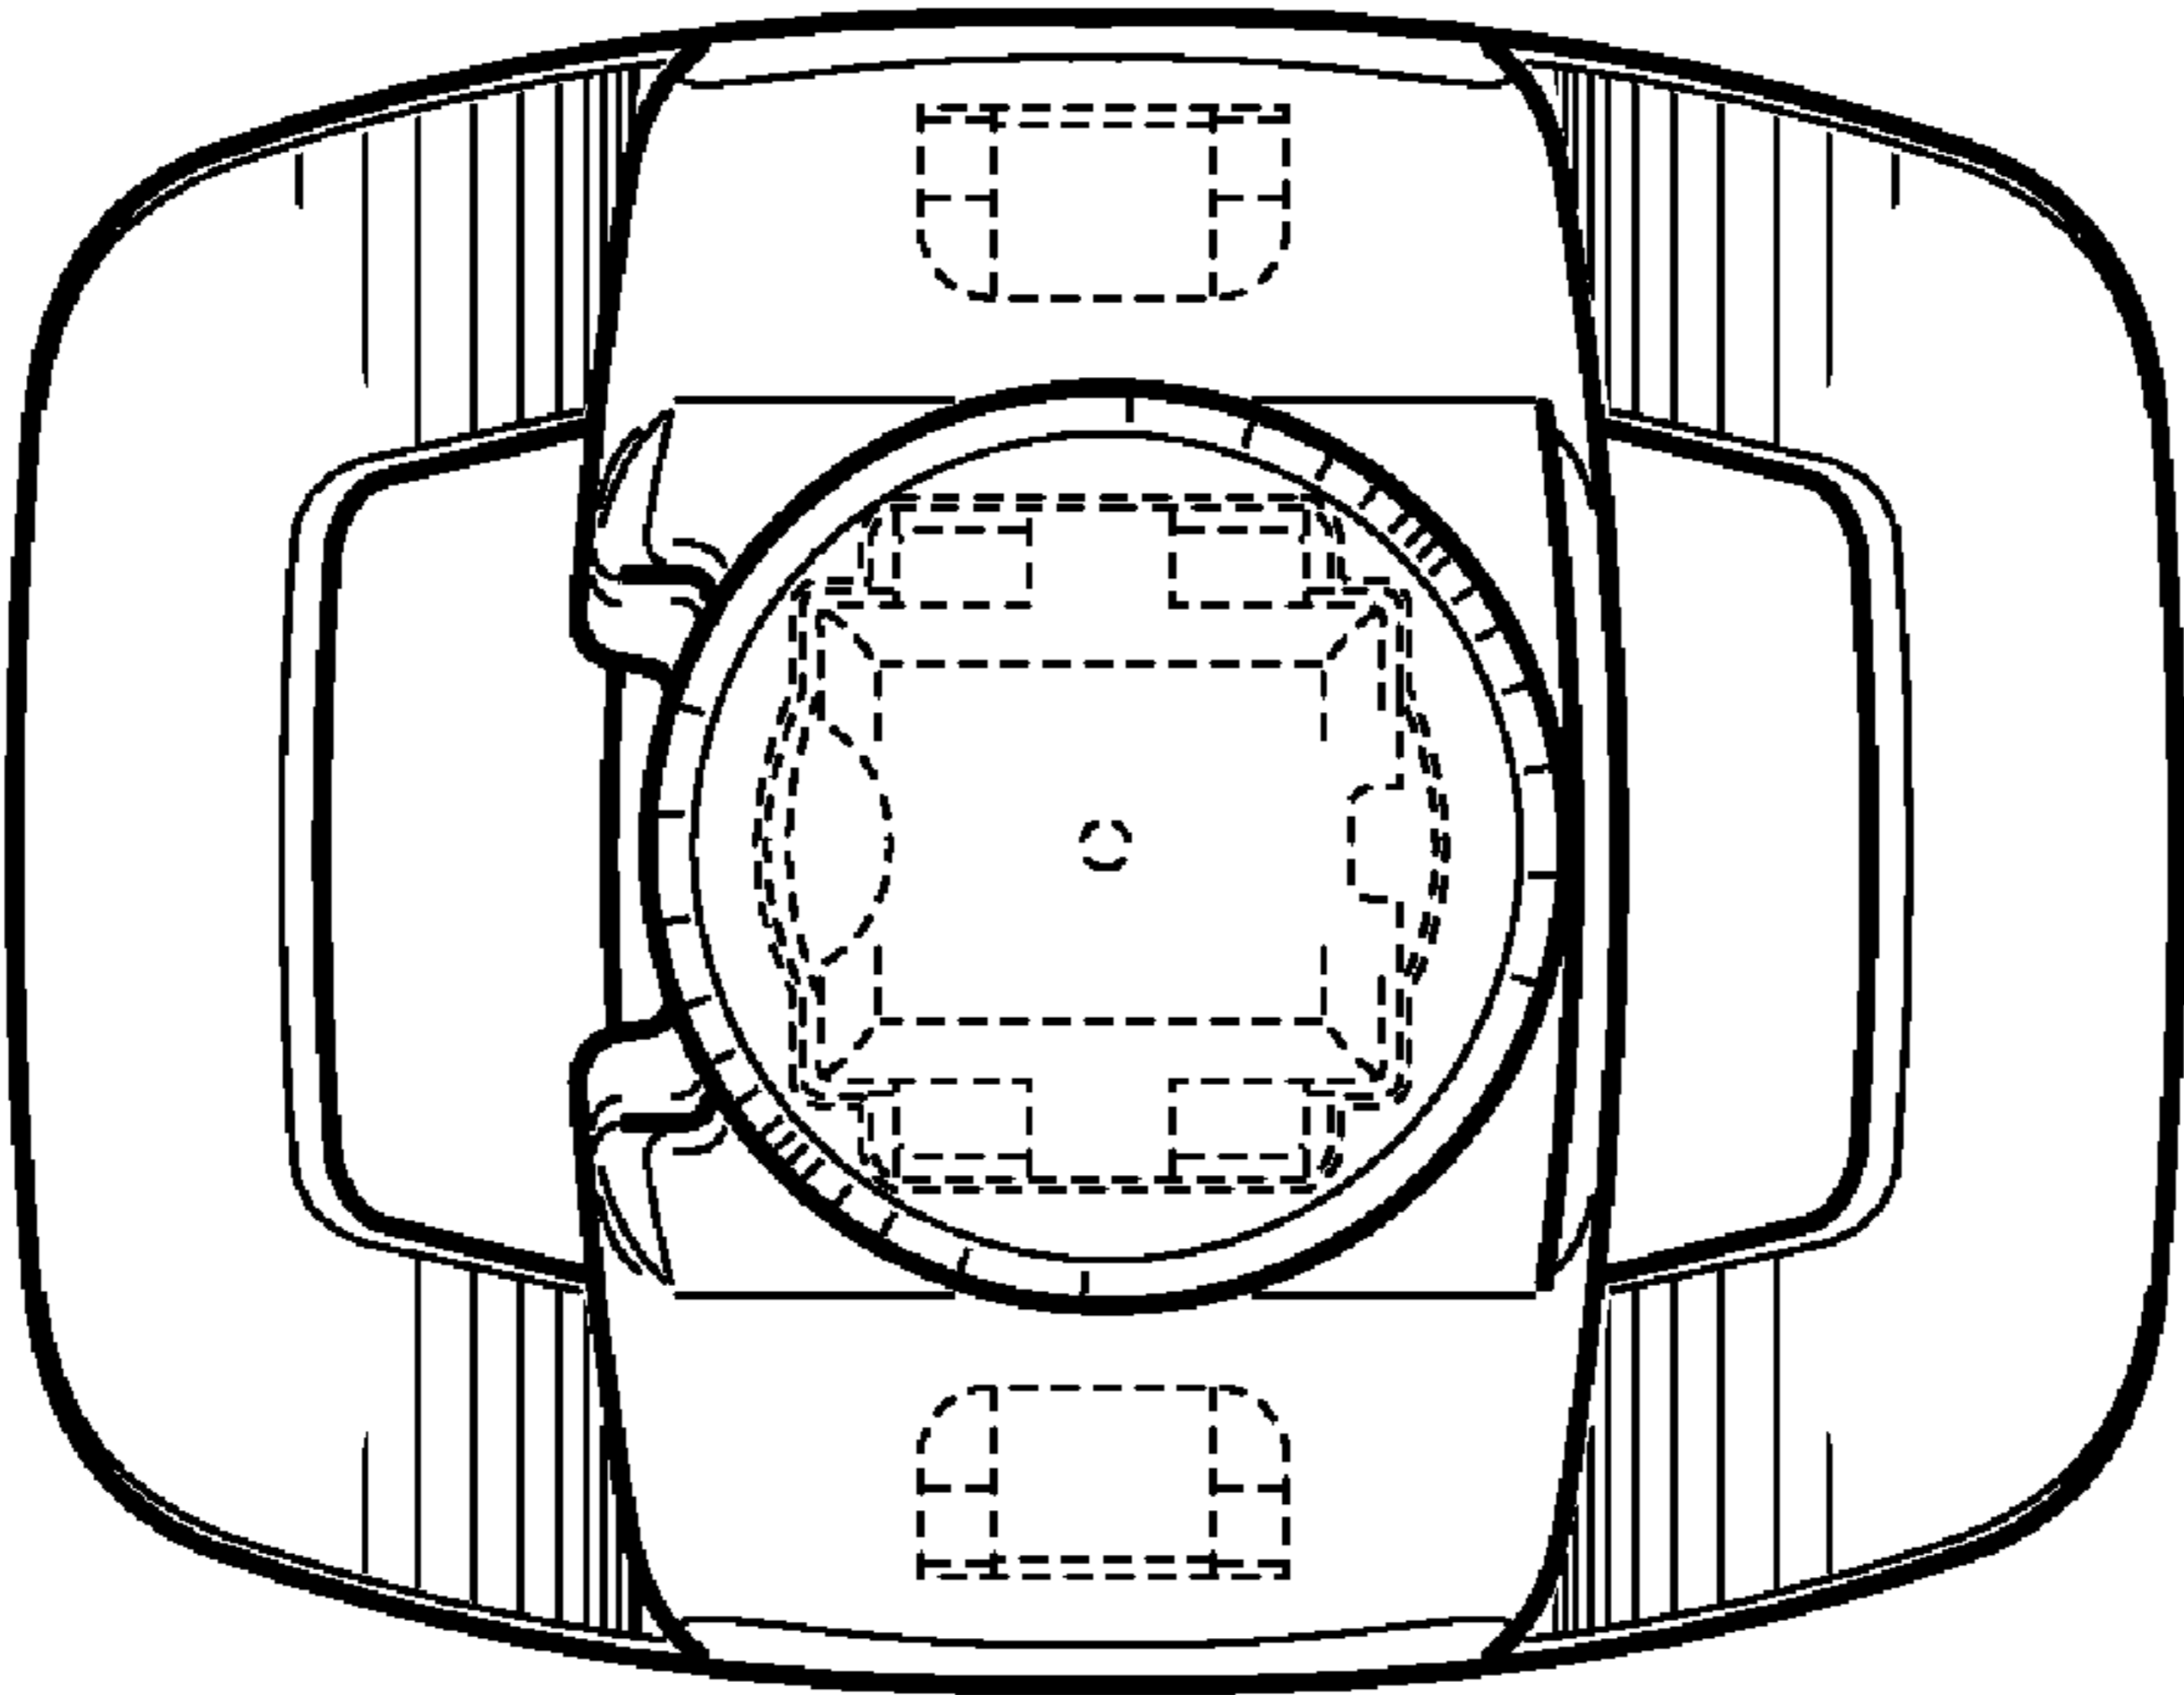


FIG. 14

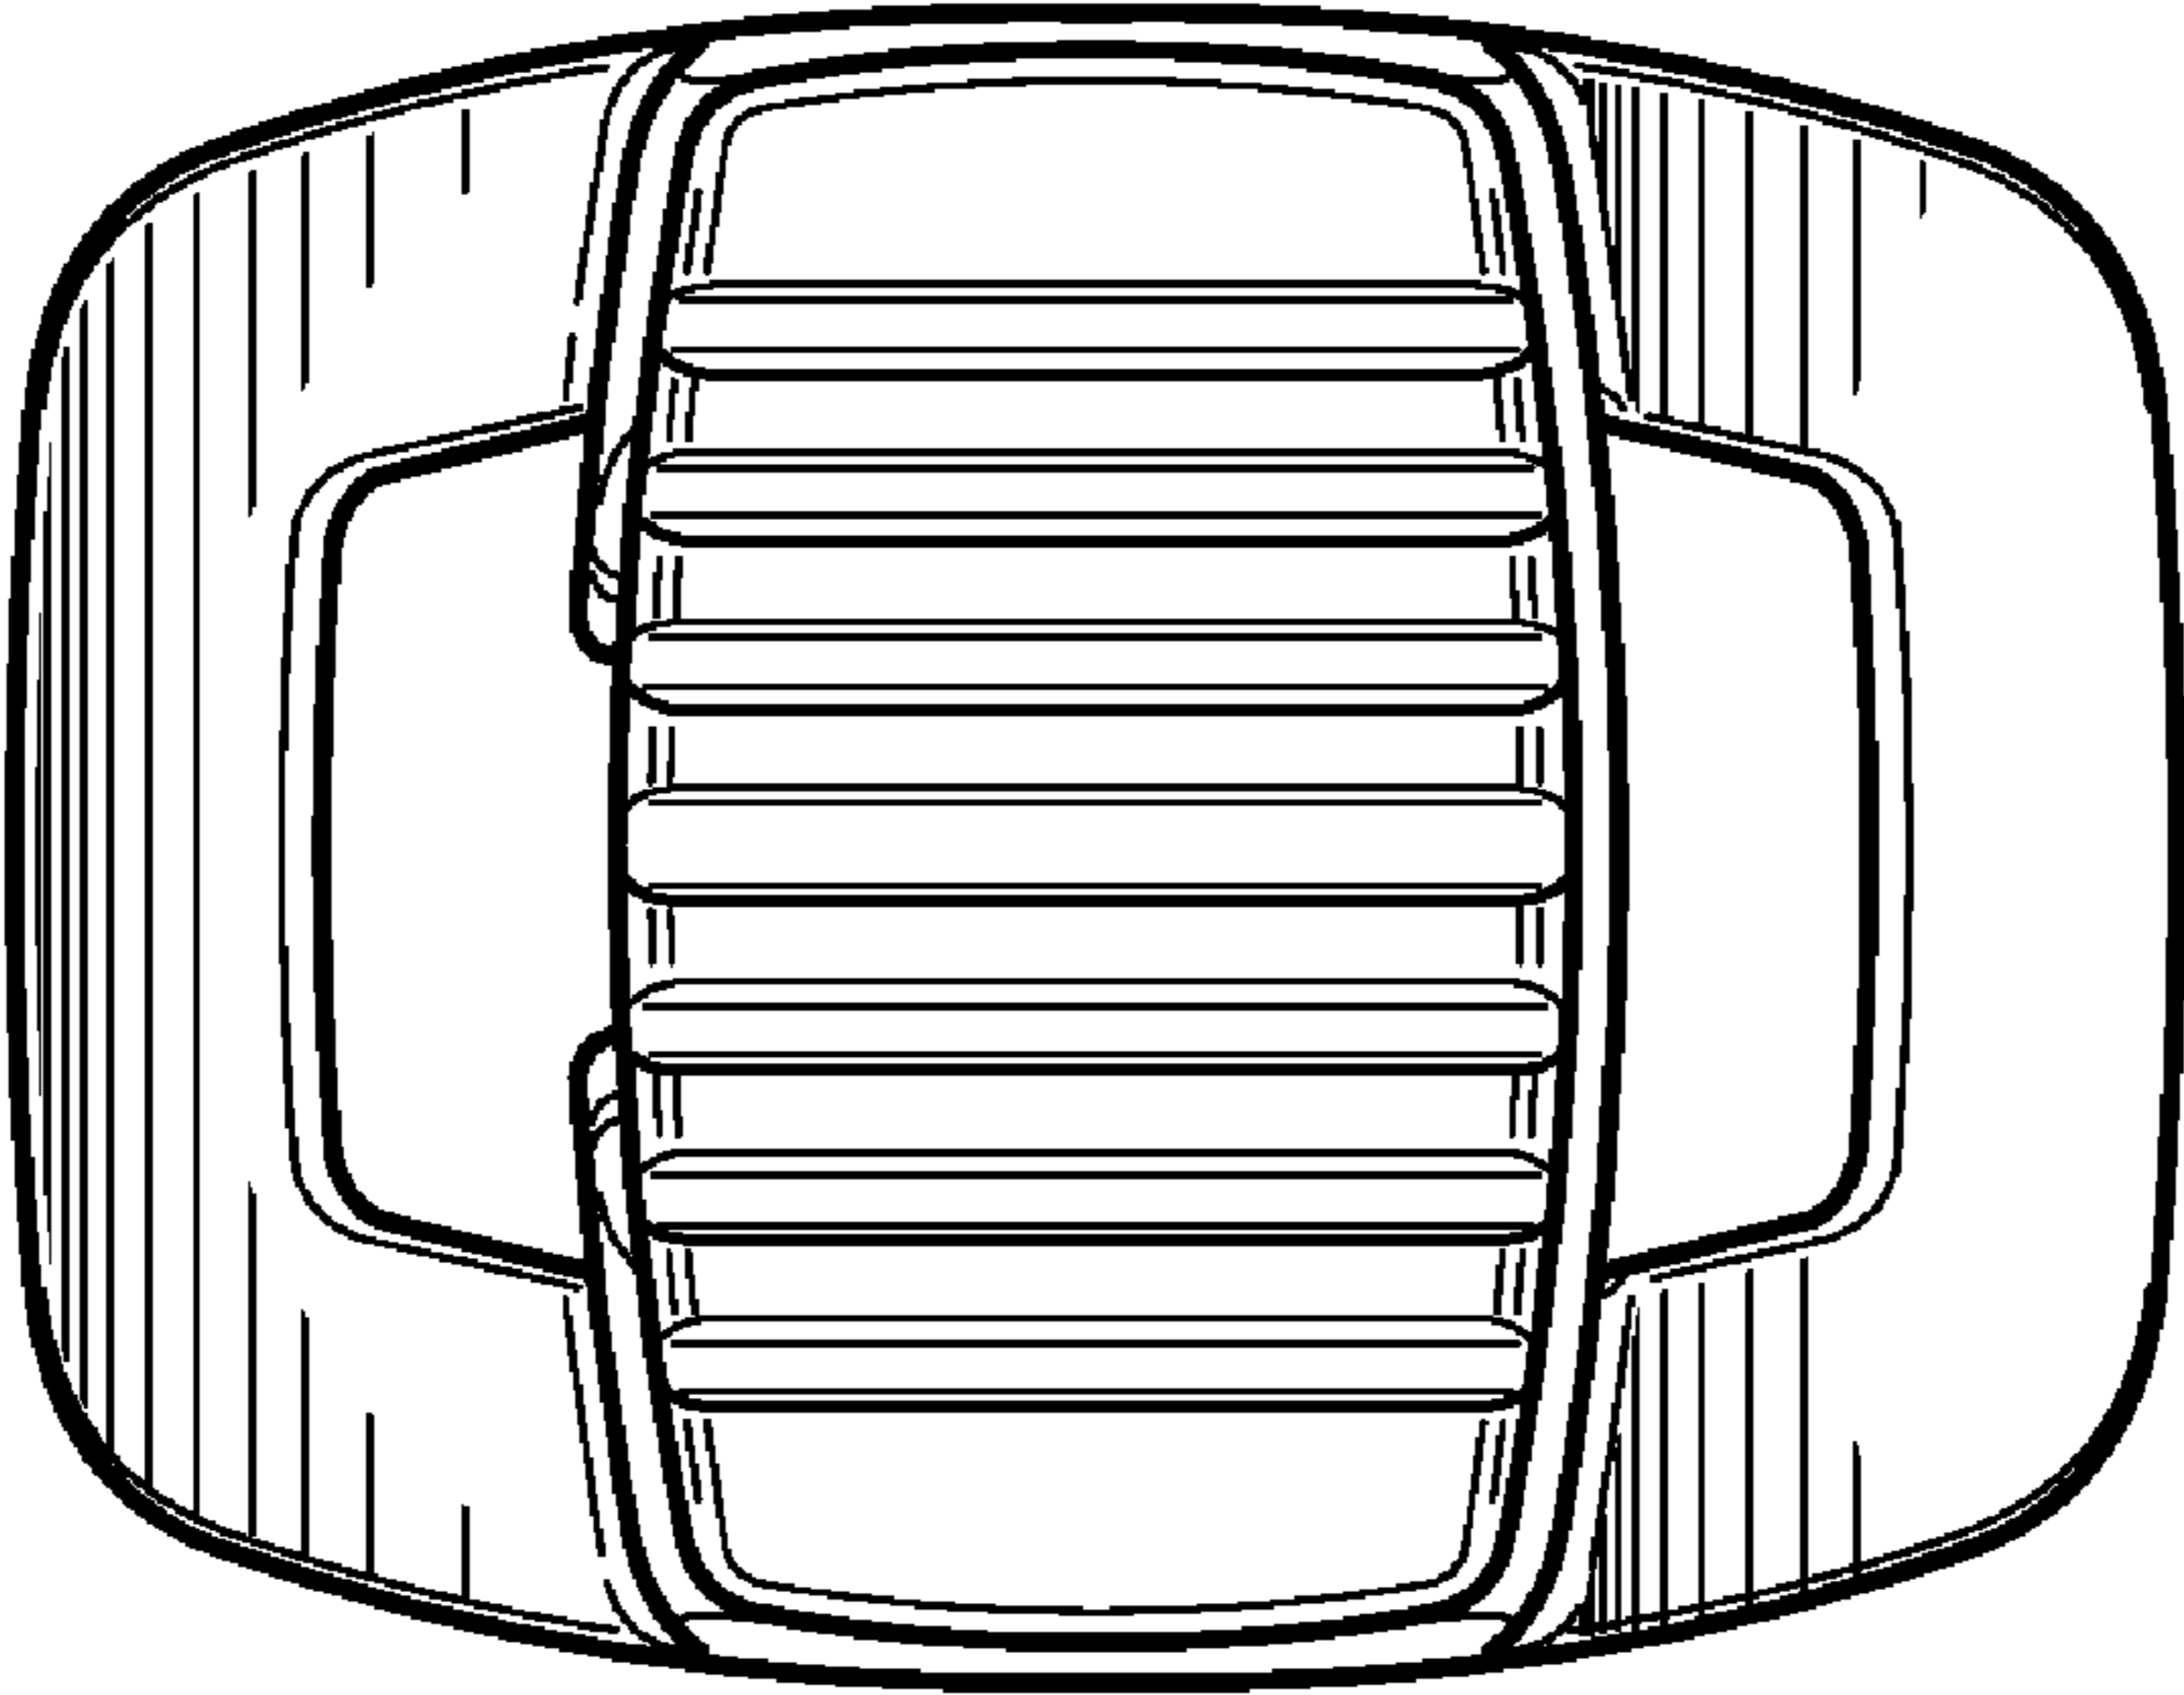


FIG. 13

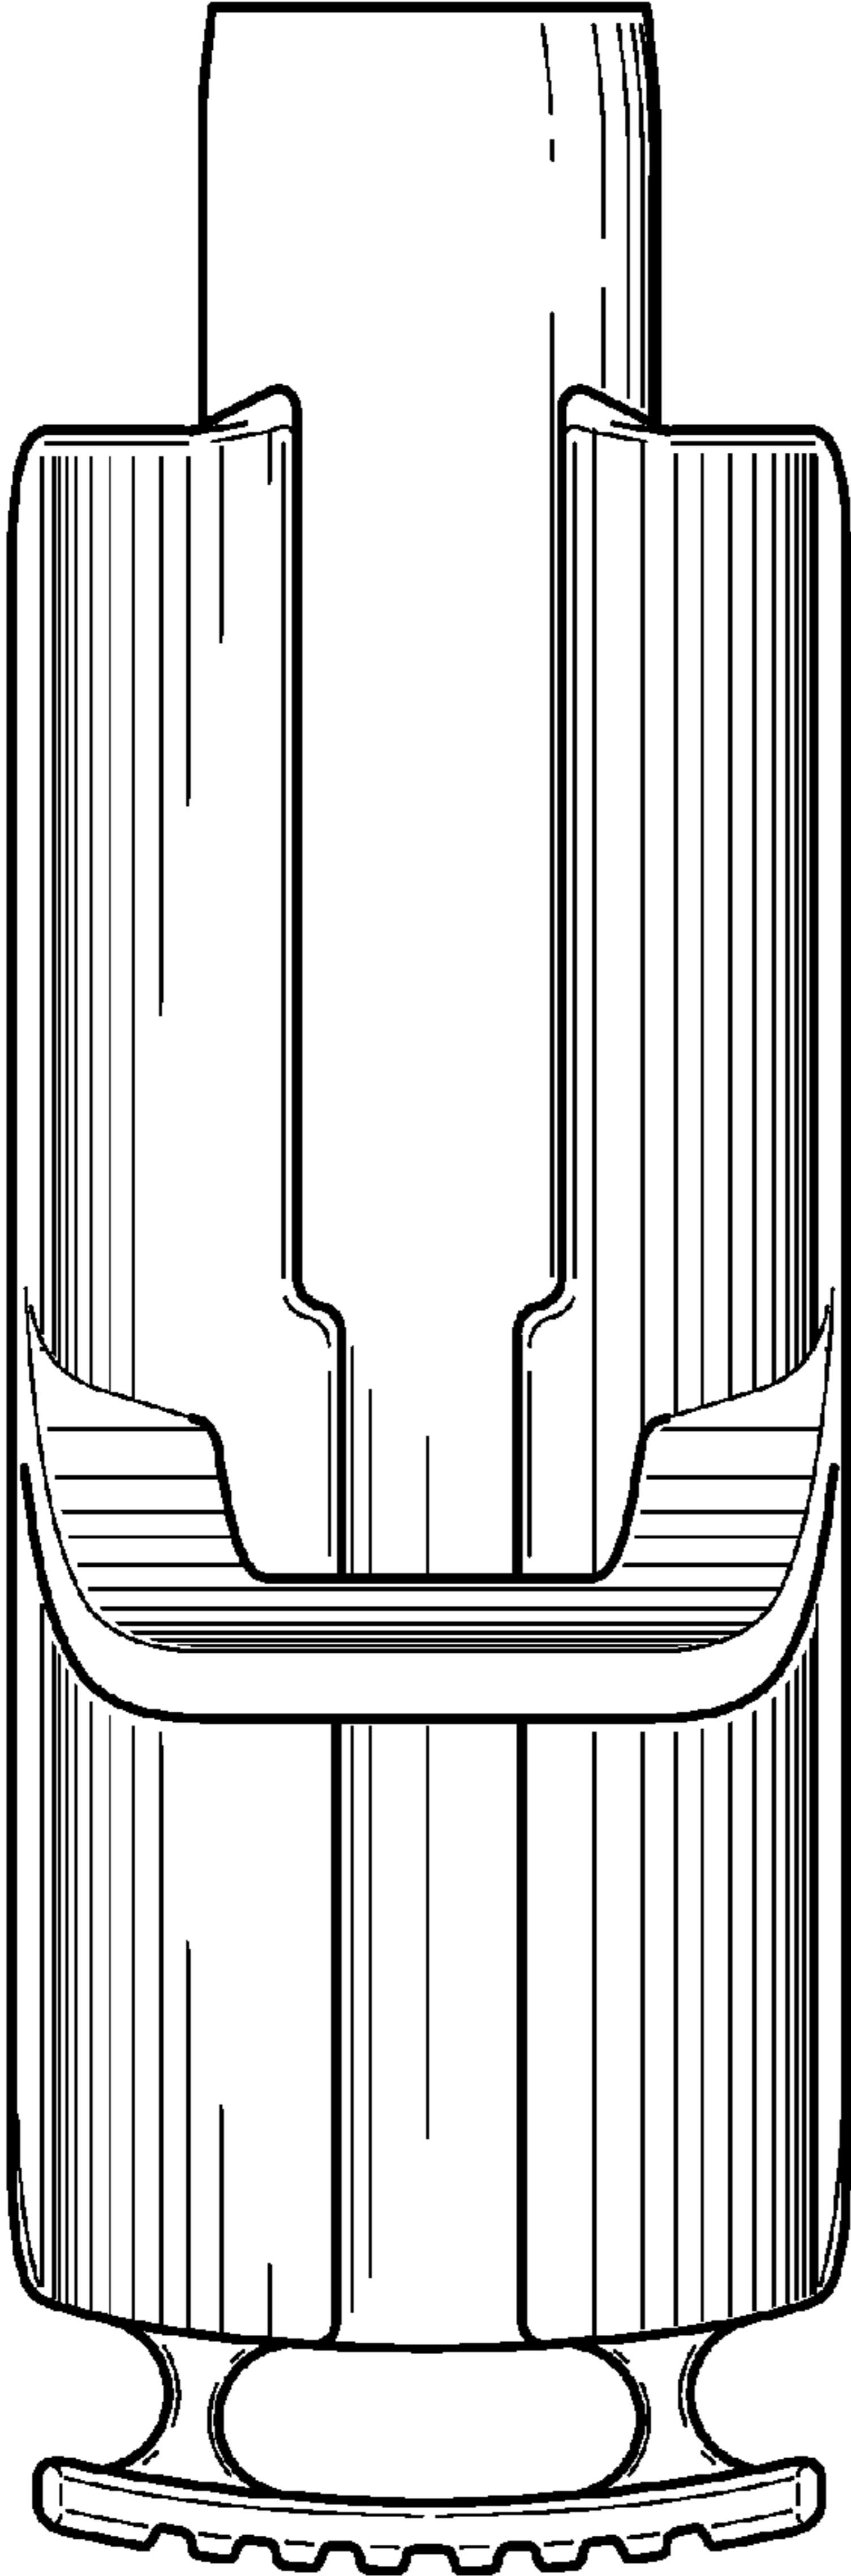


FIG. 15

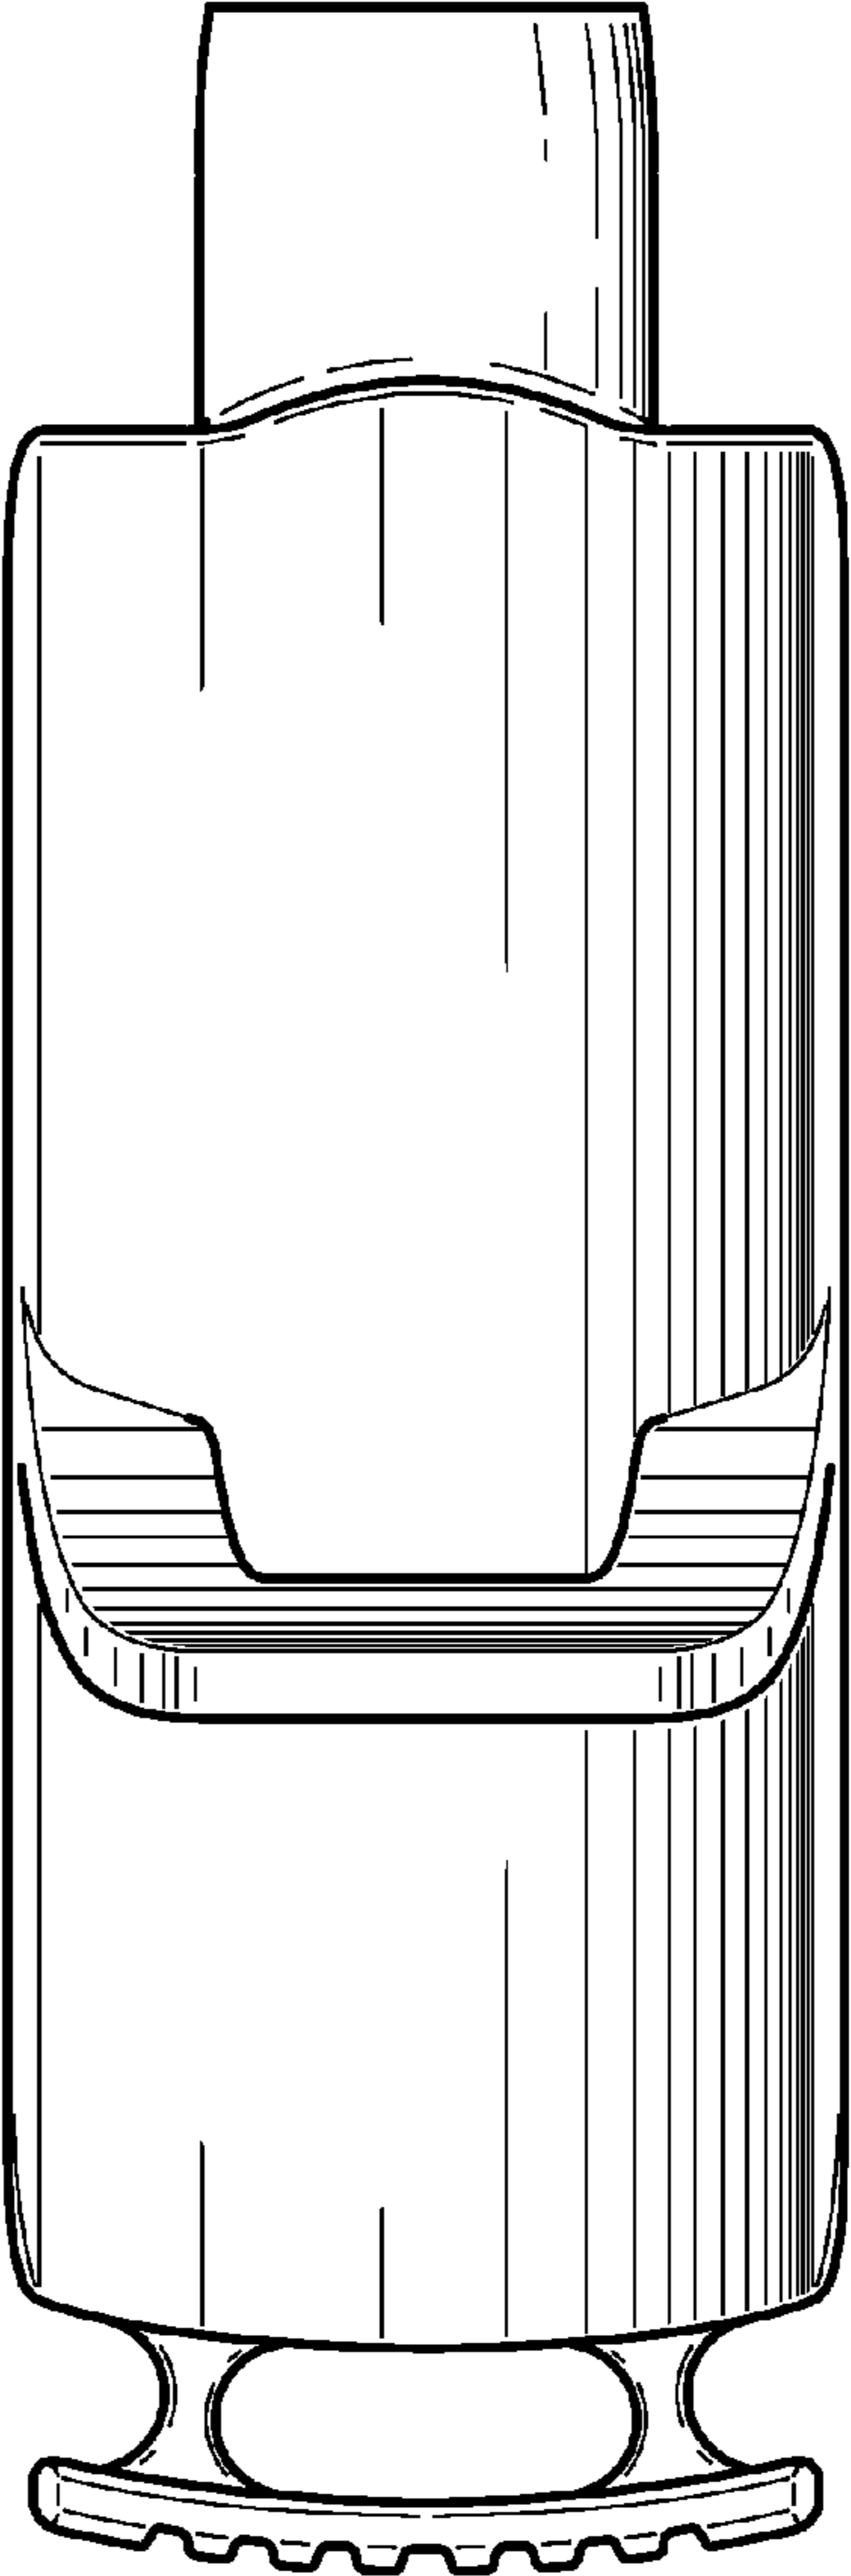


FIG. 16