



US00D645974S

(12) **United States Design Patent**
Roos et al.

(10) **Patent No.:** **US D645,974 S**
(45) **Date of Patent:** **** Sep. 27, 2011**

(54) **HEMATOLOGY TEST CASSETTE WITH
PREFILLED REAGENTS**

(75) Inventors: **Bjorn Roos**, Stockholm (SE); **Lennart
Niklasson**, Sollentuna (SE)

(73) Assignee: **Boule Medical AB**, Stockholm (SE)

(**) Term: **14 Years**

(21) Appl. No.: **29/391,164**

(22) Filed: **May 4, 2011**

Related U.S. Application Data

(60) Division of application No. 29/332,999, filed on Mar. 2, 2009, now Pat. No. Des. 639,978, which is a continuation-in-part of application No. 12/270,083, filed on Nov. 13, 2008.

(51) **LOC (9) Cl.** **24-02**

(52) **U.S. Cl.** **D24/227**

(58) **Field of Classification Search** D24/111,
D24/107-108, 169, 216, 227-232; 604/30,
604/34, 82, 113-114, 153; 417/474; 422/1,
422/61, 68.1, 99-104, 129; 600/300, 301,
600/368, 372, 481, 529, 544, 554, 561
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D305,150 S * 12/1989 Pastrone D24/111
D331,799 S * 12/1992 Kramer et al. D24/111
D350,823 S * 9/1994 Lanigan D24/111
D398,051 S * 9/1998 Lanigan et al. D24/108
D556,909 S * 12/2007 Reihanifam et al. D24/169
7,335,339 B2 * 2/2008 Berndtsson 422/549

(Continued)

FOREIGN PATENT DOCUMENTS

WO 2004/045770 6/2004

Primary Examiner — T. Chase Nelson

Assistant Examiner — Mark Cavanna

(74) *Attorney, Agent, or Firm* — Greenblum & Bernstein,
PLC

(57) **CLAIM**

The ornamental design for a hematology test cassette with prefilled reagents, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a hematology test cassette with prefilled reagents showing an embodiment of the new design, the cassette being translucent and having transparent diaphragms covering an upper surface and a bottom surface of the cassette, respectively, and with a label attached on an area of the upper surface;

FIG. 2 is a top plan view of the cassette shown in FIG. 1;

FIG. 3 is a bottom plan view of the cassette shown in FIG. 1;

FIG. 4 is a front elevational view of the cassette shown in FIG. 1;

FIG. 5 is a rear elevational view of the cassette shown in FIG. 1;

FIG. 6 is a left side elevational view of the cassette shown in FIG. 1;

FIG. 7 is a right side elevational view of the cassette shown in FIG. 1;

FIG. 8 is a perspective view of the hematology test cassette with prefilled reagents showing another embodiment of the new design, the cassette being non-translucent and having non-transparent diaphragms covering the upper surface and the bottom surface of the cassette, respectively, and with a label attached on an area of the upper surface;

FIG. 9 is a top plan view of the cassette shown in FIG. 8;

FIG. 10 is a bottom plan view of the cassette shown in FIG. 8;

FIG. 11 is a front elevational view of the cassette shown in FIG. 8;



FIG. 12 is a rear elevational view of the cassette shown in FIG. 8;

FIG. 13 is a left side elevational view of the cassette shown in FIG. 8; and,

FIG. 14 is a right side elevational view of the cassette shown in FIG. 8.

The broken lines are included for the purpose of illustrating portions of the hematology test cassette with prefilled reagents, and form no part of the claimed design.

1 Claim, 6 Drawing Sheets

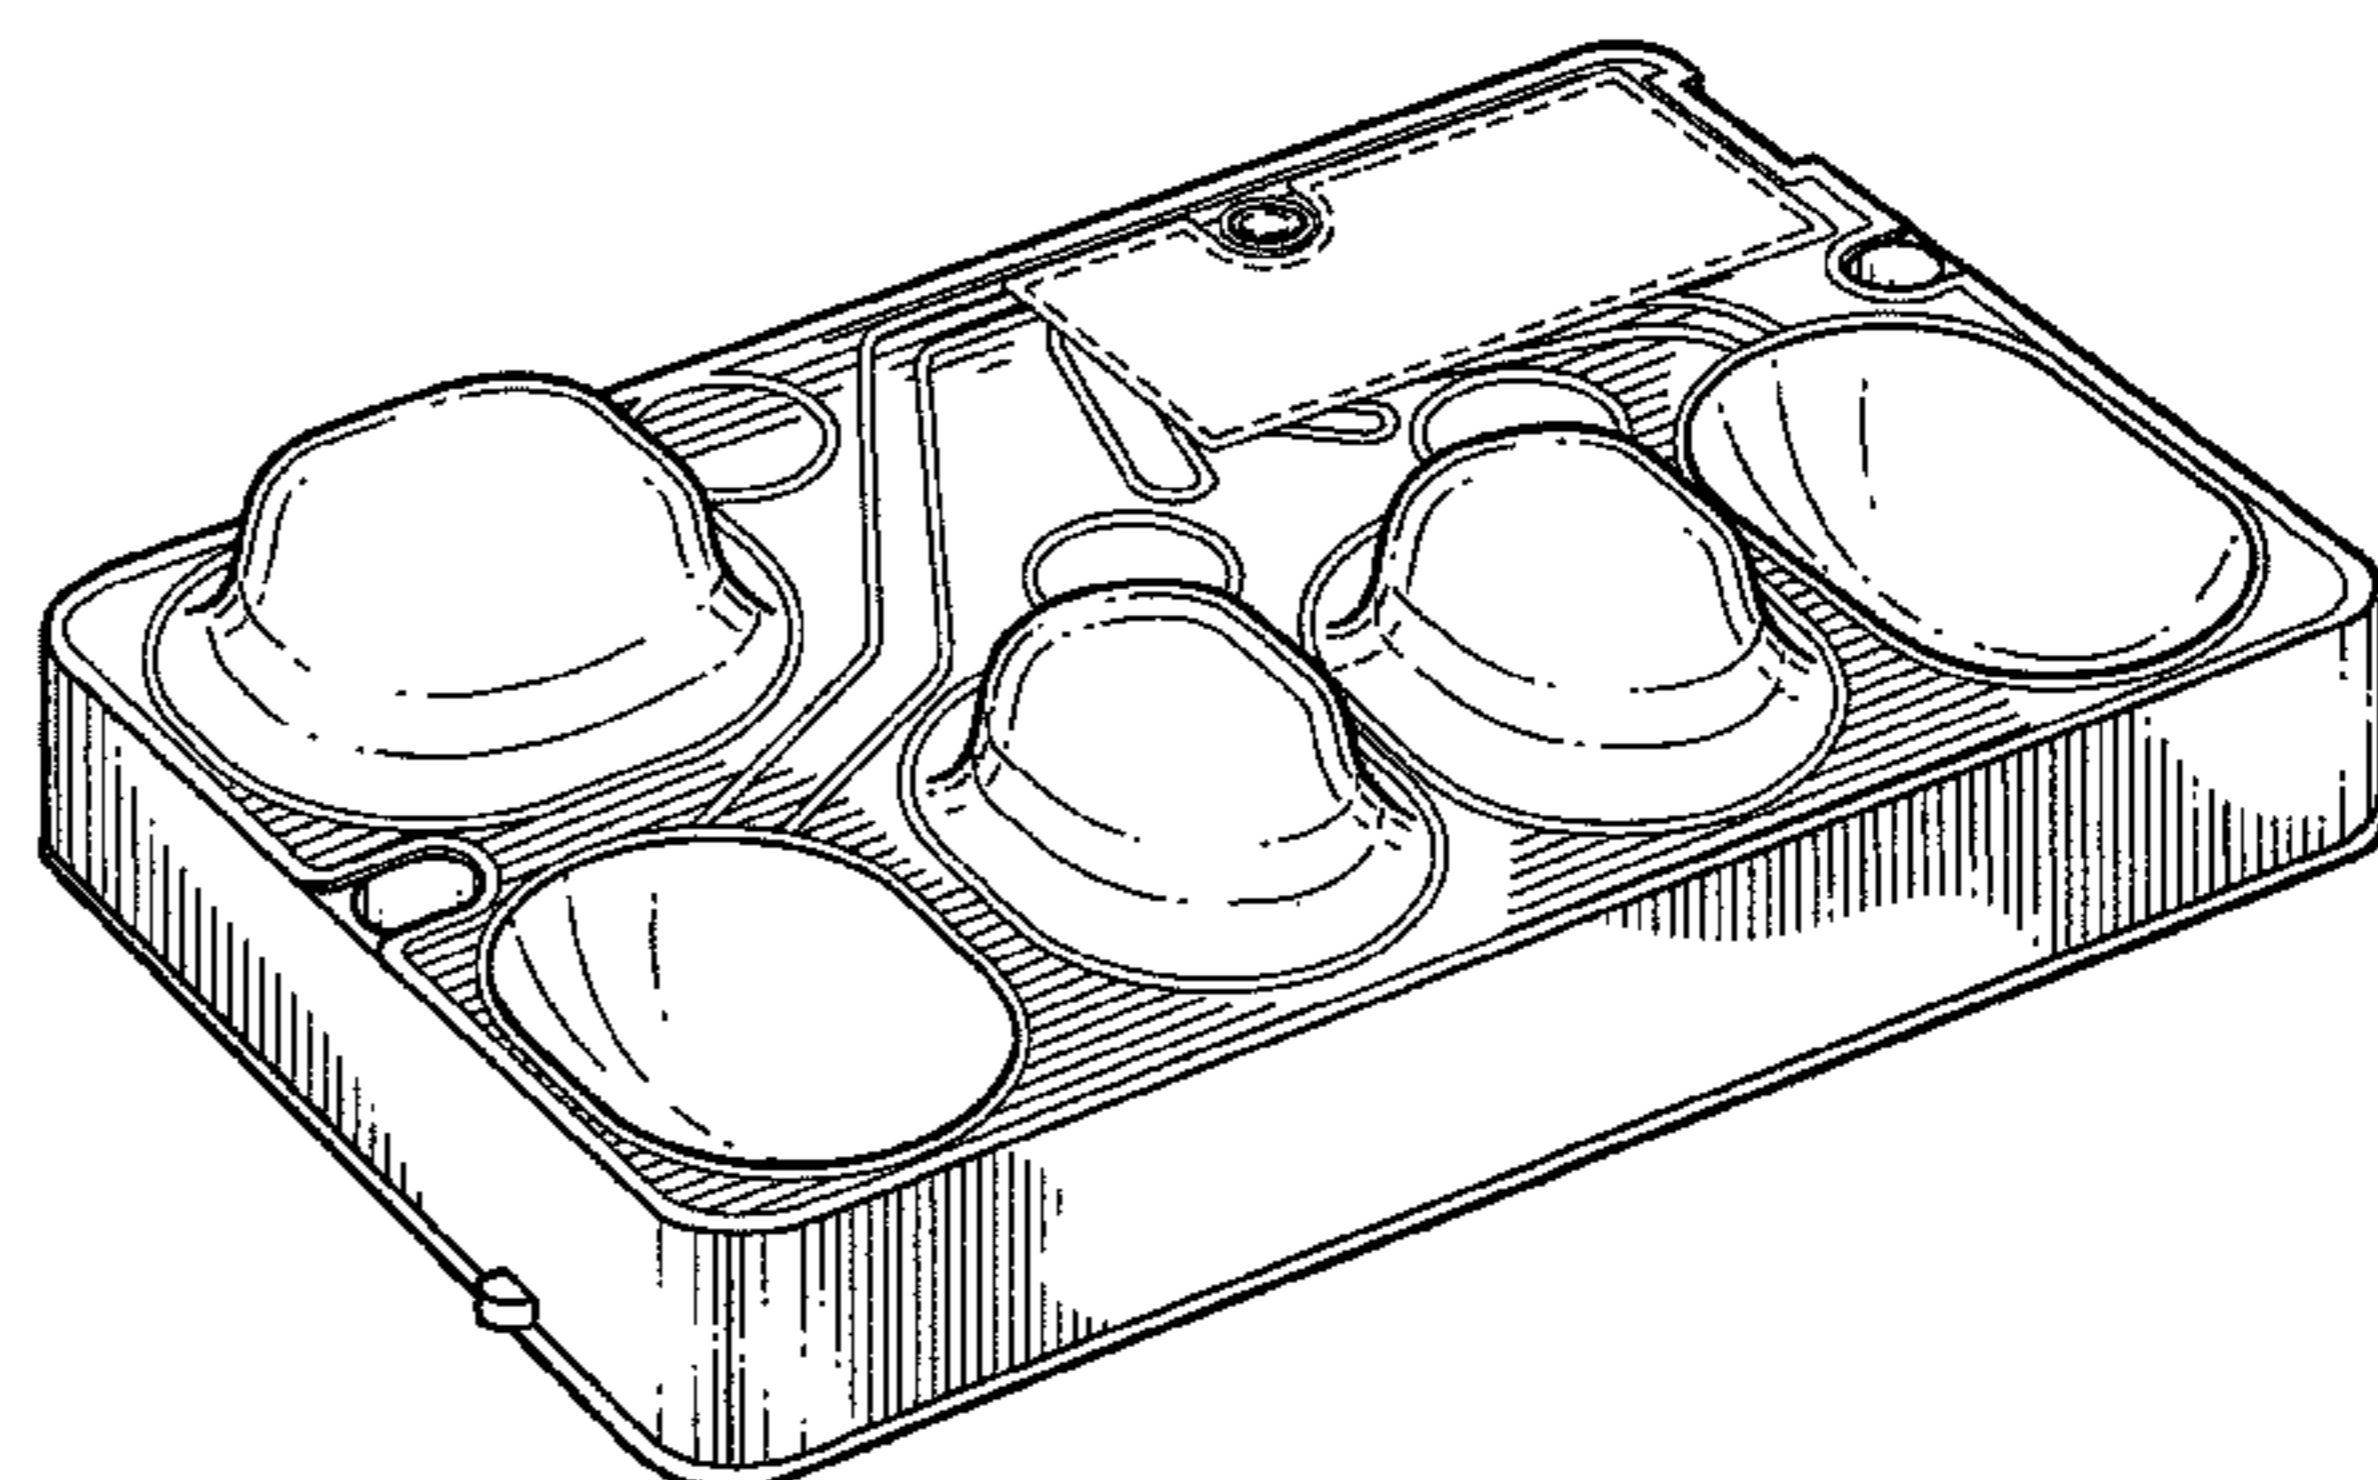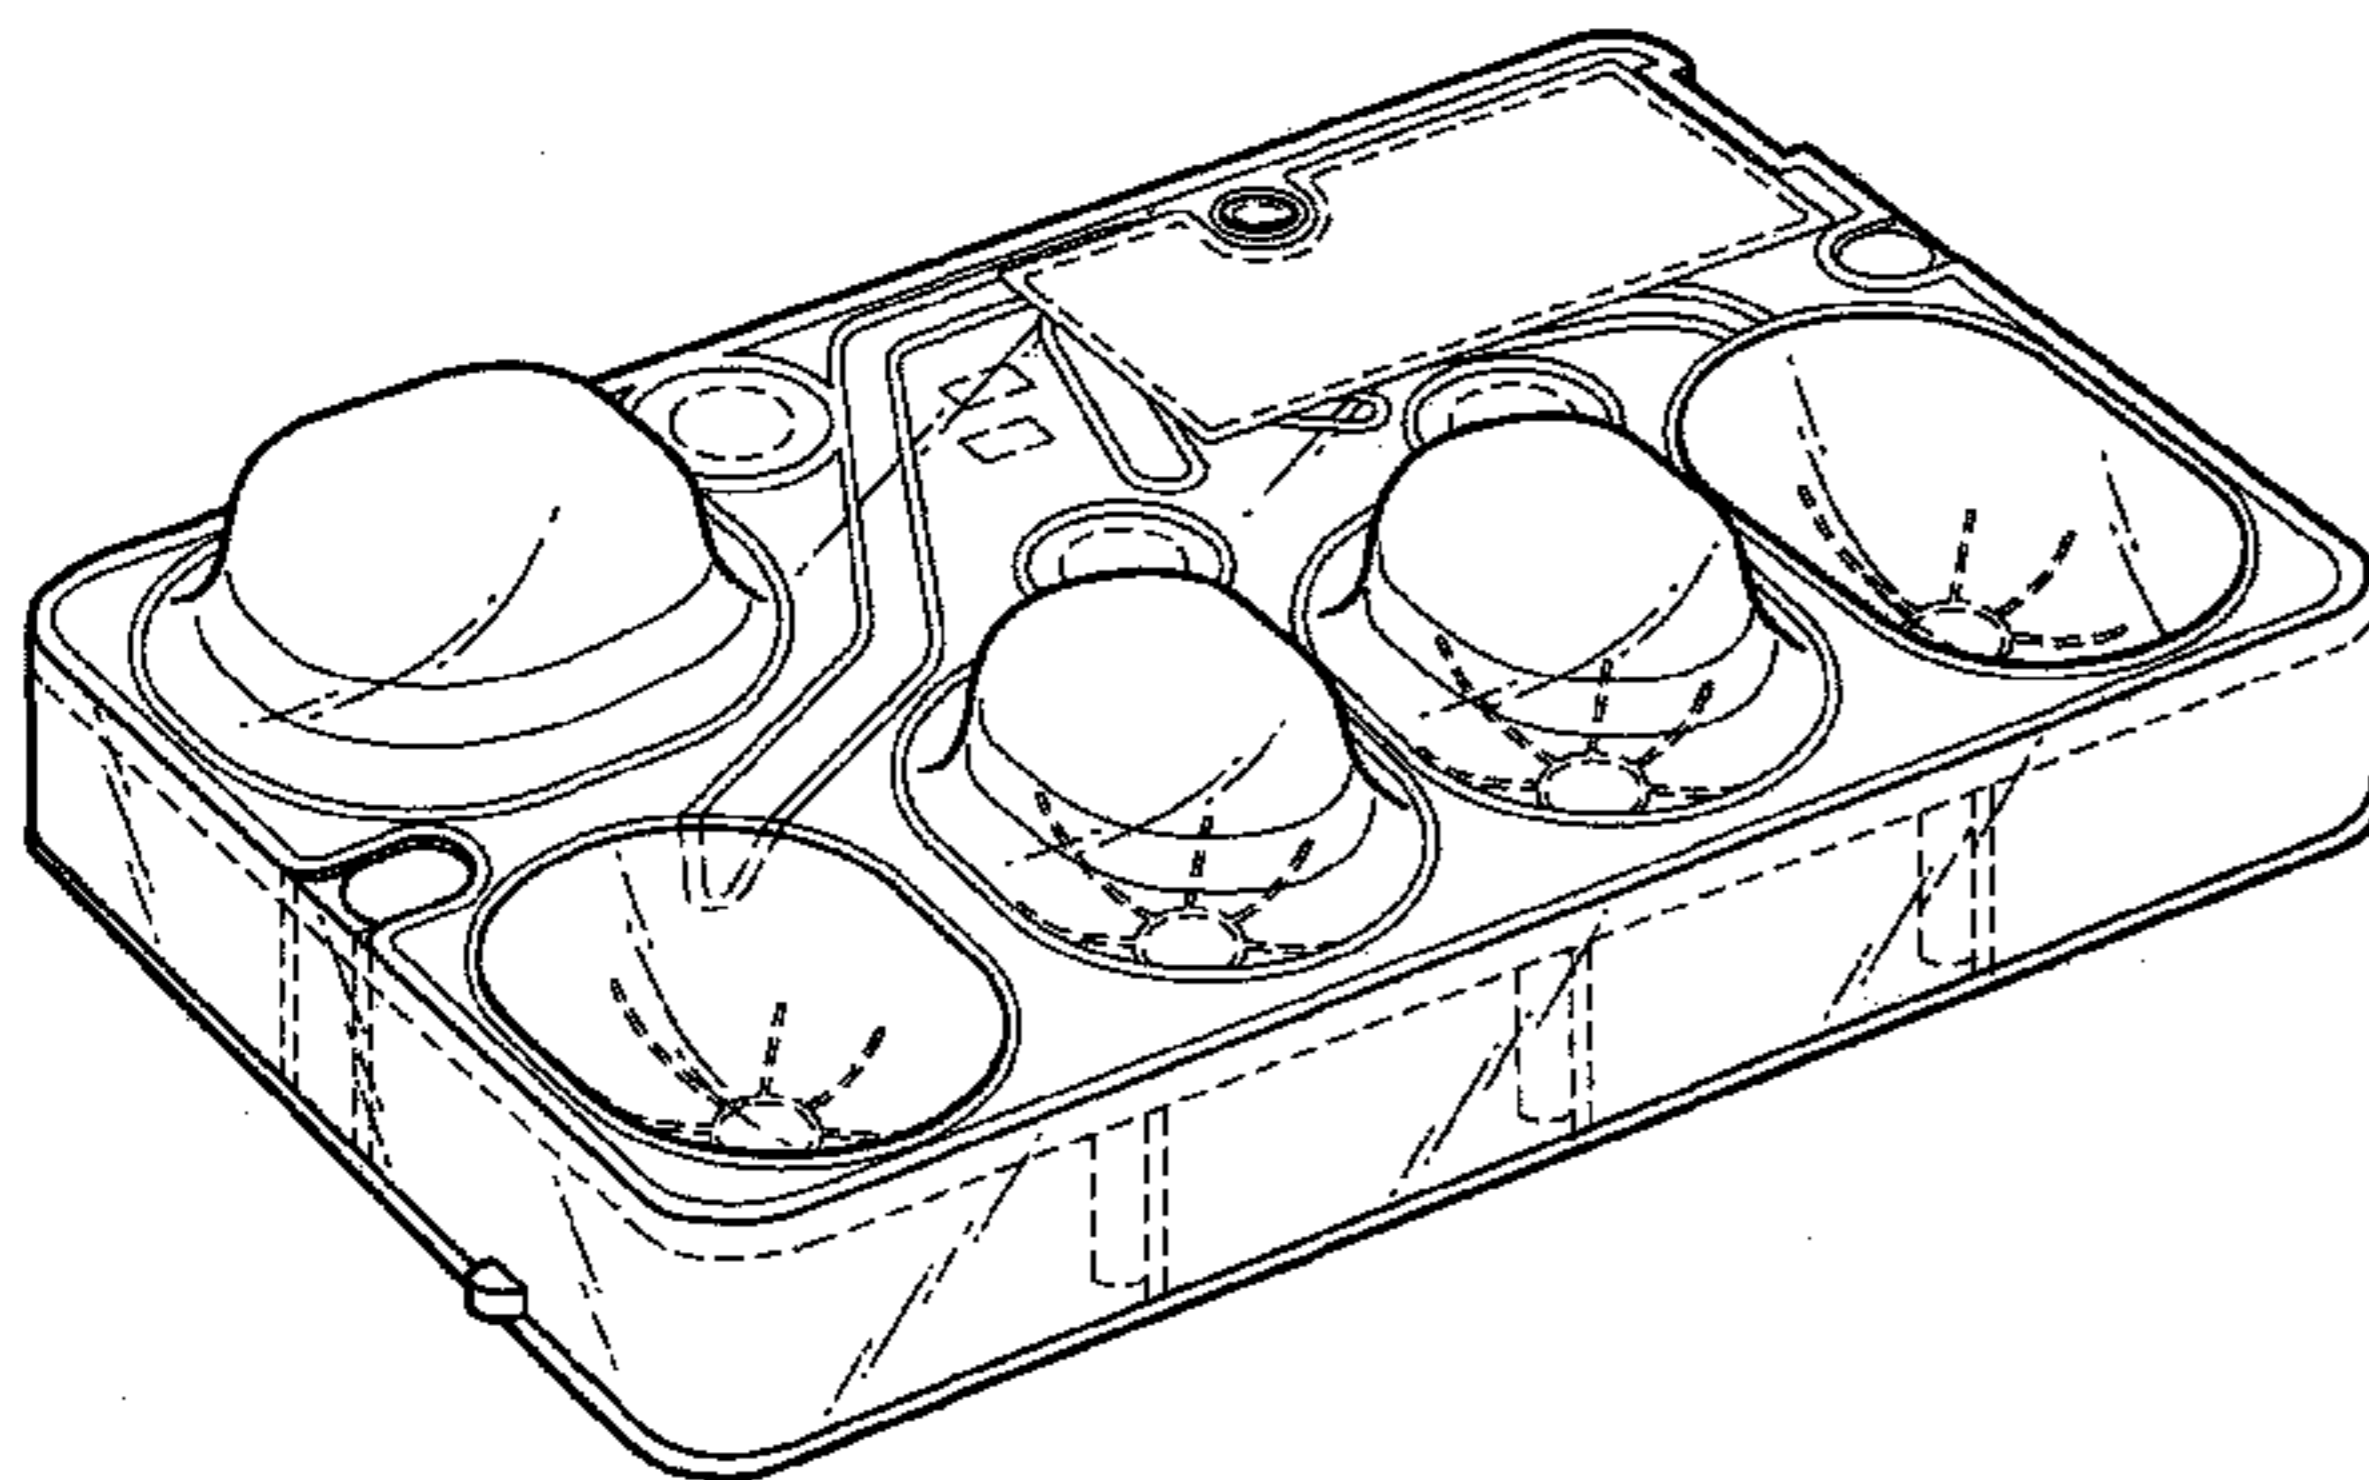

US D645,974 S

Page 2

U.S. PATENT DOCUMENTS

D576,281 S *	9/2008	Reihanifam et al.	D24/169	D615,190 S *	5/2010	McGill	D24/111
D579,553 S *	10/2008	Crnkovich et al.	D24/111	D616,539 S *	5/2010	McGill	D24/111
D615,189 S *	5/2010	McGill et al.	D24/111	2010/0120083 A1	5/2010	Ritzen et al.	

* cited by examiner

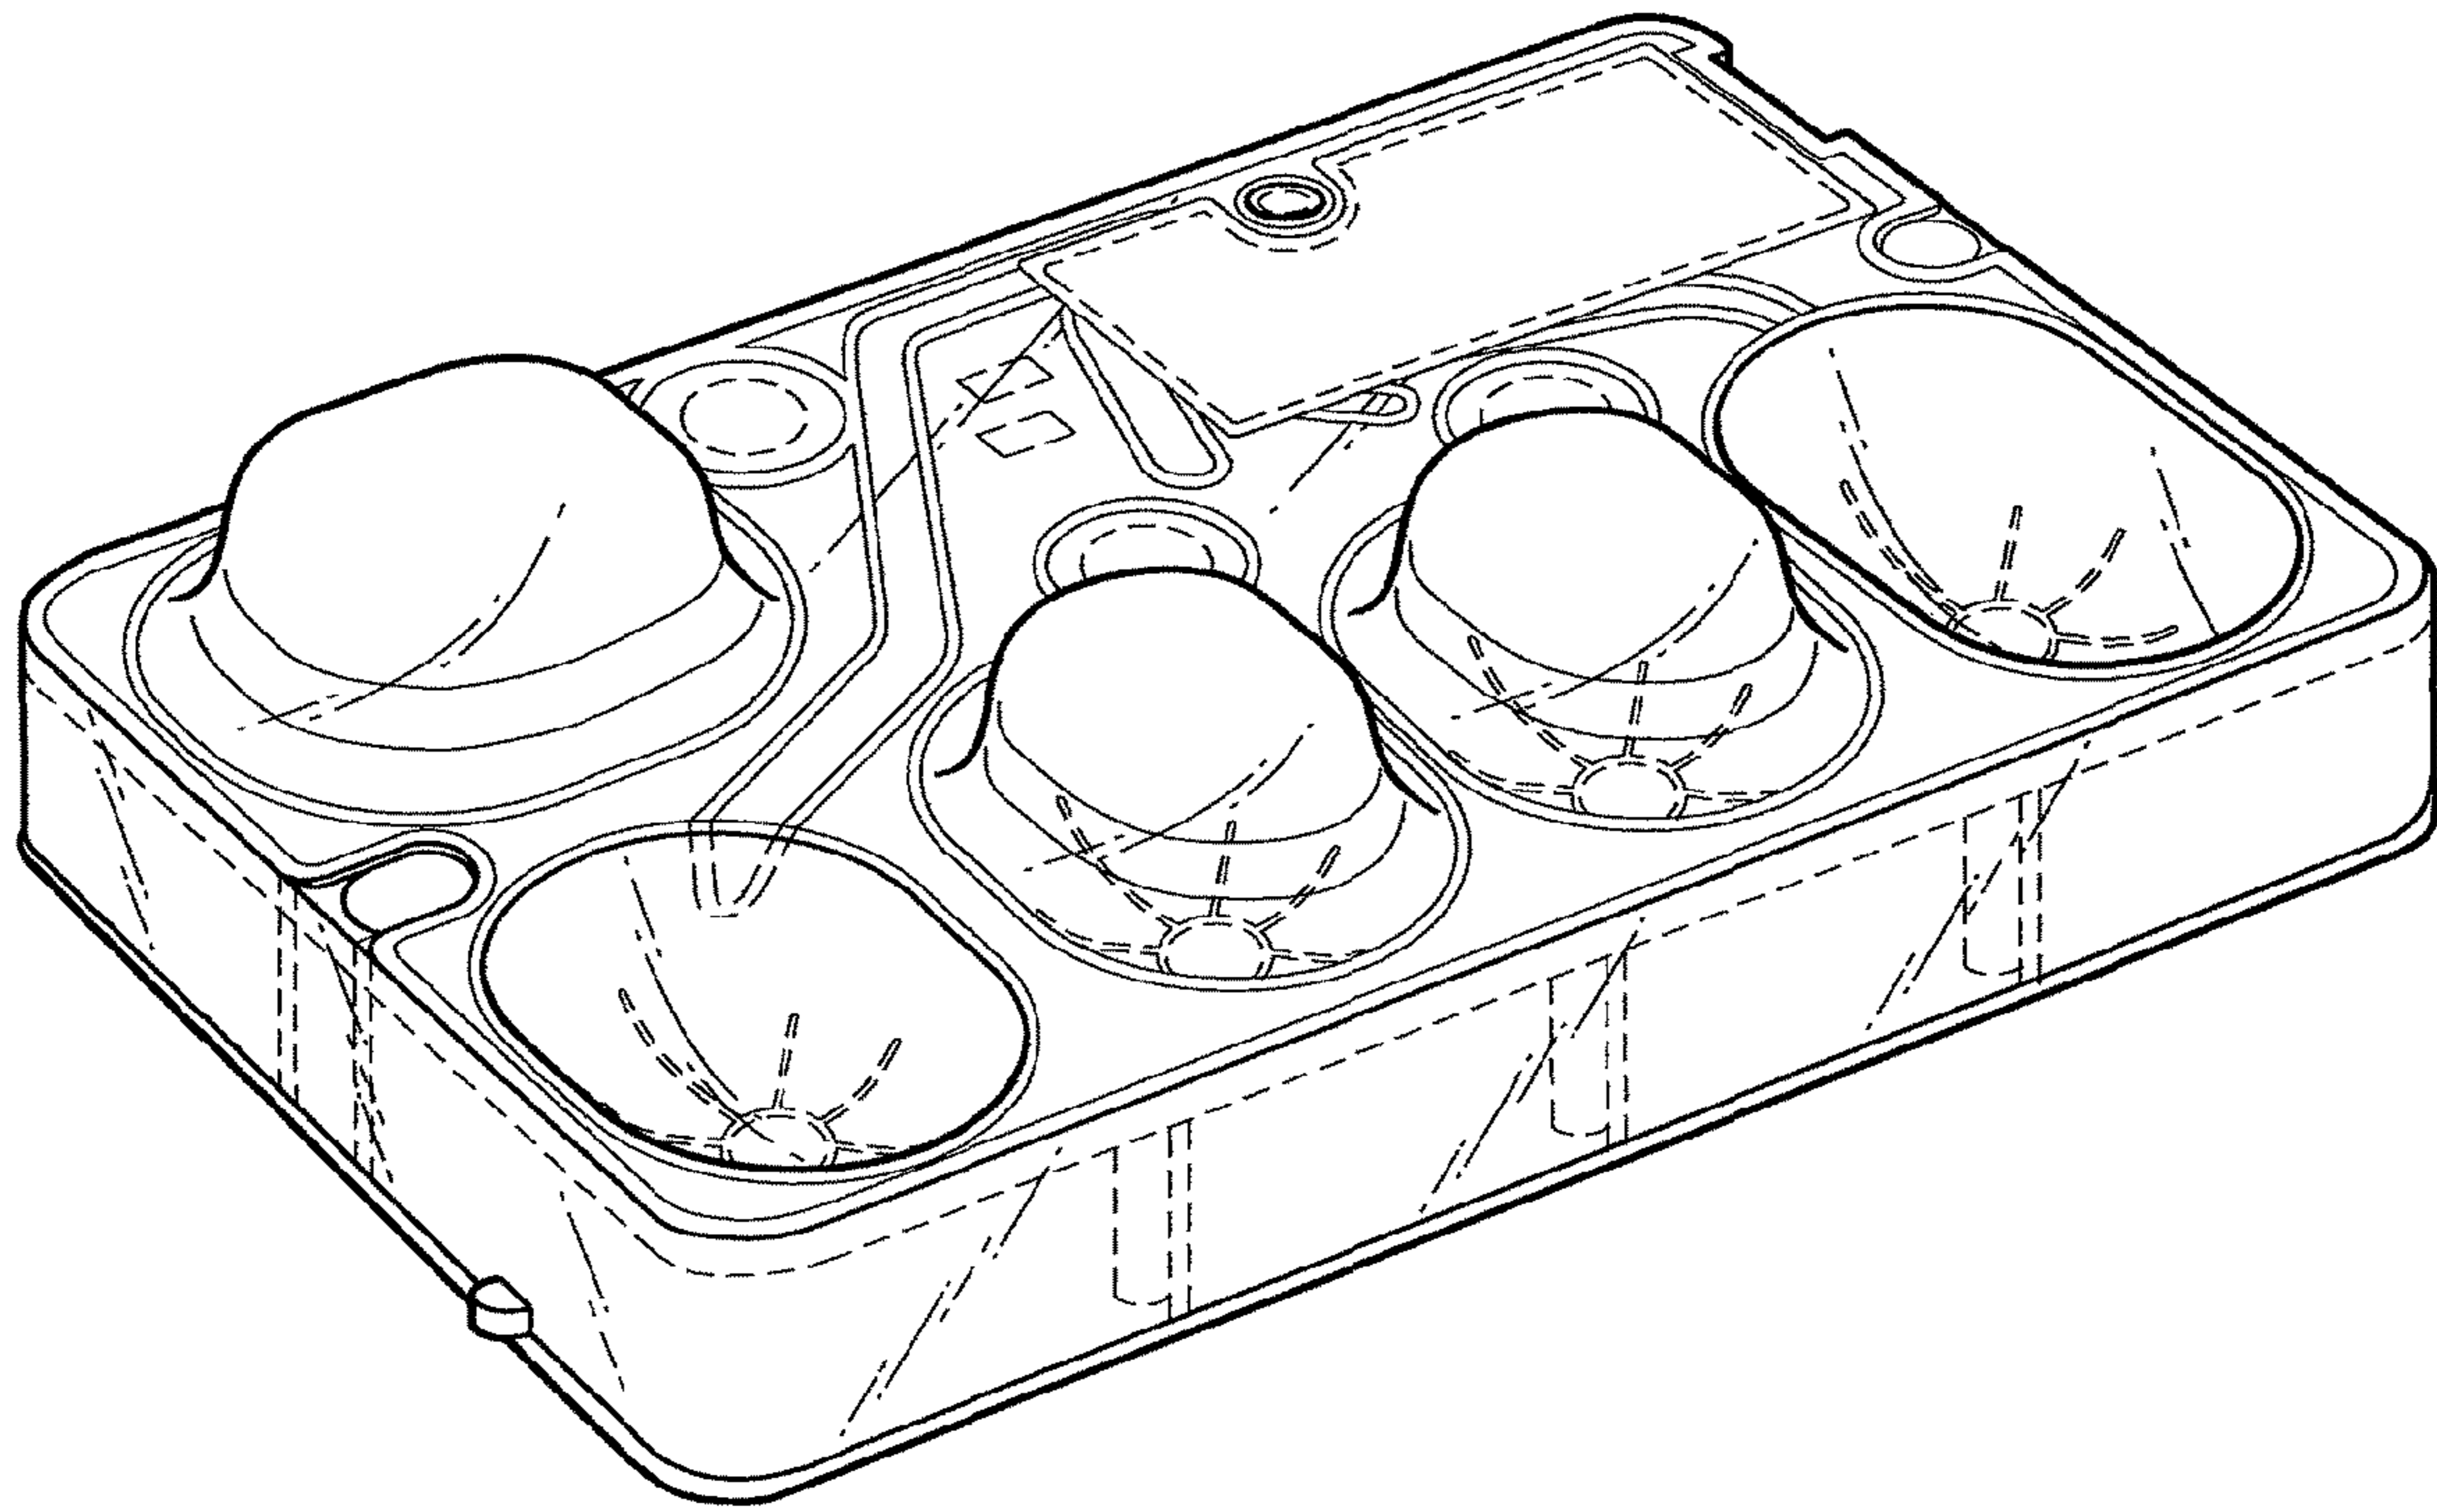


FIG. 1

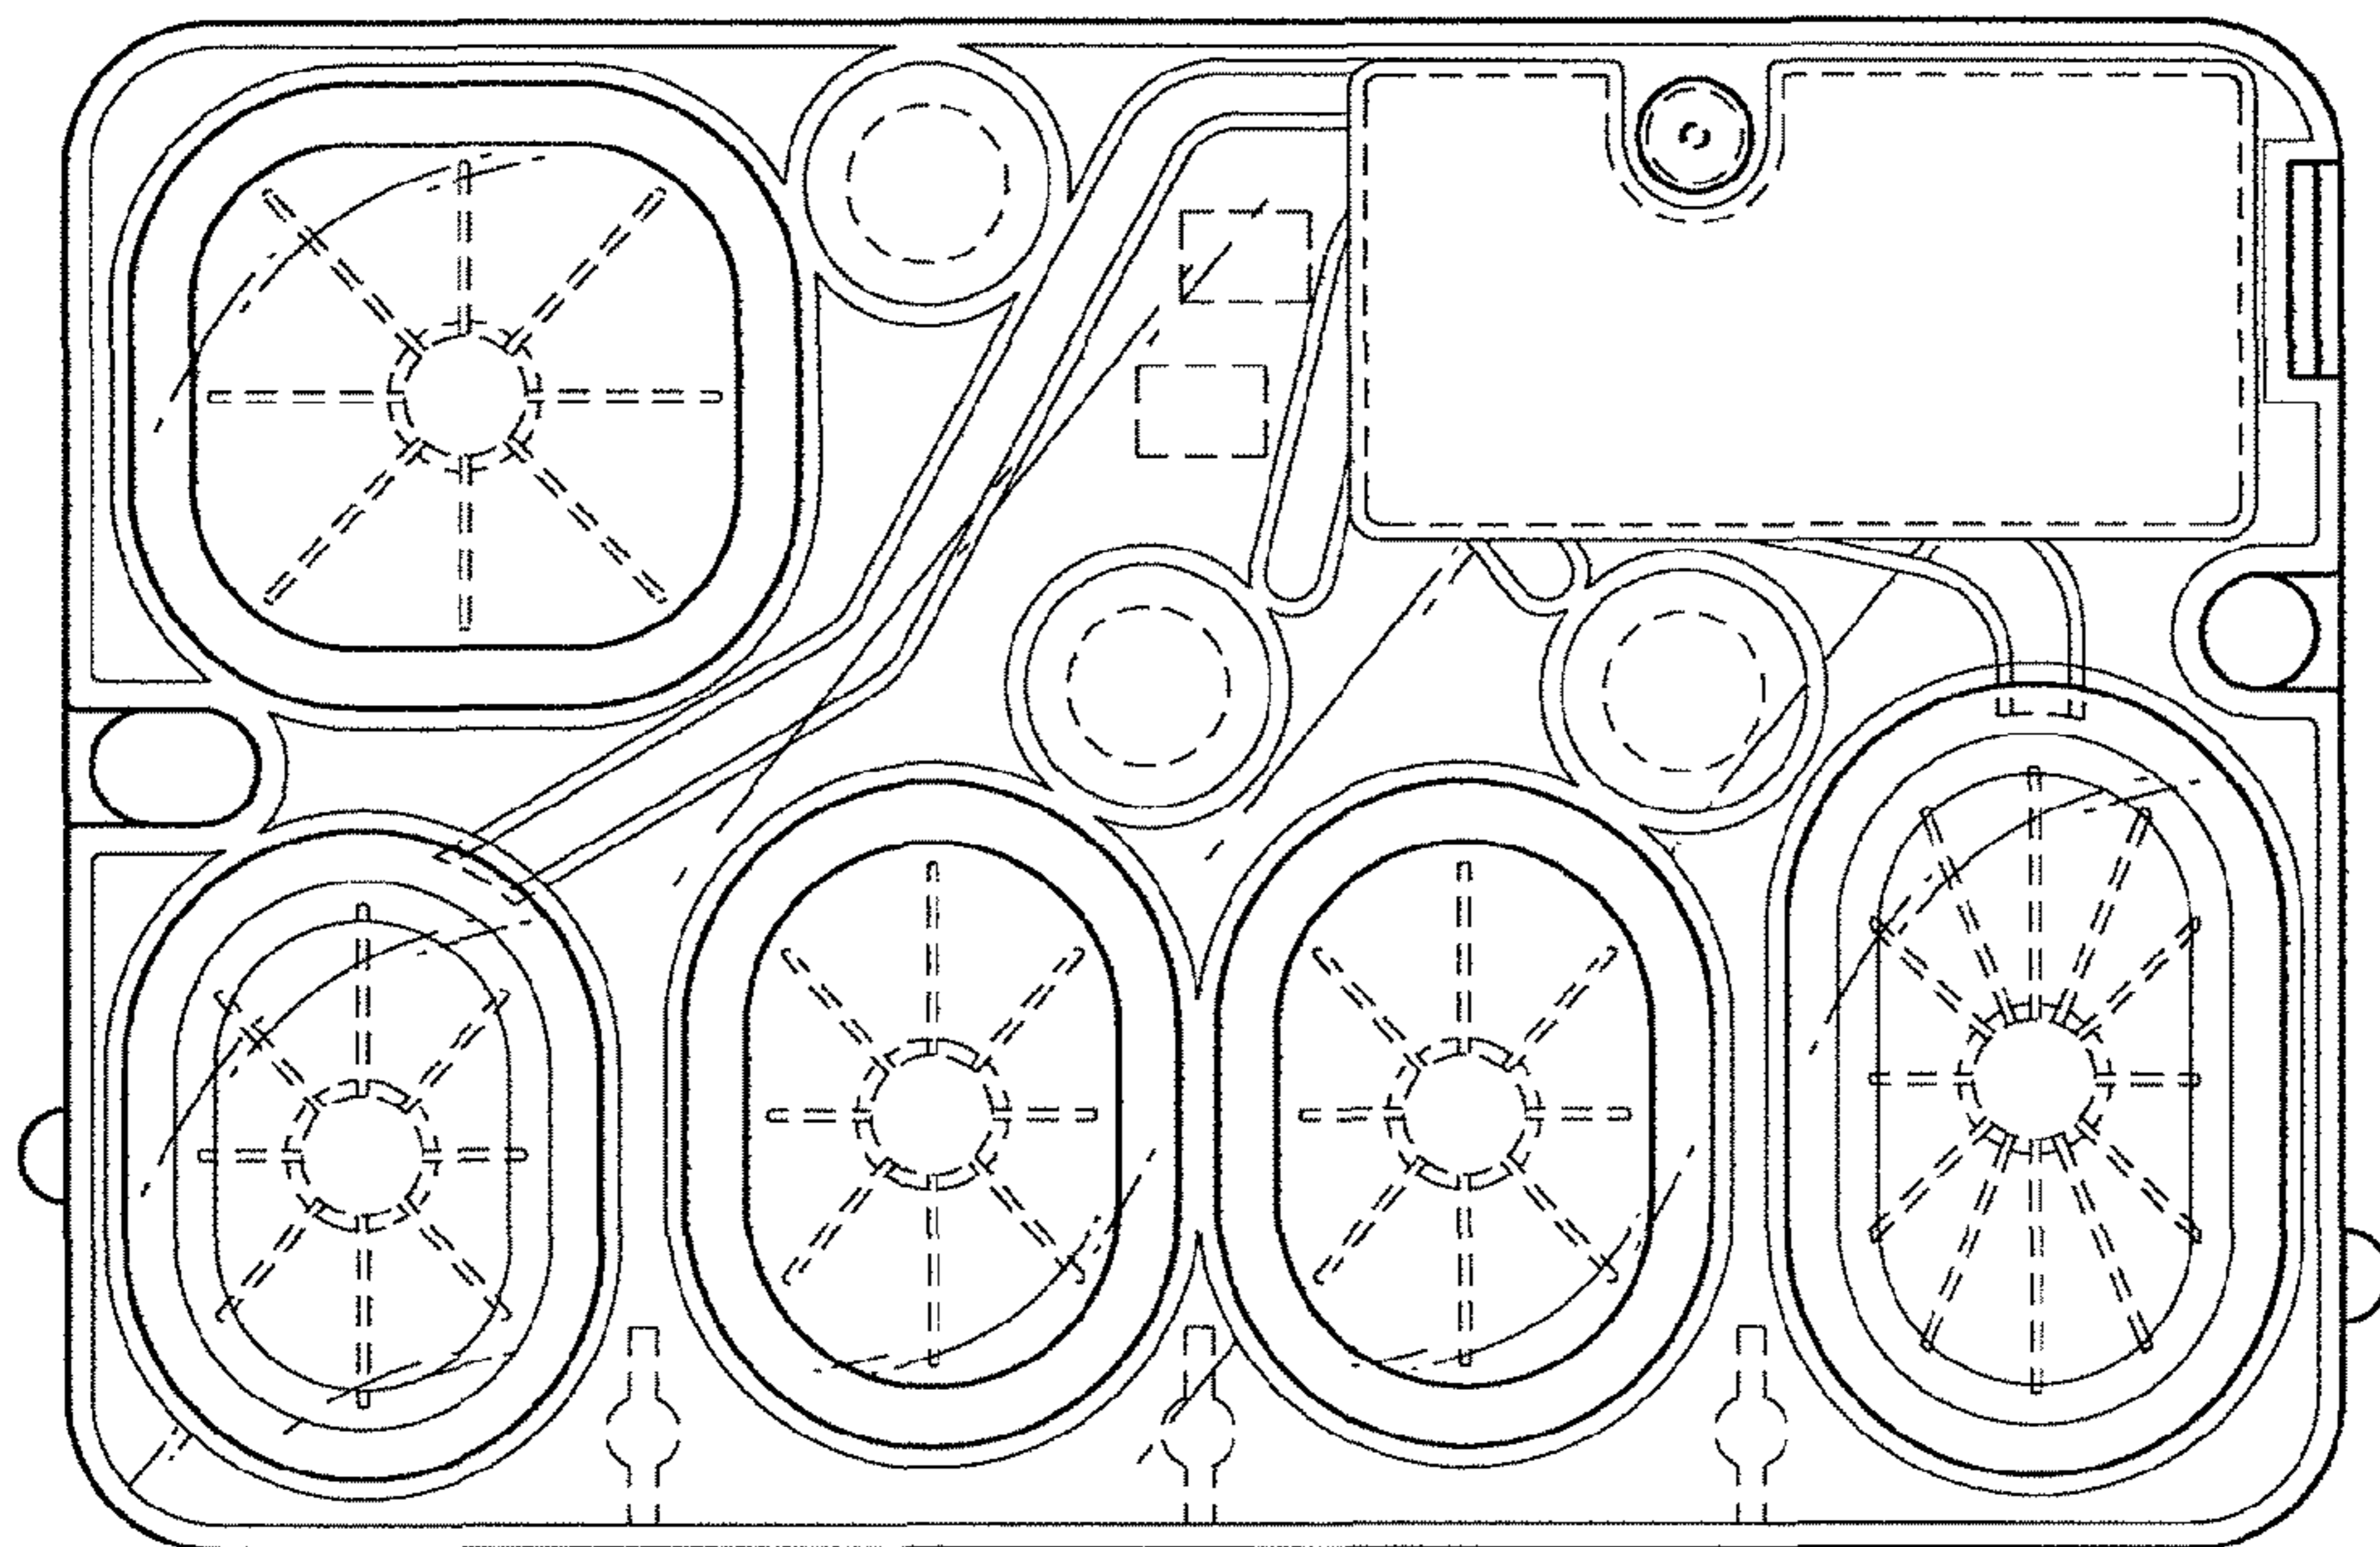


FIG. 2

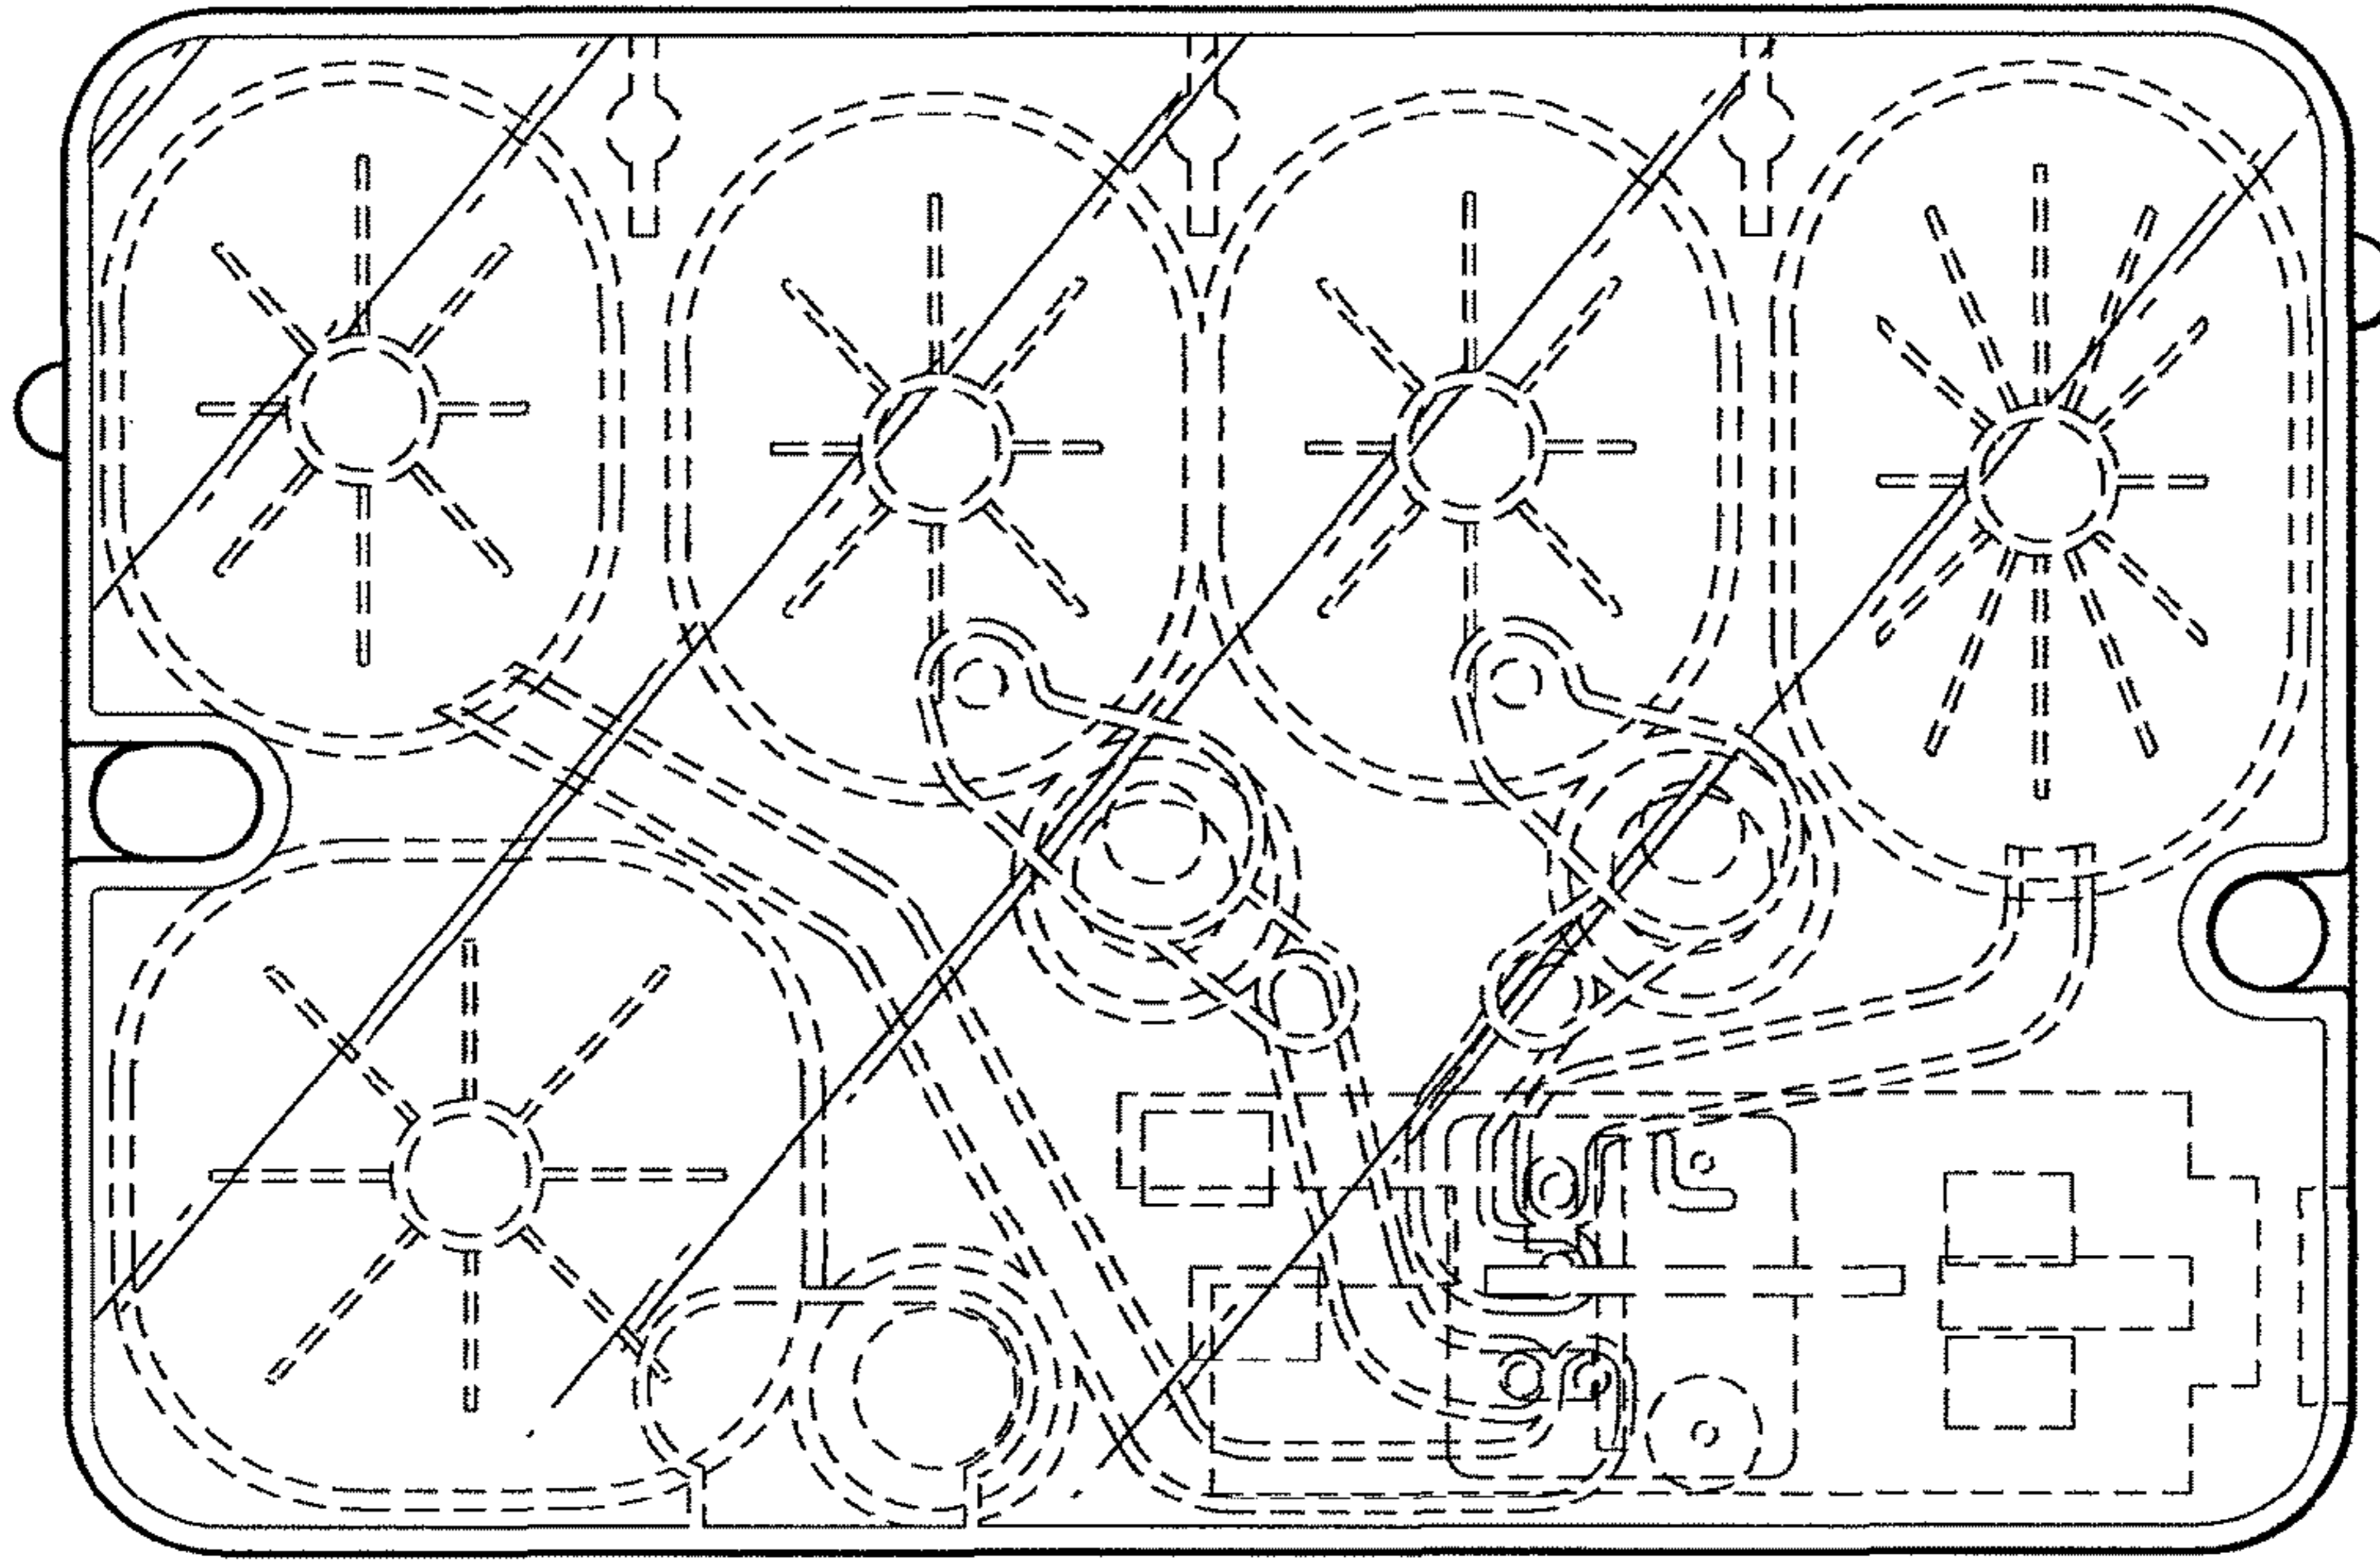


FIG. 3

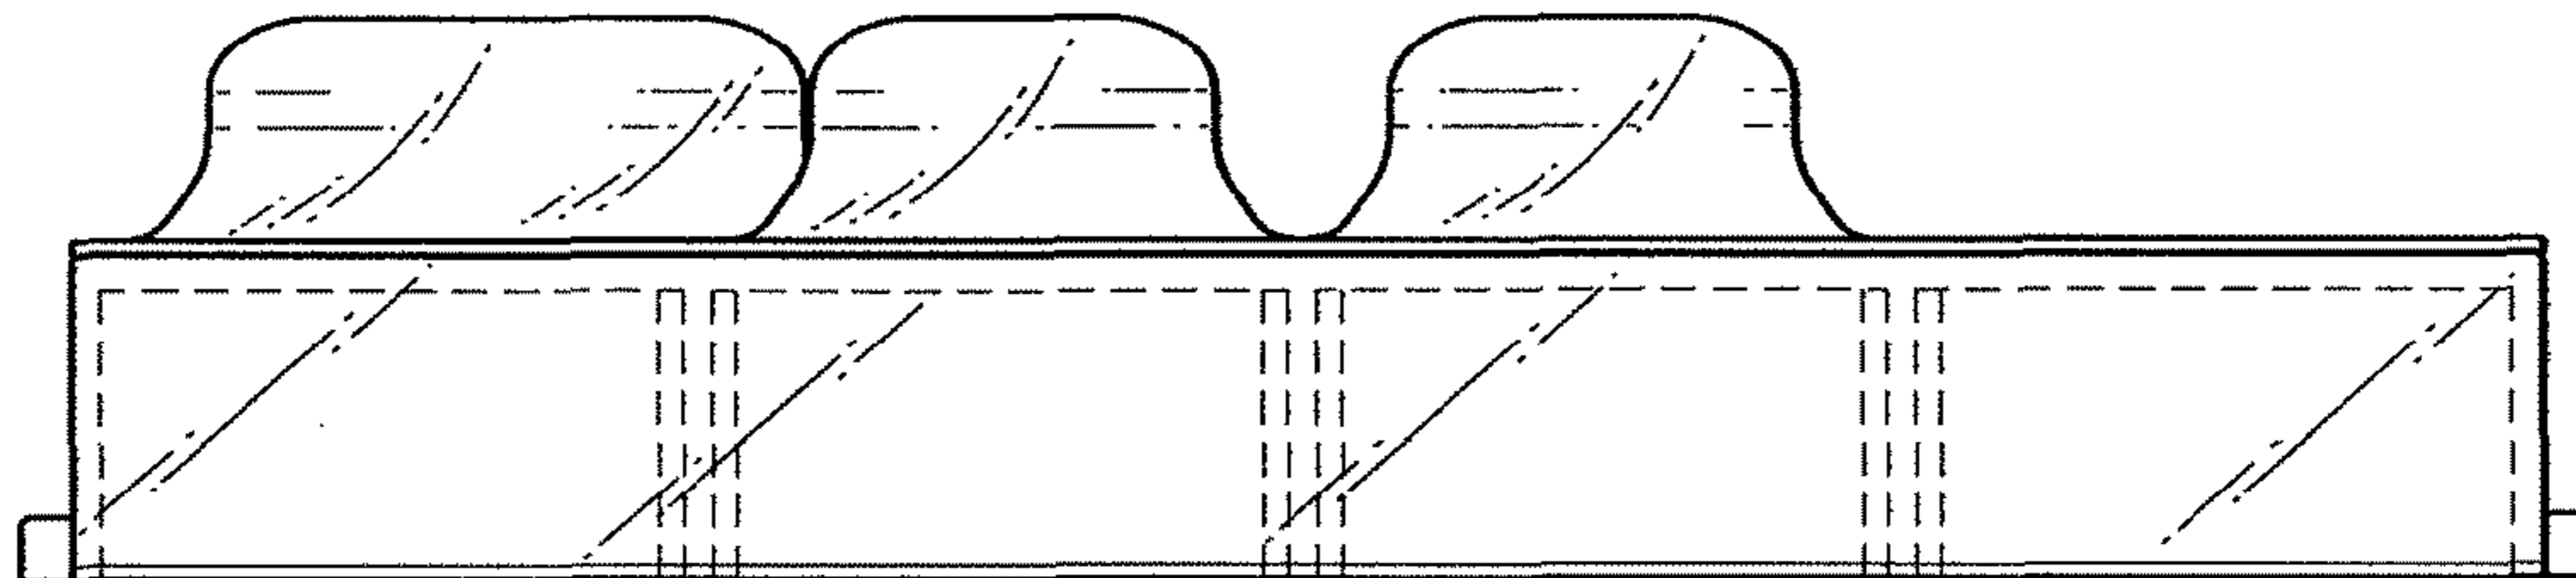


FIG. 4

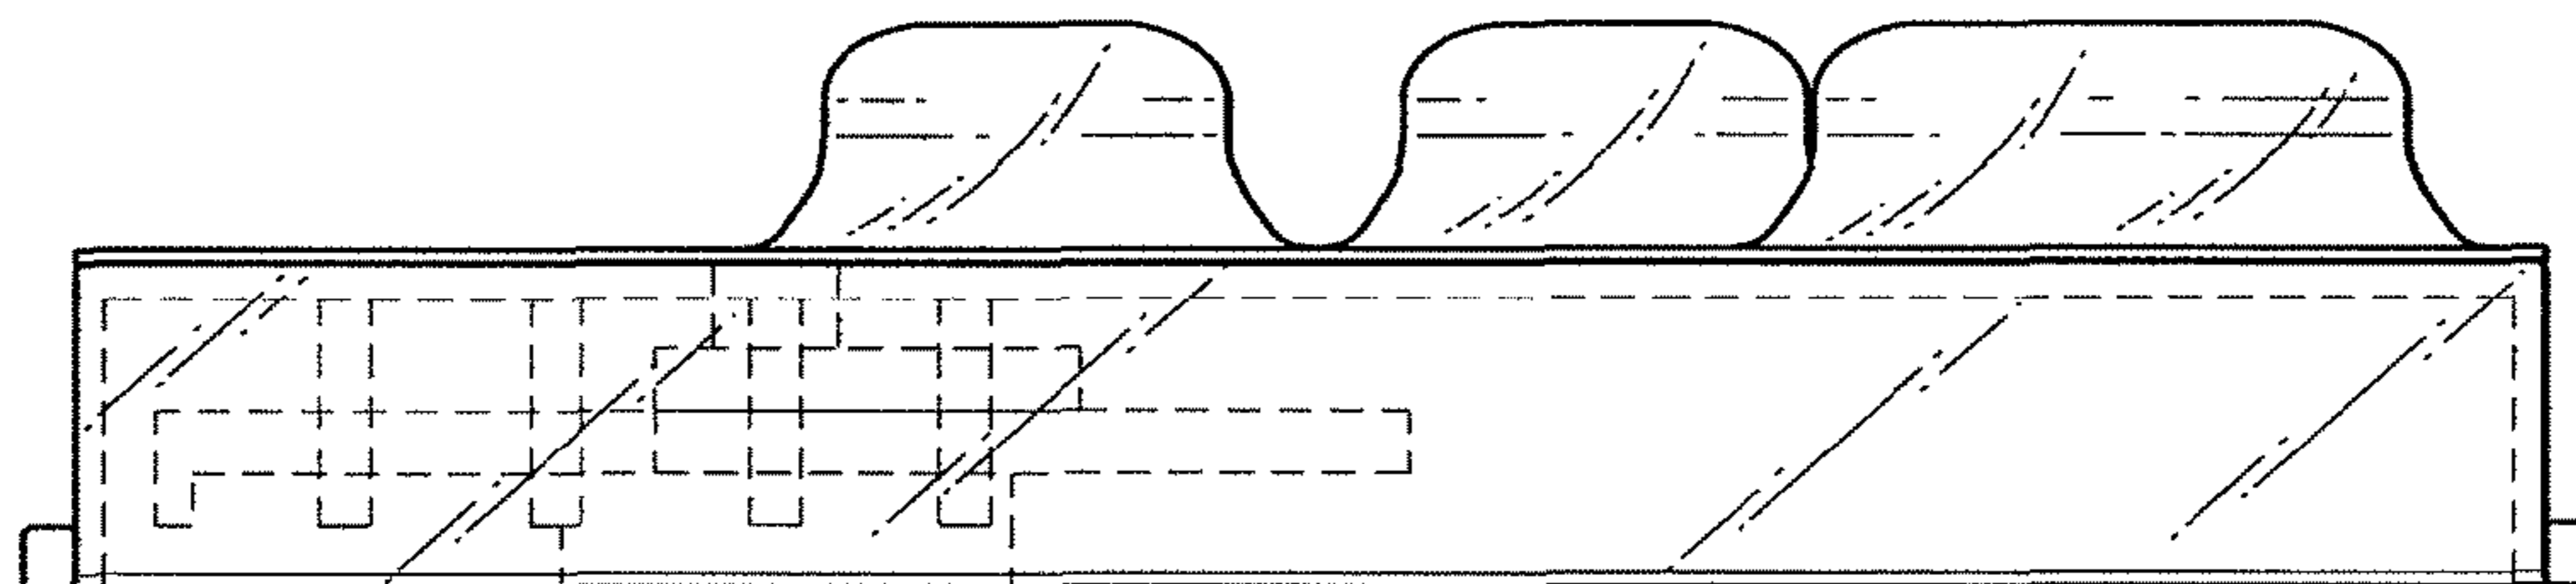


FIG. 5

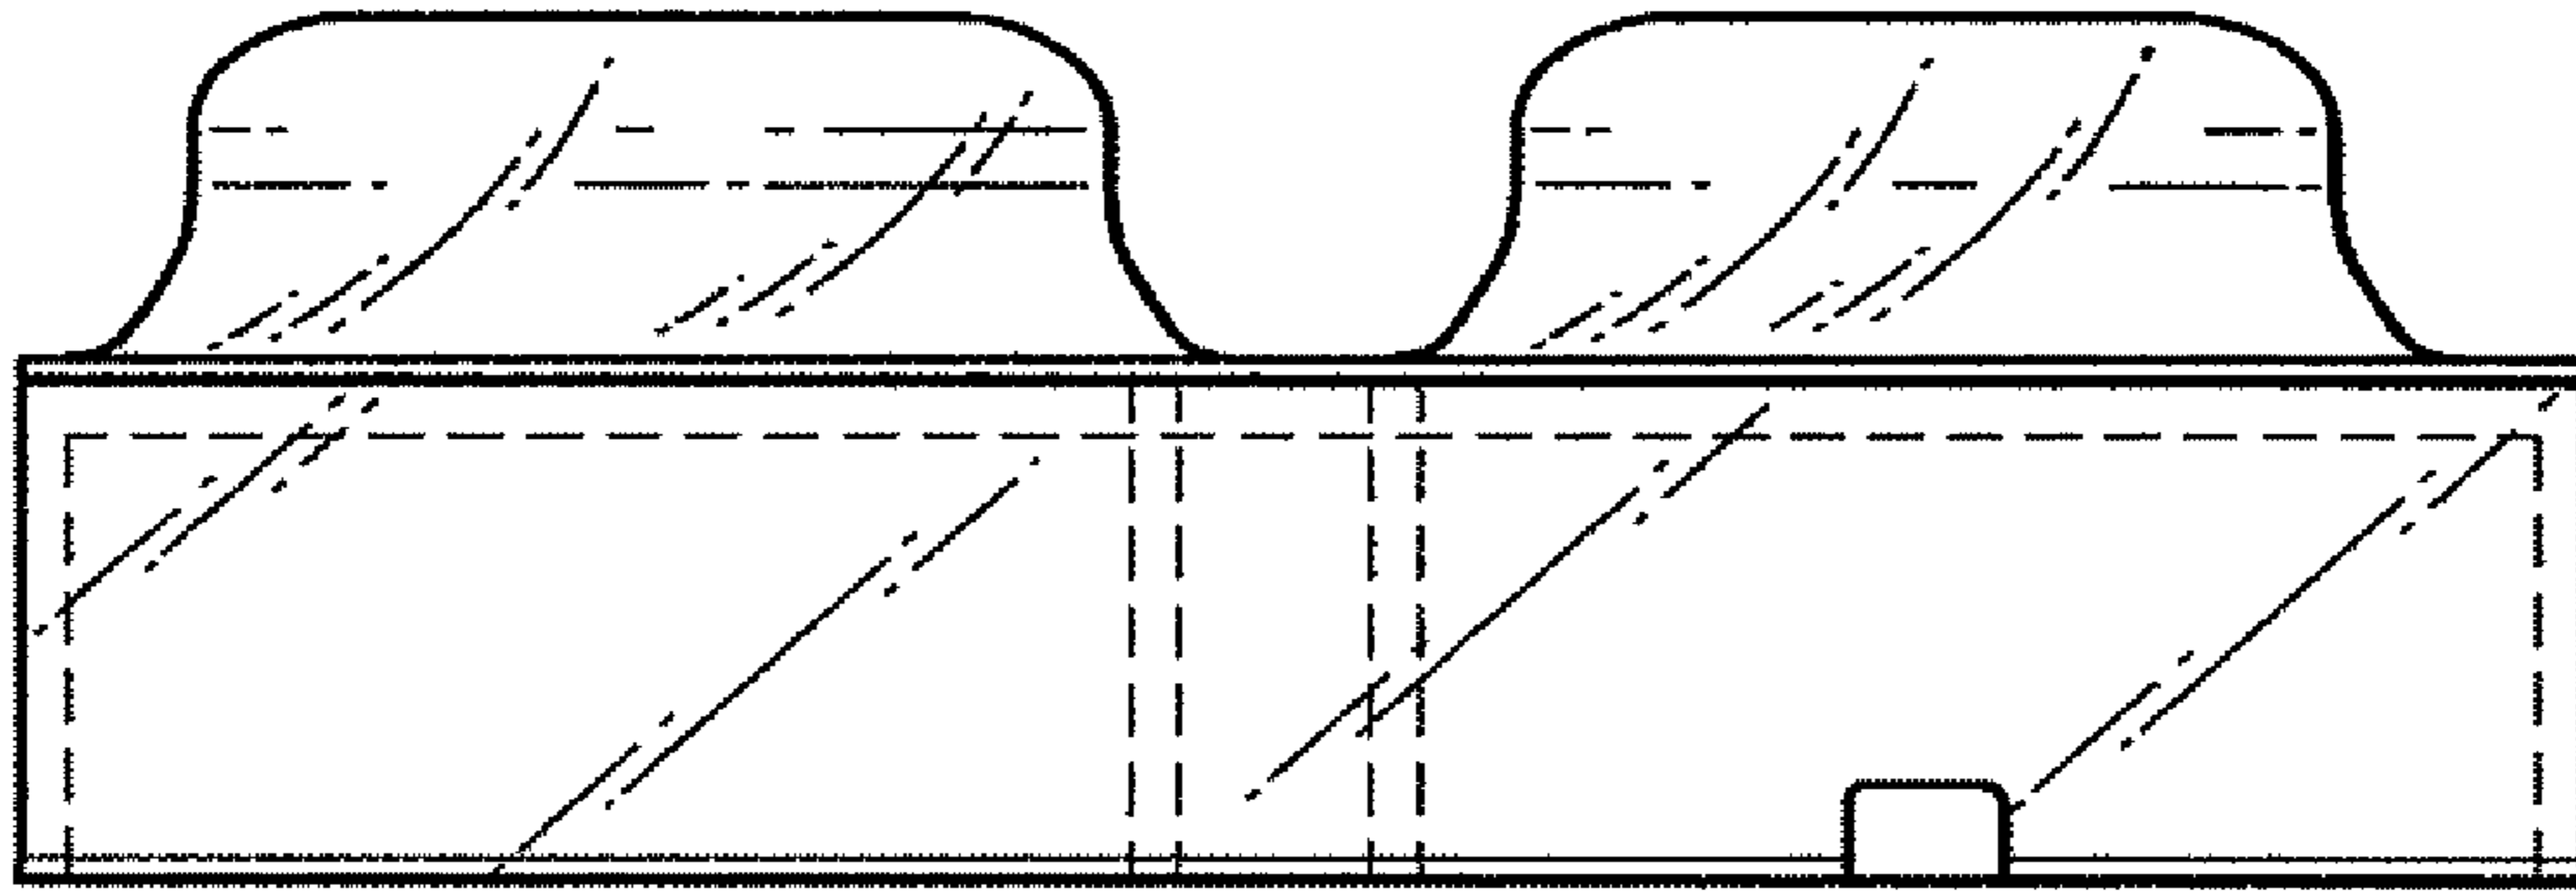


FIG. 6

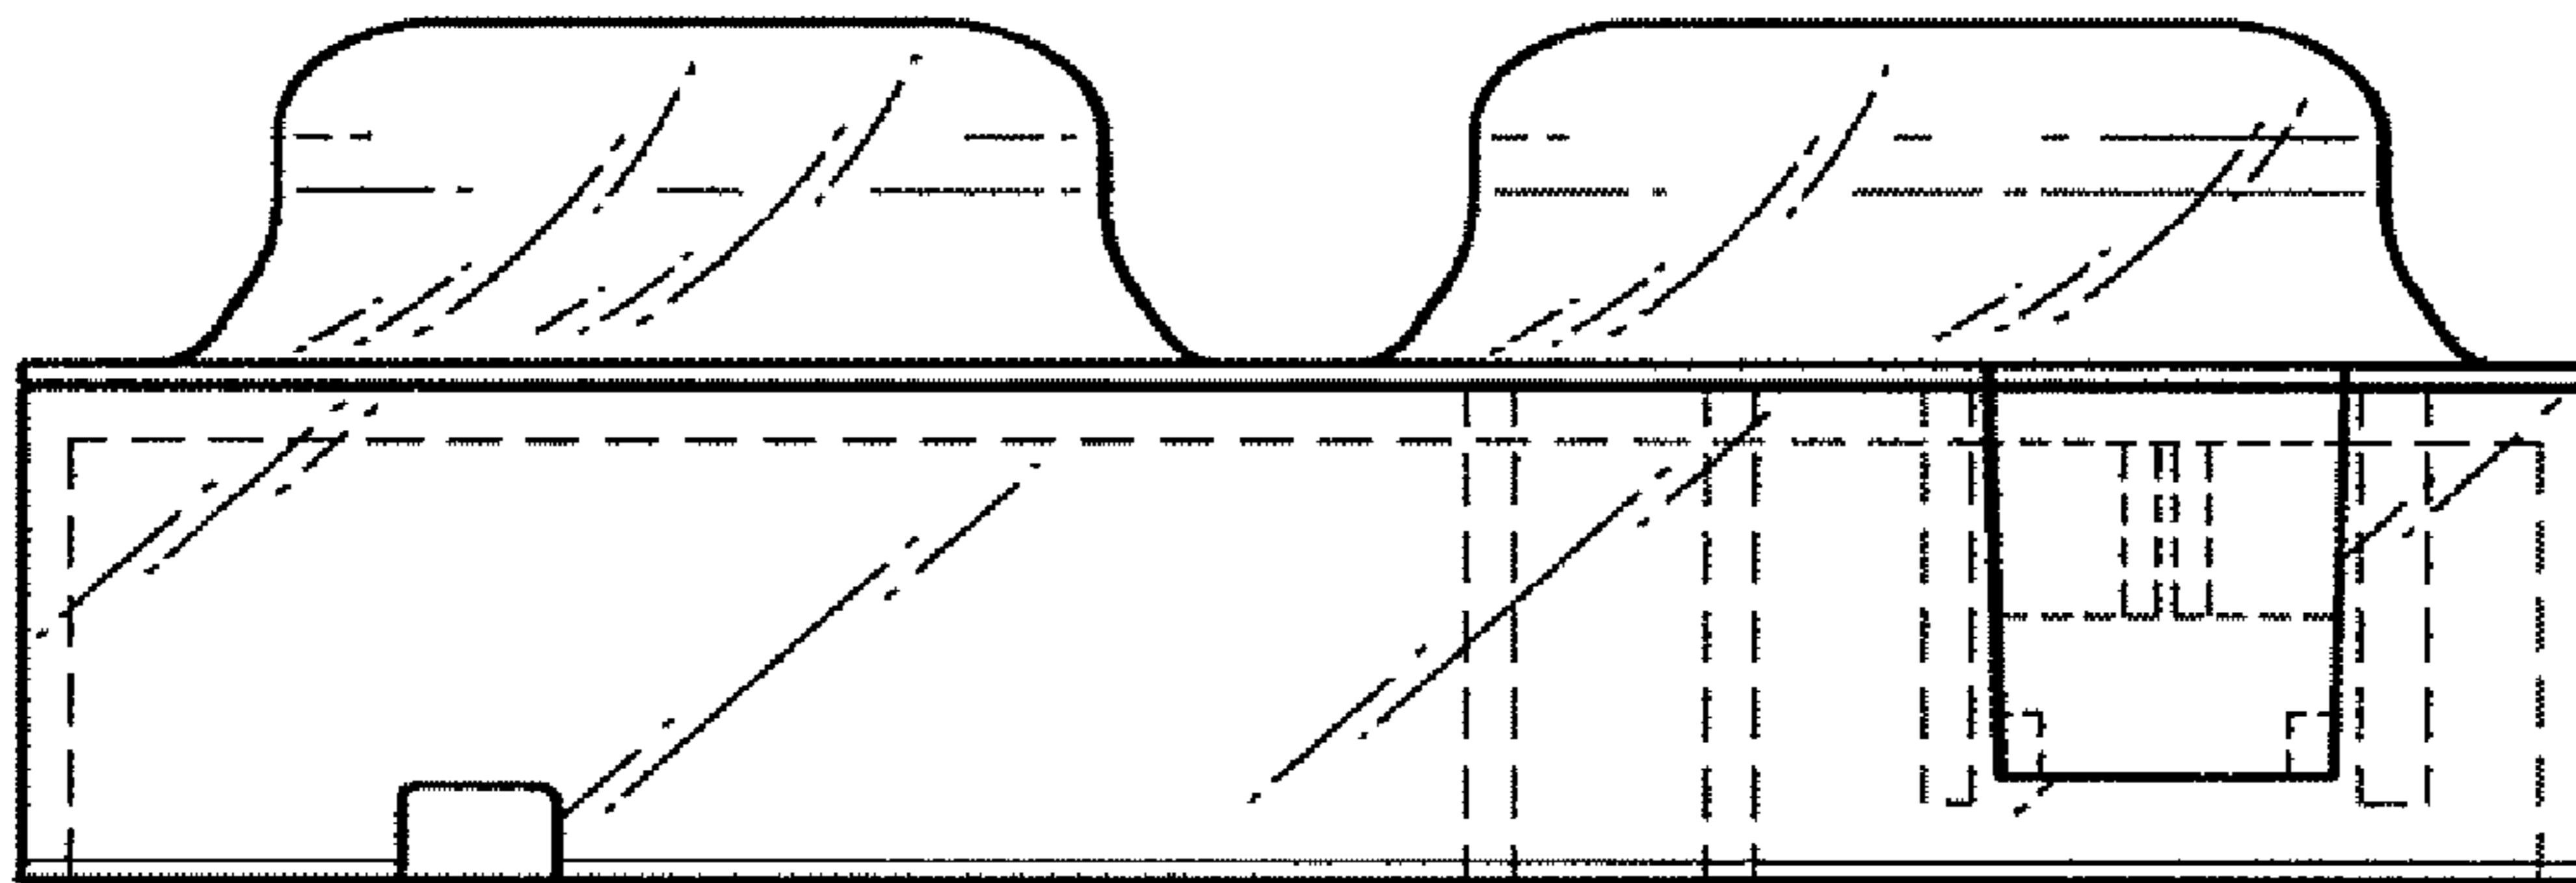


FIG. 7

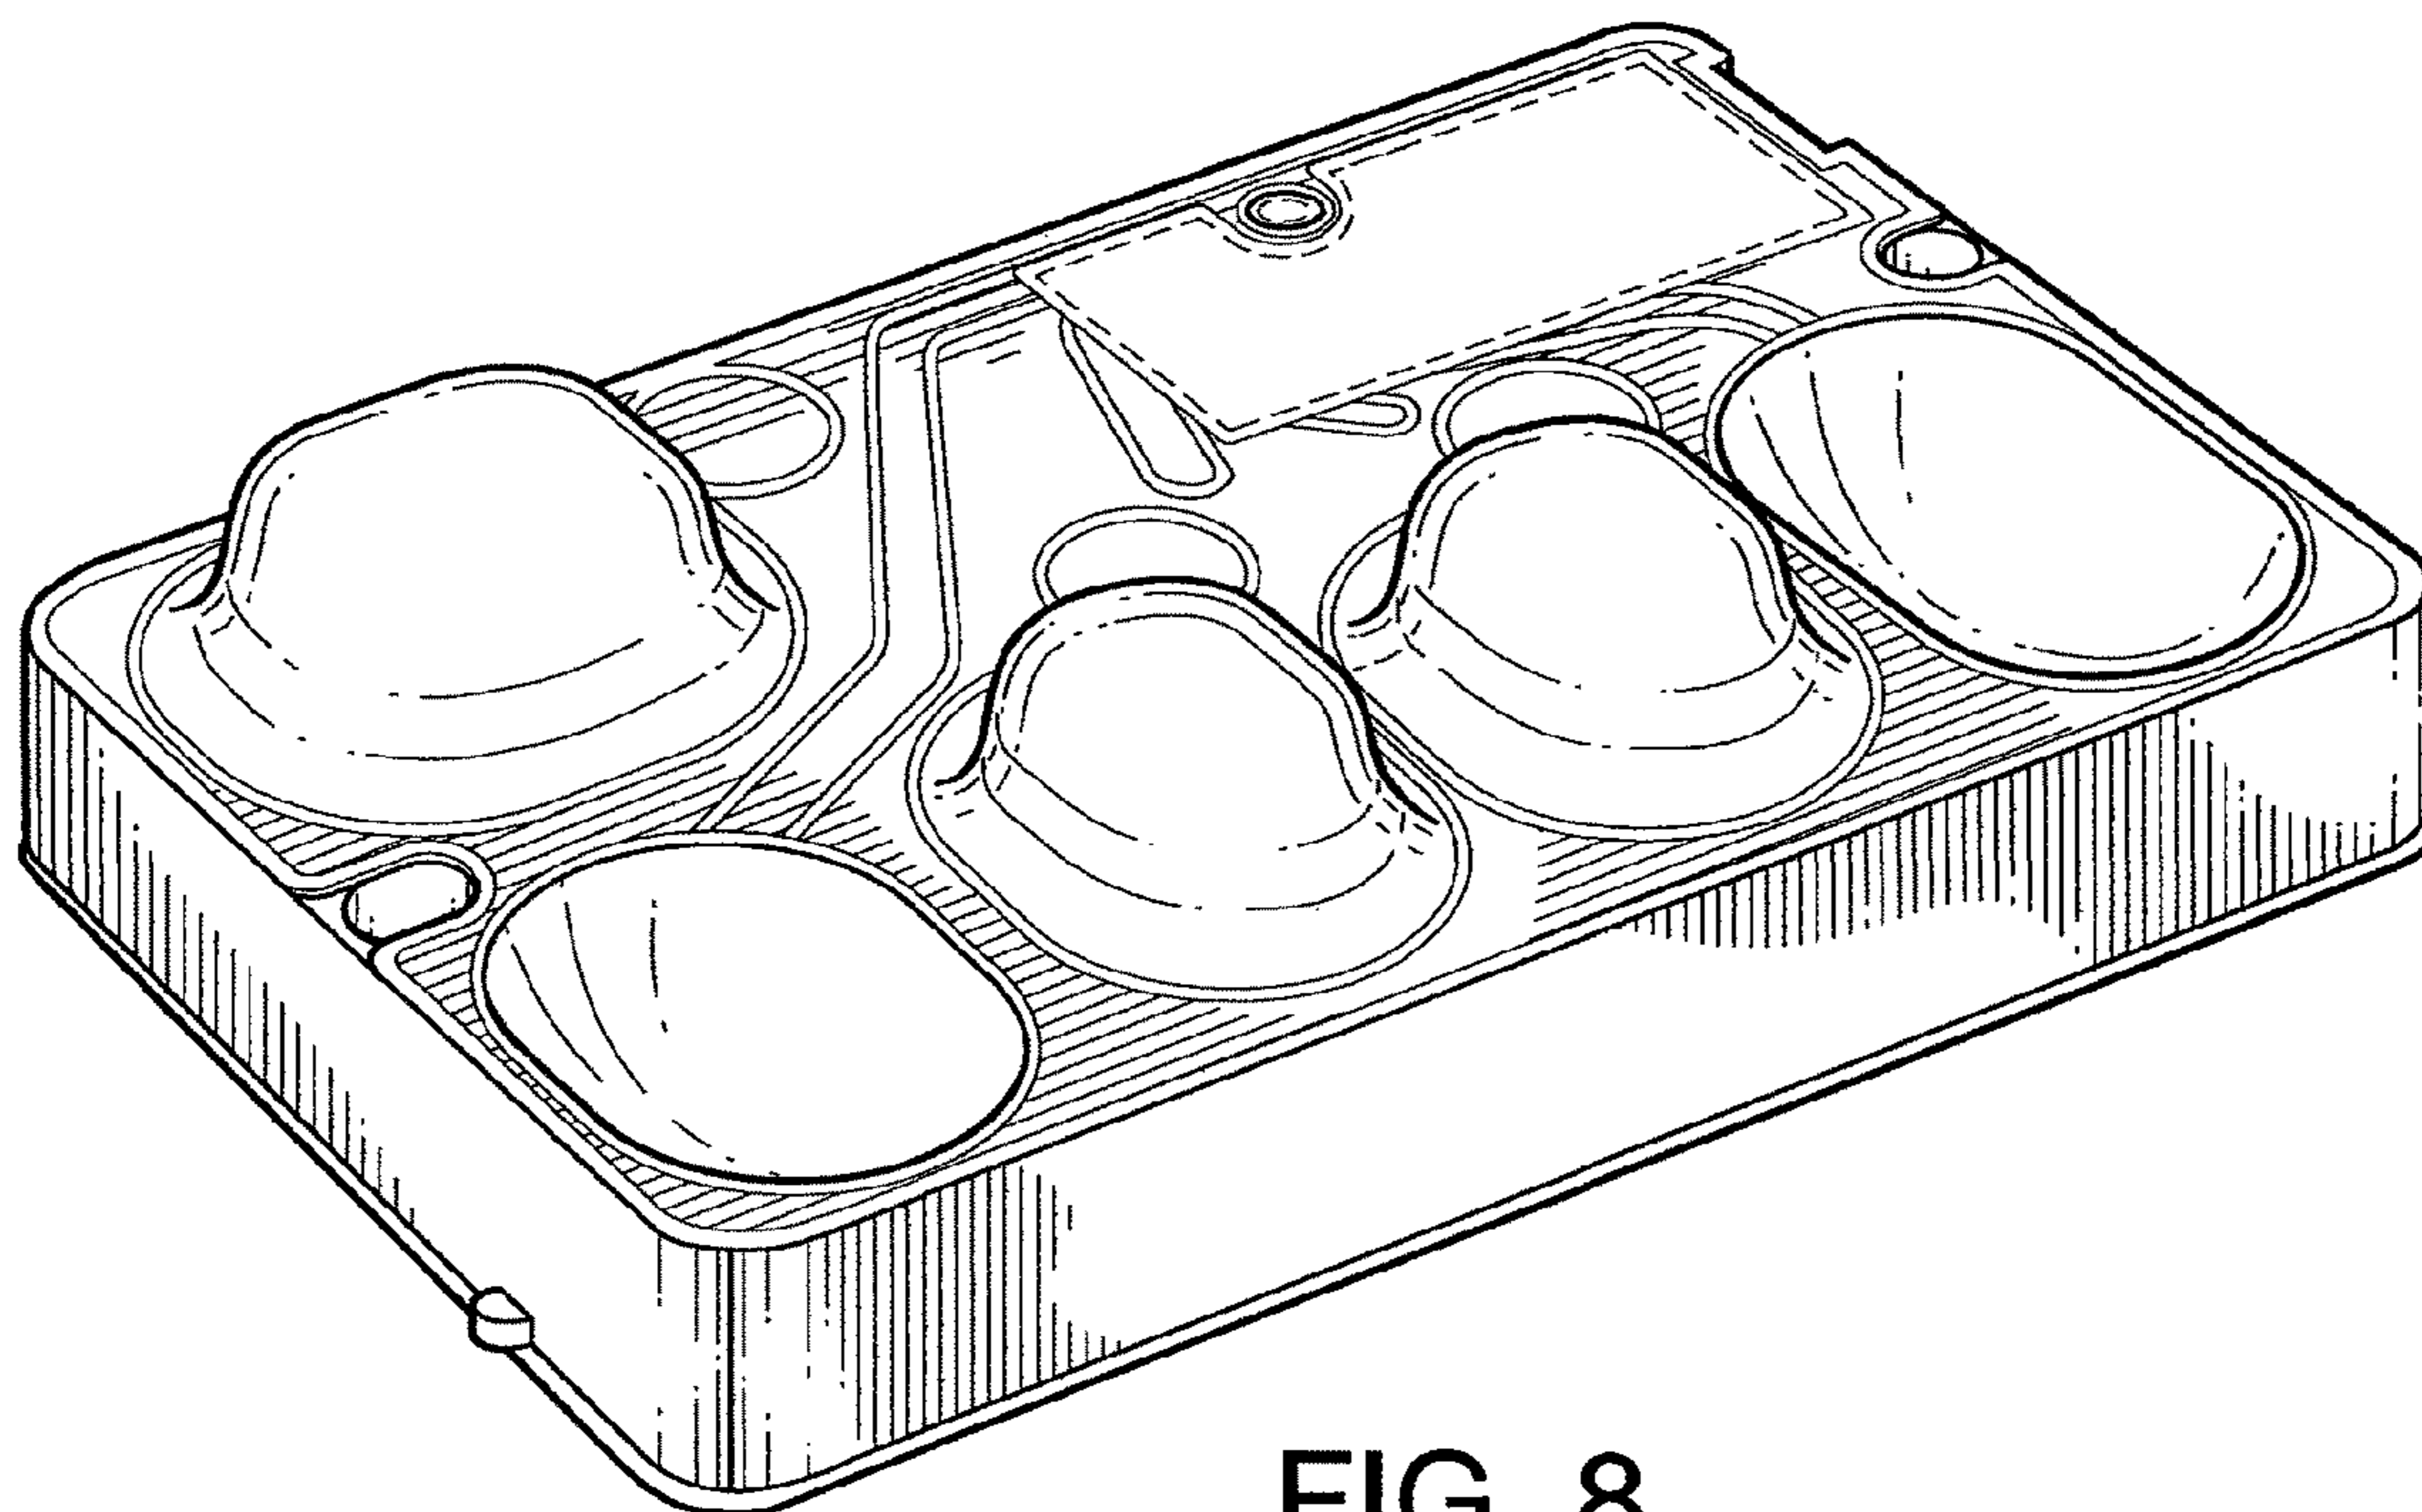


FIG. 8

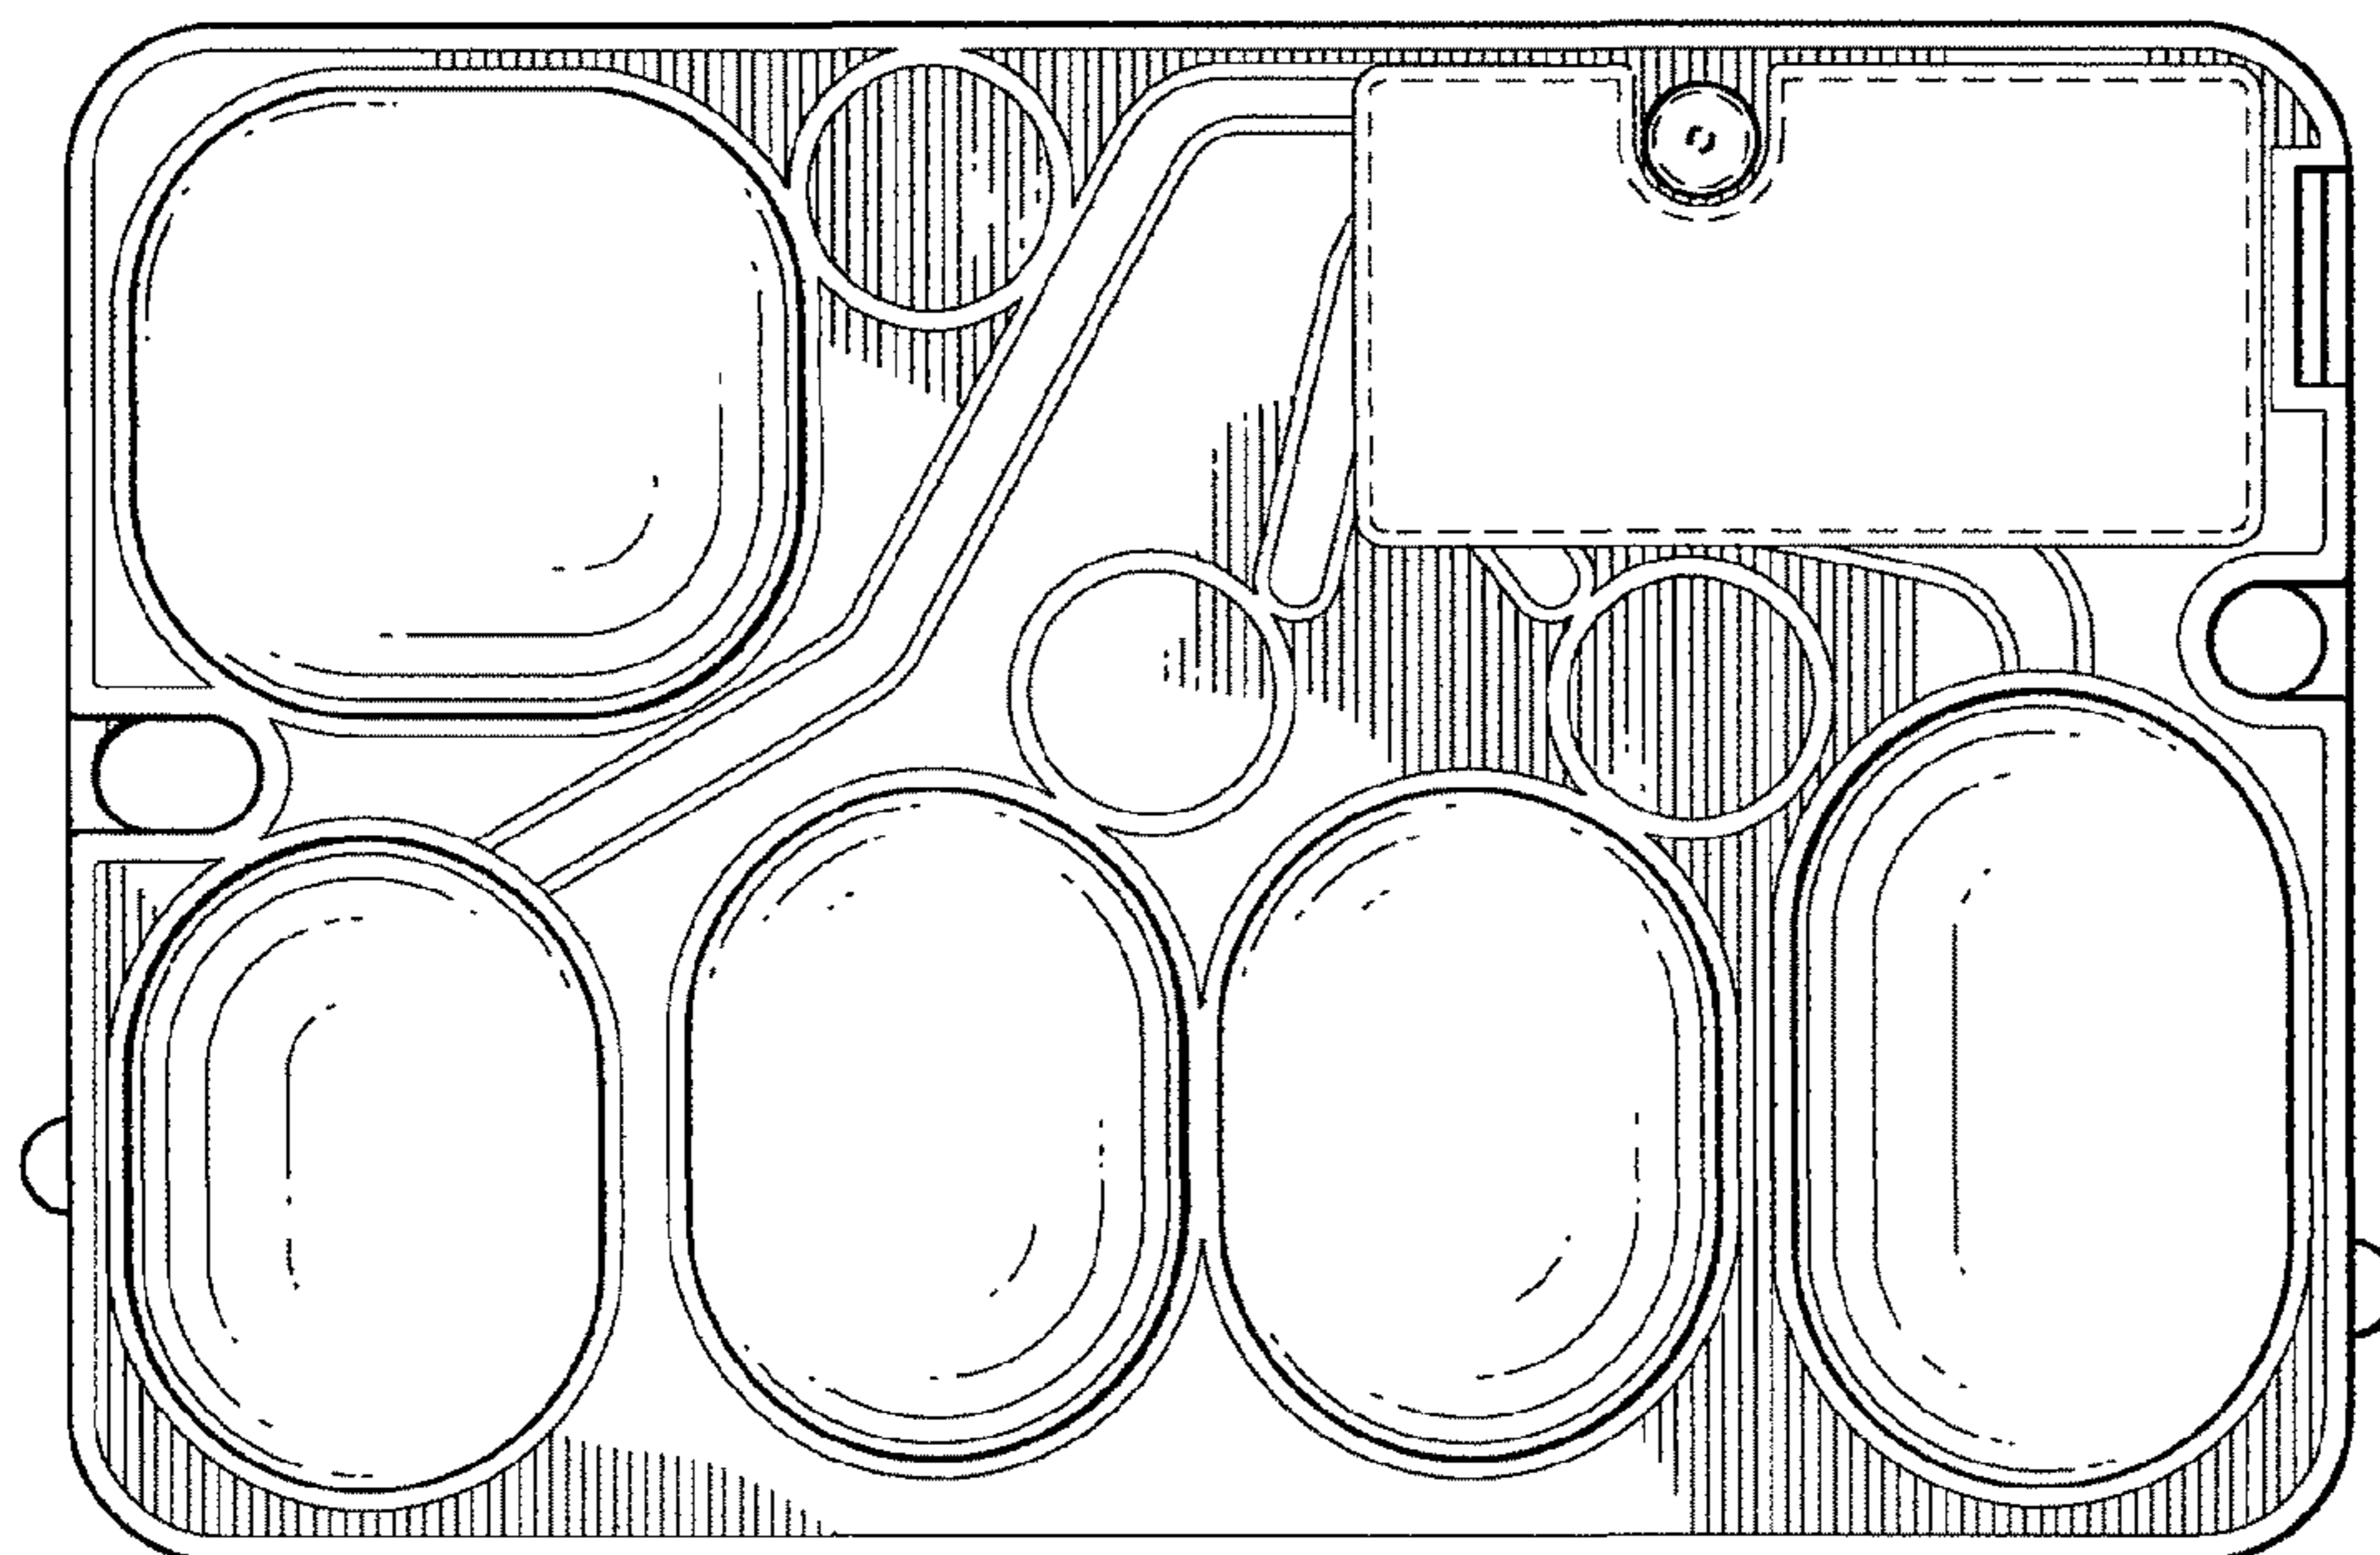


FIG. 9

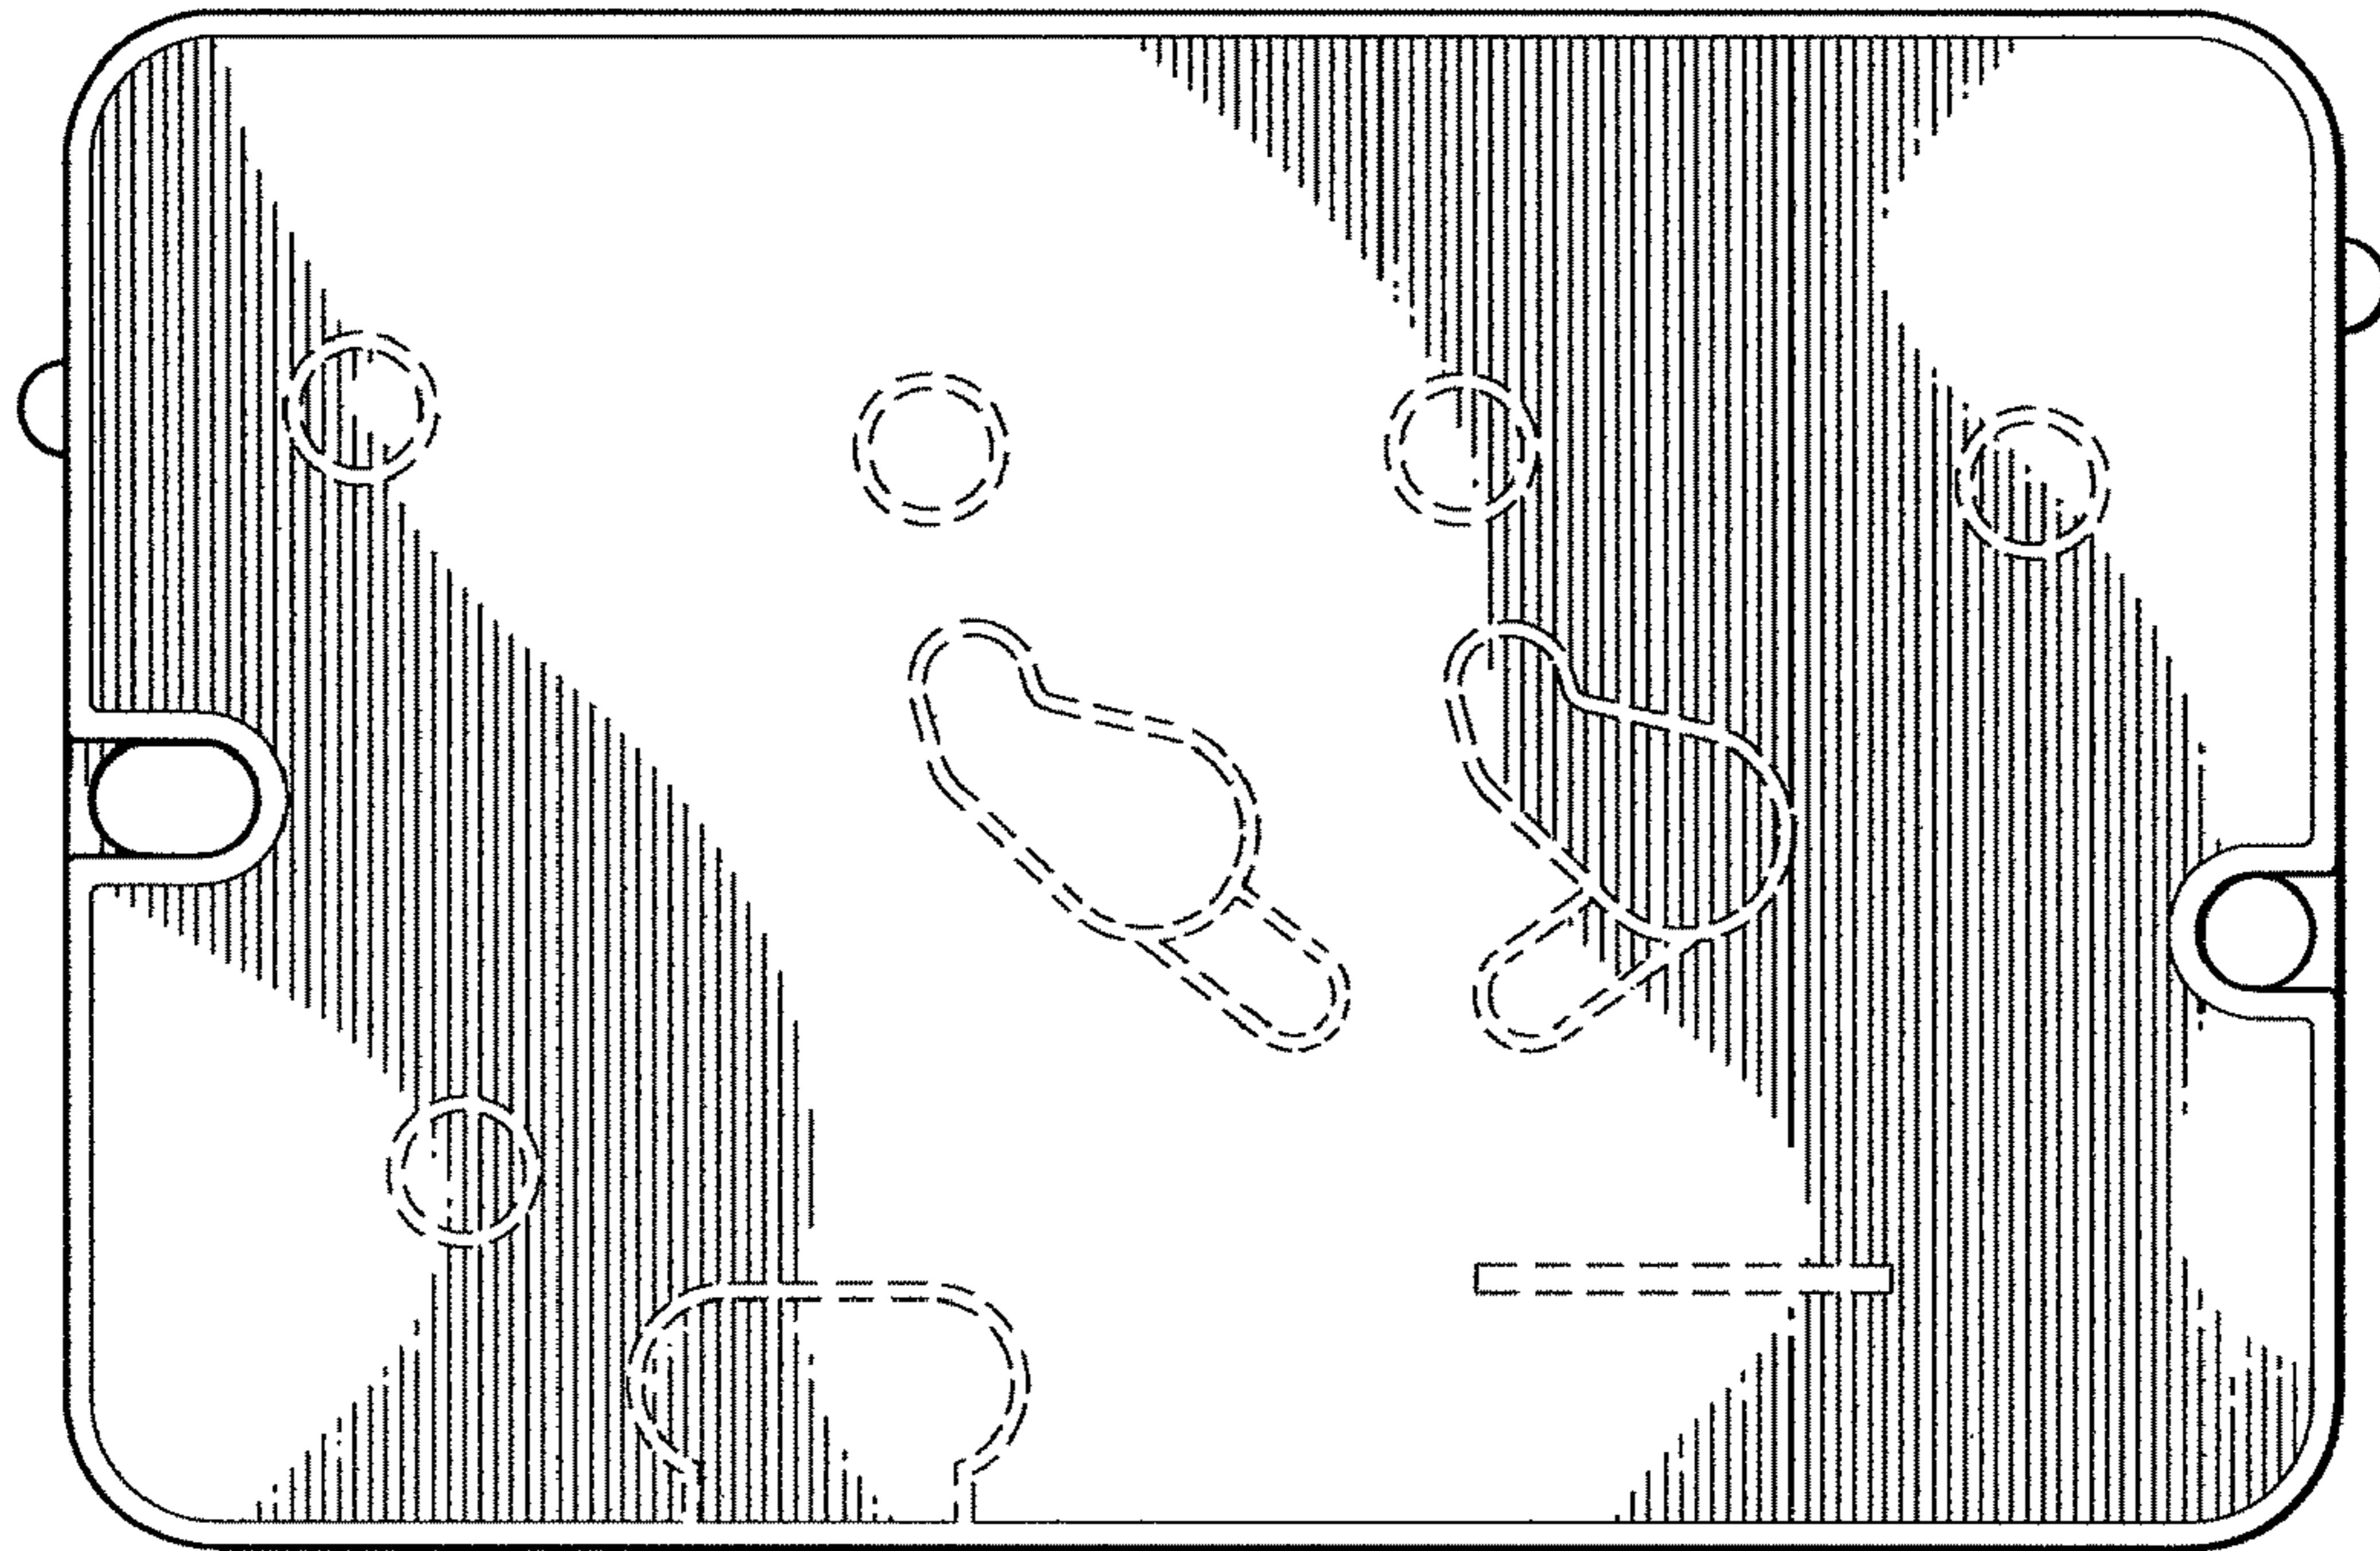


FIG. 10

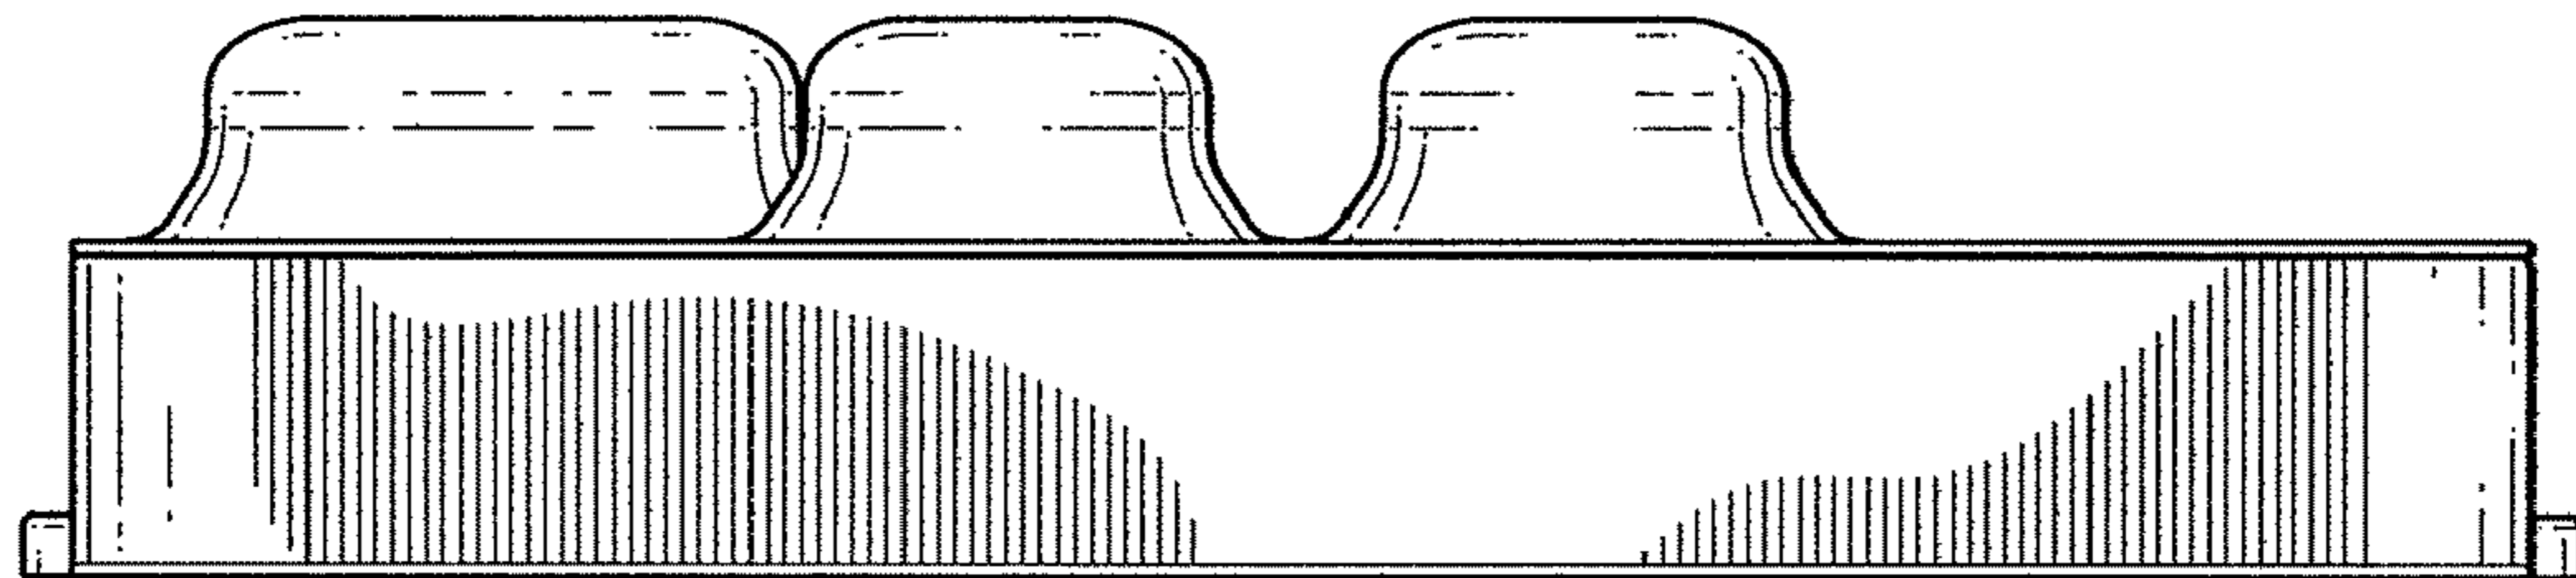


FIG. 11

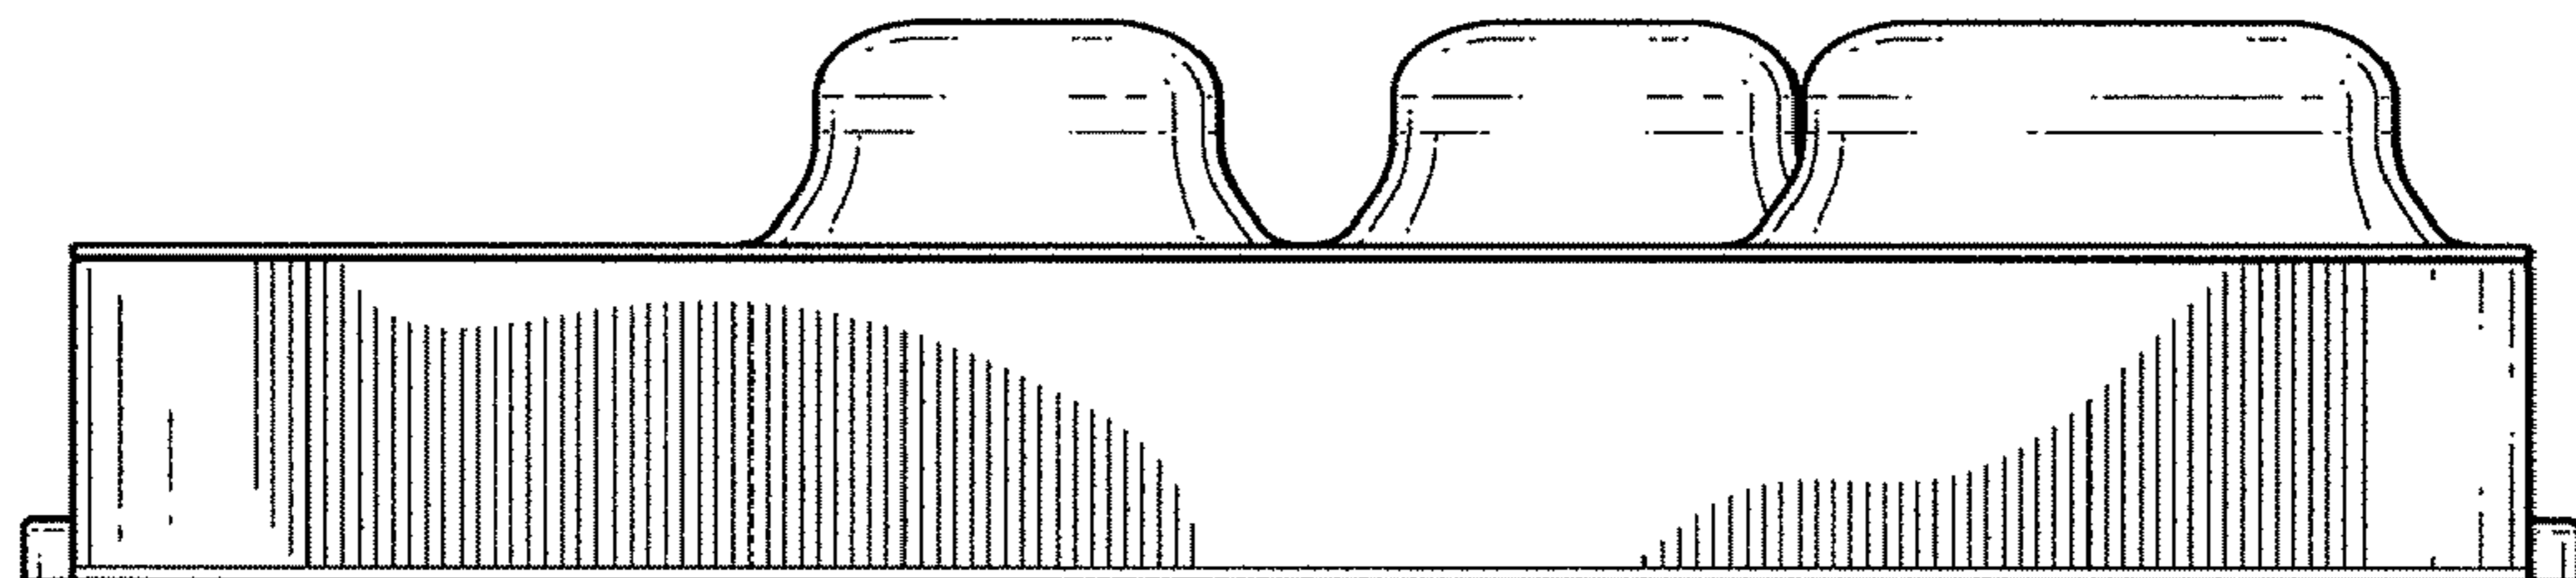


FIG. 12

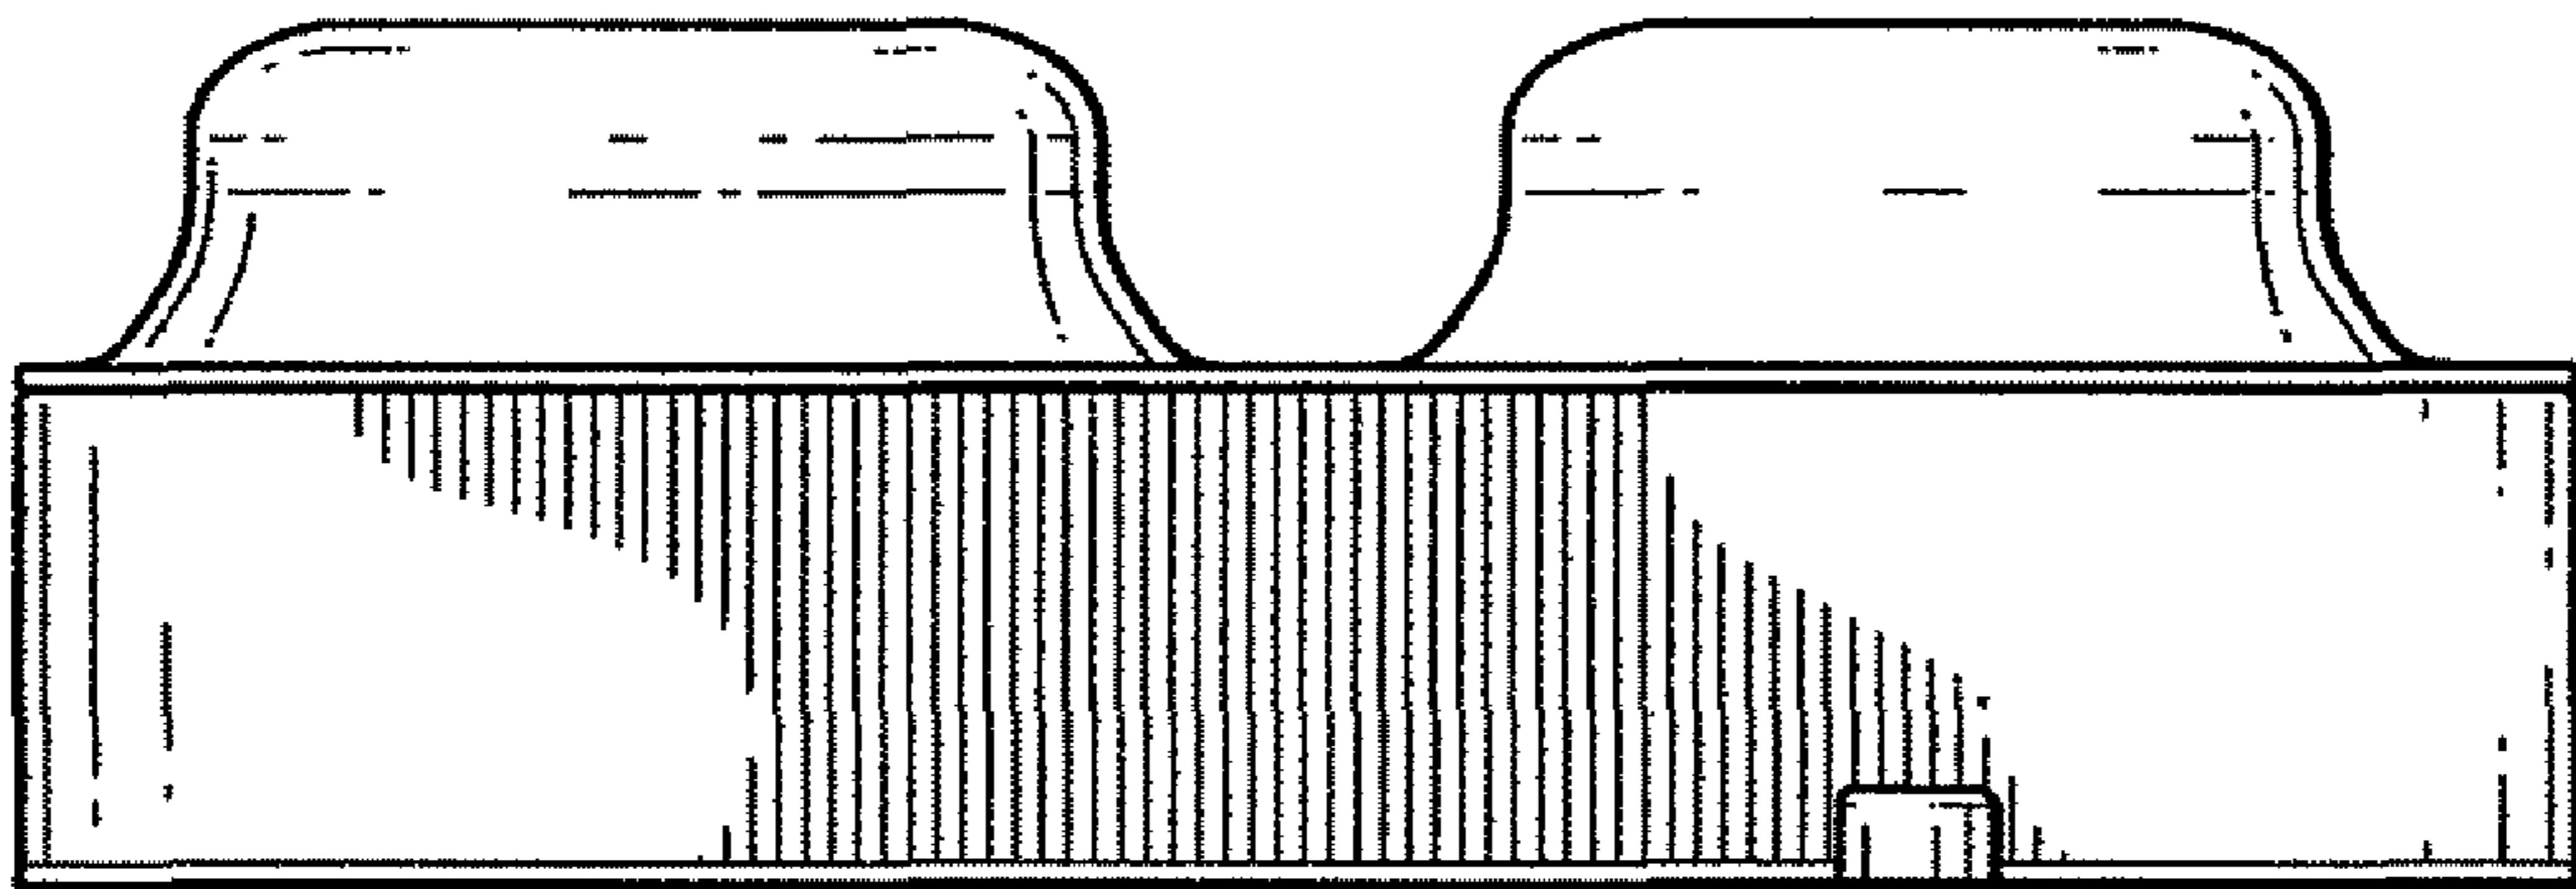


FIG. 13

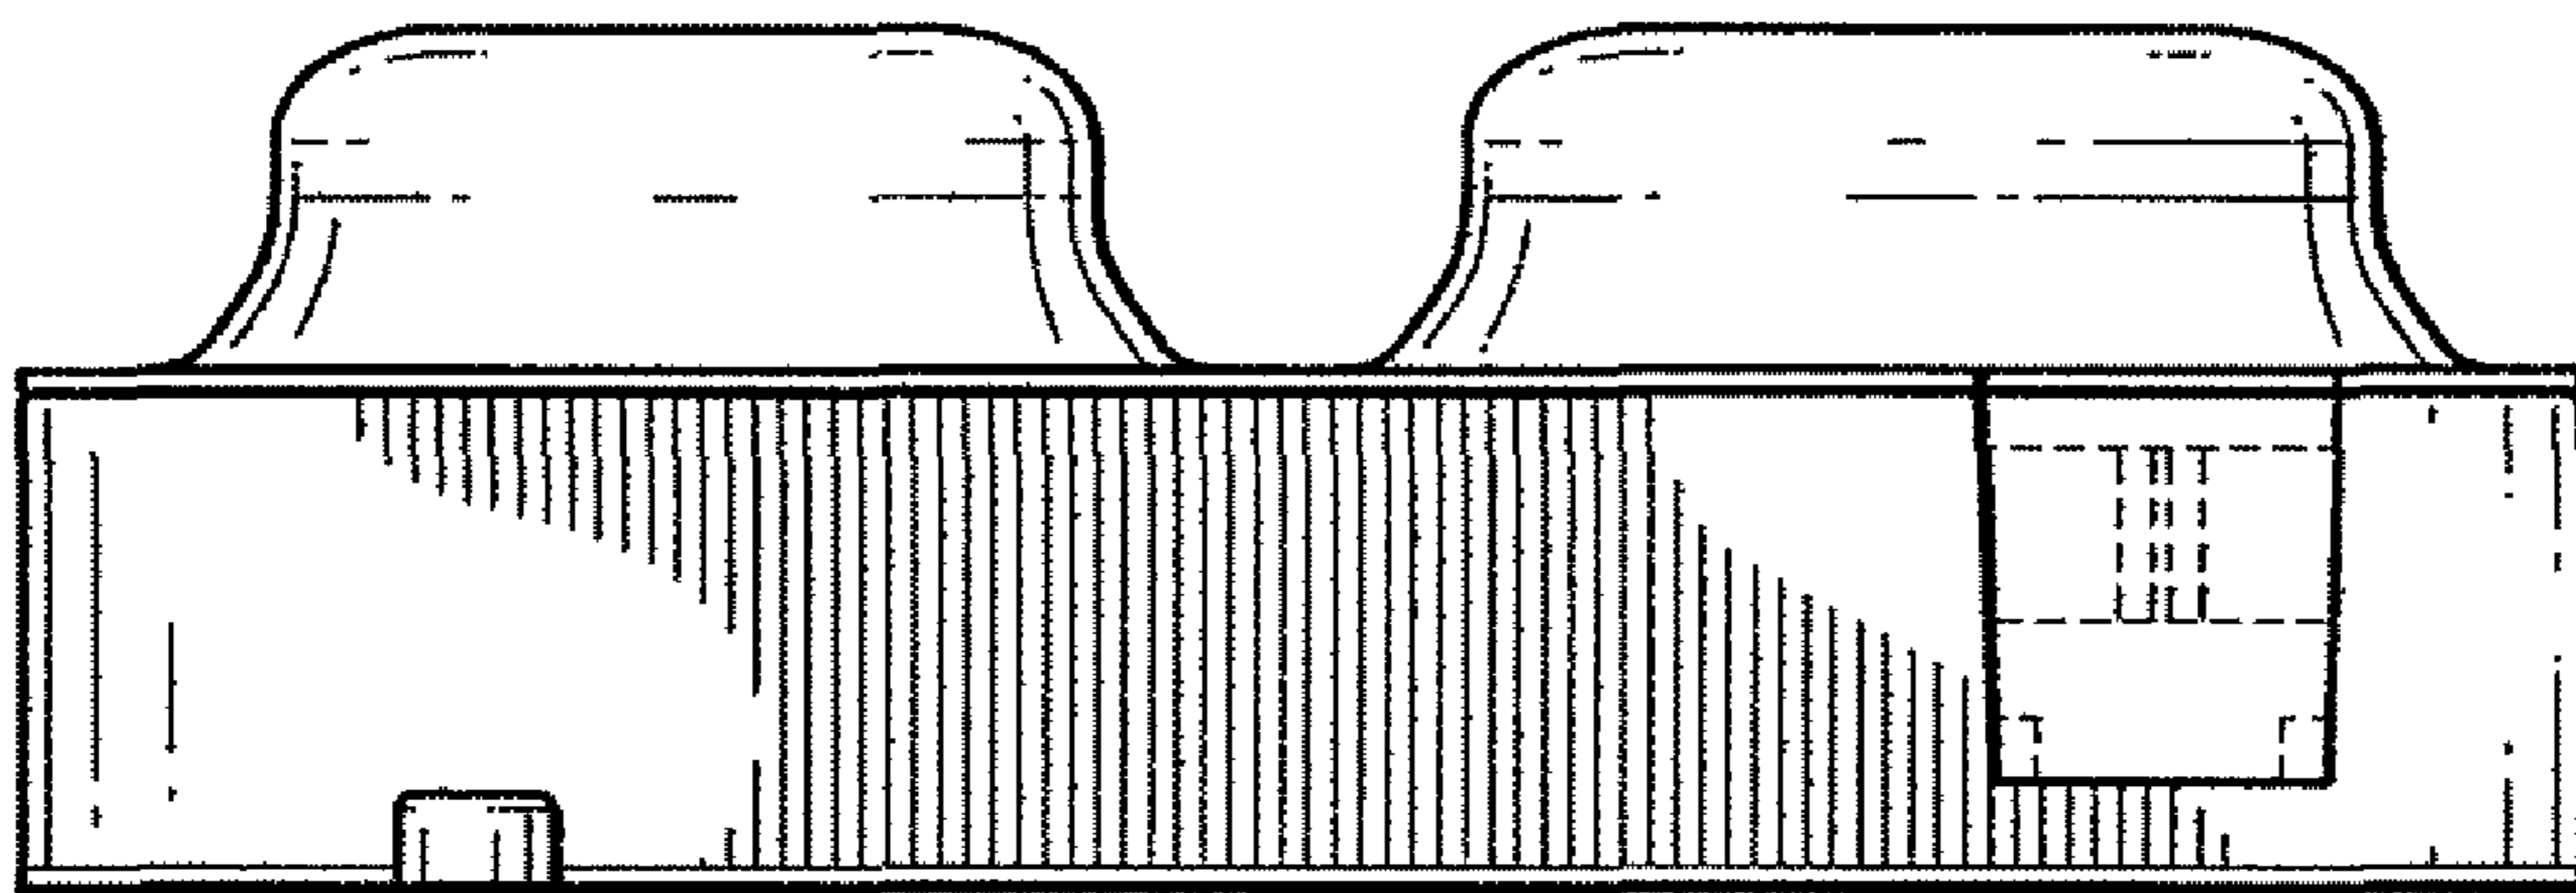


FIG. 14