



US00D647102S

(12) **United States Design Patent**
Tokunaga et al.

(10) **Patent No.:** **US D647,102 S**
(45) **Date of Patent:** **** Oct. 18, 2011**

(54) **GRAPHICAL USER INTERFACE FOR A
COMPUTER MONITOR OF AN X-RAY
TOMOGRAPHY SCANNER**

(75) Inventors: **Tatsuya Tokunaga**, Tokyo (JP); **Masaki
Takano**, Tokyo (JP); **Maiko Kawase**,
Tokyo (JP); **Mitsuaki Ogata**, Tokyo
(JP); **Keishi Okamoto**, Tokyo (JP);
Yuko Aoki, Tokyo (JP); **Takashi
Murase**, Tokyo (JP)

(73) Assignee: **Hitachi Medical Corporation**, Tokyo
(JP)

(**) Term: **14 Years**

(21) Appl. No.: **29/344,503**

(22) Filed: **Sep. 30, 2009**

(30) **Foreign Application Priority Data**

Mar. 31, 2009 (JP) 2009-7478

(51) **LOC (9) Cl.** **14-04**

(52) **U.S. Cl.** **D14/485**

(58) **Field of Classification Search** D14/485-95;
D18/24-33; D19/6, 52; D20/11; D21/324-33;
715/700-867, 973-77; D24/158-161; 250/363.01
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D483,381 S * 12/2003 Platz D14/495
D527,105 S * 8/2006 Kitayama et al. D24/158

D529,488 S * 10/2006 Uchida D14/248
D544,876 S * 6/2007 Yamazaki et al. D14/486
D547,770 S * 7/2007 Griffith D14/492
D551,672 S * 9/2007 Wirz D14/485
D553,143 S * 10/2007 Blencowe D14/486
7,378,660 B2 * 5/2008 Case et al. 250/363.01
D585,903 S * 2/2009 Yamaoka D14/485
D586,355 S * 2/2009 Mori et al. D14/486
D590,504 S * 4/2009 Ogiwara D24/158
D595,728 S * 7/2009 Scheibe et al. D14/486
D602,040 S * 10/2009 Matsuguma D14/489
D603,418 S * 11/2009 Magnani et al. D14/486
D614,635 S * 4/2010 Scalisi et al. D14/486
D625,322 S * 10/2010 Guntaur et al. D14/486
D625,416 S * 10/2010 Kasai et al. D24/158
D628,294 S * 11/2010 Baba D24/158

* cited by examiner

Primary Examiner — Melanie H Tung

(74) *Attorney, Agent, or Firm* — Antonelli, Terry, Stout &
Kraus, LLP.


(57) **CLAIM**

The ornamental design for graphical user interface for a com-
puter monitor of an x-ray tomography scanner, as shown.

DESCRIPTION

FIG. 1 is a front view of graphical user interface for a com-
puter monitor of an x-ray tomography scanner showing our
new design, the broken line drawing a computer monitor of an
x-ray tomography scanner is for illustrative purpose only and
forms no part of the claimed design; and,
FIG. 2 is an enlarged front view of graphical user interface for
a computer monitor of an x-ray tomography scanner.

1 Claim, 2 Drawing Sheets

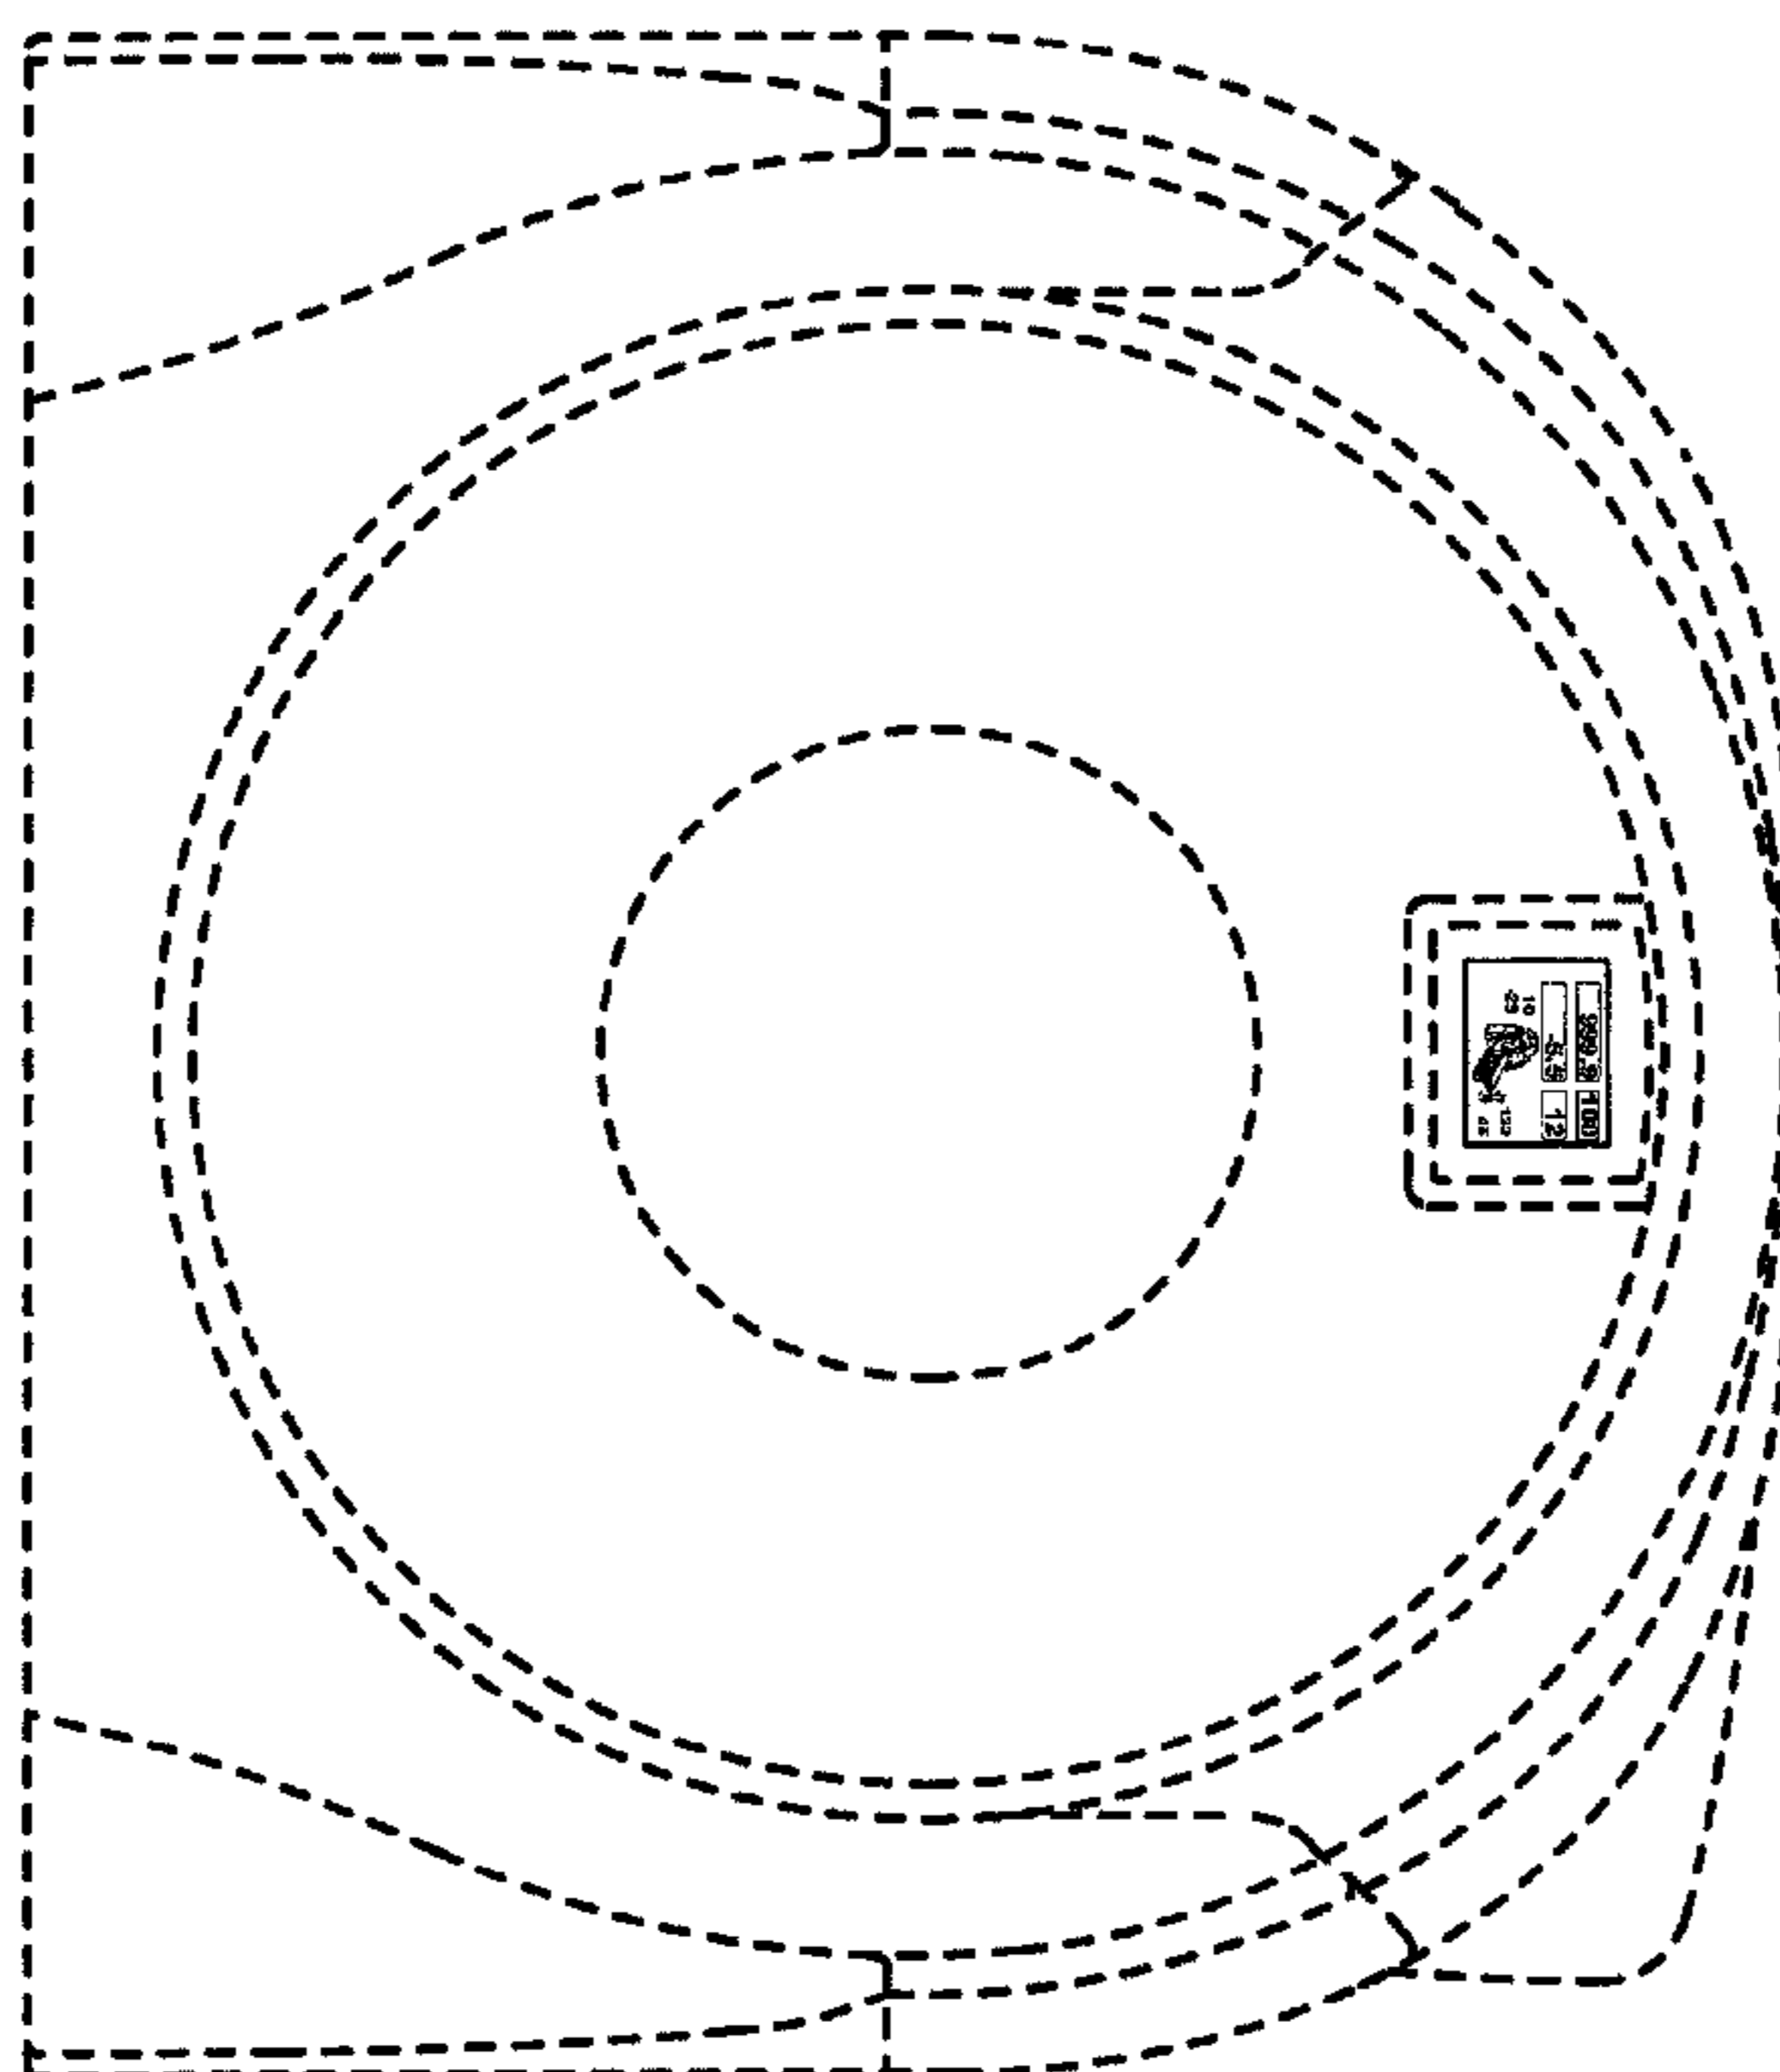

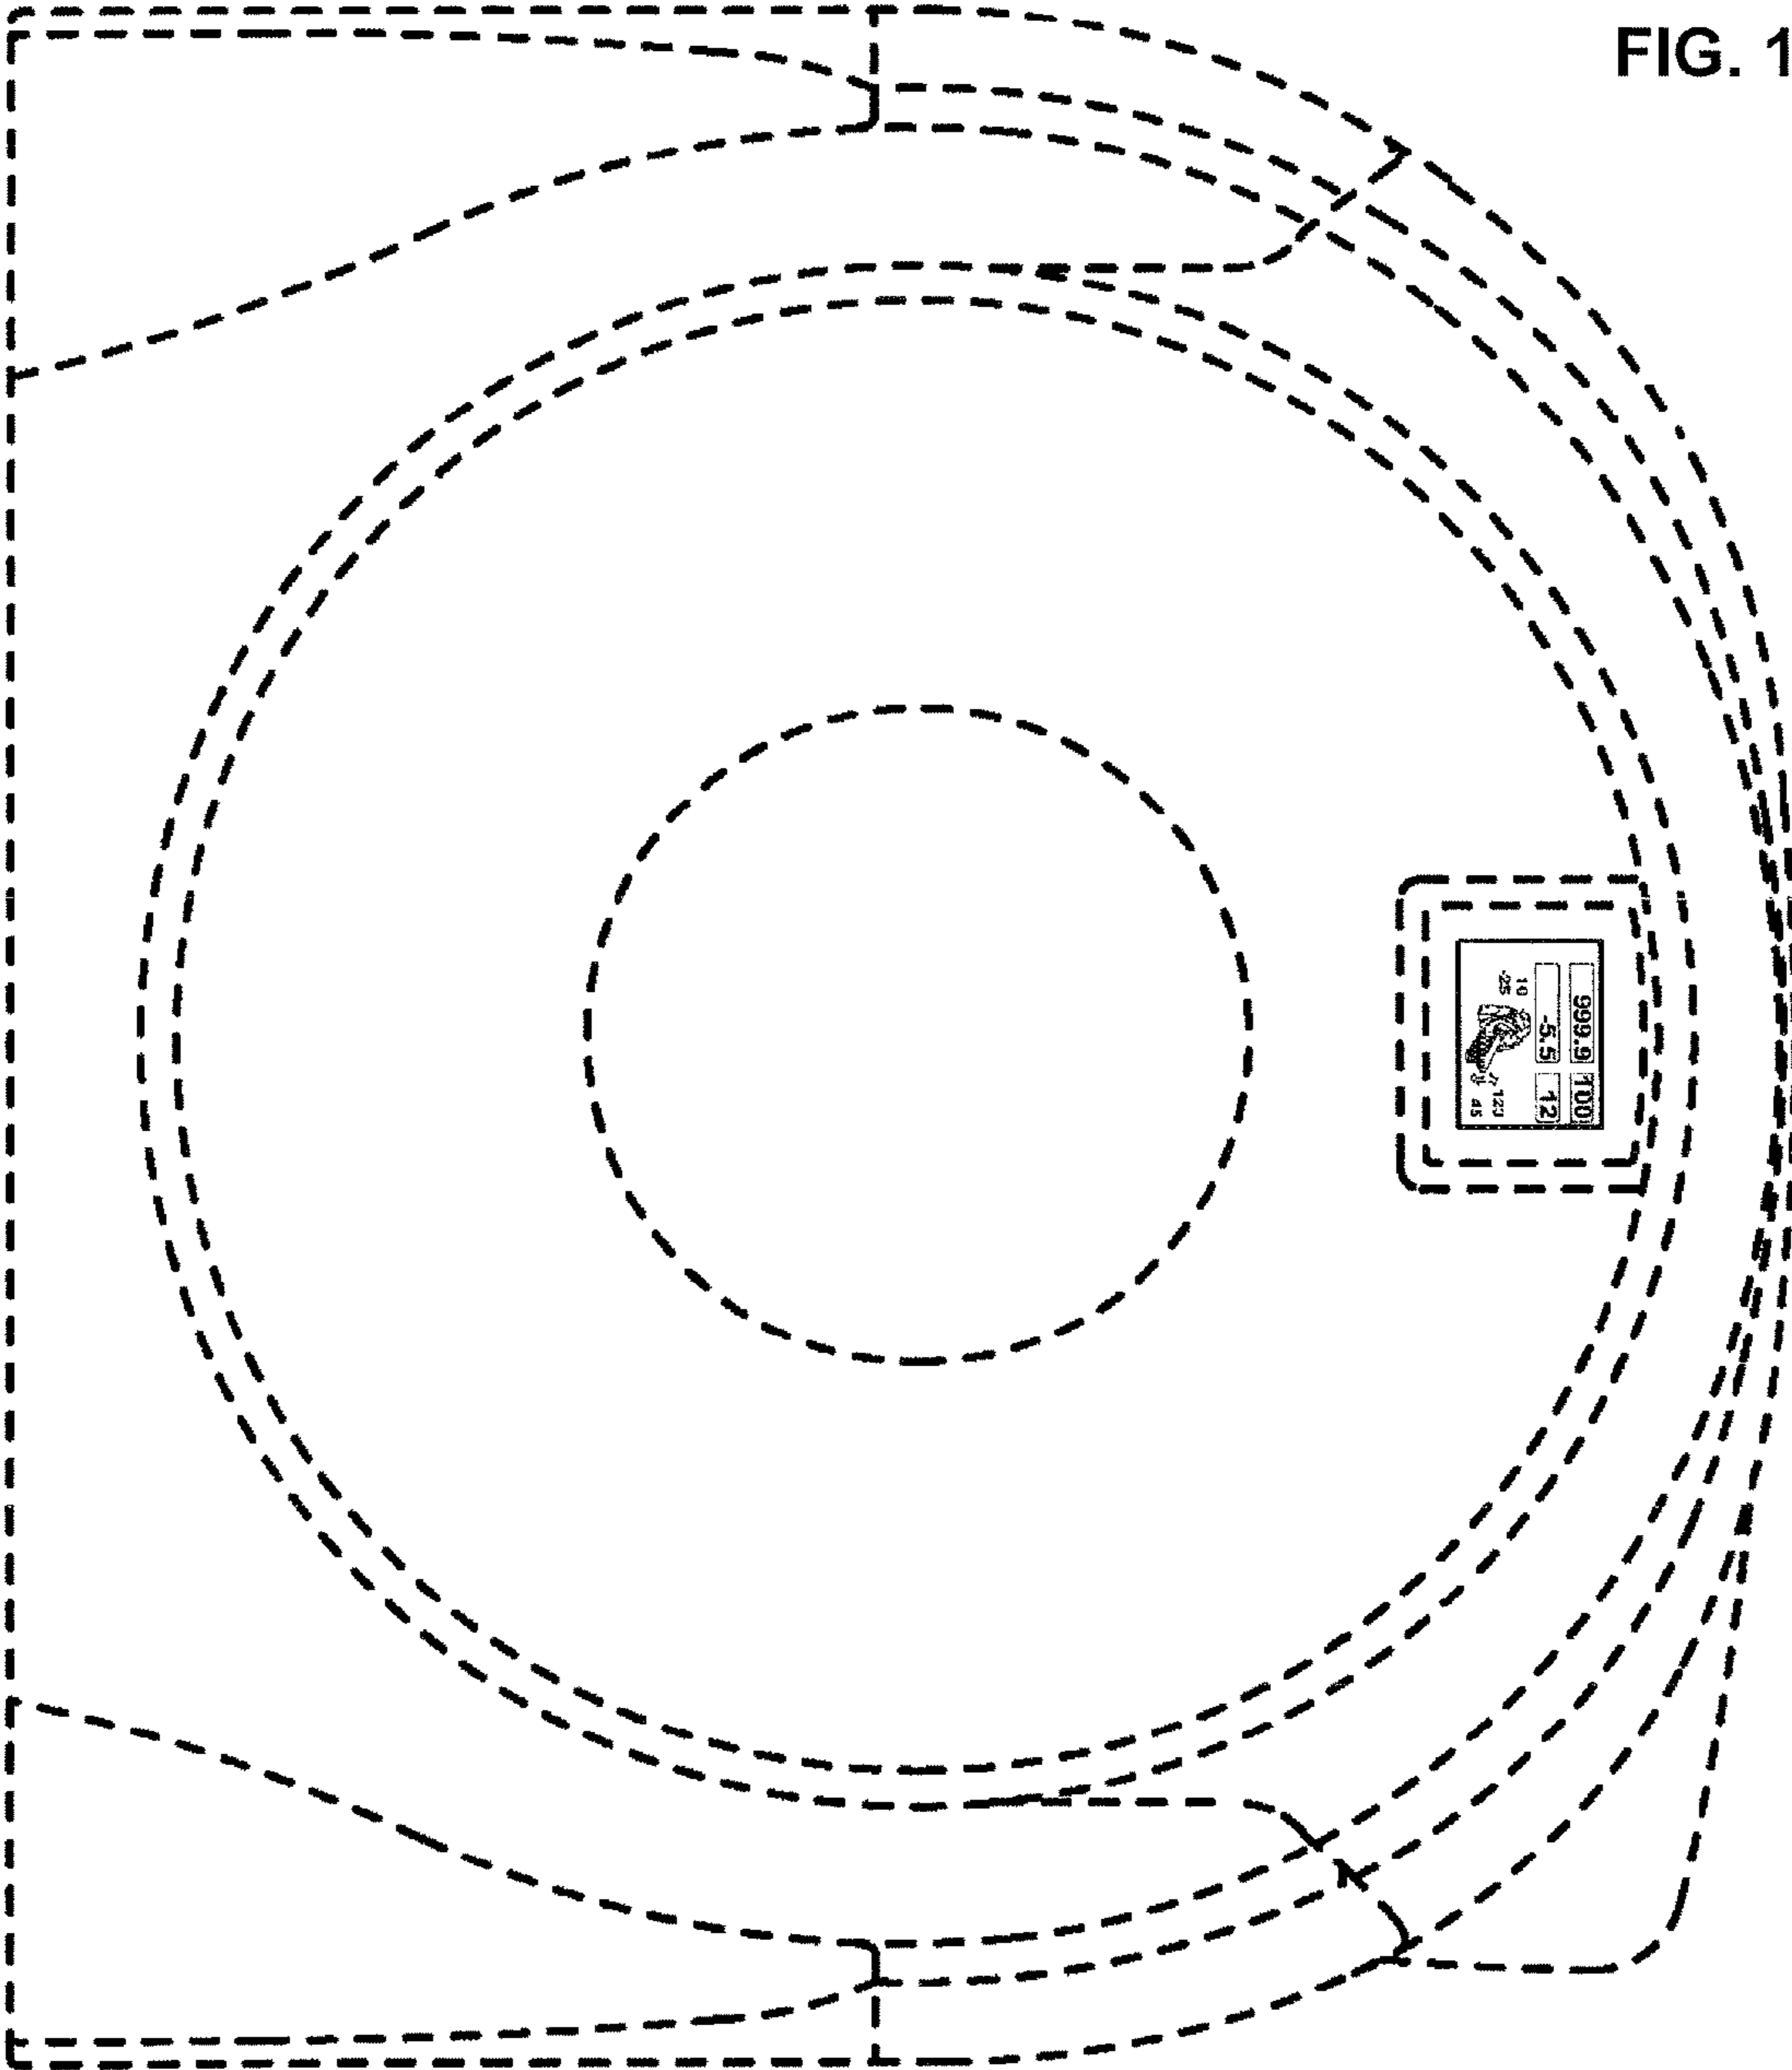


FIG. 2

