

US00D647209S

(12) **United States Design Patent**
Müller et al.

(10) **Patent No.:** **US D647,209 S**
(45) **Date of Patent:** **** Oct. 18, 2011**

(54) **LABORATORY ANALYSIS APPARATUS**

(75) Inventors: **Jan Müller**, Berlin (DE); **Florian Eckhardt**, Hennigsdorf (DE); **Stefan Thalhammer**, Straßlach (DE)

(73) Assignee: **B R A H M S Aktiengesellschaft**, Hennigsdorf (DE)

(**) Term: **14 Years**

(21) Appl. No.: **29/352,179**

(22) Filed: **Dec. 17, 2009**

(30) **Foreign Application Priority Data**

Jun. 17, 2009 (EM) 001551276

(51) **LOC (9) Cl.** **24-02**

(52) **U.S. Cl.** **D24/216**

(58) **Field of Classification Search** D24/107,
D24/158, 164, 165, 167, 170, 186–187, 231;
D10/46, 75, 81; 600/300, 301, 368, 372,
600/481, 529, 544, 554, 561; 422/1, 61,
422/68.1, 99–104, 129; 436/47, 49, 179–180
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D378,782 S * 4/1997 LaBarbera et al. D24/232
D467,349 S * 12/2002 Niedbala et al. D24/232
D489,816 S * 5/2004 Ross D24/107
D537,951 S * 3/2007 Okamoto et al. D24/233
D554,069 S * 10/2007 Bolotin et al. D13/162

D554,070 S * 10/2007 Bolotin et al. D13/162
D556,914 S * 12/2007 Okamoto et al. D24/233
D569,526 S * 5/2008 Duffy et al. D24/232
D581,823 S * 12/2008 Mori et al. D10/81
D597,216 S * 7/2009 McGuigan et al. D24/216
D607,569 S * 1/2010 Yukikado et al. D24/186
D609,343 S * 2/2010 Omaki D24/165
D609,344 S * 2/2010 Hara D24/165
D612,276 S * 3/2010 Duffy et al. D10/81
D612,949 S * 3/2010 Falkenstein D24/232

* cited by examiner

Primary Examiner — T. Chase Nelson

Assistant Examiner — Mark Cavanna

(74) *Attorney, Agent, or Firm* — Leason Ellis LLP

(57) **CLAIM**


The ornamental design for a laboratory analysis apparatus, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a laboratory analysis apparatus showing our new design in a closed position;
FIG. 2 is top plan view thereof;
FIG. 3 is a front perspective view thereof;
FIG. 4 is a left side perspective view thereof;
FIG. 5 is a right side perspective view thereof;
FIG. 6 is a rear perspective view thereof;
FIG. 7 is a bottom perspective view thereof; and,
FIG. 8 is perspective view thereof showing an open position of the apparatus.

The broken lines are included for the purpose of illustrating a portion of the laboratory analysis apparatus that forms no part of the claimed design.

1 Claim, 8 Drawing Sheets

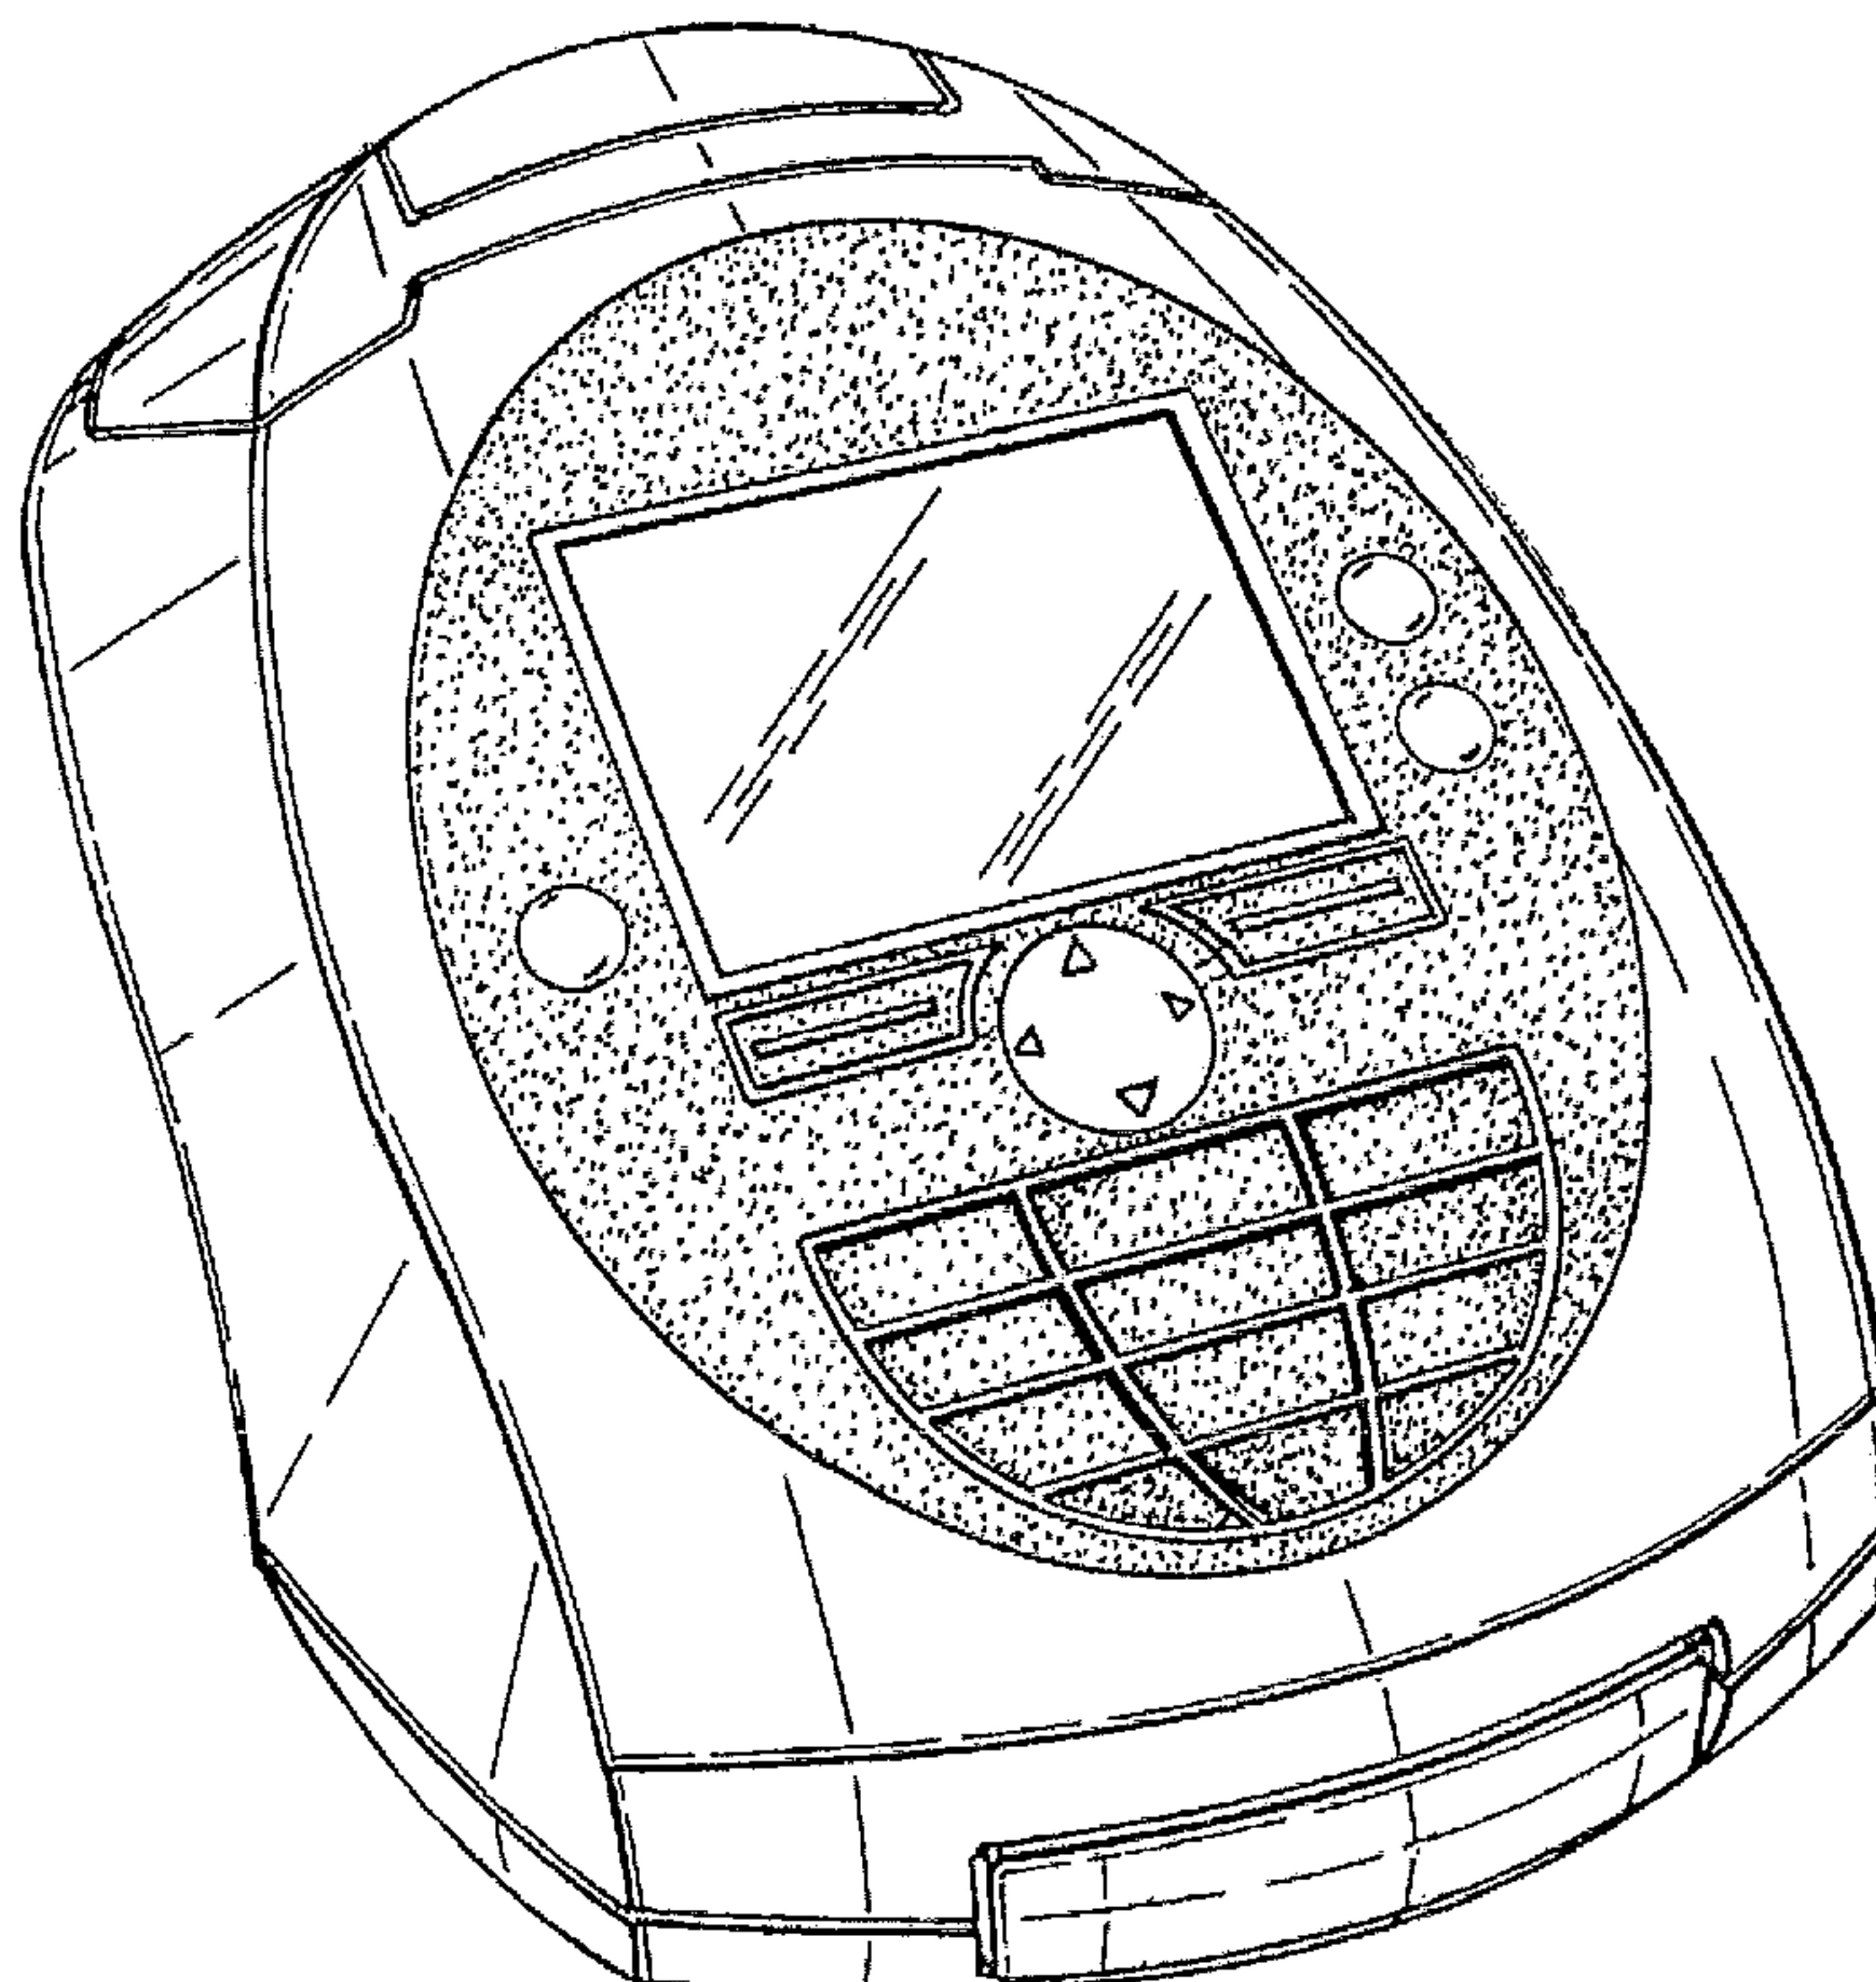

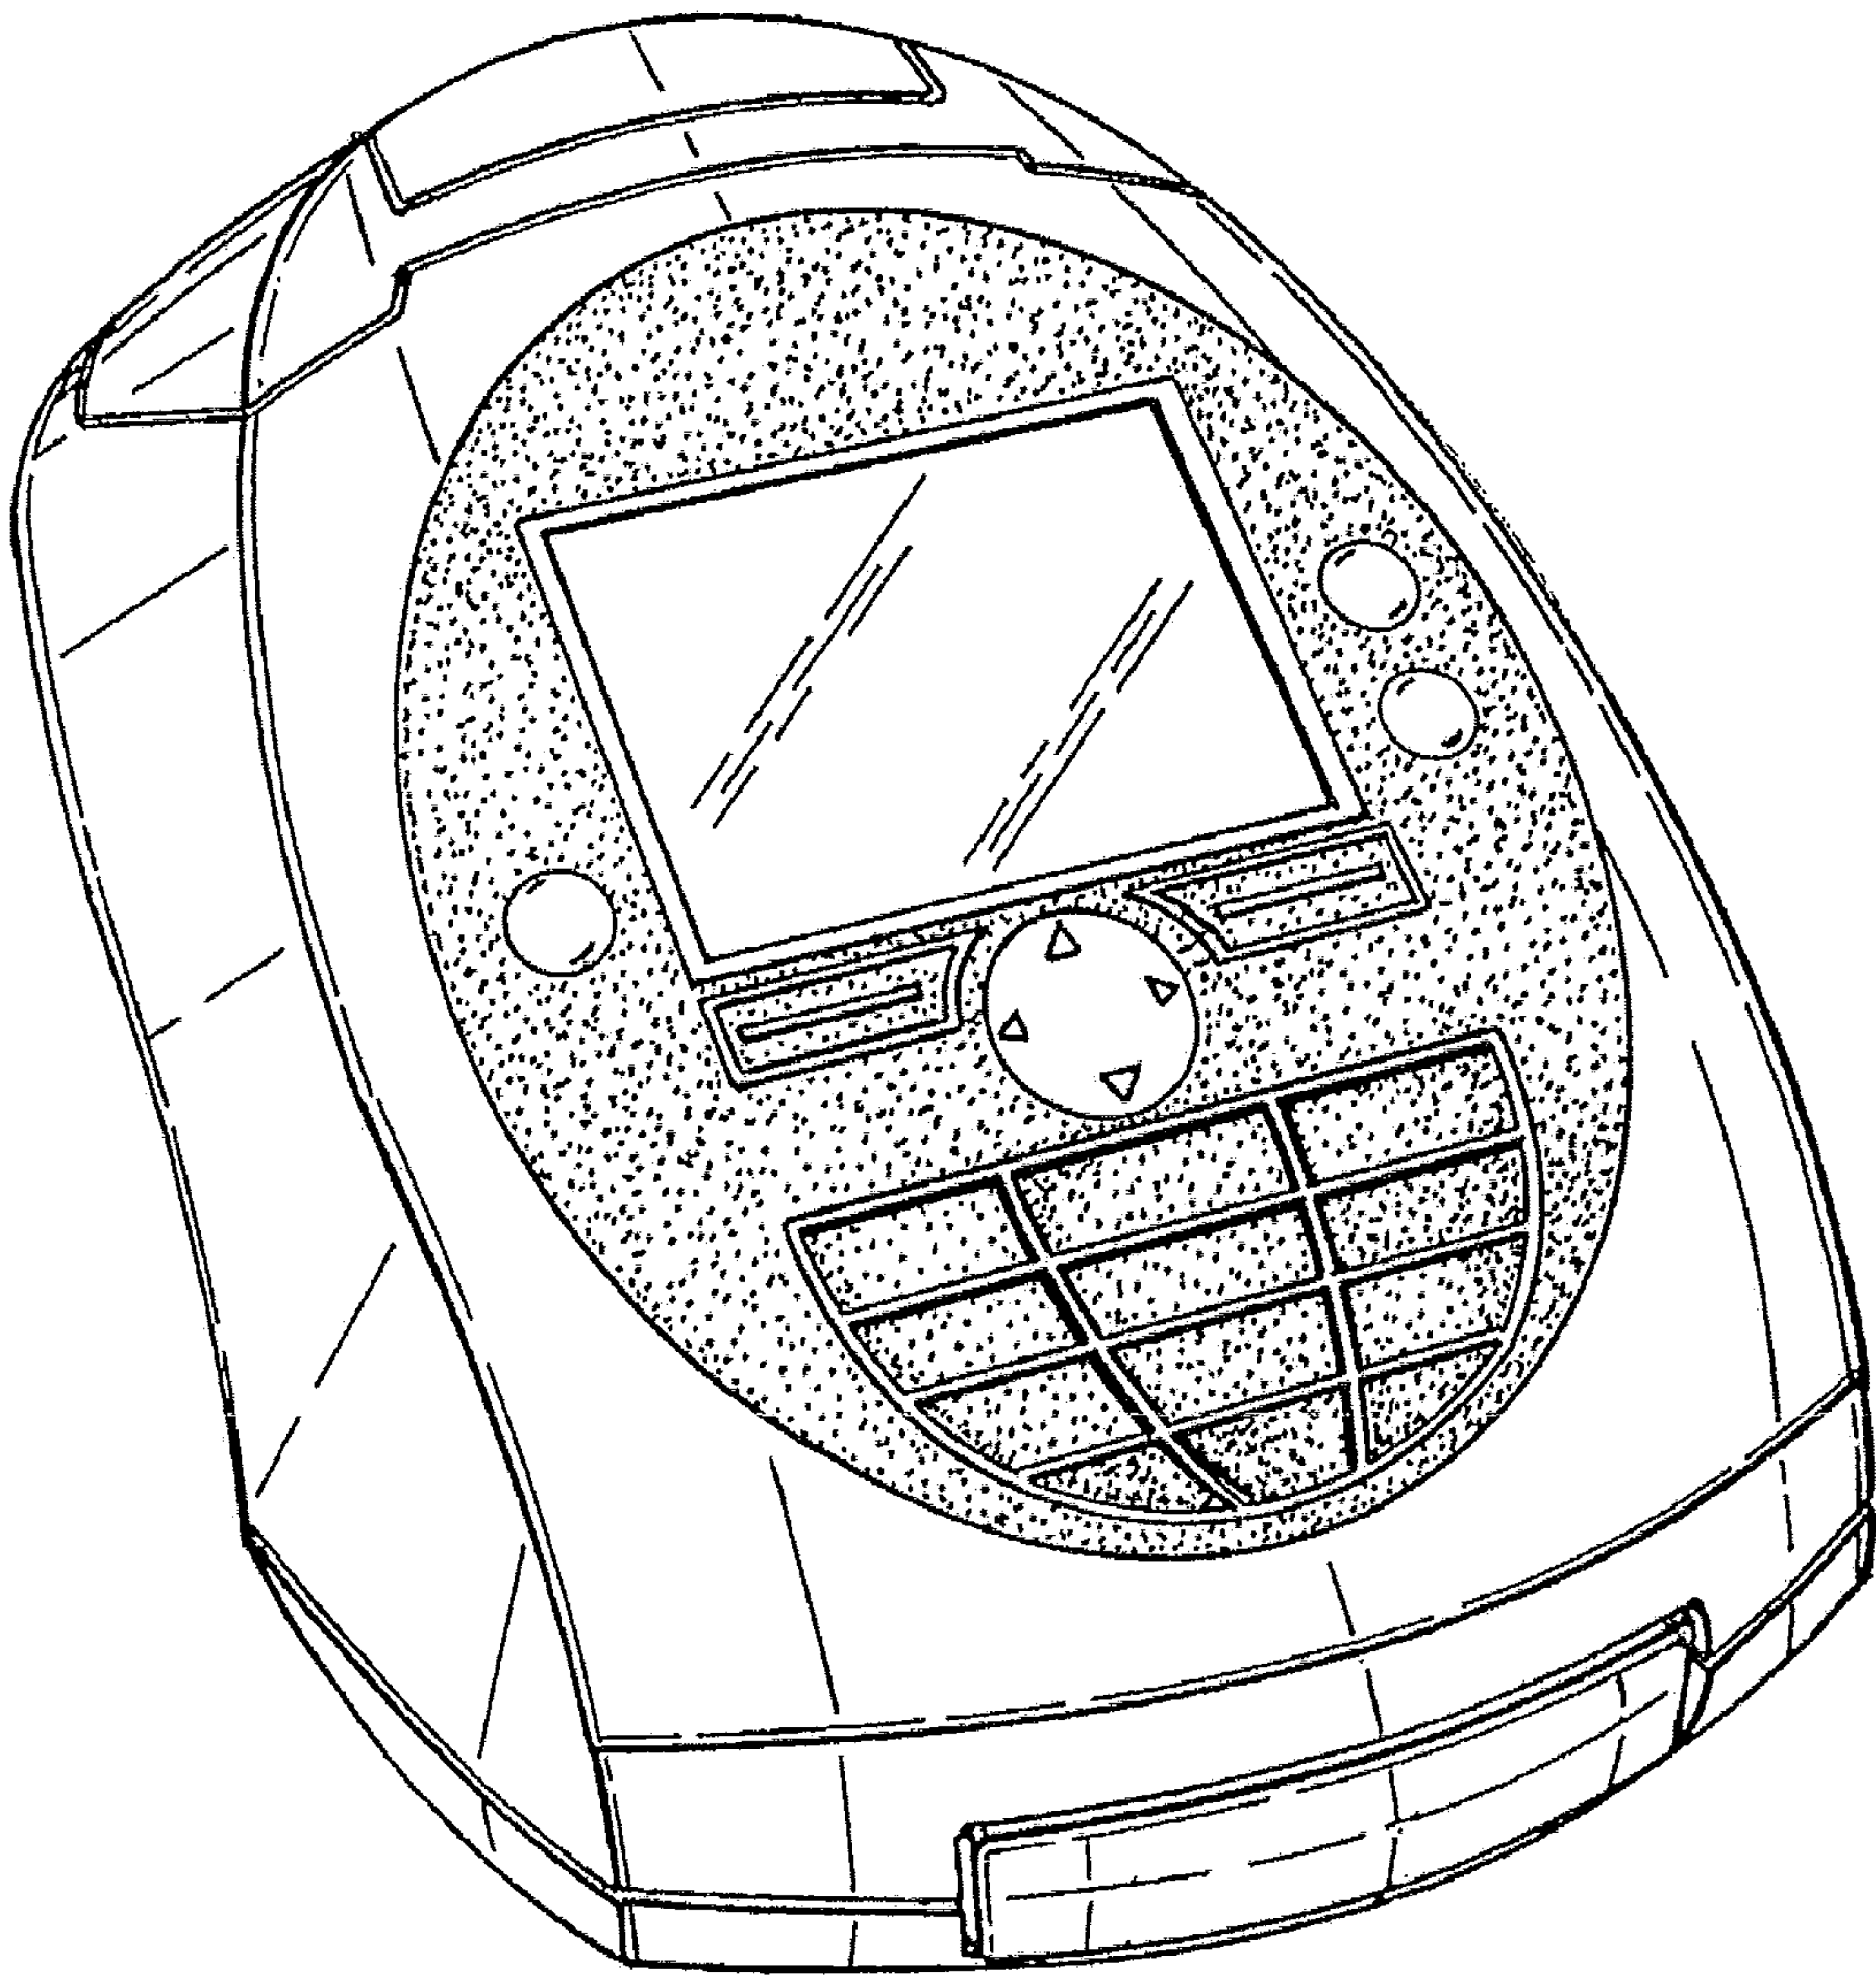


Fig. 1

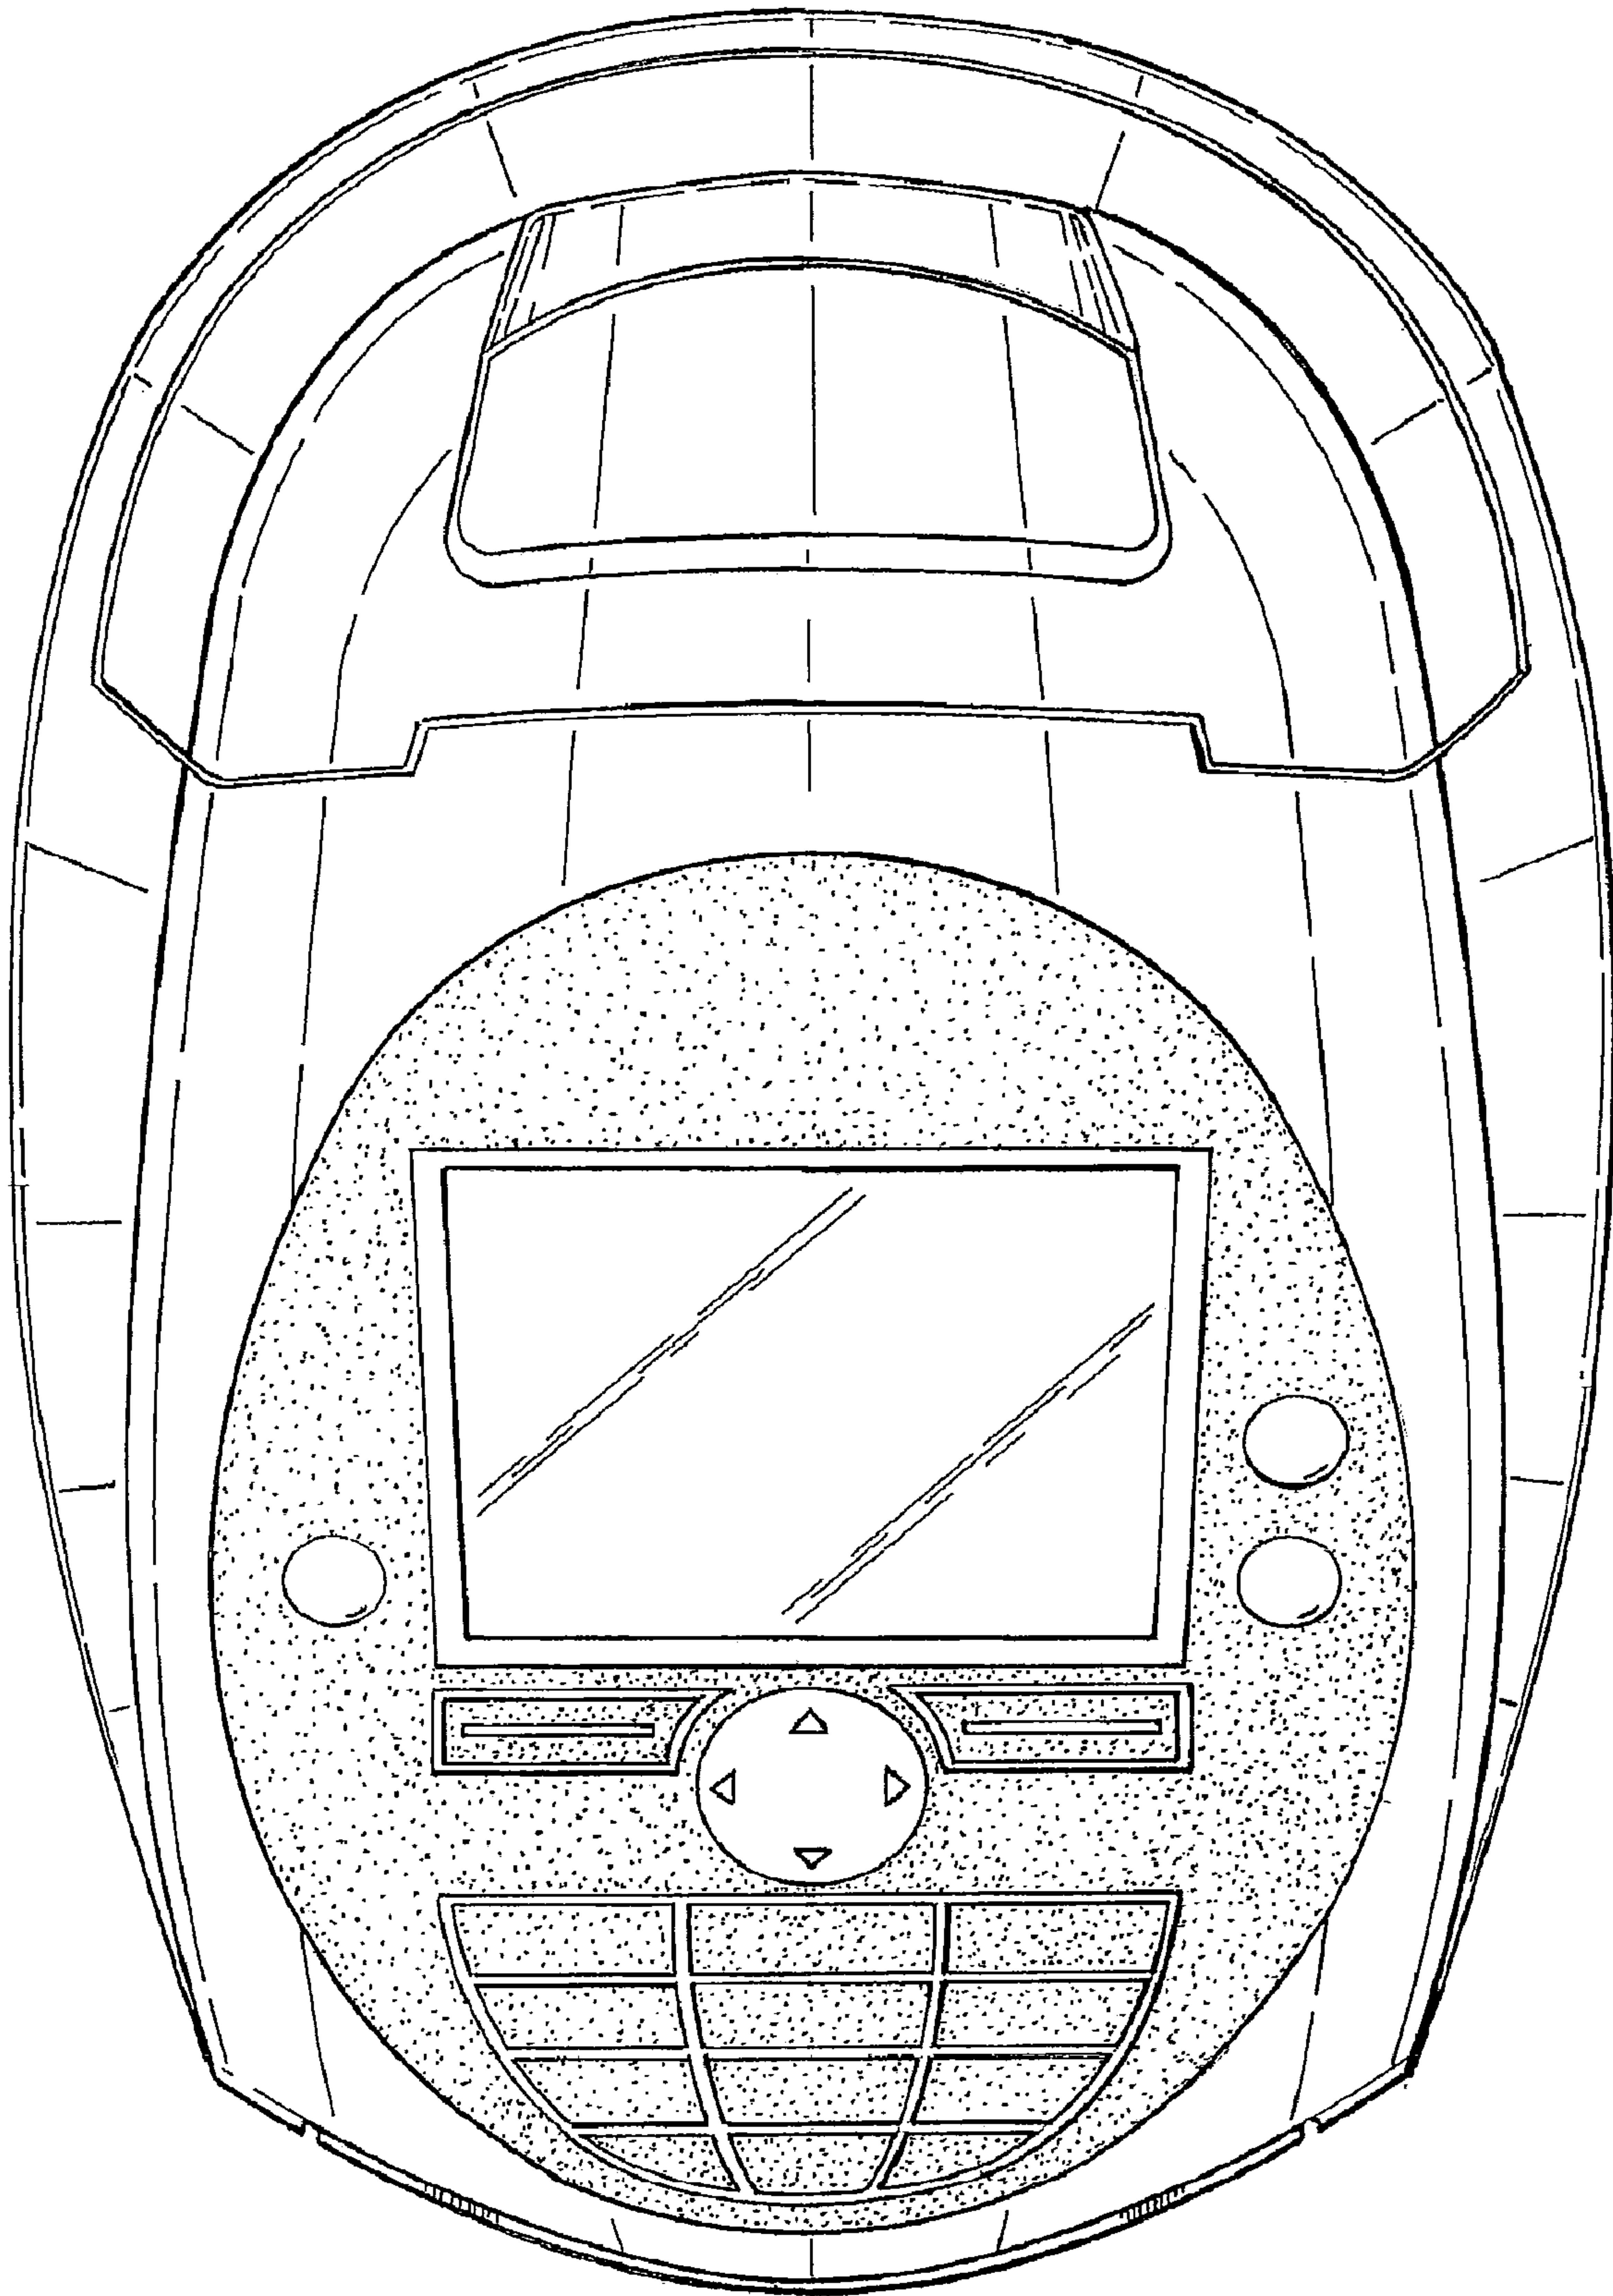


Fig. 2

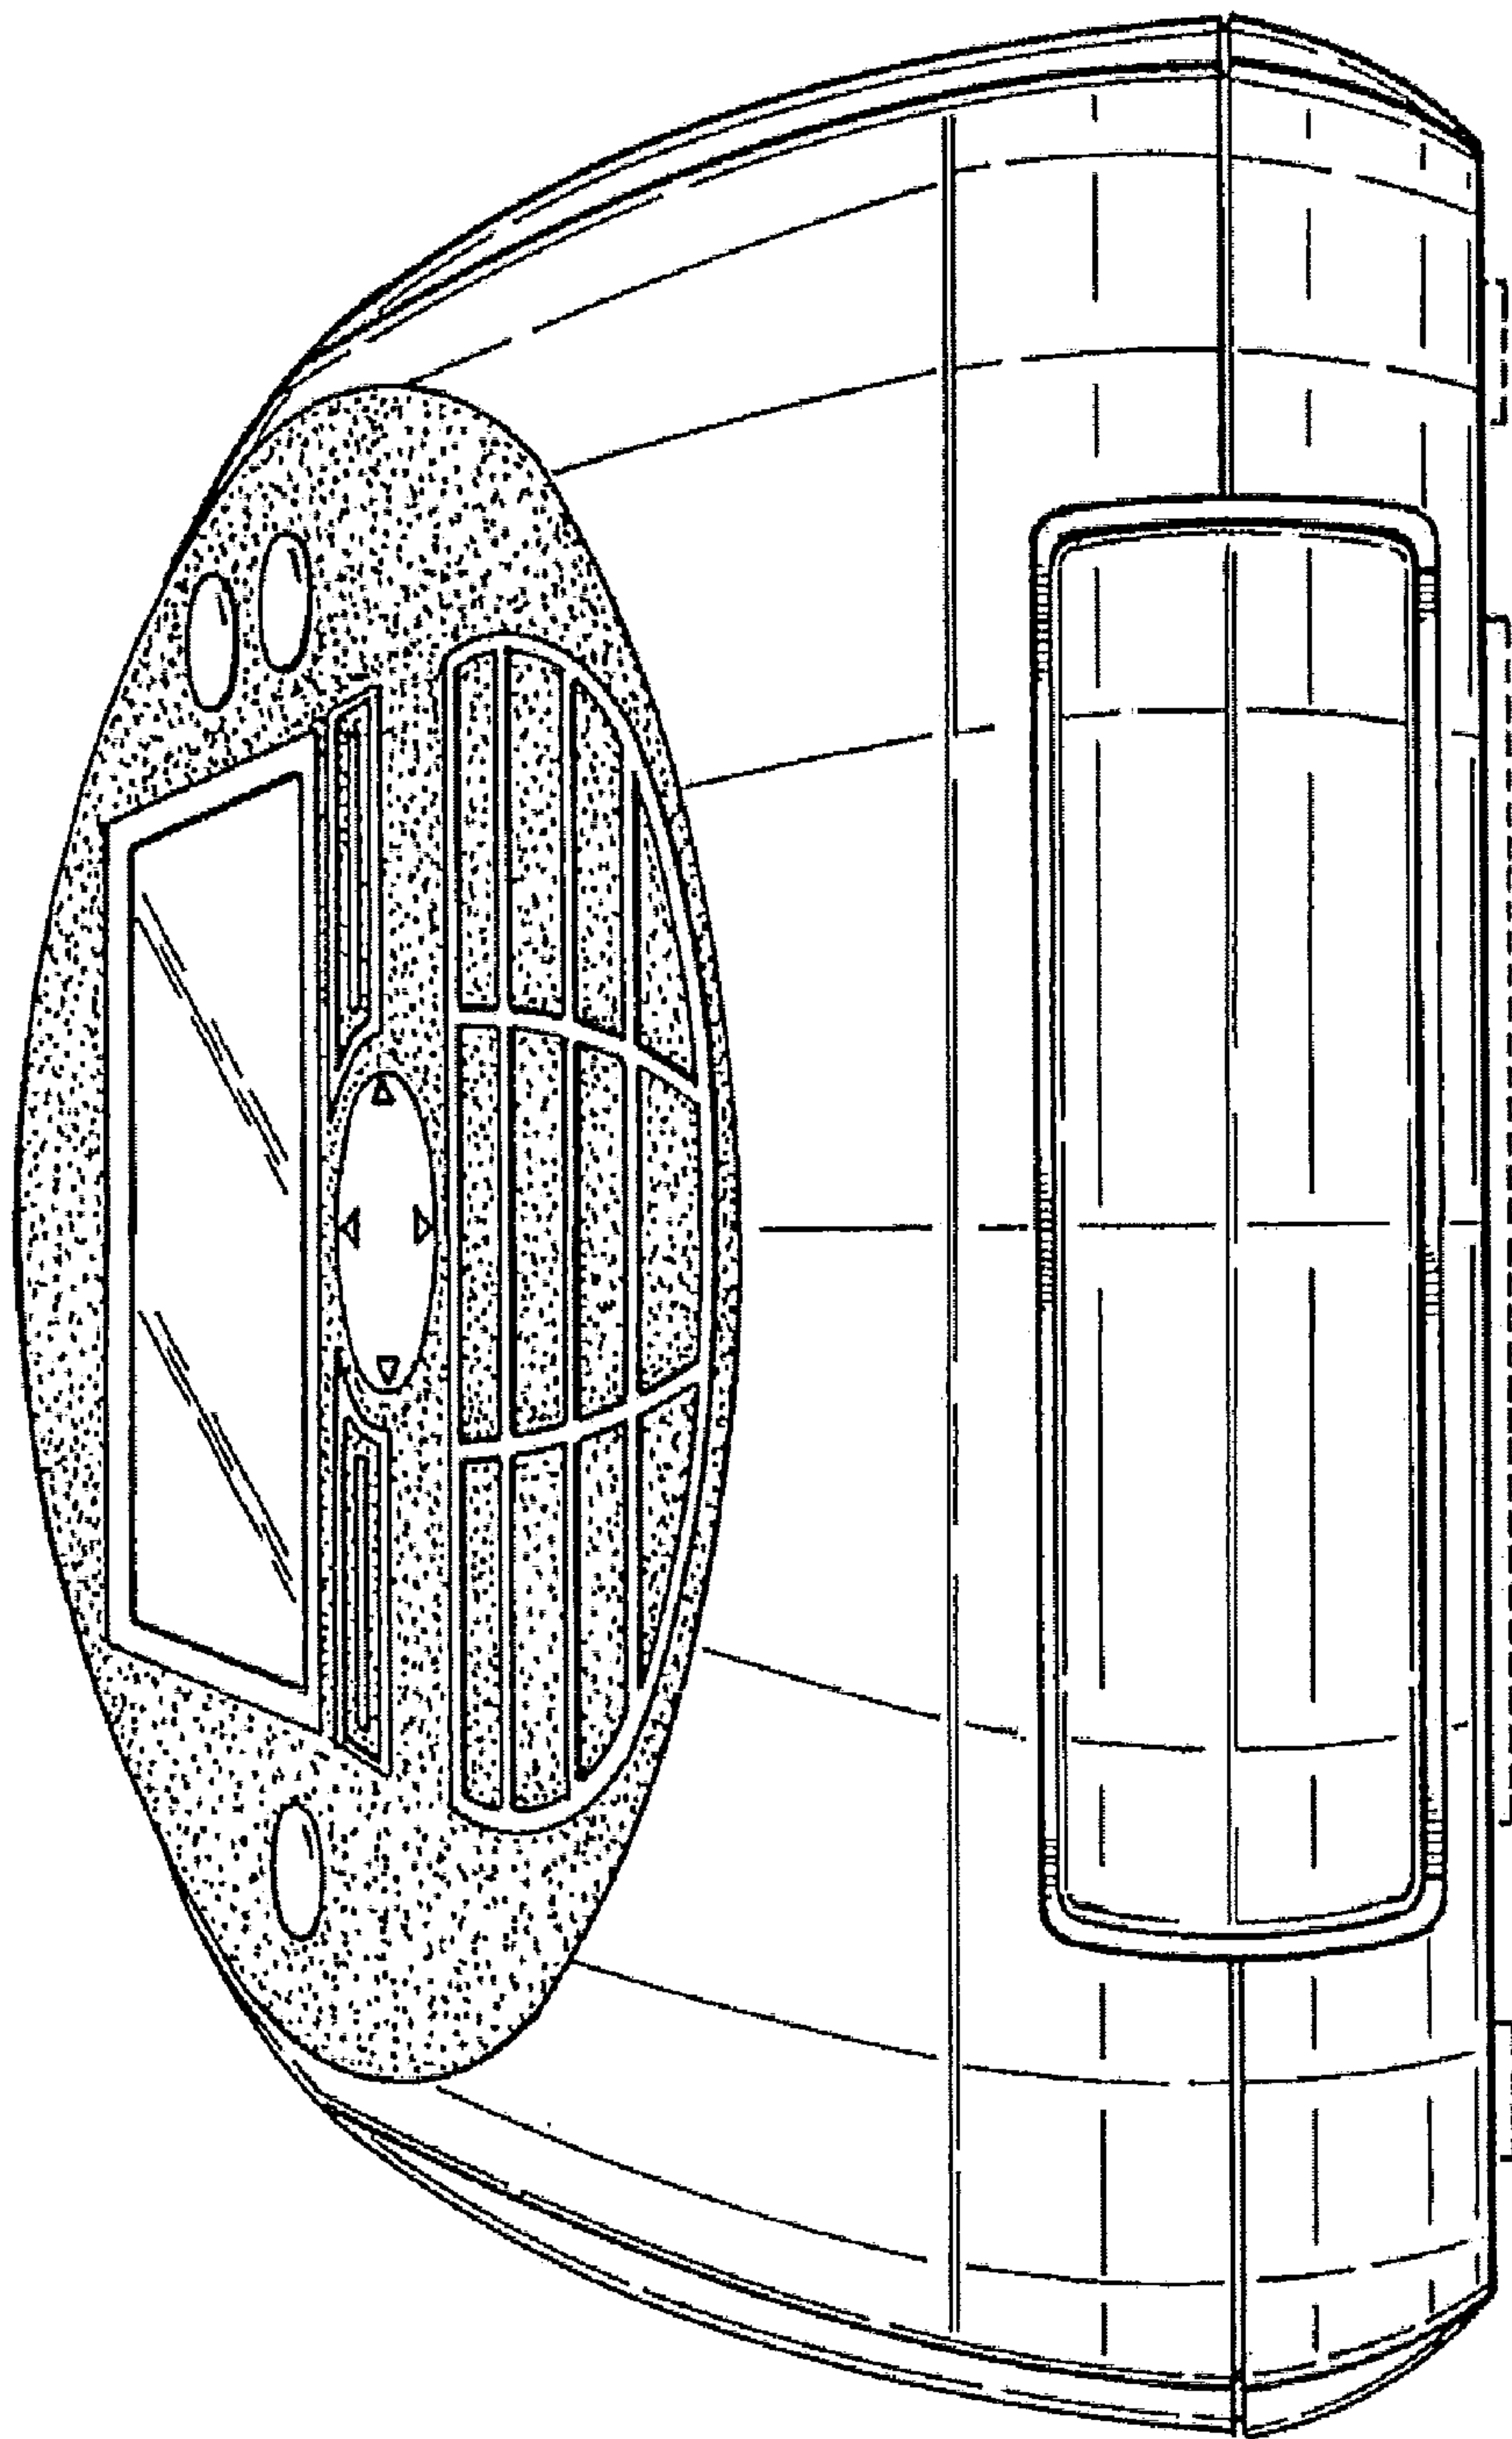


Fig. 3

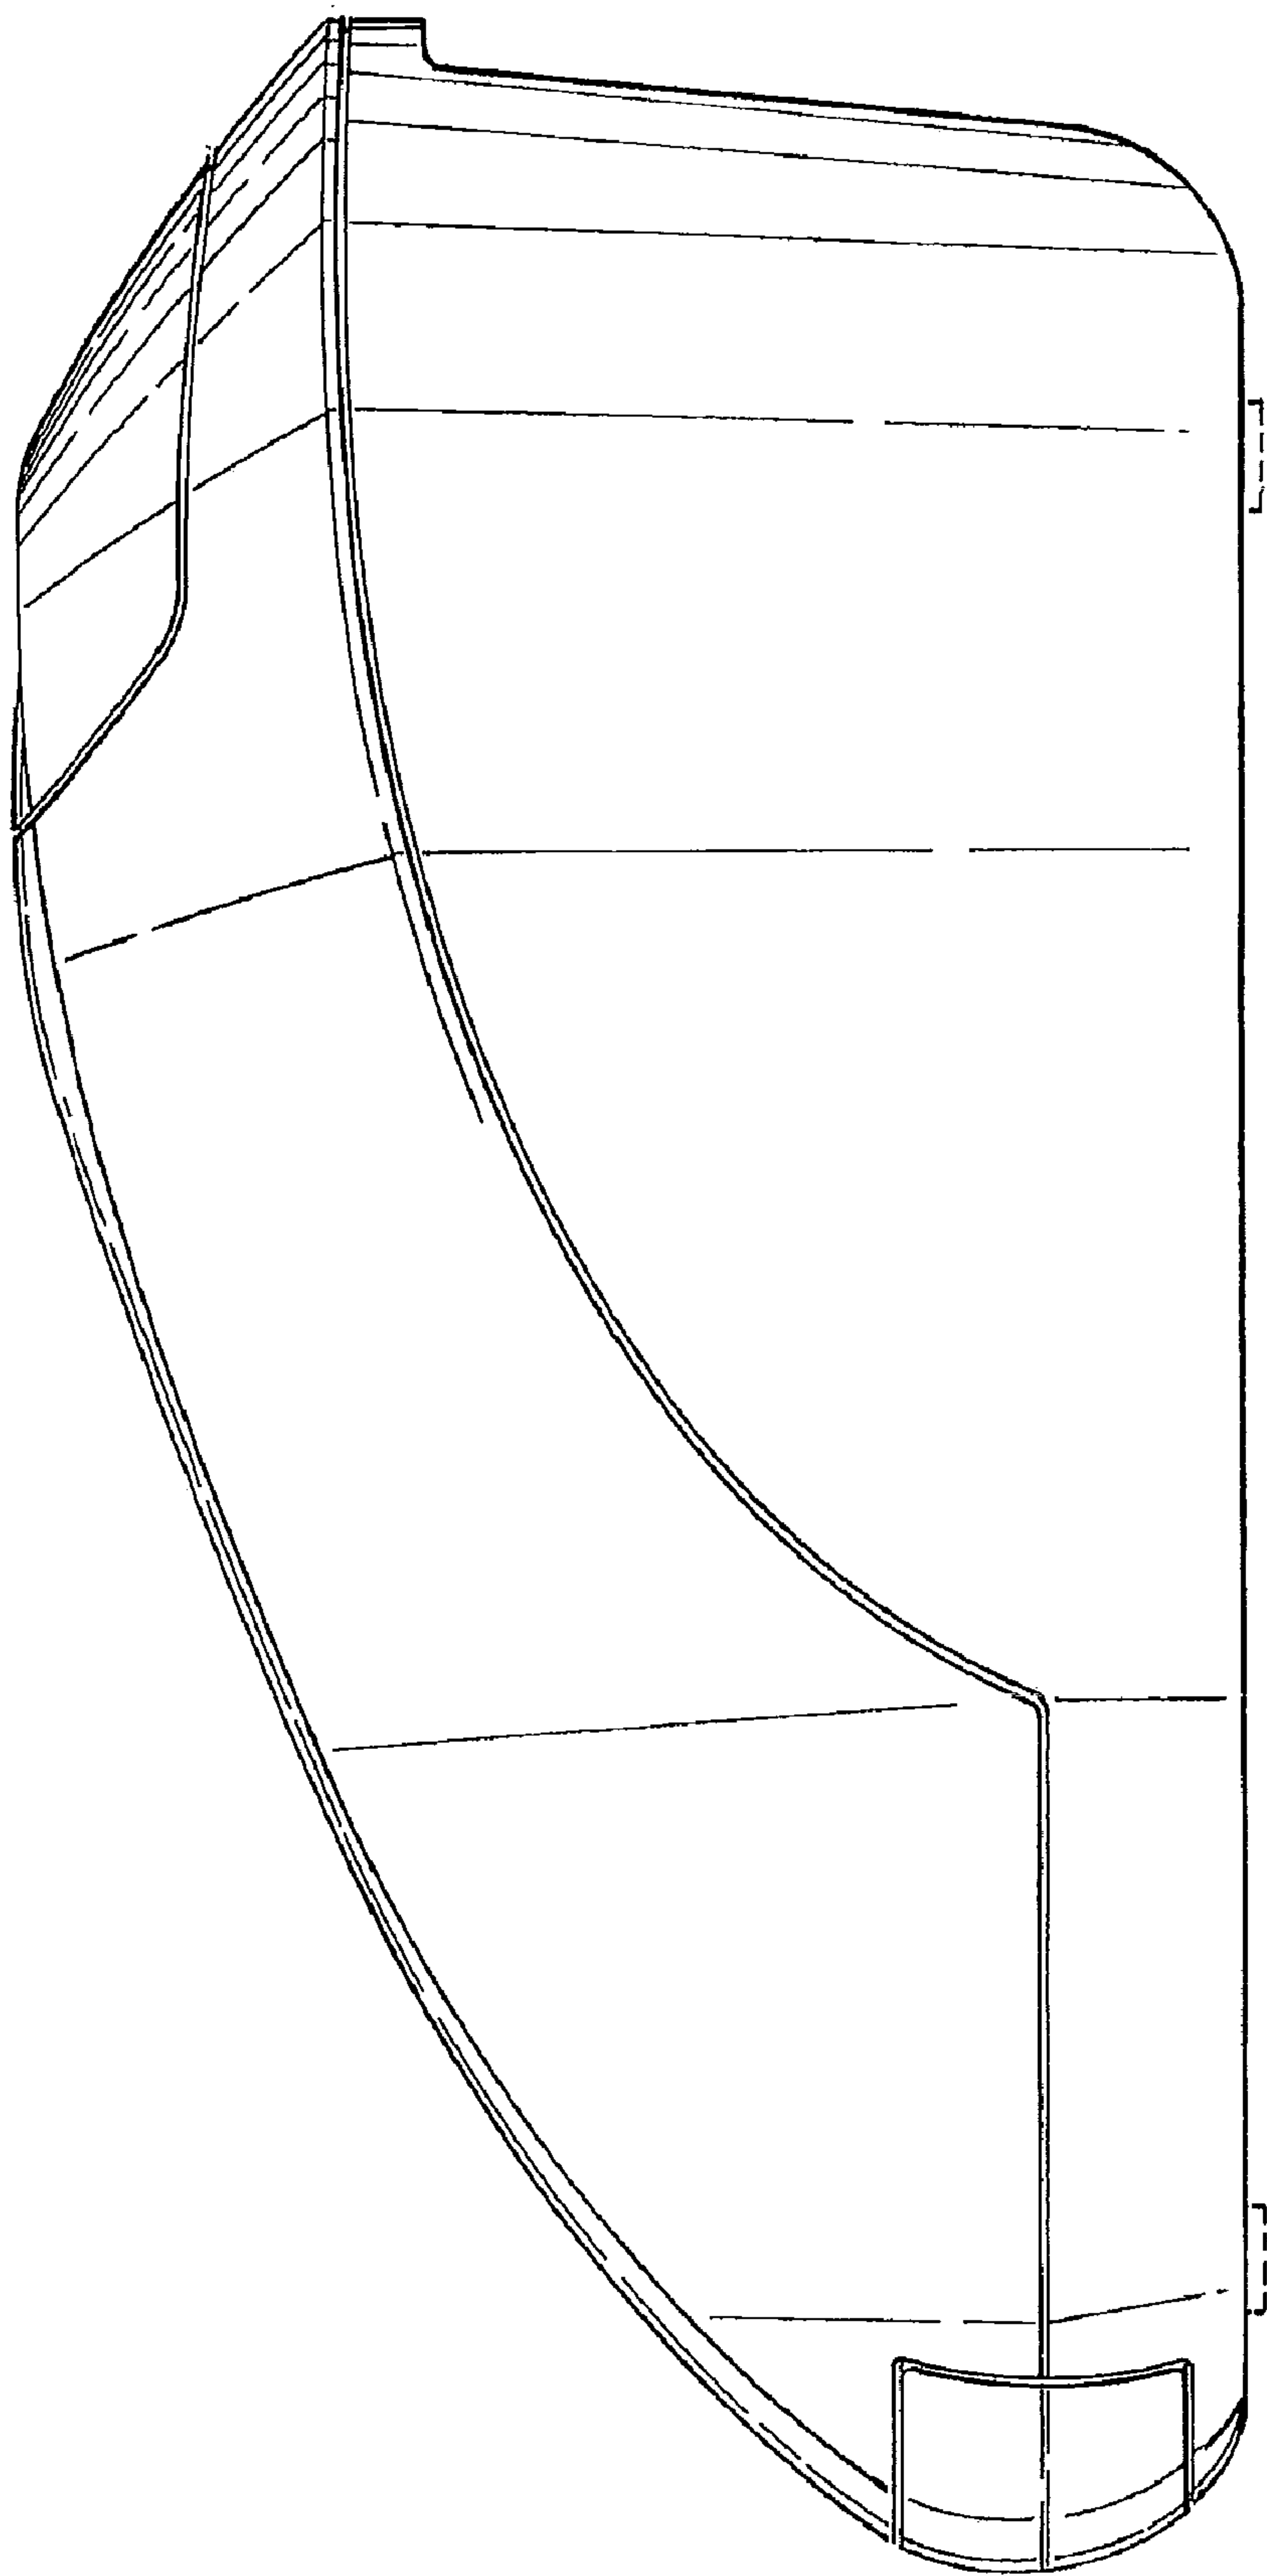


Fig. 4

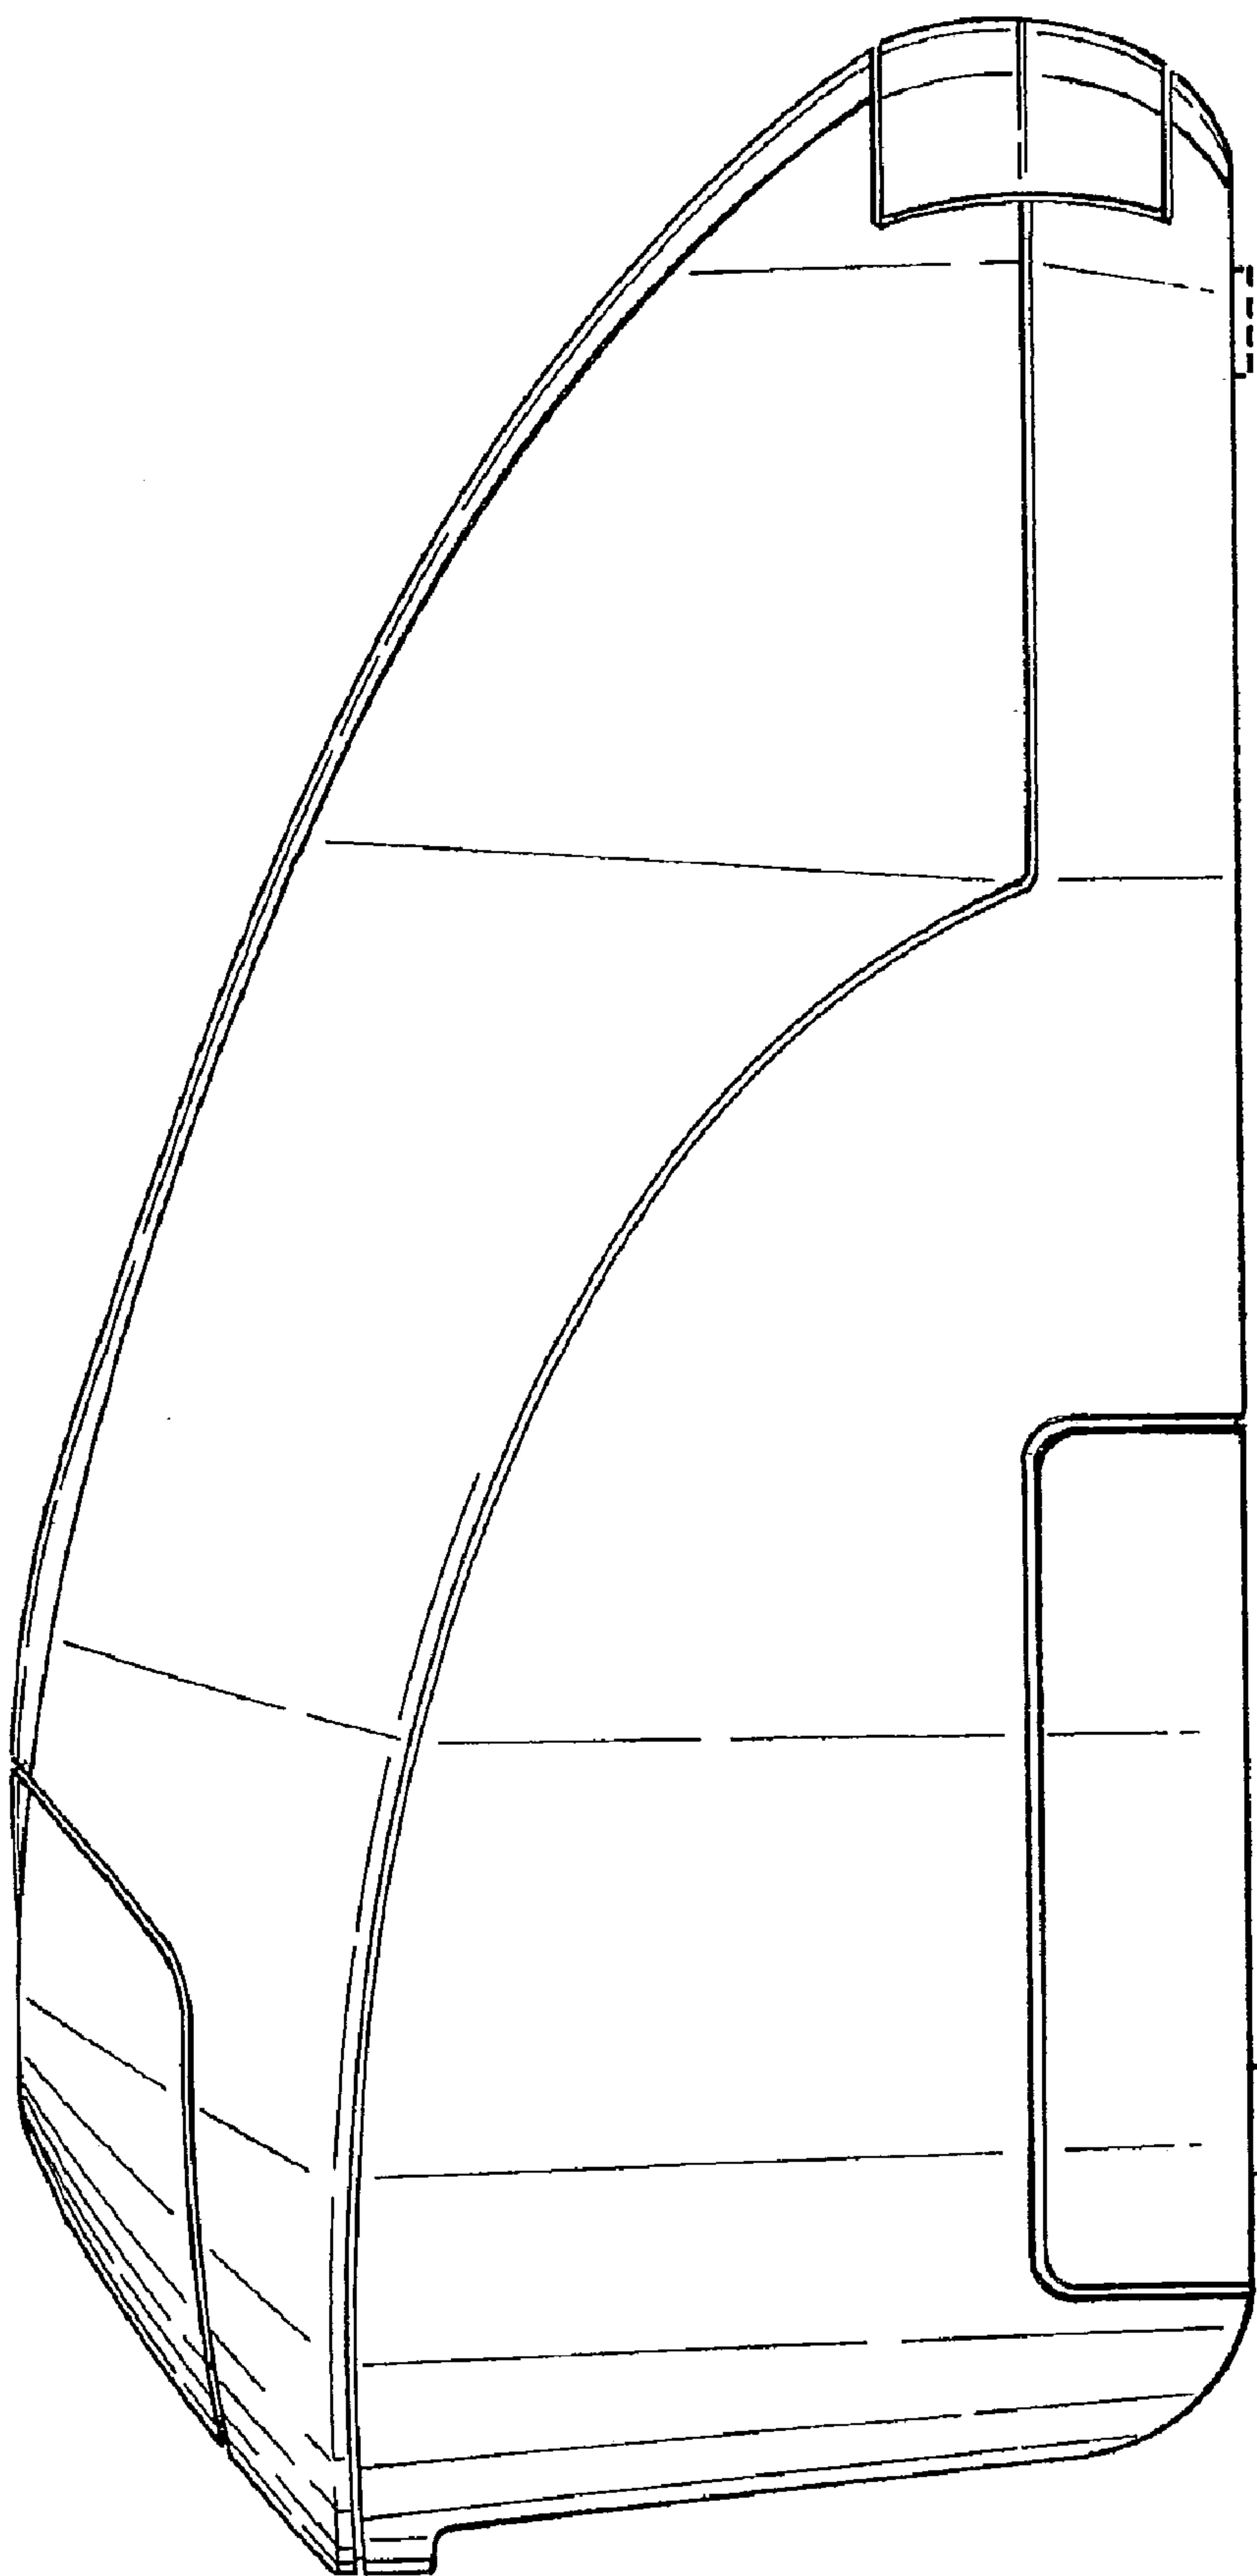


Fig. 5

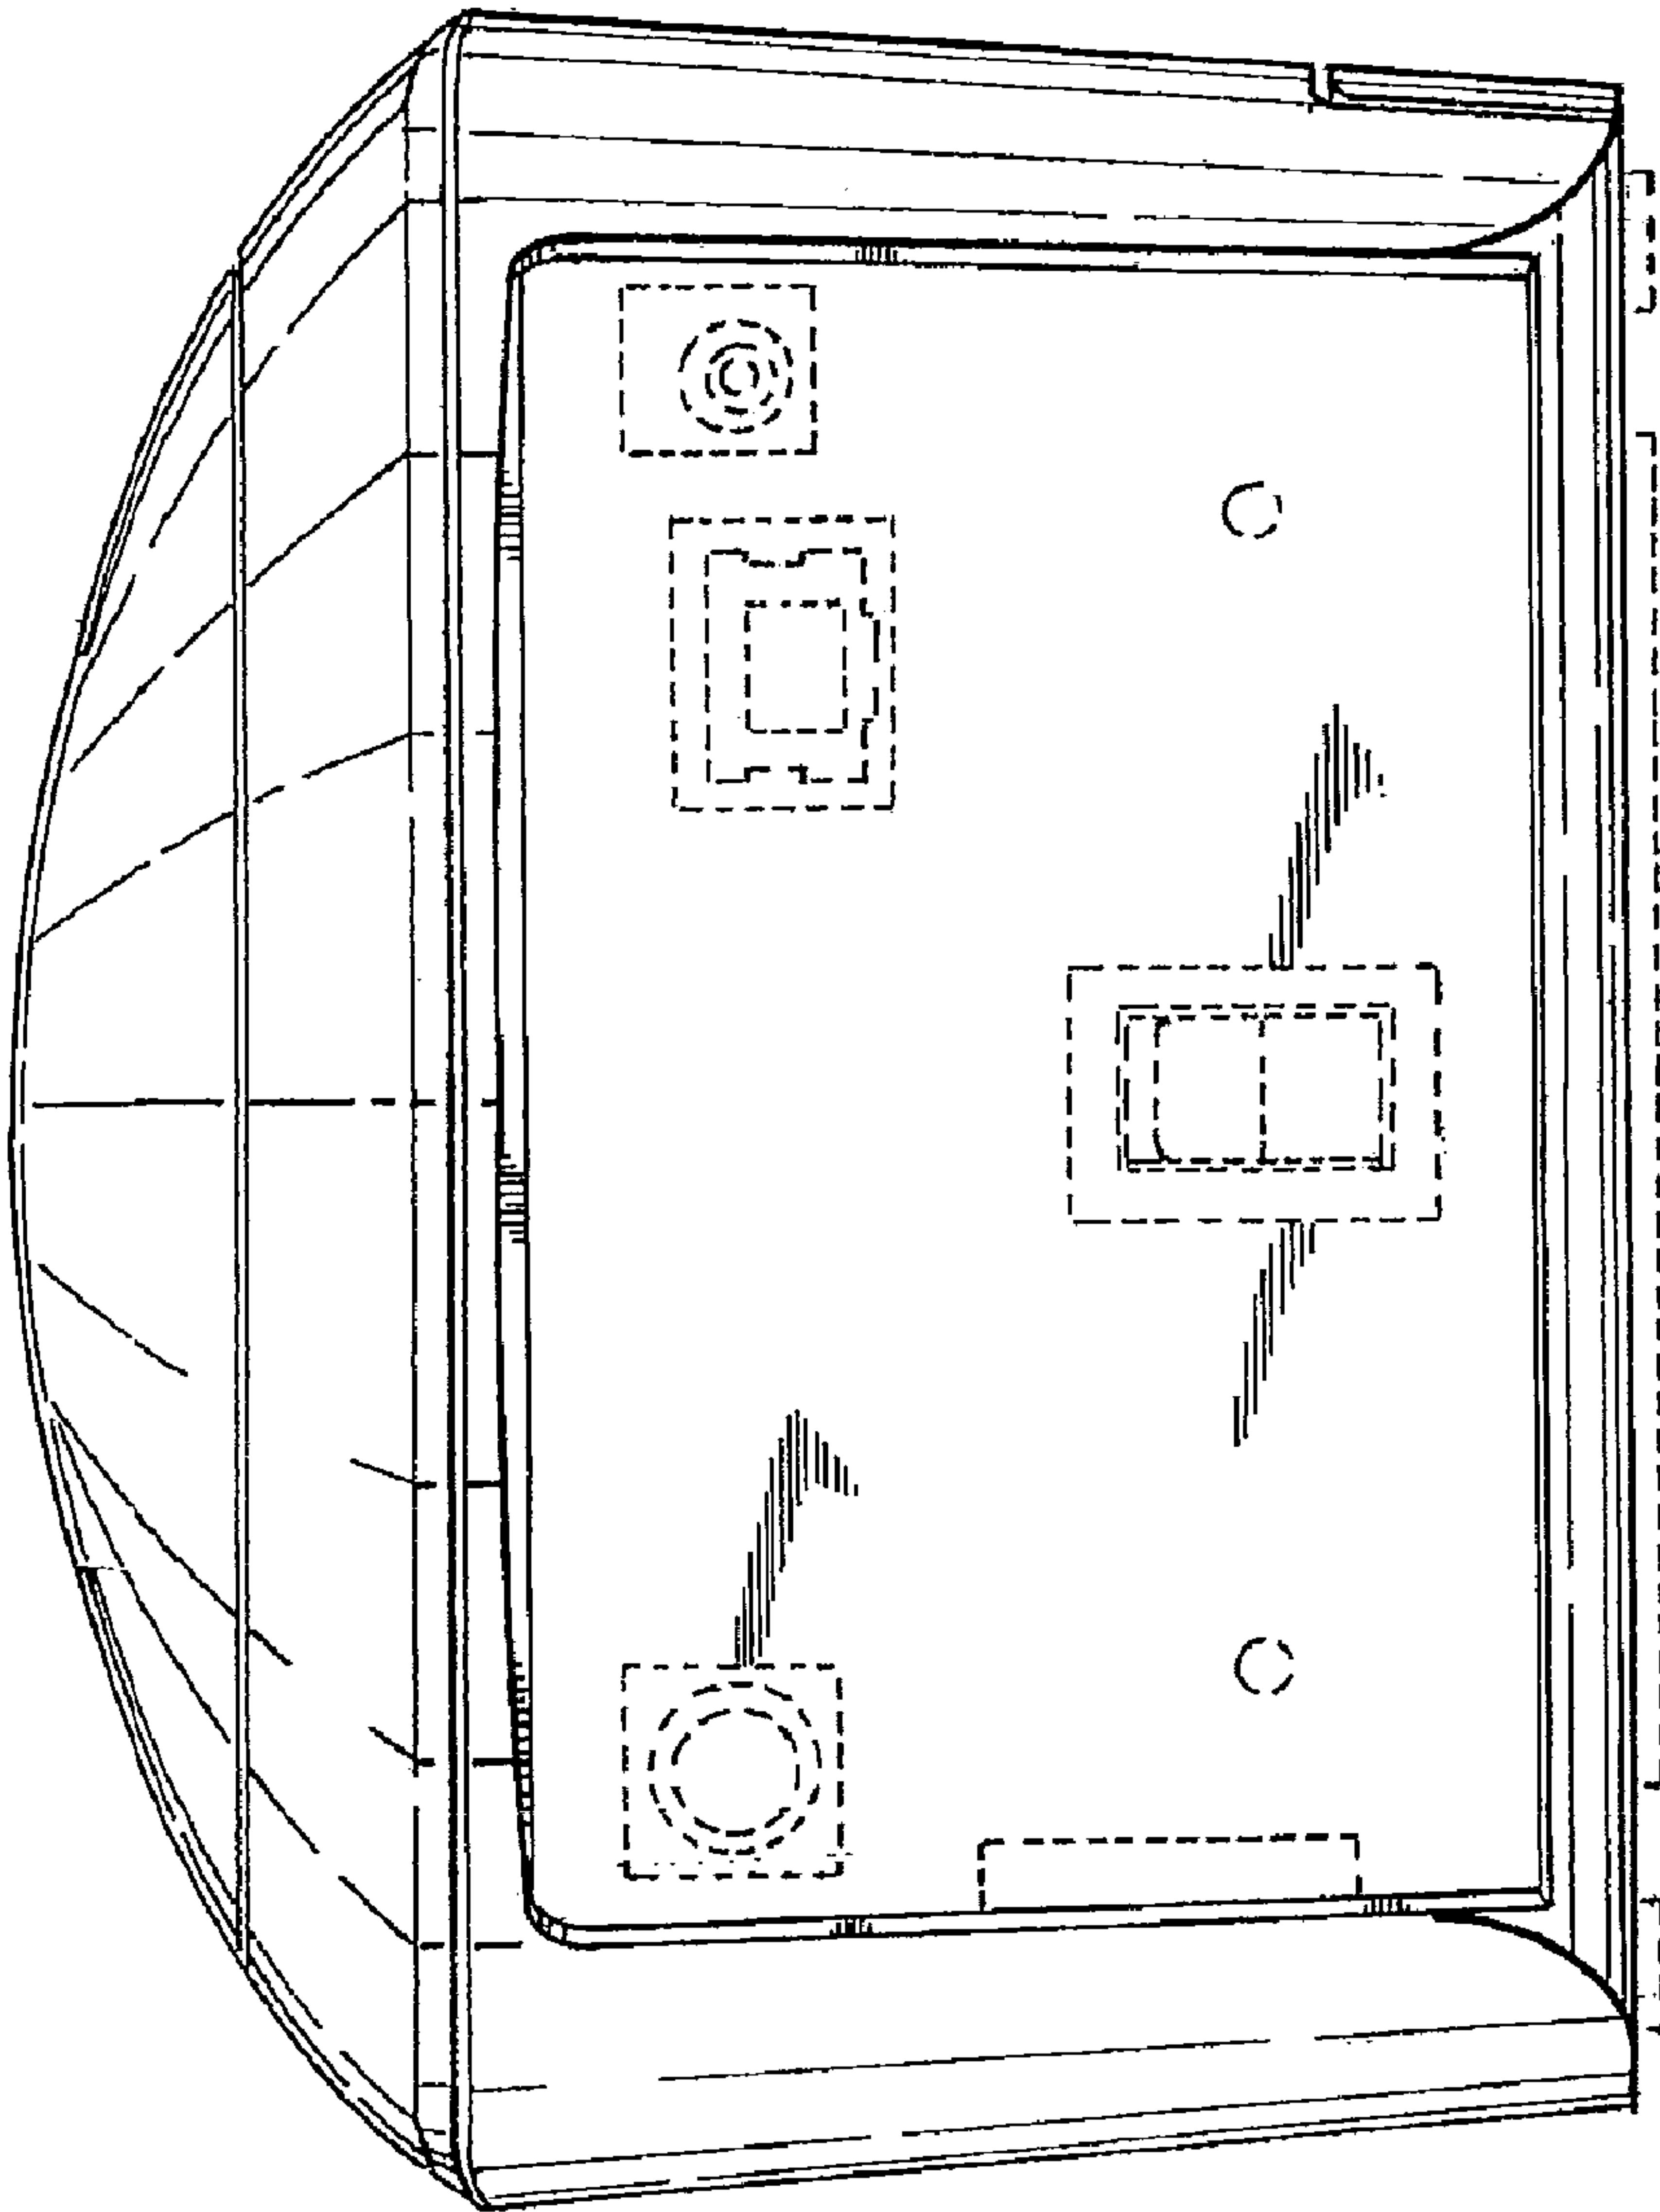


Fig. 6

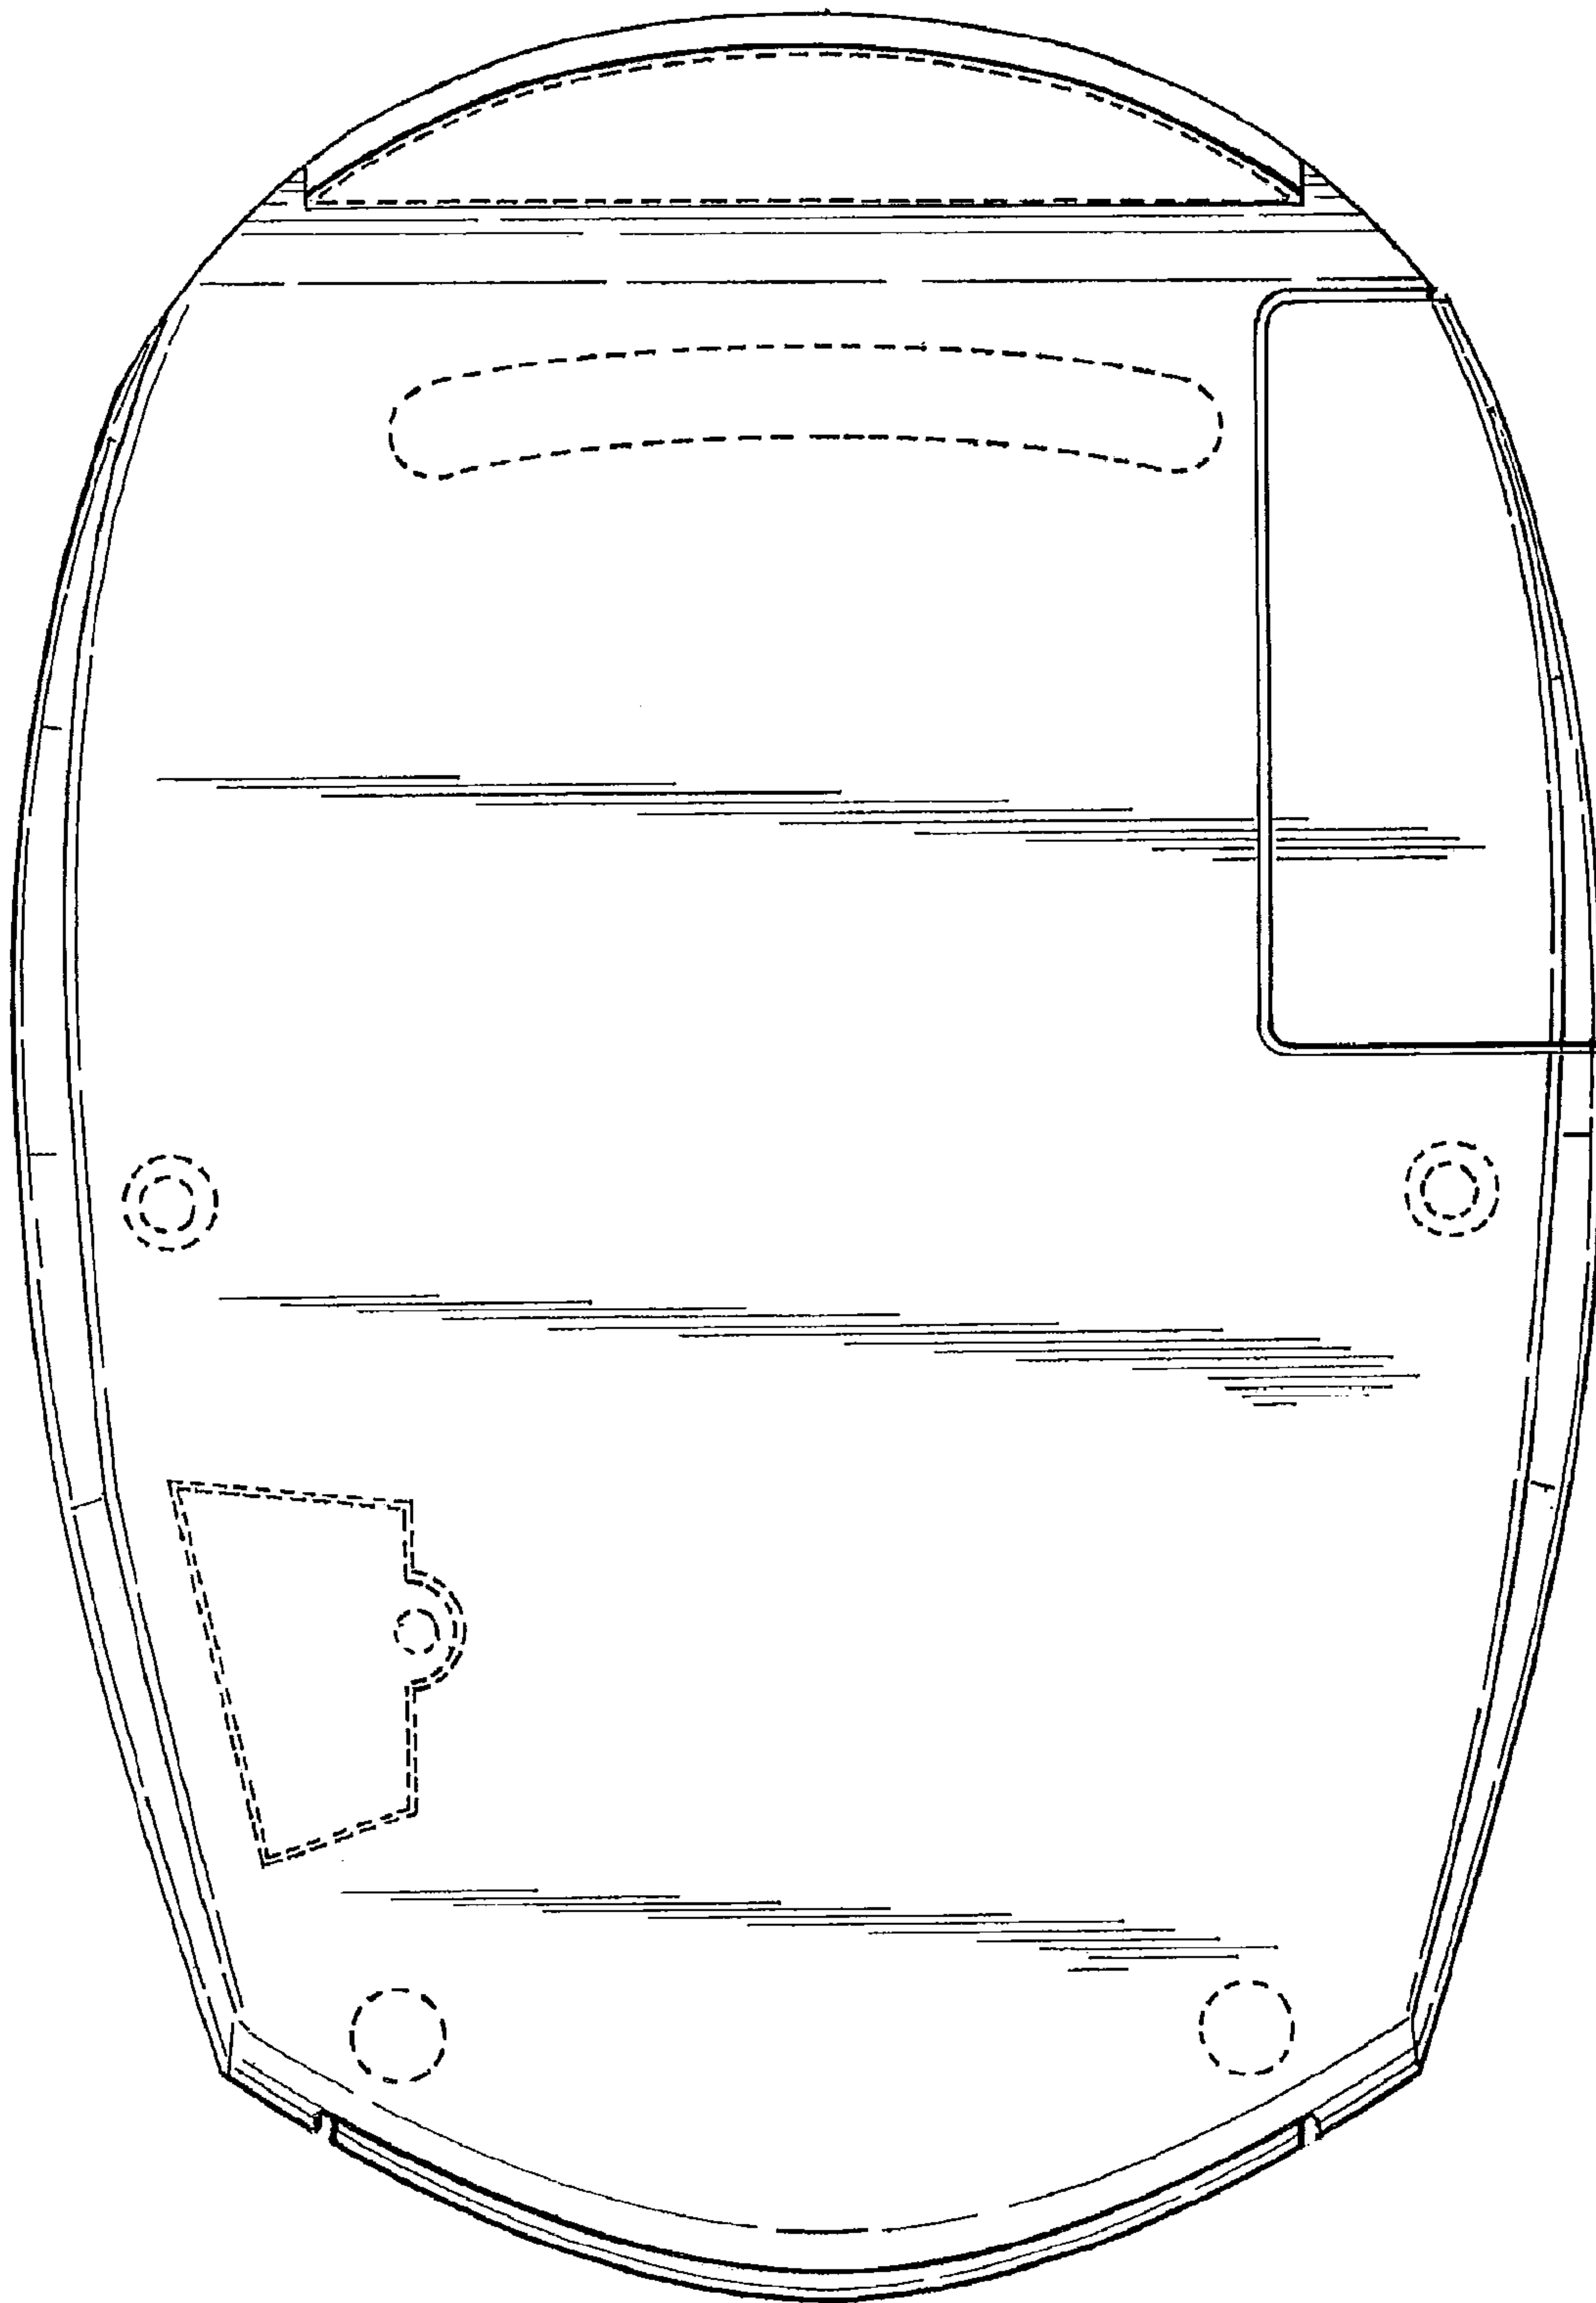


Fig. 7

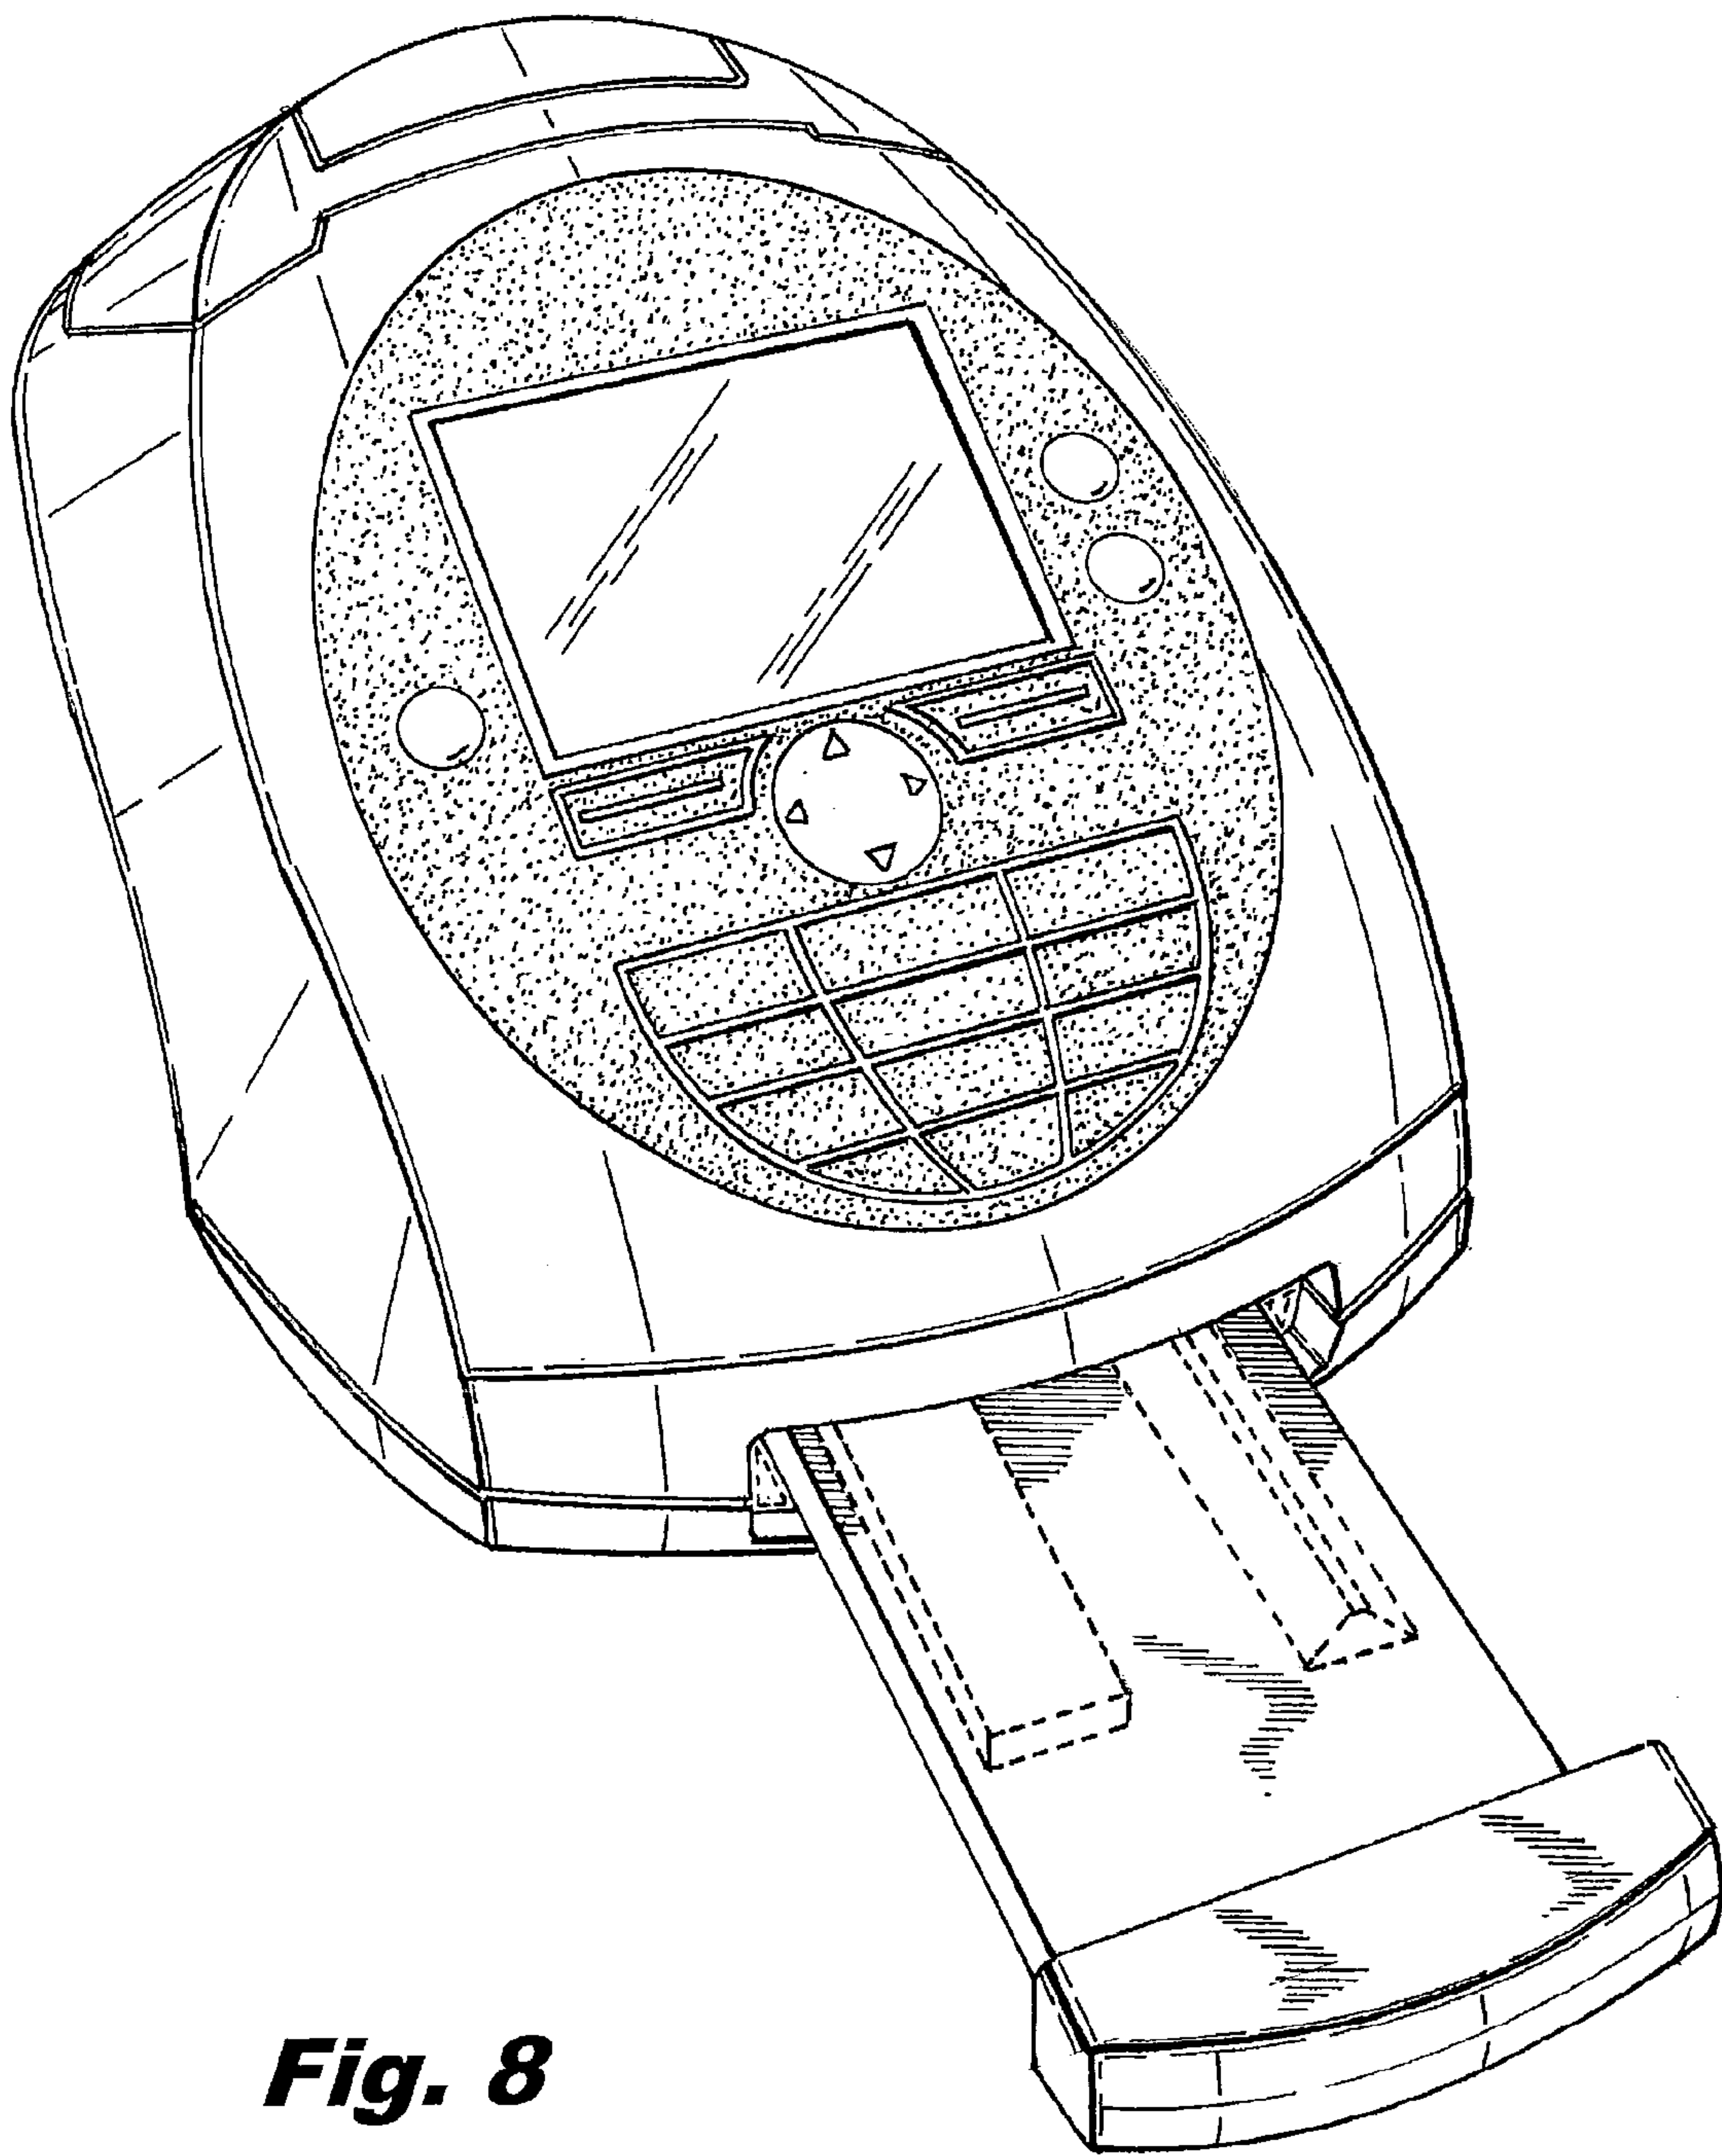


Fig. 8