



US00D651713S

(12) **United States Design Patent**  
**Shi**

(10) **Patent No.:** **US D651,713 S**  
(45) **Date of Patent:** **\*\* Jan. 3, 2012**

(54) **PRESSURE ACTIVATED SAFETY LANCET**

(75) Inventor: **Guoping Shi**, Suzhou (CN)

(73) Assignee: **Sterilance Medical (Suzhou) Inc.**,  
Suzhou (CN)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/391,976**

(22) Filed: **May 16, 2011**

(30) **Foreign Application Priority Data**

Nov. 16, 2010 (CN) ..... 2010 3 0615864

(51) **LOC (9) Cl.** ..... **26-02**

(52) **U.S. Cl.** ..... **D24/147**

(58) **Field of Classification Search** ..... D24/133,  
D24/130, 113, 114, 147, 146; 600/385, 600,  
600/573, 583, 167, 172, 181–185; 210/453  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D303,571 S \* 9/1989 Åkerfeldt ..... D24/147  
4,960,130 A \* 10/1990 Guirguis ..... 600/573  
D376,649 S \* 12/1996 Kim ..... D24/147

D412,985 S \* 8/1999 Weekes ..... D24/146  
6,537,292 B1 \* 3/2003 Lee ..... 606/182  
6,540,763 B2 \* 4/2003 Teo et al. .... 606/182  
D642,264 S \* 7/2011 Fisher et al. .... D24/146  
D645,147 S \* 9/2011 Ruf ..... D24/147  
D645,148 S \* 9/2011 Ruf ..... D24/147

\* cited by examiner

*Primary Examiner* — Ian Simmons

*Assistant Examiner* — Carissa C Fitts

(74) *Attorney, Agent, or Firm* — Oliff & Berridge, PLC


(57) **CLAIM**

The ornamental design for a pressure activated safety lancet,  
as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of a pressure activated safety lancet;  
FIG. 2 is a front view thereof, the rear view being a mirror image of the front view;  
FIG. 3 is a right-side view thereof, the left-side view being a mirror image of the right-side view;  
FIG. 4 is a top view thereof; and,  
FIG. 5 is a bottom view thereof.  
Claim

**1 Claim, 3 Drawing Sheets**

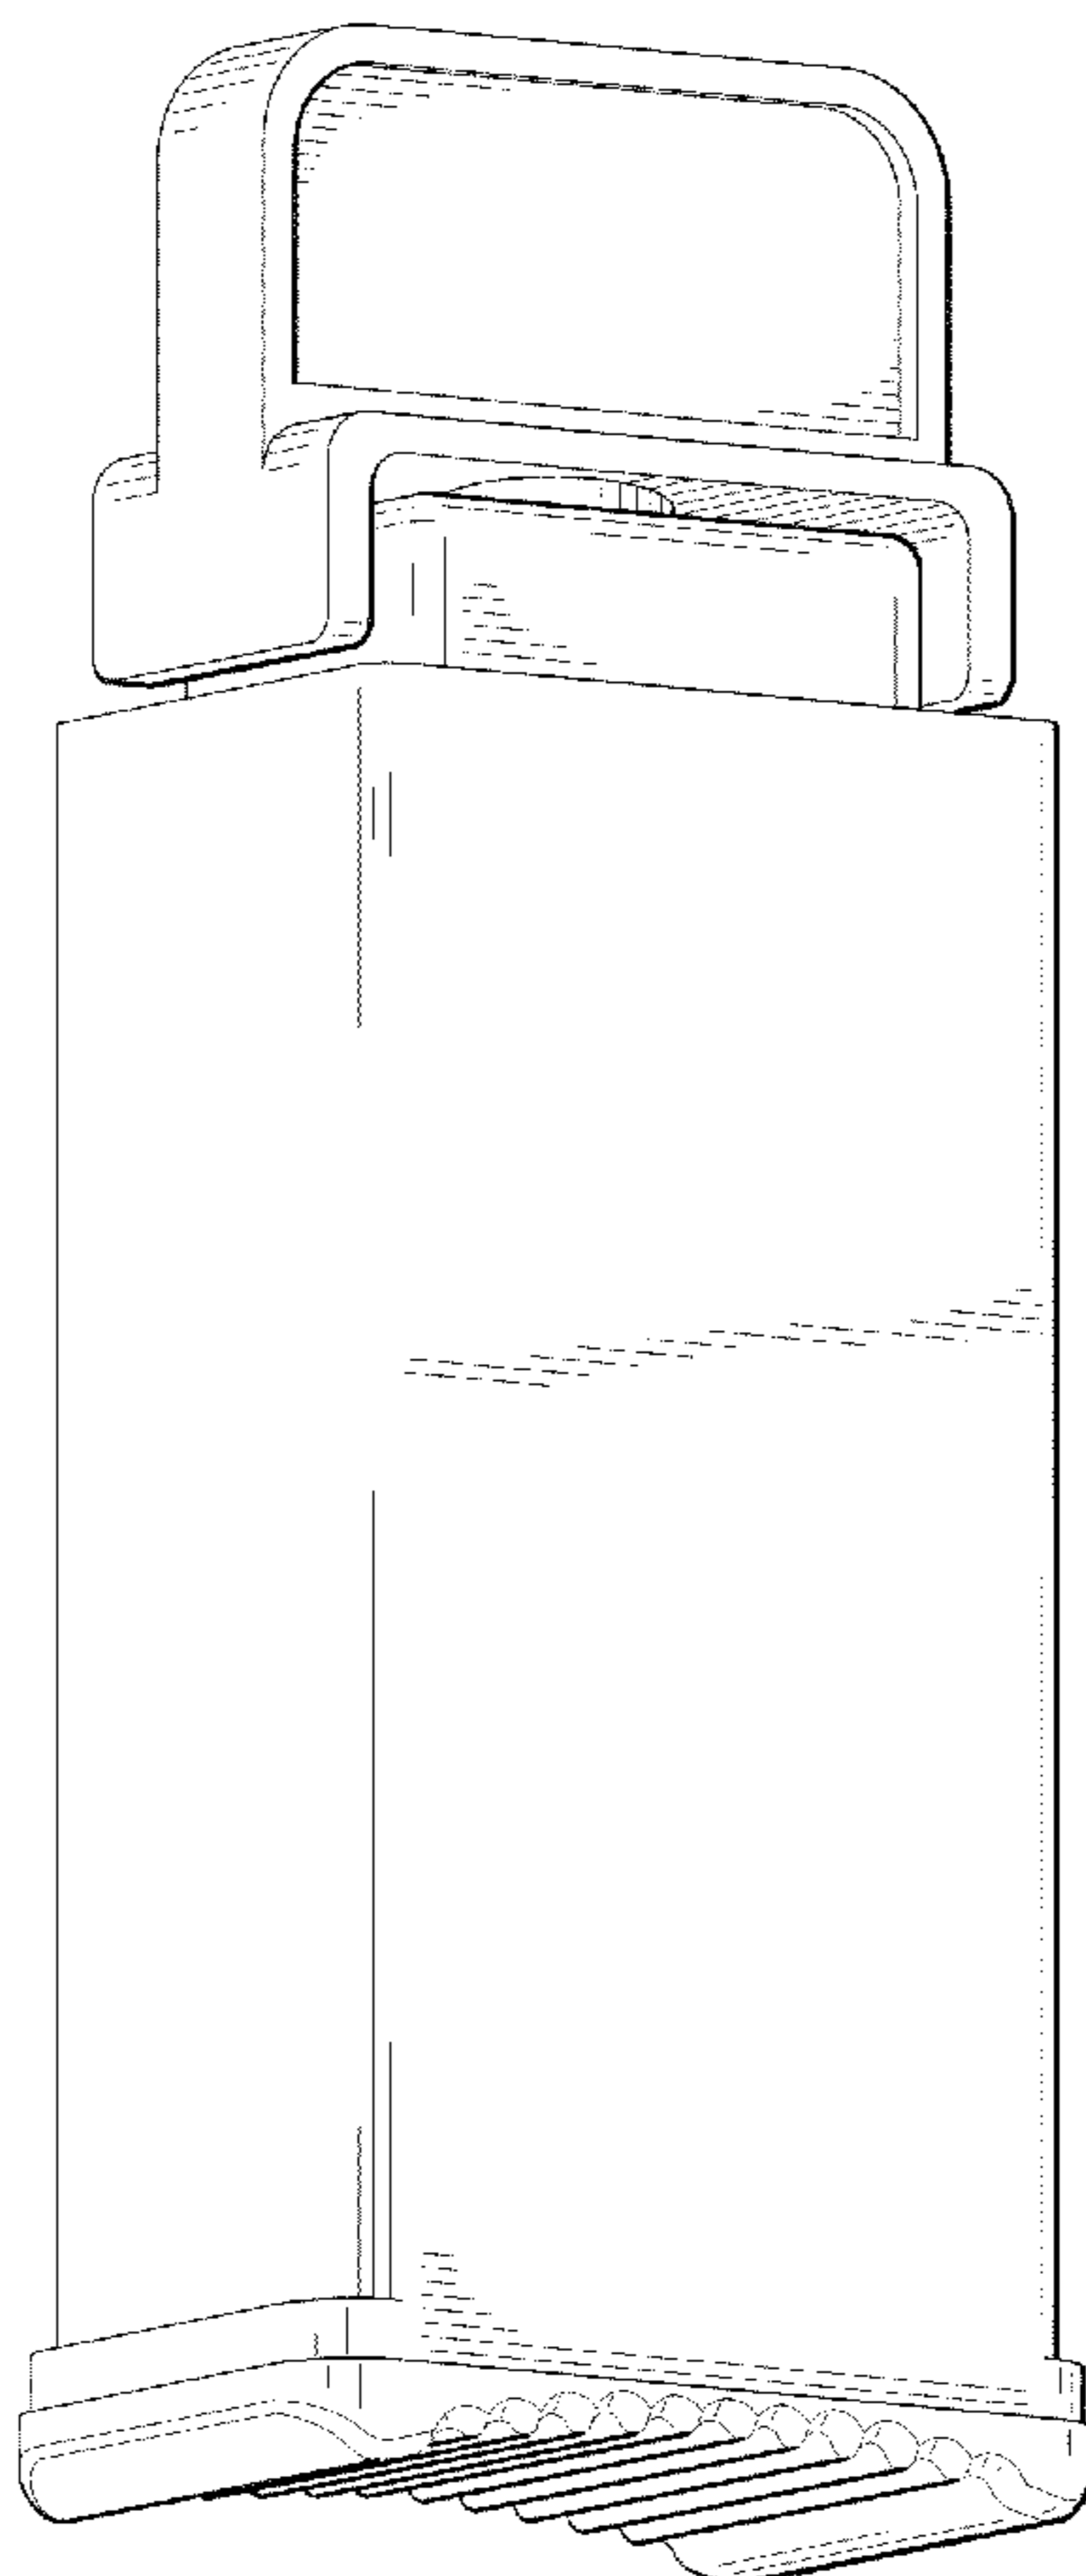

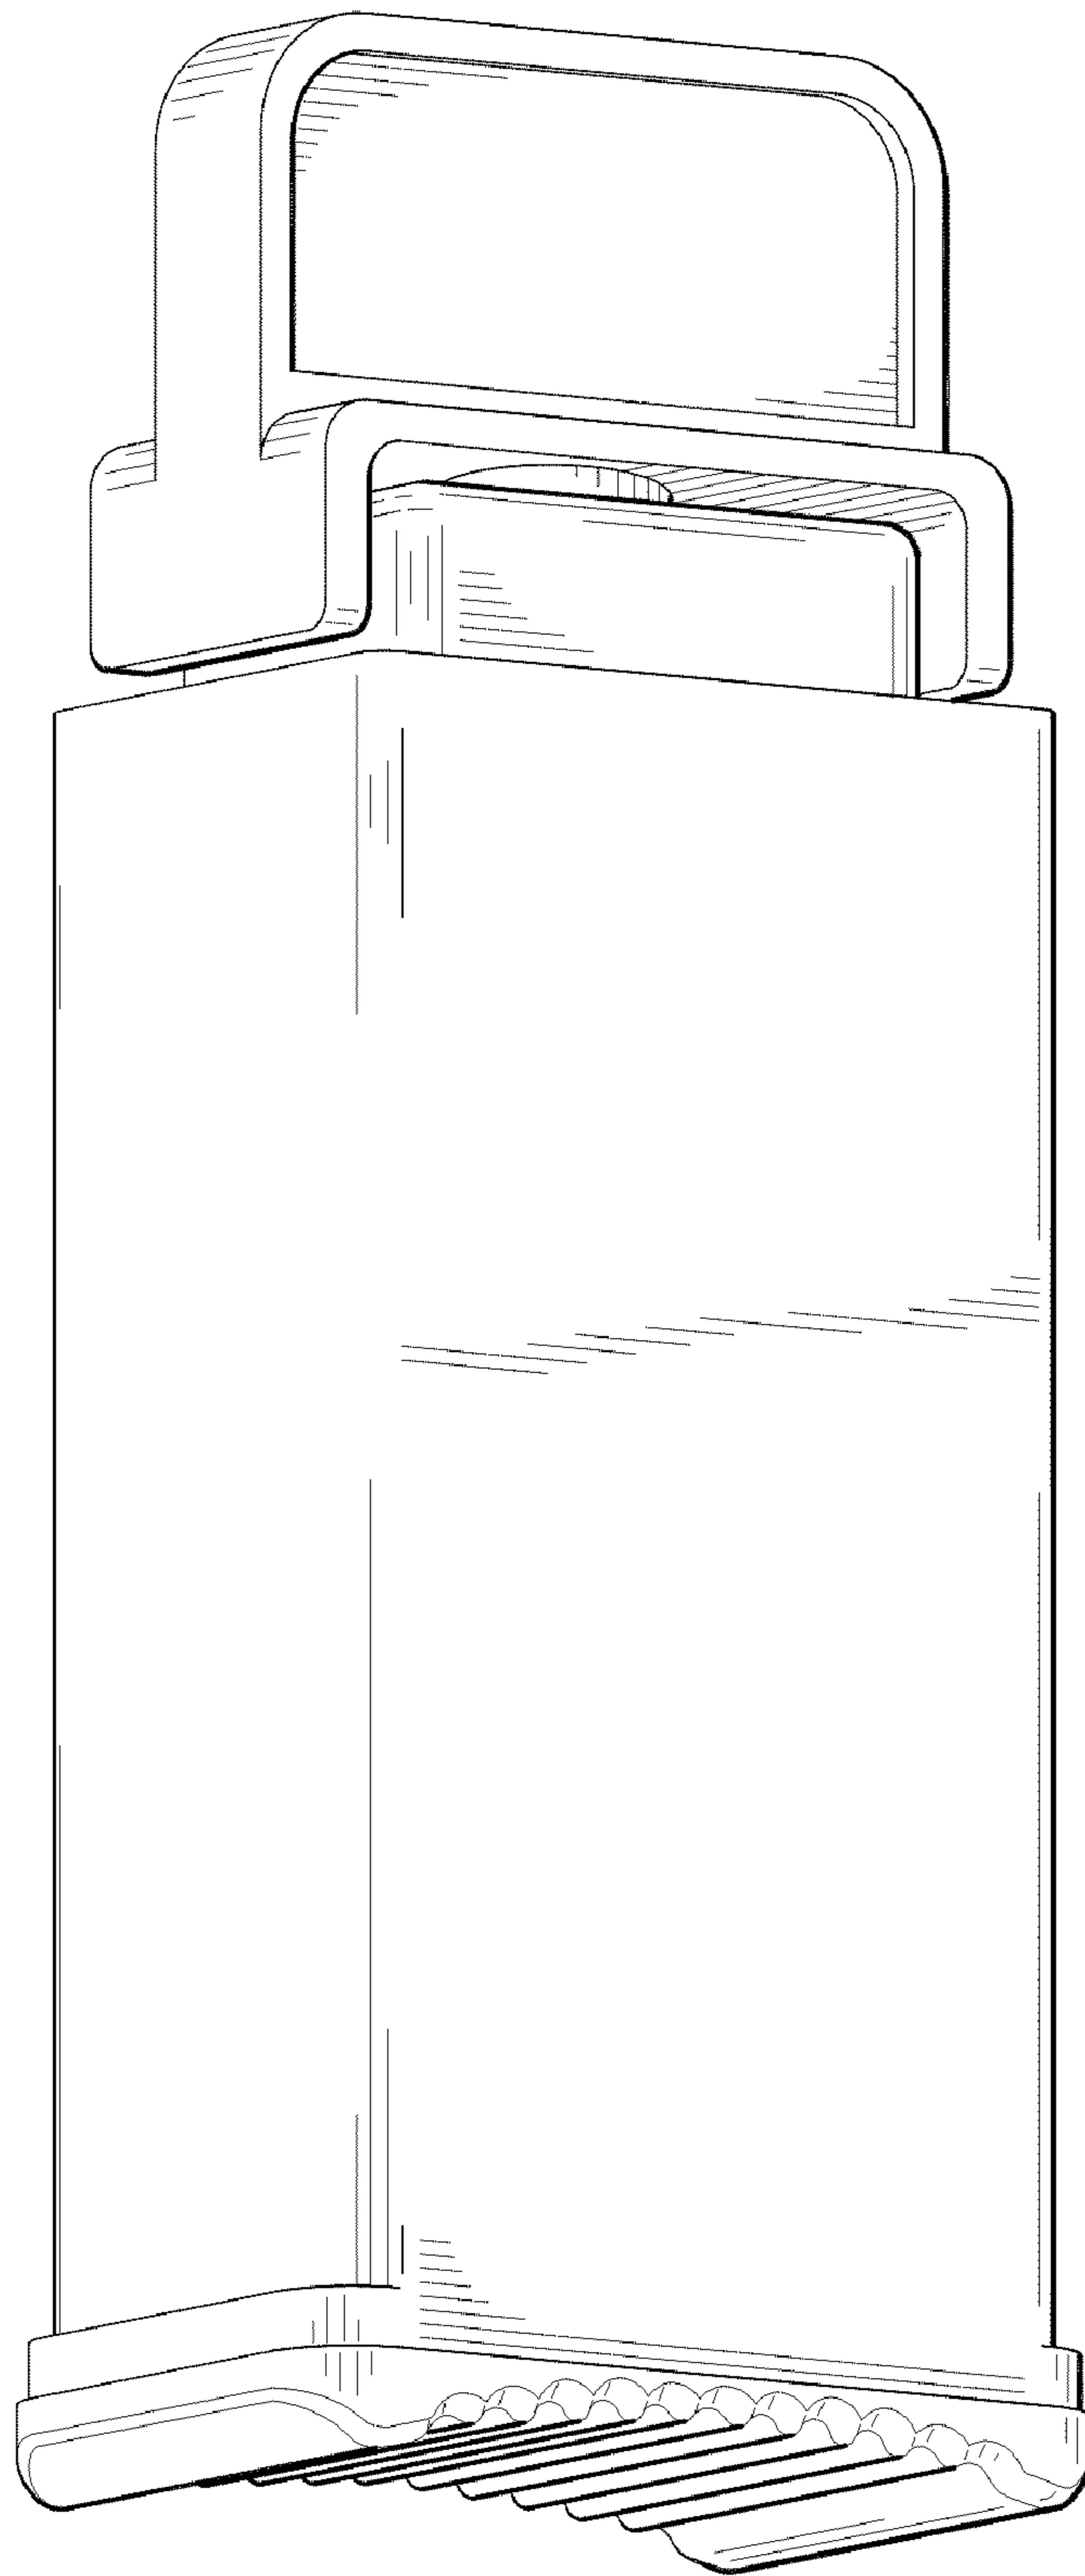


FIG. 1

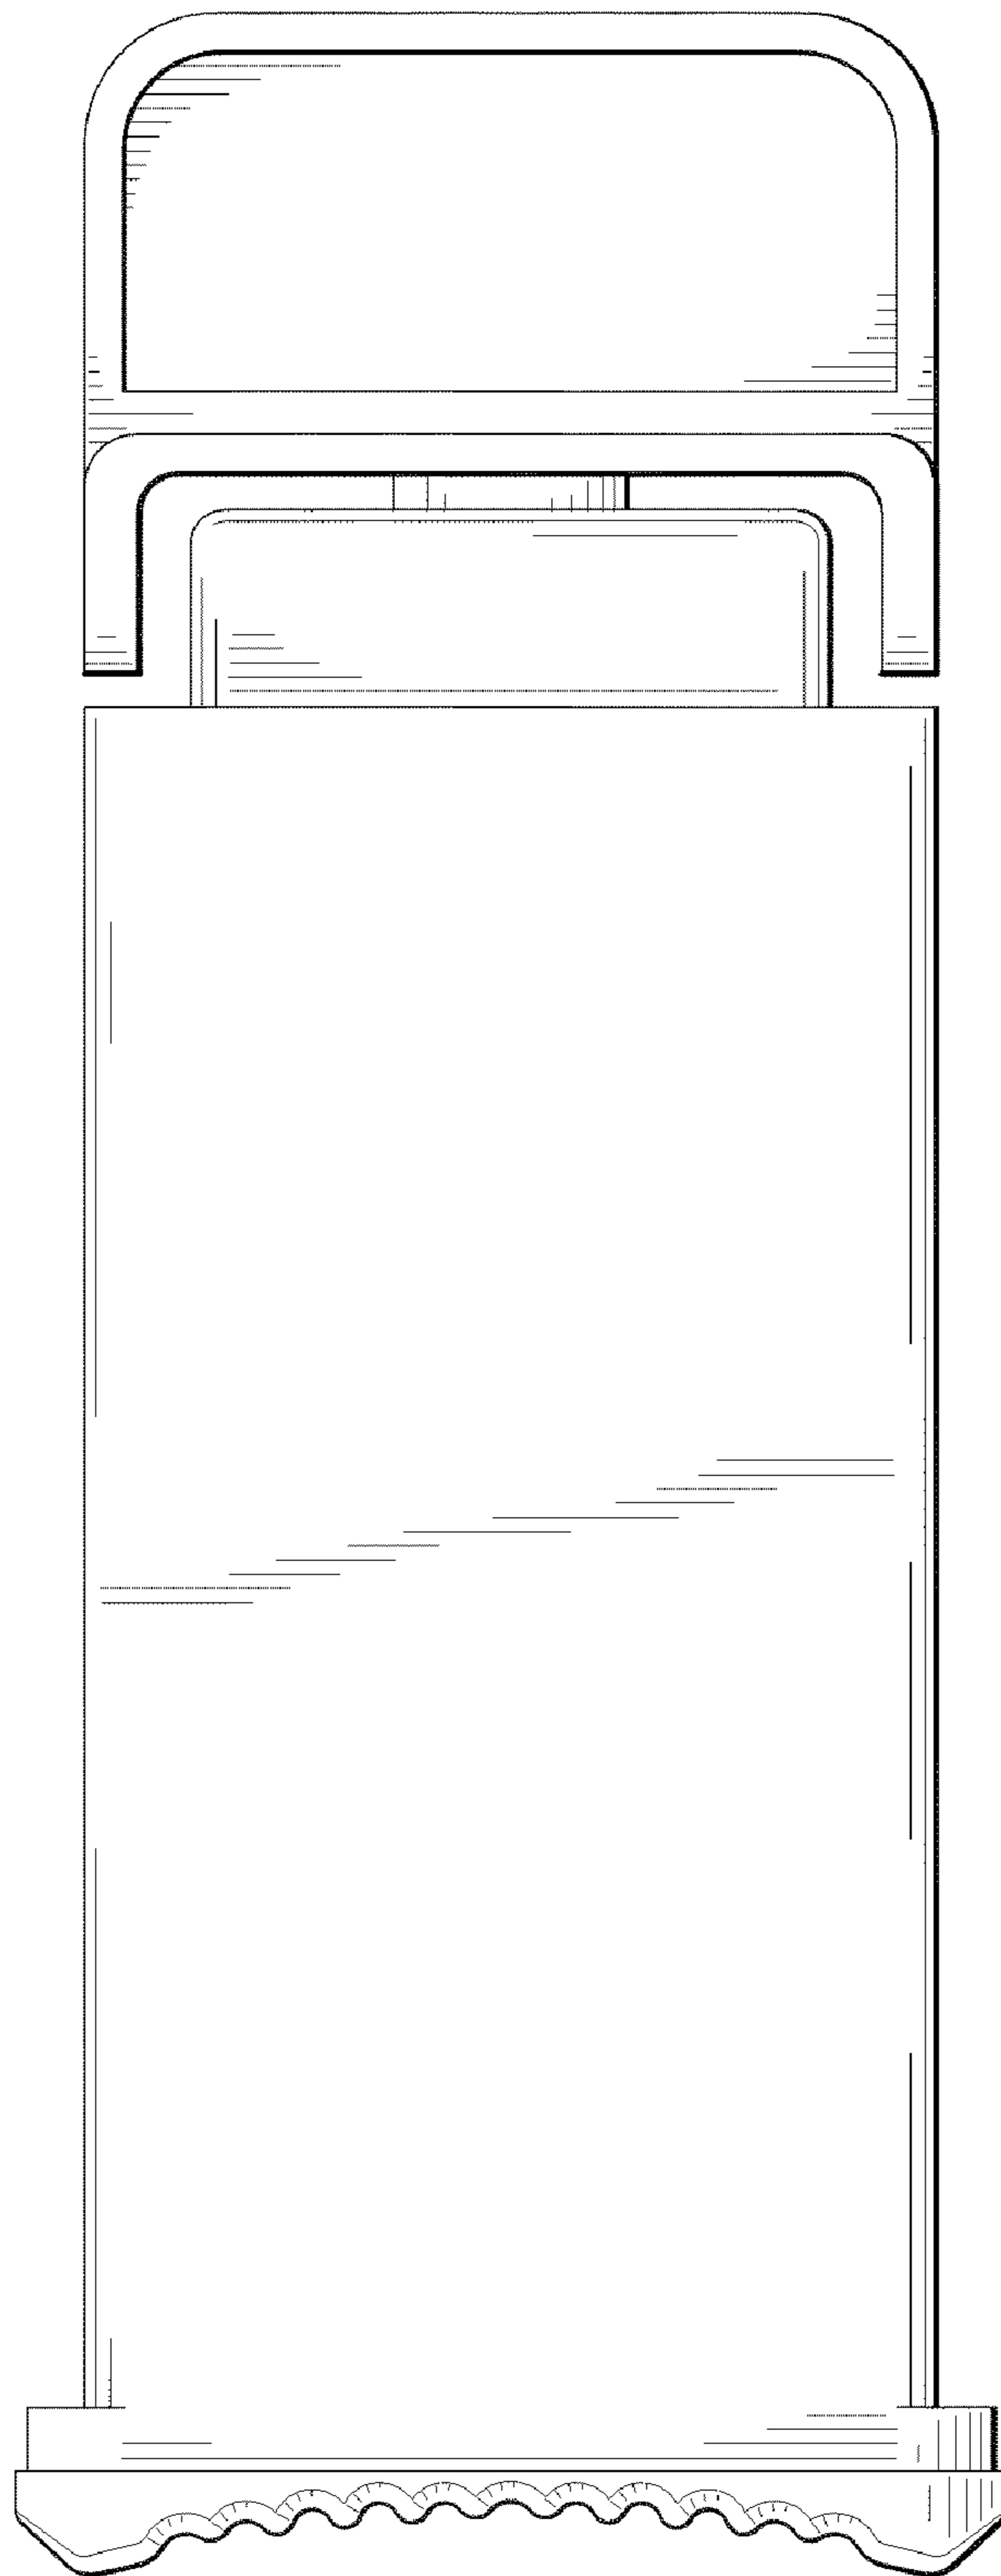


FIG. 2

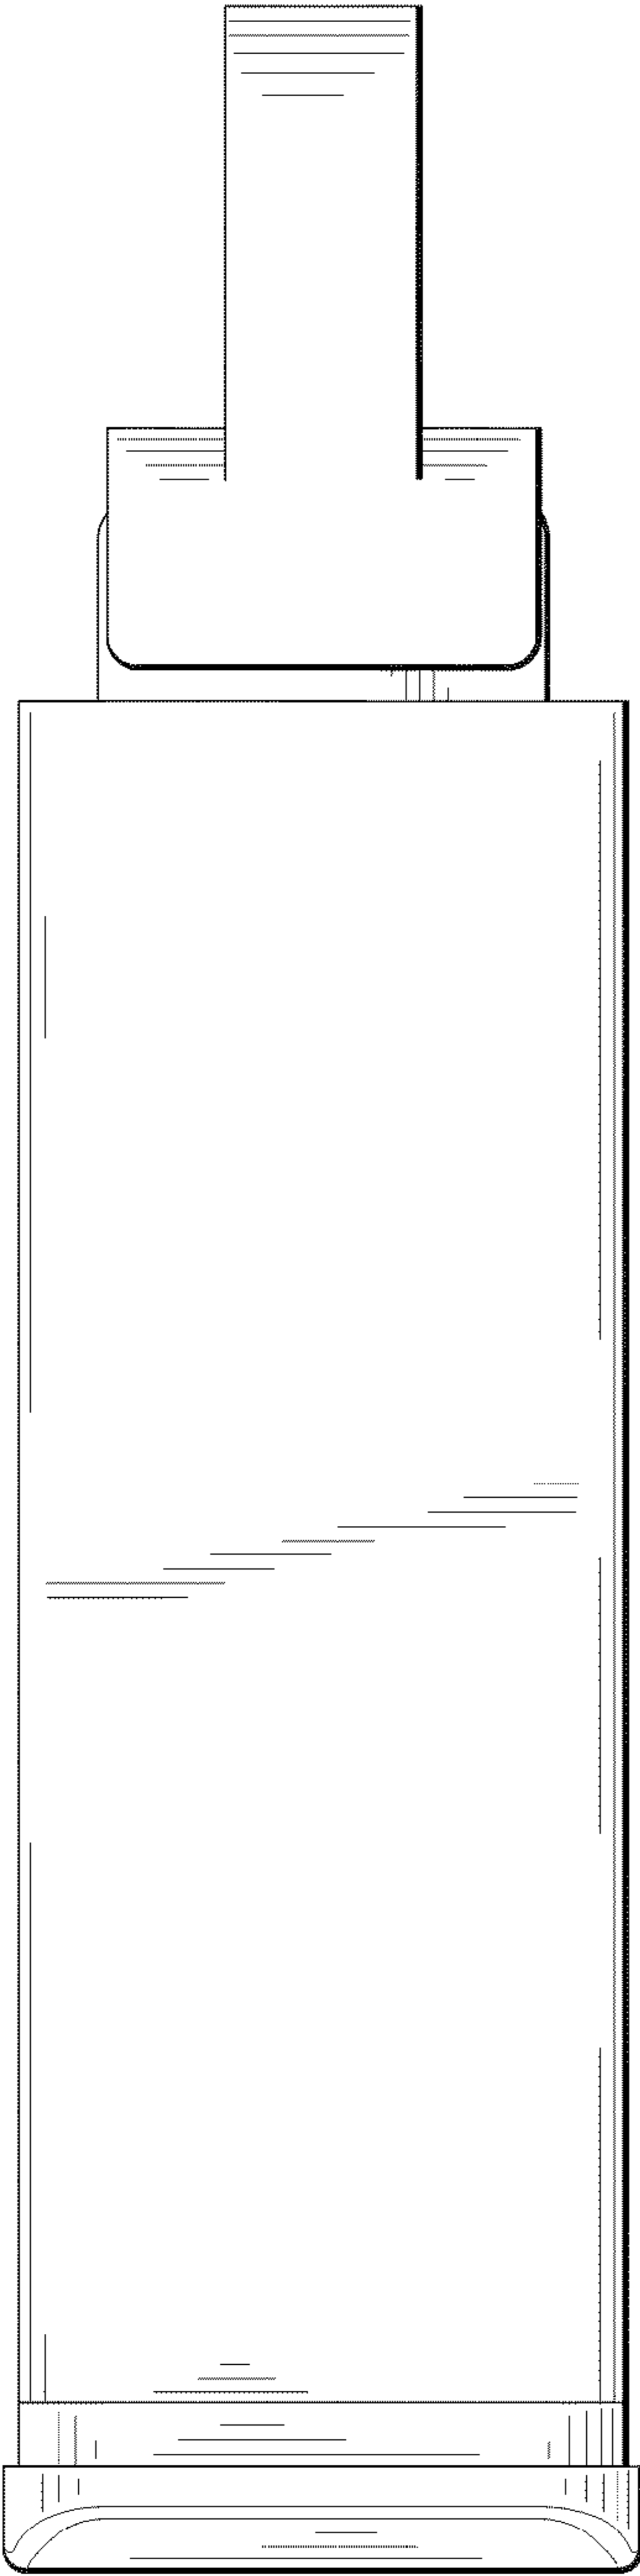


FIG. 3

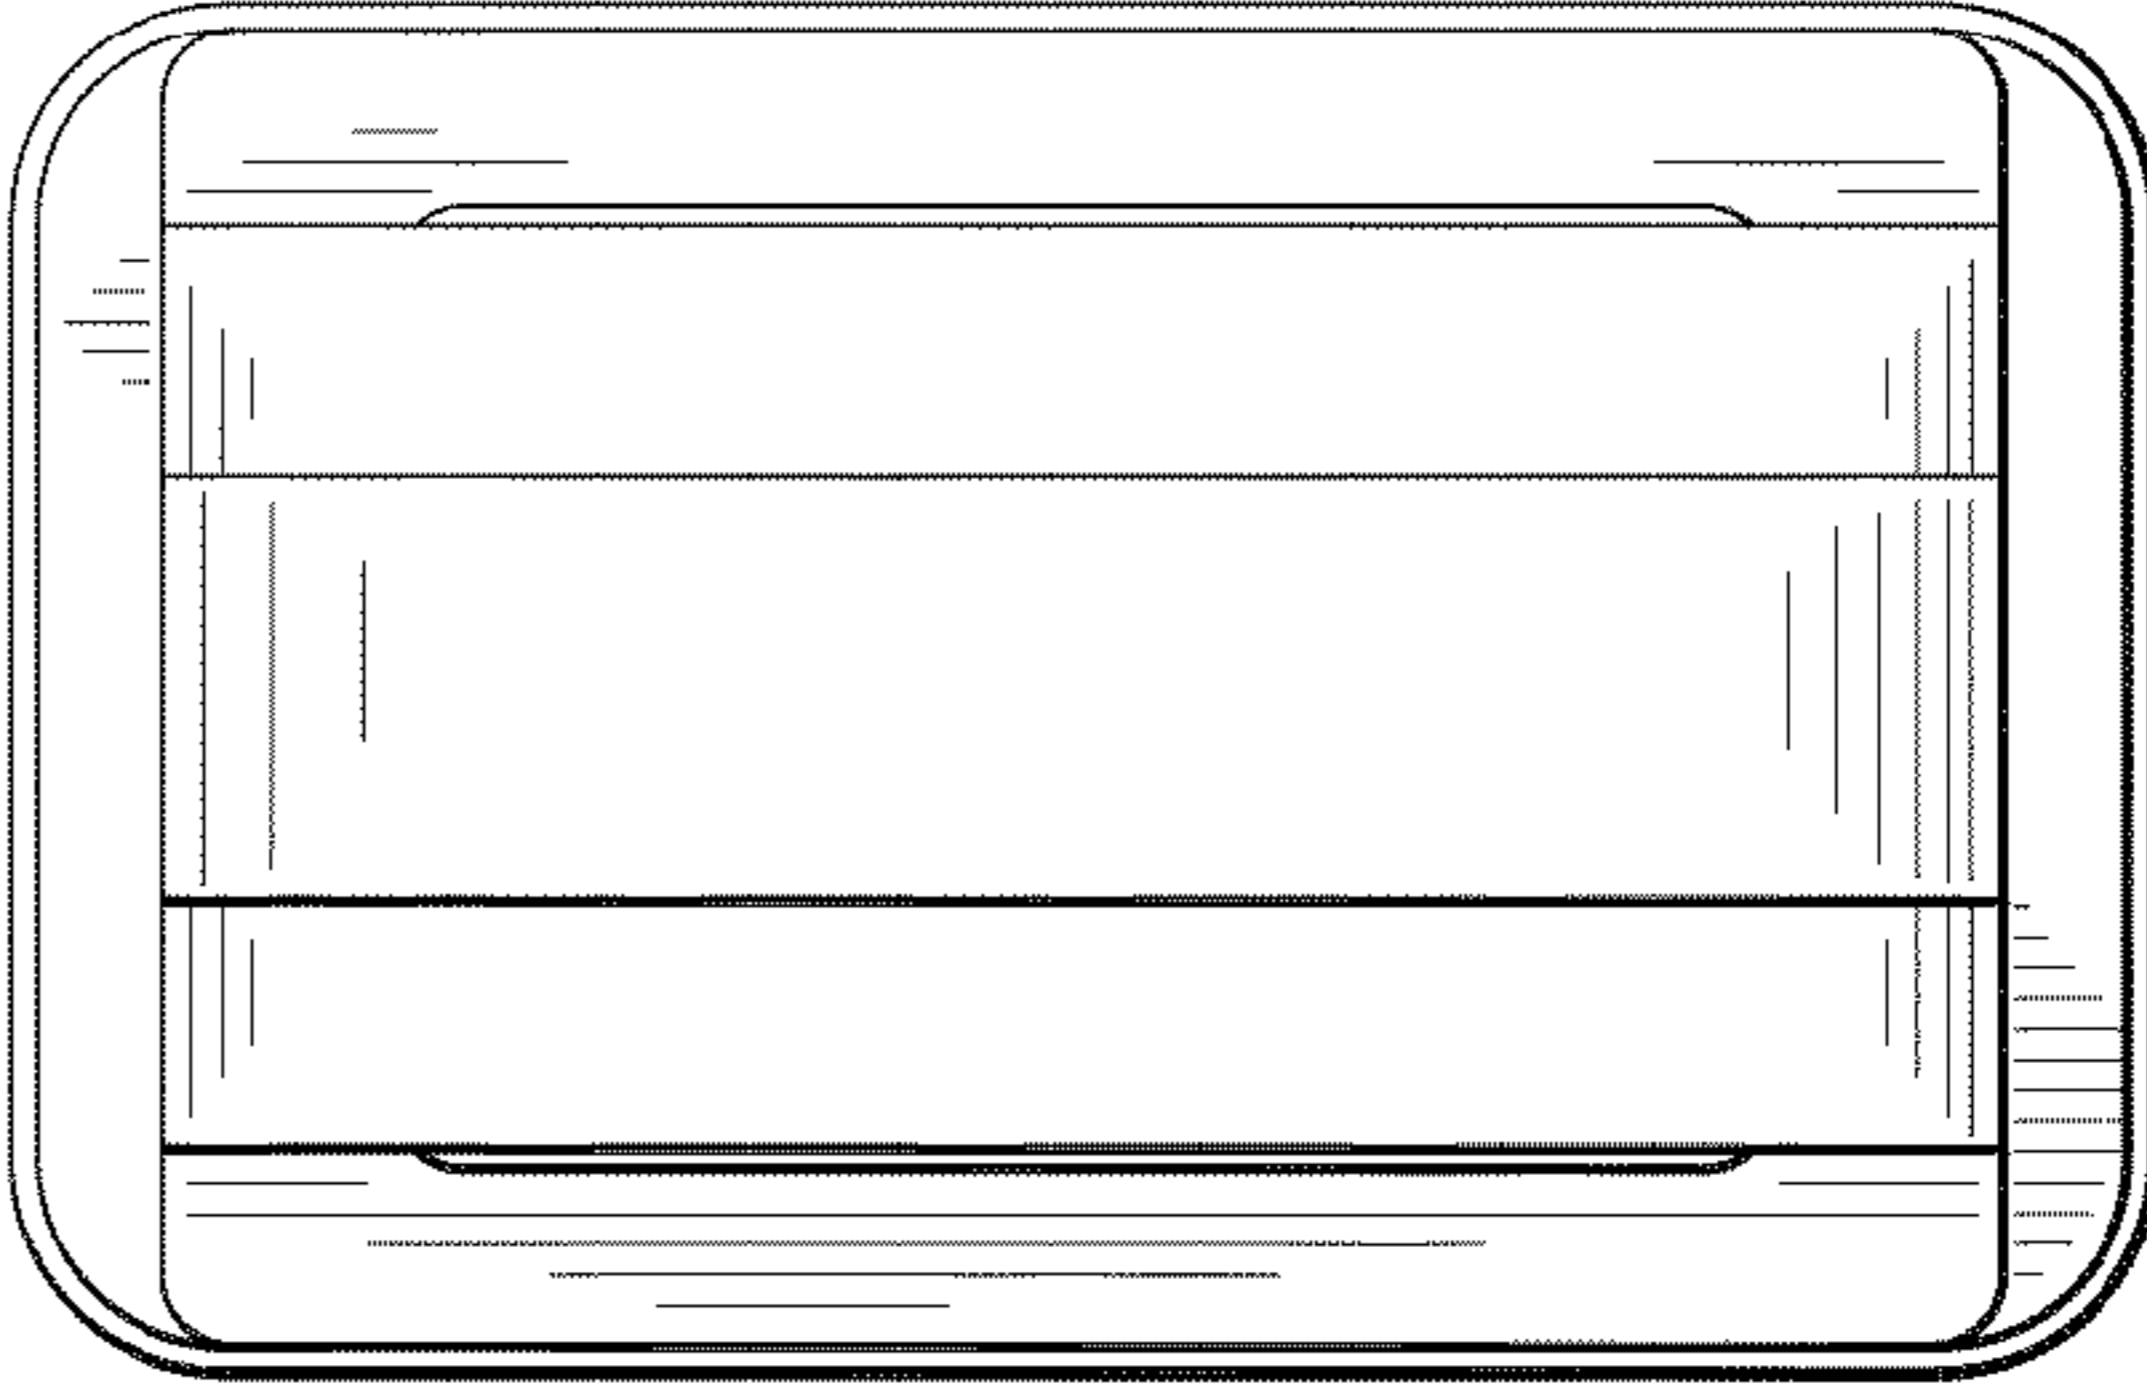


FIG. 4

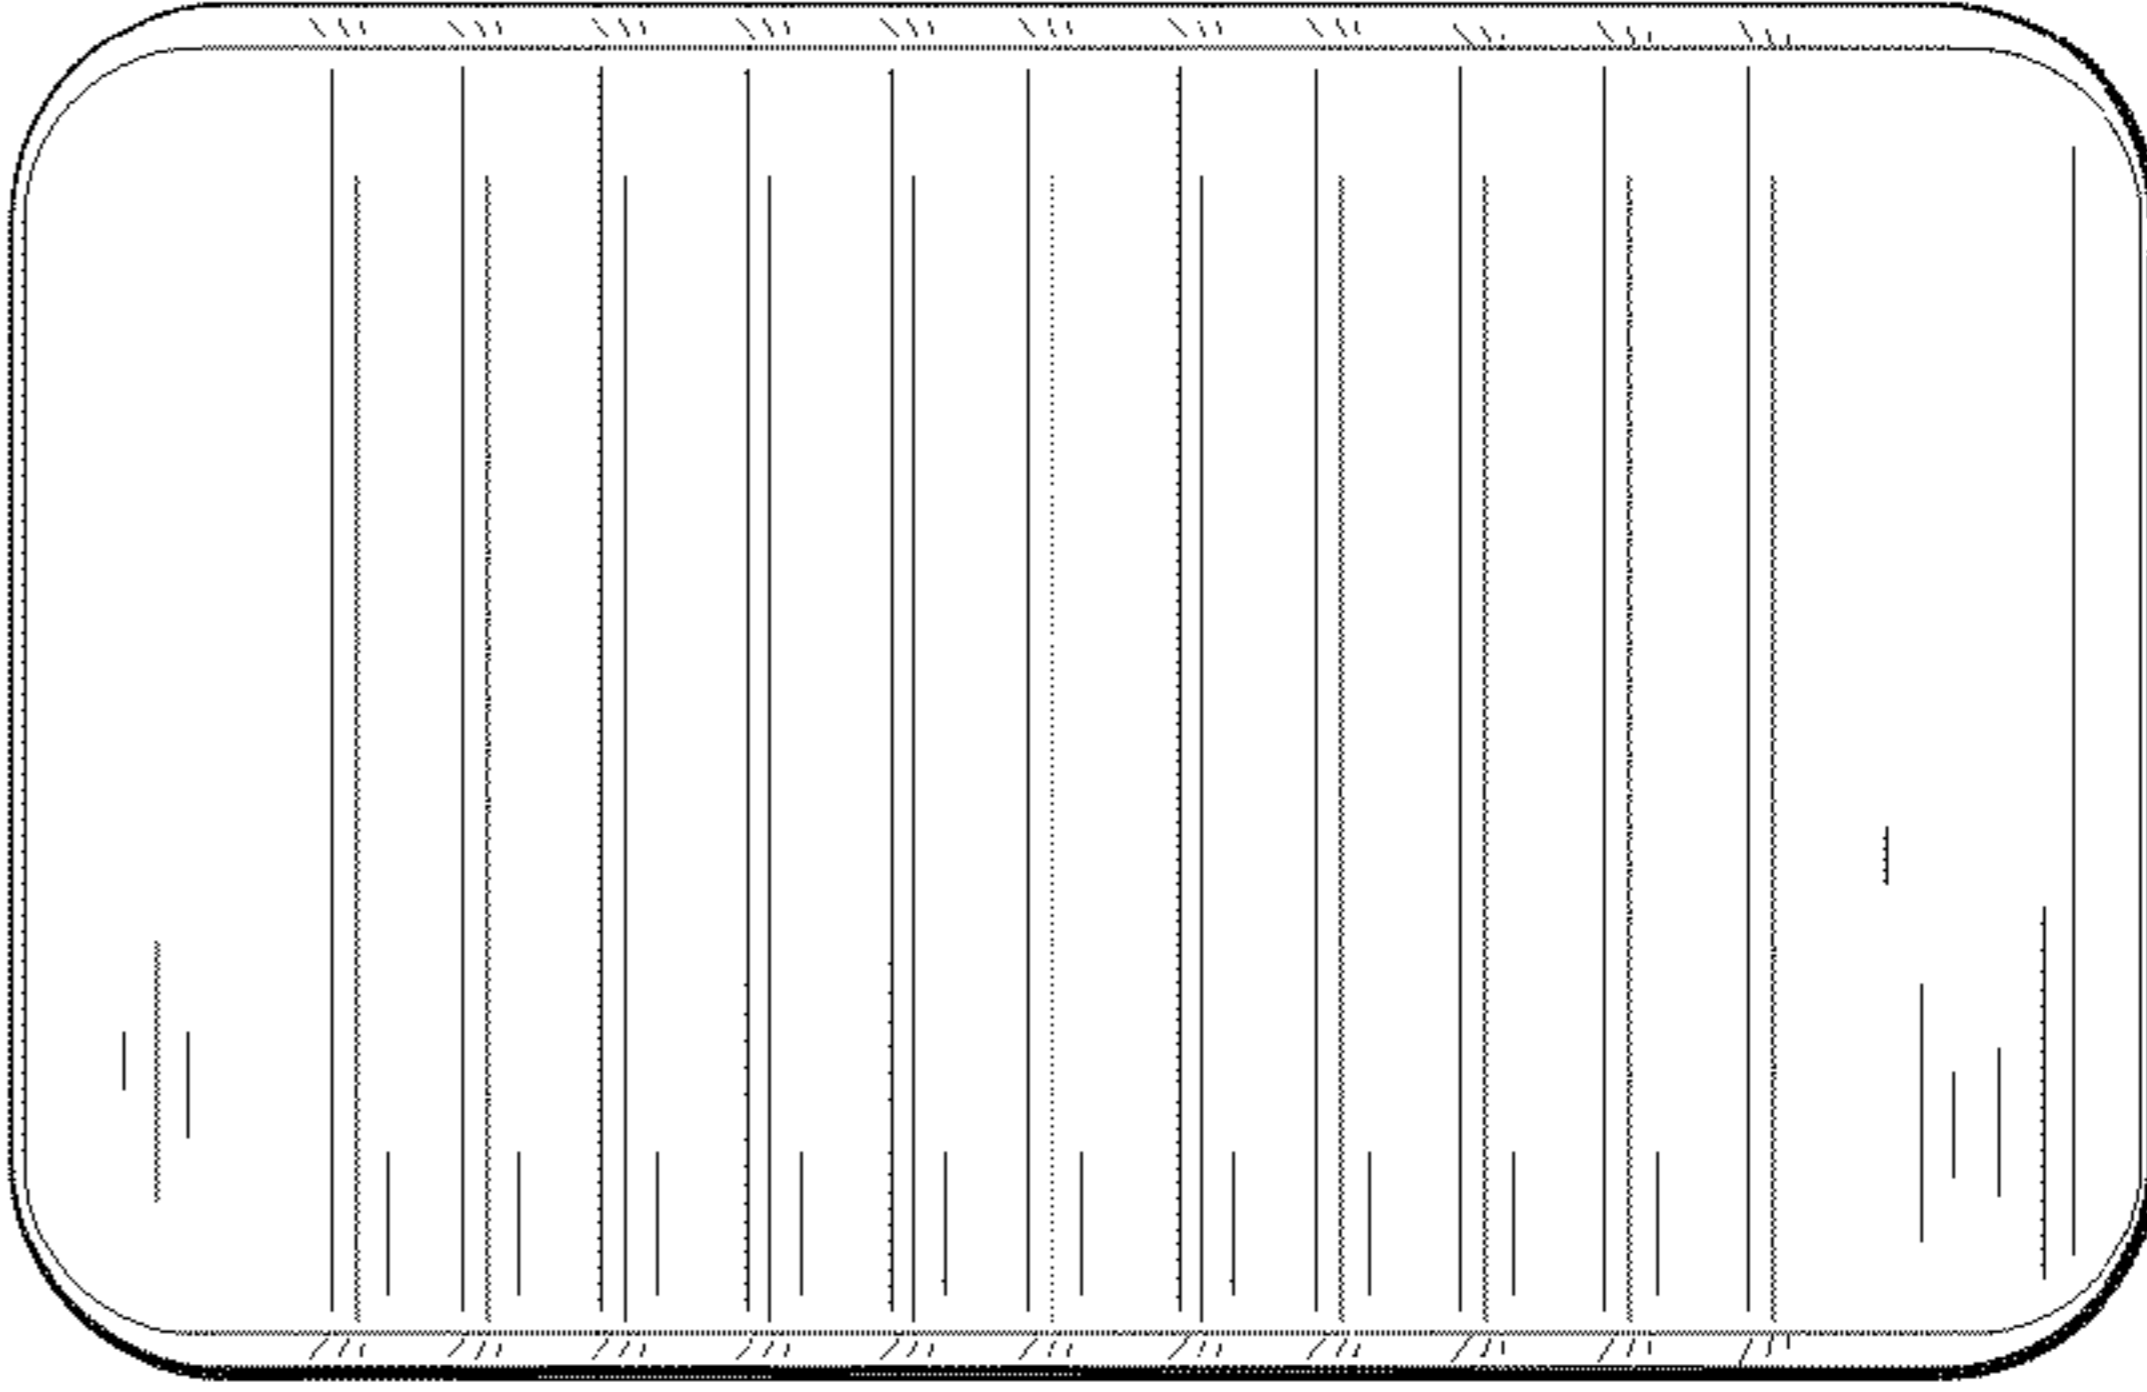


FIG. 5