



US00D651713S

(12) **United States Design Patent**
Shi

(10) **Patent No.:** **US D651,713 S**
(45) **Date of Patent:** **** Jan. 3, 2012**

(54) **PRESSURE ACTIVATED SAFETY LANCET**

(75) Inventor: **Guoping Shi**, Suzhou (CN)

(73) Assignee: **Sterilance Medical (Suzhou) Inc.**,
Suzhou (CN)

(**) Term: **14 Years**

(21) Appl. No.: **29/391,976**

(22) Filed: **May 16, 2011**

(30) **Foreign Application Priority Data**

Nov. 16, 2010 (CN) 2010 3 0615864

(51) **LOC (9) Cl.** **26-02**

(52) **U.S. Cl.** **D24/147**

(58) **Field of Classification Search** D24/133,
D24/130, 113, 114, 147, 146; 600/385, 600,
600/573, 583, 167, 172, 181-185; 210/453
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D303,571 S * 9/1989 Åkerfeldt D24/147
4,960,130 A * 10/1990 Guirguis 600/573
D376,649 S * 12/1996 Kim D24/147

D412,985 S * 8/1999 Weekes D24/146
6,537,292 B1 * 3/2003 Lee 606/182
6,540,763 B2 * 4/2003 Teo et al. 606/182
D642,264 S * 7/2011 Fisher et al. D24/146
D645,147 S * 9/2011 Ruf D24/147
D645,148 S * 9/2011 Ruf D24/147

* cited by examiner

Primary Examiner — Ian Simmons

Assistant Examiner — Carissa C Fitts

(74) *Attorney, Agent, or Firm* — Oliff & Berridge, PLC


(57) **CLAIM**

The ornamental design for a pressure activated safety lancet,
as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a pressure activated safety lancet;
FIG. 2 is a front view thereof, the rear view being a mirror image of the front view;
FIG. 3 is a right-side view thereof, the left-side view being a mirror image of the right-side view;
FIG. 4 is a top view thereof; and,
FIG. 5 is a bottom view thereof.
Claim

1 Claim, 3 Drawing Sheets

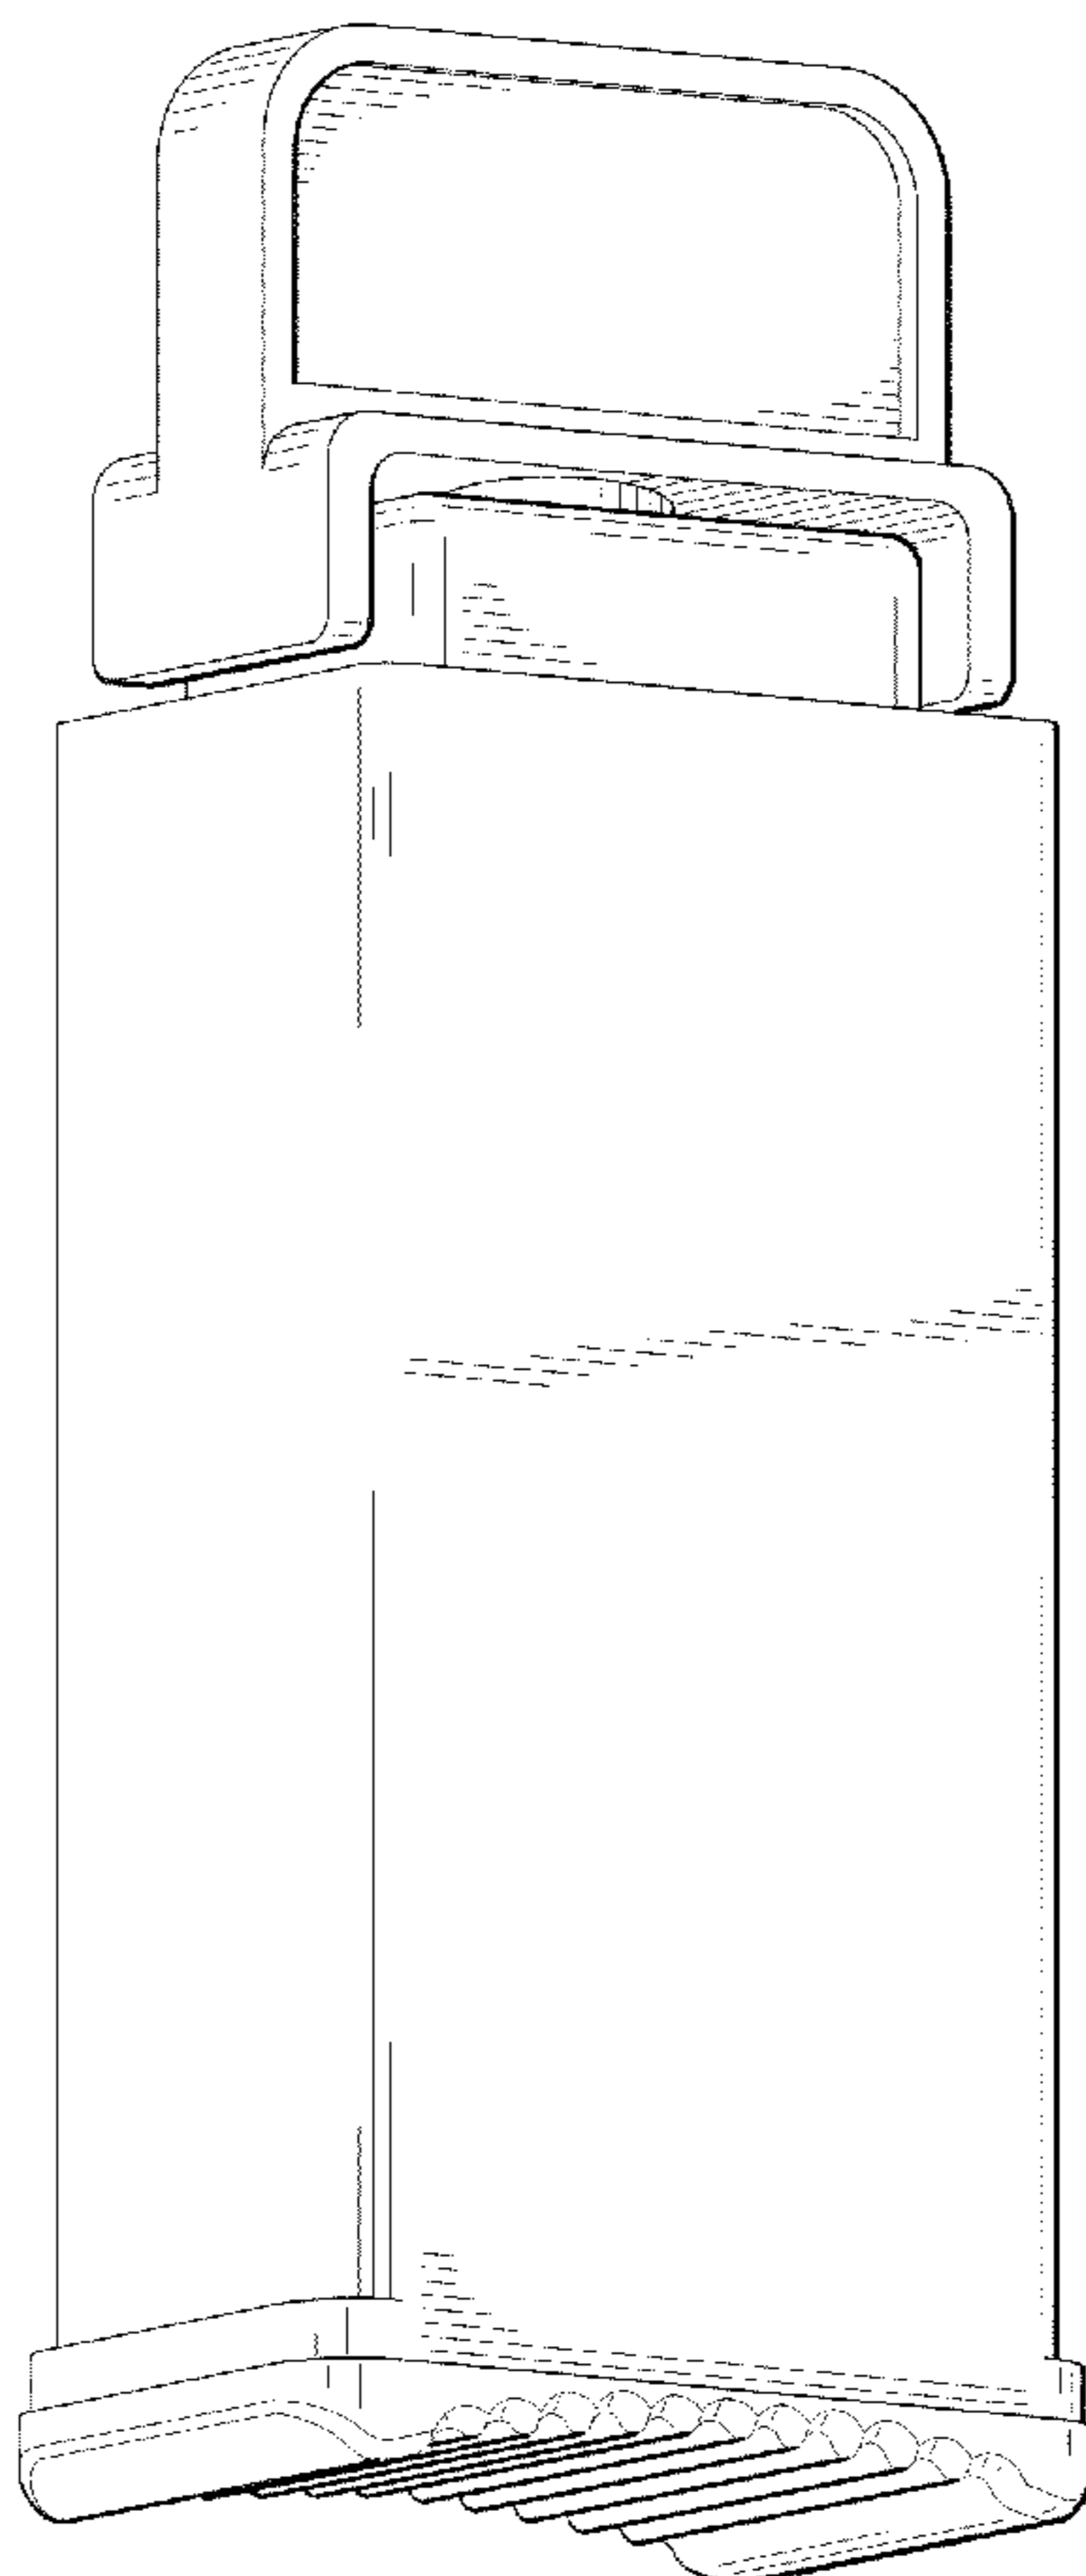

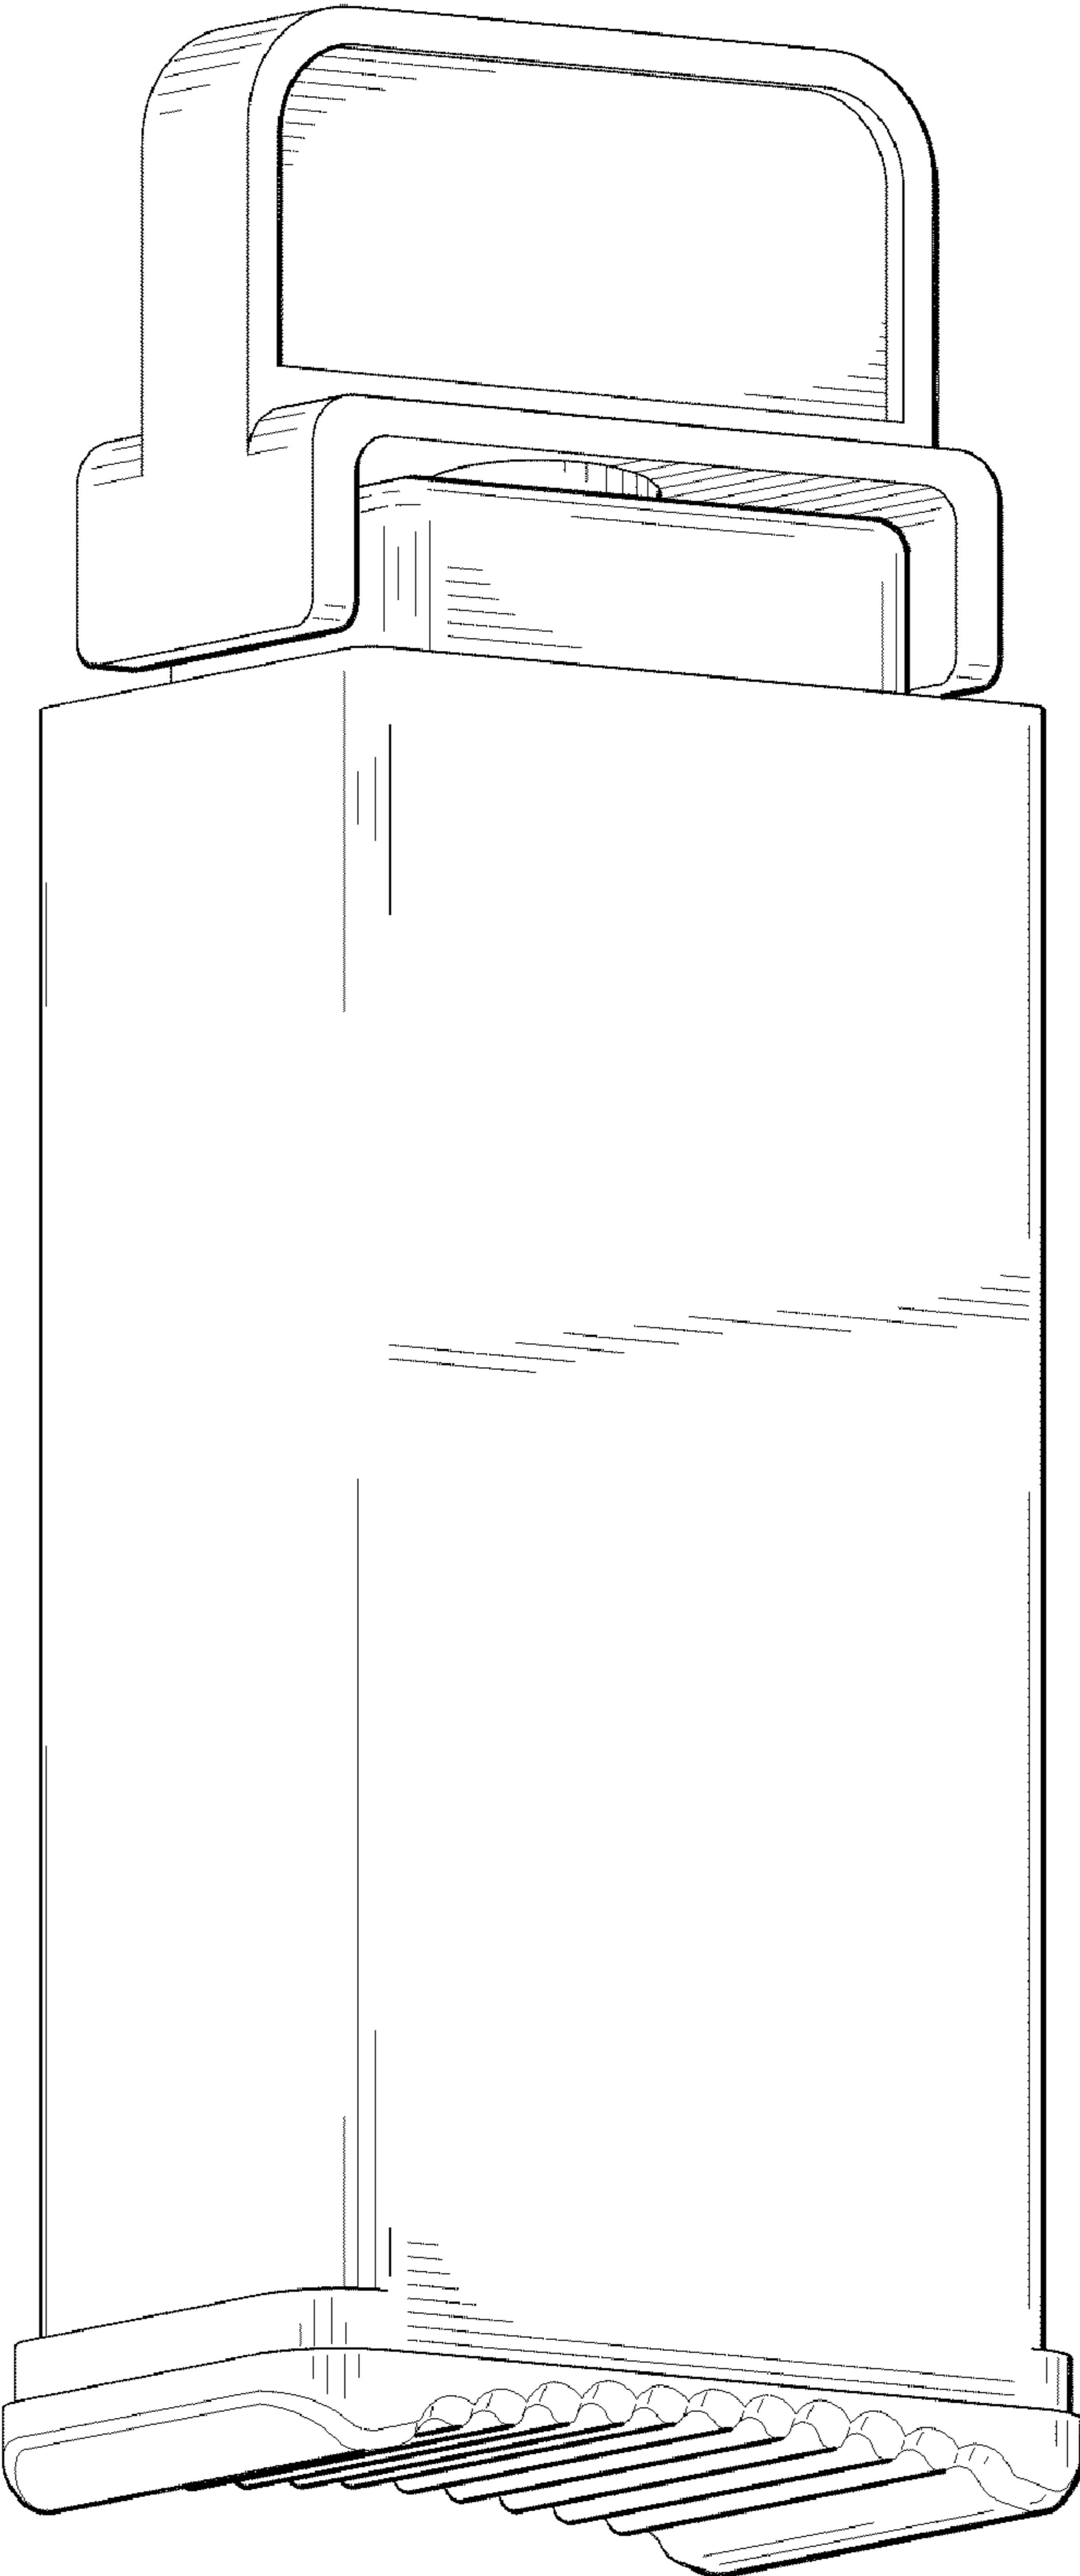


FIG. 1

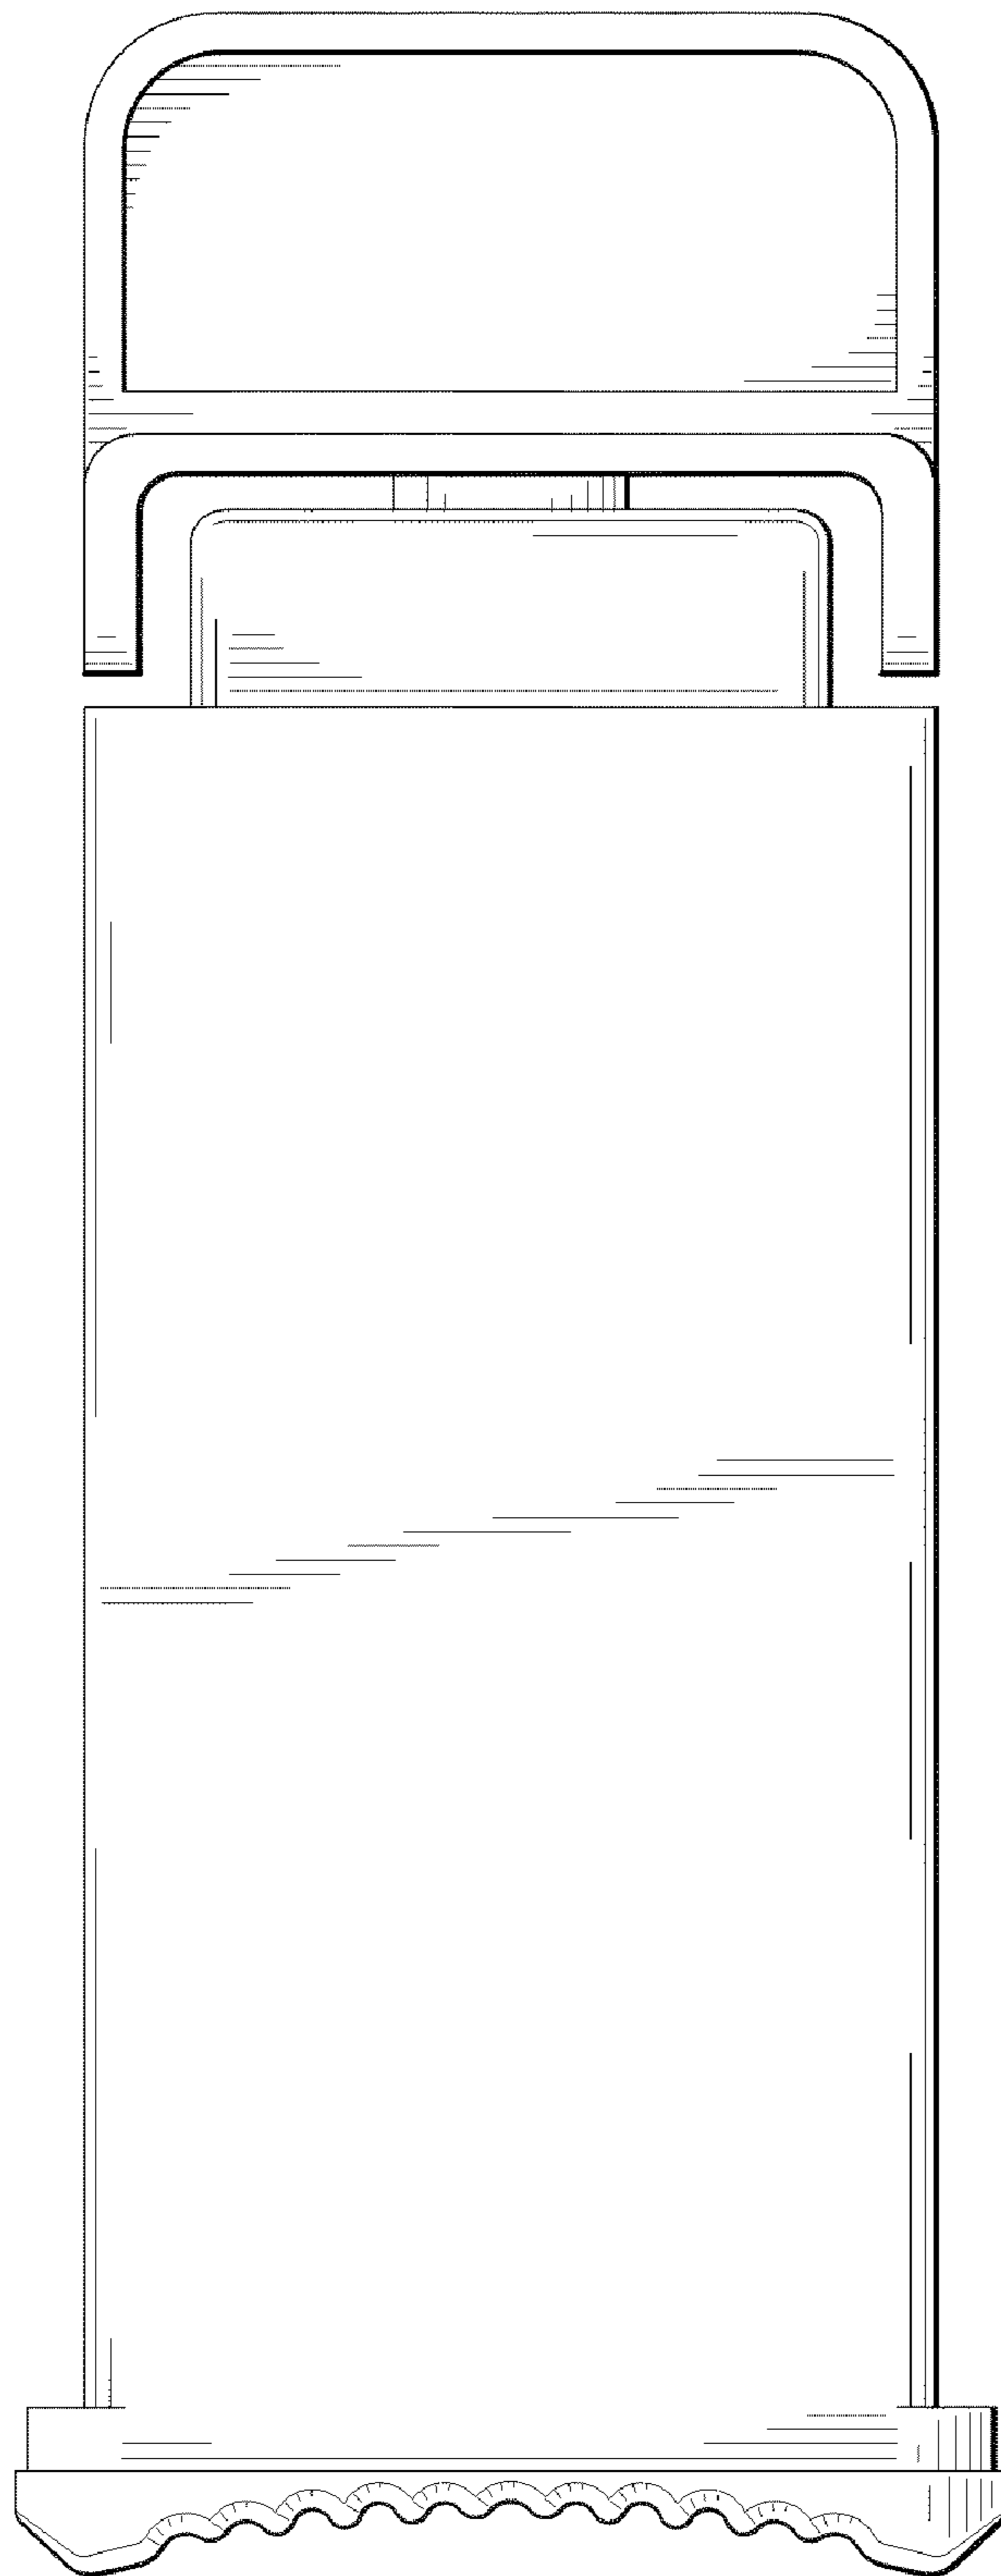


FIG. 2

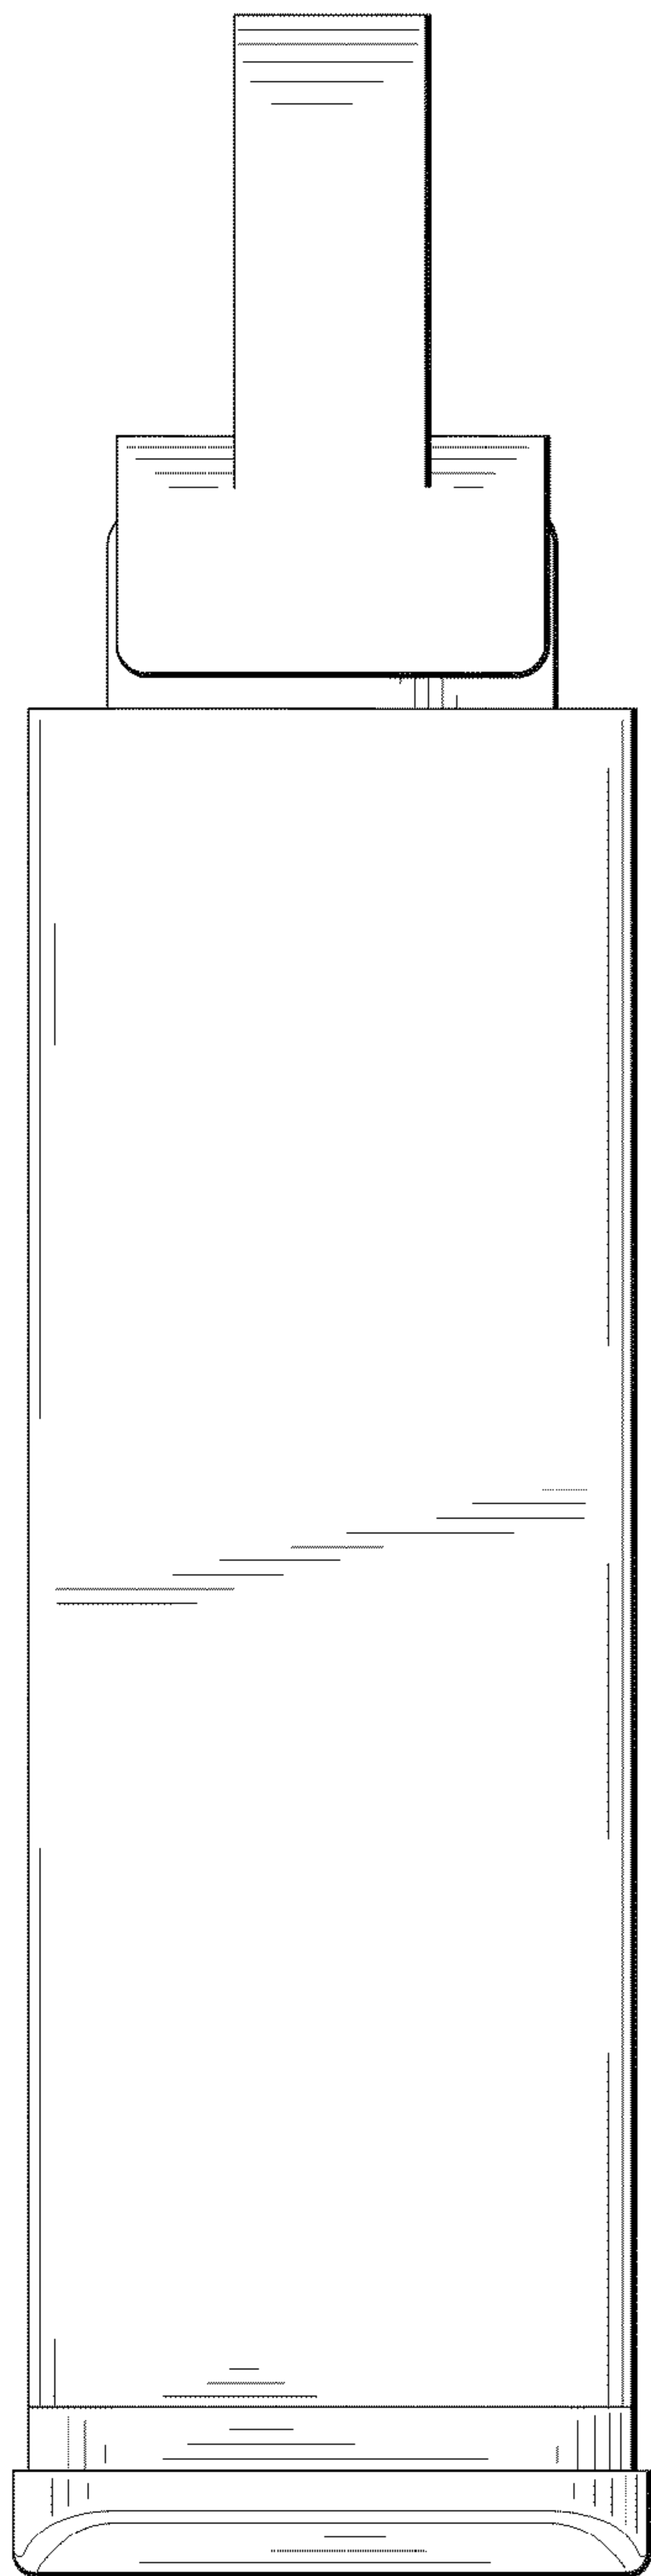


FIG. 3

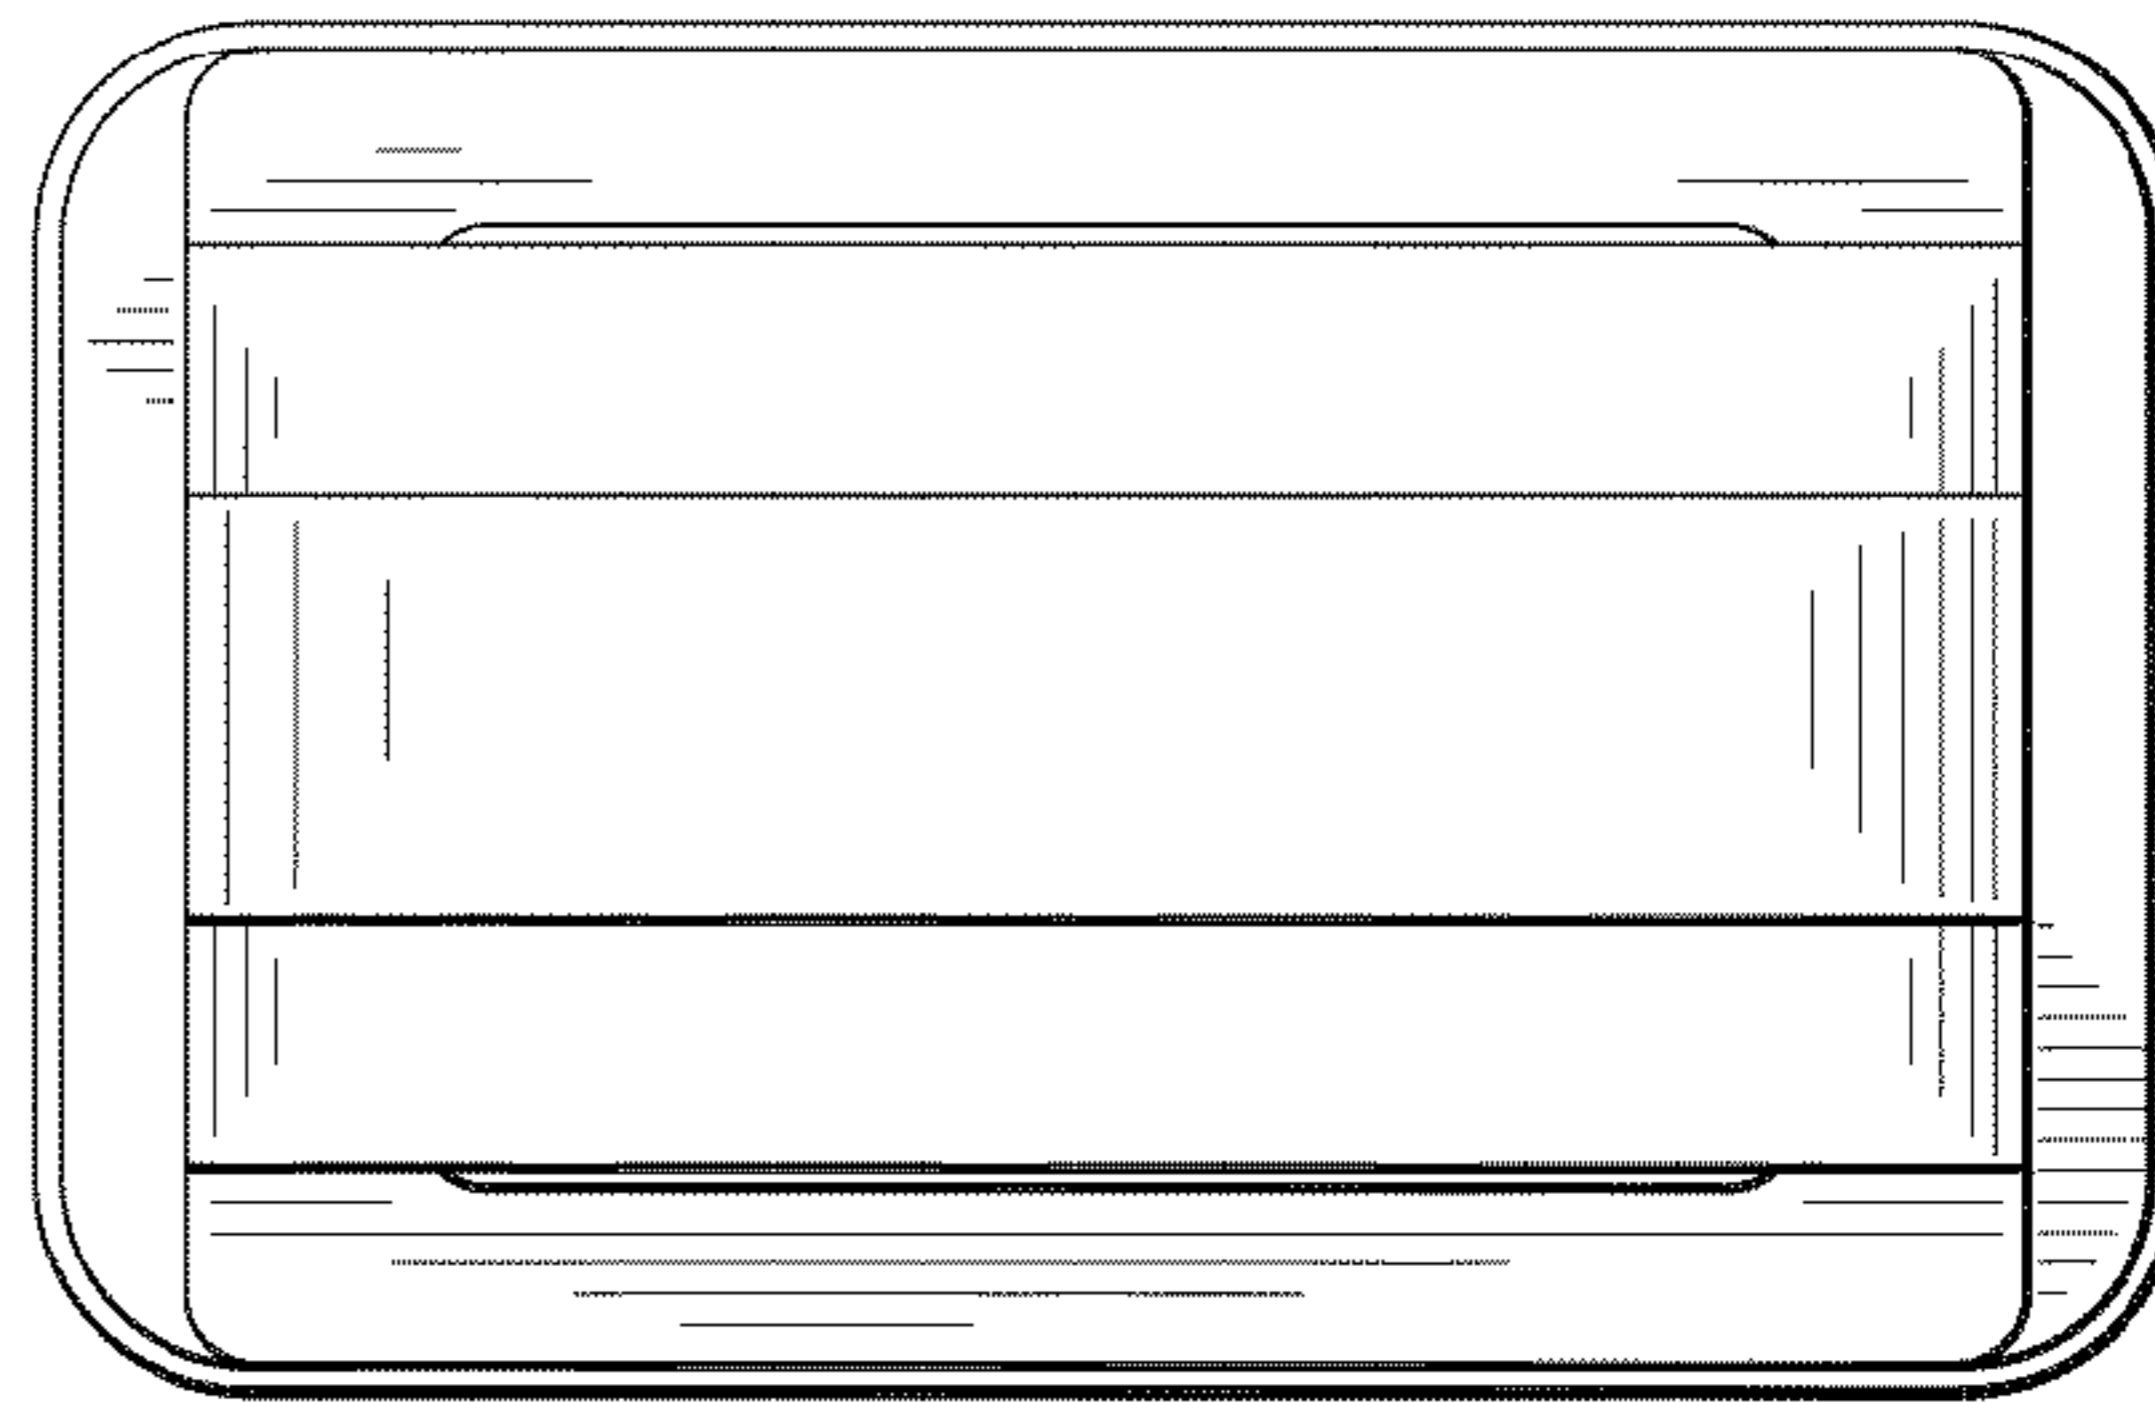


FIG. 4

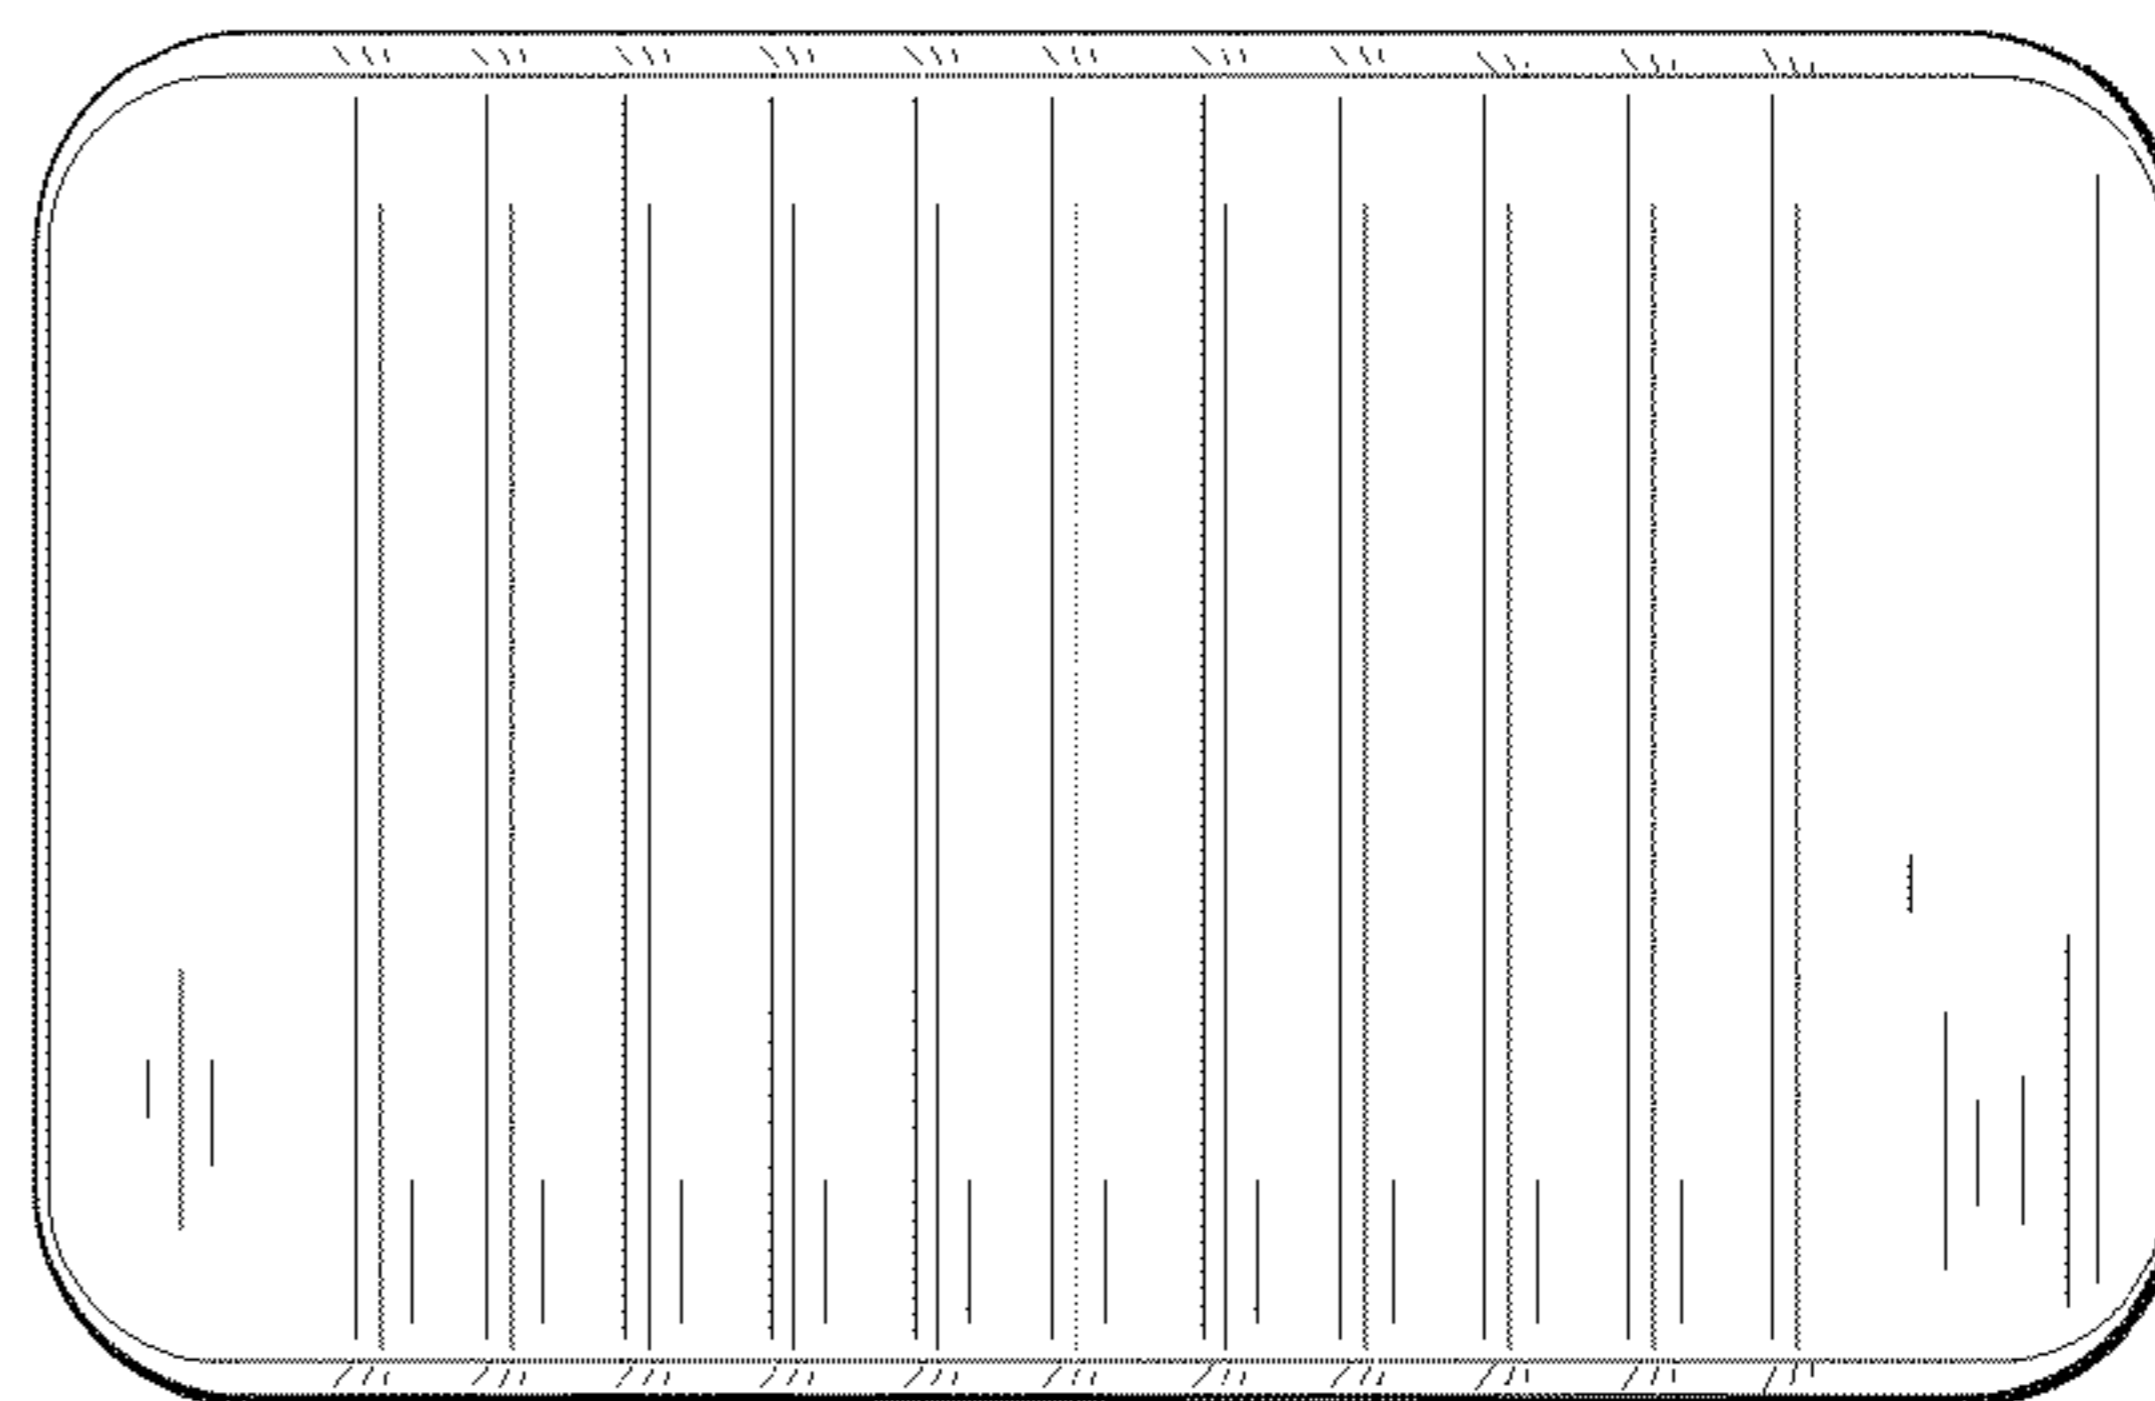


FIG. 5