



US00D652138S

(12) **United States Design Patent**  
**Nino et al.**

(10) **Patent No.:** **US D652,138 S**  
(45) **Date of Patent:** **\*\* Jan. 10, 2012**

(54) **DIVOTED MEDICAL INSTRUMENT HANDLE**

(75) Inventors: **John Nino**, Simi Valley, CA (US); **David Ivinson**, Camarillo, CA (US); **Douglas Slomski**, Chicago, IL (US)

(73) Assignee: **ECA Medical Instruments**, Newbury Park, CA (US)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/372,975**

(22) Filed: **Feb. 12, 2011**

(51) **LOC (9) Cl.** ..... **24-02**

(52) **U.S. Cl.** ..... **D24/133**

(58) **Field of Classification Search** ..... D24/133;  
D8/83, 107; 433/141; 606/1  
See application file for complete search history.

7,740,249	B1	6/2010	Gao	
7,793,573	B2	9/2010	Gao	
7,806,027	B1	10/2010	Gao	
7,810,817	B1	10/2010	Gao	
2002/0169453	A1*	11/2002	Berger	606/73
2004/0127888	A1*	7/2004	O'Neil et al.	606/1
2006/0025773	A1*	2/2006	Yevmenenko et al.	606/73

**OTHER PUBLICATIONS**

Holmed Corporation Surgical Instruments Catalog, www.holmed.net, 40 Norfolk Avenue, South Easton, MA, USA, 02375.  
 Beere Medical Line of Custom Configured Ortho-Grip Handles; www.teleflexmedicaloem.com.  
 Bradshaw Medical, Inc., Non-Ratcheting and Fixed Comfort Grip Handles; www.bradshaw-medical.com/nrds.html.  
 Paragon Medical Standard Surgical Instrumentation Catalog, www.paragonmedical.com/catalog/complete-catalog.html.  
 Quick Connectors, Gauthier Biomedical, Inc., www.gauthierbiomedical.com/products/quick-connectors/.  
 Silicone Handles, Gauthier Biomedical, Inc., www.gauthierbiomedical.com/products/silicone-handles.

(Continued)

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D163,282	S	*	5/1951	Heschel	.....	D8/14
3,360,861	A	*	1/1968	Hoffman	.....	433/3
D273,268	S	*	4/1984	Smith	.....	D8/83
5,464,407	A	*	11/1995	McGuire	.....	606/86 R
D376,204	S	*	12/1996	Huculak et al.	.....	D24/146
D386,063	S	*	11/1997	Badiali	.....	D8/107
D442,049	S	*	5/2001	Shu	.....	D8/83
D456,686	S	*	5/2002	Holland-Letz	.....	D8/83
D462,440	S	*	9/2002	Formanek	.....	D24/133
D520,320	S	*	5/2006	Corcoran	.....	D8/68
D536,786	S	*	2/2007	Schreiner et al.	.....	D24/133
D543,433	S		5/2007	Gao		
7,243,581	B1		7/2007	Gao		
D553,738	S	*	10/2007	Simonson	.....	D24/133
D557,584	S		12/2007	Gao		
D562,665	S		2/2008	Gao		
7,334,509	B1		2/2008	Gao		
D563,752	S	*	3/2008	Fach	.....	D8/83
7,389,700	B2		6/2008	Gao		
D580,730	S		11/2008	Gao		
7,467,576	B2		12/2008	Gao		
7,516,676	B2		4/2009	Gao		

*Primary Examiner* — Bridget L Eland

(74) *Attorney, Agent, or Firm* — Baker Hostetler, LLP

(57) **CLAIM**


The ornamental design for a divoted medical instrument handle, as shown and described.

**DESCRIPTION**

FIGS. 1, 2, 3, and 4 are side elevations at 90 degree offsets of a divoted medical instrument handle showing our new design; FIG. 5 is a front to back perspective view thereof; FIG. 6 is a front view thereof; and, FIG. 7 is a back view thereof.

The broken lines showing the remainder of the medical instrument are directed to environment and are for illustrative purposes only; the broken lines form no part of the claimed design.

**1 Claim, 3 Drawing Sheets**

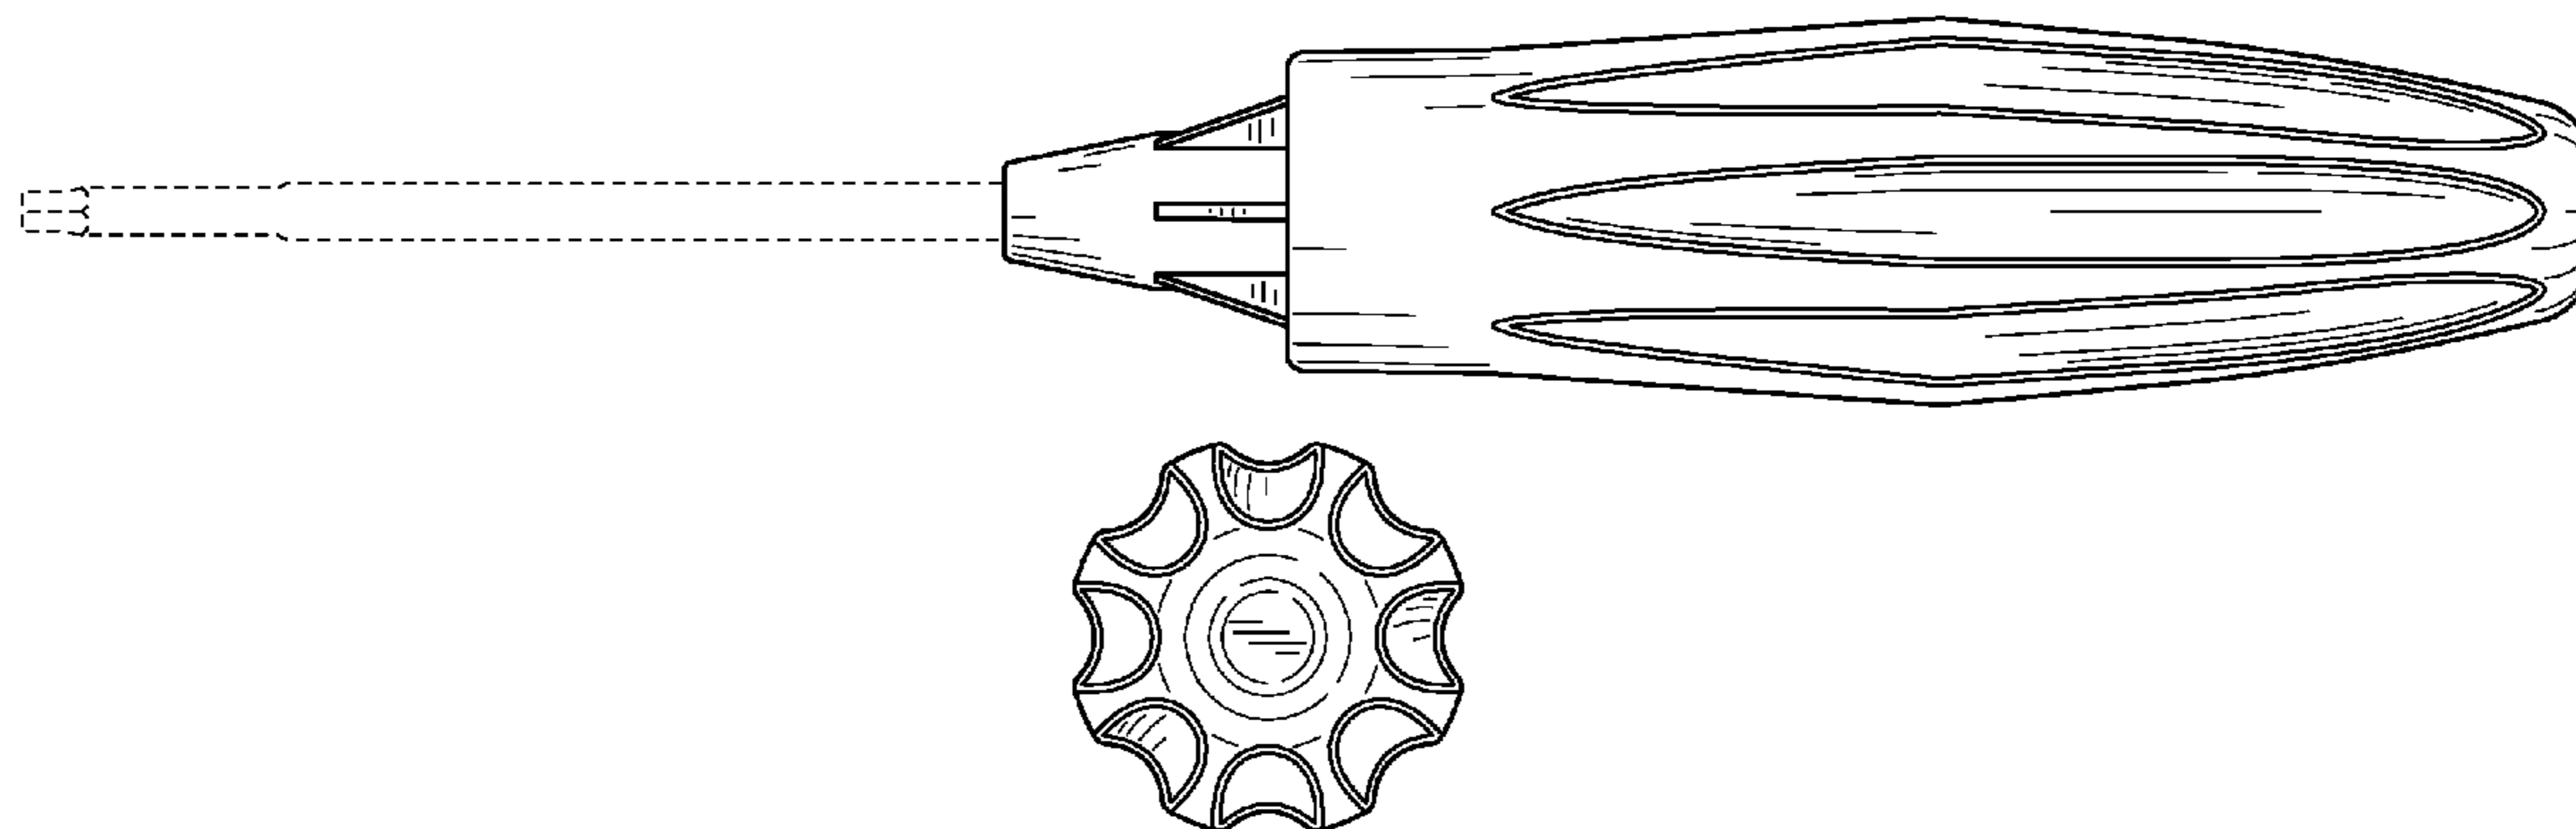

OTHER PUBLICATIONS

Ratcheting Screwdrivers, Gauthier Biomedical, Inc., [www.gauthierbiomedical.com/products/products](http://www.gauthierbiomedical.com/products/products).

Torque Instruments, Gauthier Biomedical, Inc., [www.gauthierbiomedical.com/products/torque-instruments/](http://www.gauthierbiomedical.com/products/torque-instruments/).

Symmetry Medical Inc., Radel R Instrument Handles, Silicone Instrument Handles, Ratcheting Screwdriver Handles, and Spinal Instruments; [www.symmetrymedical.com](http://www.symmetrymedical.com).

\* cited by examiner

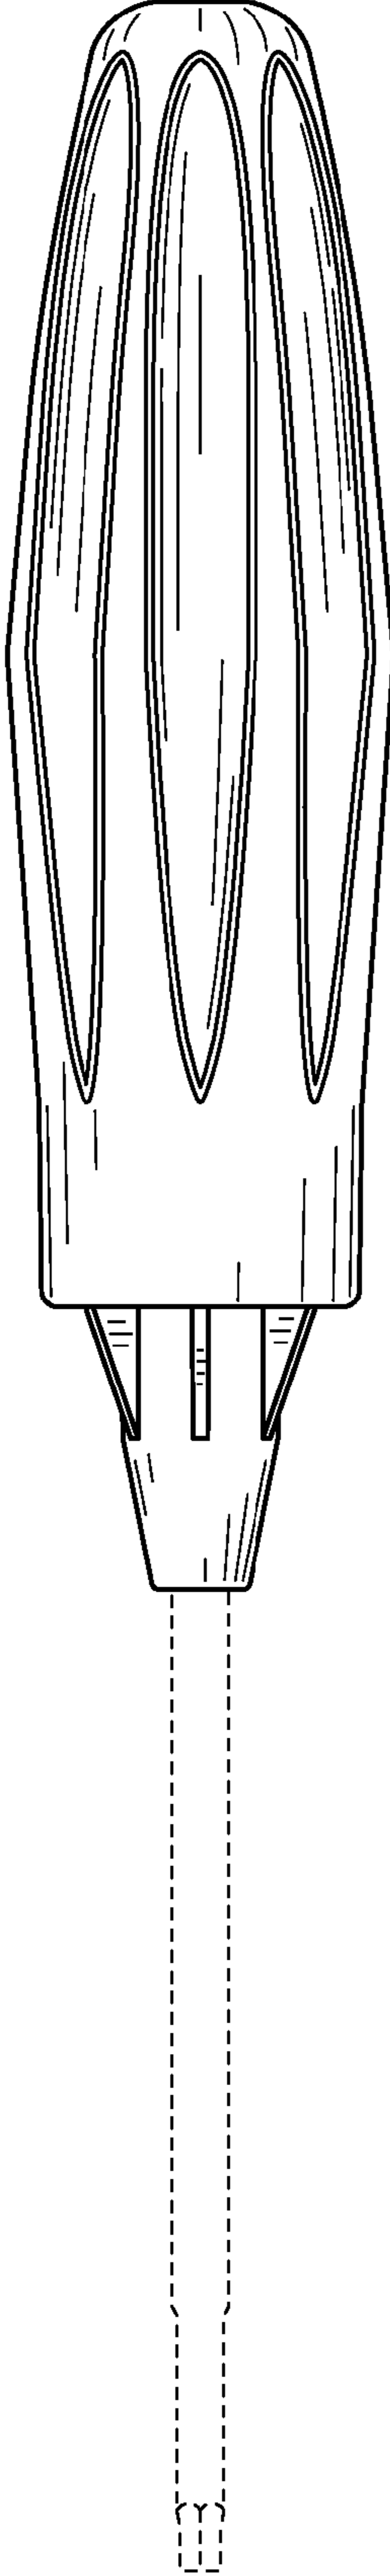


FIG. 1

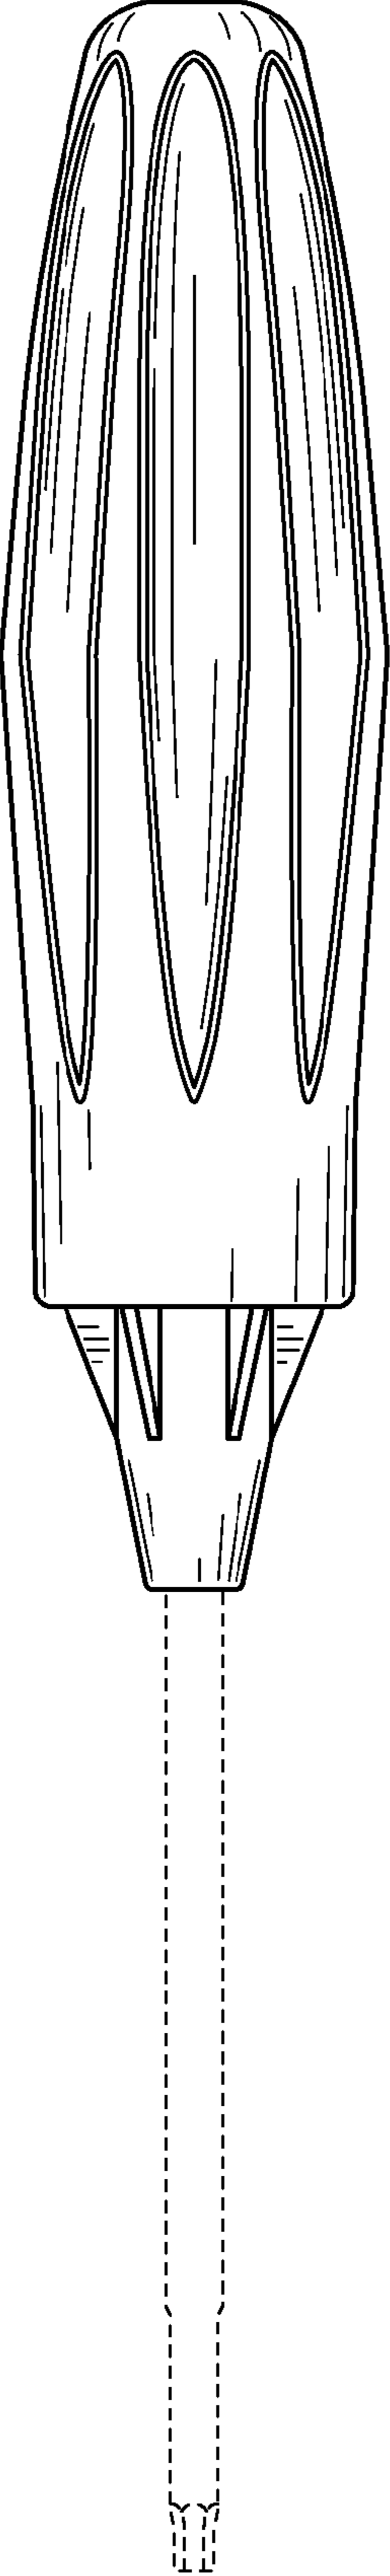


FIG. 2

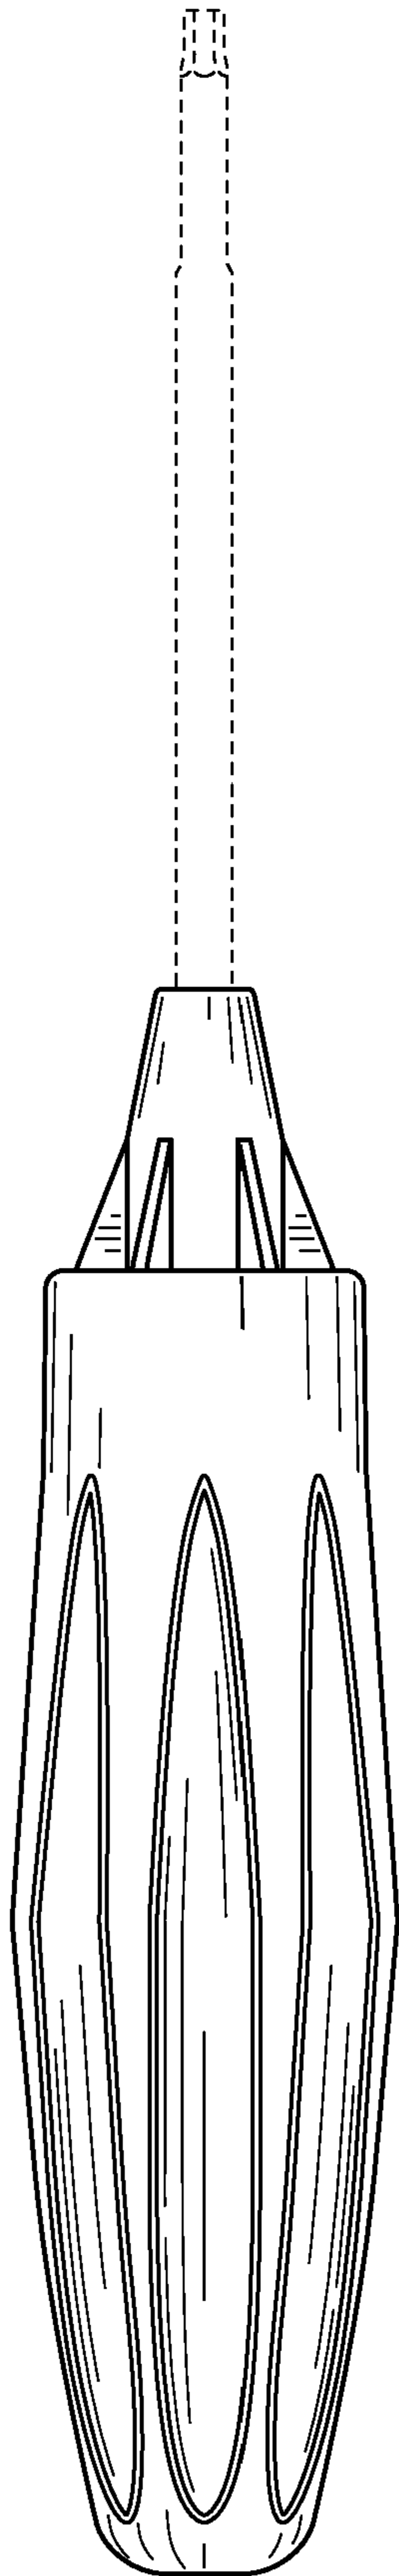


FIG. 3

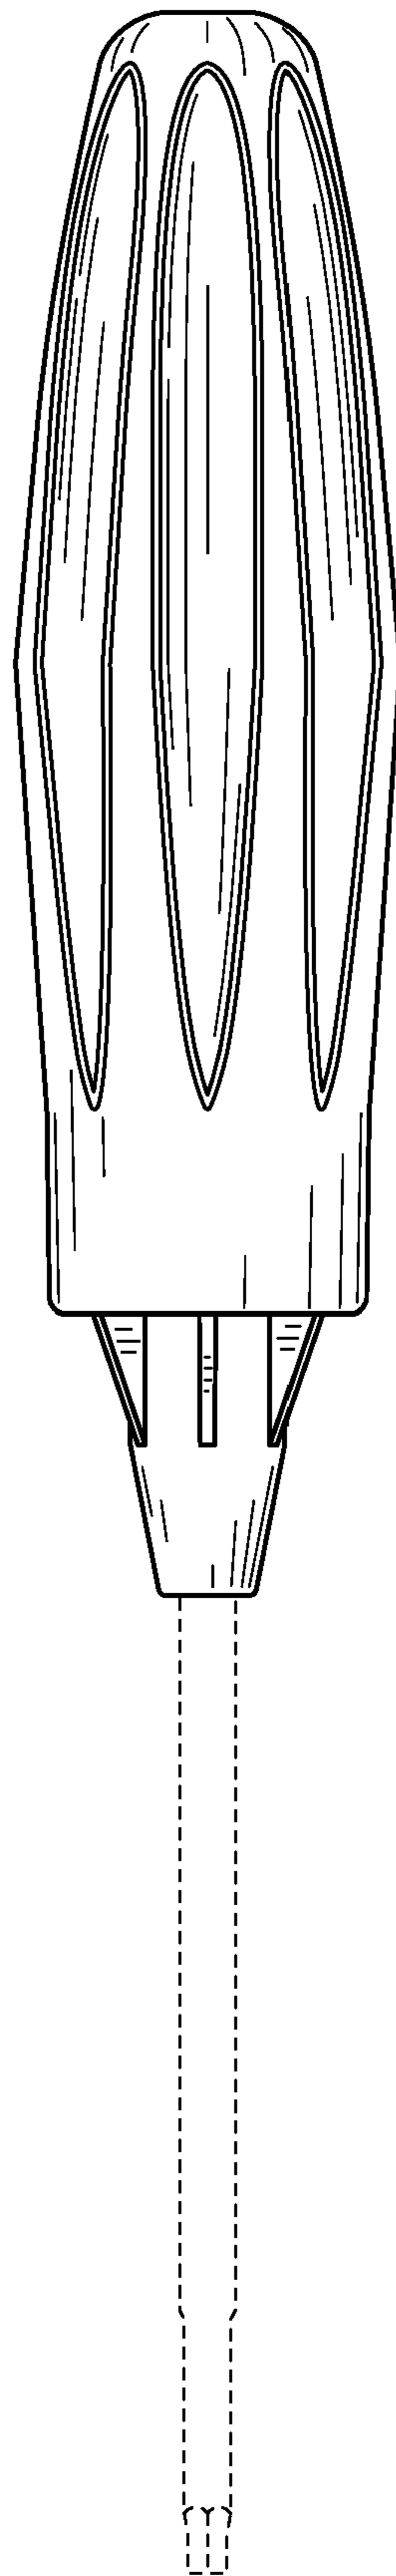


FIG. 4

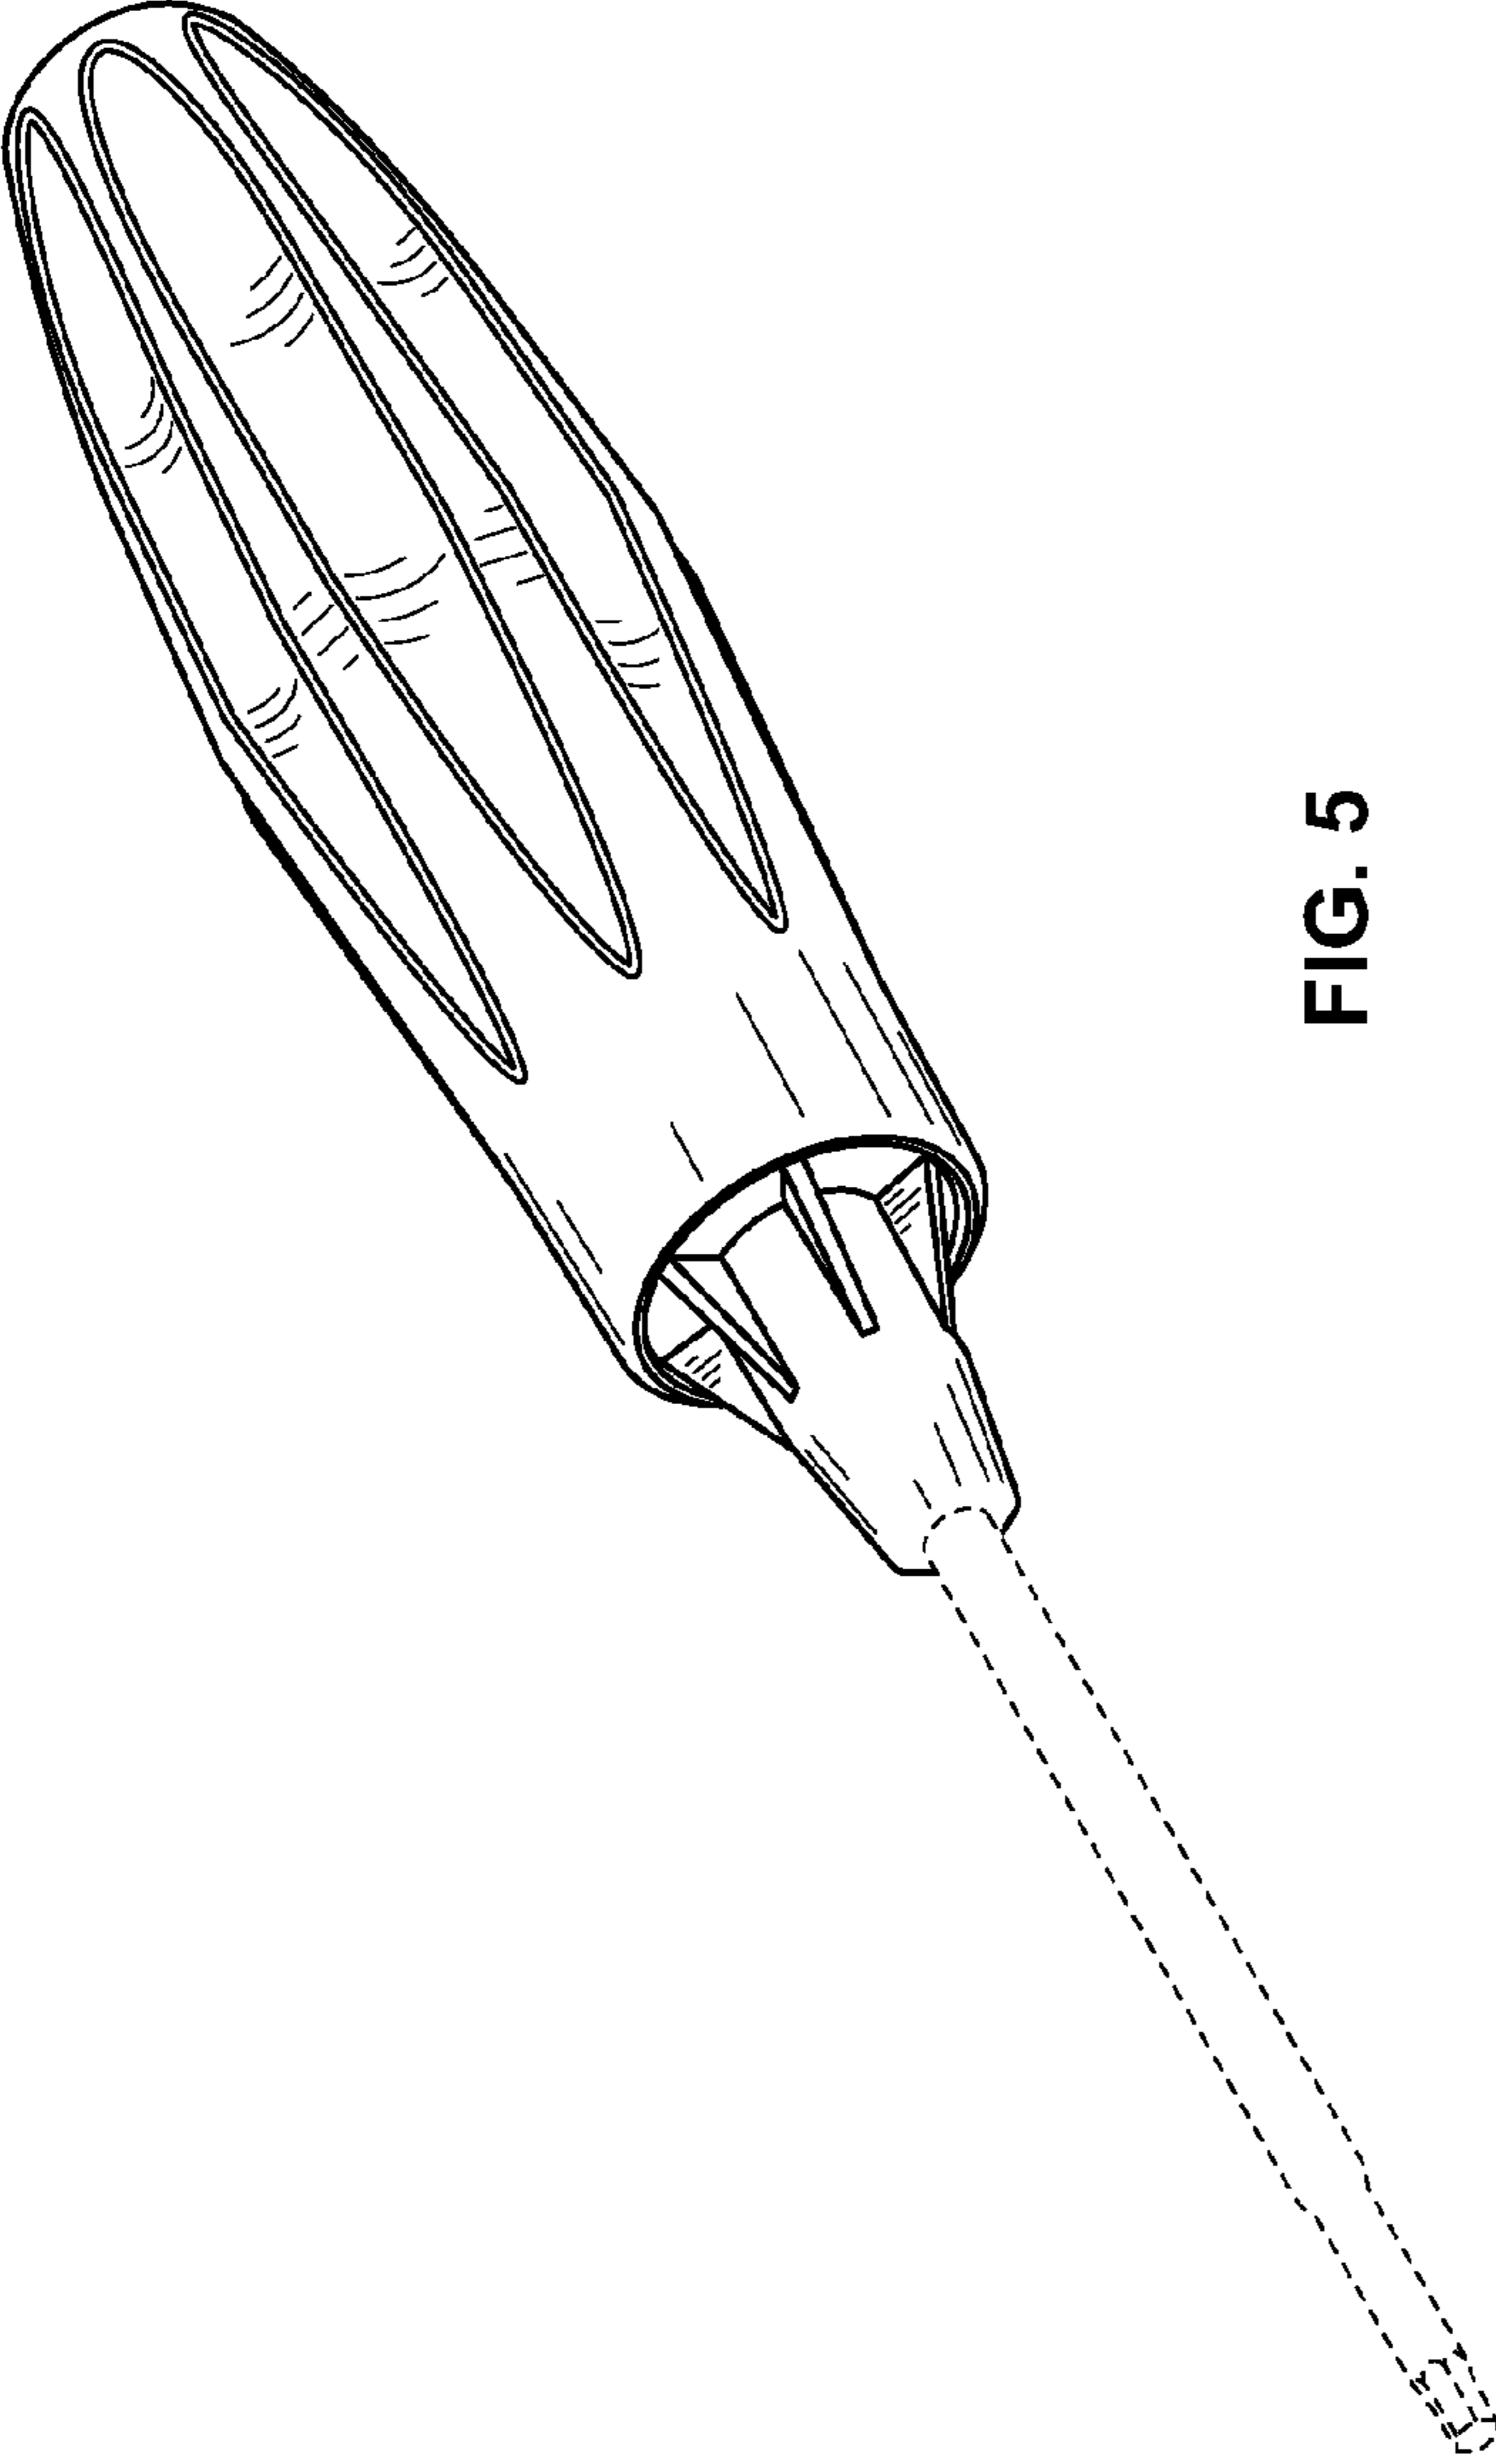


FIG. 5

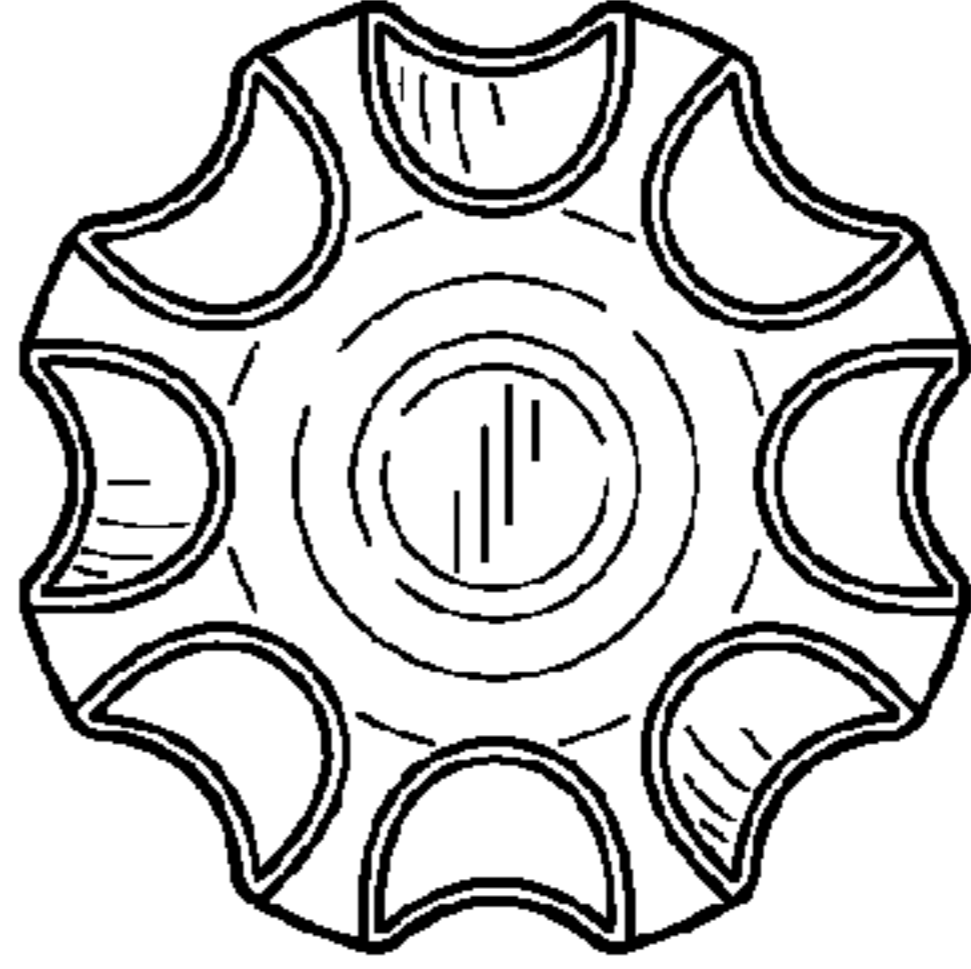


FIG. 7

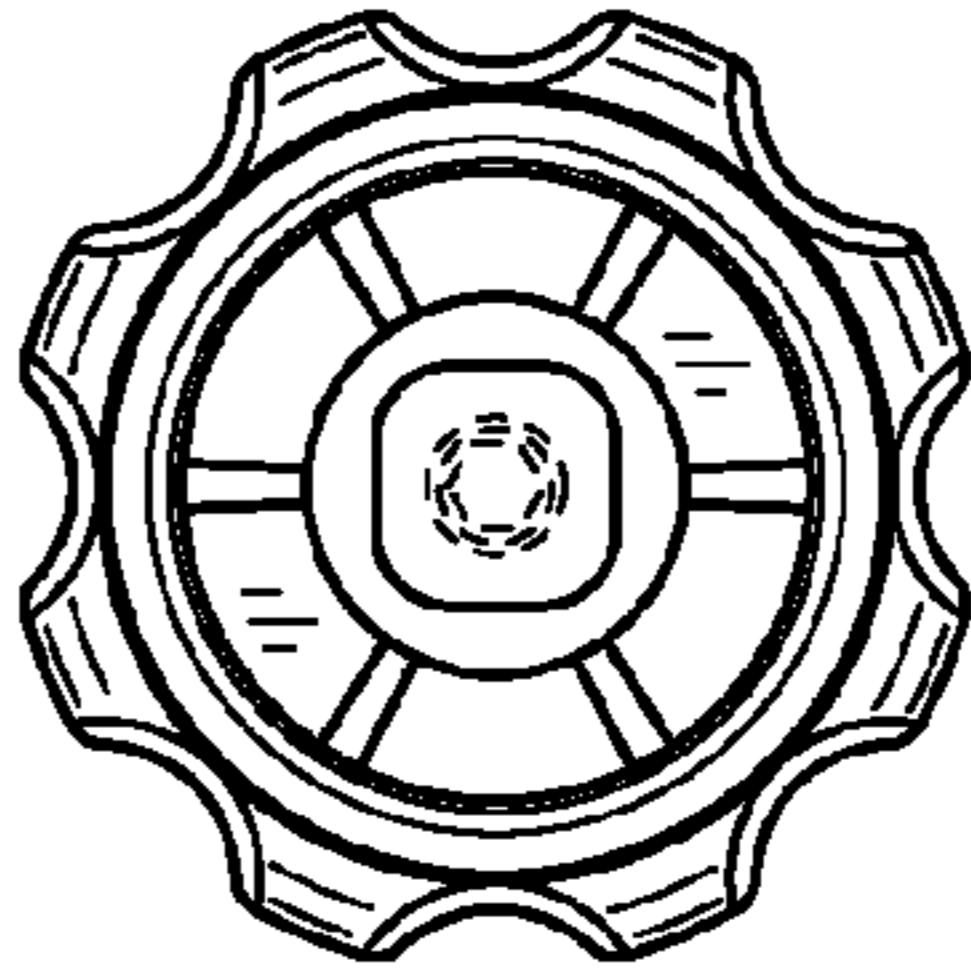


FIG. 6