



US00D653347S

(12) **United States Design Patent**
Tani et al.

(10) **Patent No.:** **US D653,347 S**
(45) **Date of Patent:** **** Jan. 31, 2012**

(54) **HOLDER FOR MEDICAL ULTRASOUND EQUIPMENT**

(75) Inventors: **Ryosuke Tani**, Ehime (JP); **Tamotsu Senda**, Ehime (JP); **Noriyuki Shinohara**, Ehime (JP)

(73) Assignee: **Panasonic Corporation**, Osaka (JP)

(**) Term: **14 Years**

(21) Appl. No.: **29/387,983**

(22) Filed: **Mar. 22, 2011**

(30) **Foreign Application Priority Data**

Oct. 27, 2010 (JP) 2010-025775

(51) **LOC (9) Cl.** **24-01**

(52) **U.S. Cl.** **D24/185**

(58) **Field of Classification Search** D24/183-186,
D24/128, 176-177, 227, 152, 232, 160, 158;
D8/356; 128/922, 660.01, 660.02, 660.03,
128/660.07, 653; 248/56, 918; D29/130
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D354,353 S * 1/1995 Ishizuka et al. D24/160
D365,148 S * 12/1995 Murakami et al. D24/160
D375,450 S * 11/1996 Bidwell et al. D8/356
D383,968 S * 9/1997 Bidwell et al. D8/356
D391,838 S * 3/1998 Bidwell et al. D8/356
D480,810 S * 10/2003 Gumisawa D24/158
D512,508 S * 12/2005 Mesaros D24/185
D544,962 S * 6/2007 Diener et al. D24/186

D554,264 S * 10/2007 Watson et al. D24/186
D560,807 S * 1/2008 Kitayama et al. D24/158
D571,011 S * 6/2008 Otoha et al. D24/158
D609,349 S * 2/2010 Pelissier et al. D24/186
D618,356 S * 6/2010 Ross D29/130
D626,239 S * 10/2010 Lia et al. D24/185
2004/0179332 A1 * 9/2004 Smith et al. 361/681

FOREIGN PATENT DOCUMENTS

JP D1068333 4/2000
JP D1400877 11/2010

* cited by examiner

Primary Examiner — T. Chase Nelson

Assistant Examiner — Mark Cavanna

(74) *Attorney, Agent, or Firm* — Brinks Hofer Gilson & Lione

(57) **CLAIM**

We claim the ornamental design for a holder for medical ultrasound equipment, as shown and described.

DESCRIPTION

FIG. 1 is a front perspective view of a holder for medical ultrasound equipment of the present invention;
FIG. 2 is a rear perspective view thereof;
FIG. 3 is a front view thereof;
FIG. 4 is a rear view thereof;
FIG. 5 is a first side view thereof;
FIG. 6 is a second side view thereof;
FIG. 7 is a top view thereof; and,
FIG. 8 is a bottom view thereof.

The broken lines are included for the purpose of illustrating portions of the holder for medical ultrasound equipment that form no part of the claimed design.

1 Claim, 5 Drawing Sheets

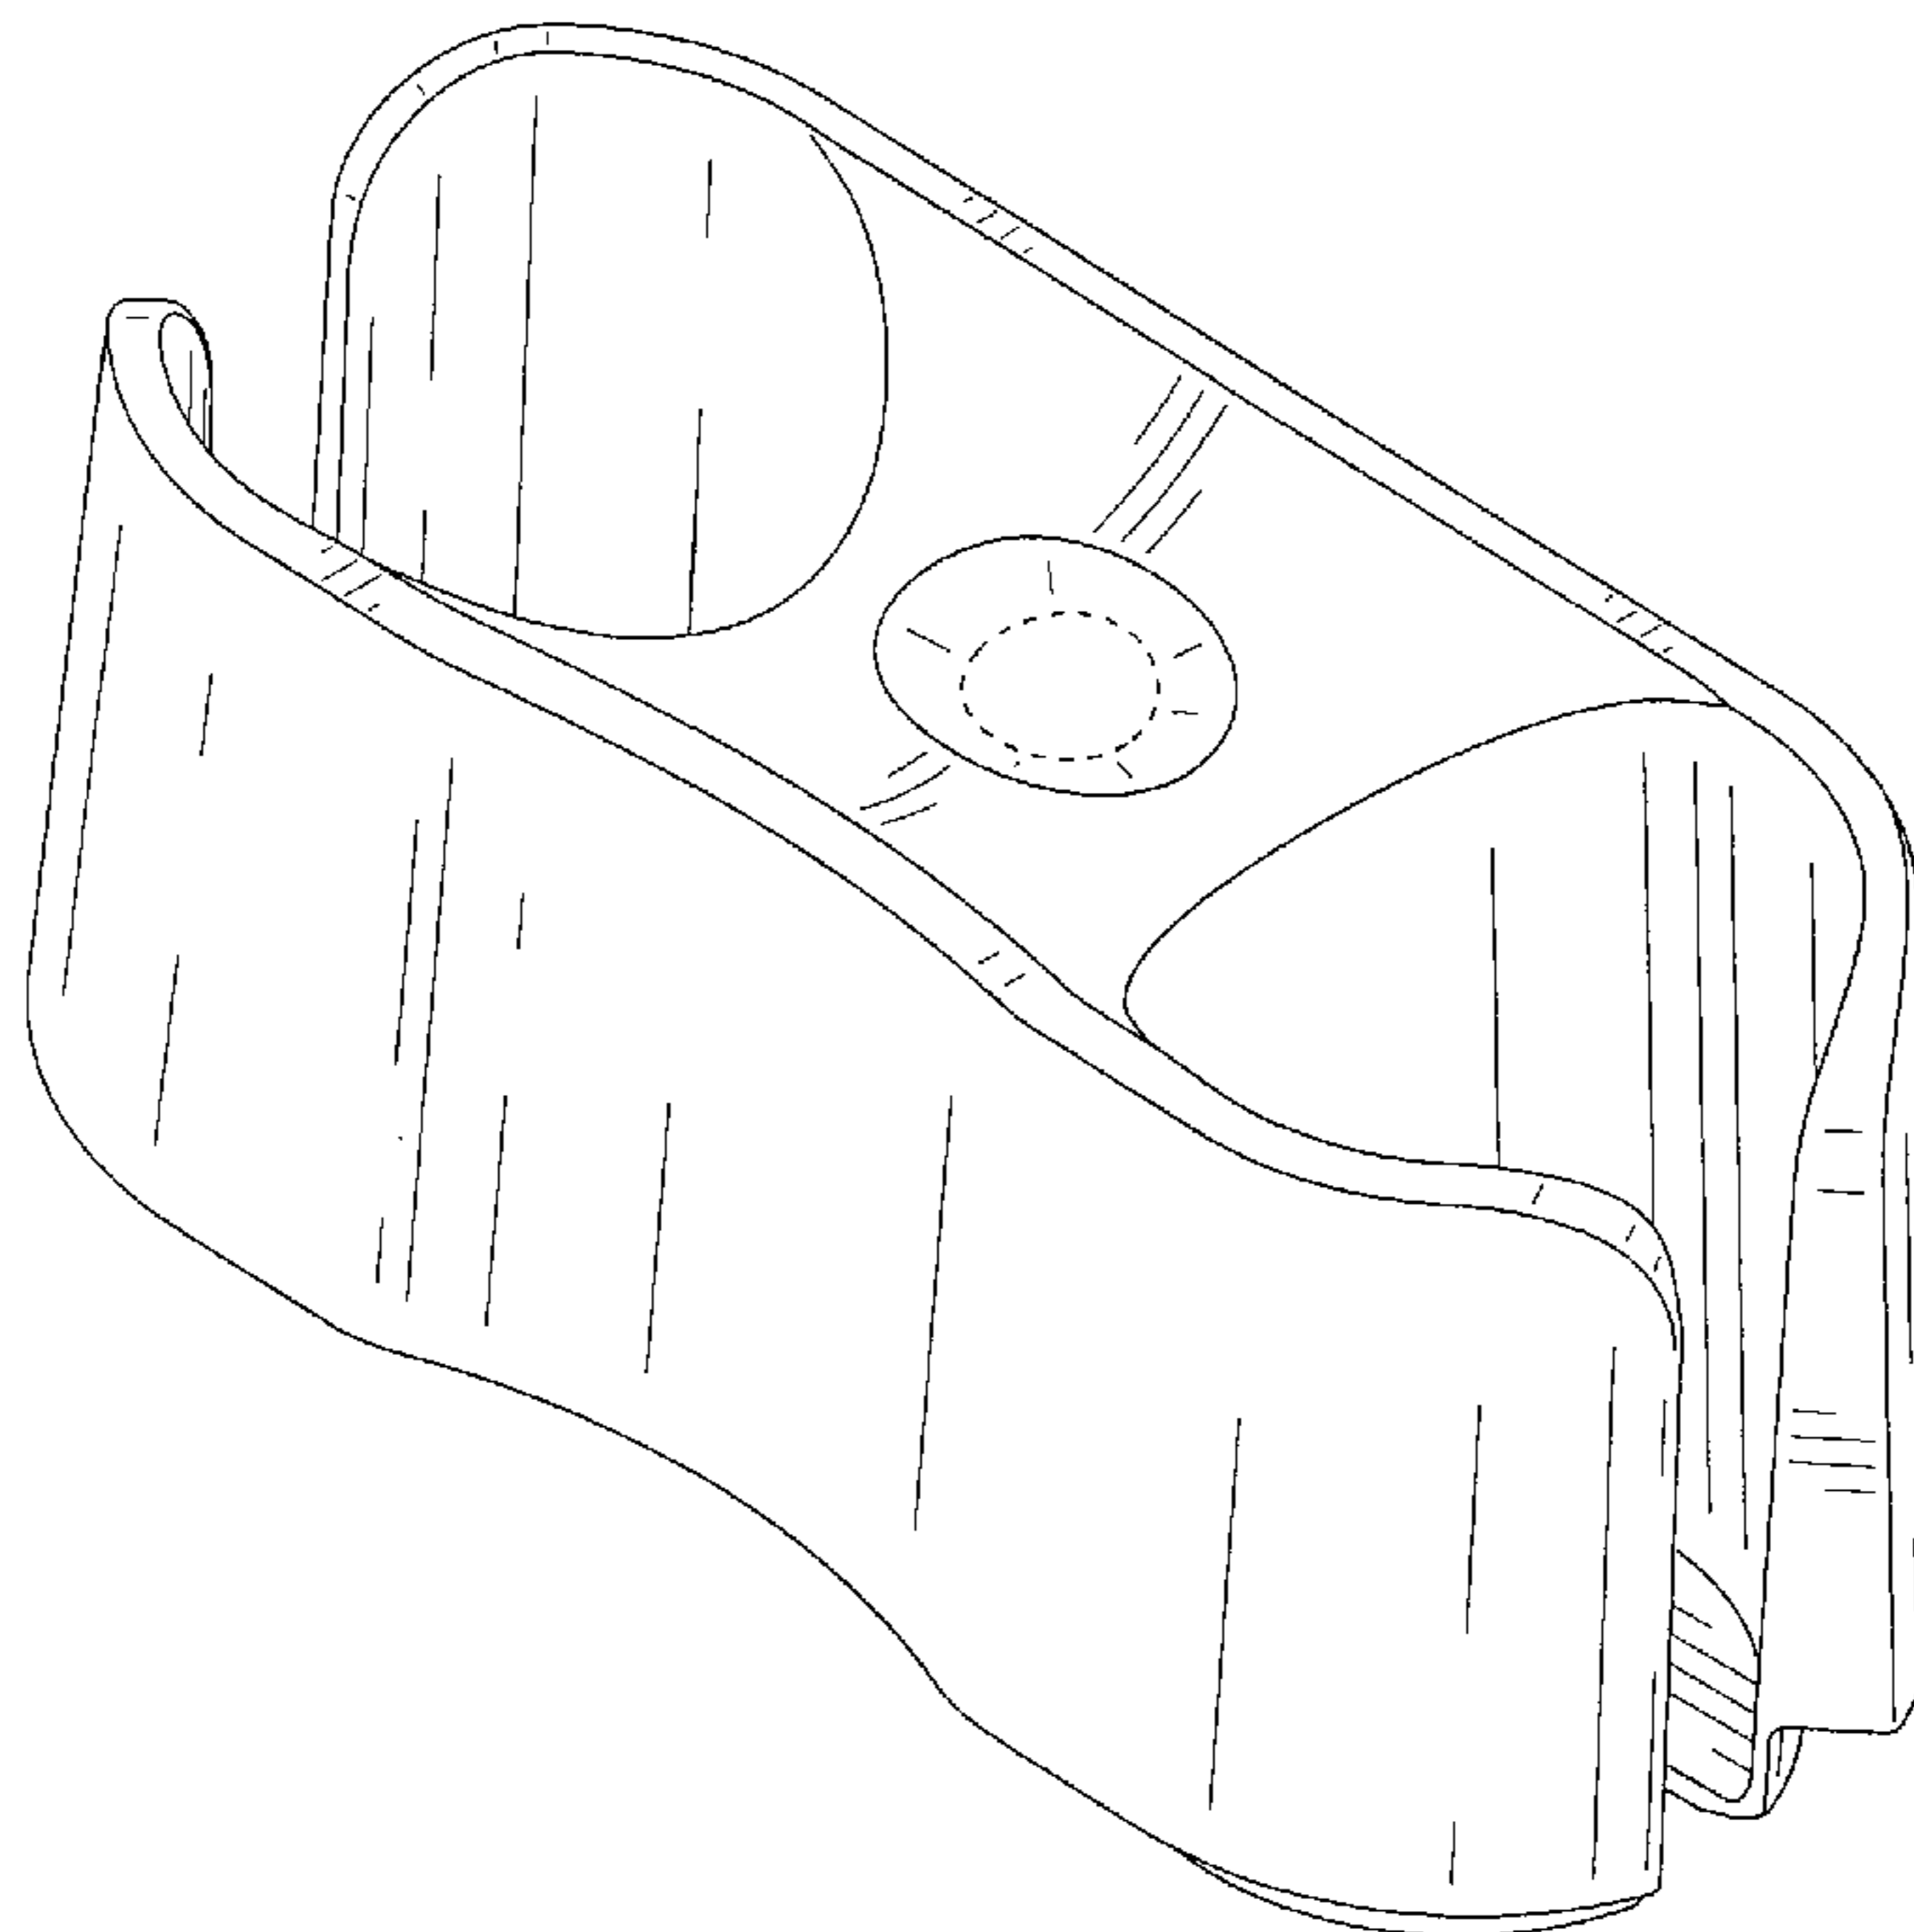


FIG.1

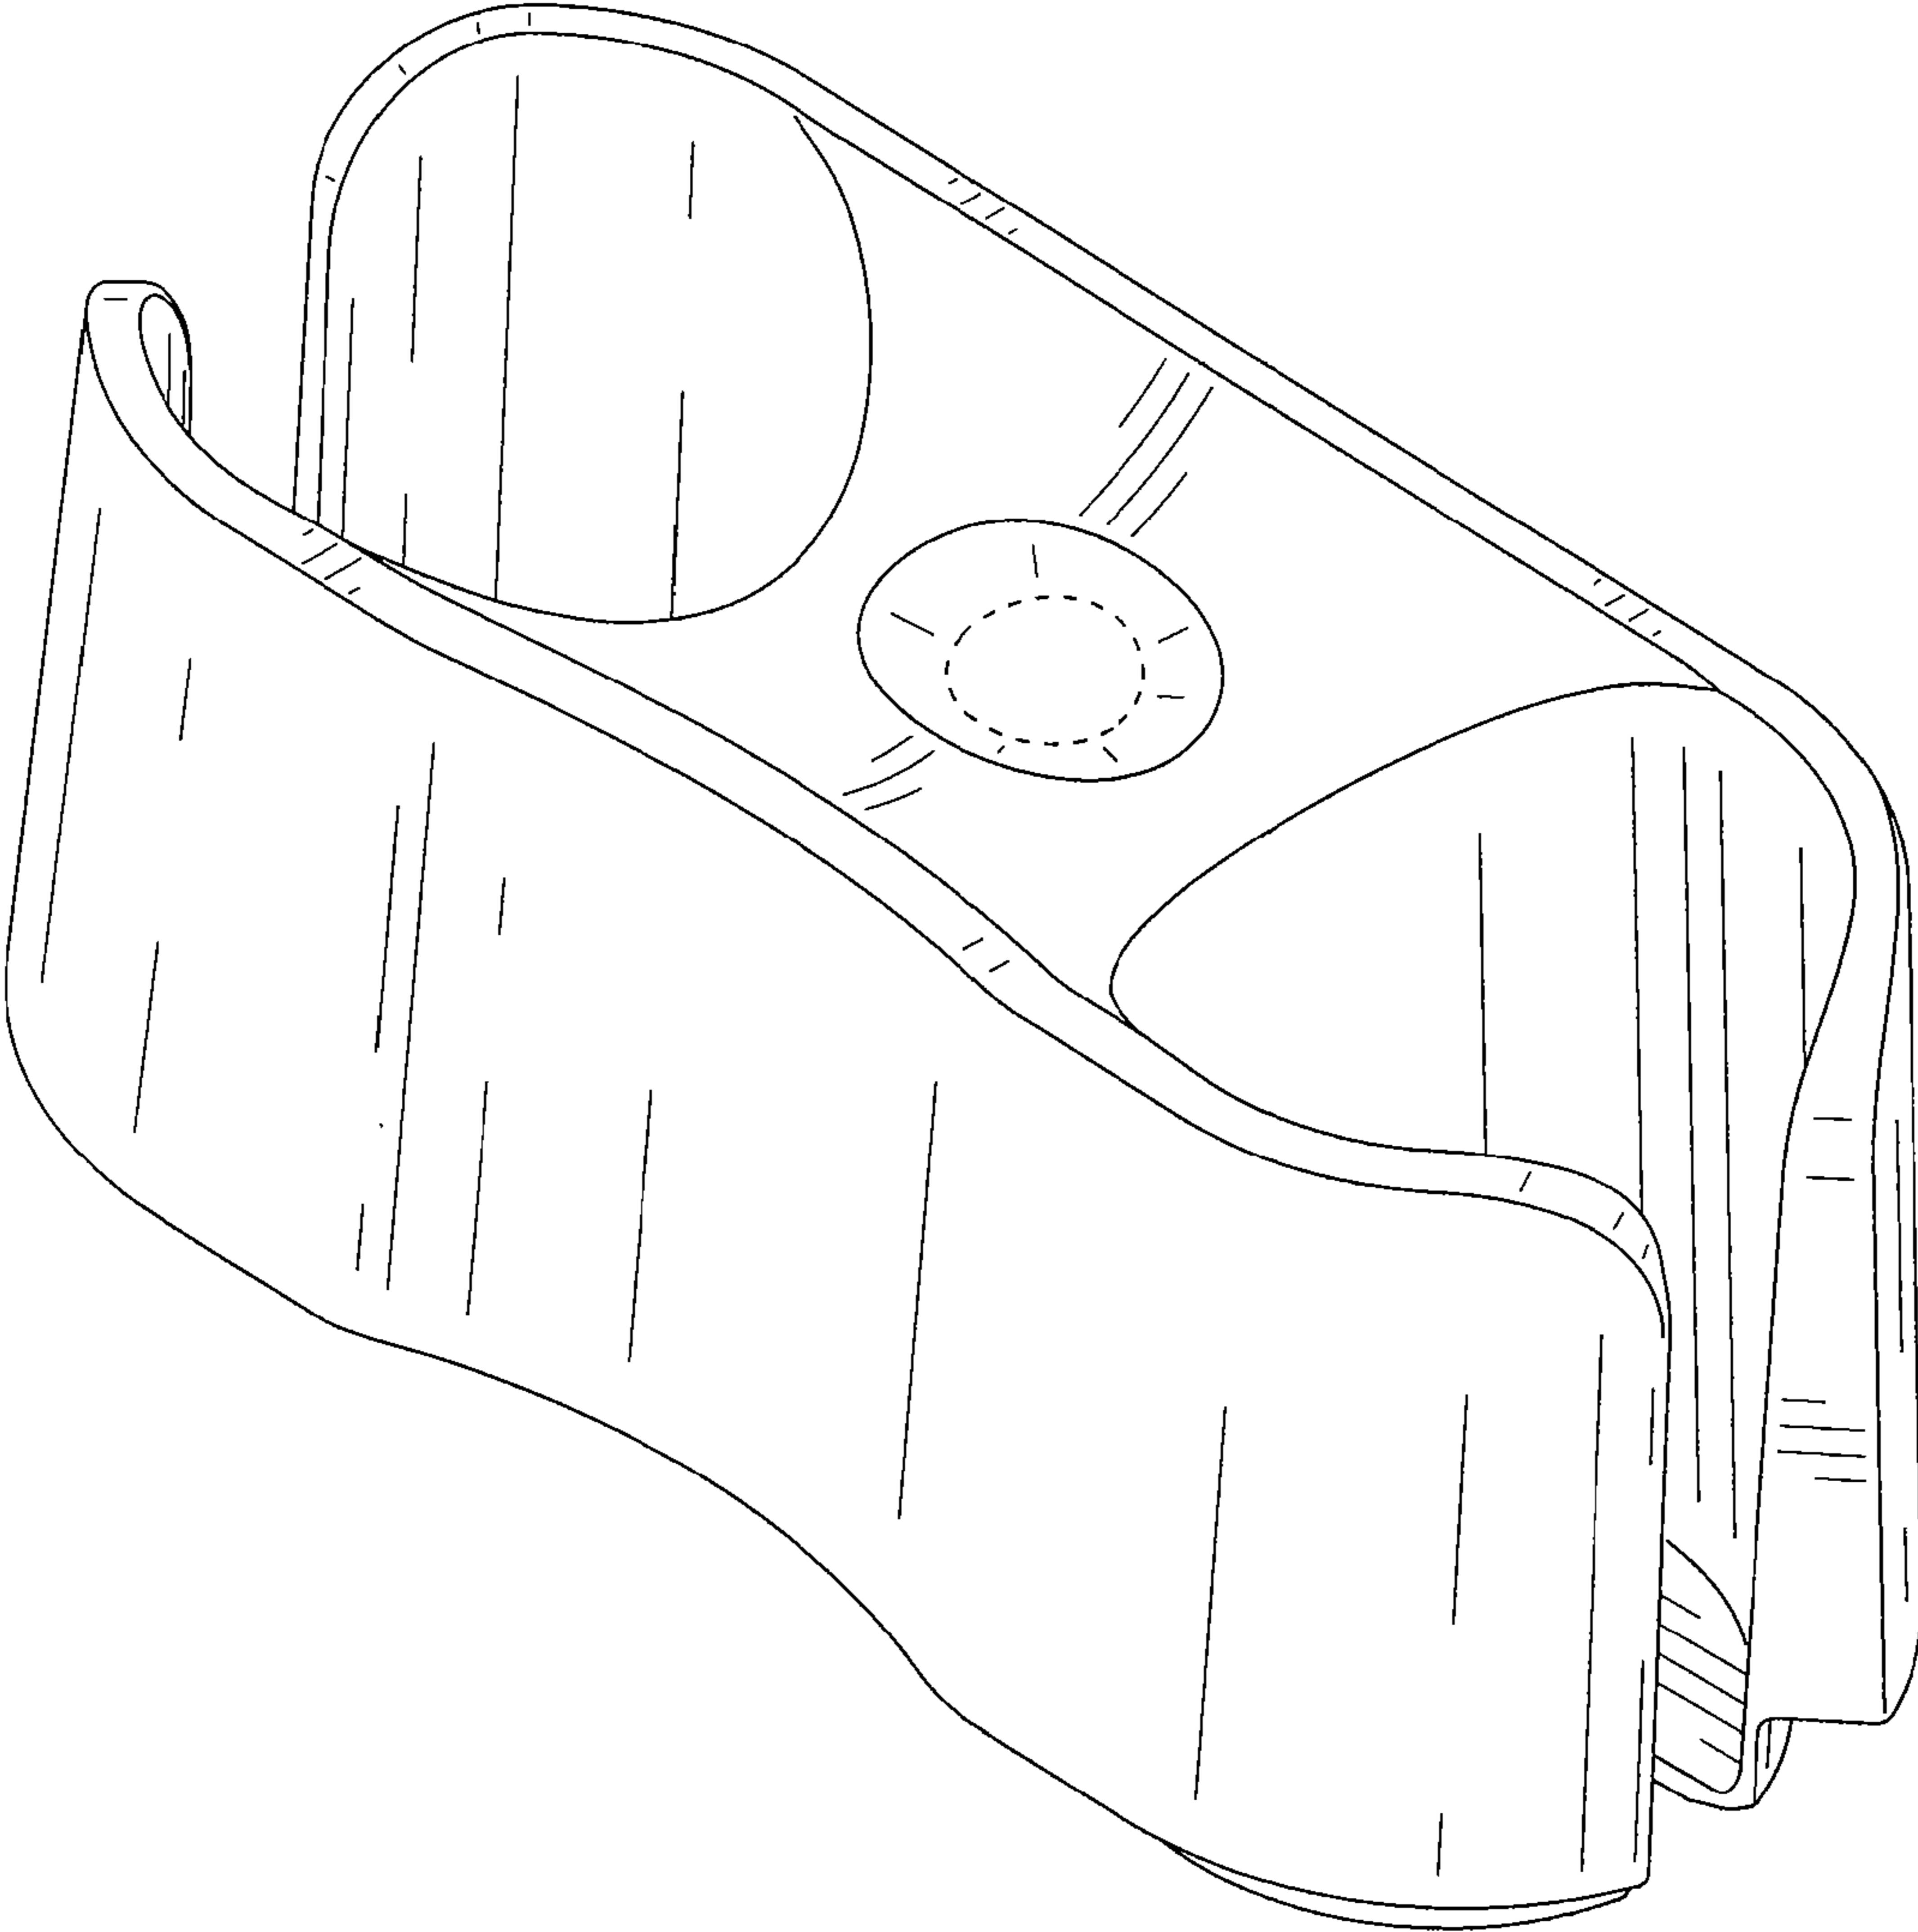


FIG.2

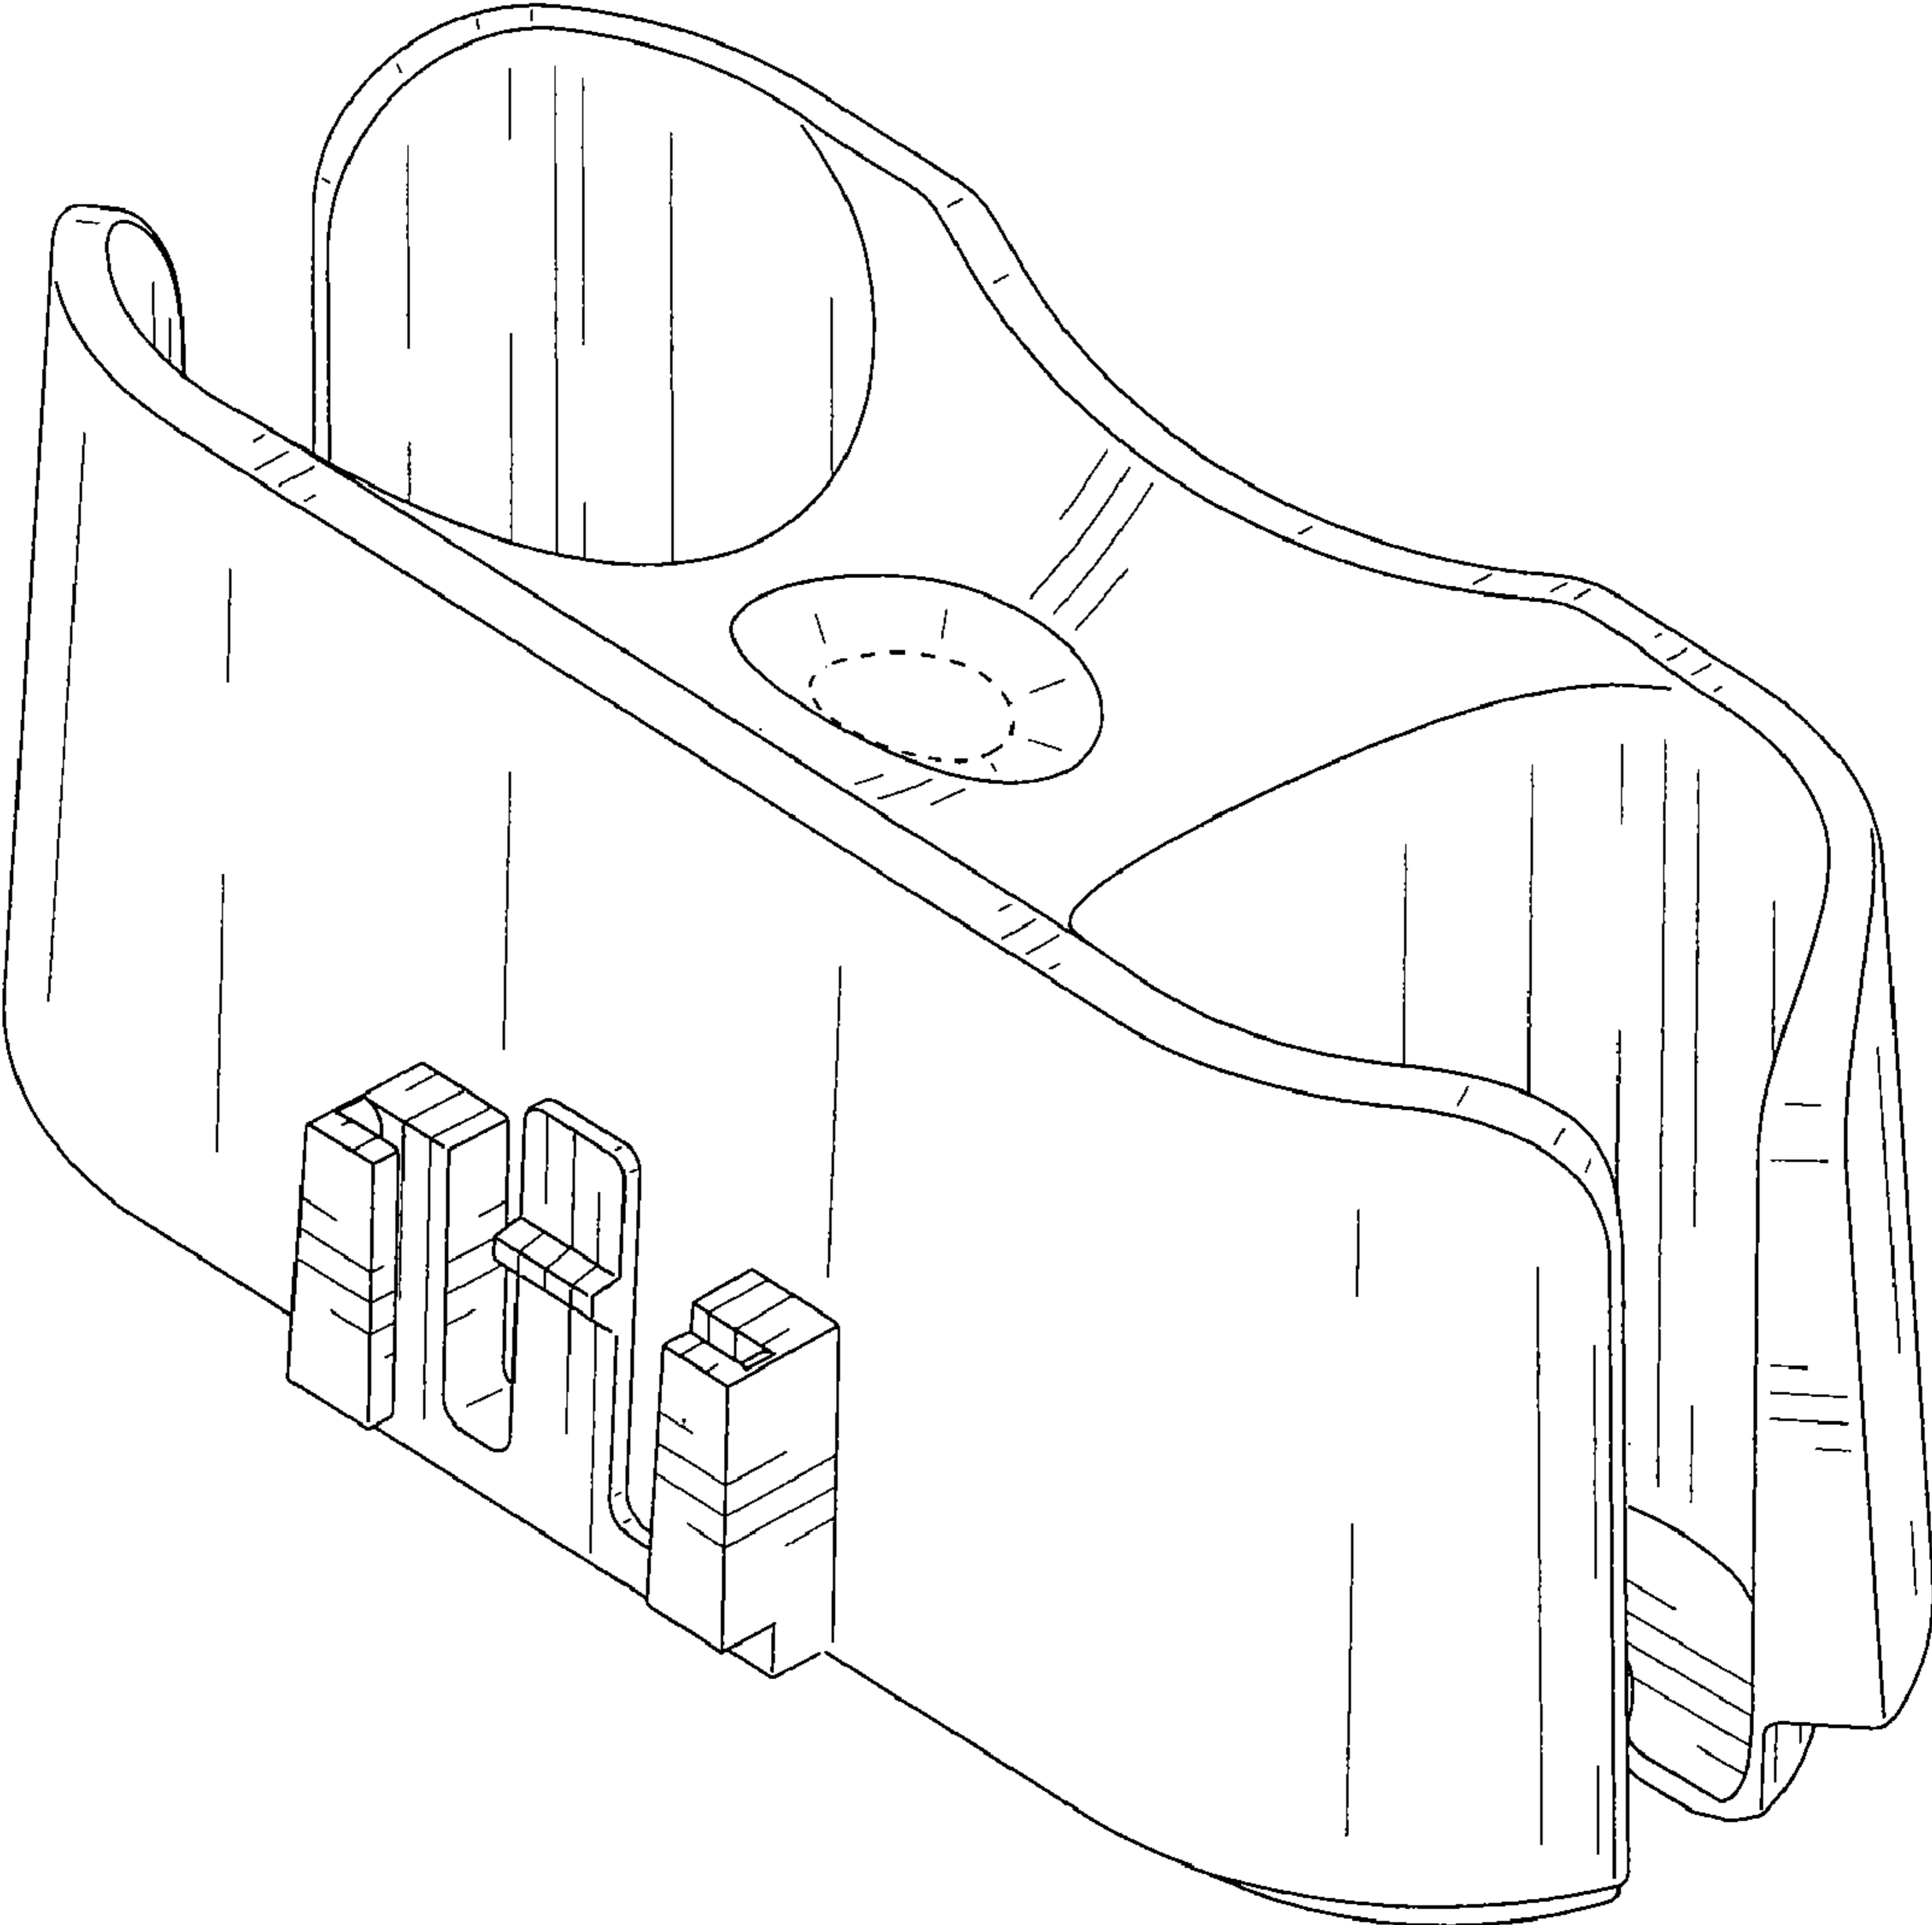


FIG.3

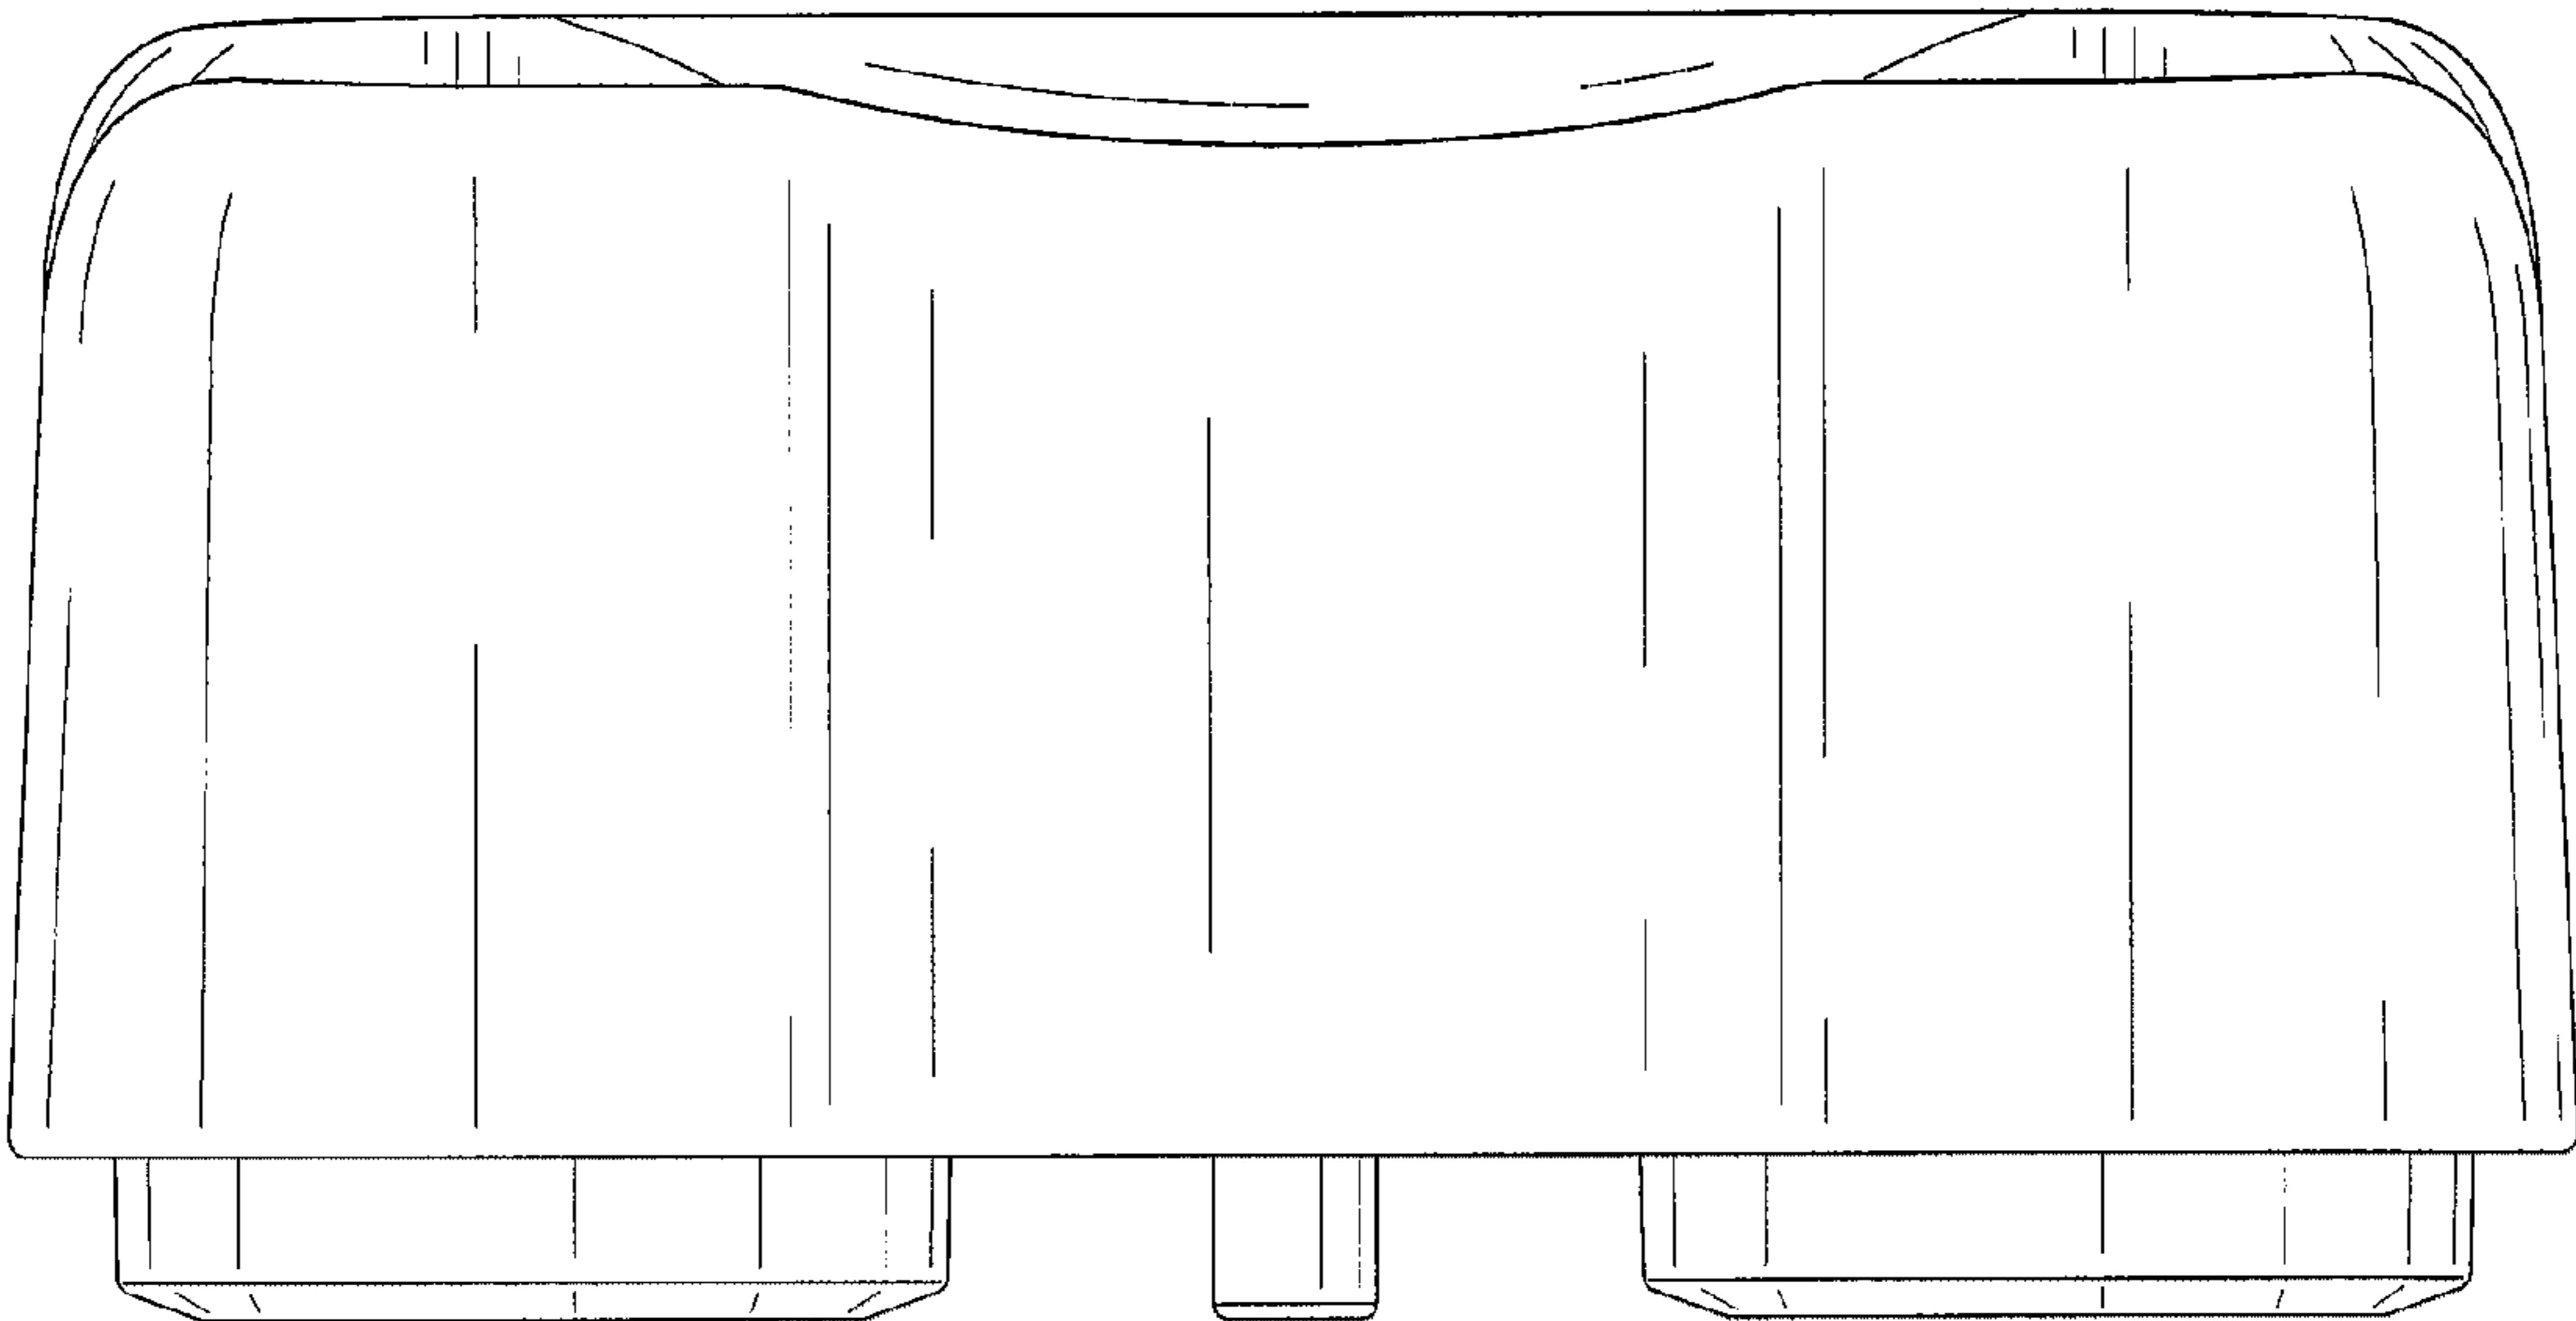


FIG.4

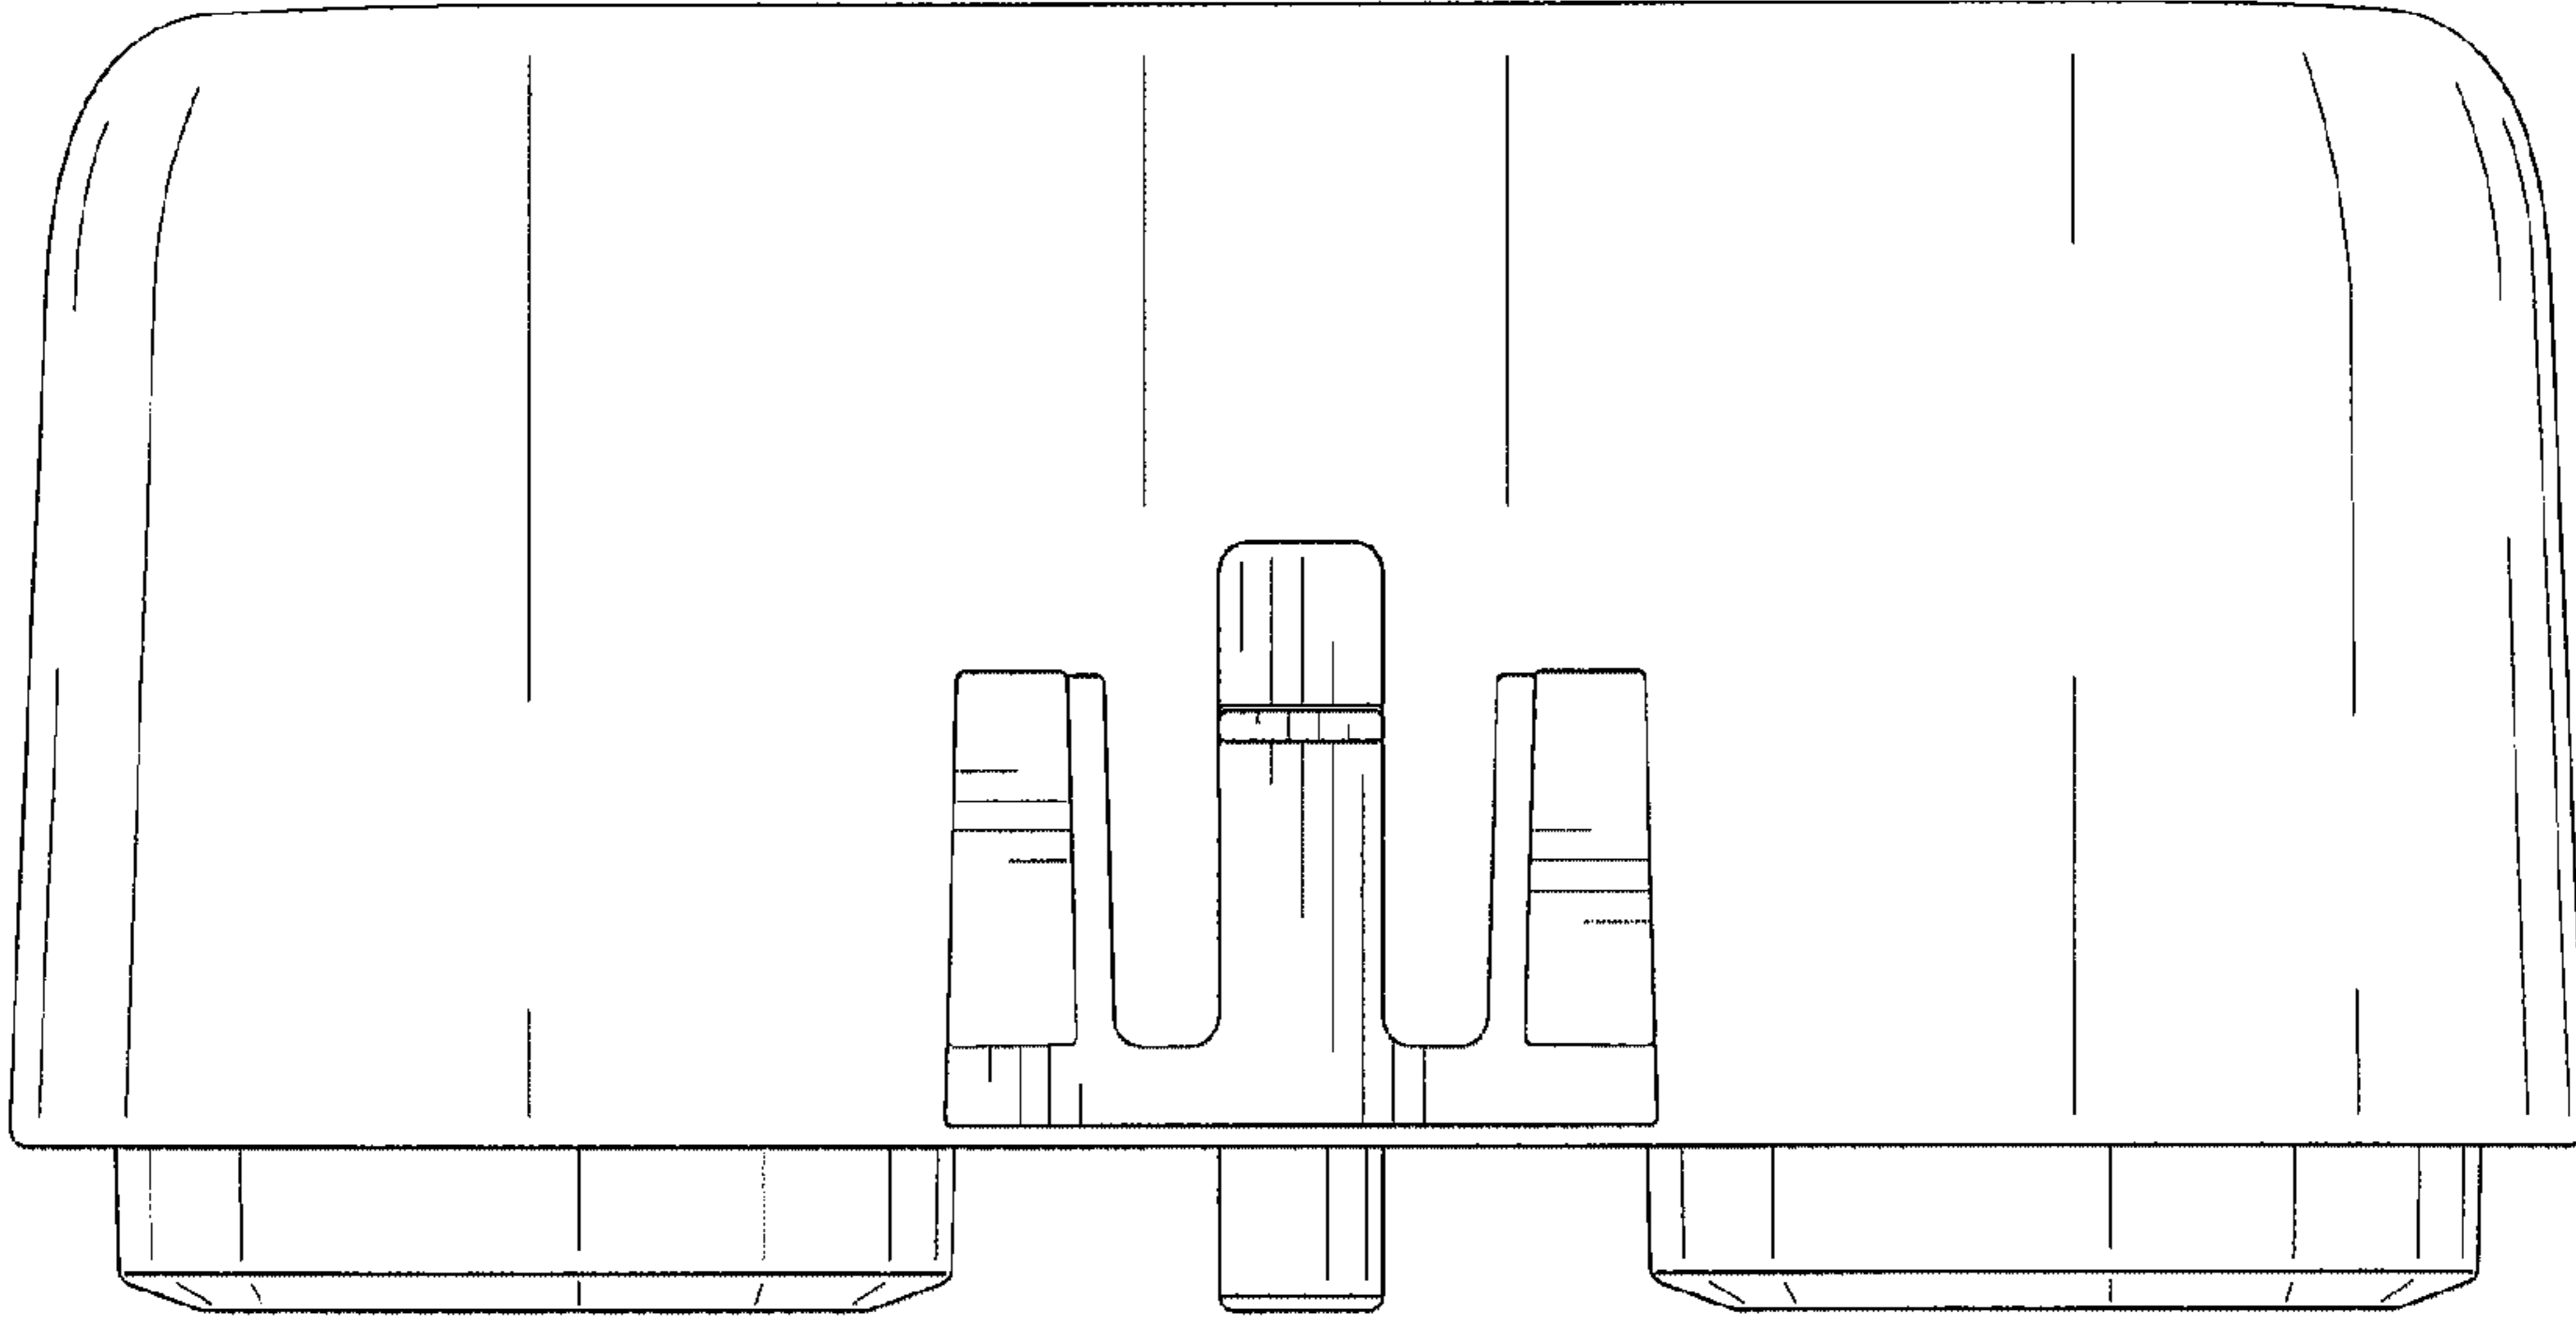


FIG.5

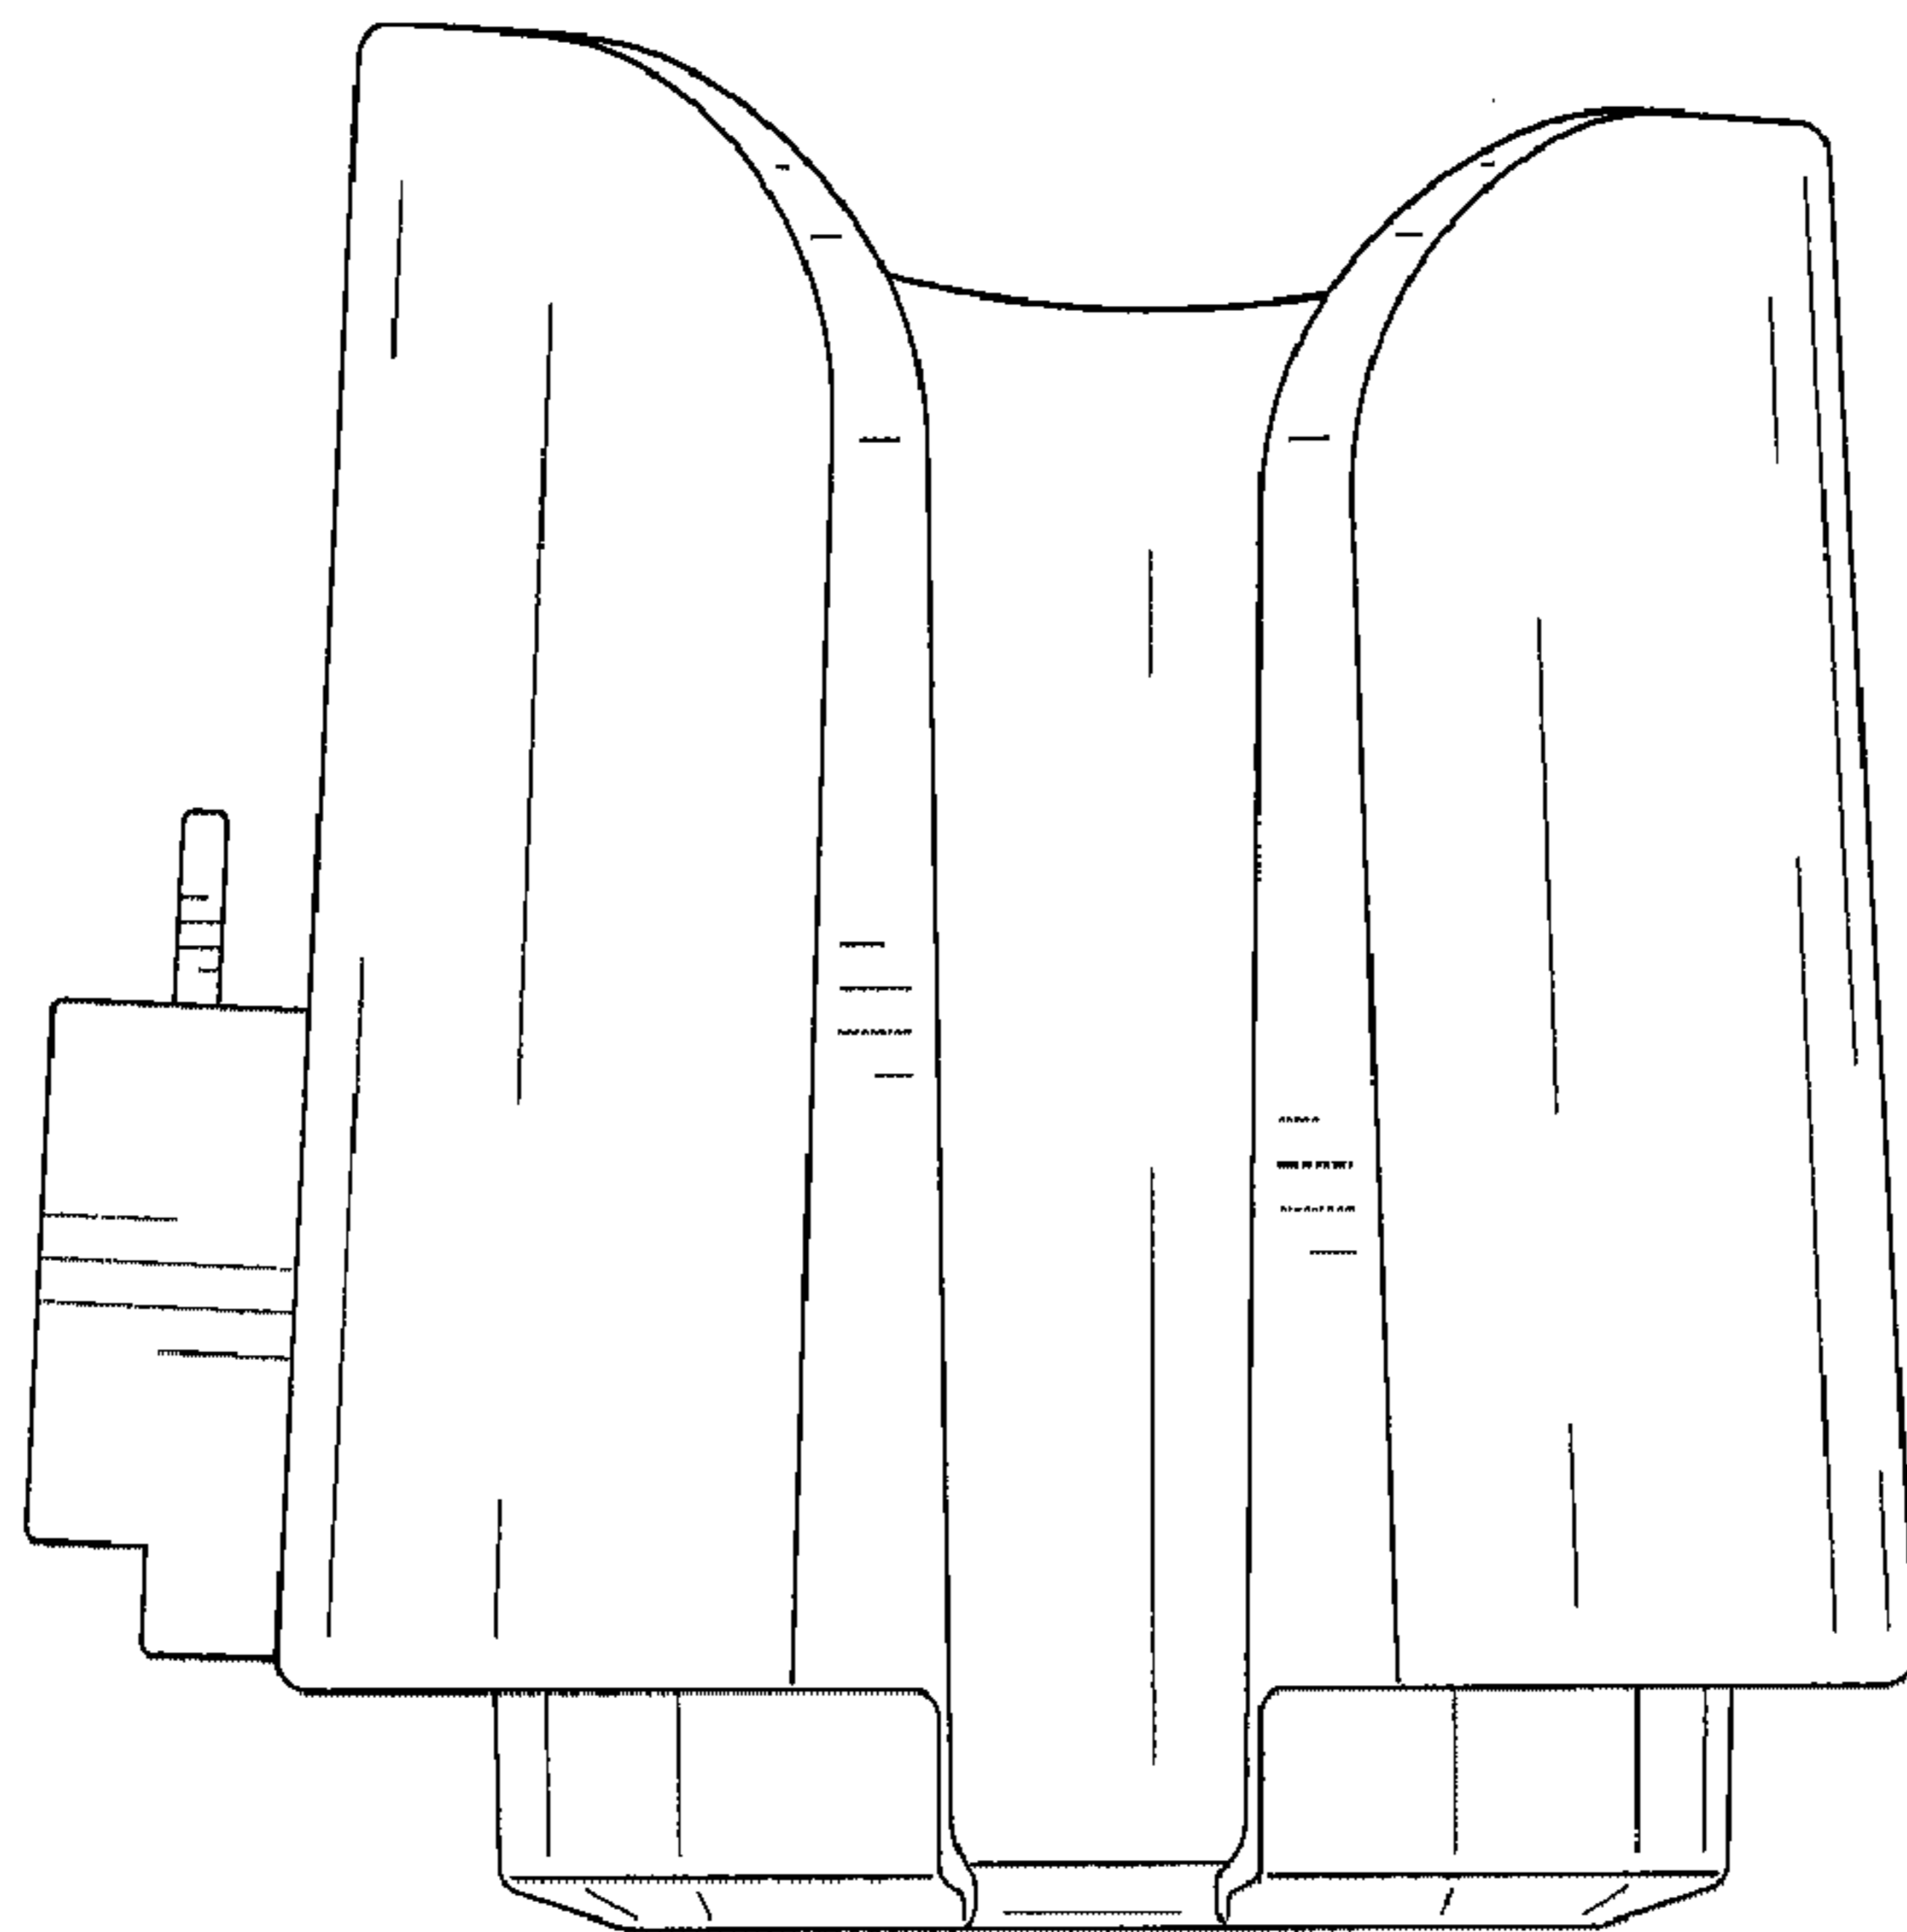


FIG.6

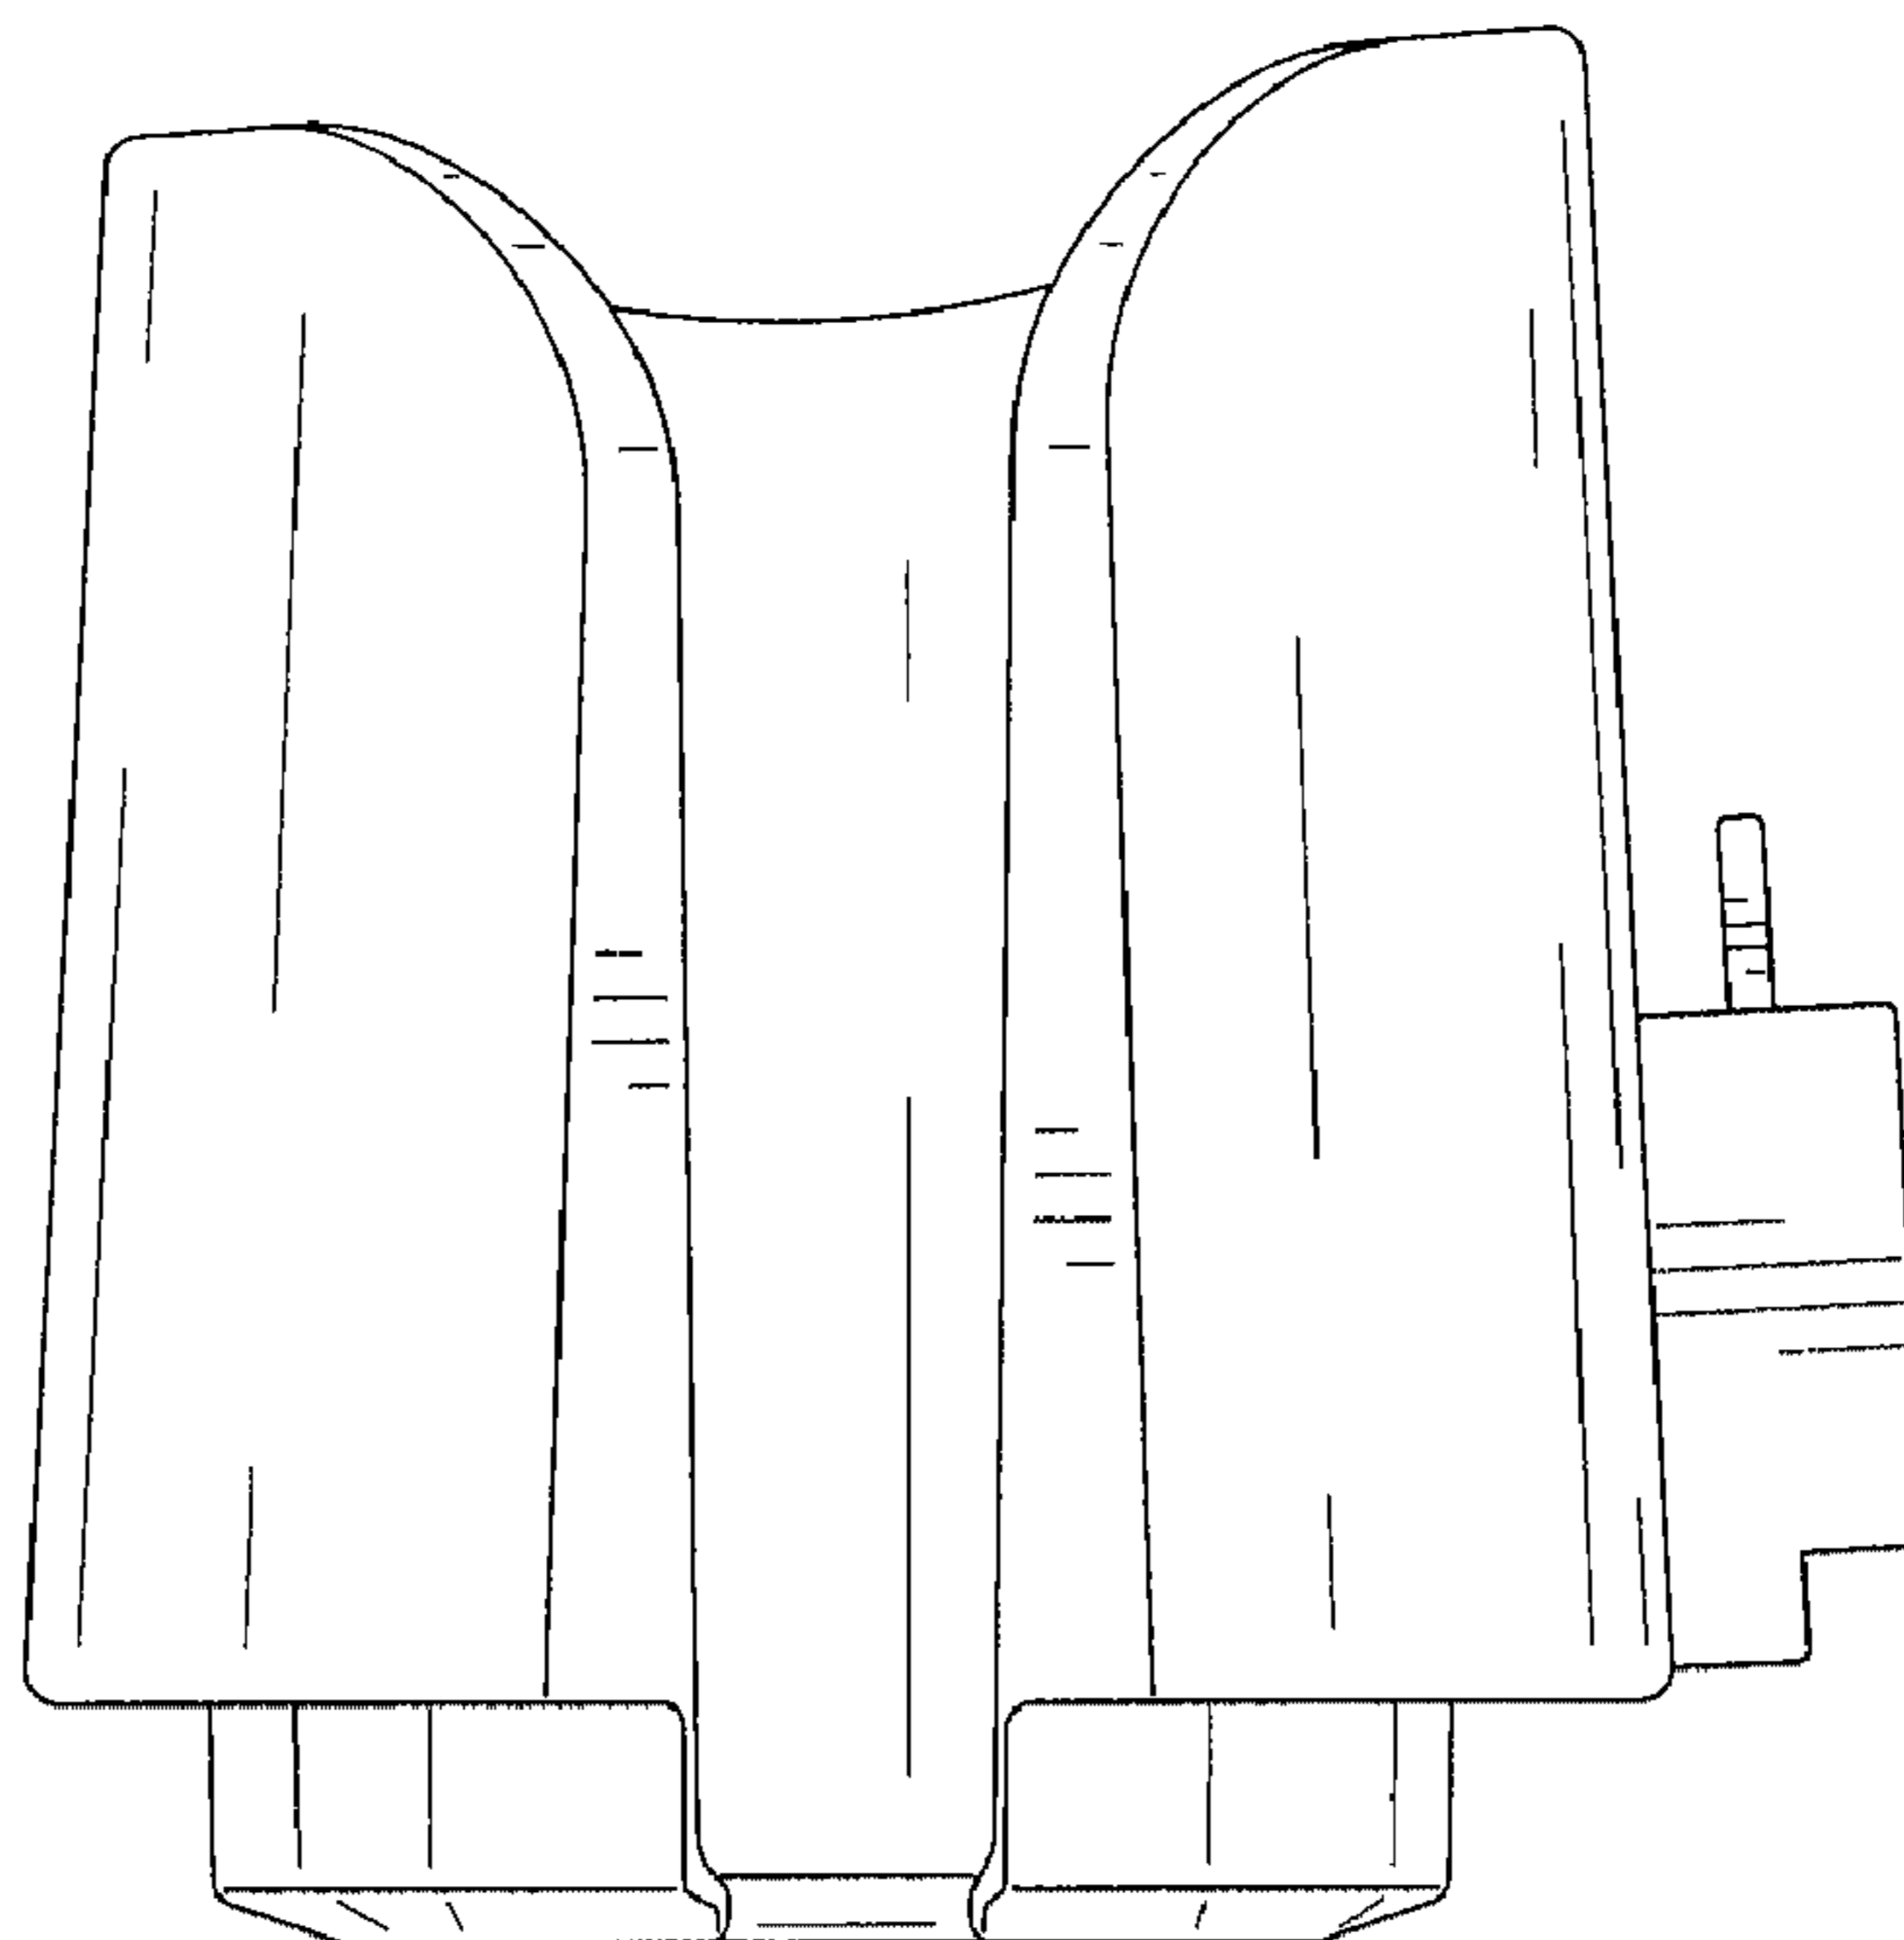


FIG.7

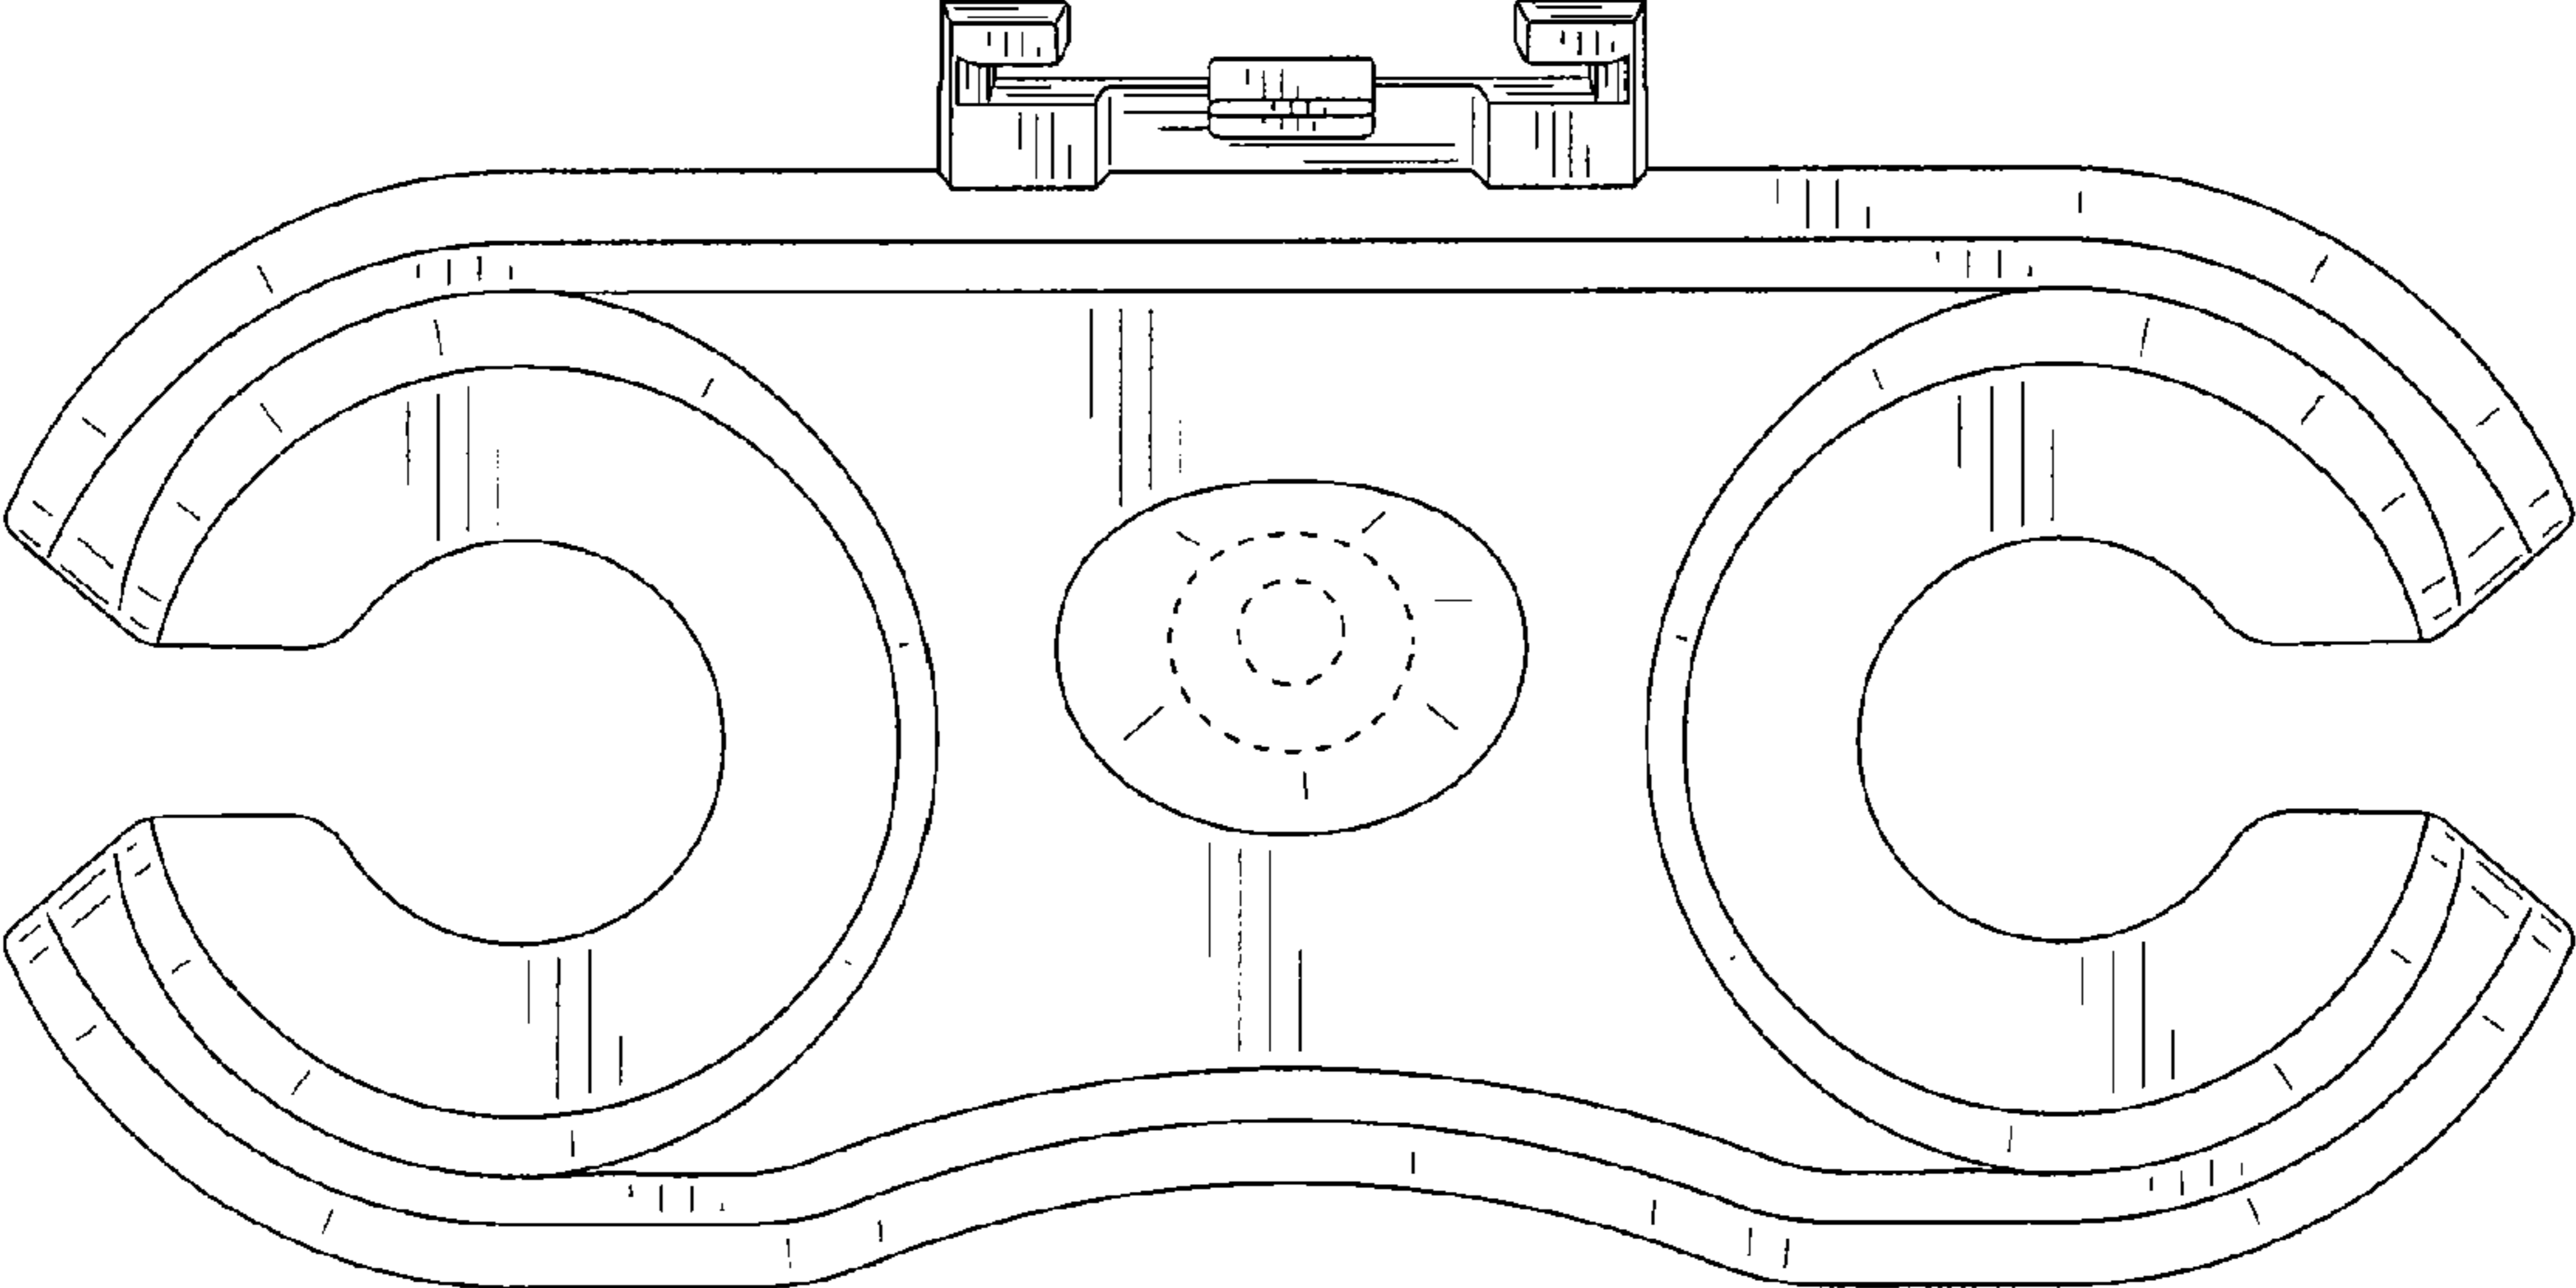


FIG.8

