



US00D654183S

(12) **United States Design Patent**  
**Oonuma et al.**

(10) **Patent No.:** **US D654,183 S**

(45) **Date of Patent:** **\*\* Feb. 14, 2012**

(54) **REAGENT AUTOLOADER WITH A SAMPLE BUFFER UNIT FOR A CLINICAL ANALYZER**

2004/0081583 A1\* 4/2004 Berndt et al. .... 422/63  
2009/0269841 A1\* 10/2009 Wojciechowski et al. . 435/289.1  
2009/0325274 A1\* 12/2009 Hamada et al. .... 422/65

(75) Inventors: **Mitsuru Oonuma**, Tokyo (JP); **Akira Omachi**, Komae (JP); **Hiroshi Watanabe**, Hitachinaka (JP); **Masanori Akutsu**, Hitachinaka (JP); **Shigeki Matsubara**, Hitachinaka (JP)

**FOREIGN PATENT DOCUMENTS**

JP D1029815 1/1999

**OTHER PUBLICATIONS**

U.S. Appl. No. 29/383,151, filed Jan. 13, 2011, Oonuma et al. copending.

U.S. Appl. No. 29/383,169, filed Jan. 13, 2011, Oonuma et al. copending.

\* cited by examiner

*Primary Examiner* — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Antonelli, Terry, Stout & Kraus, LLP.

(73) Assignee: **Hitachi High-Technologies Corporation**, Tokyo (JP)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/383,163**

(22) Filed: **Jan. 13, 2011**

(30) **Foreign Application Priority Data**

Jul. 23, 2010 (JP) ..... 2010-017873

(51) **LOC (9) Cl.** ..... **24-01**

(52) **U.S. Cl.** ..... **D24/216**

(58) **Field of Classification Search** ..... D24/216,  
D24/224, 231, 232, 186, 107, 169, 217, 233;  
D10/46, 81; 422/500, 547, 62-65, 67; 435/287.1,  
435/287.3; 436/43, 45, 47

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

4,946,651 A \* 8/1990 Liston et al. .... 422/63  
D347,478 S \* 5/1994 Pinkney ..... D24/216  
D356,967 S \* 4/1995 Takekoshi et al. .... D10/81  
6,521,183 B1 \* 2/2003 Burri et al. .... 422/65  
D508,999 S \* 8/2005 Fanning et al. .... D24/216  
D607,569 S \* 1/2010 Yukikado et al. .... D24/186  
7,678,331 B2 \* 3/2010 Shanafelter ..... 422/65  
D638,545 S \* 5/2011 Okawa et al. .... D24/186

**CLAIM**

We claim the ornamental design for a reagent autoloader with a sample buffer unit for a clinical analyzer, as shown and described.

**DESCRIPTION**

FIG. 1 is a front, top and left side perspective view of a reagent autoloader with a sample buffer unit for a clinical analyzer showing our new design;

FIG. 2 is a front elevational view thereof;

FIG. 3 is a rear elevational view thereof;

FIG. 4 is a top plan view thereof;


FIG. 5 is a bottom plan view thereof;


FIG. 6 is a left side elevational view thereof; and,

FIG. 7 is a right side elevational view thereof.


The broken lines in all drawing views are included for the purpose of illustrating portions of the reagent autoloader with a sample buffer unit for a clinical analyzer that form no part of the claimed design.

**1 Claim, 5 Drawing Sheets**

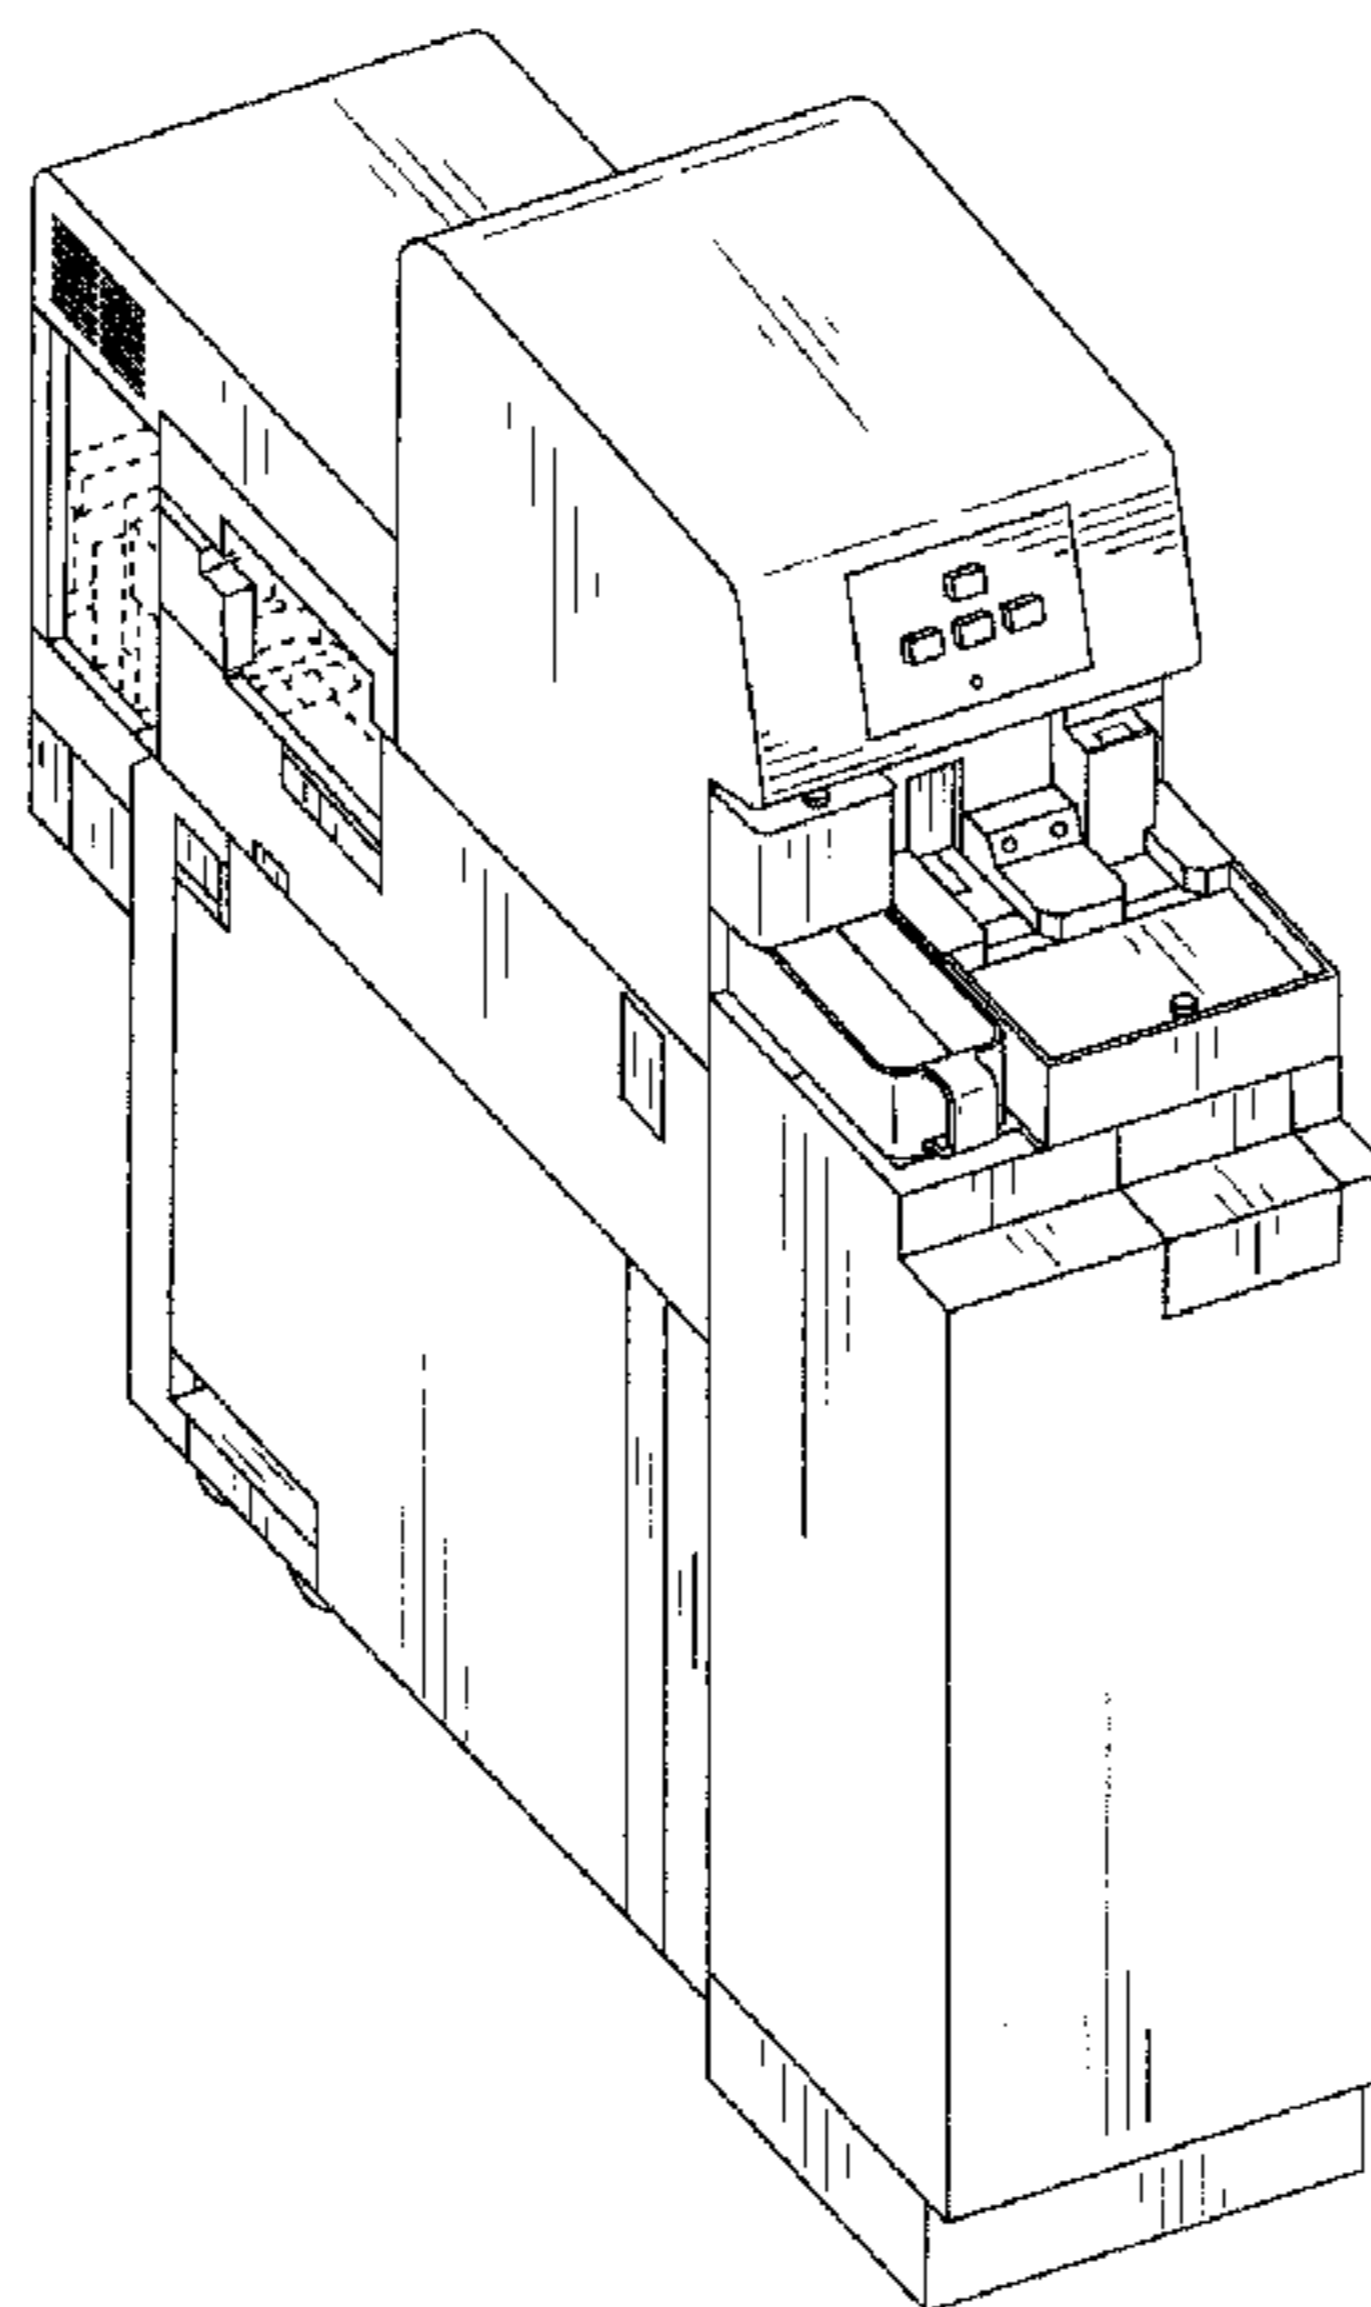


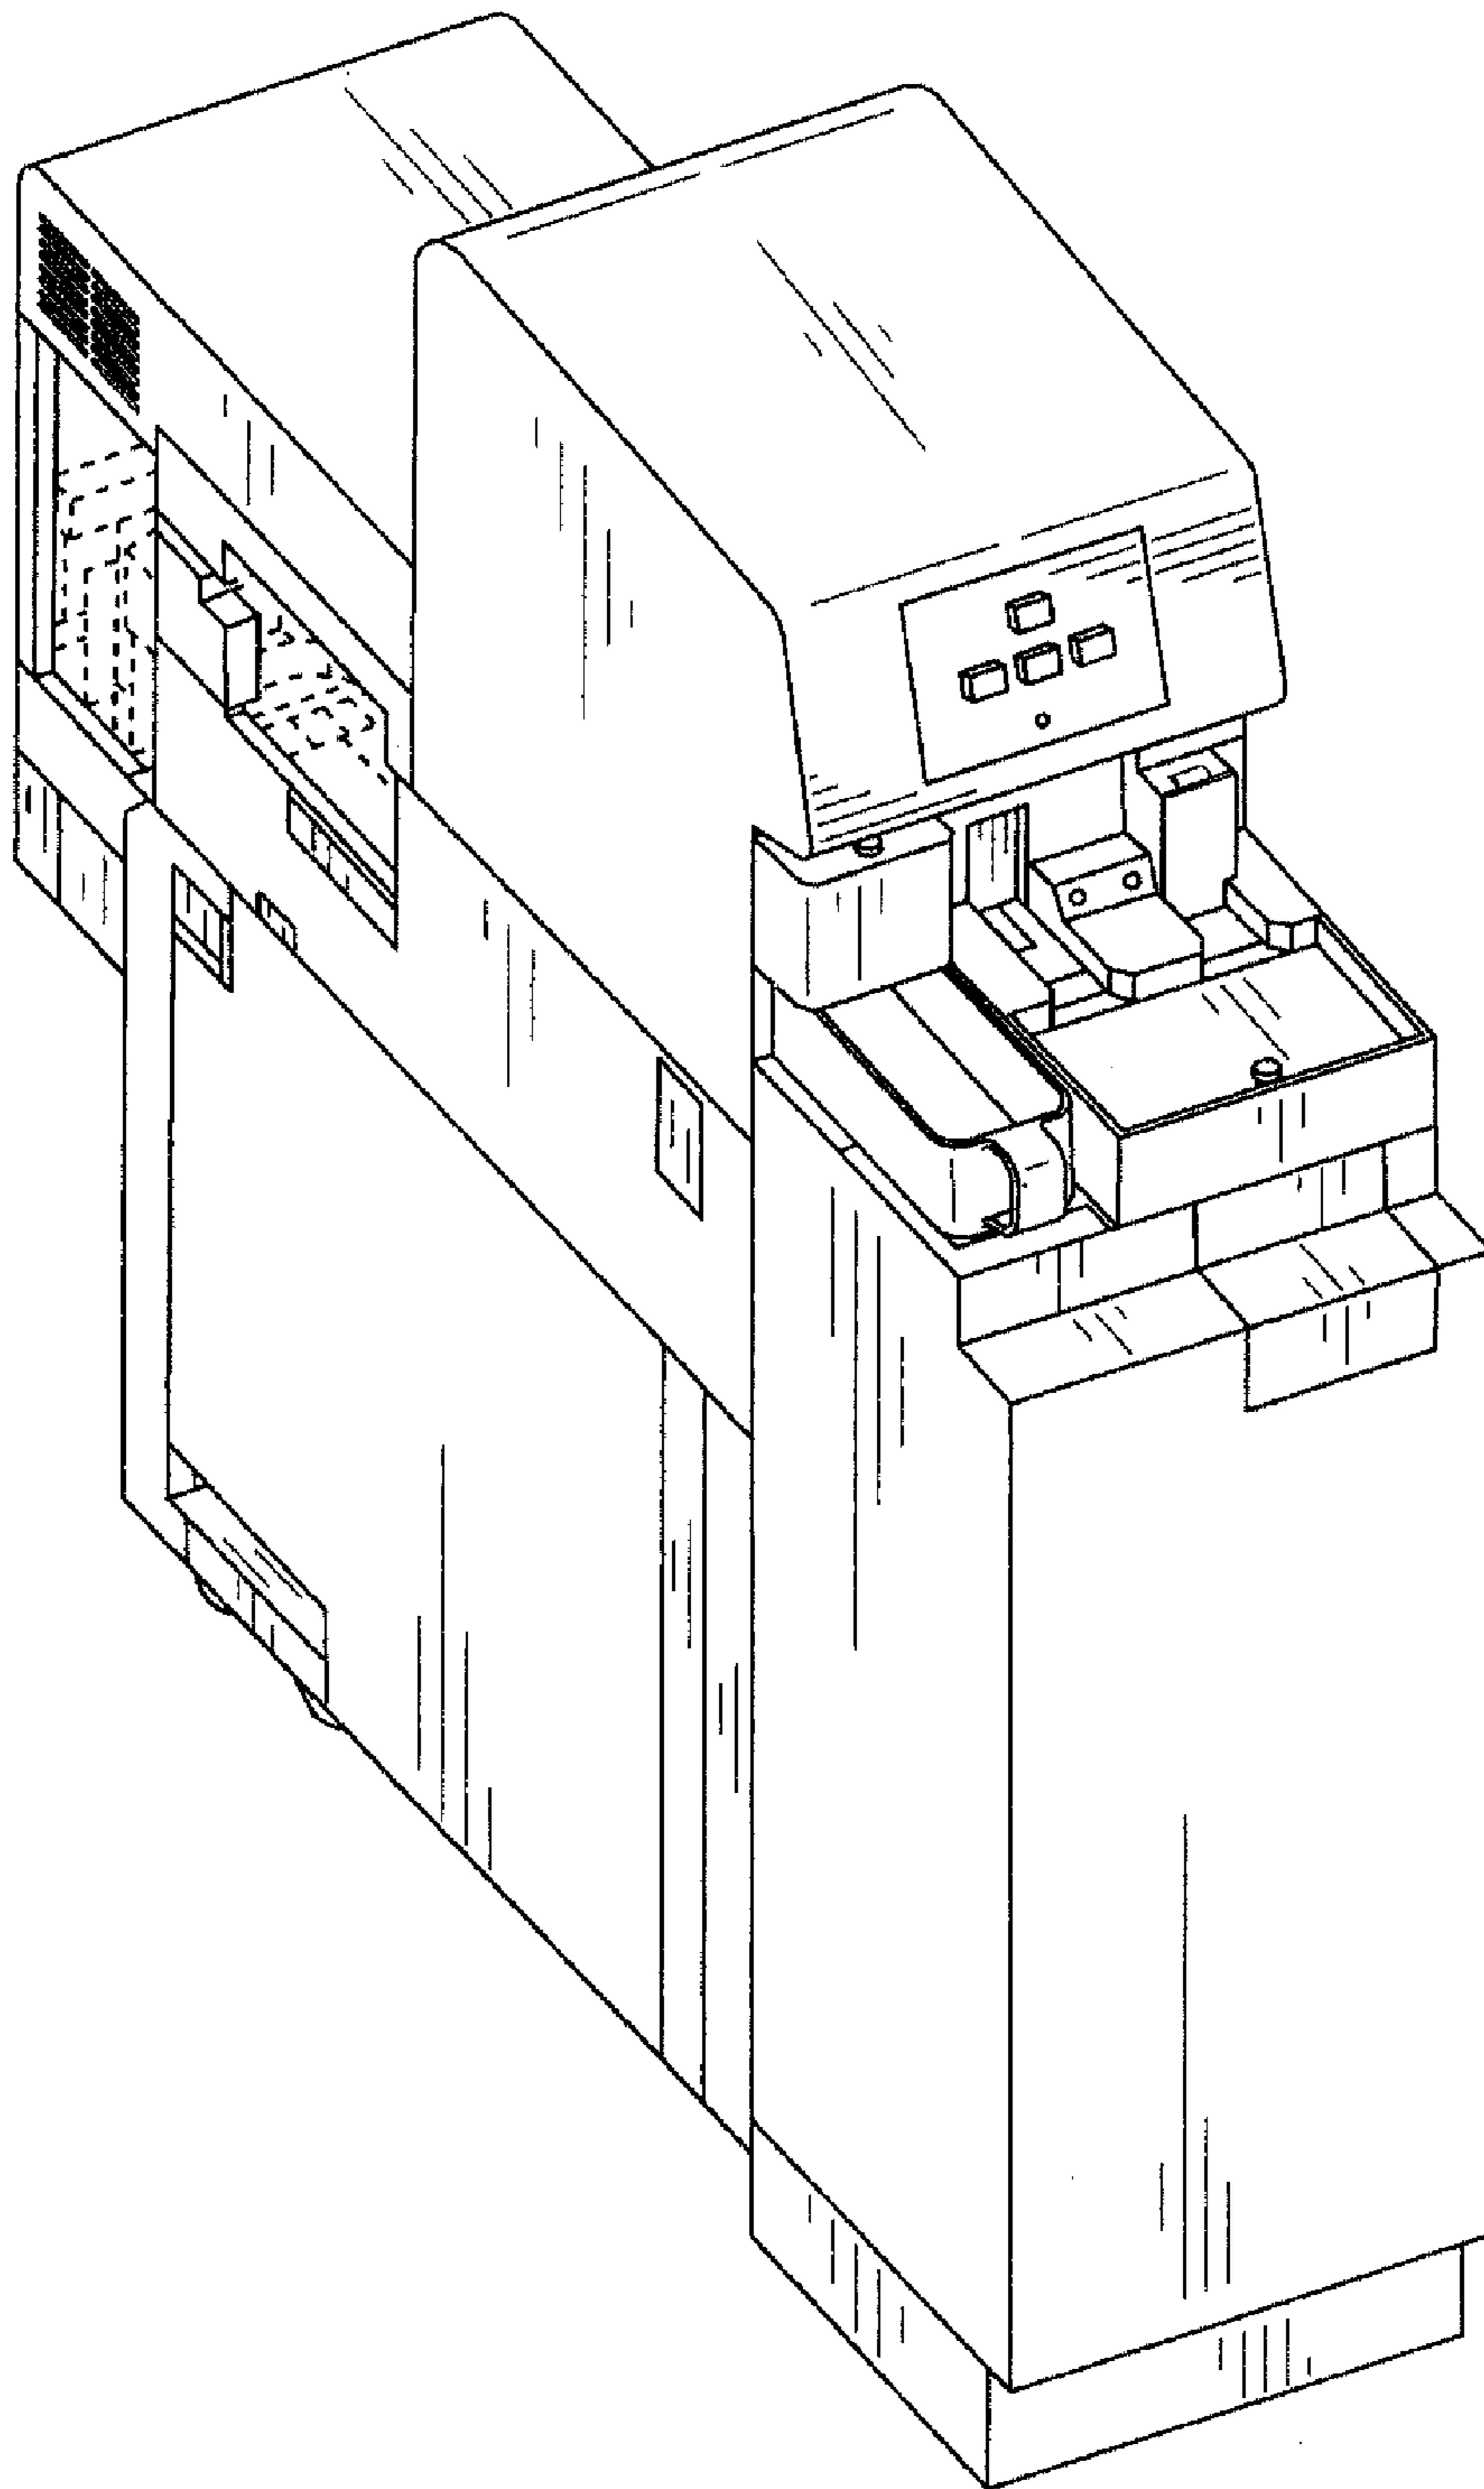


**FIG. 1**

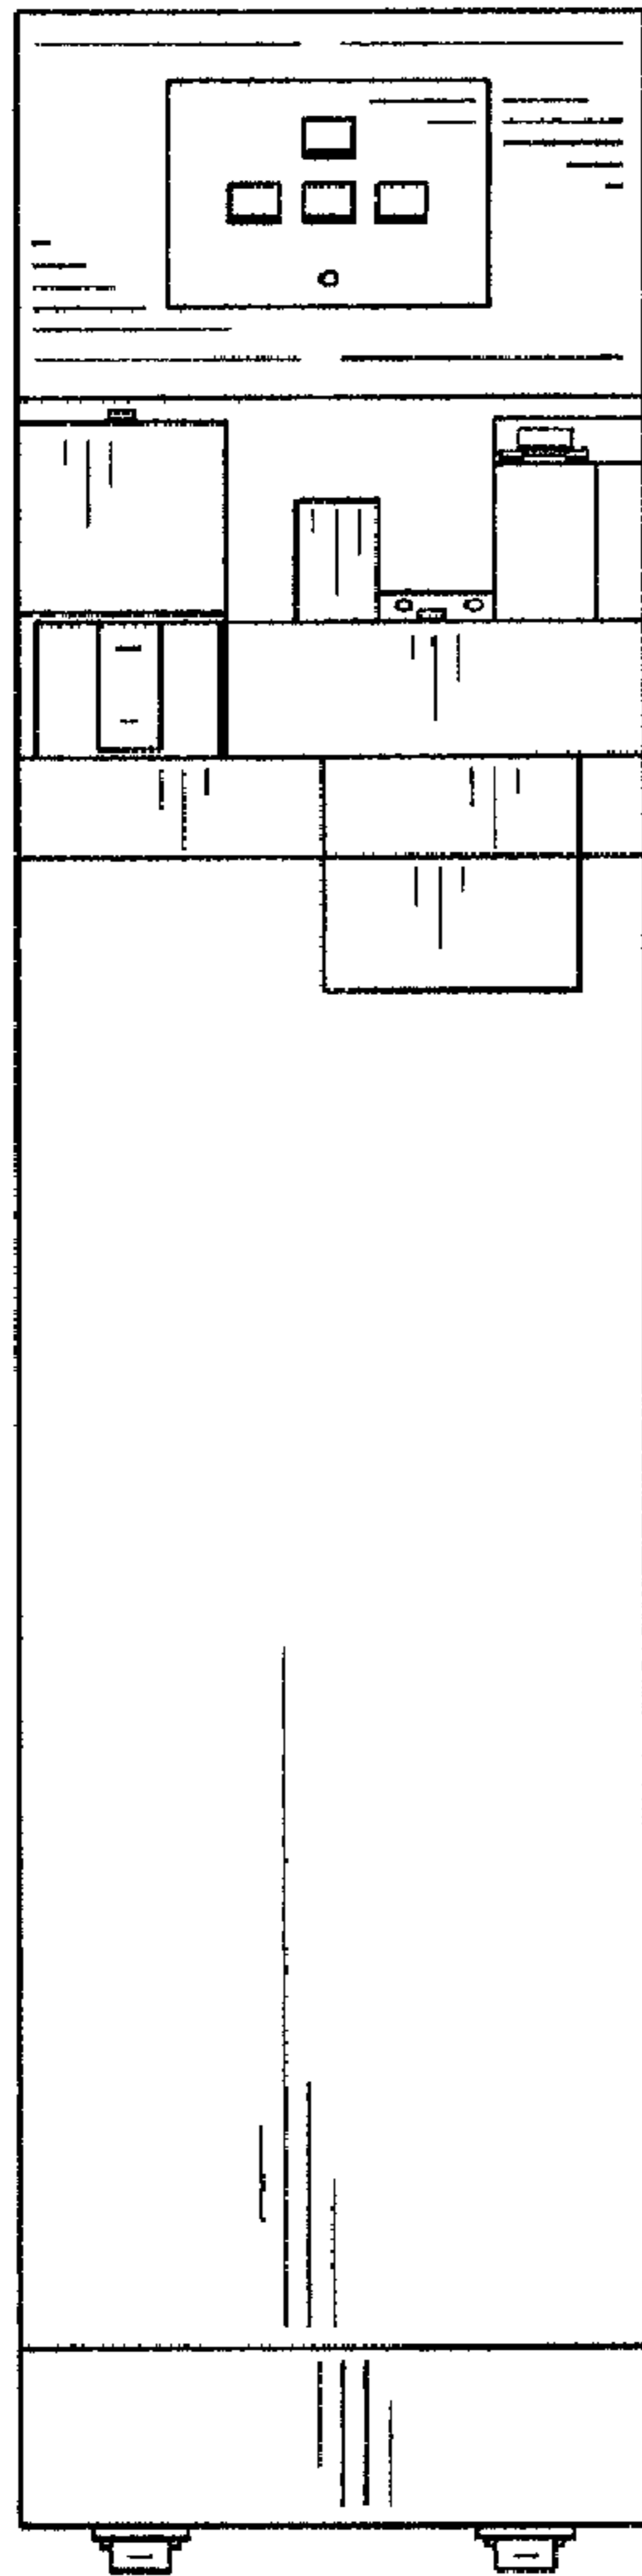


**FIG. 2**

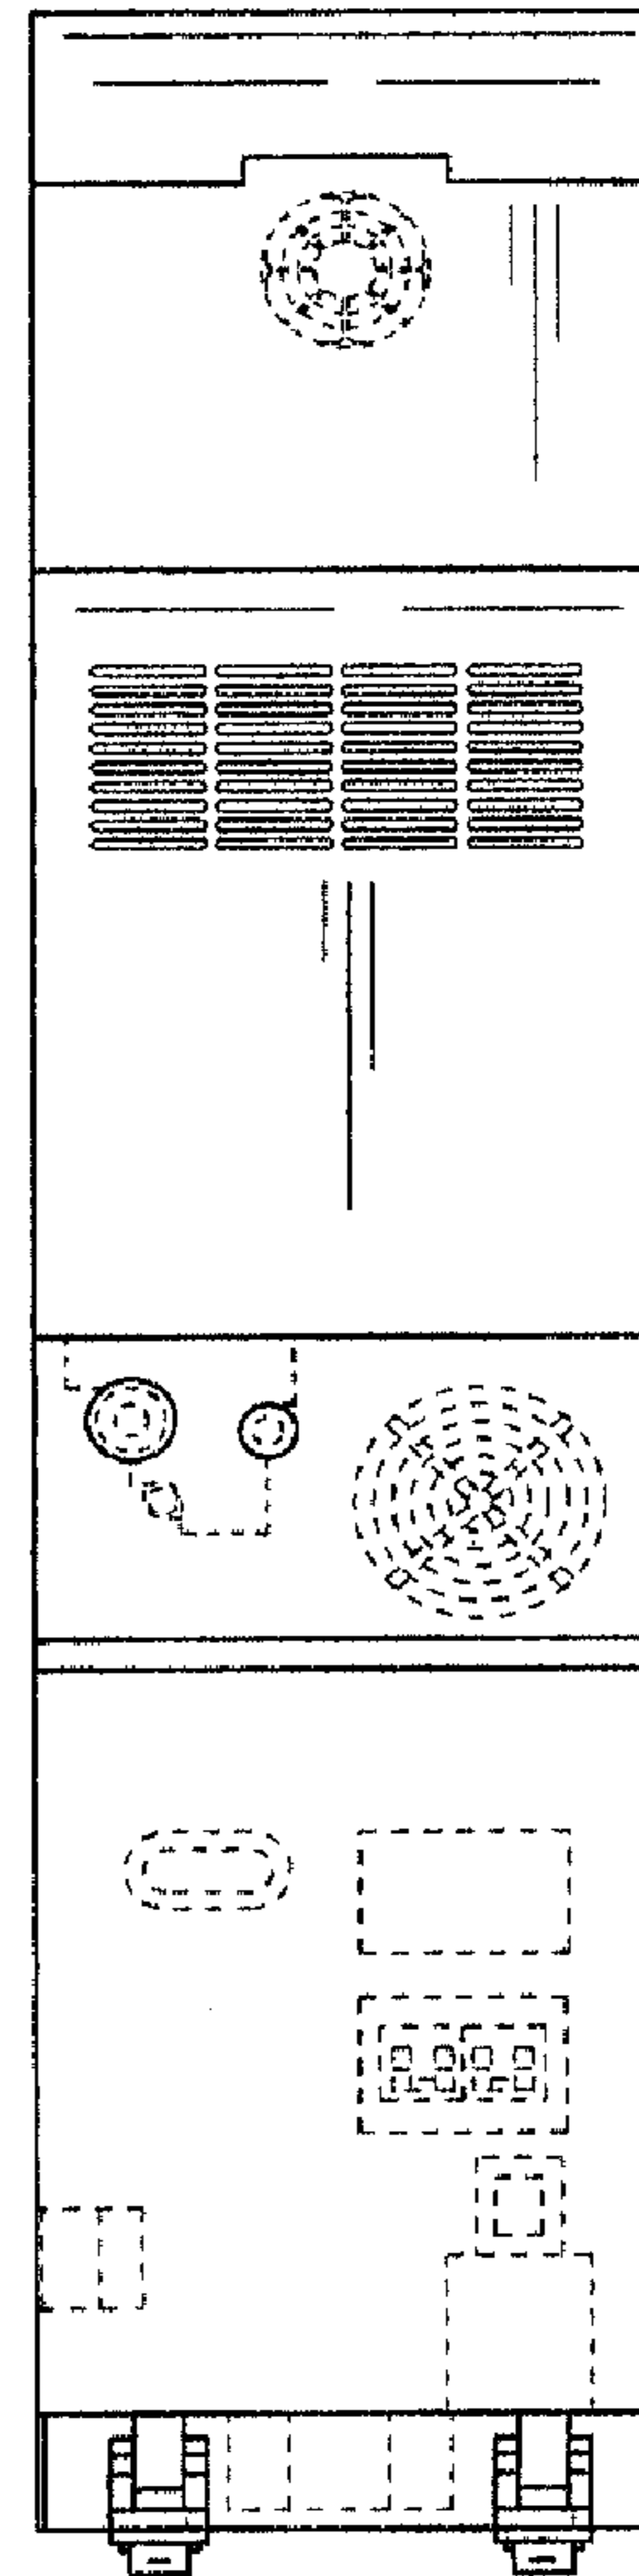


**FIG. 3**

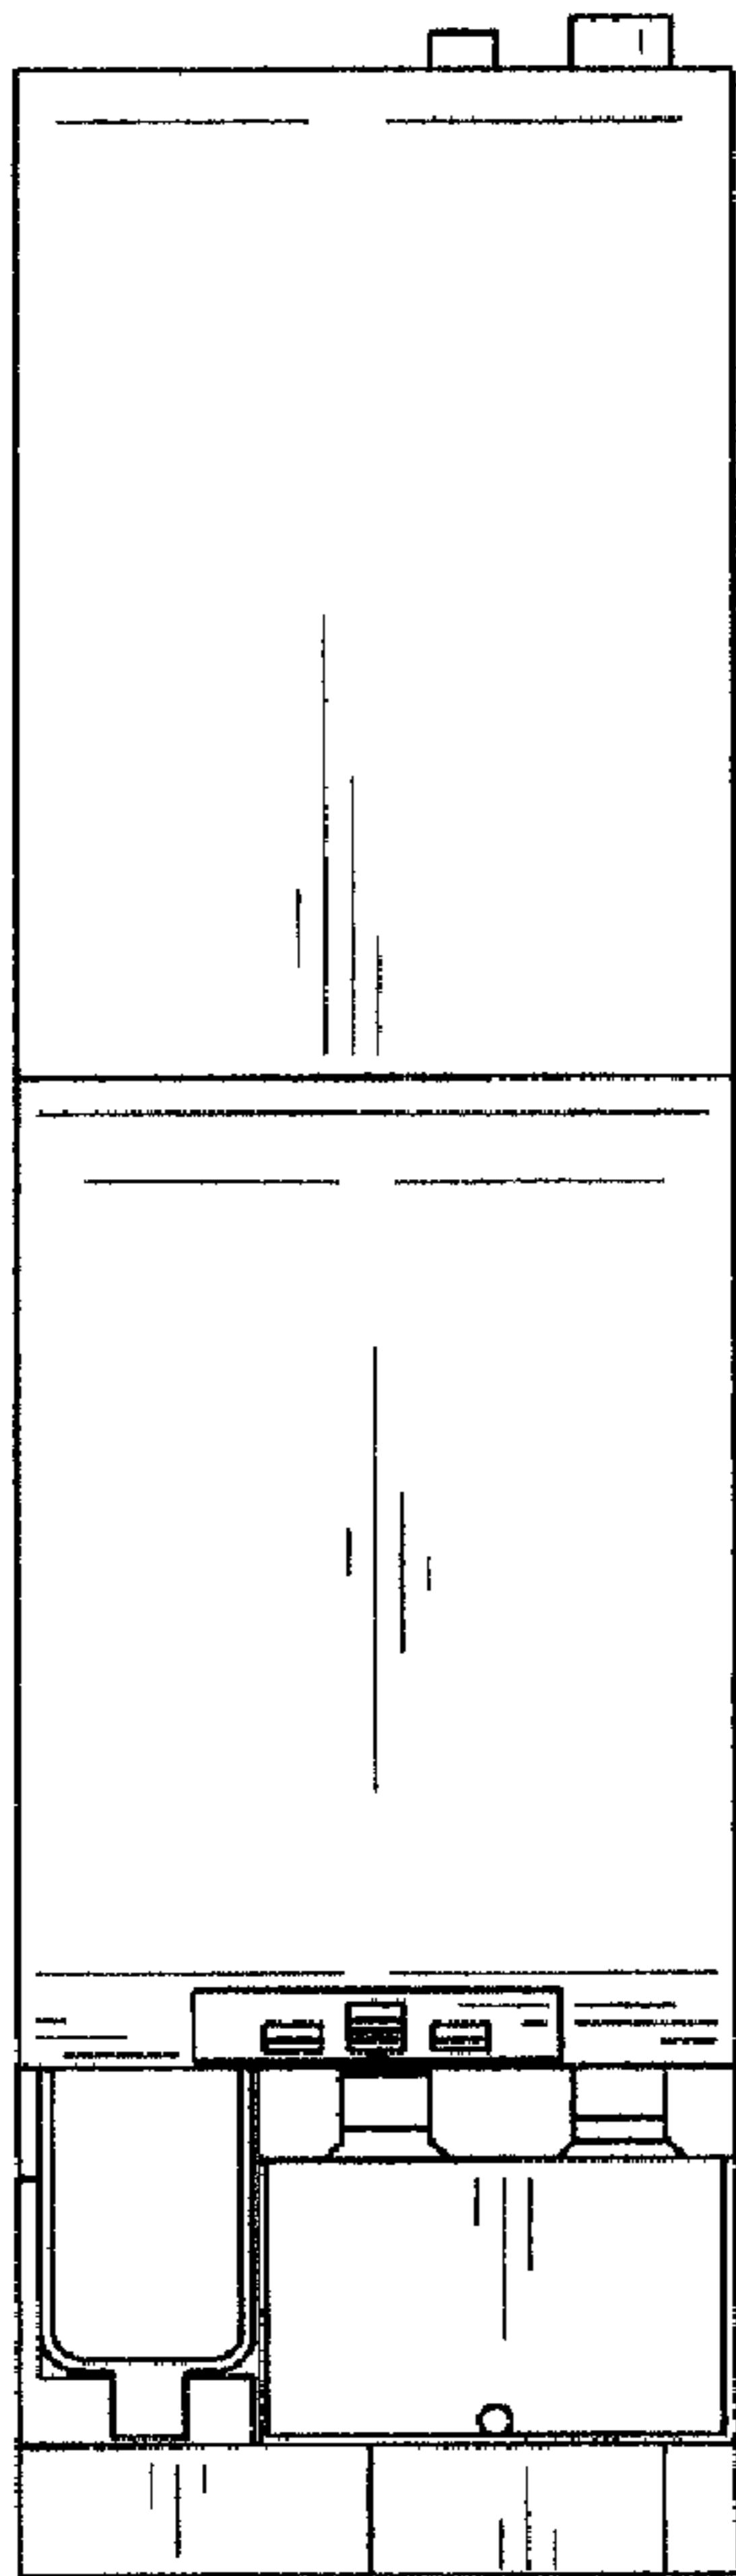


**FIG. 4**

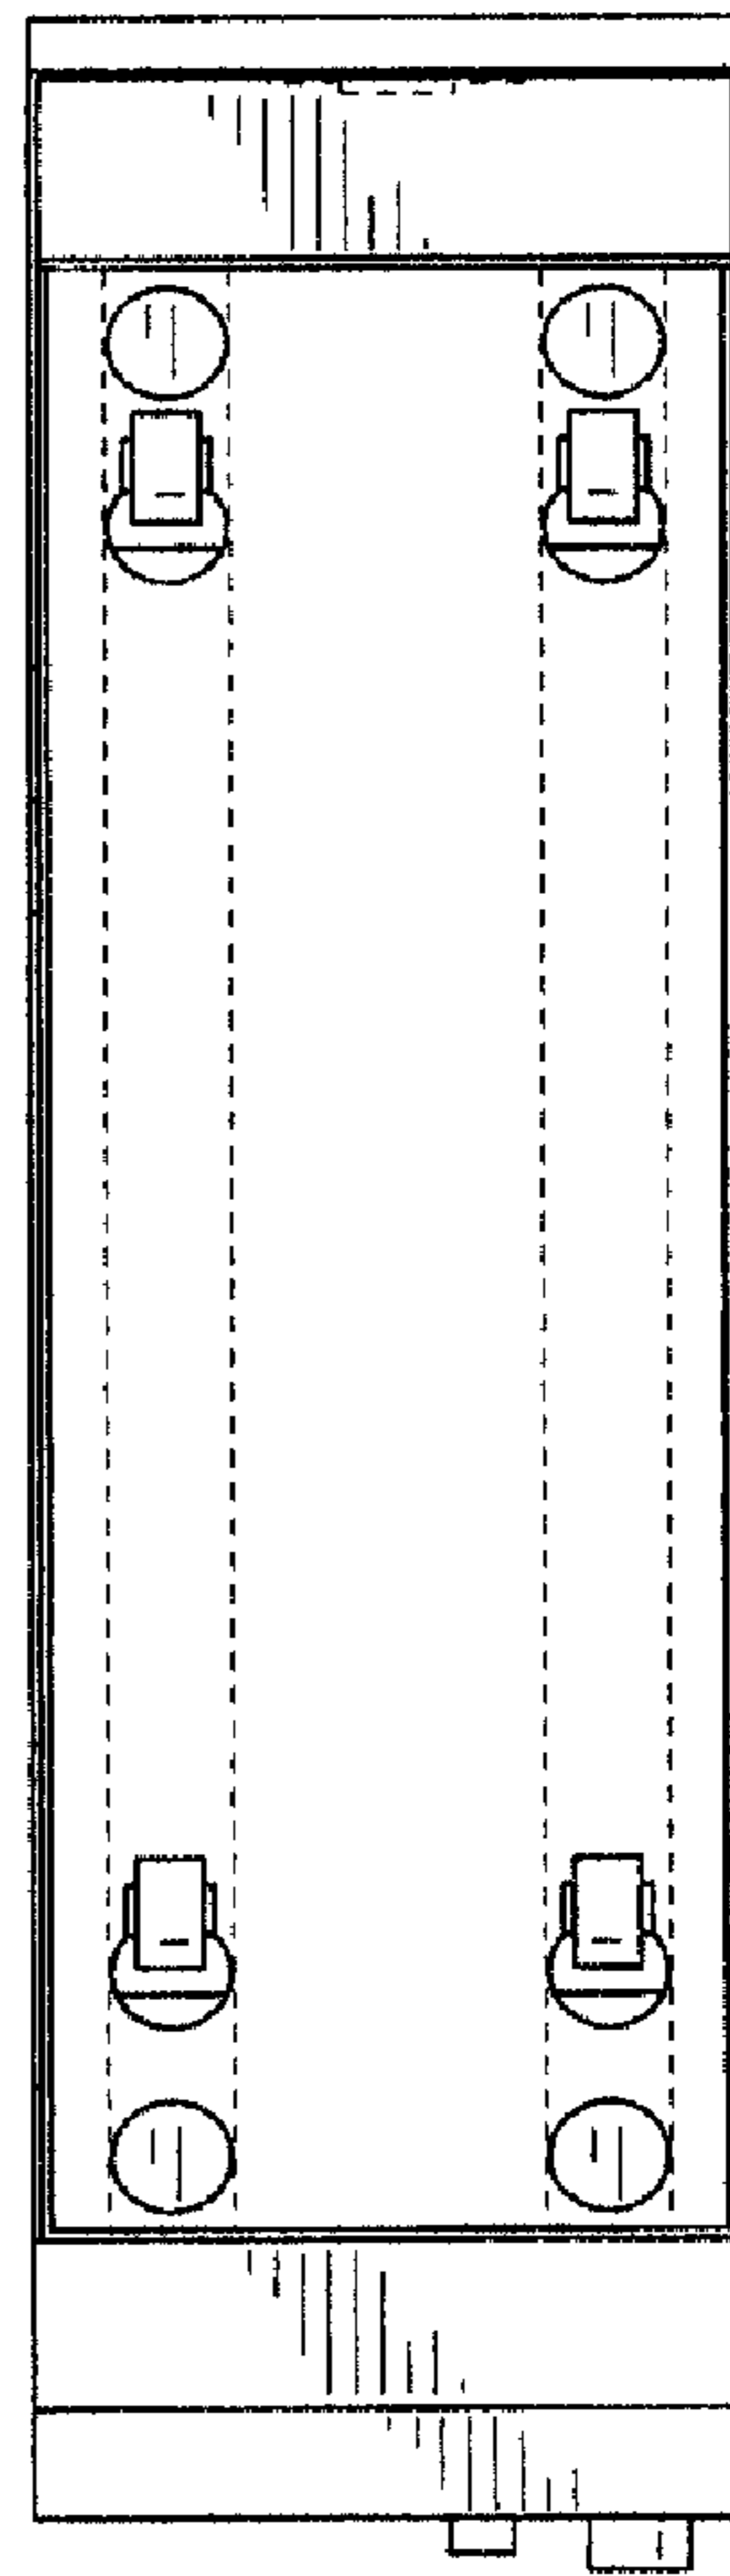

**FIG. 5**

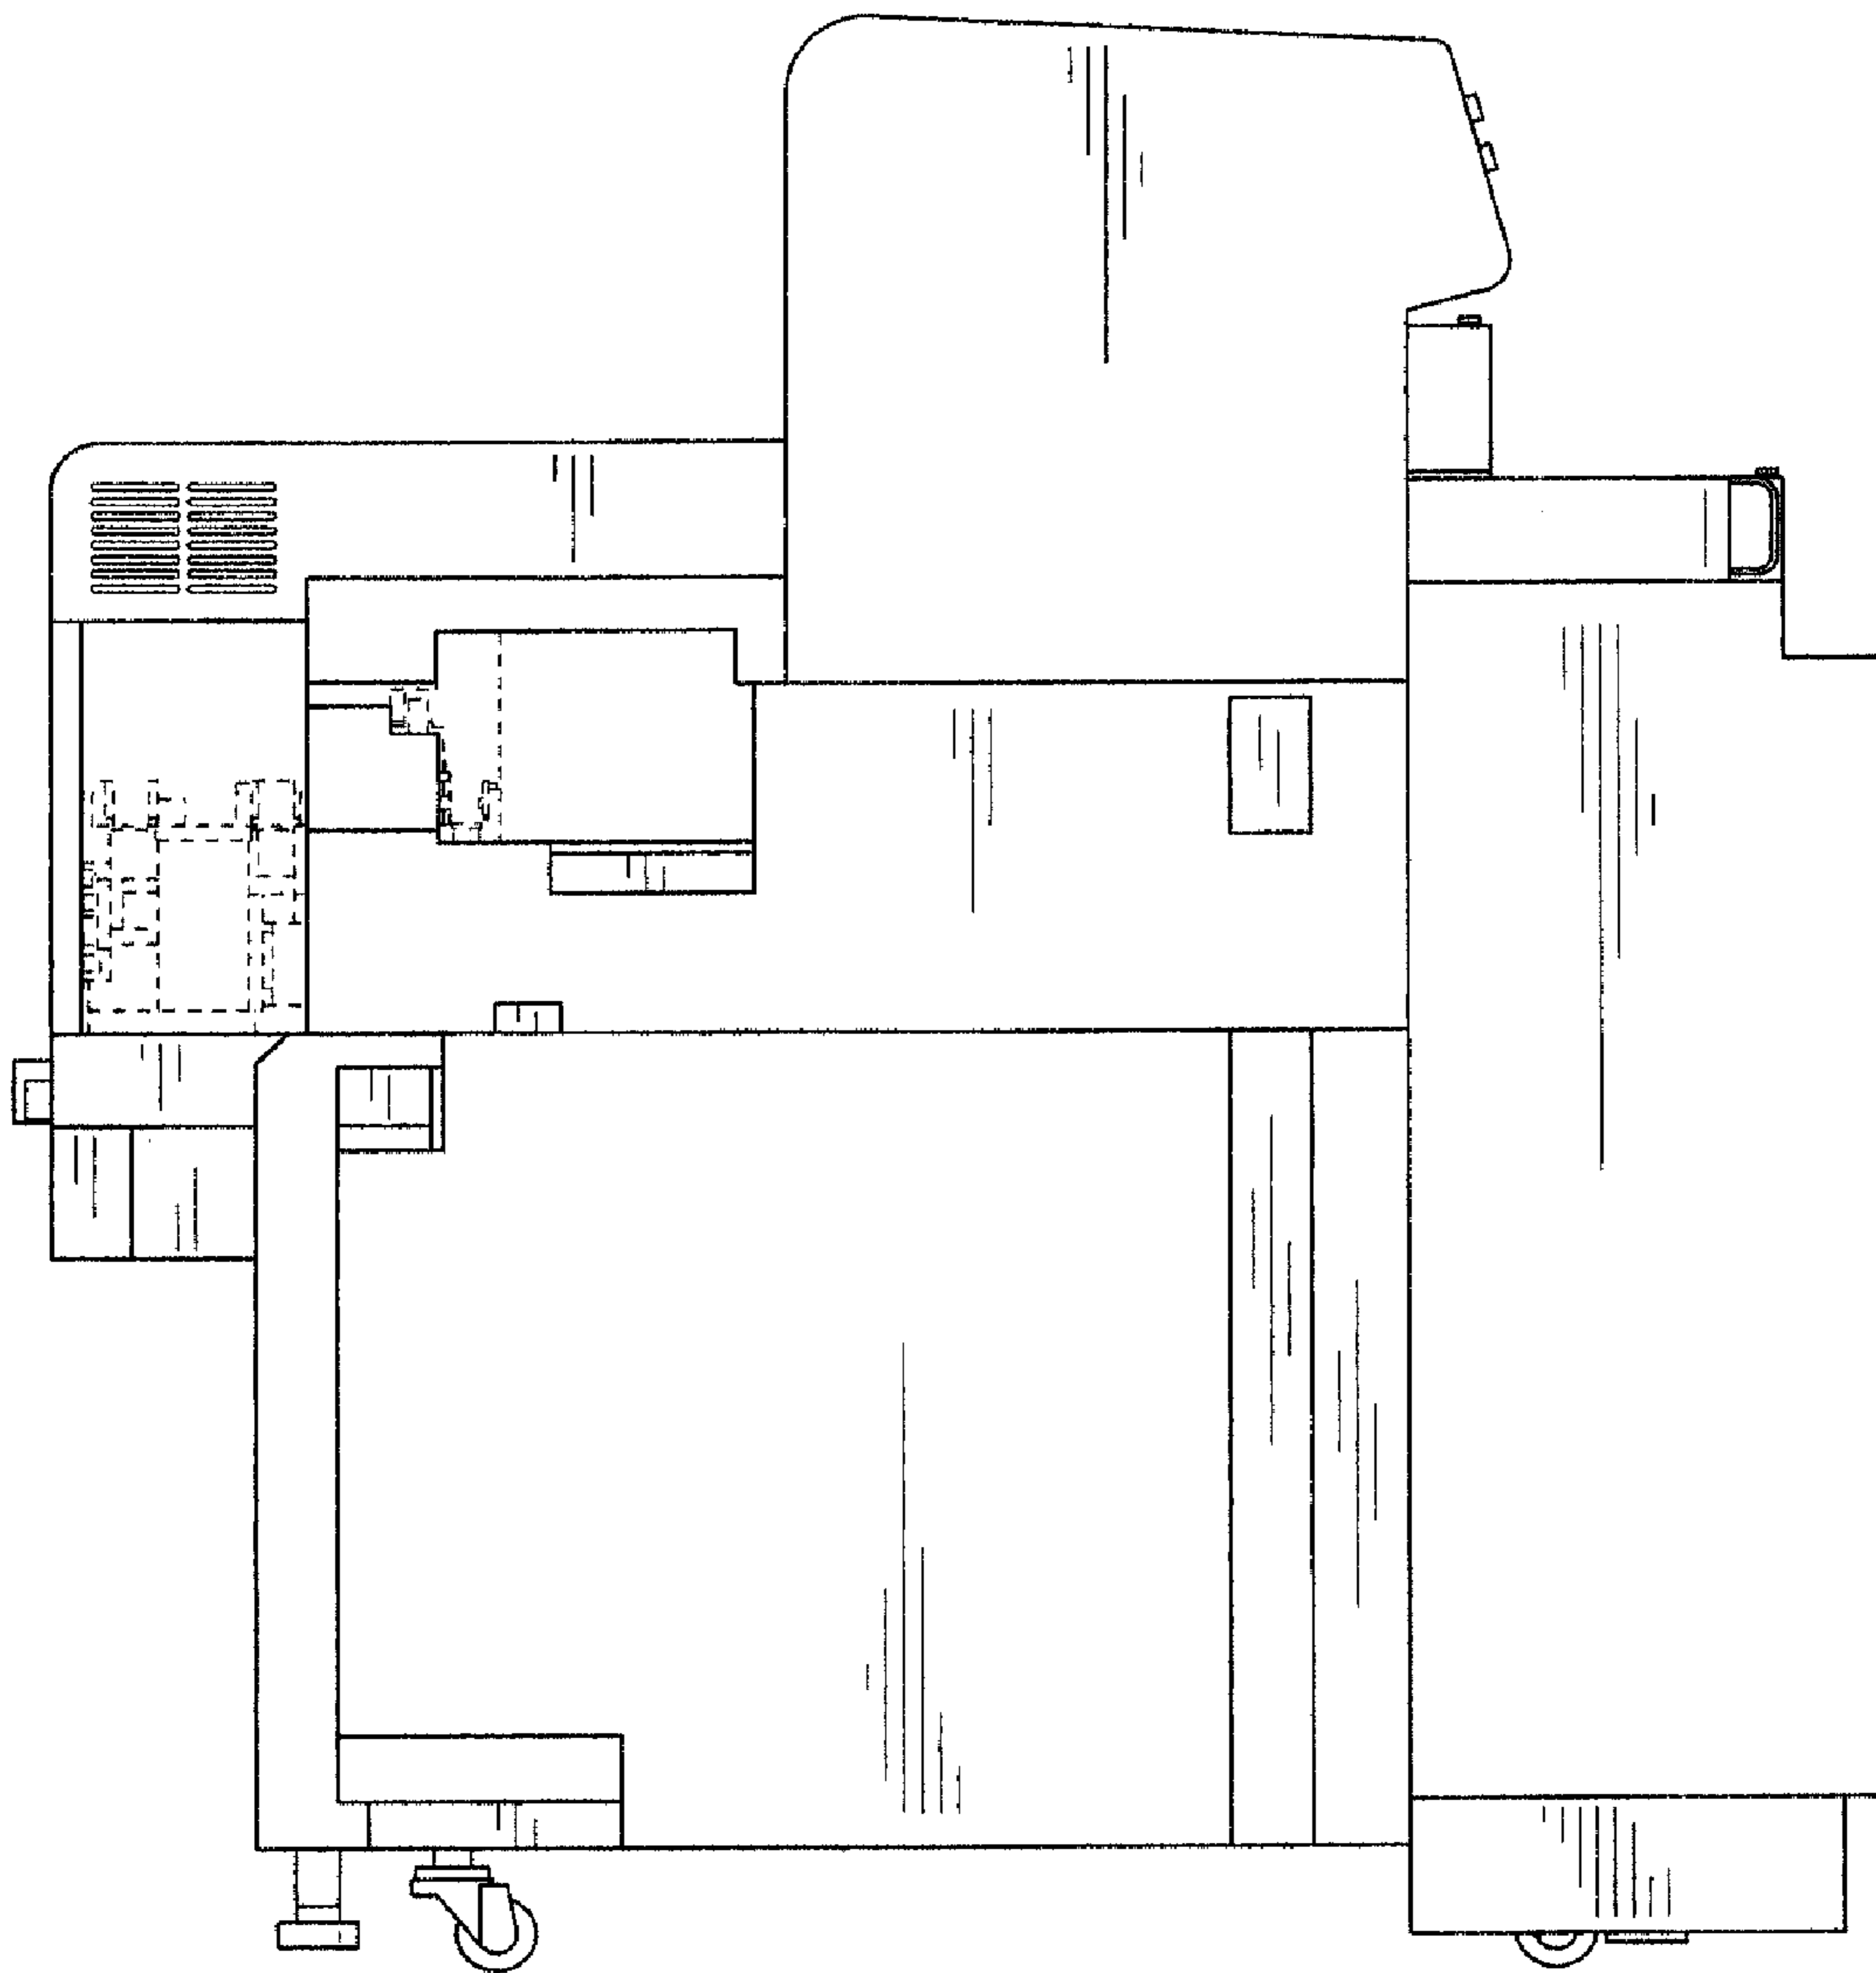

**FIG. 6**

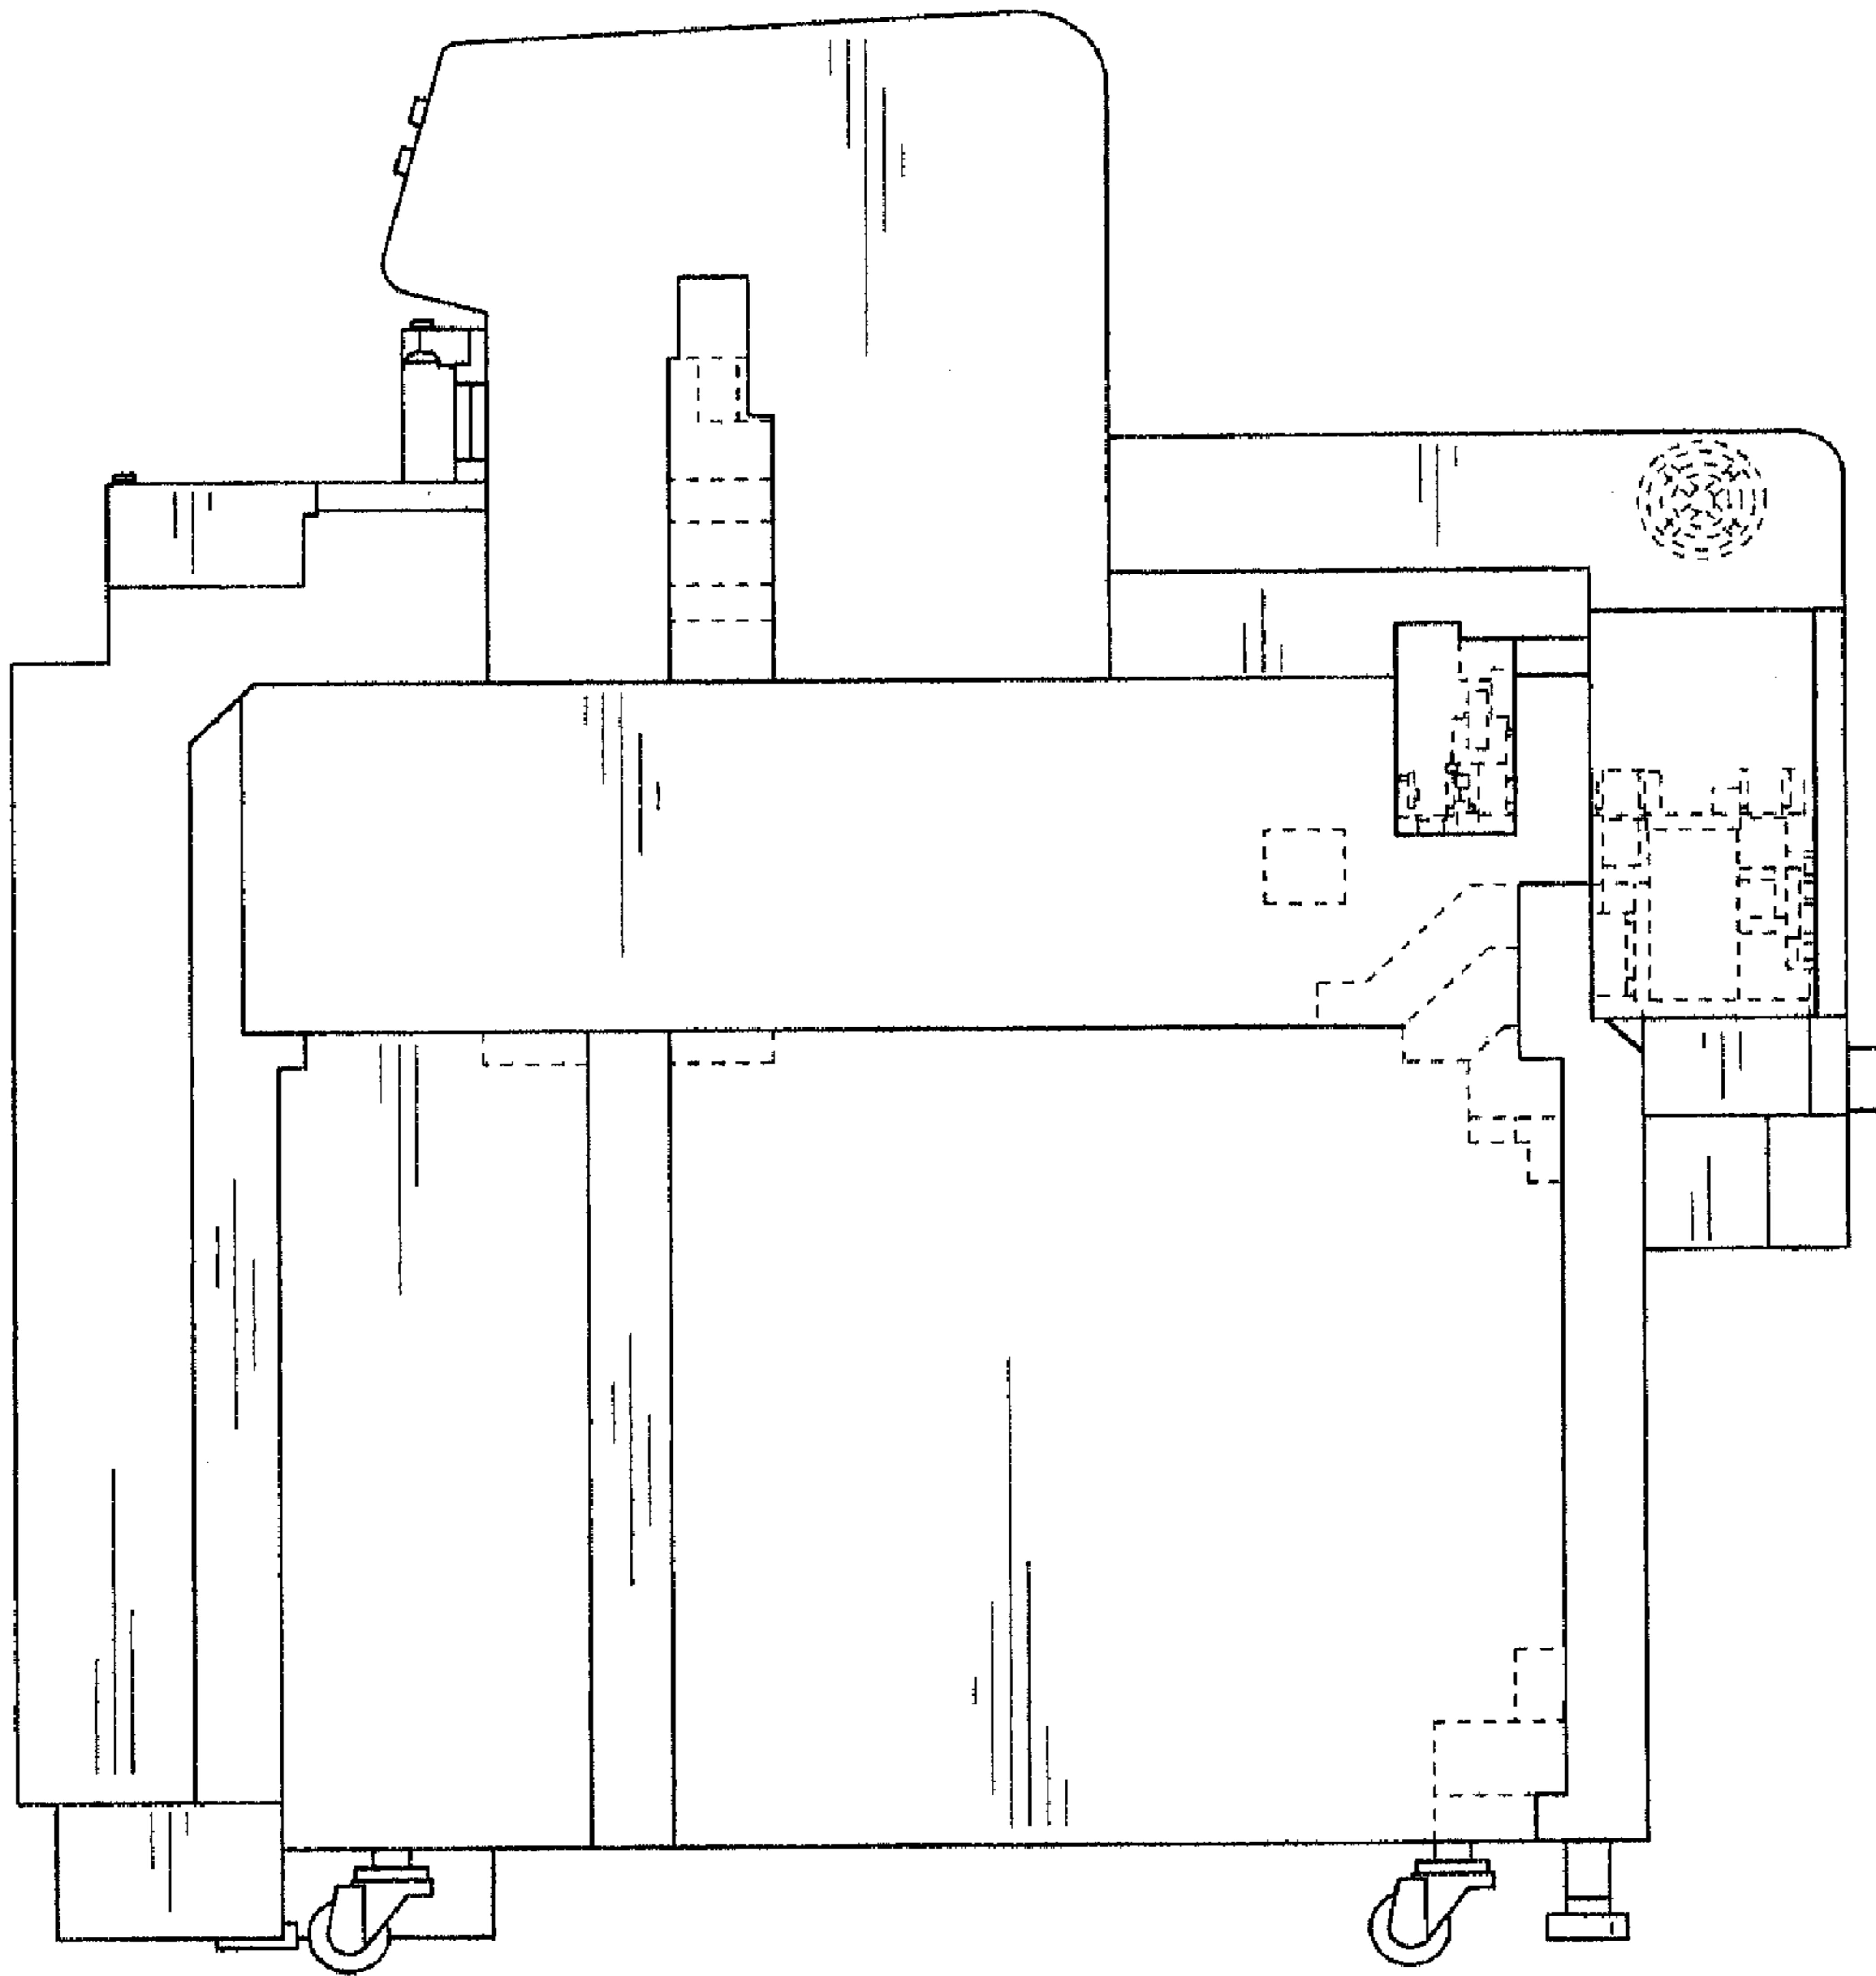

**FIG. 7**