



US00D654593S

(12) **United States Design Patent**
Kawasaki

(10) **Patent No.:** **US D654,593 S**

(45) **Date of Patent:** **** Feb. 21, 2012**

(54) **BLOOD PRESSURE MEASURING APPARATUS**

(75) Inventor: **Kazuo Kawasaki**, Osaka (JP)

(73) Assignee: **Japan Precision Instruments Inc.**,
Shibukawa-shi (JP)

(**) Term: **14 Years**

(21) Appl. No.: **29/391,613**

(22) Filed: **May 11, 2011**

(30) **Foreign Application Priority Data**

Nov. 16, 2010 (JP) 2010-027566

(51) **LOC (9) Cl.** **24-02**

(52) **U.S. Cl.** **D24/165**

(58) **Field of Classification Search** D24/164-169,
D24/107, 186; D10/46, 98; 600/301, 481-483,
600/485, 490, 493-495, 500, 503, 509; 128/900
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

| | | | | |
|-------------------|--------|---------------|-------|---------|
| D437,414 S * | 2/2001 | Kern et al. | | D24/165 |
| D473,308 S * | 4/2003 | Nakanishi | | D24/165 |
| D520,638 S * | 5/2006 | Zeindler | | D24/166 |
| D577,440 S * | 9/2008 | Ferber et al. | | D24/165 |
| D609,343 S * | 2/2010 | Omaki | | D24/165 |
| D609,344 S * | 2/2010 | Hara | | D24/165 |
| 2009/0062664 A1 * | 3/2009 | Chang et al. | | 600/485 |

OTHER PUBLICATIONS

U.S. Appl. No. 29/391,606, filed May 11, 2011, inventor: Kazuo Kawasaki, entitled: Blood Pressure Measuring Apparatus.

* cited by examiner

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Holtz, Holtz, Goodman & Chick, PC

(57) **CLAIM**


The ornamental design for a blood pressure measuring apparatus, as shown and described.

DESCRIPTION

FIG. 1 is a front, right side, top perspective view of a blood pressure measuring apparatus showing my new design; FIG. 2 is a front elevational view thereof; FIG. 3 is a rear elevational view thereof; FIG. 4 is a left side view thereof; FIG. 5 is a right side view thereof; FIG. 6 is a top plan view thereof; and, FIG. 7 is a bottom plan view thereof.

The broken lines in the figure views are included for the purpose of illustrating portions of the blood pressure measuring apparatus that form no part of the claimed design. It is understood that the area within the broken lines in FIGS. 1 and 6 is not claimed.

1 Claim, 5 Drawing Sheets

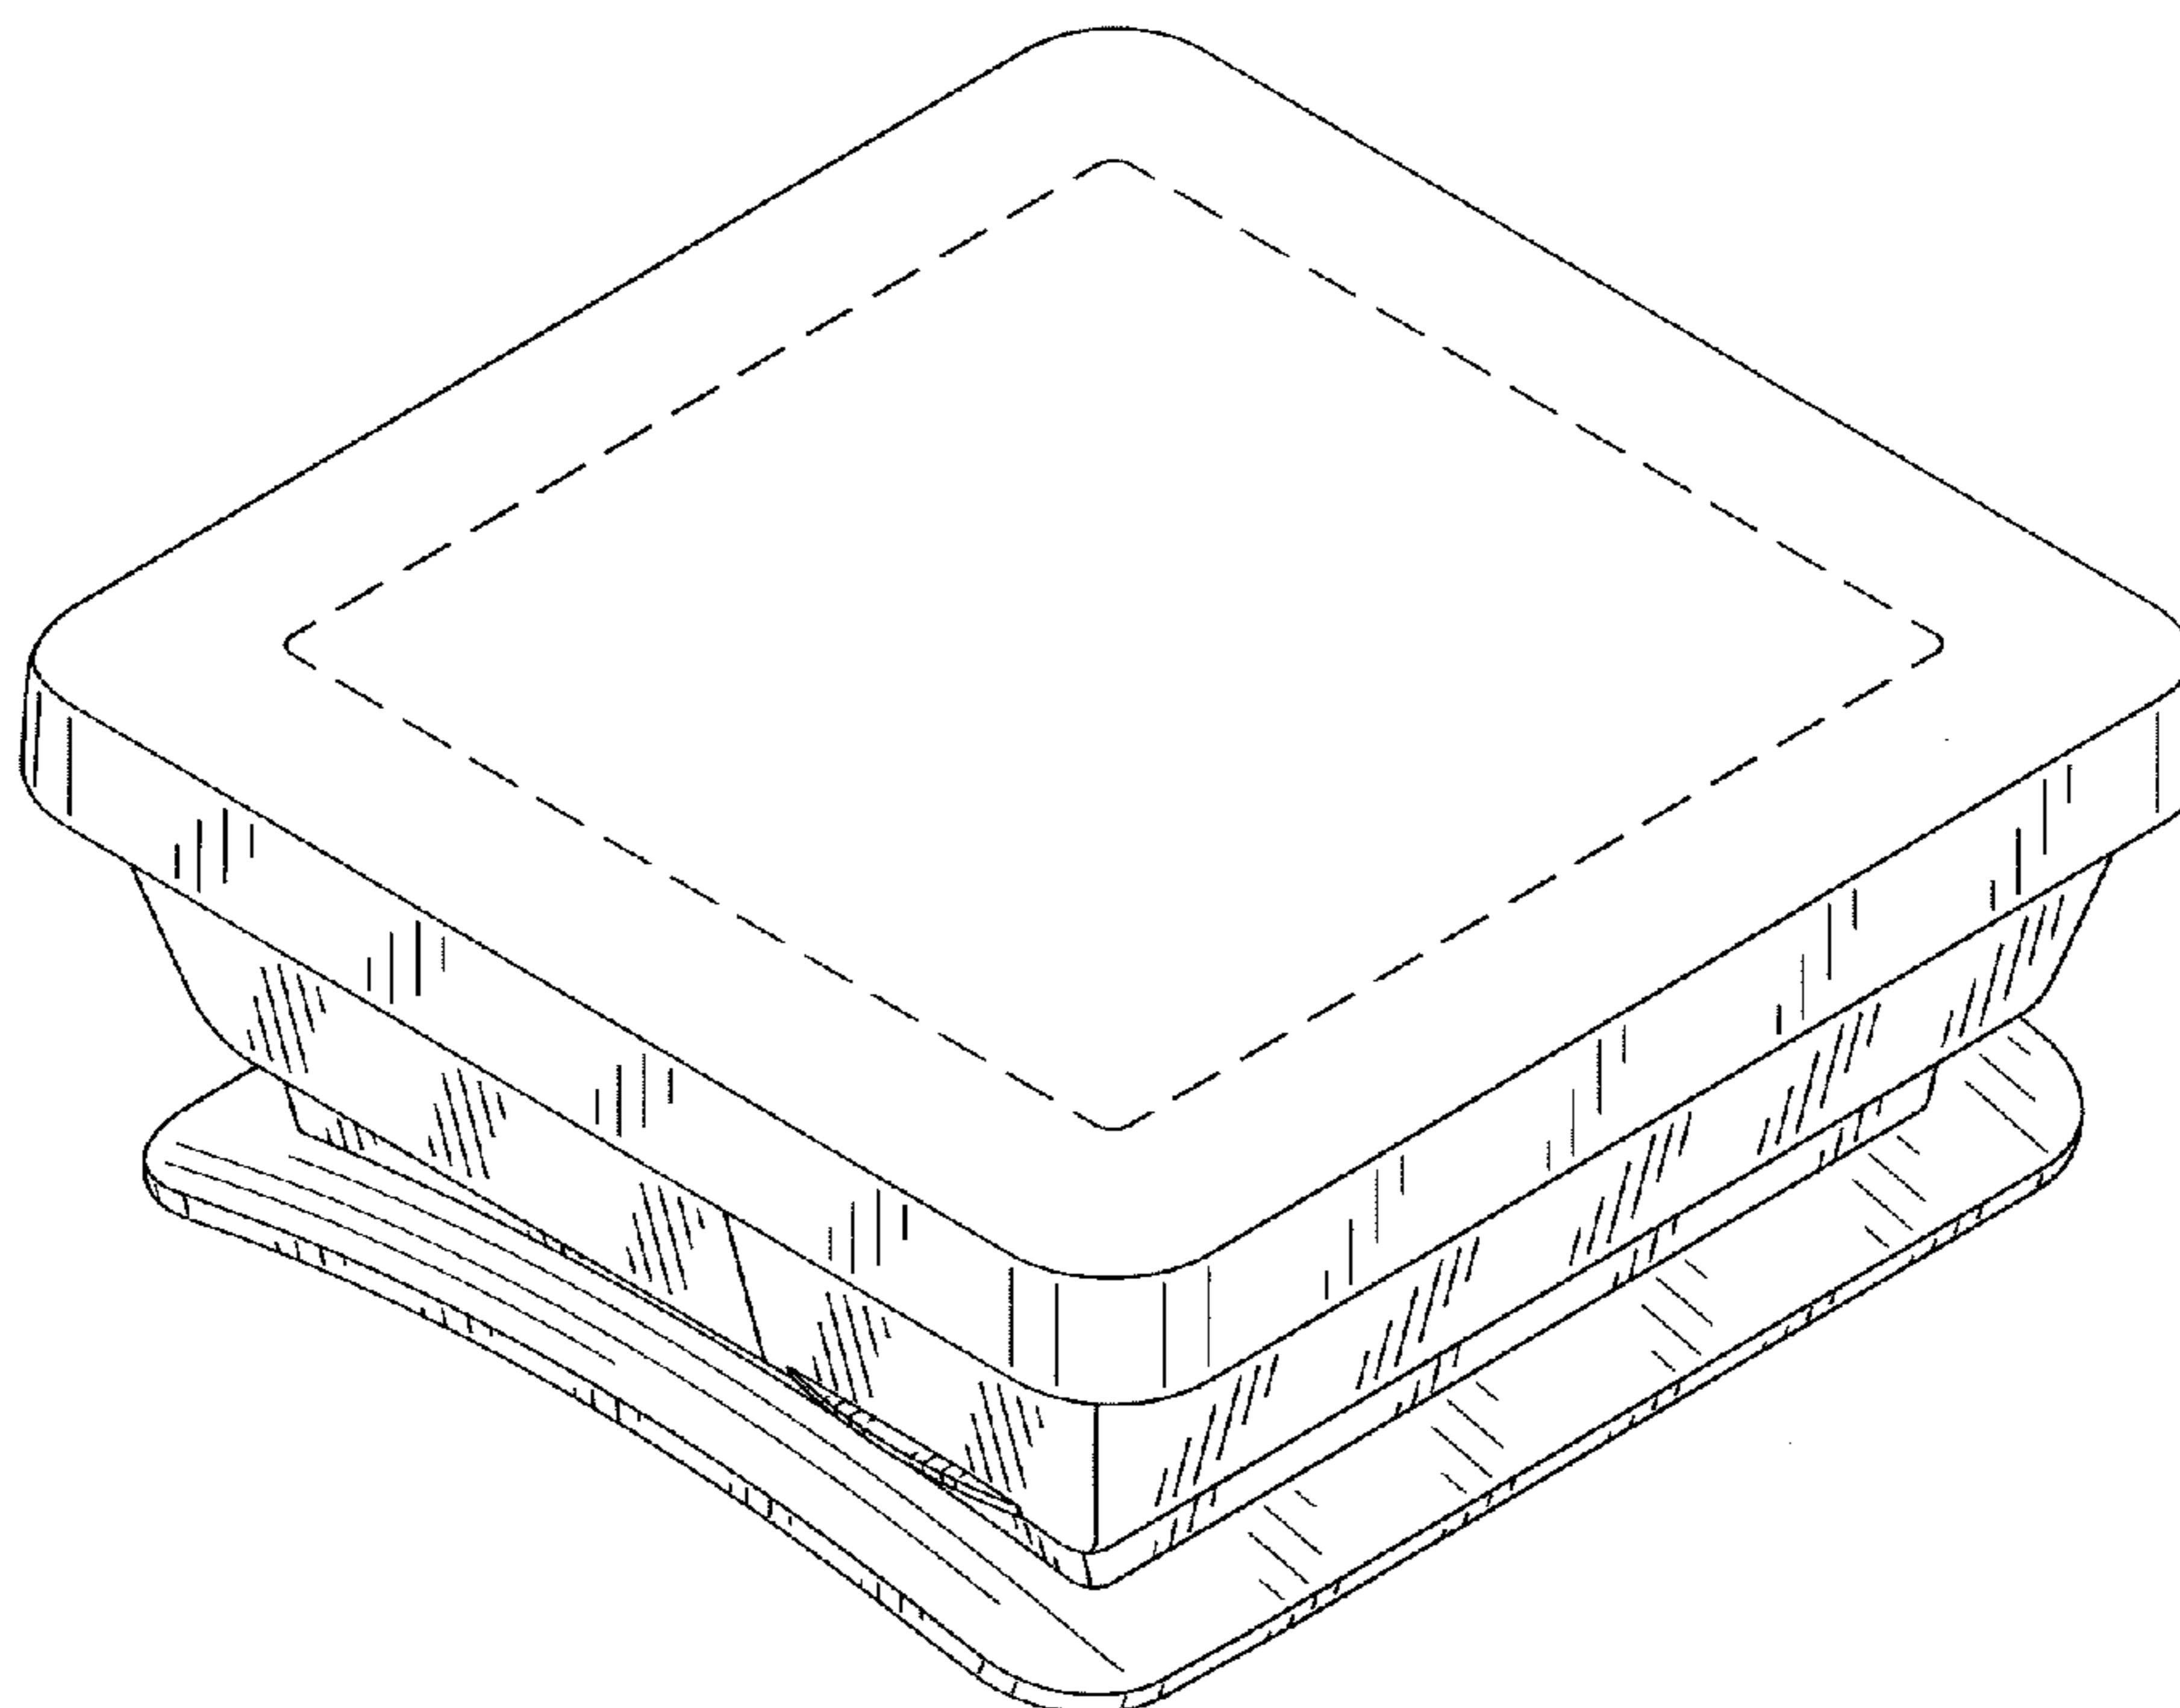

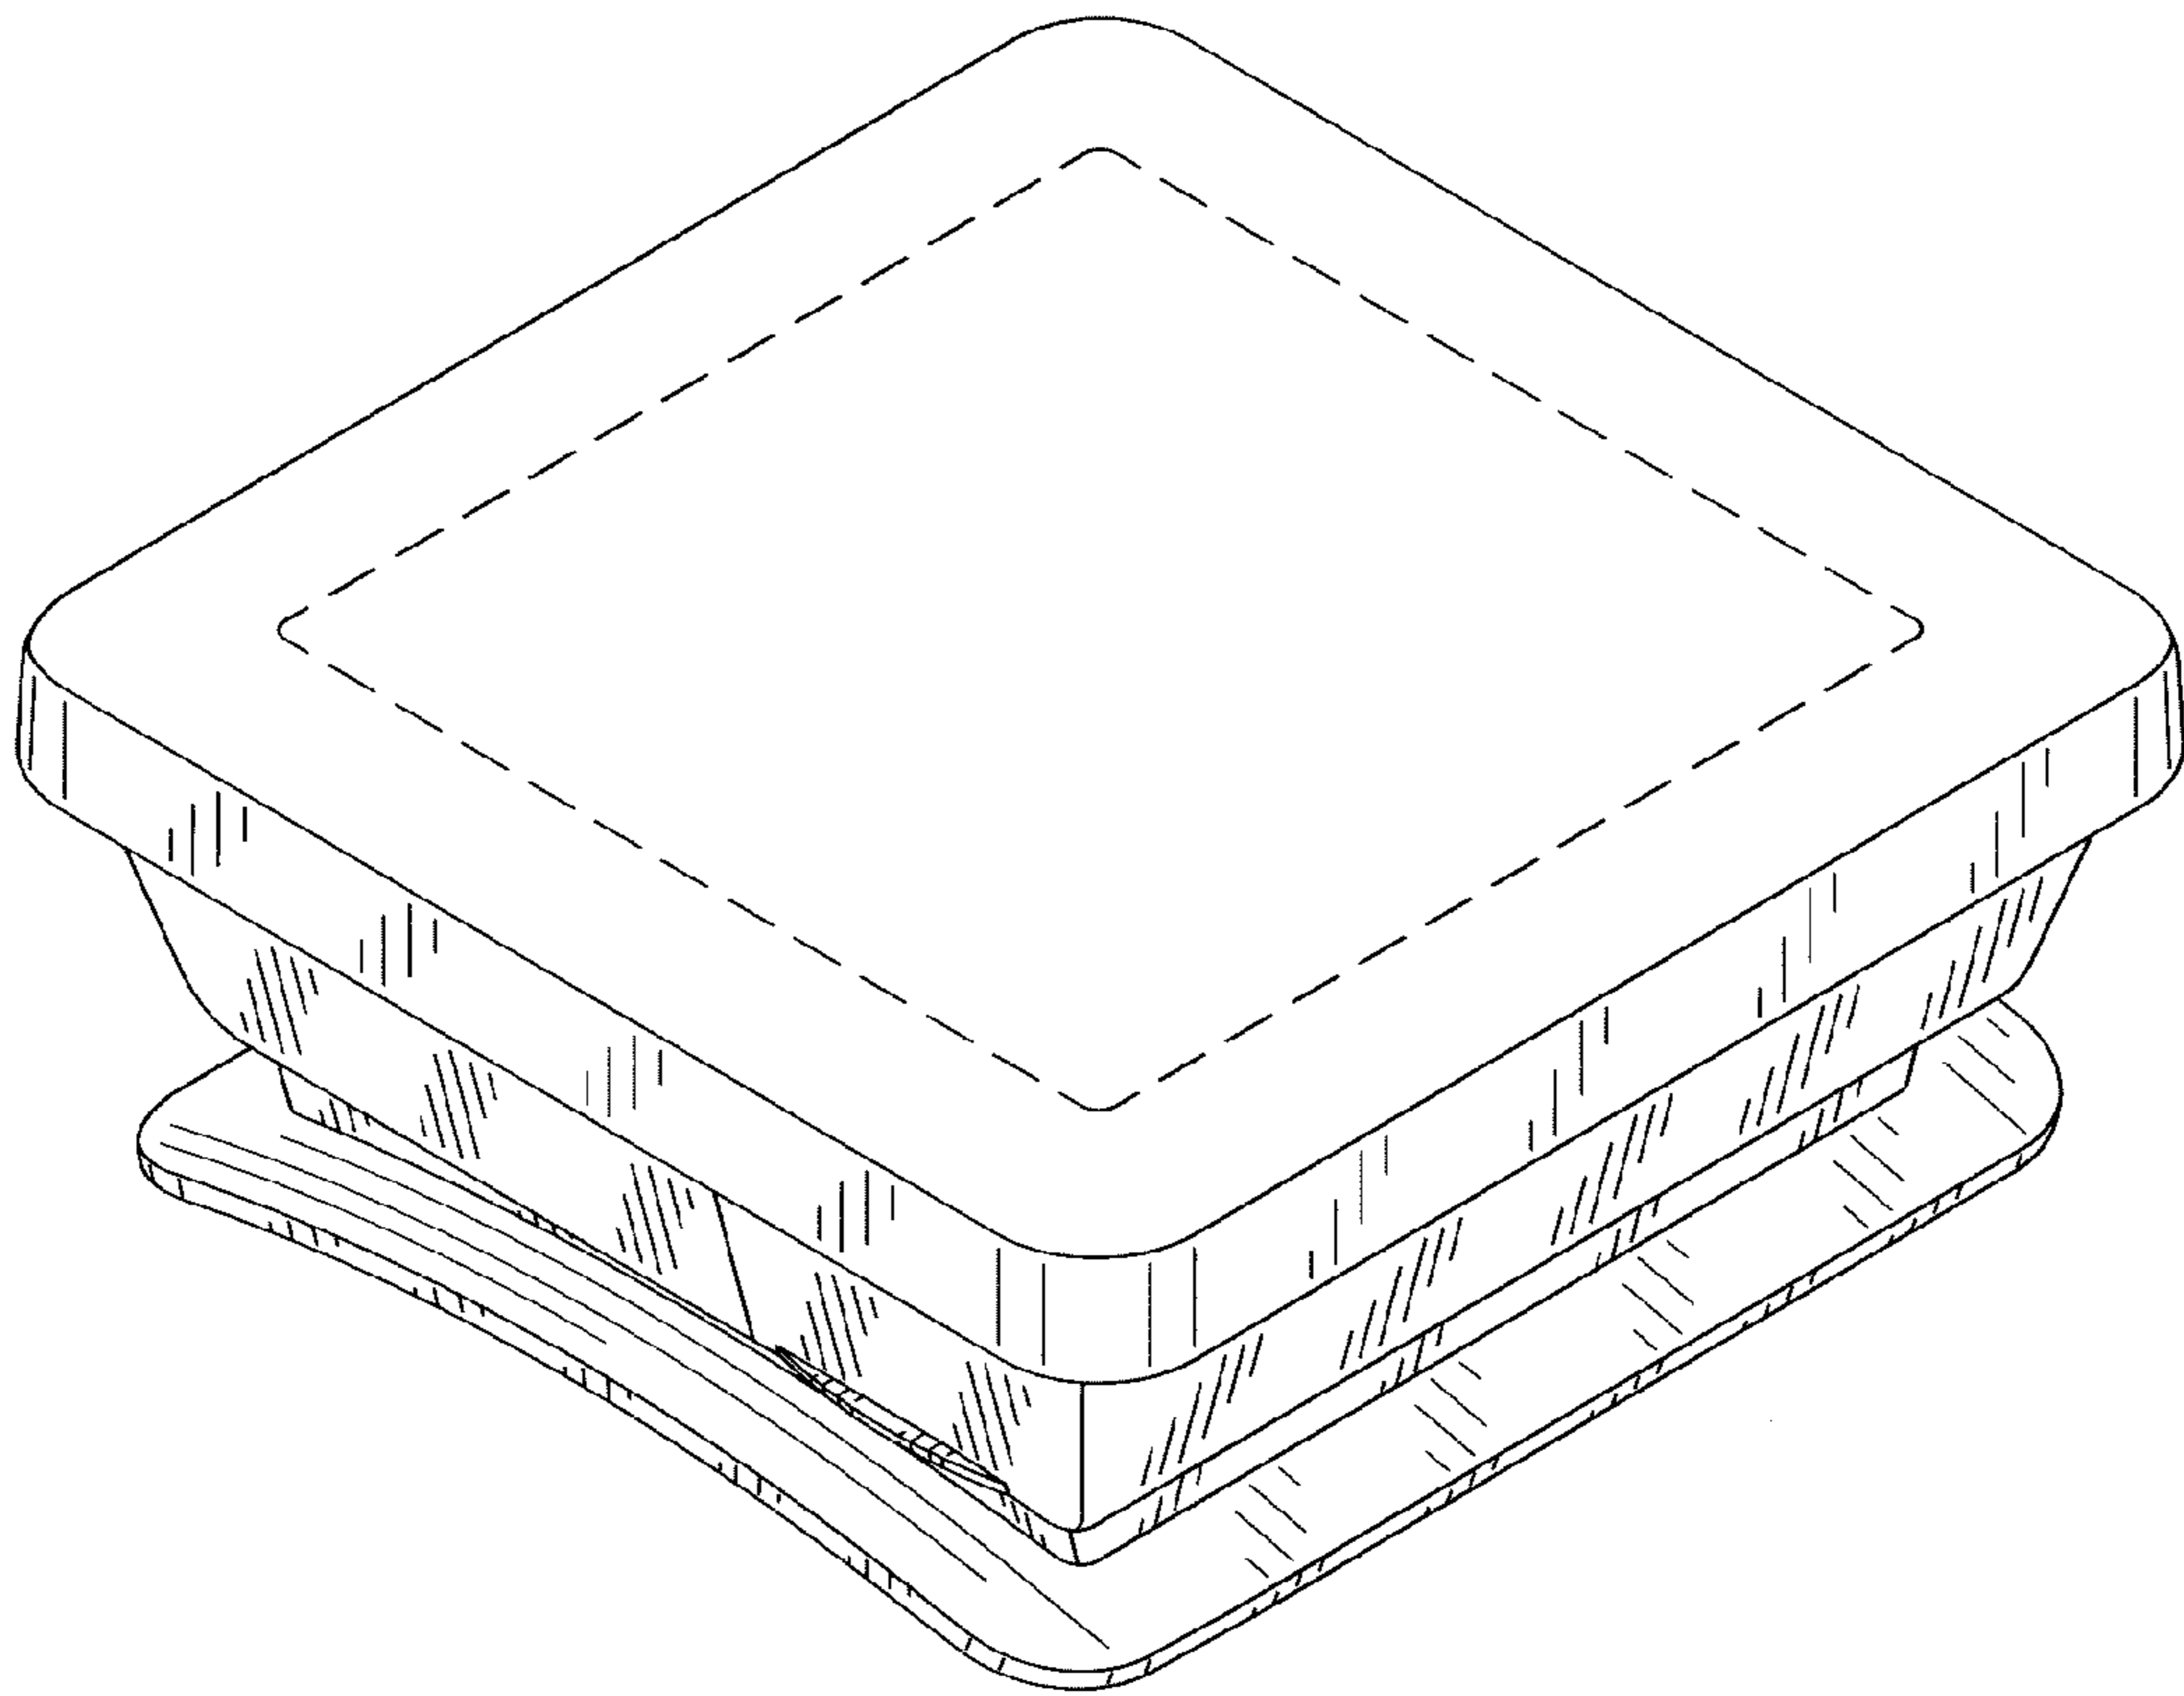


FIG. 1

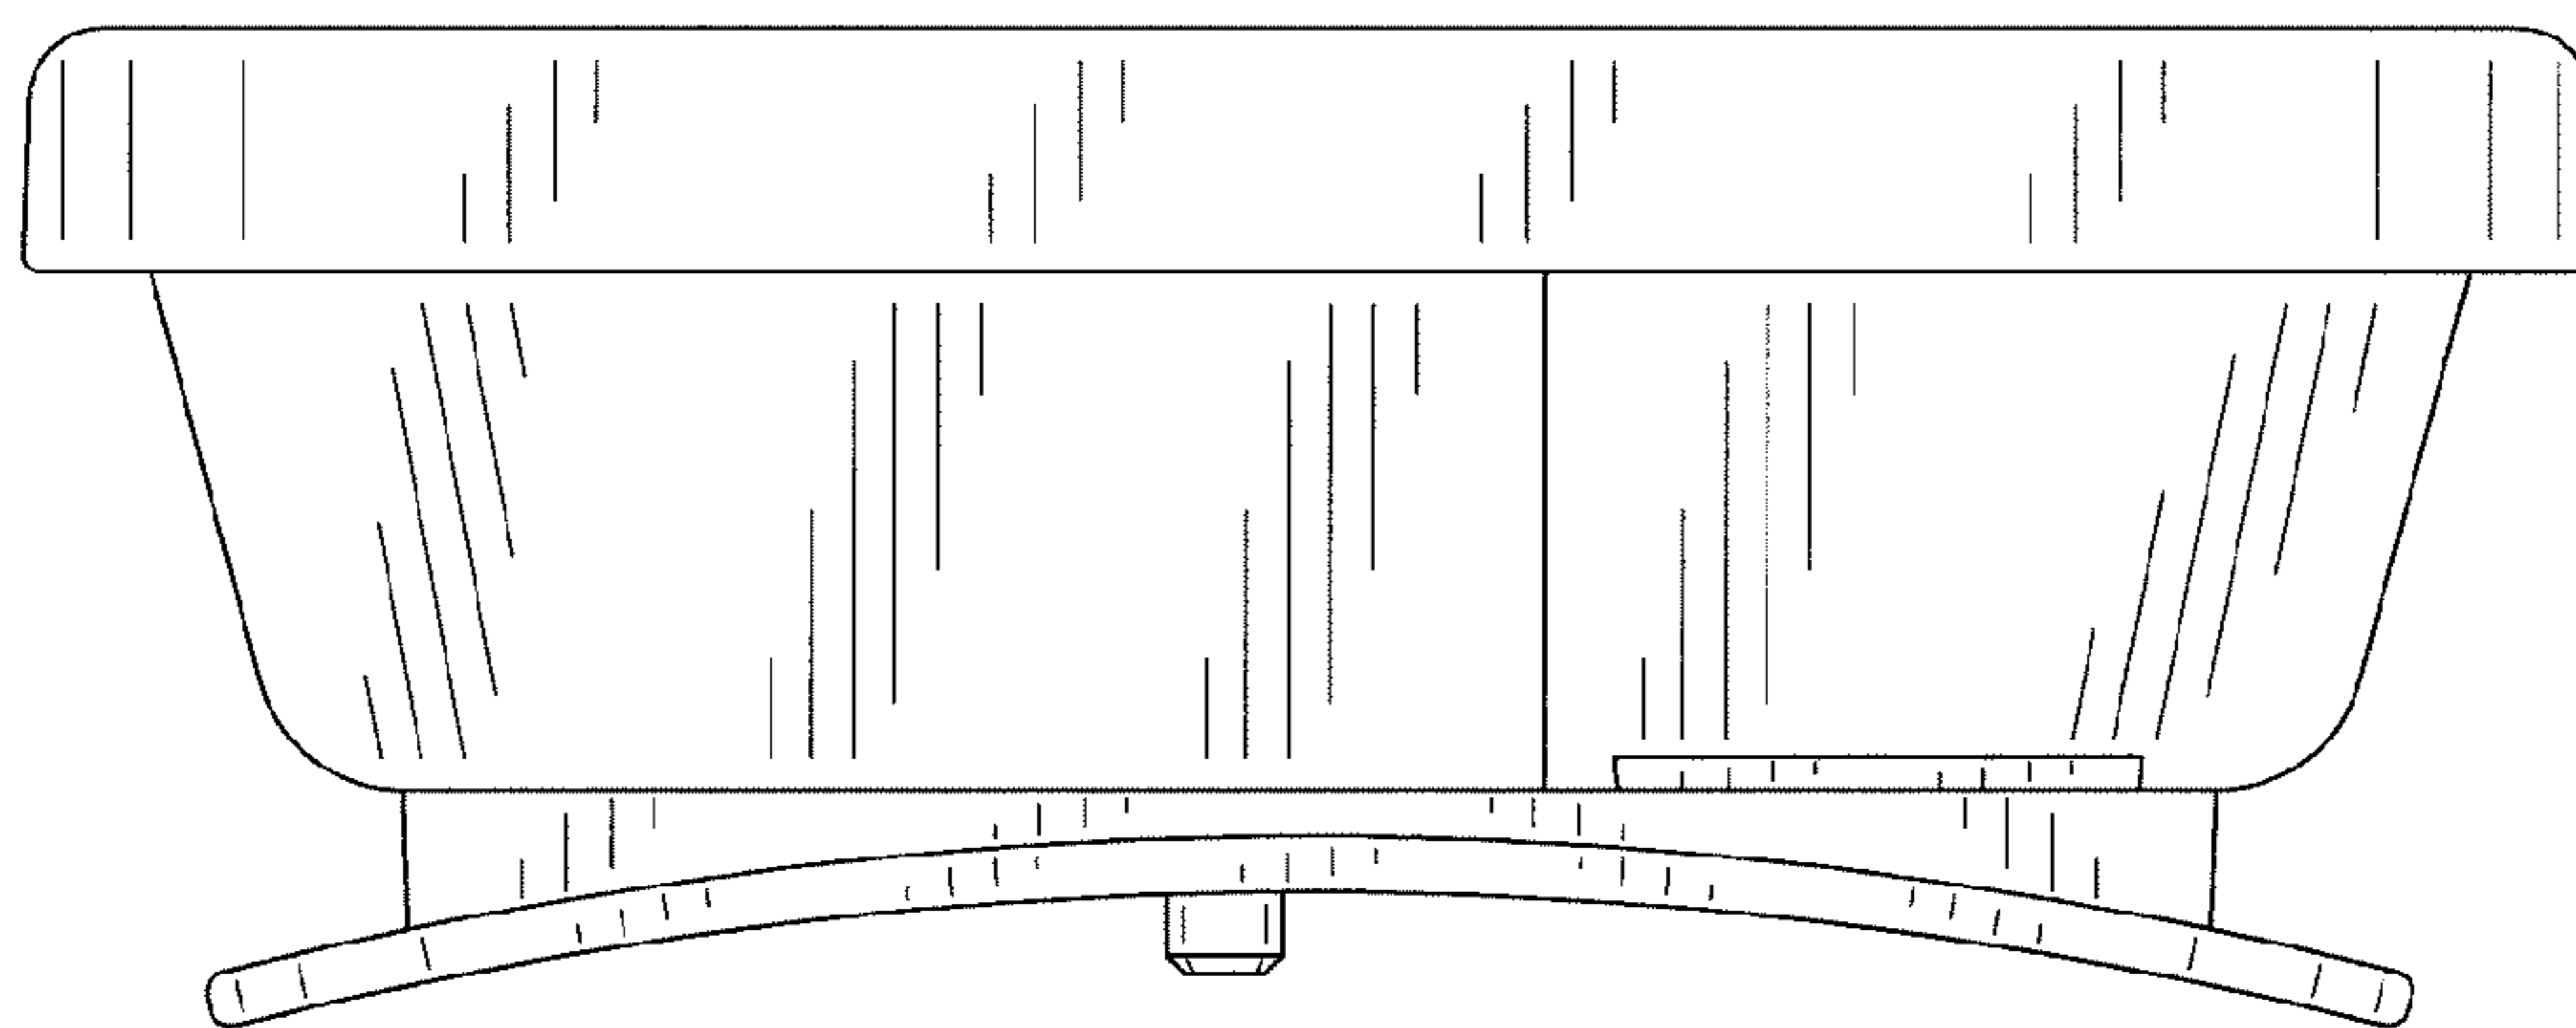


FIG. 2

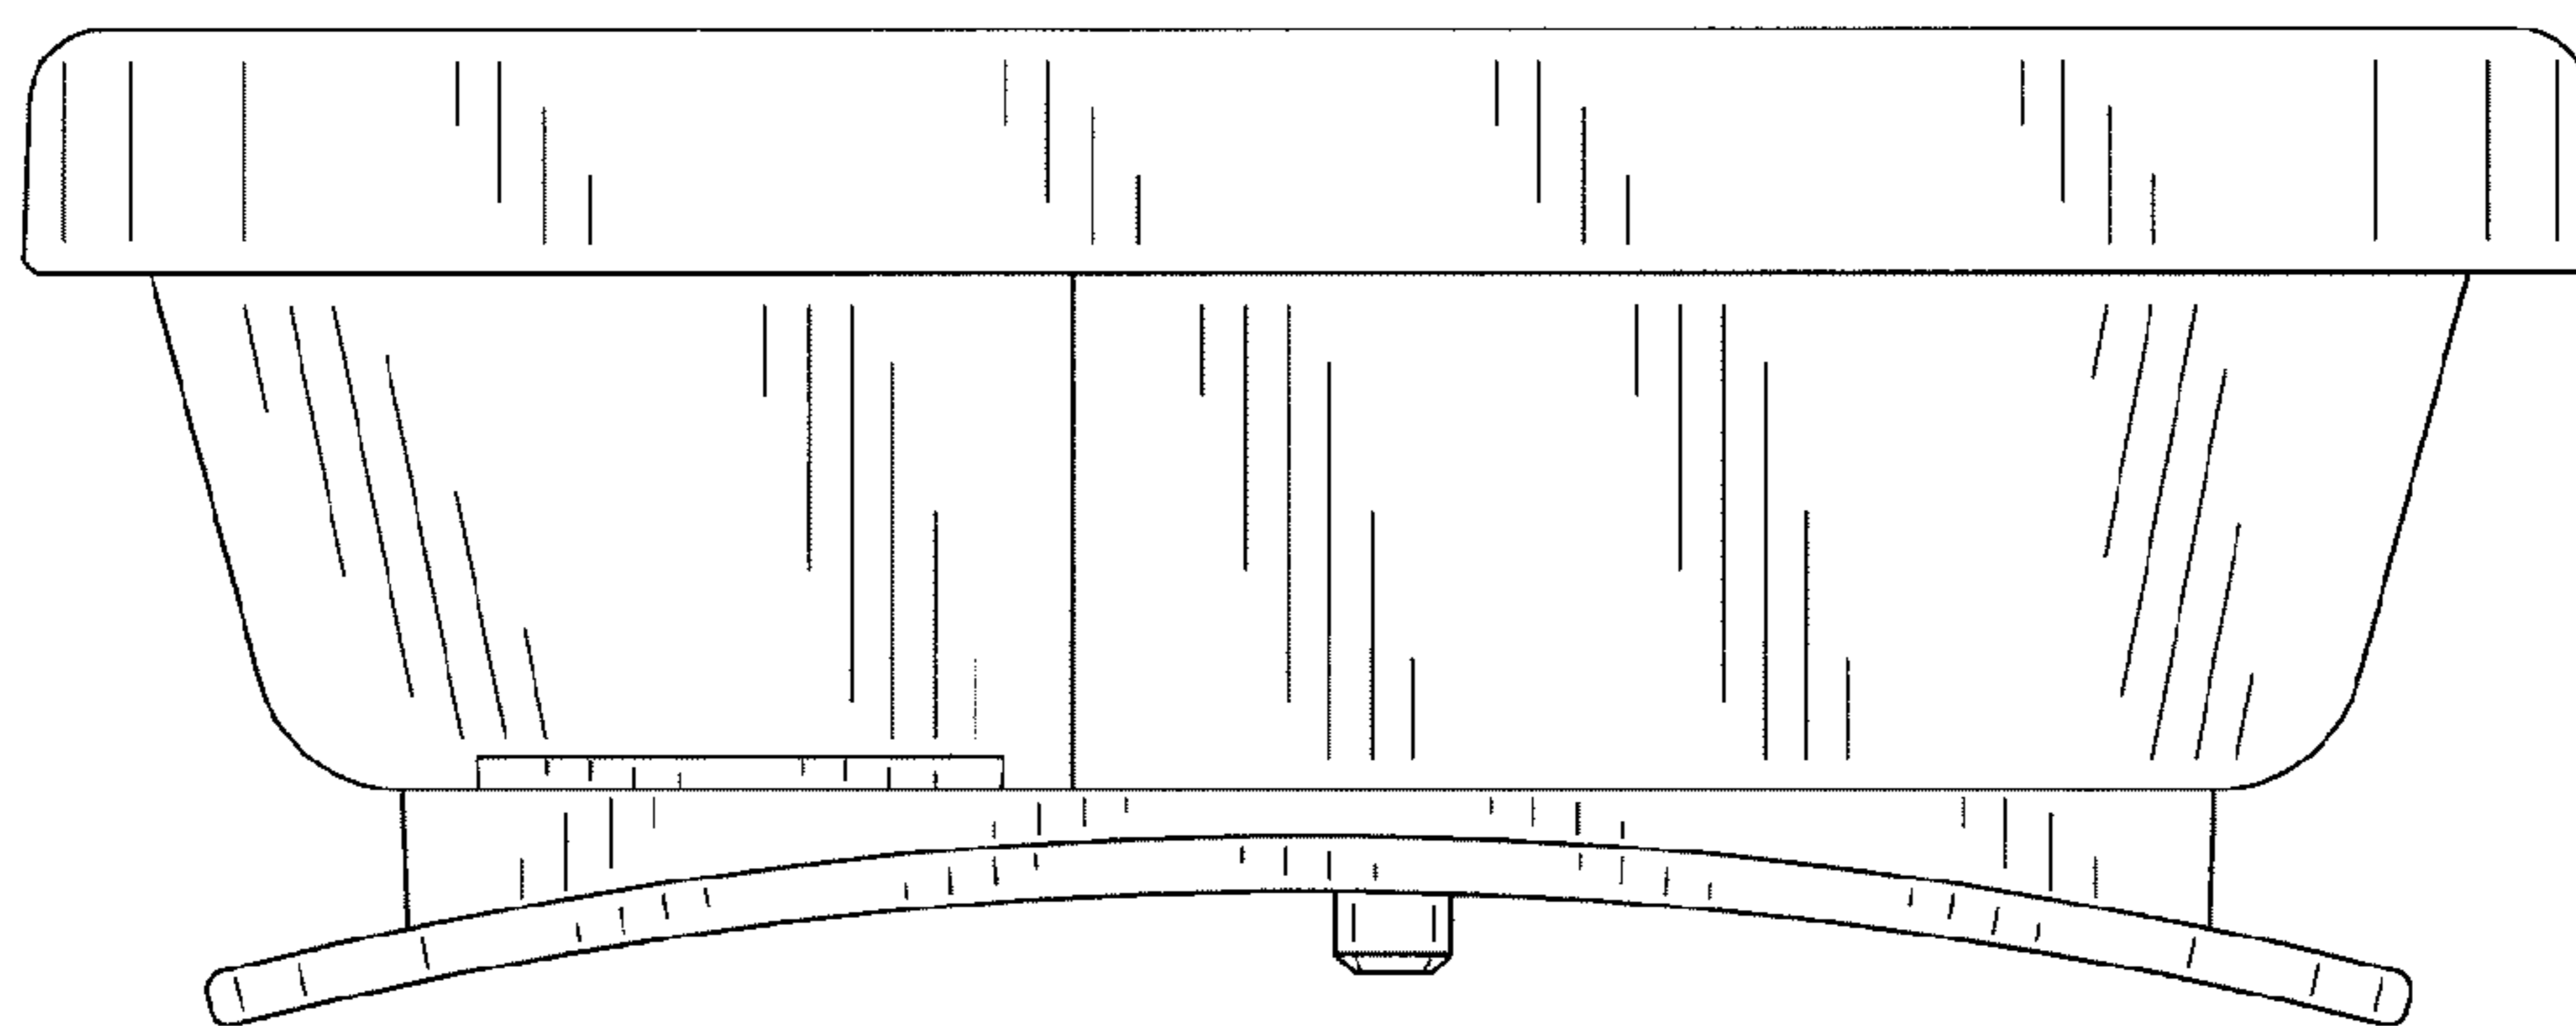


FIG. 3

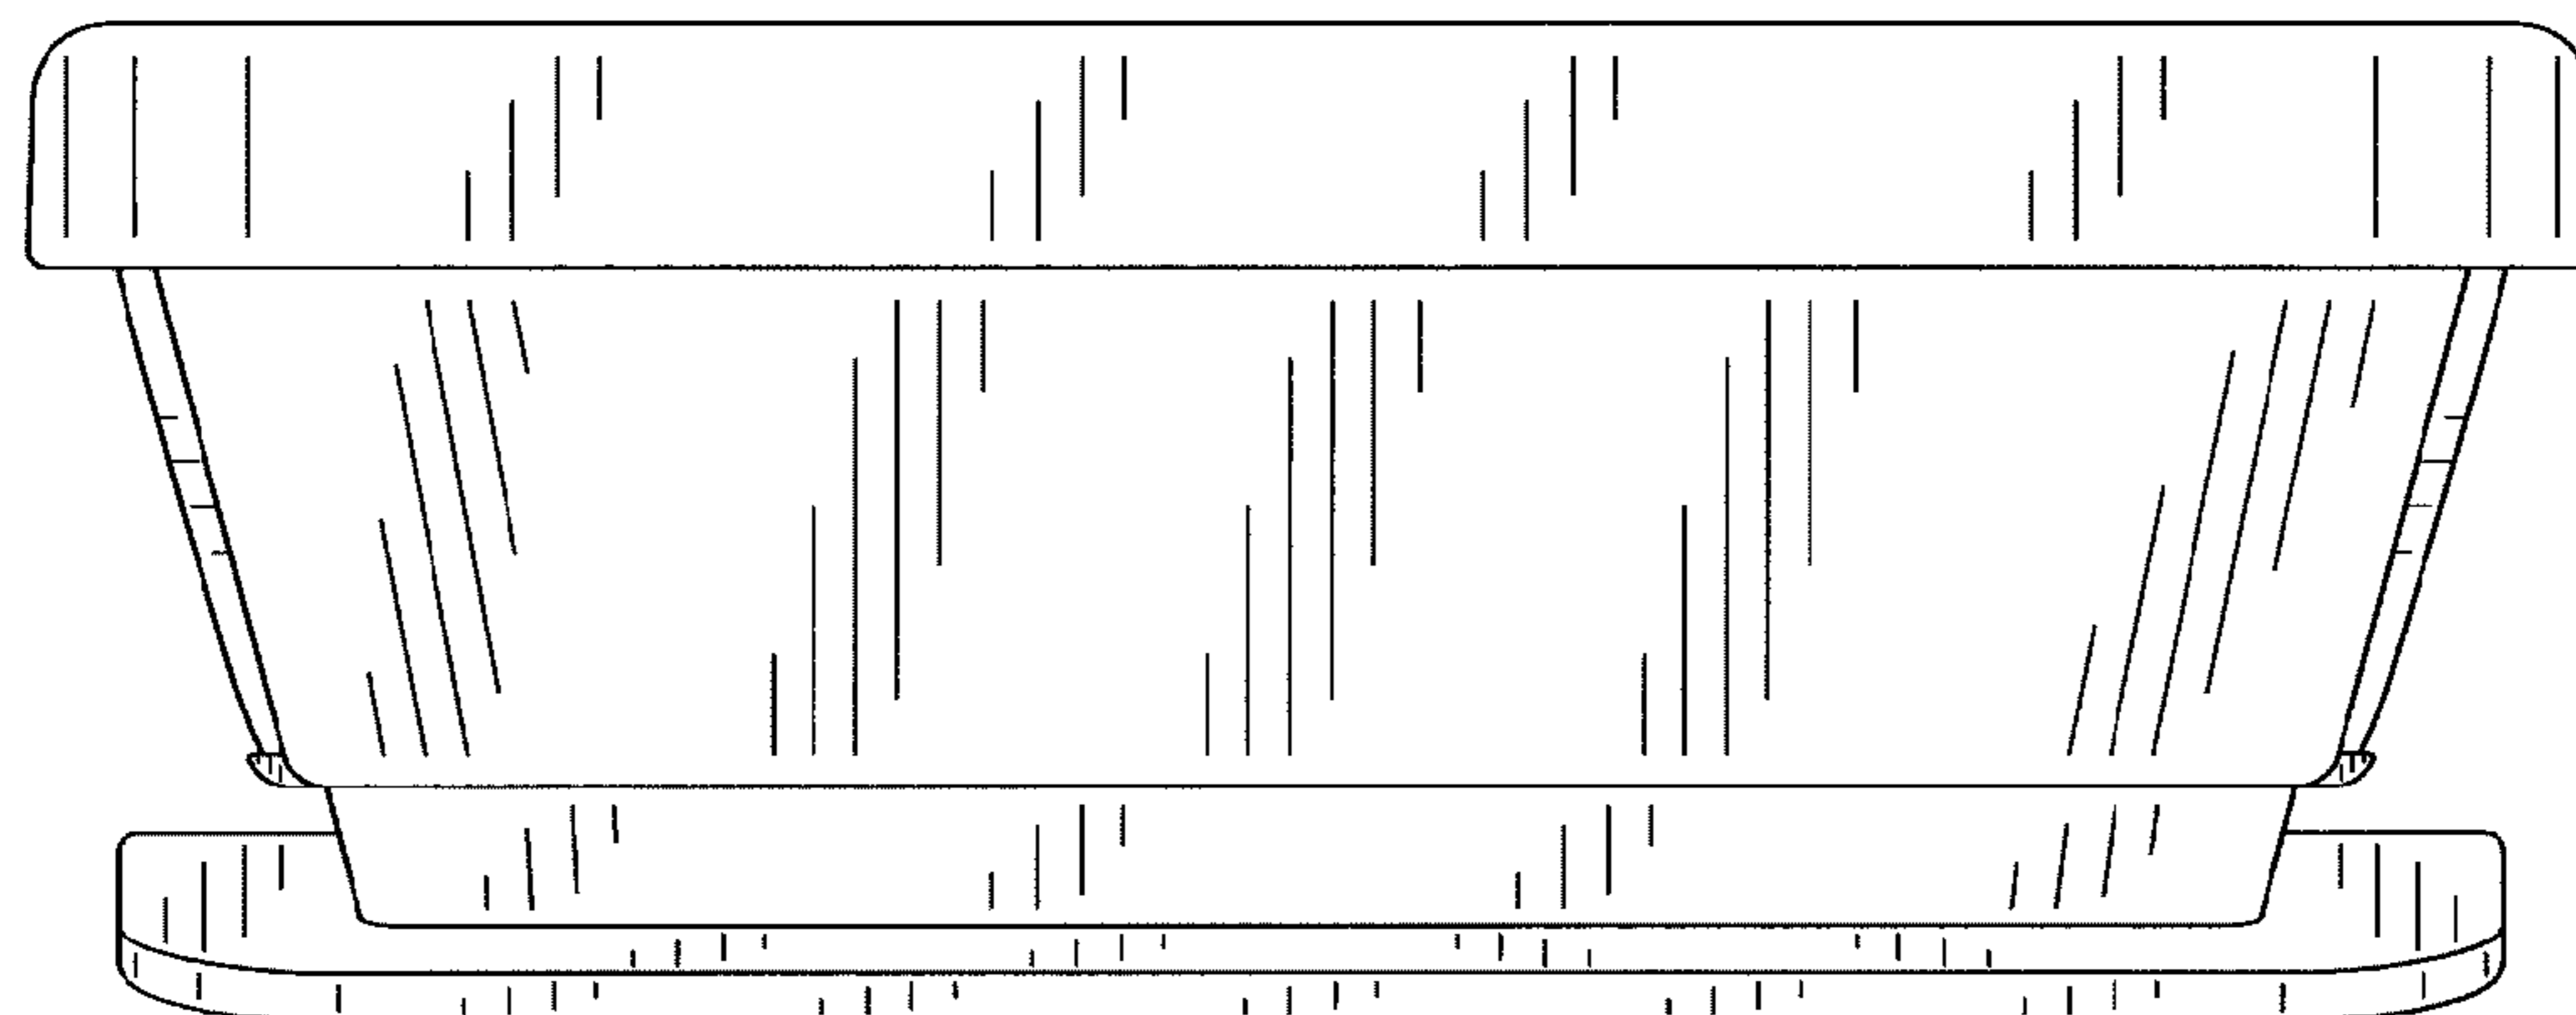


FIG. 4

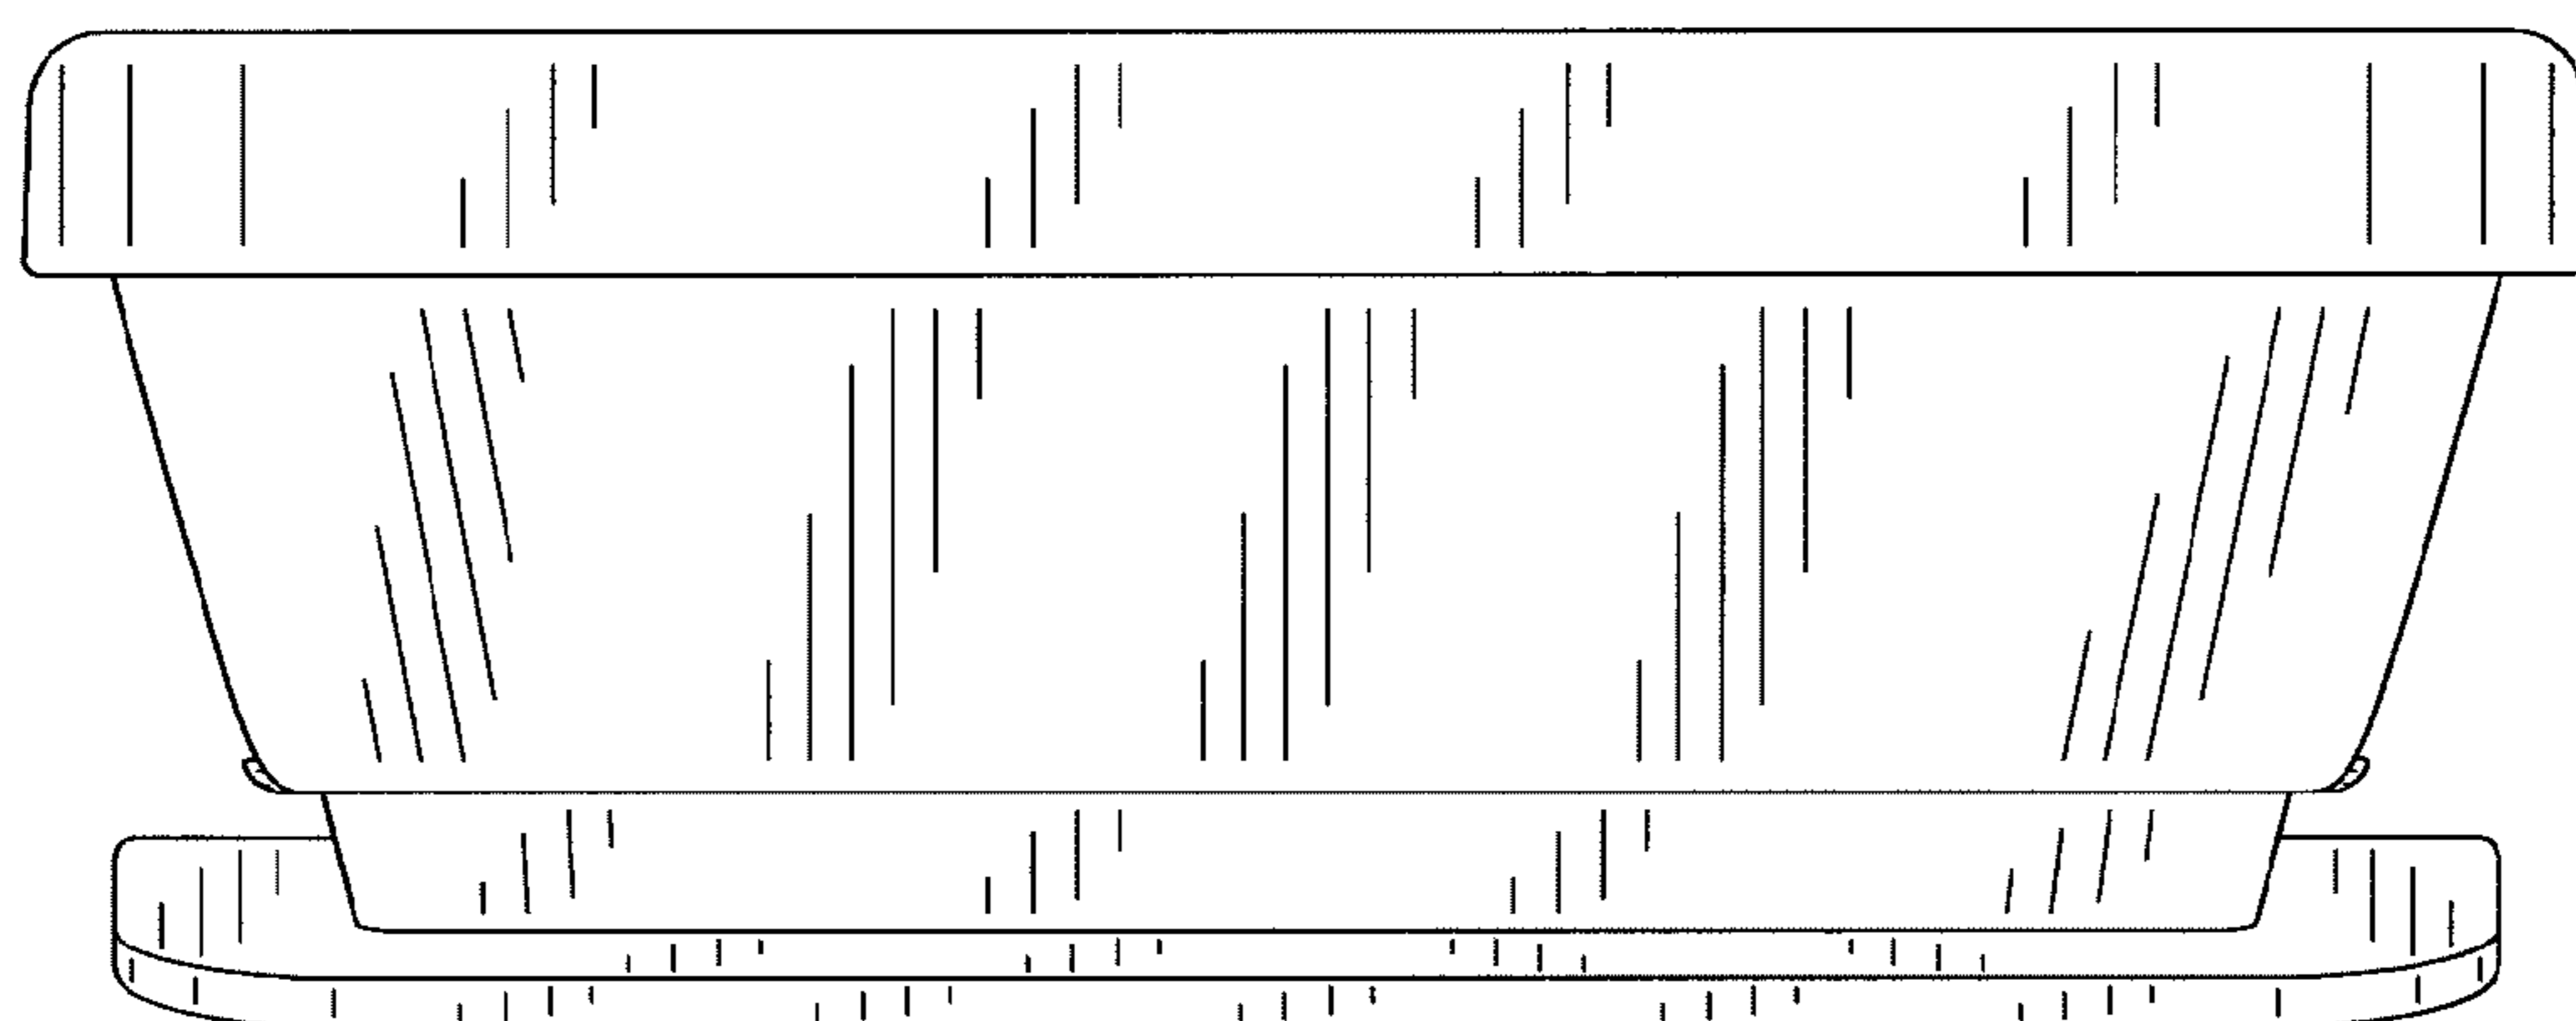


FIG. 5

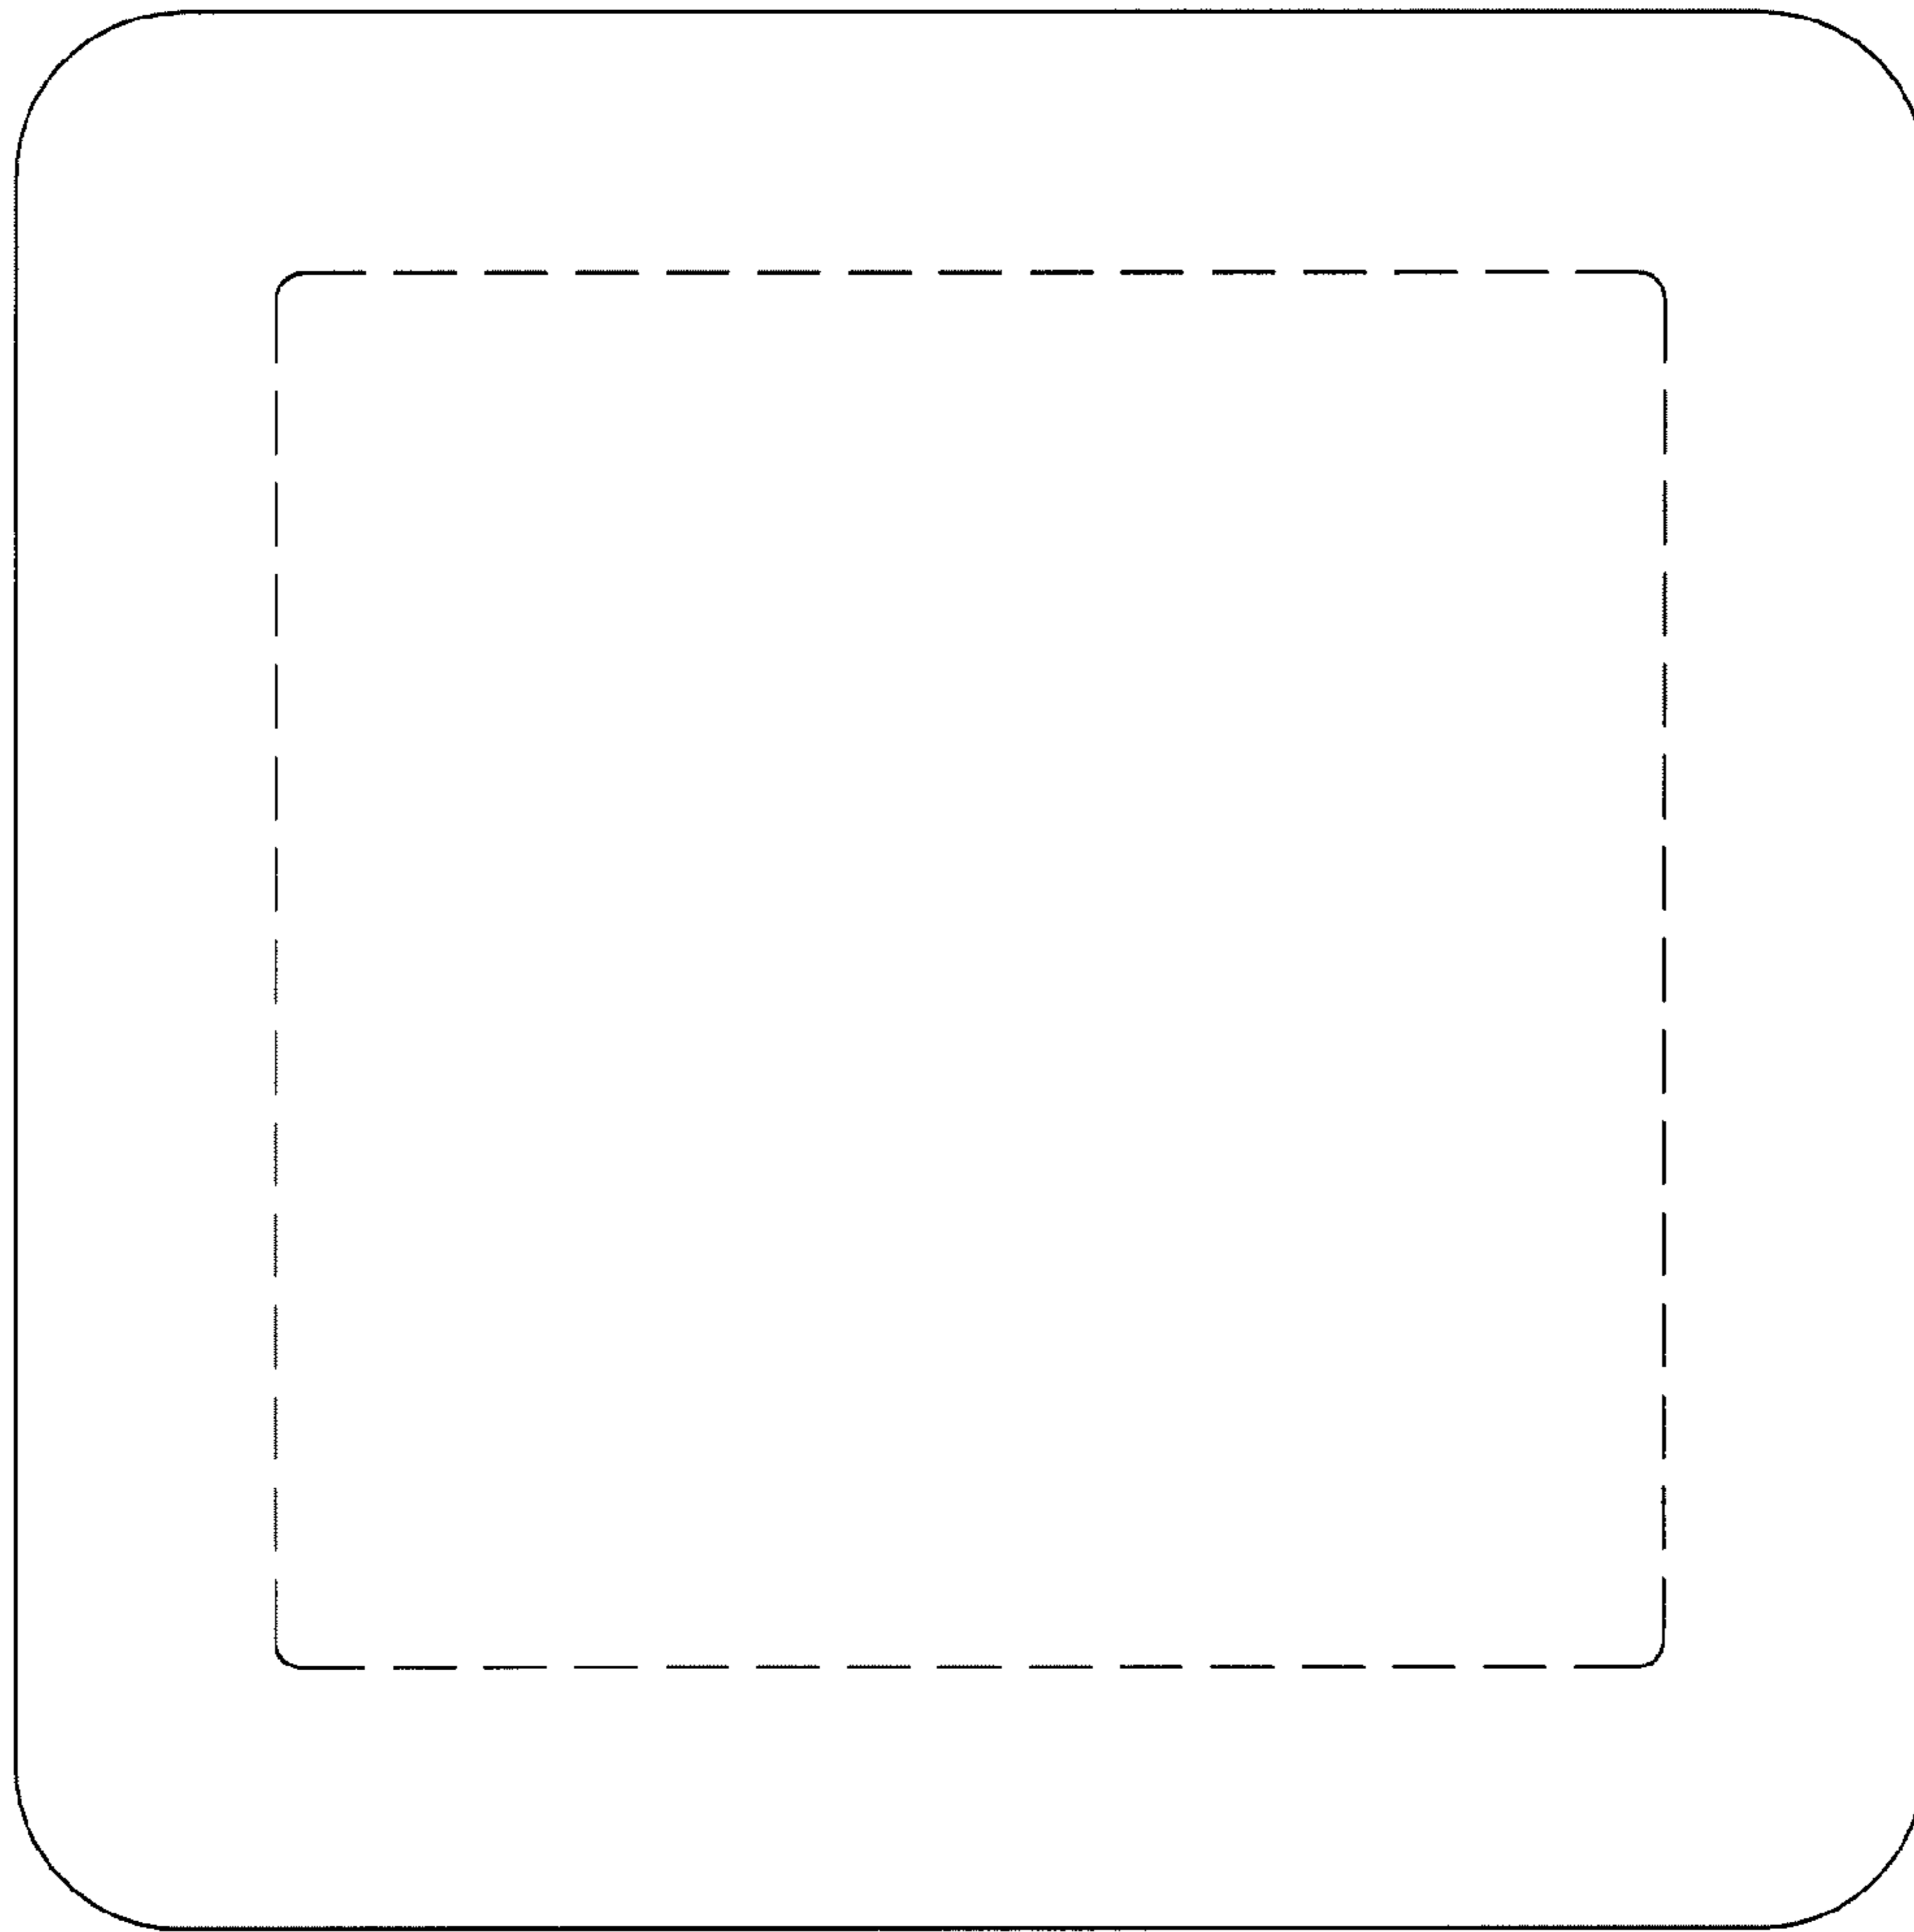


FIG. 6

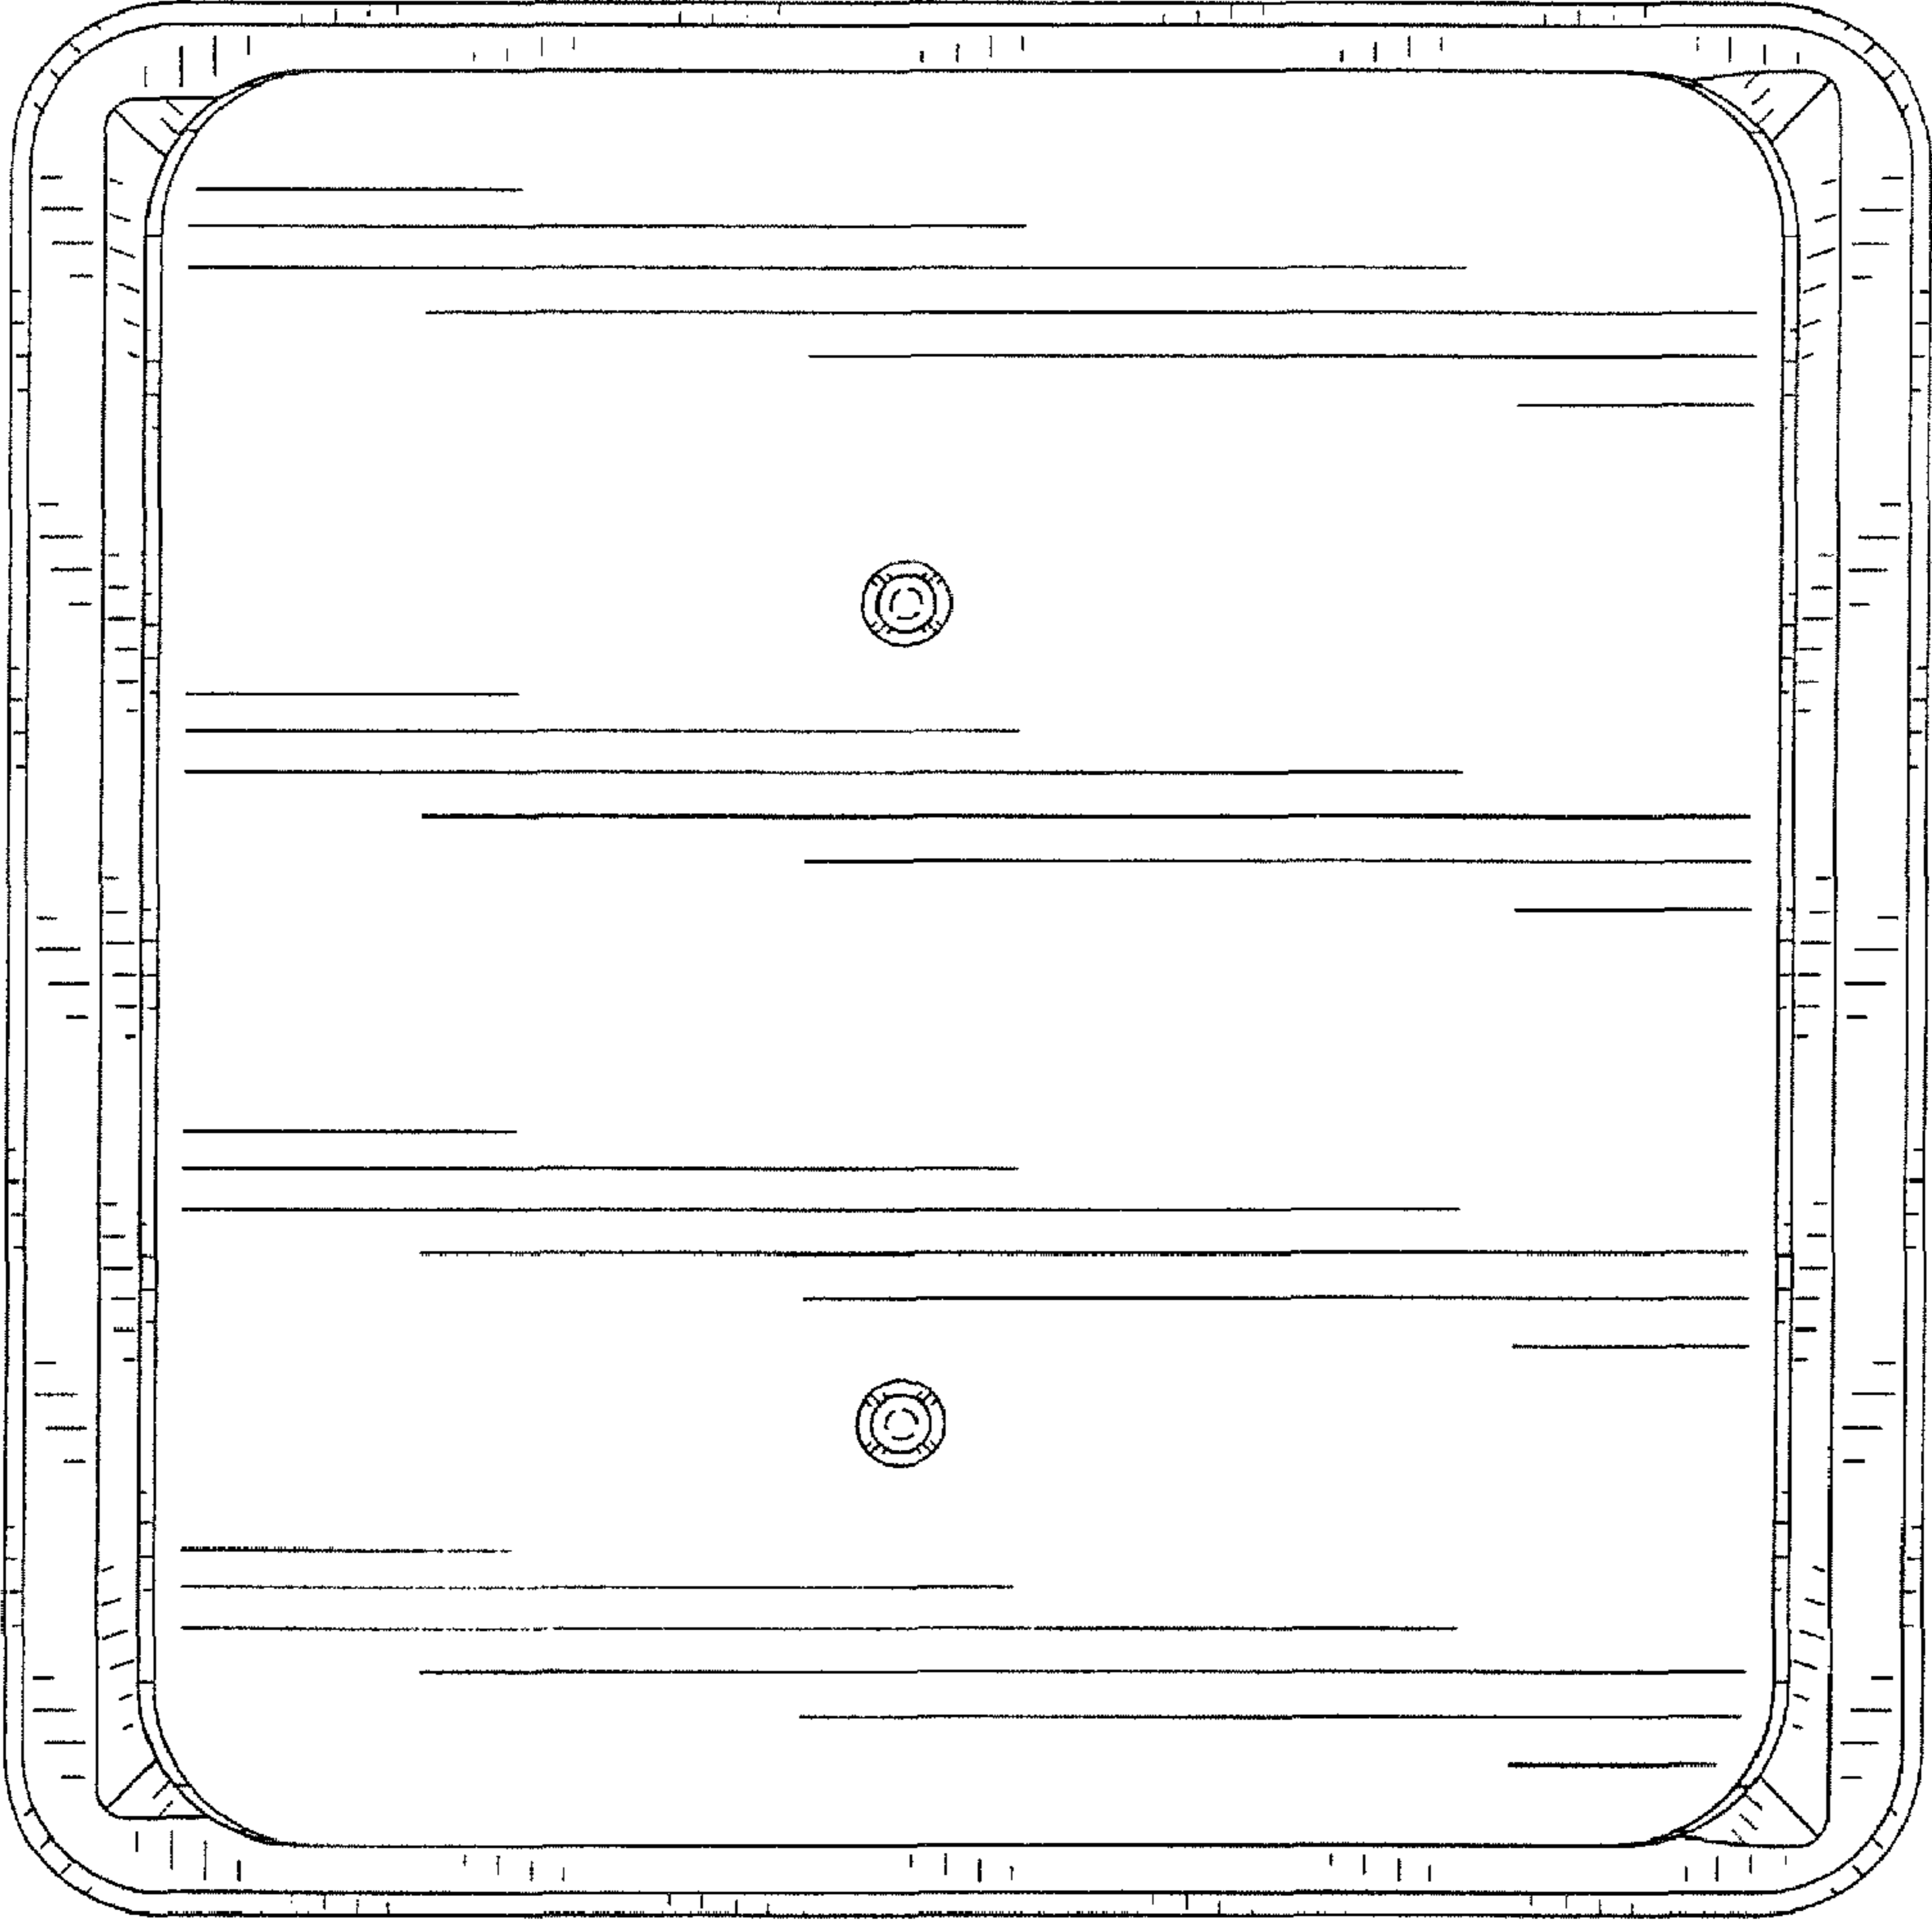


FIG. 7