



US00D655422S

(12) **United States Design Patent**  
**Oonuma et al.**

(10) **Patent No.:** **US D655,422 S**  
(45) **Date of Patent:** **\*\* Mar. 6, 2012**

(54) **IDENTIFICATION LABELER MODULE FOR CLINICAL LABORATORY AUTOMATION SYSTEM**

FOREIGN PATENT DOCUMENTS

JP D 1231257 2/2005  
JP D1397505 9/2010

(75) Inventors: **Mitsuru Oonuma**, Tokyo (JP); **Yoko Sato**, Fuchukomae (JP); **Akira Omachi**, Komae (JP); **Tetsuya Isobe**, Hitachinaka (JP); **Kazuhiro Noda**, Hitachinaka (JP)

OTHER PUBLICATIONS

Copending U.S. Appl. No. 29/384,358, filed Jan. 30, 2011, Oonuma.  
Copending U.S. Appl. No. 29/384,365, filed Jan. 30, 2011, Oonuma.  
Copending U.S. Appl. No. 29/384,370, filed Jan. 30, 2011, Oonuma.  
Copending U.S. Appl. No. 29/384,361, filed Jan. 30, 2011, Oonuma.  
Copending U.S. Appl. No. 29/384,364, filed Jan. 30, 2011, Oonuma.

(73) Assignee: **Hitachi High-Technologies Corporation**, Tokyo (JP)

\* cited by examiner

(\*\*) Term: **14 Years**

*Primary Examiner* — Anhdao Doan

(21) Appl. No.: **29/384,380**

(74) *Attorney, Agent, or Firm* — Antonelli, Terry, Stout & Kraus, LLP.

(22) Filed: **Jan. 31, 2011**

(30) **Foreign Application Priority Data**

Sep. 29, 2010 (JP) ..... 2010-023337

(51) **LOC (9) Cl.** ..... **24-01**

(52) **U.S. Cl.** ..... **D24/216**

(58) **Field of Classification Search** ..... D24/216,  
D24/224, 231, 232, 186, 107, 169, 217, 233;  
D10/46, 81; 422/500, 547, 62-65, 67; 435/287.1,  
435/287.3; 436/43, 45, 47

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,946,651 A \* 8/1990 Liston et al. .... 436/43  
D347,478 S \* 5/1994 Pinkney ..... D24/216  
D356,967 S \* 4/1995 Takekoshi et al. .... D10/81  
5,986,260 A \* 11/1999 Oonuma et al. .... 250/288  
D508,999 S \* 8/2005 Fanning et al. .... D24/216  
D523,153 S \* 6/2006 Akashi et al. .... D24/232  
2004/0081583 A1 \* 4/2004 Berndt et al. .... 422/63  
2007/0110617 A1 \* 5/2007 Nagai et al. .... 422/65  
2008/0019868 A1 \* 1/2008 Okumoto et al. .... 422/63  
2009/0325274 A1 \* 12/2009 Hamada et al. .... 422/65

(57) **CLAIM**


The ornamental design for an identification labeler module for clinical laboratory automation system, as shown and described.


**DESCRIPTION**

FIG. 1 is a front, top and right side perspective view of an identification labeler module for clinical laboratory automation system showing our new design; FIG. 2 is a front elevational view thereof; FIG. 3 is a rear elevational view thereof; FIG. 4 is a top plan view thereof; FIG. 5 is a bottom plan view thereof; FIG. 6 is a left side elevational view thereof; FIG. 7 is a right side elevational view thereof; and, FIG. 8 is a right side elevational view thereof shown in an opened position.

The broken lines in all drawing views are included for the purpose of illustrating portions of the identification labeler module for clinical laboratory automation system that form no part of the claimed design.

**1 Claim, 6 Drawing Sheets**

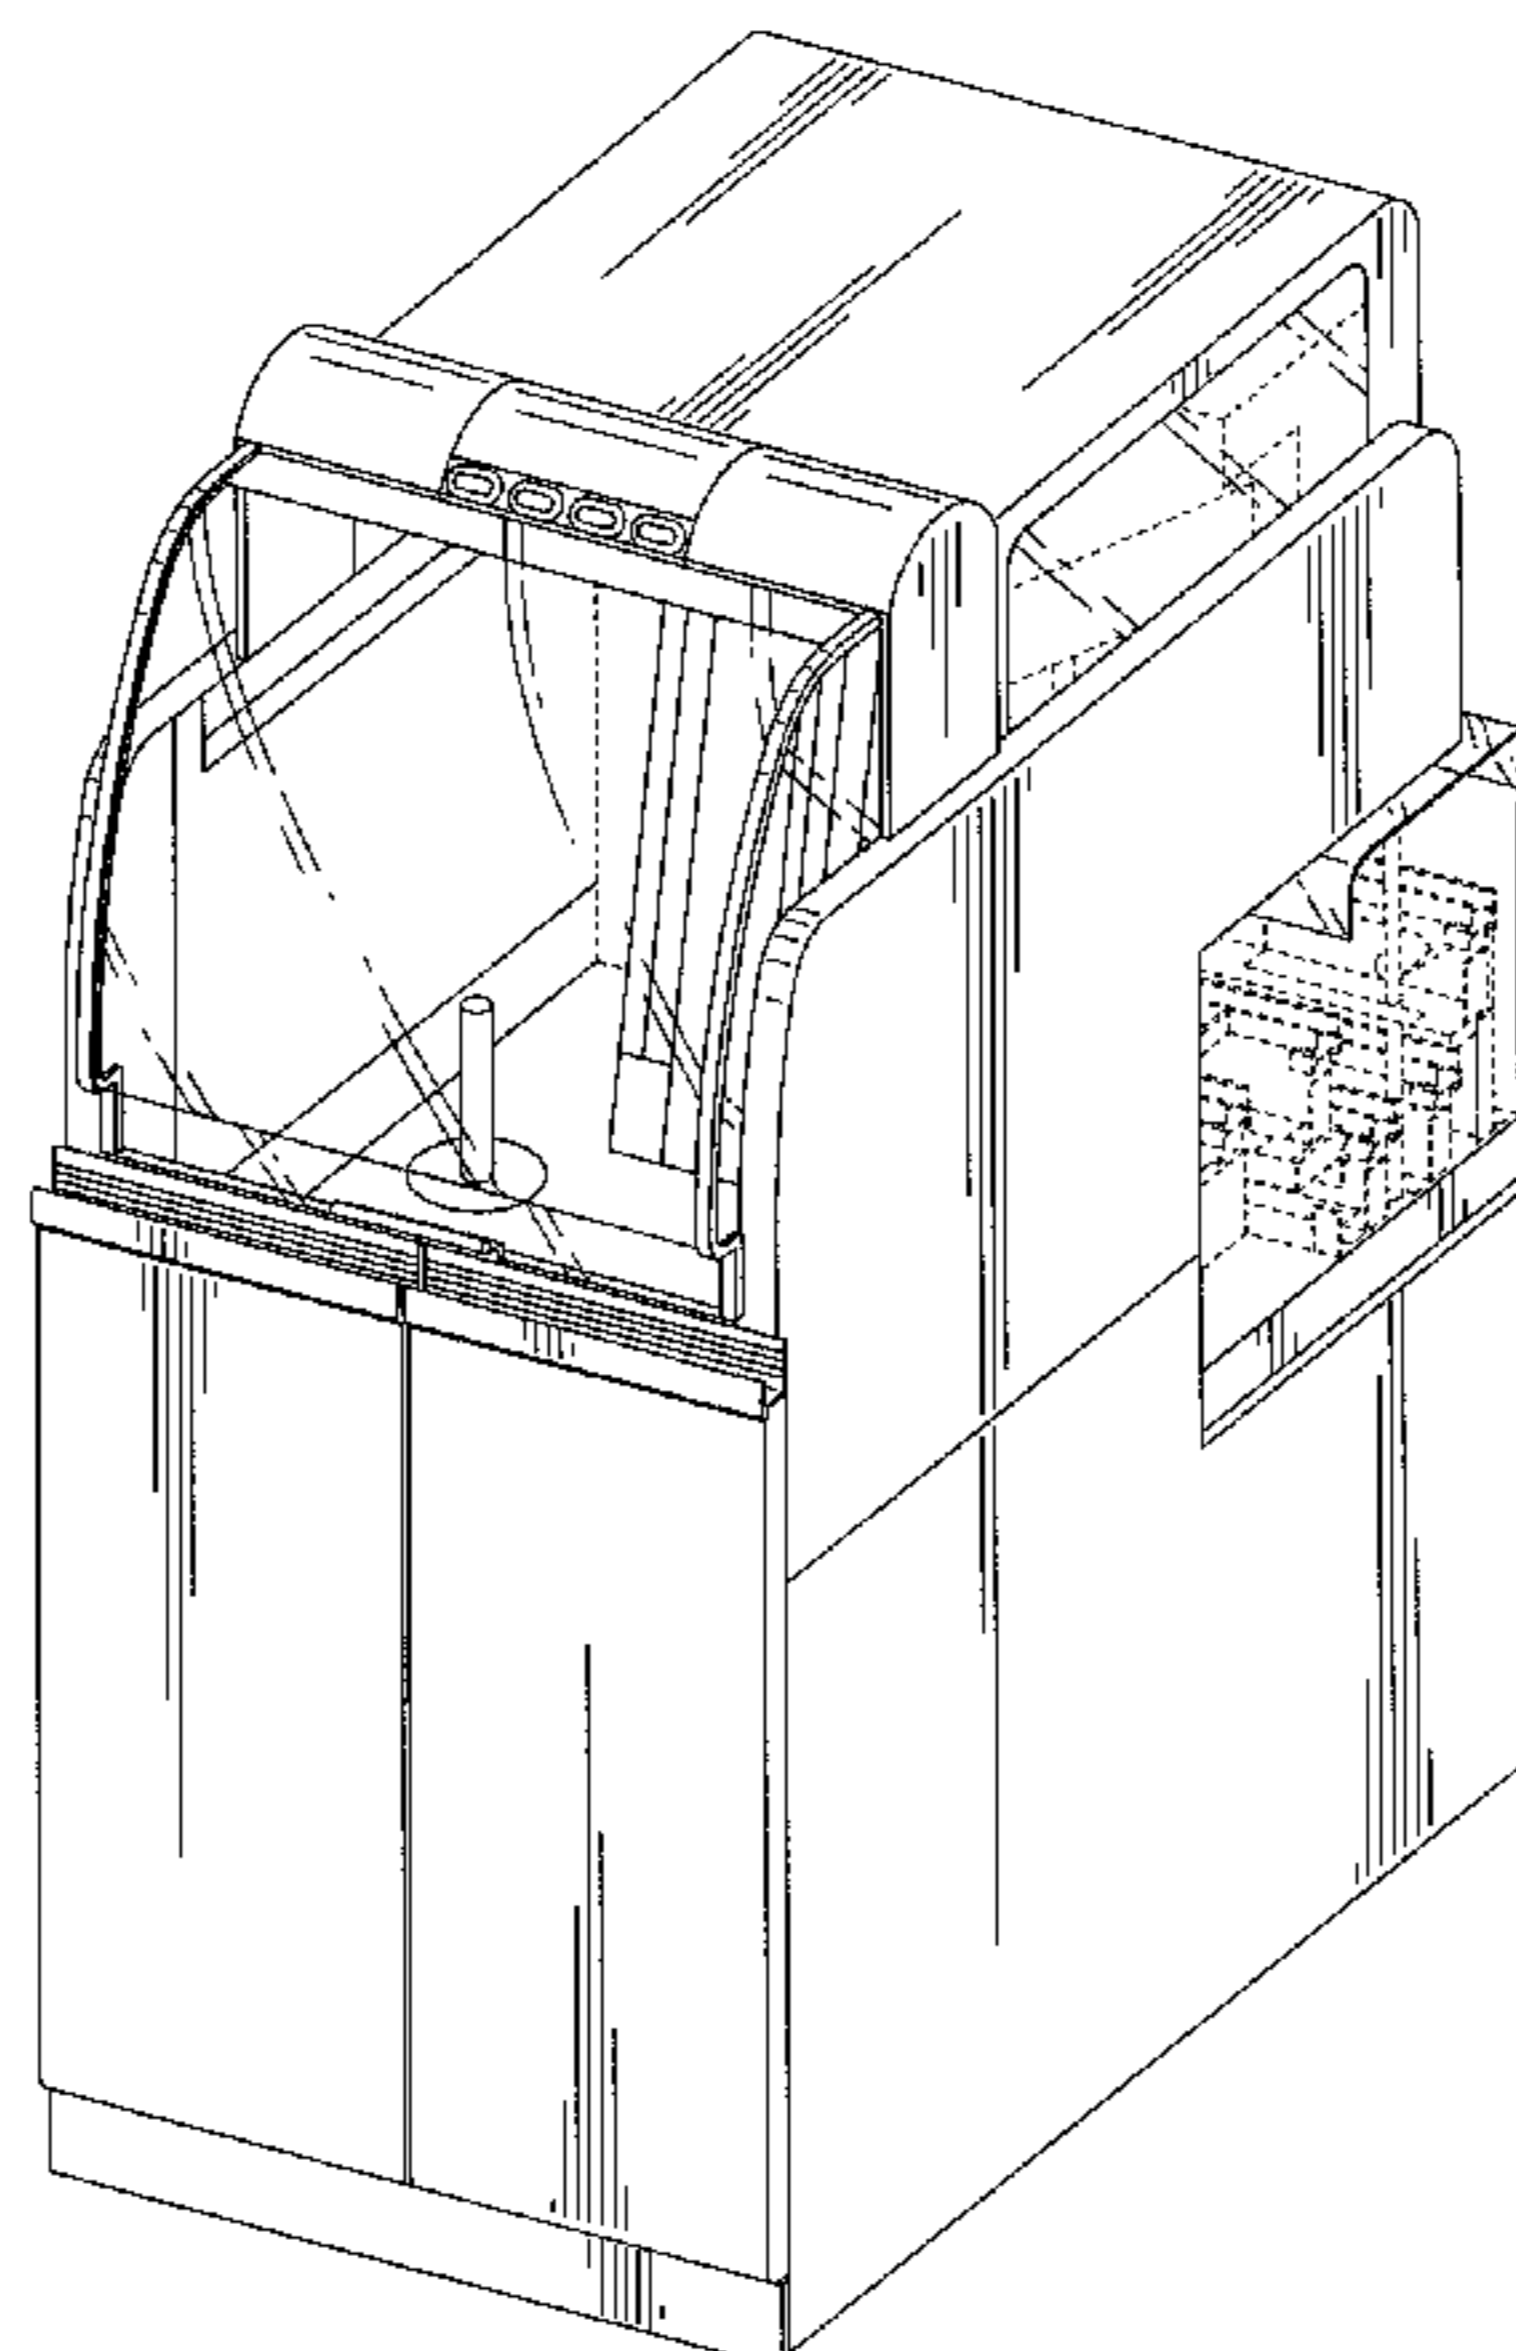

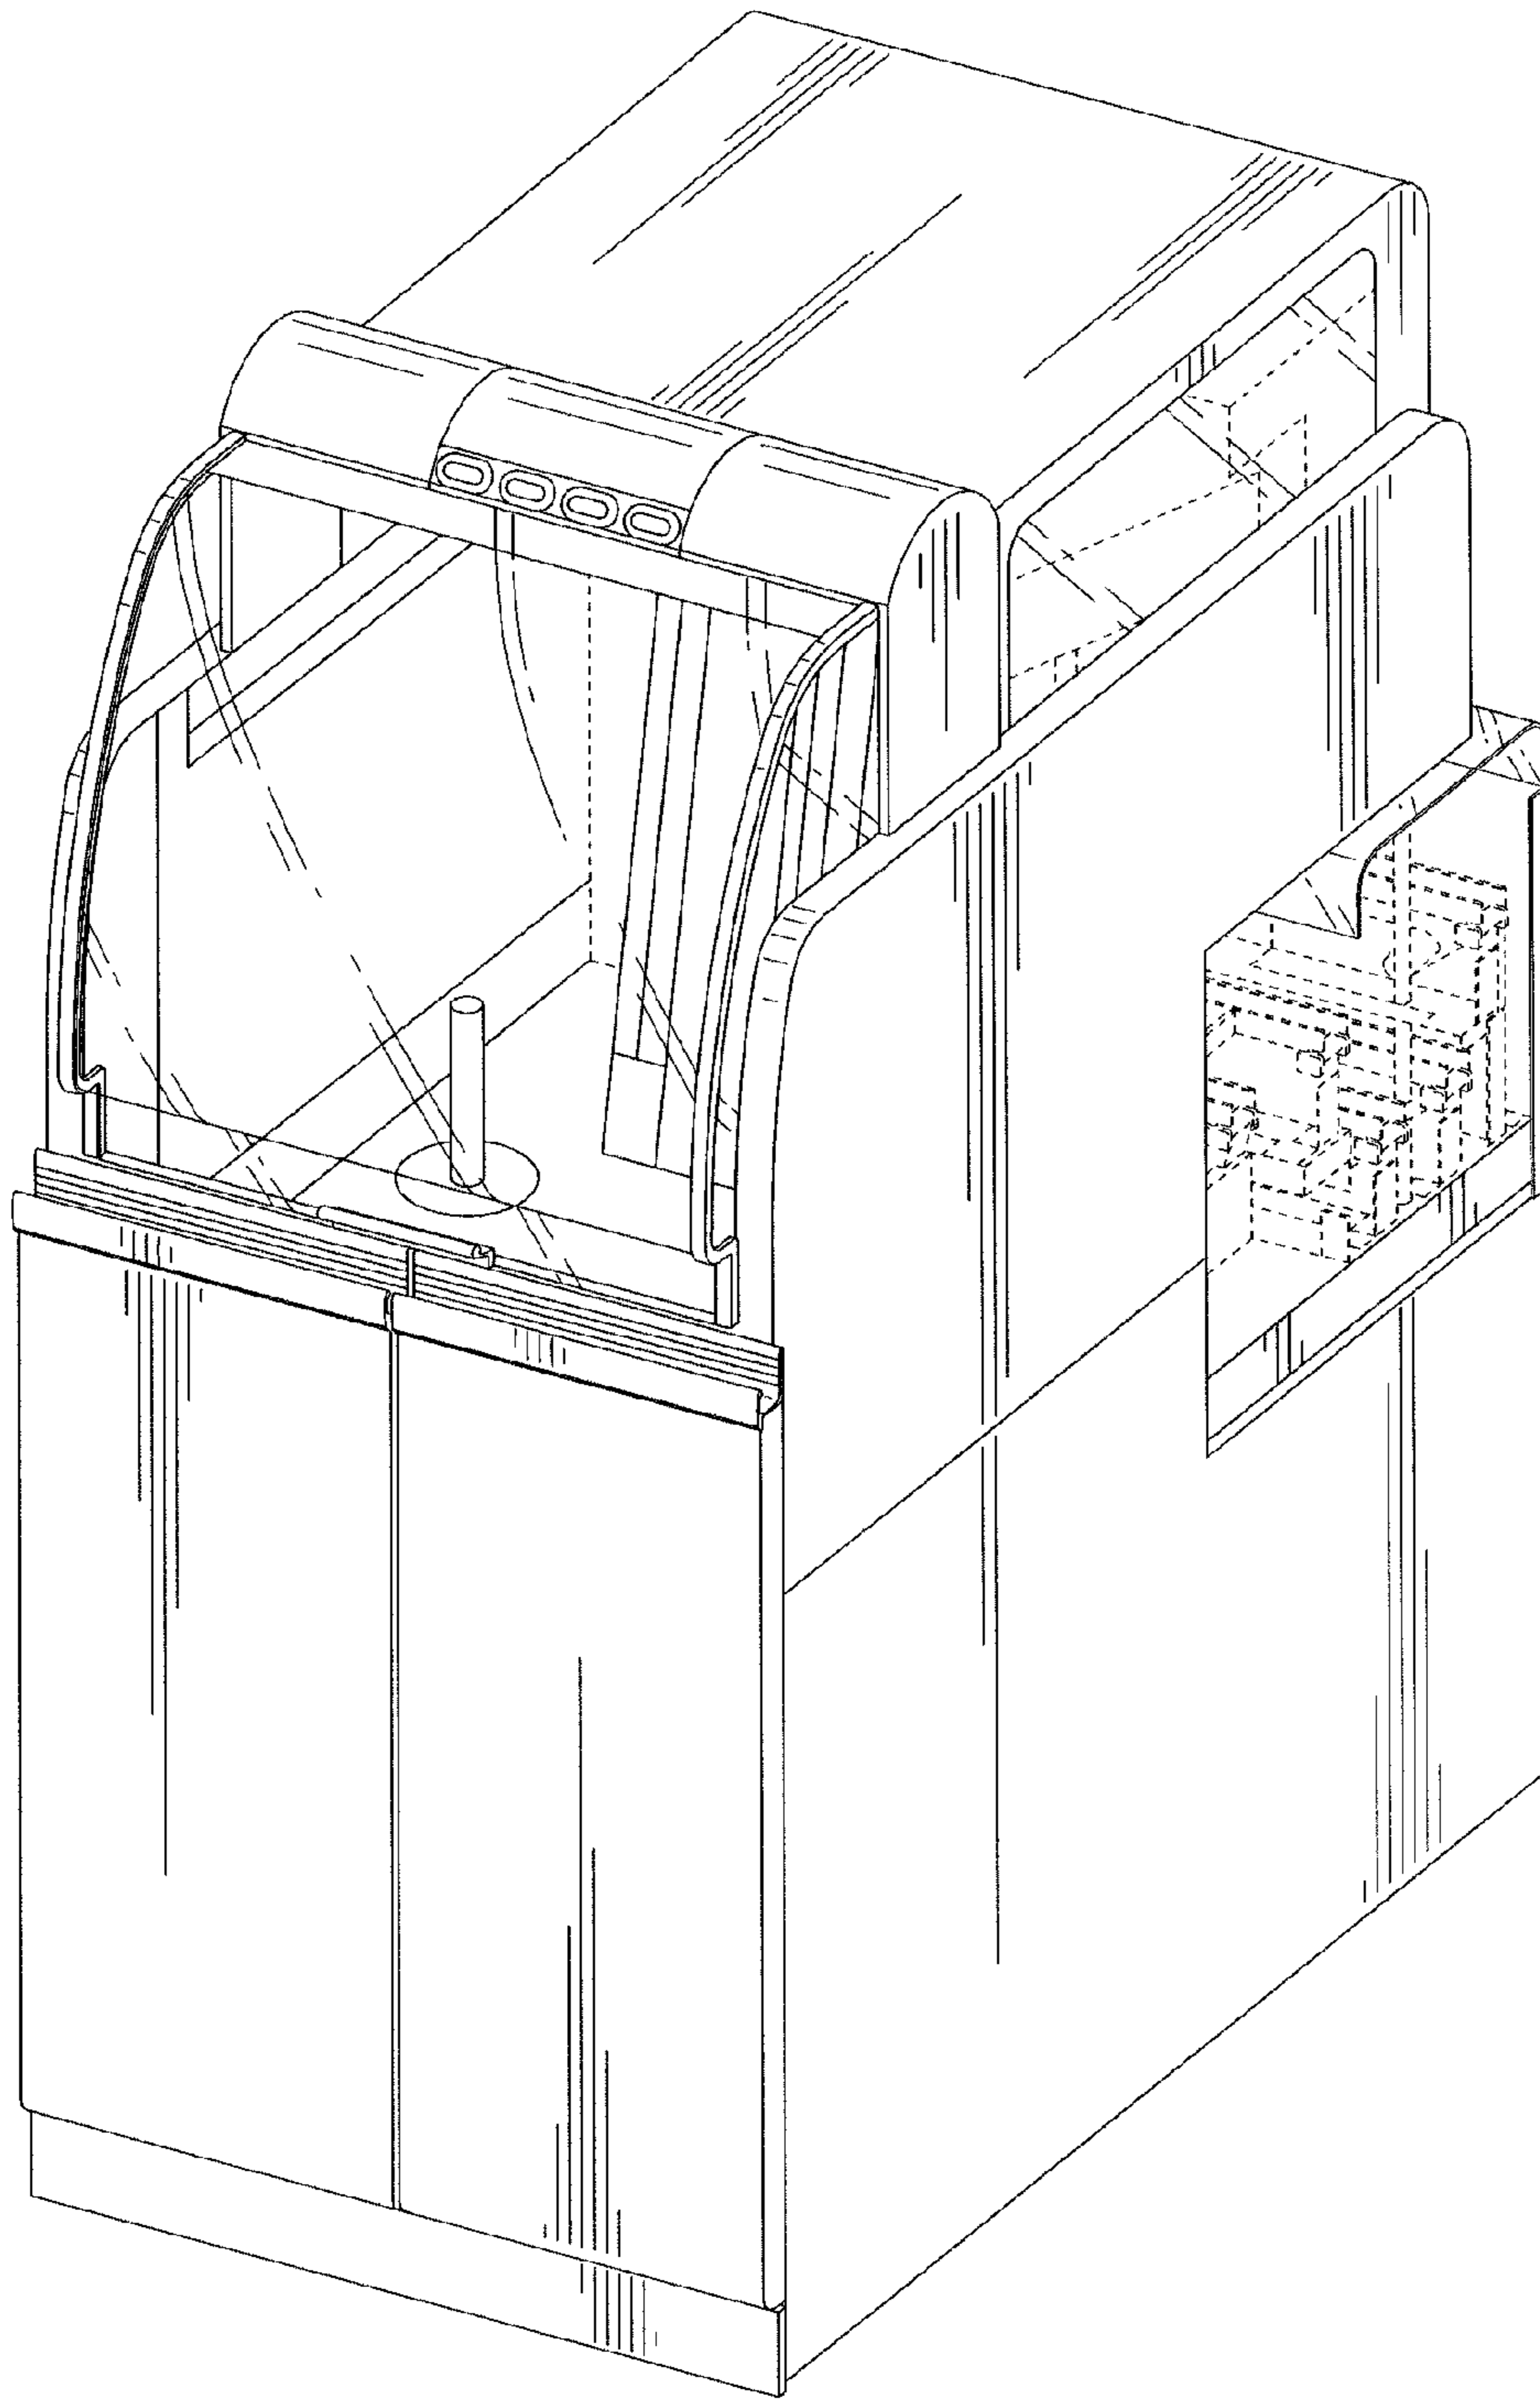

**FIG. 1**

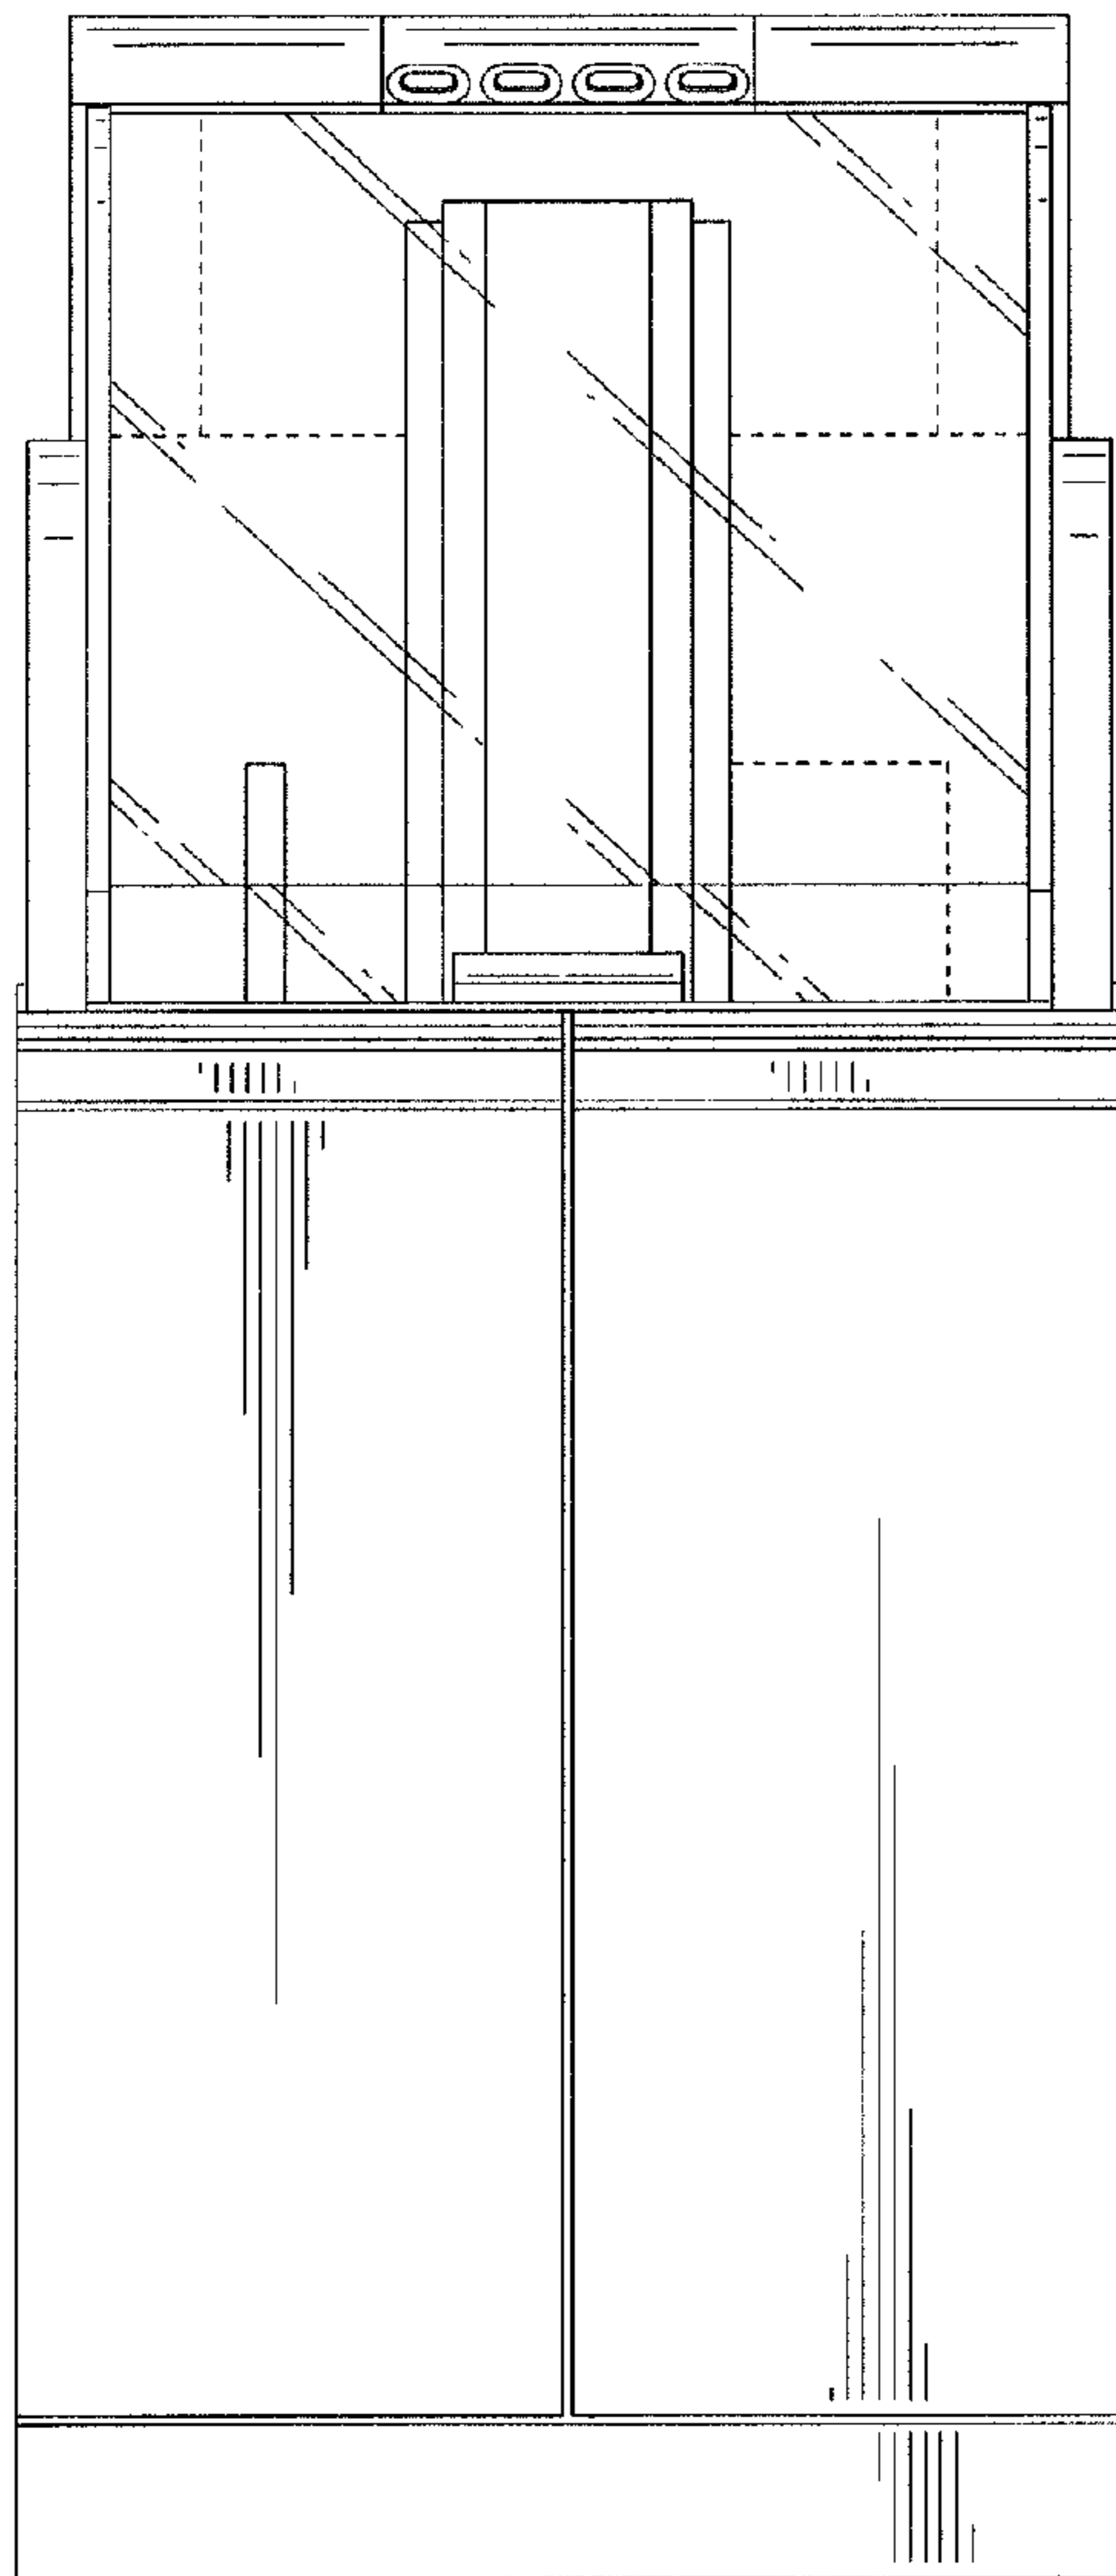


FIG. 2



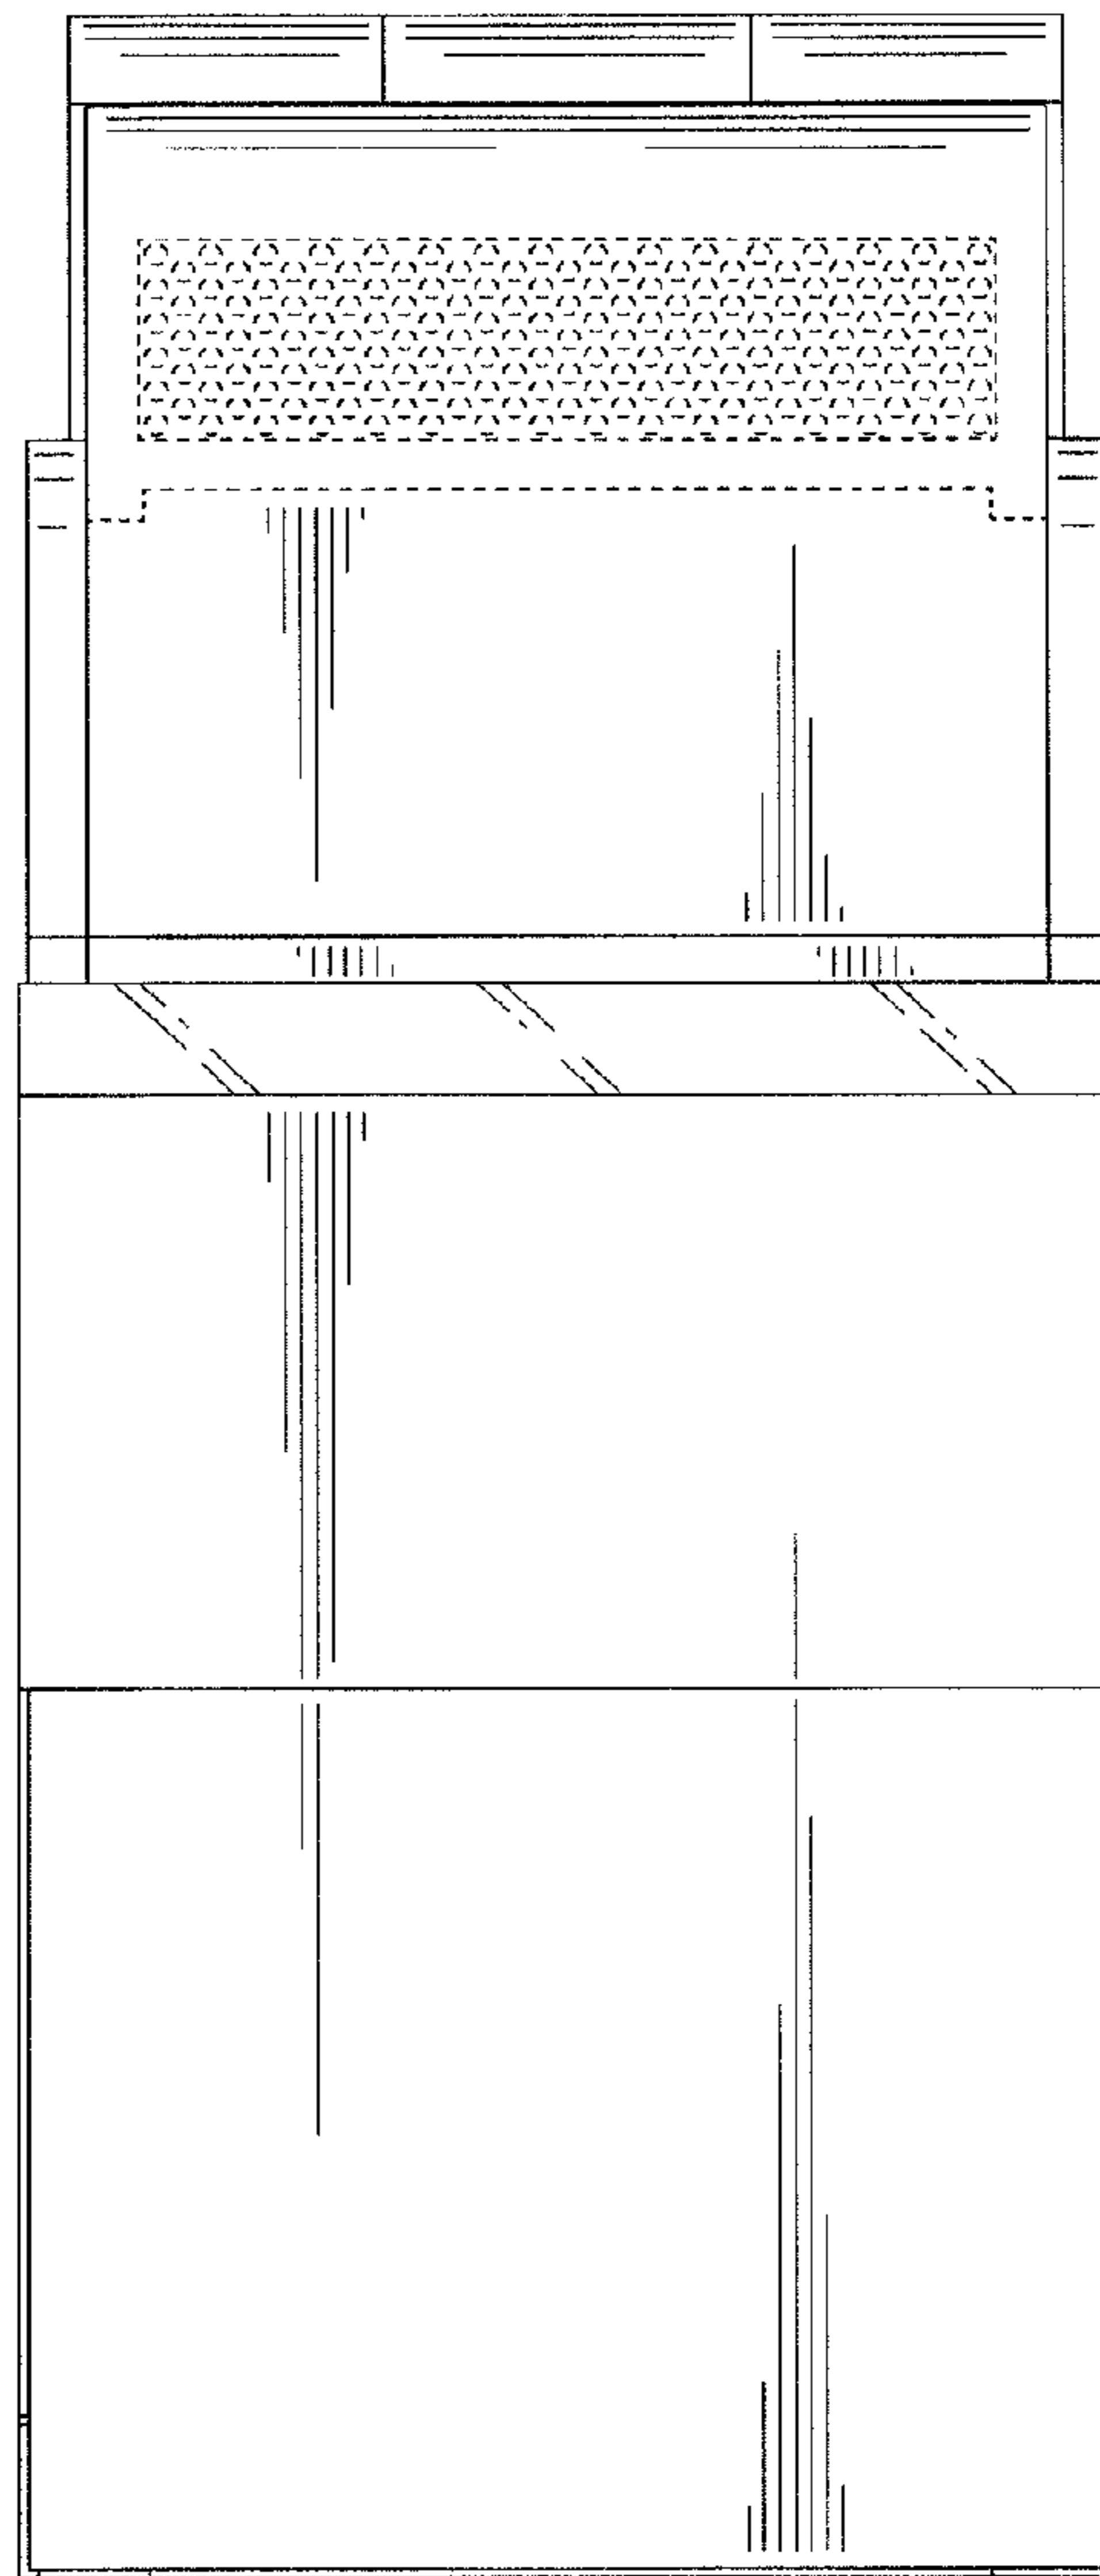


FIG. 3

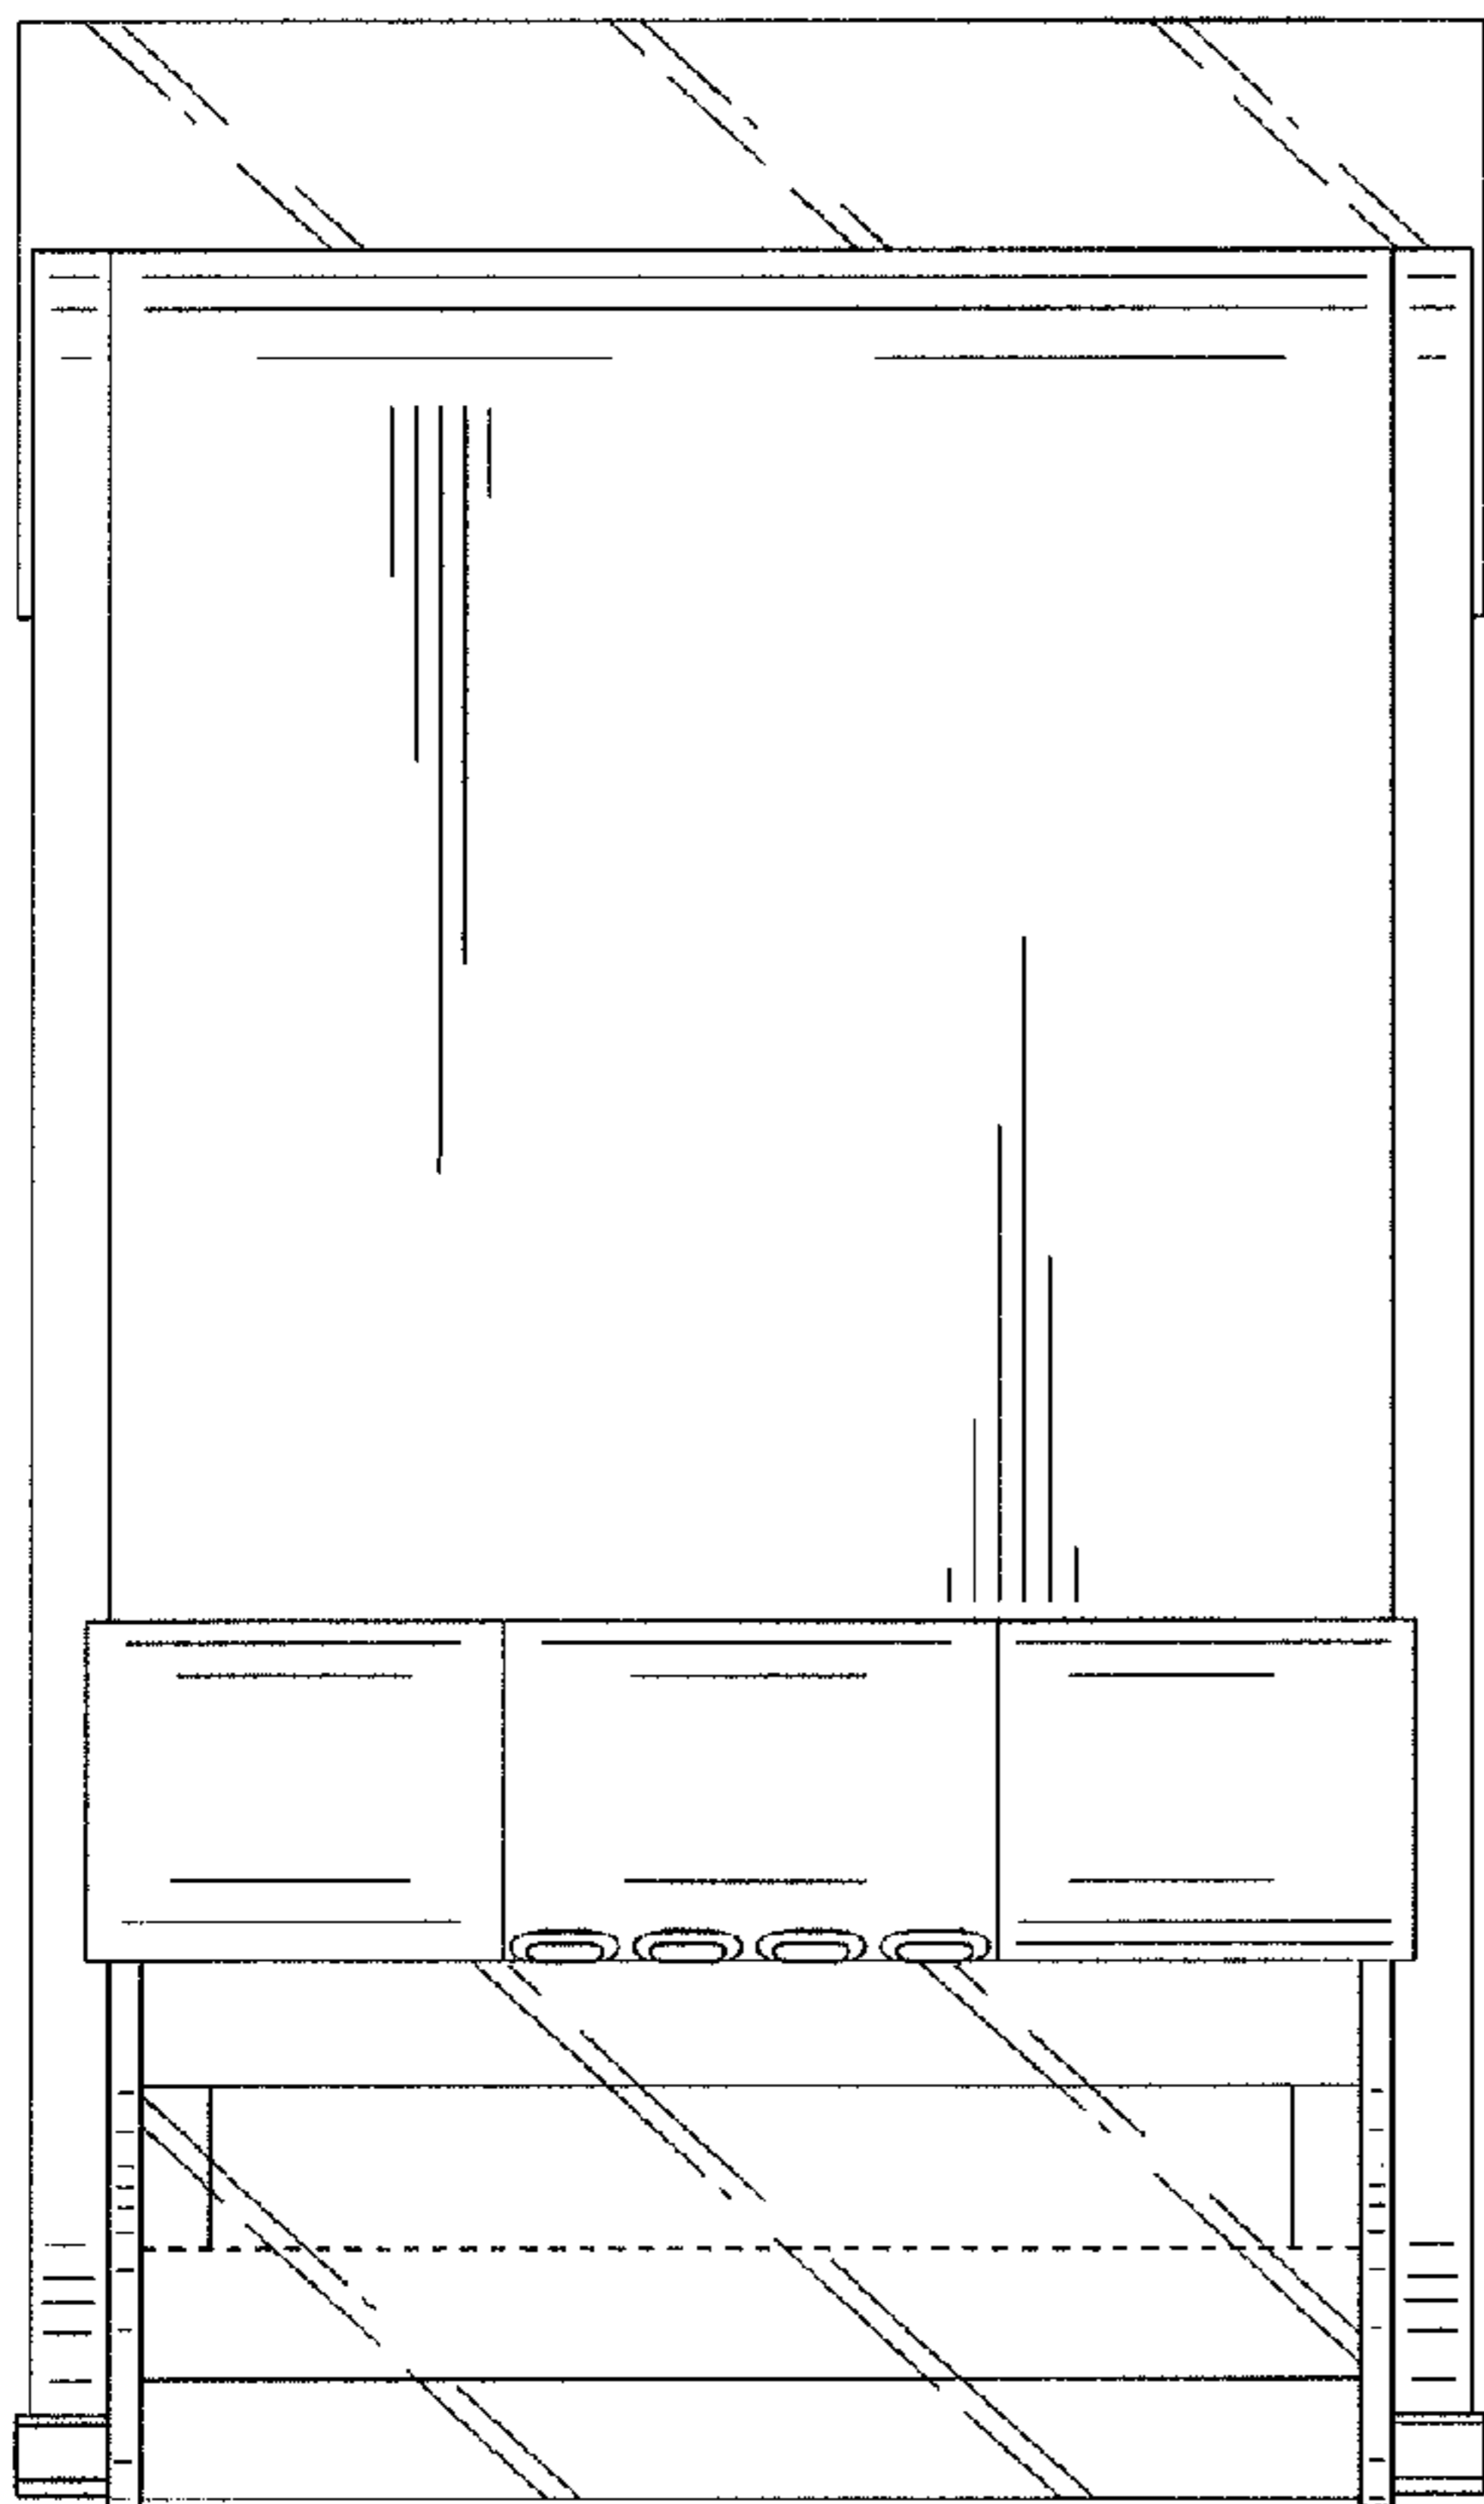

*FIG. 4*

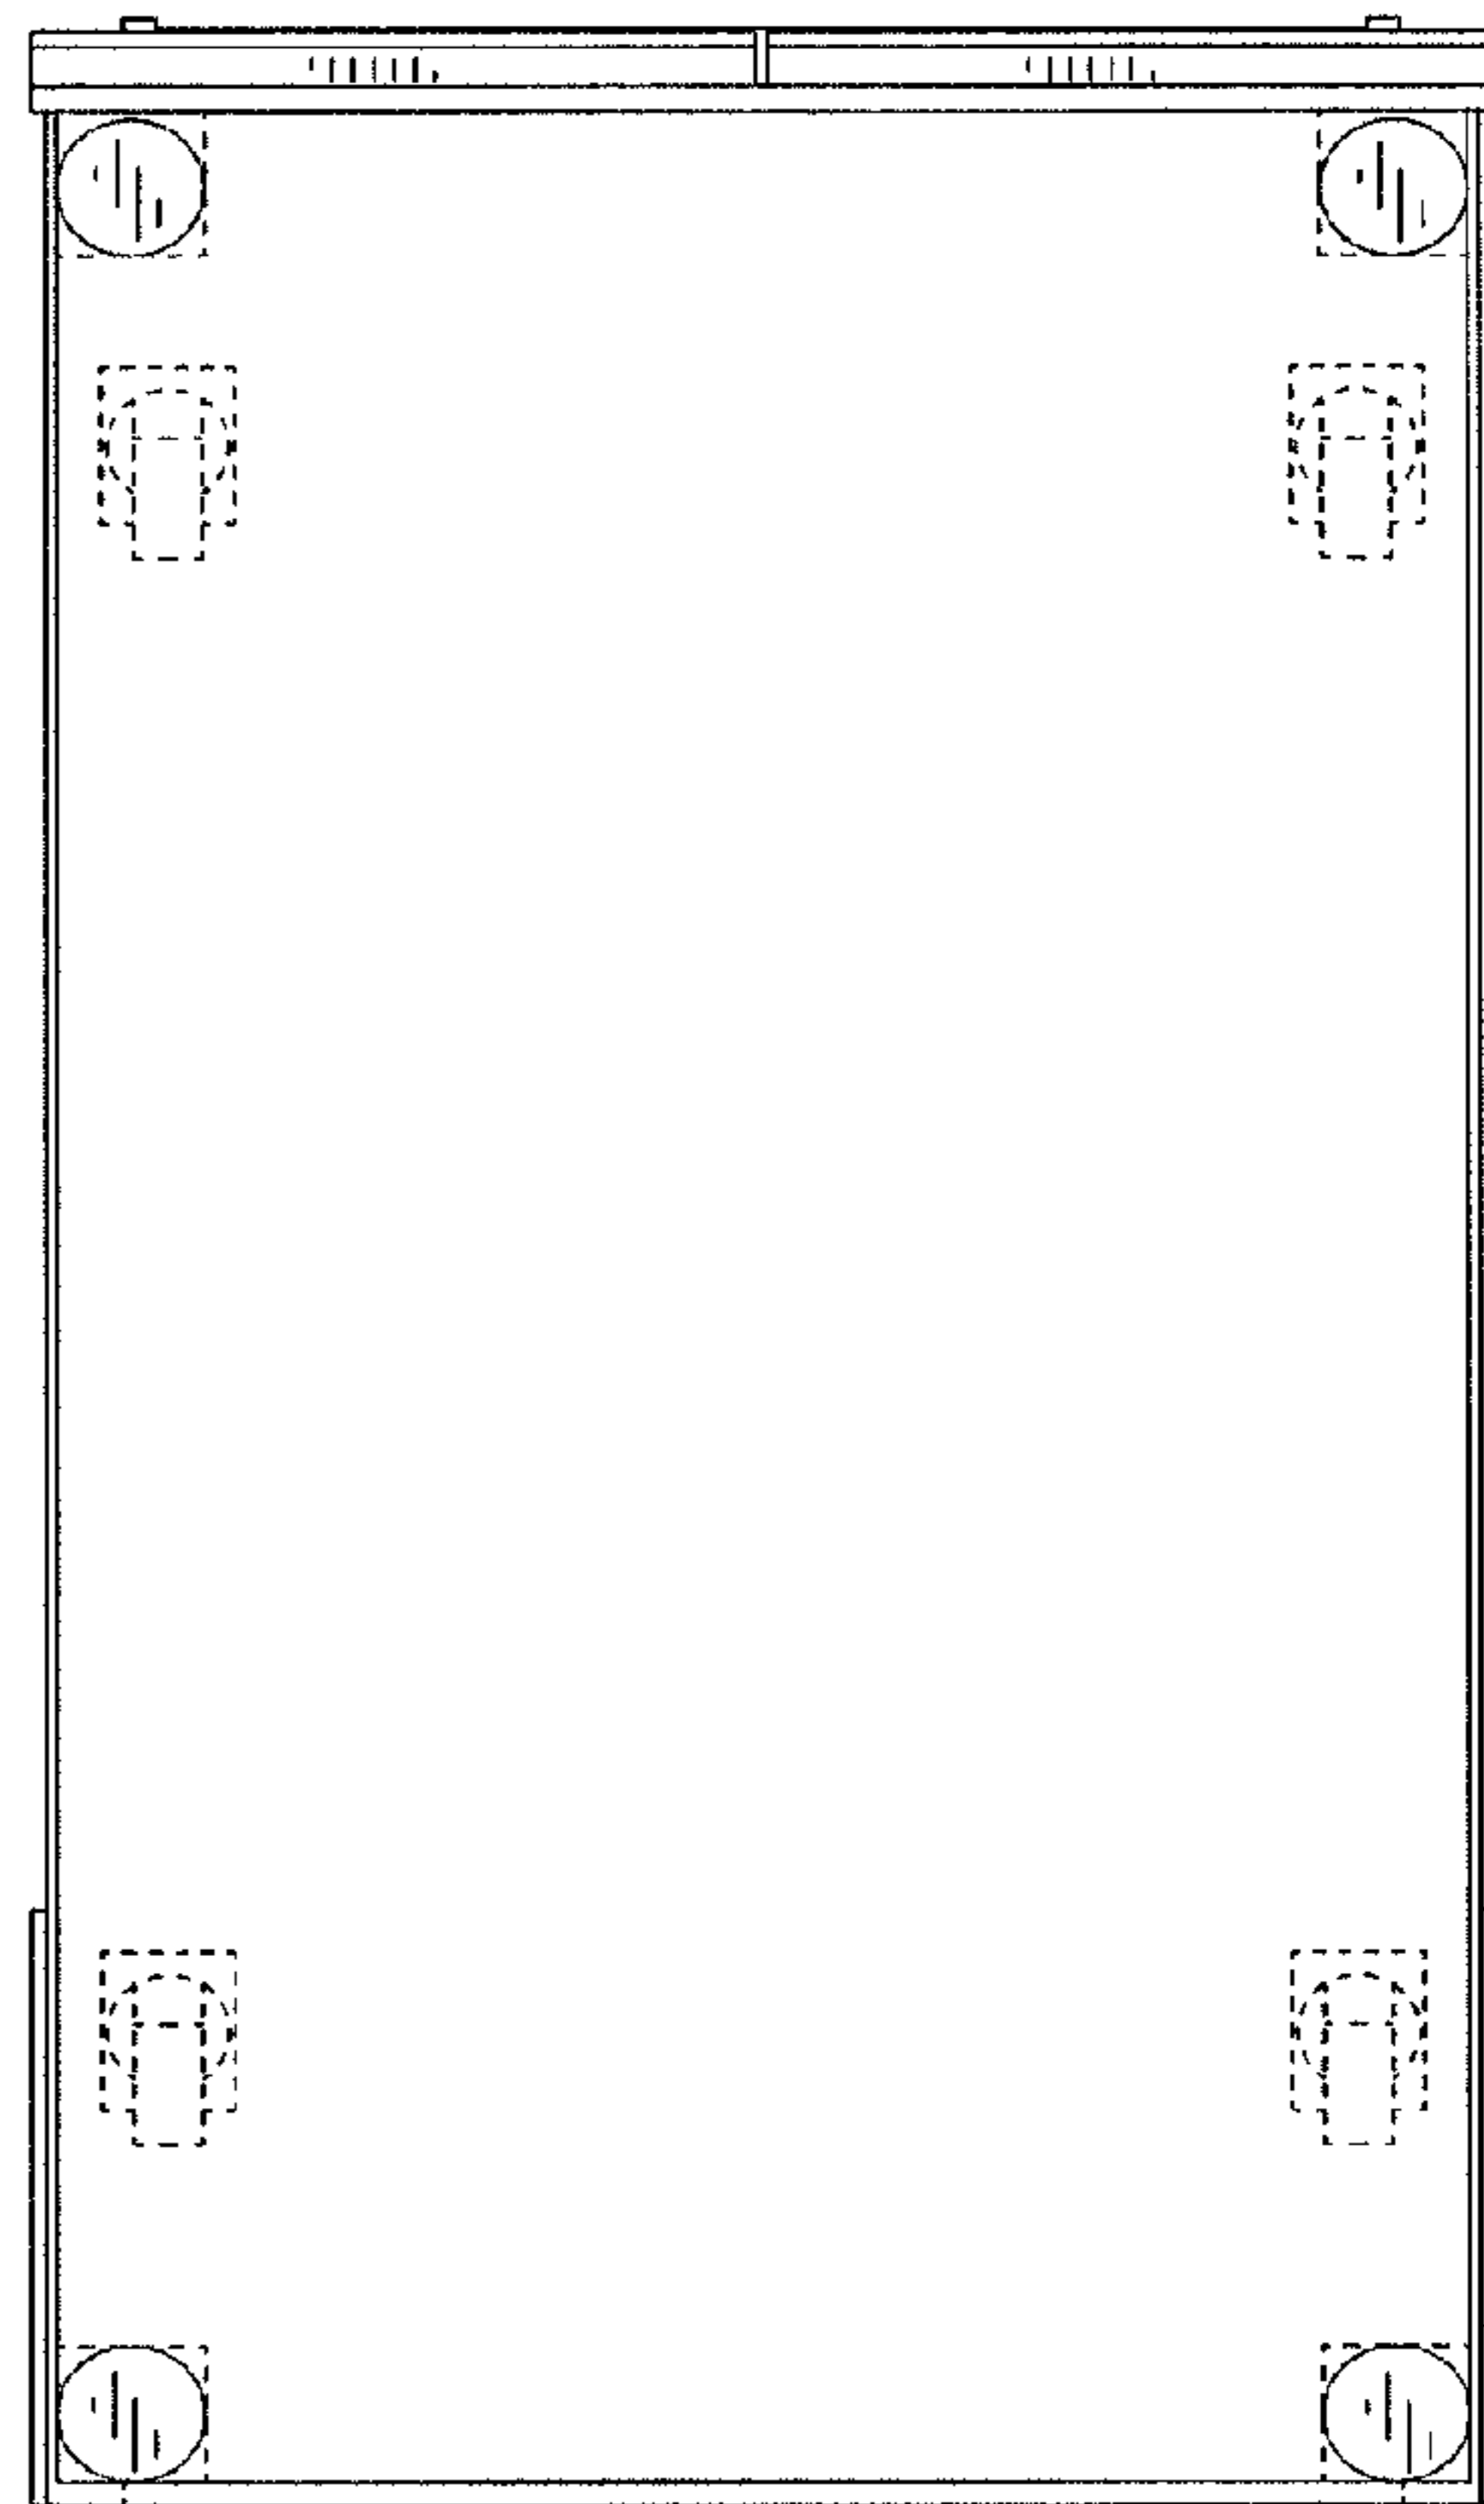

*FIG. 5*

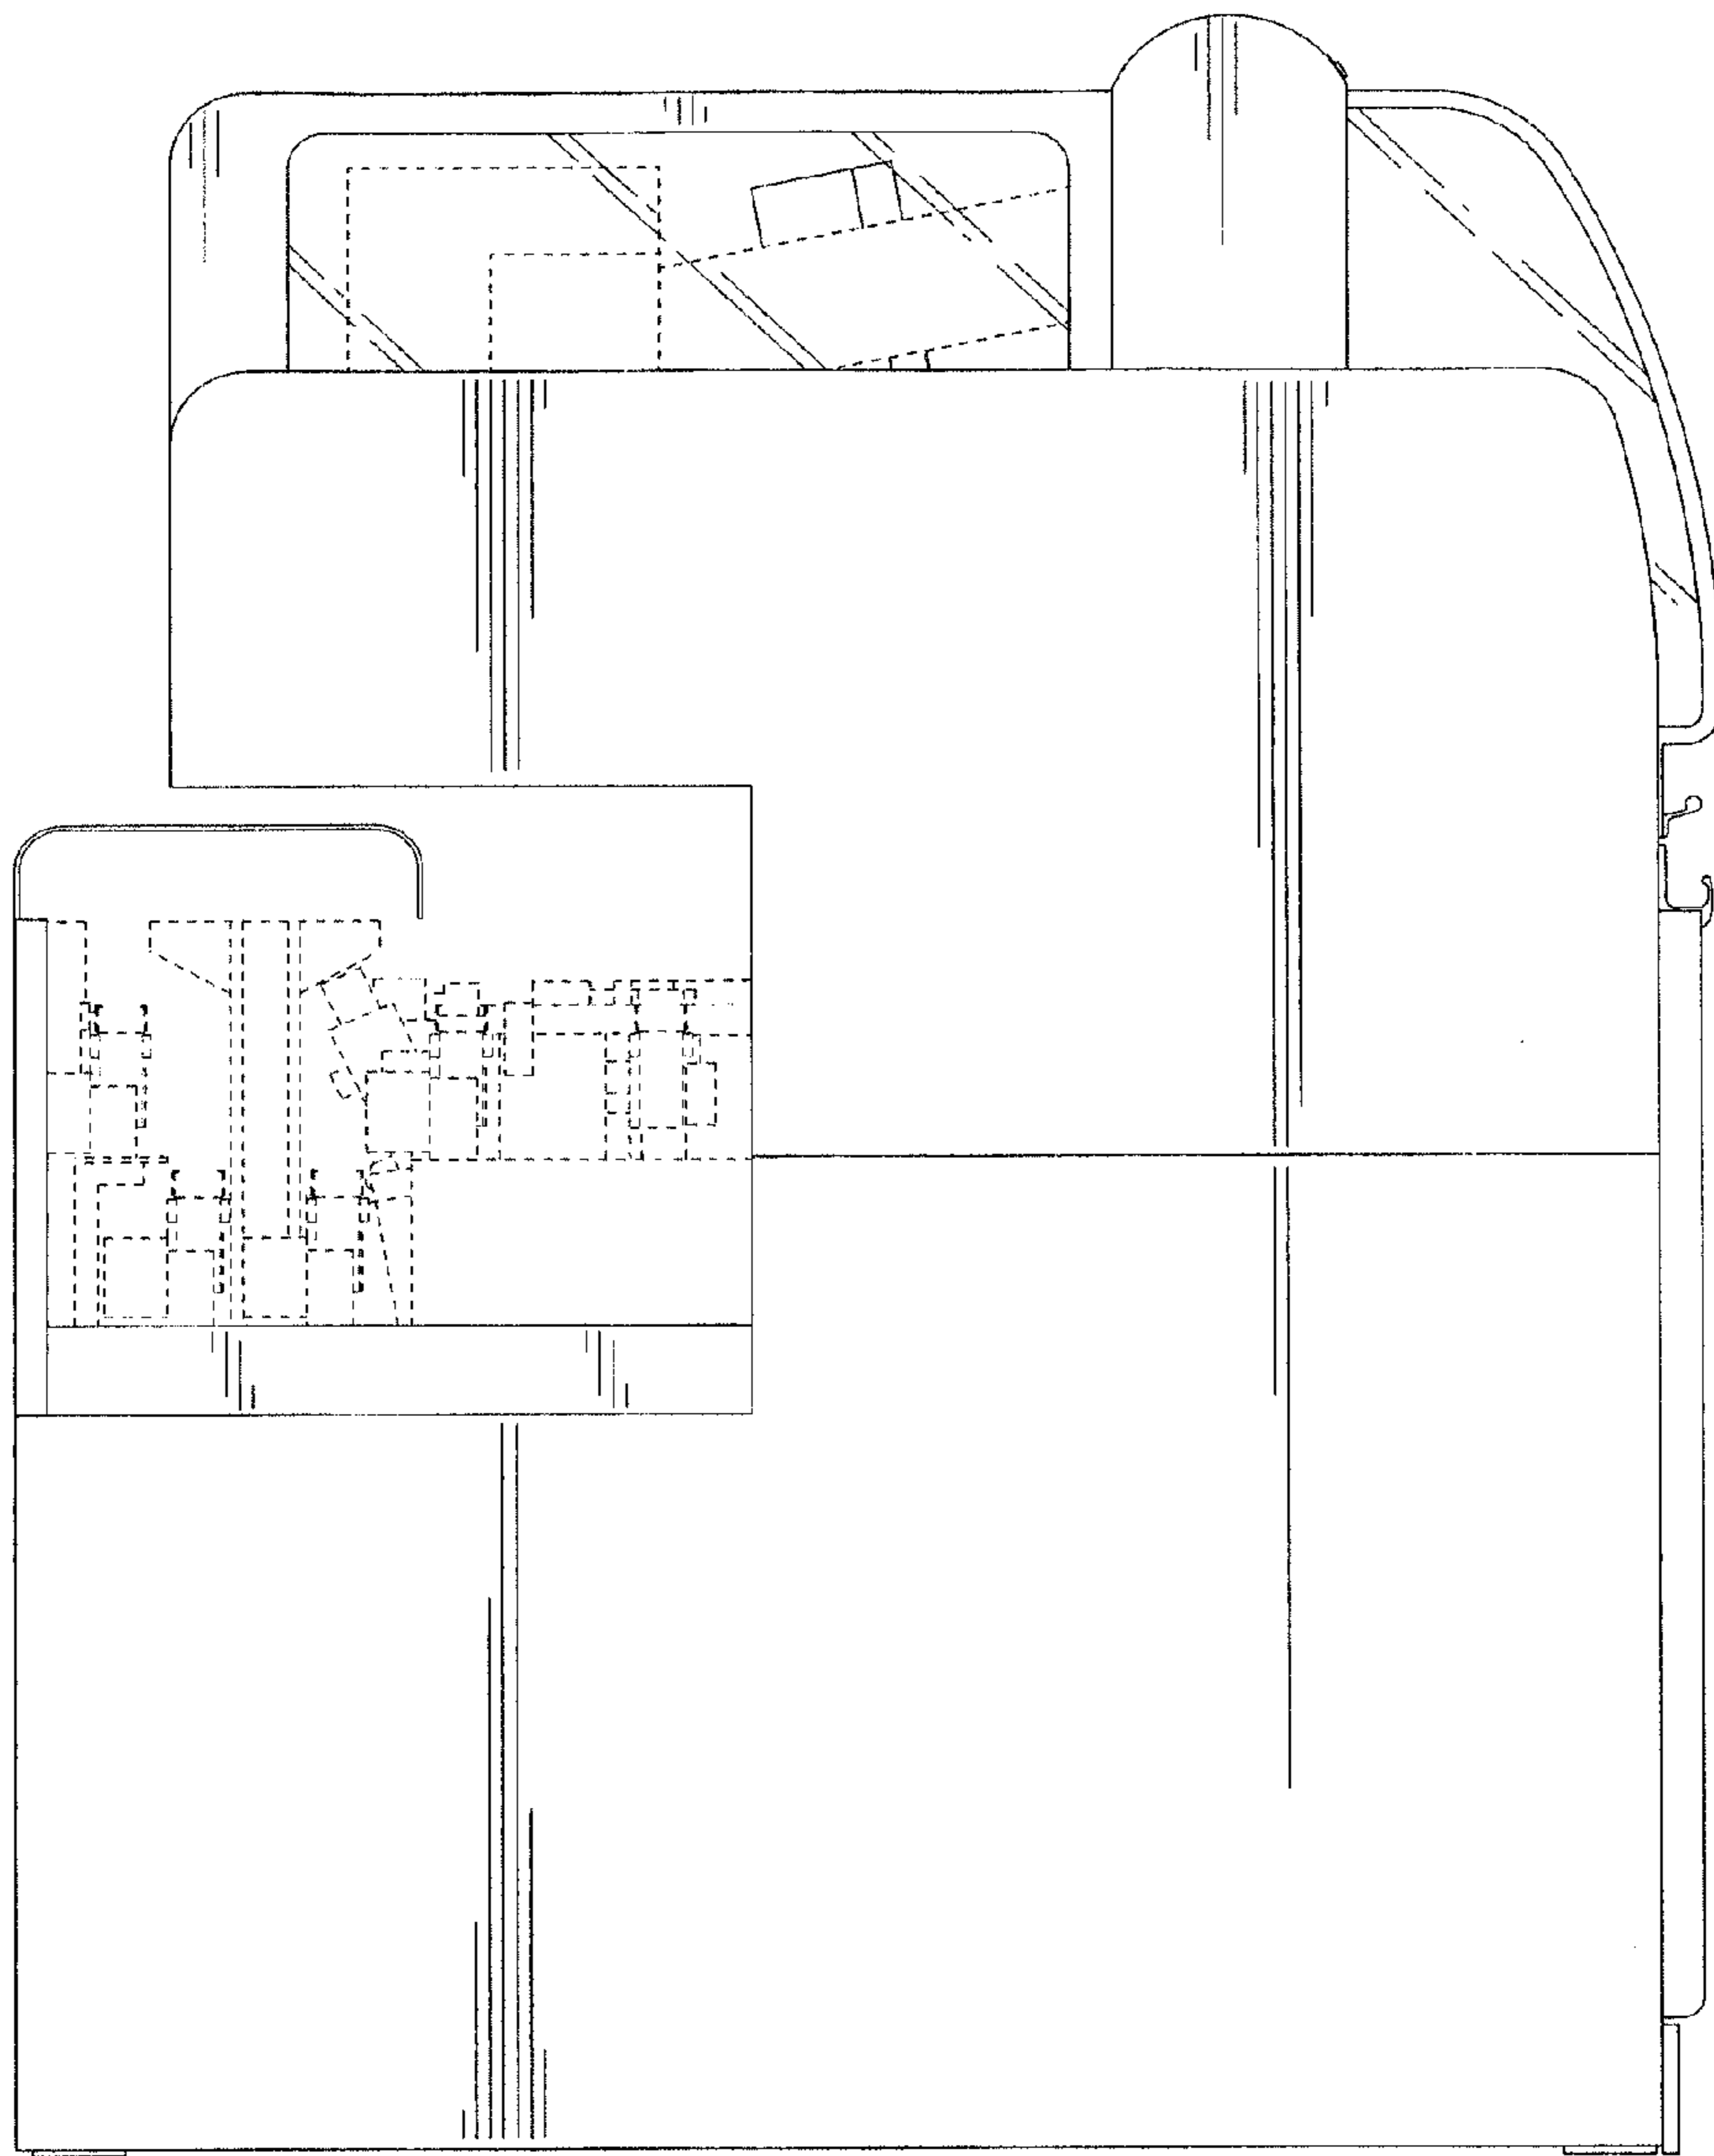


FIG. 6

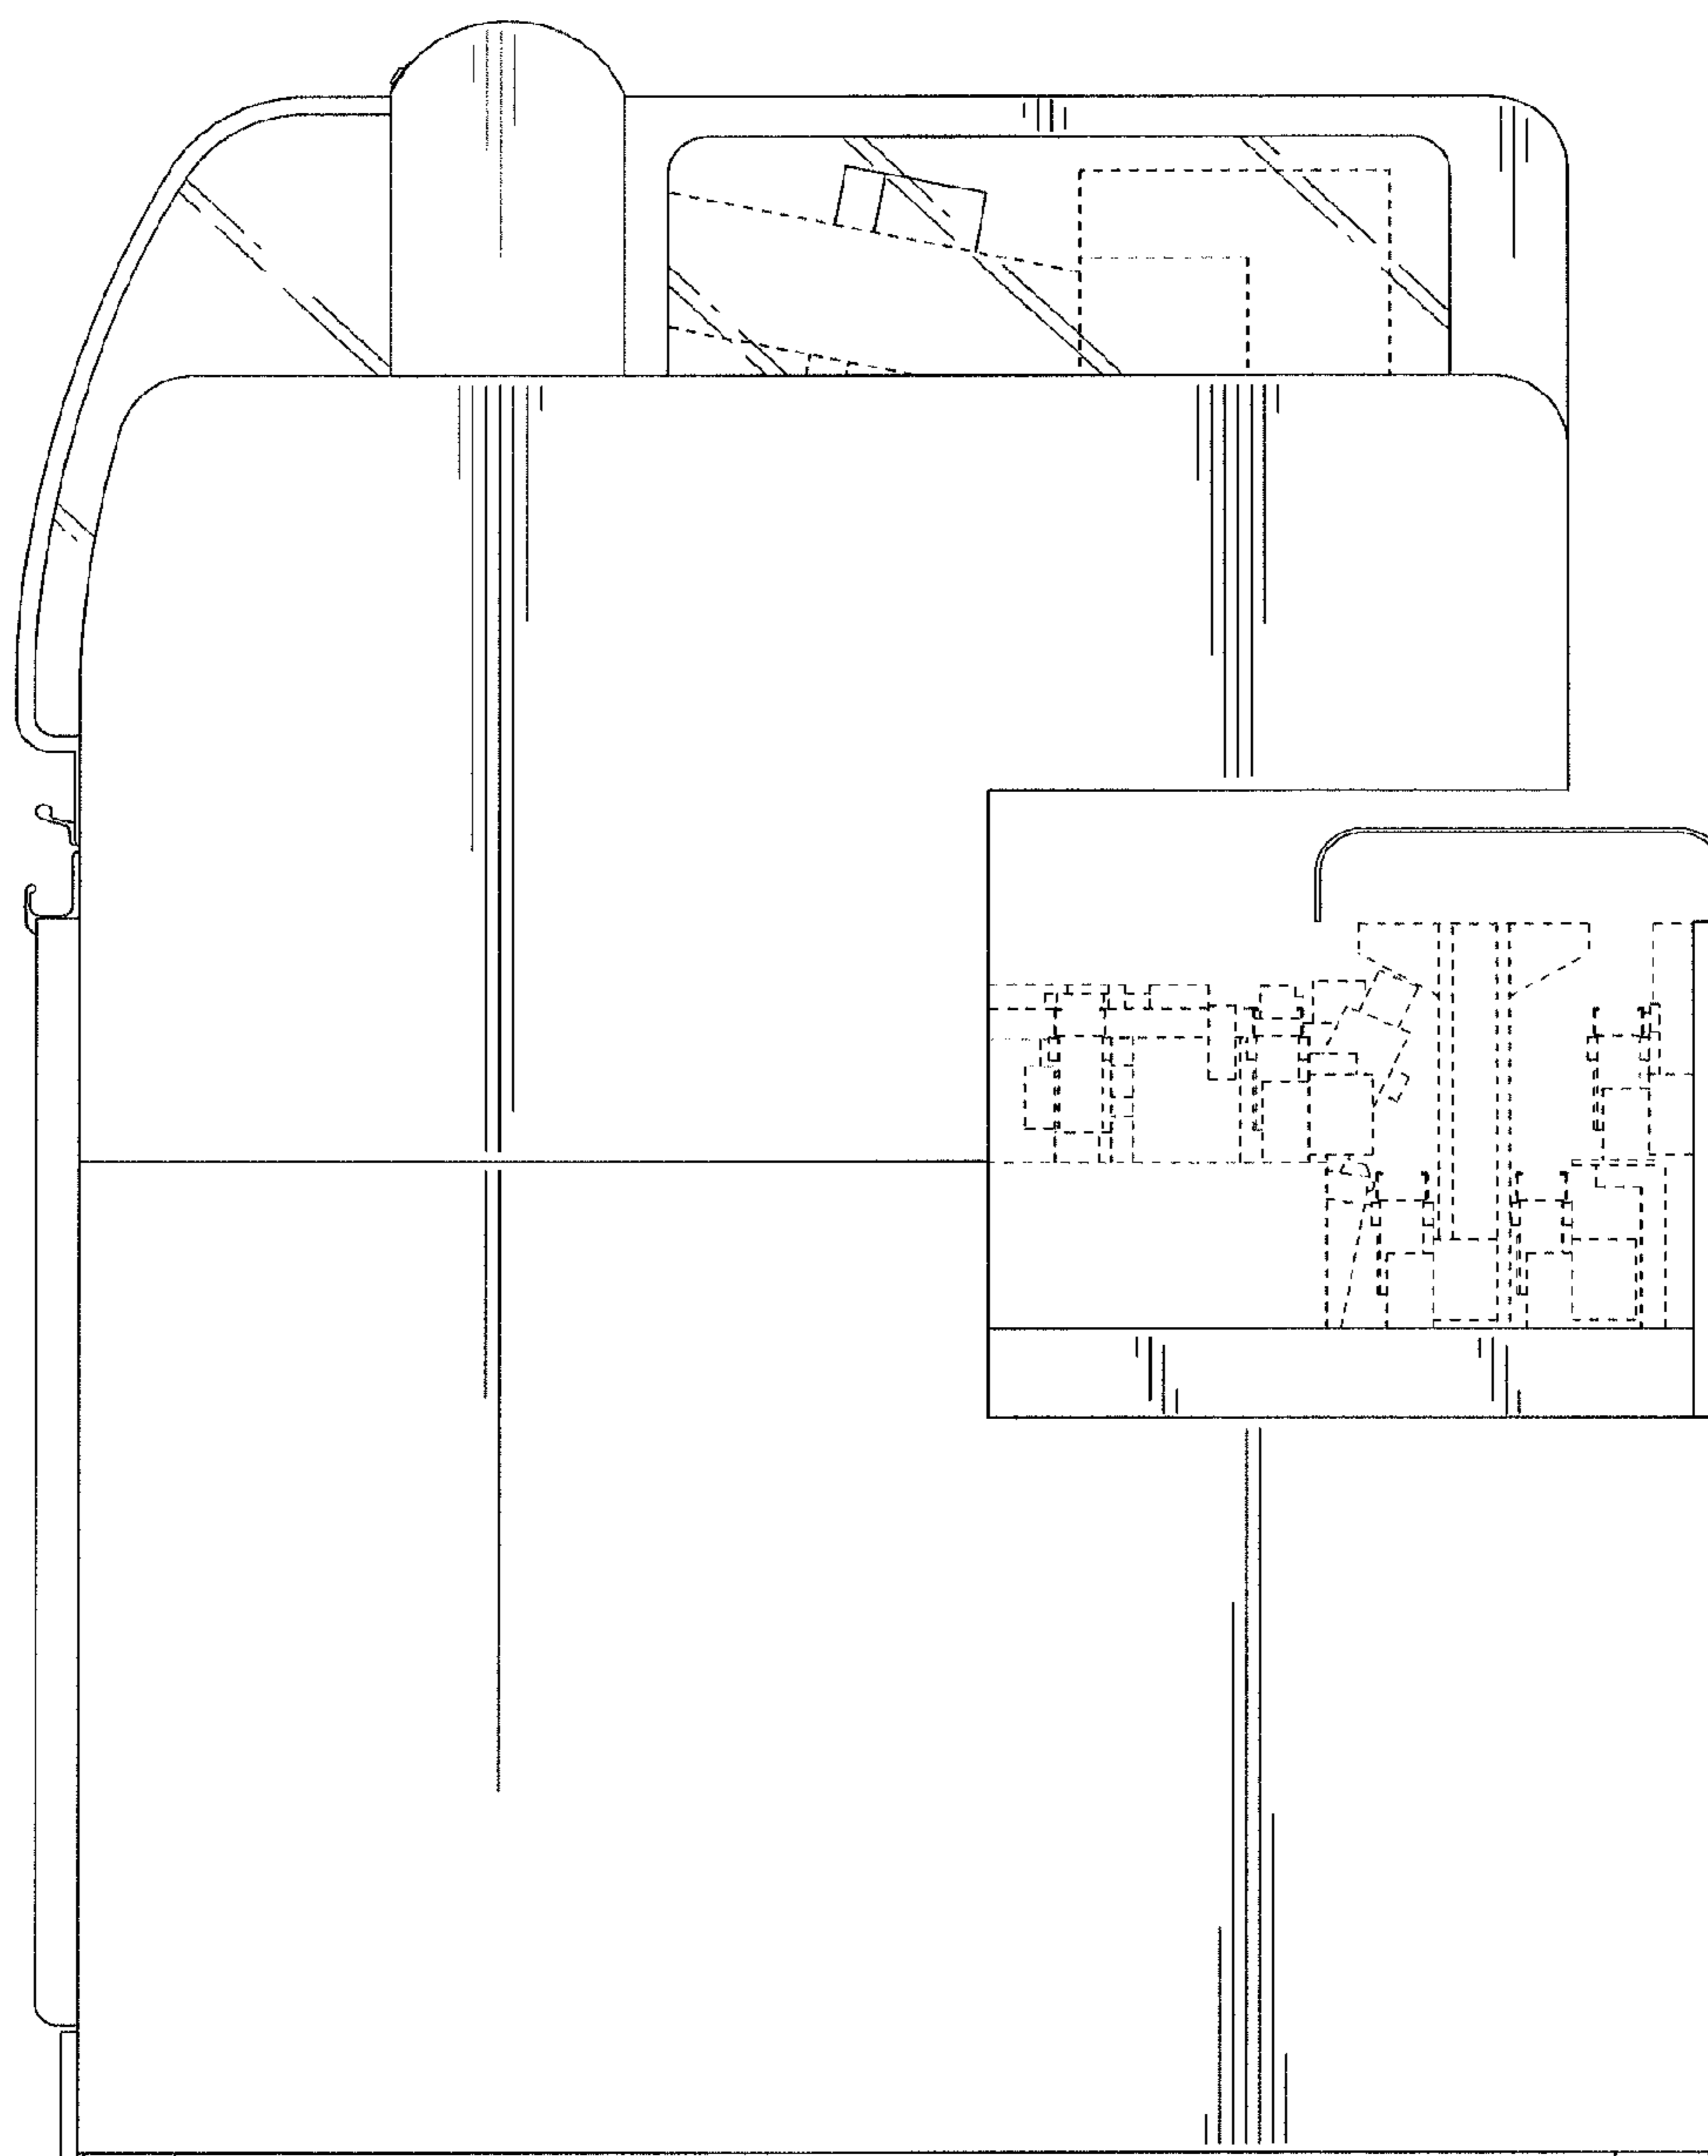


FIG. 7

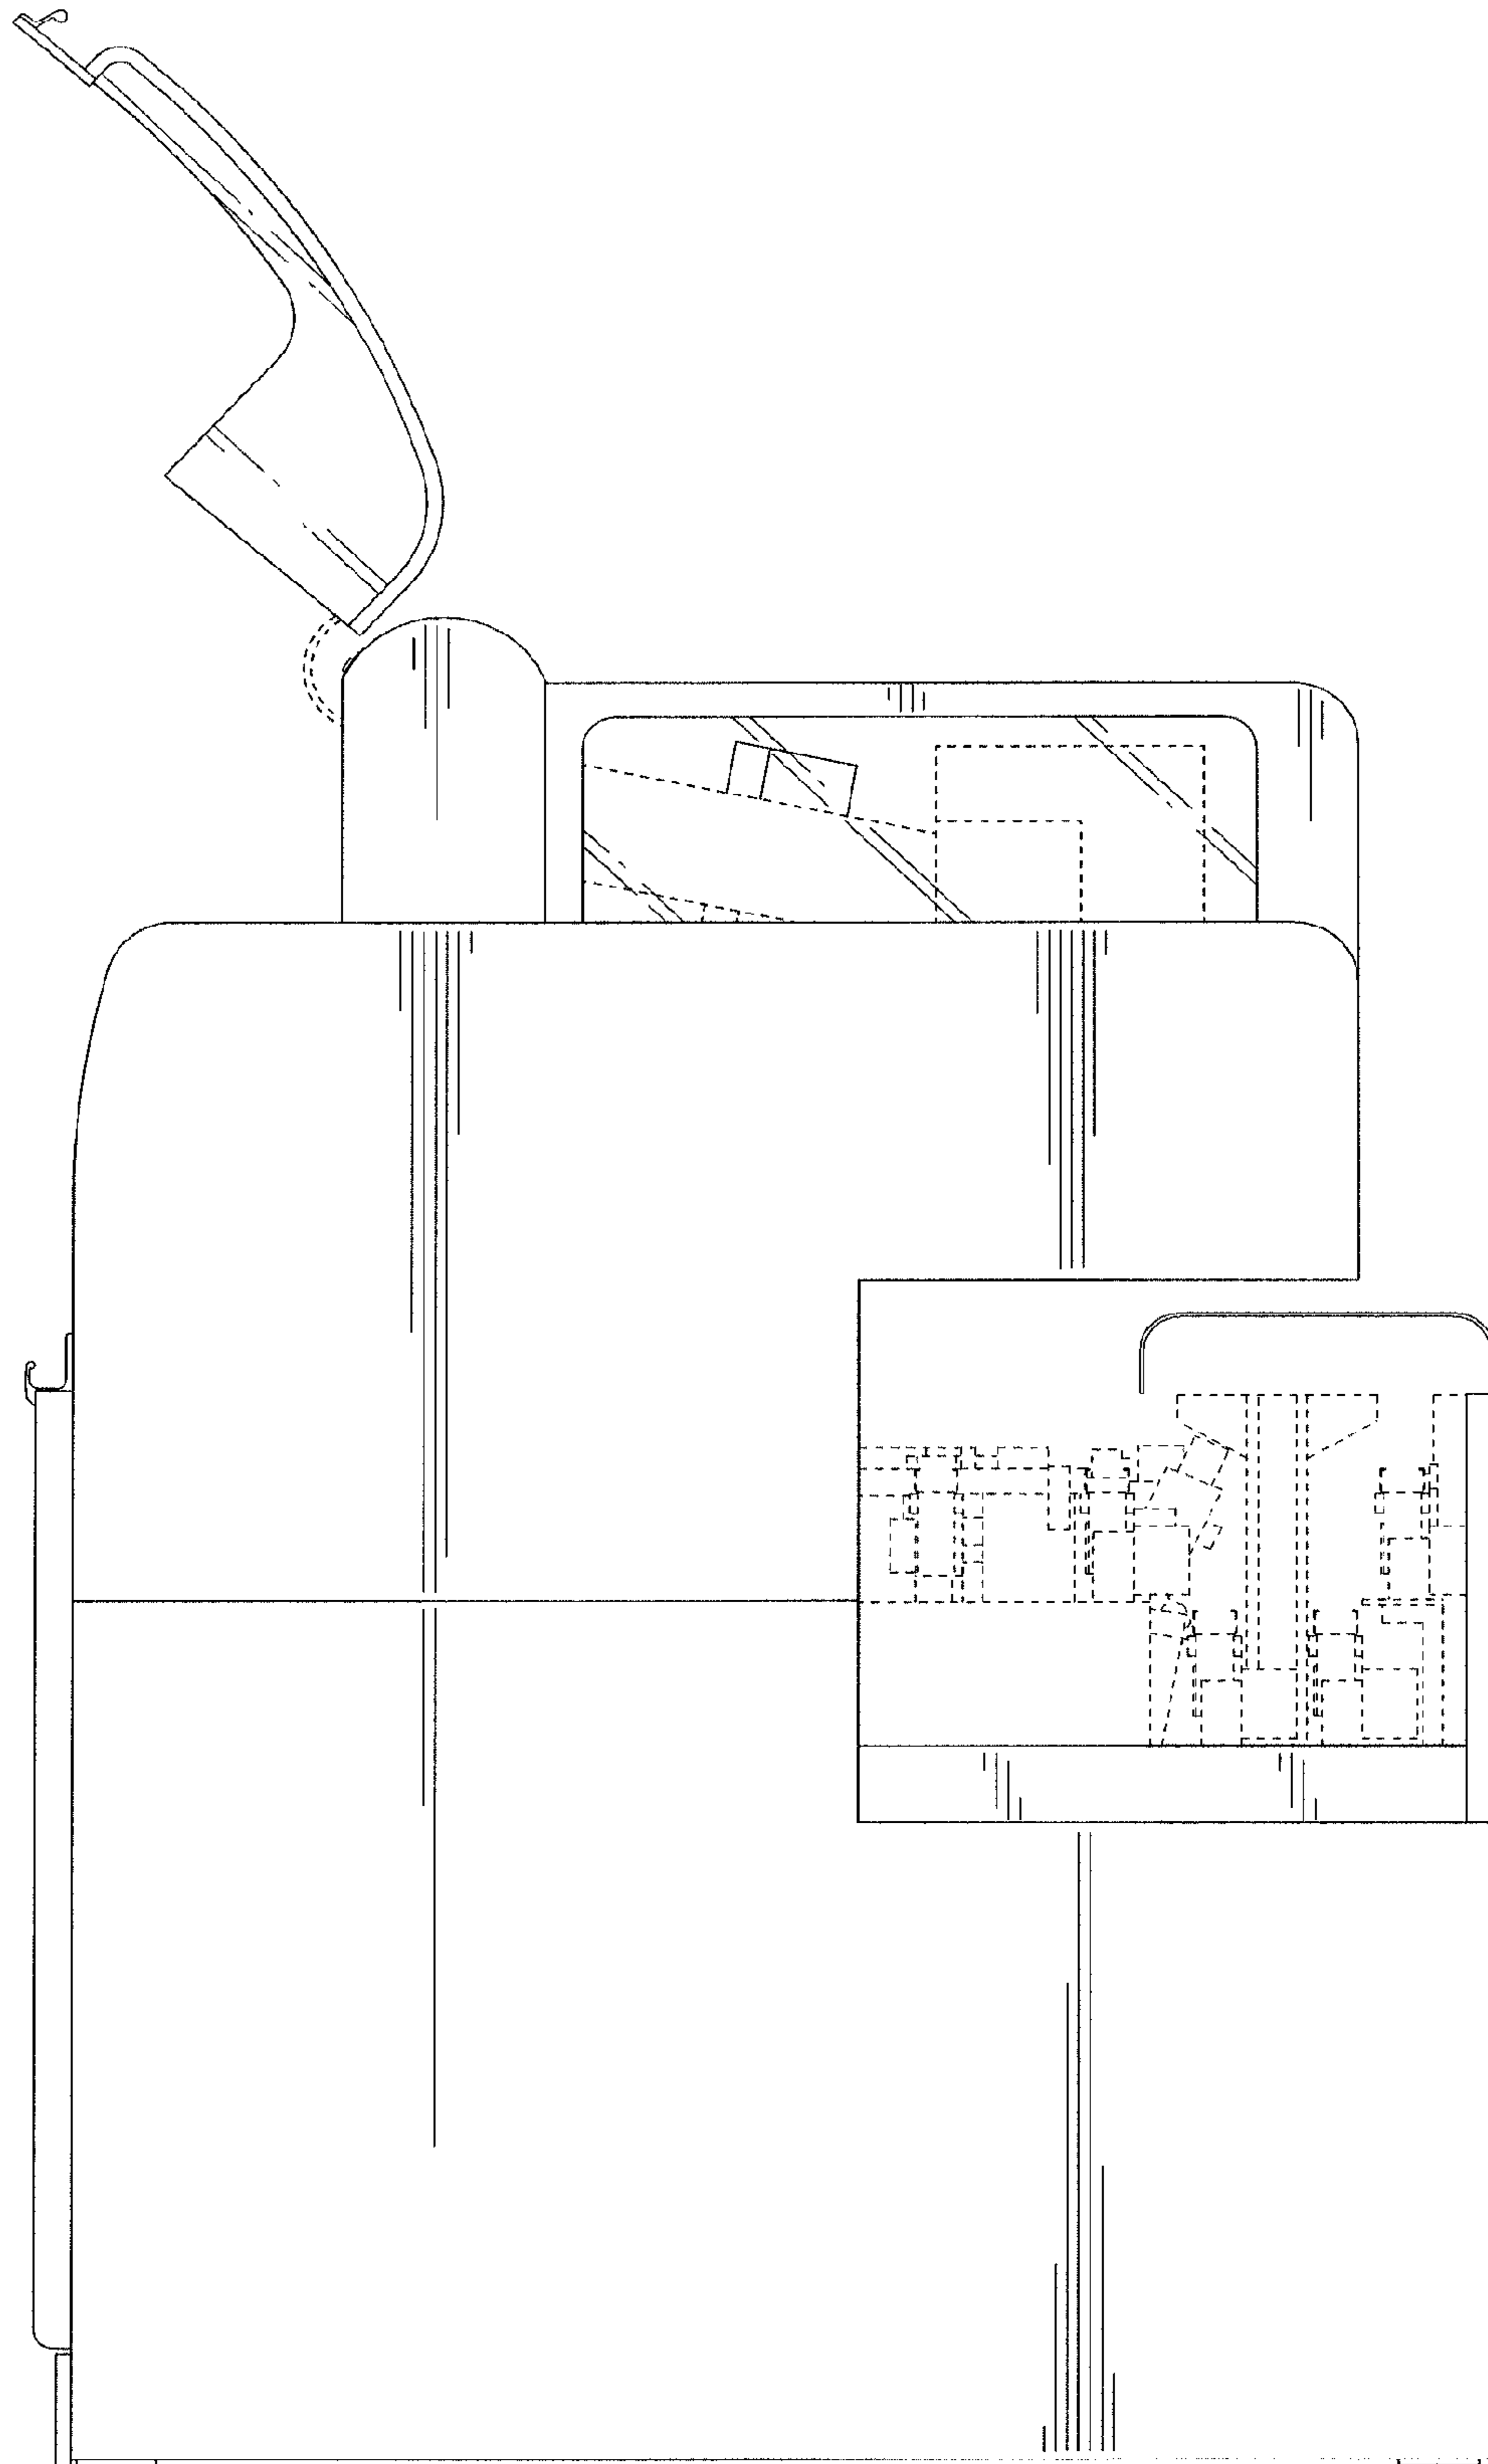


FIG. 8