



US00D657368S

(12) **United States Design Patent**  
**Magee et al.**

(10) **Patent No.:** **US D657,368 S**  
(45) **Date of Patent:** **\*\* Apr. 10, 2012**

(54) **PATIENT MONITORING DEVICE WITH GRAPHICAL USER INTERFACE**

D523,440 S \* 6/2006 Hernandez et al. .... D14/486  
(Continued)

(75) Inventors: **Marshall W. Magee**, Skaneateles, NY (US); **Shawn C. St. Pierre**, Syracuse, NY (US); **Mark E. Pingel**, Camillus, NY (US); **John P. McGlooin**, Marcellus, NY (US); **Michael D. Garrant**, Marcellus, NY (US); **Ann M. Jewell**, Weedsport, NY (US); **Jennifer M. Kilian**, New York, NY (US); **Eric J. Bailey**, Oakland, CA (US); **Roger W. Graves**, San Francisco, CA (US); **Esther N. Ahn**, San Francisco, CA (US); **Thomas A. Myers**, Syracuse, NY (US); **Corrie A. Baum**, Skaneateles, NY (US)

FOREIGN PATENT DOCUMENTS  
EP 0 707 824 A2 4/1996

OTHER PUBLICATIONS

International Search Report and Written Opinion in PCT/US2010/048450 dated Apr. 12, 2011, 9 pages.

(Continued)

*Primary Examiner* — Cathron Brooks  
*Assistant Examiner* — Deanna Fluegeman  
(74) *Attorney, Agent, or Firm* — Merchant & Gould P.C.

(73) Assignee: **Welch Allyn, Inc.**, Skaneateles Falls, NY (US)

(57) **CLAIM**

The ornamental design for a patient monitoring device with graphical user interface, as shown and described.

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/353,090**

**DESCRIPTION**

(22) Filed: **Dec. 31, 2009**

(51) **LOC (9) Cl.** ..... **32-00**

(52) **U.S. Cl.** ..... **D14/486**

(58) **Field of Classification Search** ..... D14/485-495;  
715/700-867

See application file for complete search history.

A portion of the disclosure of this patent document contains material to which a claim for copyright is made. The copyright owner has no objection to the facsimile reproduction by anyone of the patent document or the patent disclosure, as it appears in the U.S. Patent and Trademark Office patent file or records, but reserves all other copyrights whatsoever.

The single FIGURE is a front view of a patient monitoring device with a graphical user interface.


The broken line showing of the patient monitoring device is included for the purpose of illustrating the unclaimed environment of the graphical user interface and forms no part of the claimed design. The broken lines illustrating the unclaimed portions of the graphical user interface form no part of the claimed design.

(56) **References Cited**

U.S. PATENT DOCUMENTS

|              |         |               |       |         |
|--------------|---------|---------------|-------|---------|
| D366,460 S * | 1/1996  | Jorgenson     | ..... | D13/177 |
| D427,574 S * | 7/2000  | Sawada et al. | ..... | D14/486 |
| D454,139 S * | 3/2002  | Feldcamp      | ..... | D14/486 |
| D465,226 S * | 11/2002 | Friedman      | ..... | D14/486 |
| D468,322 S * | 1/2003  | Walker et al. | ..... | D14/486 |
| D510,582 S * | 10/2005 | Hoang et al.  | ..... | D14/486 |

**1 Claim, 1 Drawing Sheet**

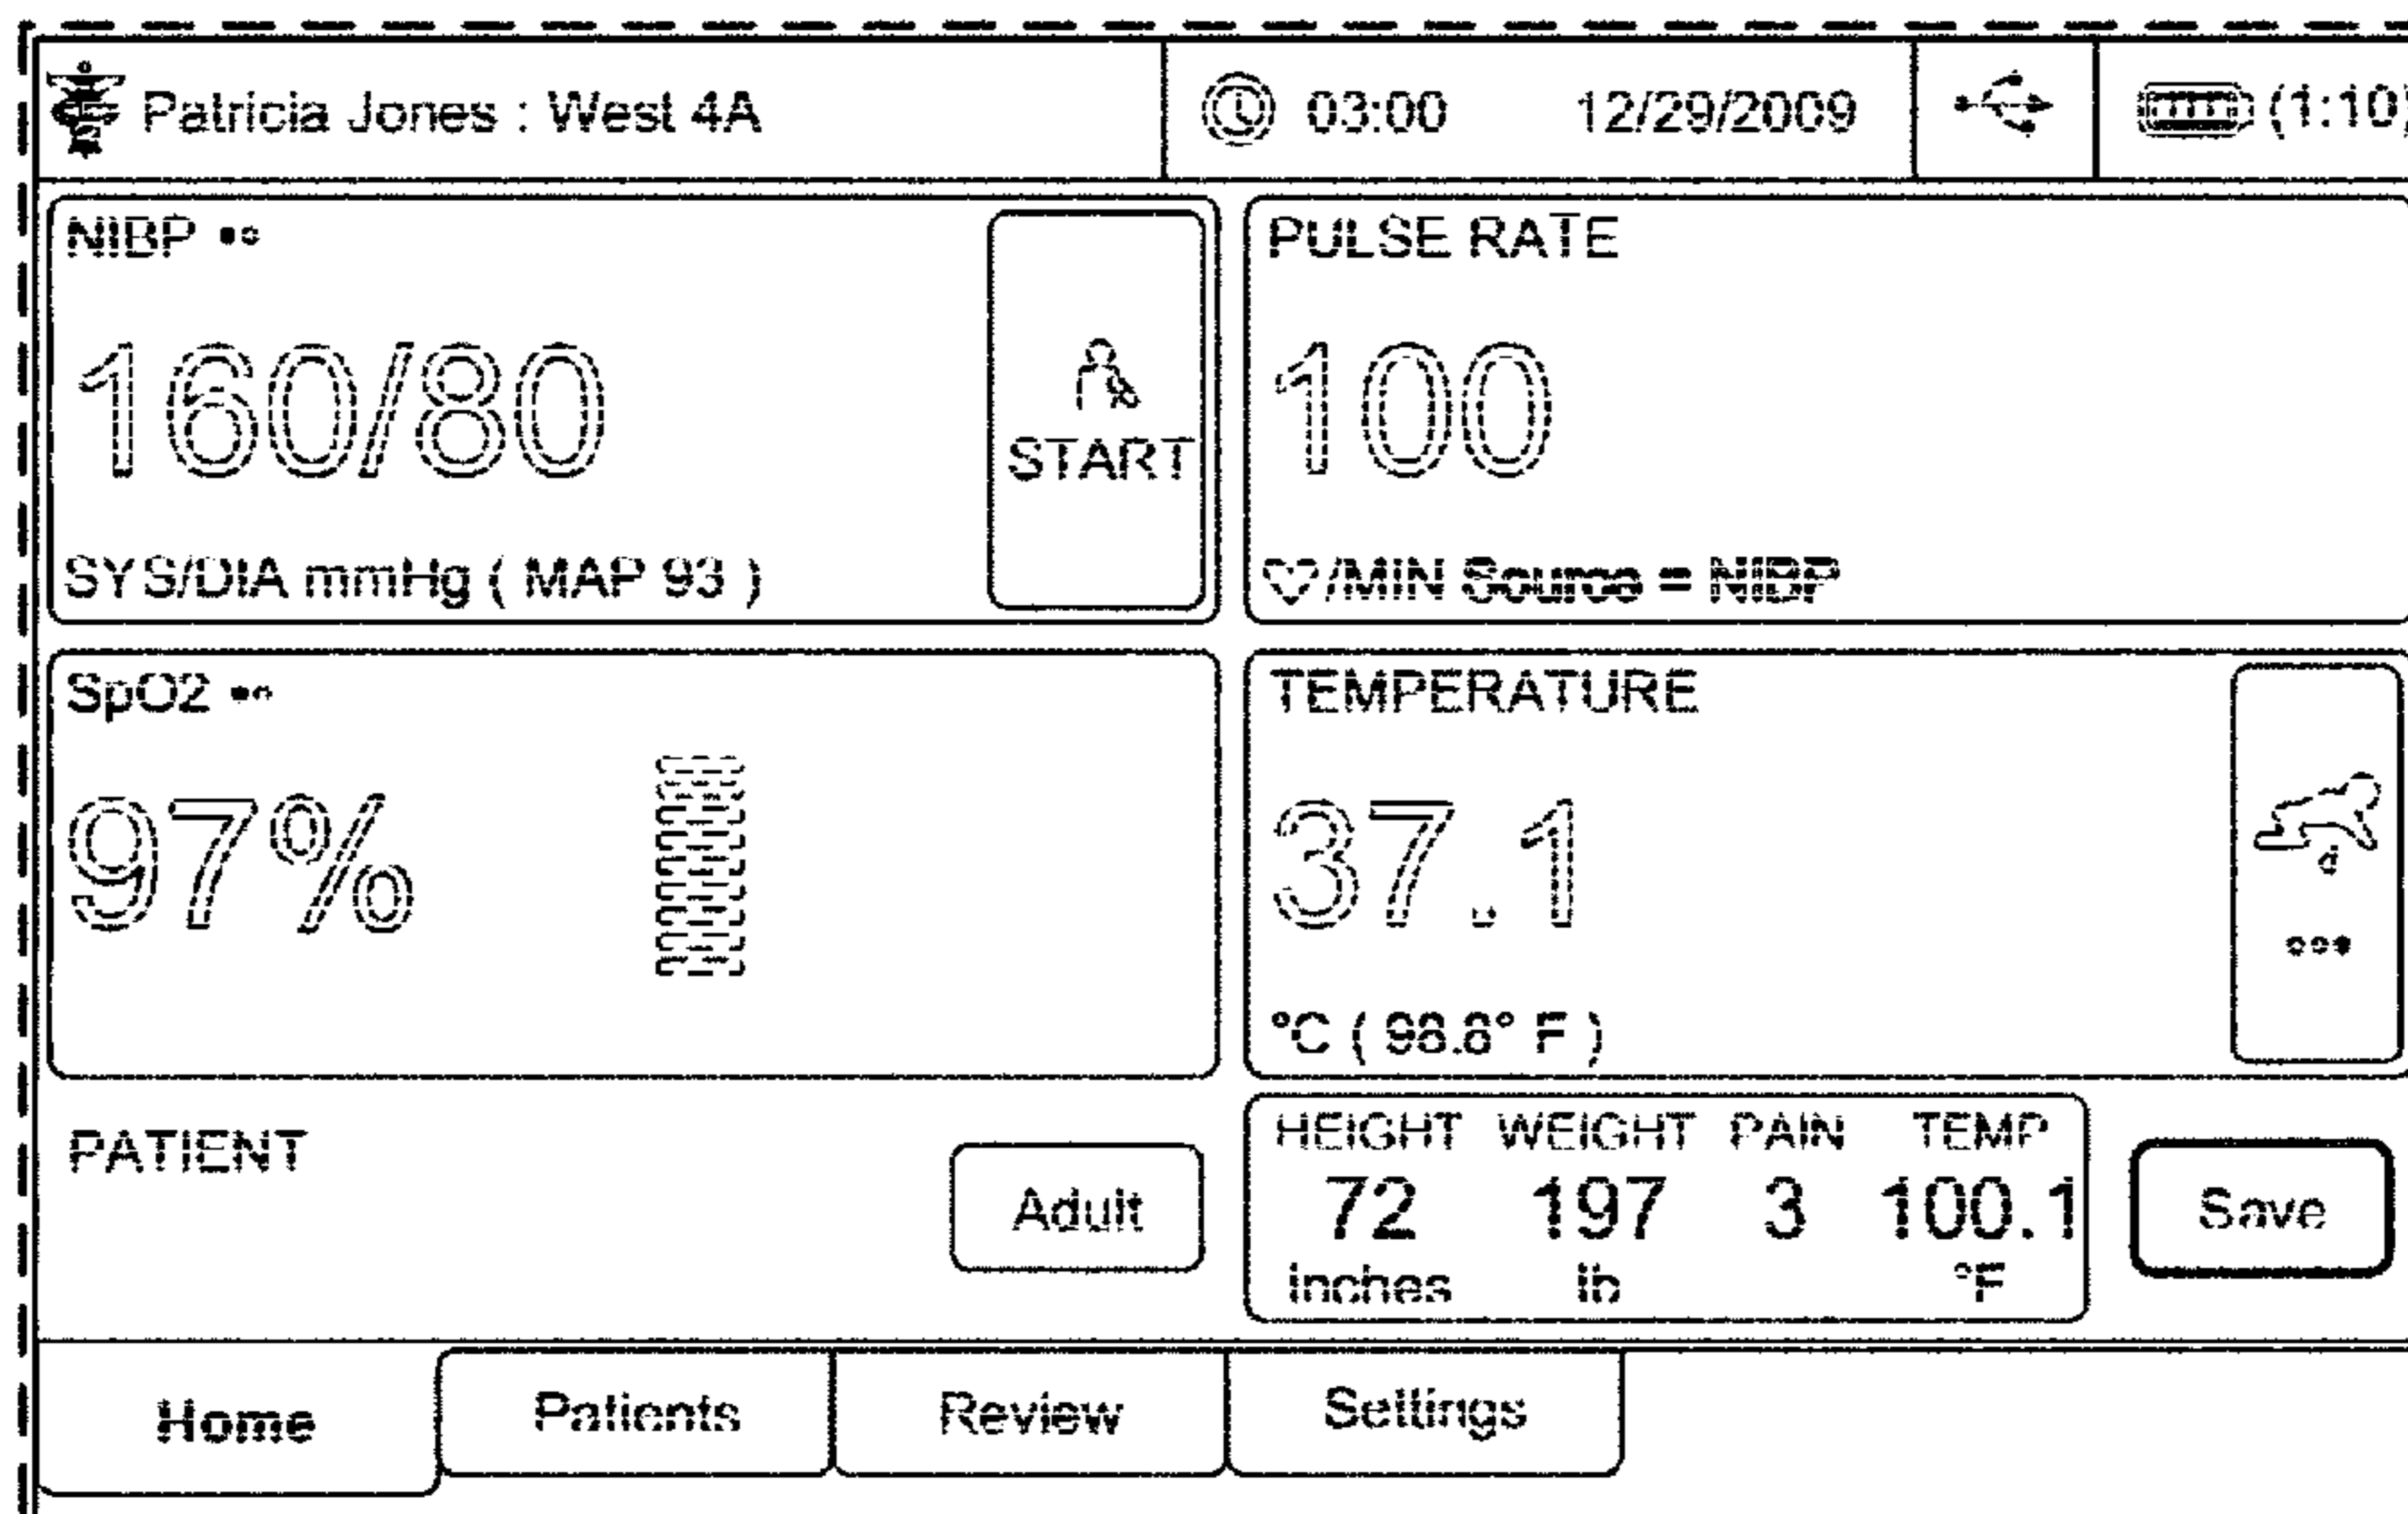

U.S. PATENT DOCUMENTS




|              |      |         |                           |          |
|--------------|------|---------|---------------------------|----------|
| D525,982     | S *  | 8/2006  | Suzuki .....              | D14/486  |
| D527,011     | S *  | 8/2006  | Bixler .....              | D14/486  |
| 7,134,994    | B2   | 11/2006 | Alpert                    |          |
| 7,336,187    | B2   | 2/2008  | Hubbard                   |          |
| D575,296     | S *  | 8/2008  | Fairfield et al. ....     | D14/485  |
| D586,818     | S *  | 2/2009  | Luck .....                | D14/485  |
| D592,675     | S *  | 5/2009  | Bhat et al. ....          | D14/486  |
| D598,929     | S *  | 8/2009  | Bhat et al. ....          | D14/486  |
| D603,416     | S *  | 11/2009 | Poling et al. ....        | D14/485  |
| D608,366     | S *  | 1/2010  | Matas .....               | D14/486  |
| D612,860     | S *  | 3/2010  | Tarara et al. ....        | D14/485  |
| D614,634     | S *  | 4/2010  | Nilson .....              | D14/486  |
| D632,699     | S *  | 2/2011  | Judy et al. ....          | D14/486  |
| D635,150     | S *  | 3/2011  | Sykes et al. ....         | D14/486  |
| D646,689     | S *  | 10/2011 | Ulliot .....              | D14/486  |
| 2002/0054141 | A1 * | 5/2002  | Yen et al. ....           | 345/804  |
| 2005/0114374 | A1 * | 5/2005  | Juszkiewicz et al. ....   | 707/101  |
| 2005/0229110 | A1 * | 10/2005 | Gegner et al. ....        | 715/800  |
| 2006/0229557 | A1   | 10/2006 | Fathallah                 |          |
| 2007/0167694 | A1   | 7/2007  | Causevic                  |          |
| 2007/0185390 | A1   | 8/2007  | Perkins                   |          |
| 2007/0276261 | A1   | 11/2007 | Banet                     |          |
| 2008/0055074 | A1   | 3/2008  | Gao                       |          |
| 2008/0058614 | A1   | 3/2008  | Banet                     |          |
| 2008/0077026 | A1   | 3/2008  | Banet                     |          |
| 2008/0103375 | A1   | 5/2008  | Kiani                     |          |
| 2008/0115081 | A1 * | 5/2008  | Sankaravadivelu et al. .. | 715/783  |
| 2008/0249377 | A1   | 10/2008 | Molducci                  |          |
| 2008/0281168 | A1   | 11/2008 | Gibson                    |          |
| 2008/0318529 | A1 * | 12/2008 | Harb .....                | 455/66.1 |
| 2009/0054743 | A1   | 2/2009  | Stewart                   |          |
| 2009/0131761 | A1   | 5/2009  | Moroney                   |          |
| 2009/0143652 | A1   | 6/2009  | Warburton                 |          |
| 2009/0149927 | A1   | 6/2009  | Kneuer                    |          |
| 2009/0158415 | A1 * | 6/2009  | Dillon .....              | 726/11   |

|              |    |         |        |
|--------------|----|---------|--------|
| 2009/0240116 | A1 | 9/2009  | Bluth  |
| 2009/0275810 | A1 | 11/2009 | Ayers  |
| 2009/0306488 | A1 | 12/2009 | Al-Ali |

OTHER PUBLICATIONS

mCare 300 Vital Signs Monitor, Spacelabs Medical, Inc., Copyright 2006, 4 pages.  
 Ultraview DM3—Dual Mode Vital Signs Monitor, Spacelabs Healthcare, Copyright 2010, 4 pages.  
 Colin Prodigy Press-Mate Prodigy II® Portable Vital Signs Monitors, DRE, Copyright 2009, accessed at: [http://www.dremed.com/catalog/product\\_info.php/products\\_id/1181](http://www.dremed.com/catalog/product_info.php/products_id/1181); 5 pages.  
 Fingertip Pulse Oximeter SPO<sub>2</sub> Monitor Oxigen Oximeter; Copyright 1995-2010, accessed at: <http://74.125.45.132/search?q=cache:ANfHne9je7gJ:cgi.ebay.com.sg/ws/eBayISAPI:d11%3FViewItem%26item%3D260412542031+“Fingertip+Pulse+Oximeter+SPO2+Monitor+Oxigen+Oximeter”&cd=2&hl=en&ct=clnk&gl=us>; 6 pages.  
 Handheld Pulse Oximeter PM-60A, Contec Medical System Co. Ltd., Jul. 31, 2009; accessed at: <http://www.tradeindia.com/selloffer/1858593/Handheld-Pulse-Oximeter-PM-60A.html>; 5 pages.  
 Multiple Vital Signs from One Non-invasive Sensor, Starr™ Life Sciences Corp., Copyright 2009, accessed at: <http://www.star-rlifesciences.com/mouseox.html>; 1 page.  
 NTIA Handheld Pulse Oximeter, Frontline Systems; Dec. 31, 2009, accessed at: <http://www.tradeindia.com/fp385774/NTIA-Handheld-Pulse-Oximeter.html>; 3 pages.  
 Portable Patient Monitors, Welch Allyn, Copyright 2005-2006 Med-Direct, Copyright 2005-2006, accessed at: <http://www.meddirect.co.nz/Product.aspx?ProductId=3476>; 1 page.  
 U.S. Appl. No. 61/243,872, filed Sep. 18, 2009.  
 U.S. Appl. No. 12/751,579, filed Mar. 31, 2010.  
 U.S. Appl. No. 12/751,602, filed Mar. 31, 2010.

\* cited by examiner

|   |   |   |
|---|---|---|
|  <p>Patricia Jones : West 4A</p> | <p>03:00 12/29/2009</p>   | <p>(1:10)</p>   |
| <p>NIBP °C</p> <p>160/80</p> <p>SYS/DIA mmHg ( MAP 93 )</p>   | <p>START</p>  | <p>PULSE RATE</p> <p>100</p> <p>♥/MIN SOURCE = NIBP</p>   |
| <p>SpO2 %</p> <p>97%</p>     | <p>TEMPERATURE</p> <p>37.1</p> <p>°C ( 98.8° F )</p>                            |  <p>Save</p> |
| <p>PATIENT</p> <p>Adult</p>   | <p>HEIGHT 72 inches</p> <p>WEIGHT 197 lb</p> <p>PAIN 3</p> <p>TEMP 100.1 °F</p> | <p>Home</p> <p>Patients</p> <p>Review</p> <p>Settings</p>   |