



US00D657368S

(12) **United States Design Patent**  
**Magee et al.**

(10) **Patent No.:** **US D657,368 S**  
(45) **Date of Patent:** **\*\* Apr. 10, 2012**

(54) **PATIENT MONITORING DEVICE WITH GRAPHICAL USER INTERFACE**

D523,440 S \* 6/2006 Hernandez et al. .... D14/486  
(Continued)

(75) Inventors: **Marshall W. Magee**, Skaneateles, NY (US); **Shawn C. St. Pierre**, Syracuse, NY (US); **Mark E. Pingel**, Camillus, NY (US); **John P. McGlooin**, Marcellus, NY (US); **Michael D. Garrant**, Marcellus, NY (US); **Ann M. Jewell**, Weedsport, NY (US); **Jennifer M. Kilian**, New York, NY (US); **Eric J. Bailey**, Oakland, CA (US); **Roger W. Graves**, San Francisco, CA (US); **Esther N. Ahn**, San Francisco, CA (US); **Thomas A. Myers**, Syracuse, NY (US); **Corrie A. Baum**, Skaneateles, NY (US)

FOREIGN PATENT DOCUMENTS  
EP 0 707 824 A2 4/1996

**OTHER PUBLICATIONS**

International Search Report and Written Opinion in PCT/US2010/048450 dated Apr. 12, 2011, 9 pages.

(Continued)

*Primary Examiner* — Cathron Brooks  
*Assistant Examiner* — Deanna Fluegeman  
(74) *Attorney, Agent, or Firm* — Merchant & Gould P.C.

(73) Assignee: **Welch Allyn, Inc.**, Skaneateles Falls, NY (US)

(57) **CLAIM**

The ornamental design for a patient monitoring device with graphical user interface, as shown and described.

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/353,090**

**DESCRIPTION**

(22) Filed: **Dec. 31, 2009**

(51) **LOC (9) Cl.** ..... **32-00**

(52) **U.S. Cl.** ..... **D14/486**

(58) **Field of Classification Search** ..... D14/485-495;  
715/700-867

See application file for complete search history.

A portion of the disclosure of this patent document contains material to which a claim for copyright is made. The copyright owner has no objection to the facsimile reproduction by anyone of the patent document or the patent disclosure, as it appears in the U.S. Patent and Trademark Office patent file or records, but reserves all other copyrights whatsoever.

The single FIGURE is a front view of a patient monitoring device with a graphical user interface.


The broken line showing of the patient monitoring device is included for the purpose of illustrating the unclaimed environment of the graphical user interface and forms no part of the claimed design. The broken lines illustrating the unclaimed portions of the graphical user interface form no part of the claimed design.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D366,460 S *	1/1996	Jorgenson	.....	D13/177
D427,574 S *	7/2000	Sawada et al.	.....	D14/486
D454,139 S *	3/2002	Feldcamp	.....	D14/486
D465,226 S *	11/2002	Friedman	.....	D14/486
D468,322 S *	1/2003	Walker et al.	.....	D14/486
D510,582 S *	10/2005	Hoang et al.	.....	D14/486

**1 Claim, 1 Drawing Sheet**

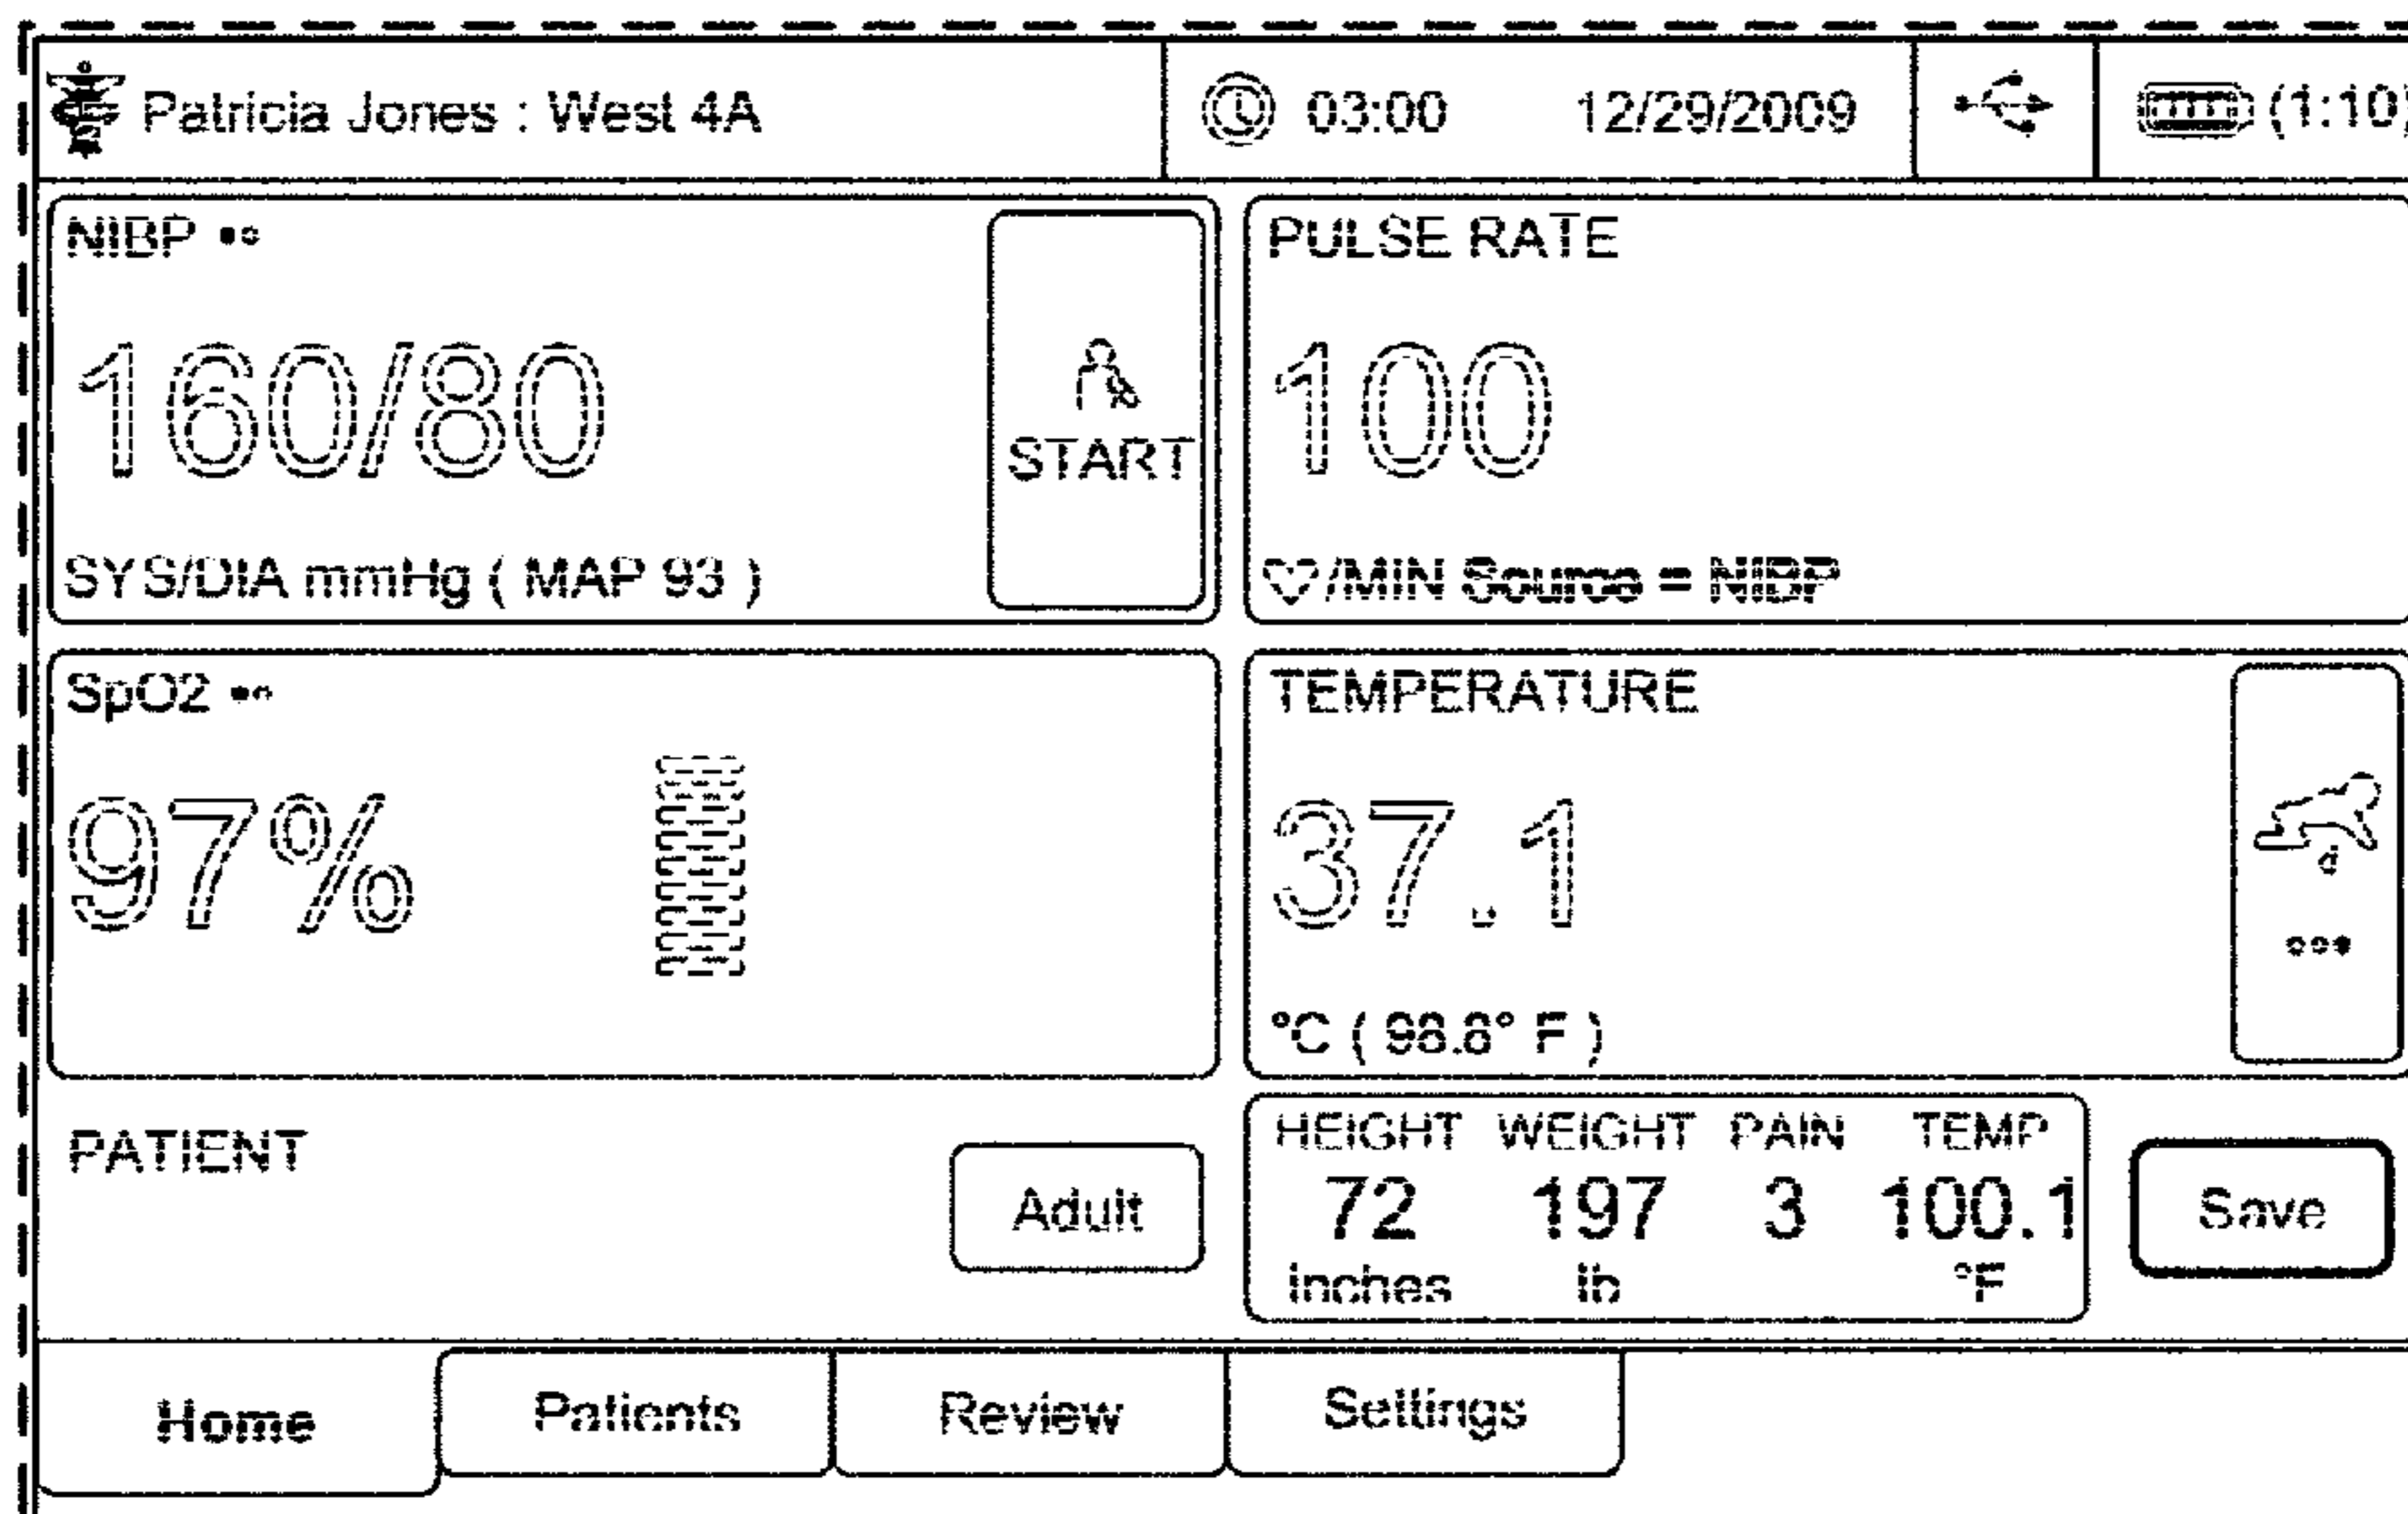

U.S. PATENT DOCUMENTS






D525,982	S *	8/2006	Suzuki .....	D14/486
D527,011	S *	8/2006	Bixler .....	D14/486
7,134,994	B2	11/2006	Alpert	
7,336,187	B2	2/2008	Hubbard	
D575,296	S *	8/2008	Fairfield et al. ....	D14/485
D586,818	S *	2/2009	Luck .....	D14/485
D592,675	S *	5/2009	Bhat et al. ....	D14/486
D598,929	S *	8/2009	Bhat et al. ....	D14/486
D603,416	S *	11/2009	Poling et al. ....	D14/485
D608,366	S *	1/2010	Matas .....	D14/486
D612,860	S *	3/2010	Tarara et al. ....	D14/485
D614,634	S *	4/2010	Nilson .....	D14/486
D632,699	S *	2/2011	Judy et al. ....	D14/486
D635,150	S *	3/2011	Sykes et al. ....	D14/486
D646,689	S *	10/2011	Ulliot .....	D14/486
2002/0054141	A1 *	5/2002	Yen et al. ....	345/804
2005/0114374	A1 *	5/2005	Juszkiewicz et al. ....	707/101
2005/0229110	A1 *	10/2005	Gegner et al. ....	715/800
2006/0229557	A1	10/2006	Fathallah	
2007/0167694	A1	7/2007	Causevic	
2007/0185390	A1	8/2007	Perkins	
2007/0276261	A1	11/2007	Banet	
2008/0055074	A1	3/2008	Gao	
2008/0058614	A1	3/2008	Banet	
2008/0077026	A1	3/2008	Banet	
2008/0103375	A1	5/2008	Kiani	
2008/0115081	A1 *	5/2008	Sankaravadivelu et al. ..	715/783
2008/0249377	A1	10/2008	Molducci	
2008/0281168	A1	11/2008	Gibson	
2008/0318529	A1 *	12/2008	Harb .....	455/66.1
2009/0054743	A1	2/2009	Stewart	
2009/0131761	A1	5/2009	Moroney	
2009/0143652	A1	6/2009	Warburton	
2009/0149927	A1	6/2009	Kneuer	
2009/0158415	A1 *	6/2009	Dillon .....	726/11

2009/0240116	A1	9/2009	Bluth
2009/0275810	A1	11/2009	Ayers
2009/0306488	A1	12/2009	Al-Ali

OTHER PUBLICATIONS

mCare 300 Vital Signs Monitor, Spacelabs Medical, Inc., Copyright 2006, 4 pages.  
 Ultraview DM3—Dual Mode Vital Signs Monitor, Spacelabs Healthcare, Copyright 2010, 4 pages.  
 Colin Prodigy Press-Mate Prodigy II® Portable Vital Signs Monitors, DRE, Copyright 2009, accessed at: [http://www.dremed.com/catalog/product\\_info.php/products\\_id/1181](http://www.dremed.com/catalog/product_info.php/products_id/1181); 5 pages.  
 Fingertip Pulse Oximeter SPO<sub>2</sub> Monitor Oxigen Oximeter; Copyright 1995-2010, accessed at: [http://74.125.45.132/search?q=cache:ANfHne9je7gJ:cgi.ebay.com.sg/ws/eBayISAPI:d11%3FViewItem%26item%3D260412542031+\"Fingertip+Pulse+Oximeter+SPO2+Monitor+Oxigen+Oximeter\"&cd=2&hl=en&ct=clnk&gl=us](http://74.125.45.132/search?q=cache:ANfHne9je7gJ:cgi.ebay.com.sg/ws/eBayISAPI:d11%3FViewItem%26item%3D260412542031+\); 6 pages.  
 Handheld Pulse Oximeter PM-60A, Contec Medical System Co. Ltd., Jul. 31, 2009; accessed at: <http://www.tradeindia.com/selloffer/1858593/Handheld-Pulse-Oximeter-PM-60A.html>; 5 pages.  
 Multiple Vital Signs from One Non-invasive Sensor, Starr™ Life Sciences Corp., Copyright 2009, accessed at: <http://www.star-rlifesciences.com/mouseox.html>; 1 page.  
 NTIA Handheld Pulse Oximeter, Frontline Systems; Dec. 31, 2009, accessed at: <http://www.tradeindia.com/fp385774/NTIA-Handheld-Pulse-Oximeter.html>; 3 pages.  
 Portable Patient Monitors, Welch Allyn, Copyright 2005-2006 Med-Direct, Copyright 2005-2006, accessed at: <http://www.meddirect.co.nz/Product.aspx?ProductId=3476>; 1 page.  
 U.S. Appl. No. 61/243,872, filed Sep. 18, 2009.  
 U.S. Appl. No. 12/751,579, filed Mar. 31, 2010.  
 U.S. Appl. No. 12/751,602, filed Mar. 31, 2010.

\* cited by examiner

 Patricia Jones : West 4A	© 03:00	12/29/2009	 (1:10)
<b>NIBP</b> °C 160/80	 START	<b>PULSE RATE</b> 100	
<b>SYS/DIA</b> mmHg ( MAP 93 )		♥/MIN SOURCE = NIBP	
<b>SpO2</b> % 97%		<b>TEMPERATURE</b> 37.1 °C ( 98.8° F )	 °C
<b>PATIENT</b>	Adult	<b>HEIGHT</b> 72 inches	<b>WEIGHT</b> 197 lb
		<b>PAIN</b> 3	<b>TEMP</b> 100.1 °F
<b>Home</b>	<b>Patients</b>	<b>Review</b>	<b>Settings</b>
			<b>Save</b>