



US00D658298S

(12) **United States Design Patent**  
**Prpa**

(10) **Patent No.:** **US D658,298 S**

(45) **Date of Patent:** **\*\* Apr. 24, 2012**

(54) **TABLE TOP IMPLANT TRACKING DEVICE**

(76) **Inventor:** **Branko Prpa, Racine, WI (US)**

(\*\*) **Term:** **14 Years**

(21) **Appl. No.:** **29/403,944**

(22) **Filed:** **Oct. 13, 2011**

(51) **LOC (9) Cl.** ..... **24-02**

(52) **U.S. Cl.** ..... **D24/186**

(58) **Field of Classification Search** ..... D24/127,  
D24/133, 186-187, 200, 206-207, 214, 231-232;  
600/49, 300, 301, 368, 372, 481, 529, 544,  
600/554, 561; 607/4, 5, 9, 30, 48, 60; 128/846,  
128/888, 899, 903-904; D10/46-47, 70,  
D10/104.1; 206/16

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D346,977	S	*	5/1994	Fiske	.....	D10/47
D356,044	S	*	3/1995	Clements	.....	D10/104.1
D374,829	S	*	10/1996	Yue	.....	D10/47
D410,399	S	*	6/1999	De Torfino	.....	D10/46
6,026,328	A	*	2/2000	Peckham et al.	.....	607/48
D459,245	S	*	6/2002	Power	.....	D10/47
D459,246	S	*	6/2002	Power et al.	.....	D10/47
D497,559	S	*	10/2004	Johnson	.....	D10/47
D512,656	S	*	12/2005	Yeung	.....	D10/47
D513,706	S	*	1/2006	Johnson	.....	D10/47
D583,261	S	*	12/2008	Johnson et al.	.....	D10/47
D596,299	S	*	7/2009	Han et al.	.....	D24/186

D614,980	S	*	5/2010	Junes	.....	D10/70
D614,981	S	*	5/2010	Junes	.....	D10/70
D616,991	S	*	6/2010	Kitayama	.....	D24/186
7,813,809	B2	*	10/2010	Strother et al.	.....	607/60
D629,525	S	*	12/2010	Ladwig et al.	.....	D24/187
D630,756	S	*	1/2011	Kitayama	.....	D24/187
D642,690	S	*	8/2011	Altmann et al.	.....	D24/186
2011/0060386	A1	*	3/2011	Woods et al.	.....	607/60
2011/0114514	A1	*	5/2011	Bagozzi et al.	.....	206/216

\* cited by examiner

*Primary Examiner* — T. Chase Nelson

*Assistant Examiner* — Mark Cavanna

(74) *Attorney, Agent, or Firm* — Whyte Hirschboeck Dudek S.C.

(57) **CLAIM**

The ornamental design for a table top implant tracking device, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of a table top implant tracking device showing my new design;

FIG. 2 is a front elevation view thereof;

FIG. 3 is a top plan view thereof;


FIG. 4 is a left elevation view thereof;

FIG. 5 is a right elevation view thereof; and,

FIG. 6 is a bottom plan view thereof.

The broken lines are included for the purpose of illustrating portions of the table top implant tracking device that form no part of the claimed design.

**1 Claim, 3 Drawing Sheets**

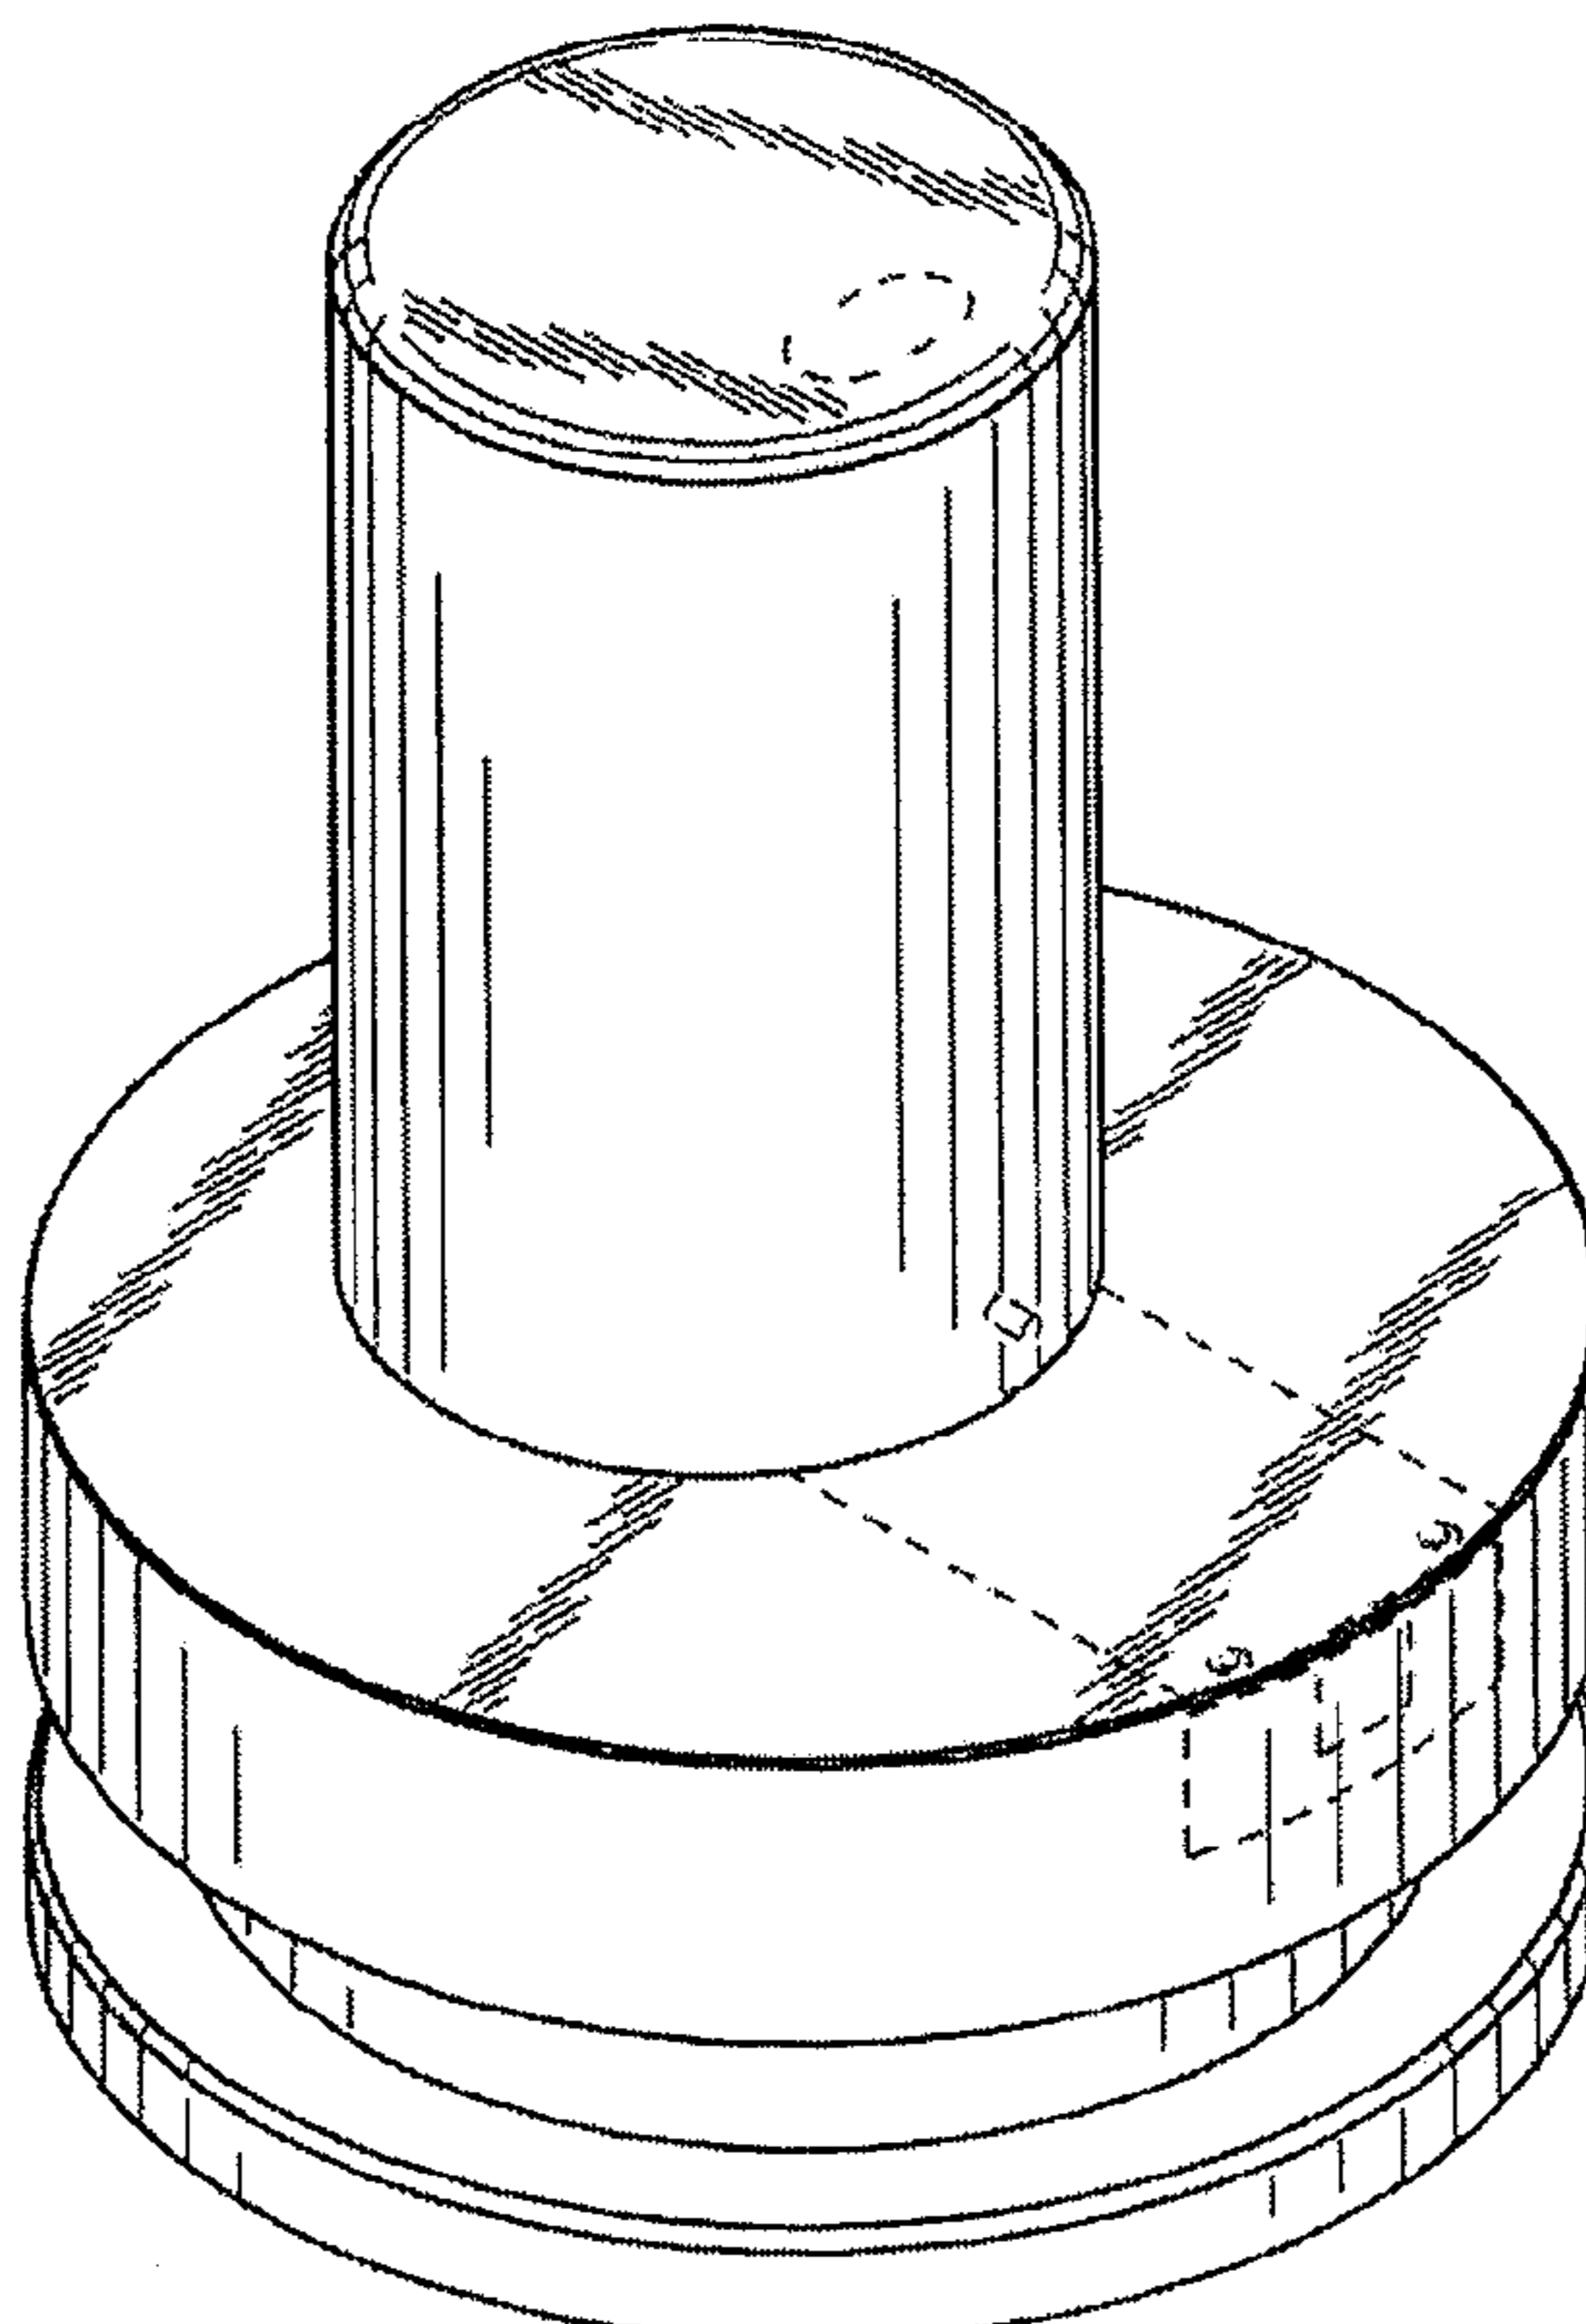

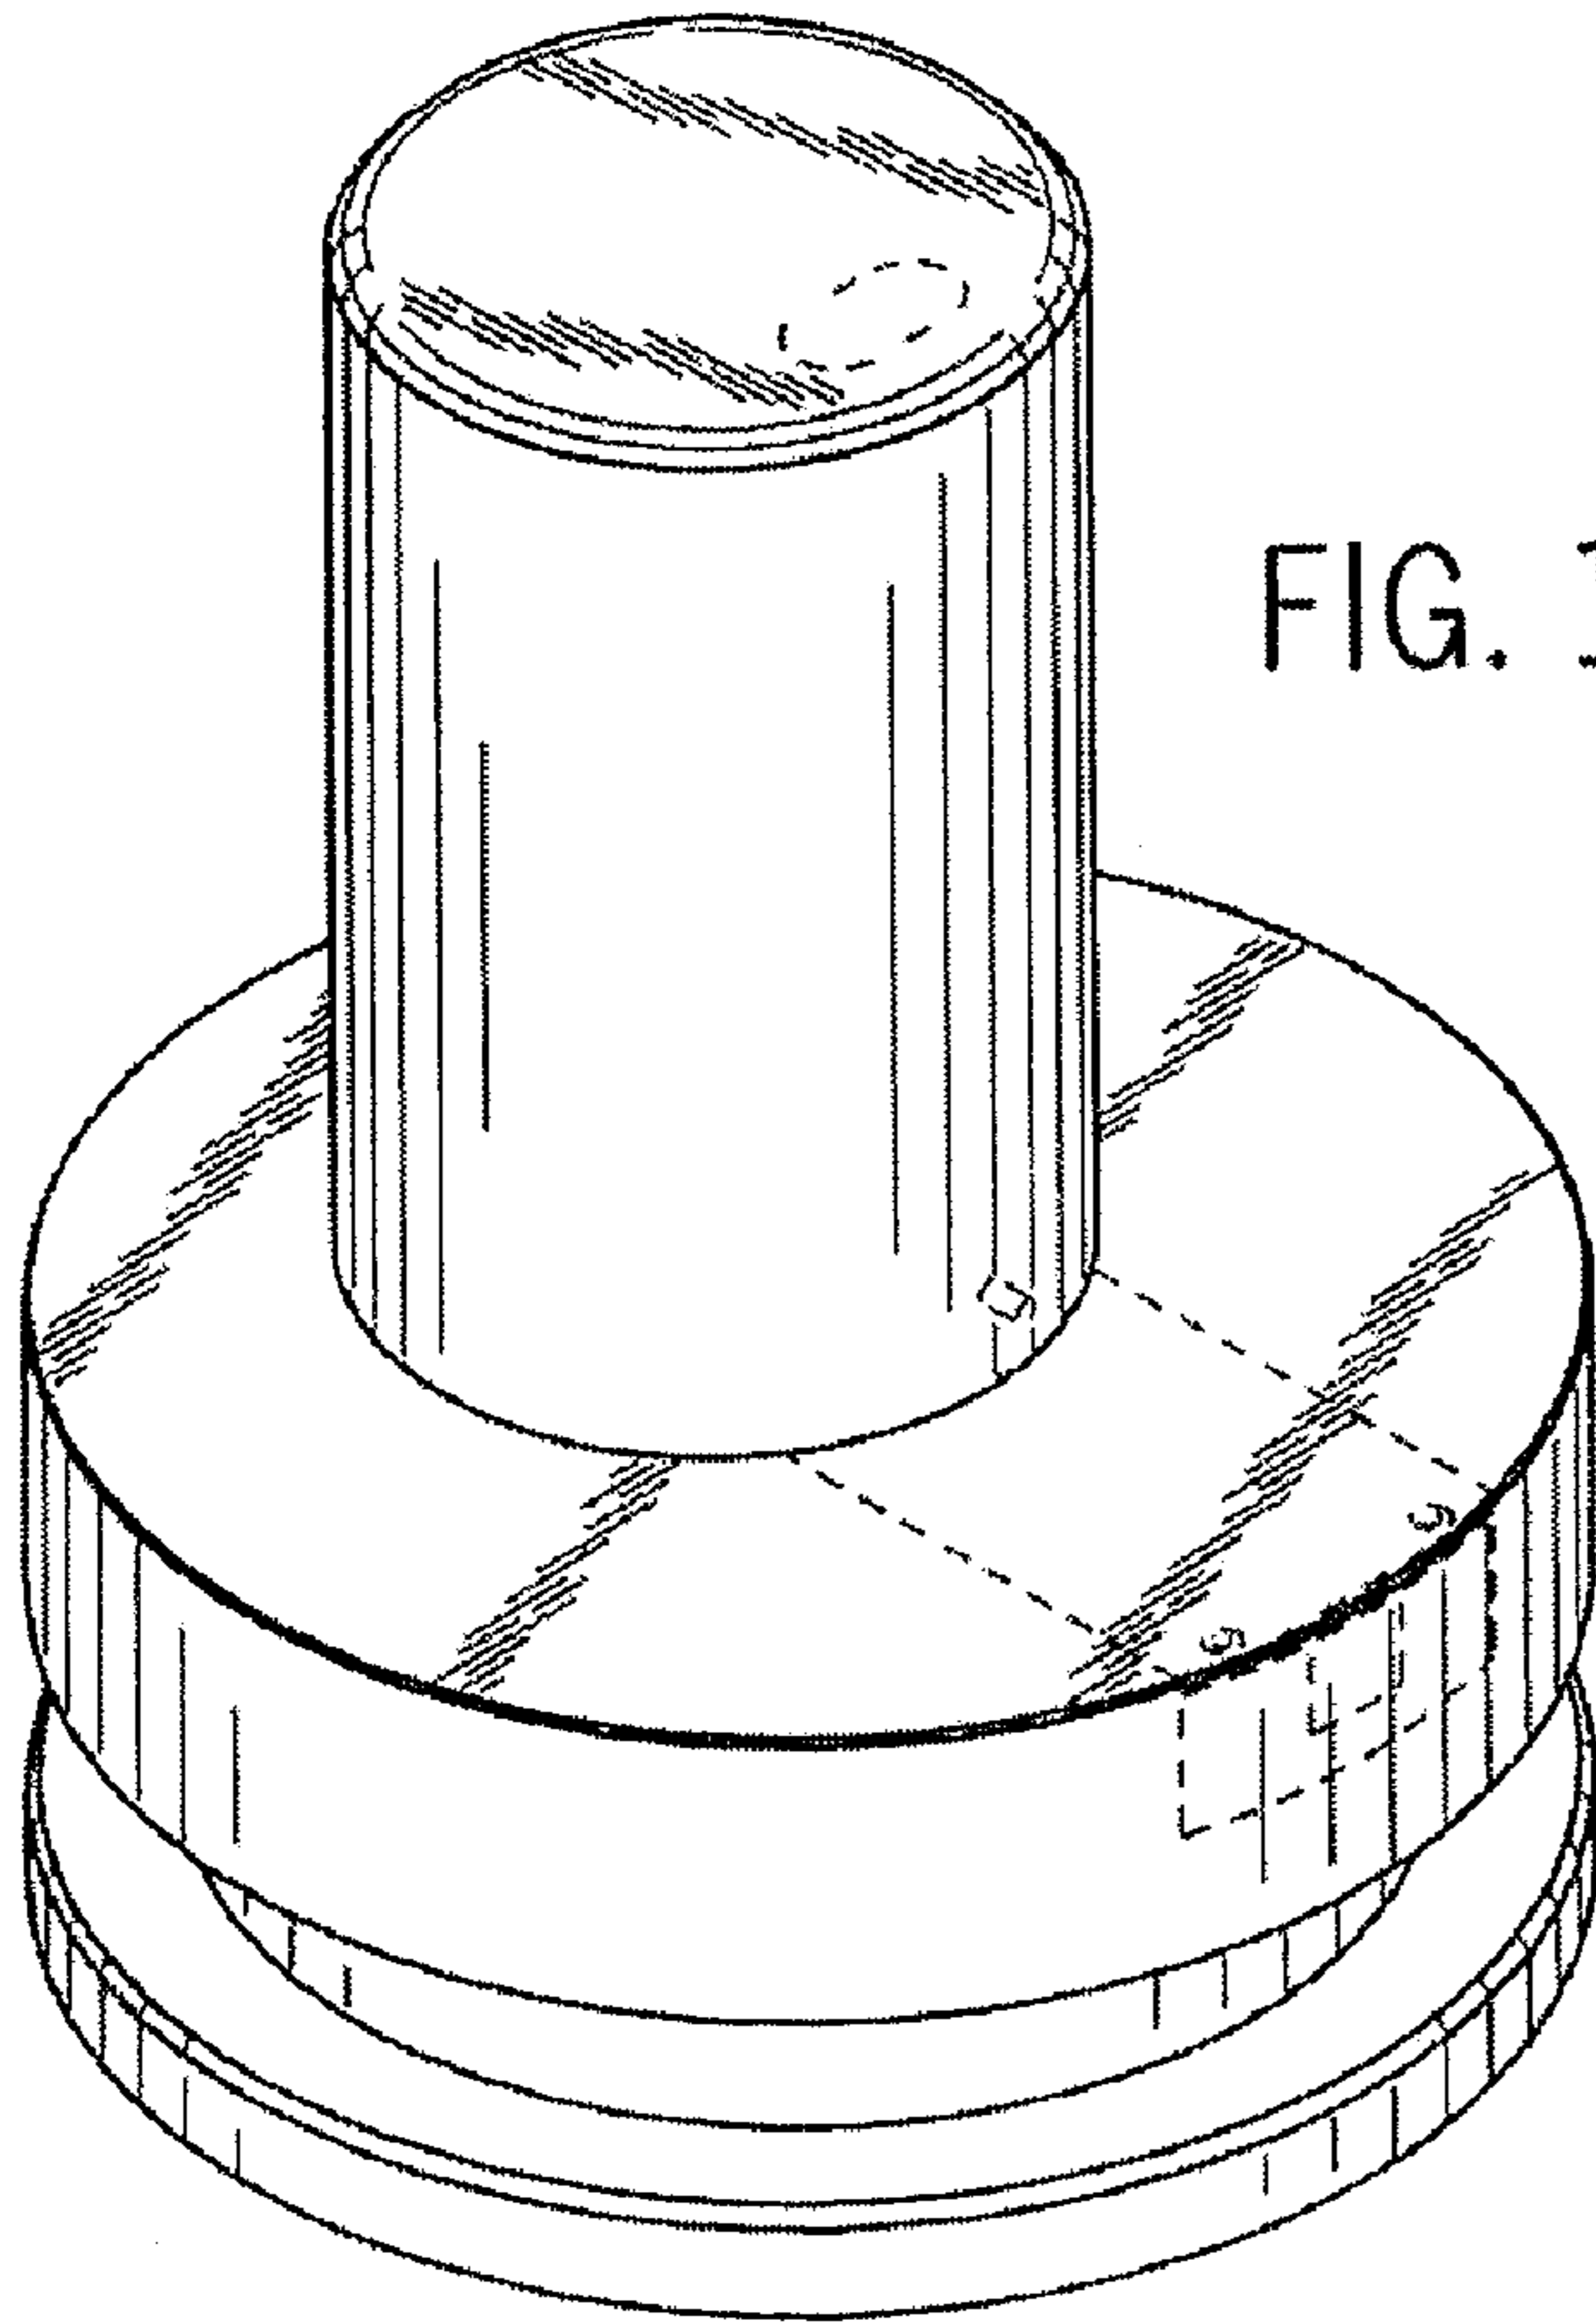


FIG. 1

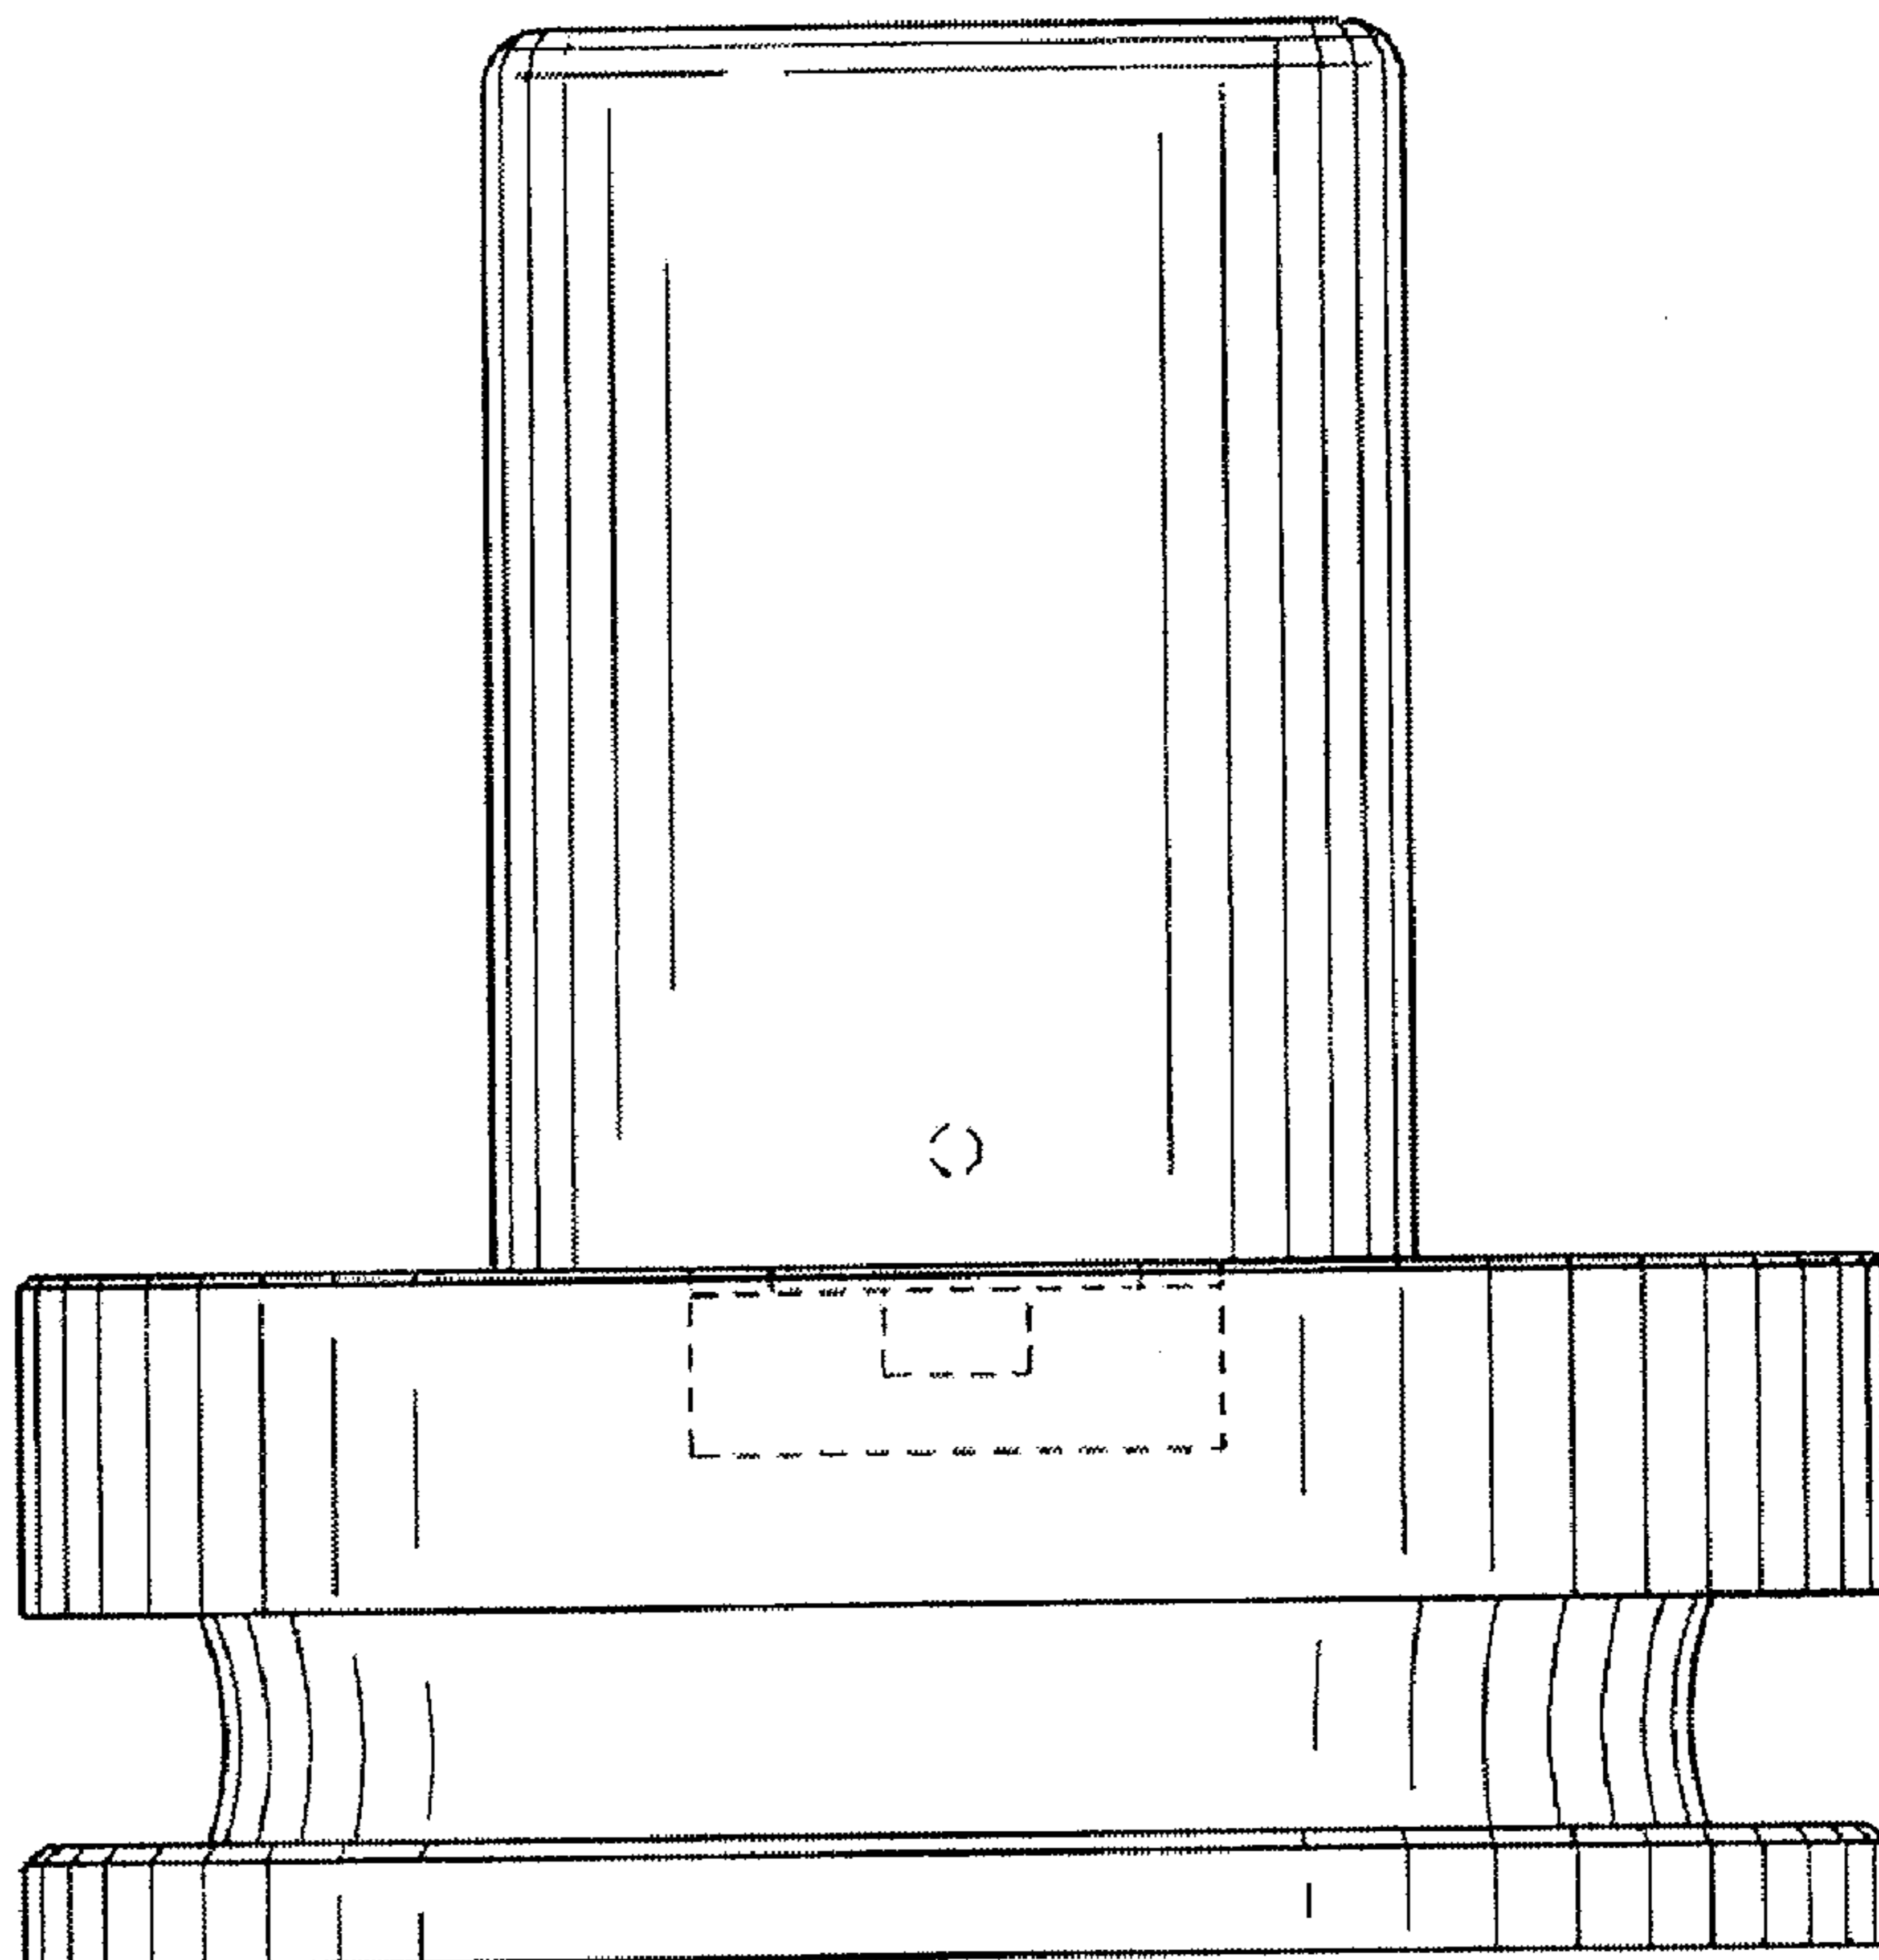


FIG. 2

FIG. 3

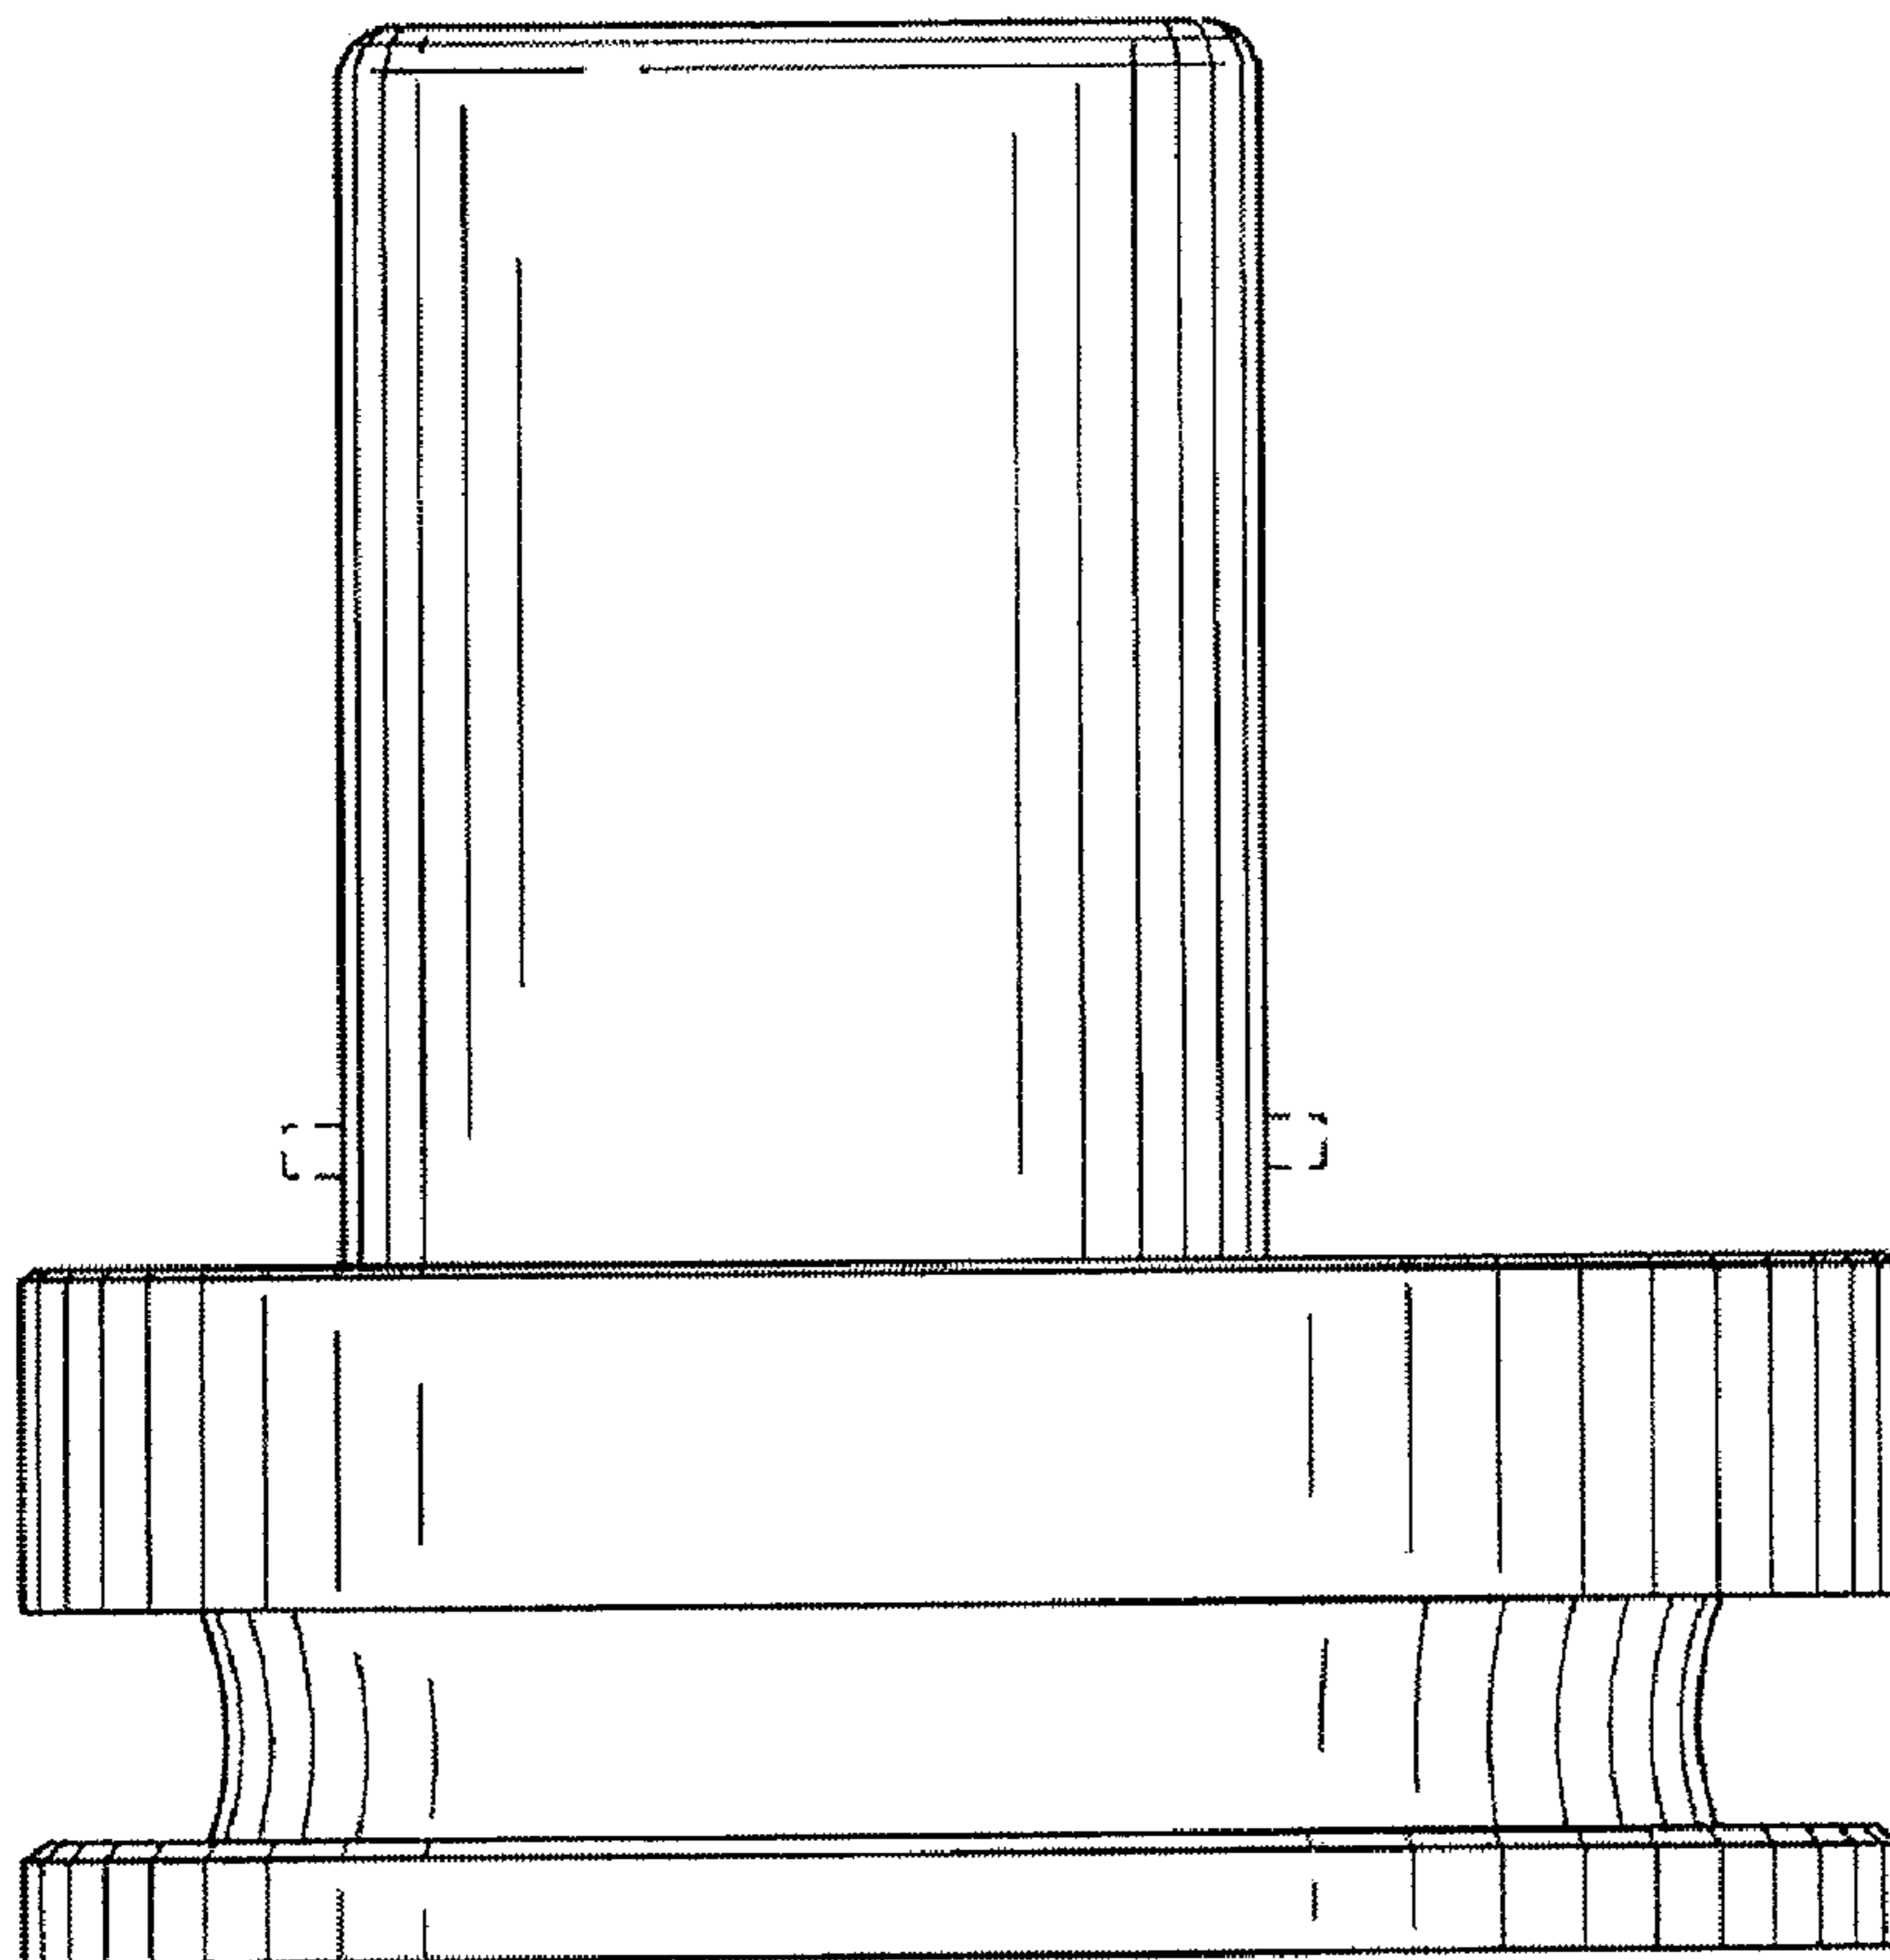
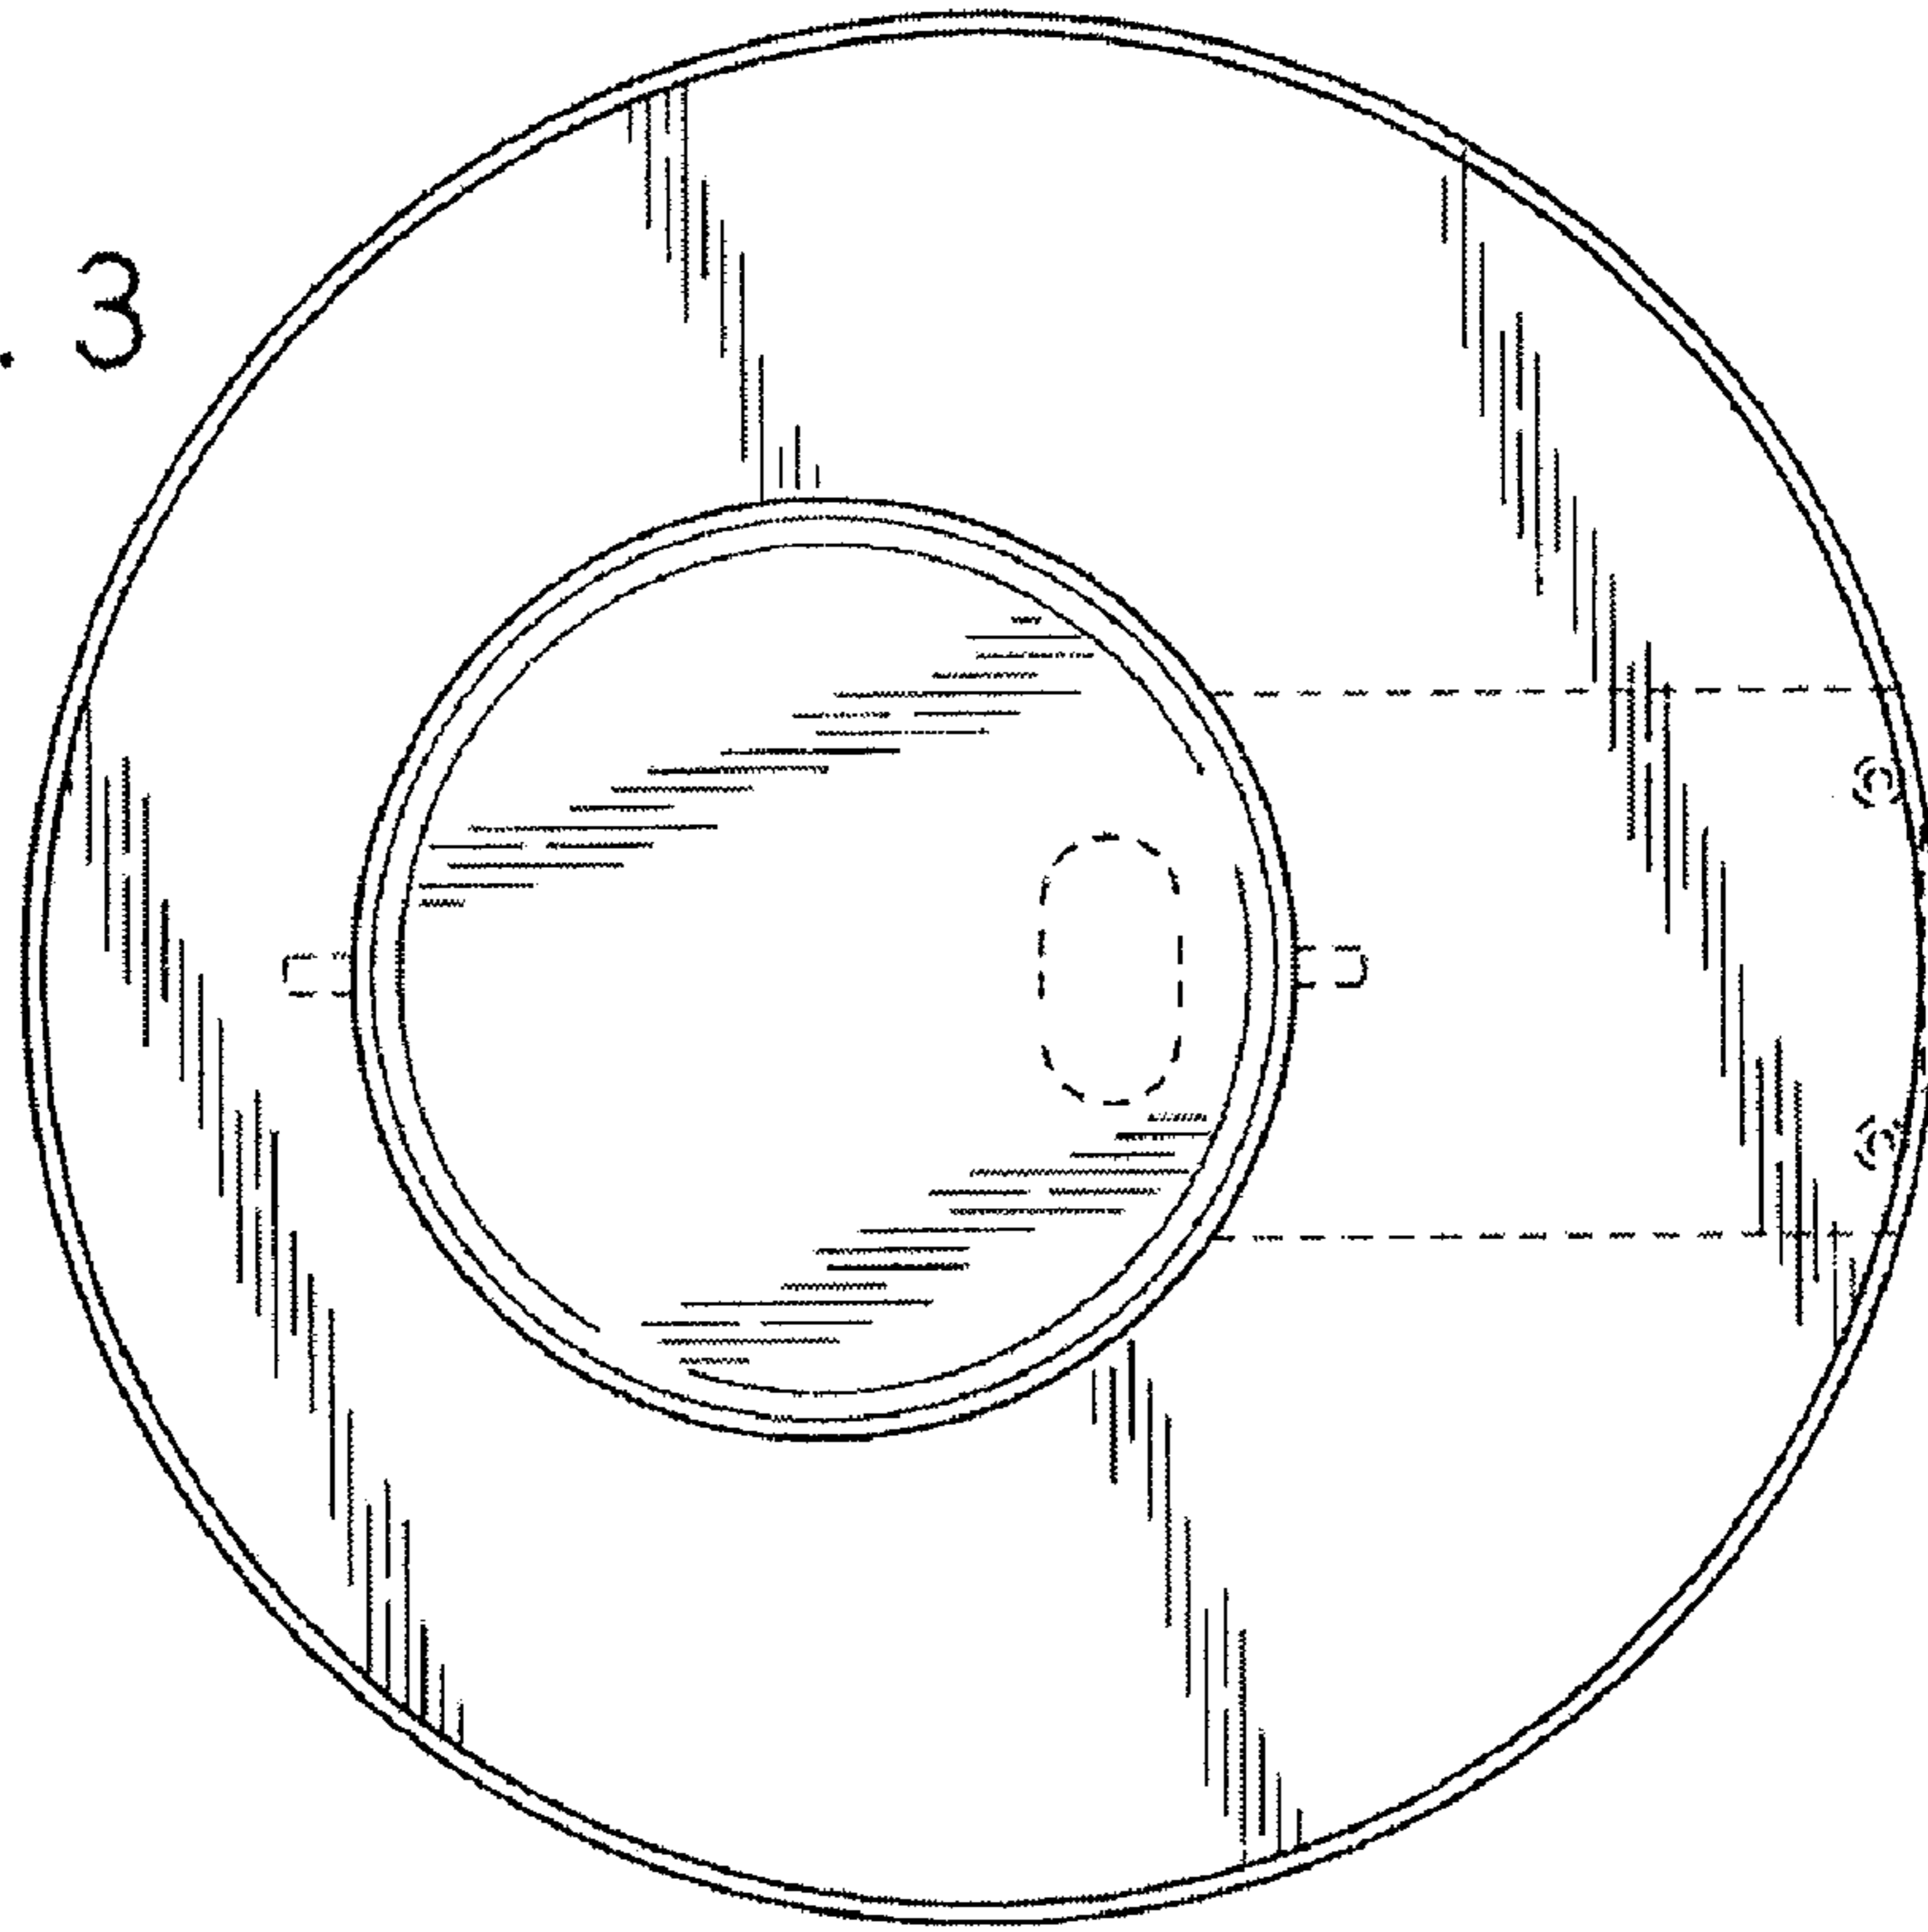


FIG. 4



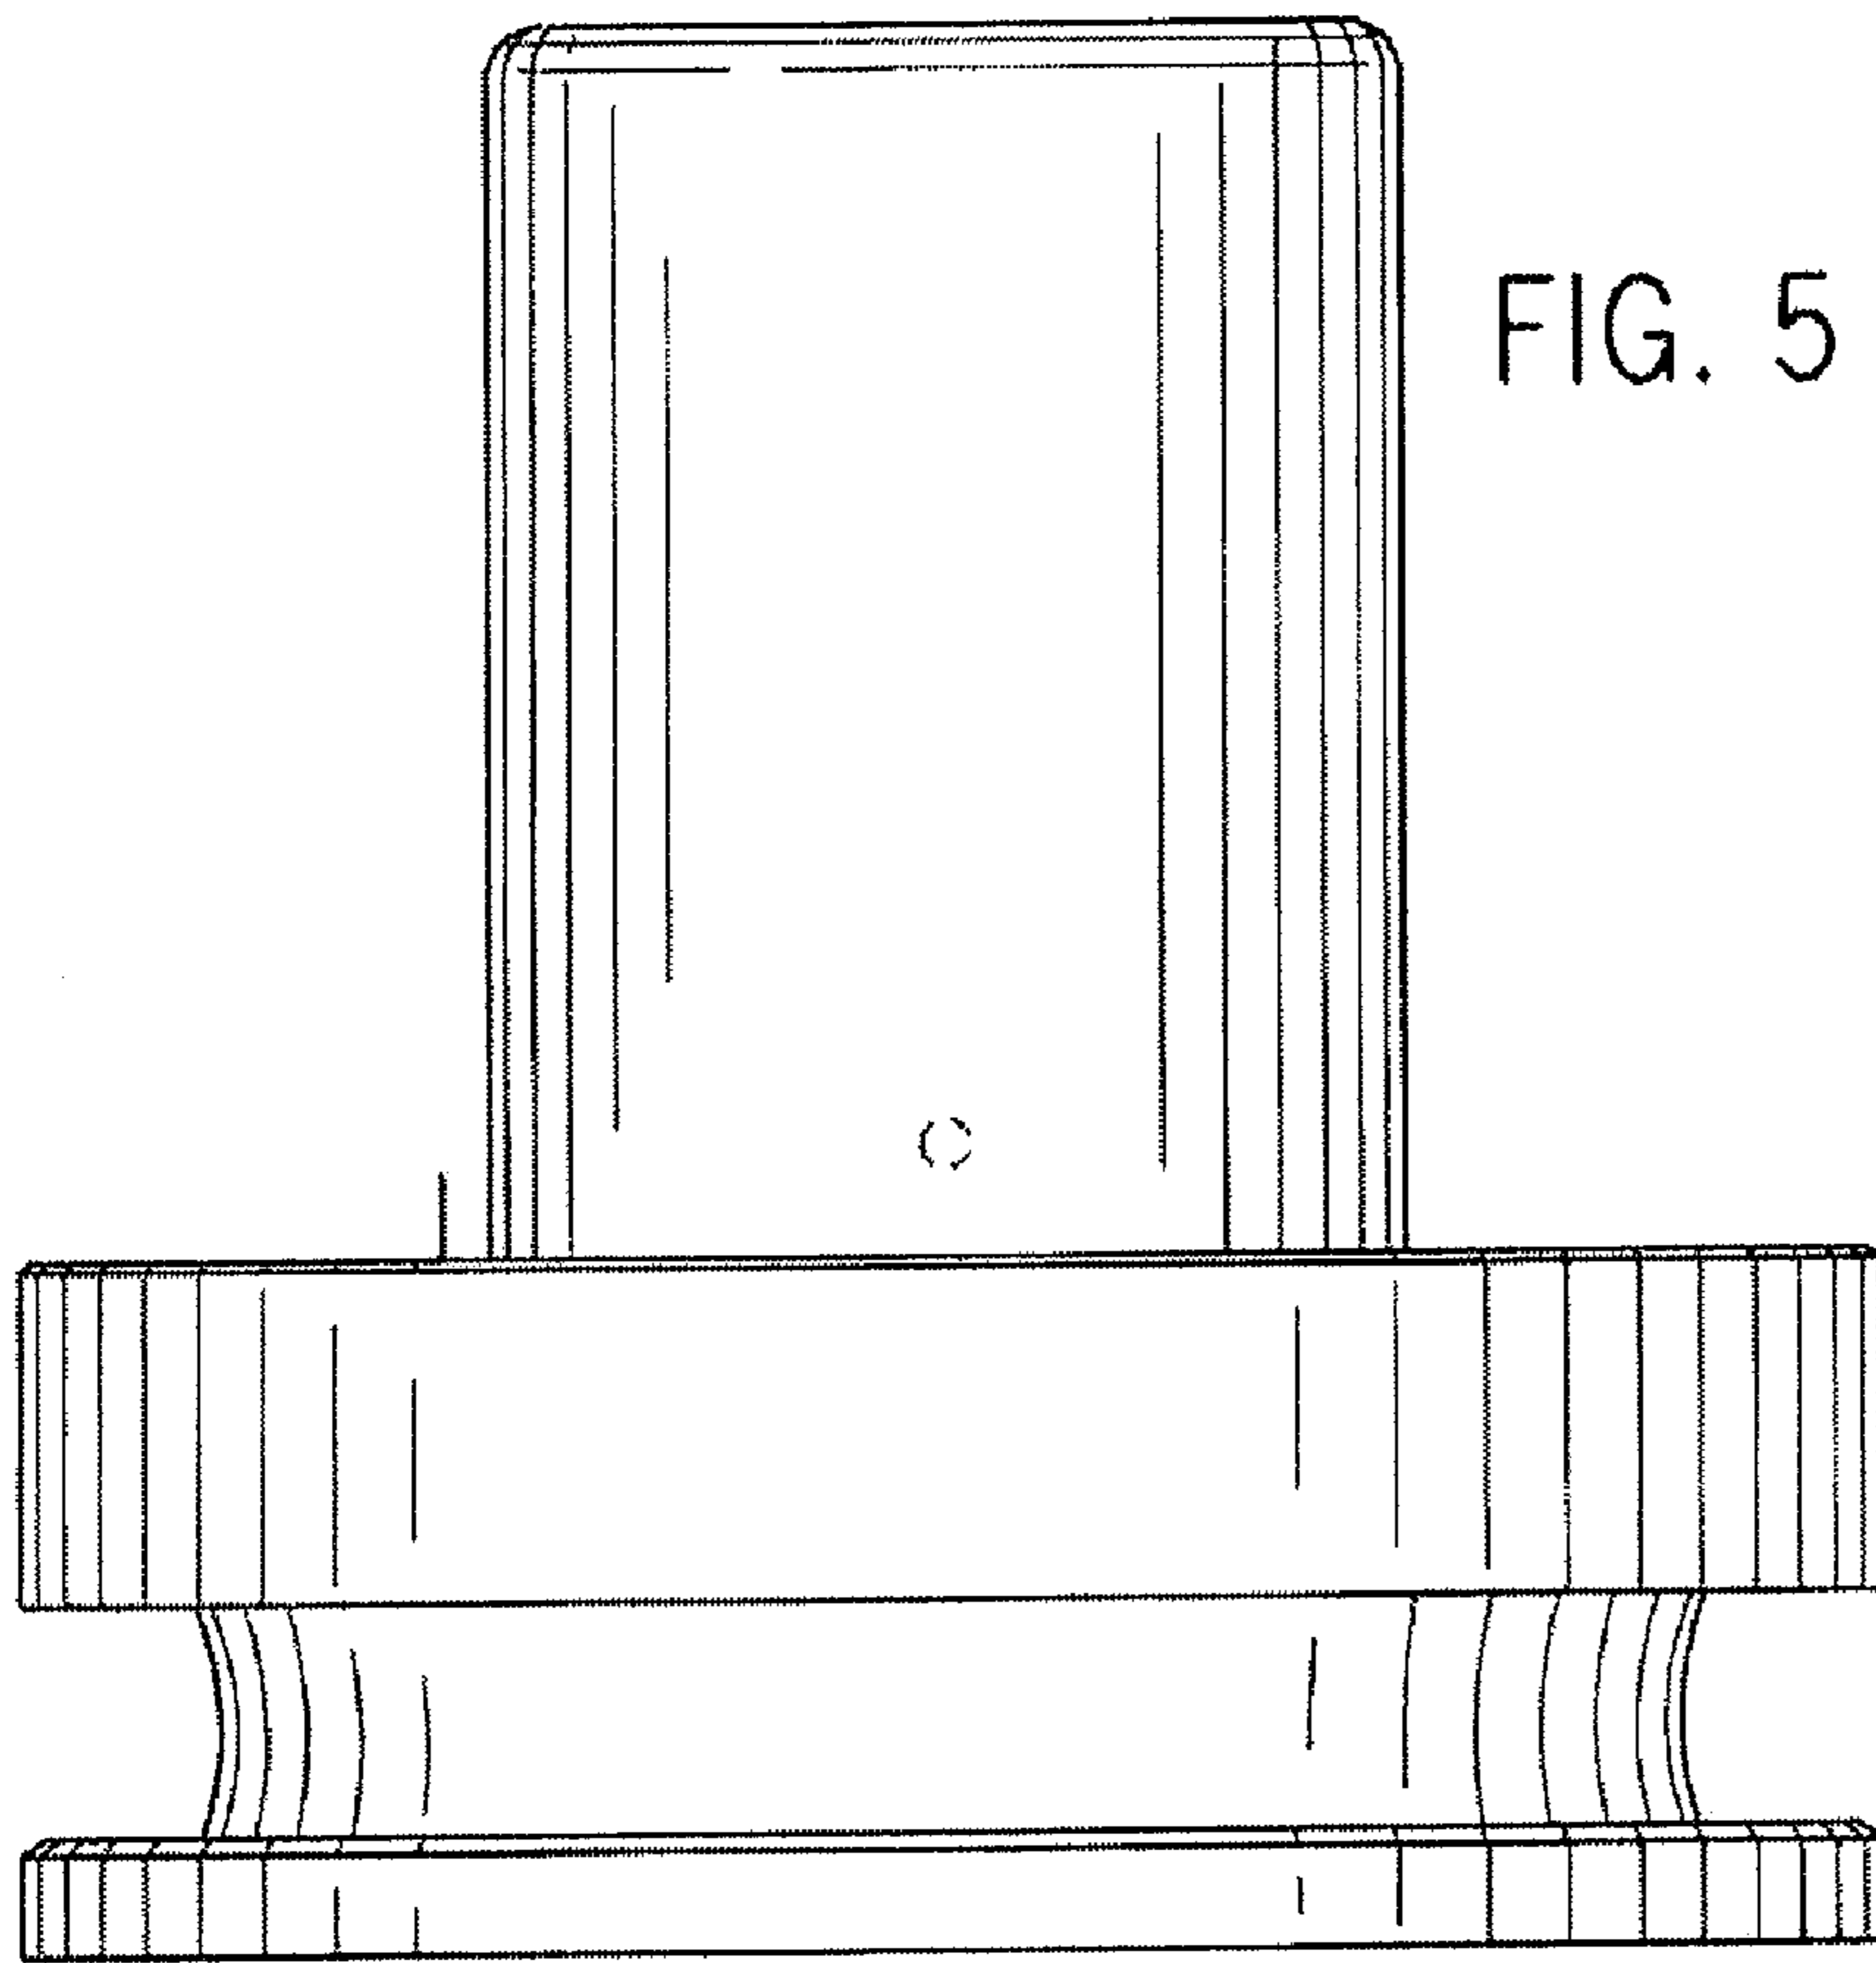


FIG. 6

