



US00D658776S

(12) **United States Design Patent**
Oonuma et al.

(10) **Patent No.:** **US D658,776 S**

(45) **Date of Patent:** **** May 1, 2012**

(54) **SAMPLE TUBE HOLDER STOCKER FOR CLINICAL LABORATORY AUTOMATION SYSTEM**

(75) Inventors: **Mitsuru Oonuma**, Tokyo (JP); **Yoko Sato**, FuchuKomae (JP); **Akira Omachi**, Komae (JP); **Tetsuya Isobe**, Hitachinaka (JP); **Kazuhiro Noda**, Hitachinaka (JP)

(73) Assignee: **Hitachi High-Technologies Corporation**, Tokyo (JP)

(**) Term: **14 Years**

(21) Appl. No.: **29/384,376**

(22) Filed: **Jan. 31, 2011**

(30) **Foreign Application Priority Data**

Sep. 29, 2010 (JP) 2010-023336

(51) **LOC (9) Cl.** **24-01**

(52) **U.S. Cl.** **D24/216**

(58) **Field of Classification Search** D24/216, D24/224, 231, 232, 186, 107, 169, 217, 233; D10/46, 81; 422/500, 547, 62-65, 67; 435/287.1, 435/287.3; 436/43, 45, 47
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

- 4,946,651 A * 8/1990 Liston et al. 436/43
- D347,478 S * 5/1994 Pinkney D24/216
- D356,967 S * 4/1995 Takekoshi et al. D10/81
- 5,986,260 A * 11/1999 Oonuma et al. 250/288

- D508,999 S * 8/2005 Fanning et al. D24/216
- D523,153 S * 6/2006 Akashi et al. D24/232
- D631,976 S 2/2011 Oonuma et al.
- 2004/0081583 A1 * 4/2004 Berndt et al. 422/63
- 2007/0110617 A1 * 5/2007 Nagai et al. 422/65
- 2008/0019868 A1 * 1/2008 Okumoto et al. 422/63
- 2009/0325274 A1 * 12/2009 Hamada et al. 422/65

* cited by examiner

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Antonelli, Terry, Stout & Kraus, LLP.

(57) **CLAIM**


We claim the ornamental design for a sample tube holder stocker for clinical laboratory automation system, as shown and described.

DESCRIPTION

FIG. 1 is a front, top and right side perspective view of a sample tube holder stocker for clinical laboratory automation system showing our new design; FIG. 2 is a front elevational view thereof; FIG. 3 is a rear elevational view thereof; FIG. 4 is a top plan view thereof; FIG. 5 is a bottom plan view thereof; FIG. 6 is a left side elevational view thereof; FIG. 7 is a right side elevational view thereof; and, FIG. 8 is a right side elevational view thereof shown in an opened position.

The broken lines shown in all drawing views are included for the purpose of illustrating portions of the sample tube holder stocker for clinical laboratory automation system that form no part of the claimed design.

1 Claim, 6 Drawing Sheets

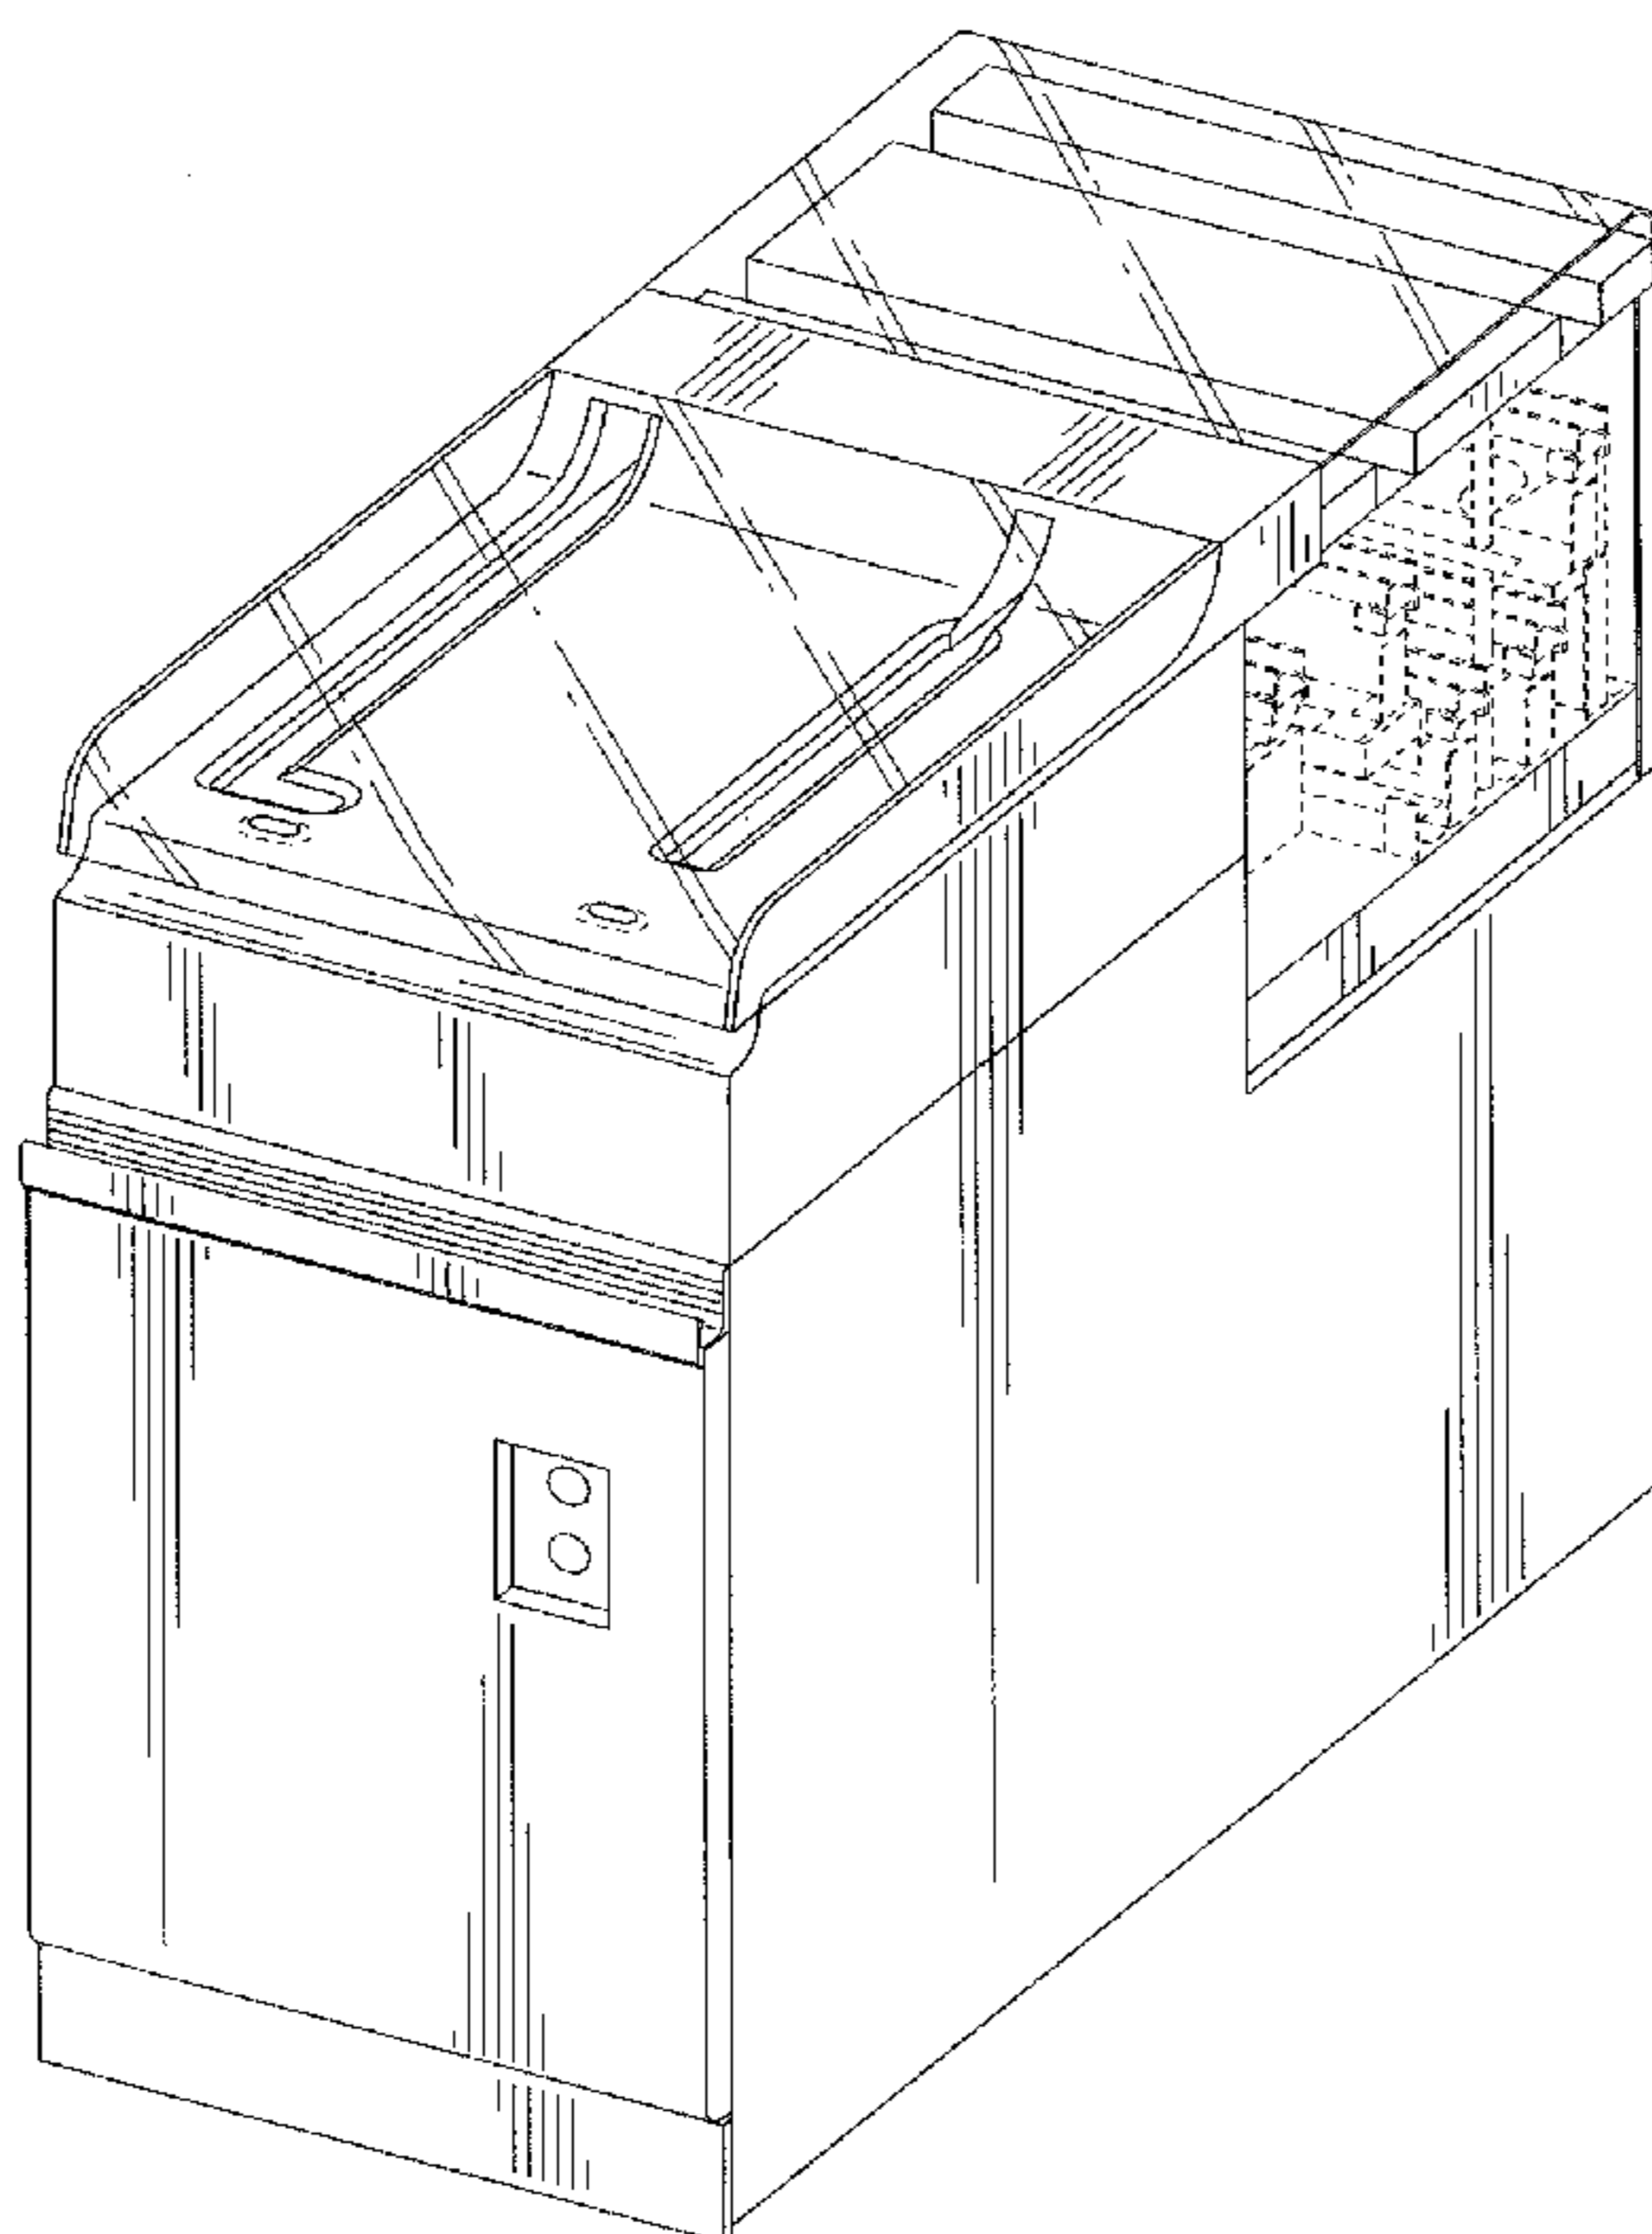

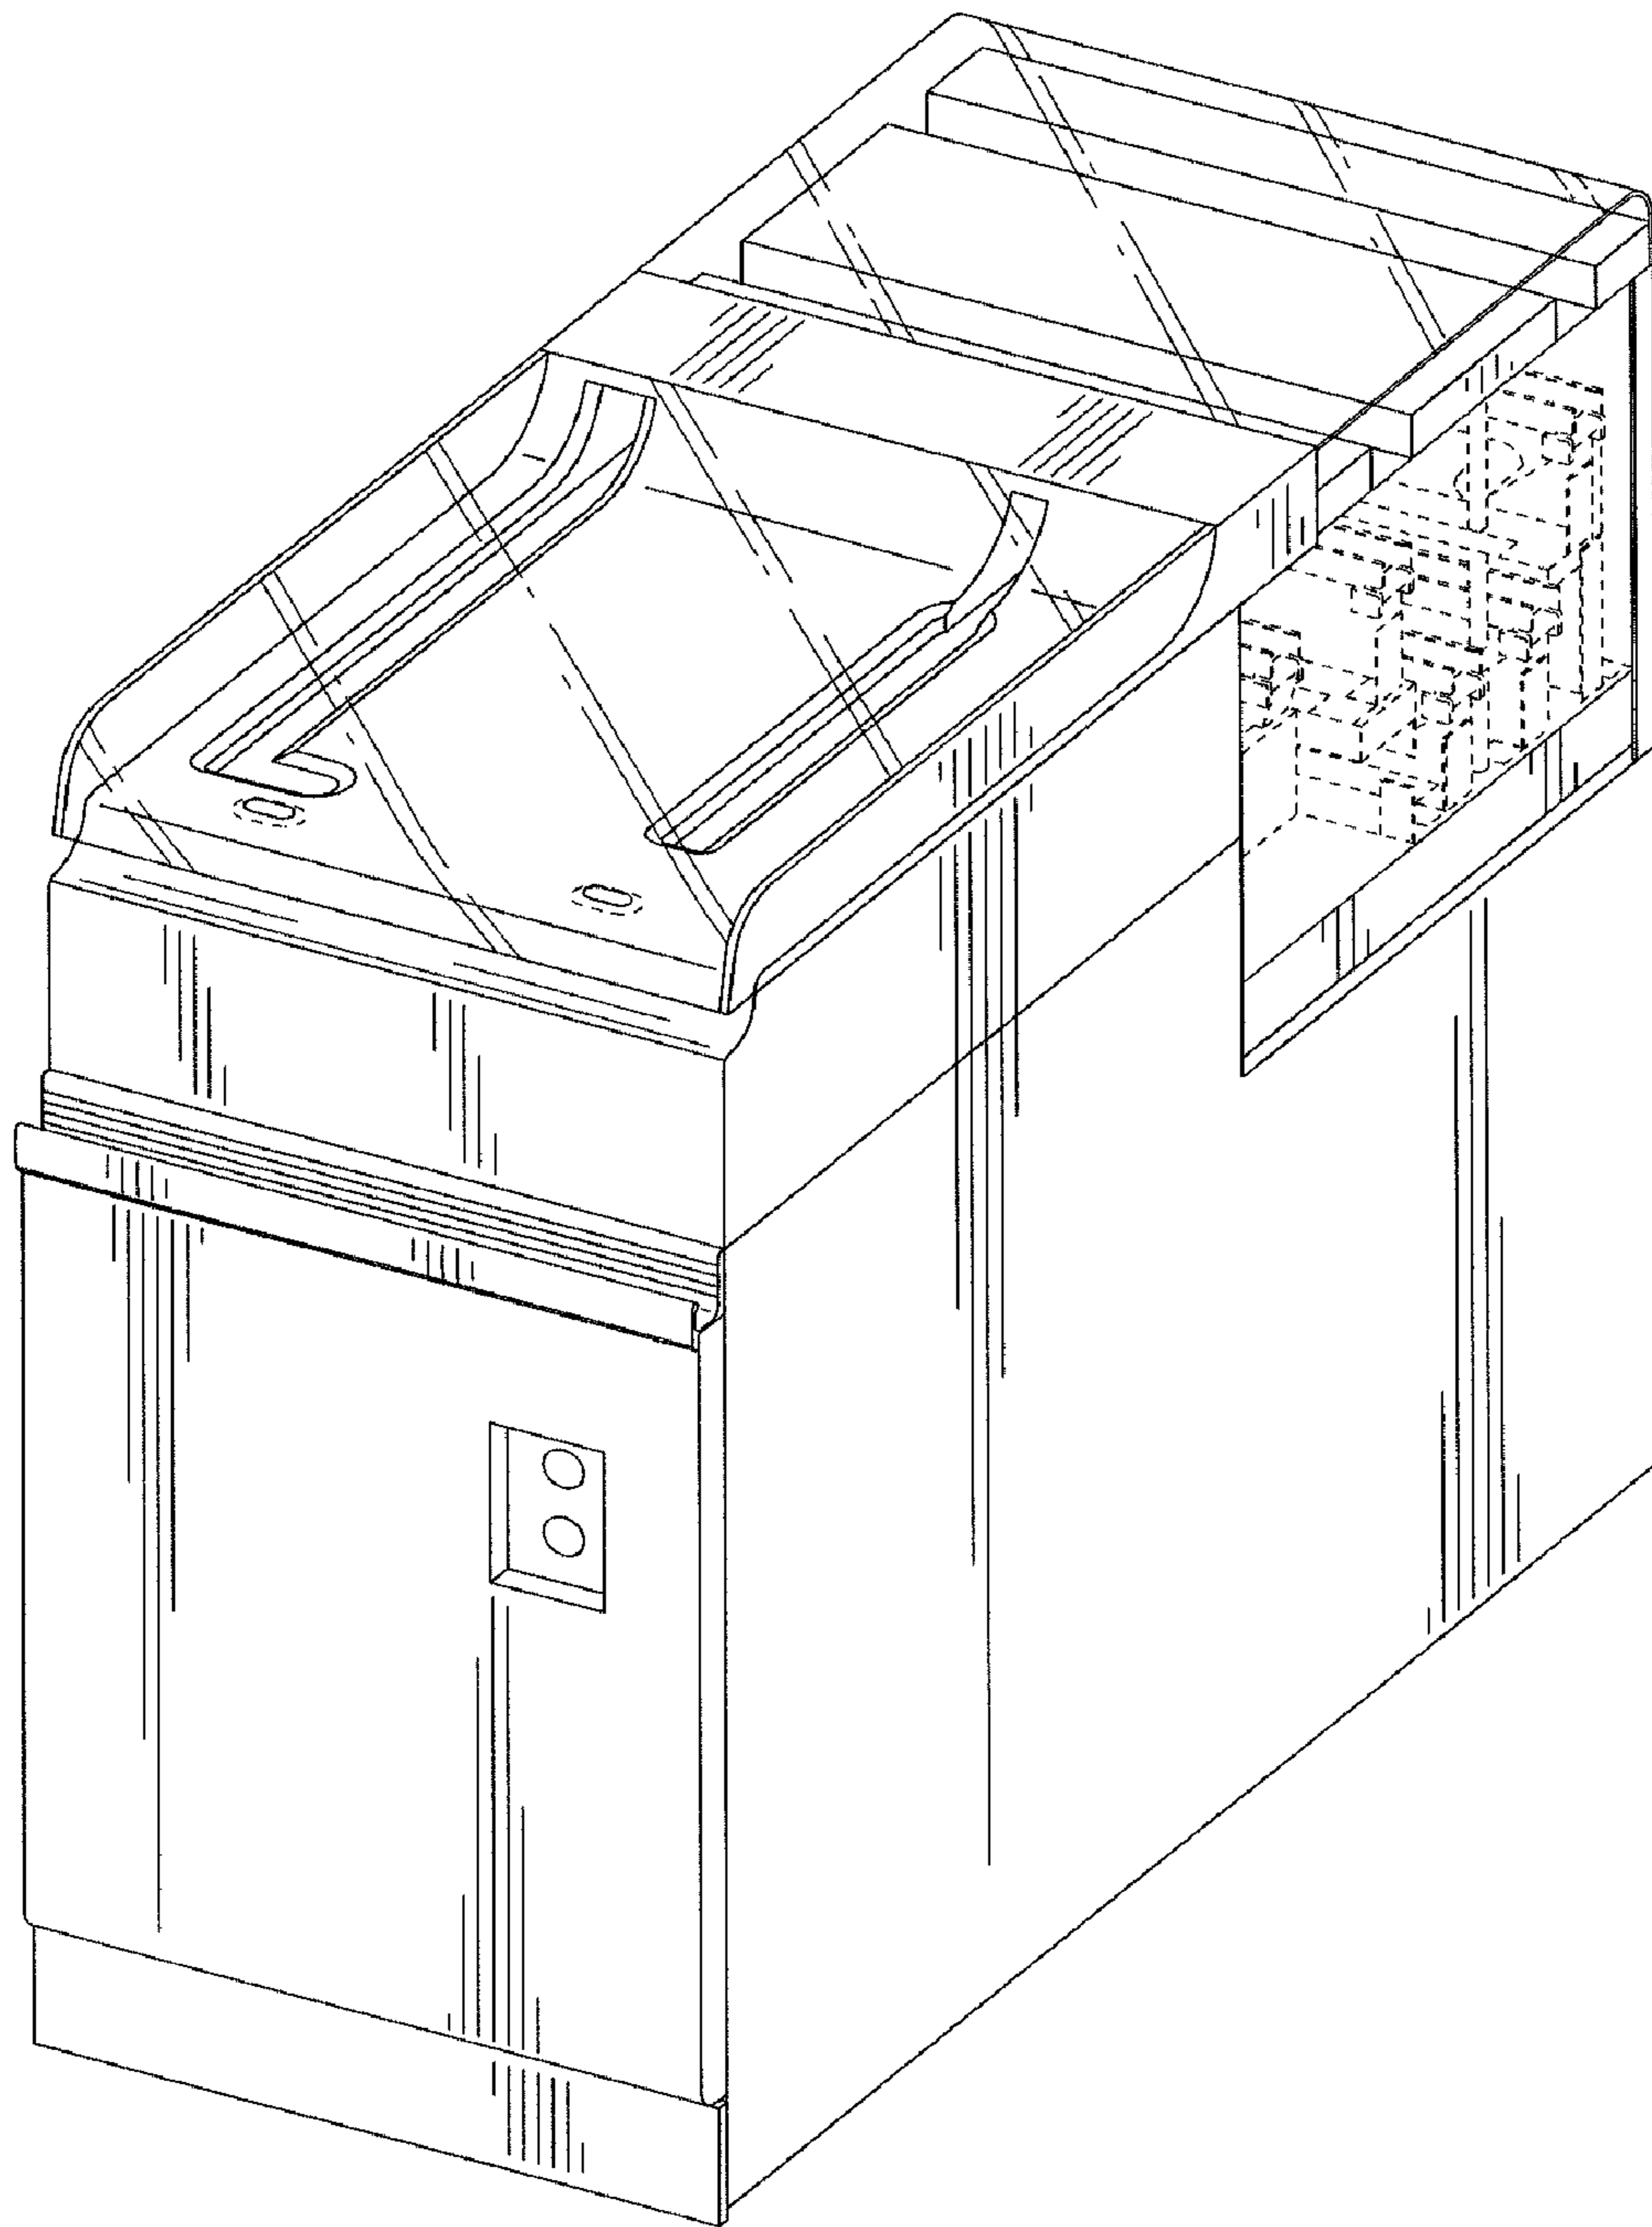


FIG. 1

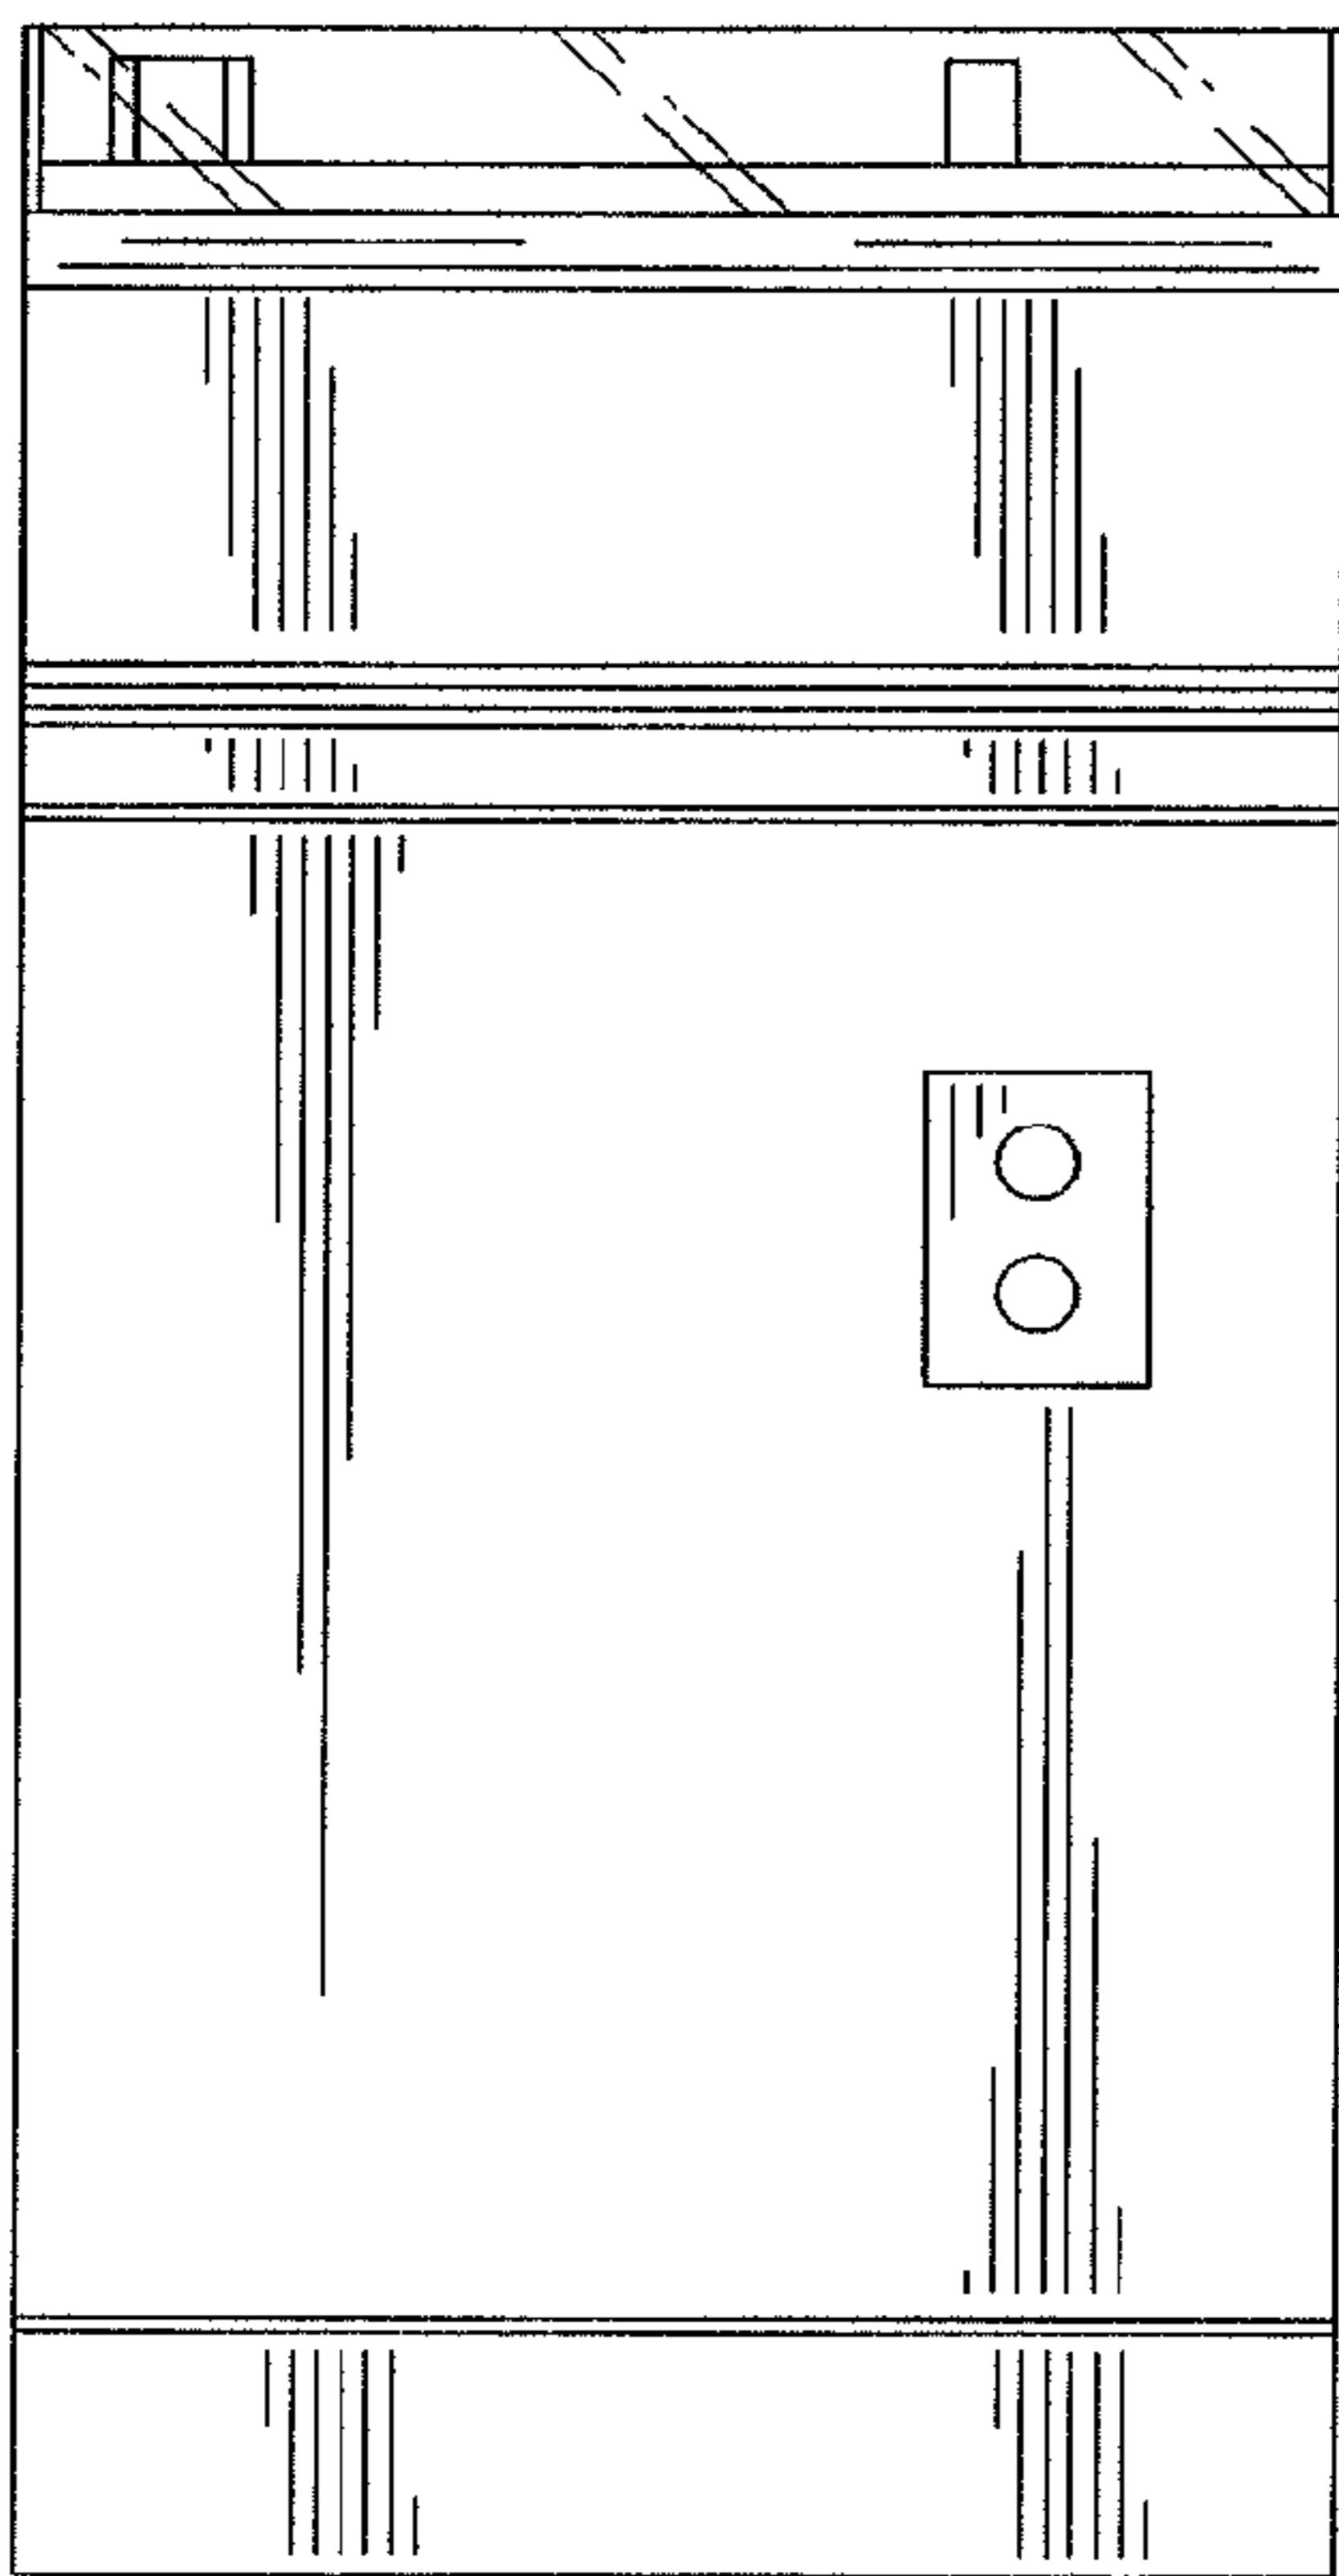


FIG. 2

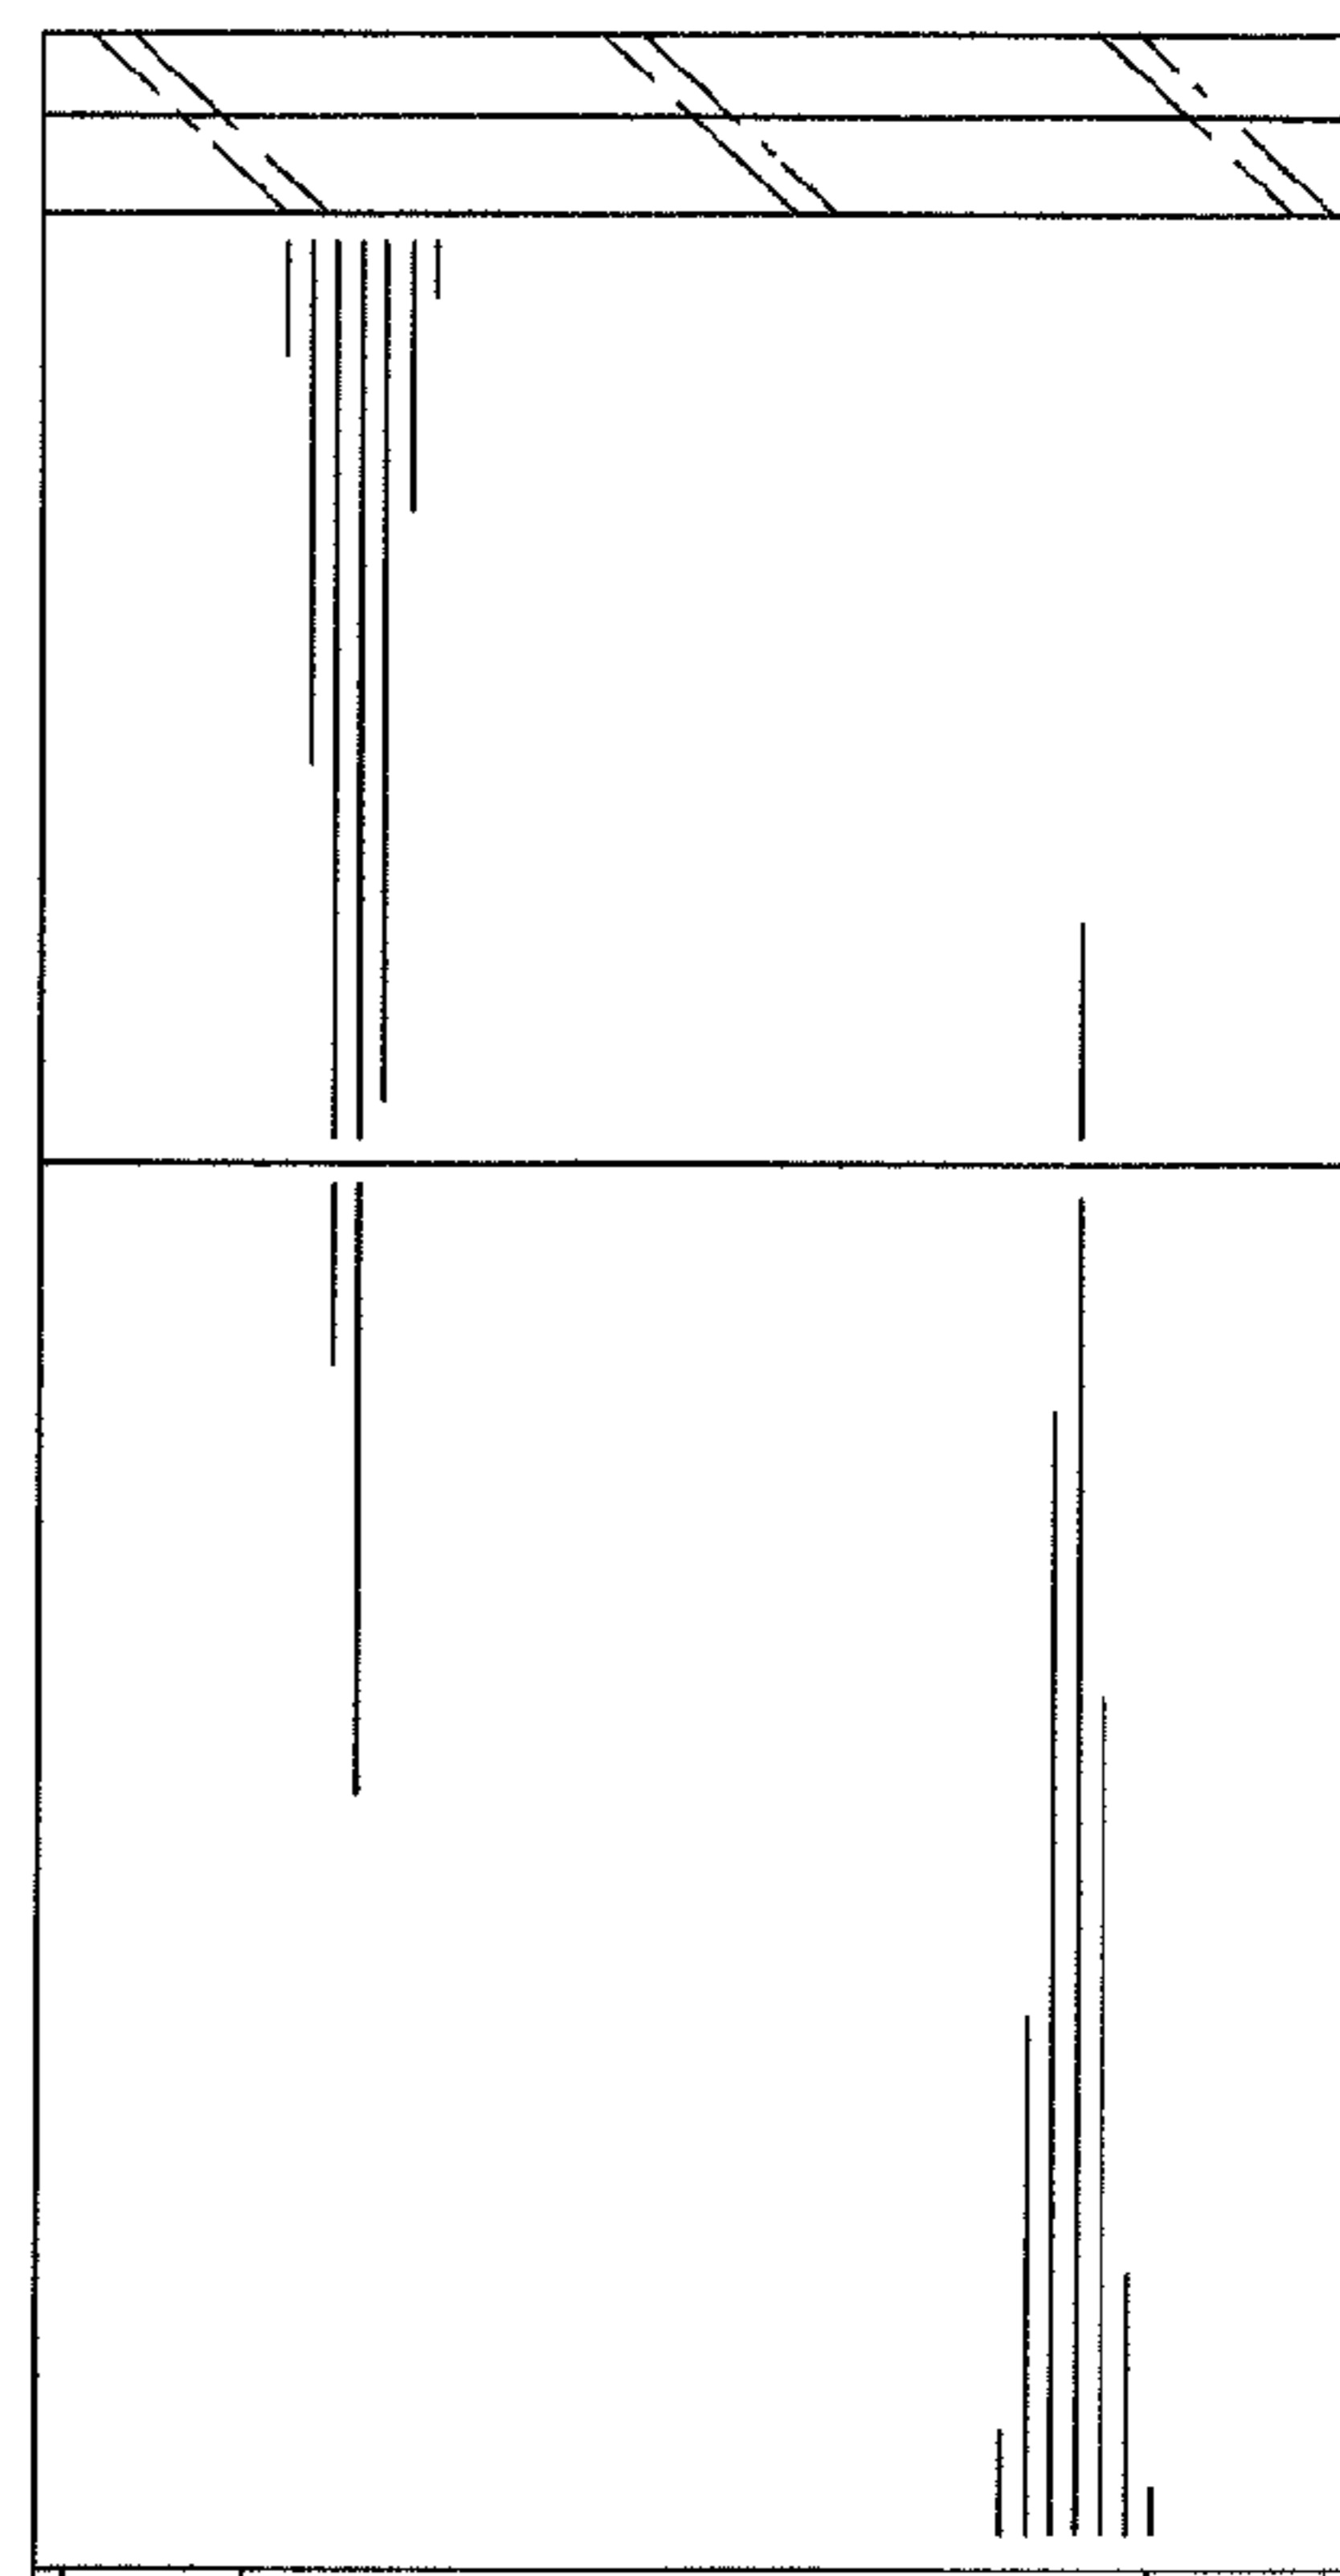


FIG. 3

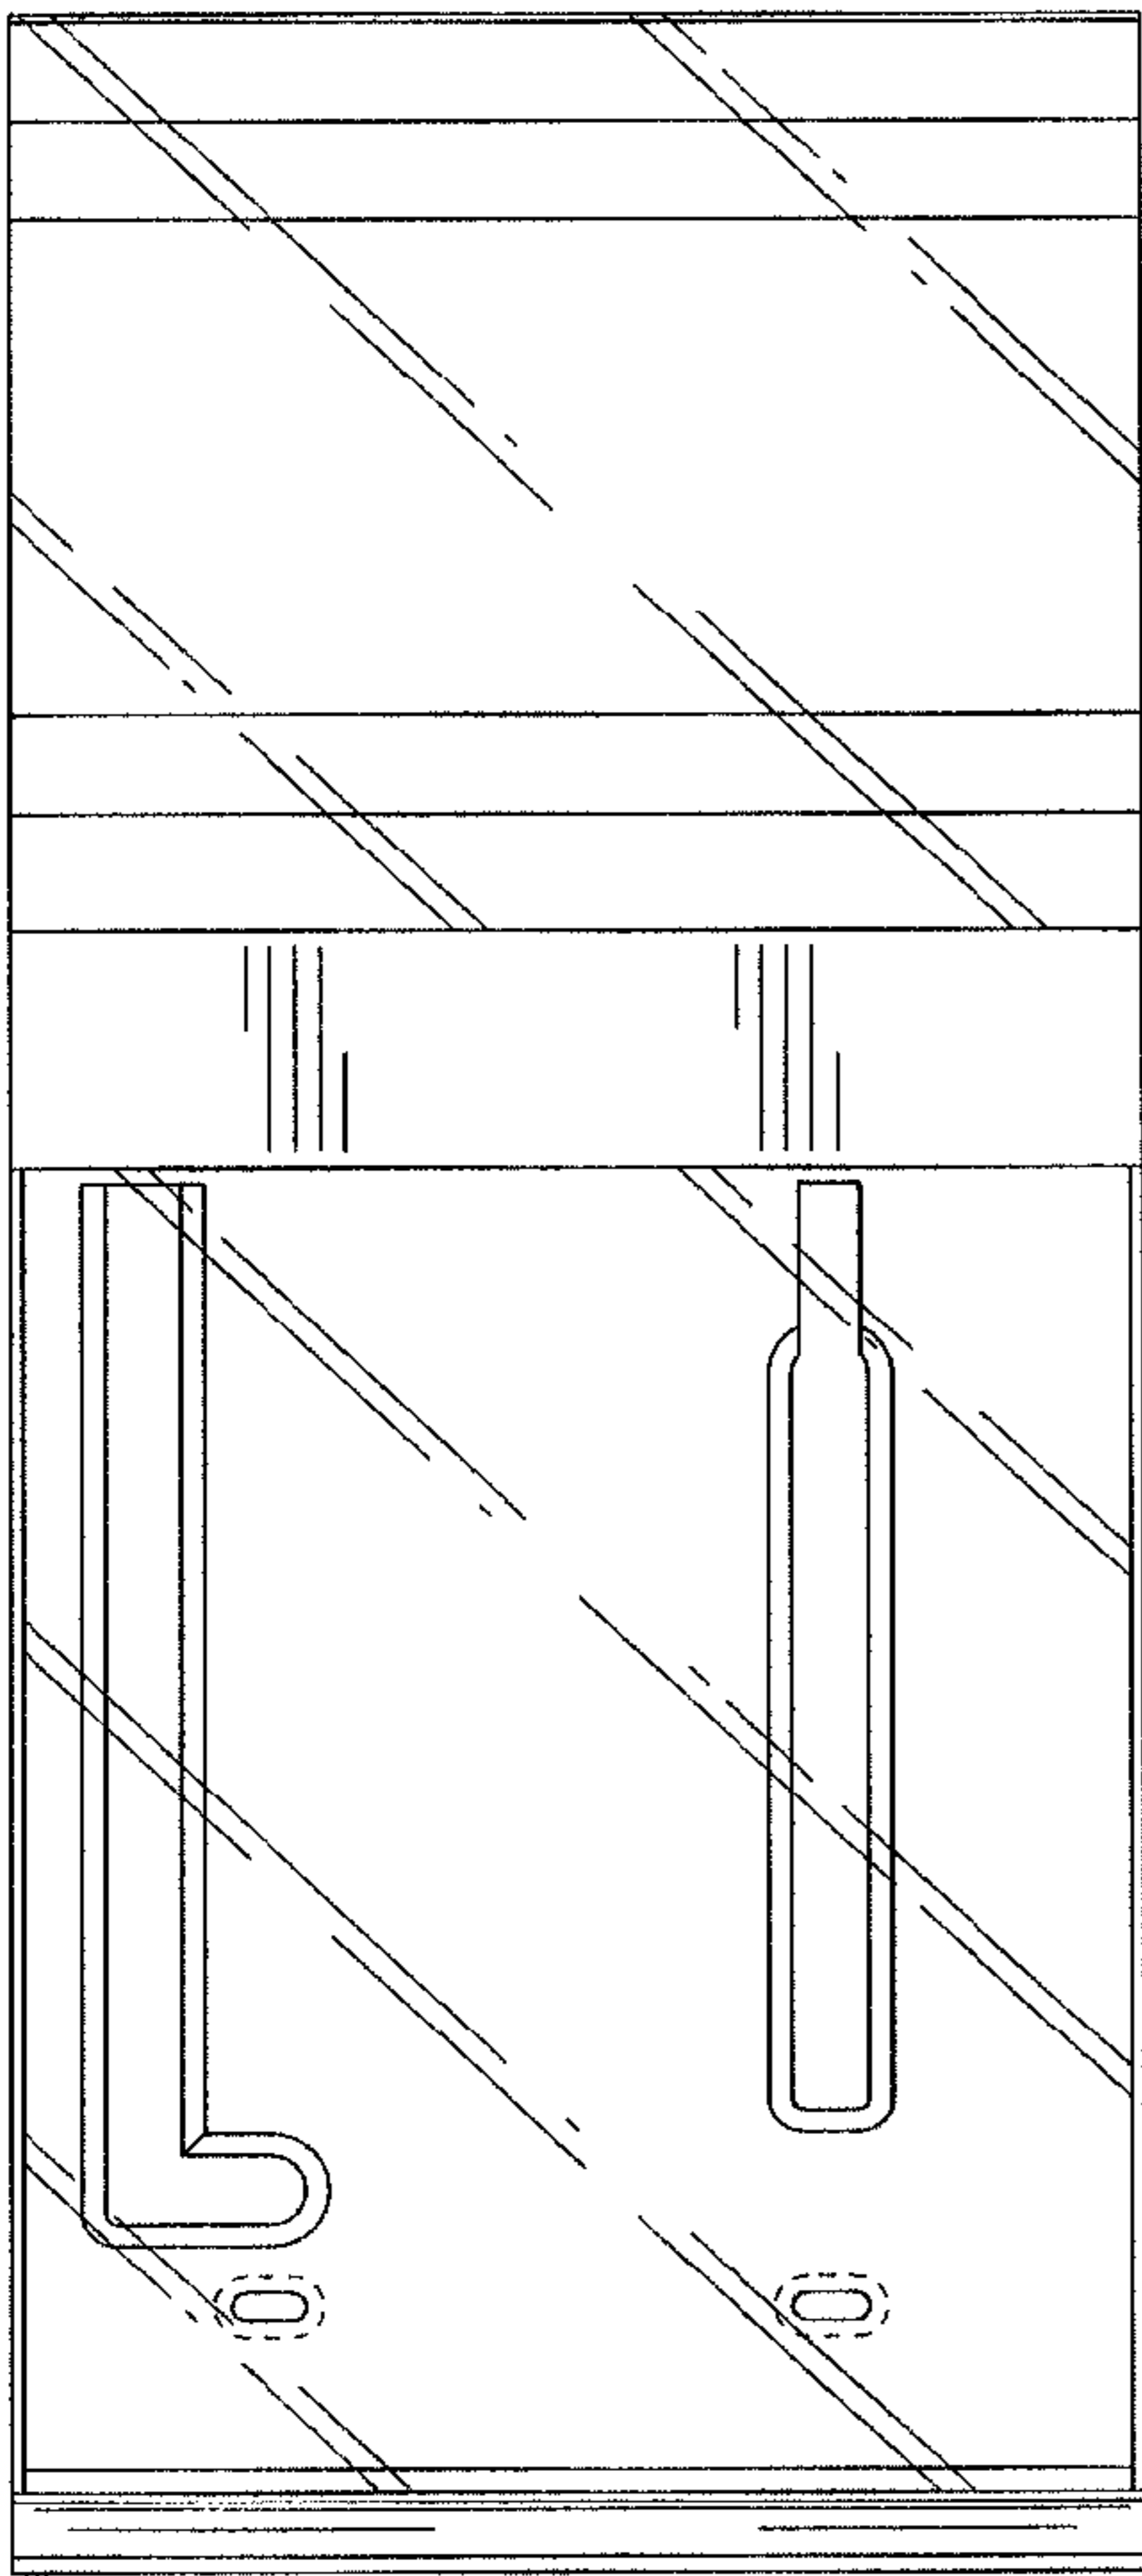


FIG. 4

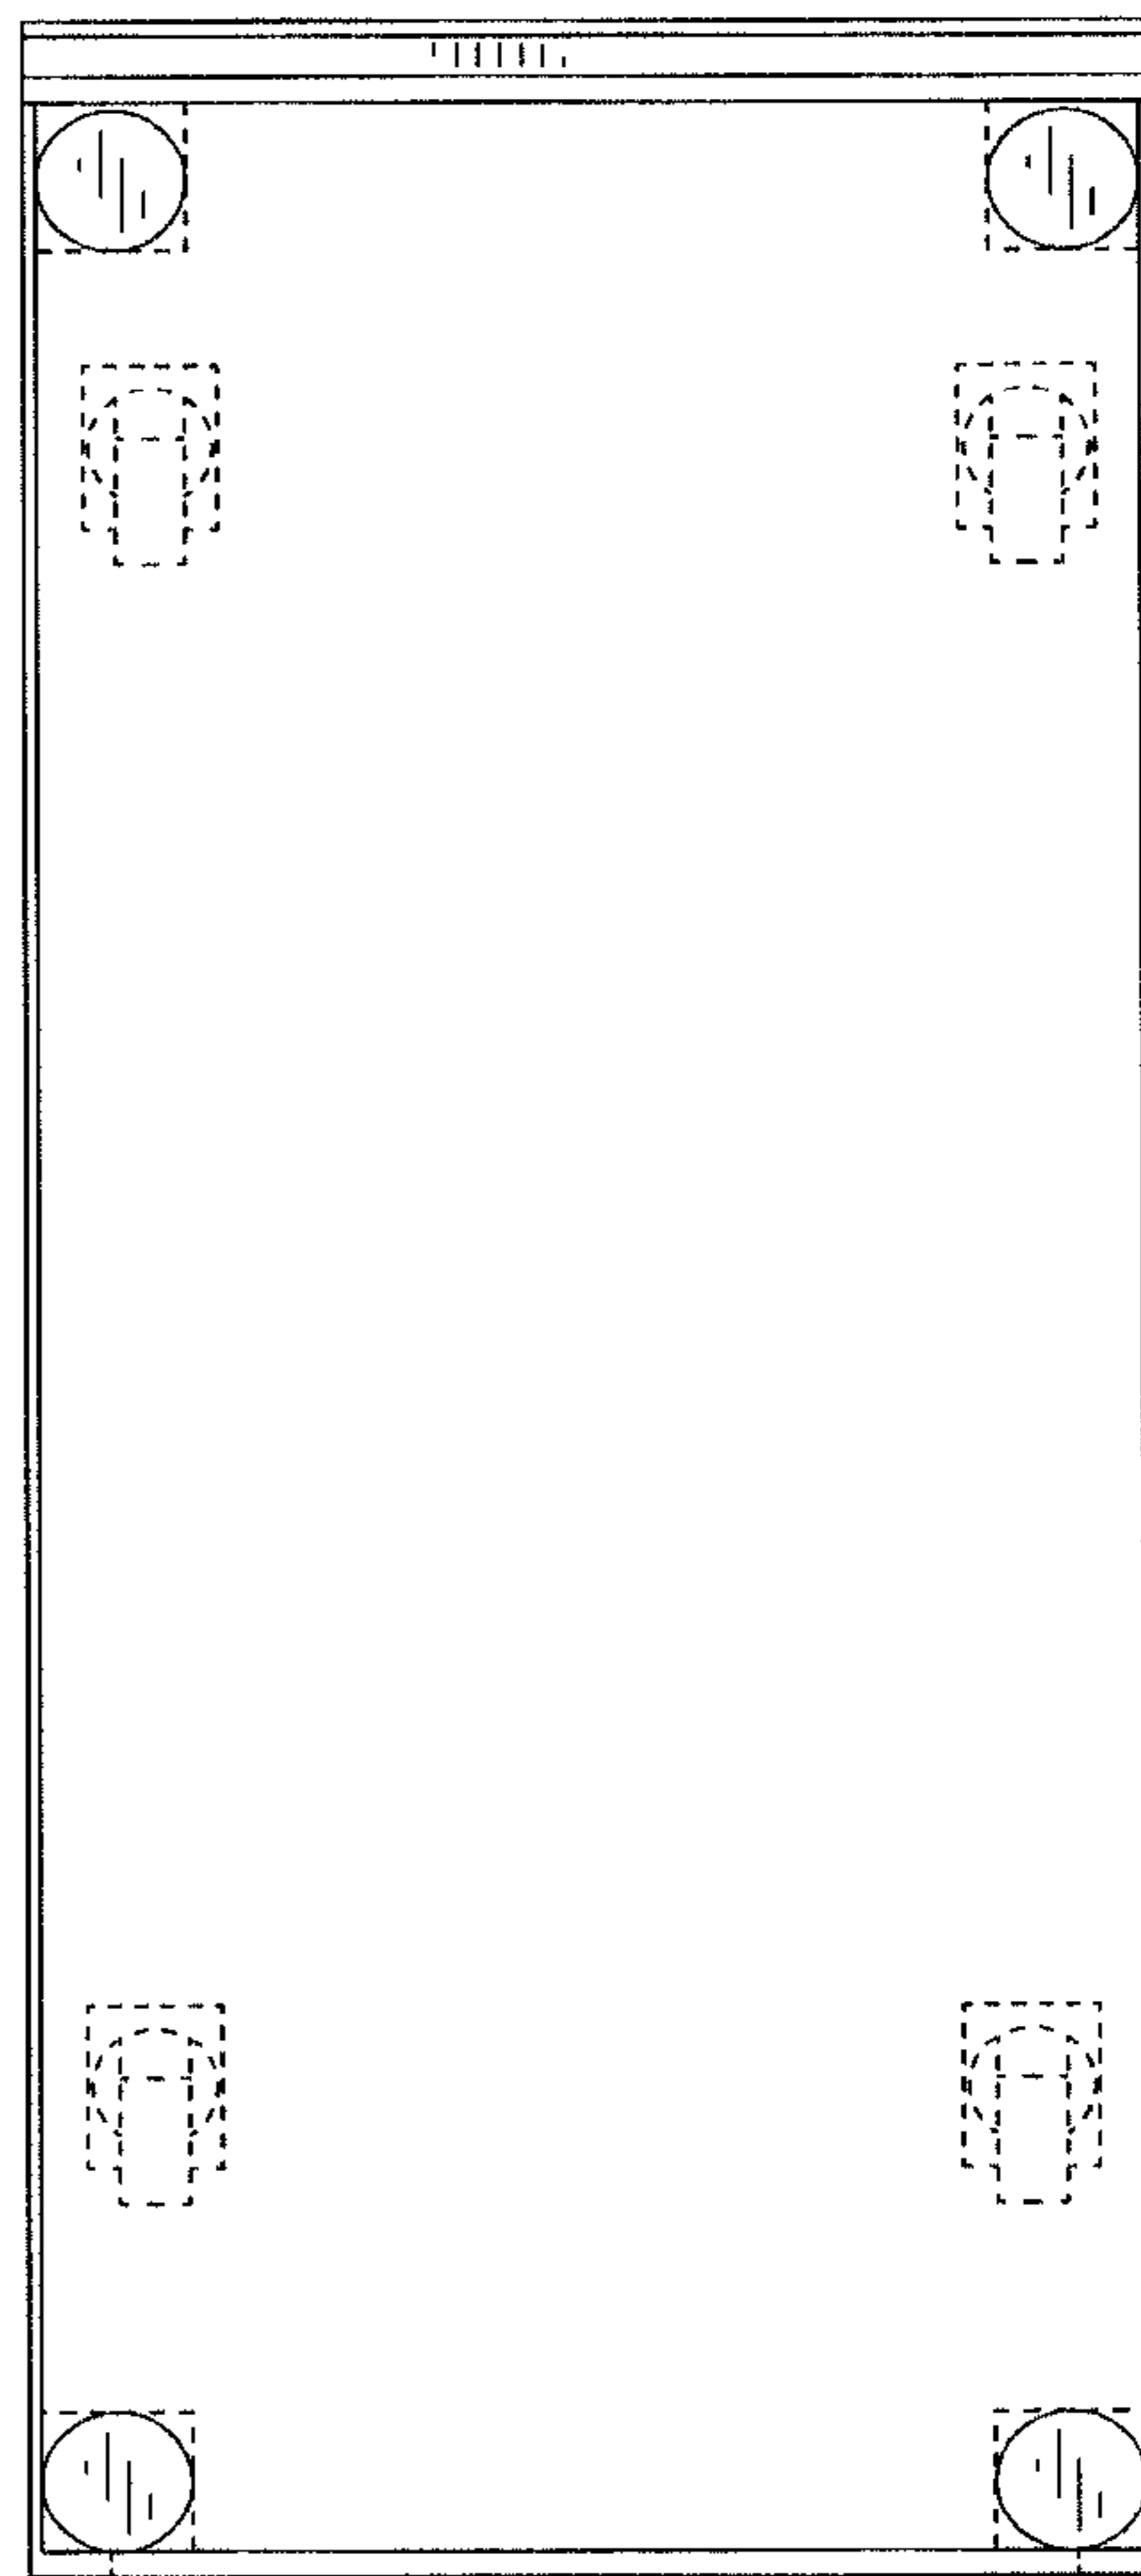


FIG. 5

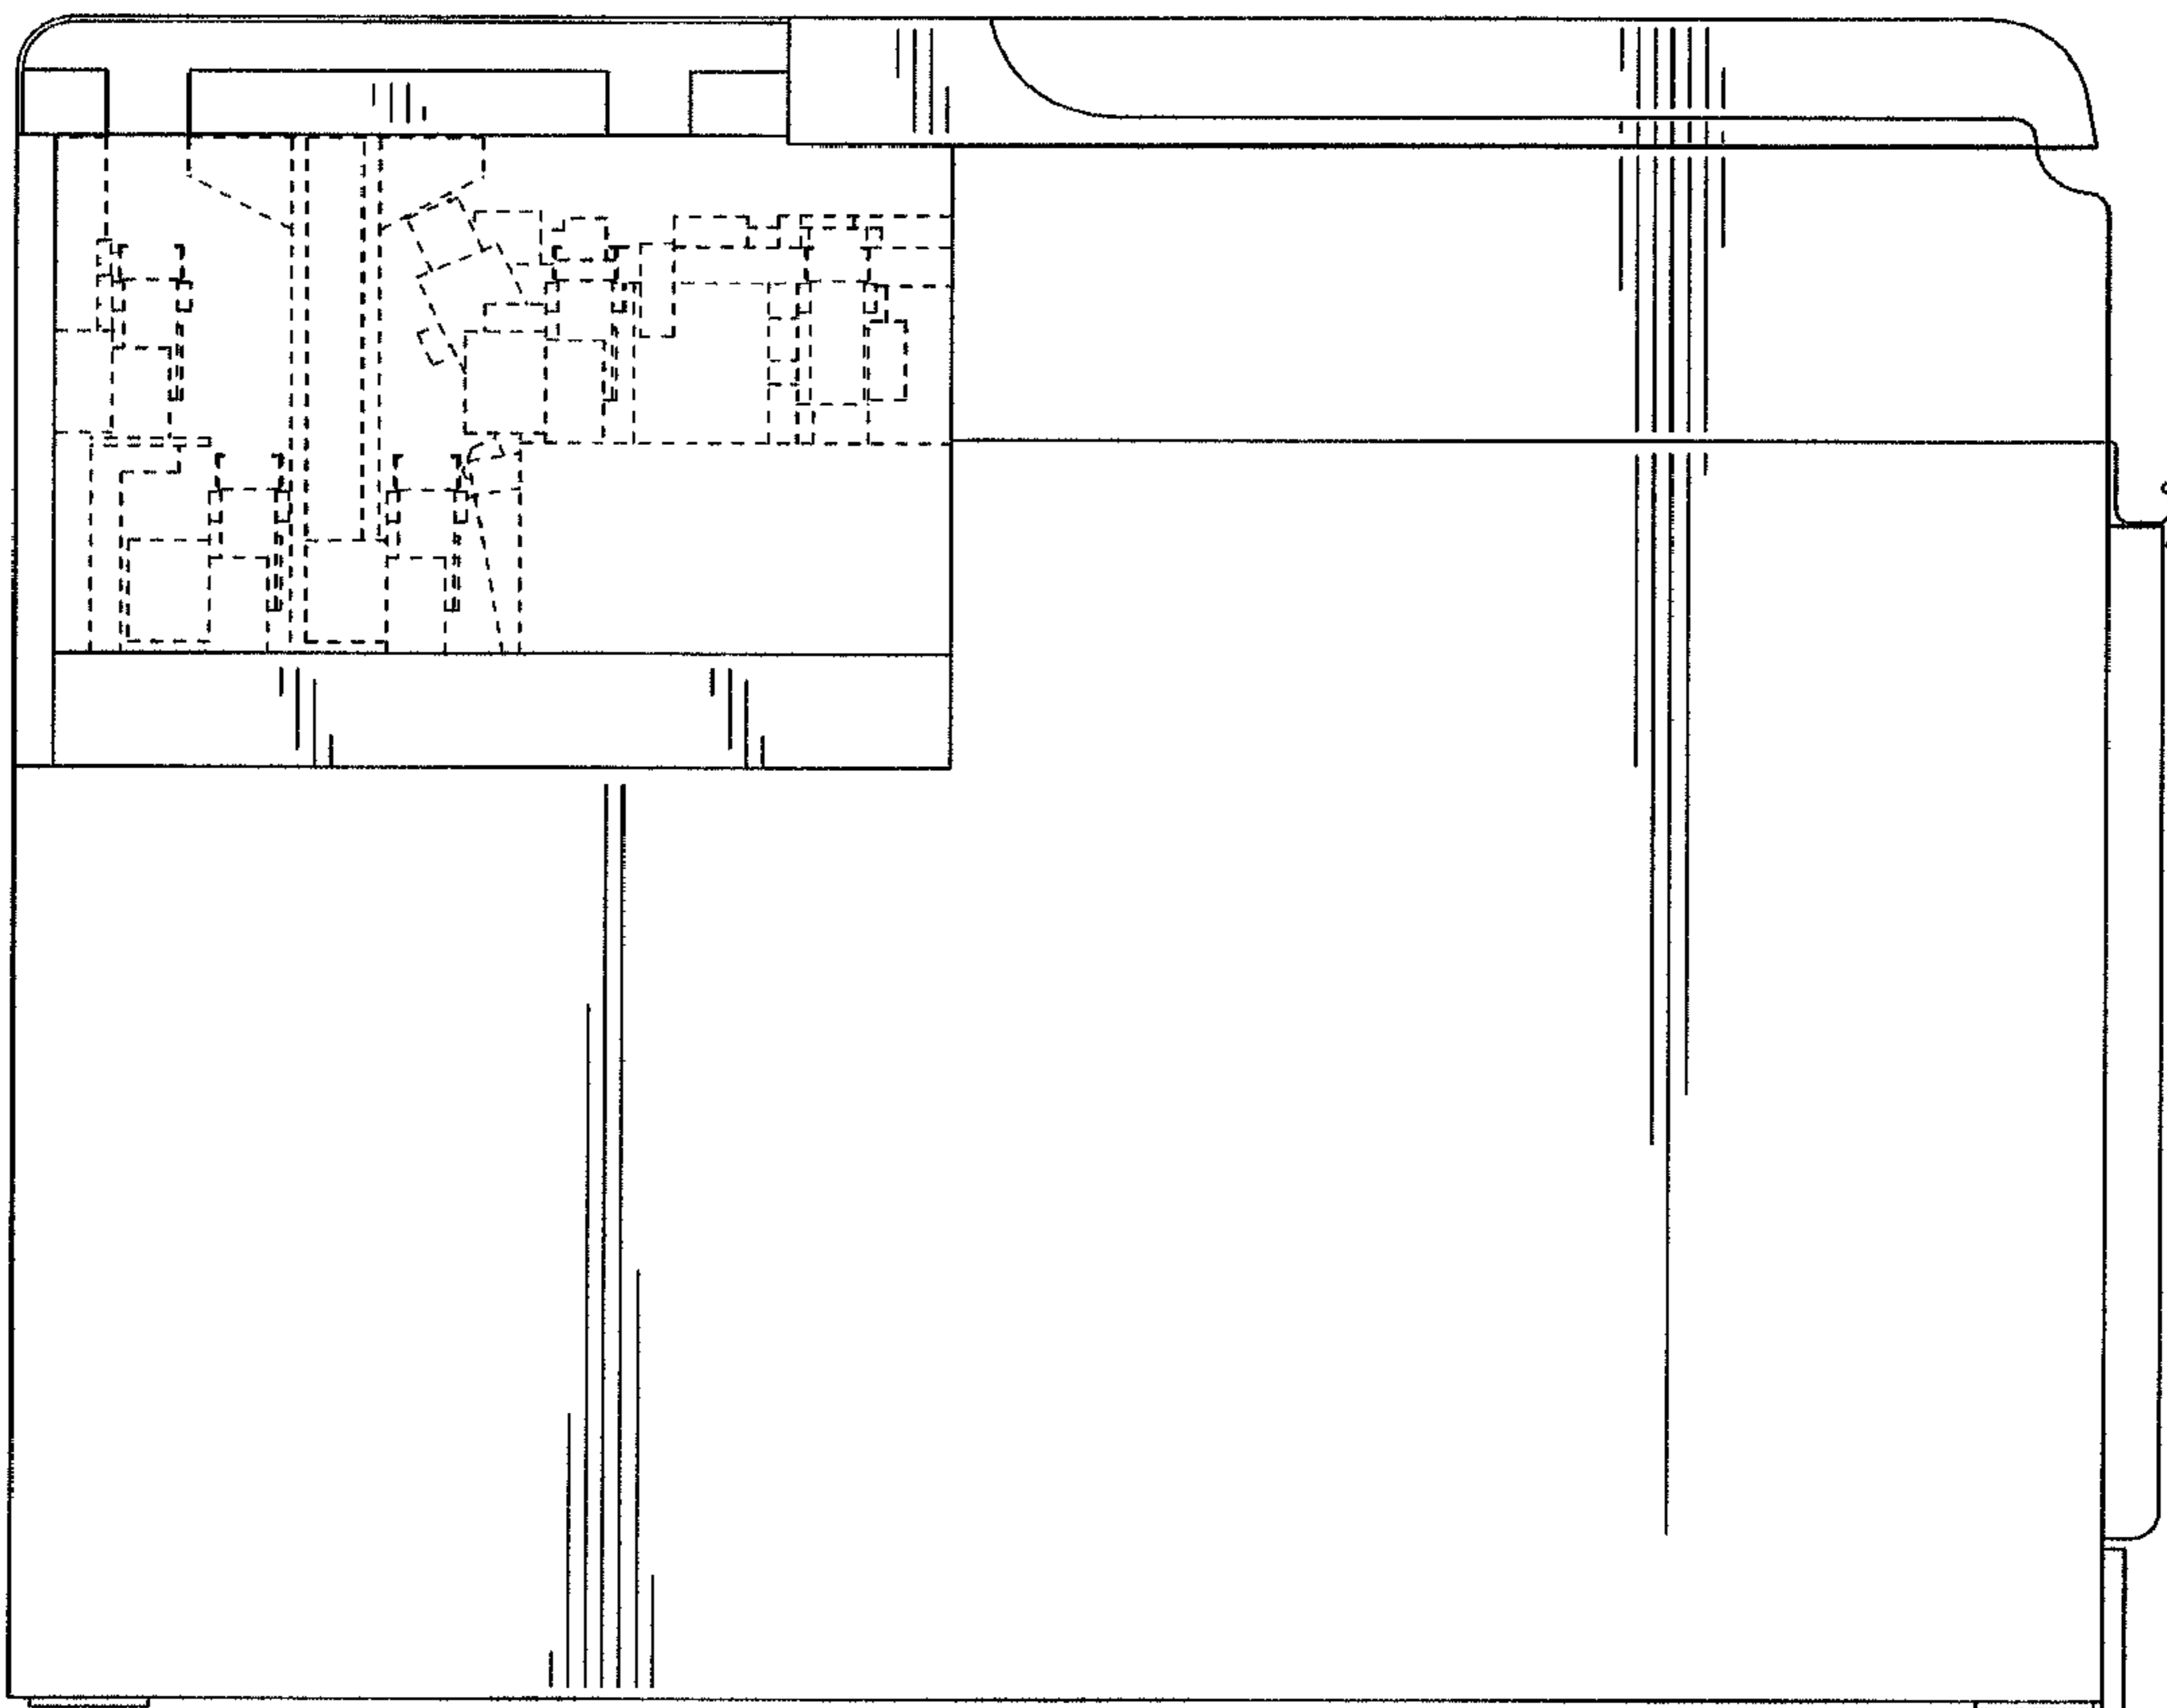


FIG. 6

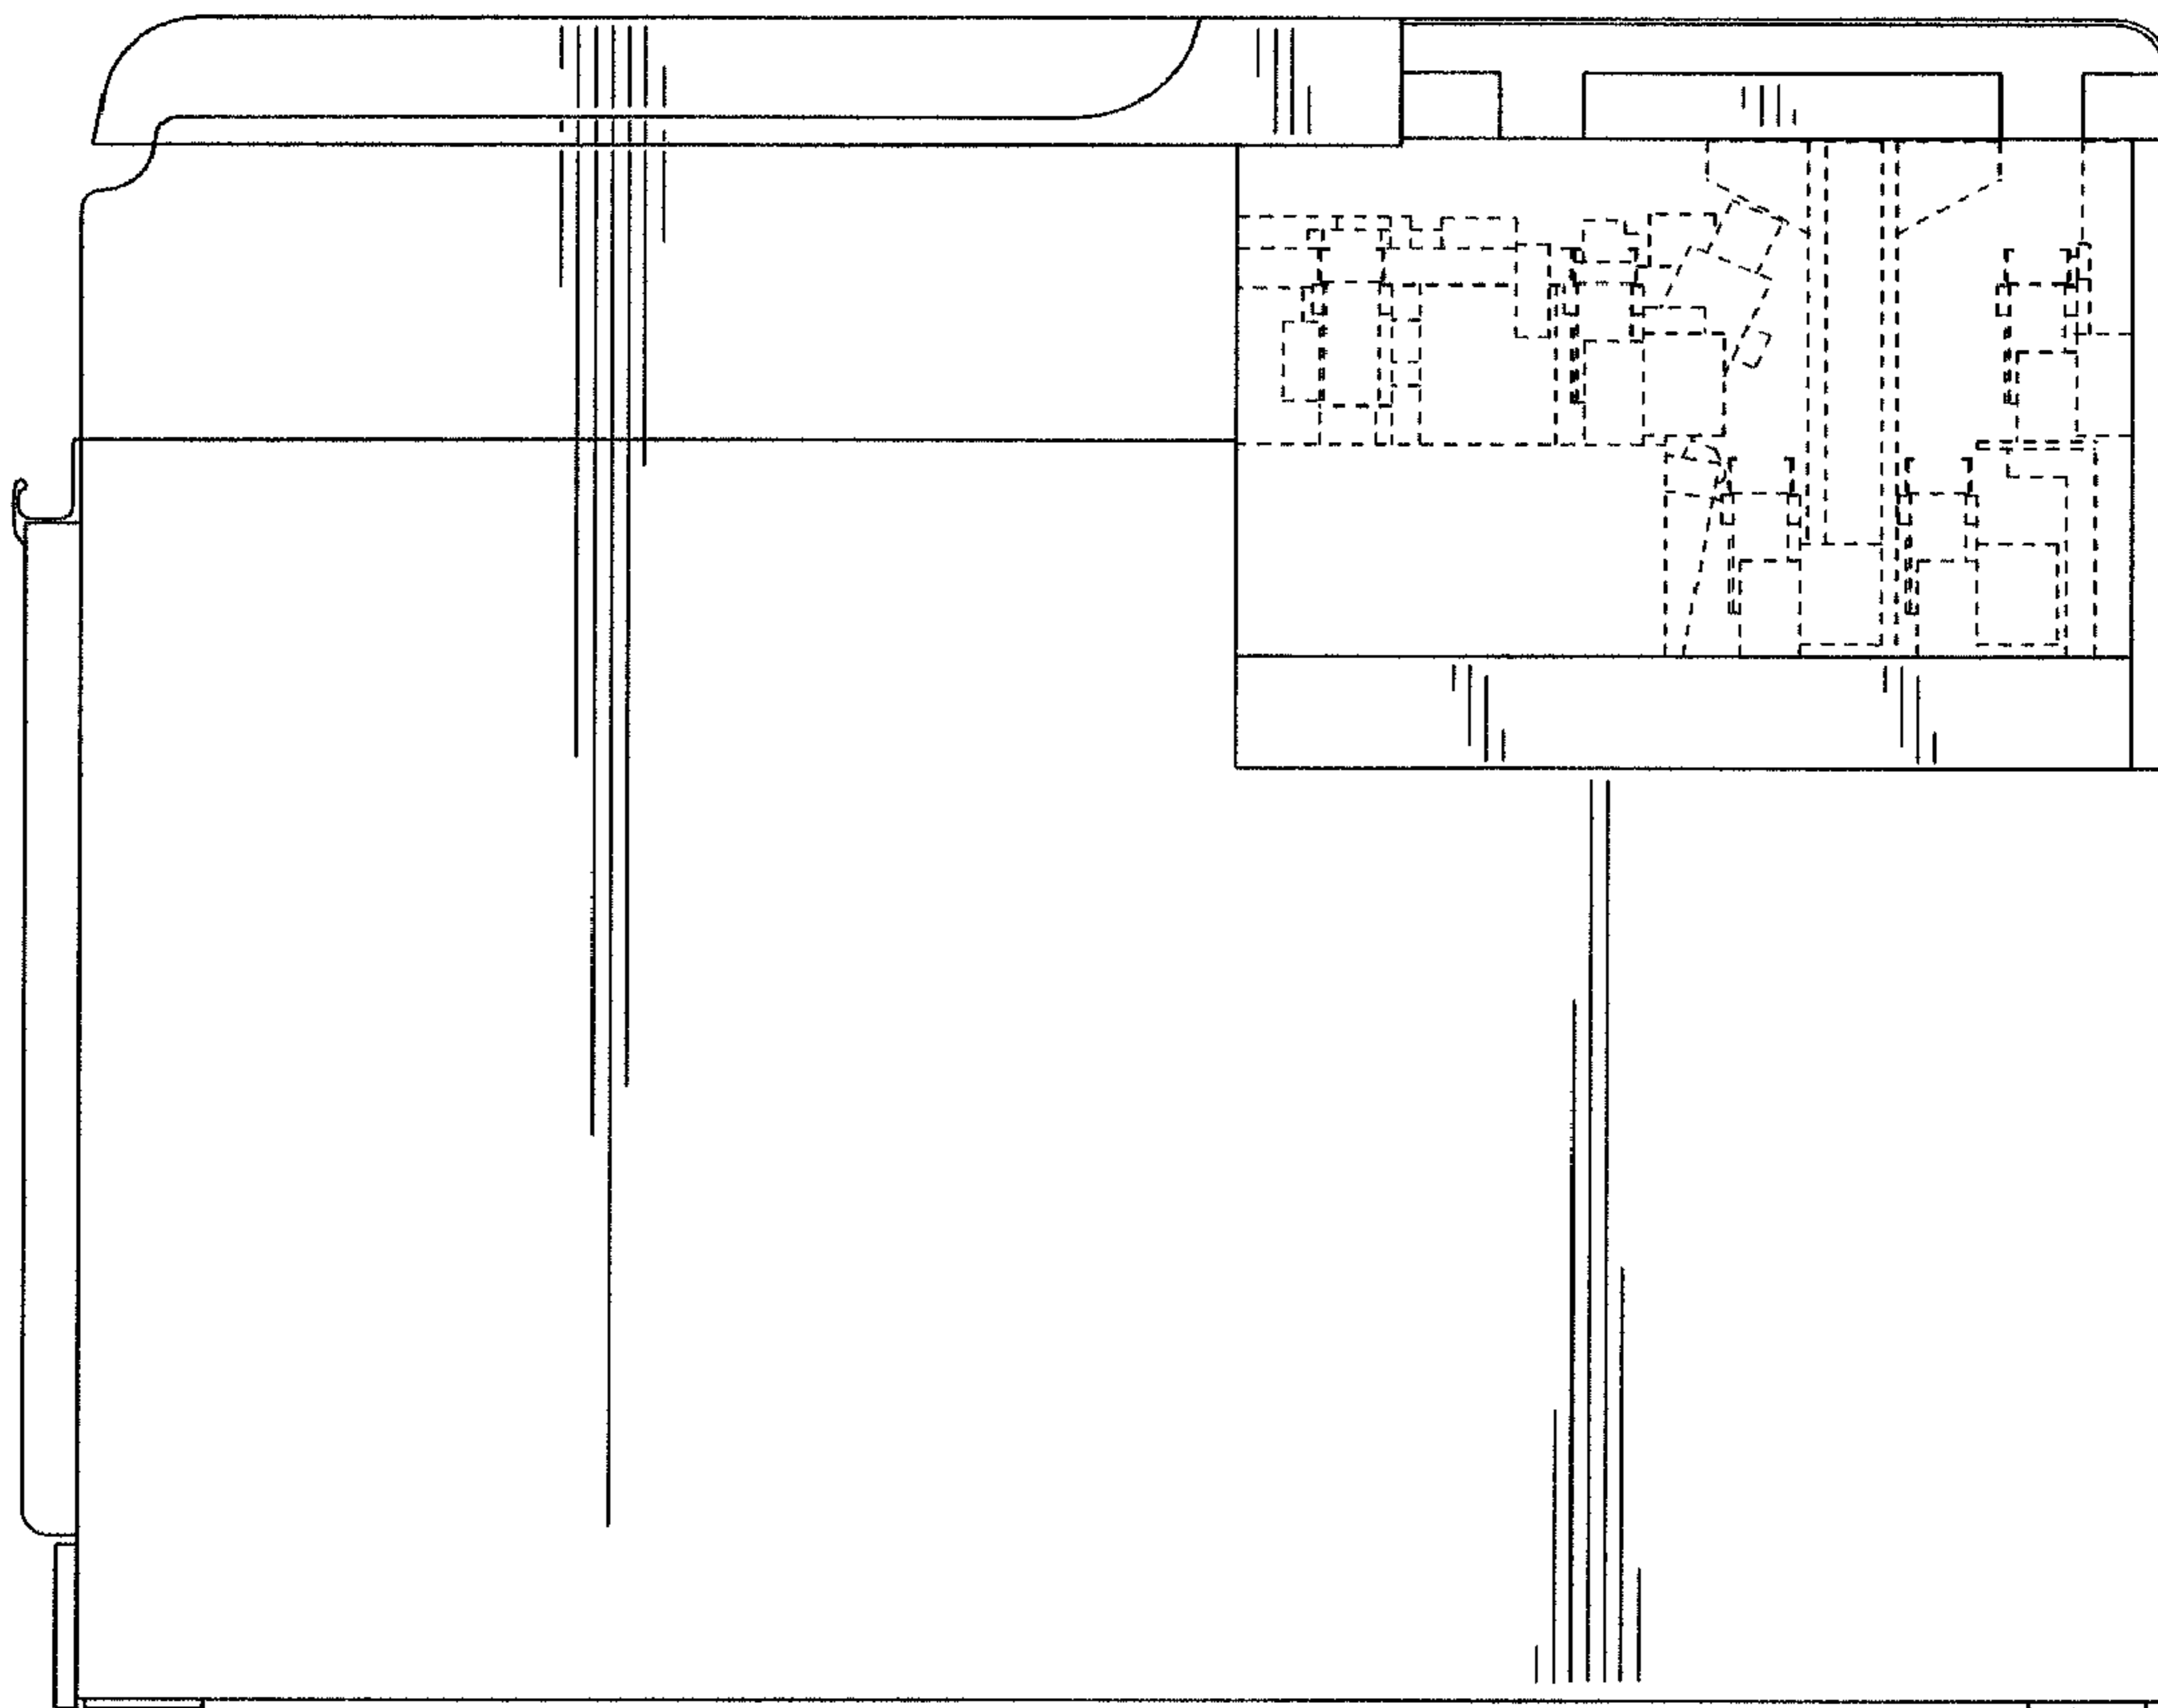


FIG. 7

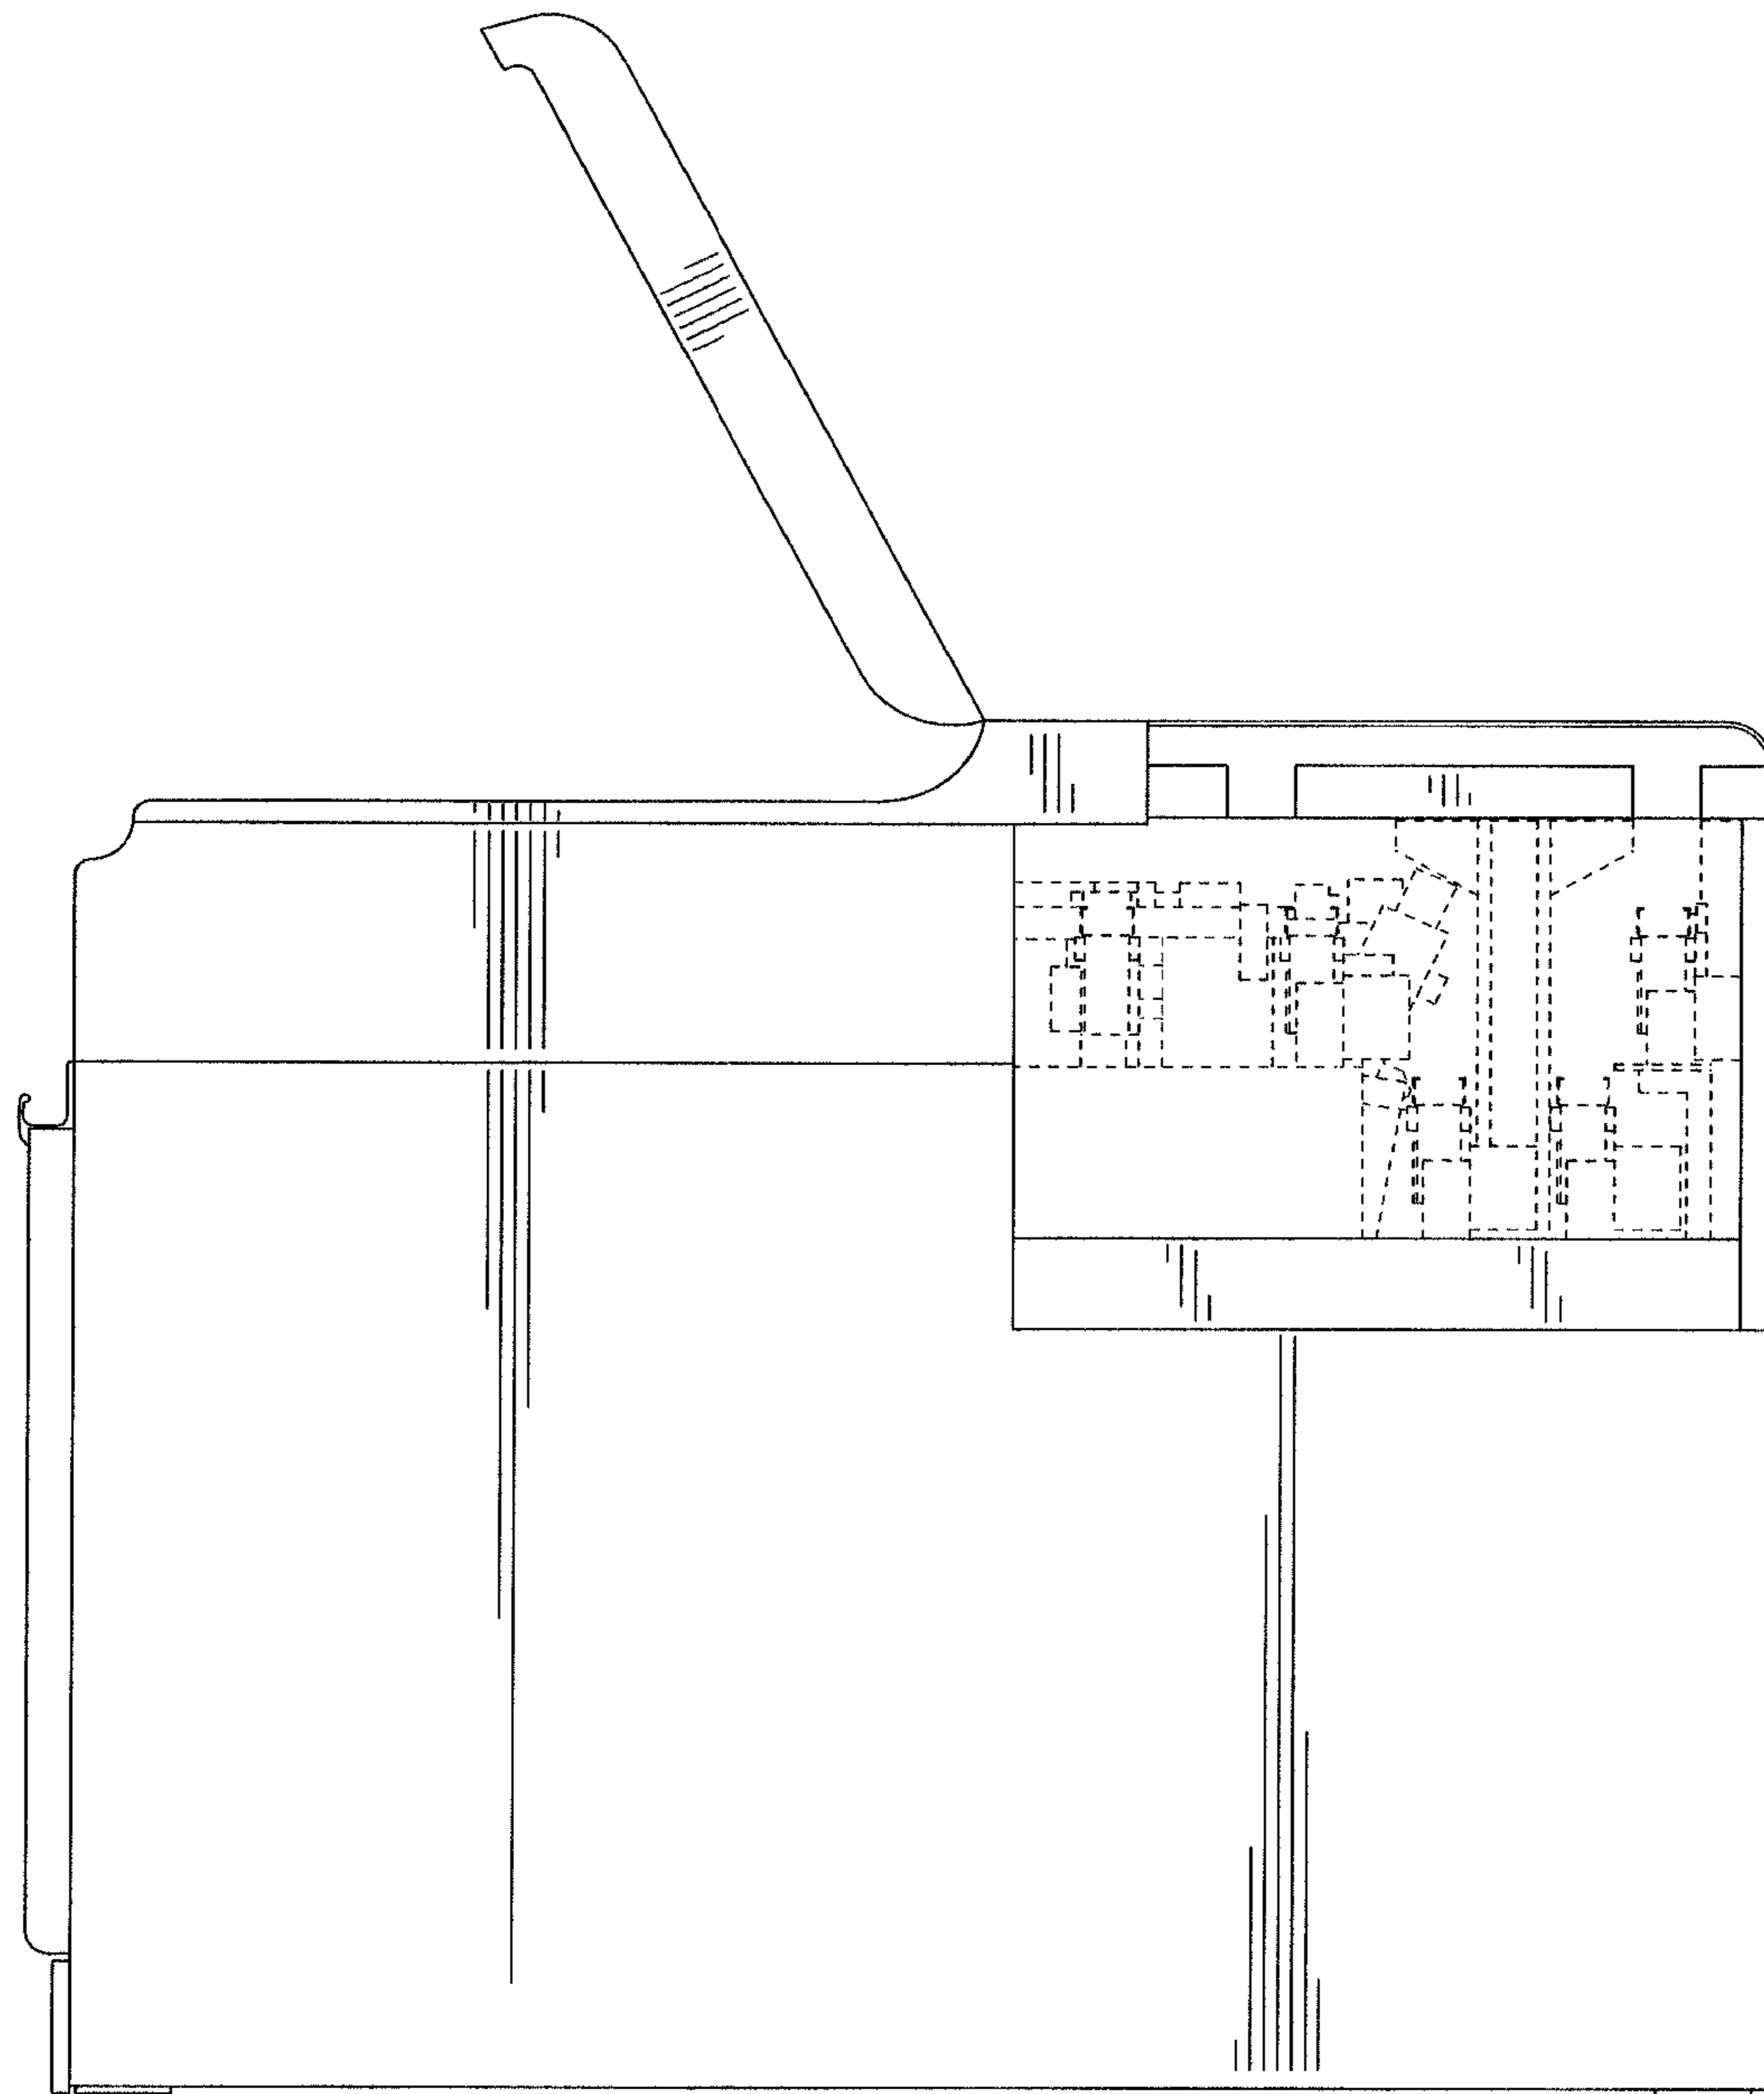


FIG. 8