

US00D659840S

(12) **United States Design Patent**
Cheng et al.

(10) **Patent No.:** **US D659,840 S**
(45) **Date of Patent:** **** May 15, 2012**

(54) **DIGITAL DIAGNOSTIC DEVICE**

(75) Inventors: **Chu-Ming Cheng**, Hsinchu (TW);
Che-Jung Kuo, Hsinchu (TW);
Chih-Lu Hsu, Hsinchu (TW);
Long-Sheng Liao, Hsinchu (TW);
Yu-Tsung Lee, Hsinchu (TW);
Jung-Sung Cheng, Hsinchu (TW);
Yi-Wen Chen, Hsinchu (TW);
Ming-Hsien Hsieh, Hsinchu (TW);
Zhan-Sheng Lin, Hsinchu (TW);
Chang-Lin Hu, Hsinchu (TW); **Shan-Yi Yang**, Hsinchu (TW)

| | | | | |
|-----------|------|---------|---------------------|---------|
| 5,373,317 | A * | 12/1994 | Salvati et al. | 348/65 |
| D358,471 | S * | 5/1995 | Cope et al. | D24/138 |
| 7,029,439 | B2 * | 4/2006 | Roberts et al. | 600/199 |
| D533,939 | S * | 12/2006 | Root et al. | D24/133 |
| 7,214,183 | B2 * | 5/2007 | Miyake | 600/131 |
| D594,555 | S * | 6/2009 | Hsu | D24/137 |
| D618,346 | S * | 6/2010 | Sisko et al. | D24/137 |
| D618,794 | S * | 6/2010 | Onuma | D24/137 |
| D619,708 | S * | 7/2010 | Ellman | D24/150 |
| D635,256 | S * | 3/2011 | Huang | D24/151 |
| D635,257 | S * | 3/2011 | Ellman | D24/137 |
| D636,080 | S * | 4/2011 | Goldberg | D24/137 |
| D637,715 | S * | 5/2011 | Clarke et al. | D24/137 |
| D637,717 | S * | 5/2011 | Clarke et al. | D24/137 |

* cited by examiner

(73) Assignee: **Medimaging Integrated Solution, Inc.**,
Hsinchu (TW)

Primary Examiner — T. Chase Nelson
Assistant Examiner — Mark Cavanna

(**) Term: **14 Years**

(74) *Attorney, Agent, or Firm* — Muncy, Geissler, Olds & Lowe, PLLC

(21) Appl. No.: **29/401,879**

(22) Filed: **Sep. 16, 2011**

(51) **LOC (9) Cl.** **24-01**

(52) **U.S. Cl.** **D24/186; D24/137**

(58) **Field of Classification Search** D24/186,
D24/133, 135, 137, 138, 150–151; 600/131,
600/184–200; 606/191–196; 320/114; 348/65
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

| | | | | |
|-----------|-----|---------|----------------------|---------|
| D222,925 | S * | 2/1972 | Hopewell | D24/137 |
| 3,698,387 | A * | 10/1972 | Moore et al. | 600/200 |
| 4,147,163 | A * | 4/1979 | Newman et al. | 600/200 |
| D286,814 | S * | 11/1986 | Brainard et al. | D24/137 |
| D288,960 | S * | 3/1987 | Riester | D24/137 |
| D289,197 | S * | 4/1987 | Ware et al. | D24/137 |
| 5,177,424 | A * | 1/1993 | Connors | 320/114 |


(57) **CLAIM**

The ornamental design for a digital diagnostic device, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a digital diagnostic device showing our new design;
FIG. 2 is a front view thereof;
FIG. 3 is a rear view thereof;
FIG. 4 is a left side view thereof;
FIG. 5 is a right side view thereof;
FIG. 6 is a top view thereof;
FIG. 7 is a bottom view thereof;
FIG. 8 is a front left perspective view thereof;
FIG. 9 is a bottom left perspective view thereof; and,
FIG. 10 is a detail top left perspective view thereof.

1 Claim, 10 Drawing Sheets

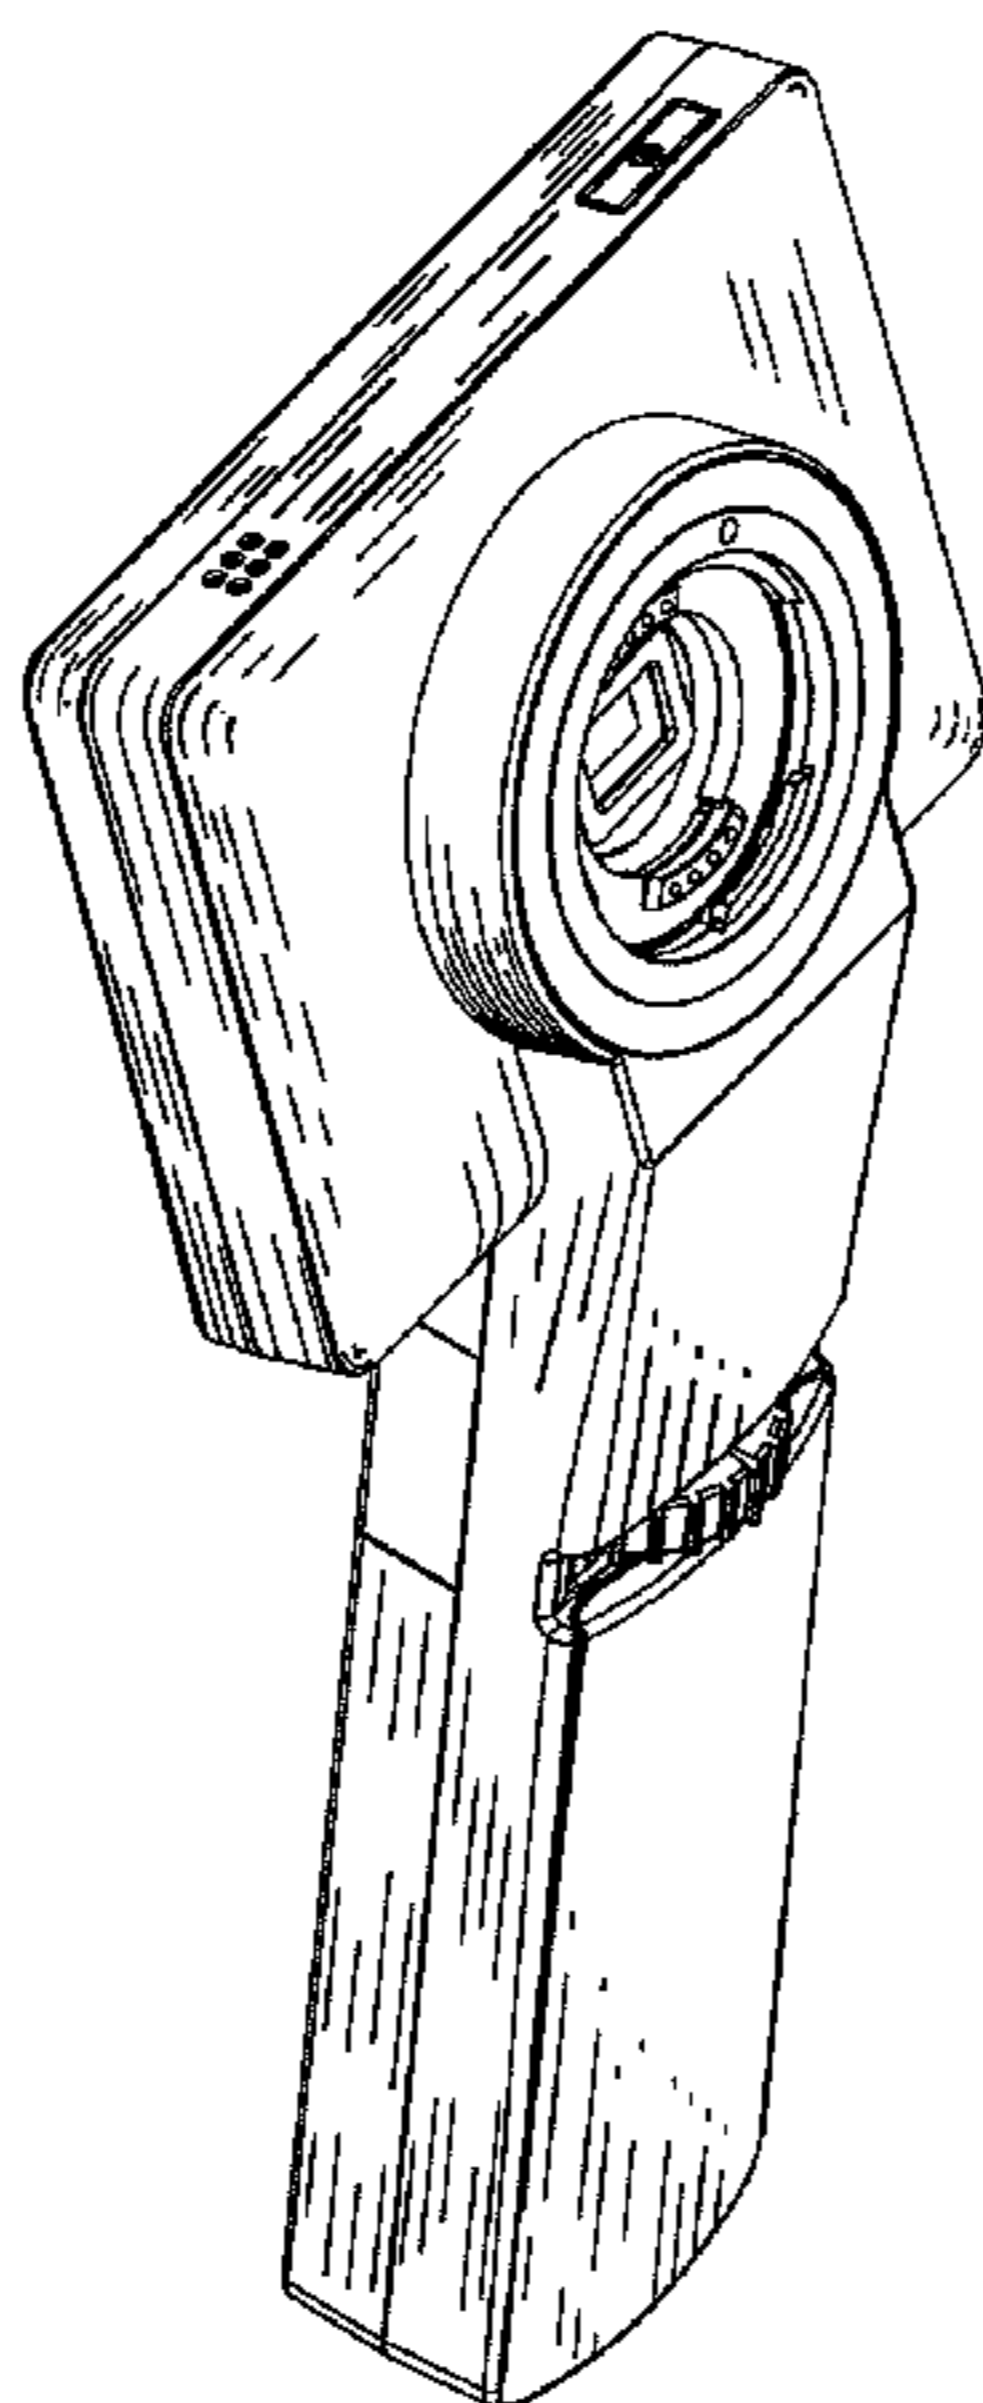

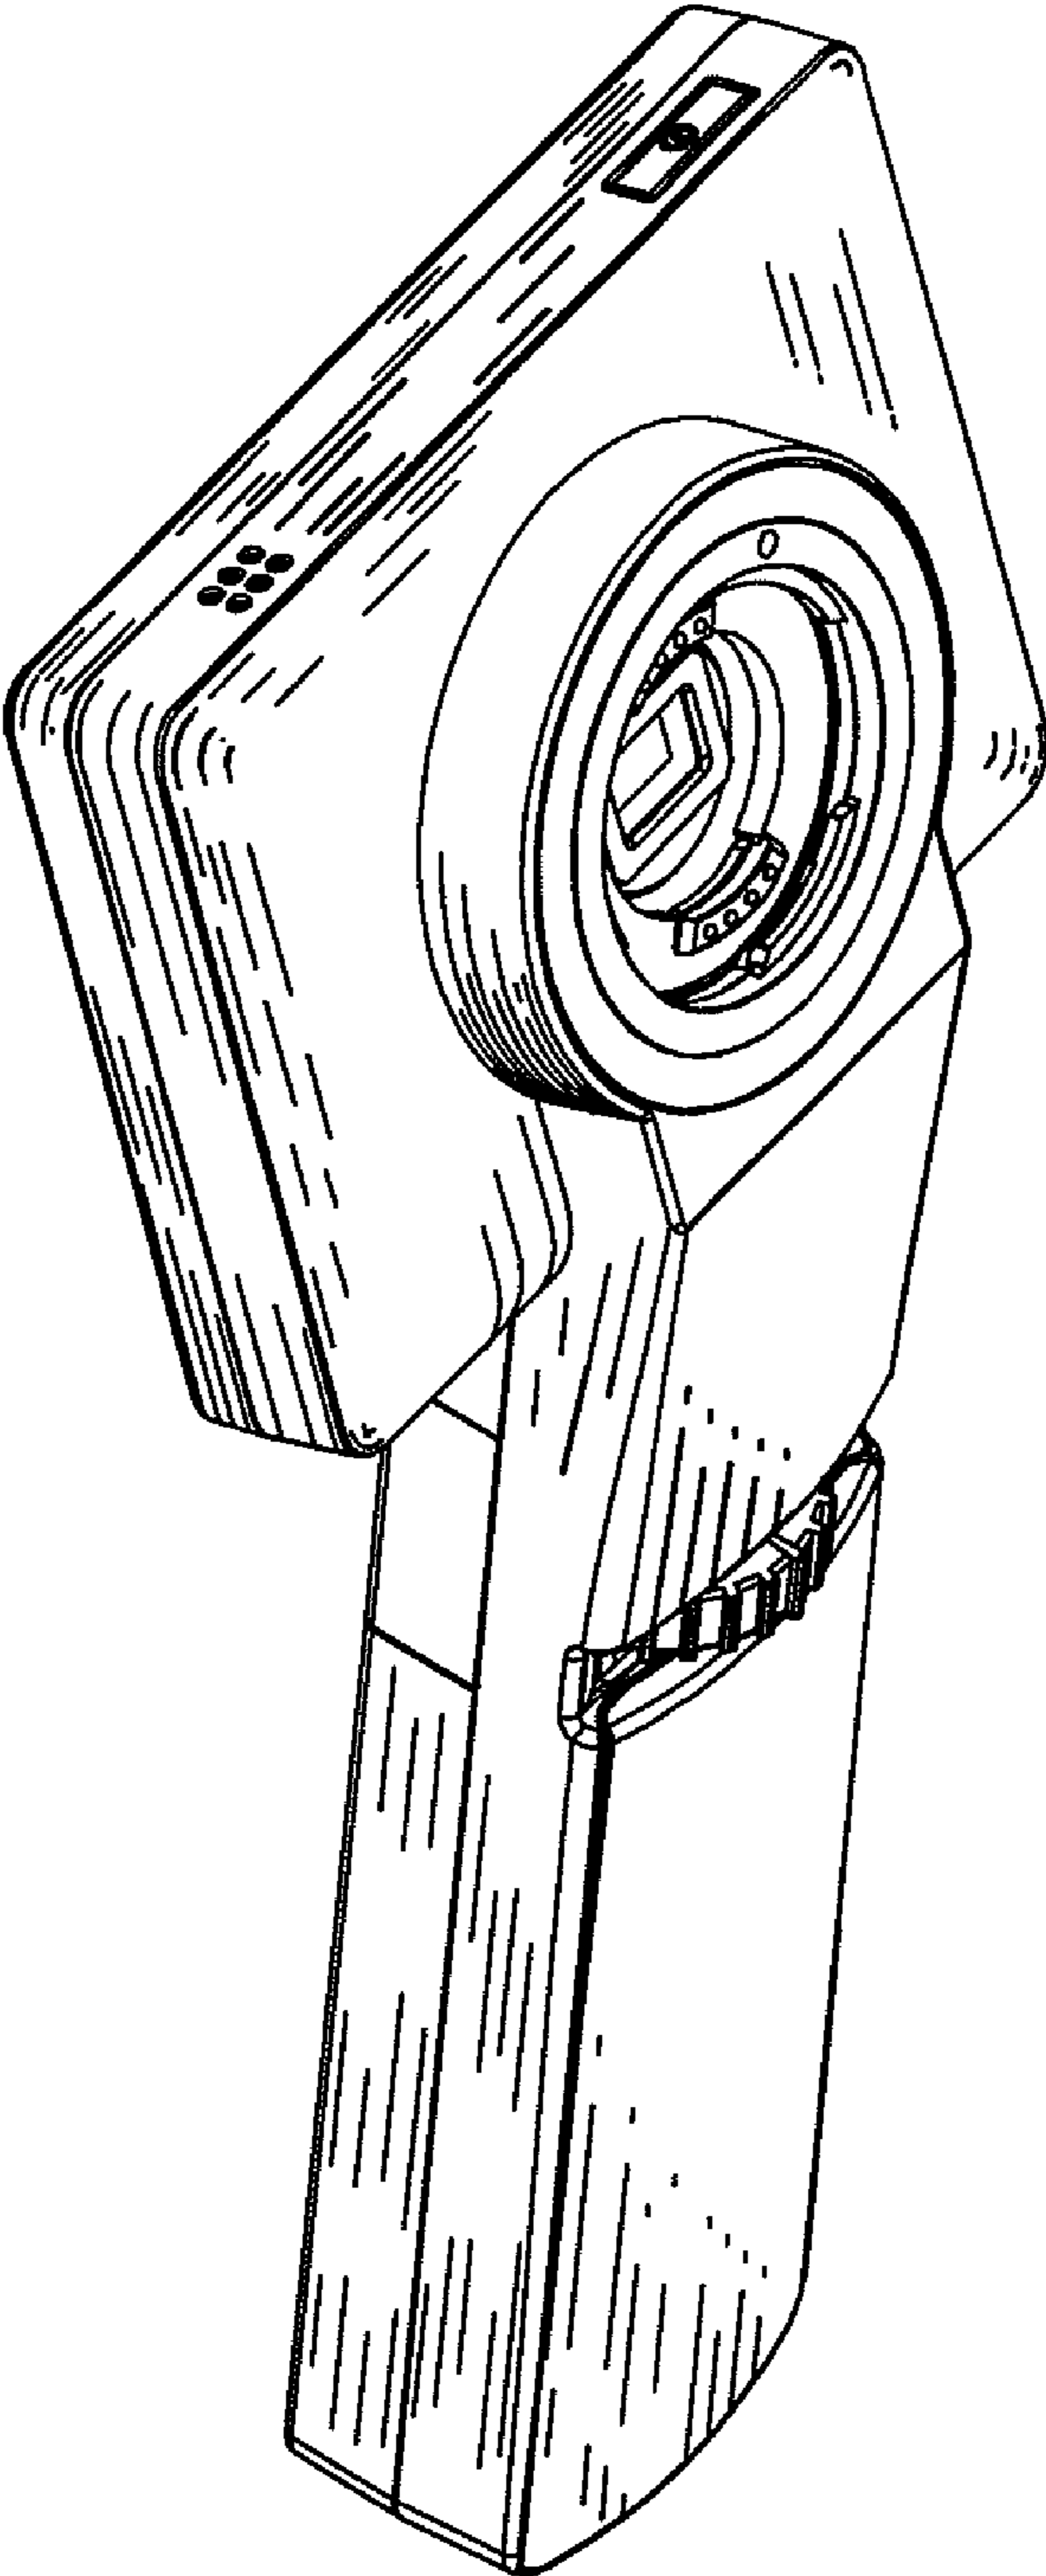


FIG.1

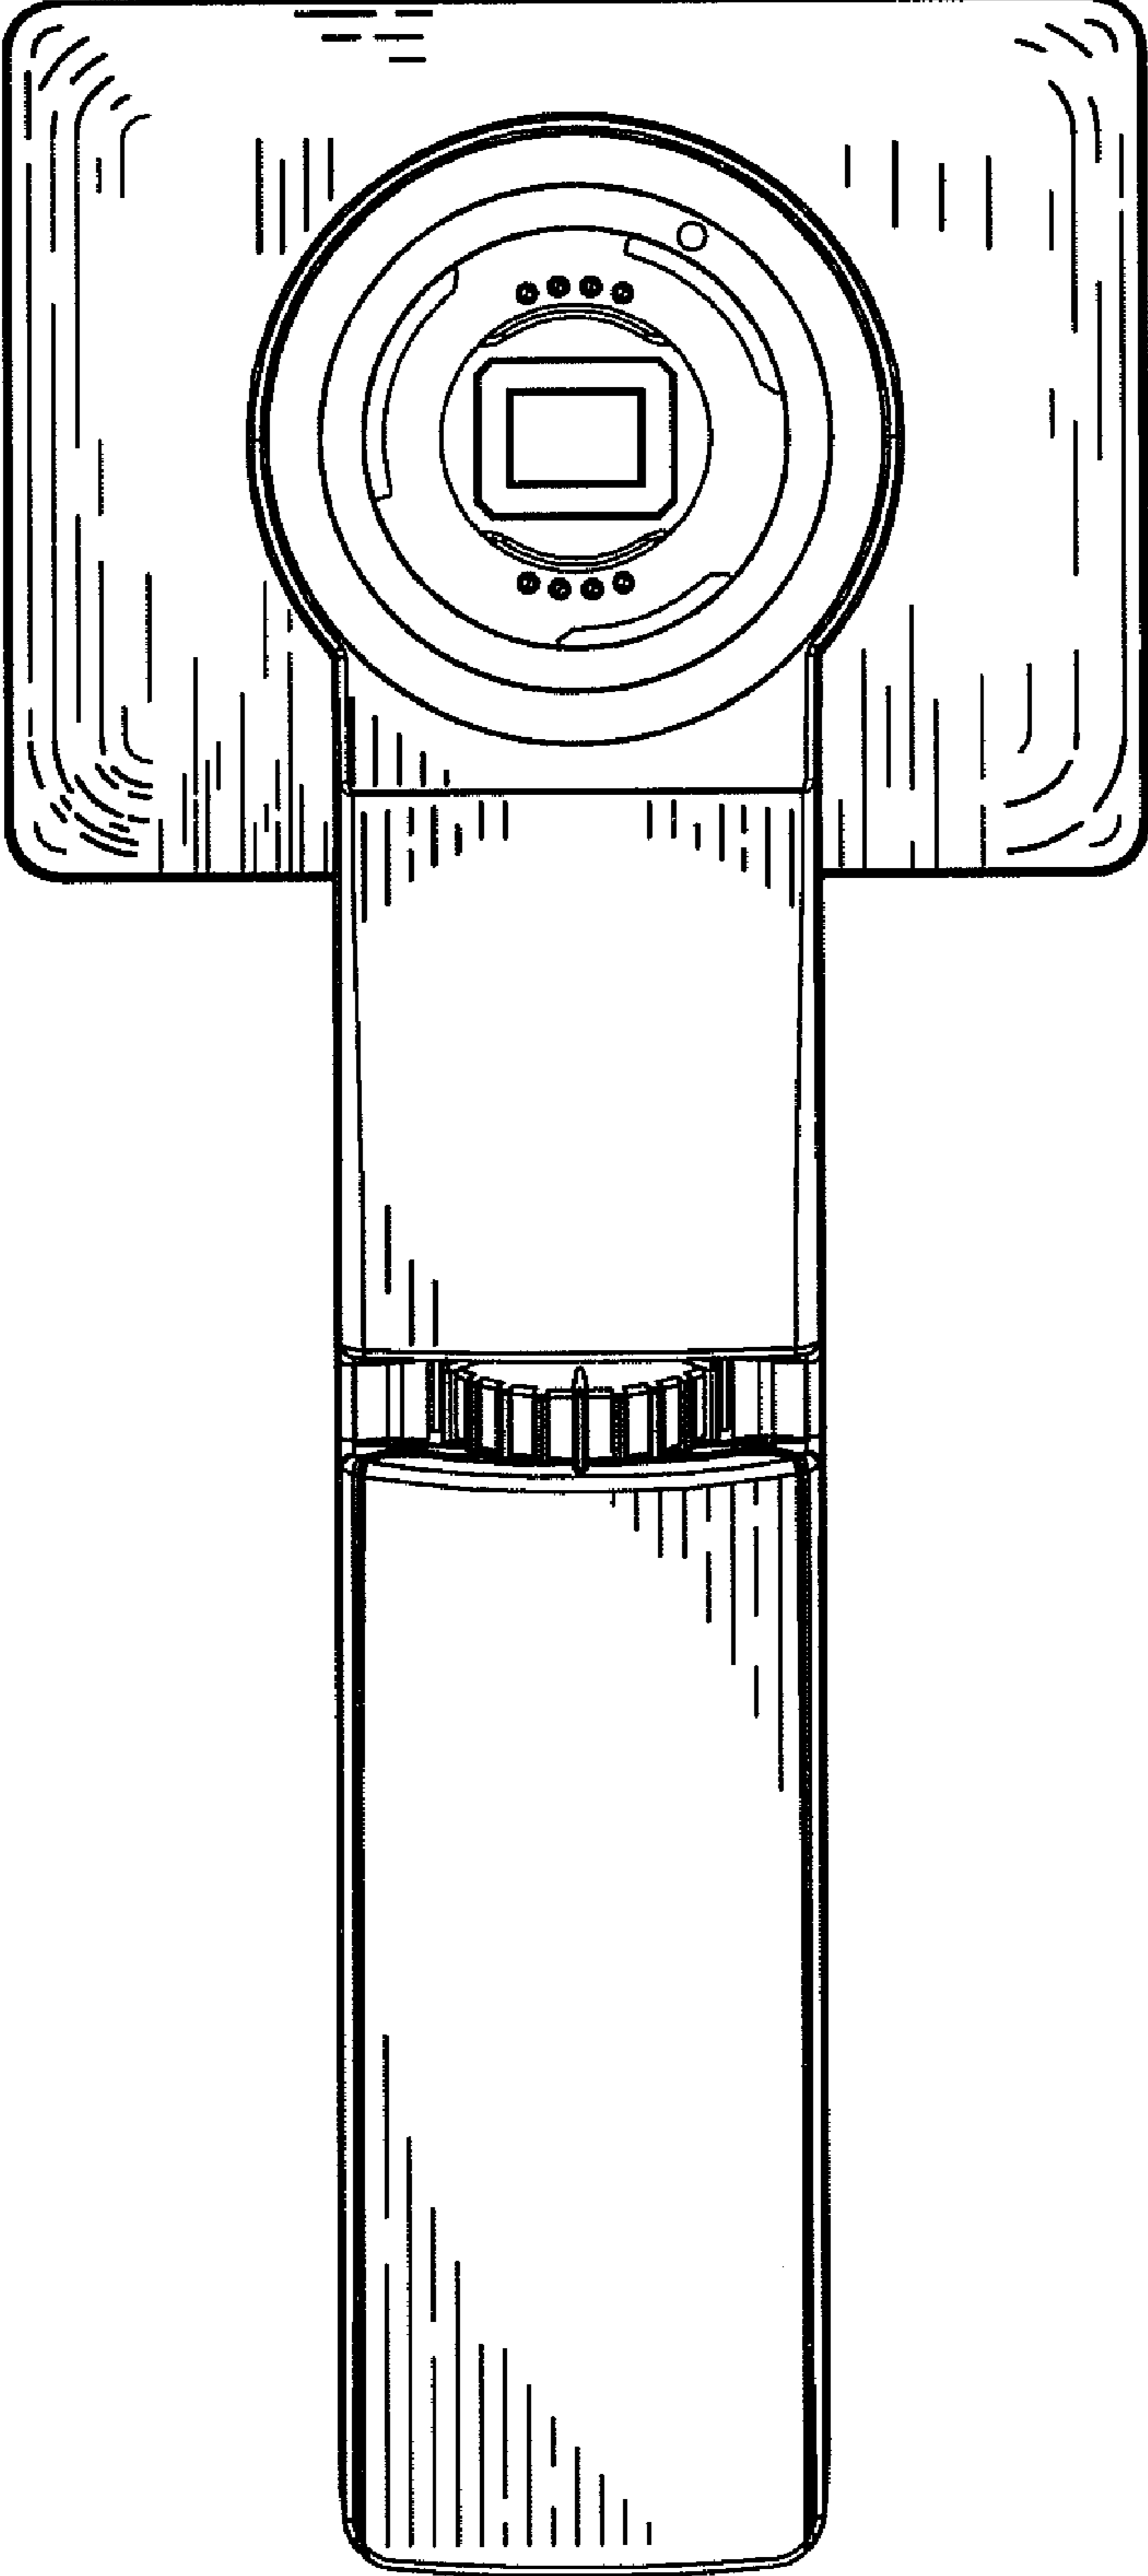


FIG.2

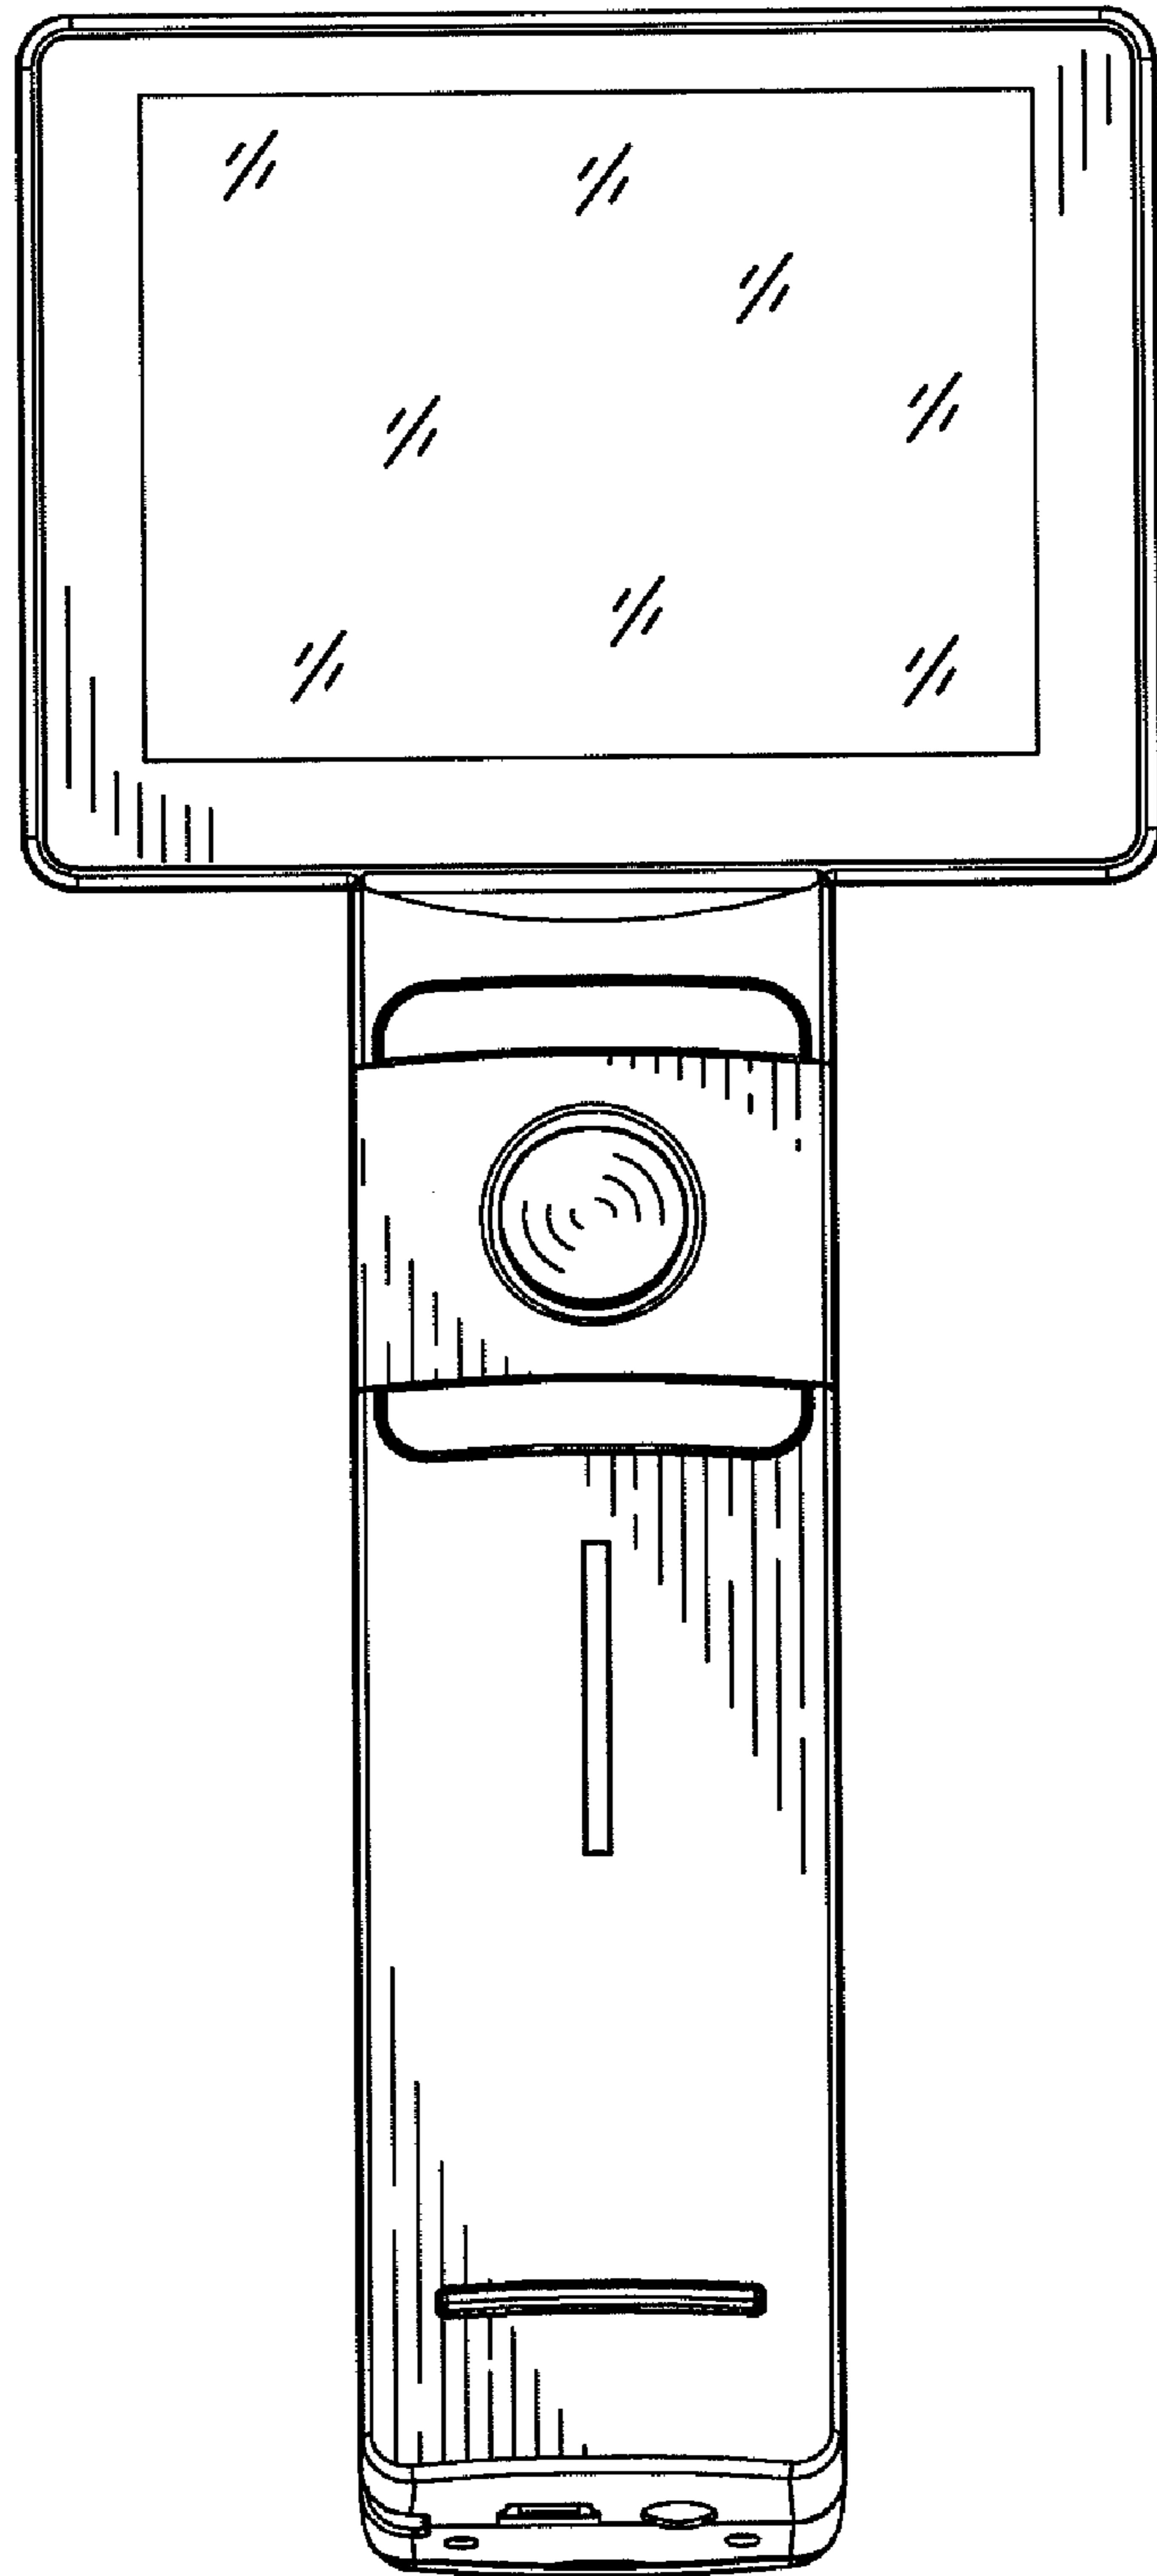


FIG.3

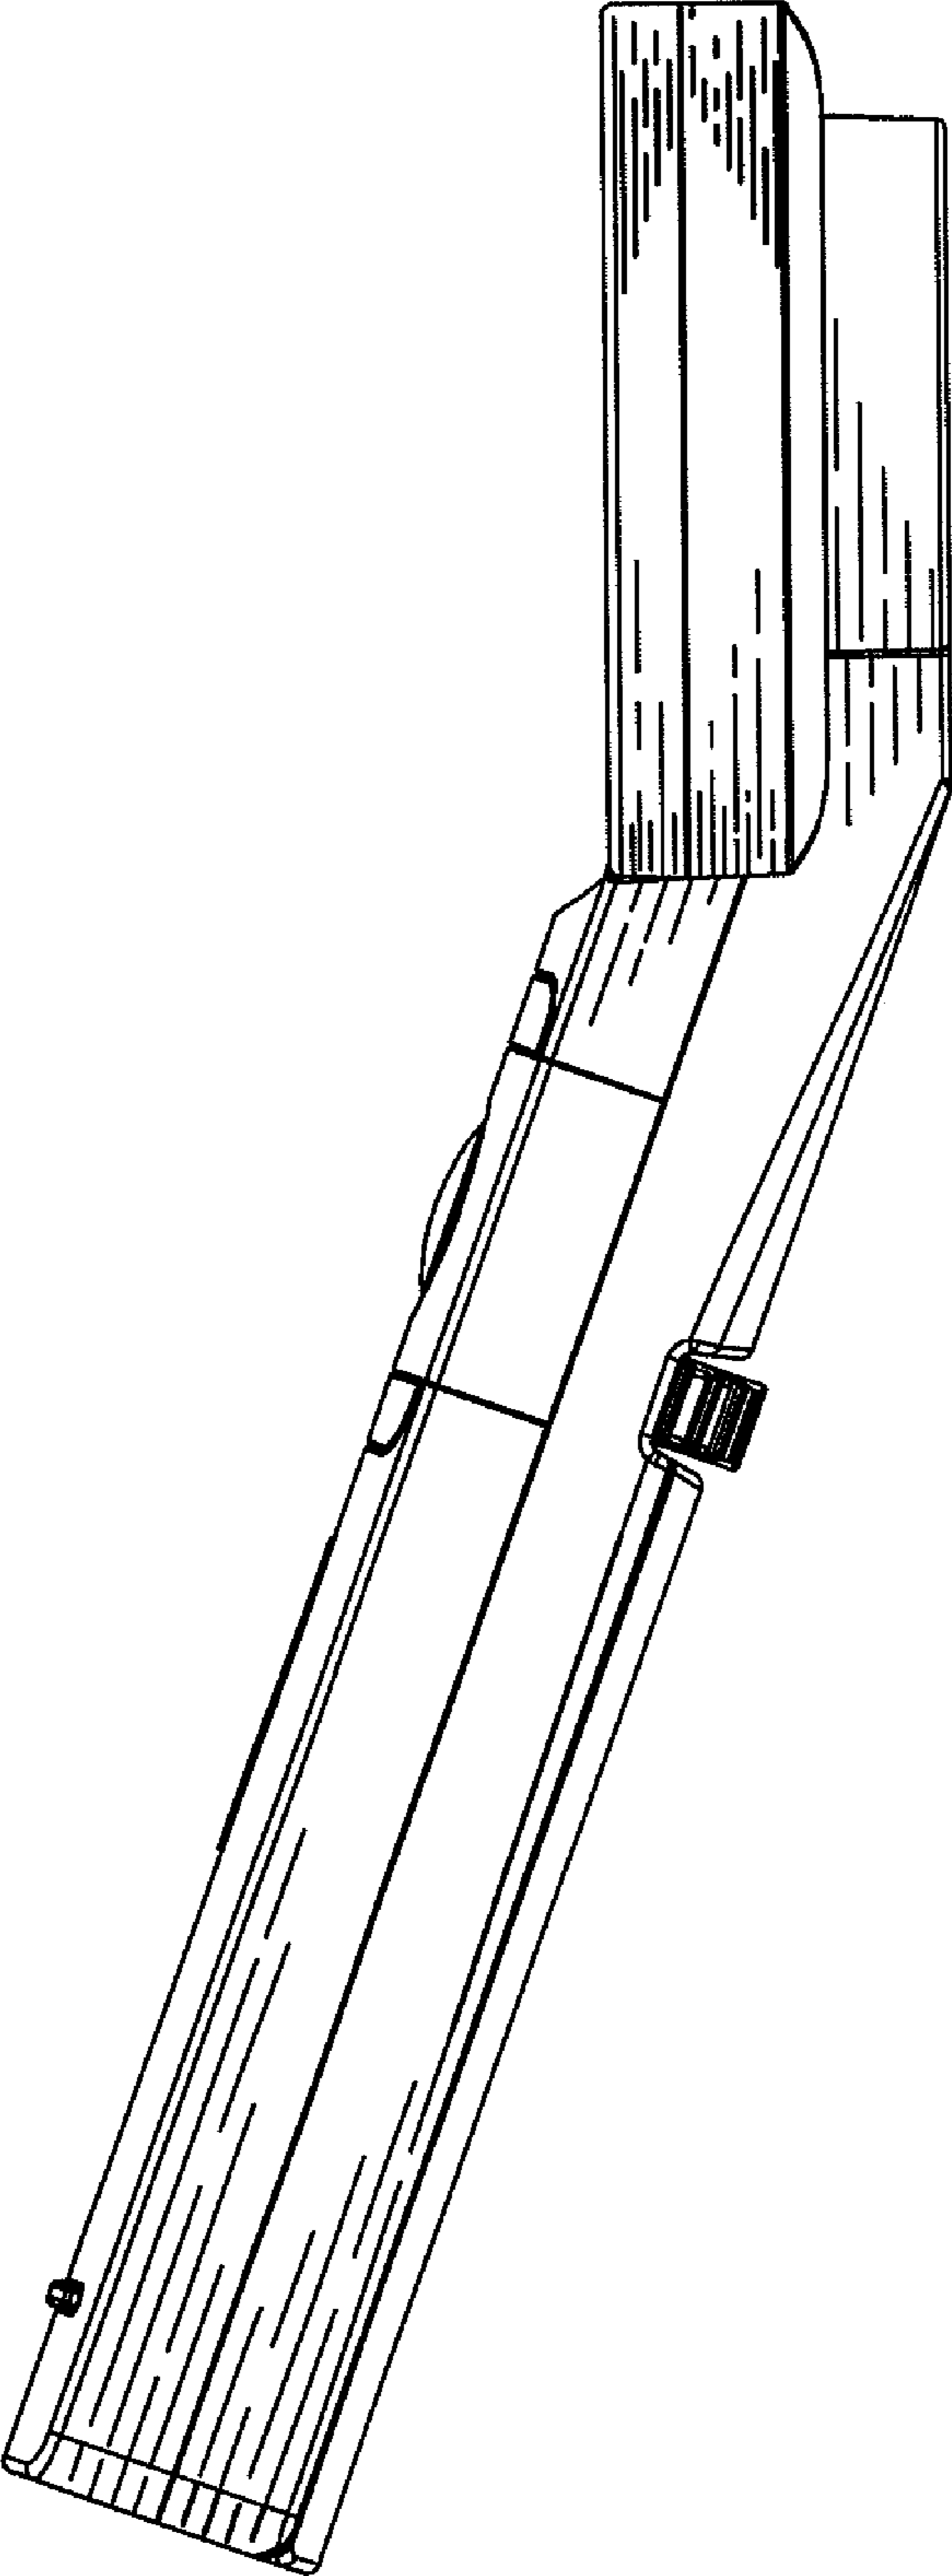


FIG.4

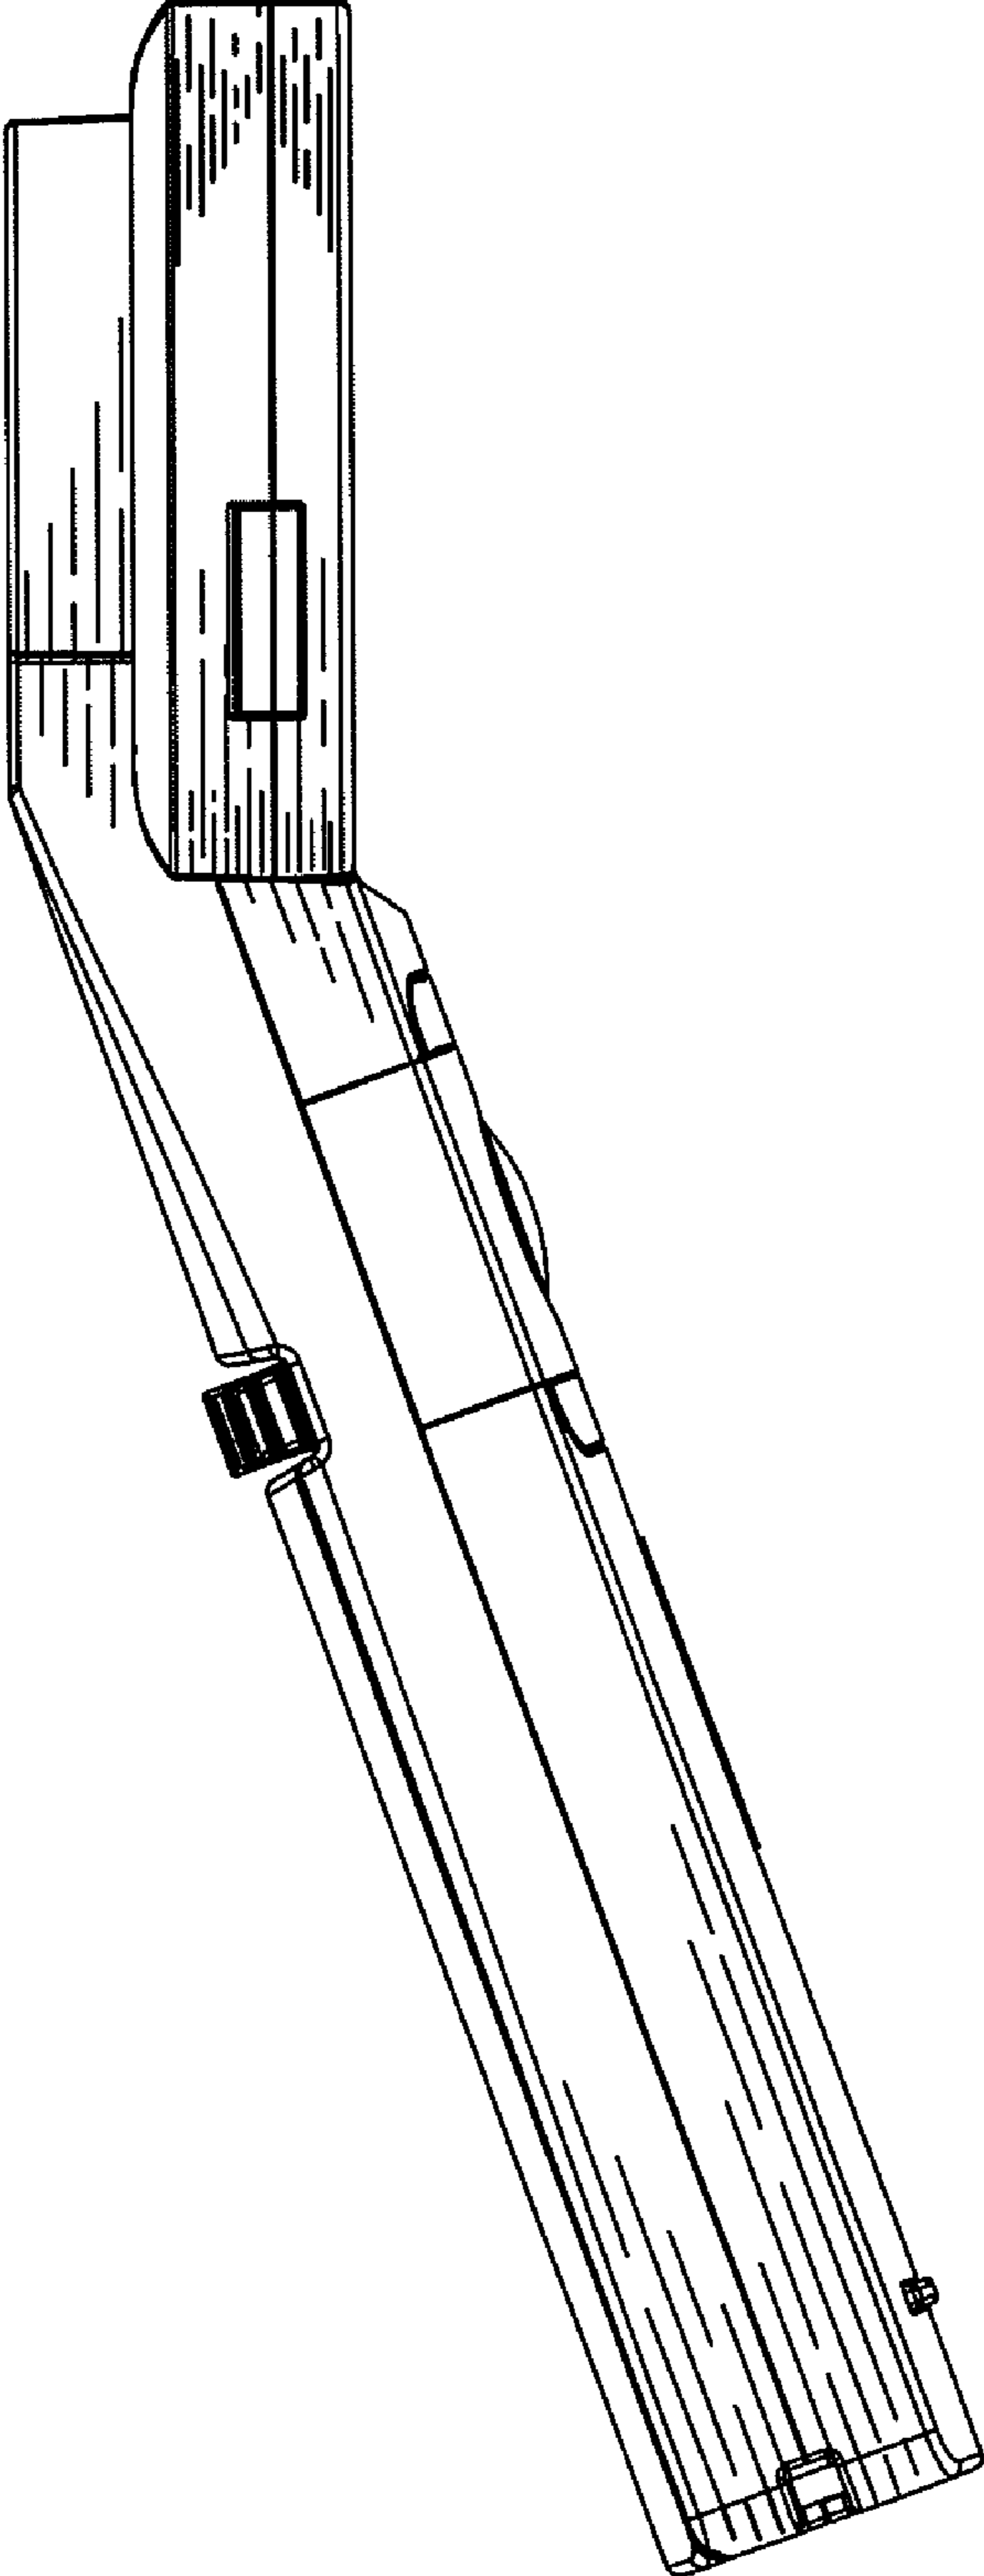


FIG.5

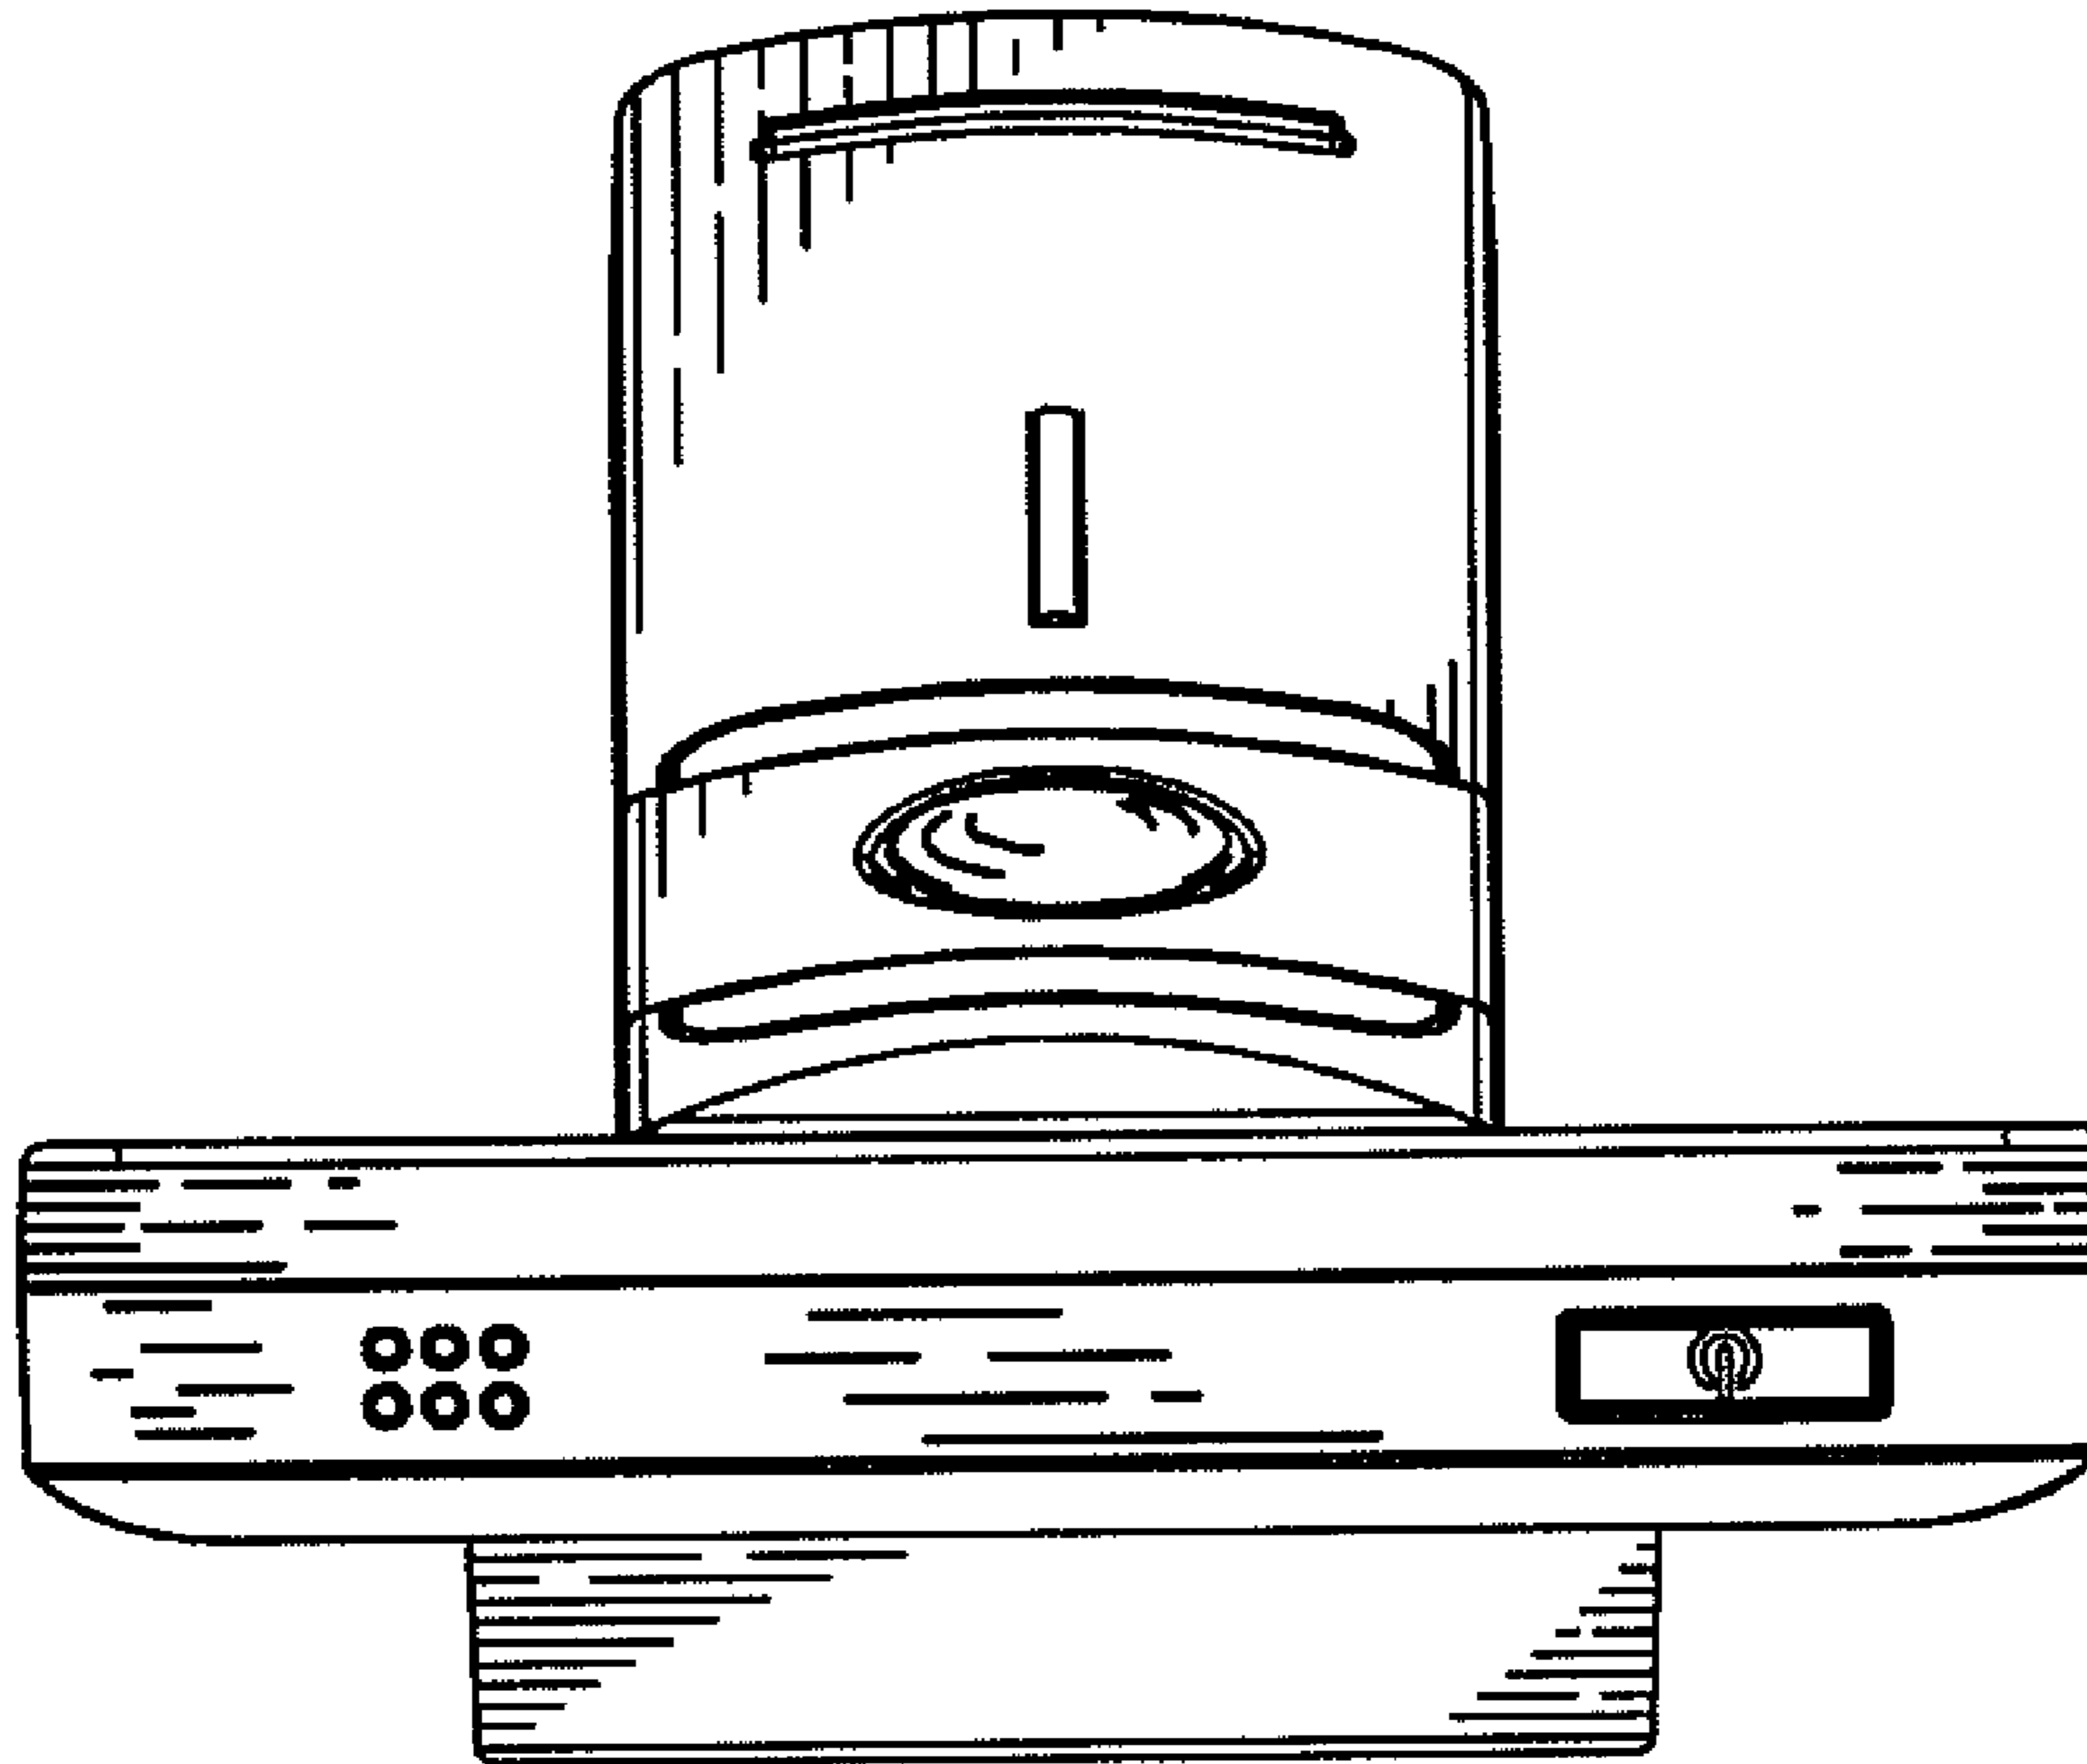


FIG.6

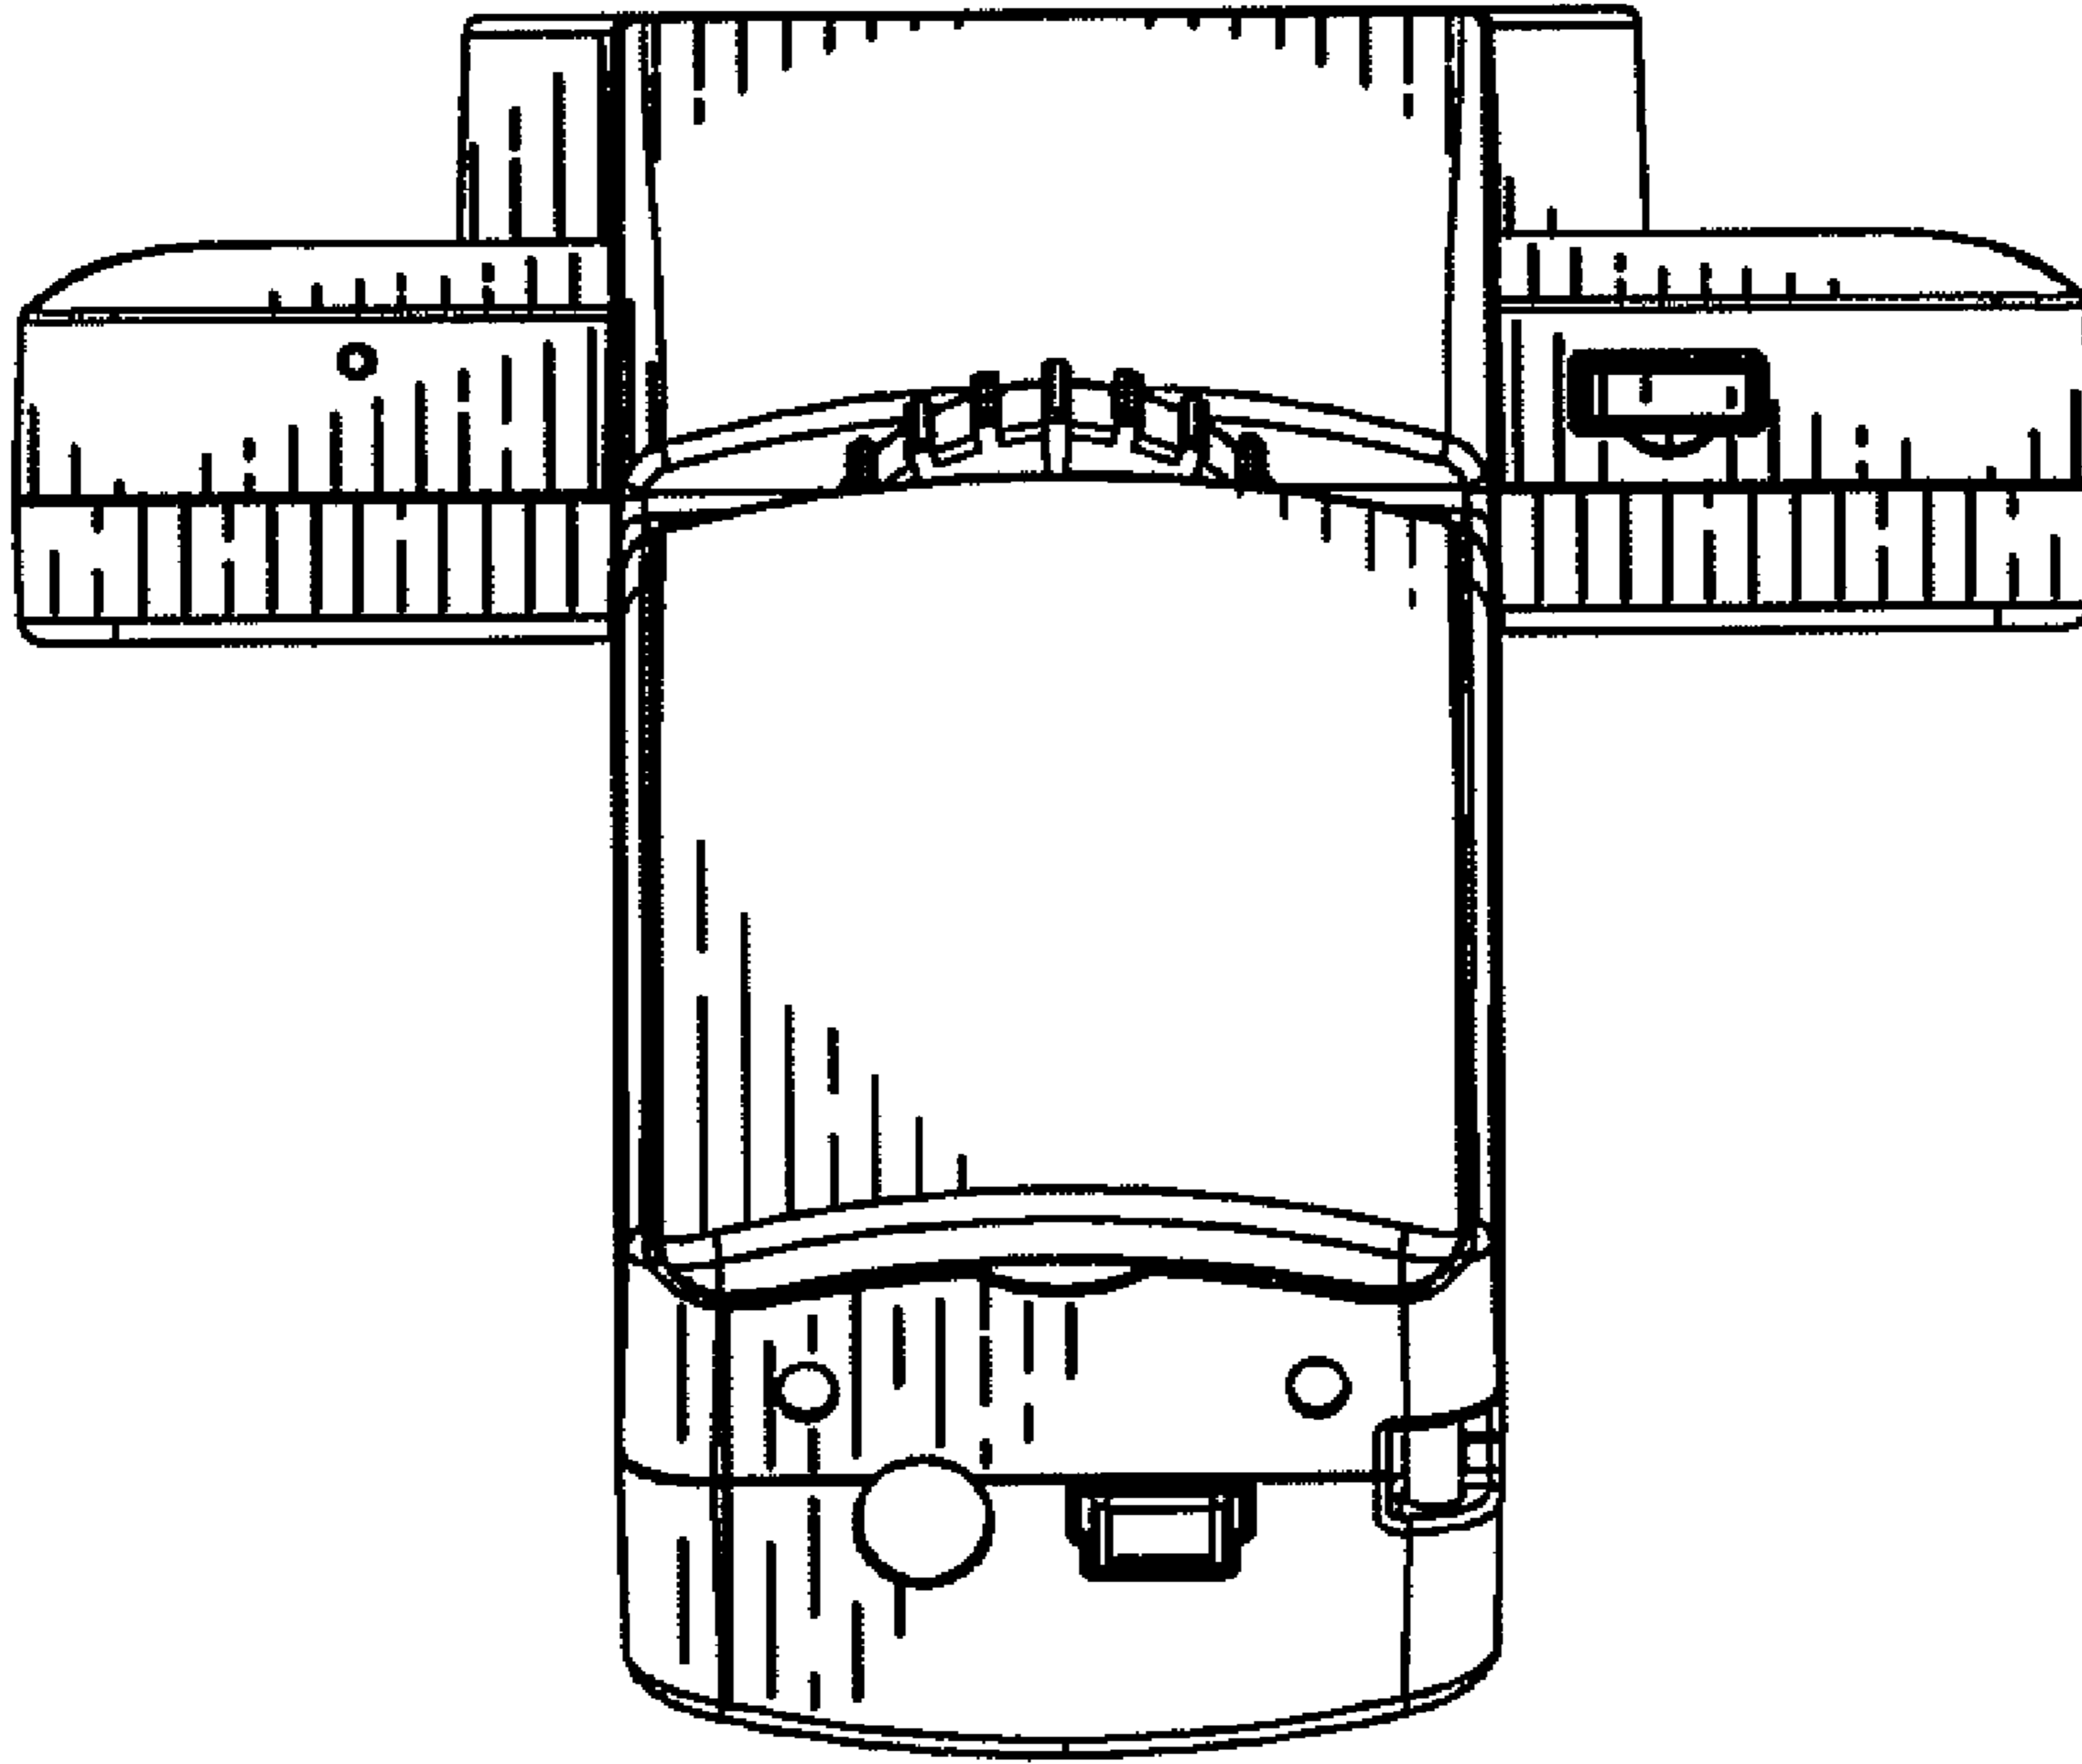


FIG.7

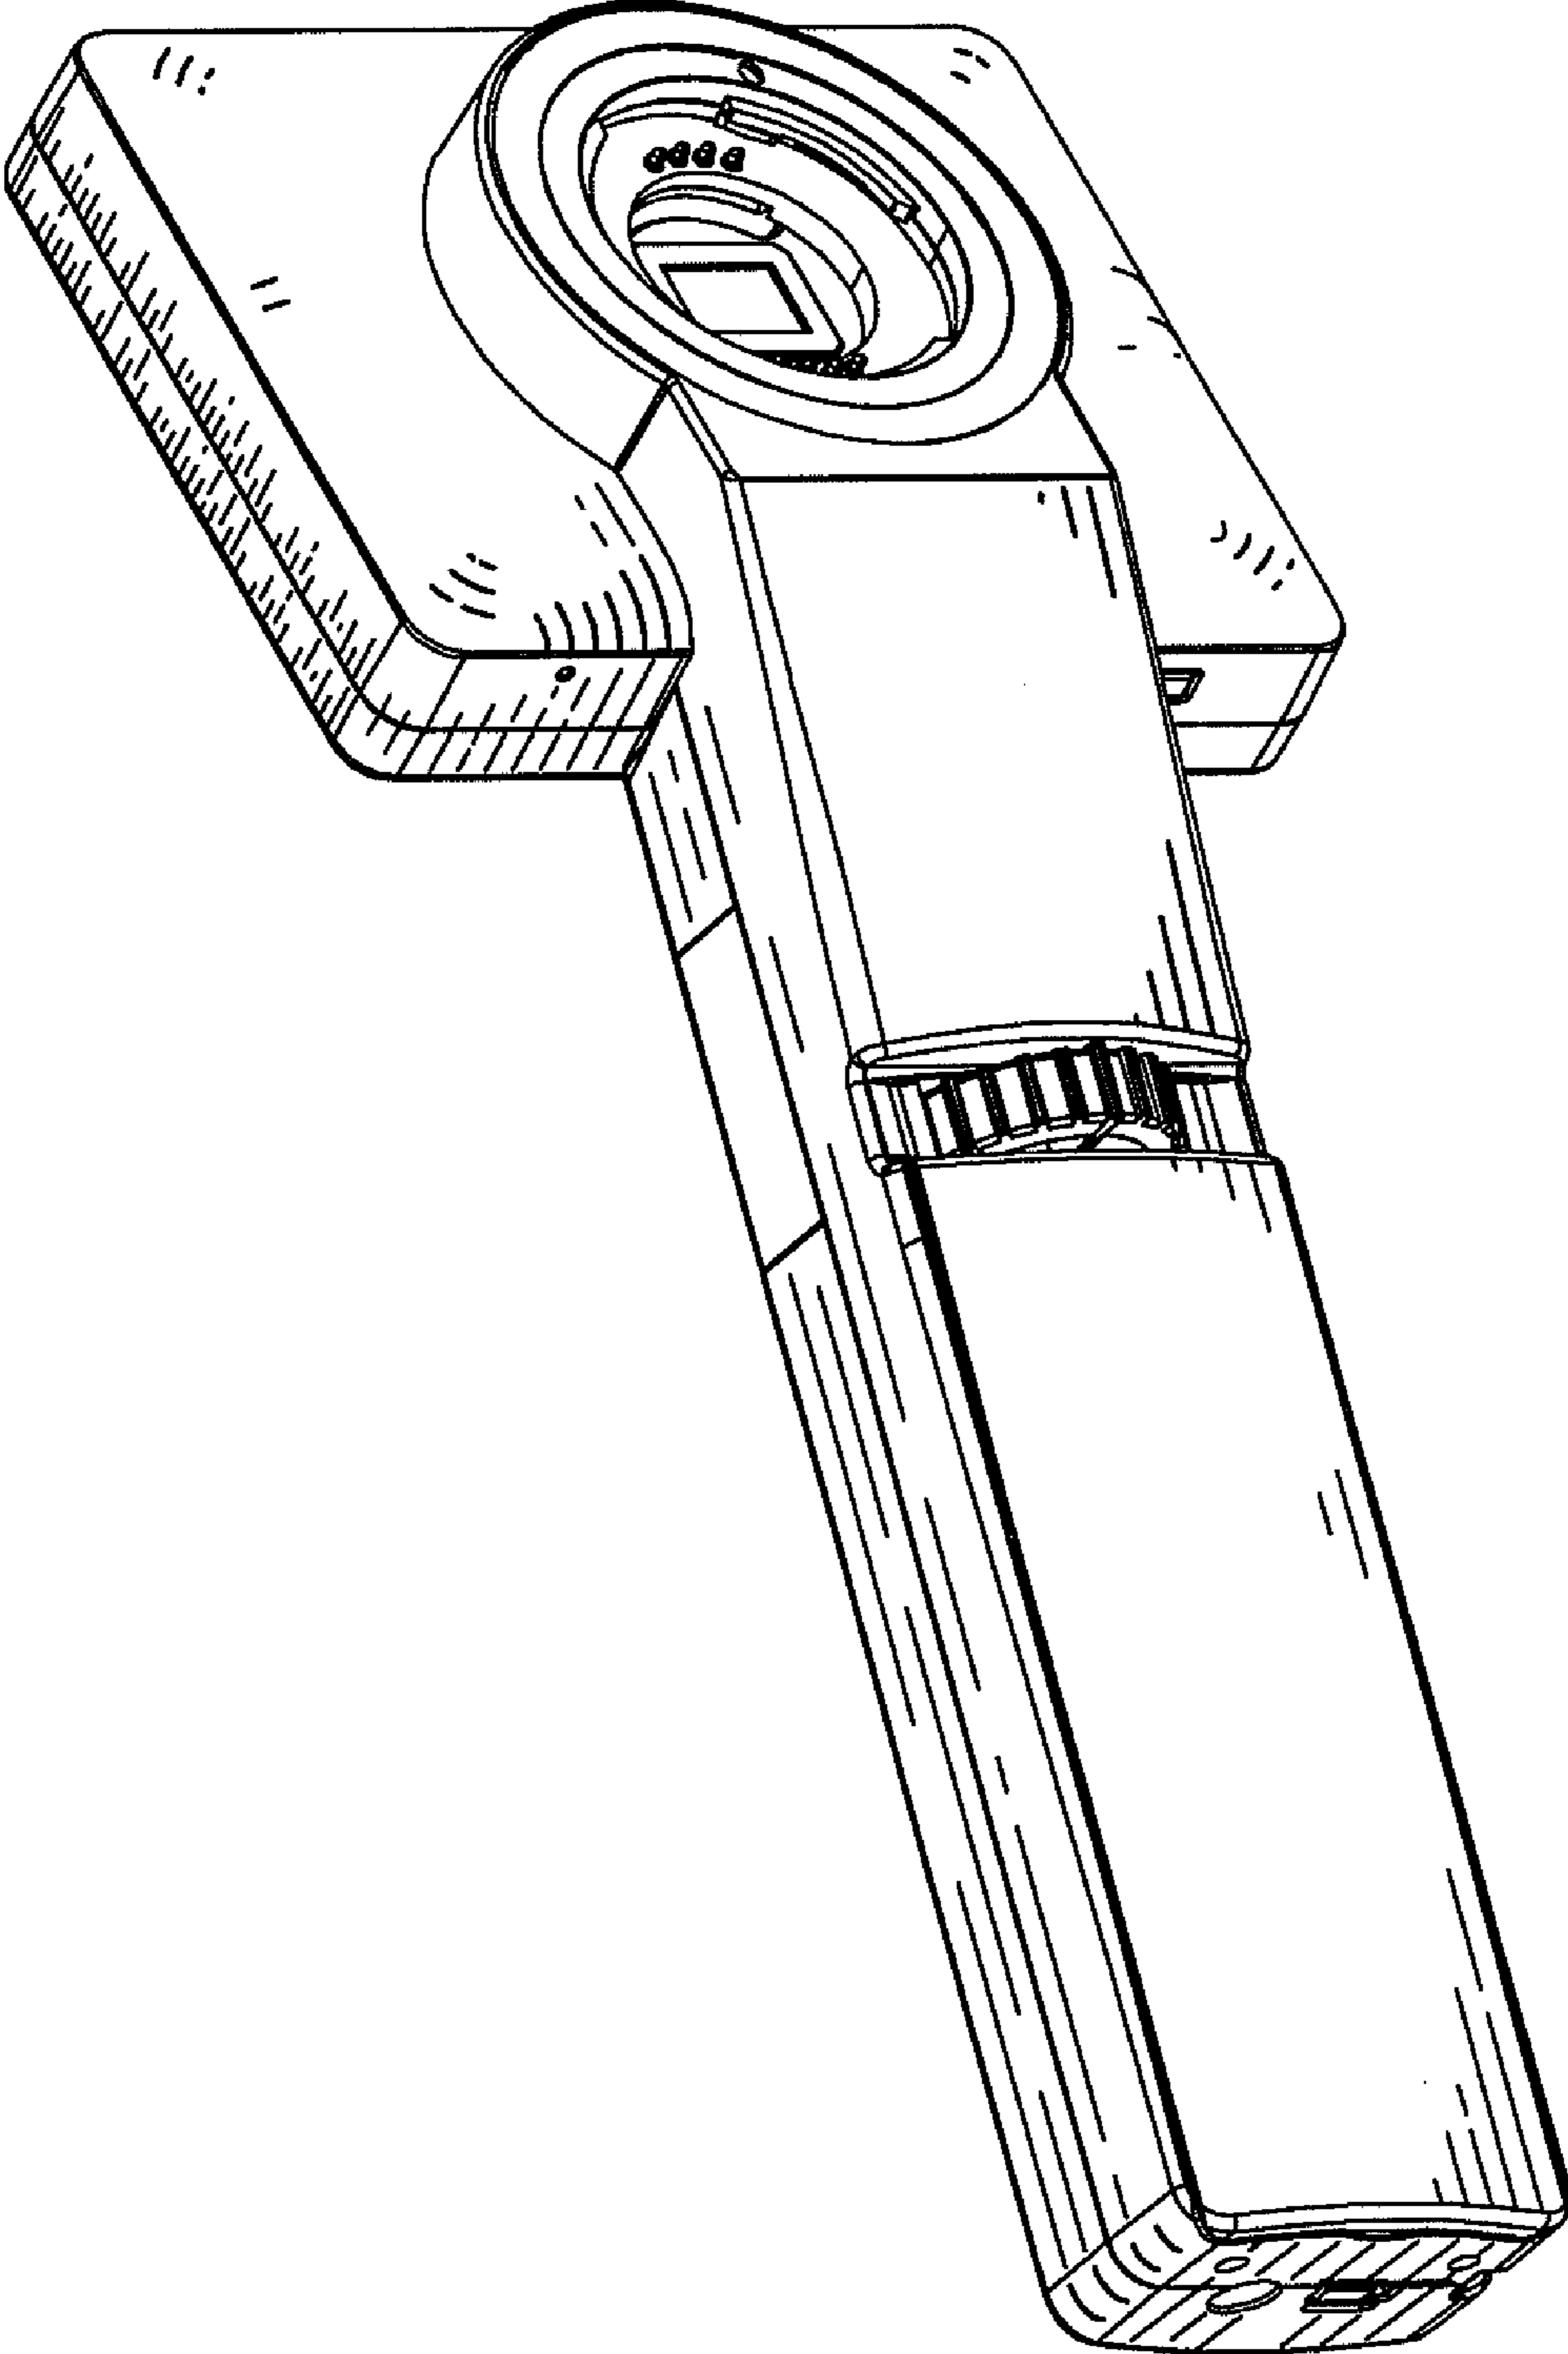


FIG.8

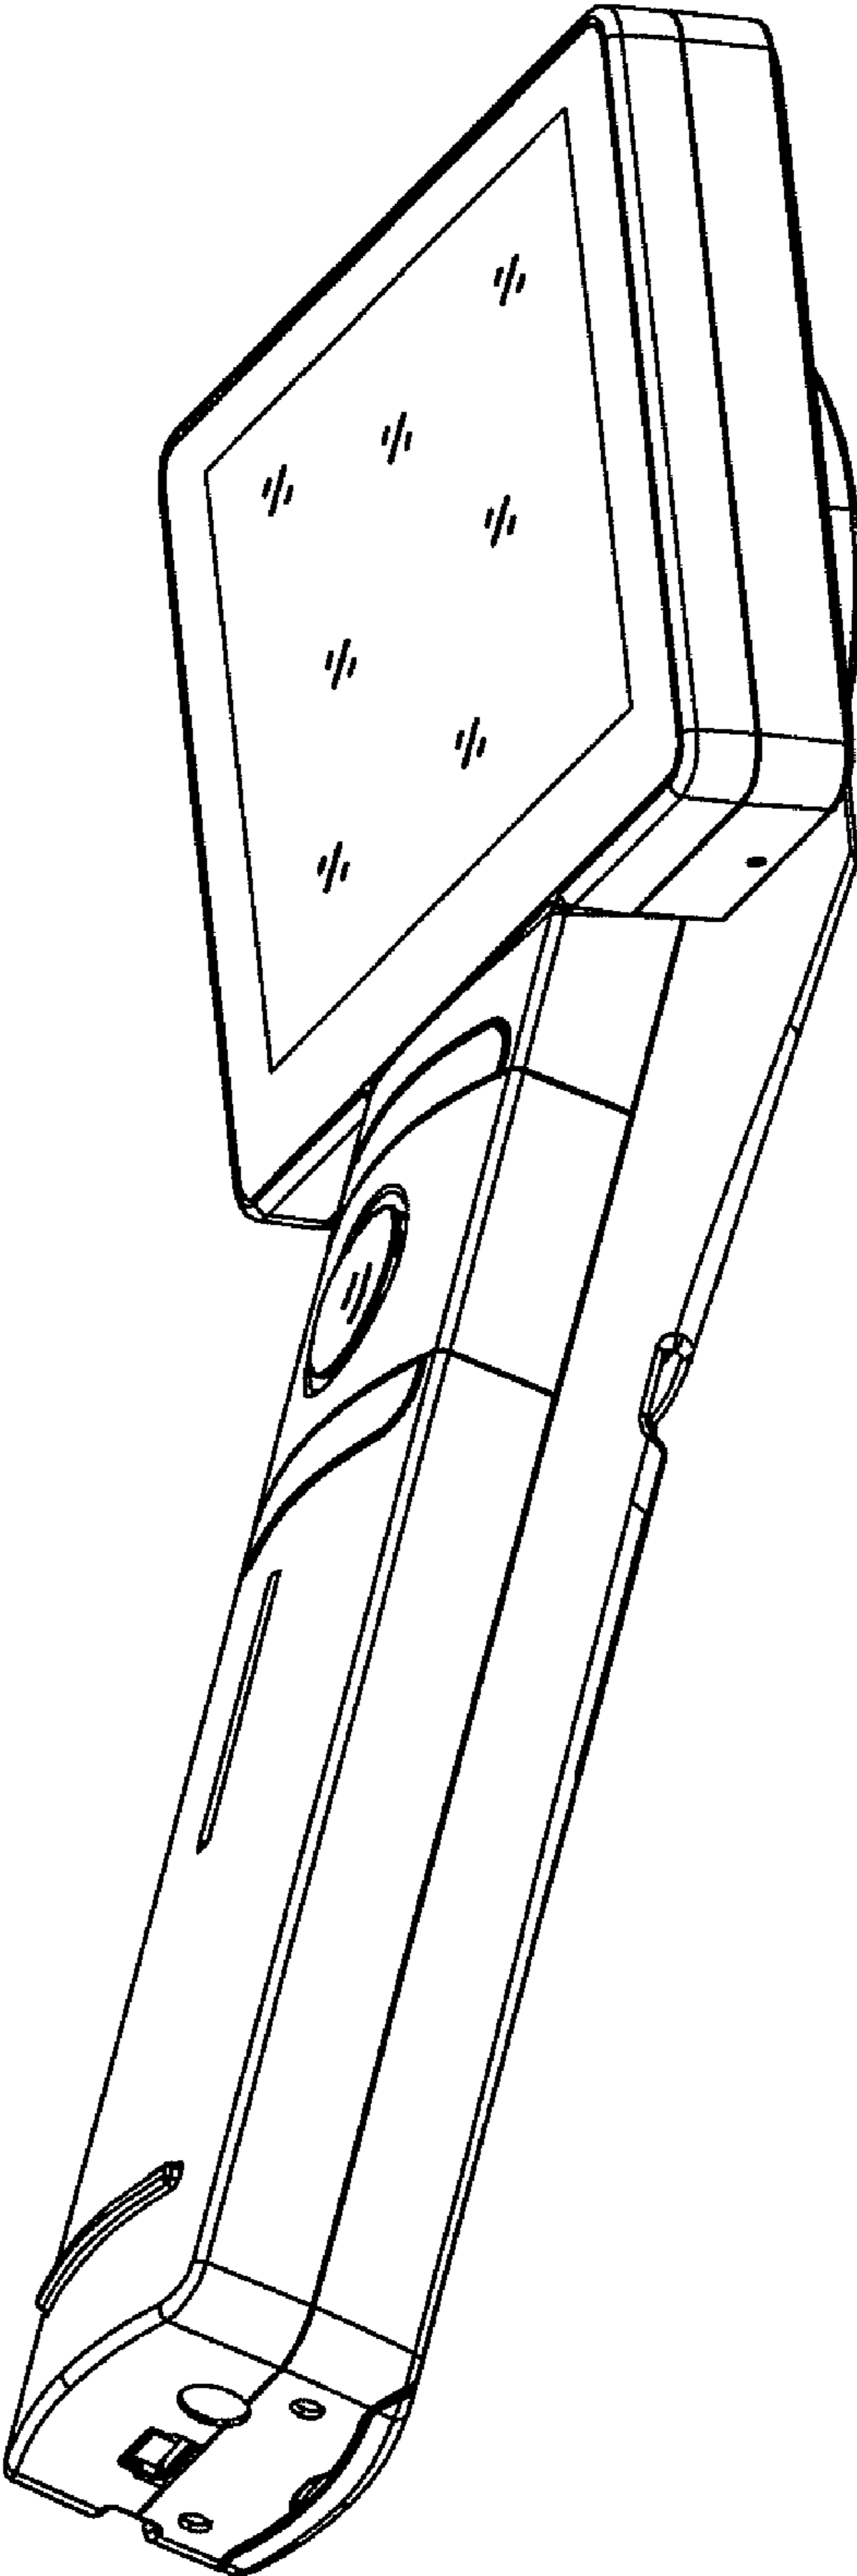


FIG.9

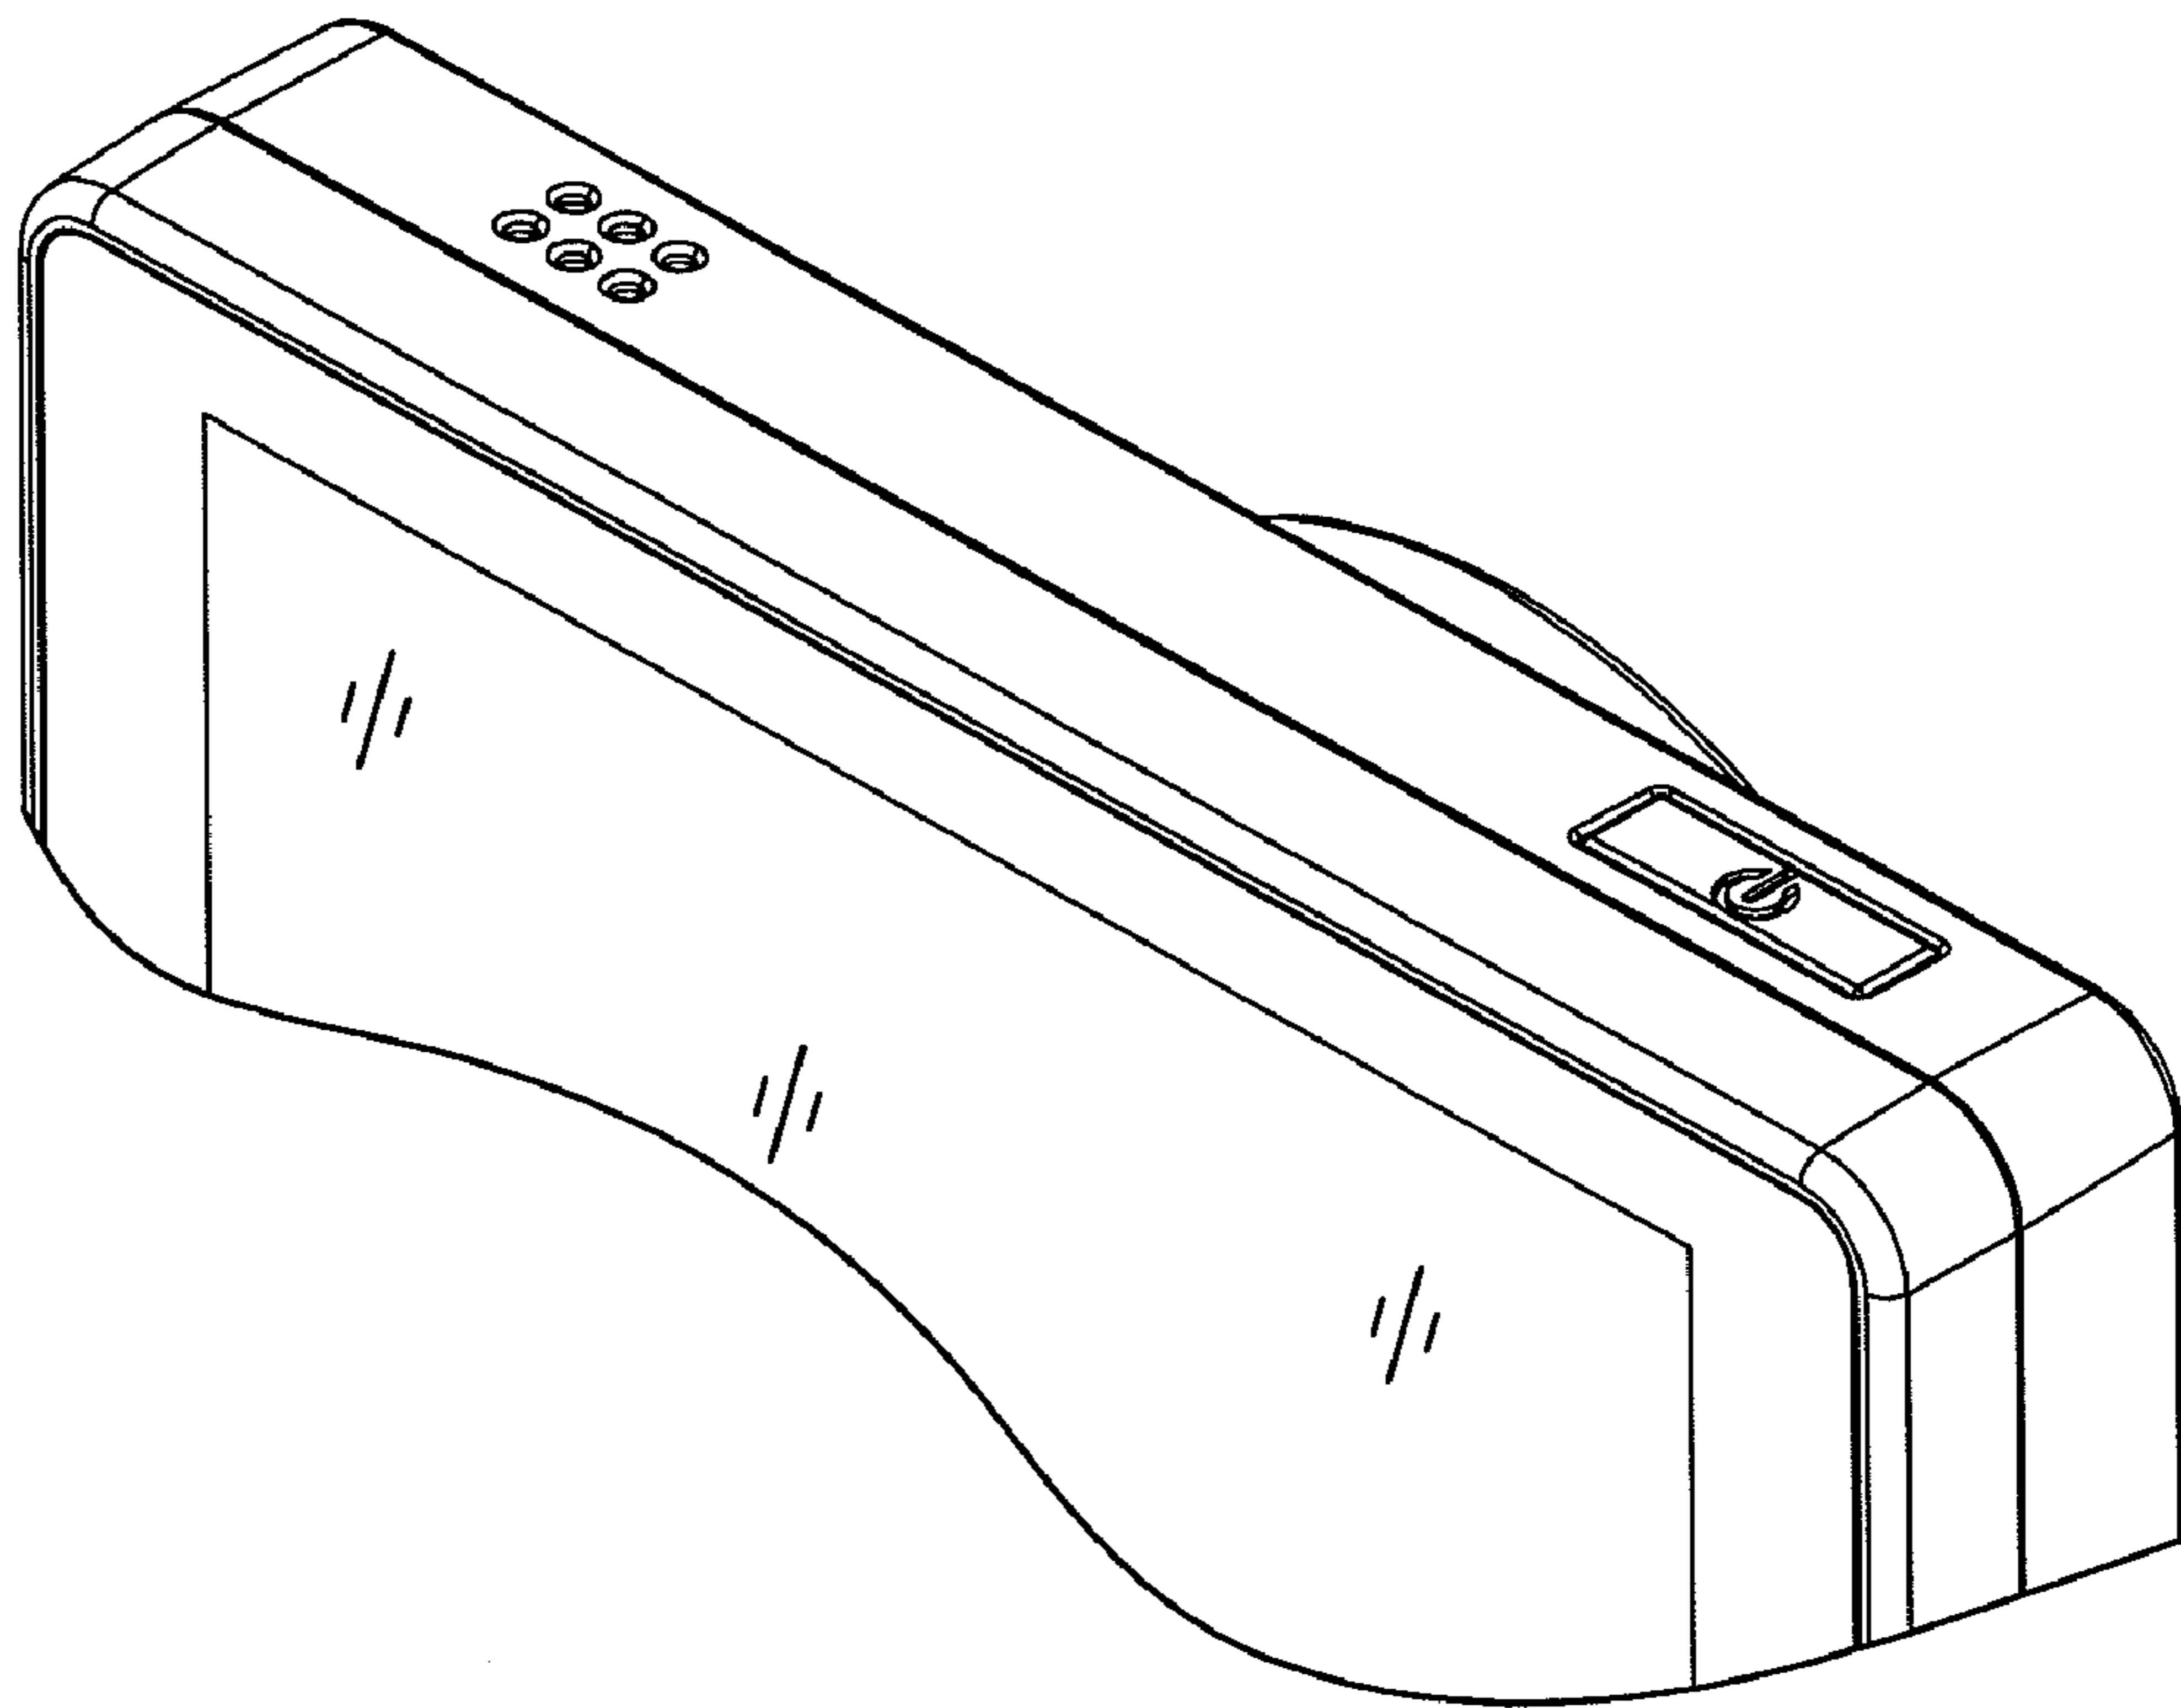


FIG.10