



US00D661395S

(12) **United States Design Patent**  
**Titolo**

(10) **Patent No.:** **US D661,395 S**  
(45) **Date of Patent:** **\*\* Jun. 5, 2012**

(54) **DECLAW CLAMP DEVICE**

(76) Inventor: **Joaquin S. Titolo**, Richton Park, IL (US)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/389,235**

(22) Filed: **Apr. 7, 2011**

(51) **LOC (9) Cl.** ..... **24-02**

(52) **U.S. Cl.** ..... **D24/143; D24/148**

(58) **Field of Classification Search** ..... D24/143,  
D24/133, 149, 153, 148; D8/52, 54, 57,  
D8/58, 93; 81/318, 424; 606/1, 151, 174,  
606/205-208

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

1,462,202	A *	7/1923	Hopper	.....	606/207
2,642,871	A *	6/1953	Thuerig	.....	606/207
3,035,582	A *	5/1962	Seiger	.....	606/205
3,176,689	A *	4/1965	Yahr	.....	606/208
3,209,753	A *	10/1965	Hawkins et al.	.....	606/207
D321,055	S *	10/1991	Carchidi	.....	D24/152
5,320,637	A *	6/1994	Borders, Jr.	.....	606/207
5,997,566	A *	12/1999	Tobin	.....	606/205
6,205,699	B1 *	3/2001	Bogni	.....	606/207
D575,400	S *	8/2008	Patterson et al.	.....	D24/143

OTHER PUBLICATIONS

Codman "Stone Clamp Applying Forceps", p. G-24, "Allis Classic Tissue Forceps and Allis Classic Delicate", p. G-29, "Thoms-Allis Tissue Forceps", p. G-31.\*

Dr. Titolo Declaw Clamp 6¼", 2005-2010 [retrieved on Jan. 30, 2012]. Retrieved from the Internet: <URL: <http://www.germedusa.com/p-5230-dr-titolo-declaw-clamp-6-14.aspx>>.\*

\* cited by examiner

*Primary Examiner* — Wan Laymon

(74) *Attorney, Agent, or Firm* — Davis M. Chin, Jr.; Davis Chin

(57) **CLAIM**

The ornamental design for a declaw clamp device, as shown and described.

**DESCRIPTION**

FIG. 1 is a front plan view of a declaw clamp device showing my design;

FIG. 2 is a rear plan view of the design shown in FIG. 1;

FIG. 3 is a left side elevational view of the design shown in FIG. 1;

FIG. 4 is a right side elevational view of the design shown in FIG. 1;



FIG. 5 is a top end view of the design shown in FIG. 1;


FIG. 6 is a bottom end view of the design shown in FIG. 1;

FIG. 7 is a prospective view of the declaw clamp device showing my design, with the sharpened edges being illustrated in the closed position; and,


FIG. 8 is a prospective view of the declaw clamp device showing my design, with the sharpened edges being illustrated in the open position.

**1 Claim, 3 Drawing Sheets**

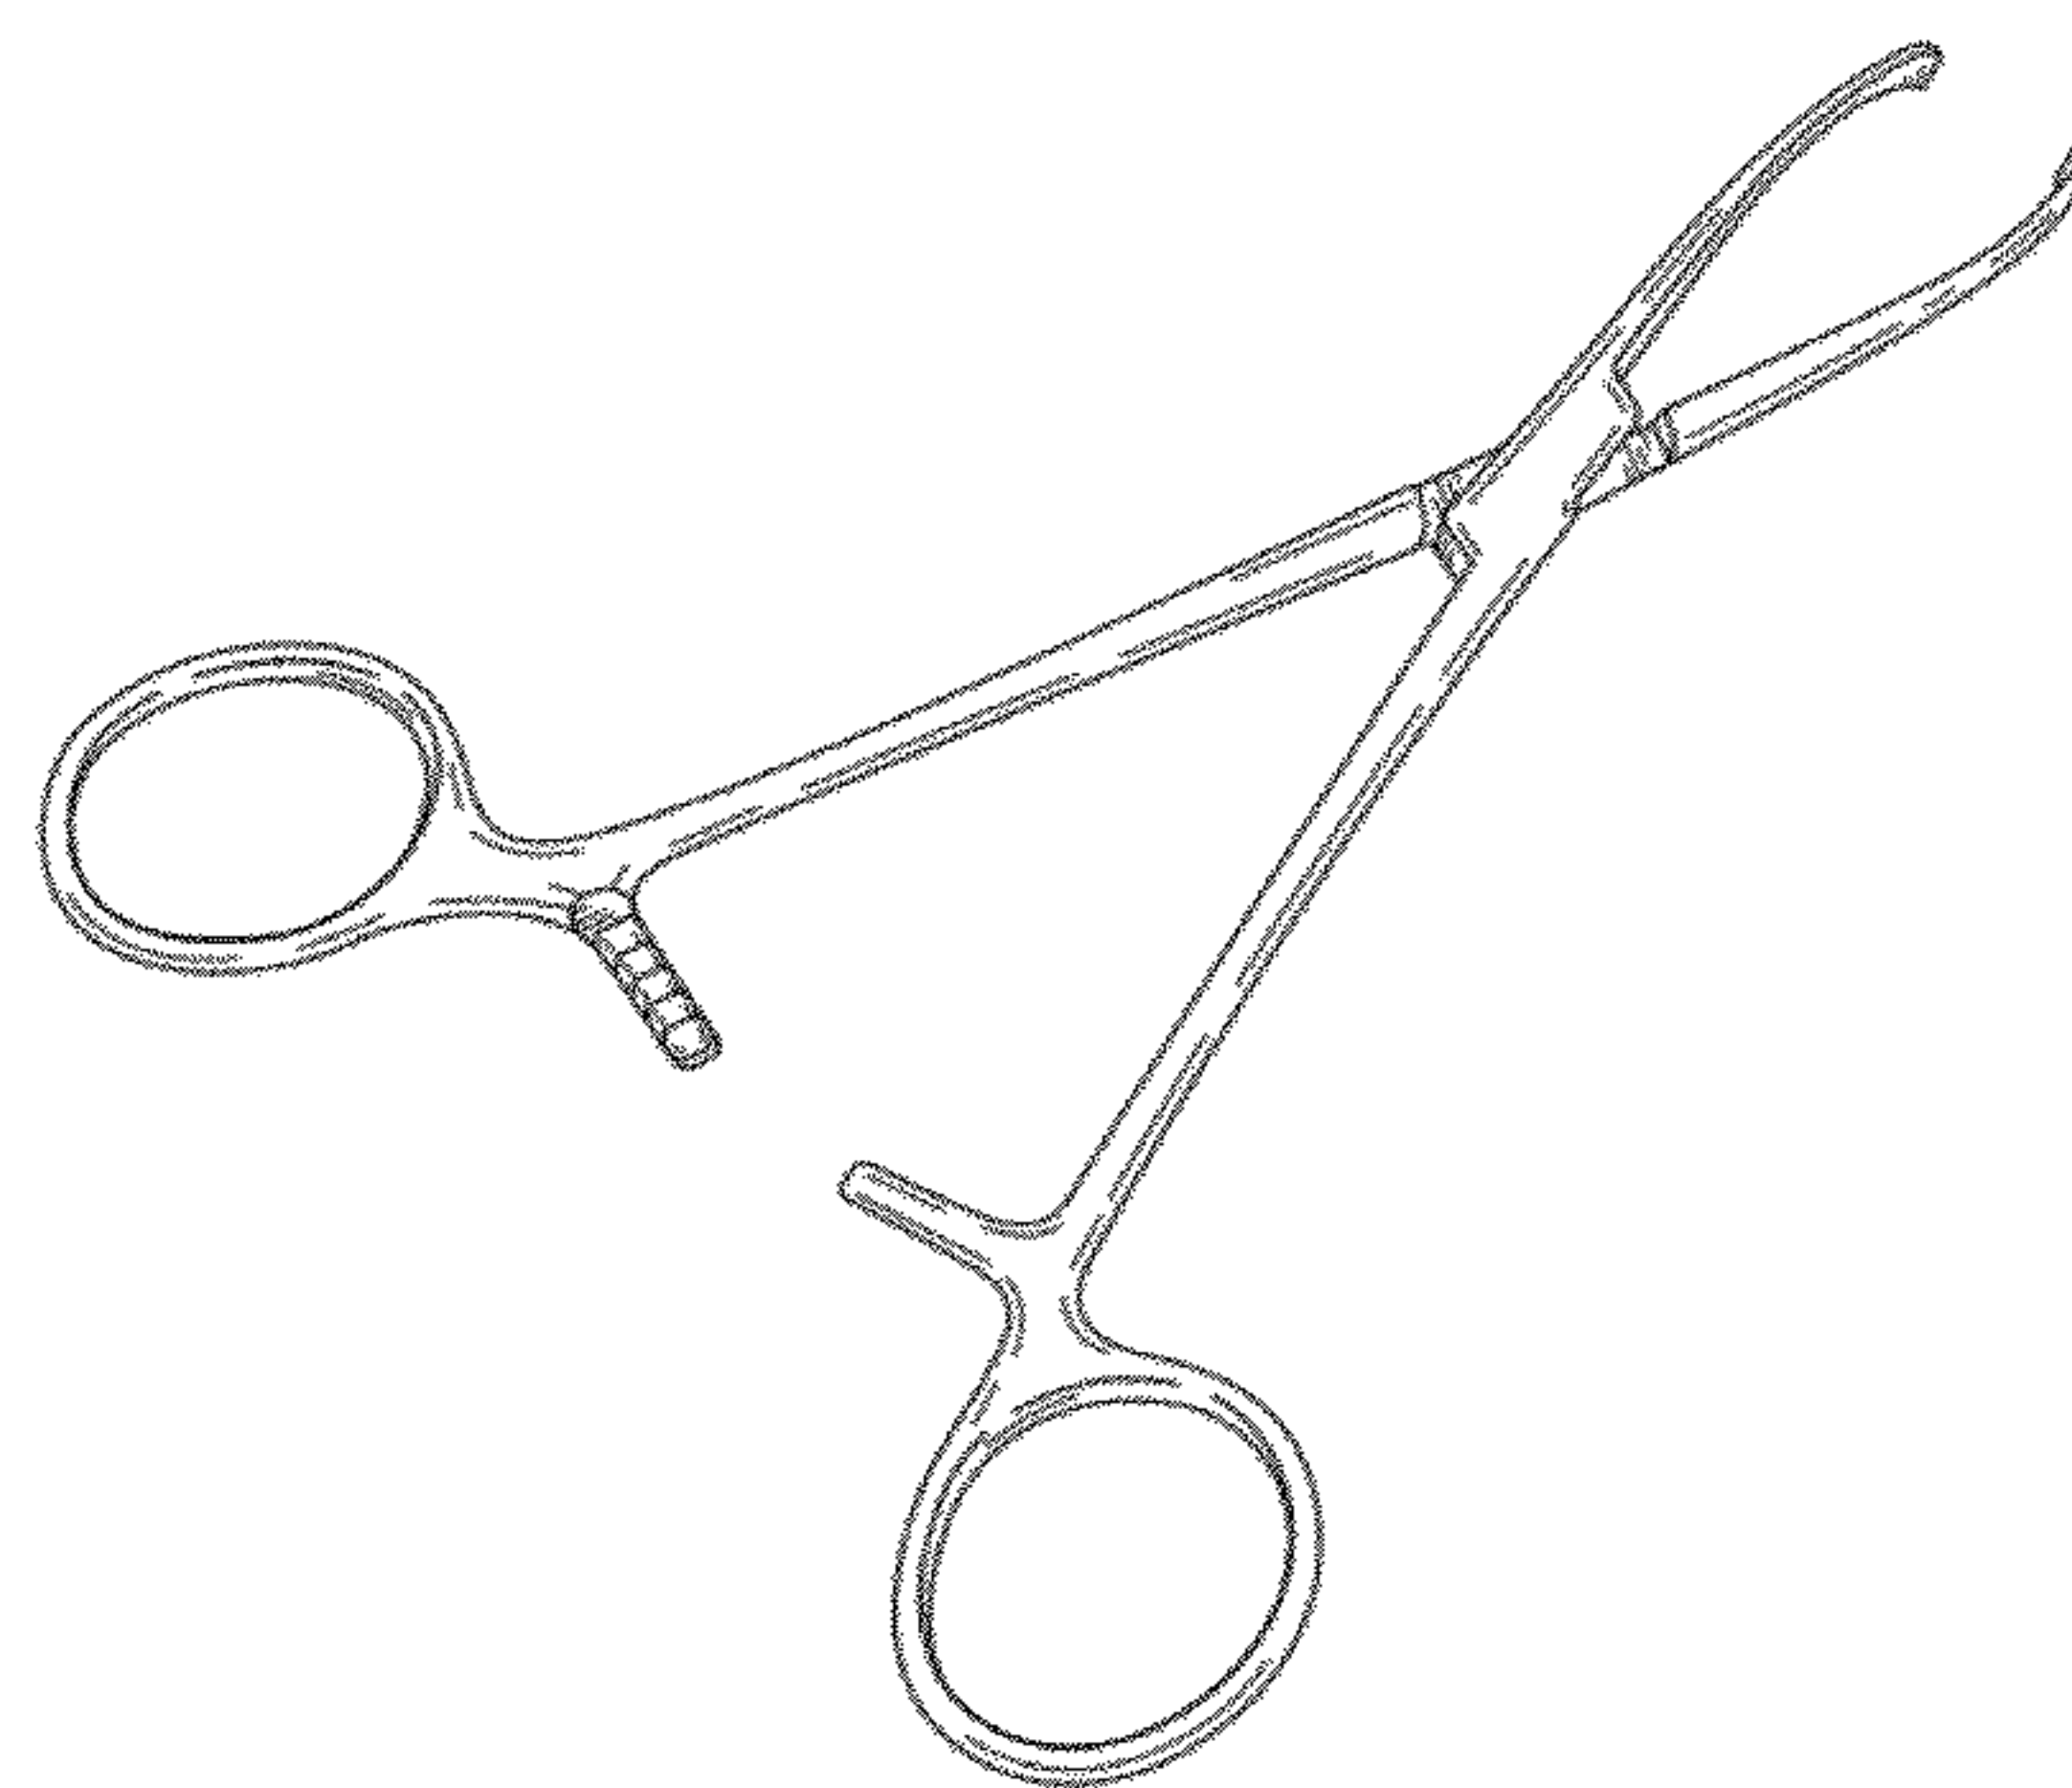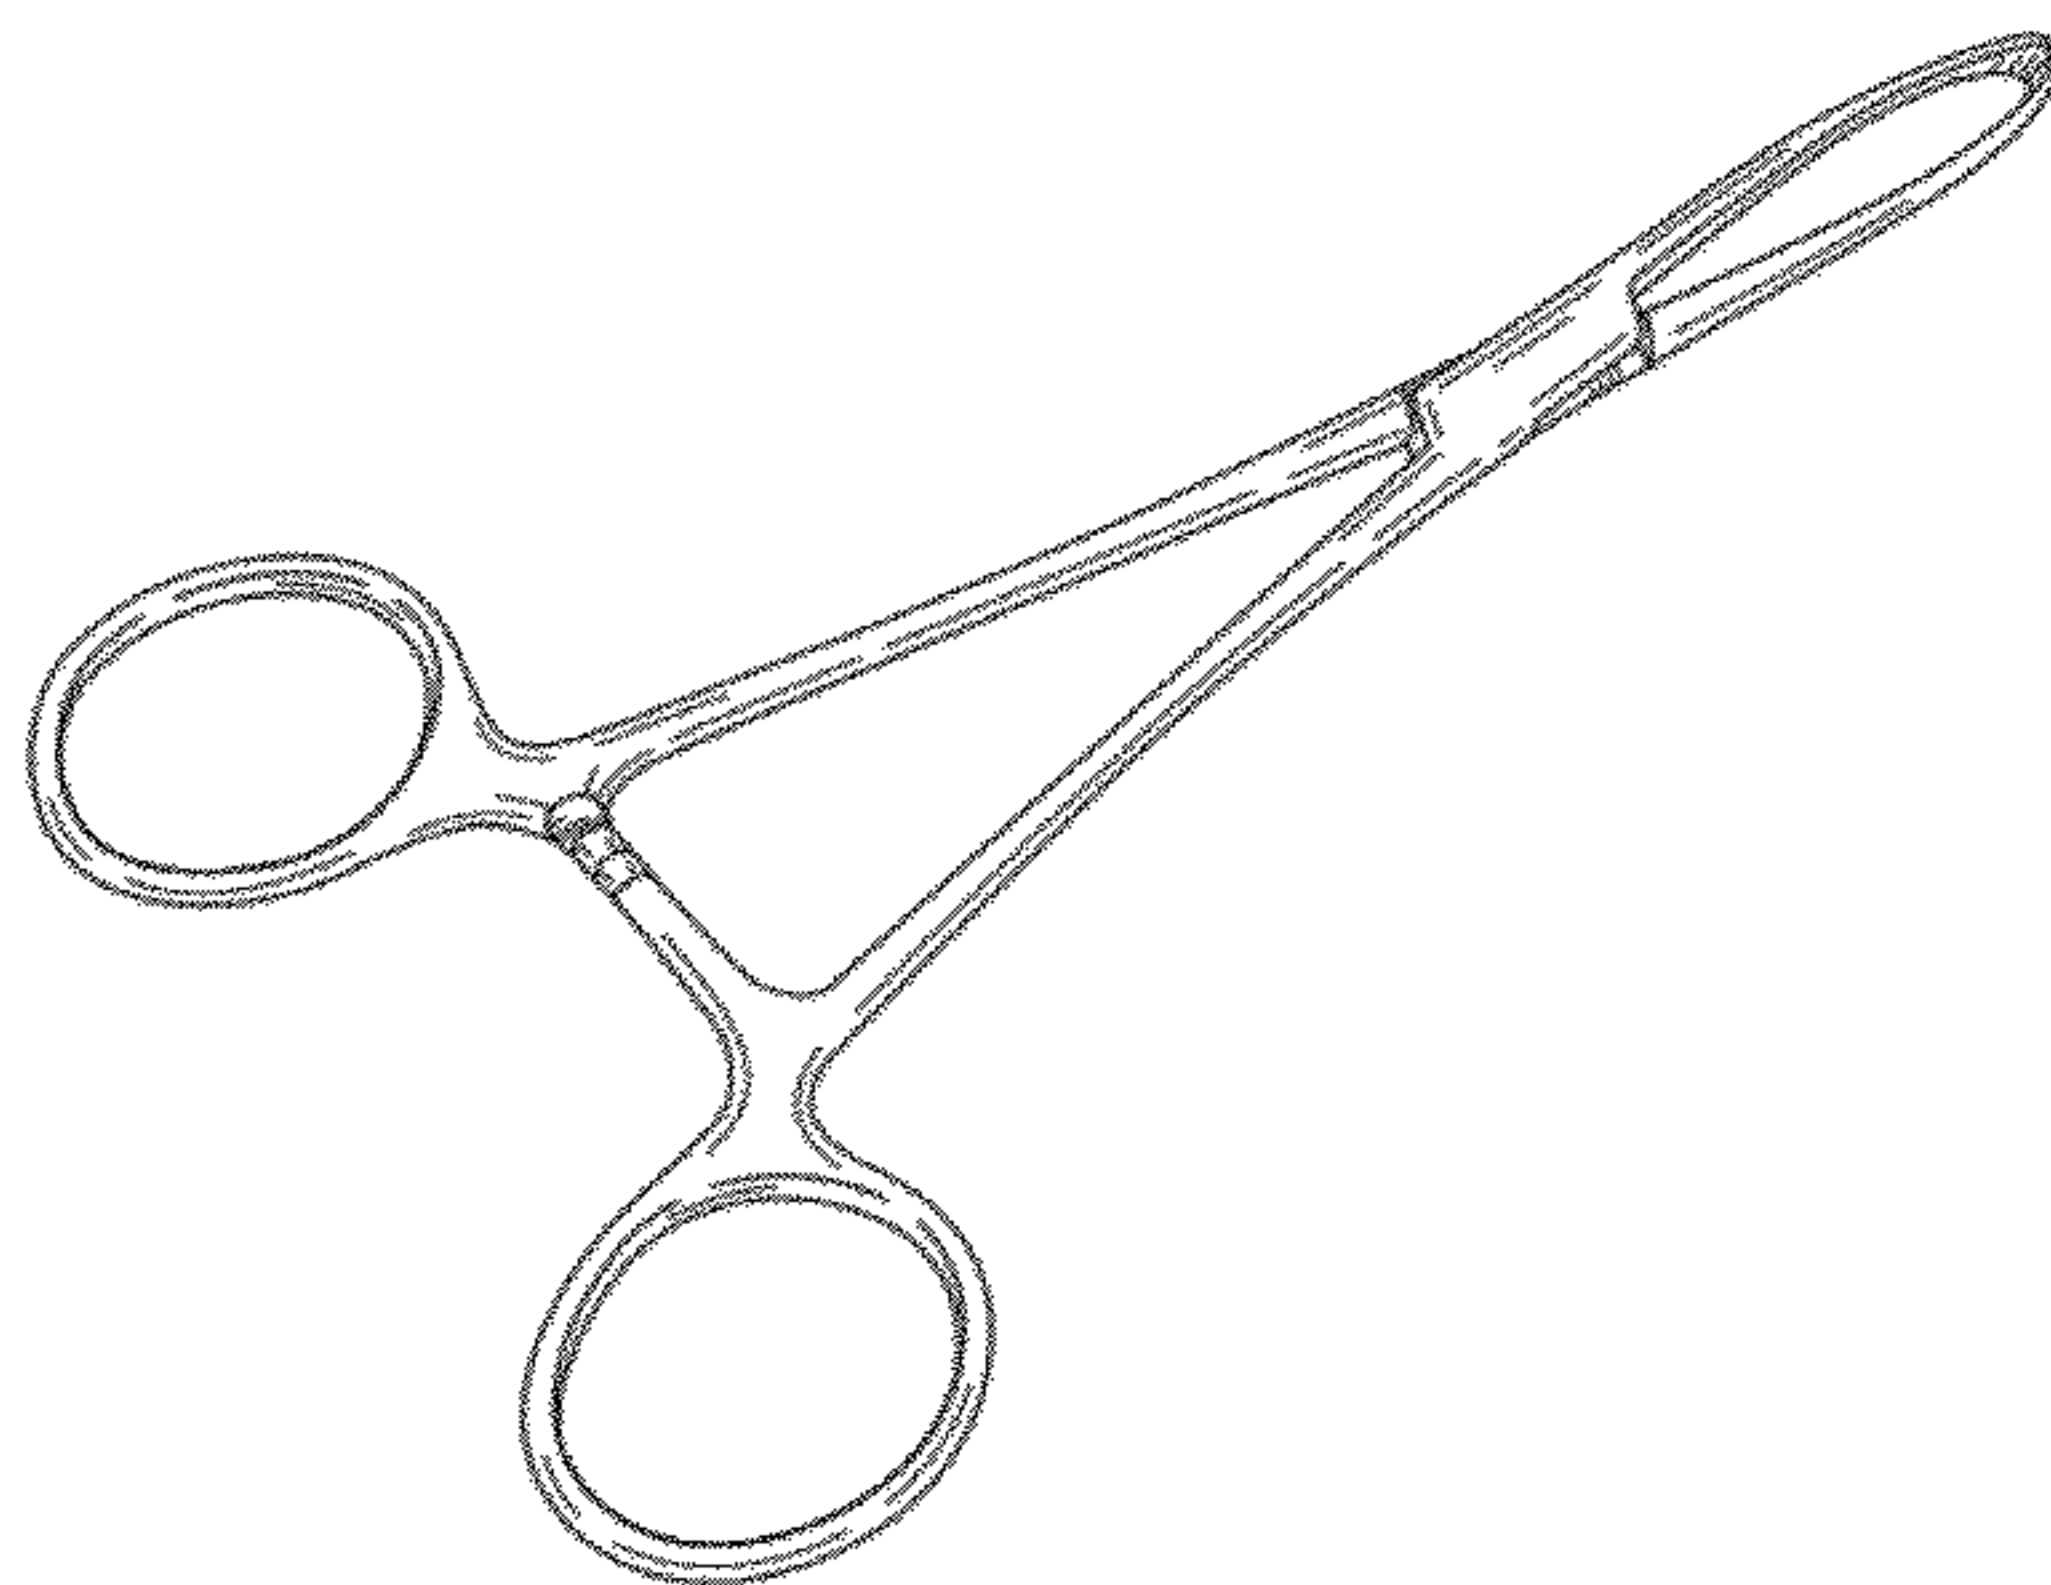

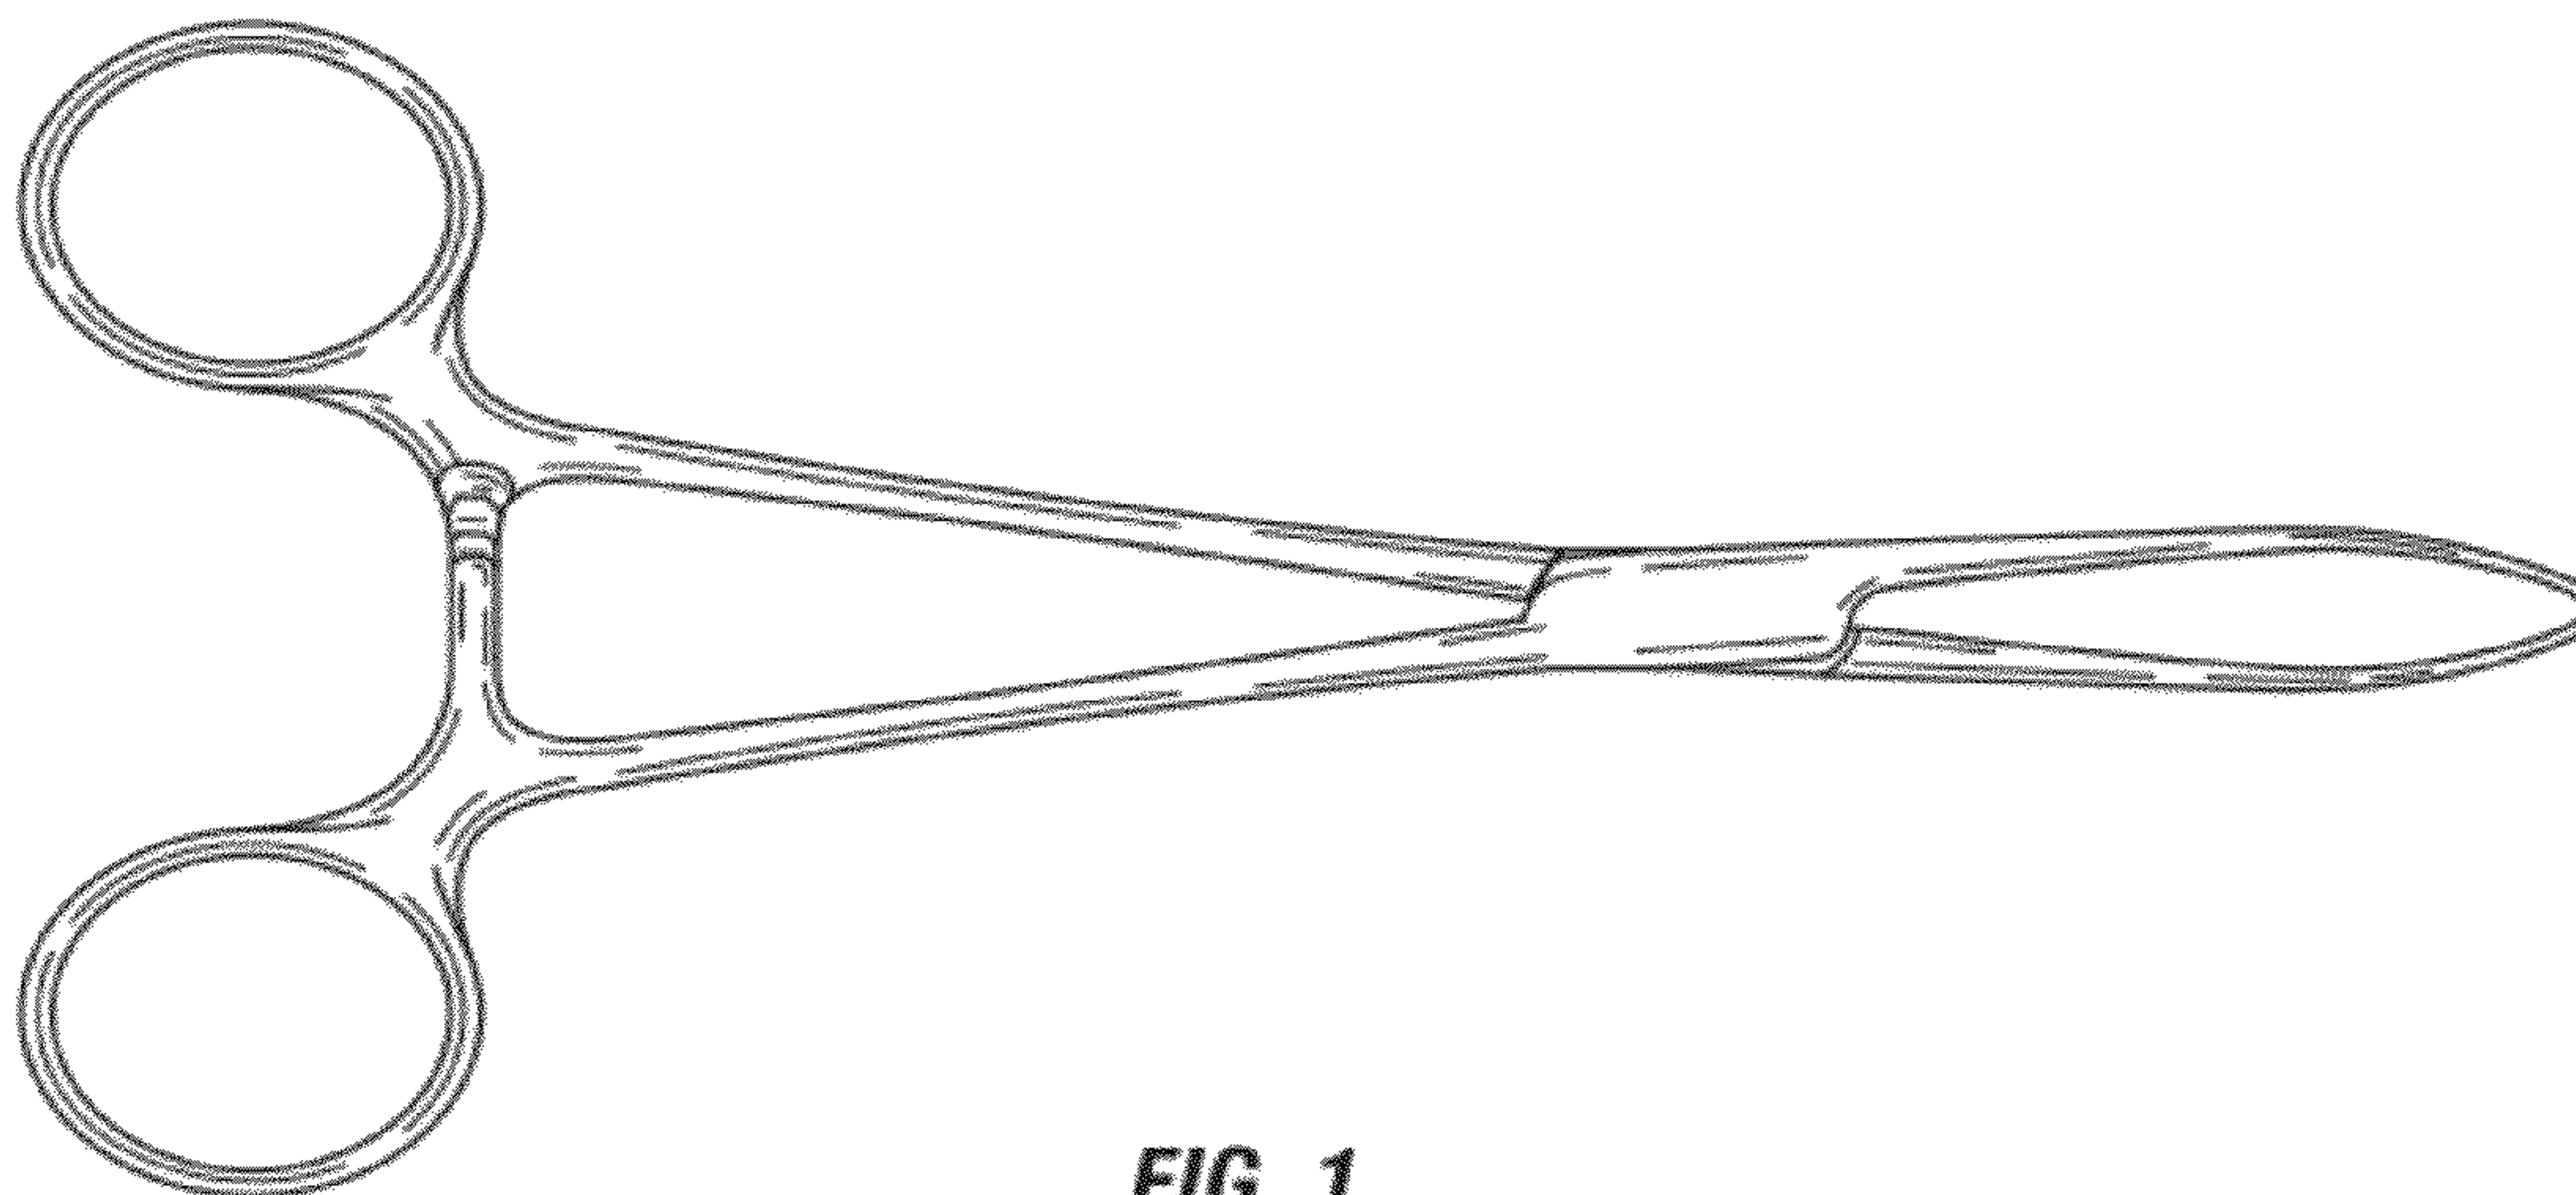


**FIG. 1**

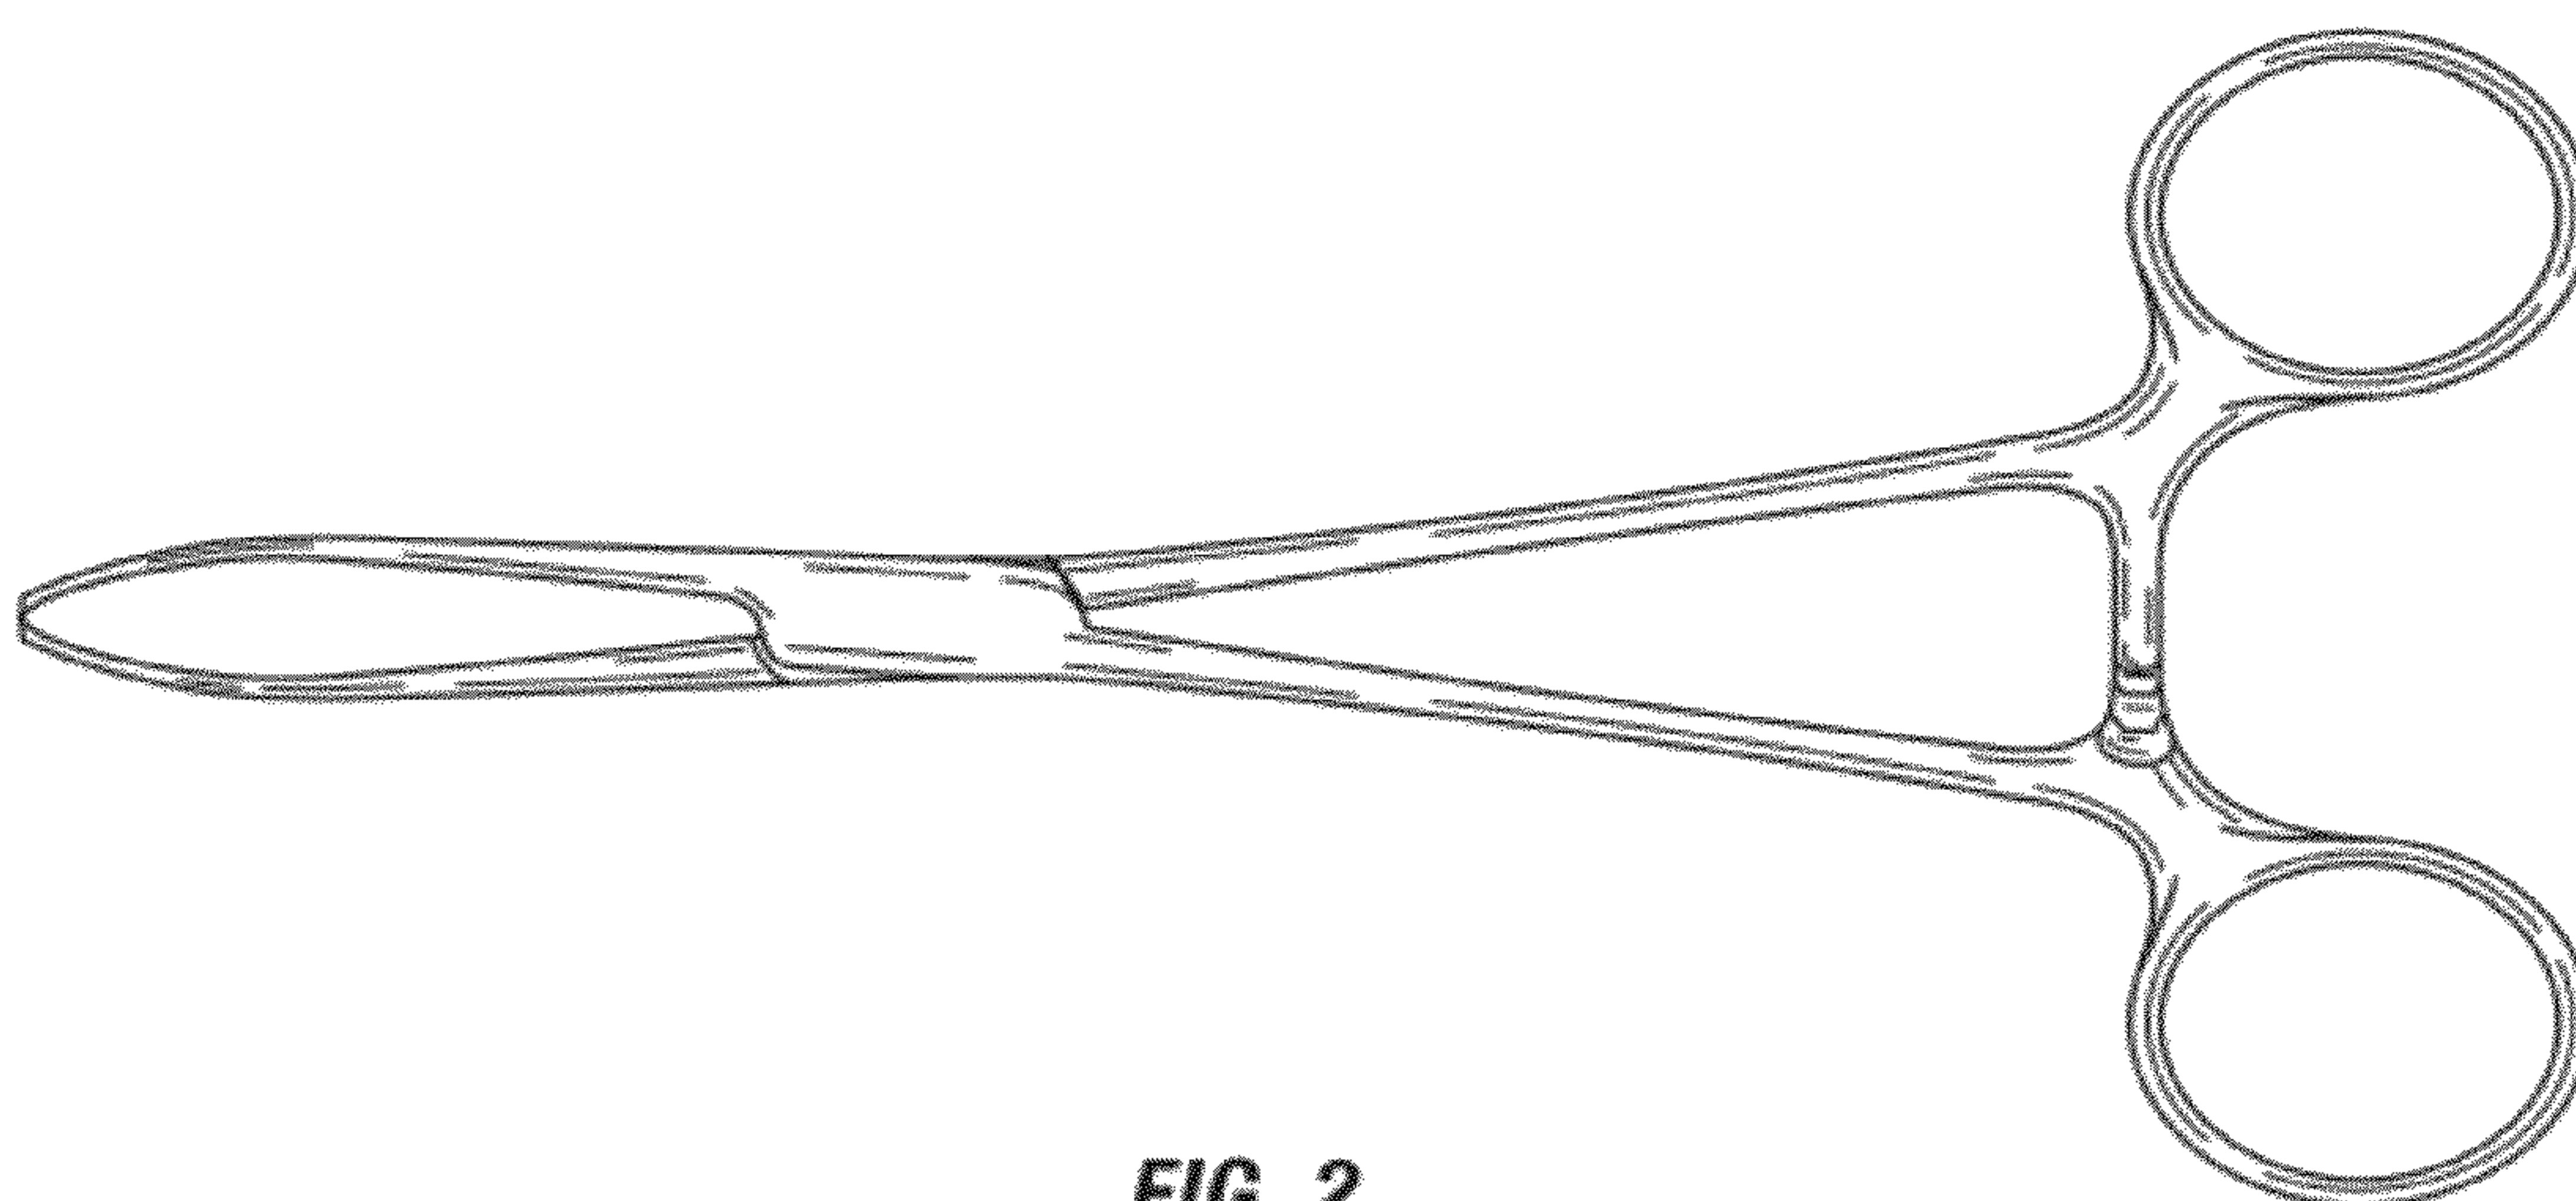

**FIG. 2**



**FIG. 3**

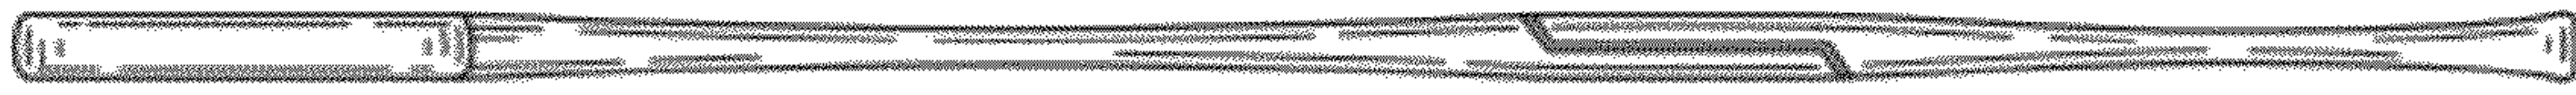

**FIG. 4**




**FIG. 5**




**FIG. 6**



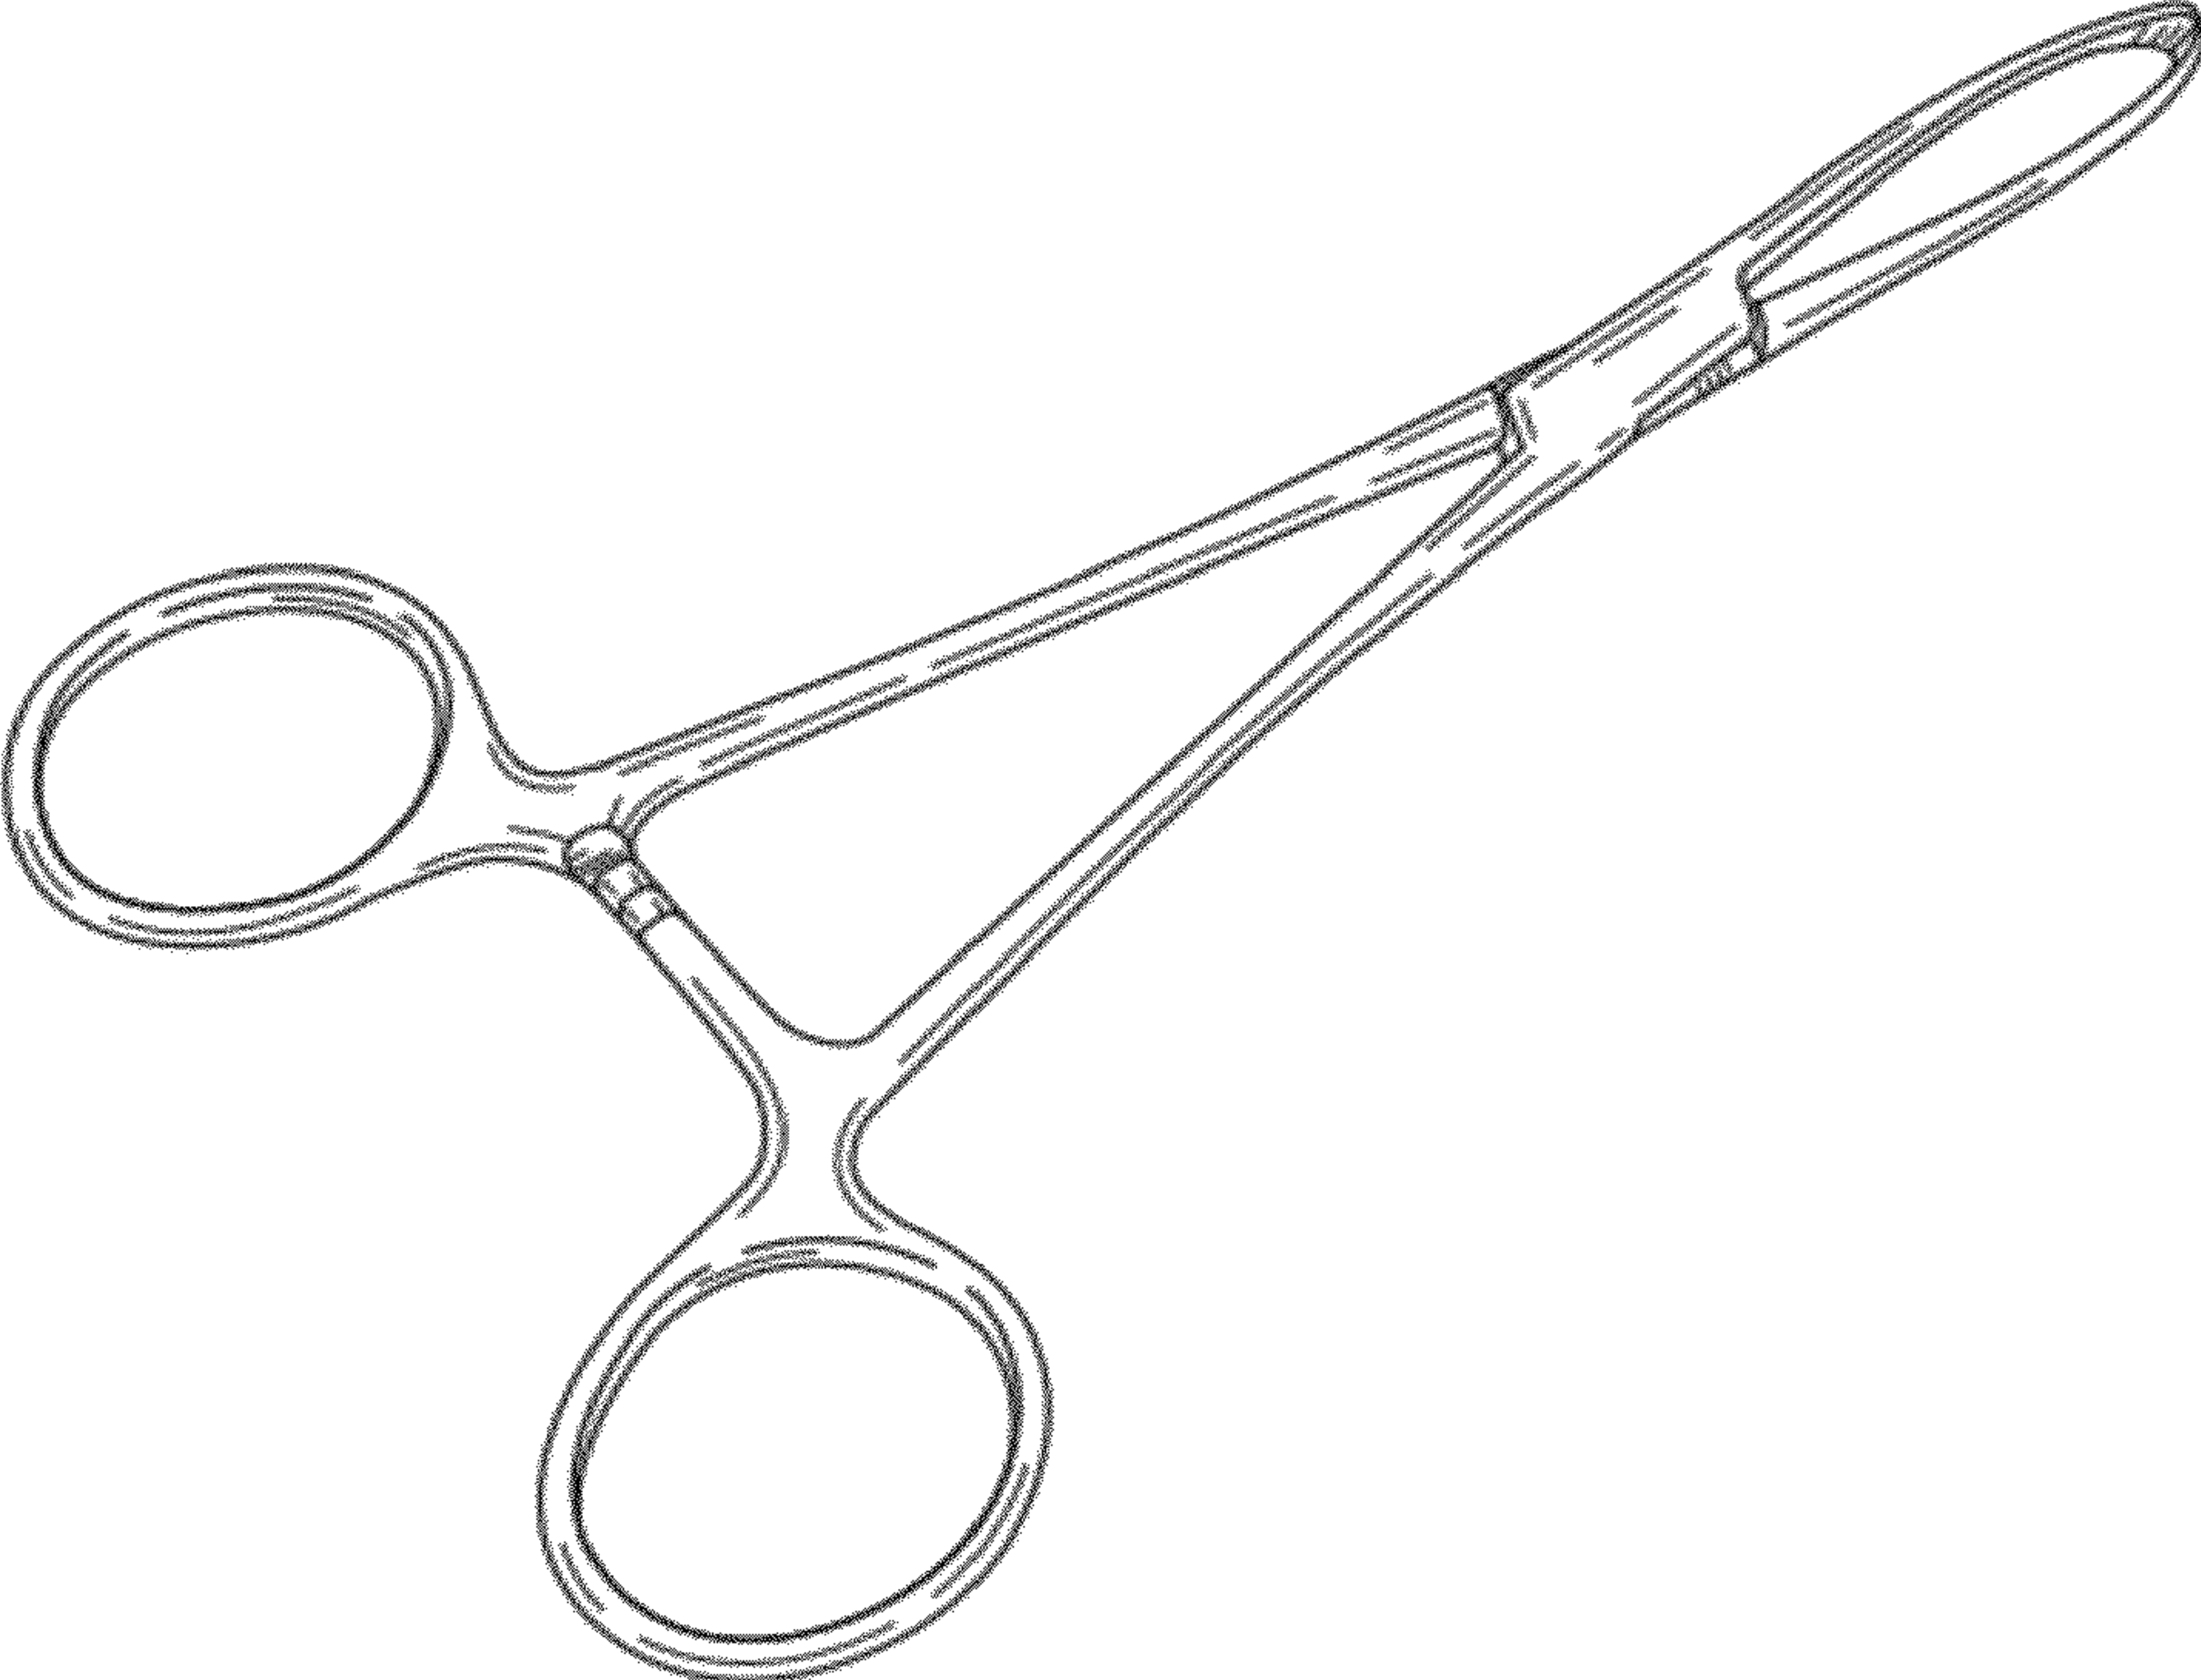

**FIG. 7**

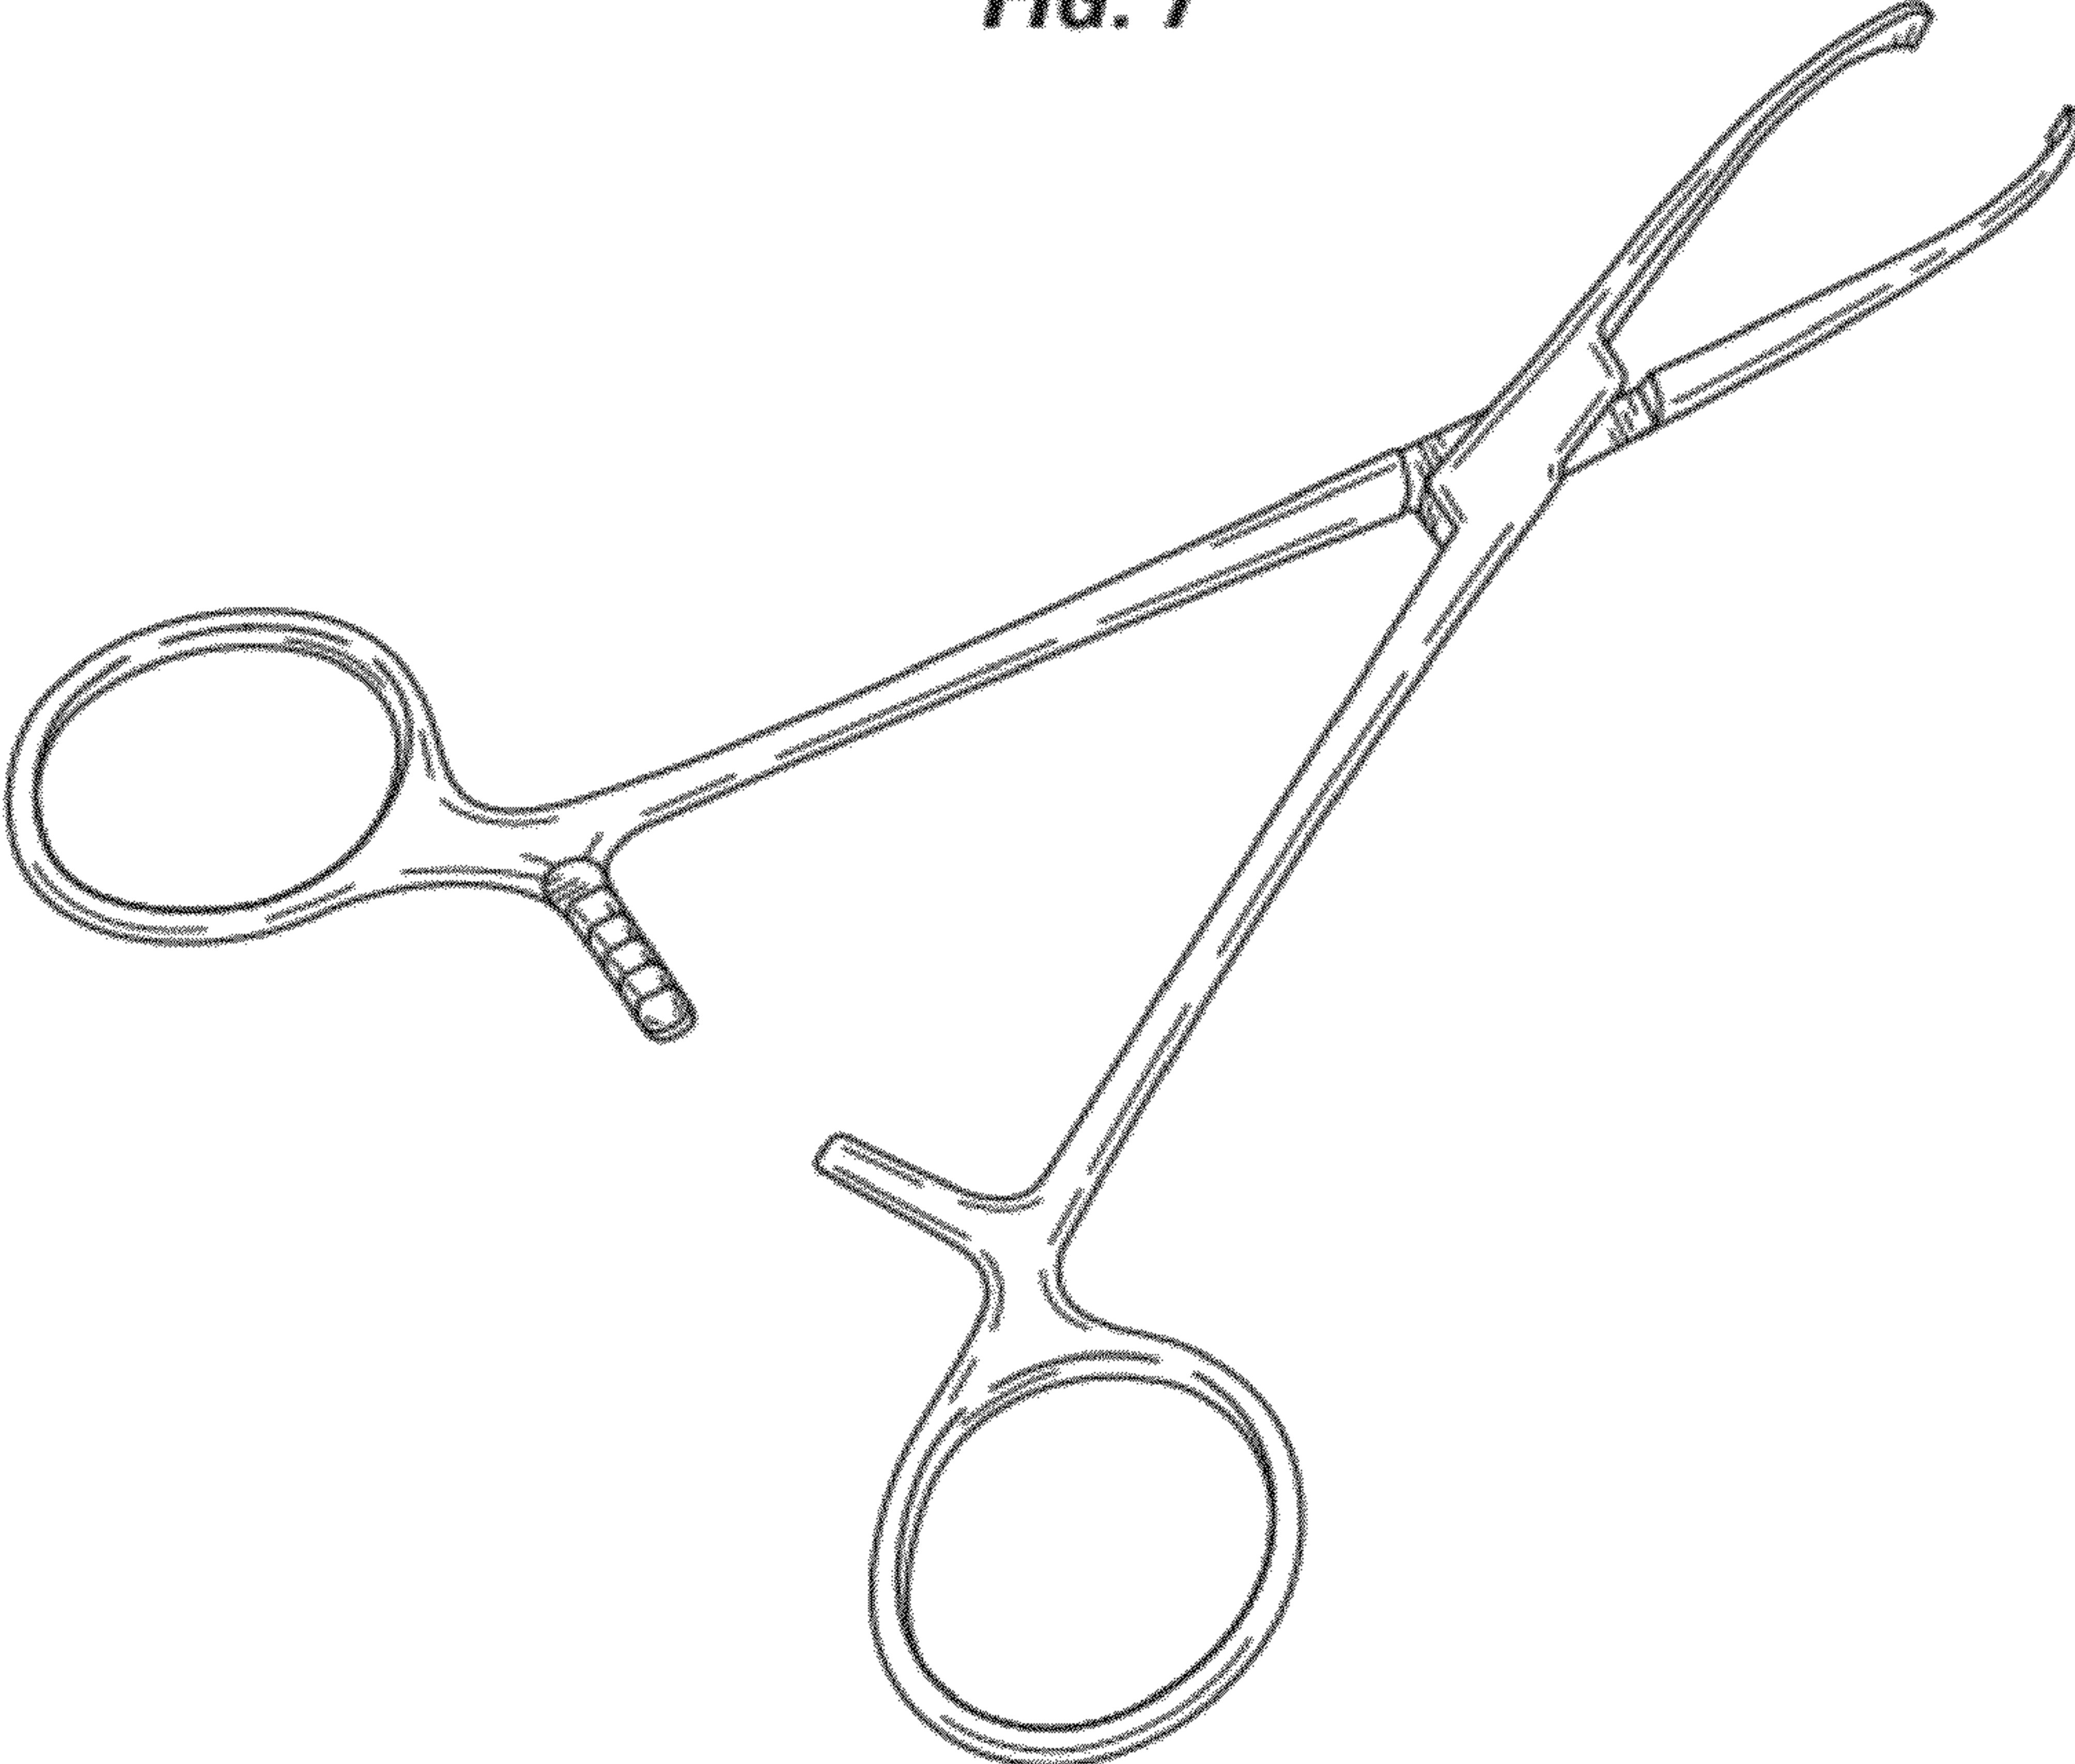

**FIG. 8**