

US00D663421S

(12) **United States Design Patent**
Steiner et al.

(10) **Patent No.:** **US D663,421 S**
(45) **Date of Patent:** **** Jul. 10, 2012**

(54) **HAND-HELD BLOOD GLUCOSE METER**

(75) Inventors: **Bettina Steiner**, Indianapolis, IN (US);
Lisa Yanz, Chicago, IL (US); **Sona N. Patadia-Rao**, Chicago, IL (US);
Michael F. DeRossi, Lindenhurst, IL (US); **Sofia E. Galbraith**, Solothurn (CH); **Joseph Brian Lewis**, Indianapolis, IN (US)

(73) Assignees: **Roche Diagnostics Operations, Inc.**, Indianapolis, IN (US); **Roche Diagnostics International AG**, Steinhausen (CH)

(**) Term: **14 Years**

(21) Appl. No.: **29/377,012**

(22) Filed: **Oct. 15, 2010**

(51) **LOC (9) Cl.** **24-01**

(52) **U.S. Cl.** **D24/169**

(58) **Field of Classification Search** D24/165-169,
D24/107, 186, 216, 223, 231, 232; D10/46,
D10/81; D14/341; 422/56, 58, 68.1; 600/316,
600/322, 347, 365, 368

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D431,486 S	10/2000	Iseli et al.	
D475,462 S *	6/2003	Maeda et al.	D24/167
D494,144 S	8/2004	Guzman et al.	
D510,711 S	10/2005	Syme et al.	
D549,830 S *	8/2007	Behar et al.	D24/186
D551,350 S *	9/2007	Lorimer et al.	D24/186
D557,422 S	12/2007	Arbogast et al.	
D558,757 S *	1/2008	Andre et al.	D14/341
D569,521 S	5/2008	Omaki	
D586,466 S	2/2009	Smith et al.	
D598,109 S	8/2009	Collins et al.	
D601,257 S	9/2009	Berlinger et al.	
D606,129 S *	12/2009	Ben-Moshe	D14/341
D606,659 S	12/2009	Kiani et al.	

D612,274 S	3/2010	Heidemann et al.	
D612,355 S *	3/2010	Luo	D14/138 AC
D613,411 S	4/2010	Collins et al.	
D617,802 S	6/2010	Holliday et al.	
D621,048 S *	8/2010	Severe et al.	D24/167
D621,515 S *	8/2010	Chua et al.	D24/186
D626,651 S *	11/2010	Brauer et al.	D24/169
D644,218 S *	8/2011	Akana et al.	D14/341
D648,303 S *	11/2011	Park et al.	D14/138 G

OTHER PUBLICATIONS

“Noah’s Apple iPhone Review,” www.phonedog.com, 9 pages, published Aug. 11, 2010.

“iPhone,” en.wikipedia.org, 24 pages, published Aug. 29, 2010.

www.jewelpump.com, 2 pages, published Sep. 1, 2010.

www.cellnovo.com, 1 page, published Sep. 1, 2010.

Cellnovo touch screen diabetes pump, 94 pages, published prior to Oct. 2010.

U.S. Design Patent Application entitled “Blood Analyte Meter and Accessory Therefor,” 42 pages, filed with USPTO prior to Oct. 2010.

* cited by examiner

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Harness, Dickey

(57) **CLAIM**

We claim the ornamental design for a hand-held blood glucose meter including ports, buttons and a display screen, as shown and described.

DESCRIPTION

FIG. 1 is a front perspective view of a hand-held blood glucose meter;

FIG. 2 is a rear perspective view thereof;

FIG. 3 is a side elevational view thereof;

FIG. 4 is a front elevational view thereof;

FIG. 5 is another side elevational view thereof;


FIG. 6 is an end view thereof;

FIG. 7 is another end view thereof; and,

FIG. 8 is a rear elevational view thereof.

The broken and dashed lines illustrate portions of the design that form no part of the claim.

1 Claim, 4 Drawing Sheets

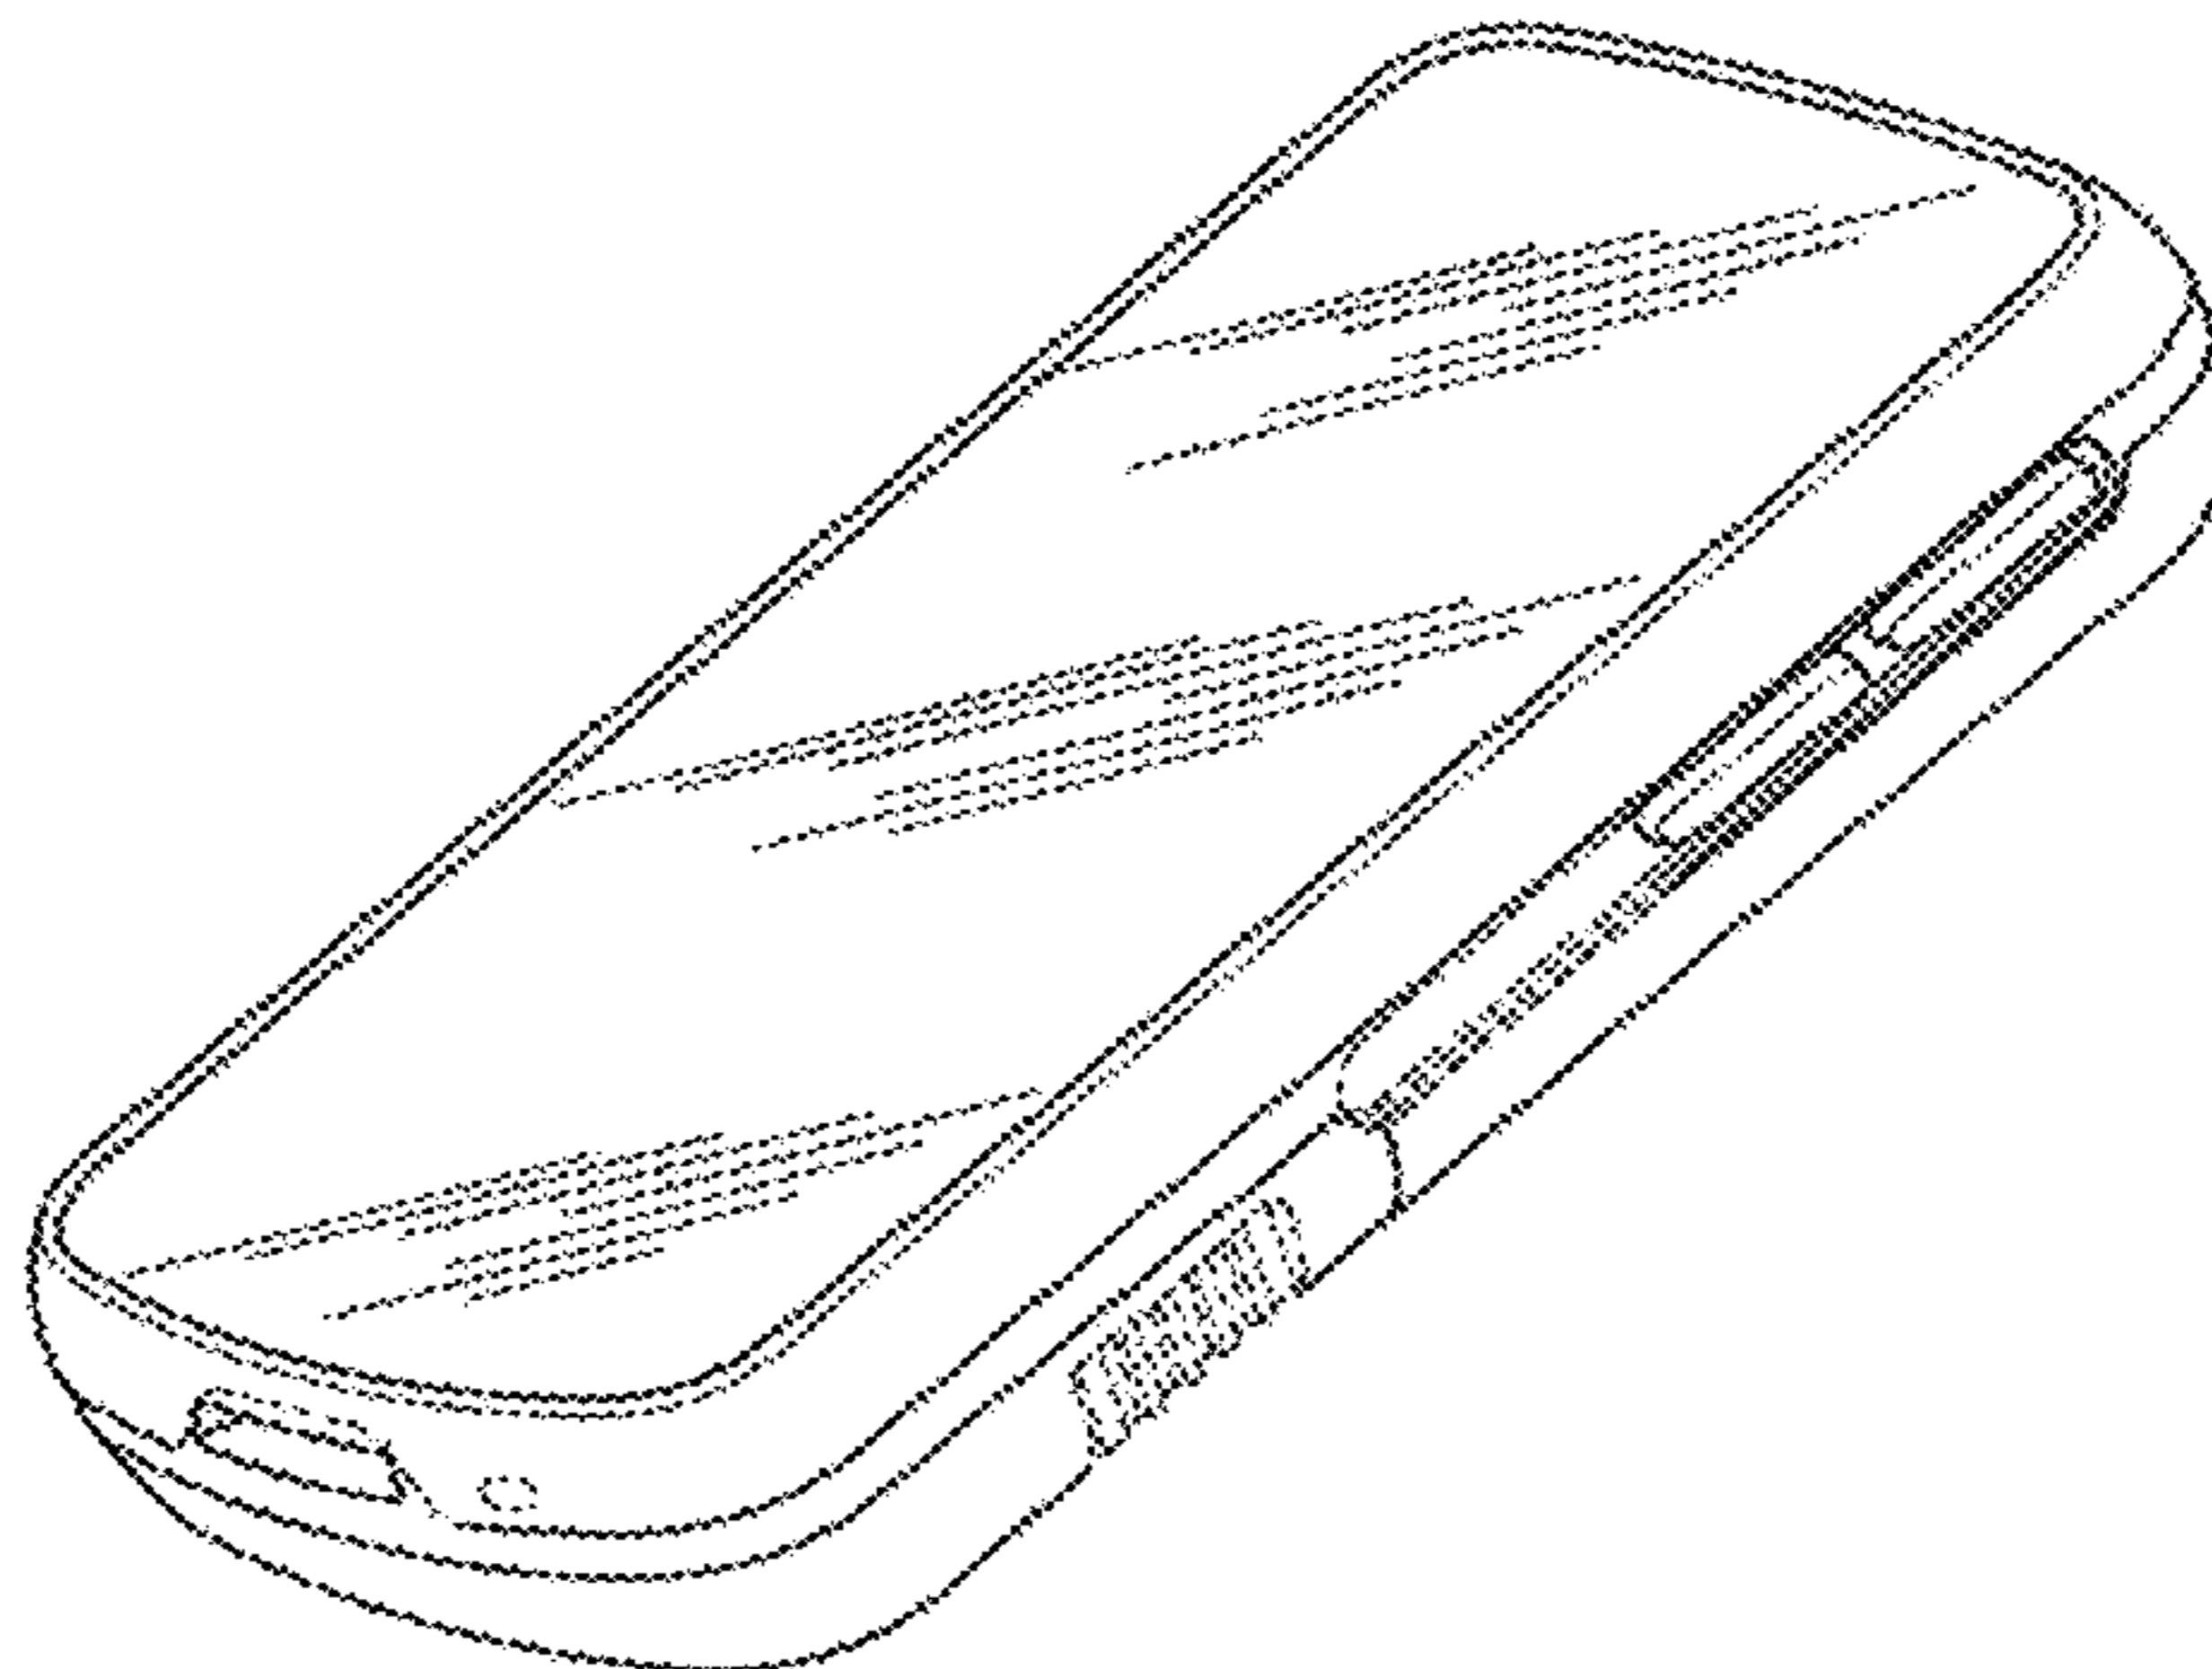

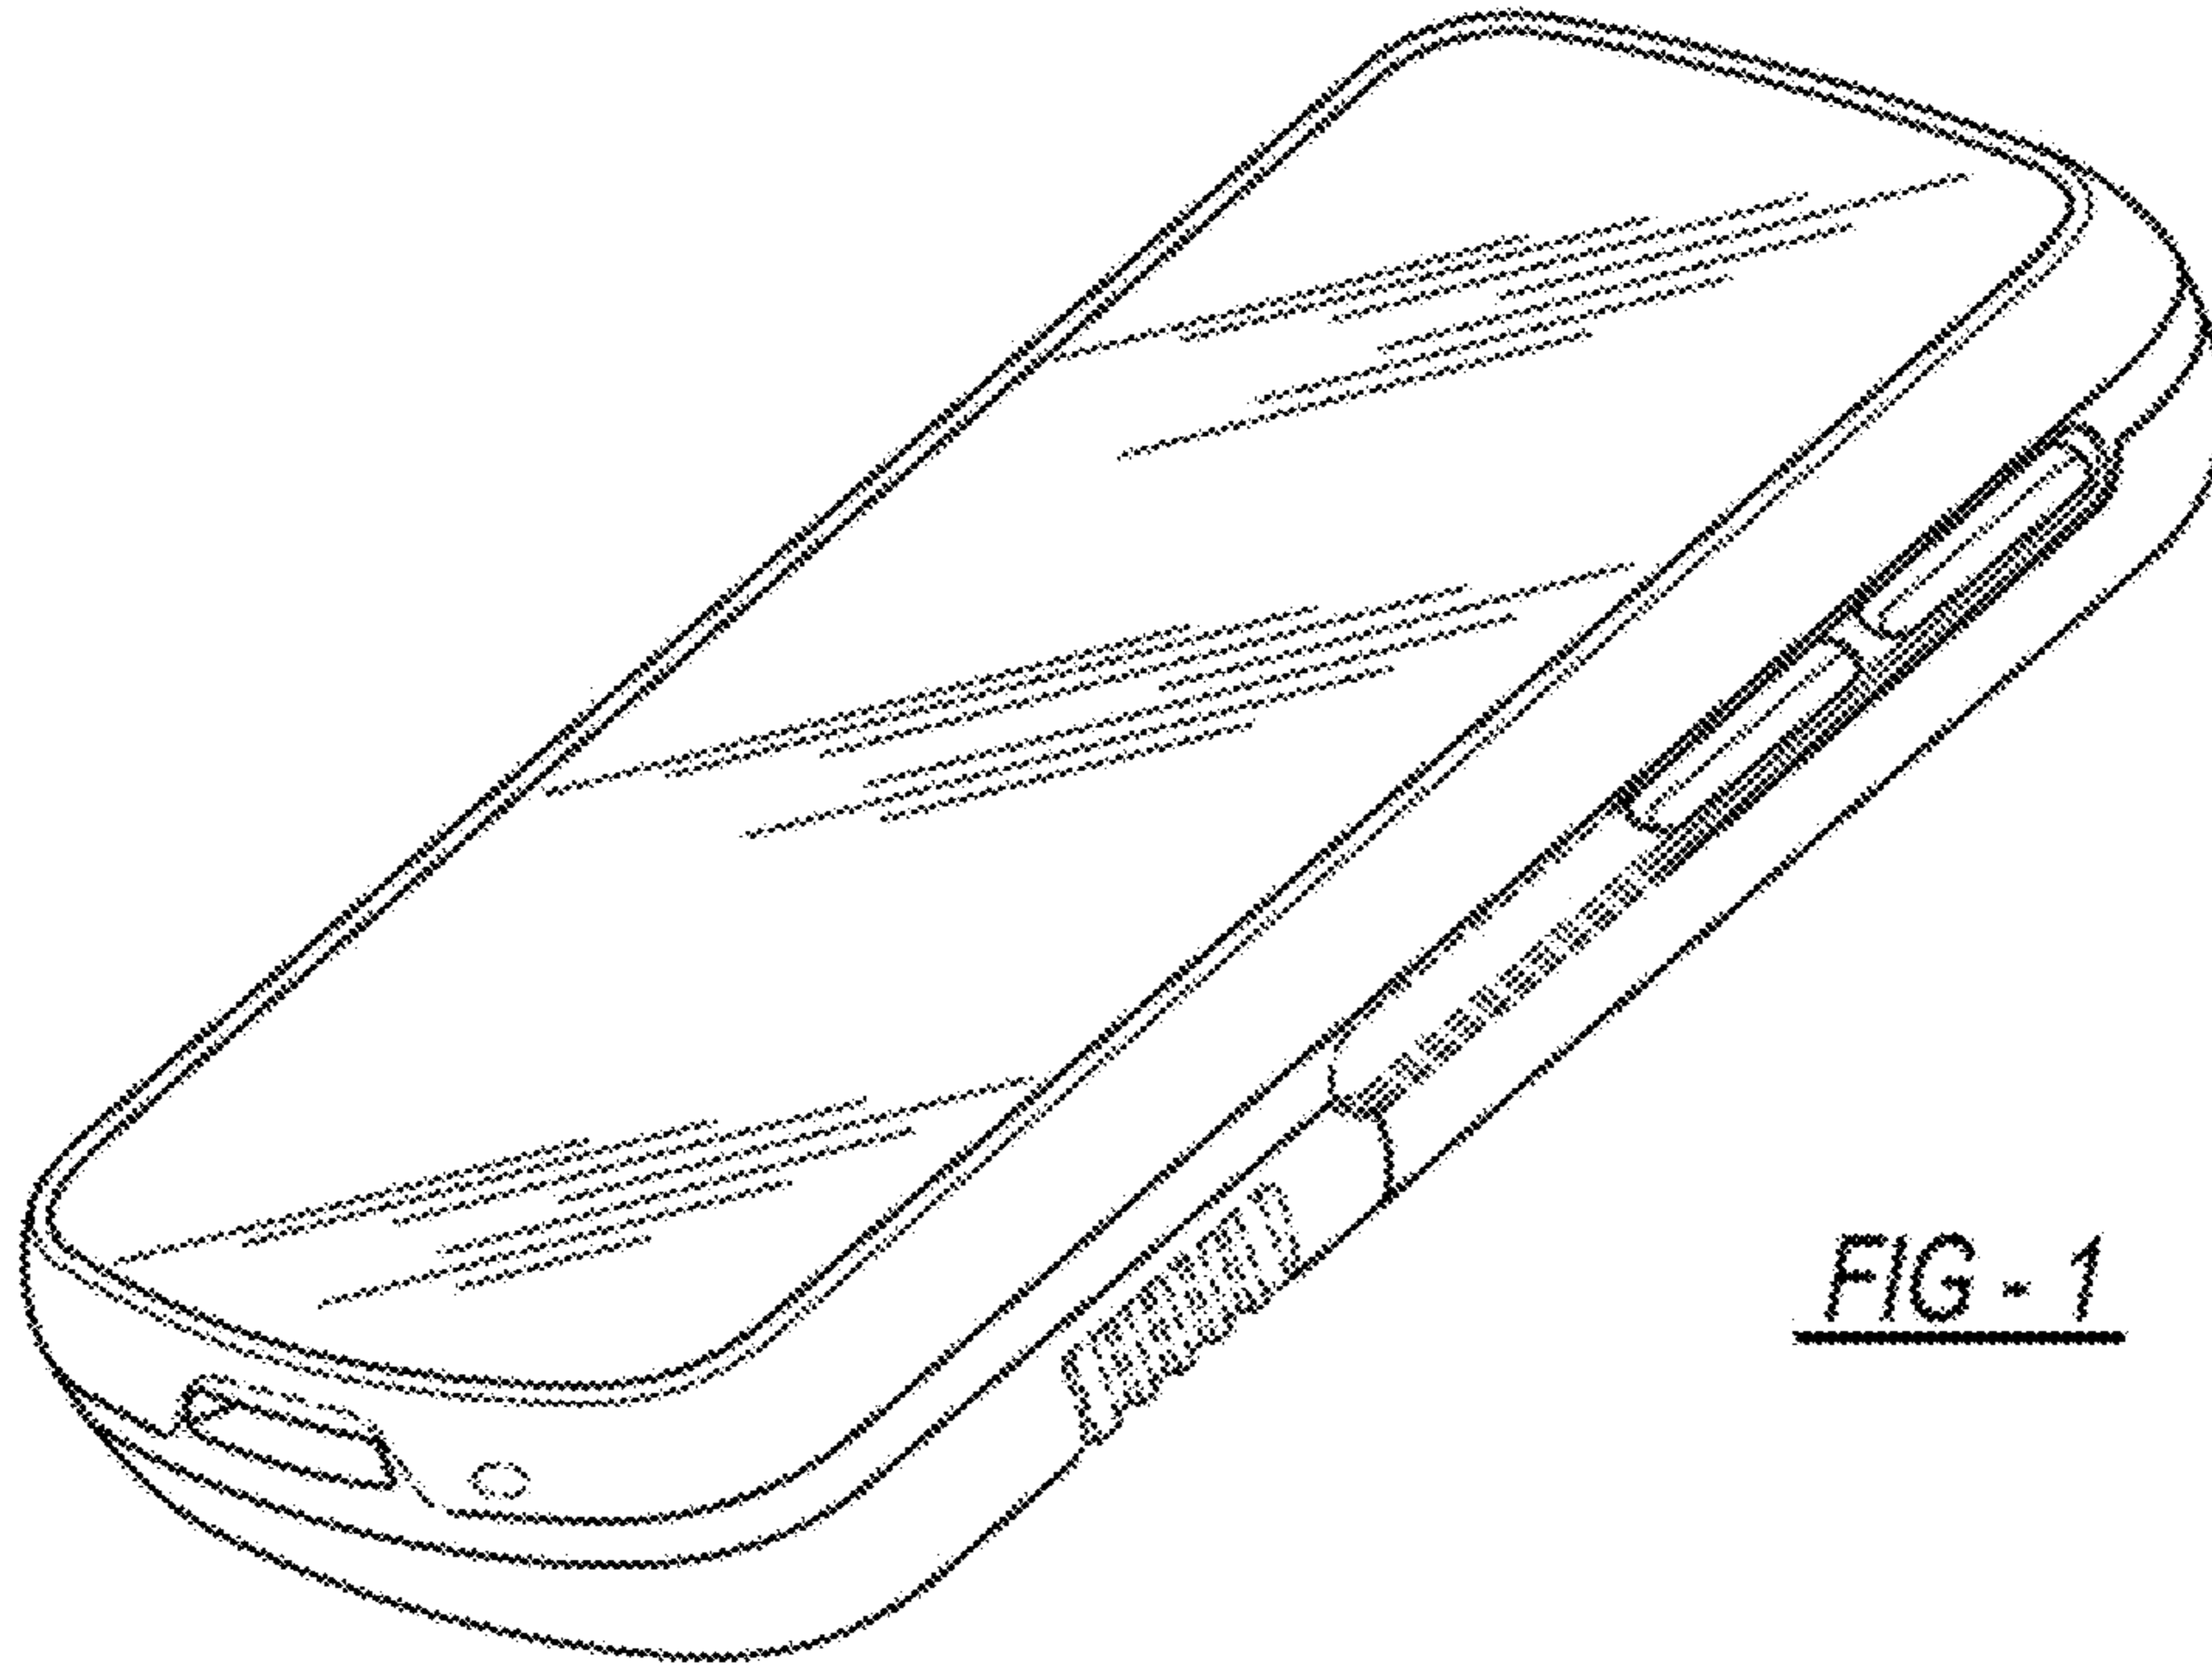


FIG - 1

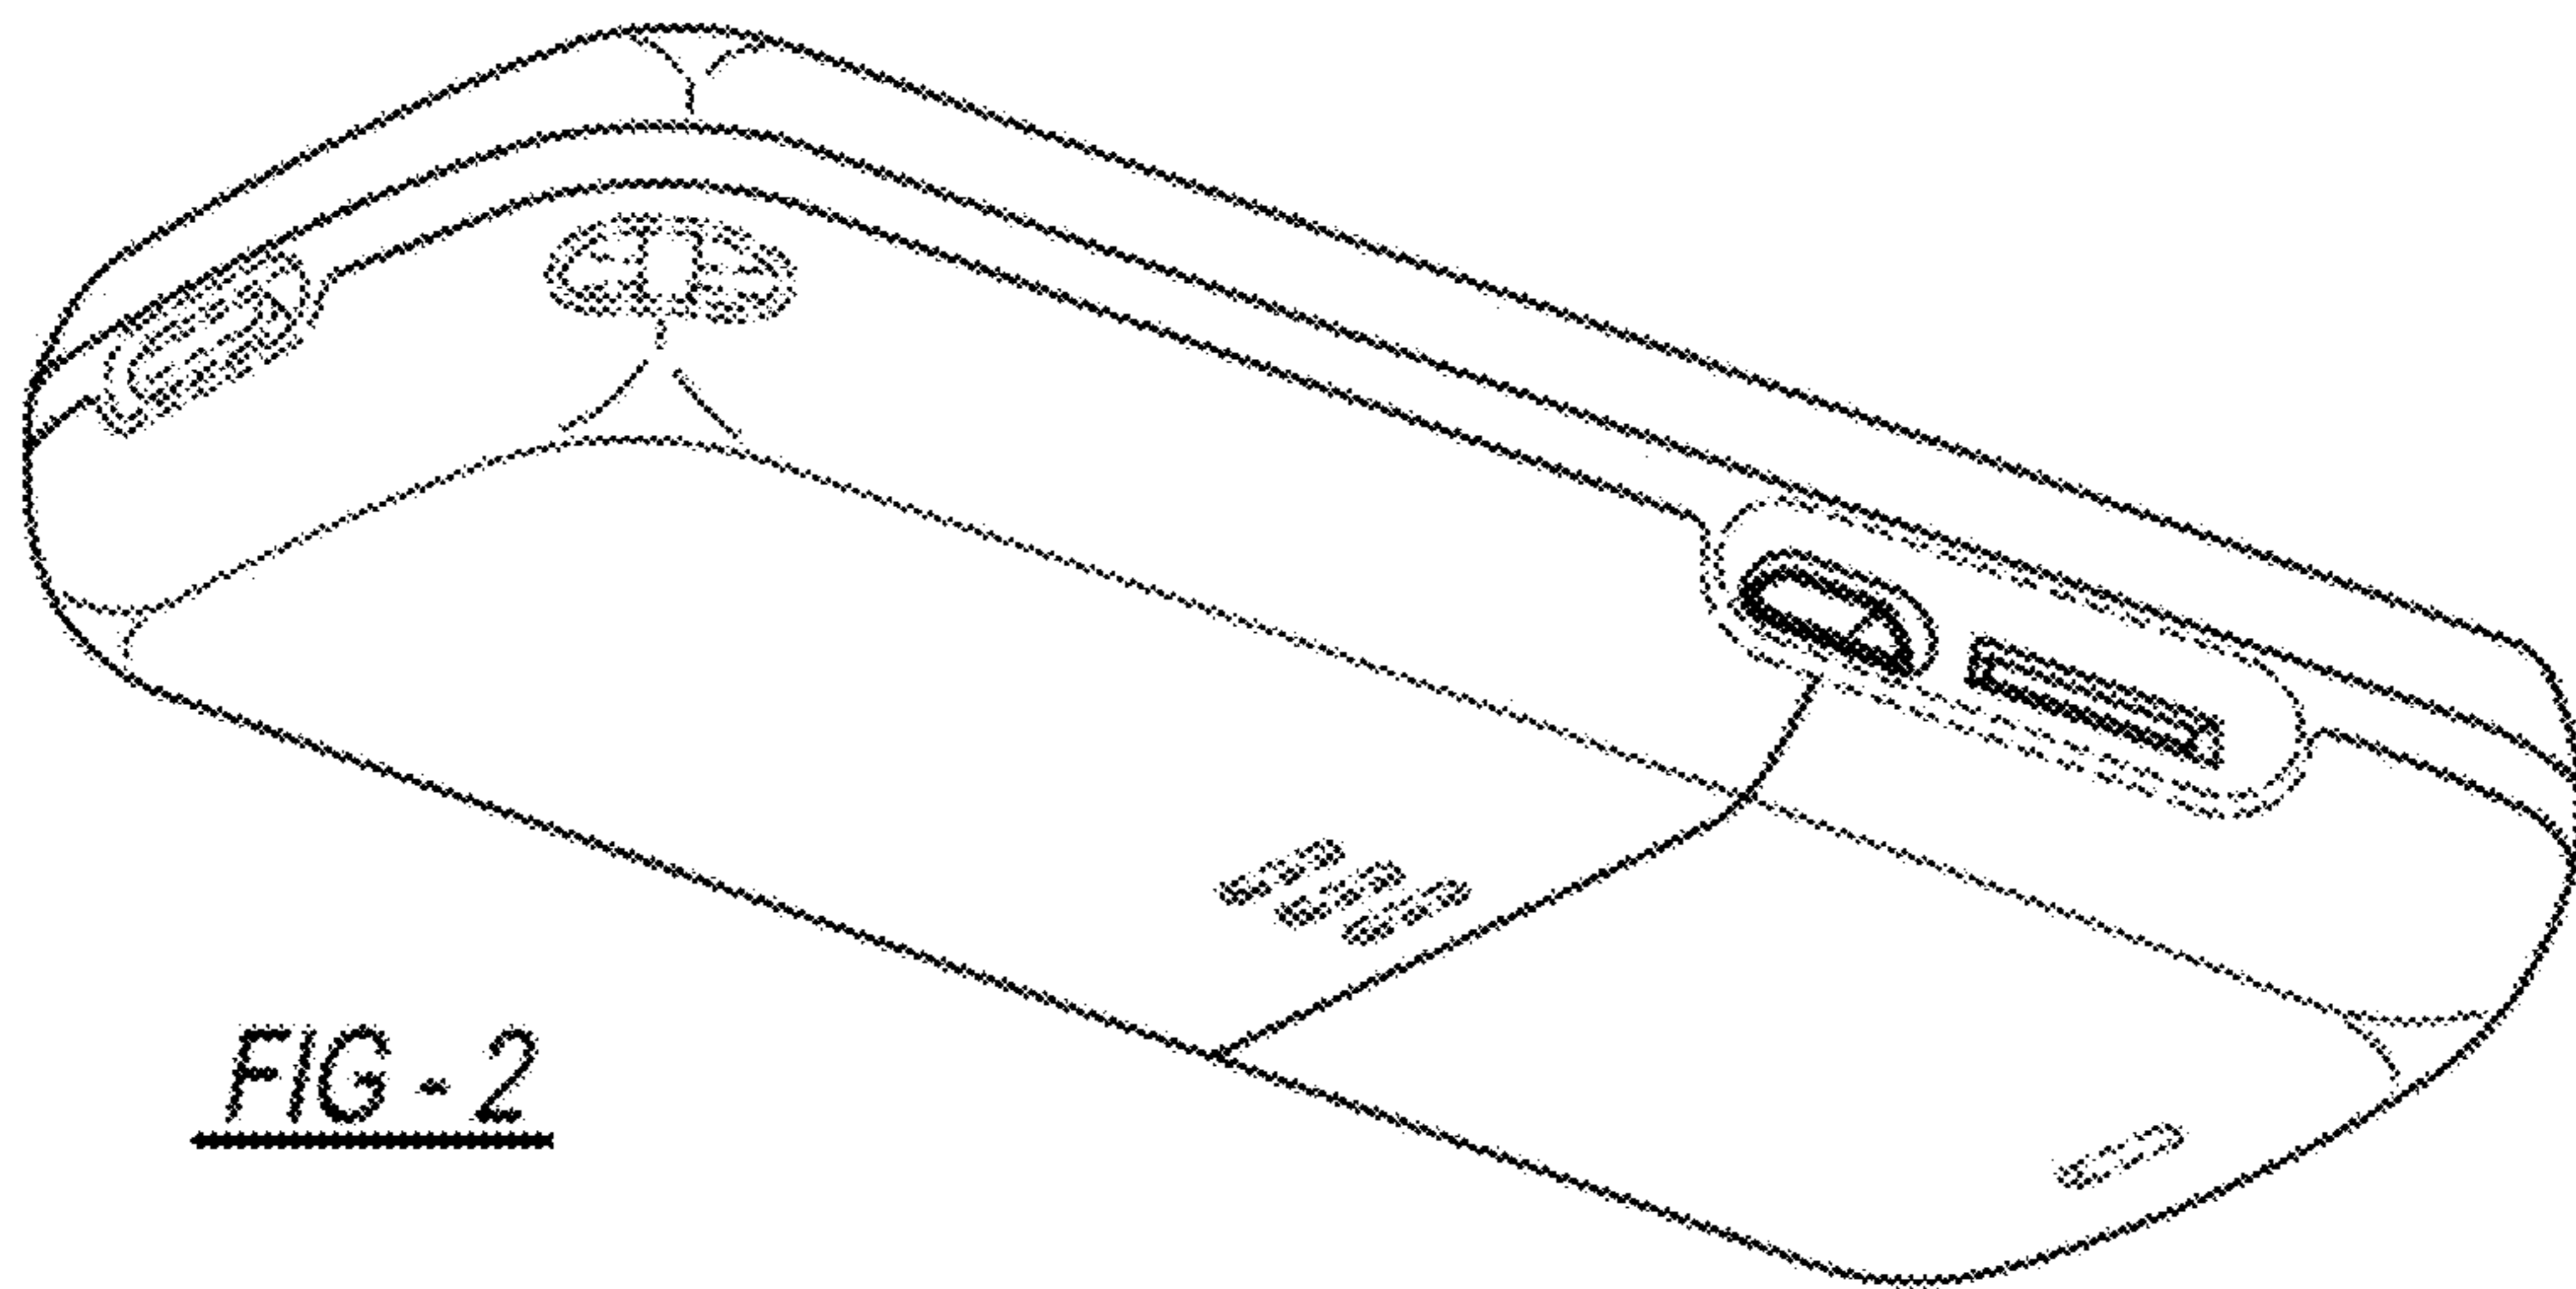


FIG - 2

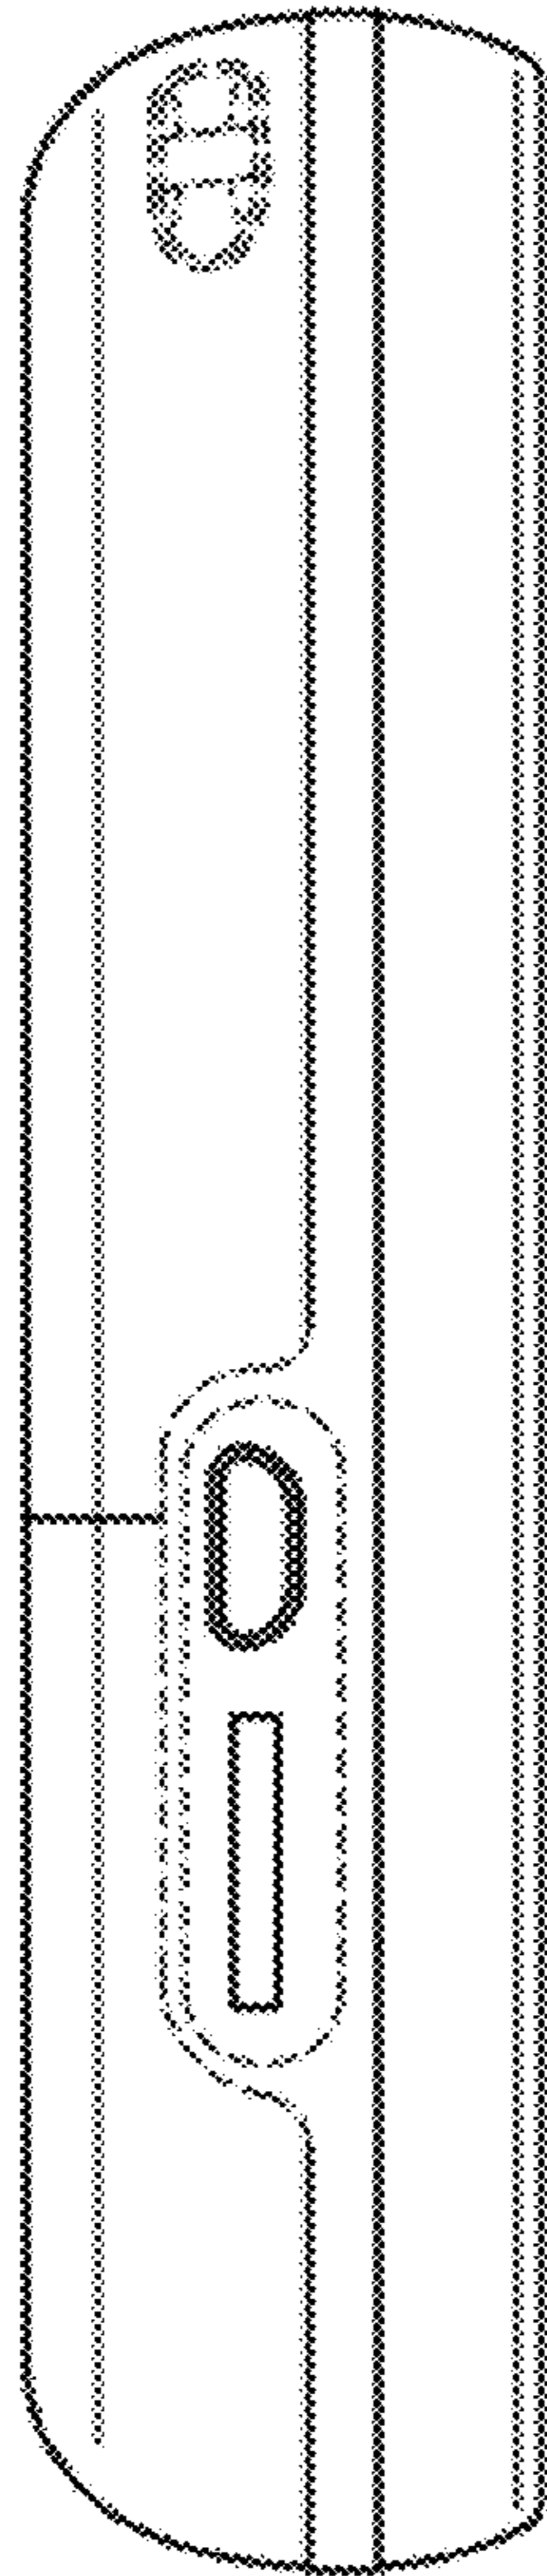


FIG - 3

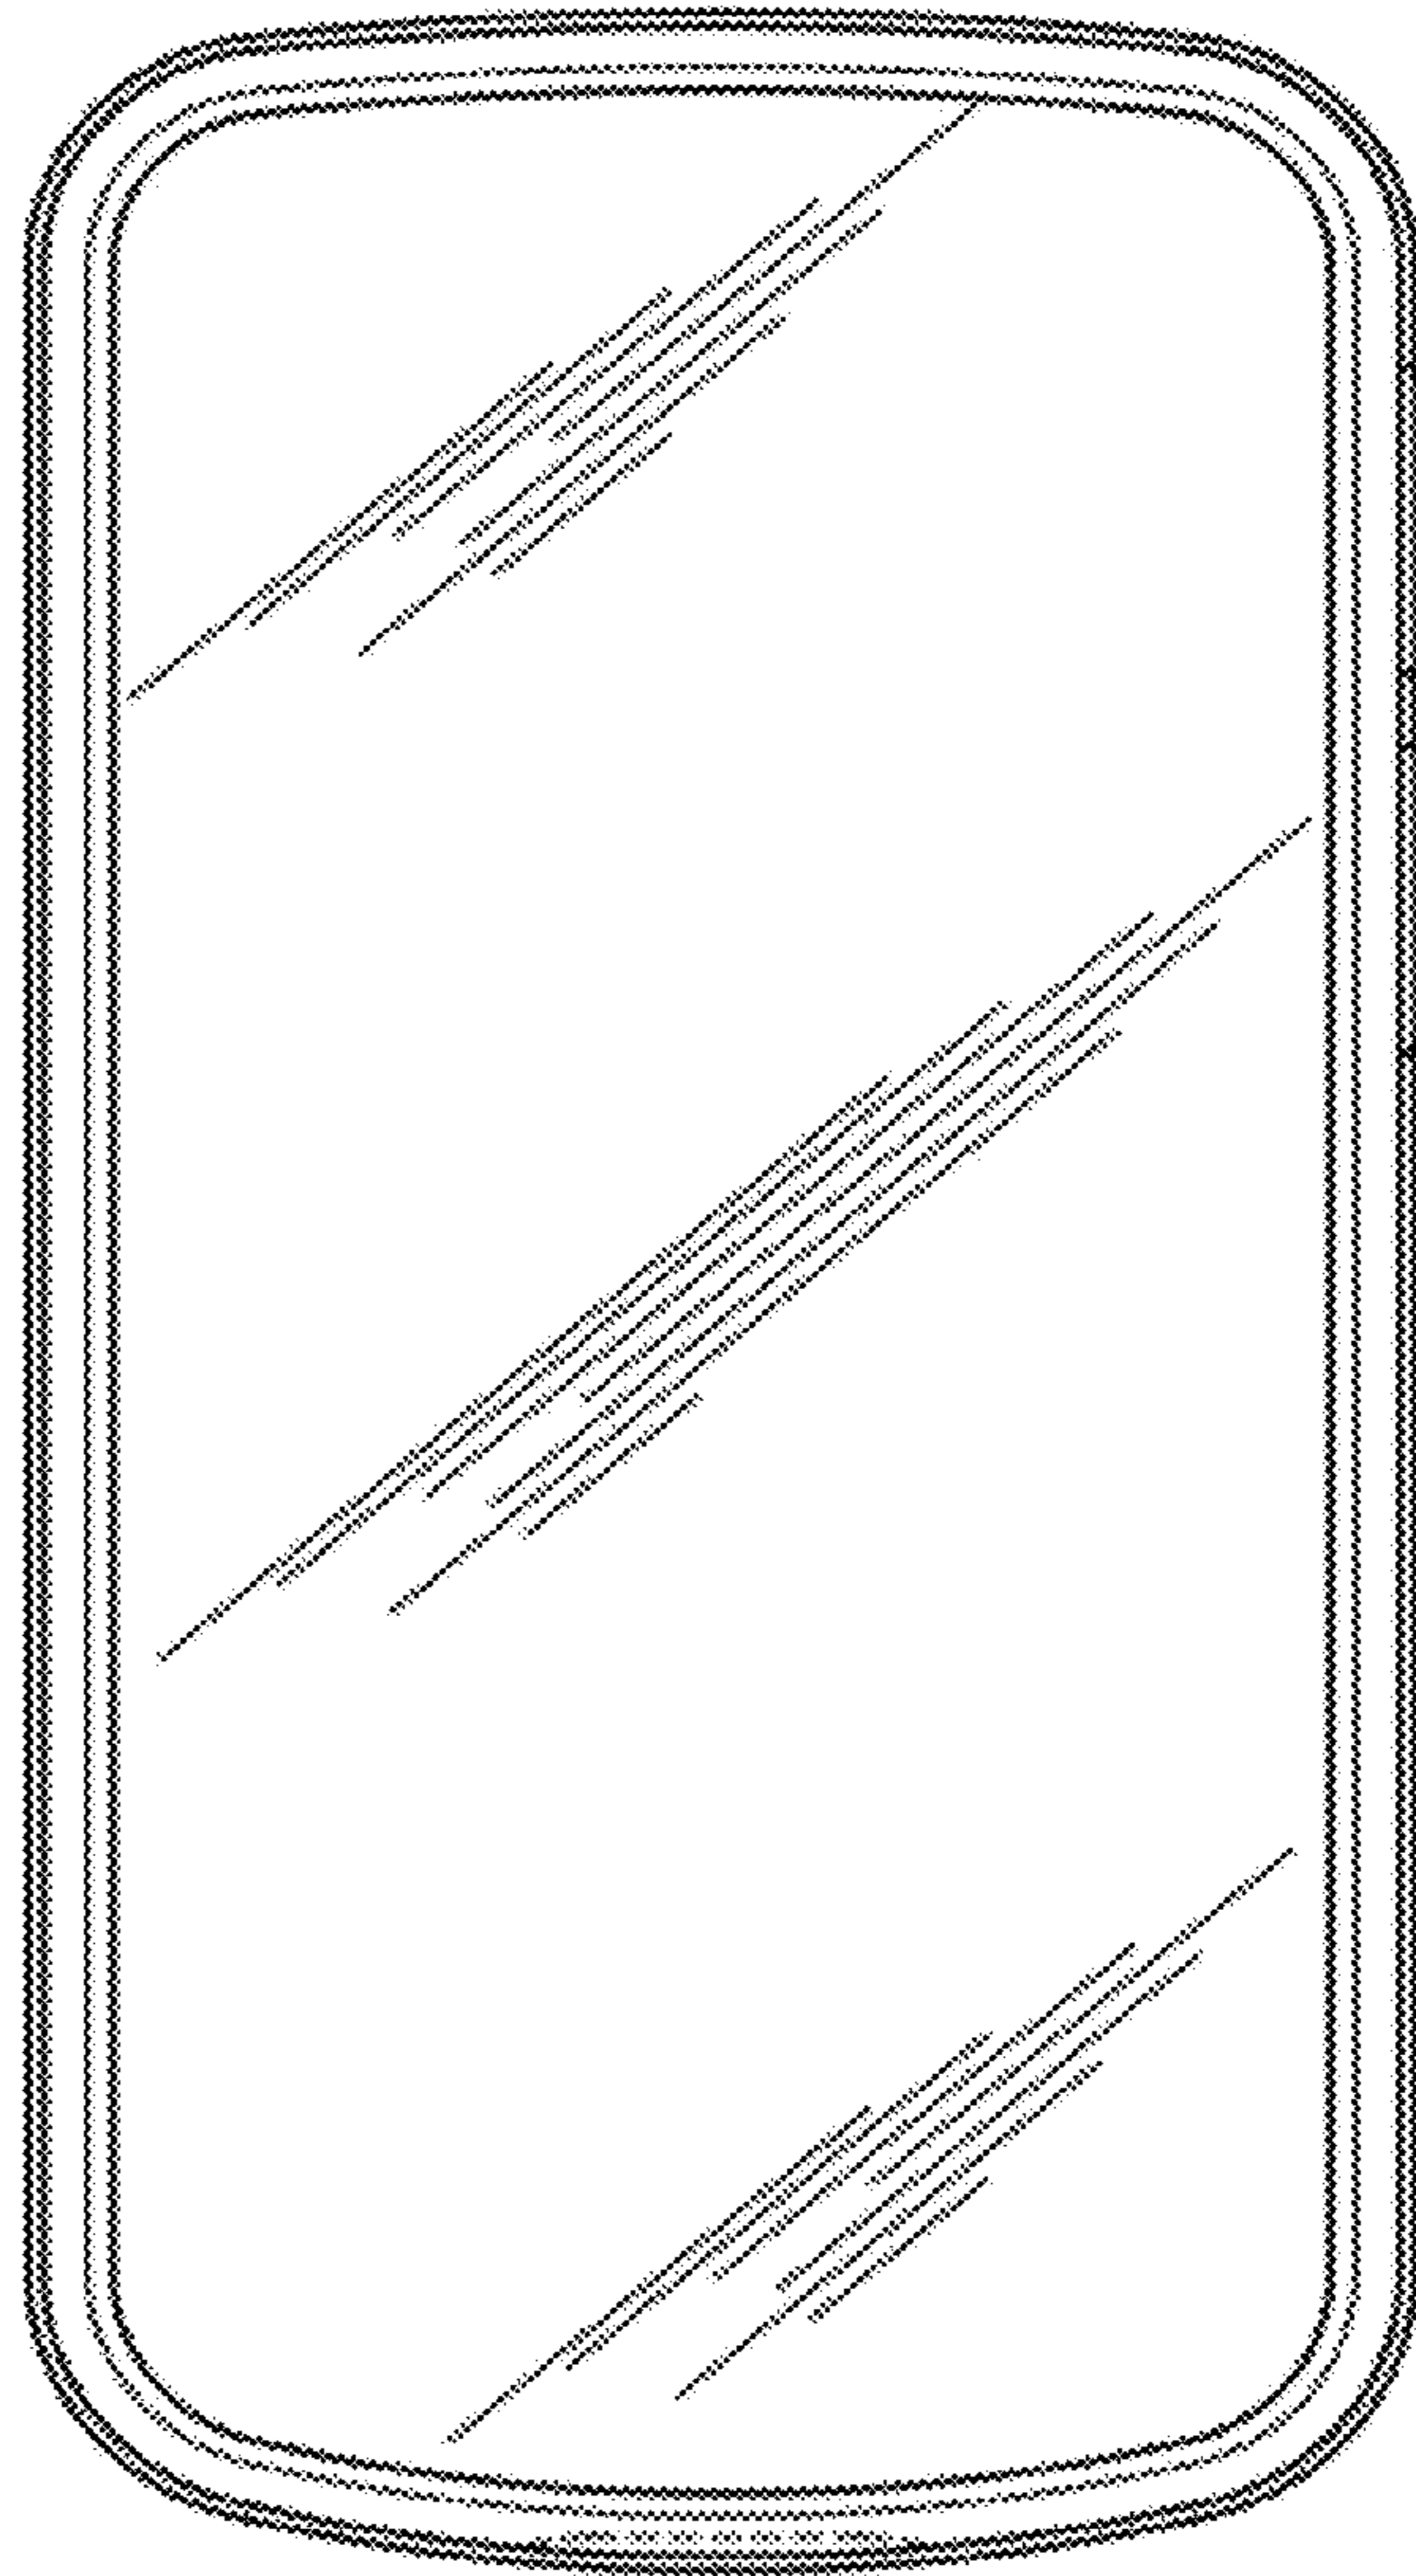


FIG - 4

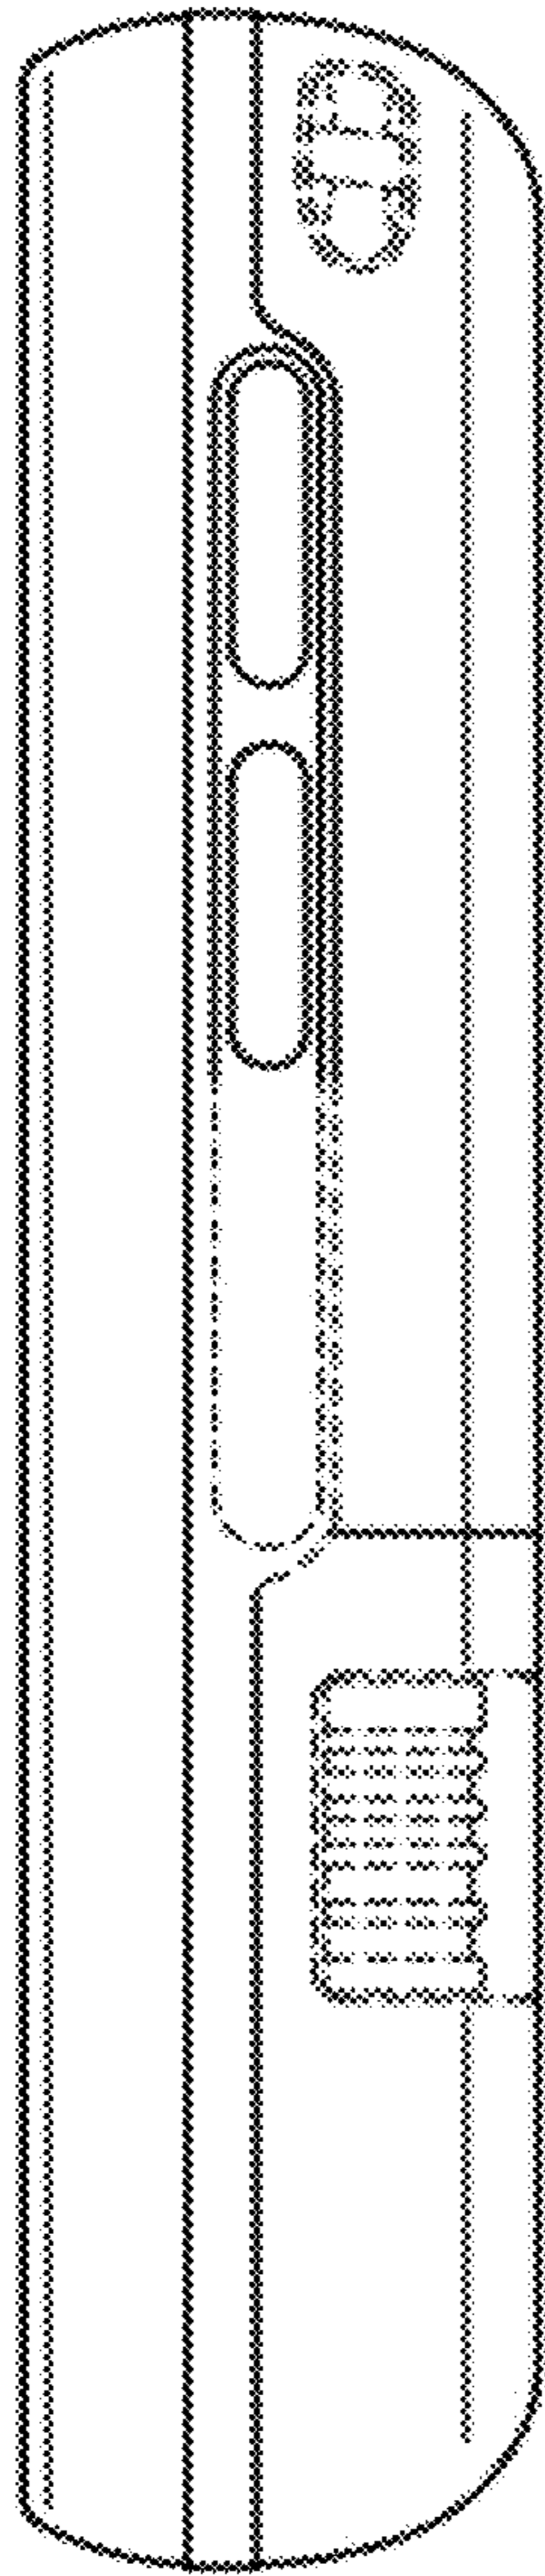


FIG - 5

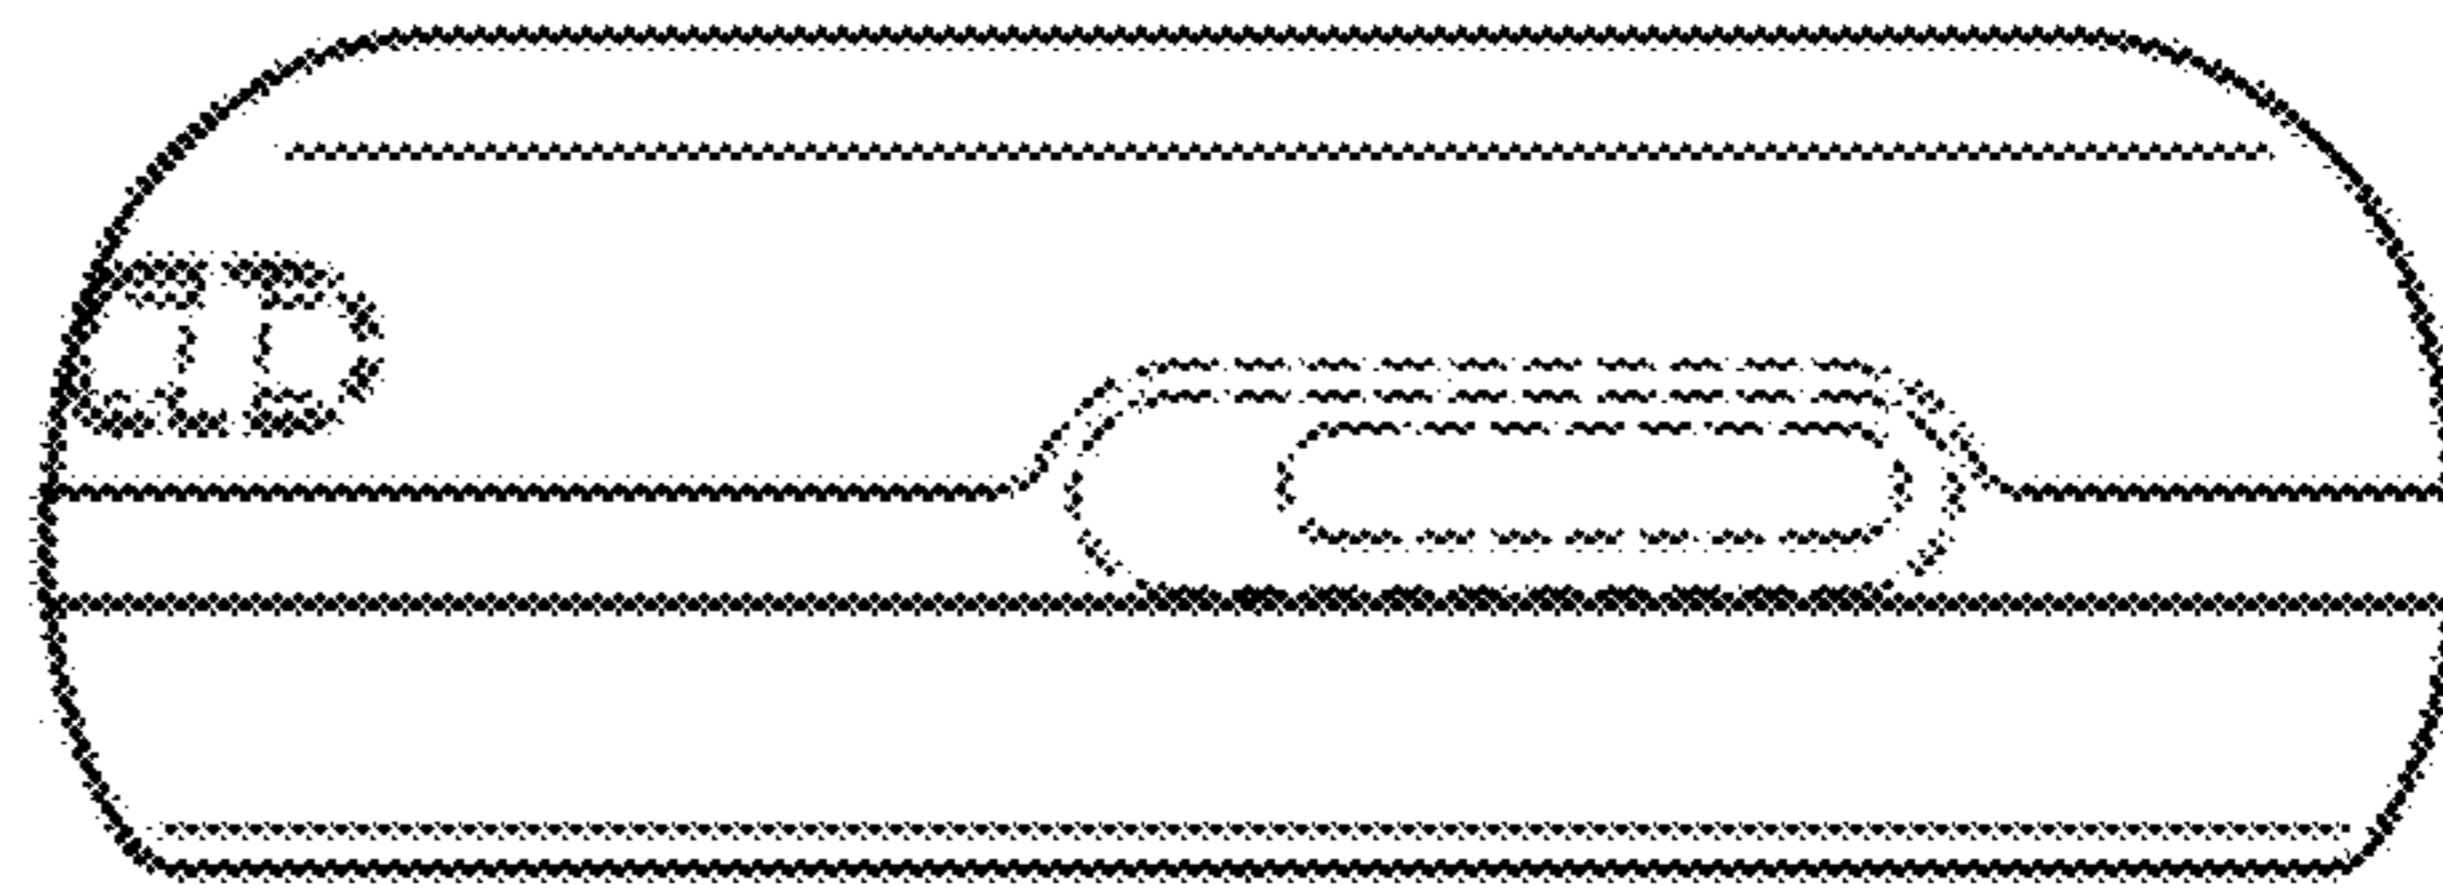


FIG - 6



FIG - 7

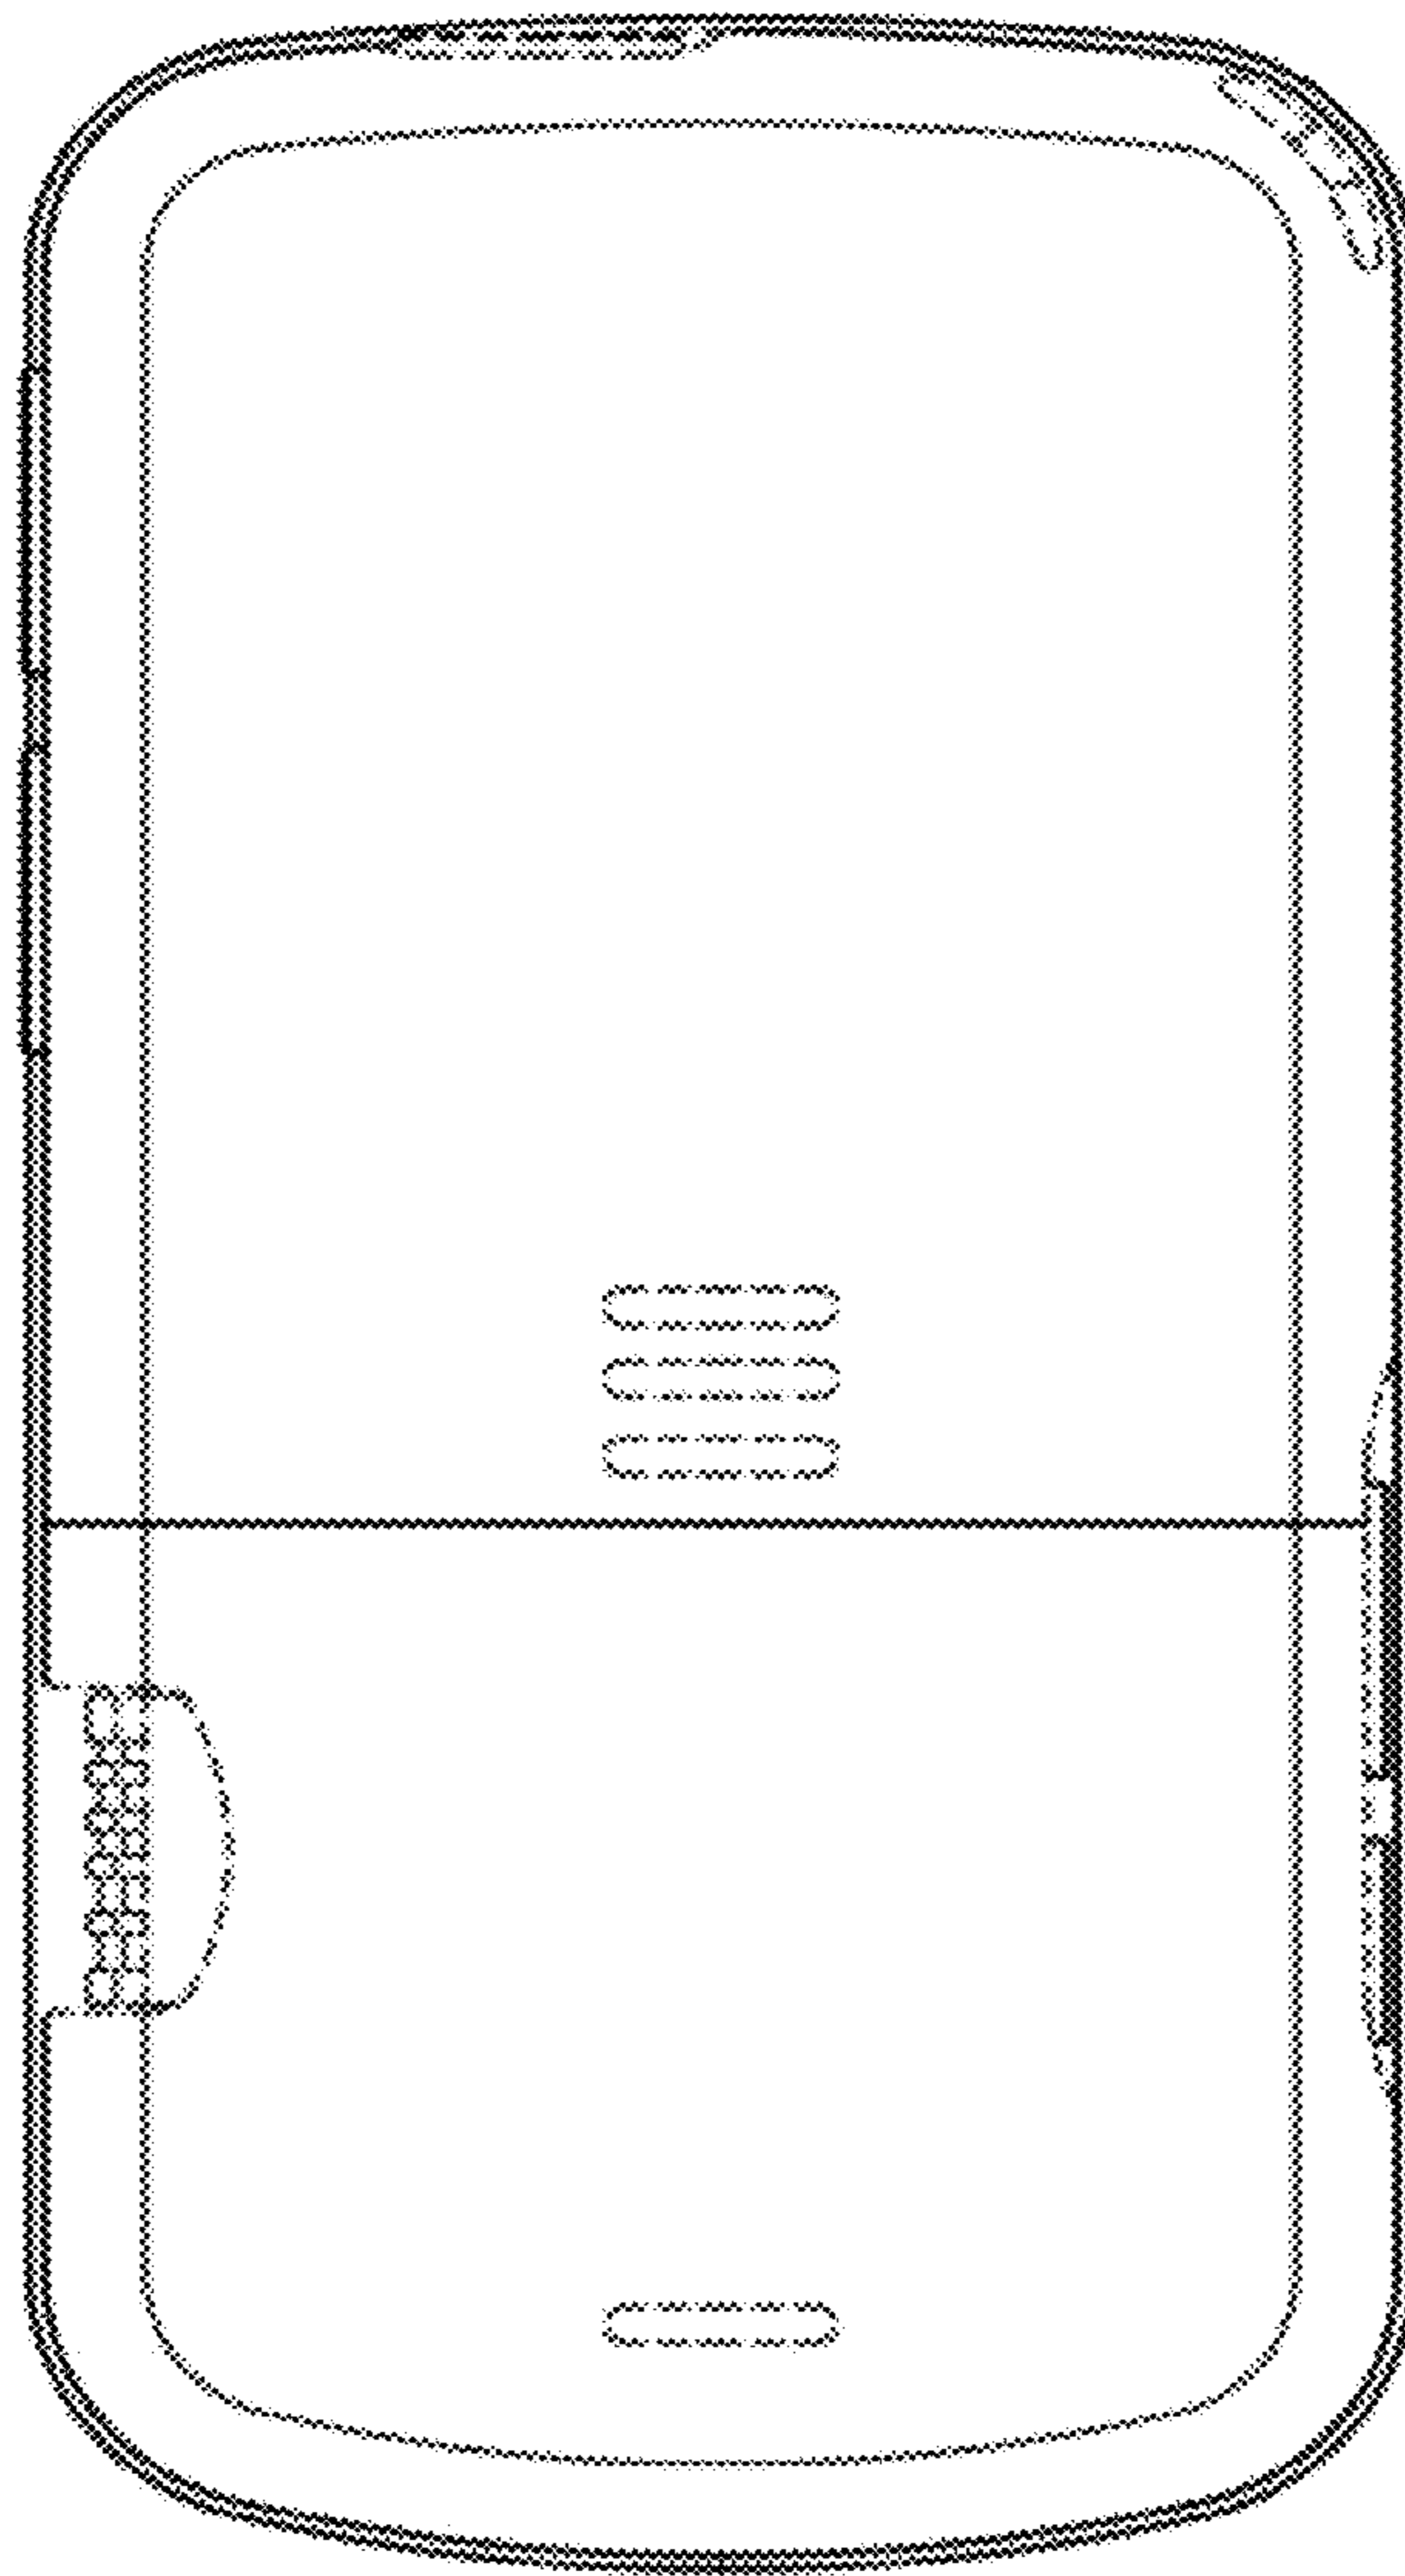


FIG - 8