



US00D663427S

(12) **United States Design Patent**
Sharps

(10) **Patent No.:** **US D663,427 S**
(45) **Date of Patent:** **** Jul. 10, 2012**

- (54) **TORSO-SUPPORT APPARATUS**
- (75) Inventor: **Lewis Sharps**, Bryn Mawr, PA (US)
- (73) Assignee: **Operating Room Safety Enterprises, LLC**, Berwyn, PA (US)
- (**) Term: **14 Years**
- (21) Appl. No.: **29/386,121**
- (22) Filed: **Feb. 24, 2011**

- 6,526,610 B1 3/2003 Hand et al.
- 6,622,324 B2 * 9/2003 VanSteenburg et al. 5/621
- 6,941,951 B2 9/2005 Hubert et al.
- 7,036,512 B2 5/2006 Harnois
- 7,137,160 B2 11/2006 Hand et al.
- 7,152,261 B2 12/2006 Jackson
- 7,197,778 B2 4/2007 Sharps
- 7,343,635 B2 3/2008 Jackson
- 7,343,916 B2 3/2008 Biondo et al.
- 7,520,008 B2 4/2009 Wong et al.
- 7,600,281 B2 * 10/2009 Skripps 5/621
- D604,422 S * 11/2009 Albrecht et al. D24/183
- 7,614,639 B2 11/2009 Tholkes et al.

(Continued)

Related U.S. Application Data

- (63) Continuation-in-part of application No. 12/905,018, filed on Oct. 14, 2010.
 - (51) **LOC (9) Cl.** **24-01**
 - (52) **U.S. Cl.** **D24/184**
 - (58) **Field of Classification Search** D24/183-184, D24/171; D6/360, 392; 5/600, 608, 610, 5/613-614, 621-624, 632; 602/32; 128/845-846; 606/242
- See application file for complete search history.

OTHER PUBLICATIONS

Allen Medical Systems, "Intraoperative Adjustment from Kyphosis to Lordosis", Announcement Allen Medical Systems, Feb. 6, 2006, pp. 1-4.

(Continued)

Primary Examiner — T. Chase Nelson
Assistant Examiner — Mark Cavanna
(74) *Attorney, Agent, or Firm* — Offit Kurman, P.A.; Robert R. Axenfeld

(56) **References Cited**

U.S. PATENT DOCUMENTS

- 3,750,659 A 8/1973 Loomans
- 4,029,089 A 6/1977 Mulholland
- D248,406 S * 7/1978 Hodge D6/360
- 4,296,761 A 10/1981 Tyo
- 4,354,485 A * 10/1982 Safadago 606/242
- 4,827,541 A * 5/1989 Vollman et al. 5/613
- D304,614 S * 11/1989 Guttormsen D24/183
- D307,055 S 4/1990 Johnston
- D320,663 S * 10/1991 Brann D24/183
- 5,088,706 A * 2/1992 Jackson 5/608
- 5,131,106 A 7/1992 Jackson
- D344,802 S * 3/1994 Kuck et al. D24/183
- D347,604 S 6/1994 Ernst et al.
- D356,527 S 3/1995 Wohnsen et al.
- 5,489,258 A 2/1996 Wohnsen et al.
- 5,618,055 A 4/1997 Mulholland
- 6,076,525 A * 6/2000 Hoffman 128/845
- 6,154,901 A 12/2000 Carr
- 6,428,497 B1 * 8/2002 Crouch 602/32


(57) **CLAIM**

The ornamental design for a torso-support apparatus, as shown and described.

DESCRIPTION

FIG. 1 is a top-isometric-view of an exemplary torso-support apparatus;
FIG. 2 a bottom-isometric-view thereof;
FIG. 3 is a right-side view thereof;
FIG. 4 is head-end-side view thereof;
FIG. 5 is a foot-end-side view thereof;
FIG. 6 is top-view thereof; and,
FIG. 7 is bottom-view thereof.
The broken lines showing the apparatus, or portion thereof, is not a part of the claimed design.

1 Claim, 4 Drawing Sheets

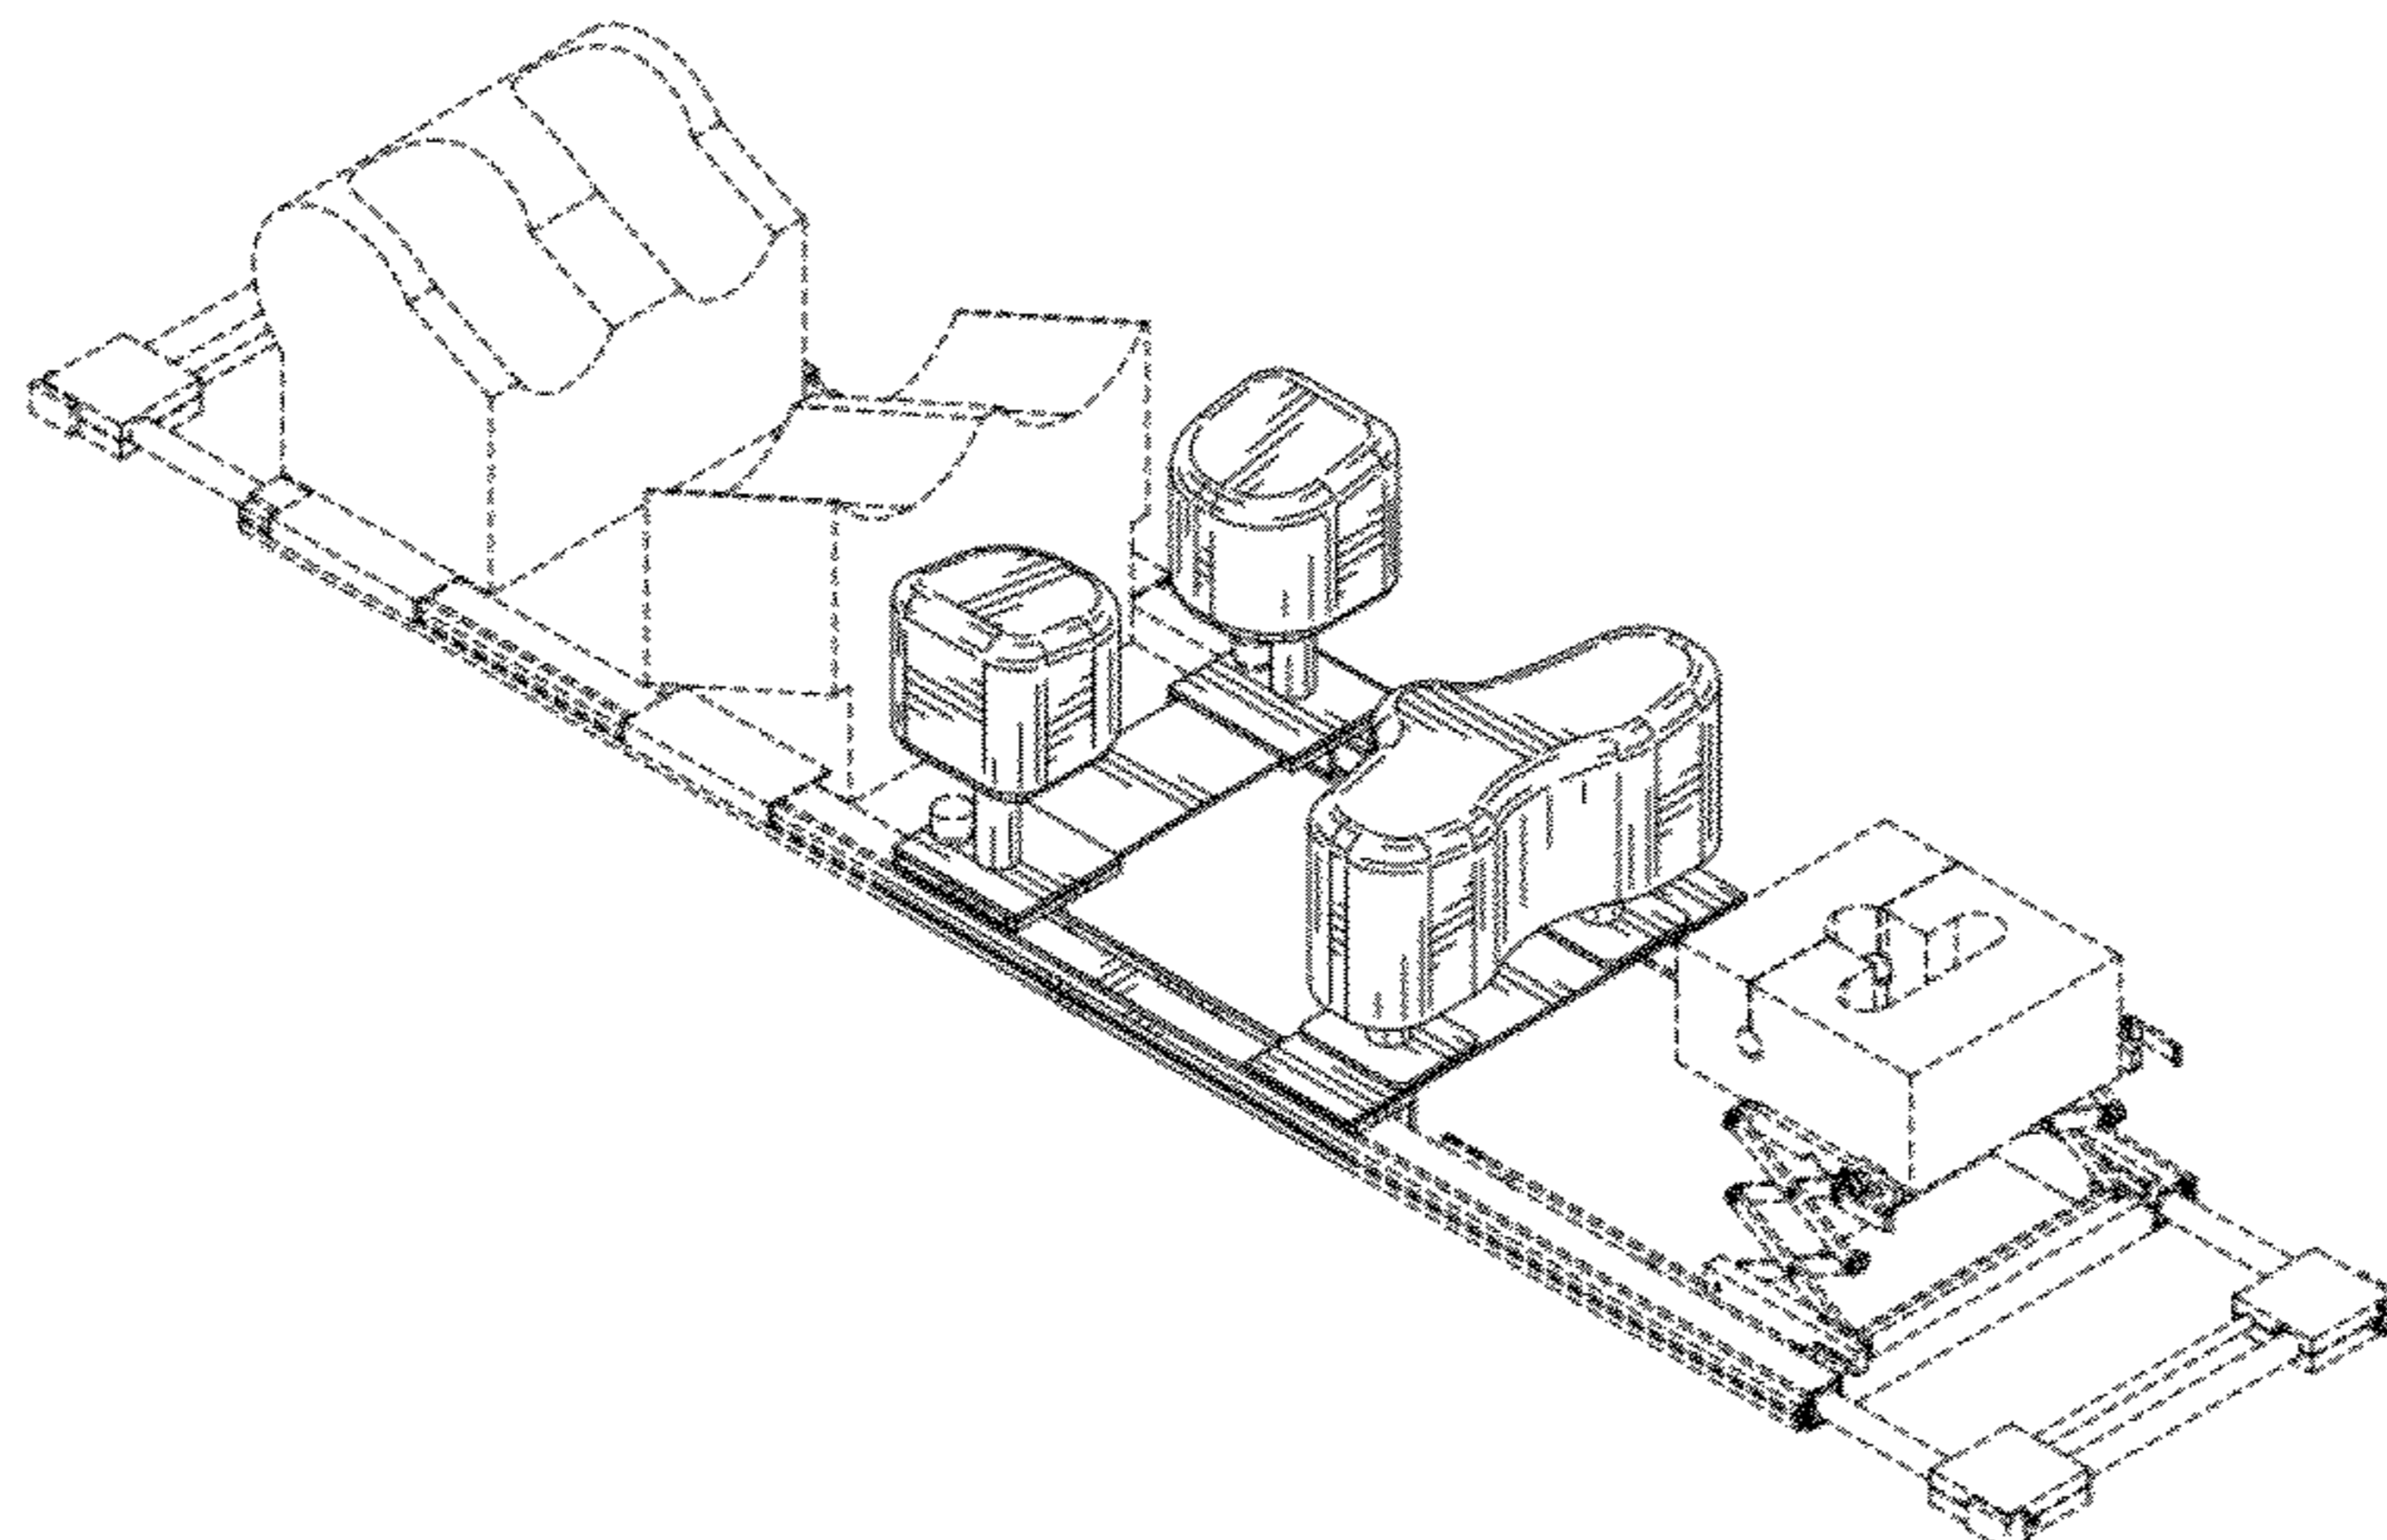

US D663,427 S

Page 2

U.S. PATENT DOCUMENTS

D612,942	S	3/2010	Verdon-Roe
2006/0242765	A1	11/2006	Skripps et al.
2007/0192960	A1	8/2007	Jackson
2009/0282614	A1	11/2009	Jackson
2010/0024128	A1	2/2010	Skripps

OTHER PUBLICATIONS

PCT Search Report mailed Feb. 17, 2011 for PCT Application No. PCT/US2010/052740.
"Radiolucent Wilson Frame", Orthopedic Systems, Inc. (OSI),
Poster, 1998, 1 page.

* cited by examiner

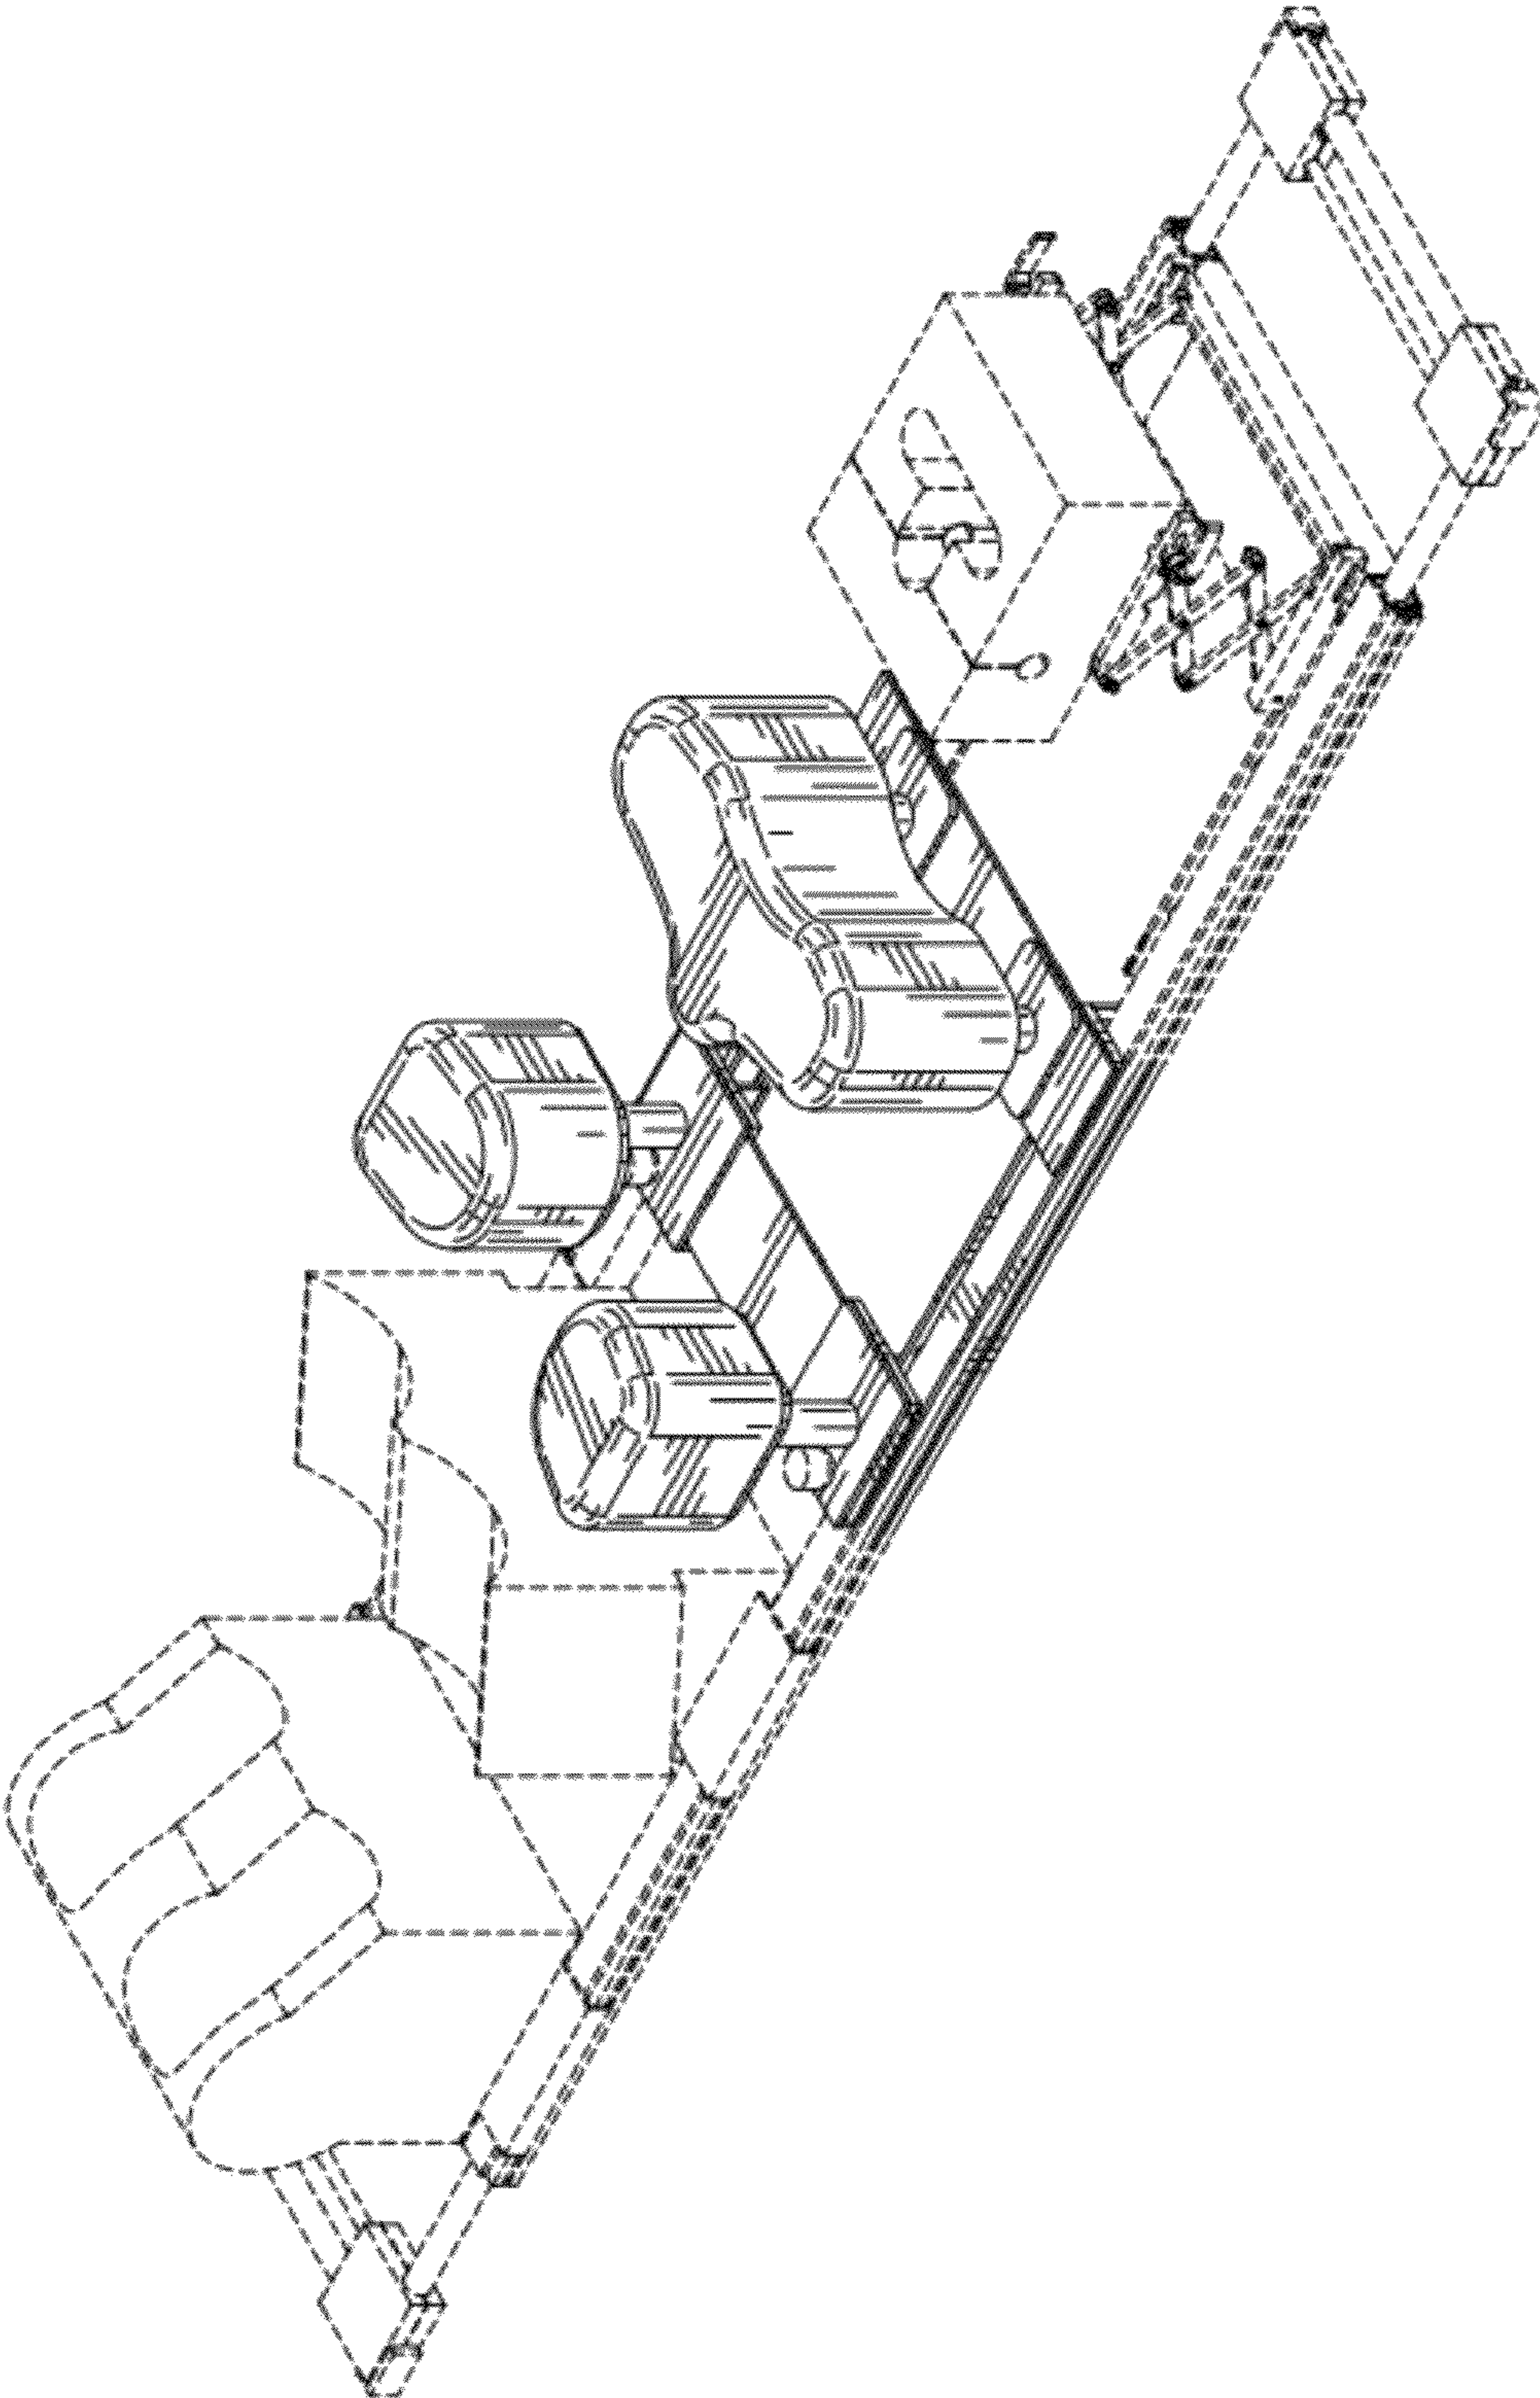


FIG. 1

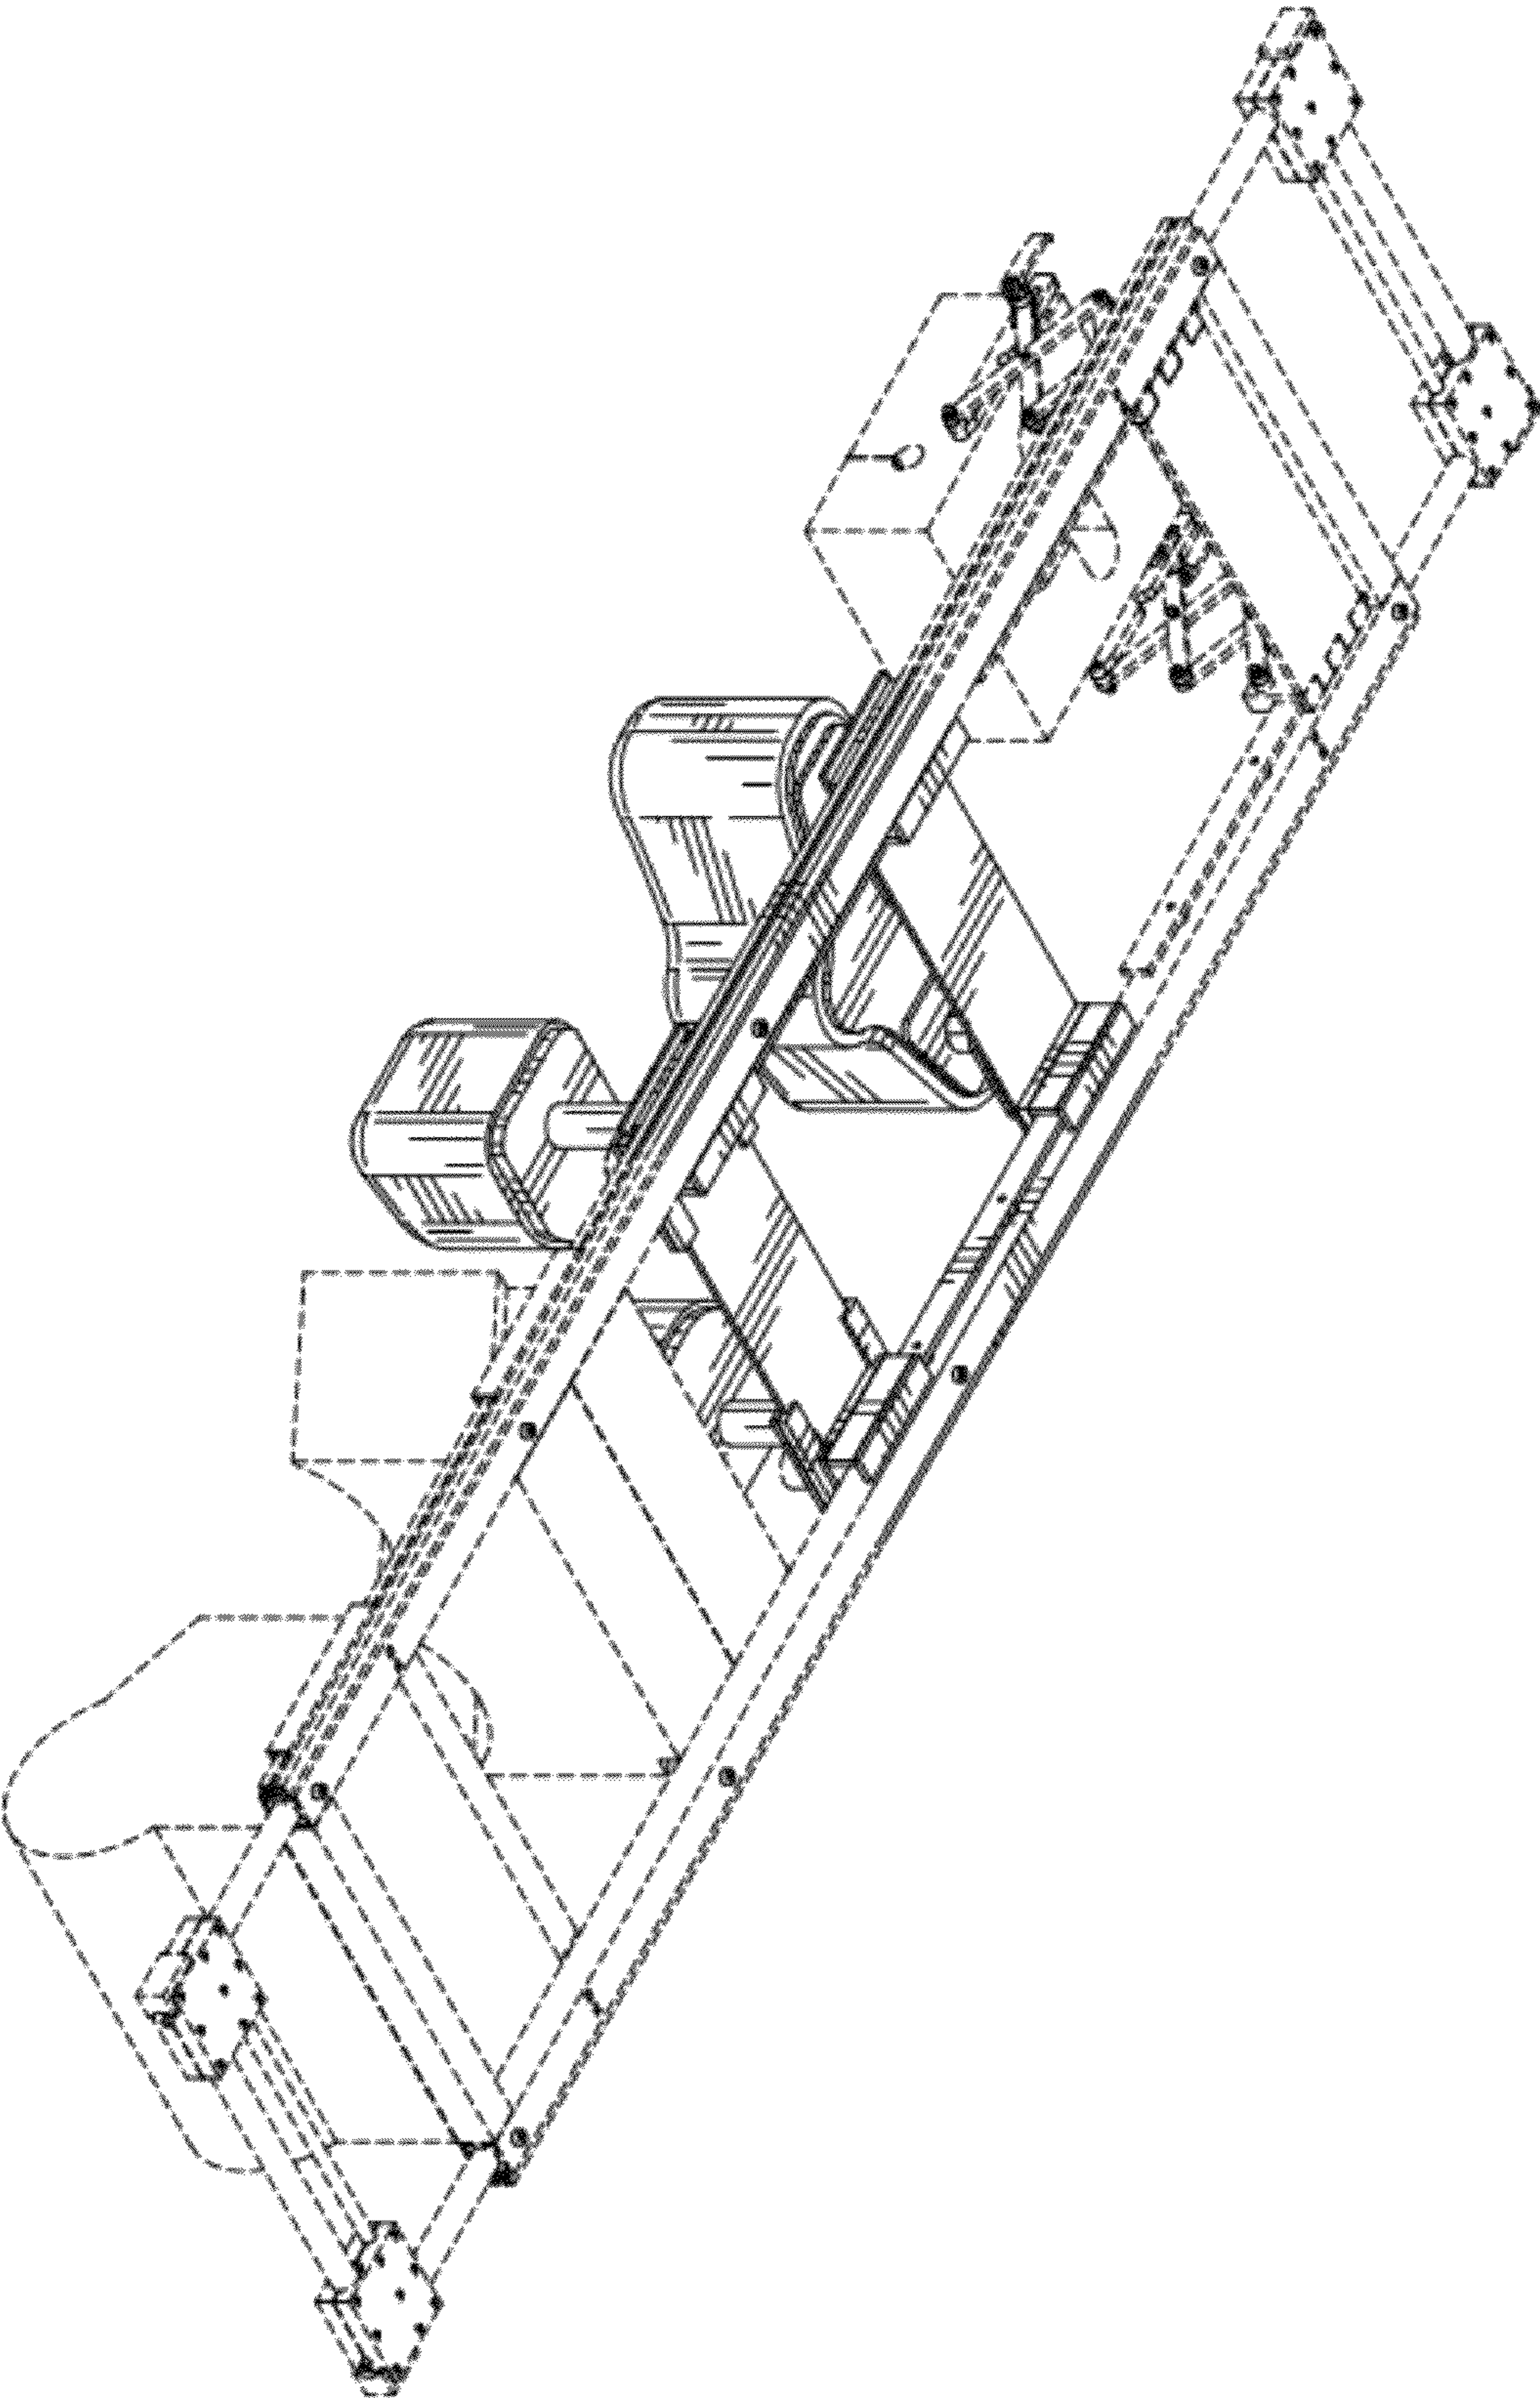


FIG. 2

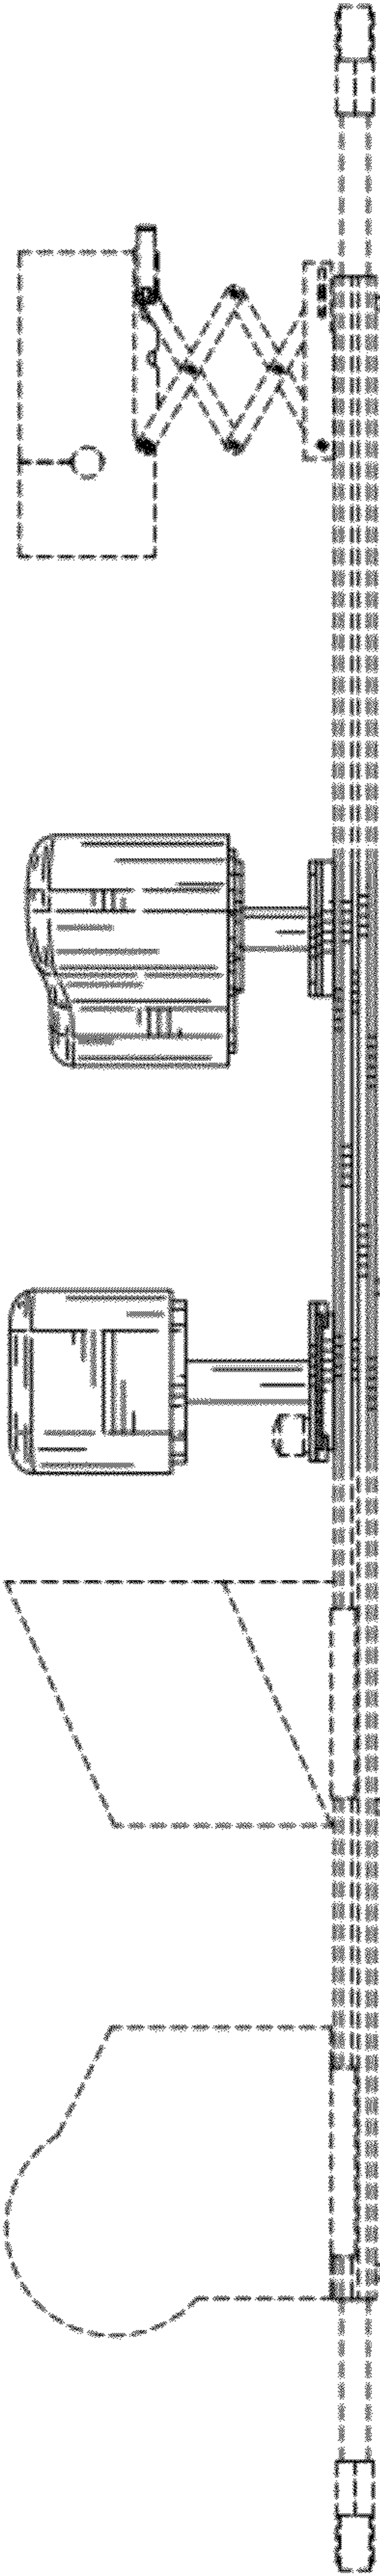


FIG. 3

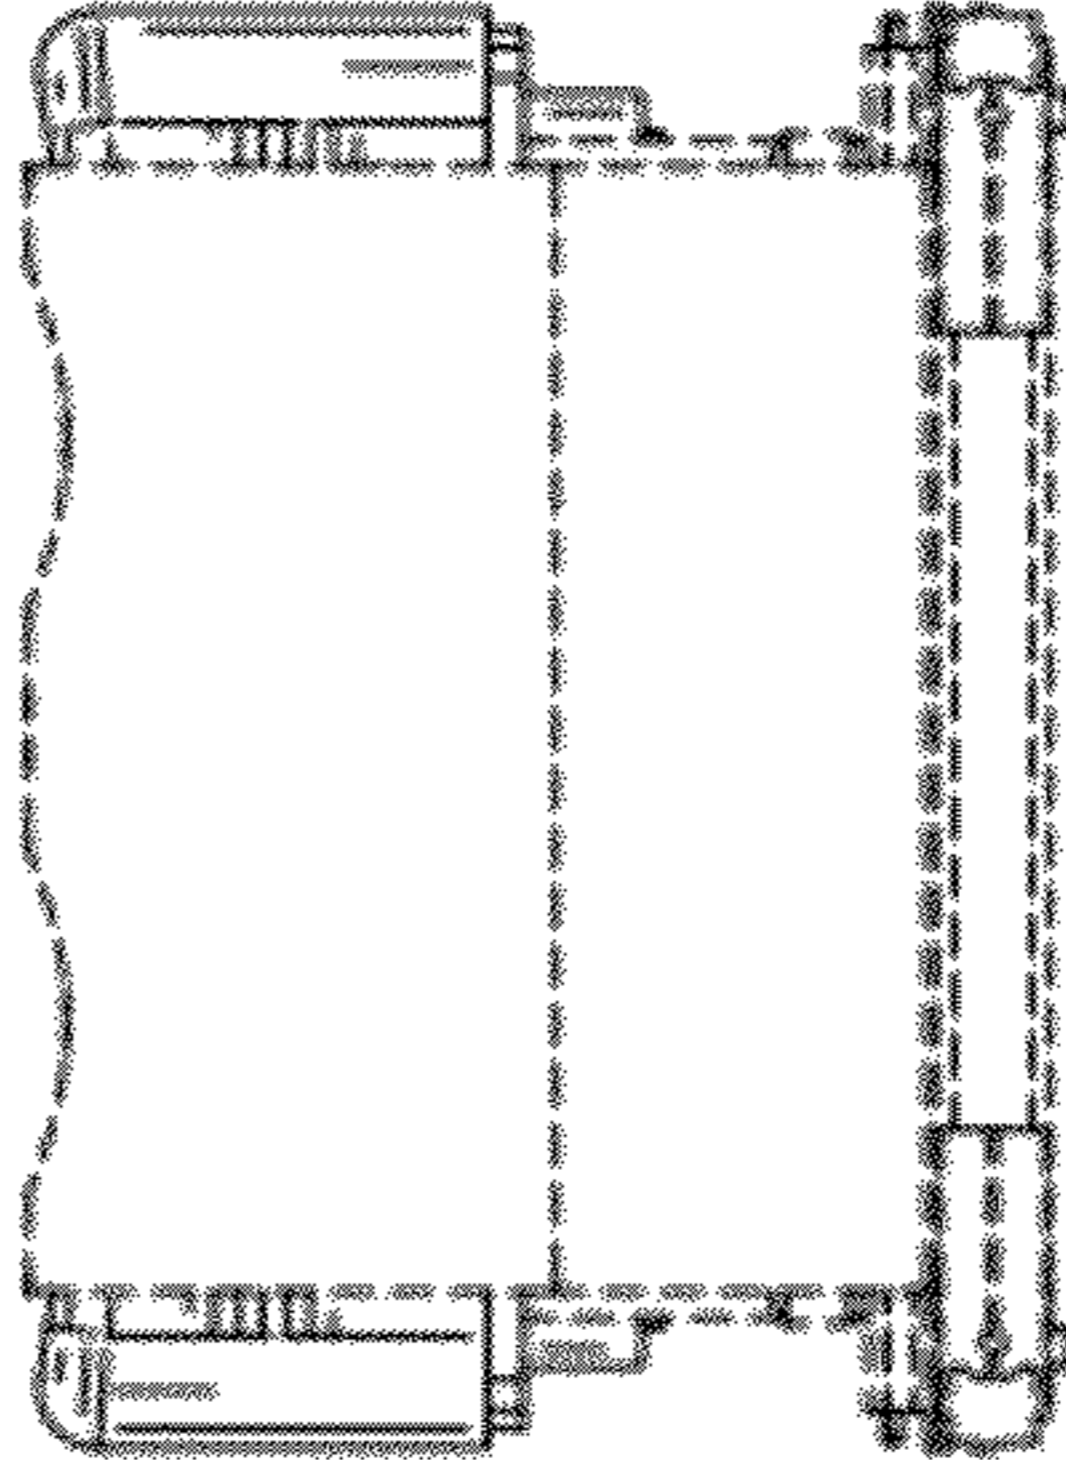


FIG. 5

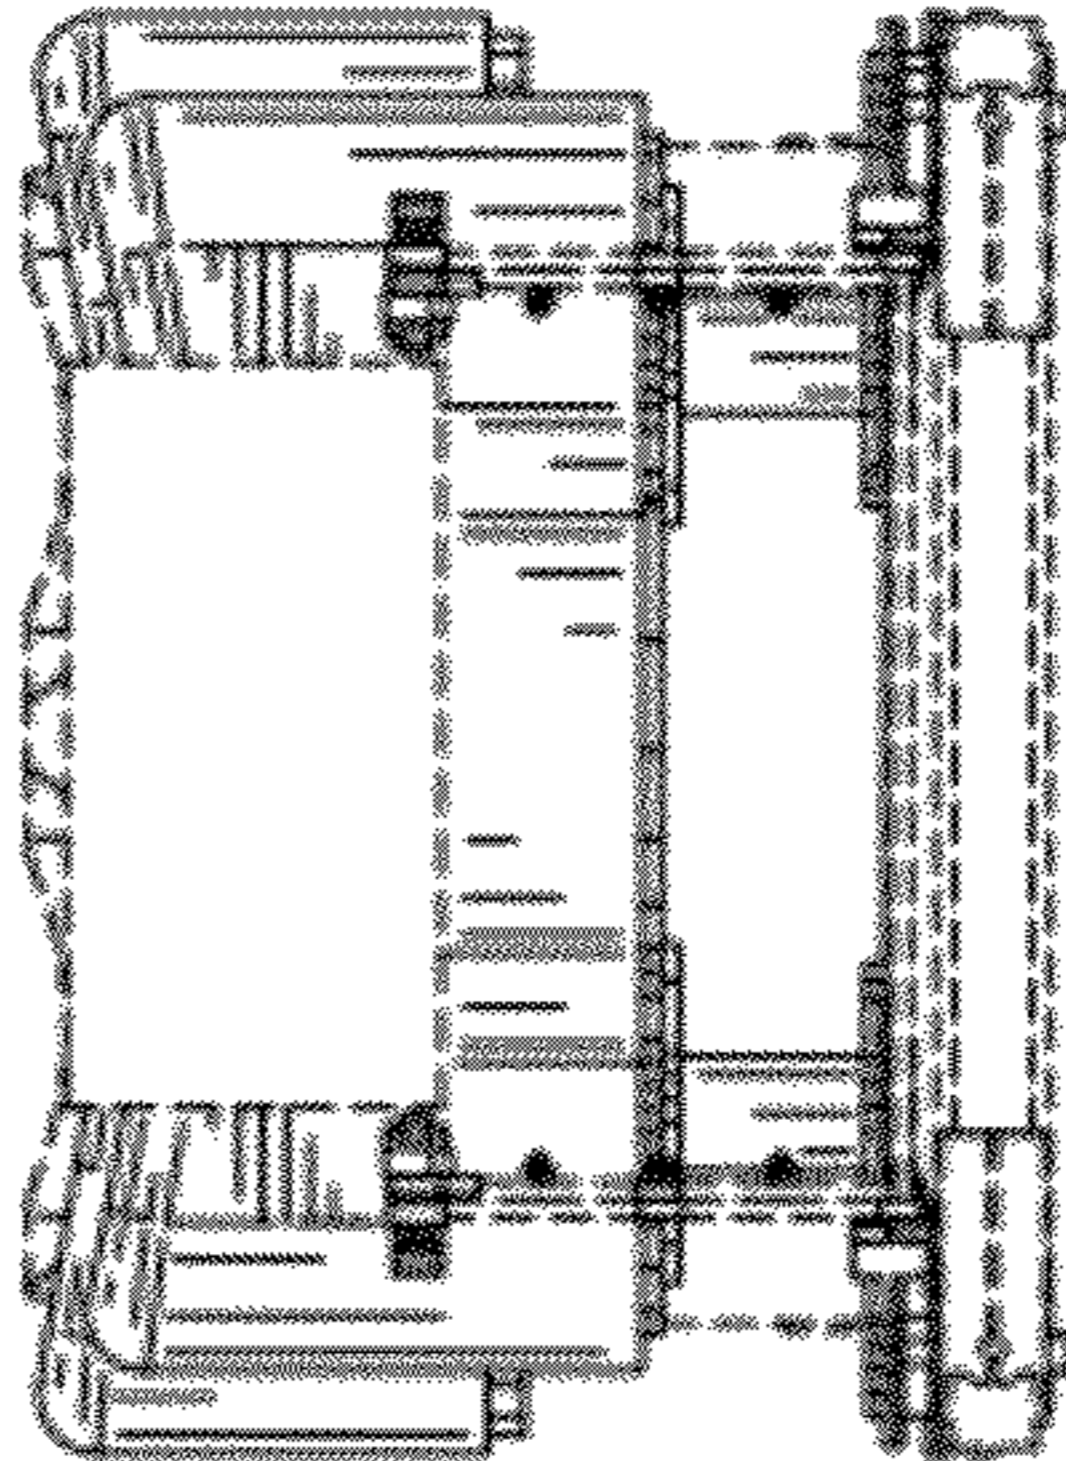


FIG. 4

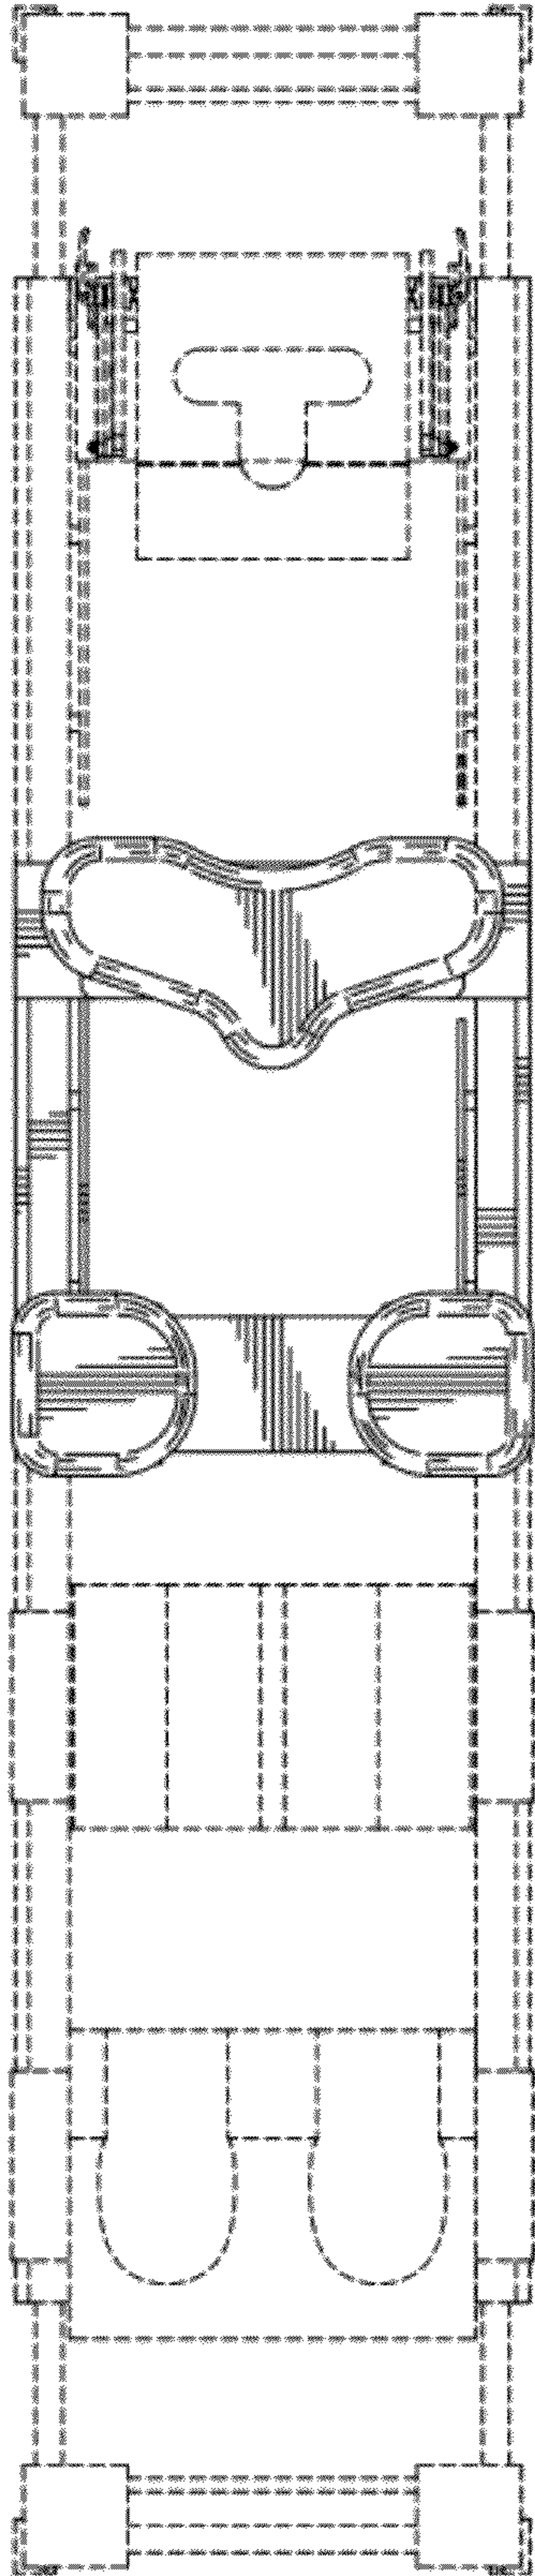


FIG. 6

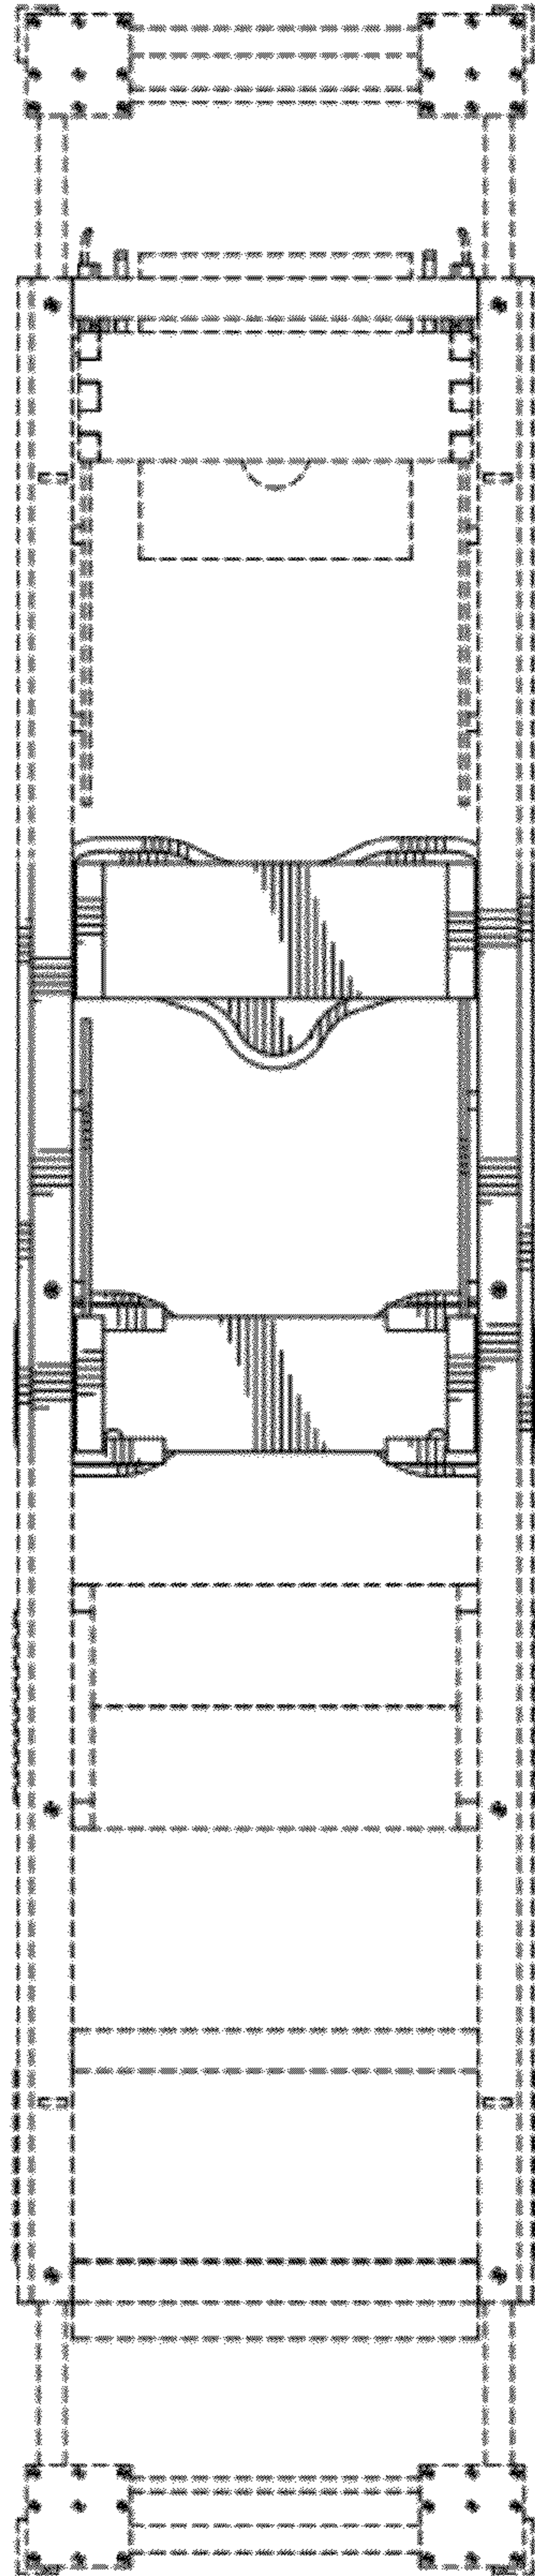


FIG. 7