



US00D663834S

(12) **United States Design Patent**  
**Kyvik et al.**

(10) **Patent No.:** **US D663,834 S**  
(45) **Date of Patent:** **\*\* Jul. 17, 2012**

(54) **SLOTTED CATHETER ANCHOR PAD WITH  
RELEASE LAYER**

(75) Inventors: **Kurt Kyvik**, Ocala, FL (US); **Scott  
Ryan**, Ocala, FL (US); **Arthur  
Parkhurst**, Ocala, FL (US)

(73) Assignee: **Zefon International, Inc.**, Ocala, FL  
(US)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/406,914**

(22) Filed: **Nov. 21, 2011**

(51) **LOC (9) Cl.** ..... **24-02**

(52) **U.S. Cl.** ..... **D24/128**

(58) **Field of Classification Search** ..... D24/127-130,  
D24/189; 604/179-180, 187, 227; 602/58-59;  
128/DIG. 26

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D492,411	S *	6/2004	Bierman	.....	D24/128
D503,977	S *	4/2005	Bierman	.....	D24/128
D528,206	S *	9/2006	Bierman	.....	D24/128
D608,444	S *	1/2010	Kyvik et al.	.....	D24/130
D616,091	S *	5/2010	Kyvik et al.	.....	D24/128
D616,542	S *	5/2010	Kyvik et al.	.....	D24/128
D616,983	S *	6/2010	Kyvik et al.	.....	D24/128
D625,002	S *	10/2010	Kyvik et al.	.....	D24/128
D652,509	S *	1/2012	Kyvik et al.	.....	D24/128
2010/0298778	A1 *	11/2010	Bracken et al.	.....	604/180
2011/0021997	A1 *	1/2011	Kyvik et al.	.....	604/180

\* cited by examiner

*Primary Examiner* — Eric Goodman

(74) *Attorney, Agent, or Firm* — Thomas C. Saitta

(57) **CLAIM**

The ornamental design for a slotted catheter anchor pad with release layer, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of the slotted catheter anchor pad with release layer, shown with the release layers in a spread position.

FIG. 2 is a top view of the slotted catheter anchor pad with release layer, shown in the neutral position.

FIG. 3 is a bottom view of the slotted catheter anchor pad with release layer, shown in the neutral position.

FIG. 4 is a left side view of the slotted catheter anchor pad with release layer, shown in the neutral position, the right side view being a mirror image.

FIG. 5 is a rear view of the slotted catheter anchor pad with release layer.

FIG. 6 is a front view of the slotted catheter anchor pad with release layer.

FIG. 7 is a perspective view of the slotted catheter anchor pad with the release layer removed.

FIG. 8 is a top view of the slotted catheter anchor pad with the release layer removed.


FIG. 9 is a bottom view of the slotted catheter anchor pad with release layer removed.


FIG. 10 is a left side view of the slotted catheter anchor pad with release layer removed, the right side view being a mirror image.

FIG. 11 is a rear view of the slotted catheter anchor pad with release layer removed; and,


FIG. 12 is a front view of the slotted catheter anchor pad with release layer removed.

**1 Claim, 5 Drawing Sheets**

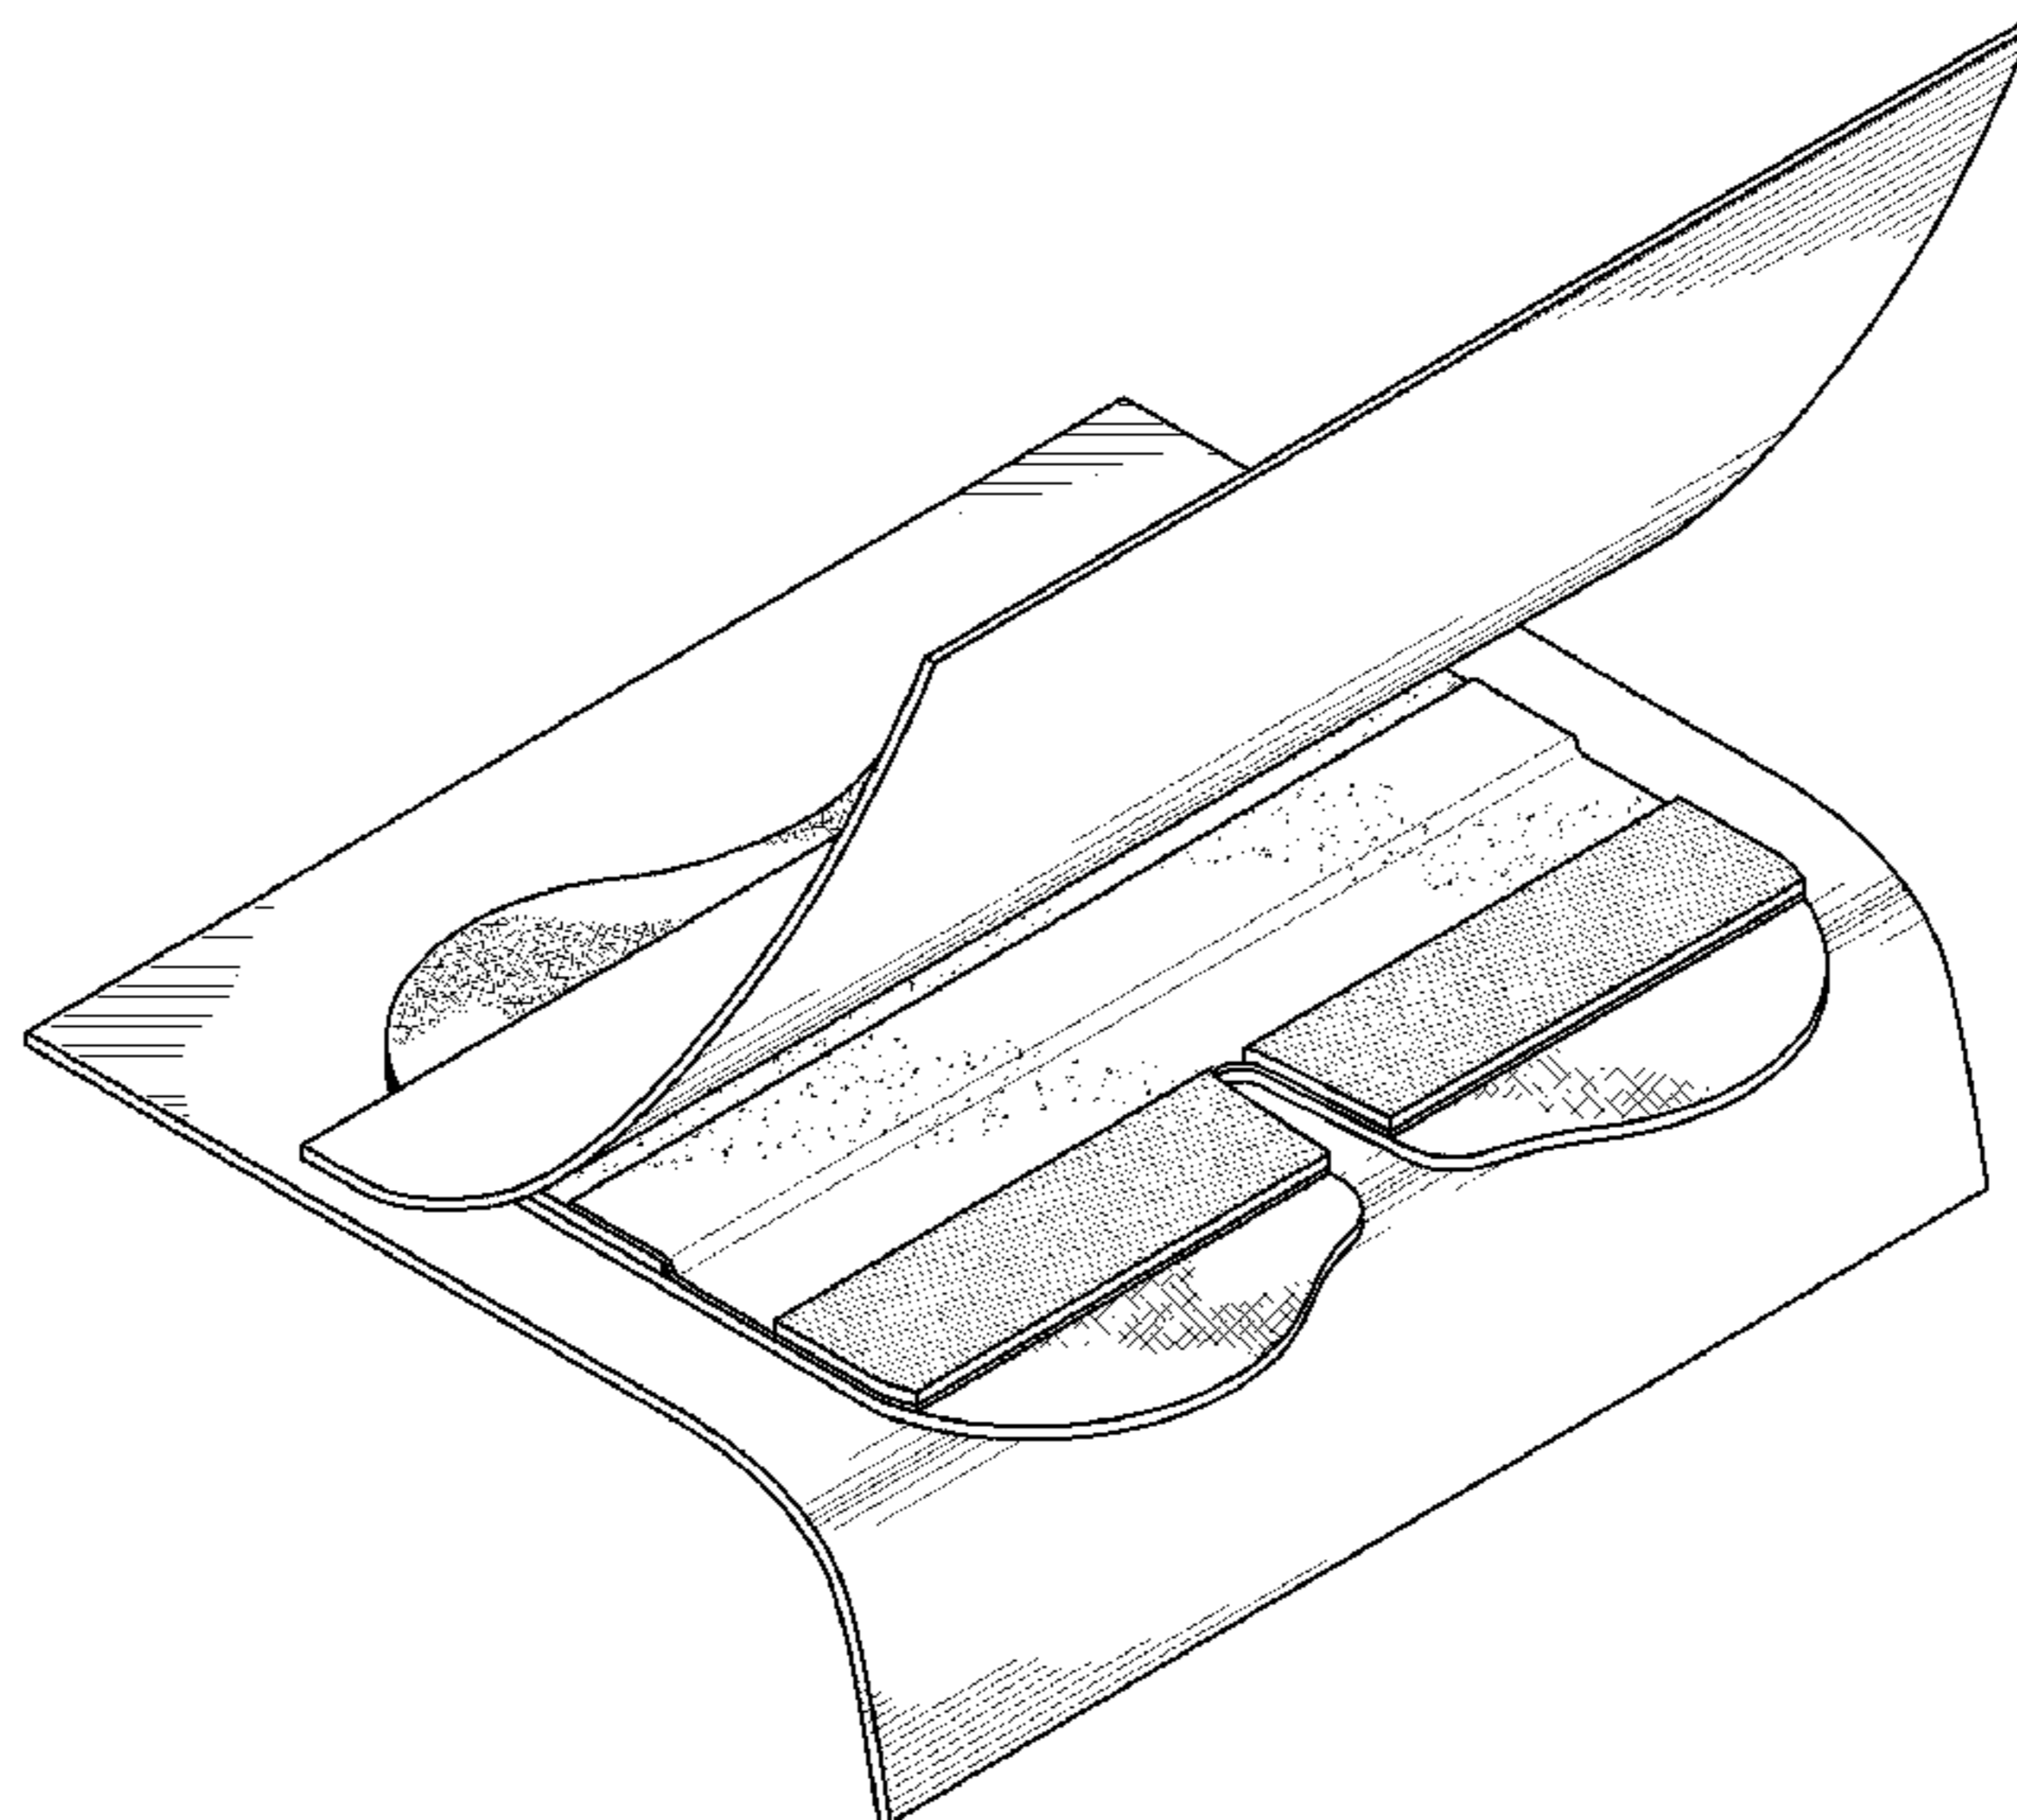


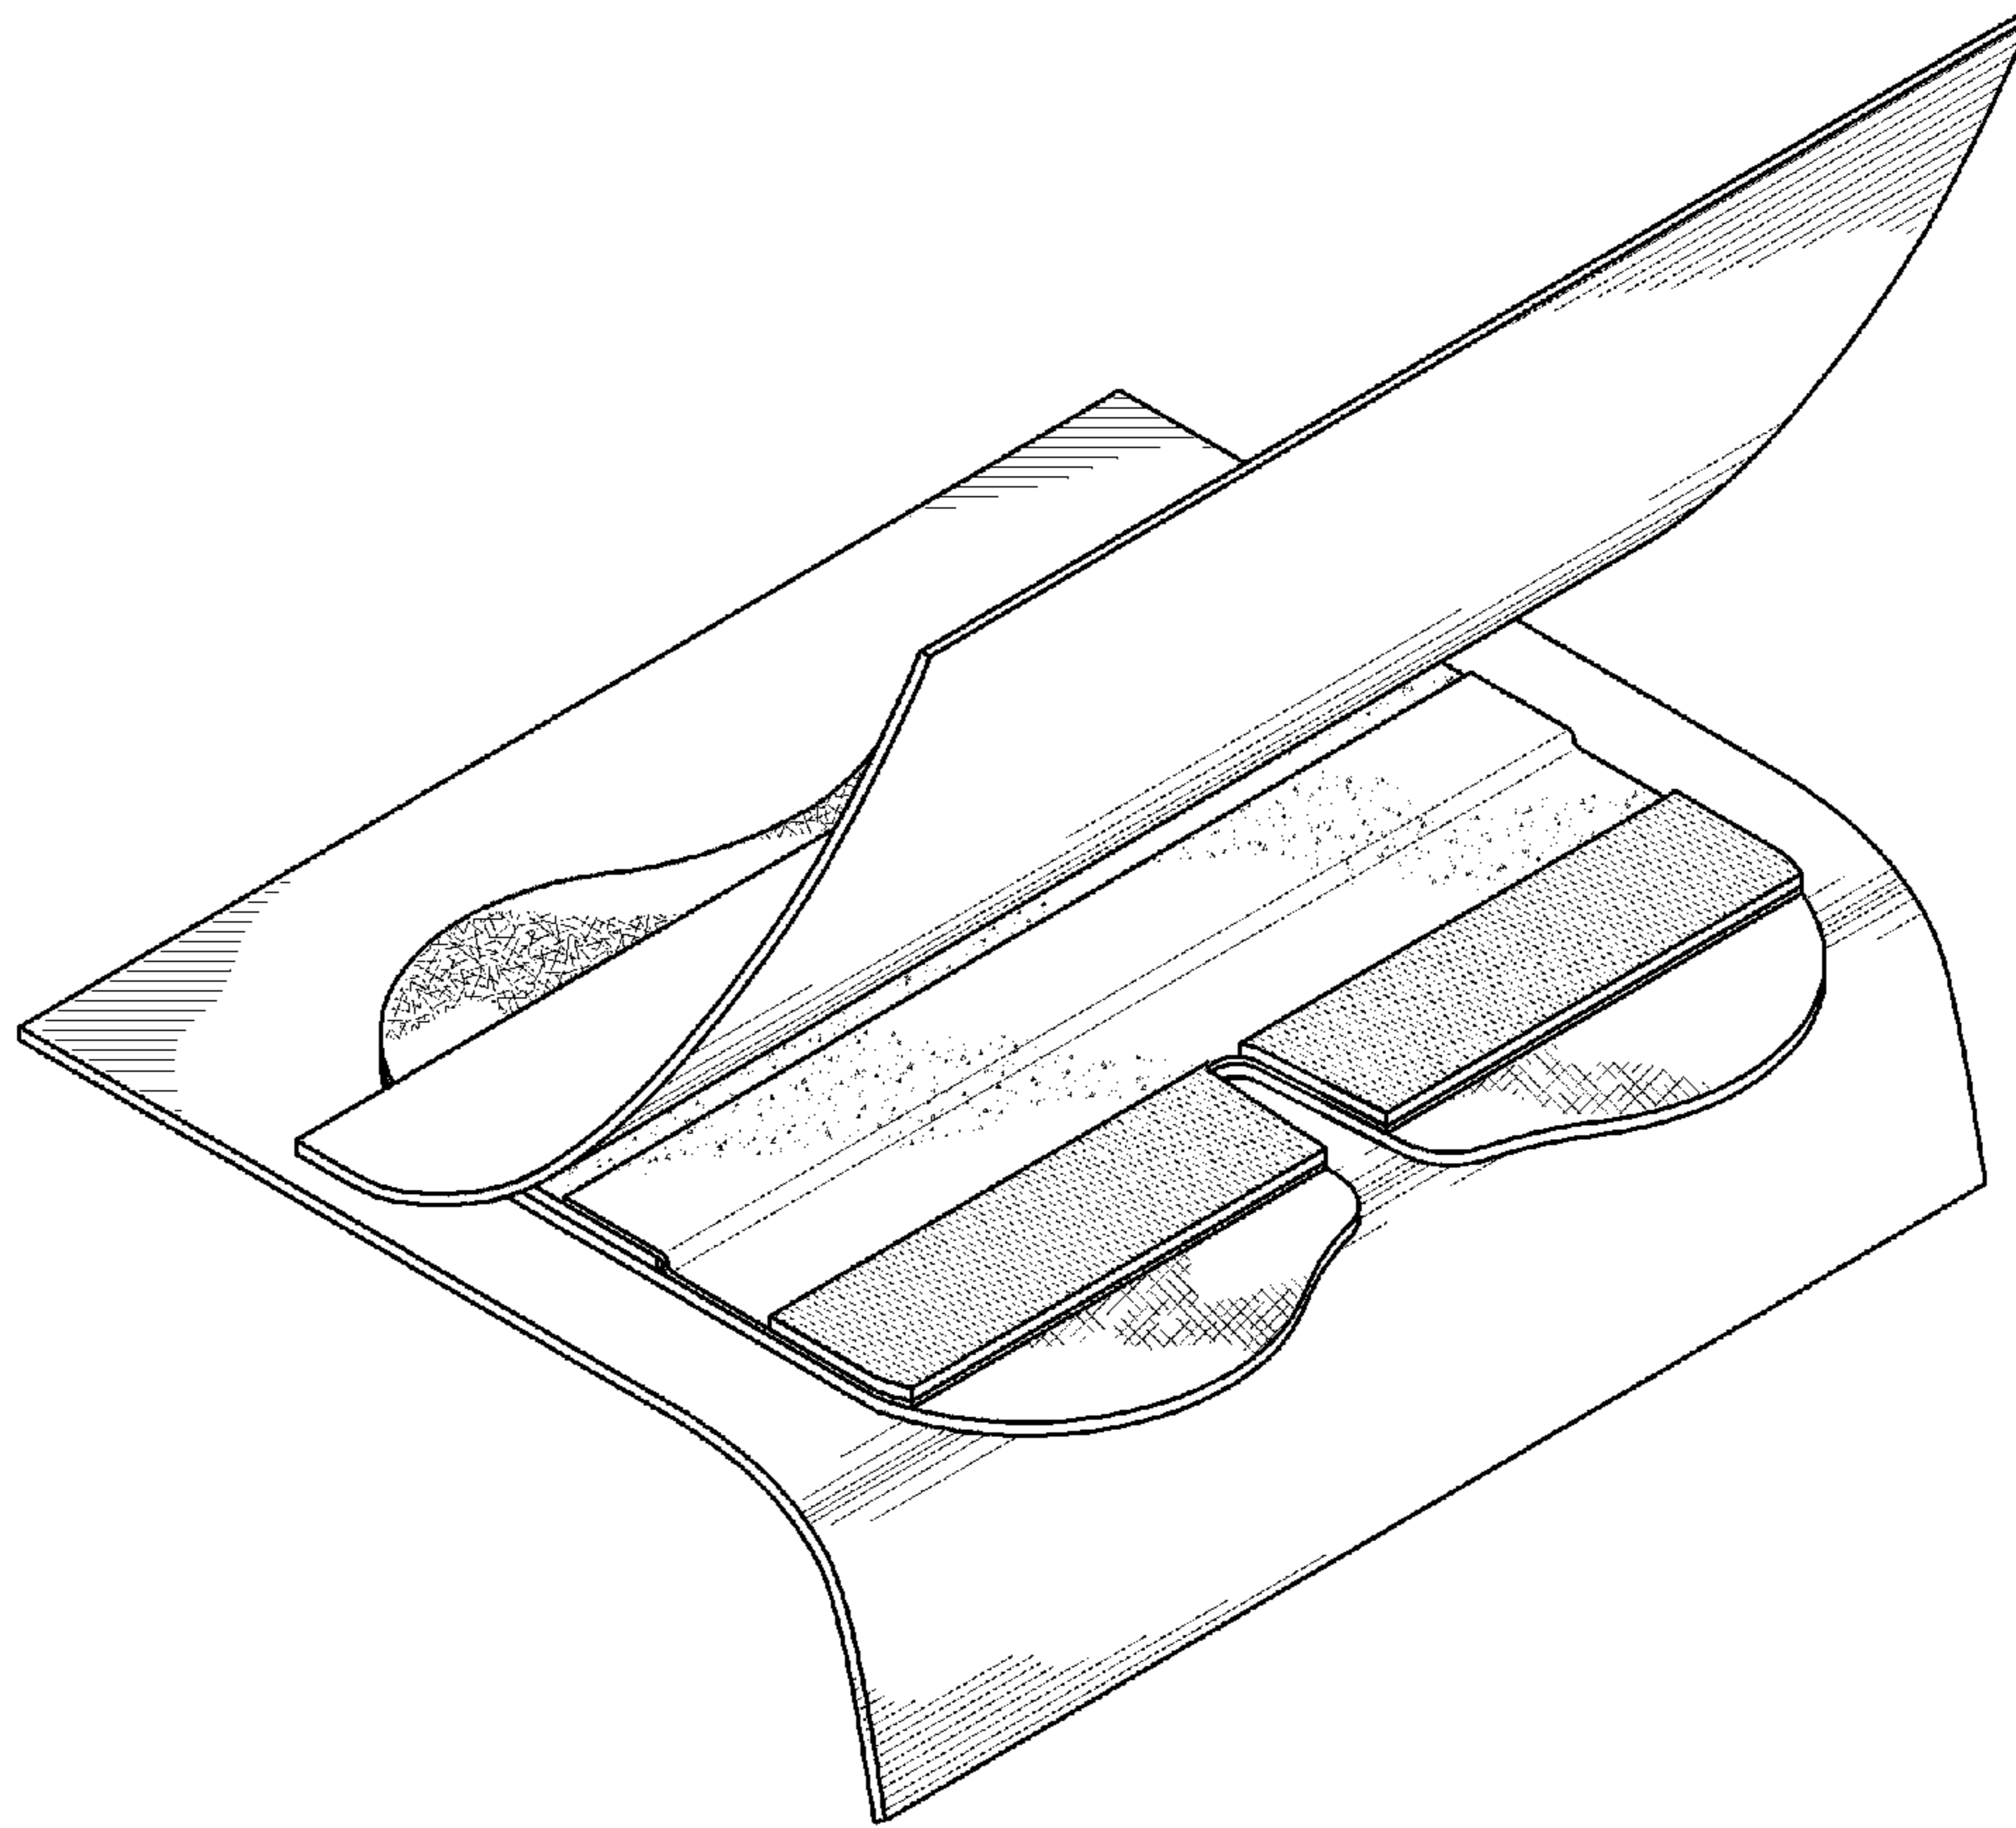

*Fig. 1*

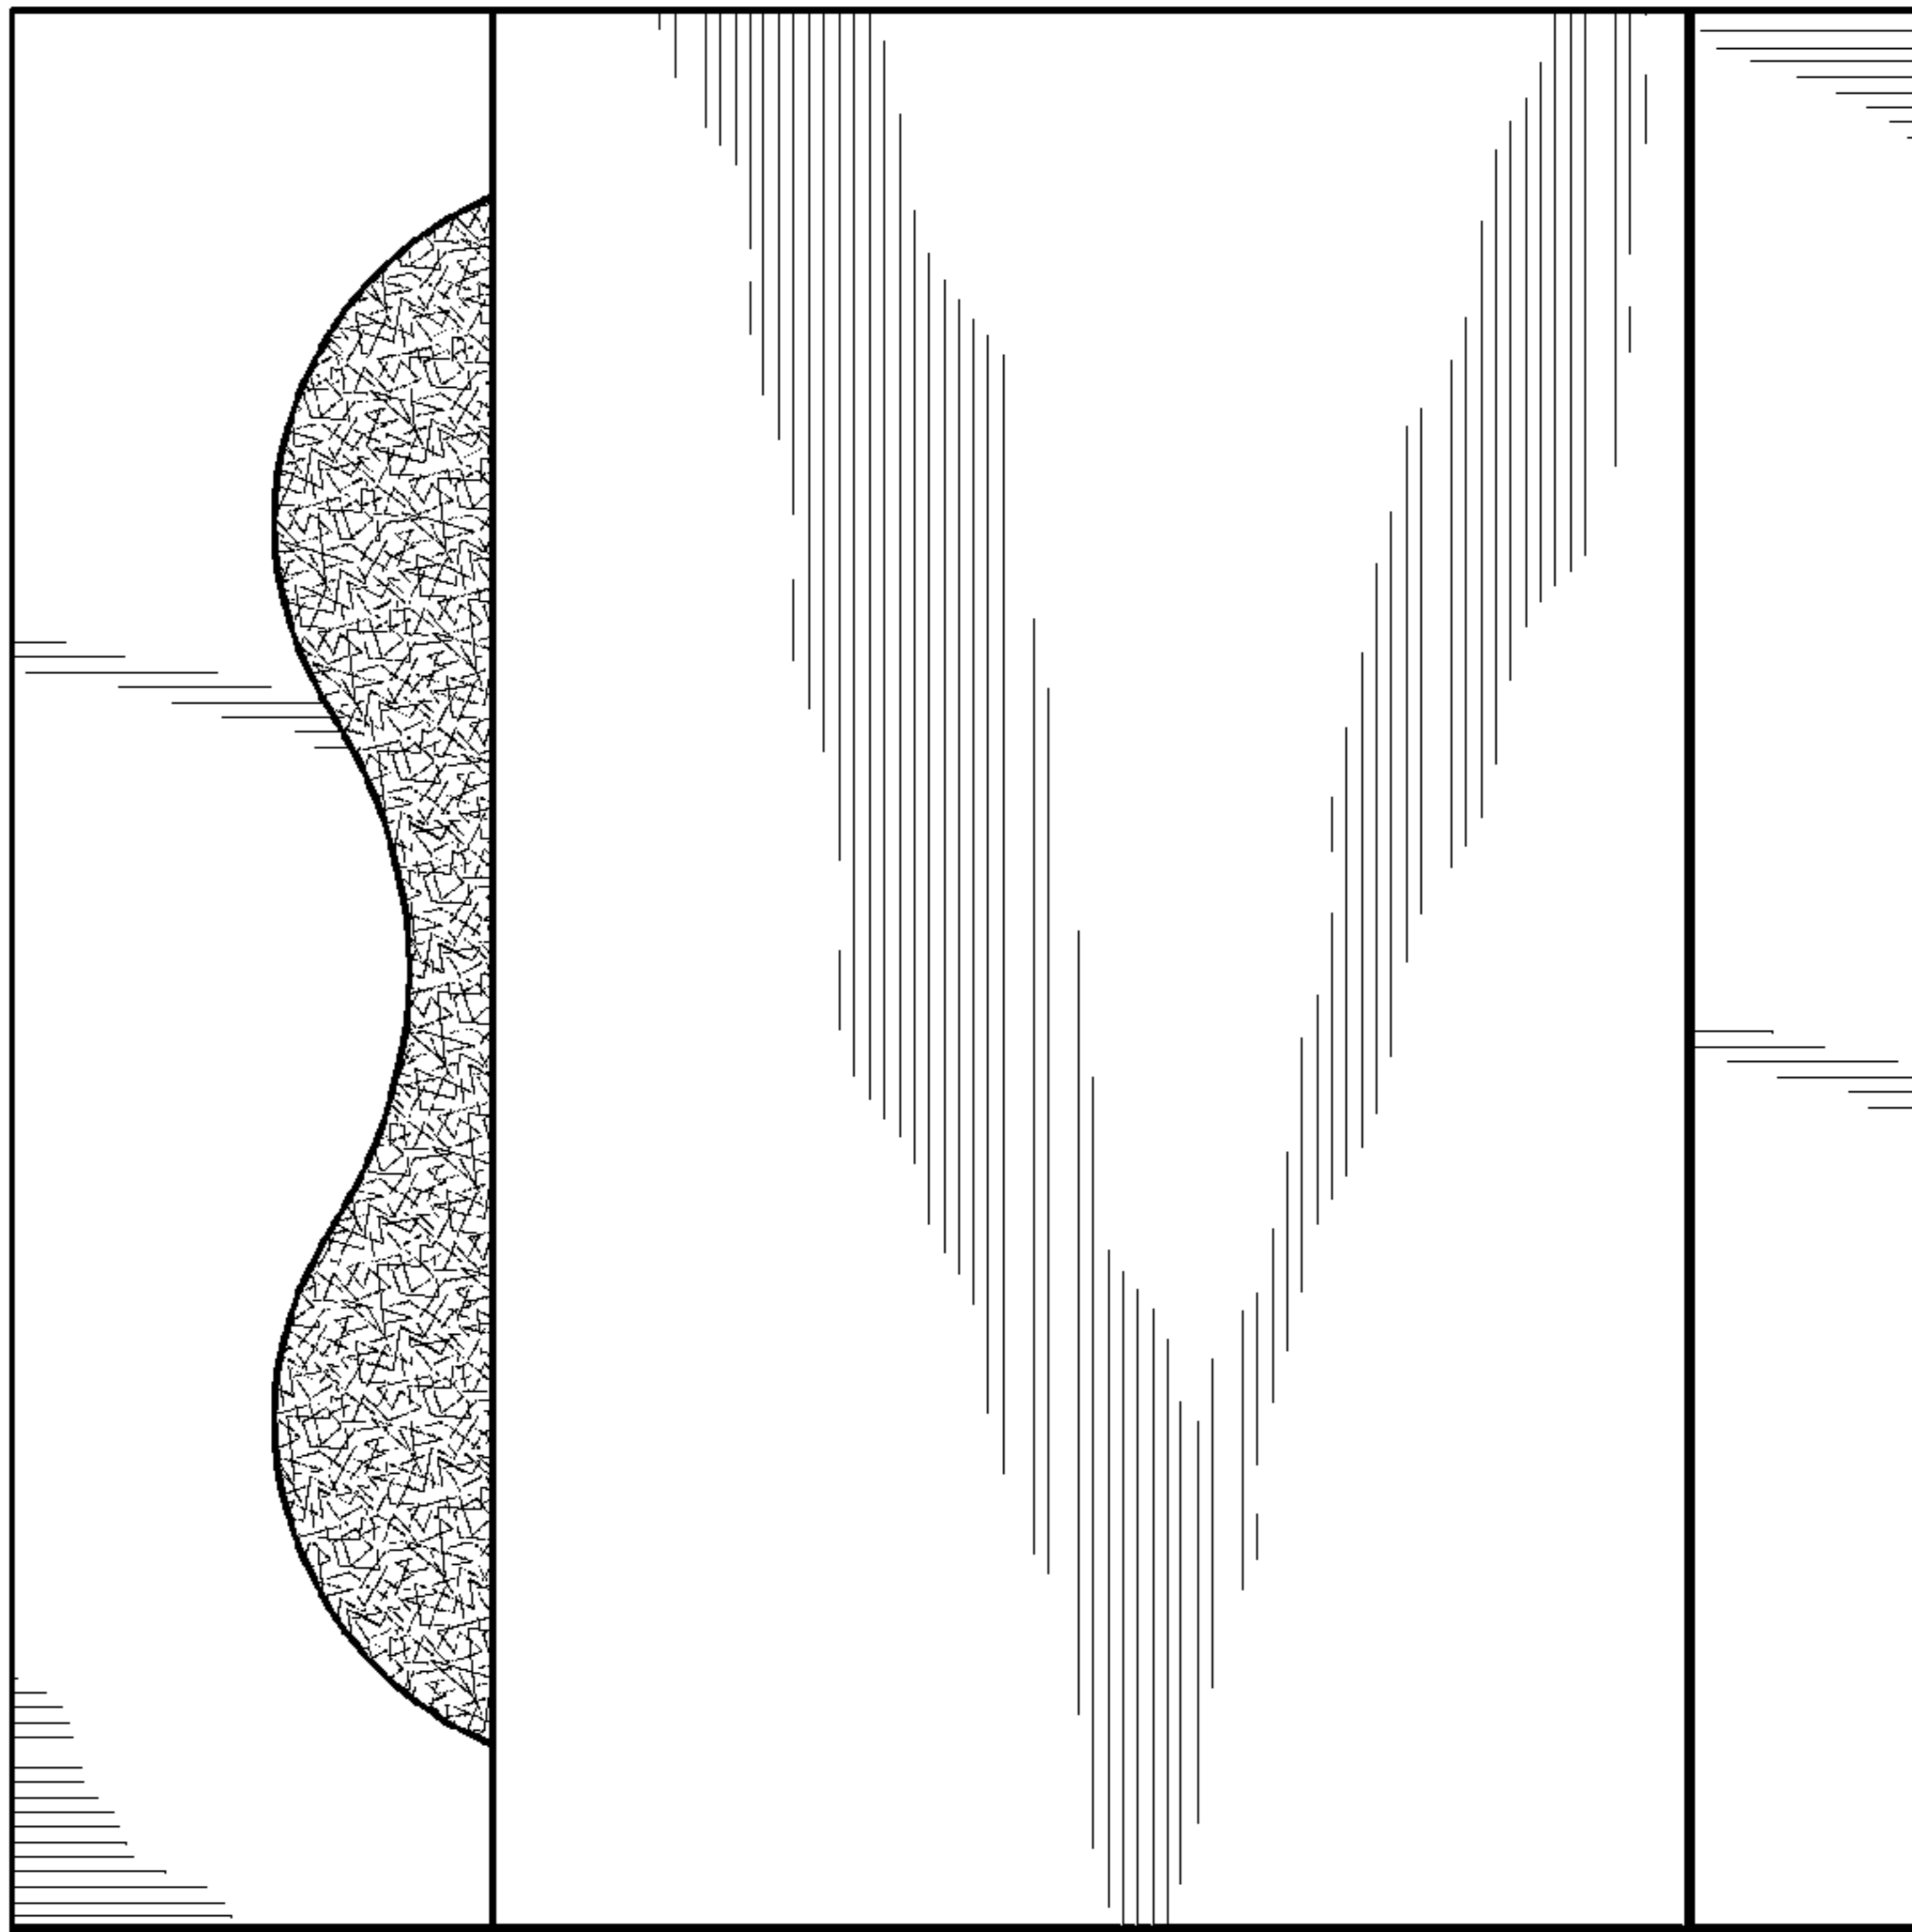


*Fig. 2*




*Fig. 3*




*Fig. 4*

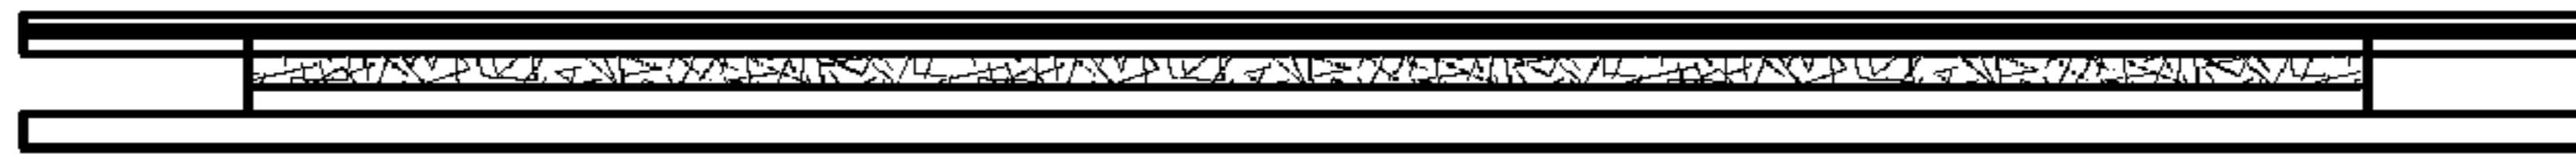


*Fig. 5*

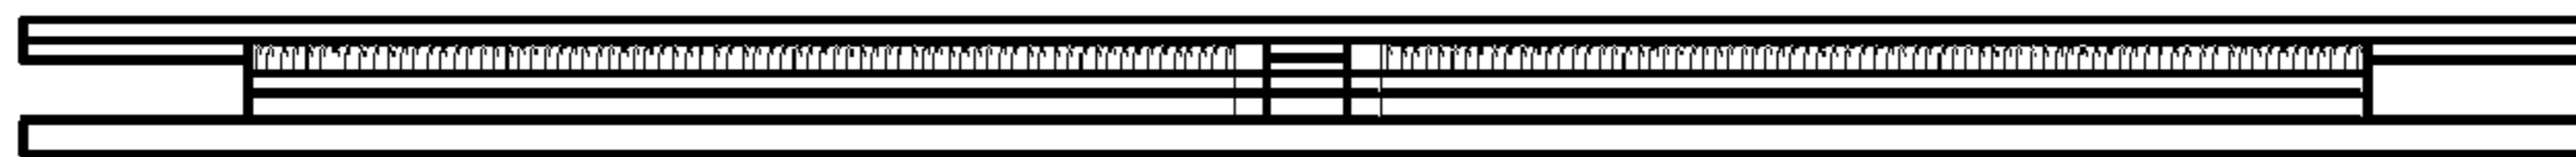


*Fig. 6*

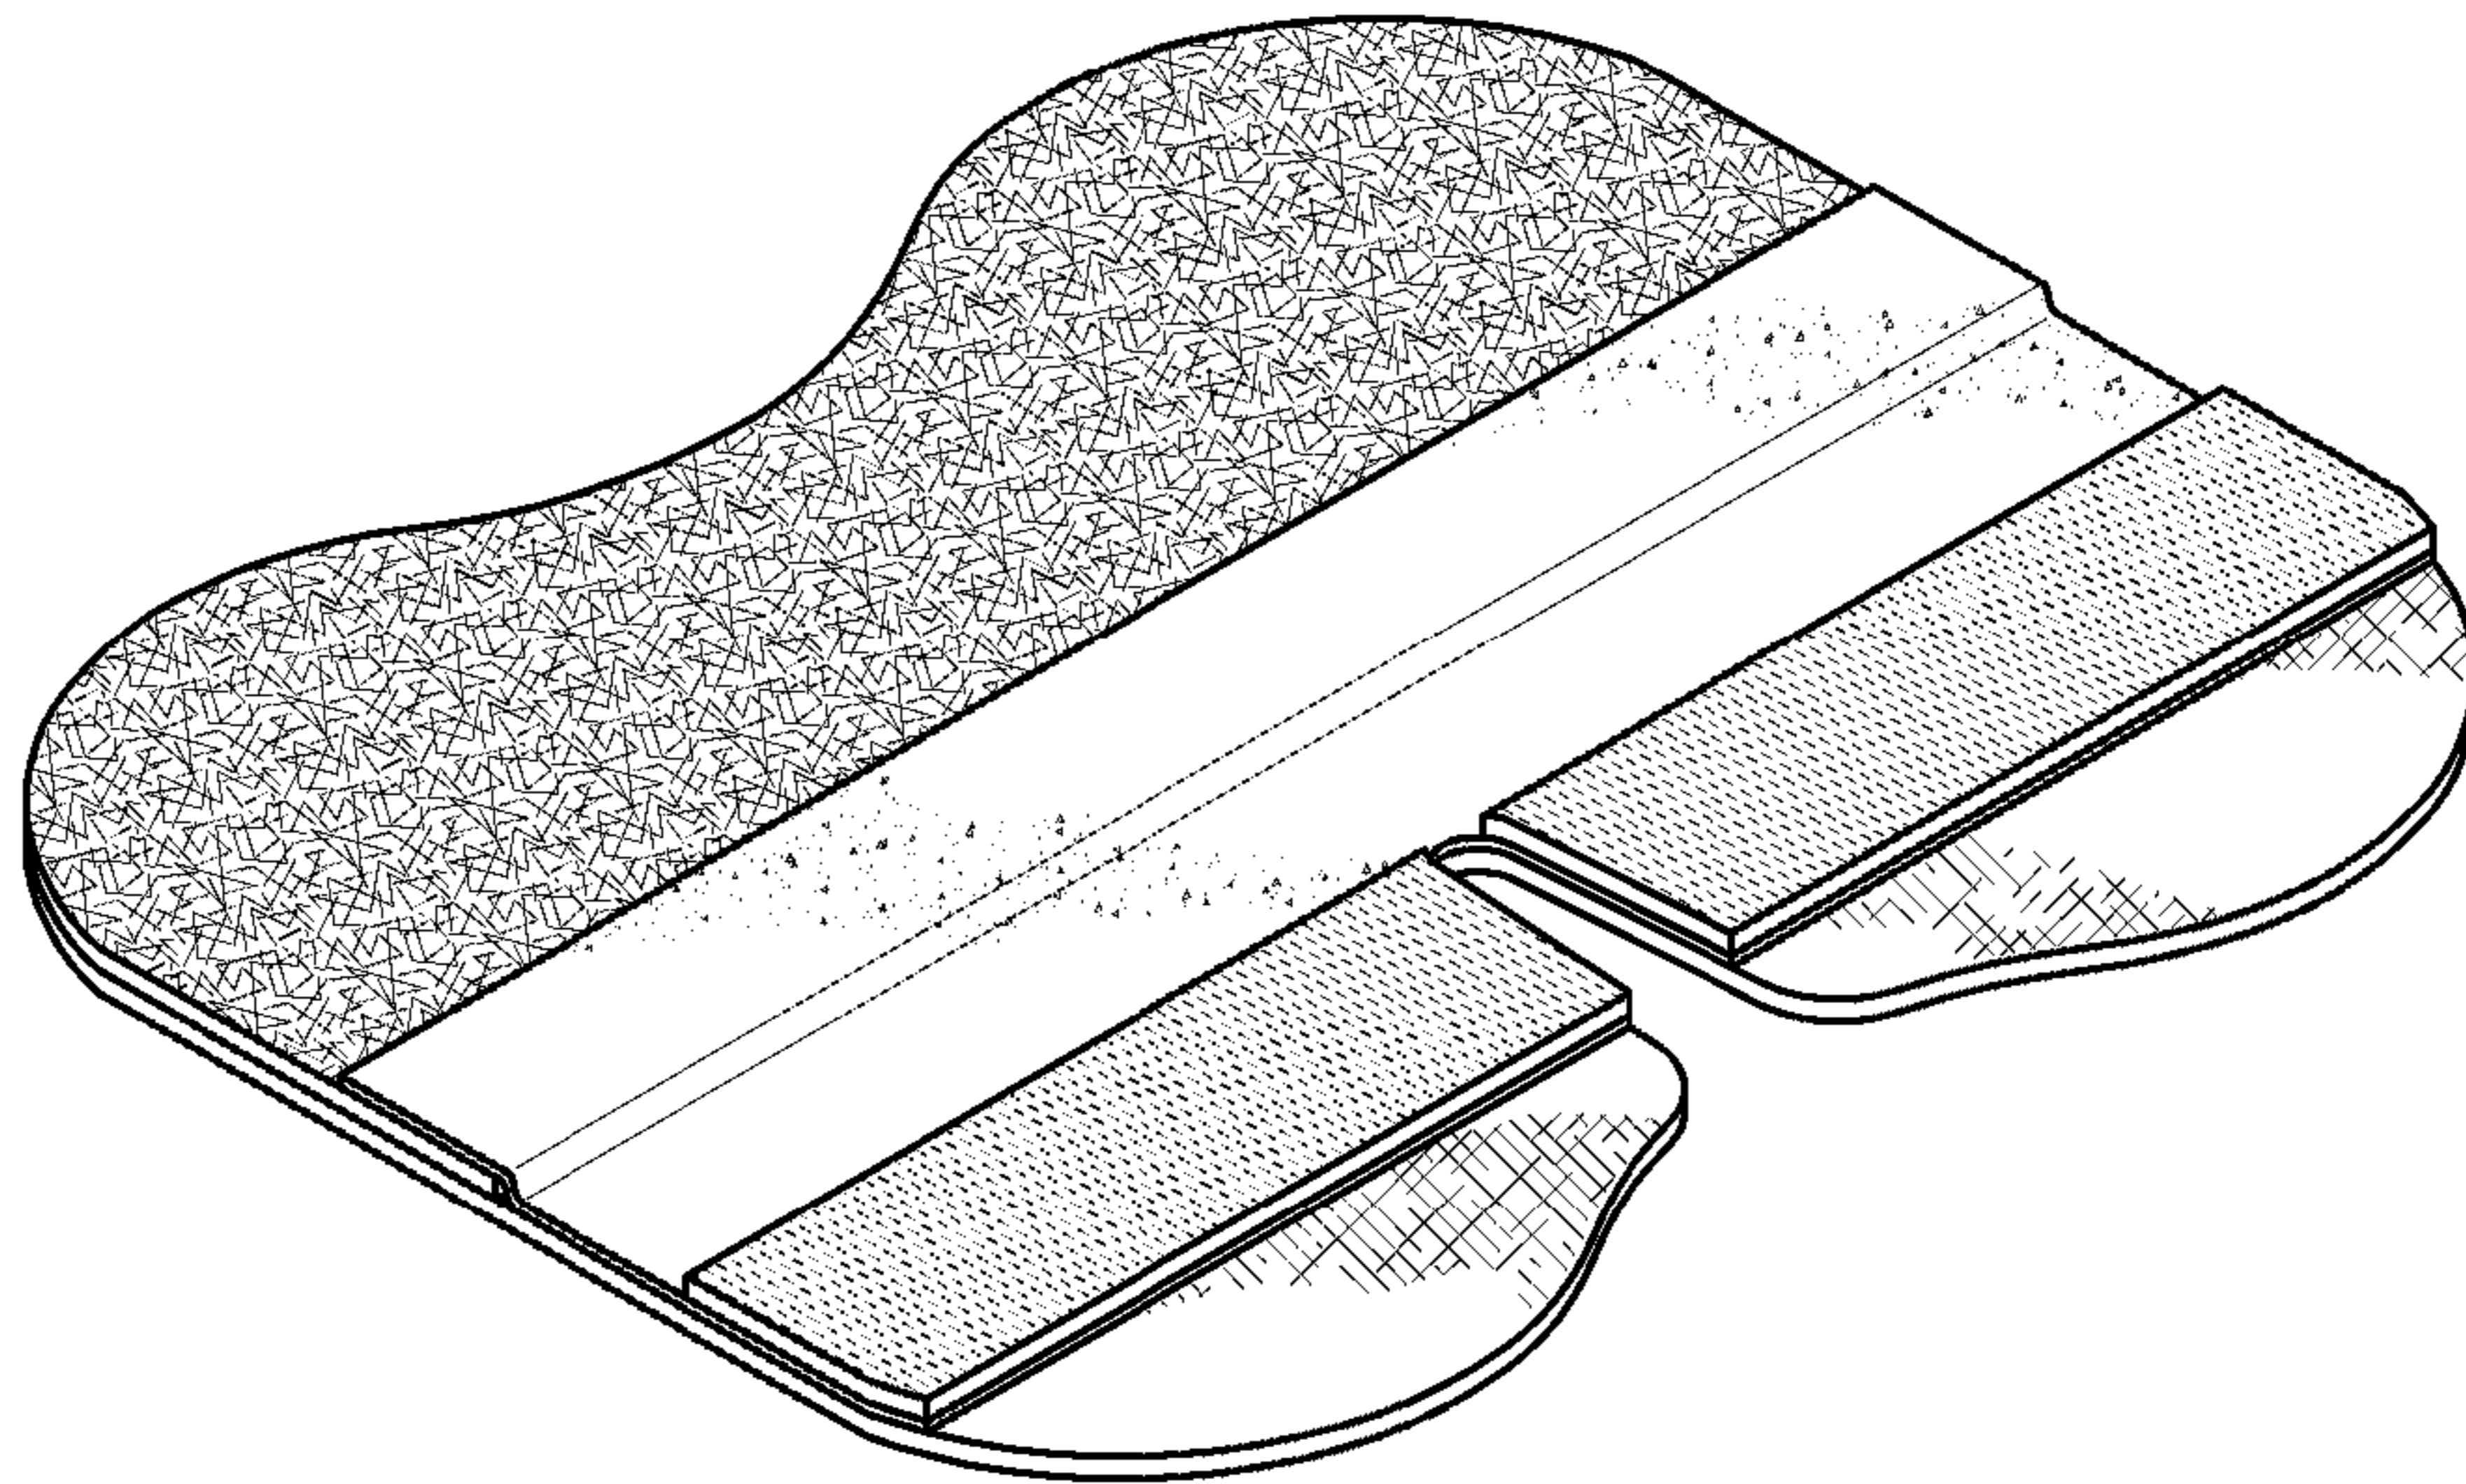

*Fig. 7*

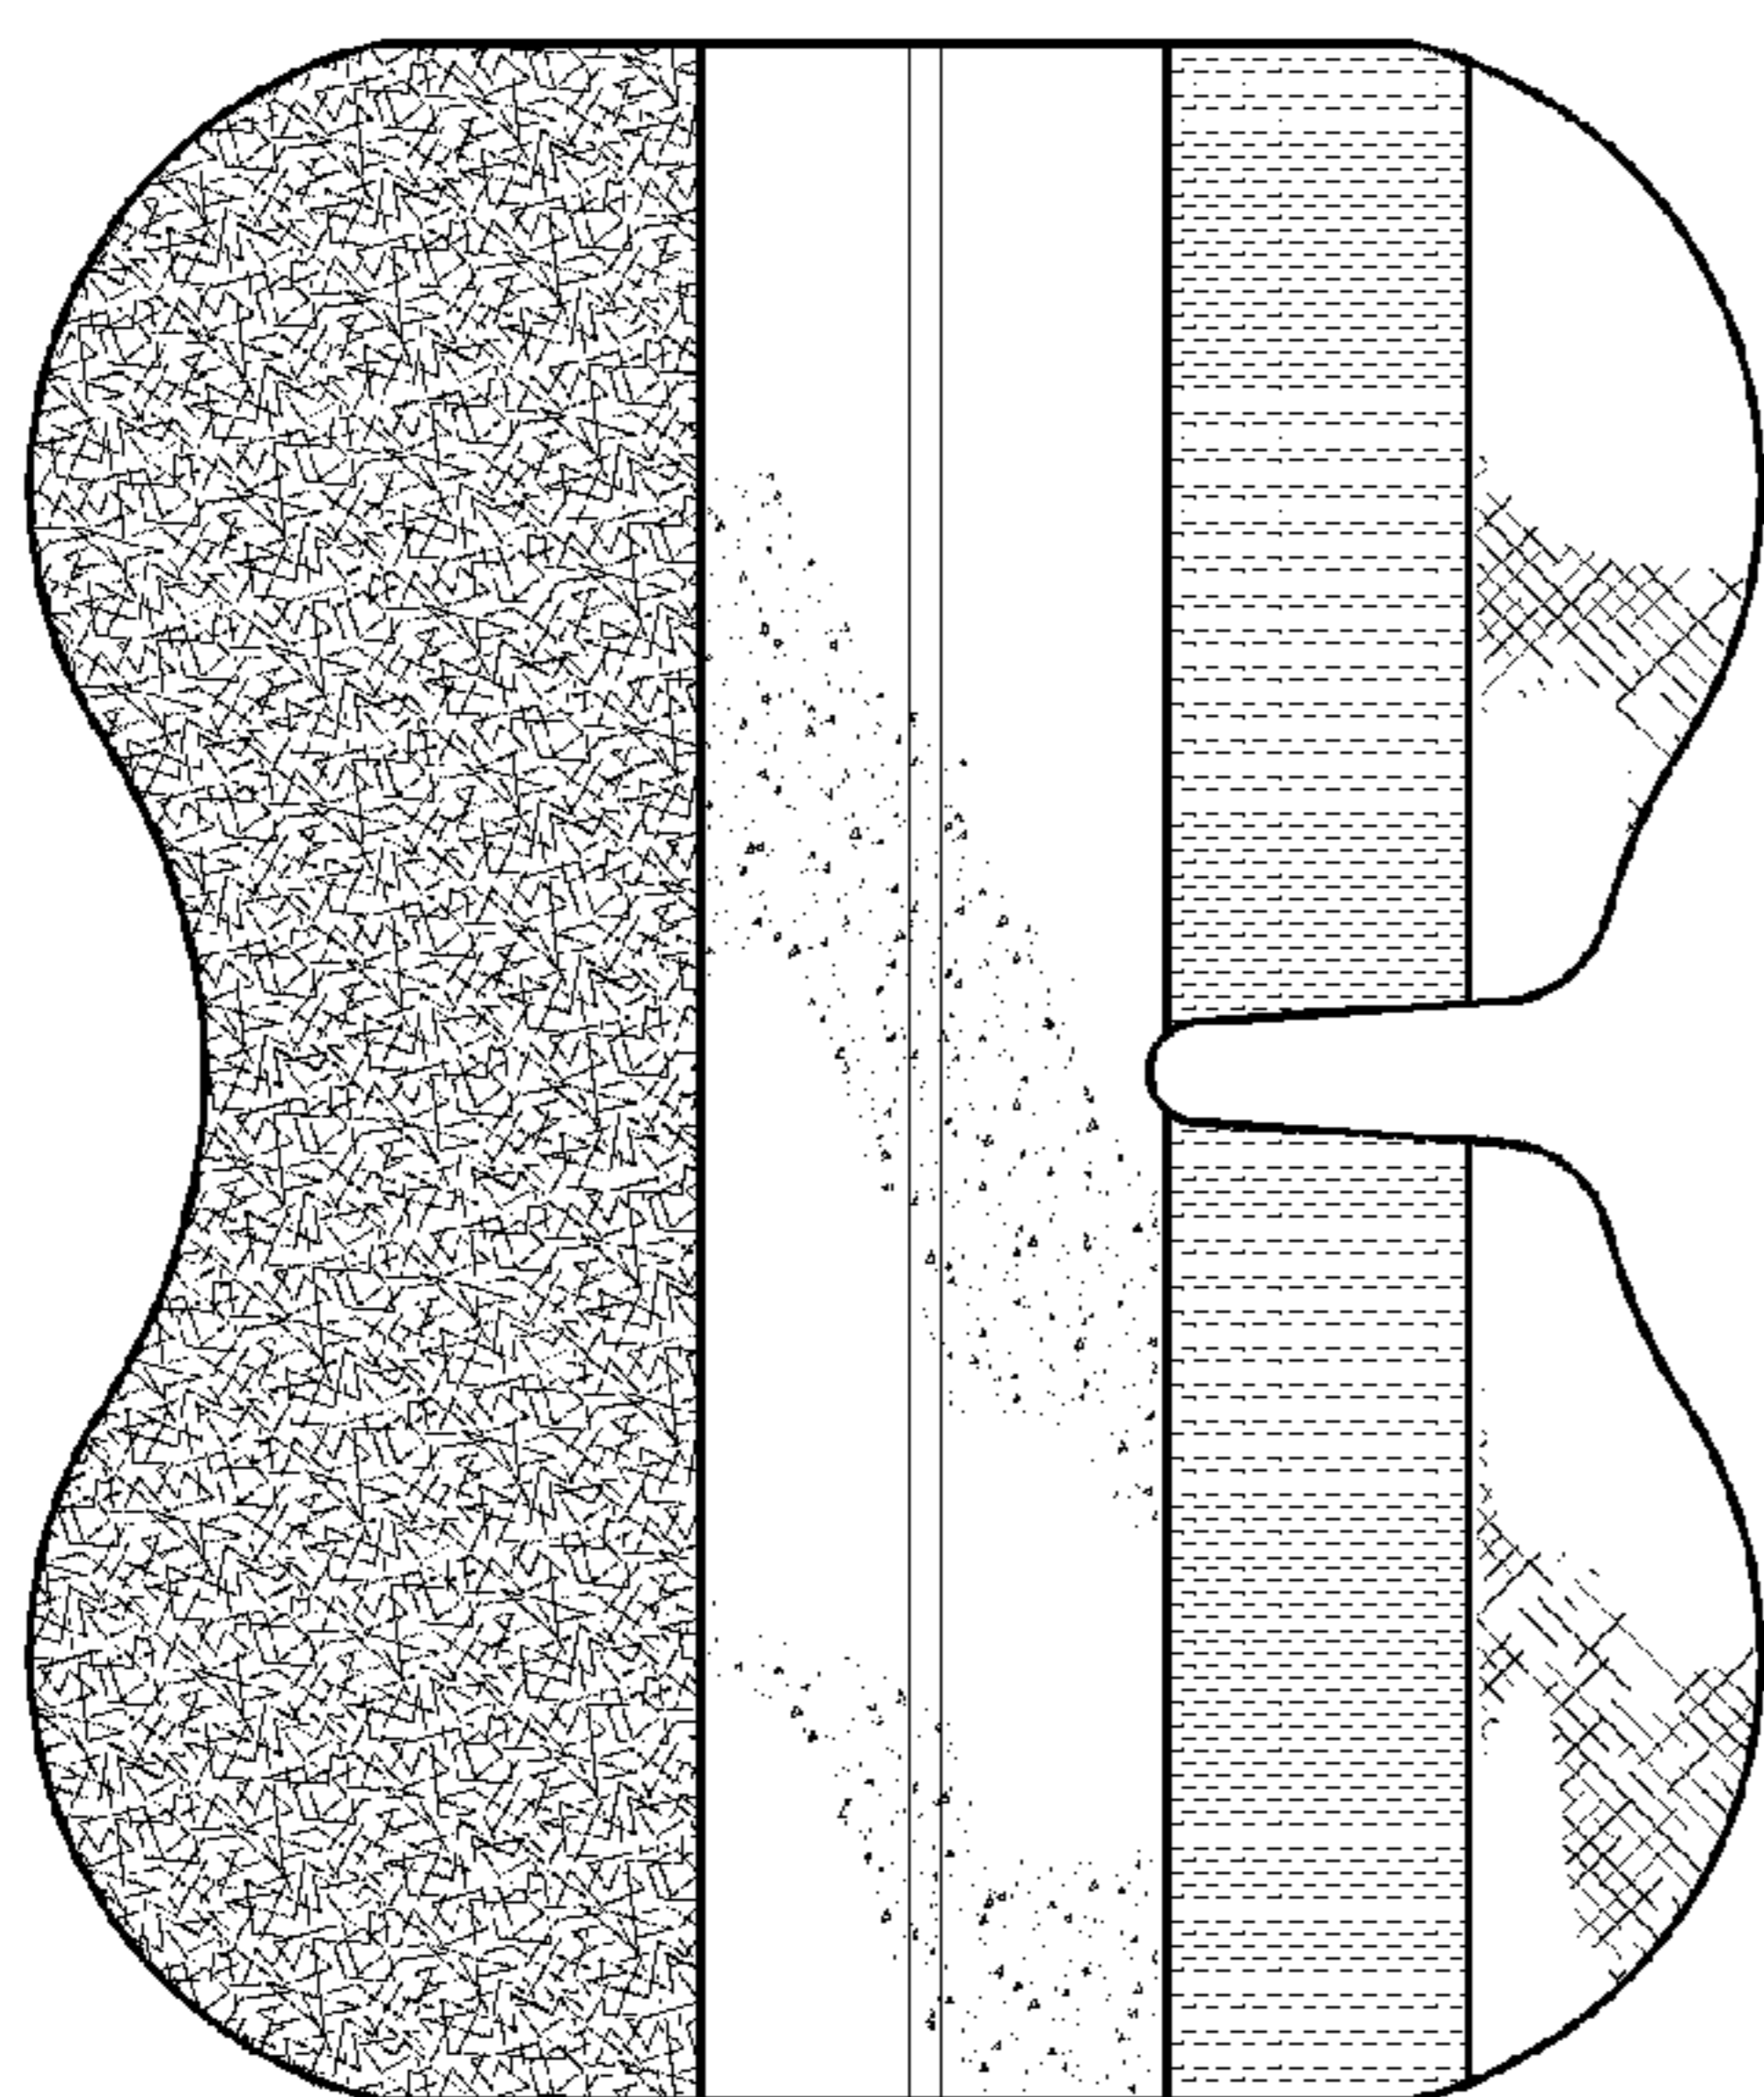


*Fig. 8*

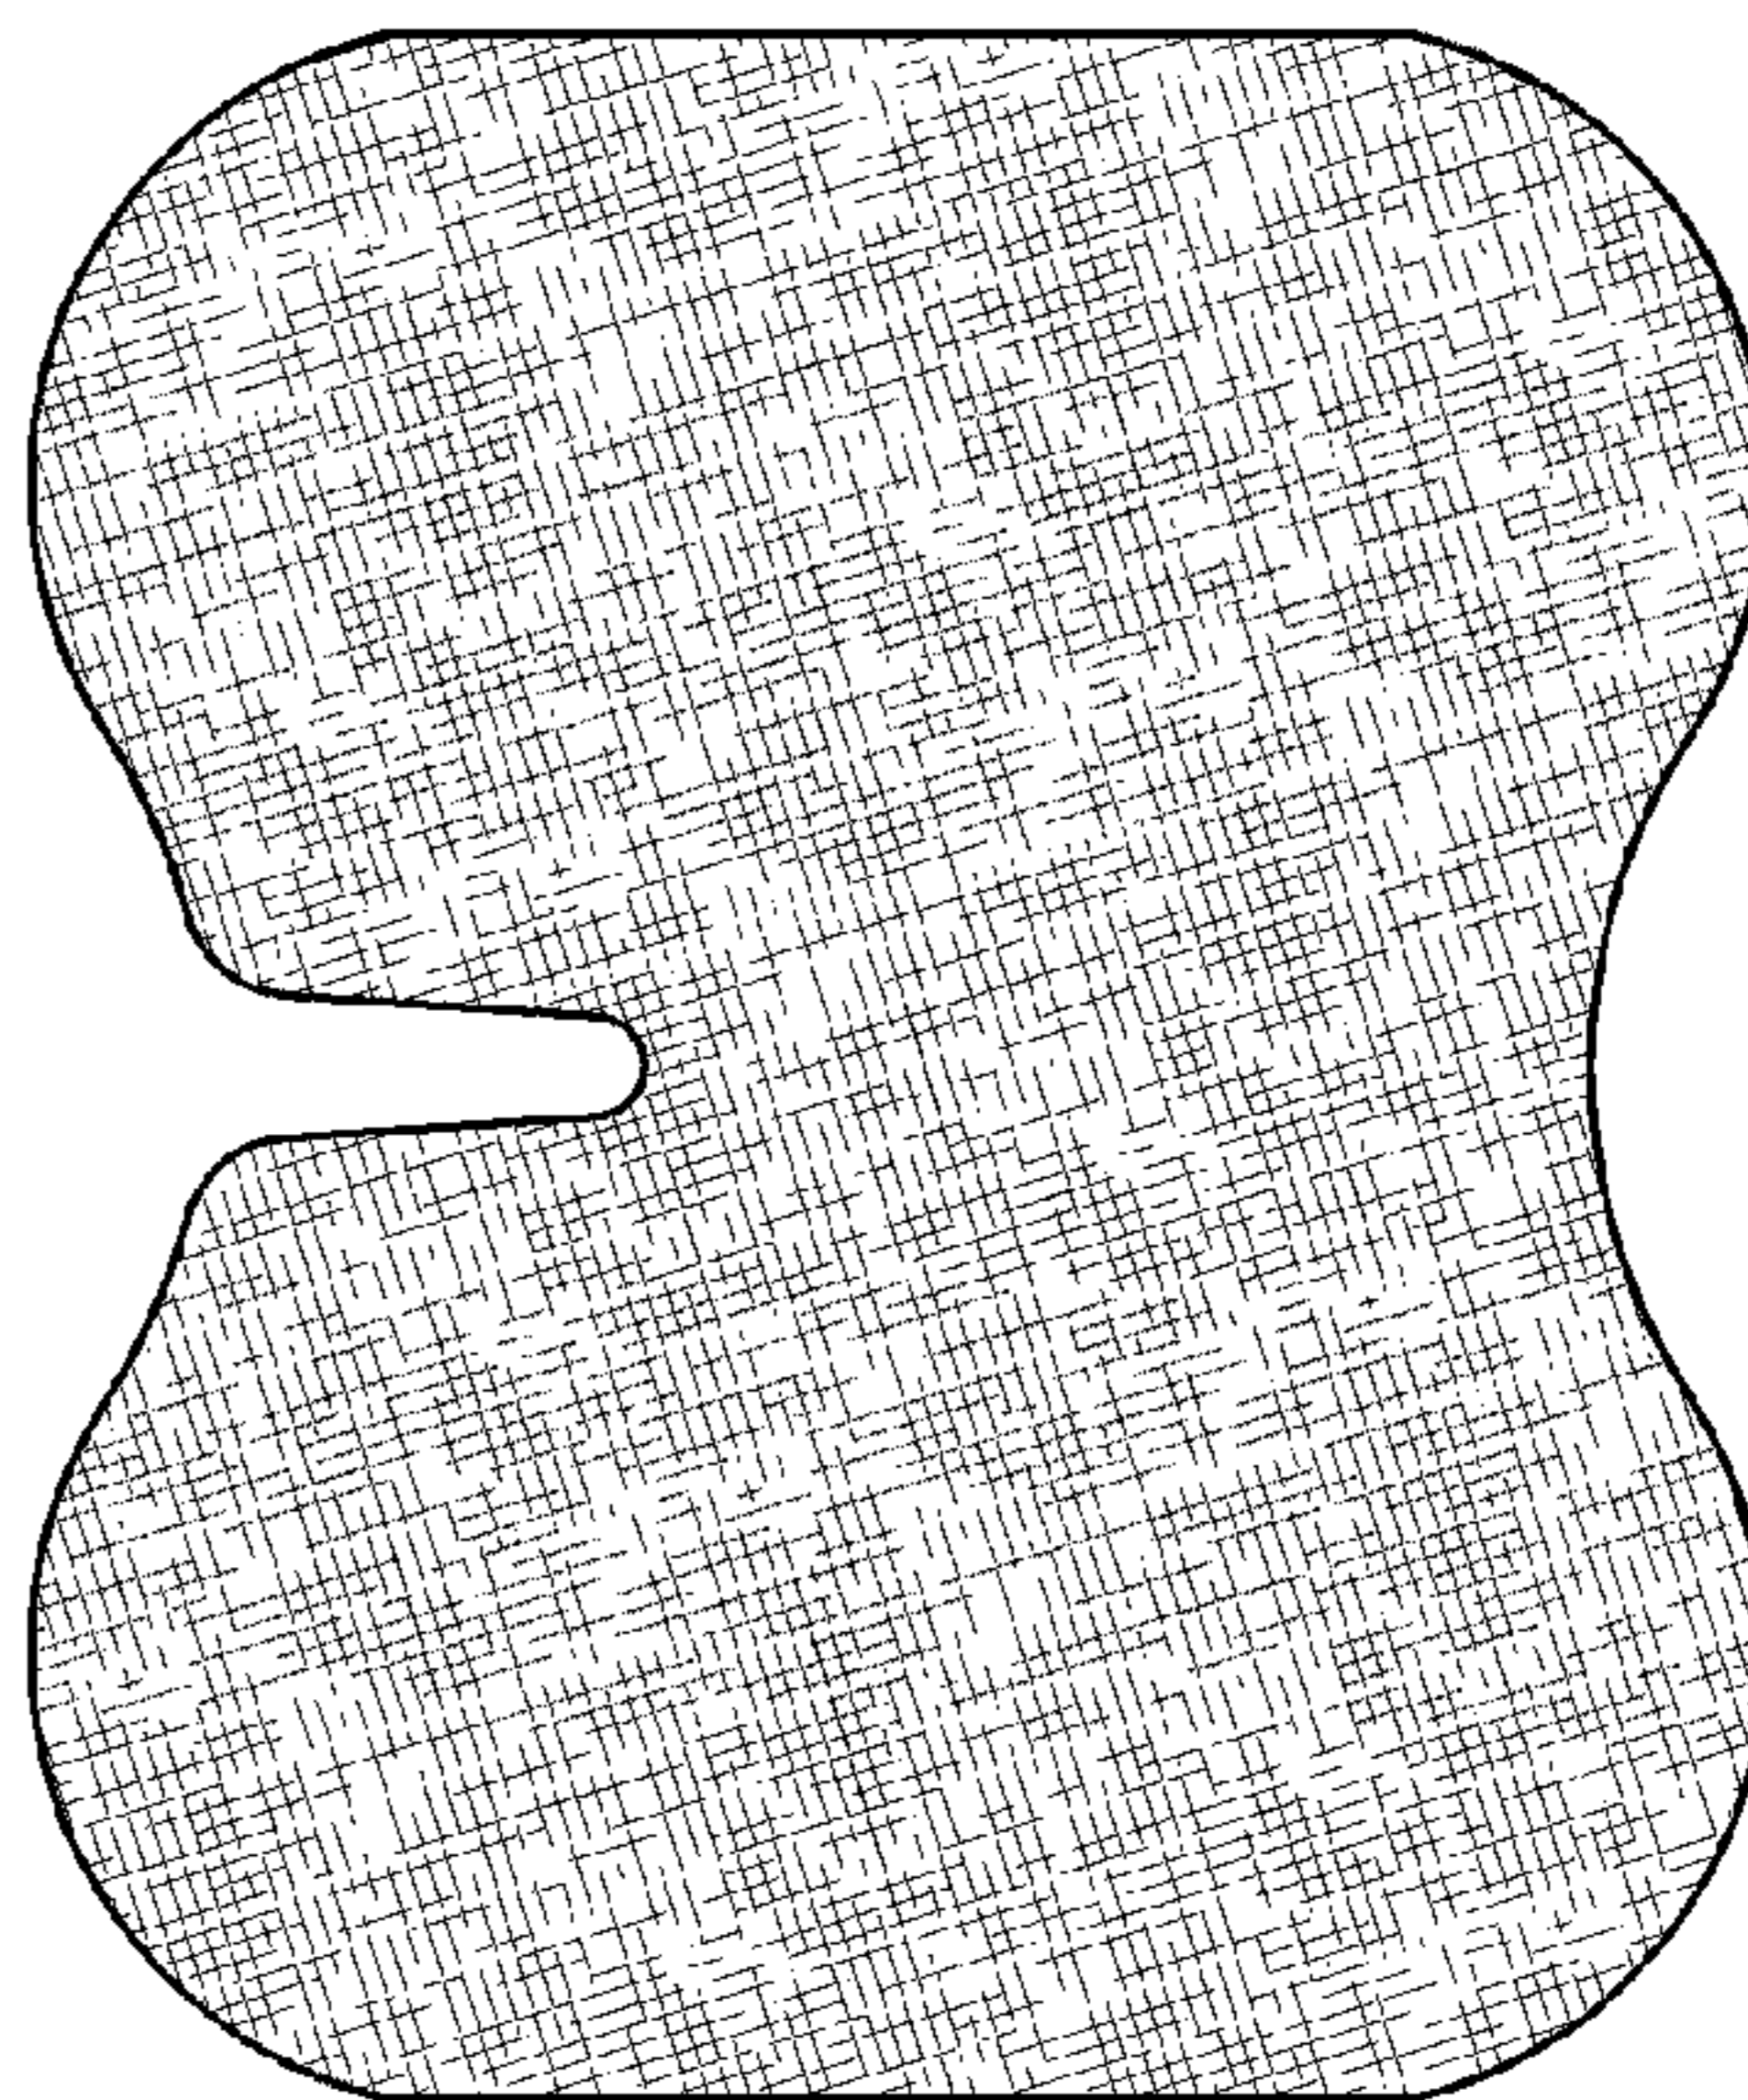

*Fig. 9*



*Fig. 10*



*Fig. 11*



*Fig. 12*