



US00D664258S

(12) **United States Design Patent**  
**Harkin et al.**

(10) **Patent No.:** **US D664,258 S**  
(45) **Date of Patent:** **\*\* Jul. 24, 2012**

(54) **DIAGNOSTIC DEVICE**

(75) Inventors: **Thomas Harkin**, Bristol (GB);  
**Christopher Kilbane**, Bristol (GB);  
**Sebastian Liedtke**, Heidelberg (DE)

(73) Assignee: **Roche Diagnostics Operations, Inc.**,  
Indianapolis, IN (US)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/410,473**

(22) Filed: **Jan. 9, 2012**

(30) **Foreign Application Priority Data**

Jul. 15, 2011	(EM)	001285605-0001
Jul. 15, 2011	(EM)	001285605-0002
Jul. 15, 2011	(EM)	001285605-0003
Jul. 15, 2011	(EM)	001285605-0004

(51) **LOC (9) Cl.** ..... **24-01**

(52) **U.S. Cl.** ..... **D24/186; D24/169**

(58) **Field of Classification Search** ..... D24/169,  
D24/186, 133, 146, 200, 158; D10/81; 600/309,  
600/316, 322, 365, 368; 422/56, 63, 65,  
422/102, 104

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D461,895 S *	8/2002	Barnes et al.	.....	D24/158
D493,532 S *	7/2004	Levaughn et al.	.....	D24/147
D505,726 S *	5/2005	Ryan	.....	D24/200
D530,424 S *	10/2006	Manser et al.	.....	D10/81
D544,605 S *	6/2007	Gumisawa et al.	.....	D24/186
D549,830 S *	8/2007	Behar et al.	.....	D24/186

(Continued)

*Primary Examiner* — T. Chase Nelson

*Assistant Examiner* — Mark Cavanna

(74) *Attorney, Agent, or Firm* — Bose McKinney & Evans  
LLP

(57) **CLAIM**

The ornamental design for a diagnostic device, as shown and described.

**DESCRIPTION**

FIG. 1 is a first perspective view of the diagnostic device that illustrates the novel design;

FIG. 2 is a second perspective view of the diagnostic device of FIG. 1;

FIG. 3 is a top view of the diagnostic device of FIG. 1;

FIG. 4 is a left view of the diagnostic device of FIG. 1;

FIG. 5 is a right view of the diagnostic device of FIG. 1;

FIG. 6 is a front view of the diagnostic device of FIG. 1;

FIG. 7 is a rear view of the diagnostic device of FIG. 1;

FIG. 8 is a bottom view of the diagnostic device of FIG. 1;

FIG. 9 is a bottom perspective view of the diagnostic device of FIG. 1;

FIG. 10 is a first perspective view of the diagnostic device of FIG. 1 without the removable lancing device;

FIG. 11 is a second perspective view of the diagnostic device of FIG. 10;

FIG. 12 is a top view of the diagnostic device of FIG. 10;

FIG. 13 is a left view of the diagnostic device of FIG. 10;

FIG. 14 is a right view of the diagnostic device of FIG. 10;


FIG. 15 is a front view of the diagnostic device of FIG. 10;

FIG. 16 is a rear view of the diagnostic device of FIG. 10;

FIG. 17 is a bottom view of the diagnostic device of FIG. 10; and,

FIG. 18 is a bottom perspective view of the diagnostic device of FIG. 10.

**1 Claim, 14 Drawing Sheets**

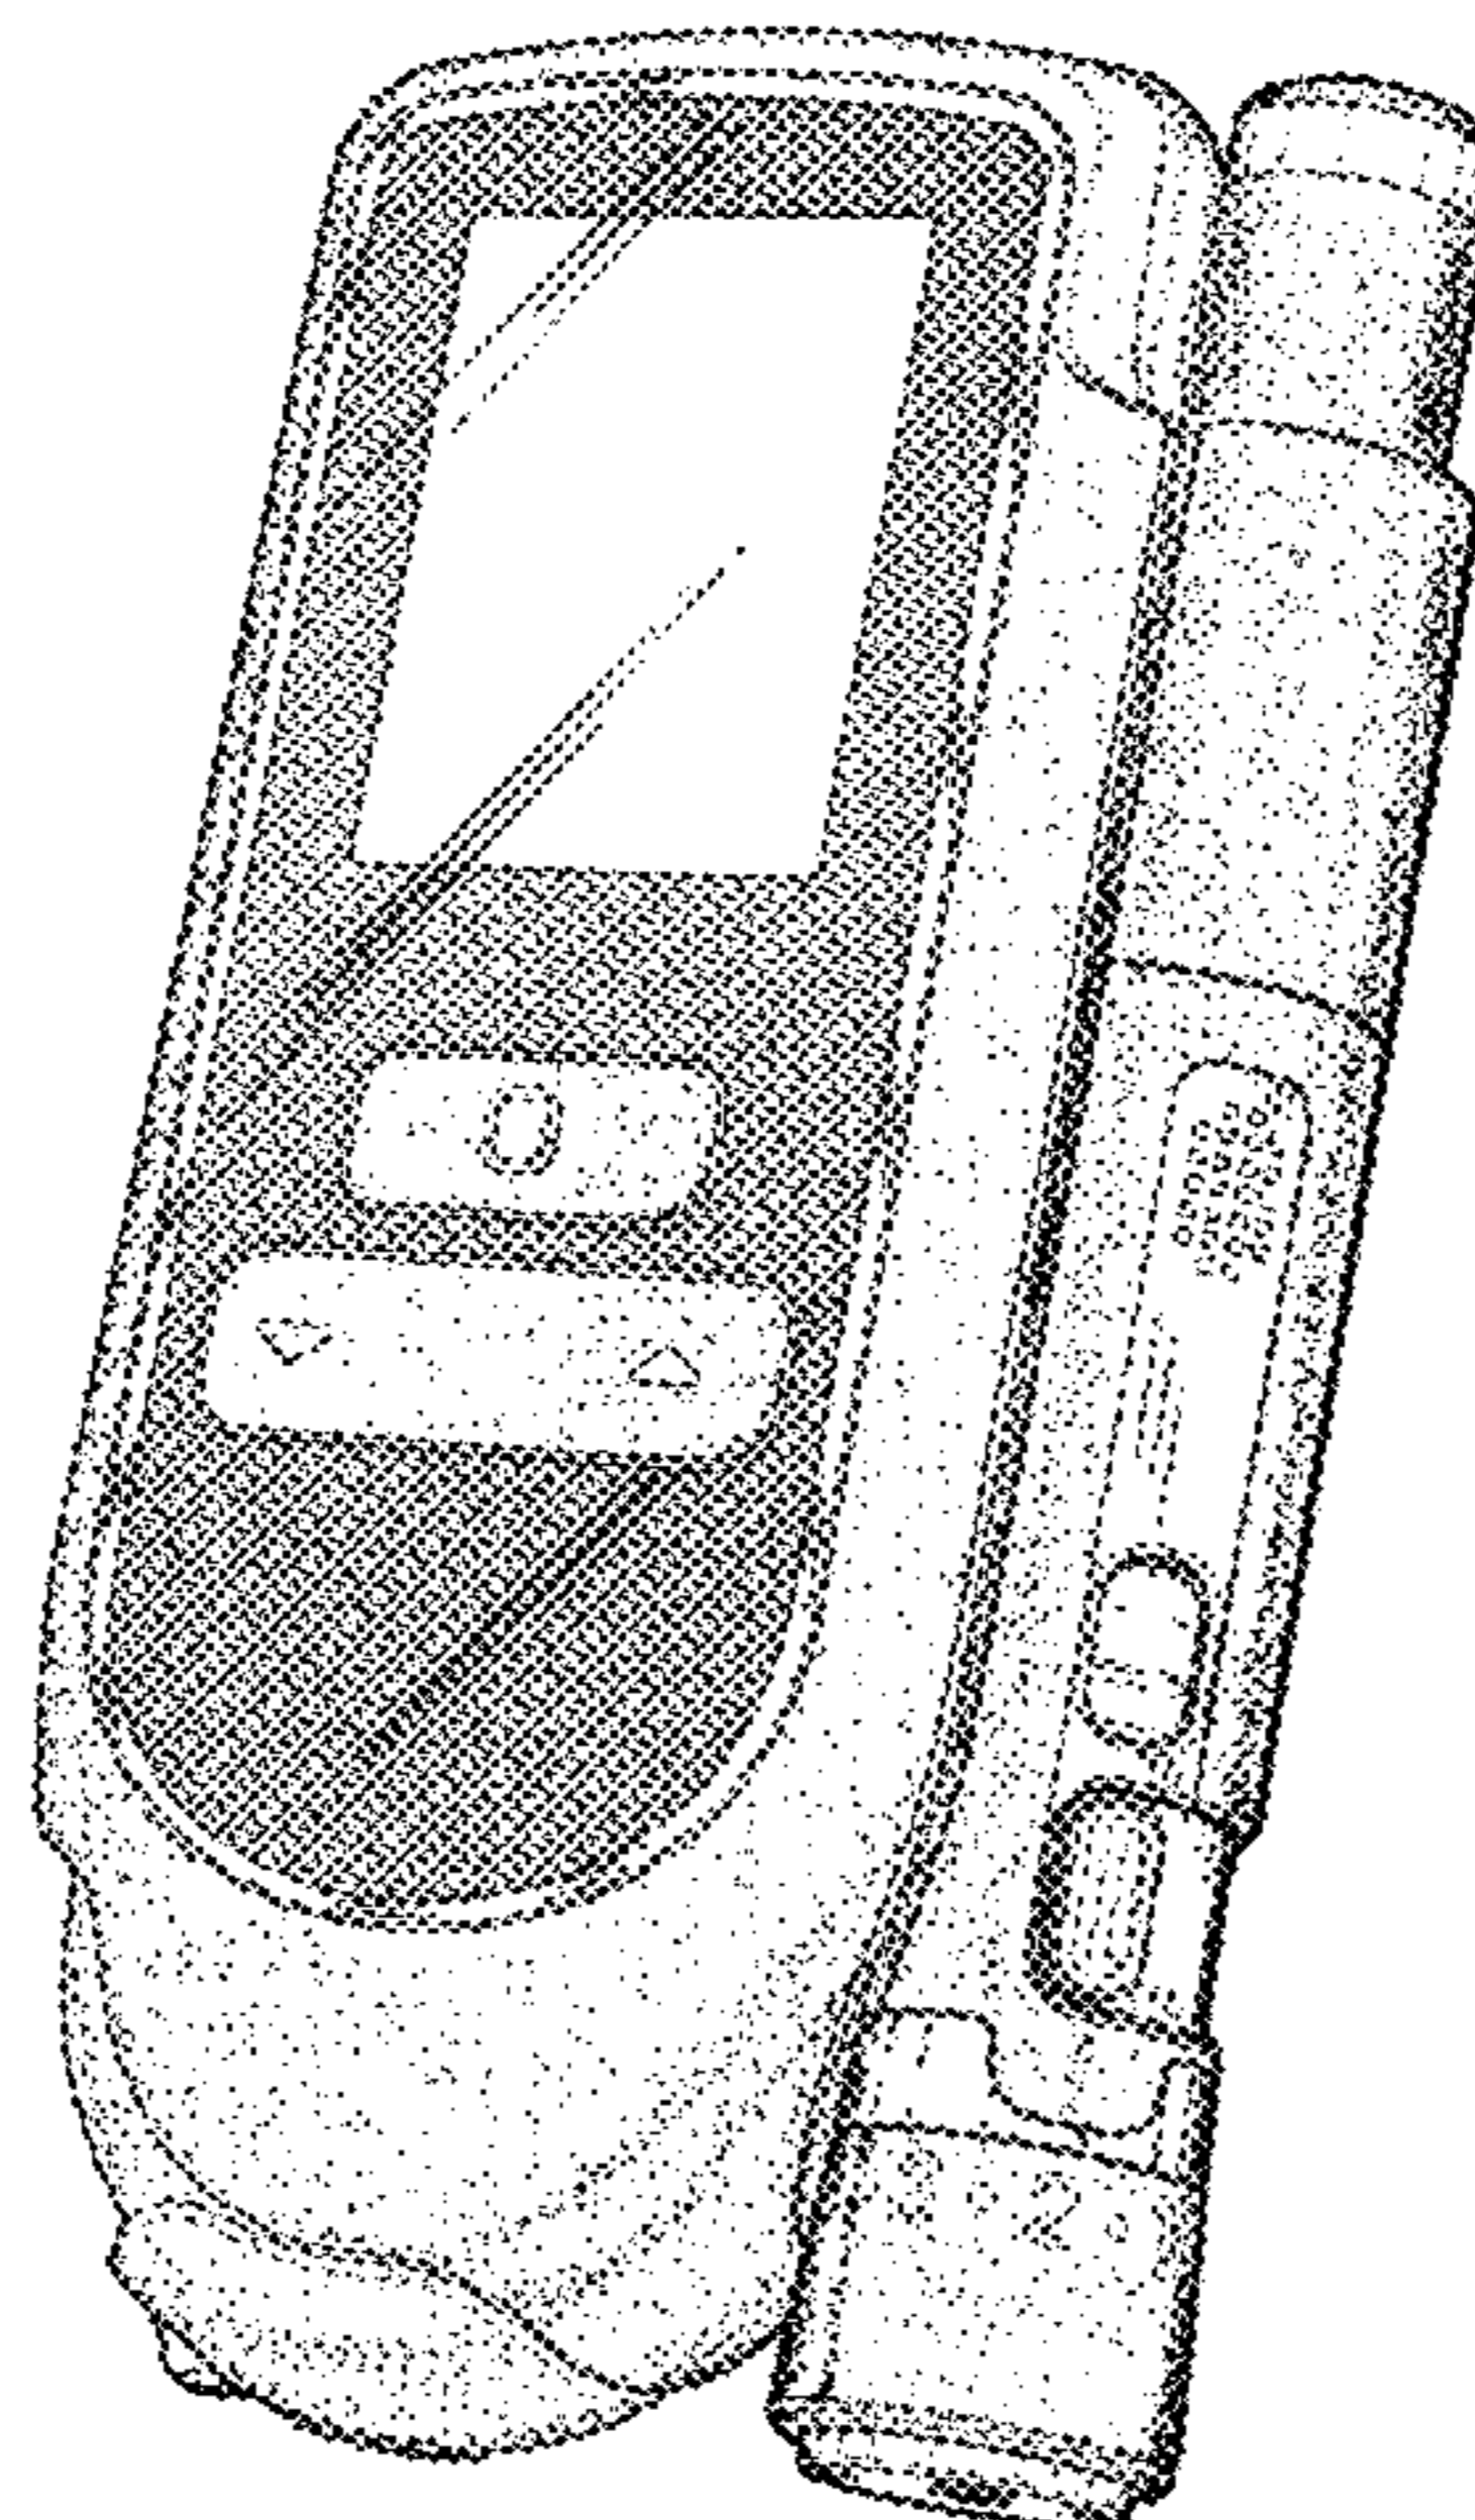

# US D664,258 S


Page 2

---


## U.S. PATENT DOCUMENTS

D550,363 S *	9/2007	Hannant et al. ....	D24/186	D629,522 S *	12/2010	Moscovita et al. ....	D24/169
D566,273 S *	4/2008	Gutmann et al. ....	D24/146	D634,432 S	3/2011	Liedtke et al.	
D569,982 S *	5/2008	Loerwald .....	D24/186	D634,435 S *	3/2011	Chua et al. ....	D24/186
D600,349 S *	9/2009	Bell et al. ....	D24/169	D637,287 S *	5/2011	Mudd et al. ....	D24/133
D610,688 S *	2/2010	Donars et al. ....	D24/169	D648,024 S *	11/2011	Harkin et al. ....	D24/146


\* cited by examiner

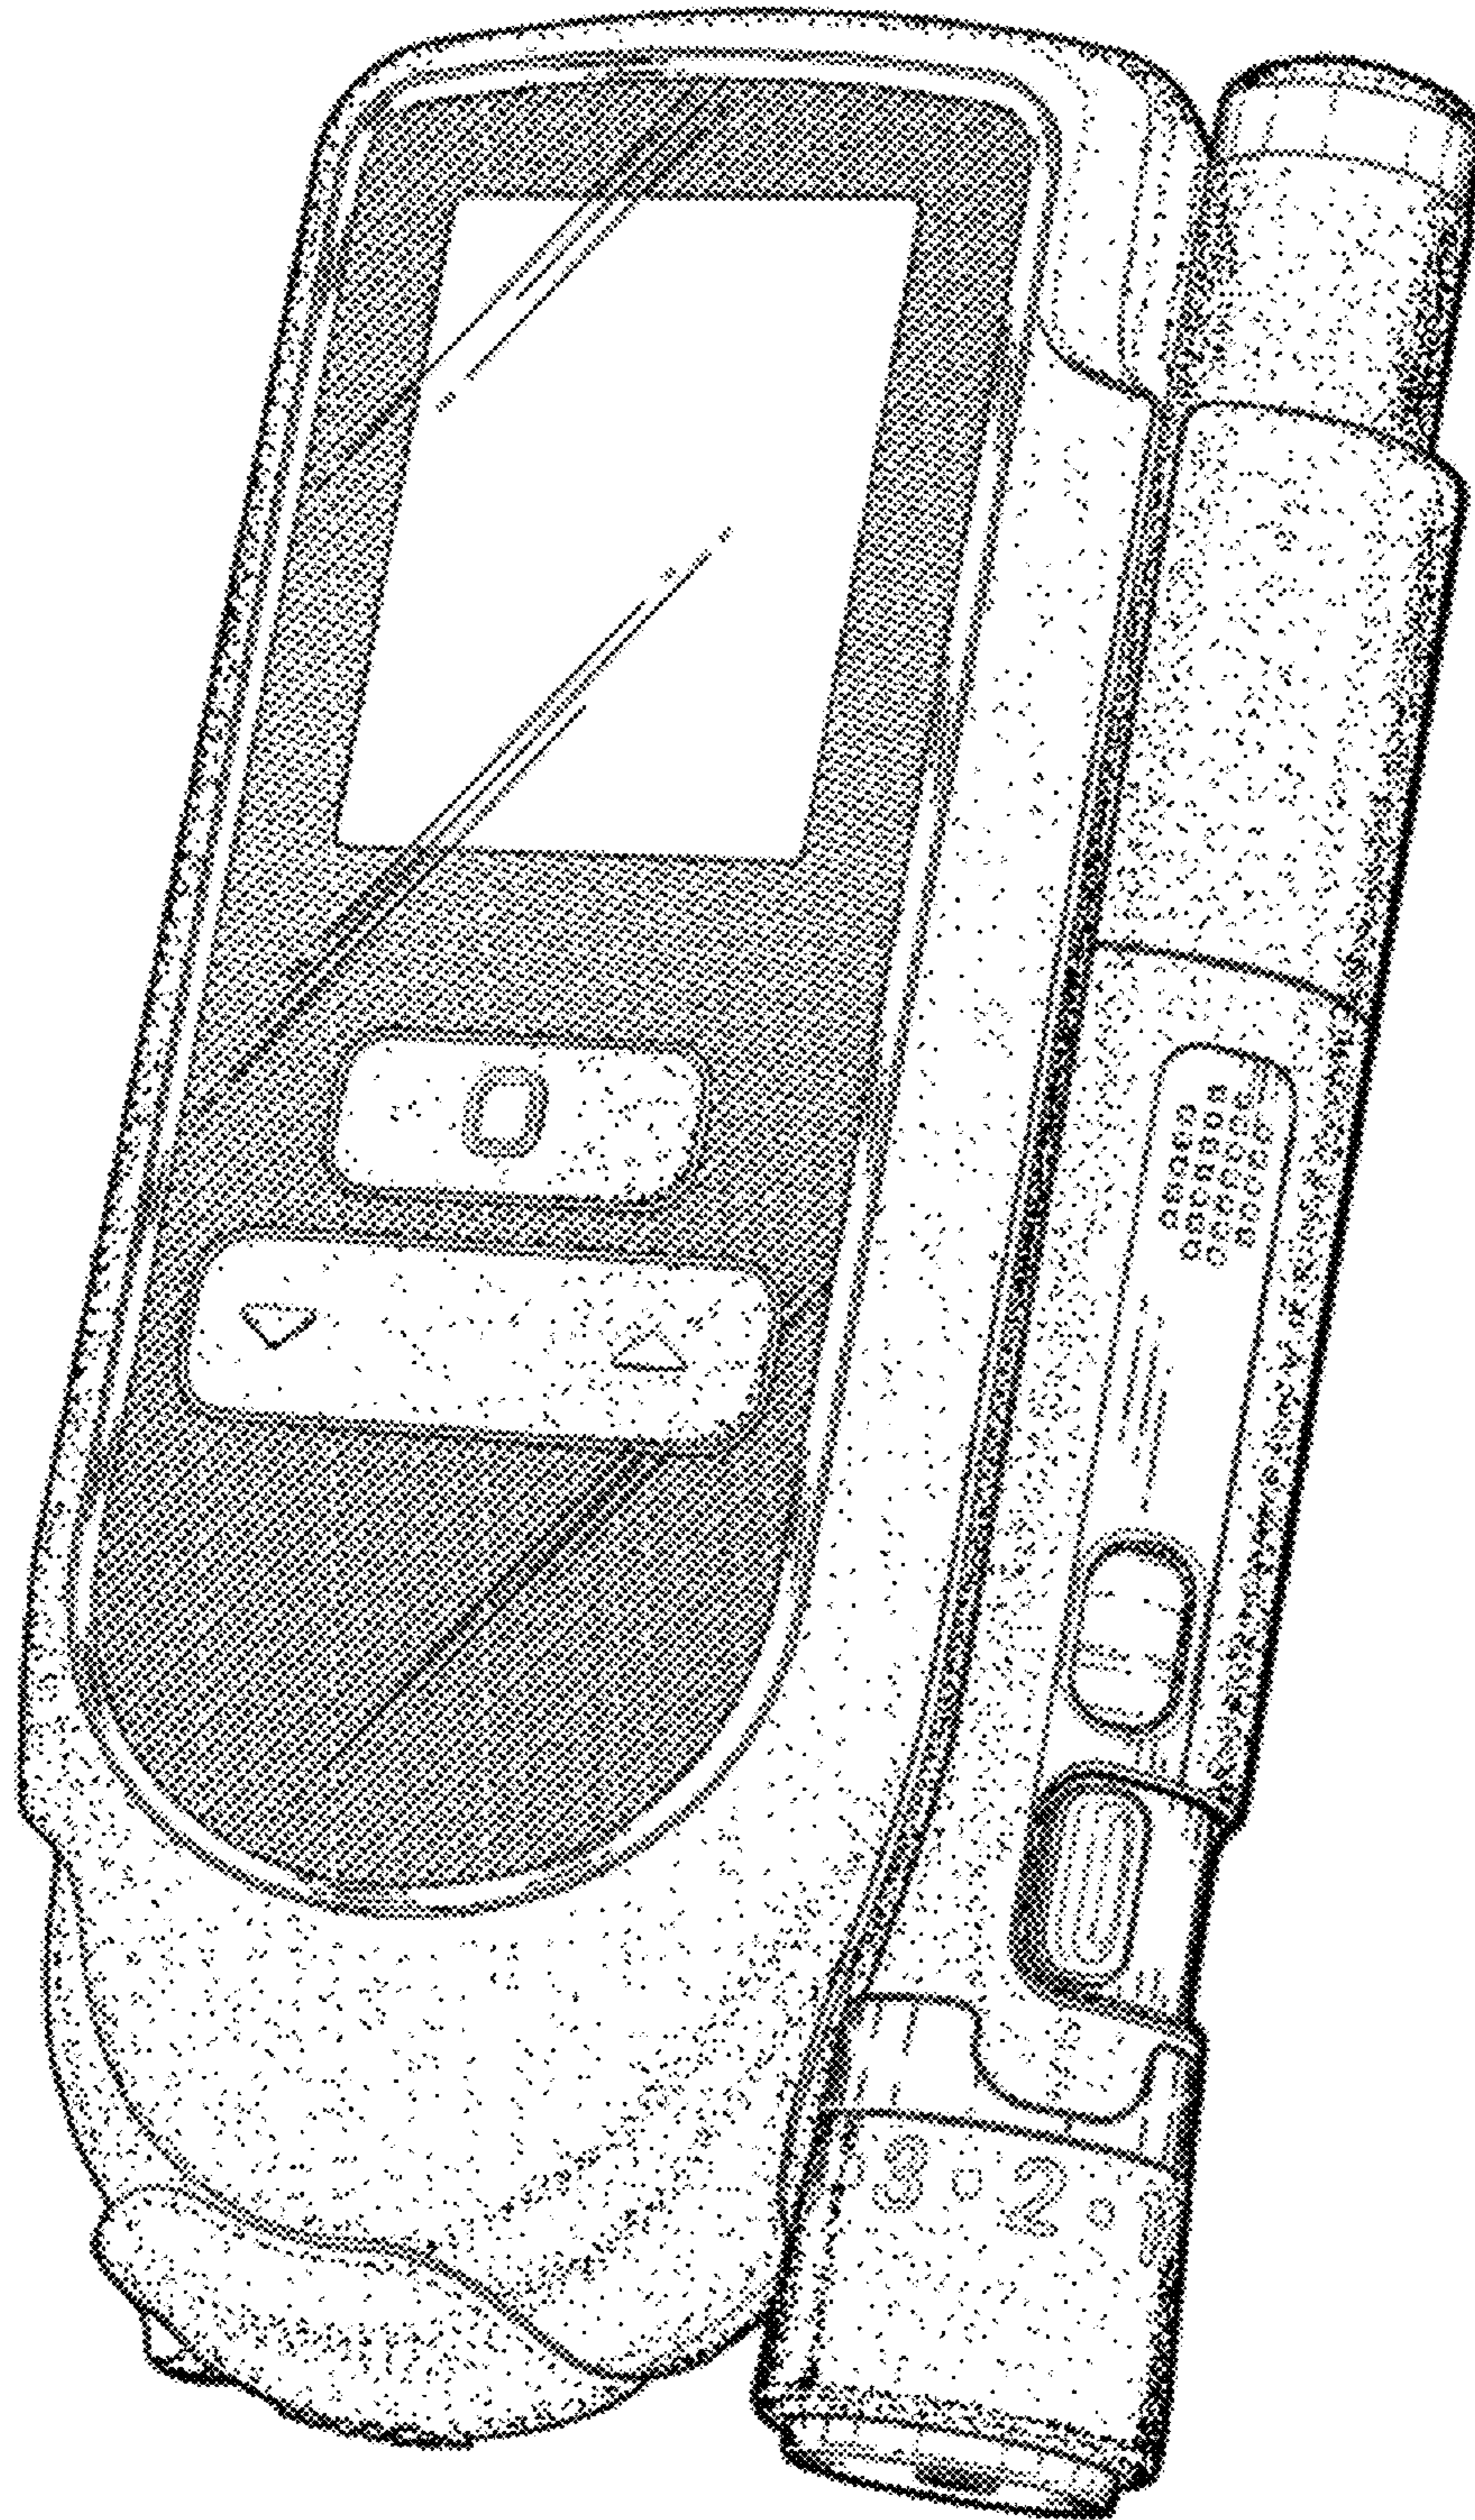


**Fig. 1**

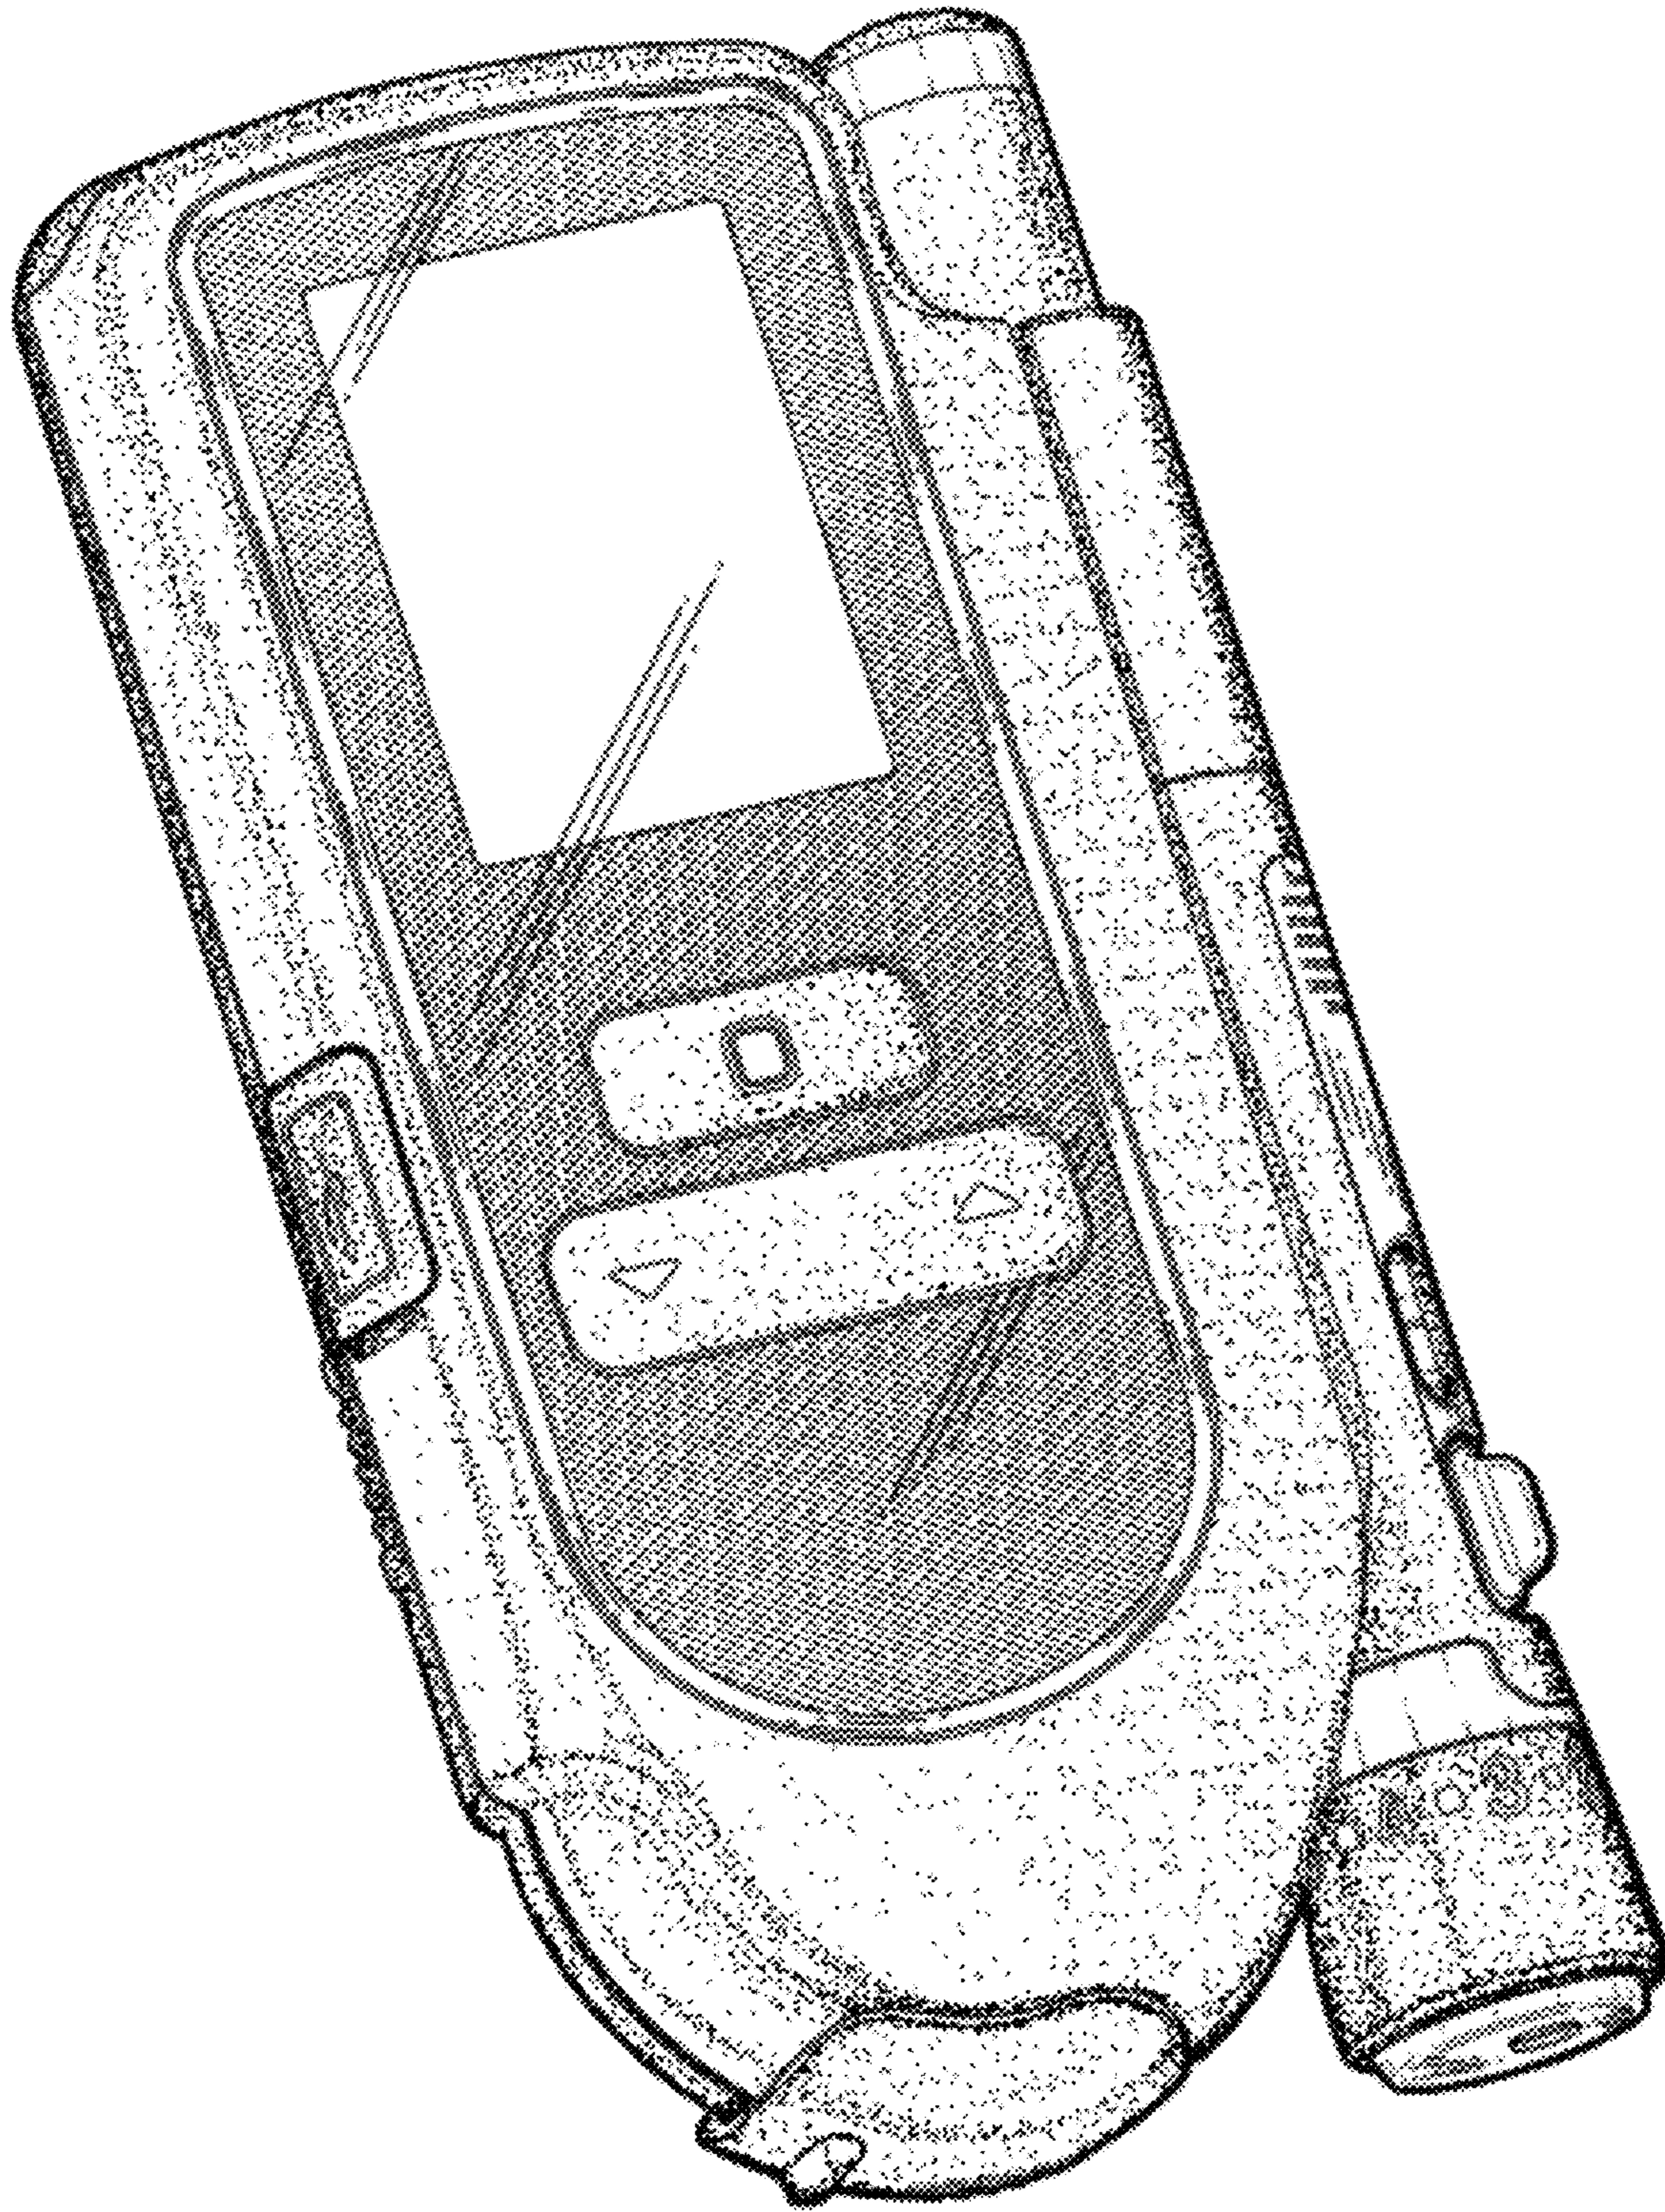


**Fig. 2**

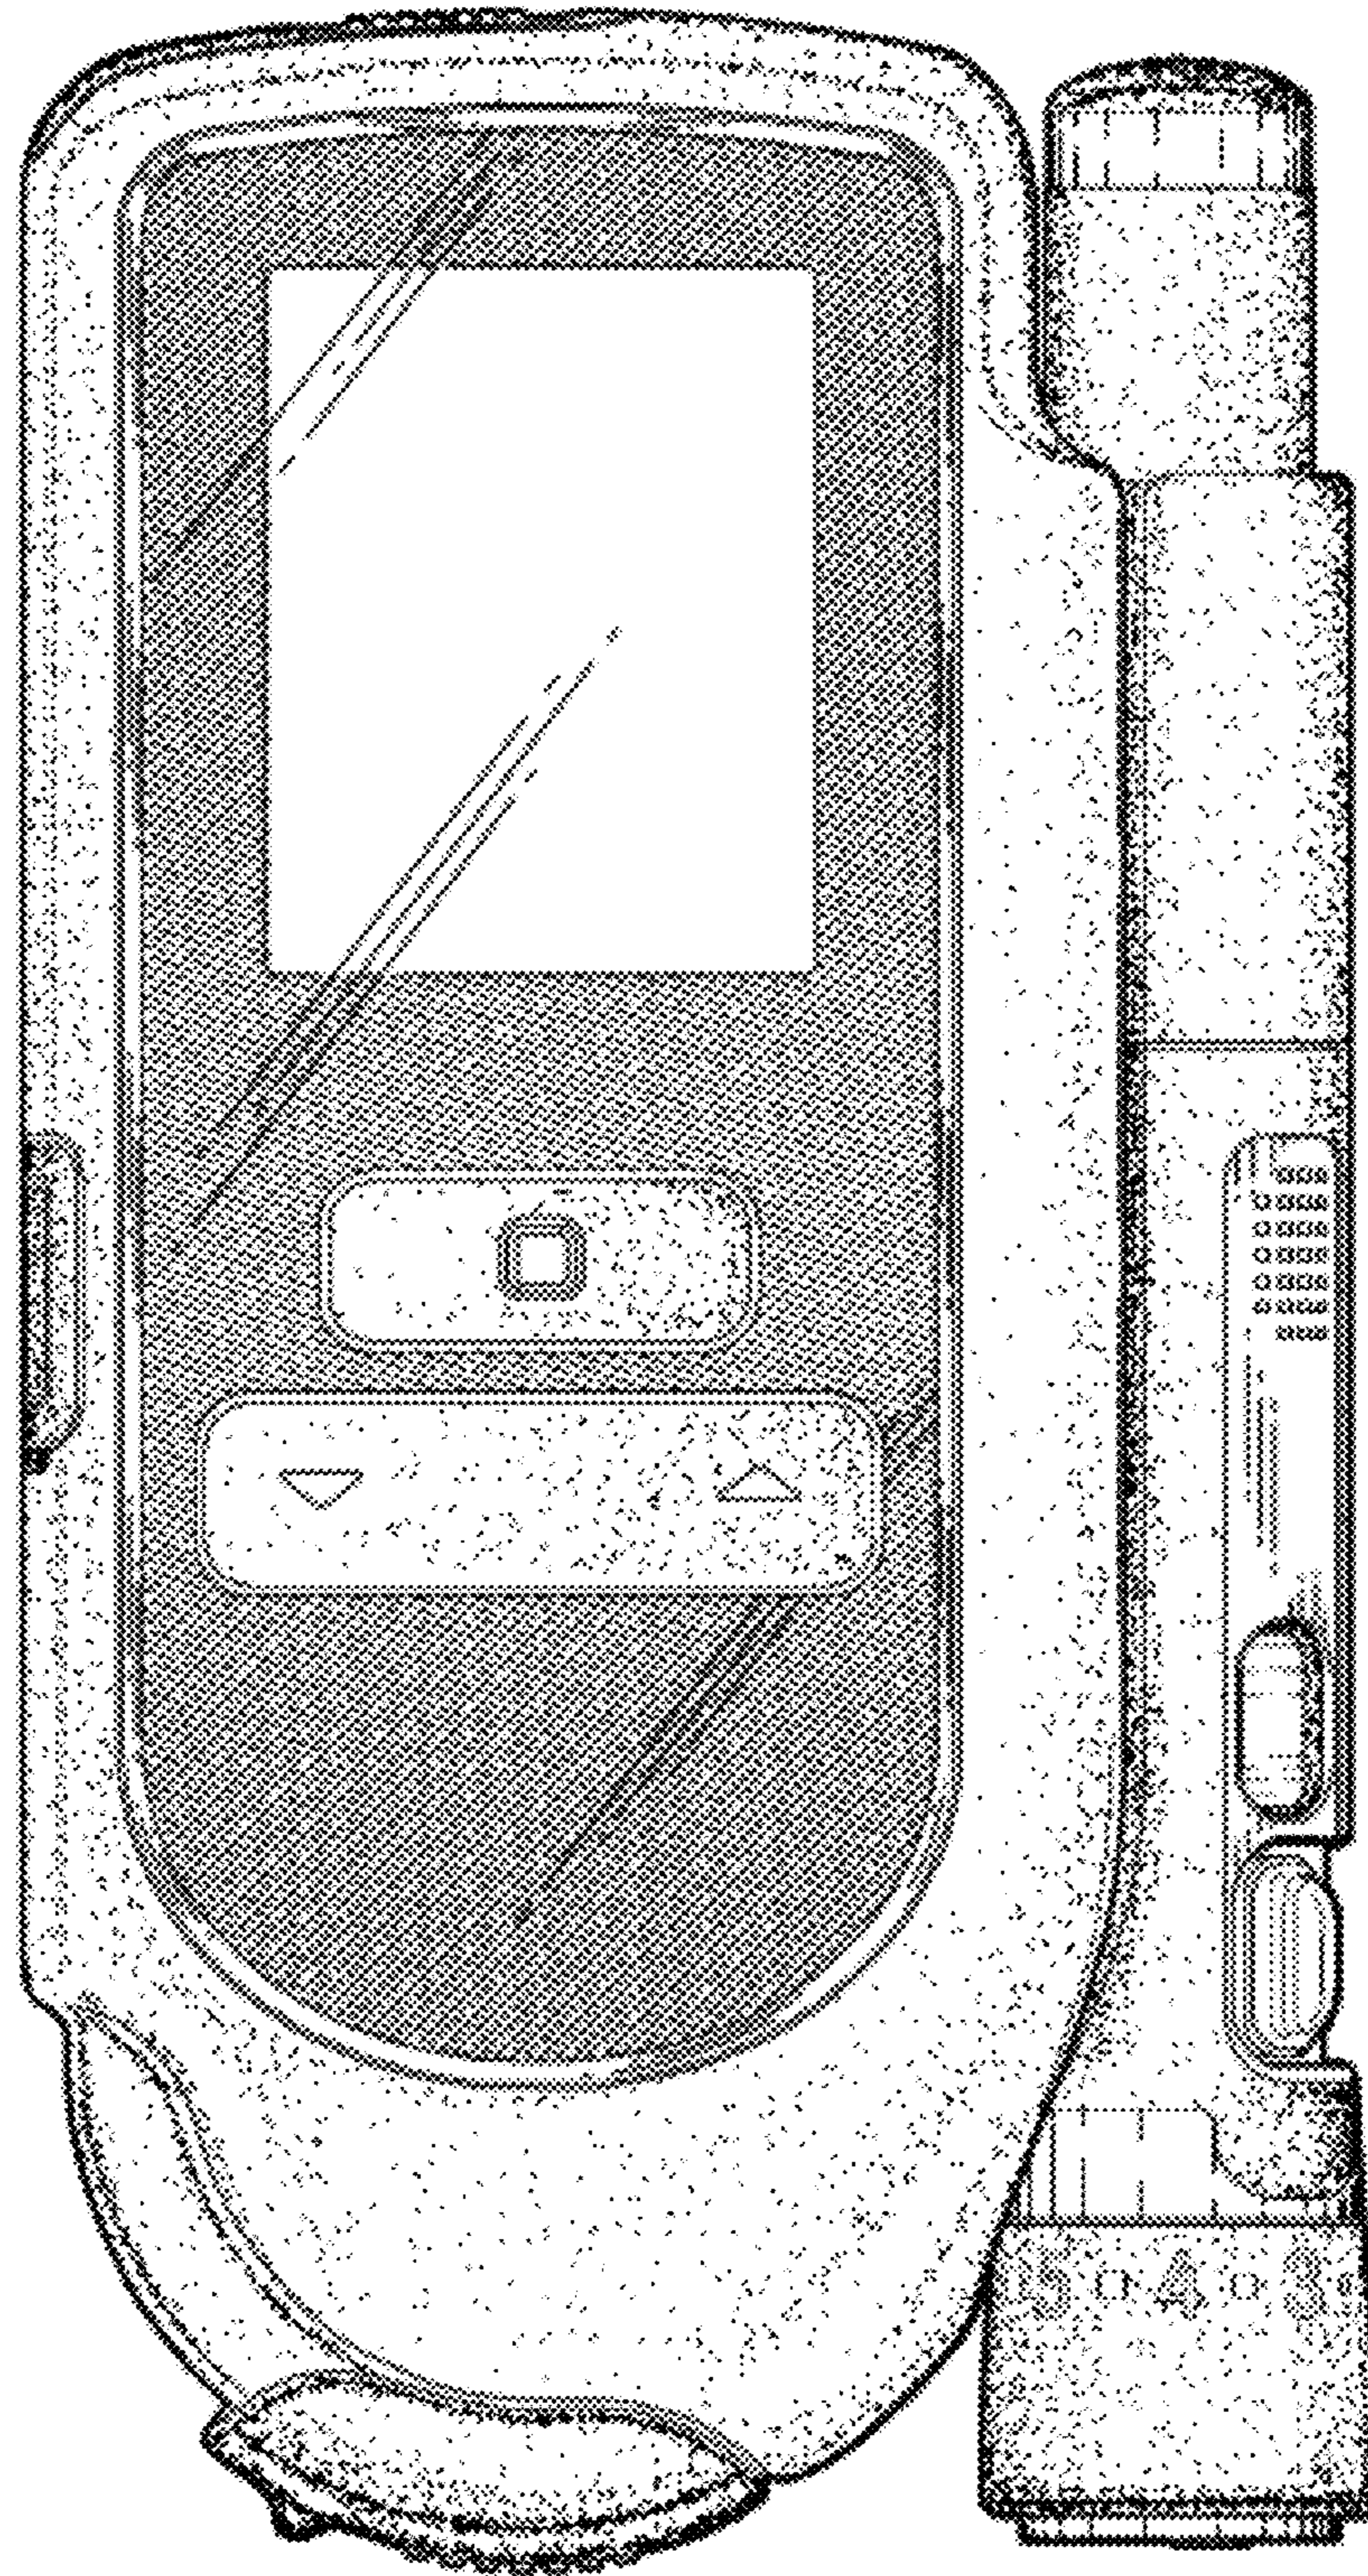


**Fig. 3**

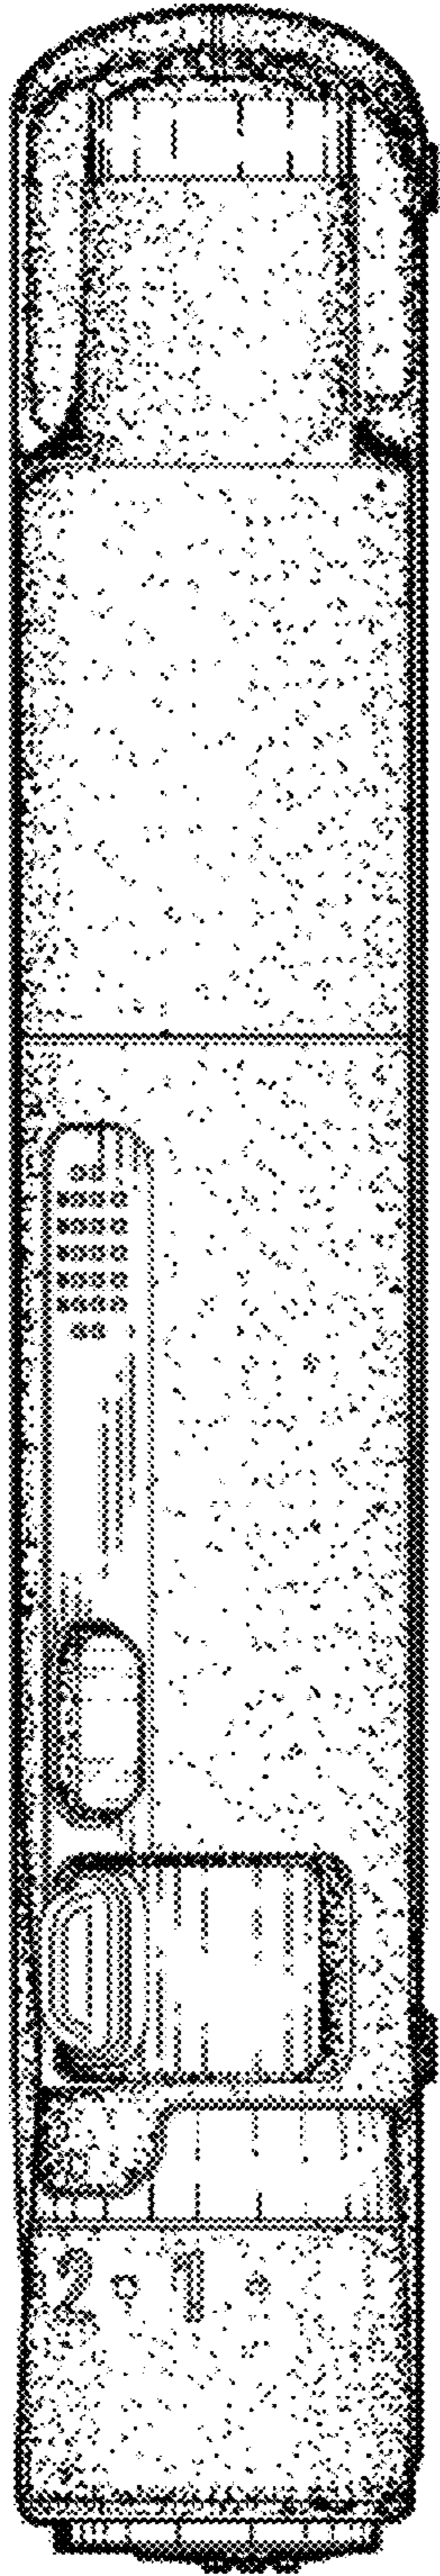


**Fig. 4**

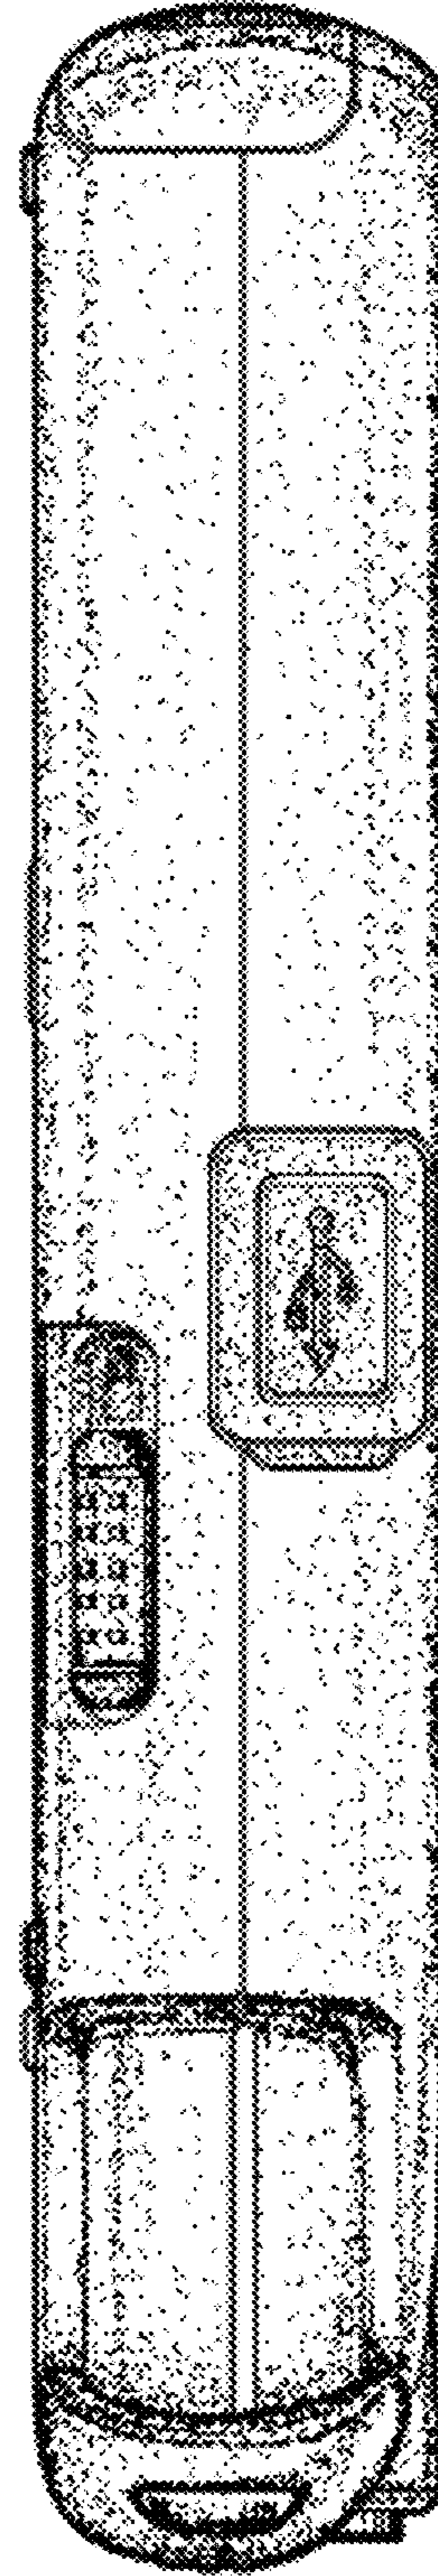


**Fig. 5**

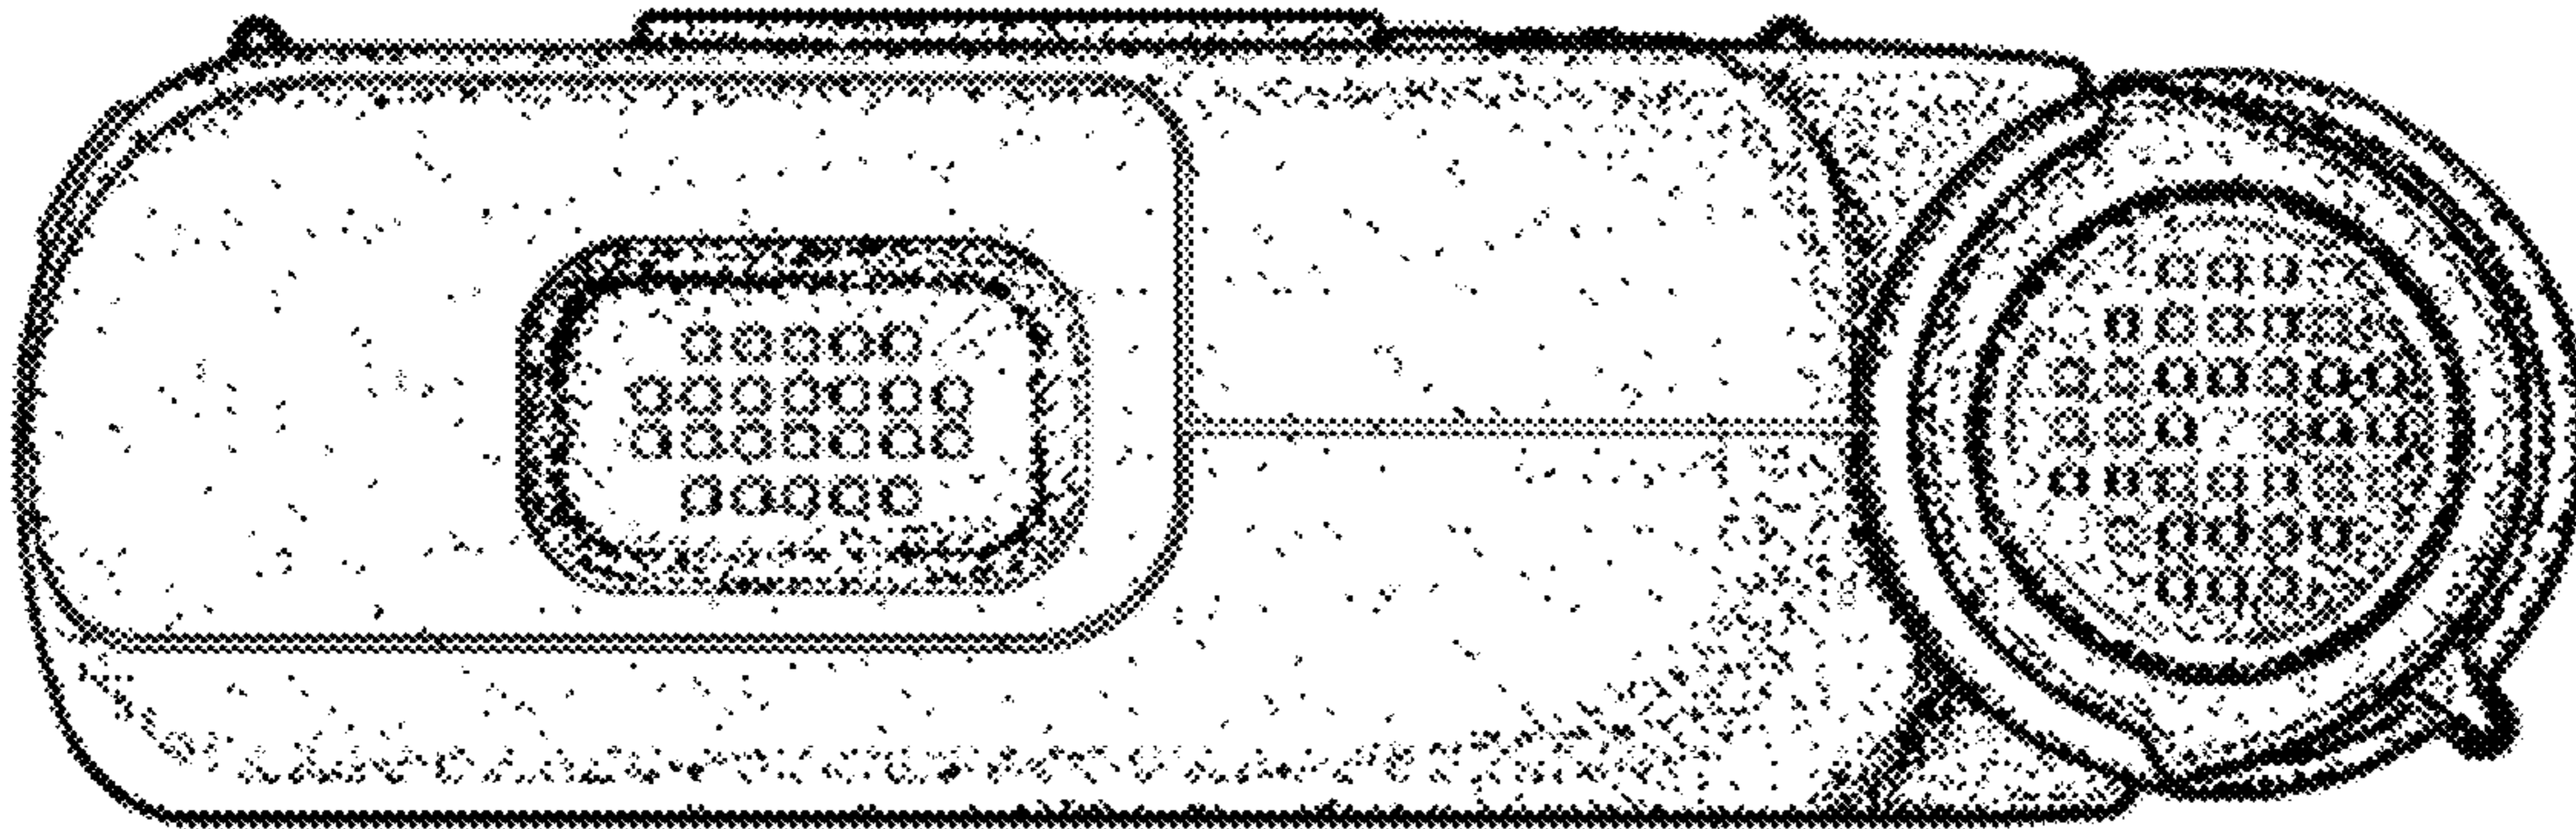

**Fig. 7**

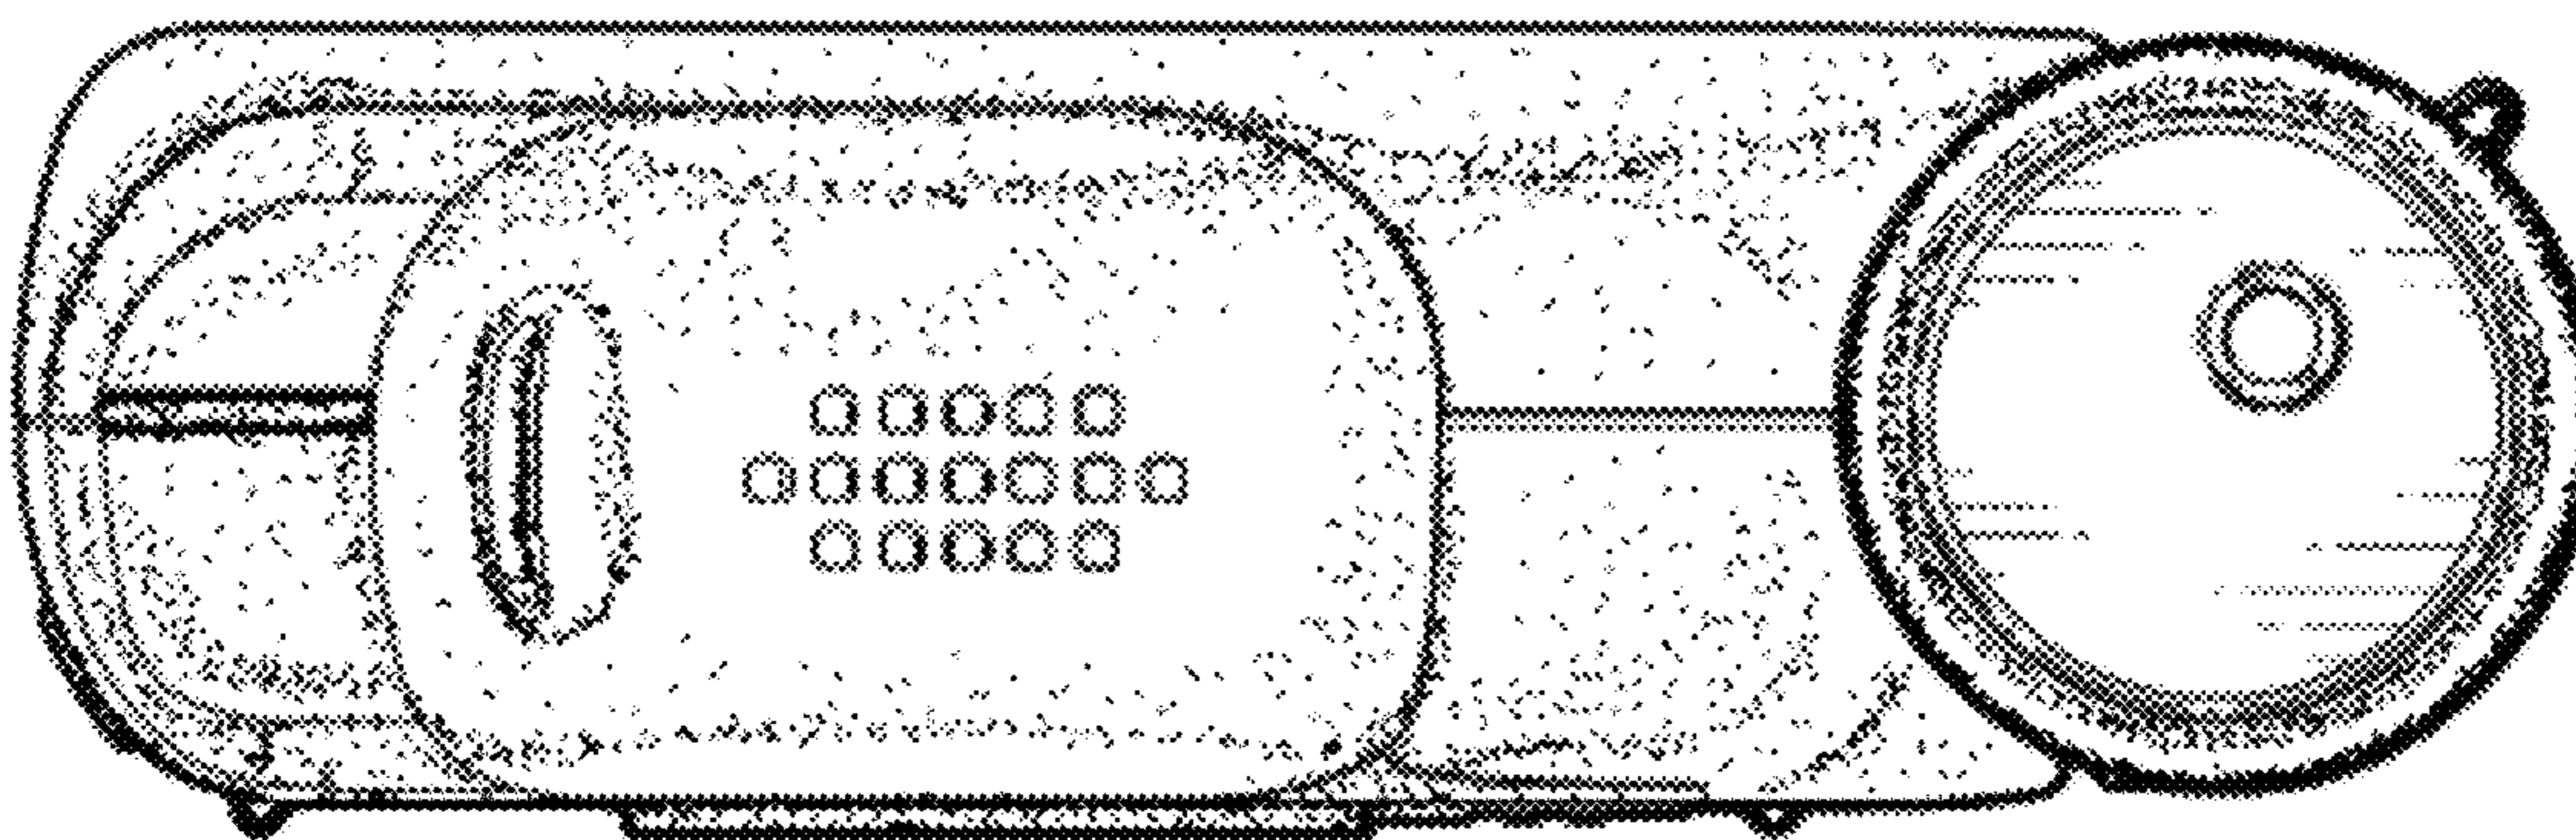


**Fig. 6**

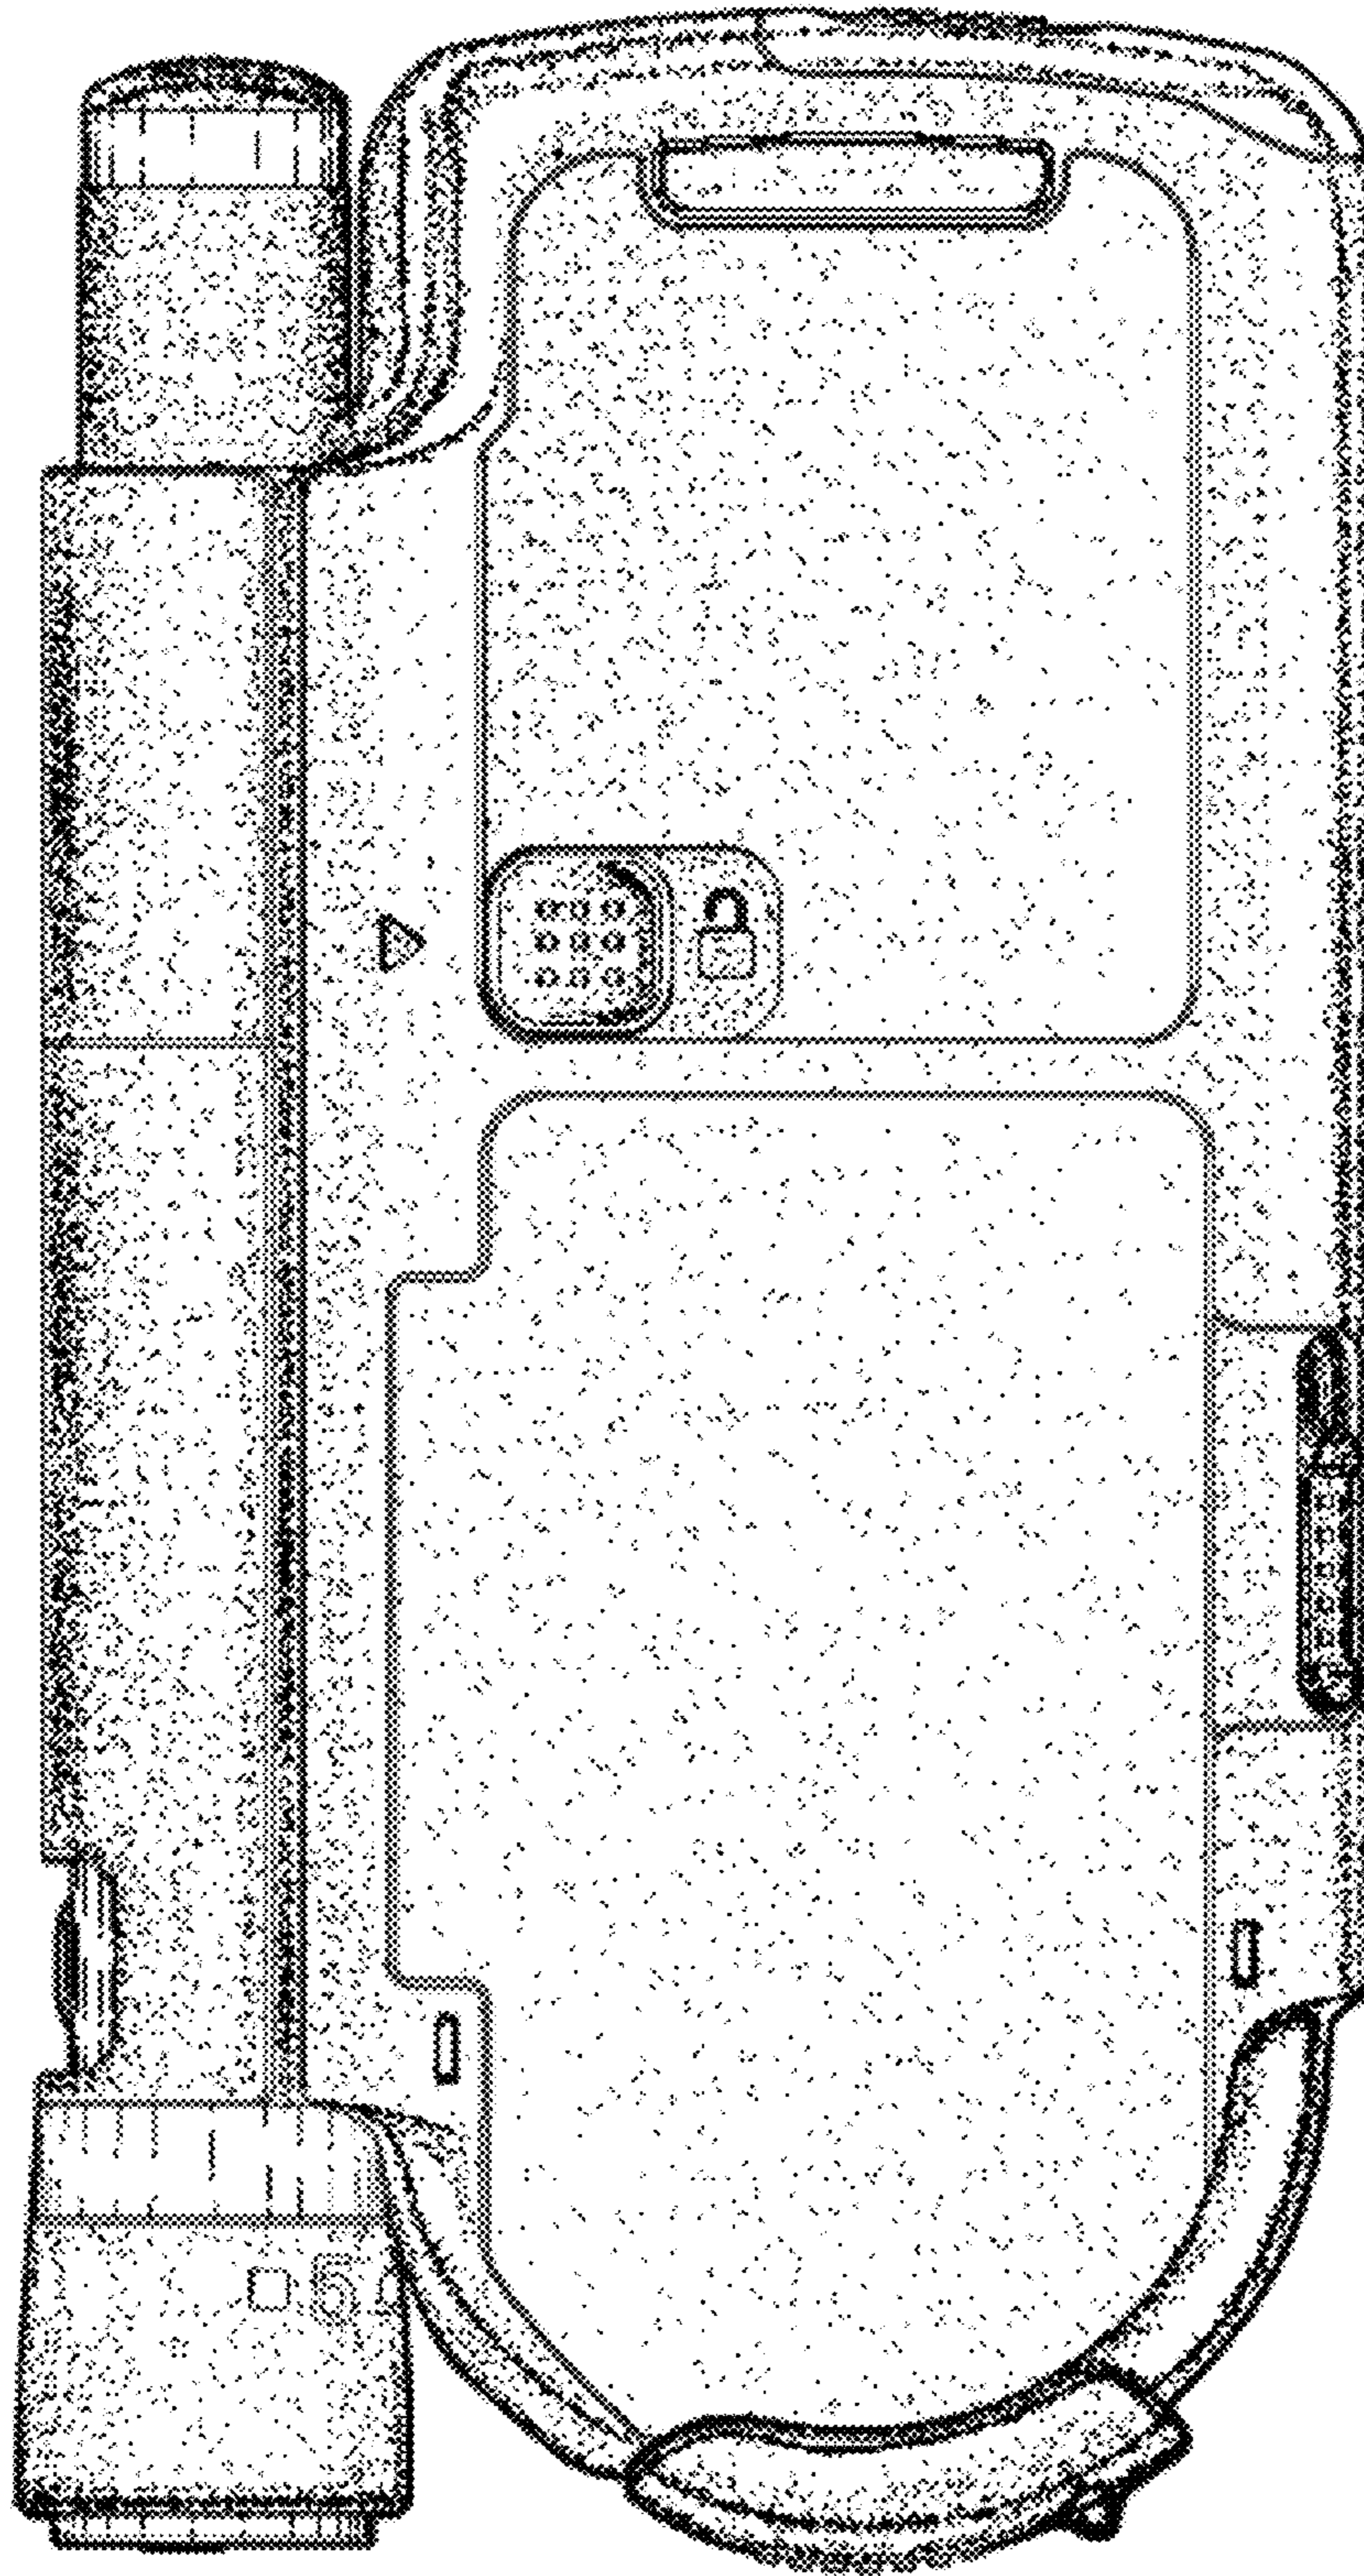


**Fig. 8**




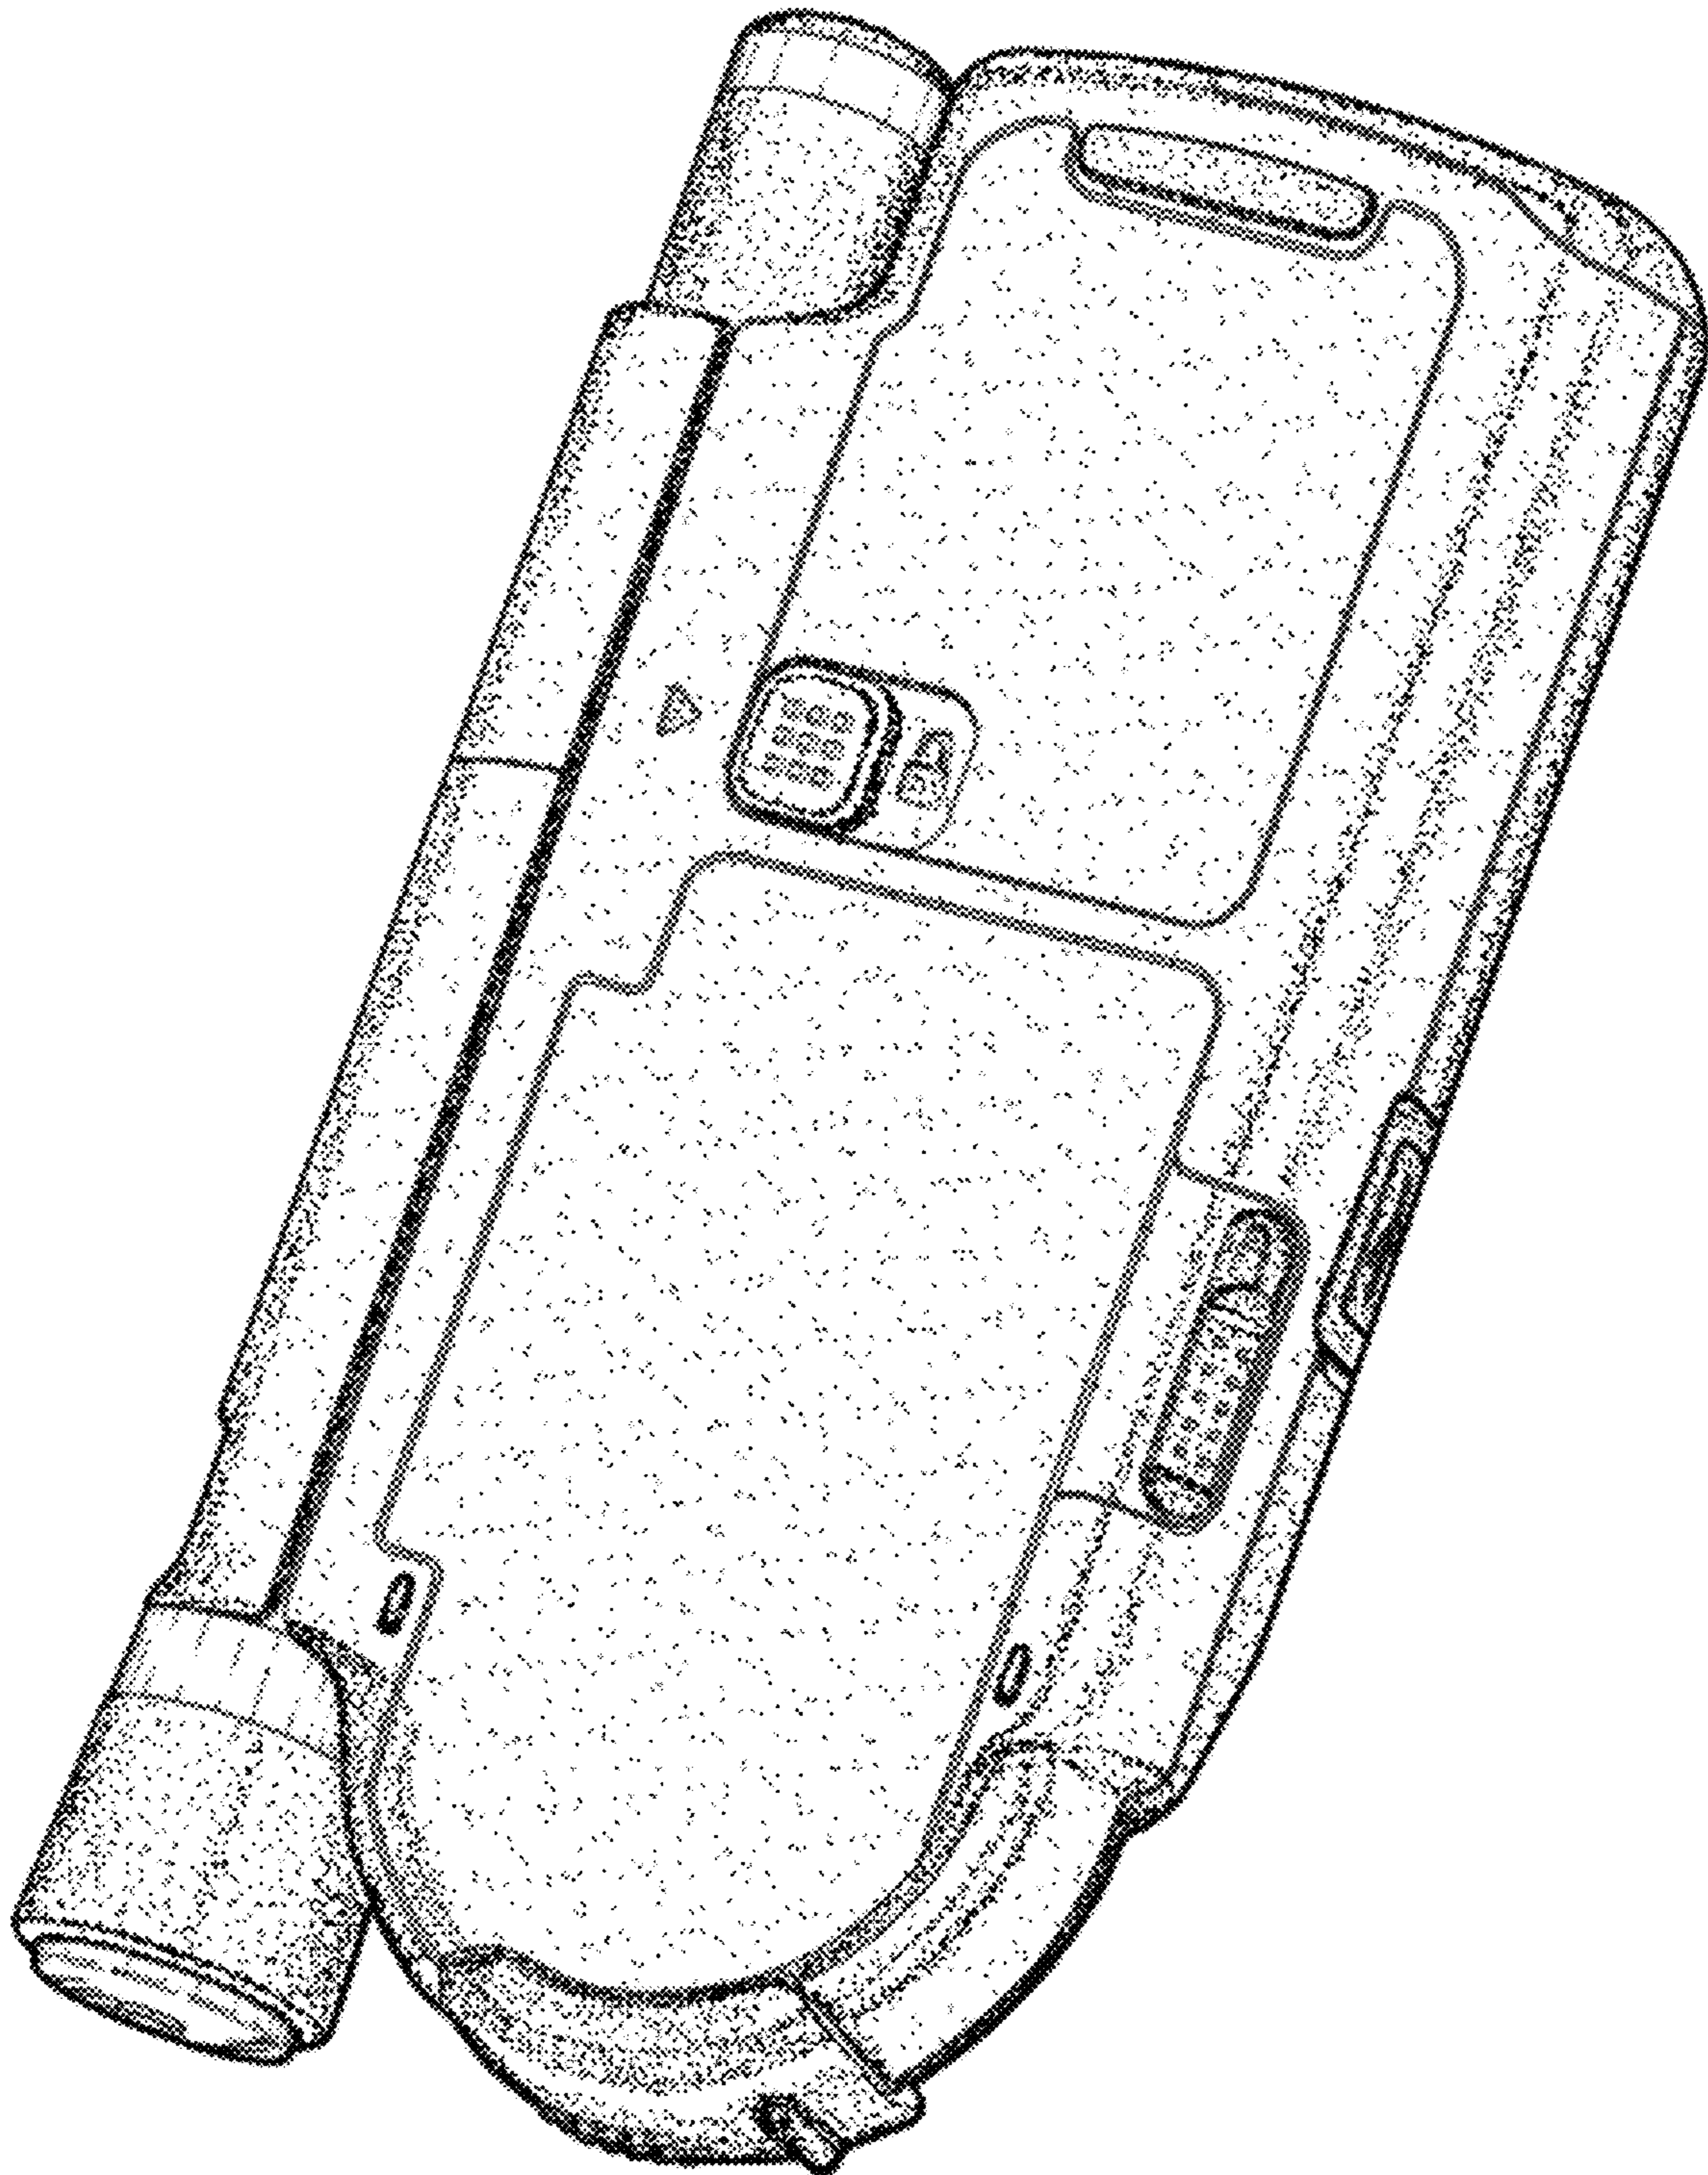


**Fig. 9**

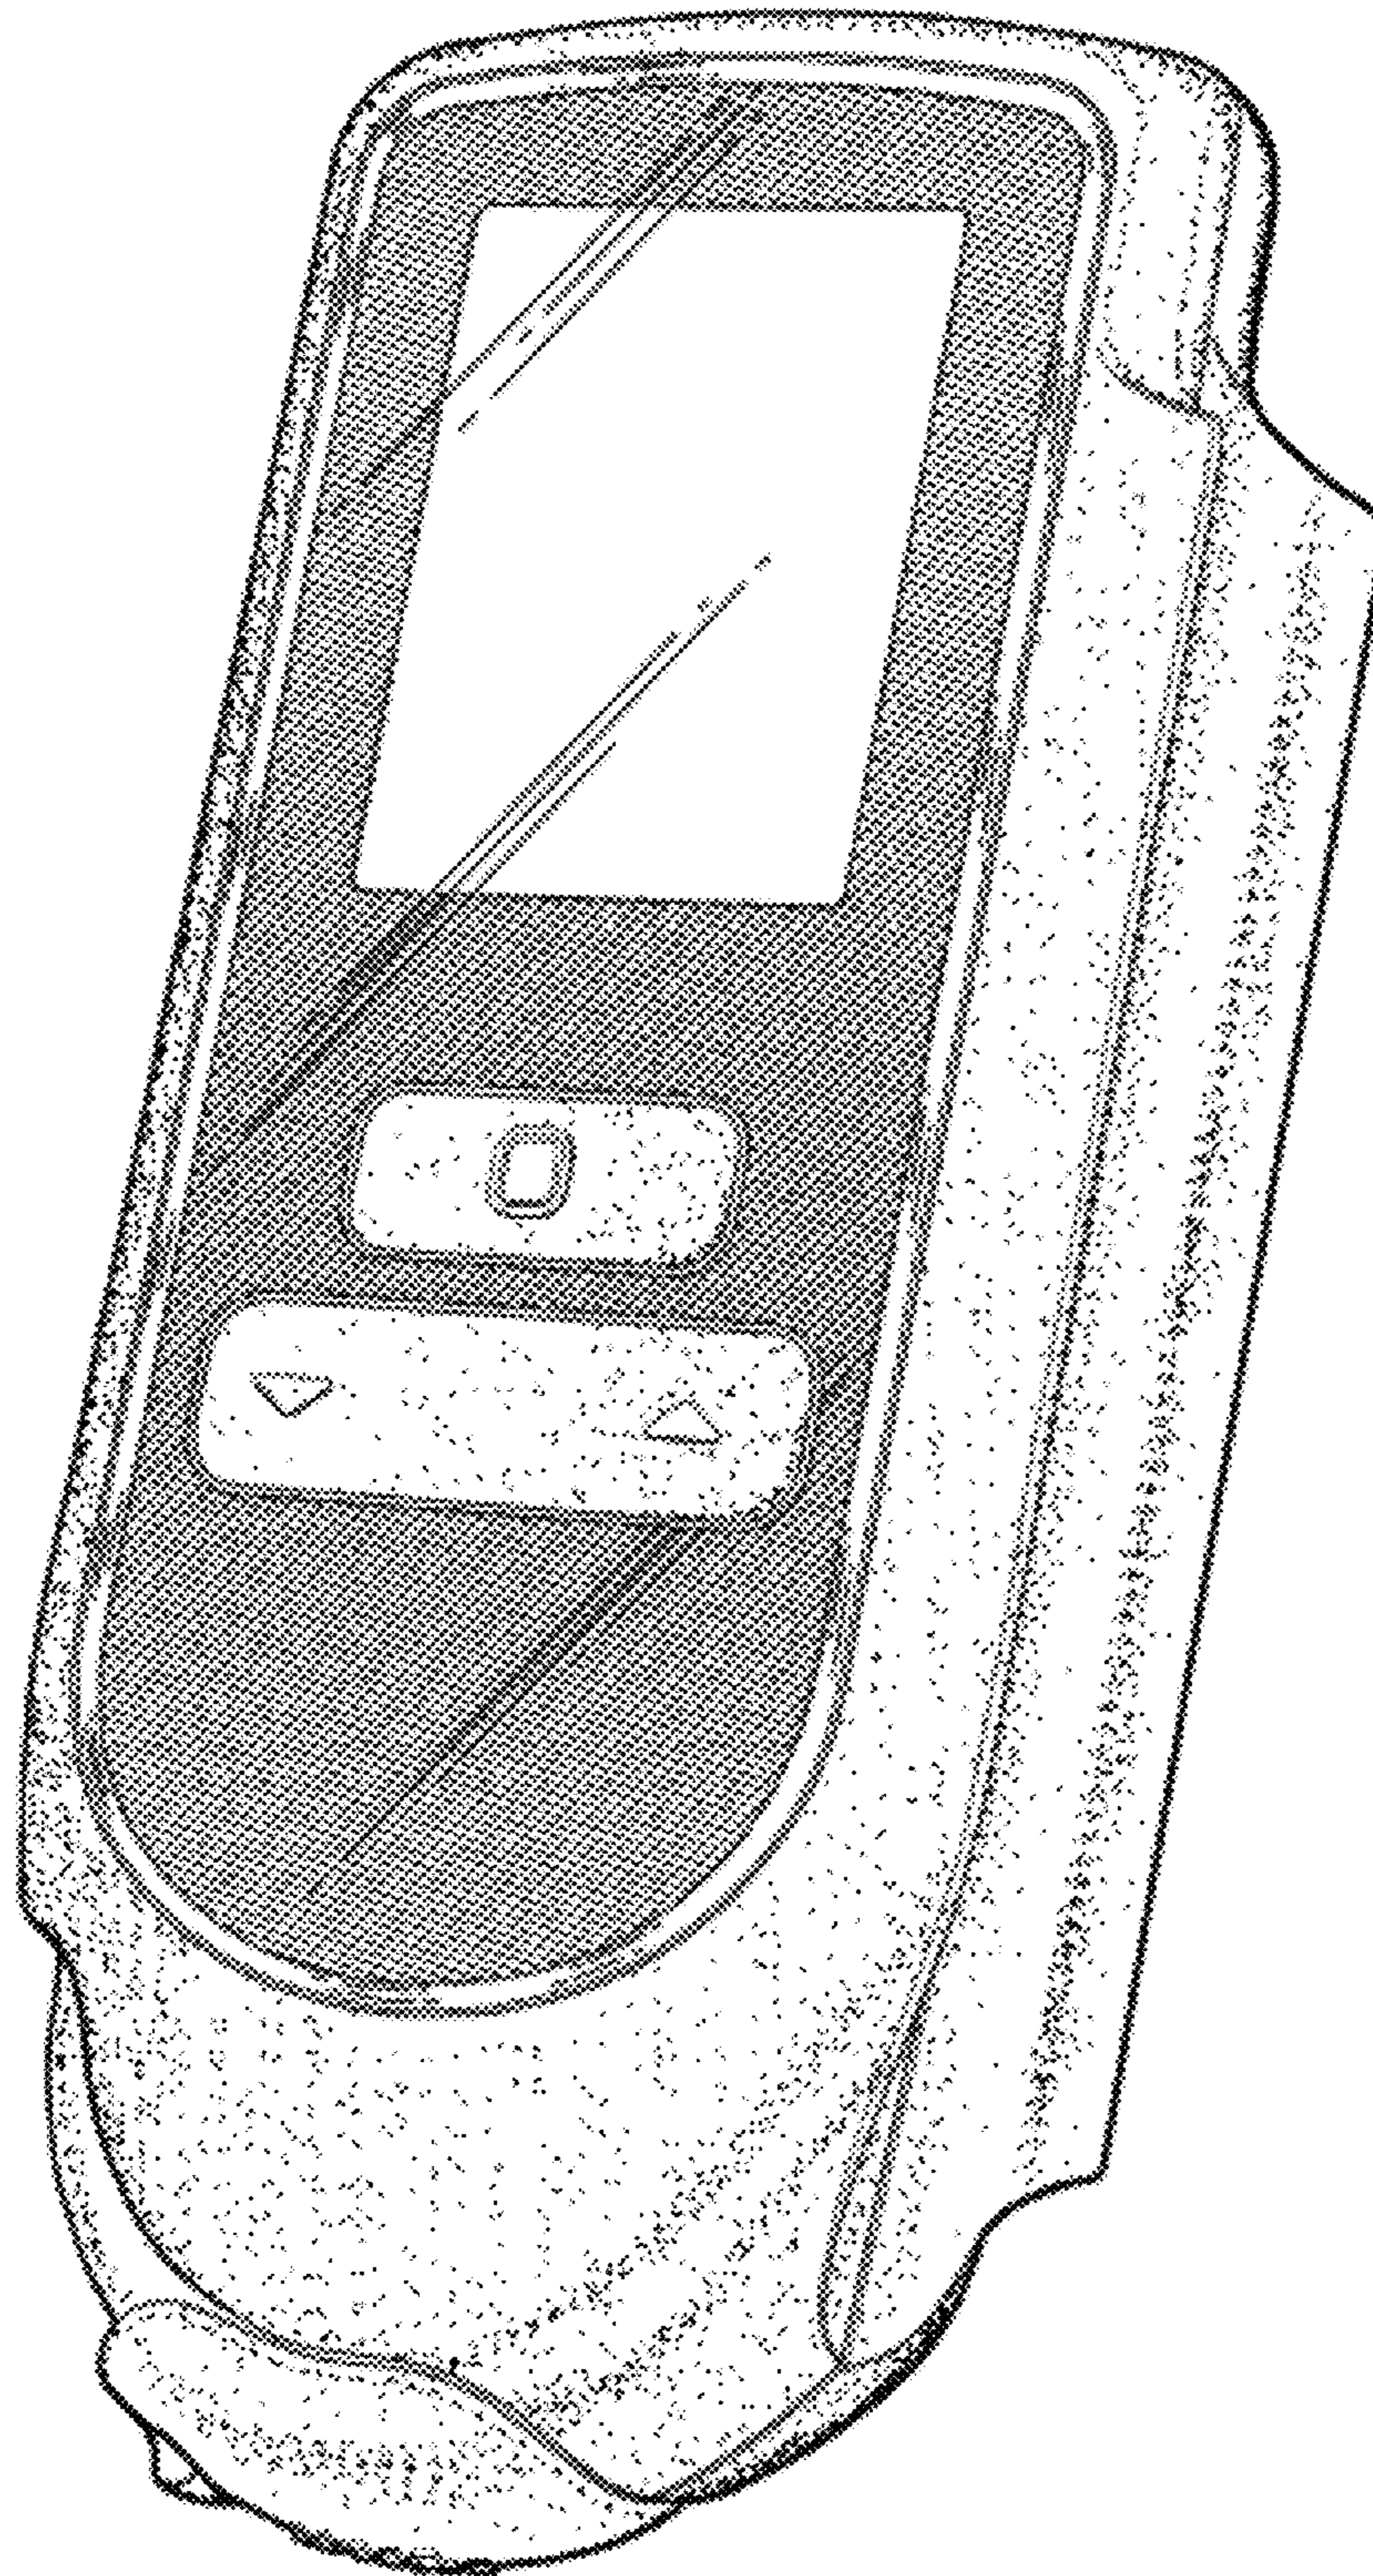


**Fig. 10**

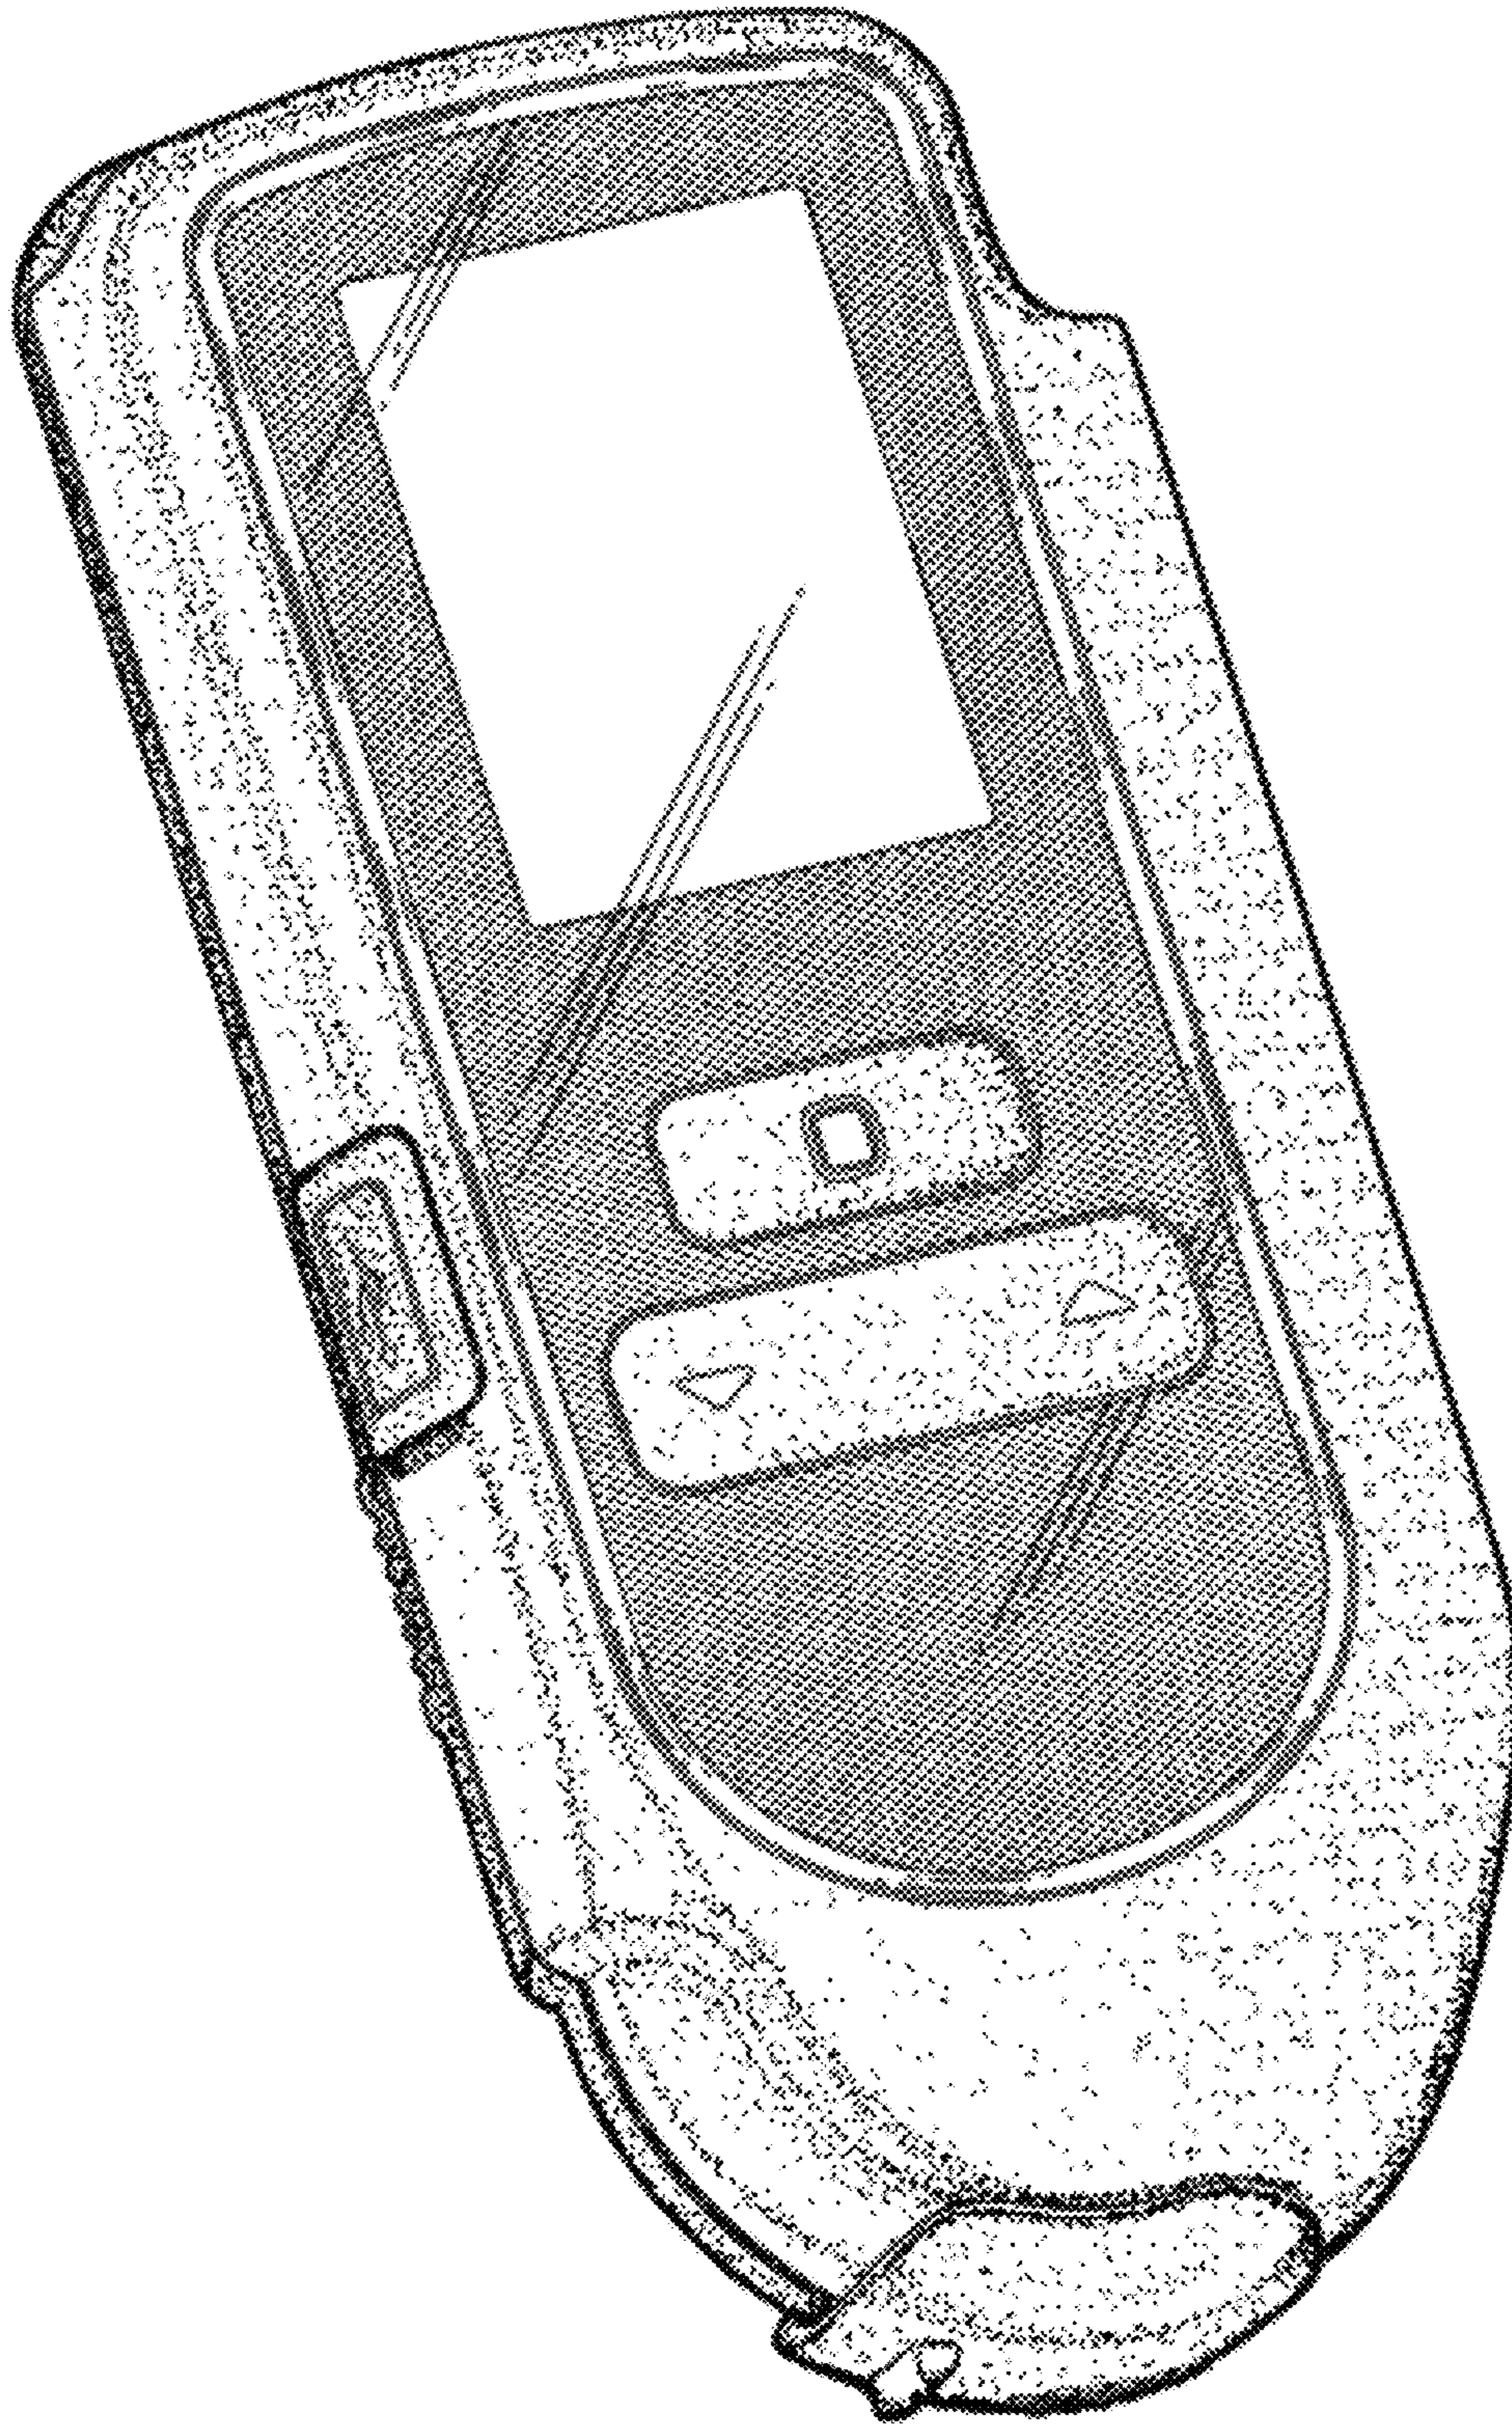

**Fig. 11**

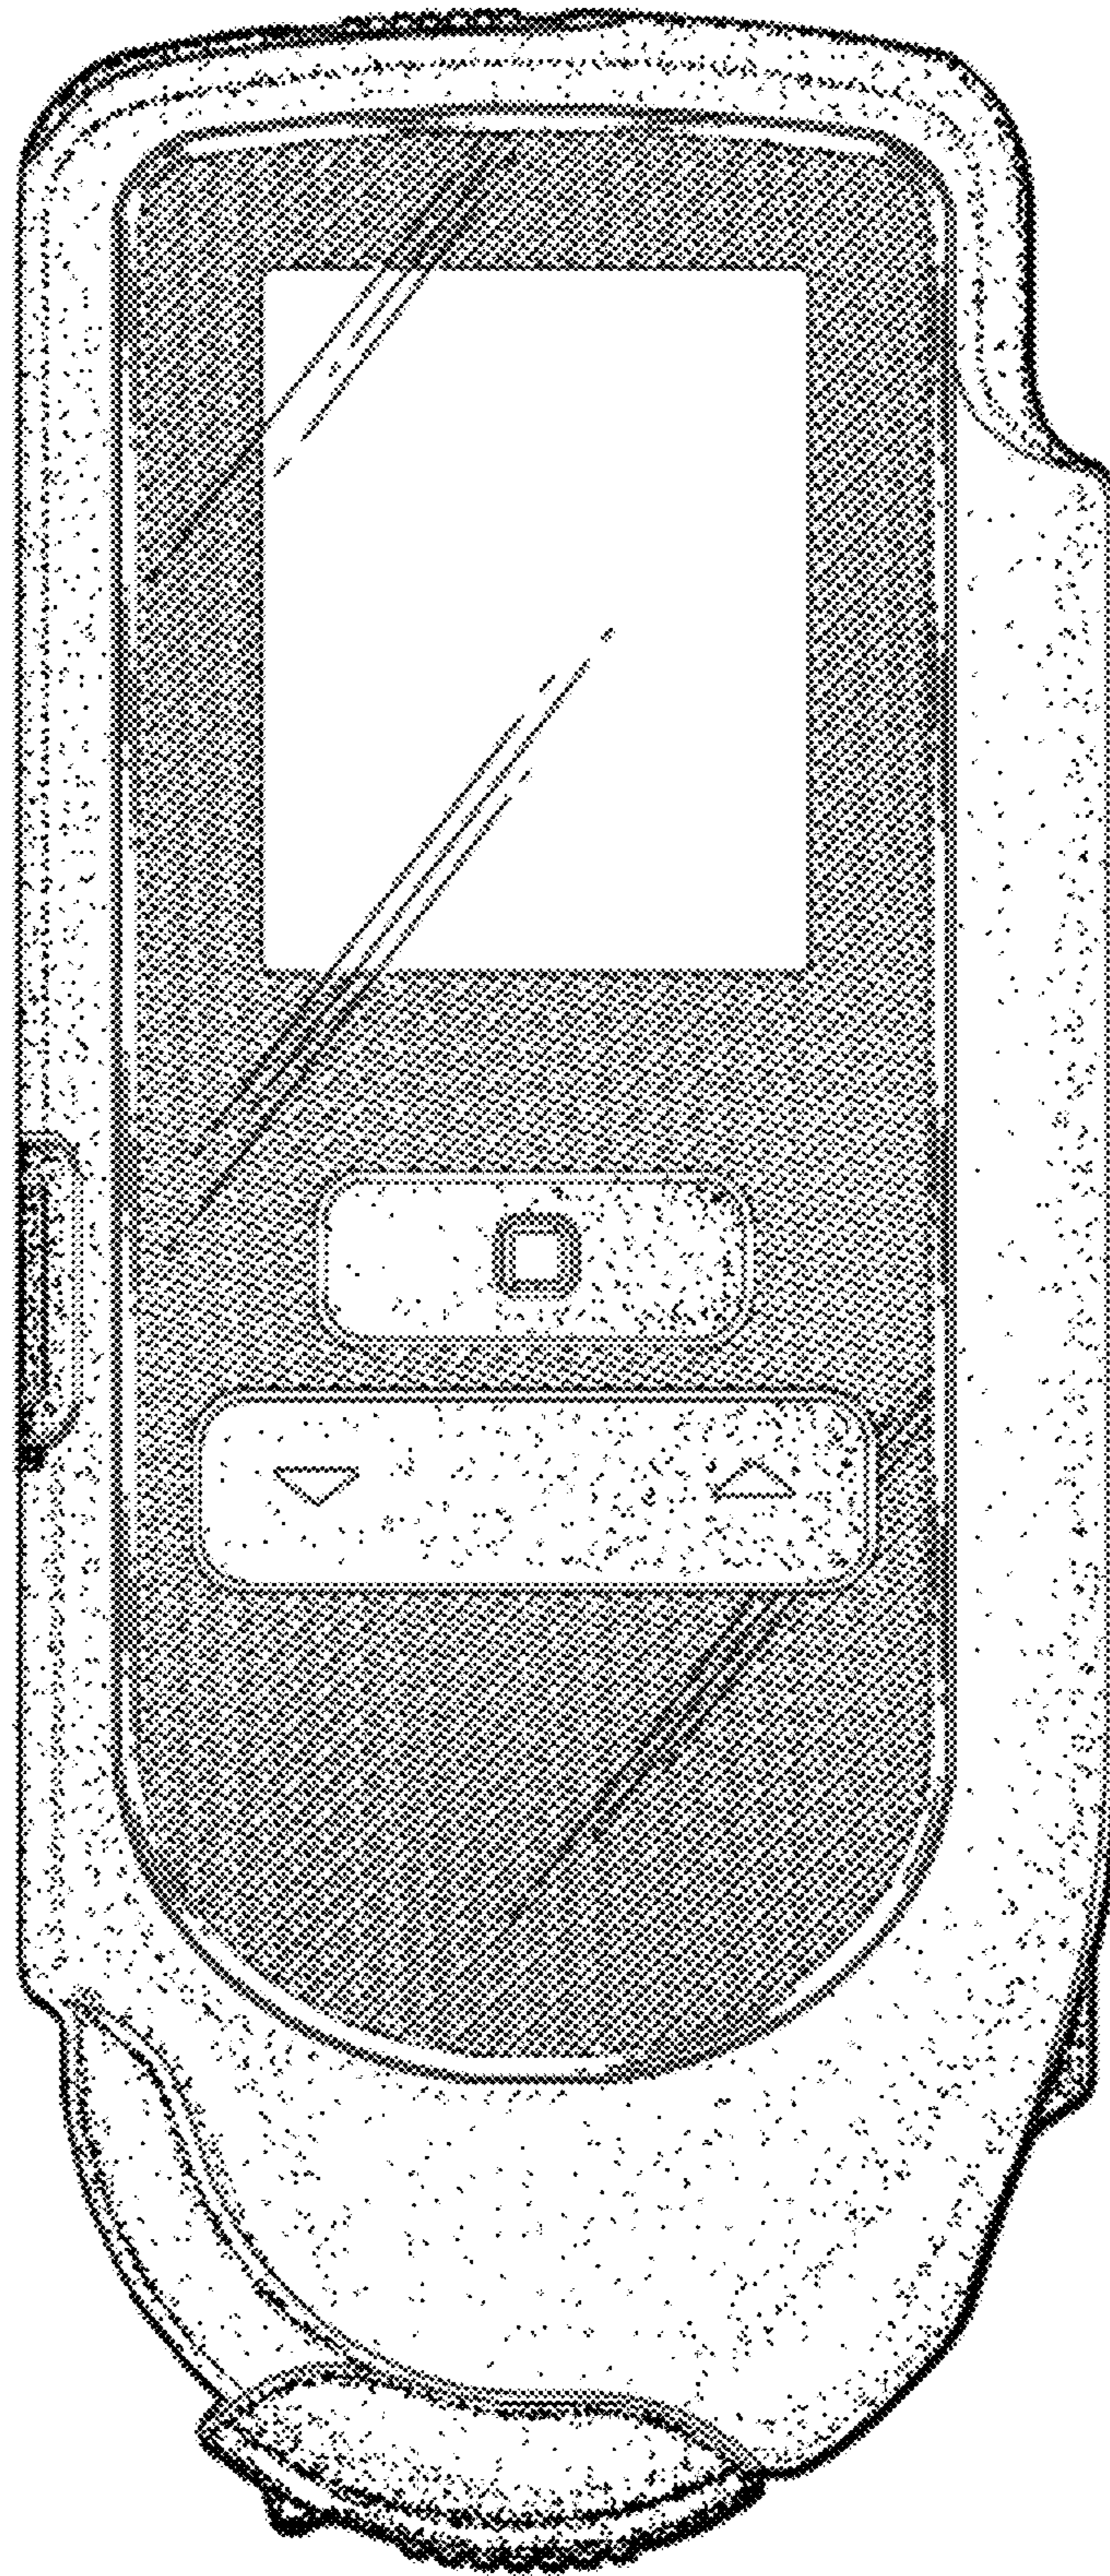


**Fig. 12**

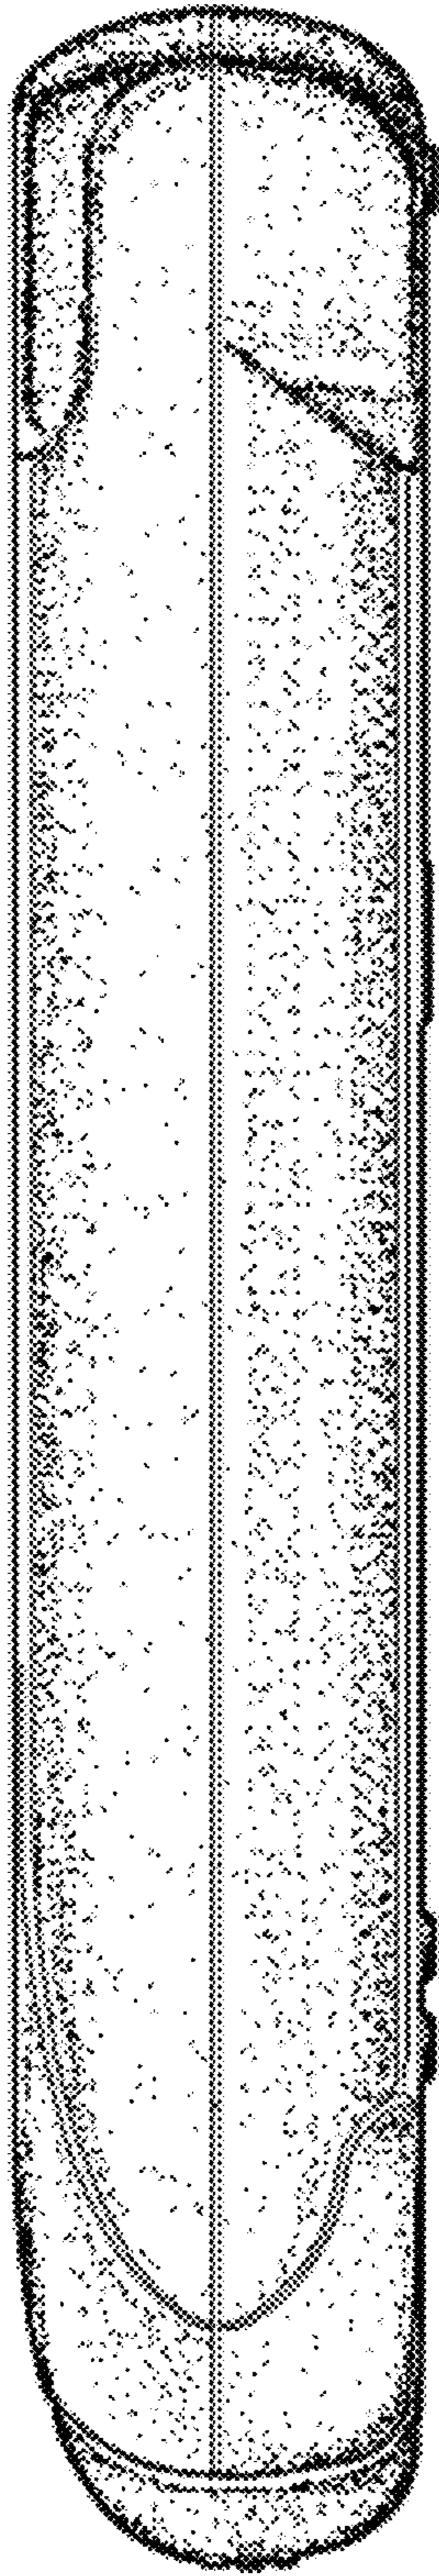


**Fig. 13**




**Fig. 14**

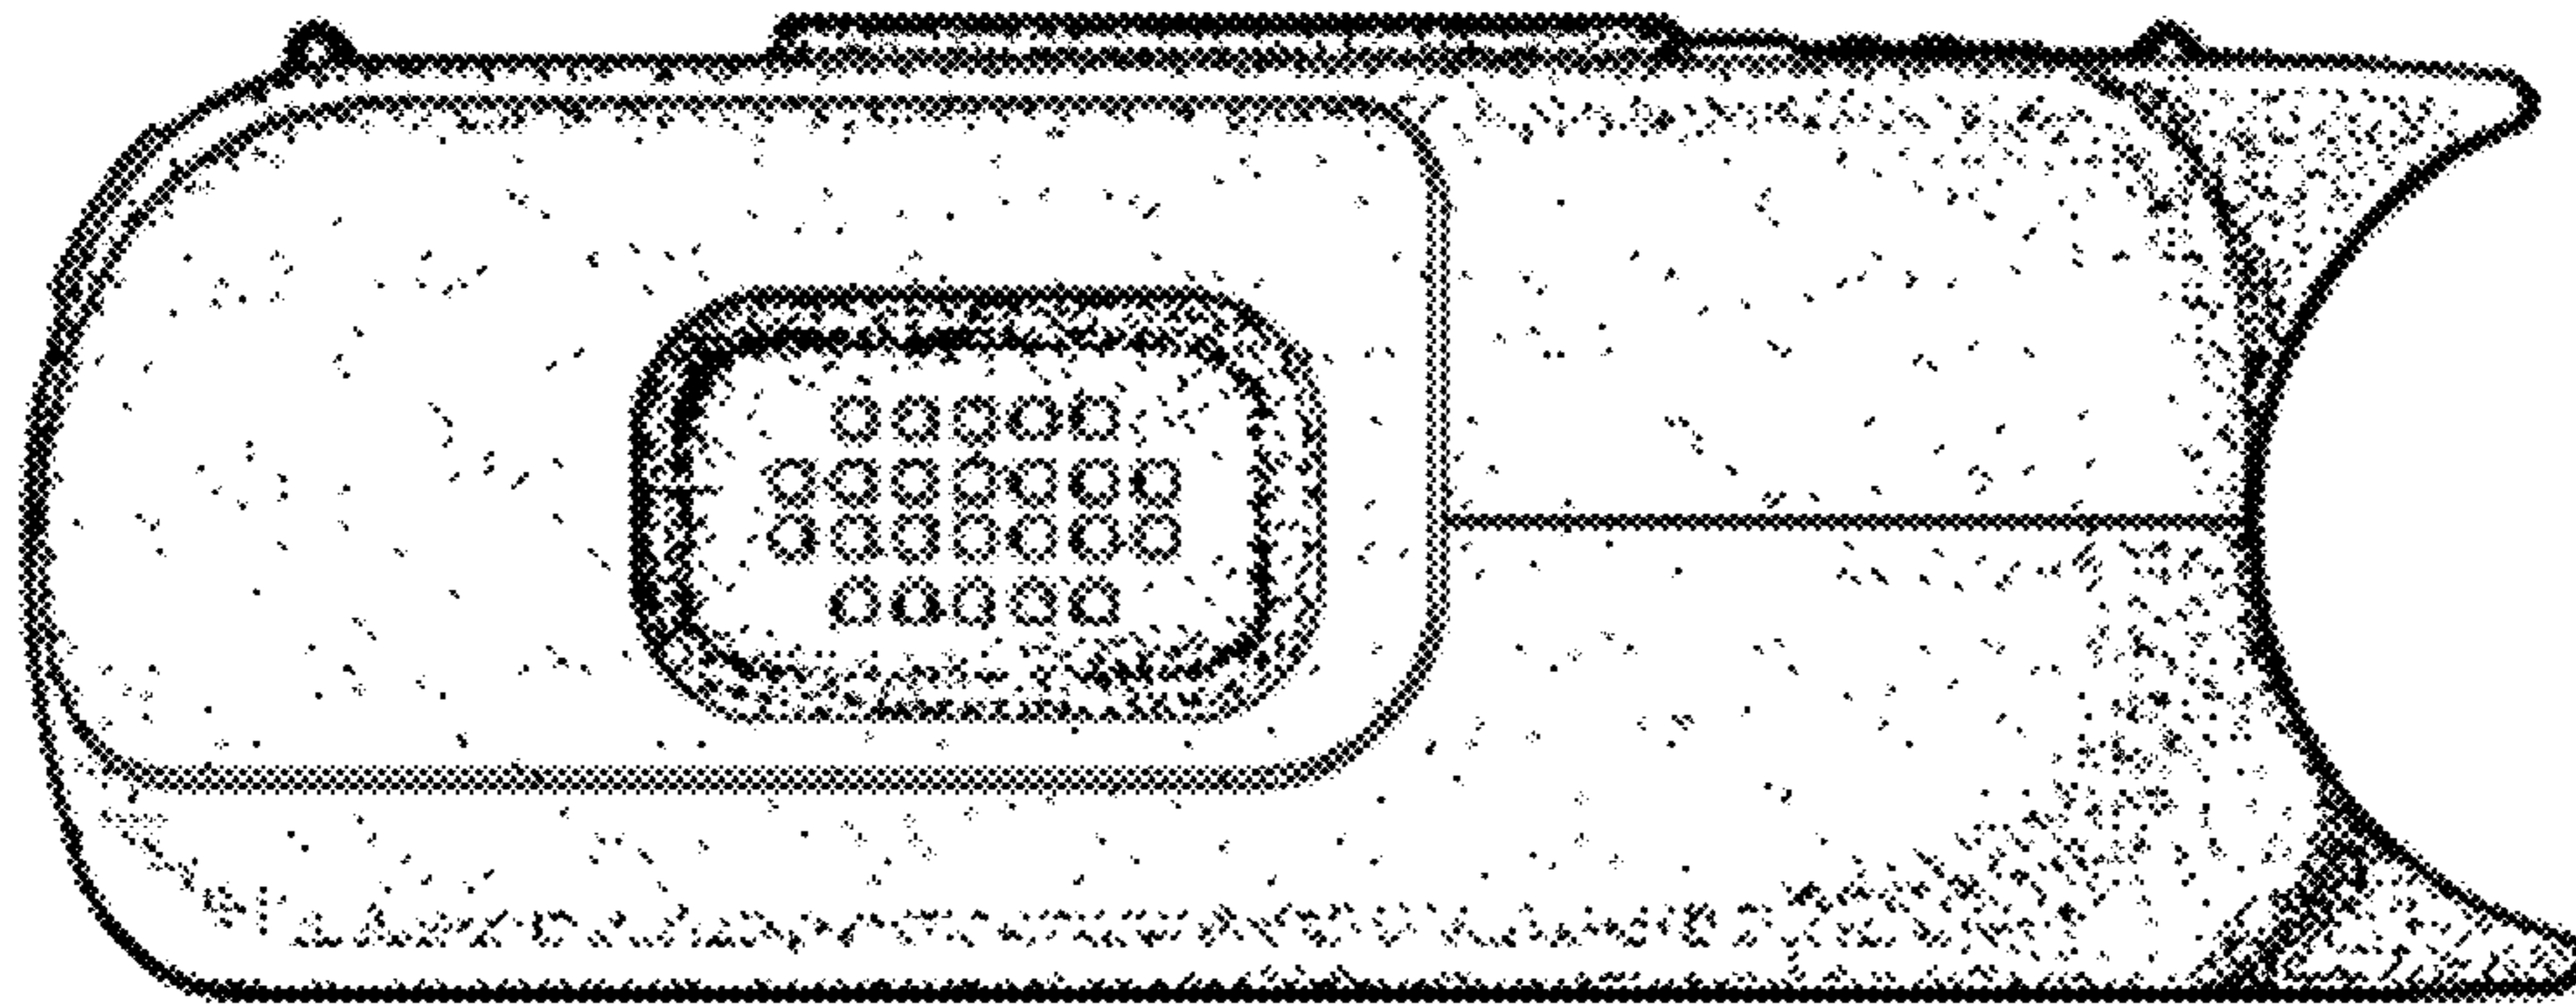


**Fig. 16**

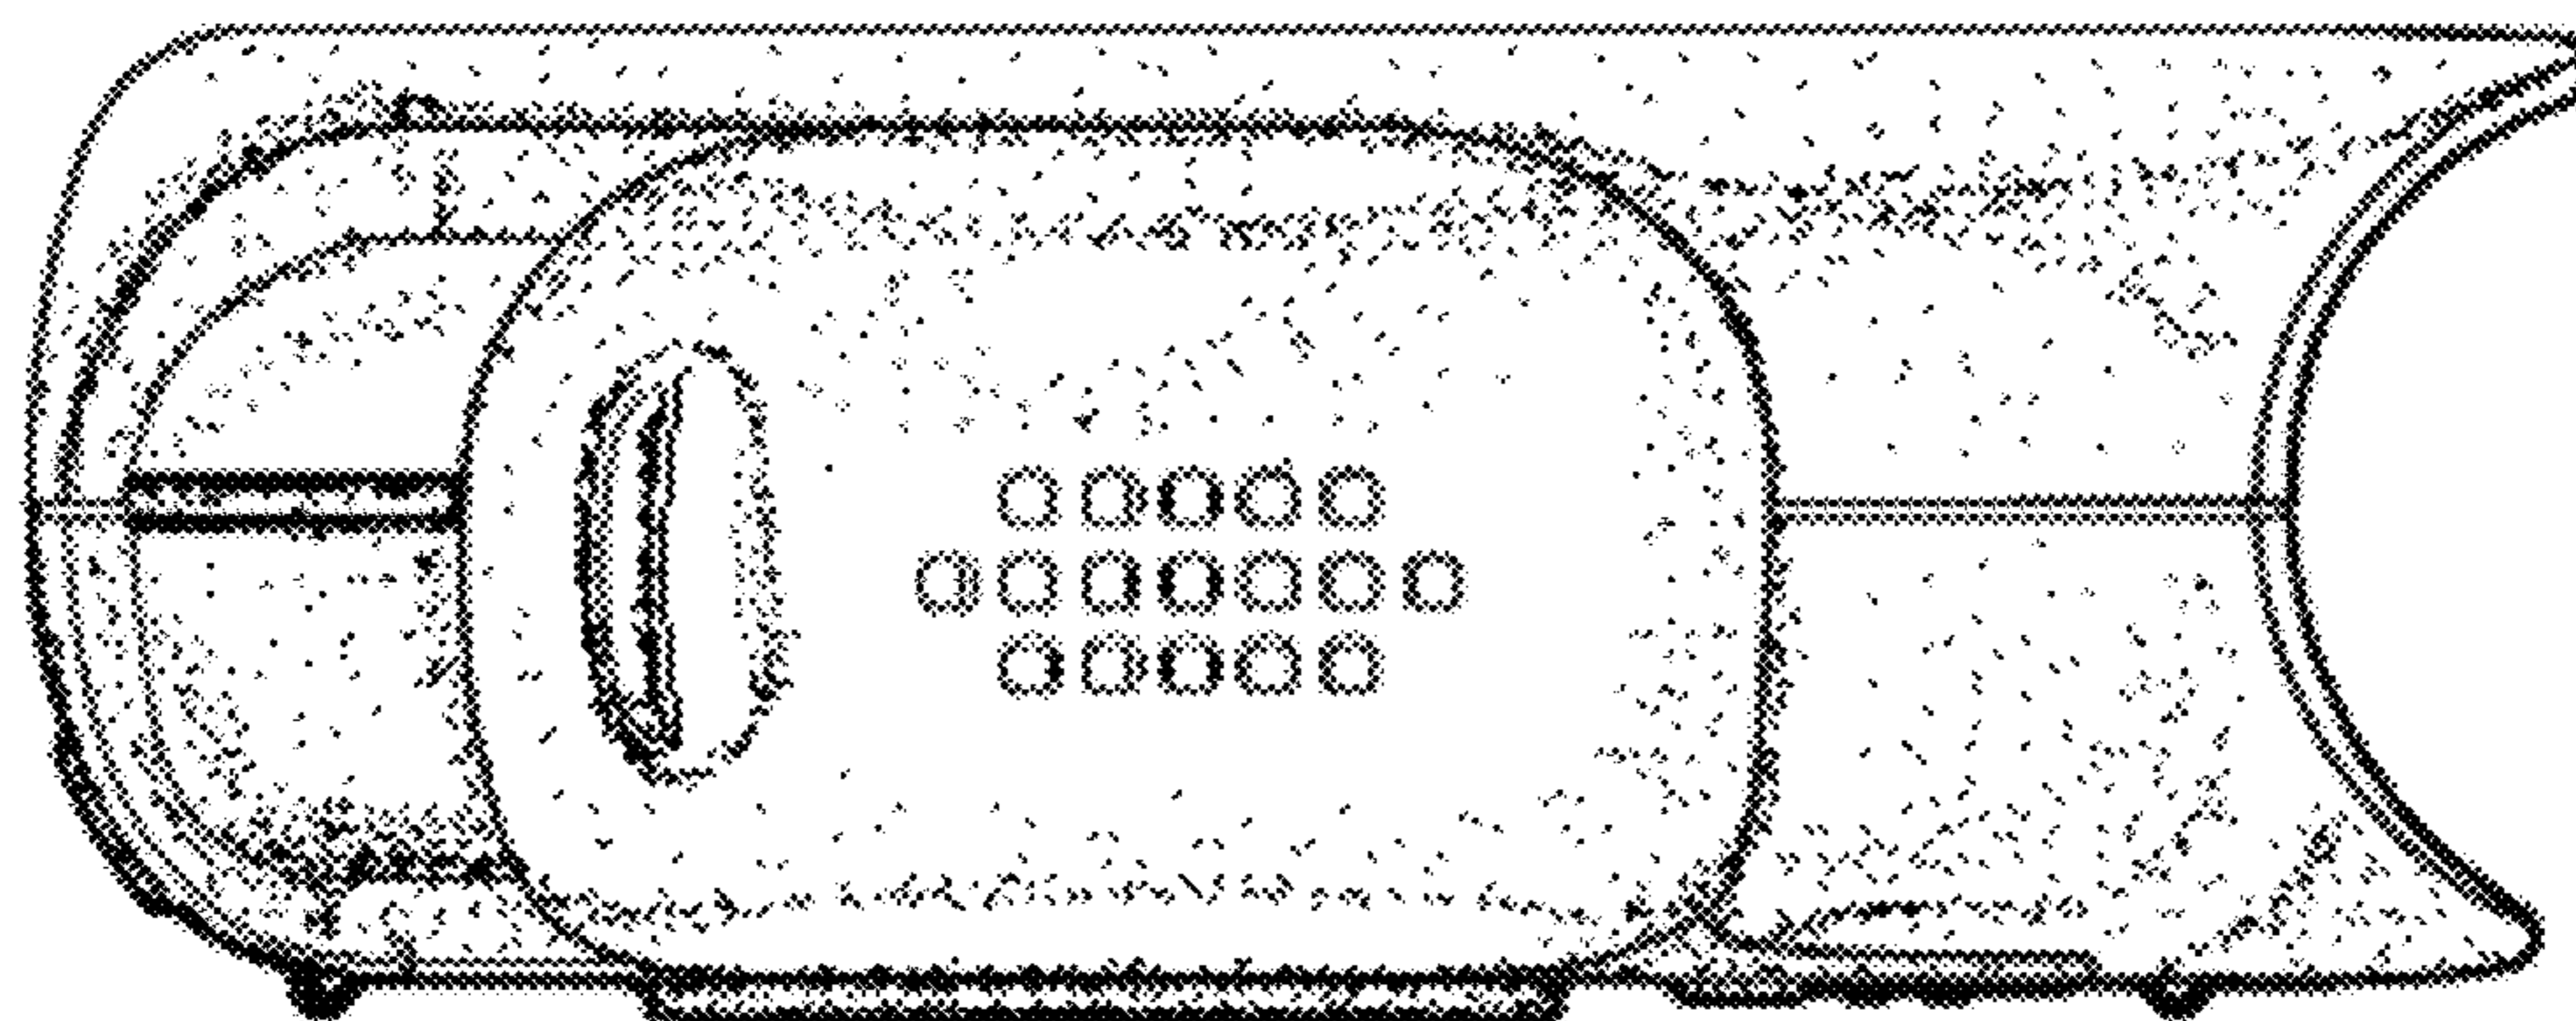

**Fig. 15**

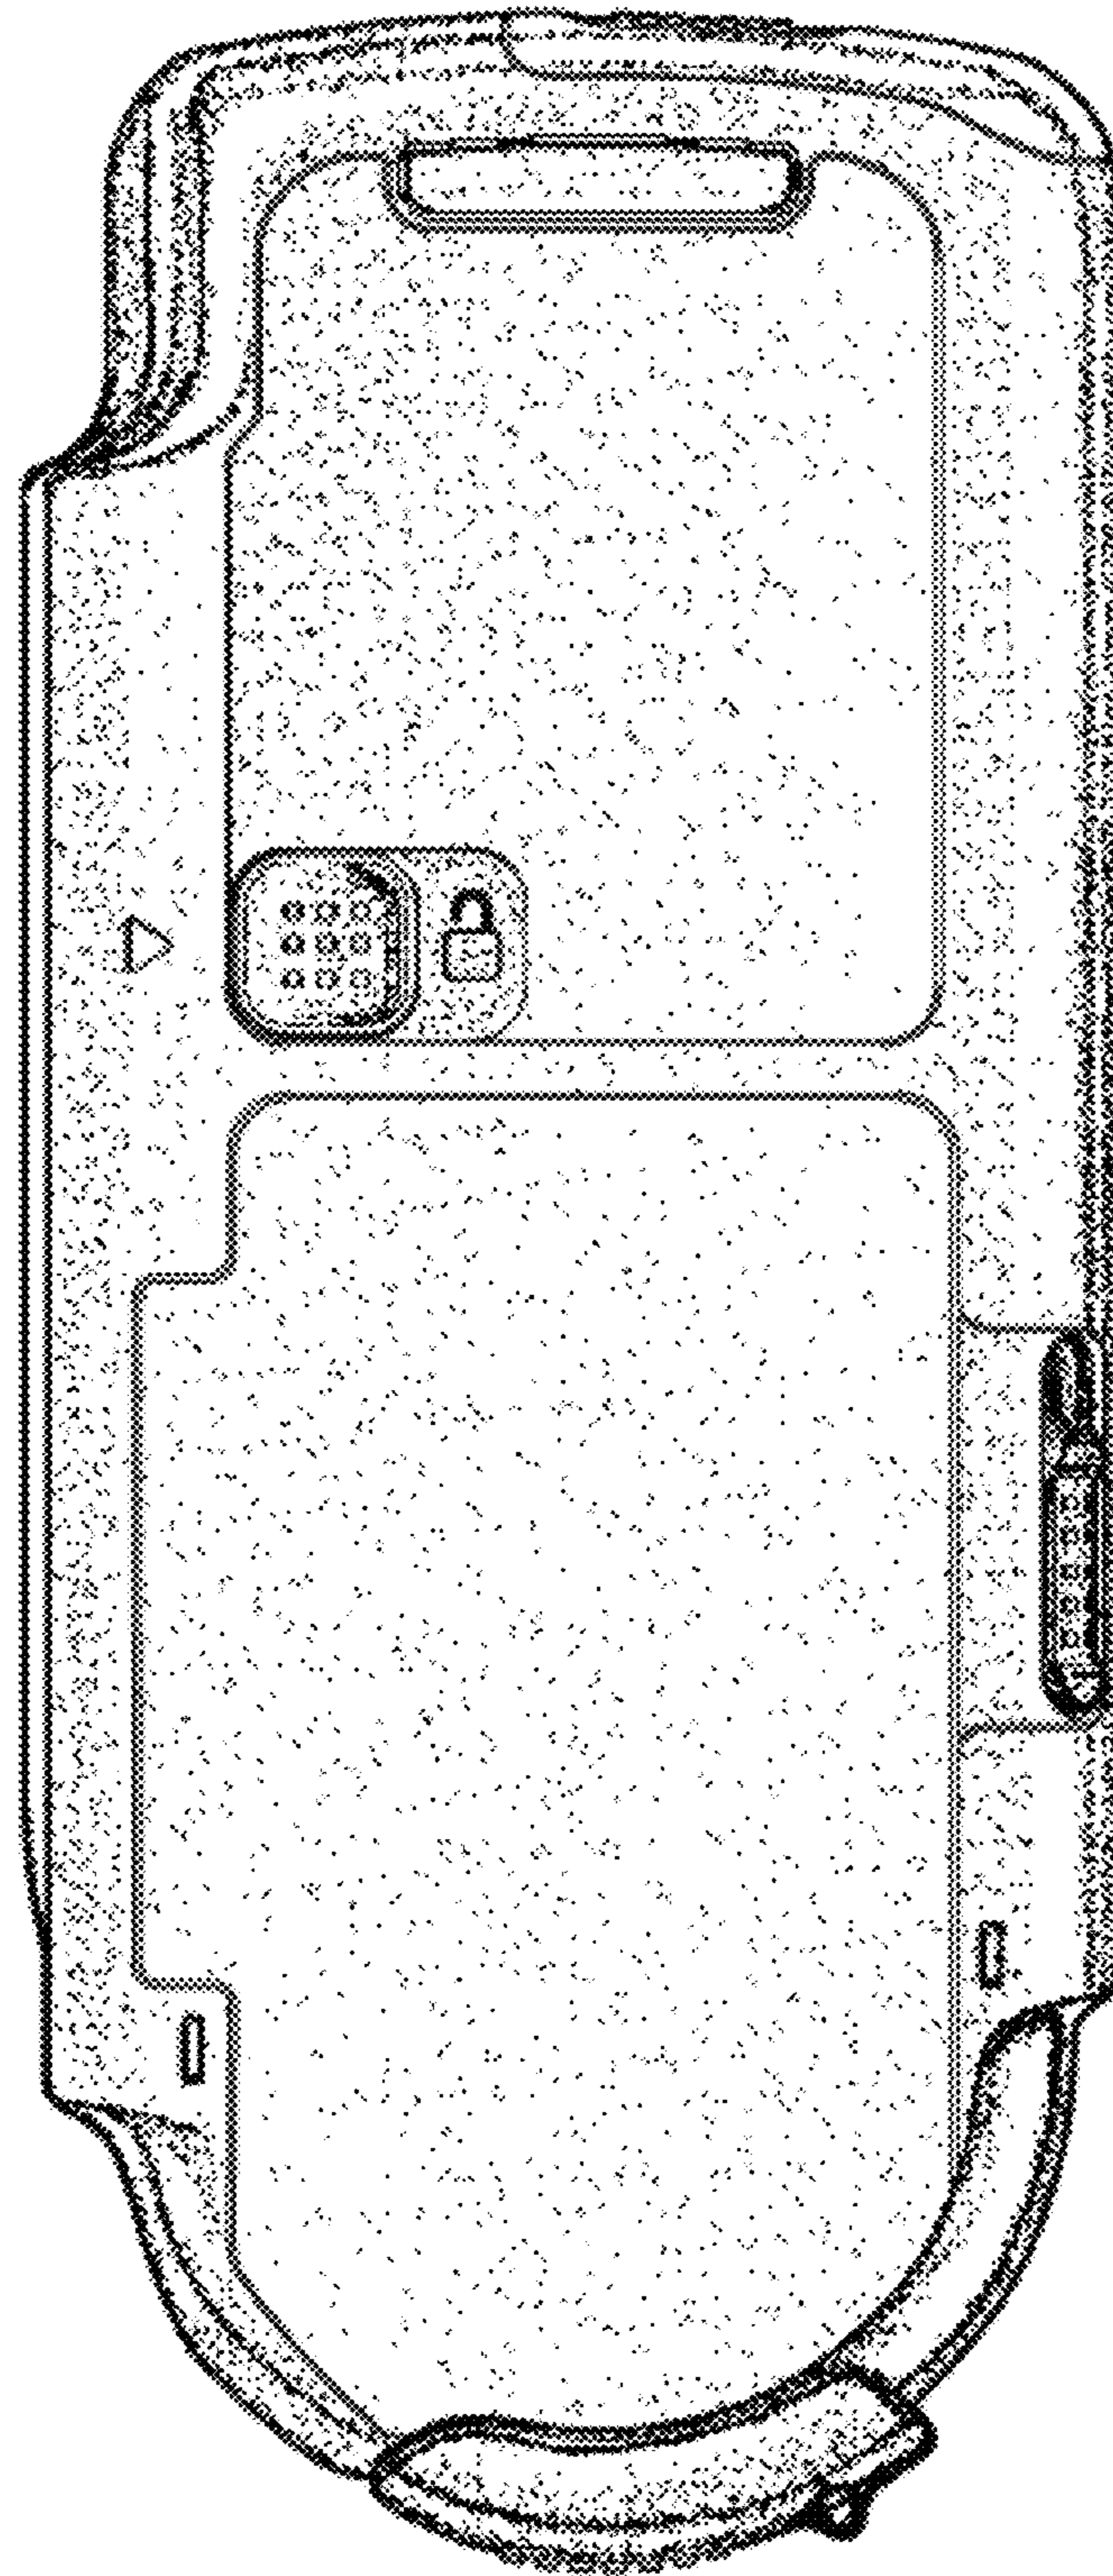

**Fig. 17**

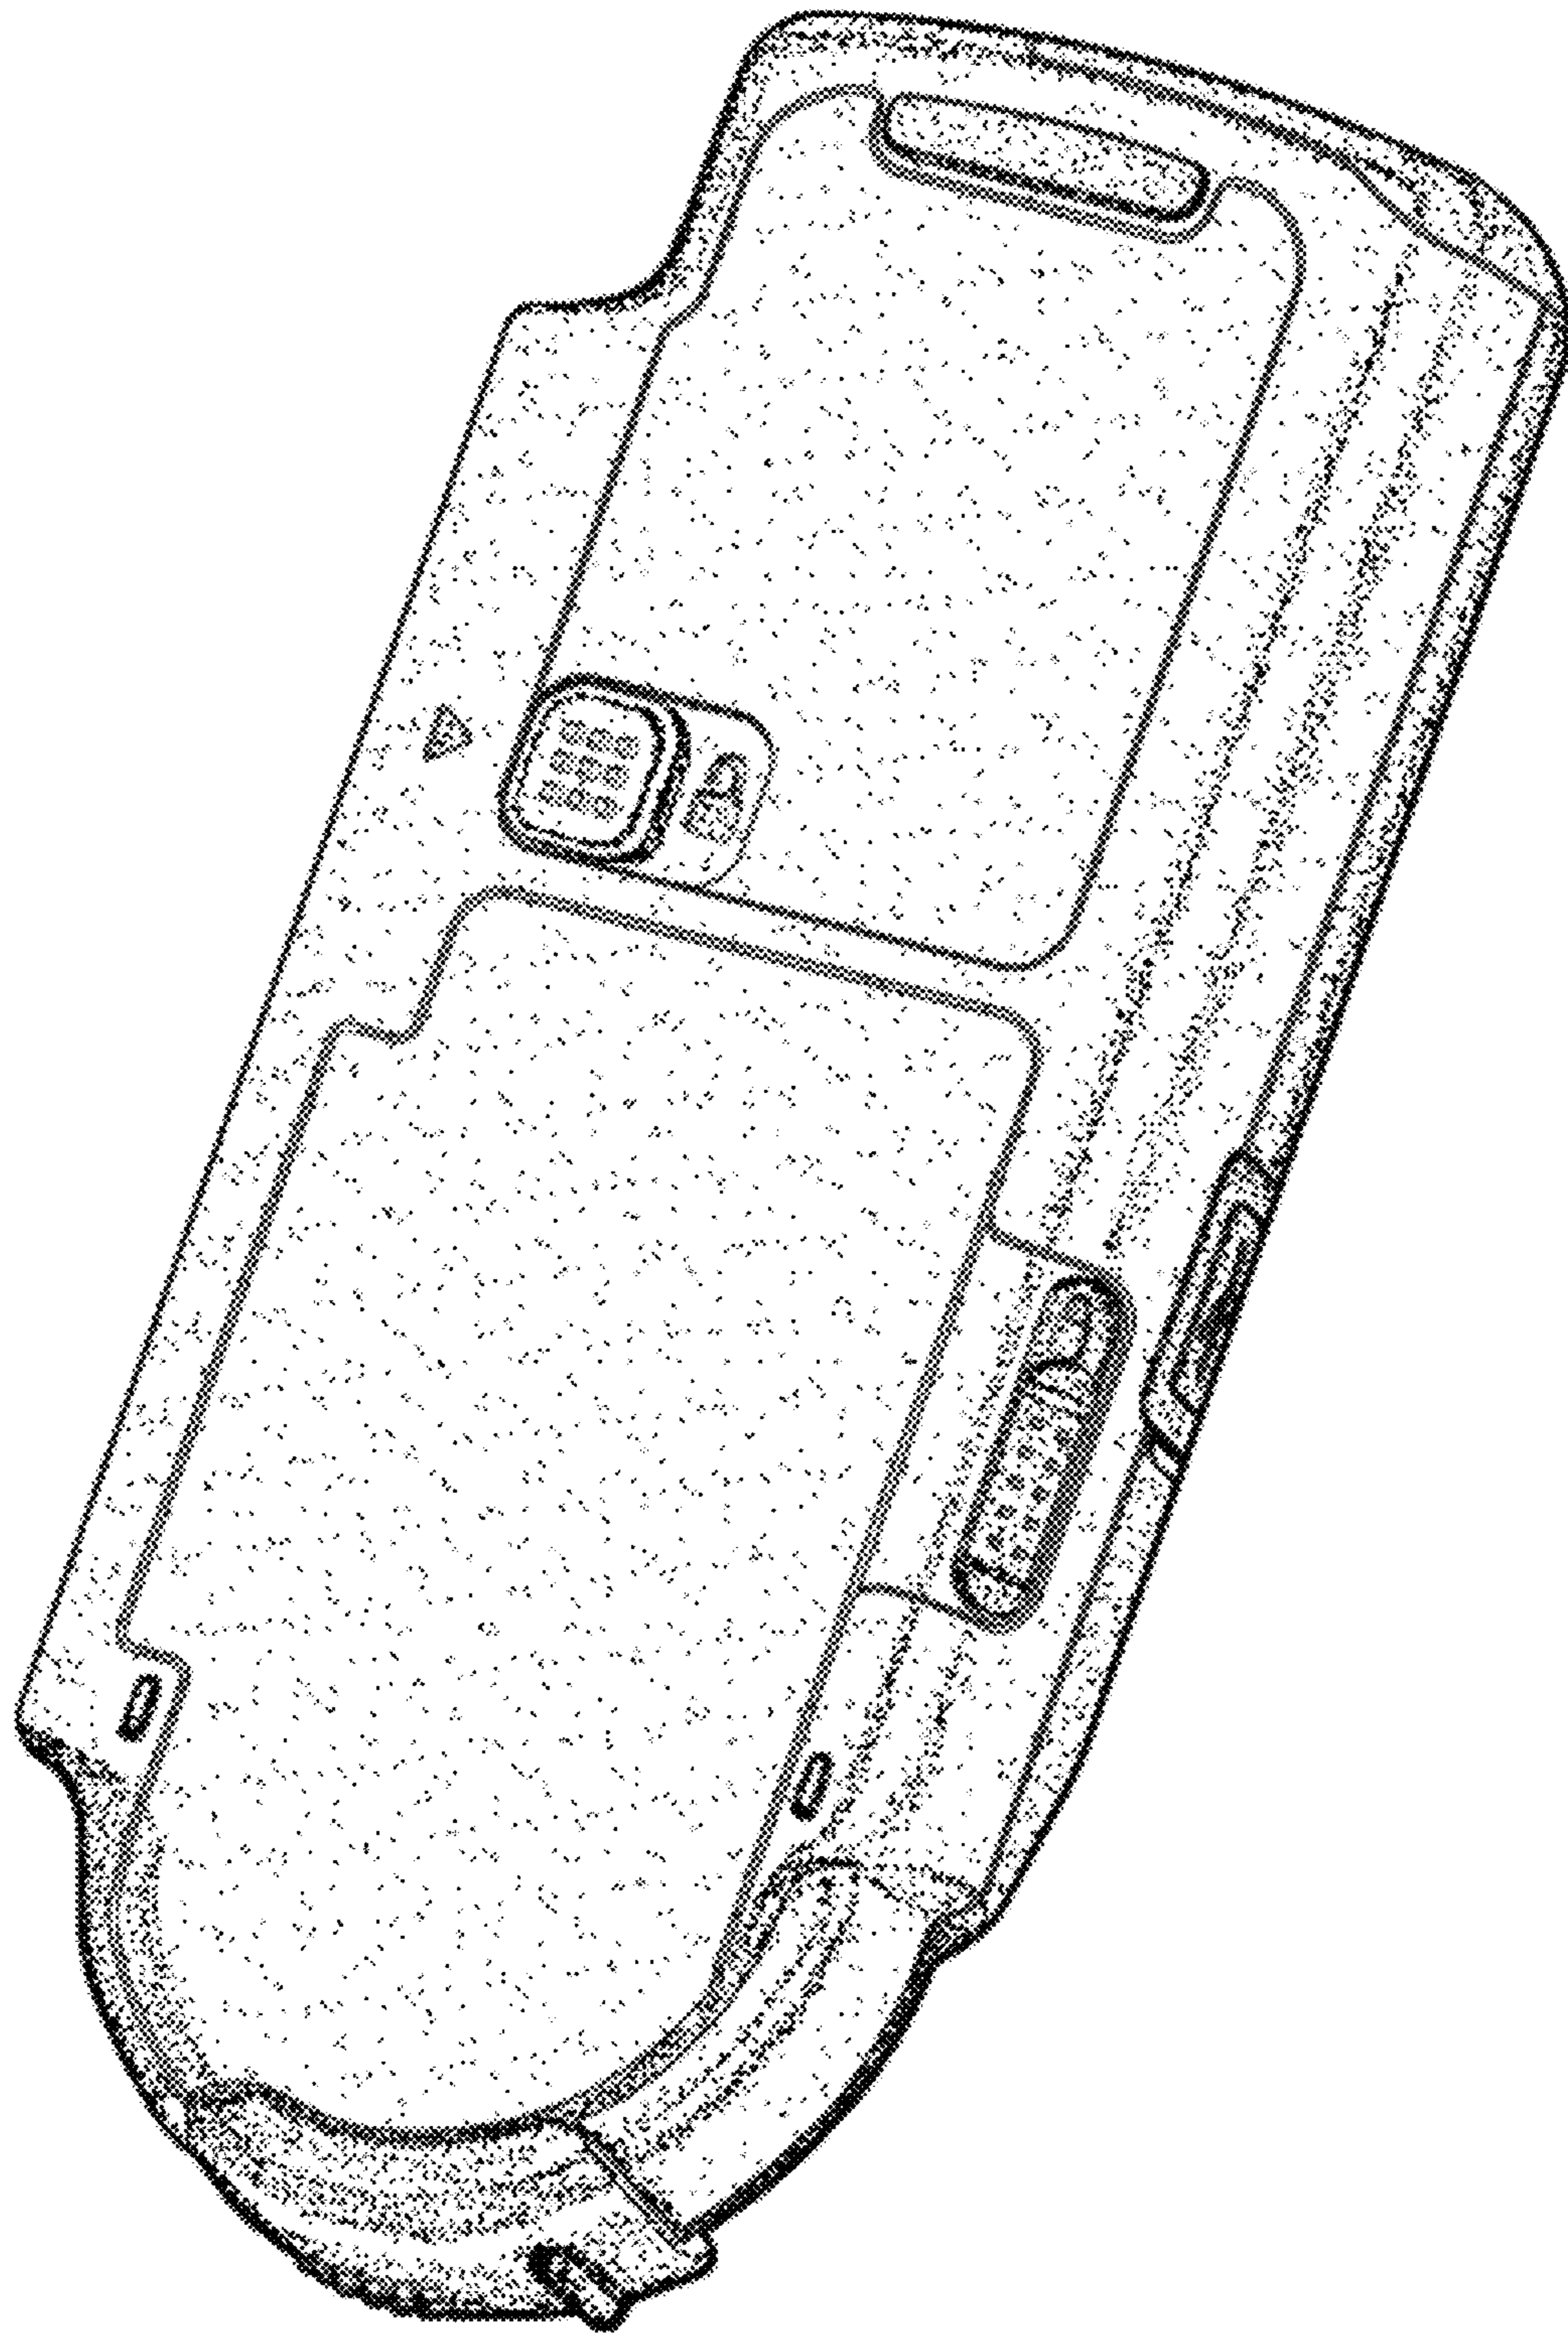

**Fig. 18**