



US00D665085S

(12) **United States Design Patent**
Strother et al.

(10) **Patent No.:** **US D665,085 S**

(45) **Date of Patent:** **** Aug. 7, 2012**

(54) **ELECTRICAL STIMULATOR AND MOUNTING PATCH ASSEMBLY**

(75) Inventors: **Robert B. Strother**, Willoughby Hills, OH (US); **Jonathan L. Sakai**, Fairview Park, OH (US); **Joseph W. Boggs, II**, Carrboro, NC (US); **Kathryn W. Stager**, University Heights, OH (US); **Maria E. Bennett**, Beachwood, OH (US)

(73) Assignee: **NDI Medical, LLC**, Cleveland, OH (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/388,996**

(22) Filed: **Apr. 5, 2011**

(51) **LOC (9) Cl.** **24-01**

(52) **U.S. Cl.** **D24/187**

(58) **Field of Classification Search** D24/168,
D24/186-187, 200, 232; D13/182; 600/372-384,
600/391-397, 386; 607/62, 109, 121, 139,
607/149, 152, 153

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,539,996	A *	9/1985	Engel	600/392
D385,037	S *	10/1997	Jensen	D24/187
D409,307	S *	5/1999	Phleps et al.	D24/158
6,527,442	B2 *	3/2003	Carroll	378/189
D478,666	S *	8/2003	Cianciosi	D24/158
D504,722	S *	5/2005	Cianciosi	D24/158
D536,673	S *	2/2007	Silber	D24/187
D565,184	S *	3/2008	Royzen	D24/168
D567,949	S *	4/2008	Lash et al.	D24/168
D568,479	S *	5/2008	Mao et al.	D24/168
D584,414	S *	1/2009	Lash et al.	D24/187
D587,375	S *	2/2009	Mao et al.	D24/168
D624,189	S *	9/2010	Rutt et al.	D24/187
D629,524	S *	12/2010	Zeller et al.	D24/187
2010/0036445	A1	2/2010	Sakai et al.	

FOREIGN PATENT DOCUMENTS

EP 00242606-001 10/2010

* cited by examiner

Primary Examiner — T. Chase Nelson

Assistant Examiner — Mark Cavanna

(74) *Attorney, Agent, or Firm* — Ryan Kromholz & Manion, S.C.

(57) **CLAIM**

The ornamental design electrical stimulator and mounting patch assembly, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of the electrical stimulator portion shown separately for clarity of illustration of an electrical stimulator and mounting patch assembly showing my new design.

FIG. 2 is a front elevation view thereof.

FIG. 3 is a rear elevation view thereof.

FIG. 4 is a bottom plan view thereof.

FIG. 5 is a top plan view thereof.

FIG. 6 is a right side elevation view thereof.

FIG. 7 is a left side elevation view thereof.

FIG. 8 is a perspective view of the mounting patch portion of the electrical stimulator and mounting patch assembly shown separately for clarity of illustration.

FIG. 9 is a front elevation view thereof.

FIG. 10 is a rear elevation view thereof.

FIG. 11 is a bottom plan thereof.

FIG. 12 is a top plan view thereof.

FIG. 13 is a right side elevation view thereof.

FIG. 14 is a left side elevation view thereof.

FIG. 15 is a perspective view of an electrical stimulator and mounting patch assembly shown assembled.

FIG. 16 is a front elevation view thereof.

FIG. 17 is a rear elevation view thereof.

FIG. 18 is a bottom plan view thereof.


FIG. 19 is a top plan view thereof.

FIG. 20 is a right side elevation thereof; and,

FIG. 21 is a left side elevation view thereof.

The broken lines are included for the purpose of illustrating portions of the electrical stimulator and mounting patch assembly that form no part of the claimed design.

1 Claim, 6 Drawing Sheets

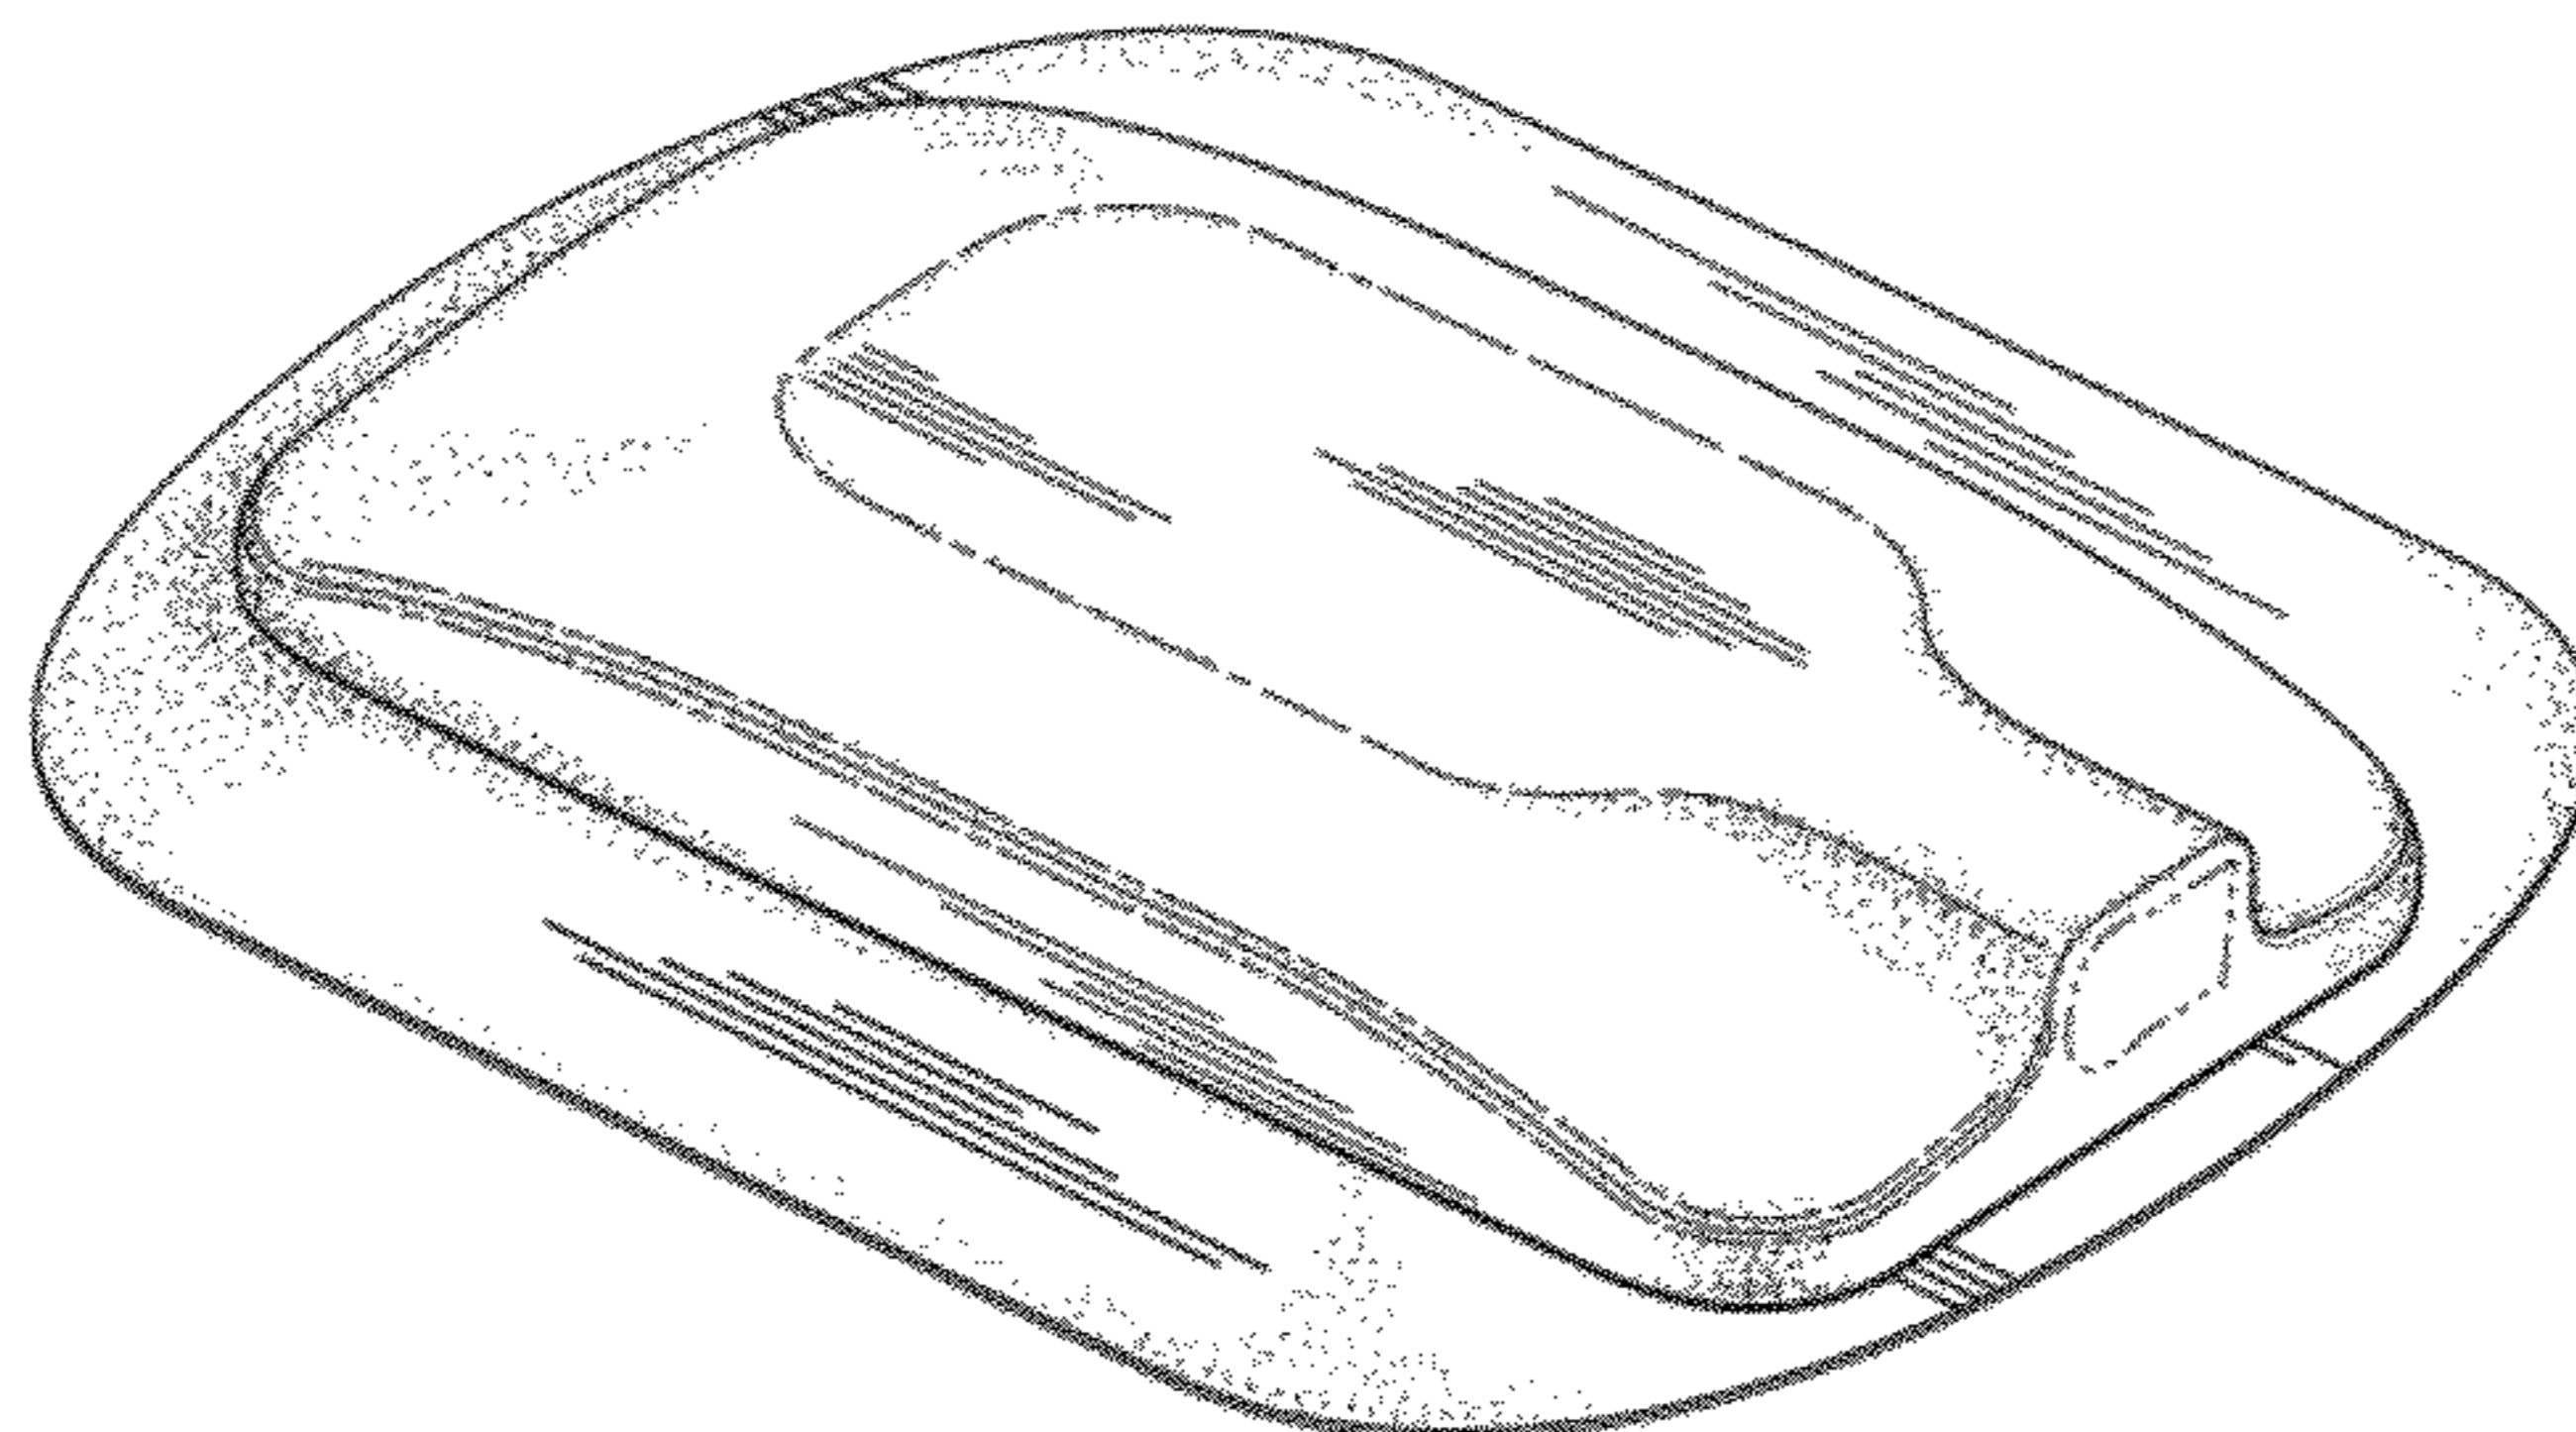

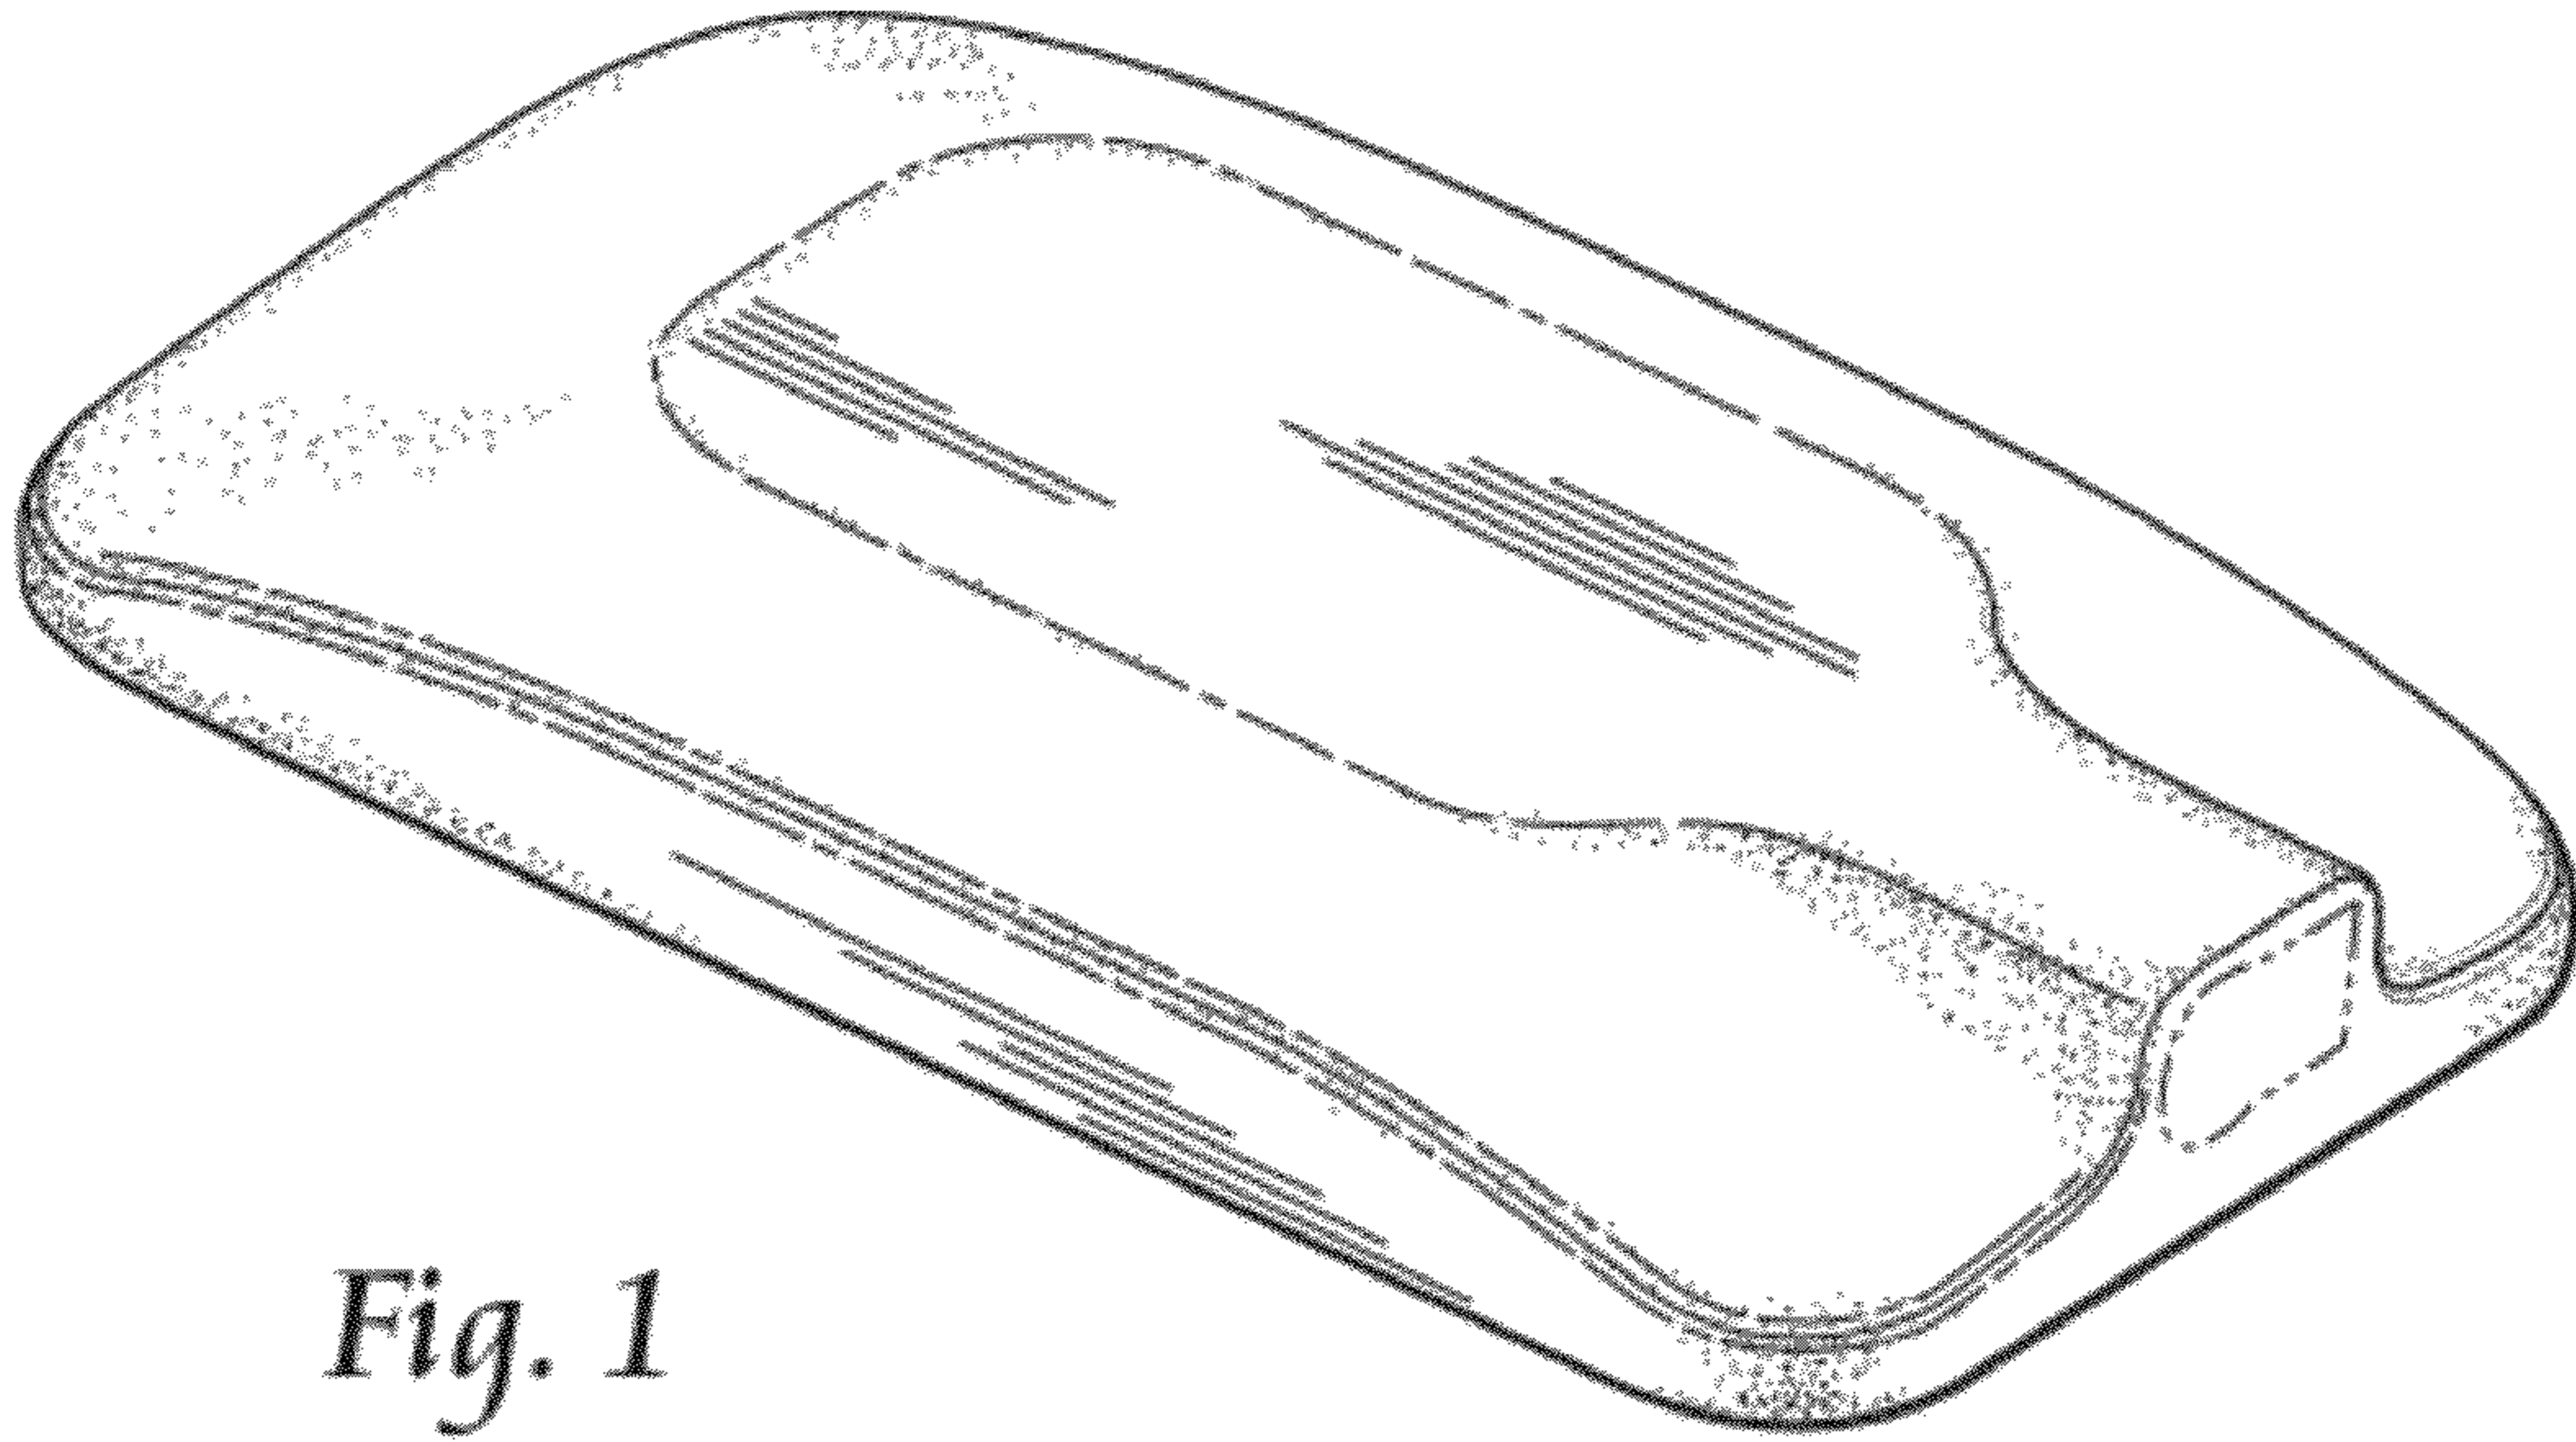


Fig. 1

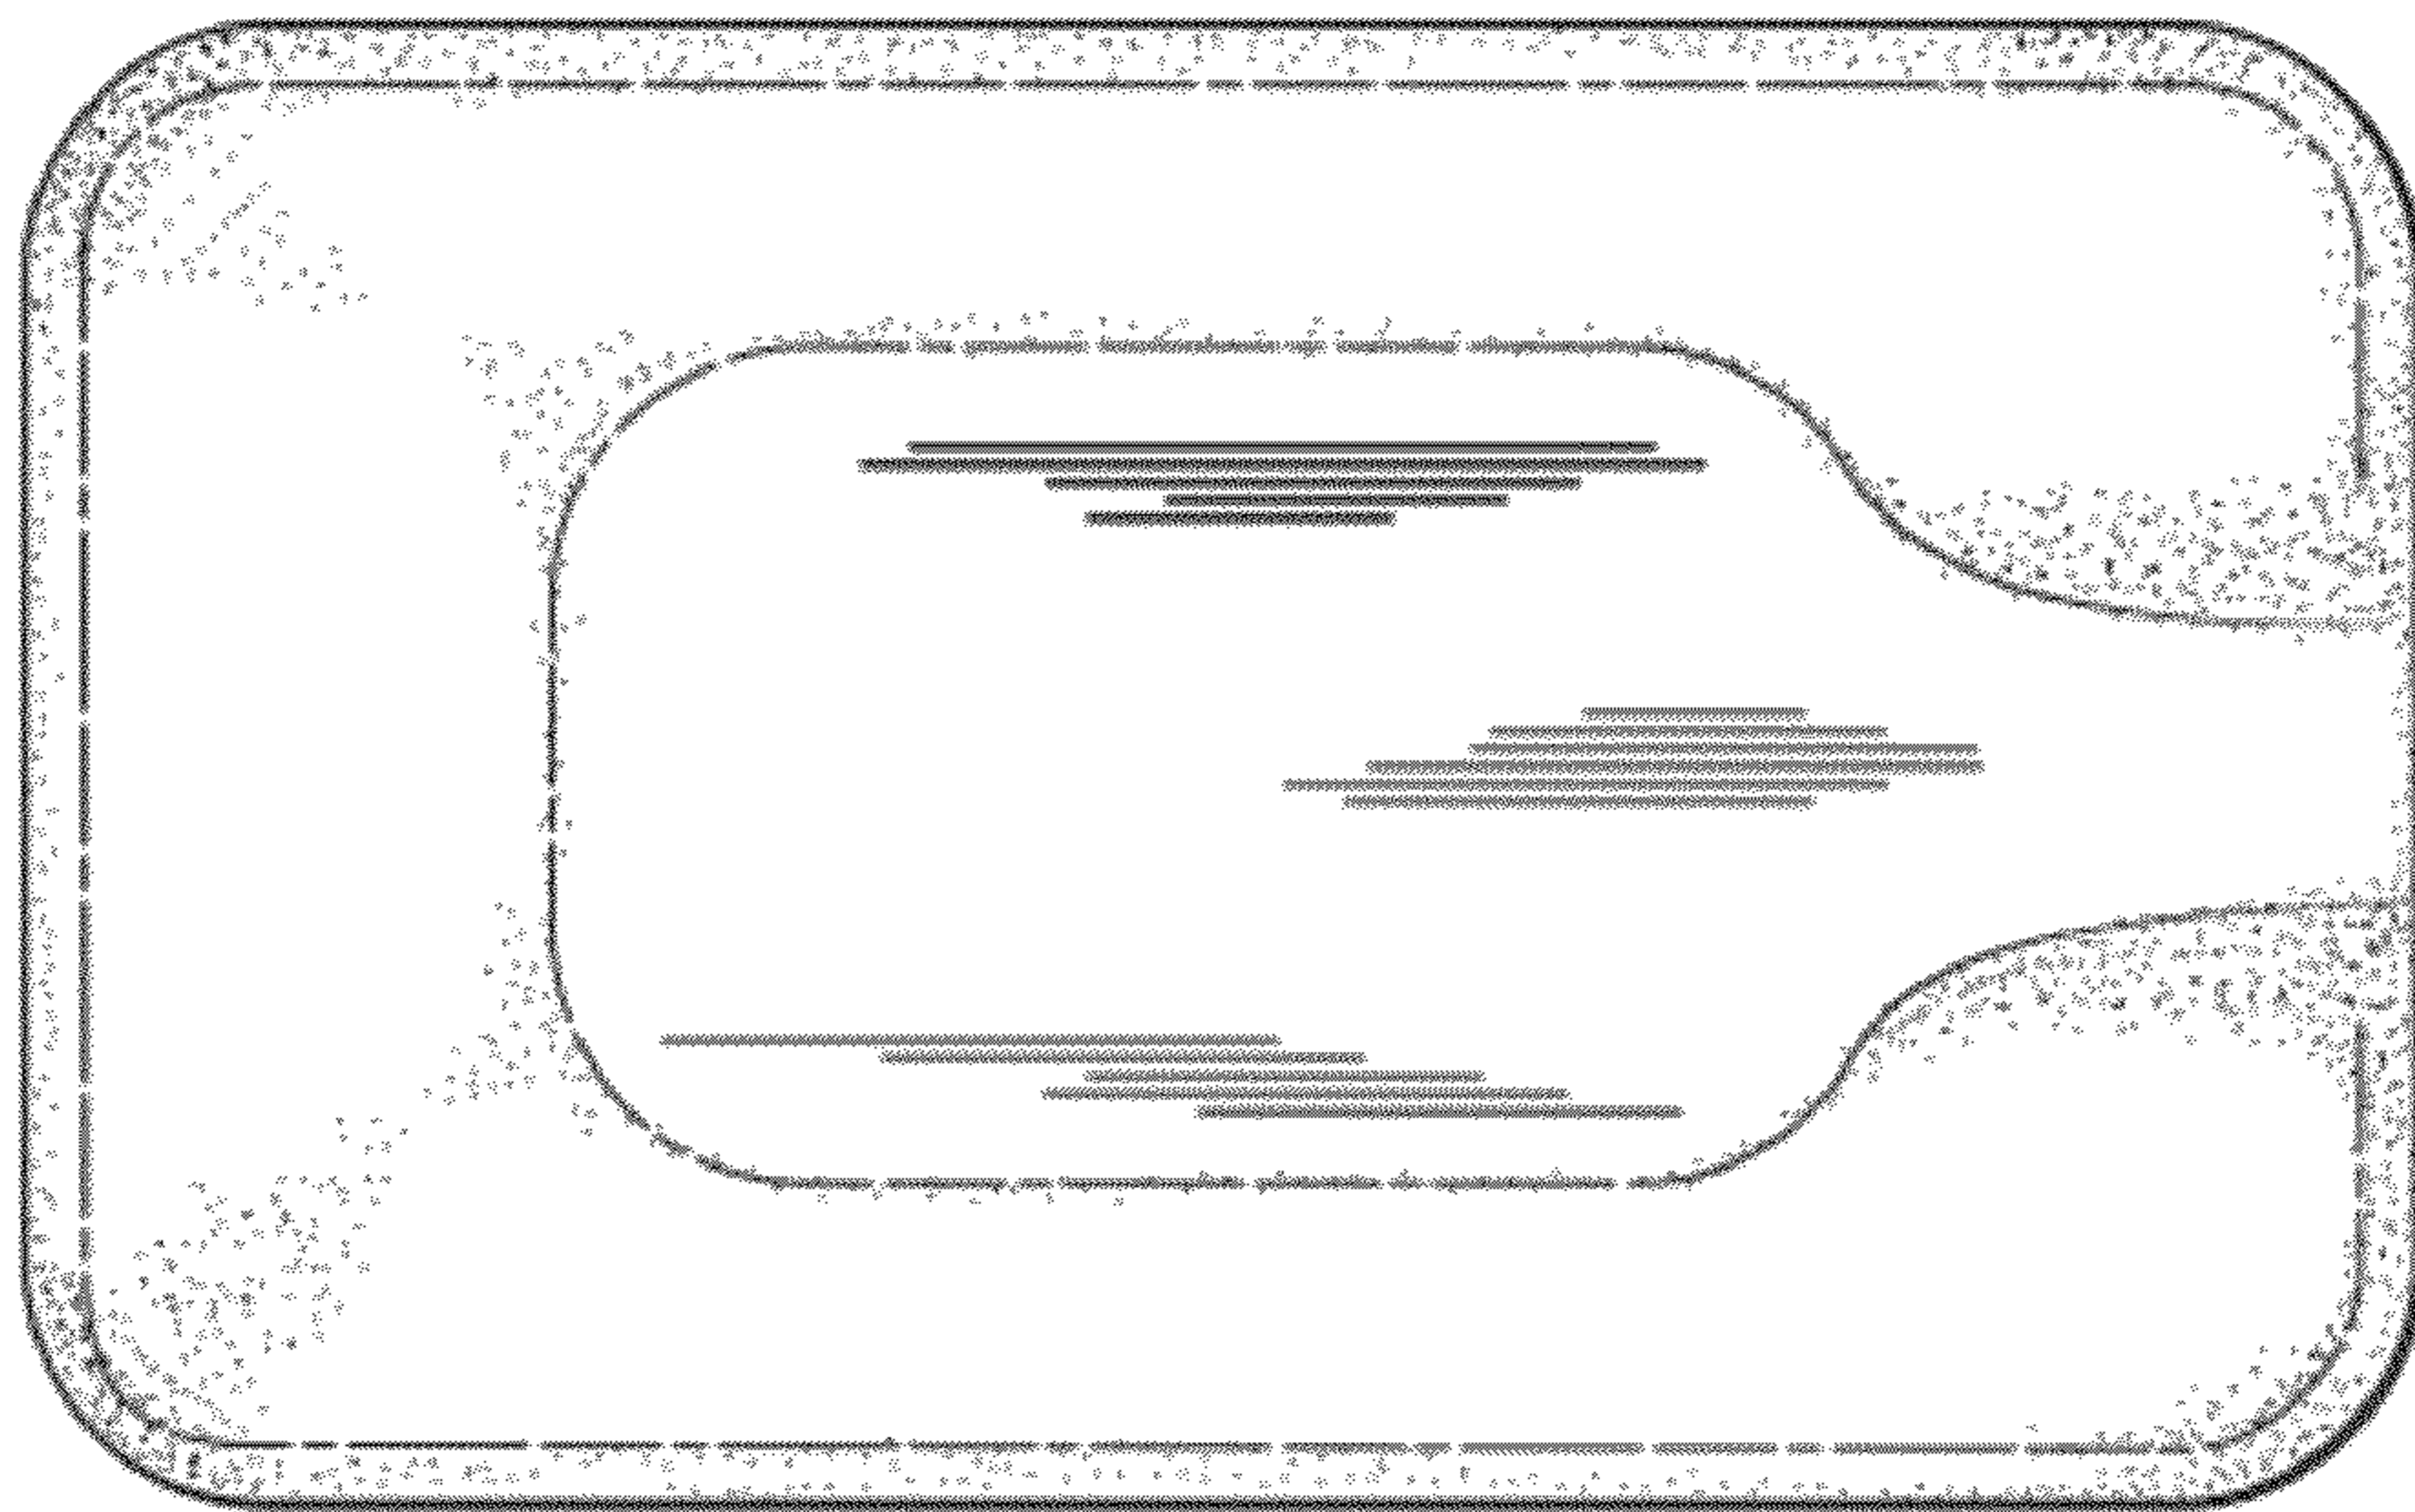


Fig. 2

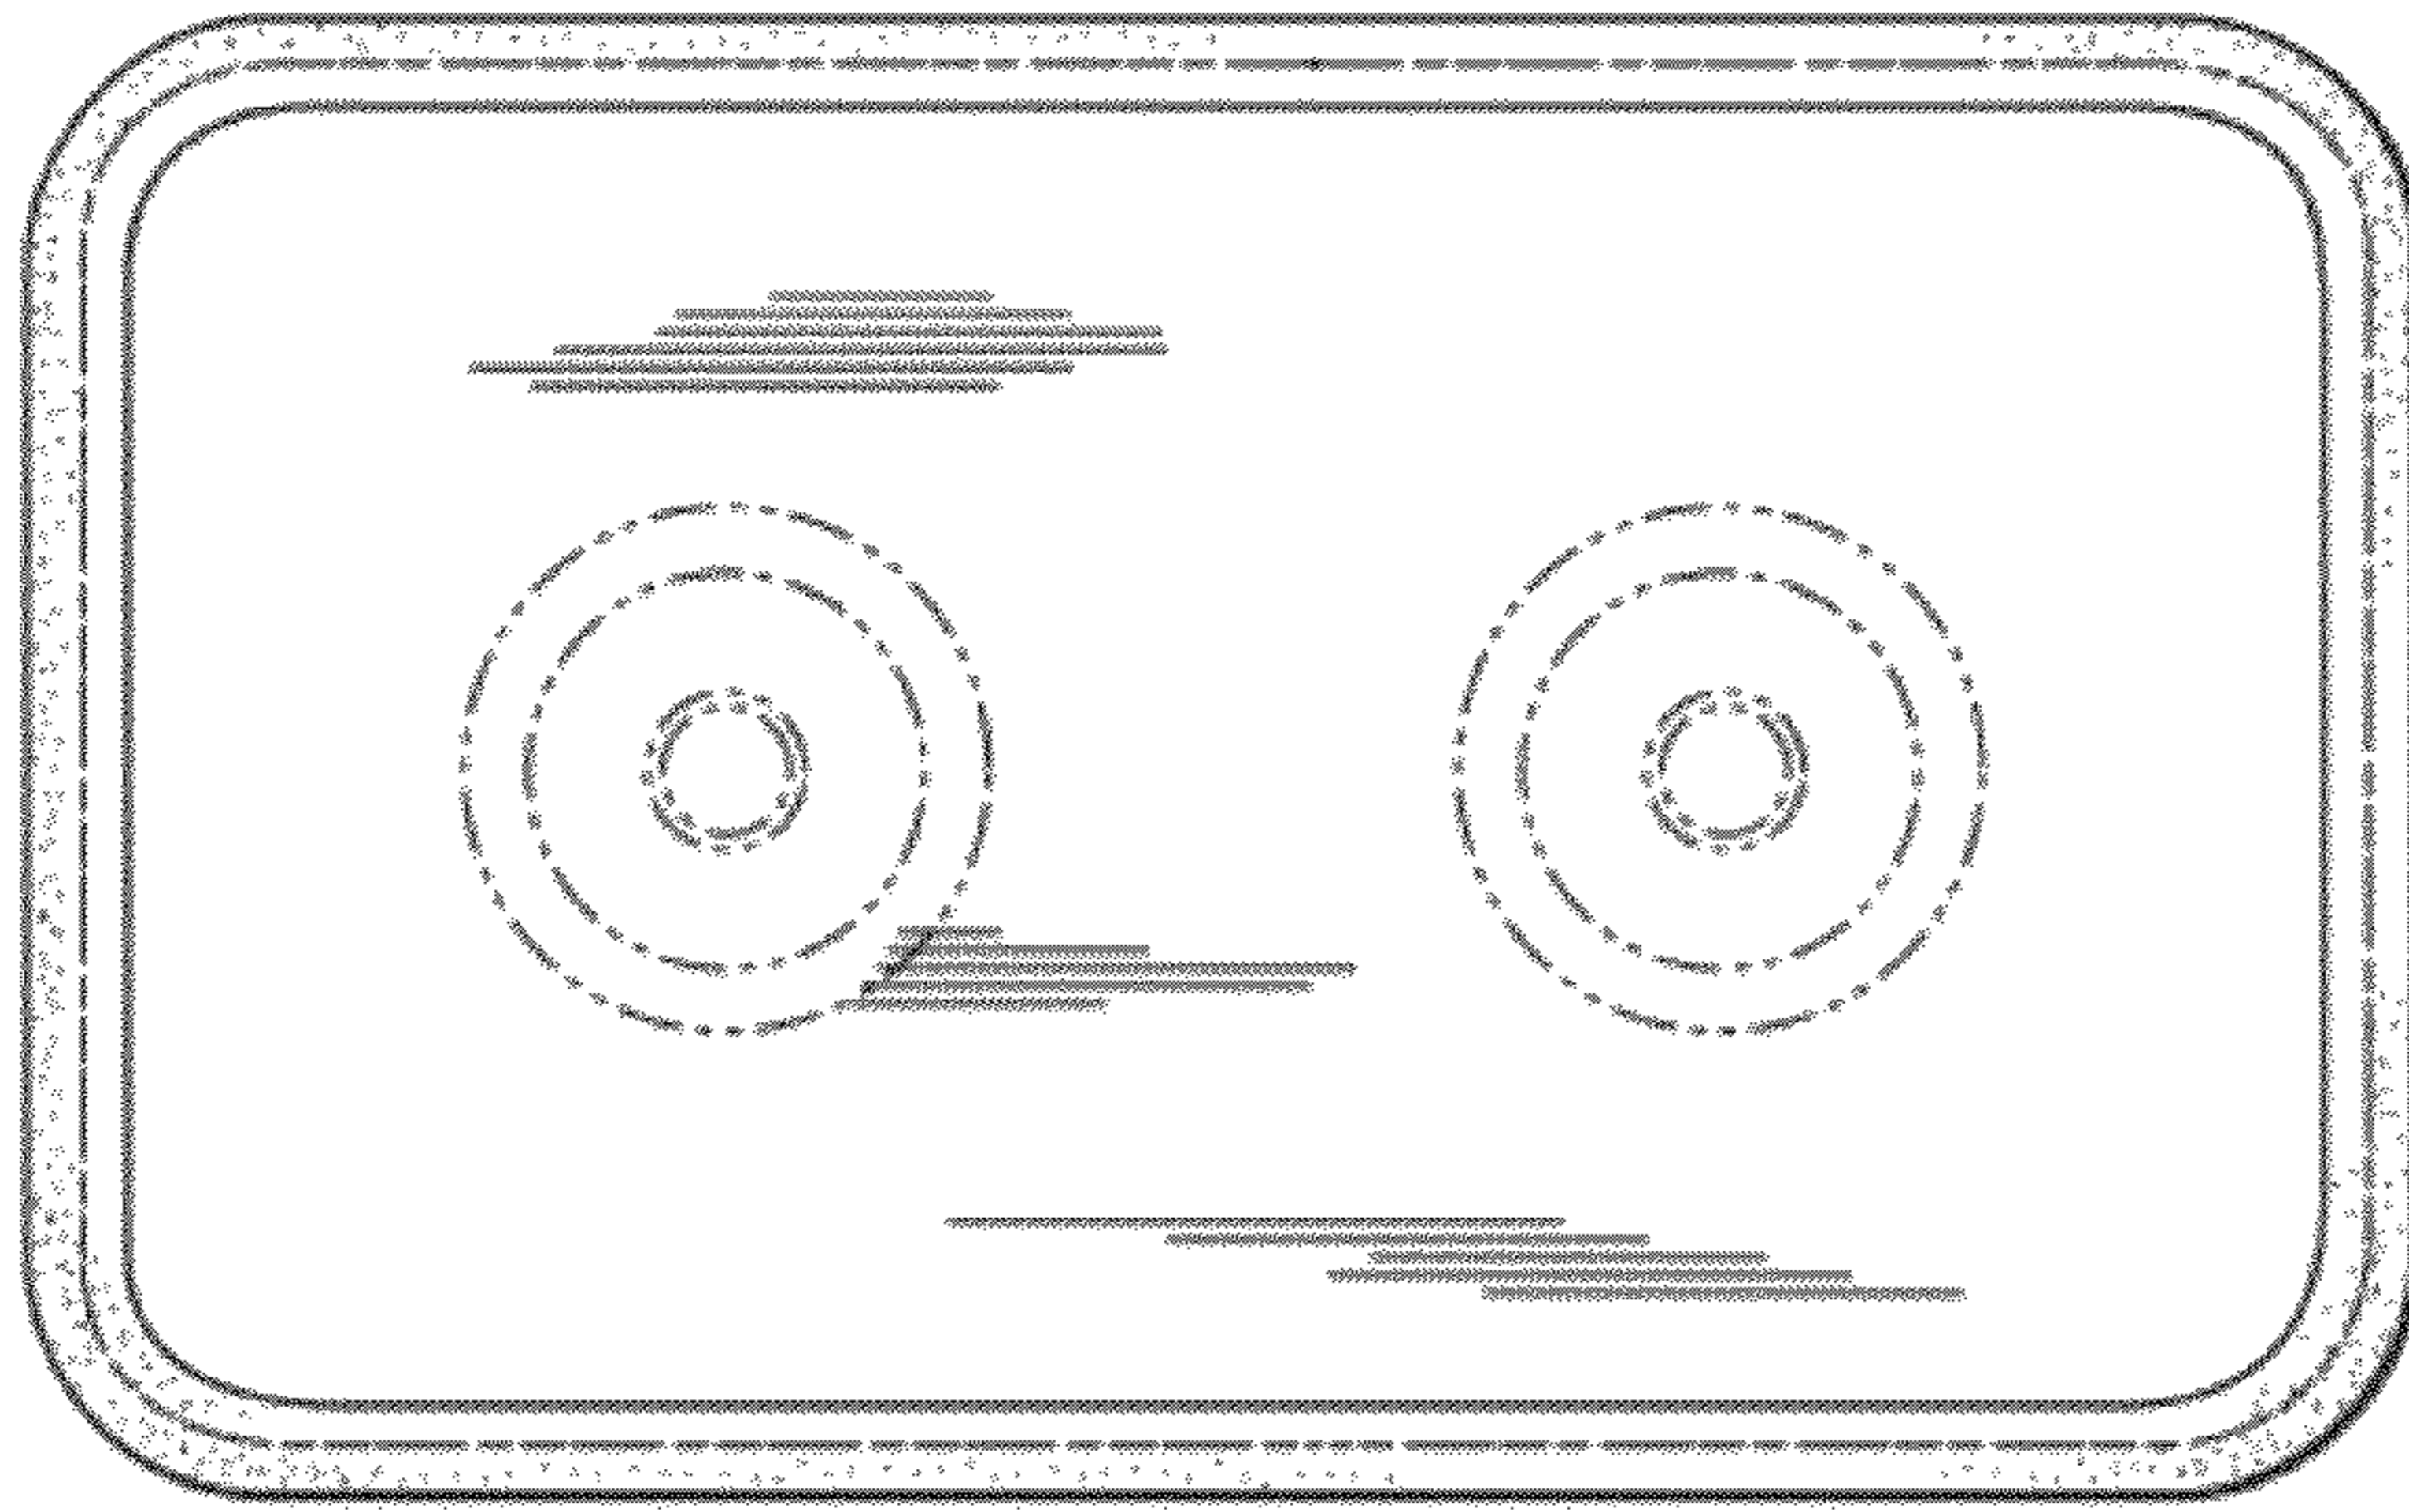


Fig. 3

Fig. 4

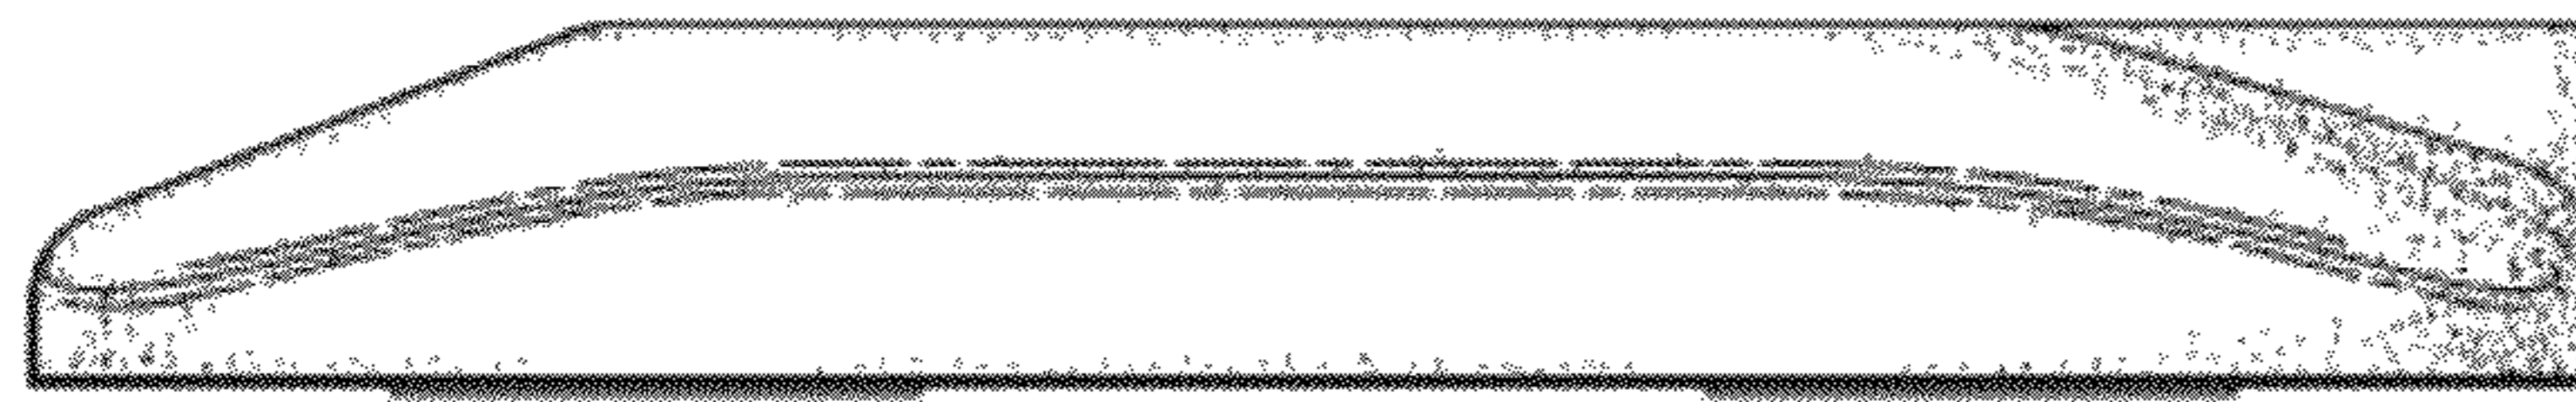
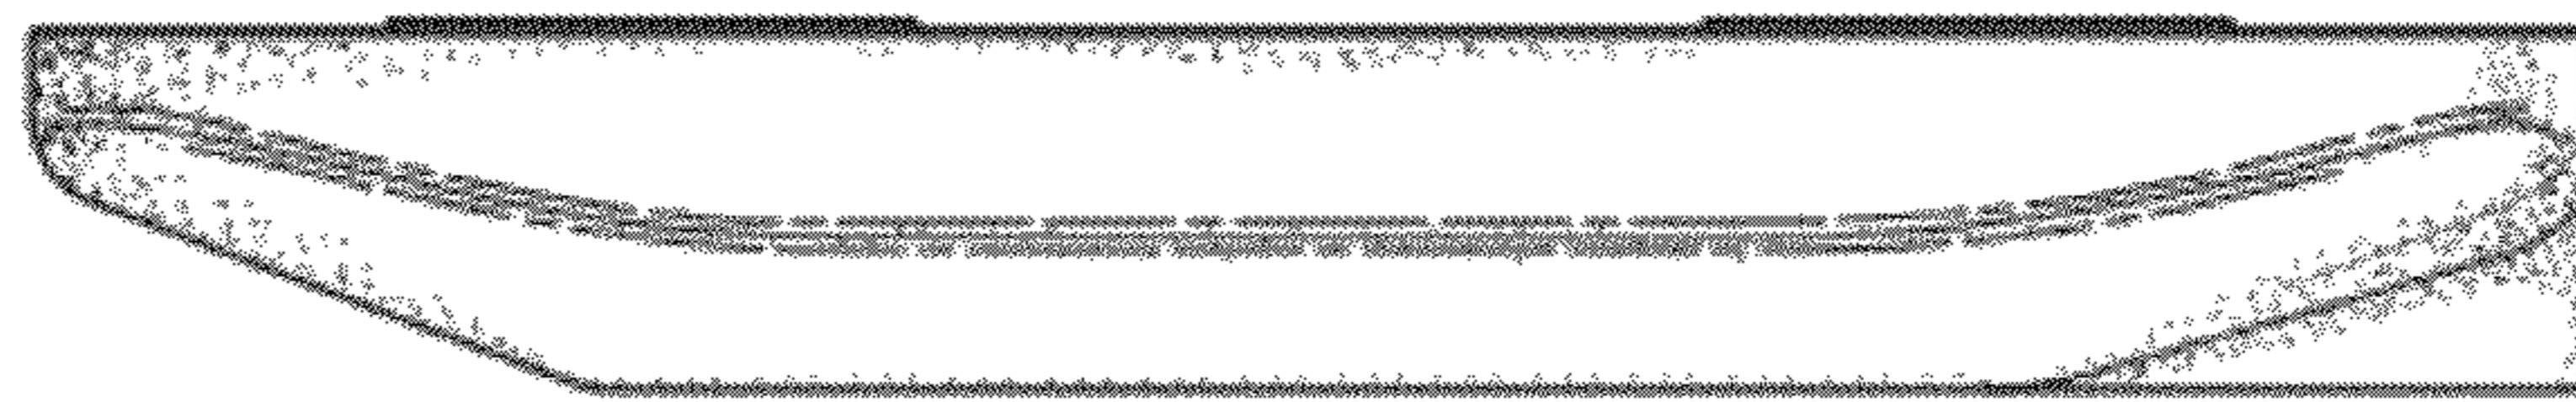


Fig. 5

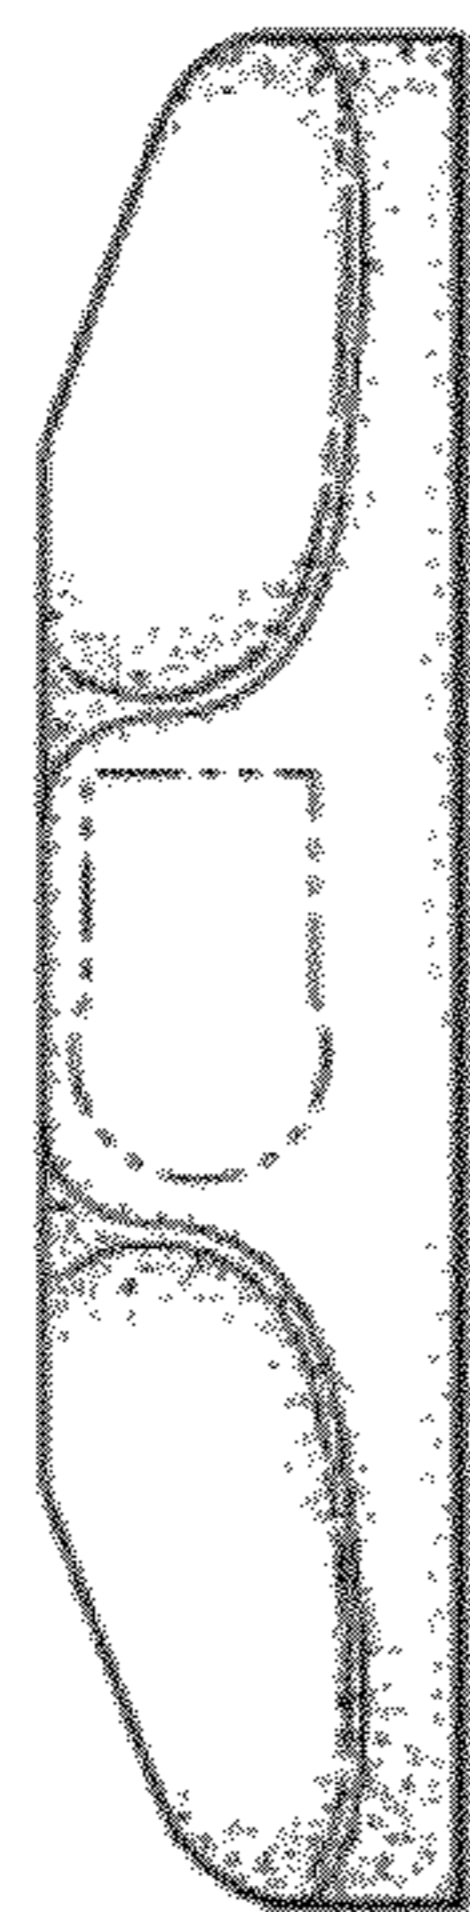


Fig. 6

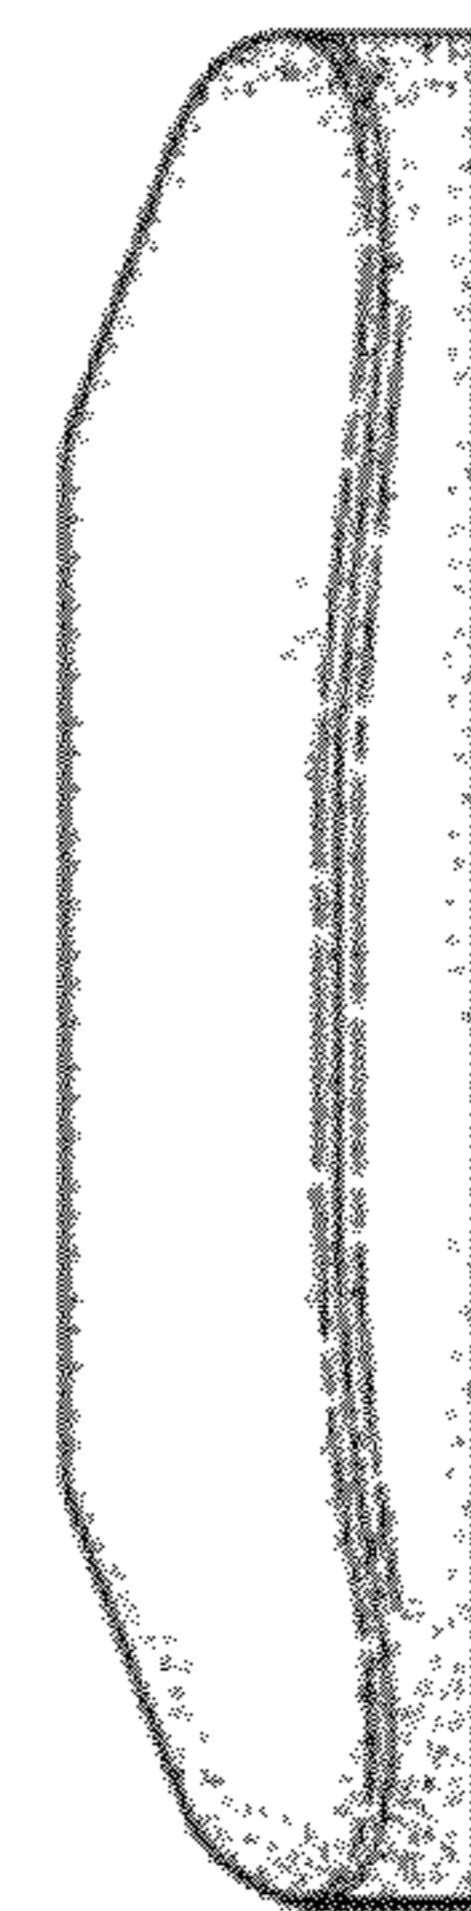


Fig. 7

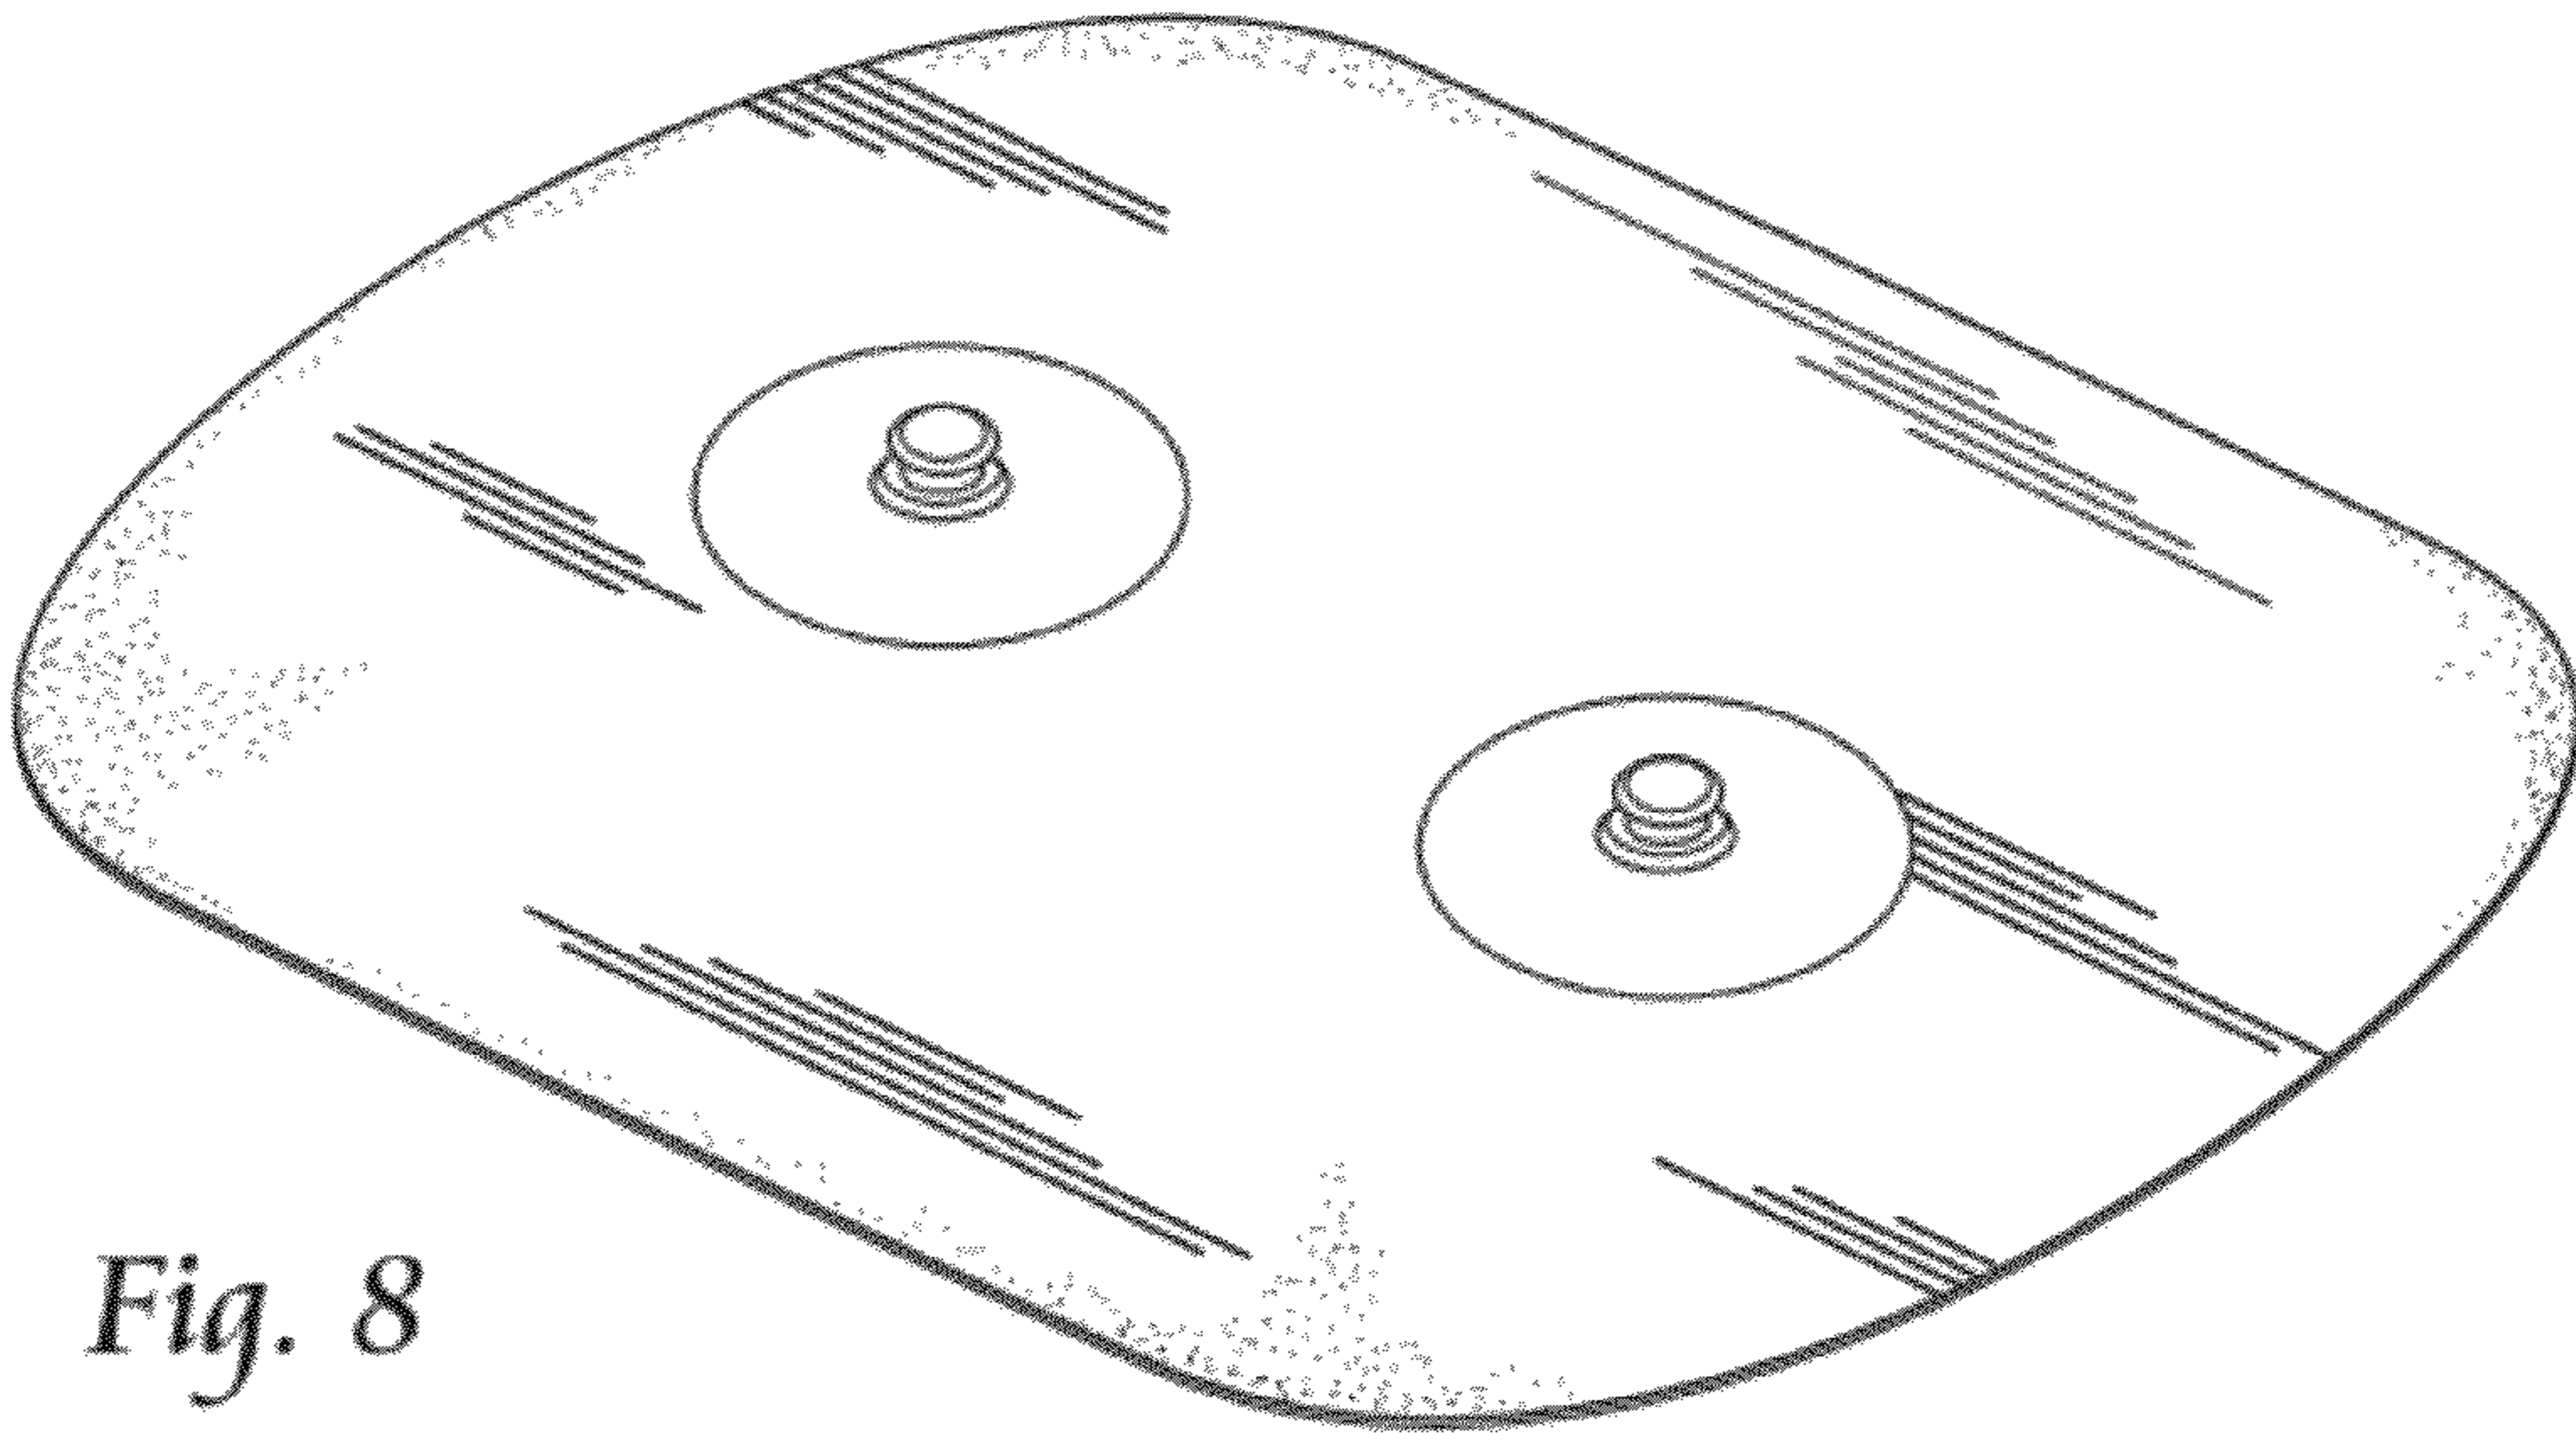


Fig. 8

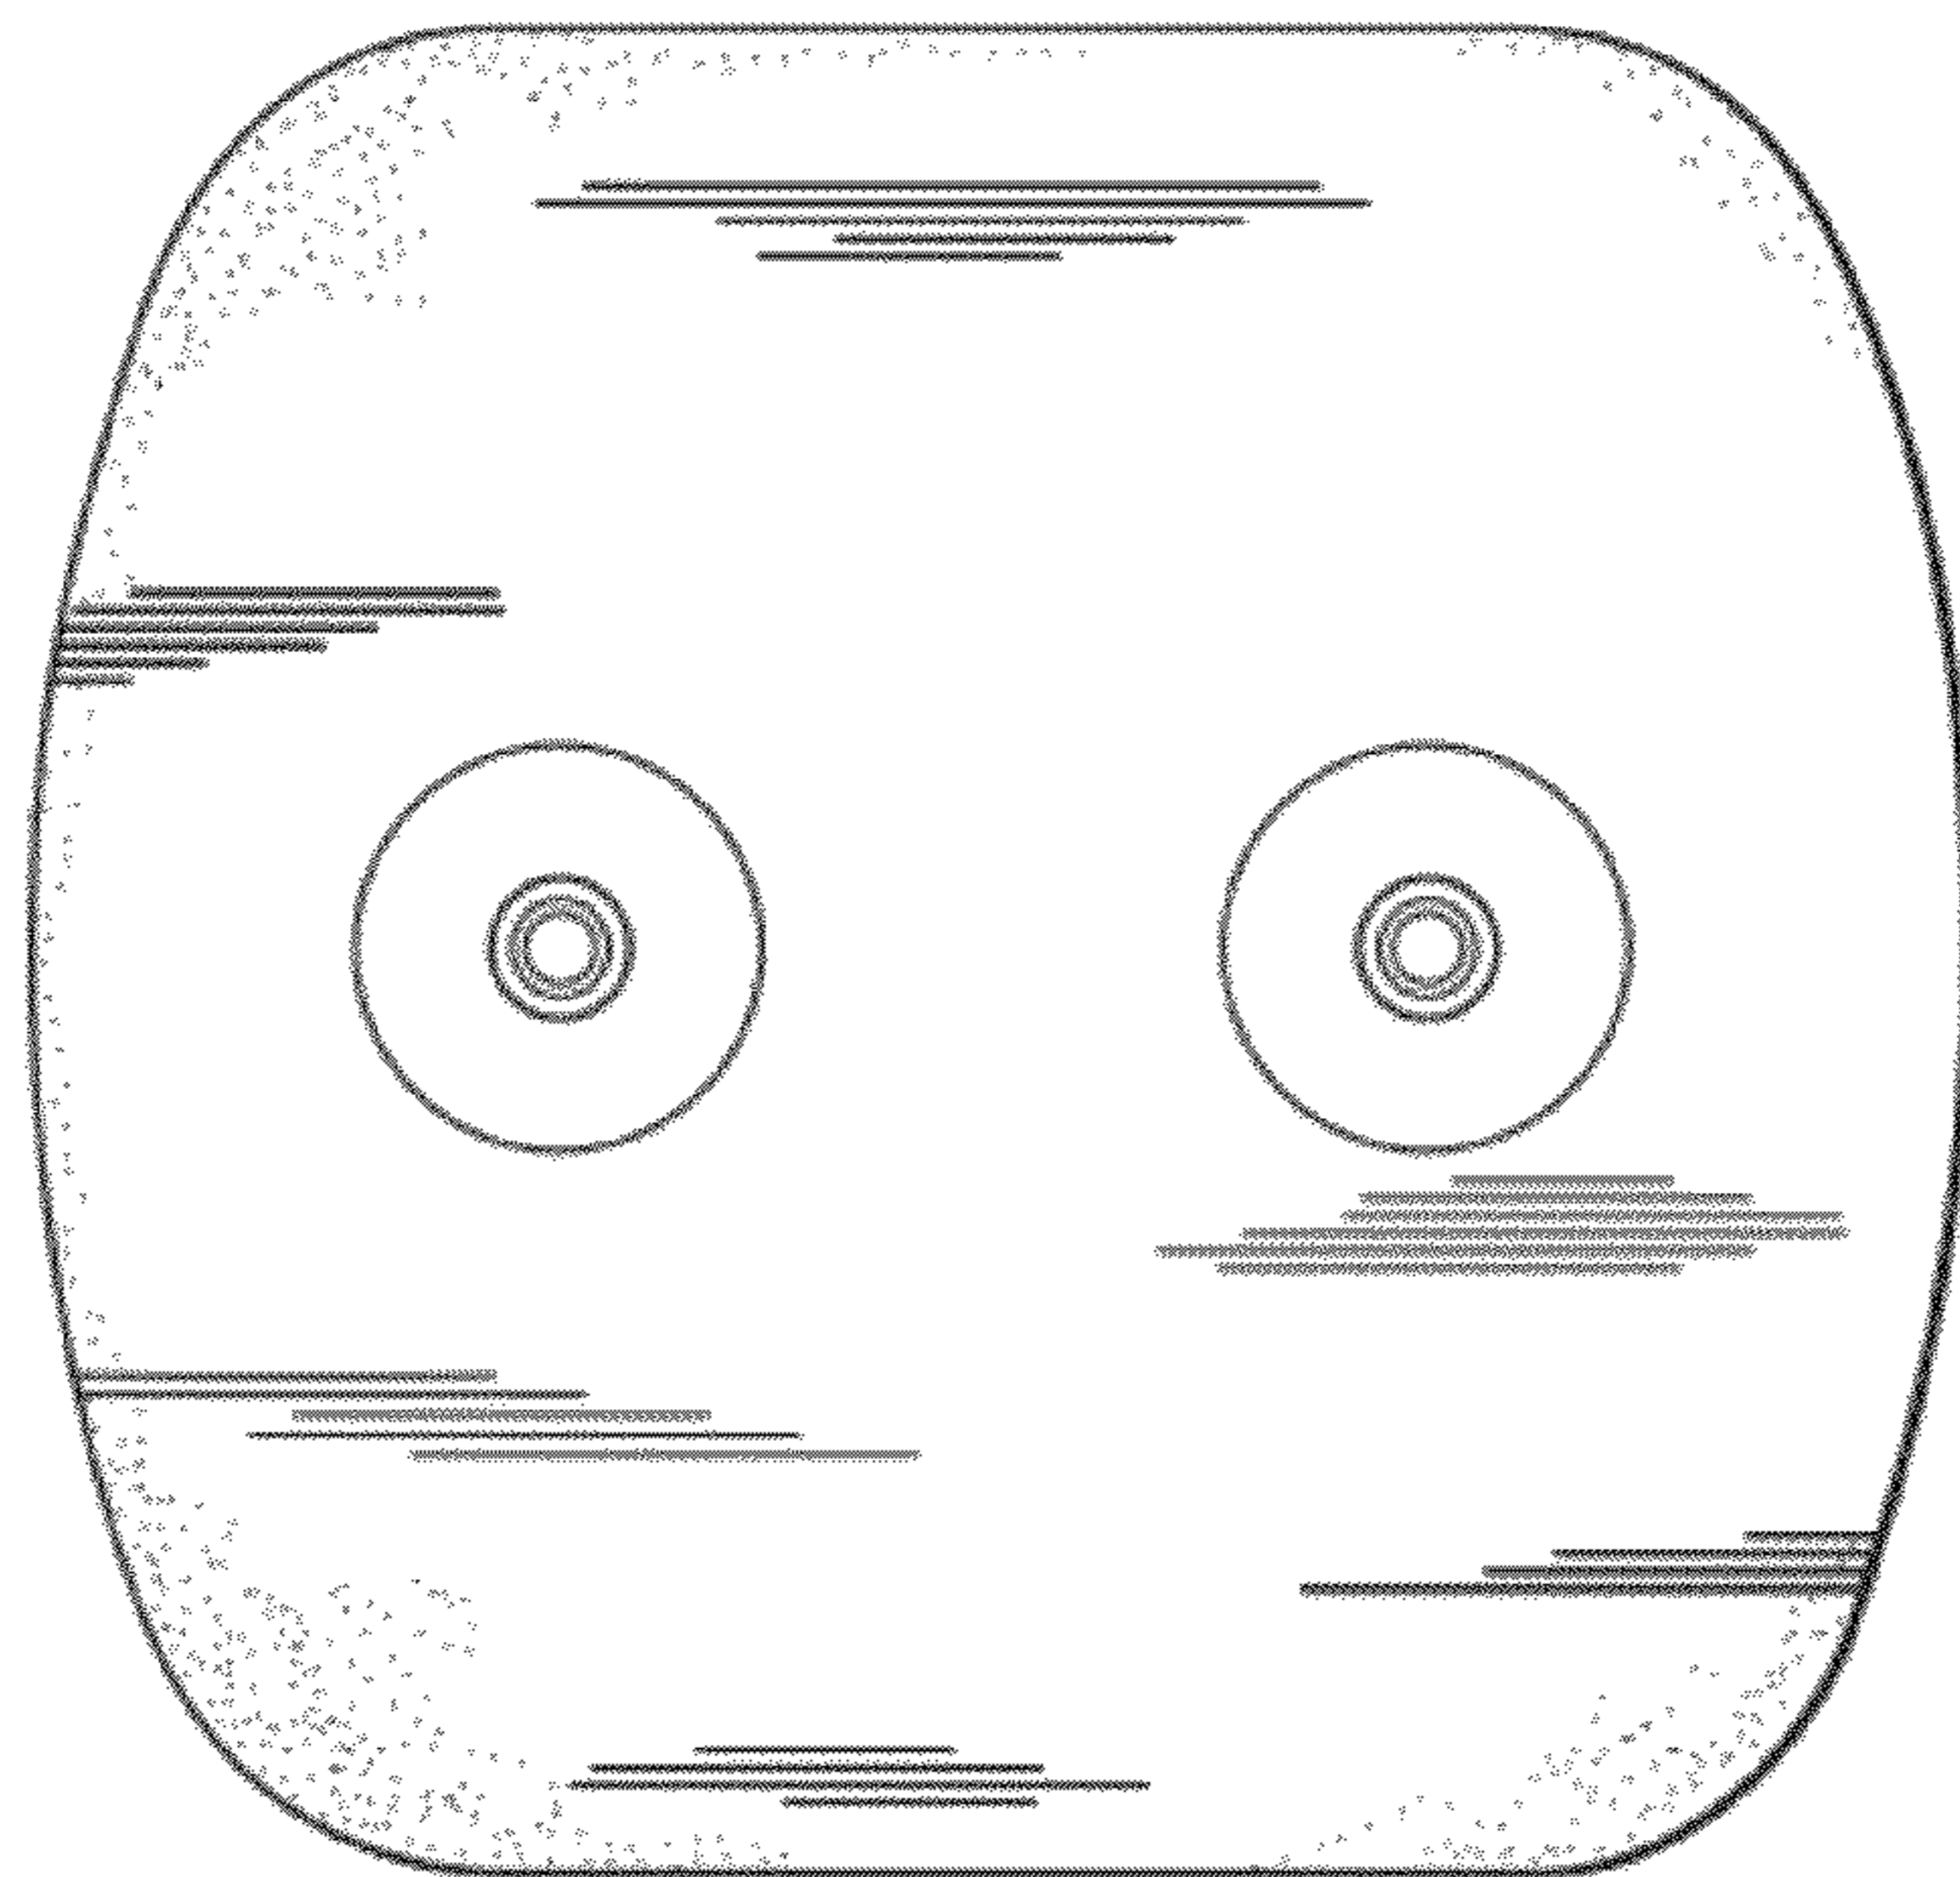


Fig. 9

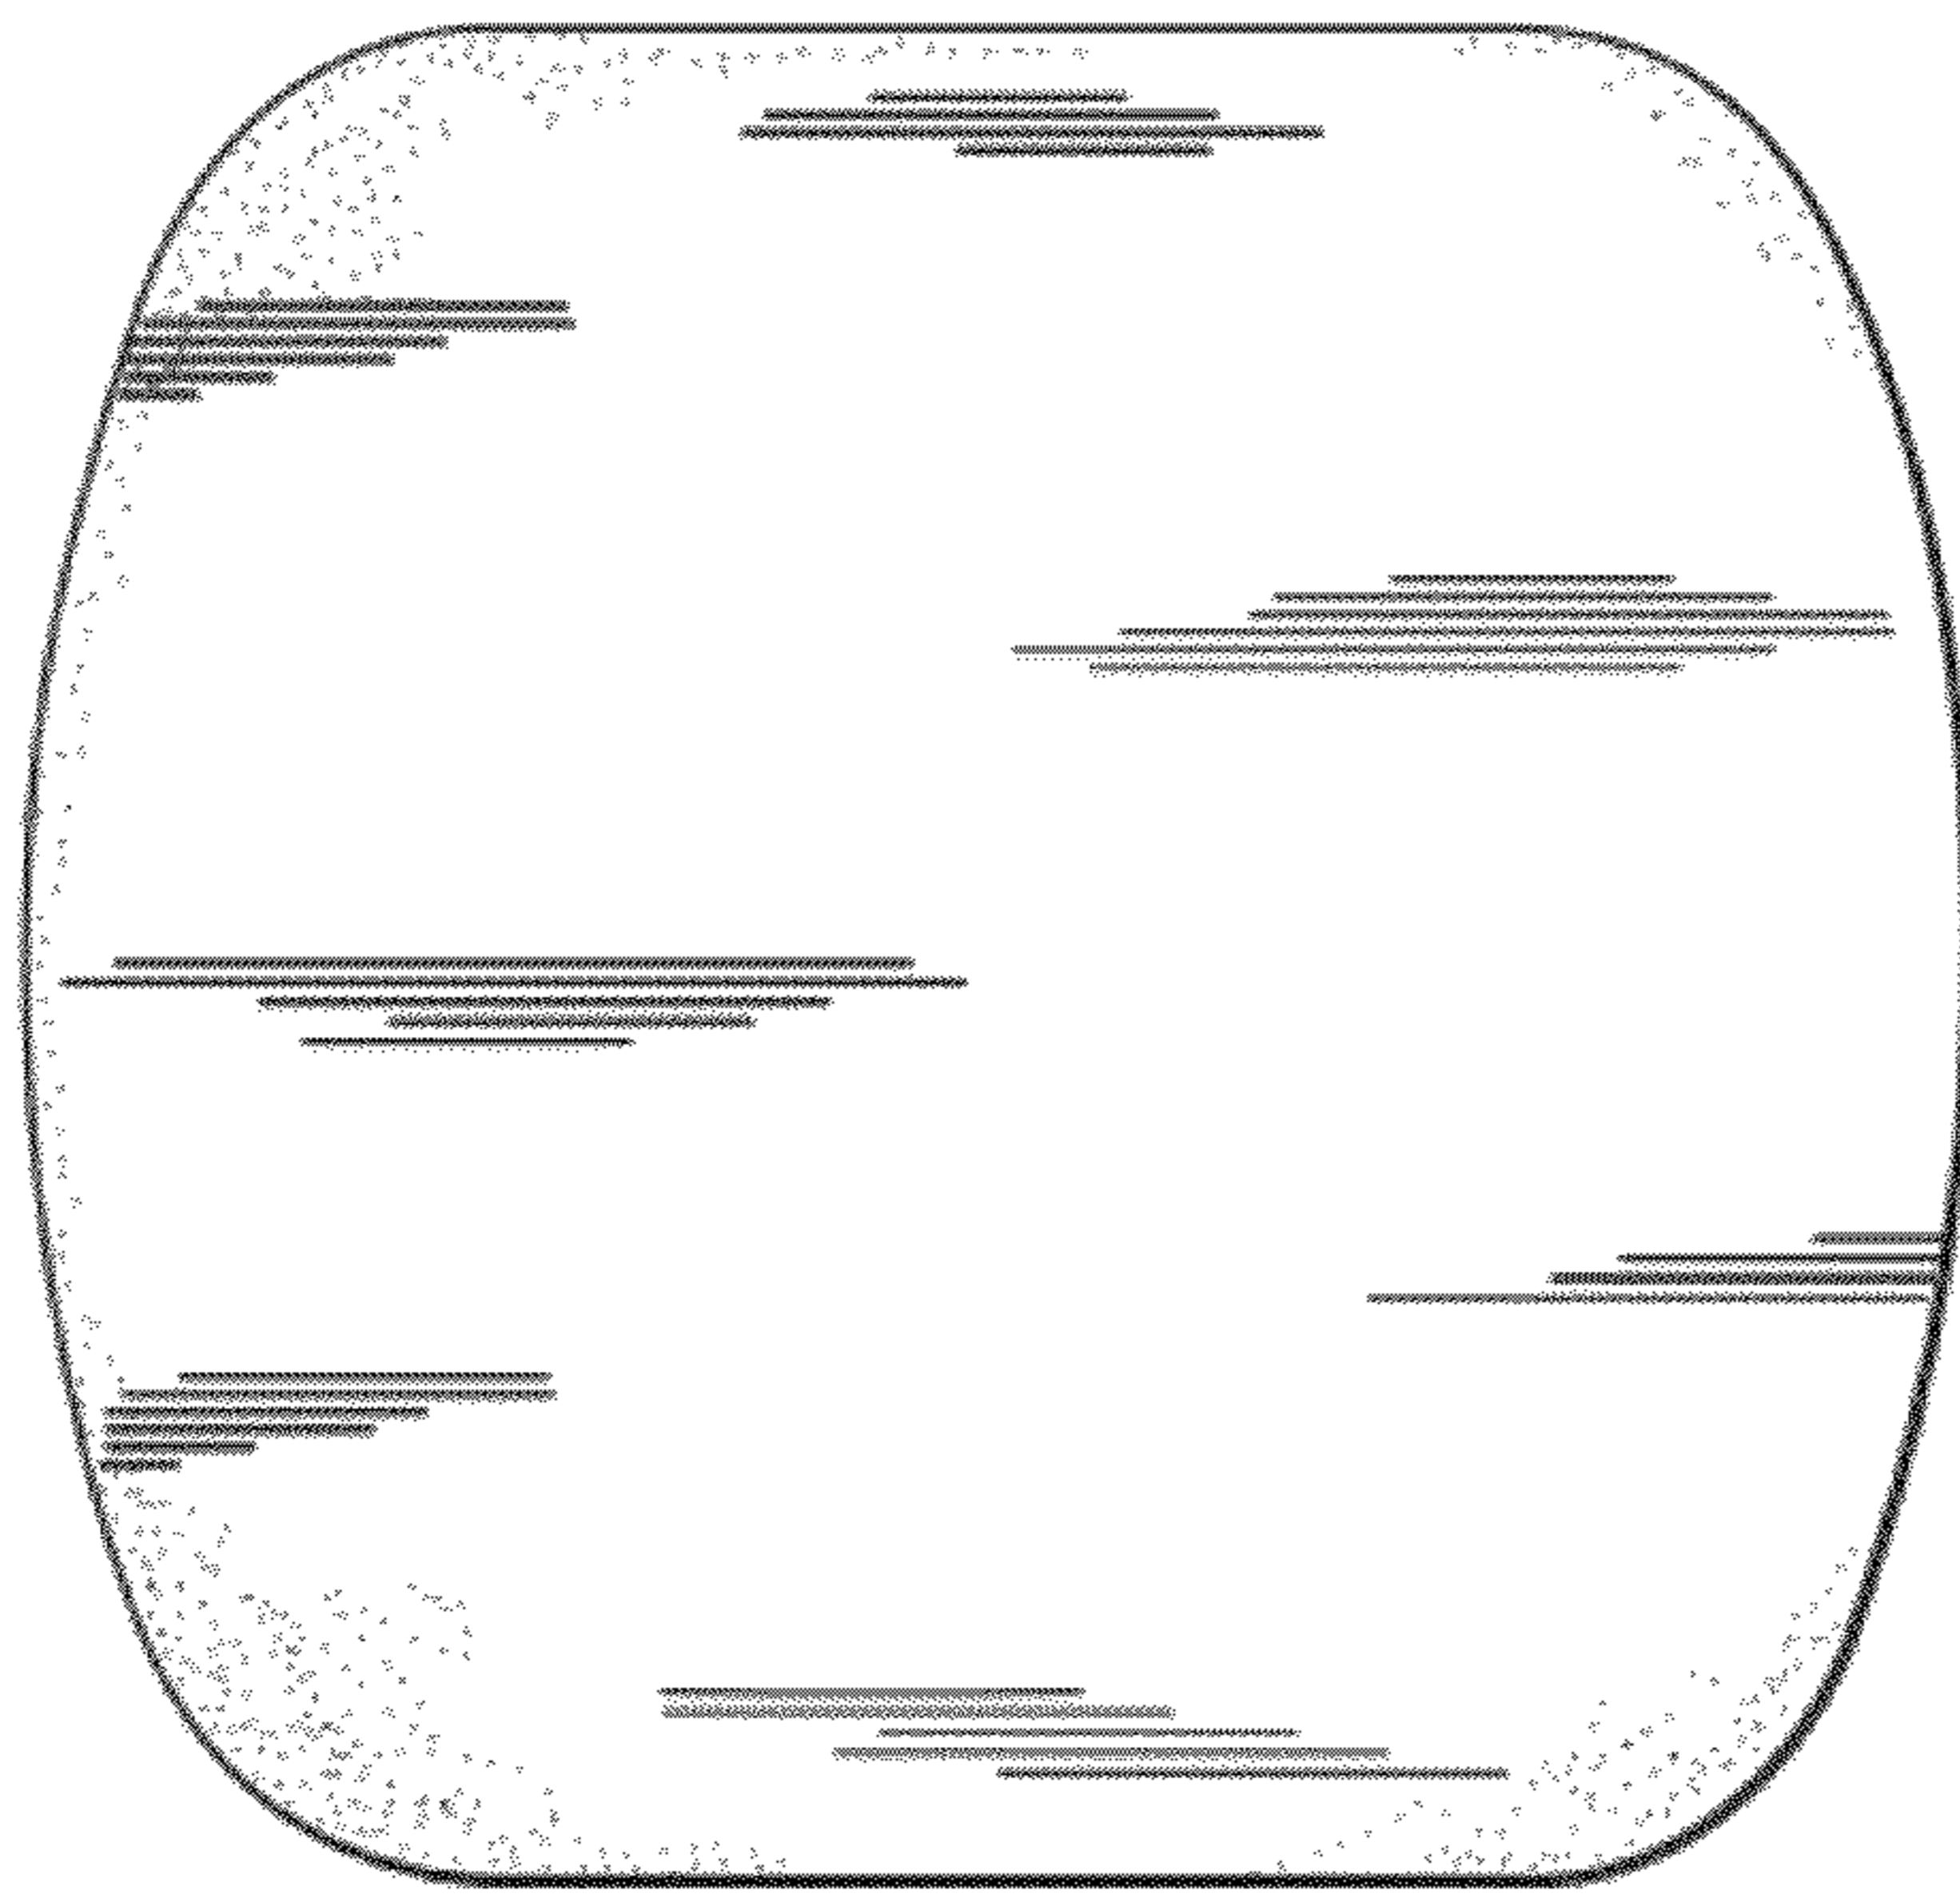


Fig. 10



Fig. 11

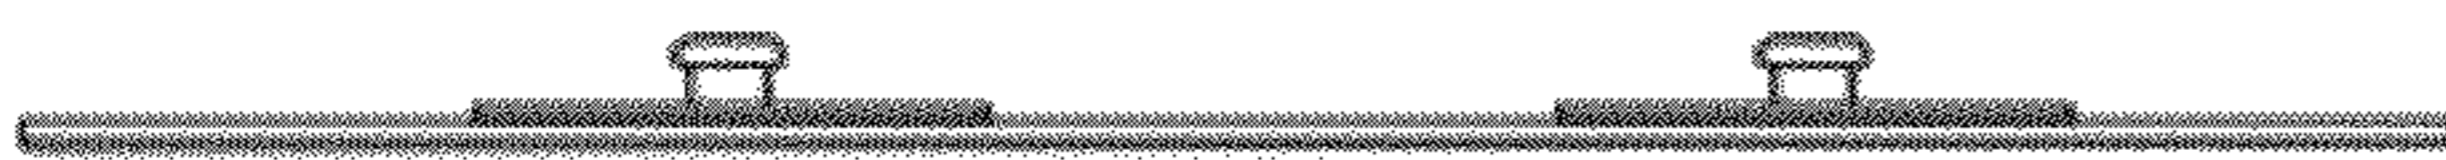


Fig. 12



Fig. 13



Fig. 14

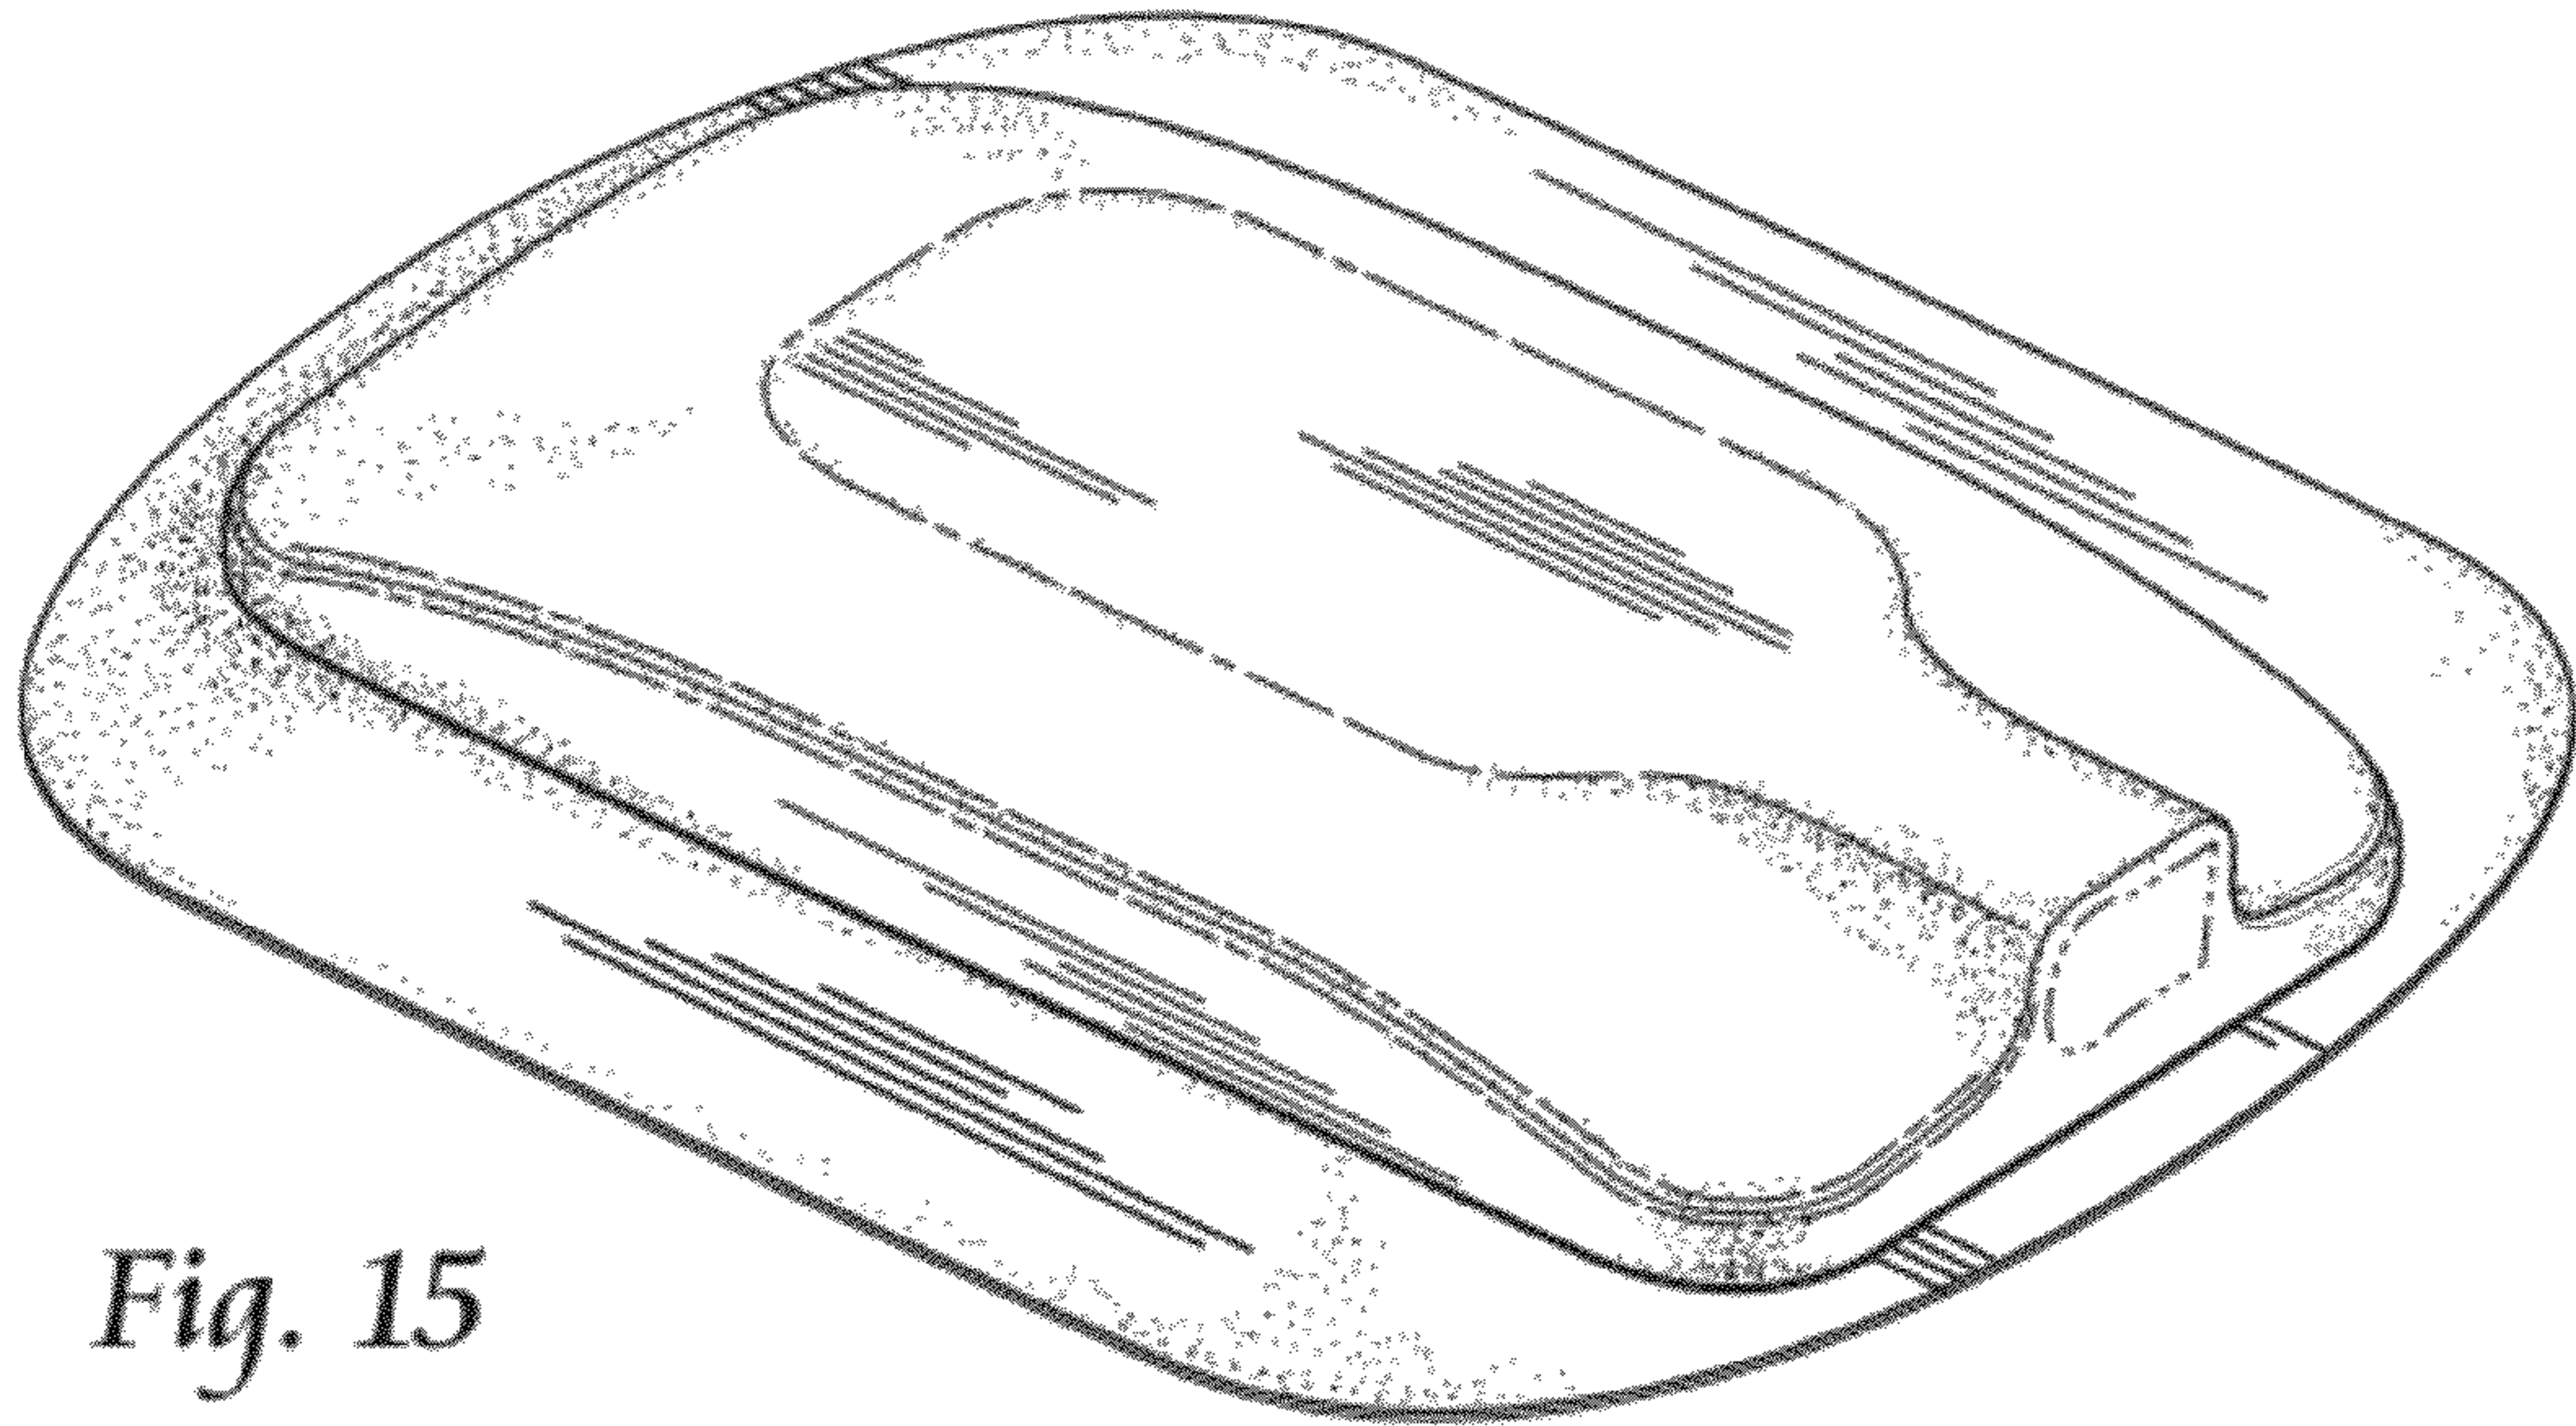


Fig. 15

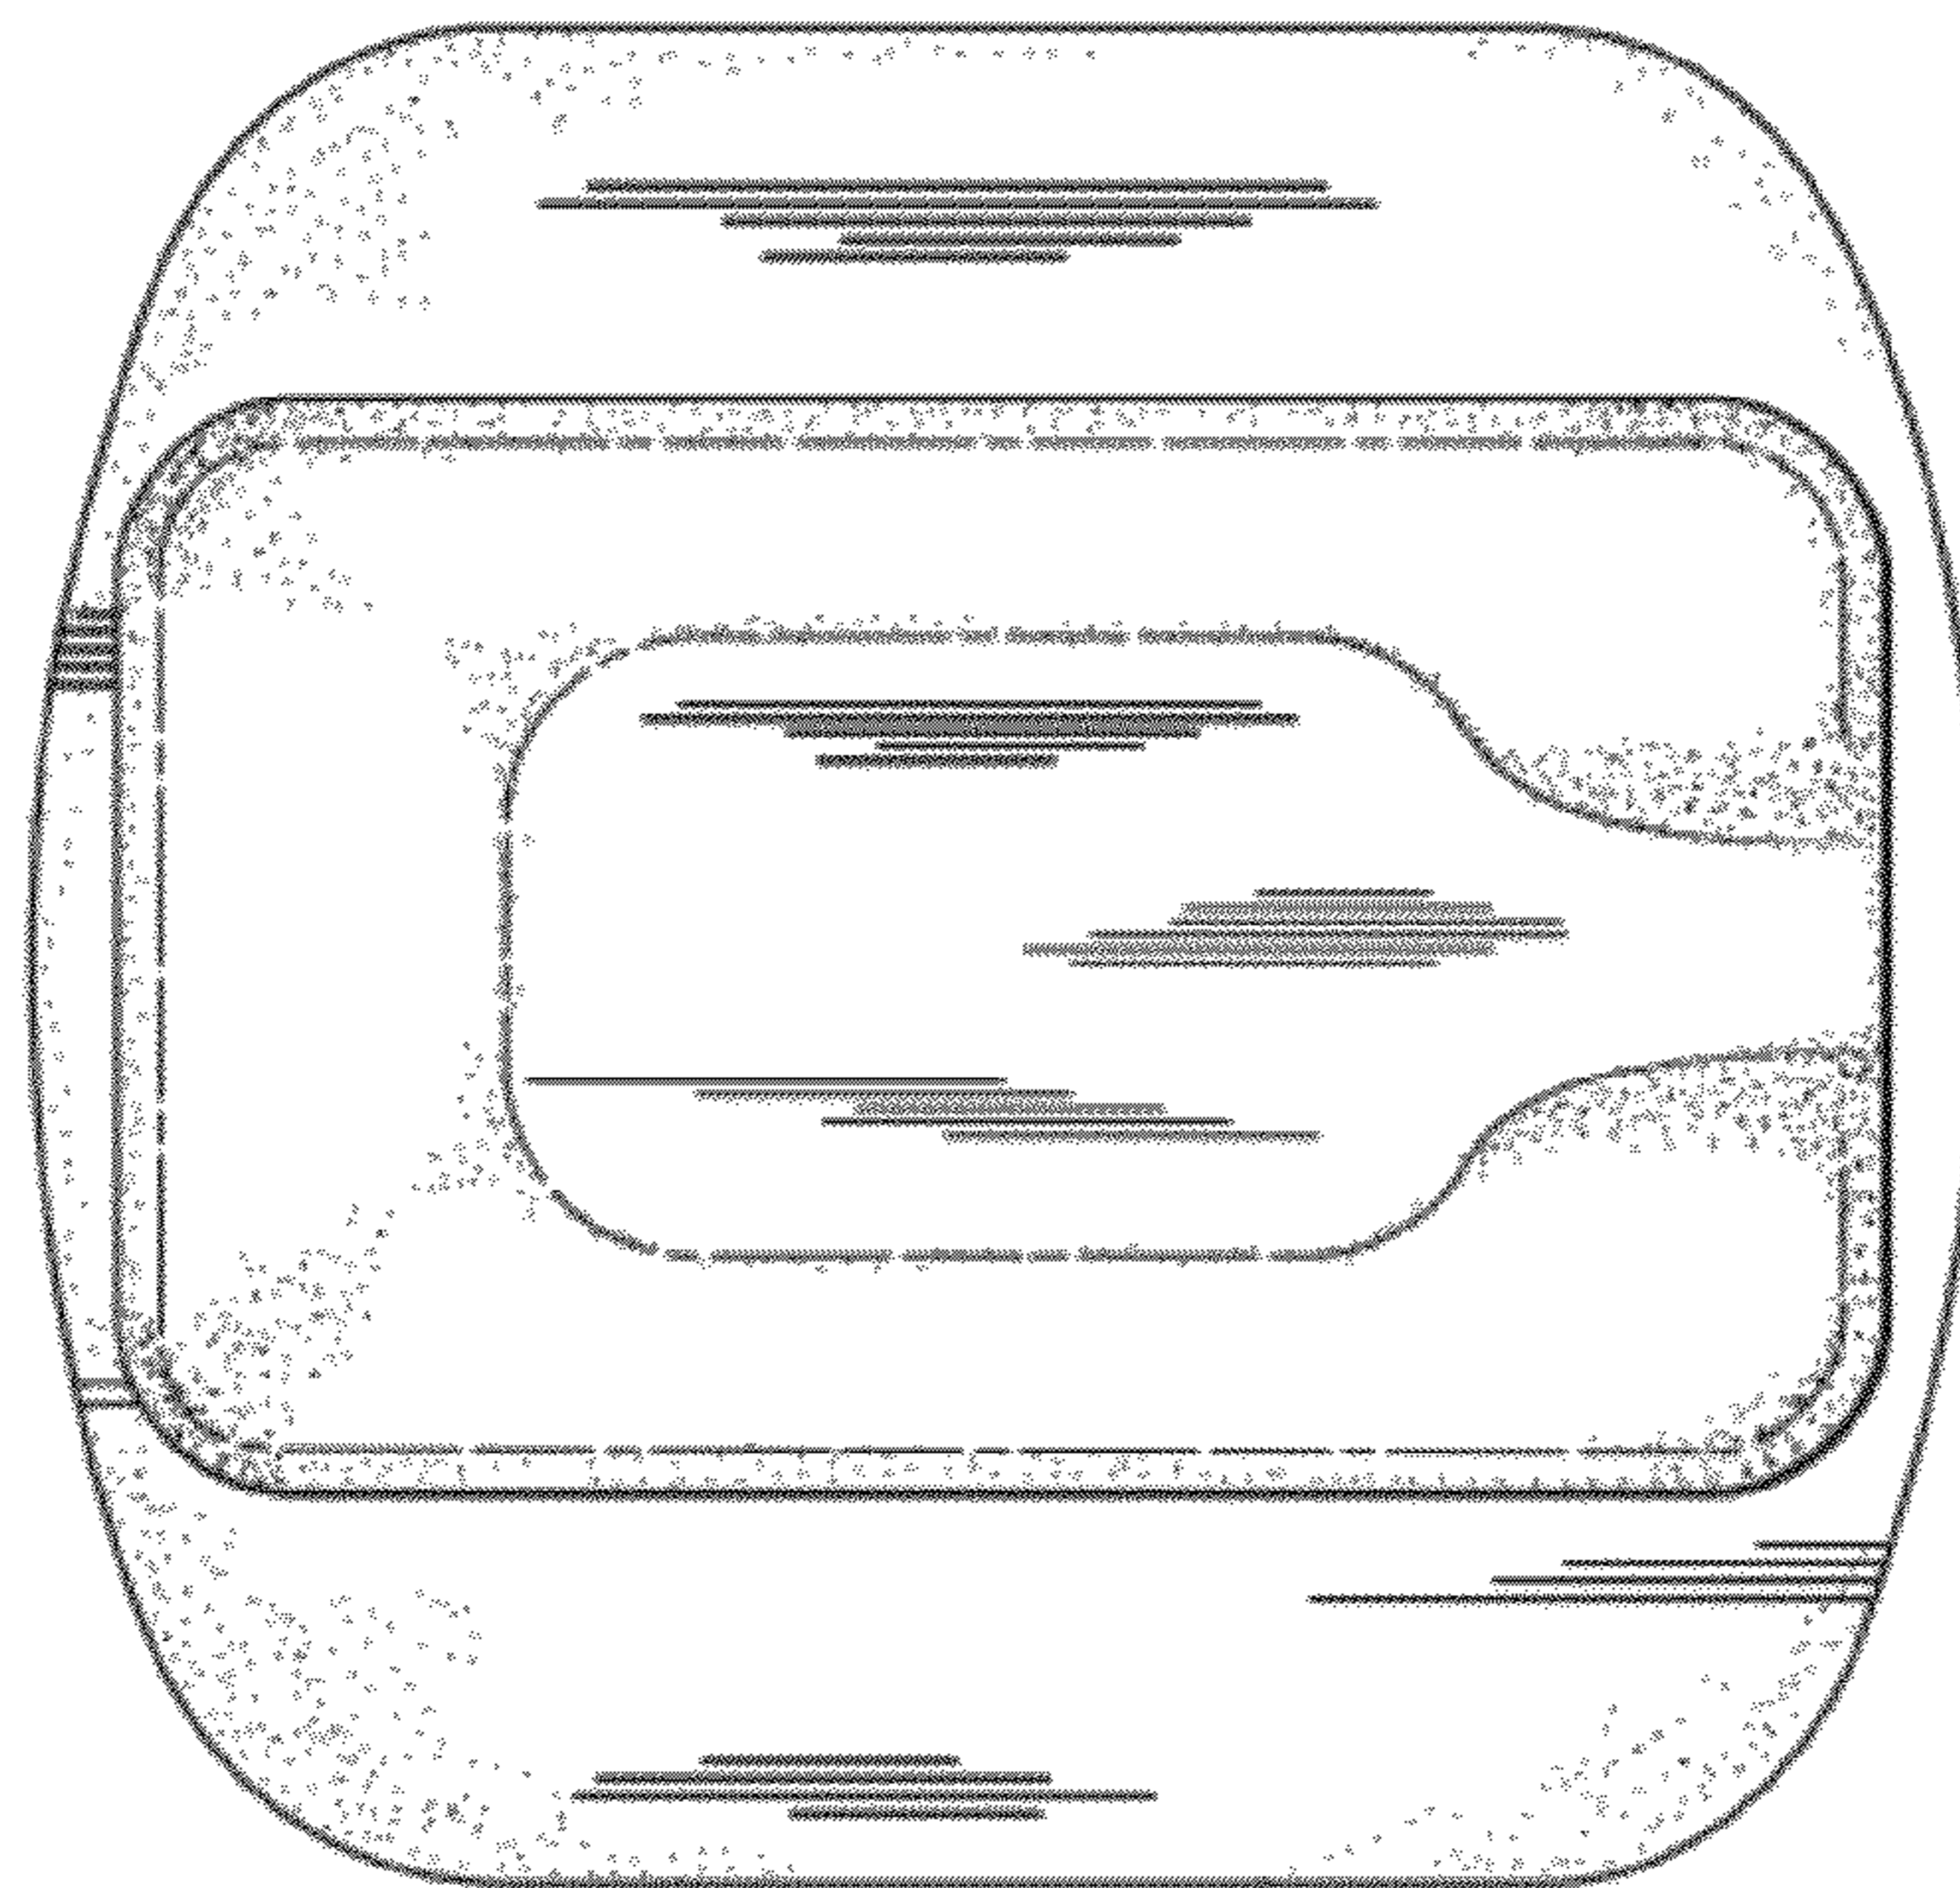


Fig. 16

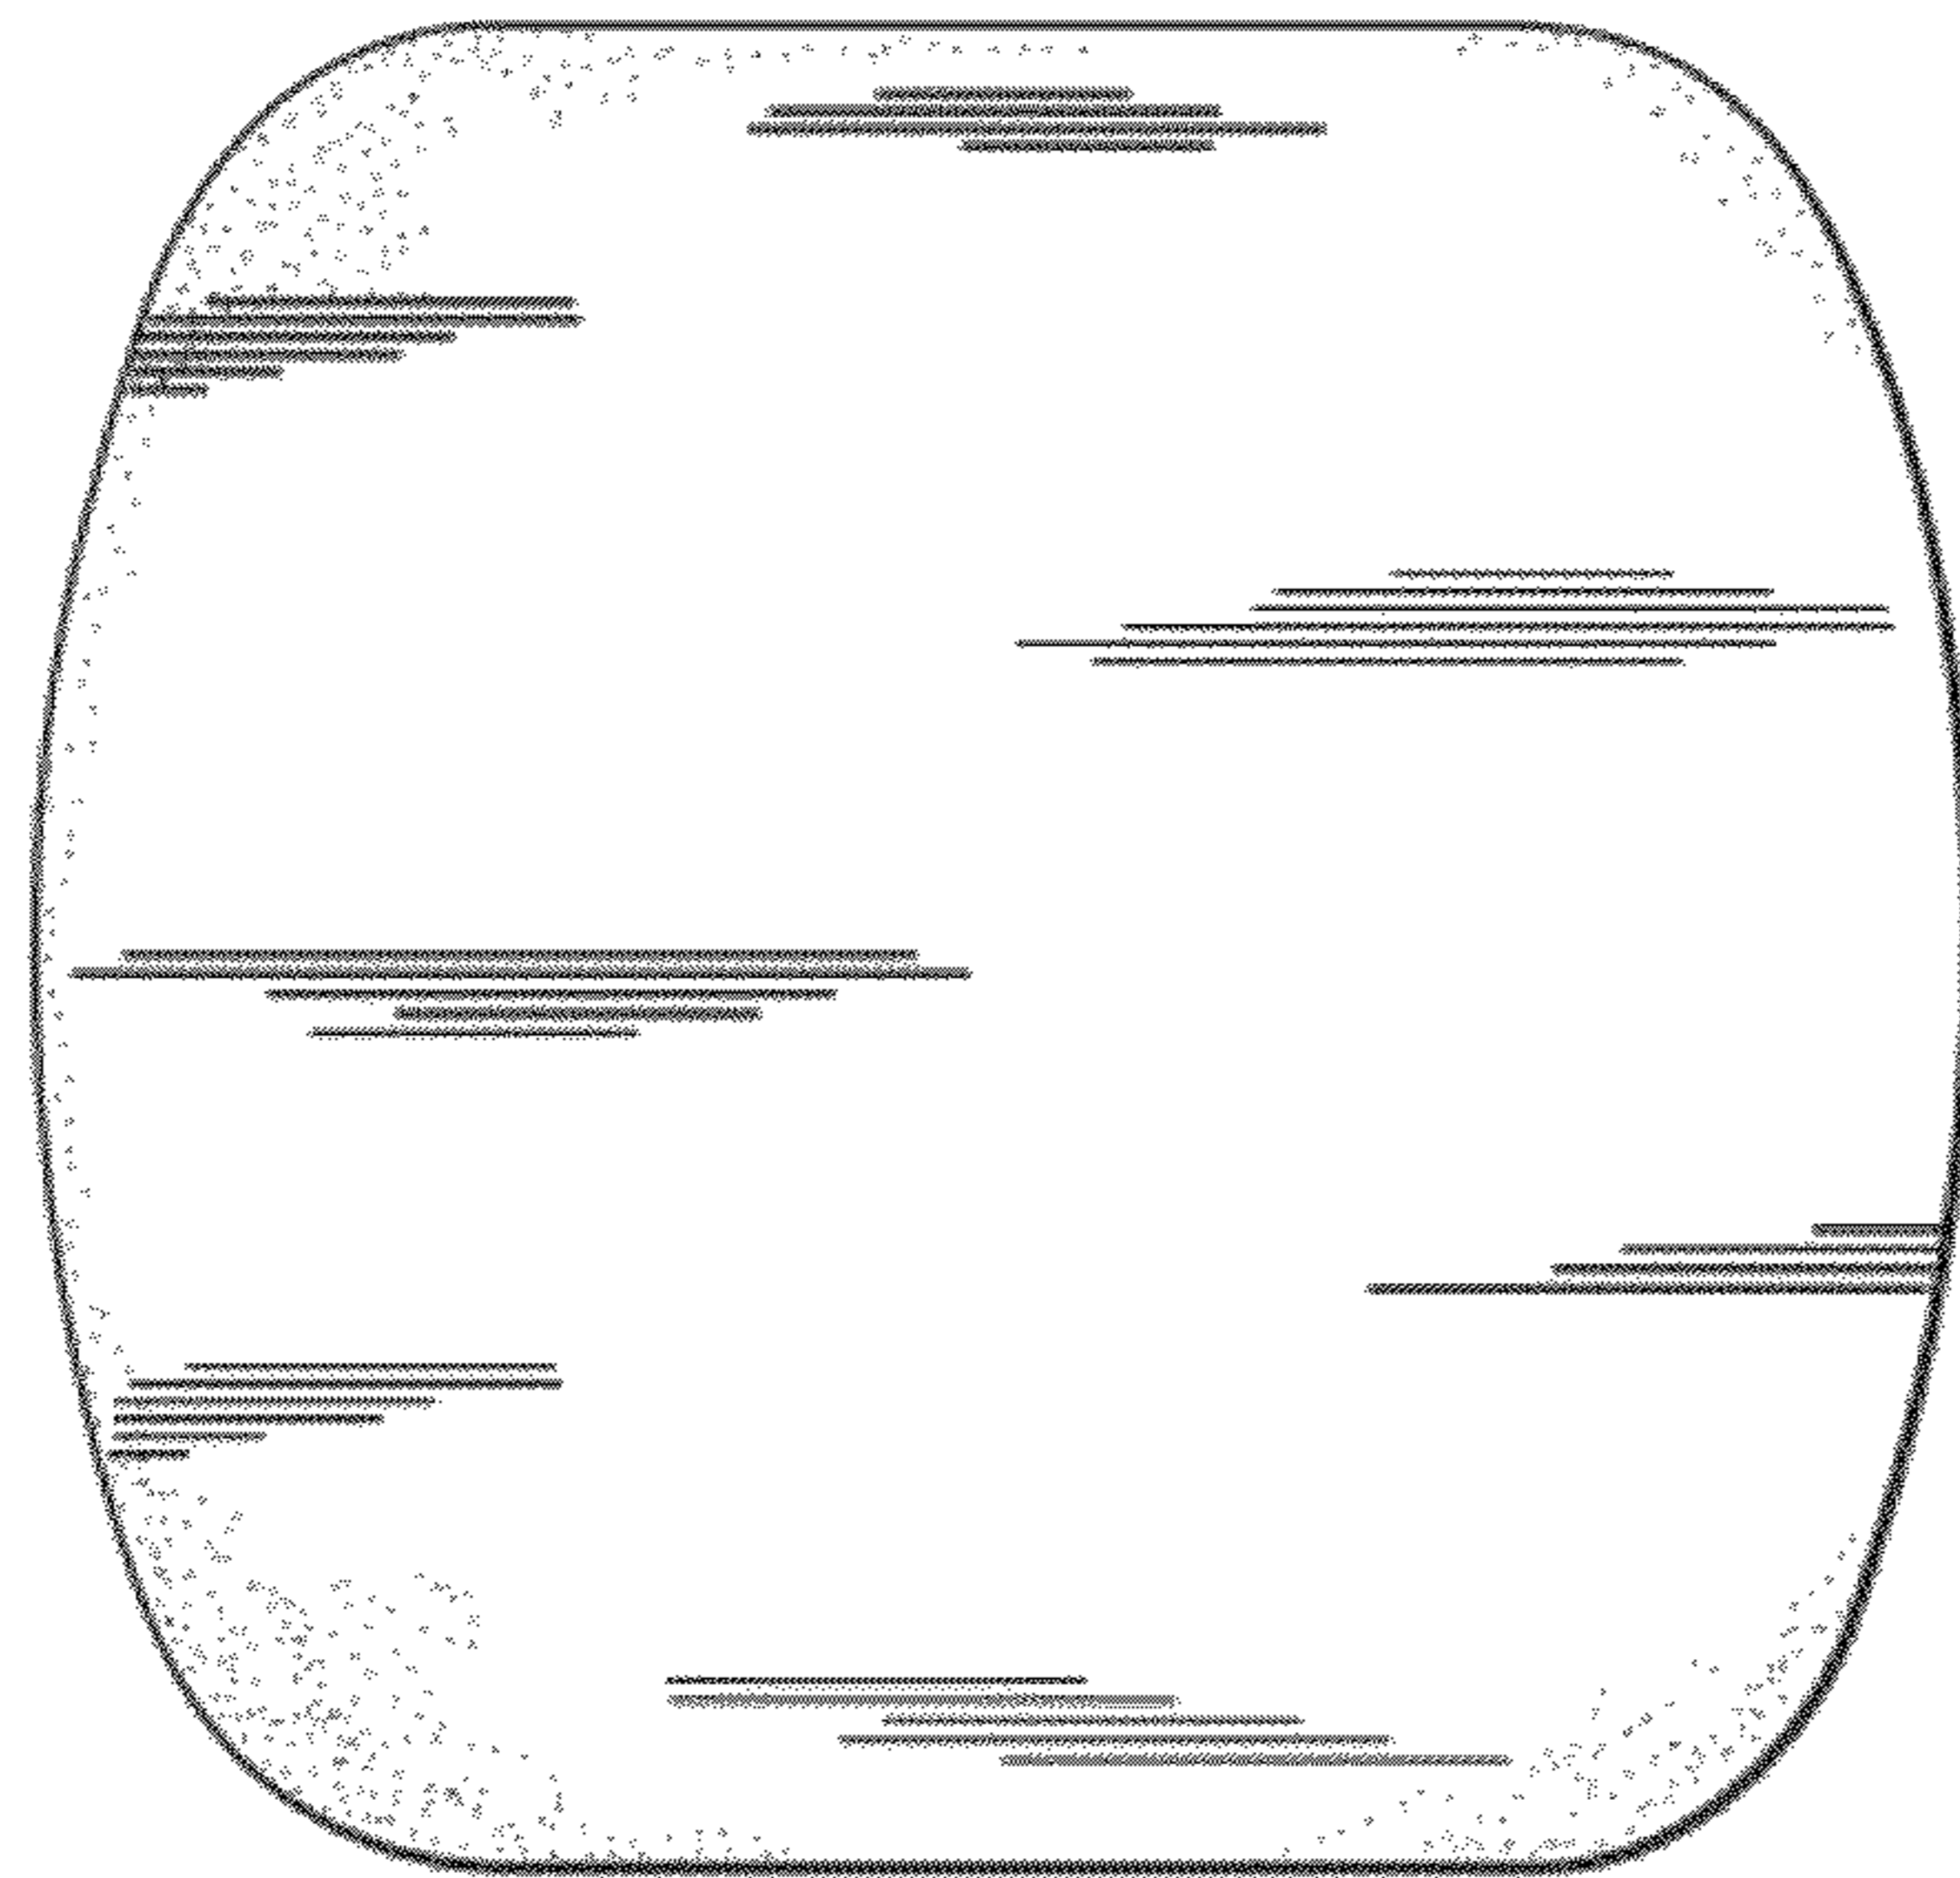


Fig. 17

Fig. 18

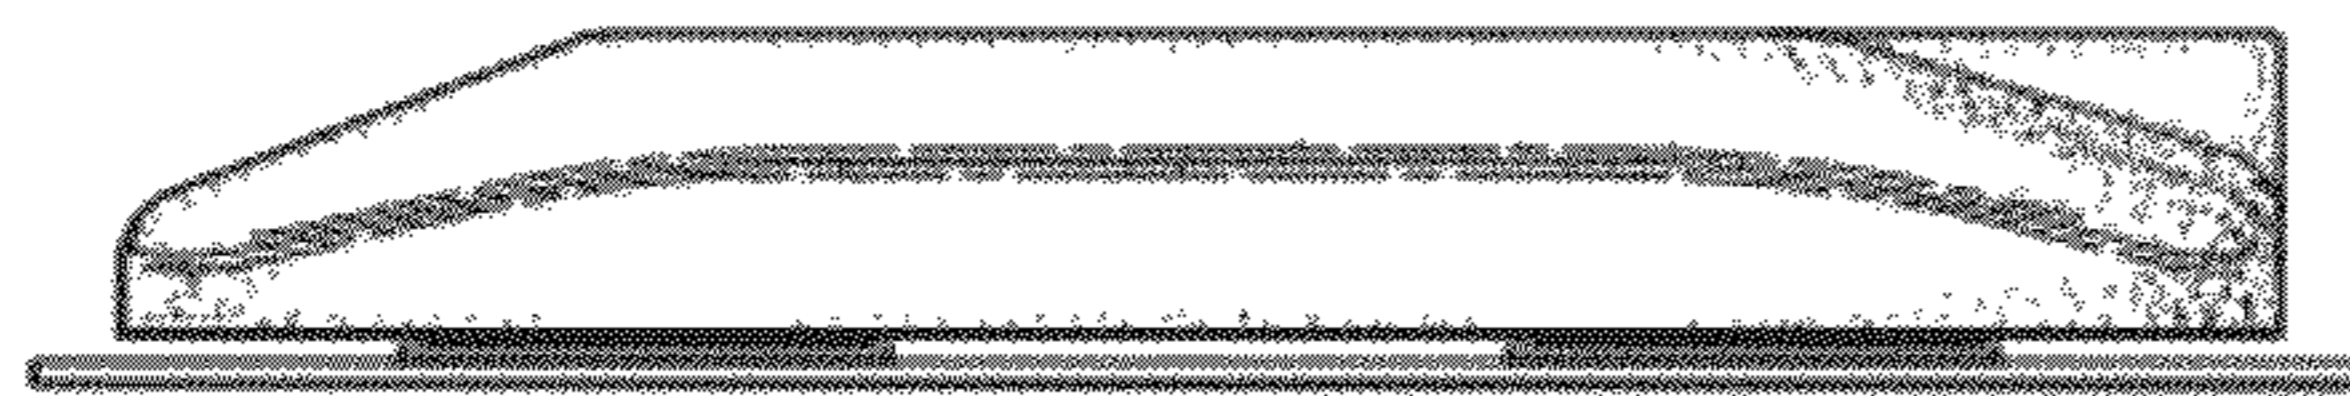
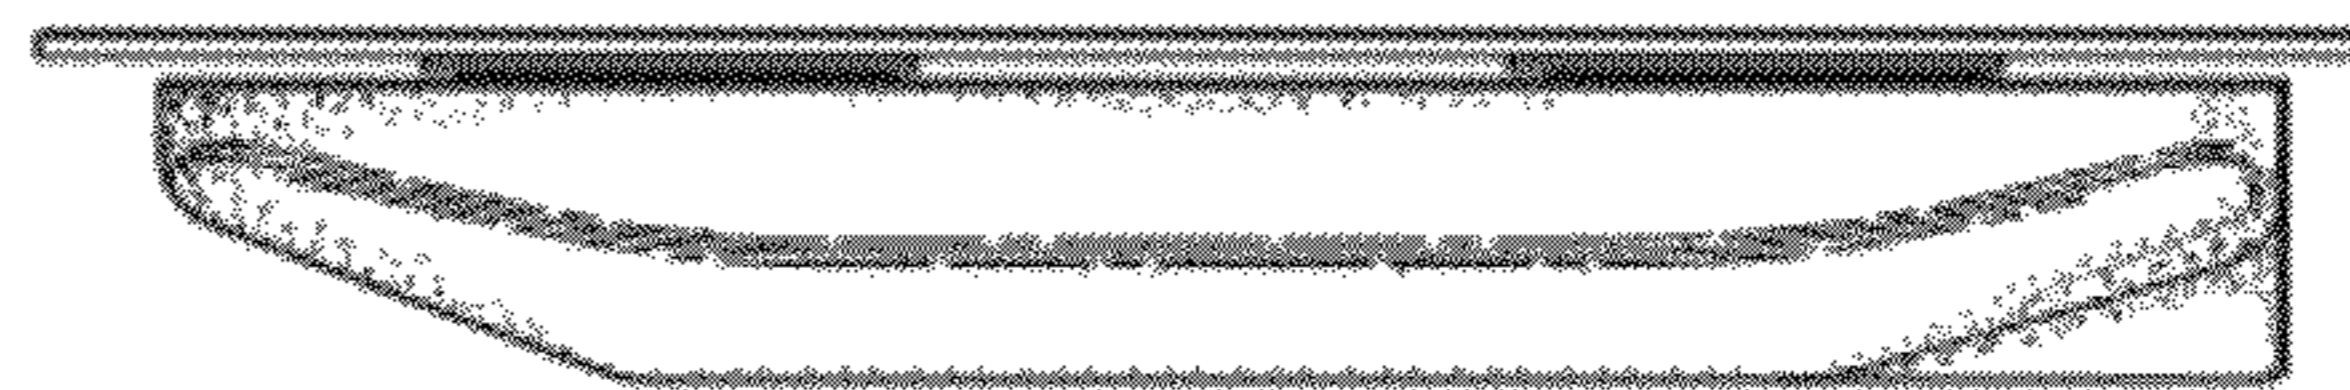


Fig. 19

Fig. 20

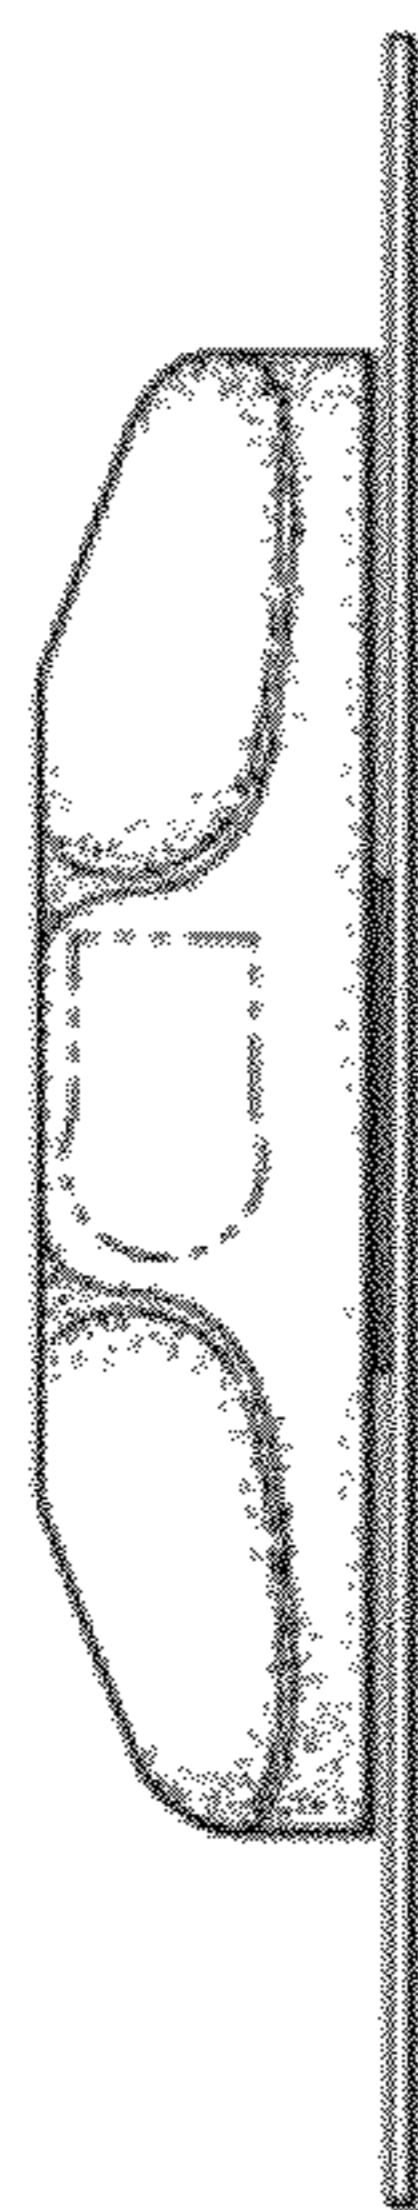


Fig. 21

