



US00D666712S

(12) **United States Design Patent**
Laurence

(10) **Patent No.:** **US D666,712 S**
(45) **Date of Patent:** **** Sep. 4, 2012**

(54) **SINGLE USE SUCTION CATHETER WITH
COLOR-KEYED SUCTION DEPTH
INDICATORS**

(76) Inventor: **William Andrew Laurence**, Richardson,
TX (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/378,884**

(22) Filed: **Nov. 10, 2010**

Related U.S. Application Data

(63) Continuation-in-part of application No. 29/327,757,
filed on Nov. 12, 2008, now Pat. No. Des. 629,515.

(51) **LOC (9) Cl.** **24-02**

(52) **U.S. Cl.** **D24/130**

(58) **Field of Classification Search** D24/115,
D24/127-131, 133; 128/207.14-207.18,
128/200.26, DIG. 26, 200.24, 205.23; 600/28,
600/45, 93.01, 19, 23, 96.01, 100.01; 116/280,
116/307, 308, 311-315, 318, 319
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,623,924 A * 4/1997 Lindenman et al. 128/207.17
5,765,559 A * 6/1998 Kim 128/207.15
D398,989 S 9/1998 Ashlin
5,873,362 A * 2/1999 Parker 128/207.14
6,609,521 B1 8/2003 Belani et al.
6,668,832 B2 12/2003 Hipolito et al.
6,889,693 B2 5/2005 Hipolito et al.

6,978,784 B2 12/2005 Pekar
7,328,701 B2 2/2008 Green
D605,758 S 12/2009 Schwartz et al.
D629,515 S * 12/2010 Laurence D24/130
2004/0084051 A1 5/2004 Hipolito et al.
2006/0225741 A1 10/2006 Rothman

* cited by examiner

Primary Examiner — Eric Goodman

(74) *Attorney, Agent, or Firm* — QuickPatents, Inc.; Kevin
Prince

(57) **CLAIM**

What is claimed is the ornamental design for a single use
suction catheter with color-keyed suction depth
indicators, as
shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a single use suction catheter
with color-keyed suction depth indicators, showing my new
design;

FIG. 2 is a front elevational view thereof;

FIG. 3 is a rear elevational view thereof;

FIG. 4 is a right-side elevational view thereof;


FIG. 5 is a left-side elevational view thereof;

FIG. 6 is a bottom plan view thereof; and,

FIG. 7 is a top plan view thereof.

The broken lines showing a finger tip control connector in
FIGS. 1-7 are environmental matter, and form no part of the
claimed design. Portions of the catheter with color-keyed
suction depth indicators have been lined to represent color.

1 Claim, 4 Drawing Sheets

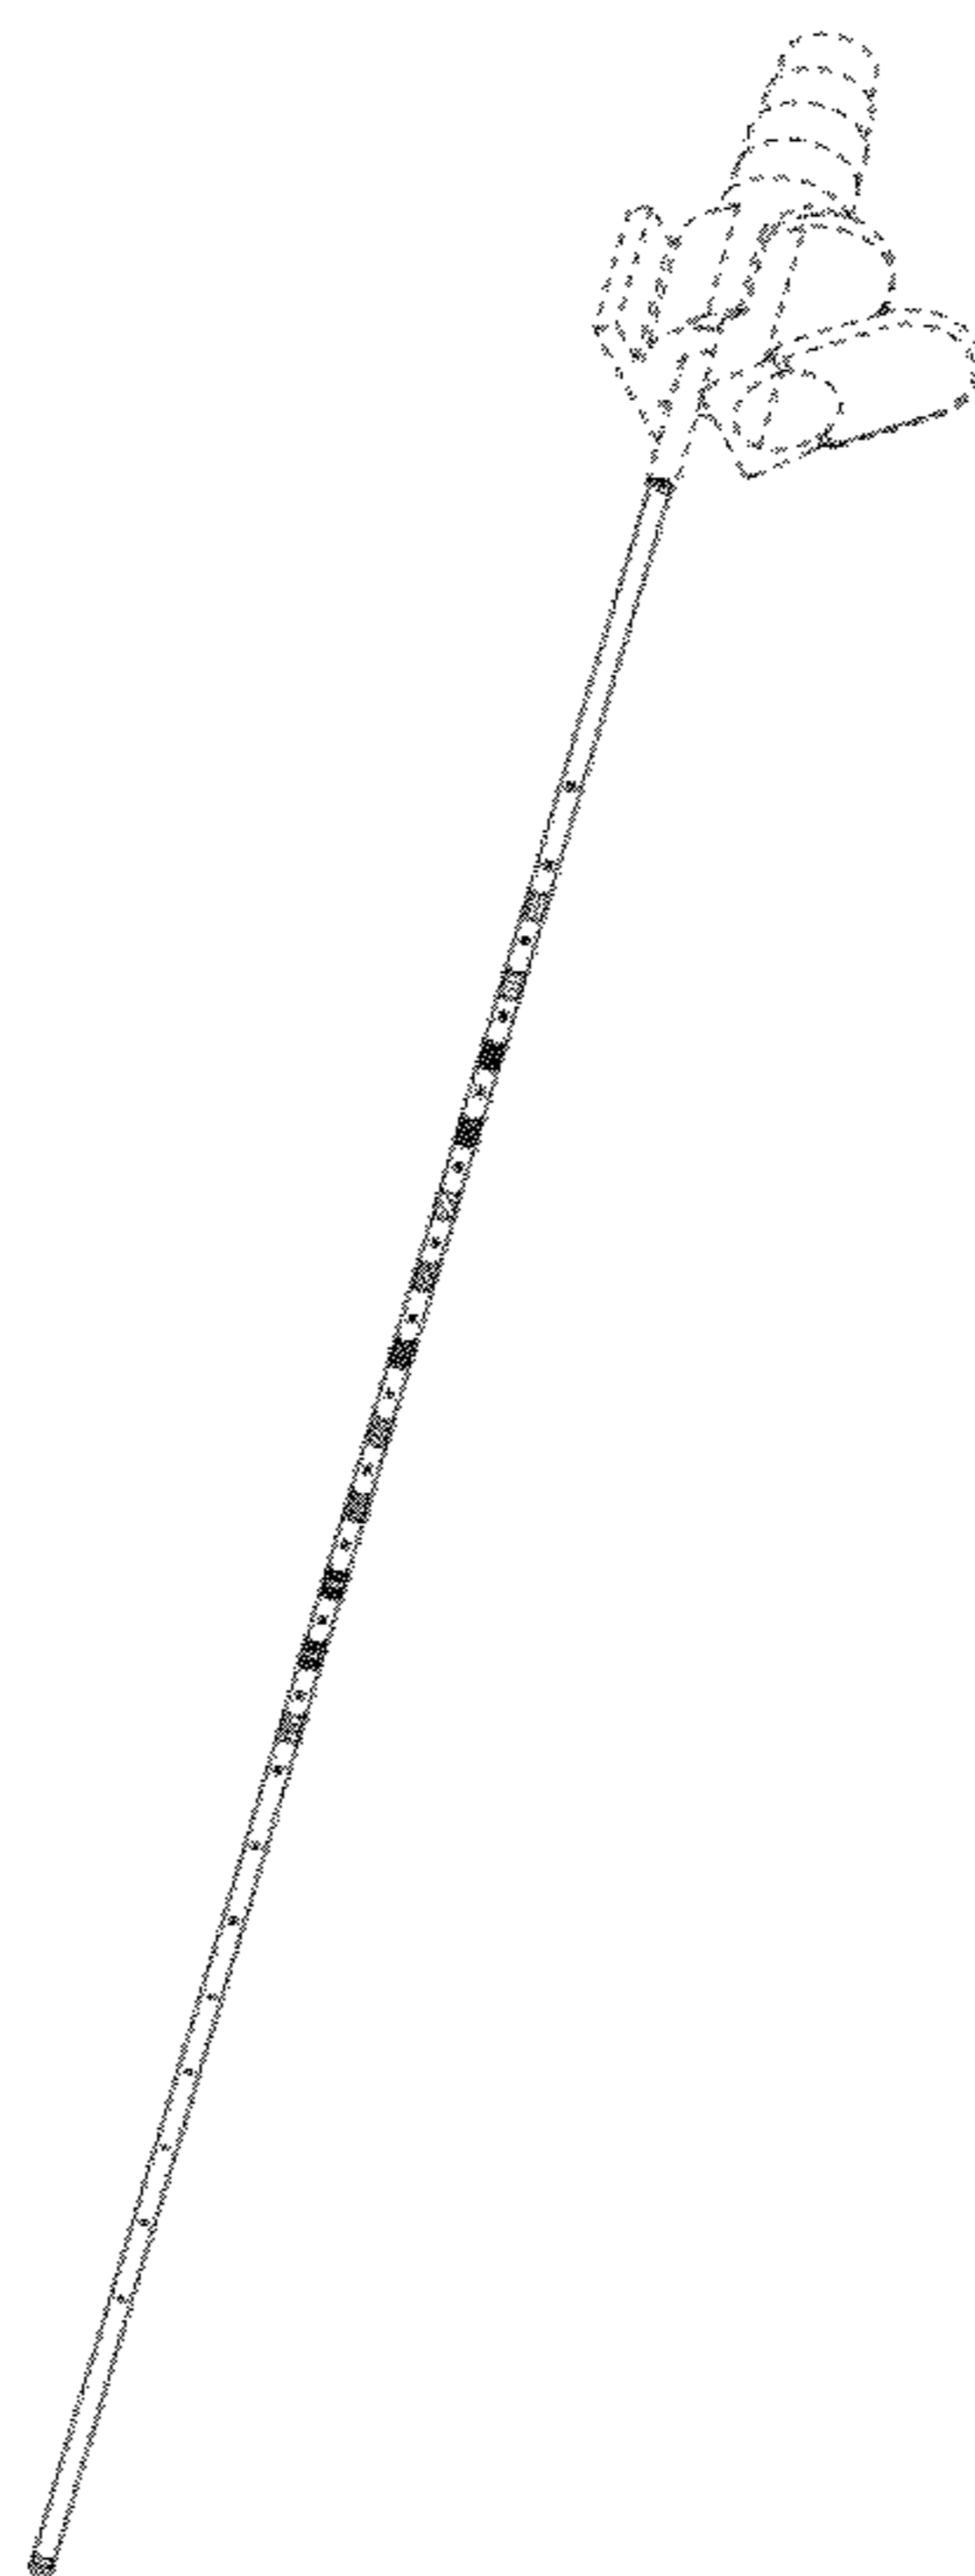

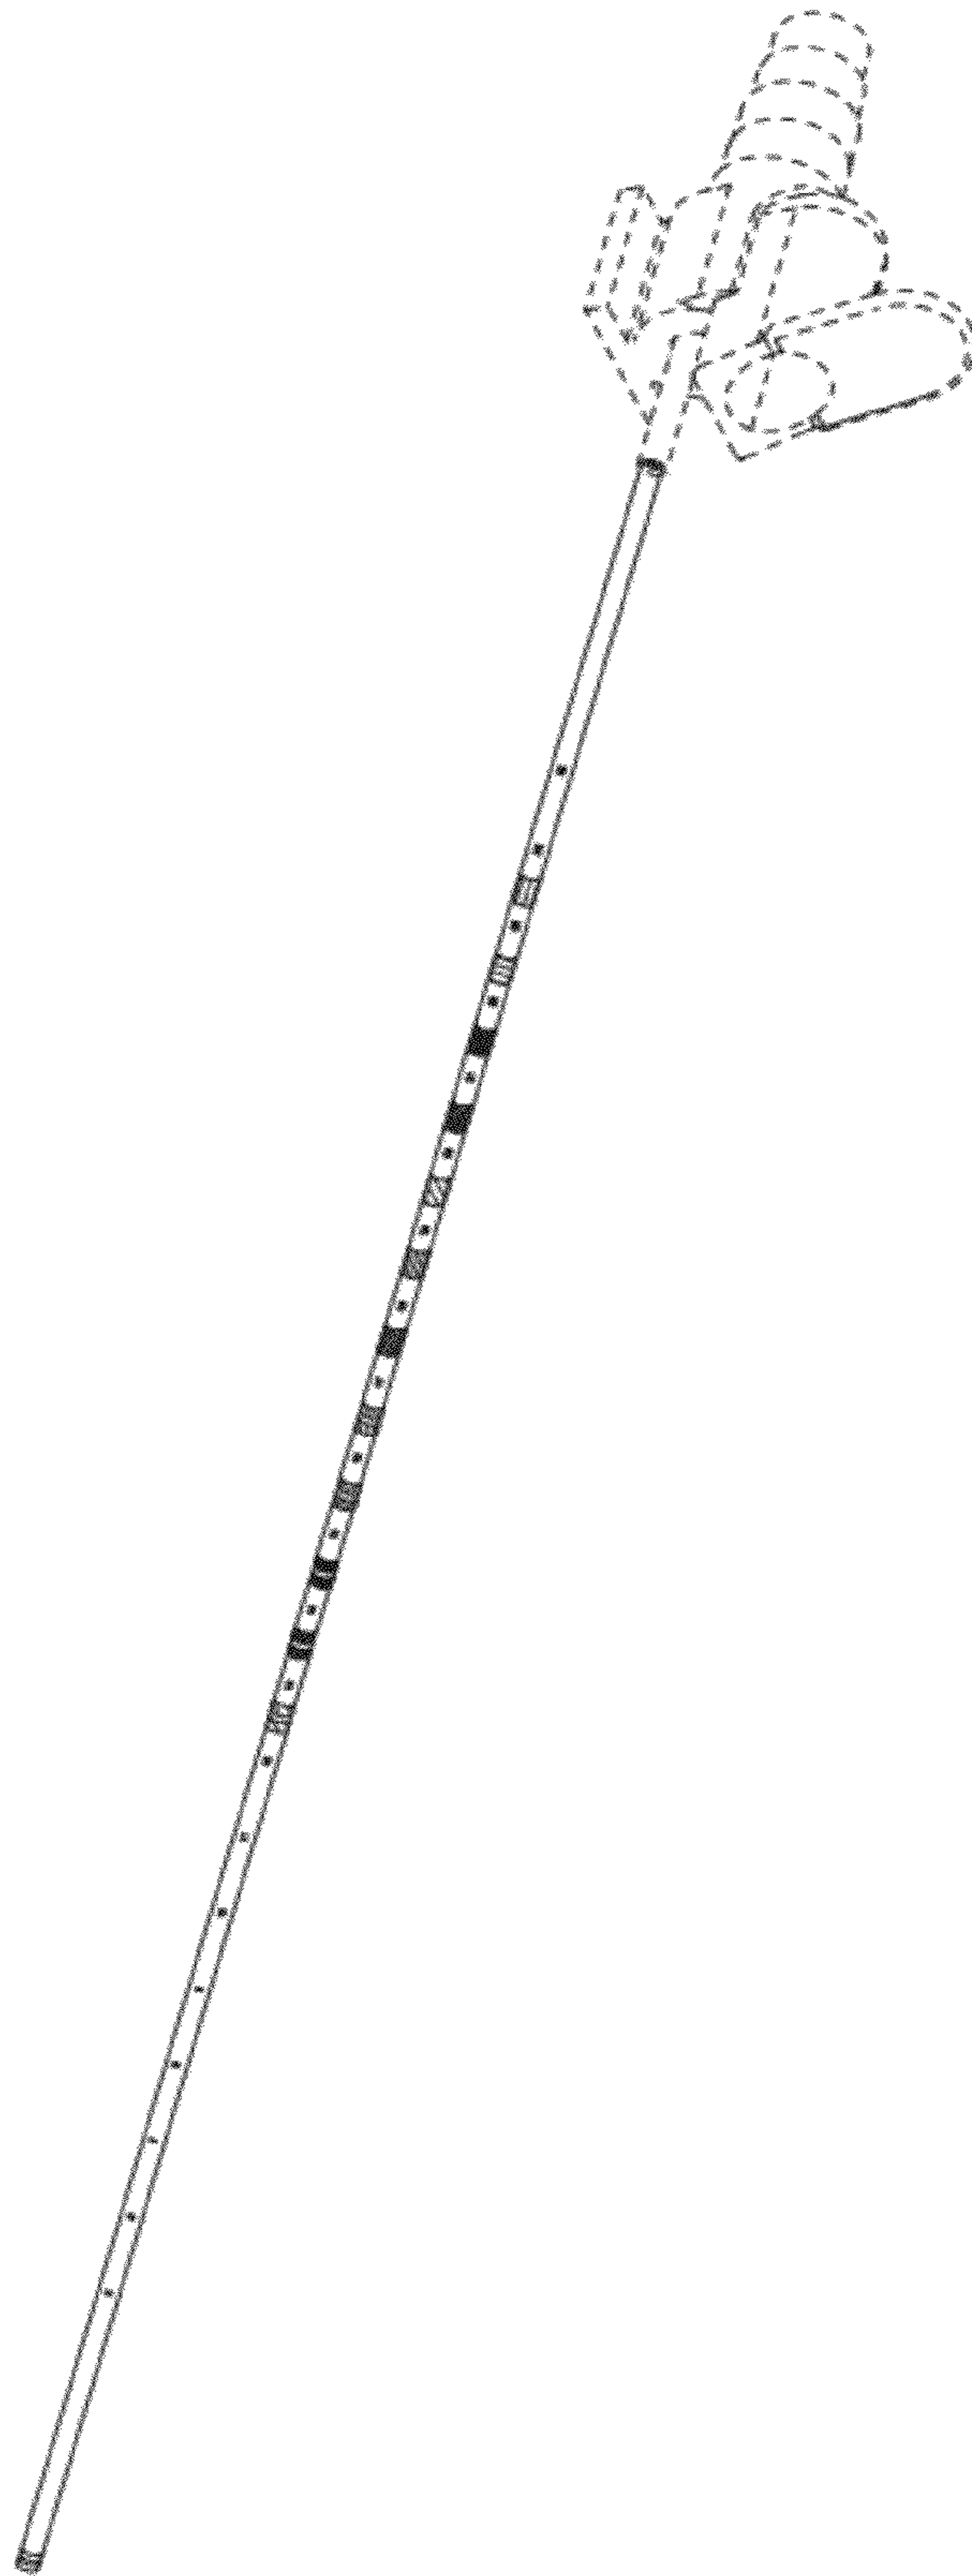


FIG. 1

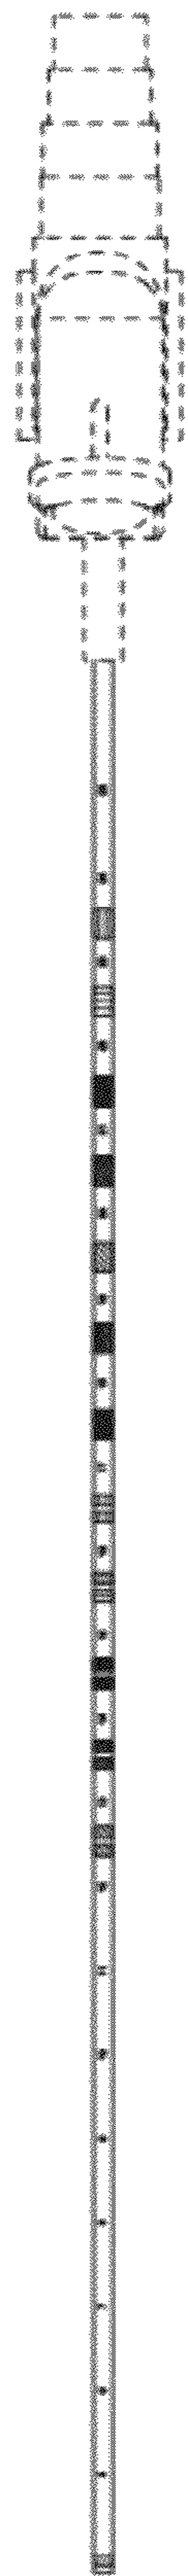


FIG. 2

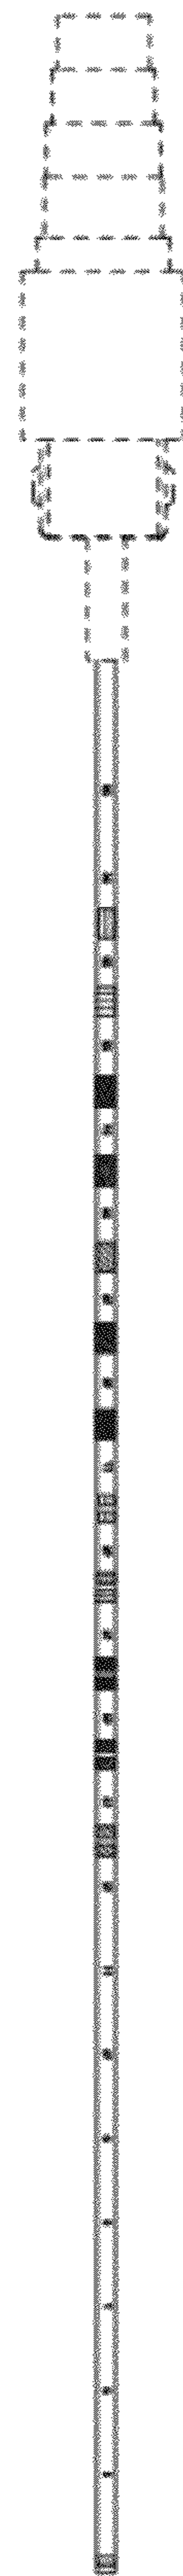


FIG. 3

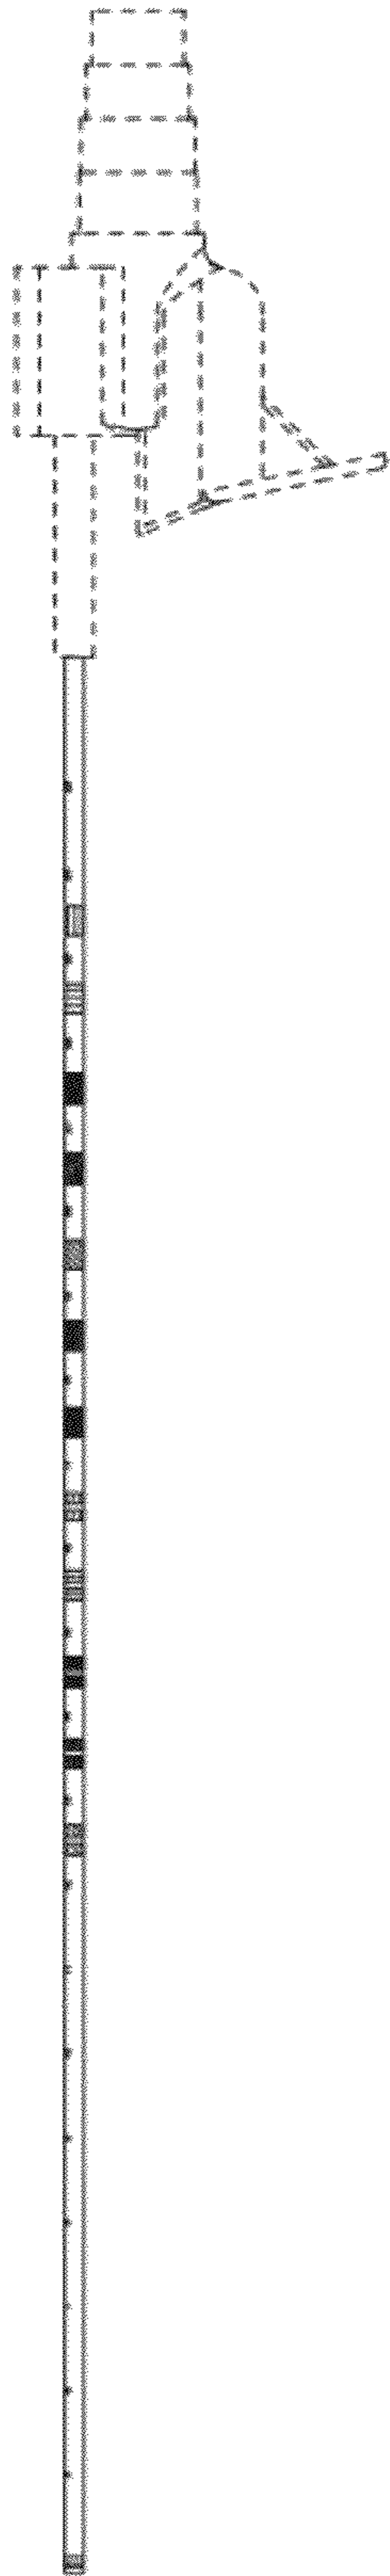


FIG. 4

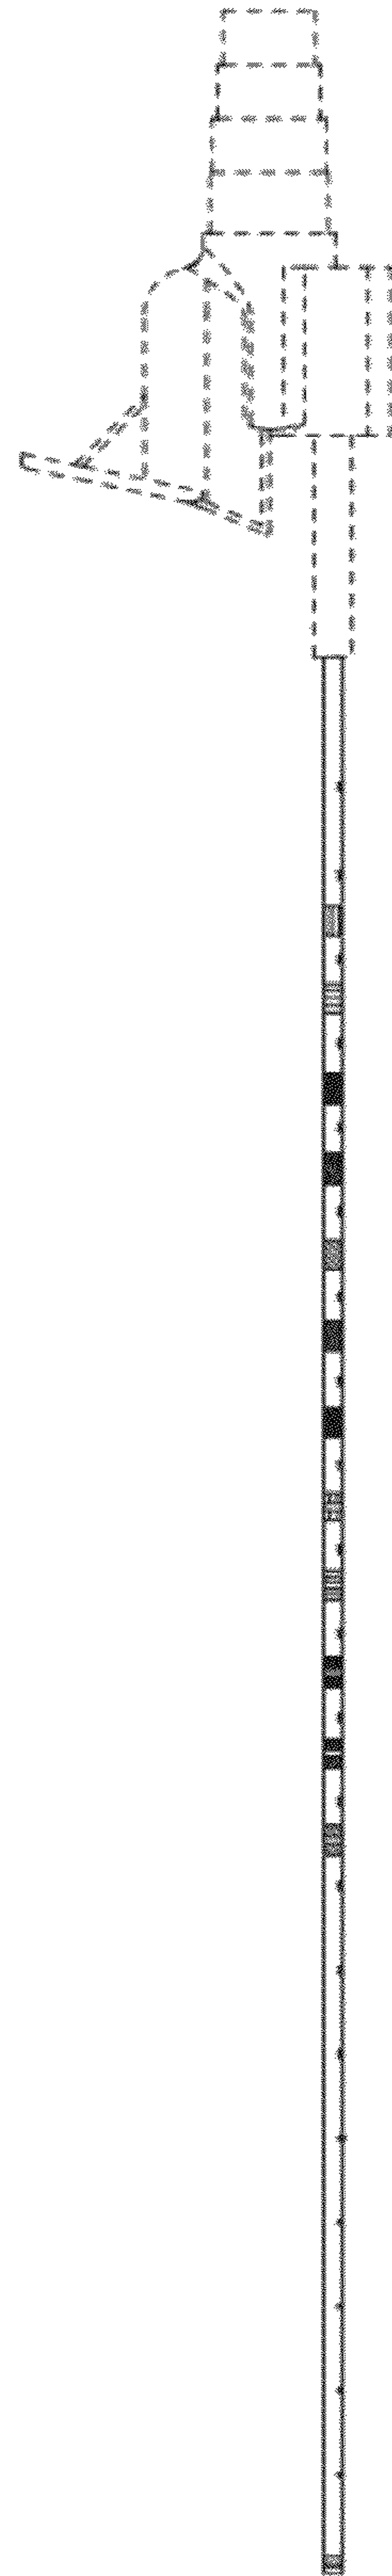


FIG. 5

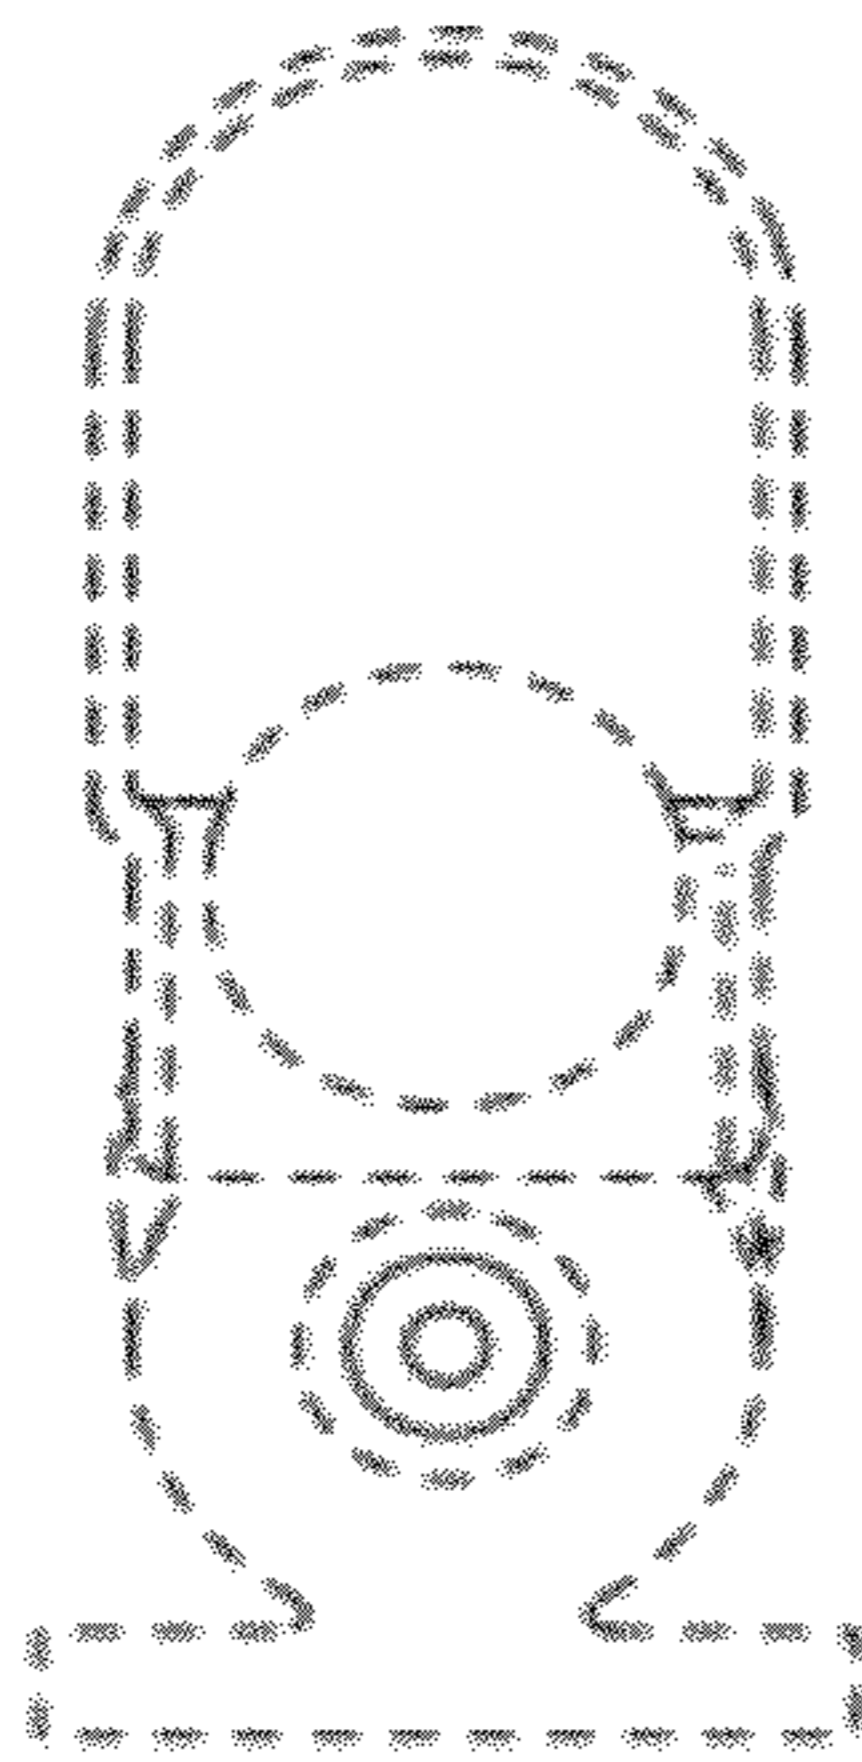


FIG. 6

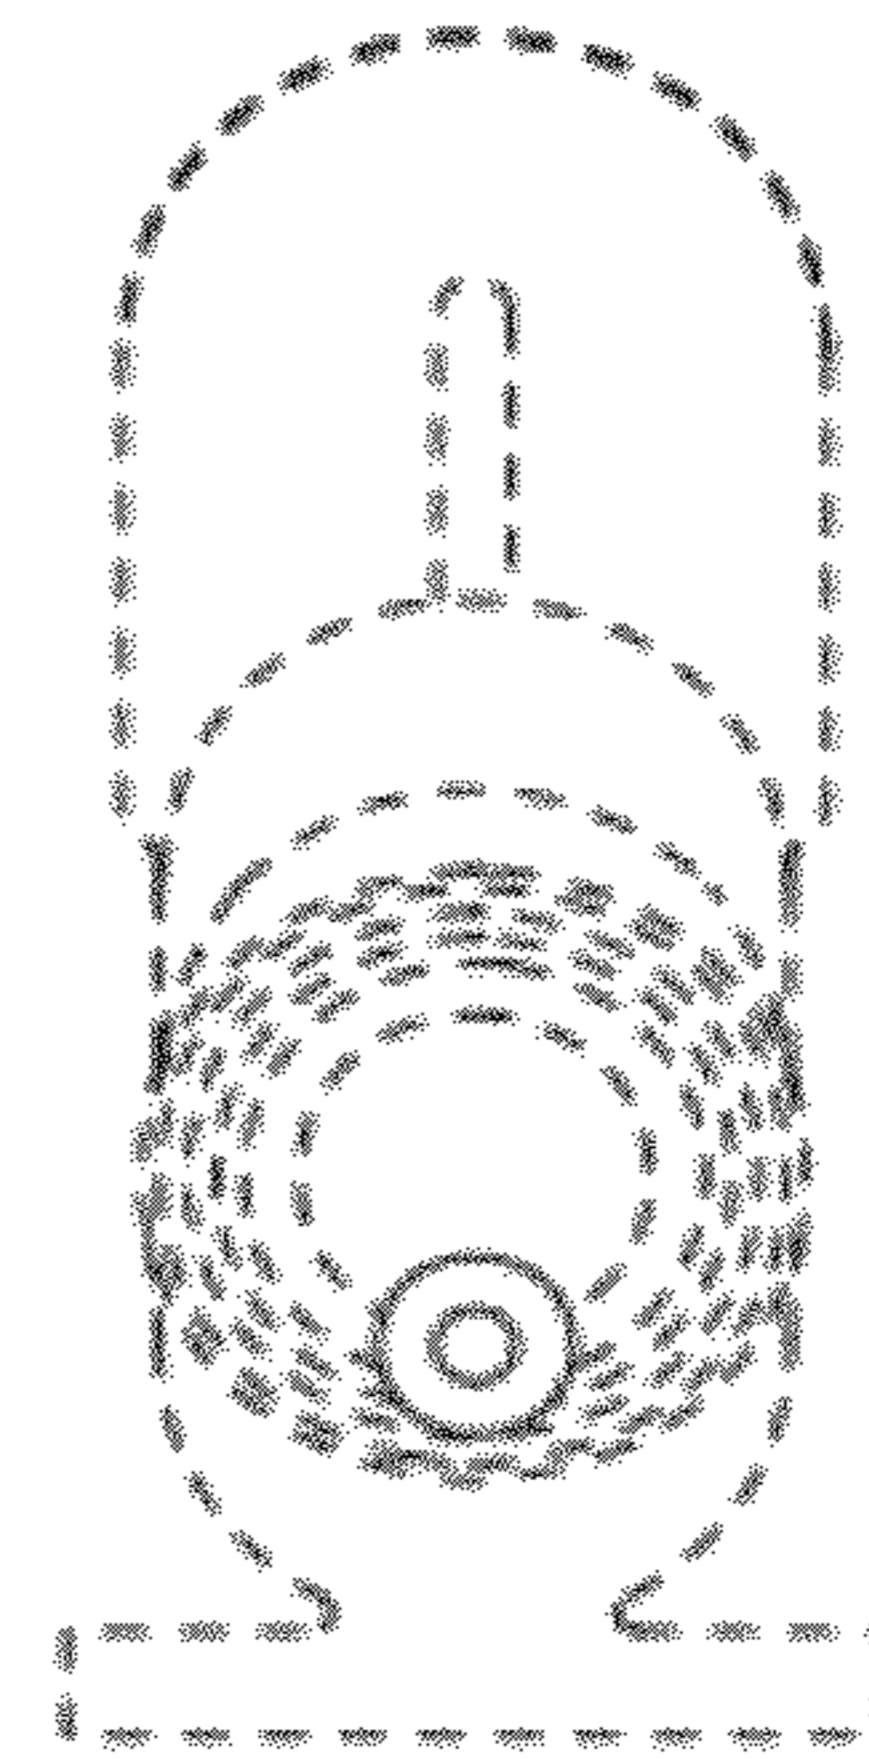


FIG. 7