

US00D666727S

(12) **United States Design Patent**  
**Held**

(10) **Patent No.:** **US D666,727 S**

(45) **Date of Patent:** **\*\* Sep. 4, 2012**

(54) **INDICATING COMMUNICATION AND CONTROL PANEL FOR A MEDICAL OPERATING ROOM**

(75) Inventor: **Manfred Held**, Hamburg (DE)

(73) Assignee: **Olympus Winter & IBE GmbH**, Hamburg (DE)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/342,871**

(22) Filed: **Sep. 2, 2009**

(30) **Foreign Application Priority Data**

Mar. 6, 2009 (EM) ..... 001101034-0001  
Mar. 6, 2009 (EM) ..... 001101034-0002  
Mar. 6, 2009 (EM) ..... 001101034-0003

(51) **LOC (9) Cl.** ..... **24-01**

(52) **U.S. Cl.** ..... **D24/186**

(58) **Field of Classification Search** ..... D24/107,  
D24/111, 127, 138, 158, 160, 169, 231-232,  
D24/185; D10/40, 81, 102-103, 104.1, 106.95;  
D13/162-164, 177; D14/159, 257, 443;  
D15/146; 600/300, 301, 368, 372, 481, 529,  
600/544, 554, 561; 200/5 A, 5 R; 361/622,  
361/627

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D275,851 S \* 10/1984 Bambeck ..... D13/164  
D286,435 S \* 10/1986 Atkinson ..... D24/127  
D287,005 S \* 12/1986 Newton ..... D13/162  
D287,228 S \* 12/1986 Newton ..... D10/81  
D299,953 S \* 2/1989 King et al. .... D24/169  
D323,488 S \* 1/1992 Darnell et al. .... D13/162  
D324,104 S \* 2/1992 Cecil et al. .... D24/158  
D332,100 S \* 12/1992 Blattner et al. .... D14/257

D334,062 S \* 3/1993 Davis et al. .... D24/160  
D334,542 S \* 4/1993 Lowe et al. .... D10/104.1  
D342,683 S \* 12/1993 Cohen ..... D13/164  
D354,747 S \* 1/1995 Herbstritt et al. .... D14/443  
D355,717 S \* 2/1995 Murakami et al. .... D24/158  
D356,792 S \* 3/1995 Murakami et al. .... D24/158  
D364,107 S \* 11/1995 Nesicolaci ..... D10/103  
D394,435 S \* 5/1998 Parsadayan et al. .... D14/159  
D404,391 S \* 1/1999 Herbstritt et al. .... D13/162  
D412,208 S \* 7/1999 Nelson et al. .... D24/158  
D515,514 S \* 2/2006 Butler et al. .... D13/164  
D523,146 S \* 6/2006 Ogiwara ..... D24/158  
D529,871 S \* 10/2006 Butler et al. .... D13/164  
D546,770 S \* 7/2007 Herbstritt ..... D13/162  
D590,352 S \* 4/2009 Jacoby et al. .... D13/164

(Continued)

*Primary Examiner* — T. Chase Nelson

*Assistant Examiner* — Mark Cavanna

(74) *Attorney, Agent, or Firm* — Rankin, Hill & Clark LLP

(57) **CLAIM**

I claim the ornamental design for an indicating communication and control panel for a medical operating room, as shown and described.

**DESCRIPTION**


FIG. 1 is a front perspective view of an indicating communication and control panel for a medical operating room showing my new design;

FIG. 2 is a front view thereof;

FIG. 3 is a top view of the panel shown in FIG. 1, with the bottom view being a mirror image of the top view; and, FIG. 4 is a left side view of the panel shown in FIG. 1, with the right side view being a mirror image of the left side view.

The broken lines in the drawings show environmental structure that forms no part of the claimed design. Portions of the drawings have been lined for color. The push button has been lined for the color red and a horizontal stripe at the top of the design has been lined for the color BLUE.

**1 Claim, 2 Drawing Sheets**

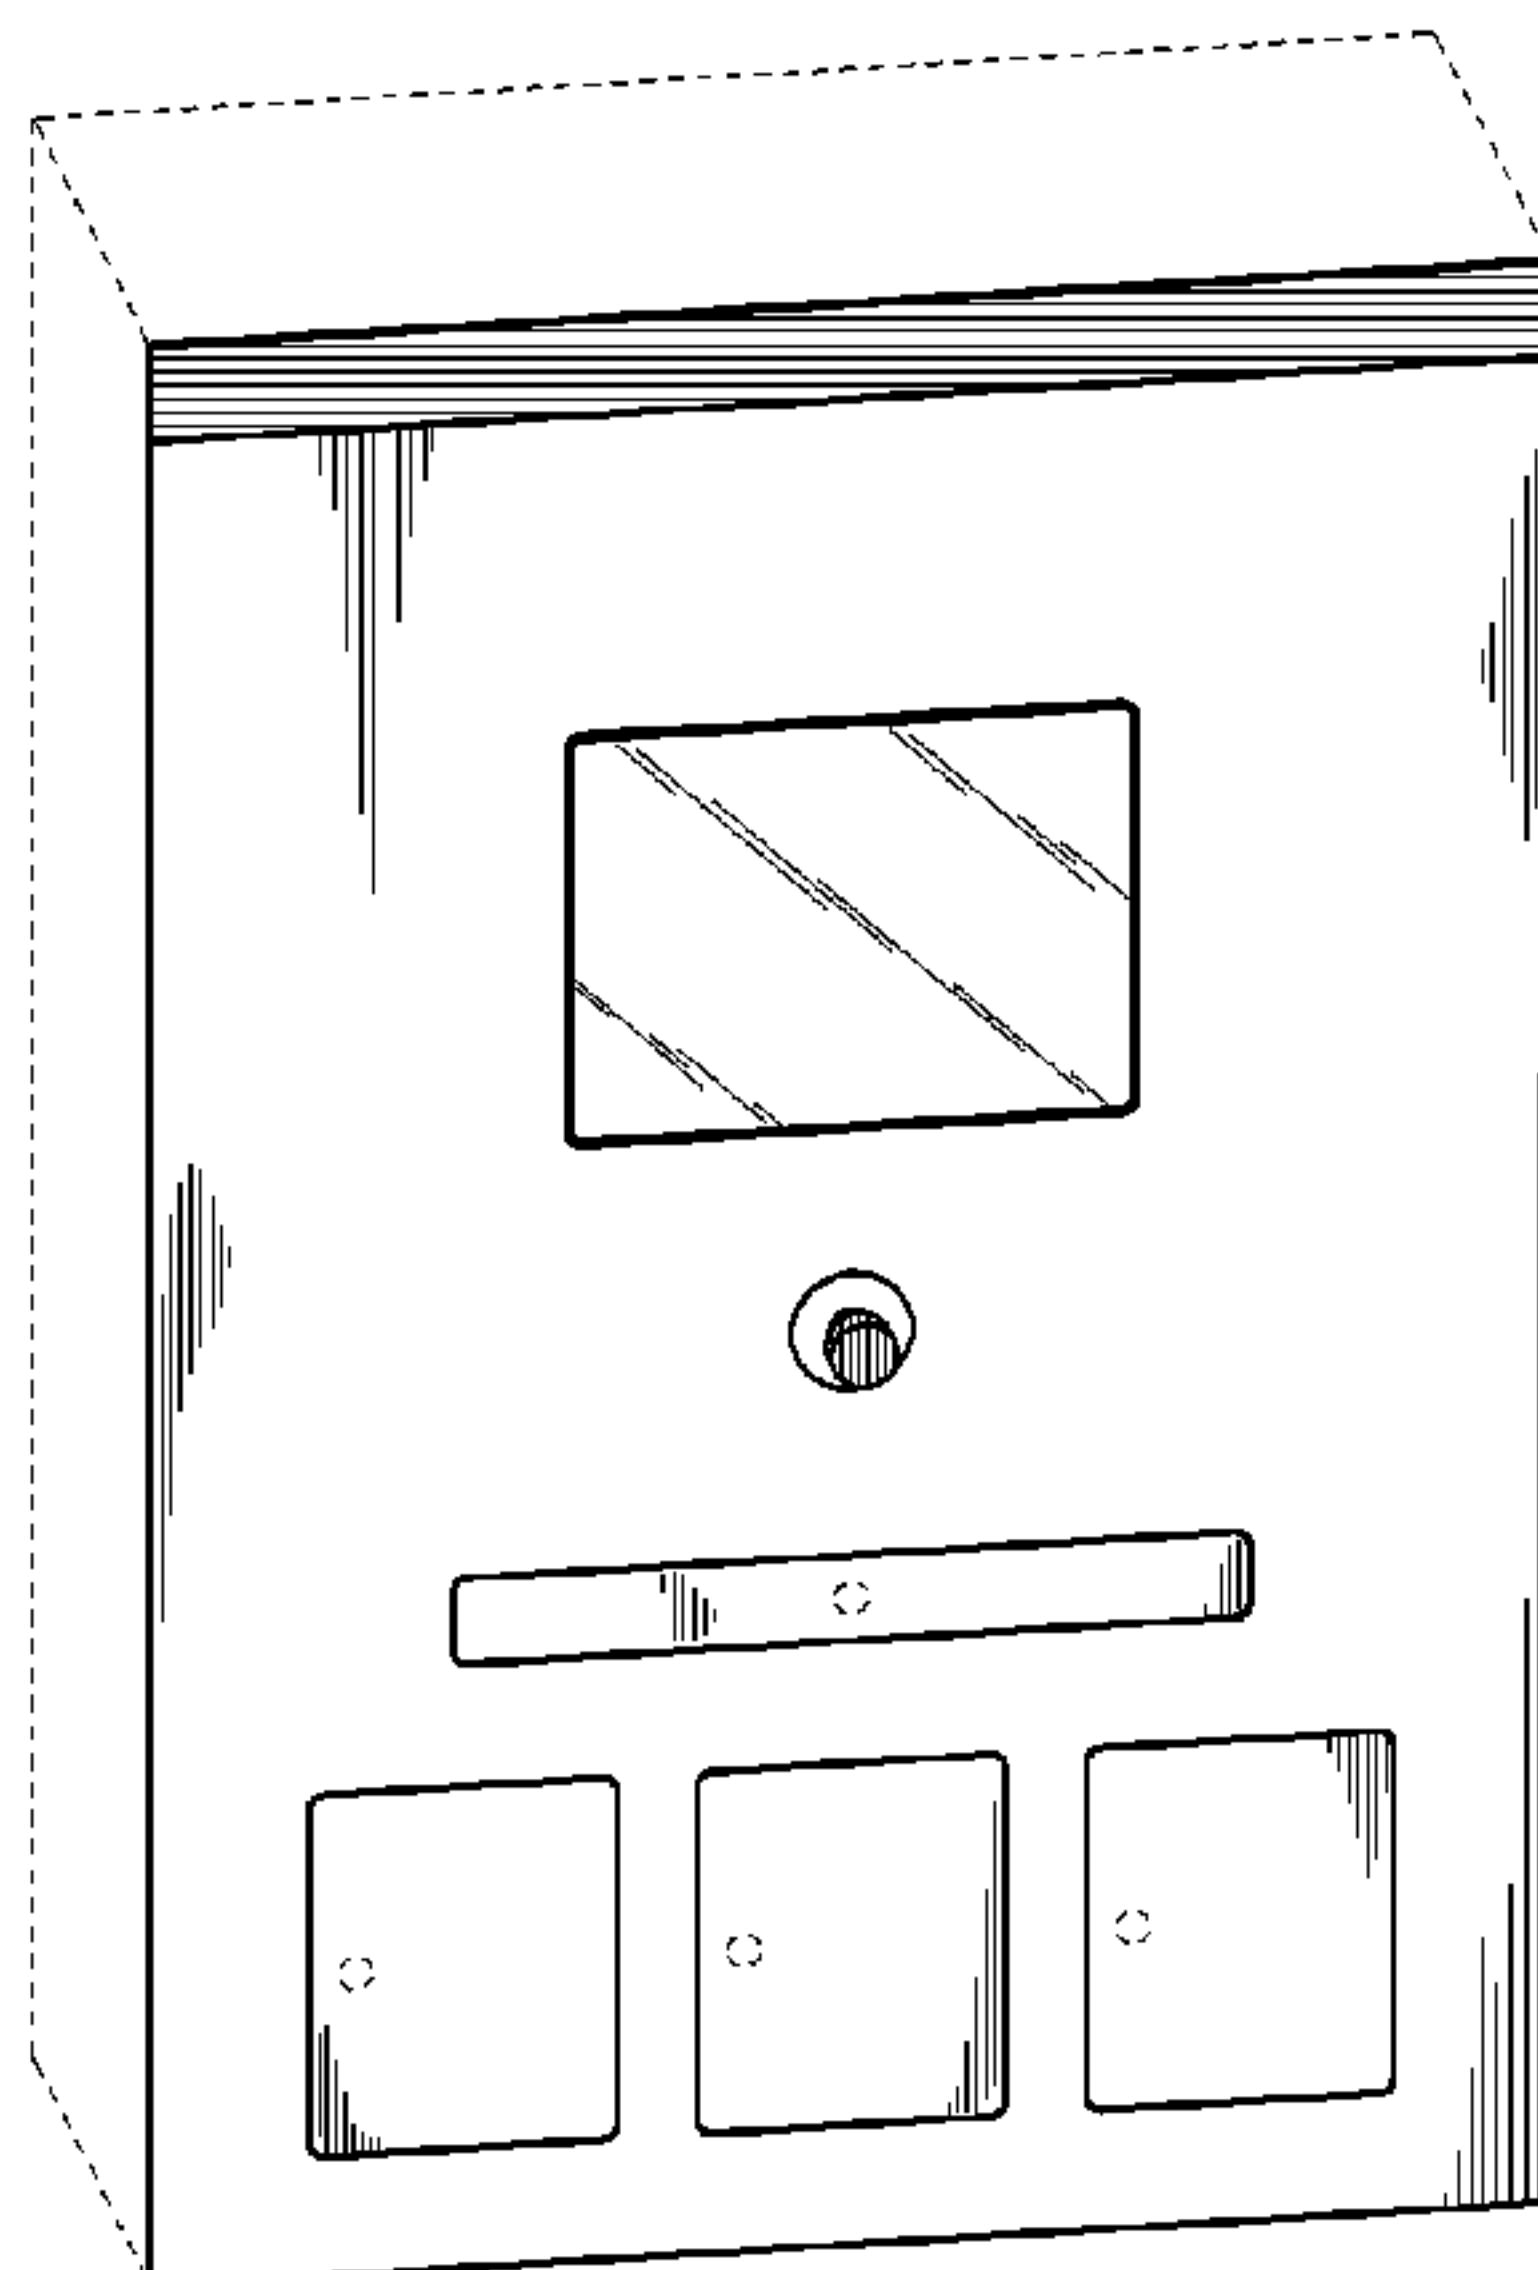

# US D666,727 S

Page 2

---

## U.S. PATENT DOCUMENTS

D601,514 S *	10/2009	Lin	.....	D13/177	D633,117 S *	2/2011	de la Hamayde	.....	D15/146
D604,845 S *	11/2009	Hibi et al.	.....	D24/138	D635,101 S *	3/2011	Farrow	.....	D13/162
D608,302 S *	1/2010	Liu	.....	D13/164	D639,753 S *	6/2011	Saari	.....	D13/177
D630,115 S *	1/2011	Mizukami	.....	D10/106.95	D643,377 S *	8/2011	Brennan, Iii et al.	.....	D13/164
D630,537 S *	1/2011	Mizukami	.....	D10/106.95	D645,570 S *	9/2011	Oonuma et al.	.....	D24/232

\* cited by examiner

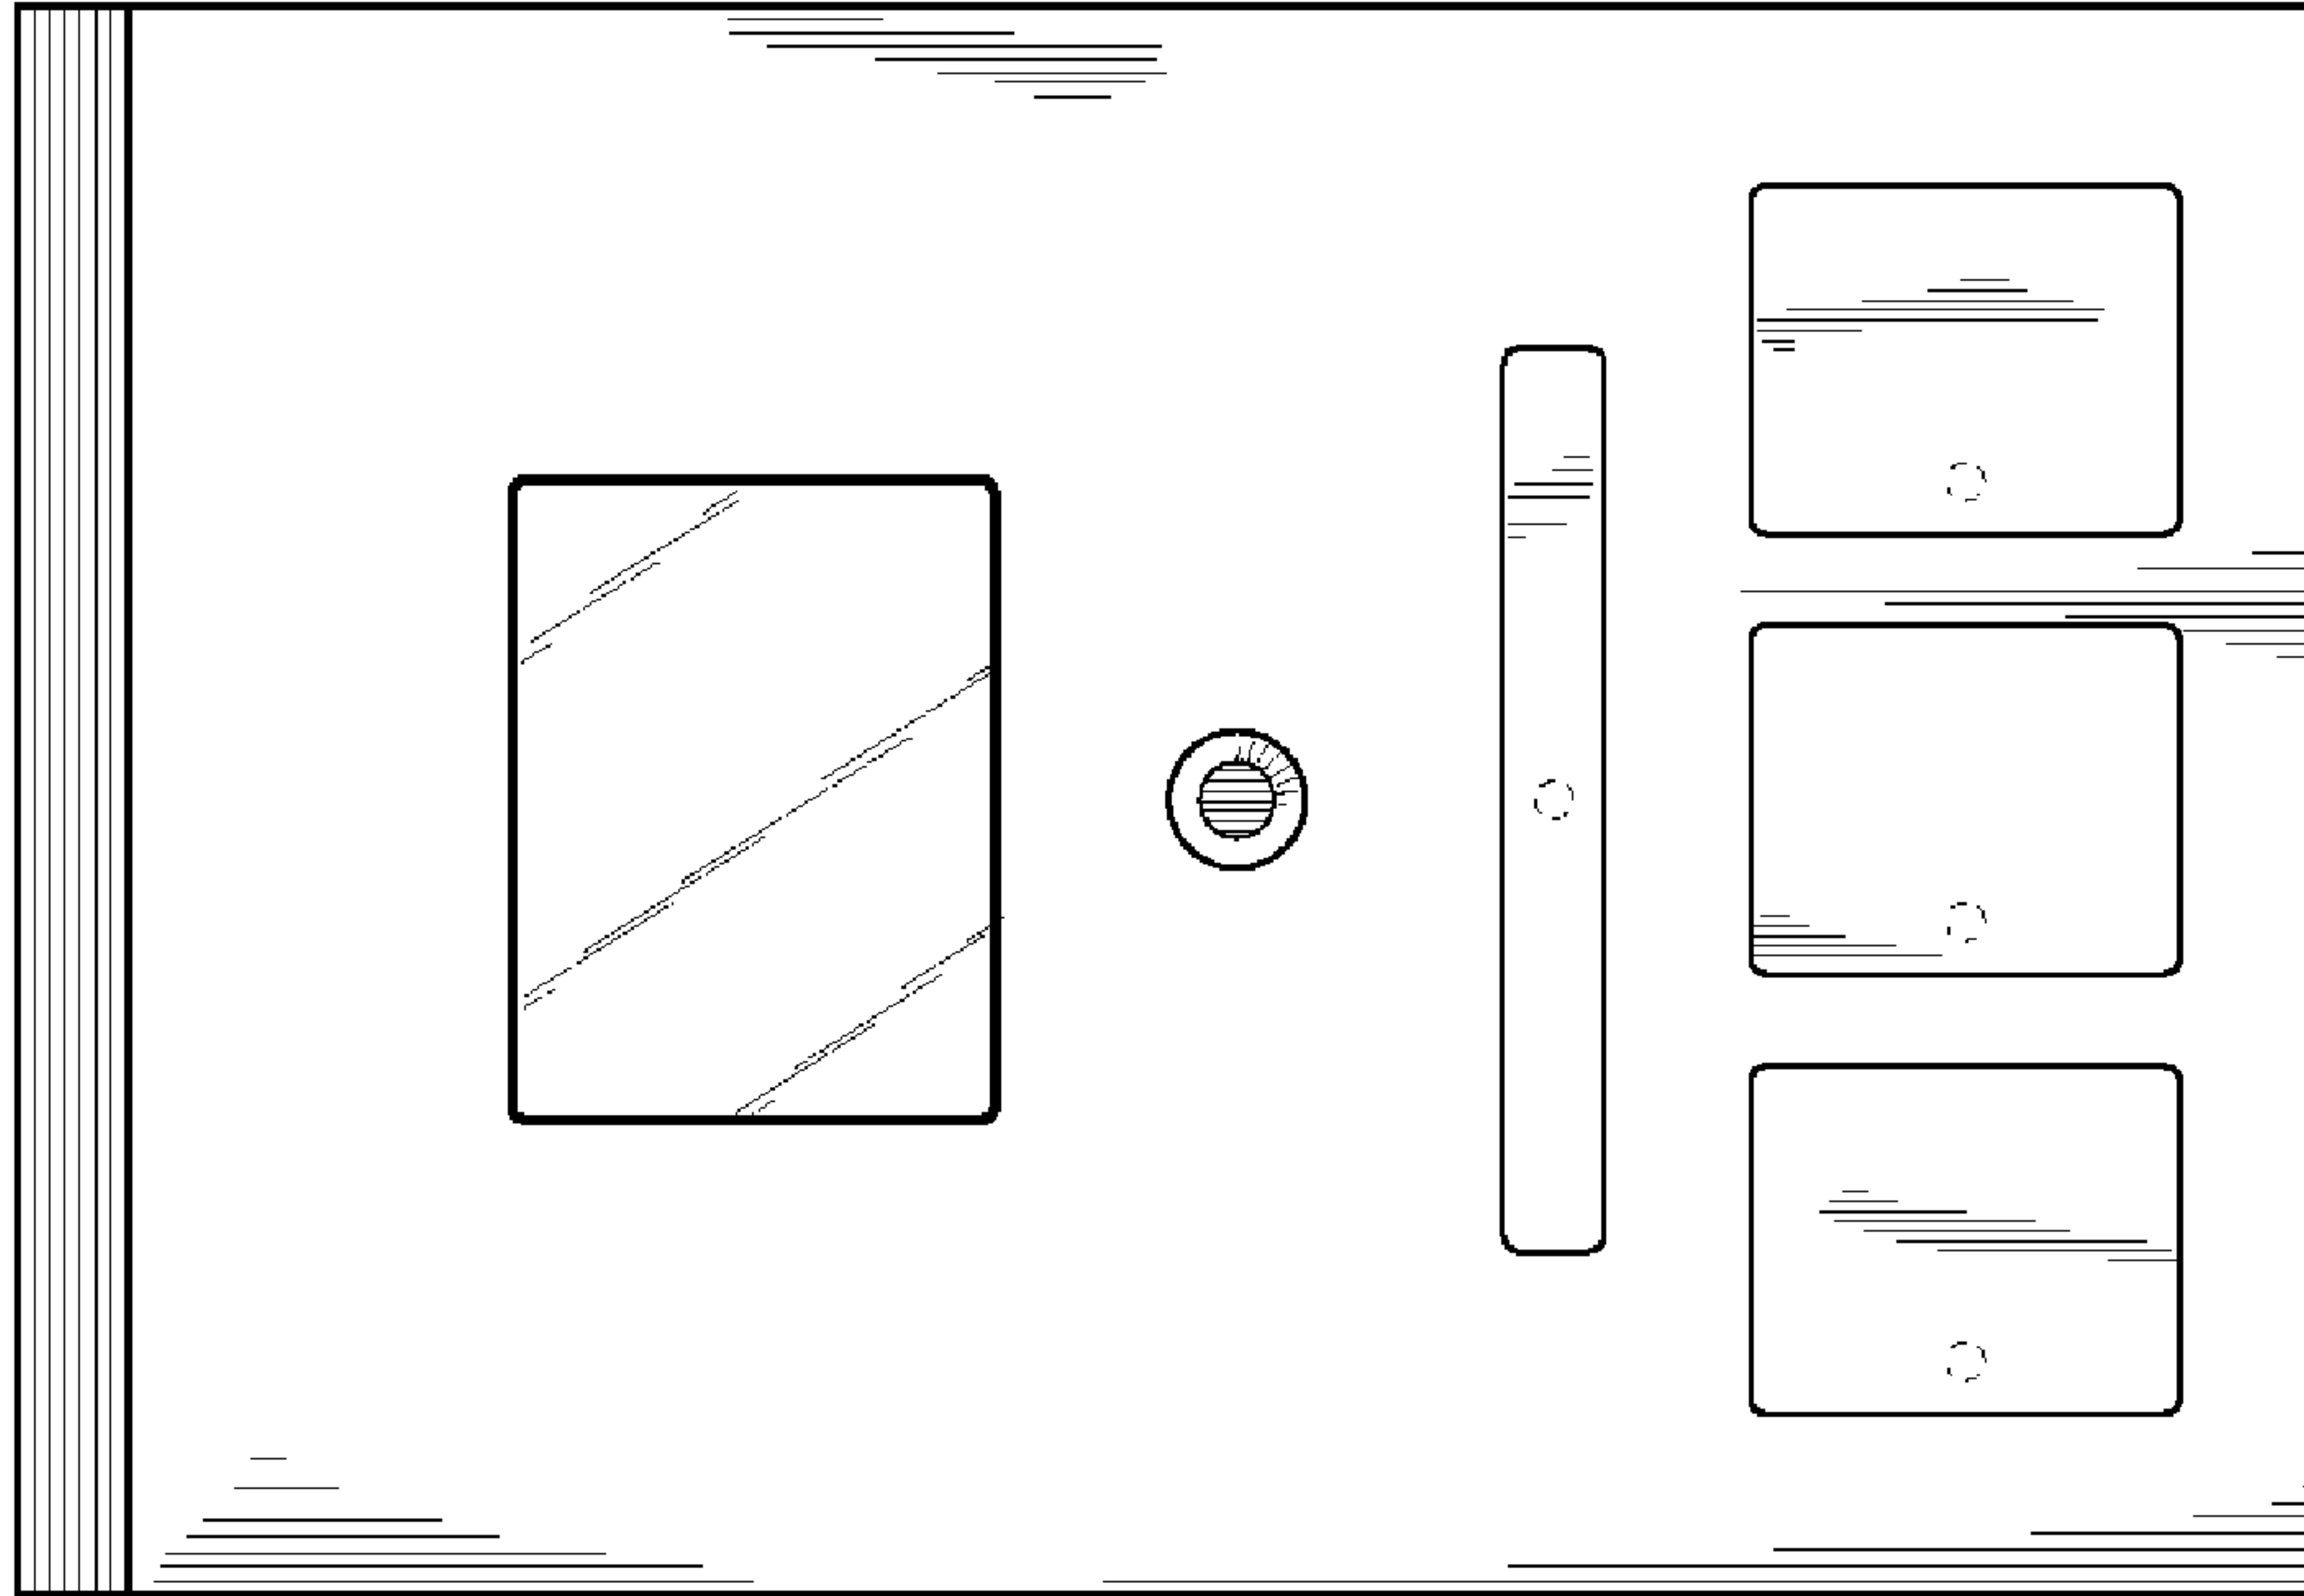


Fig. 2

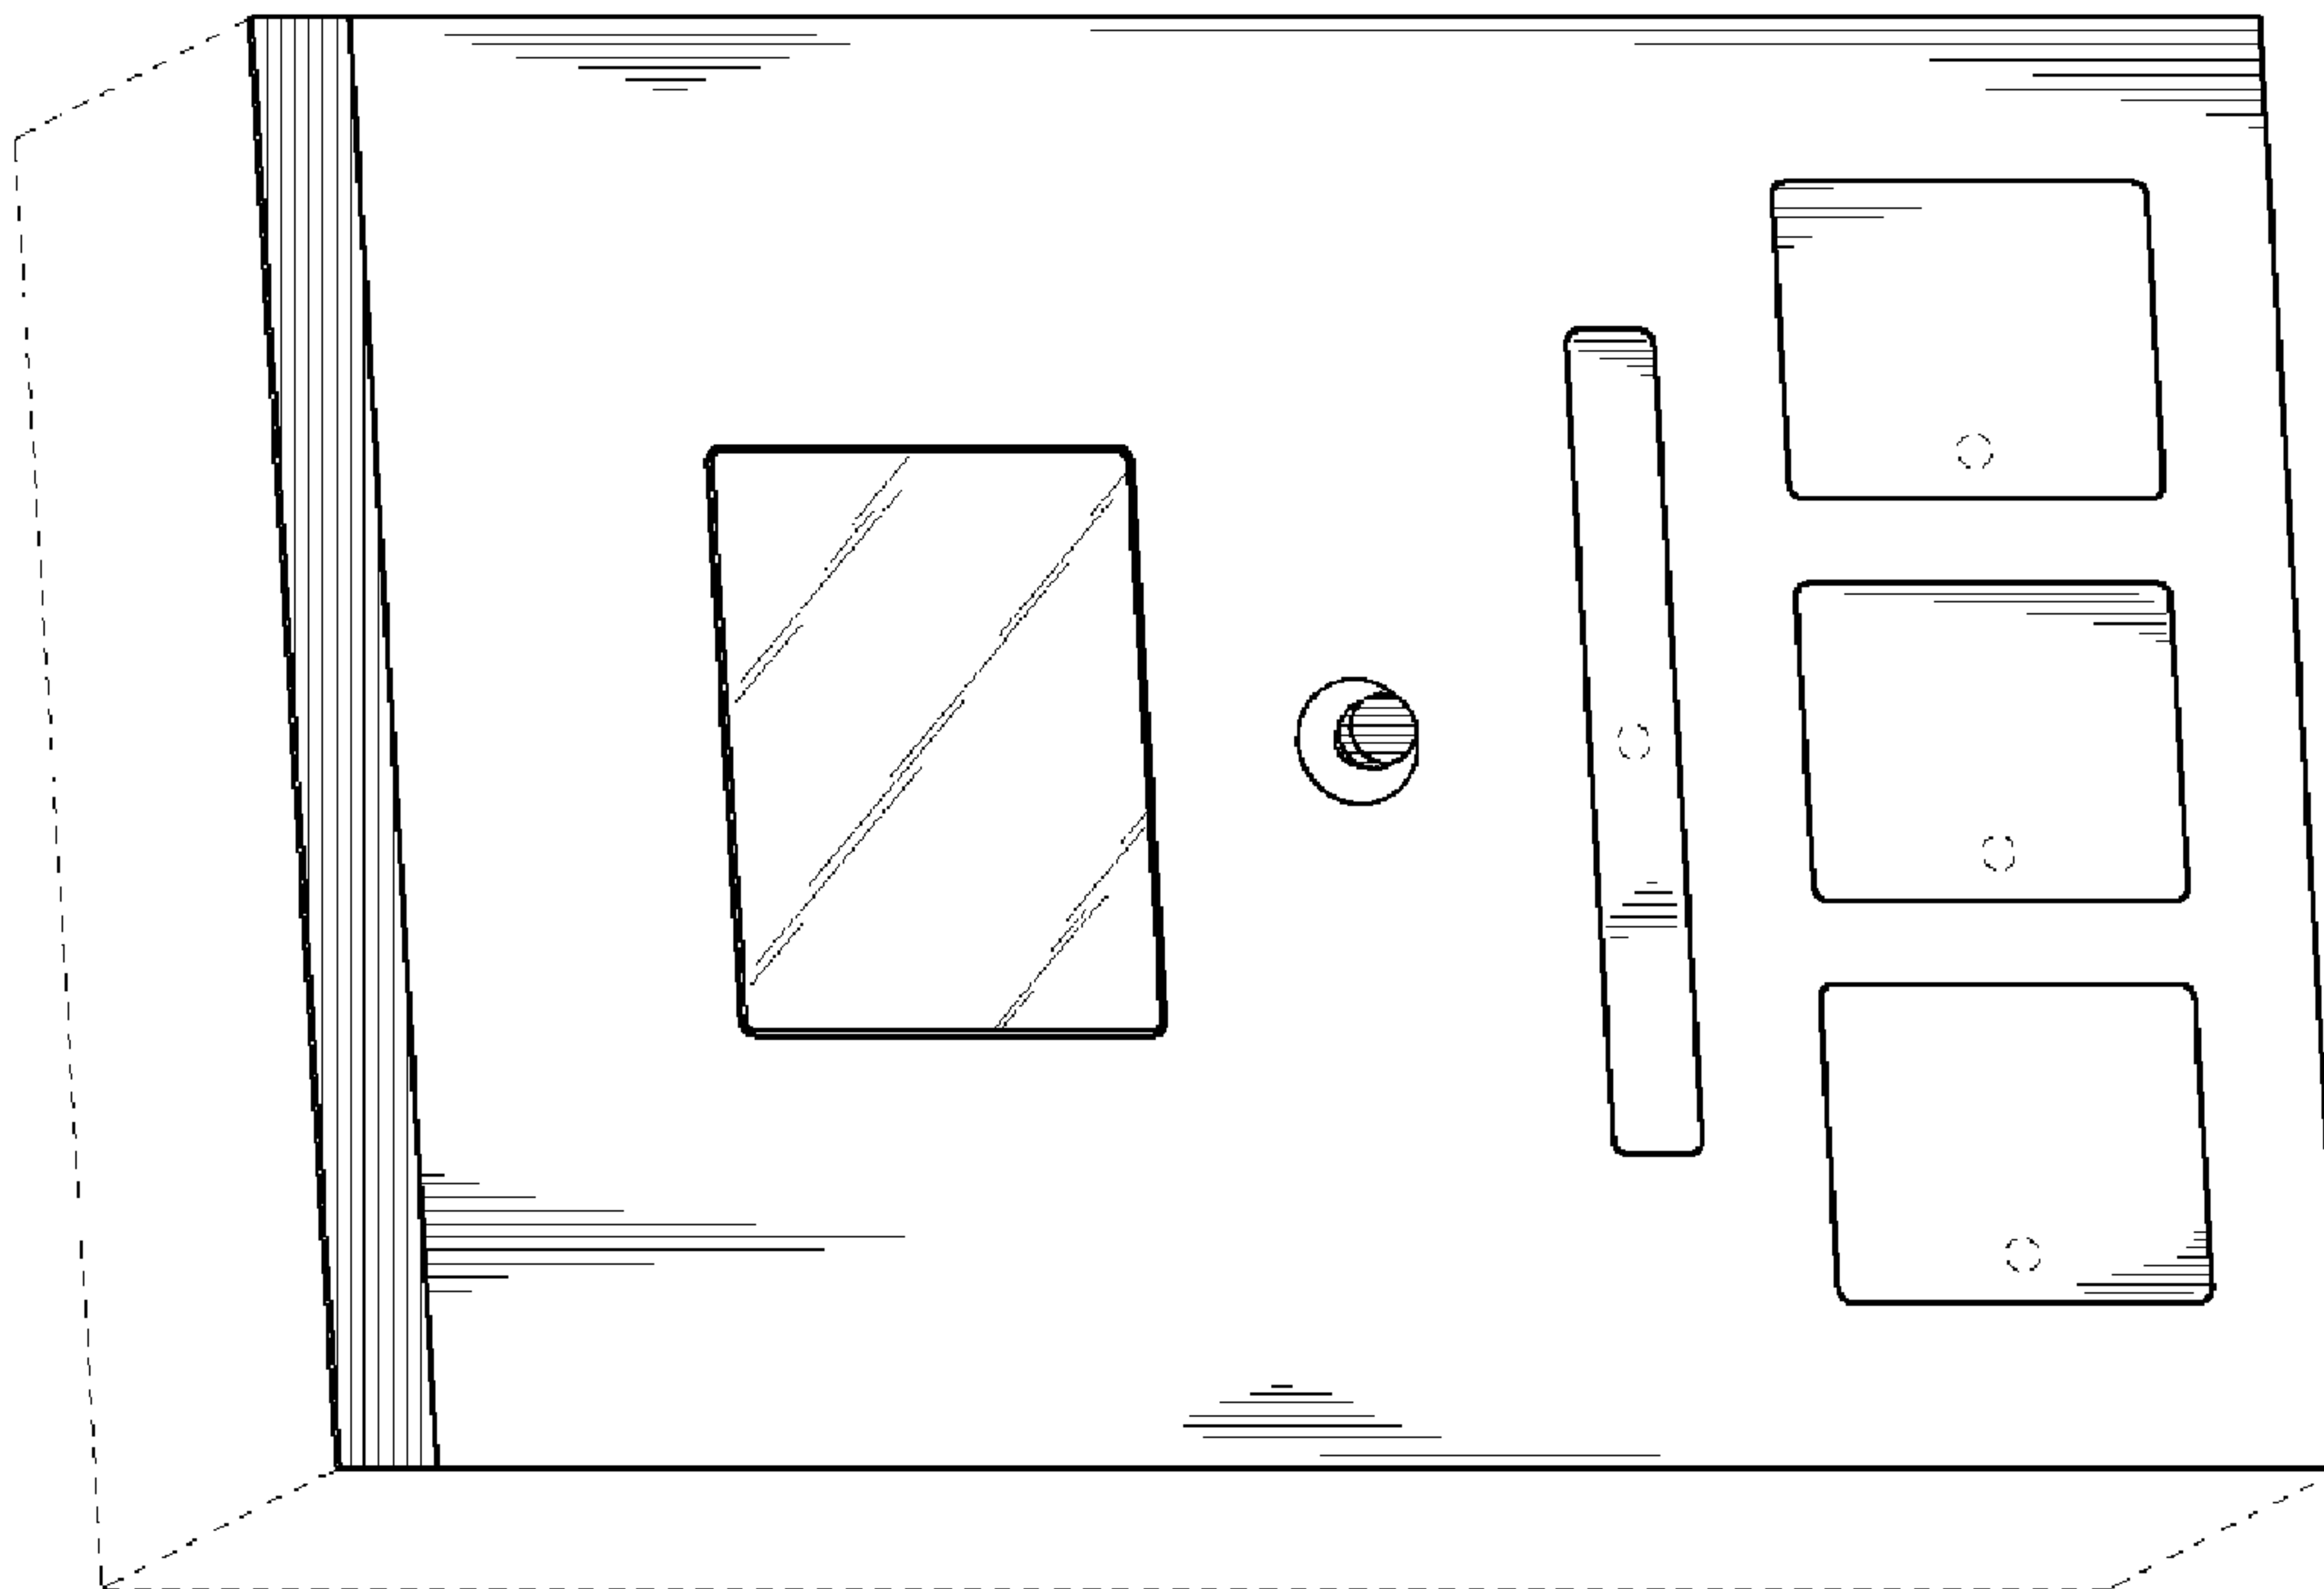


Fig. 1




Fig. 4

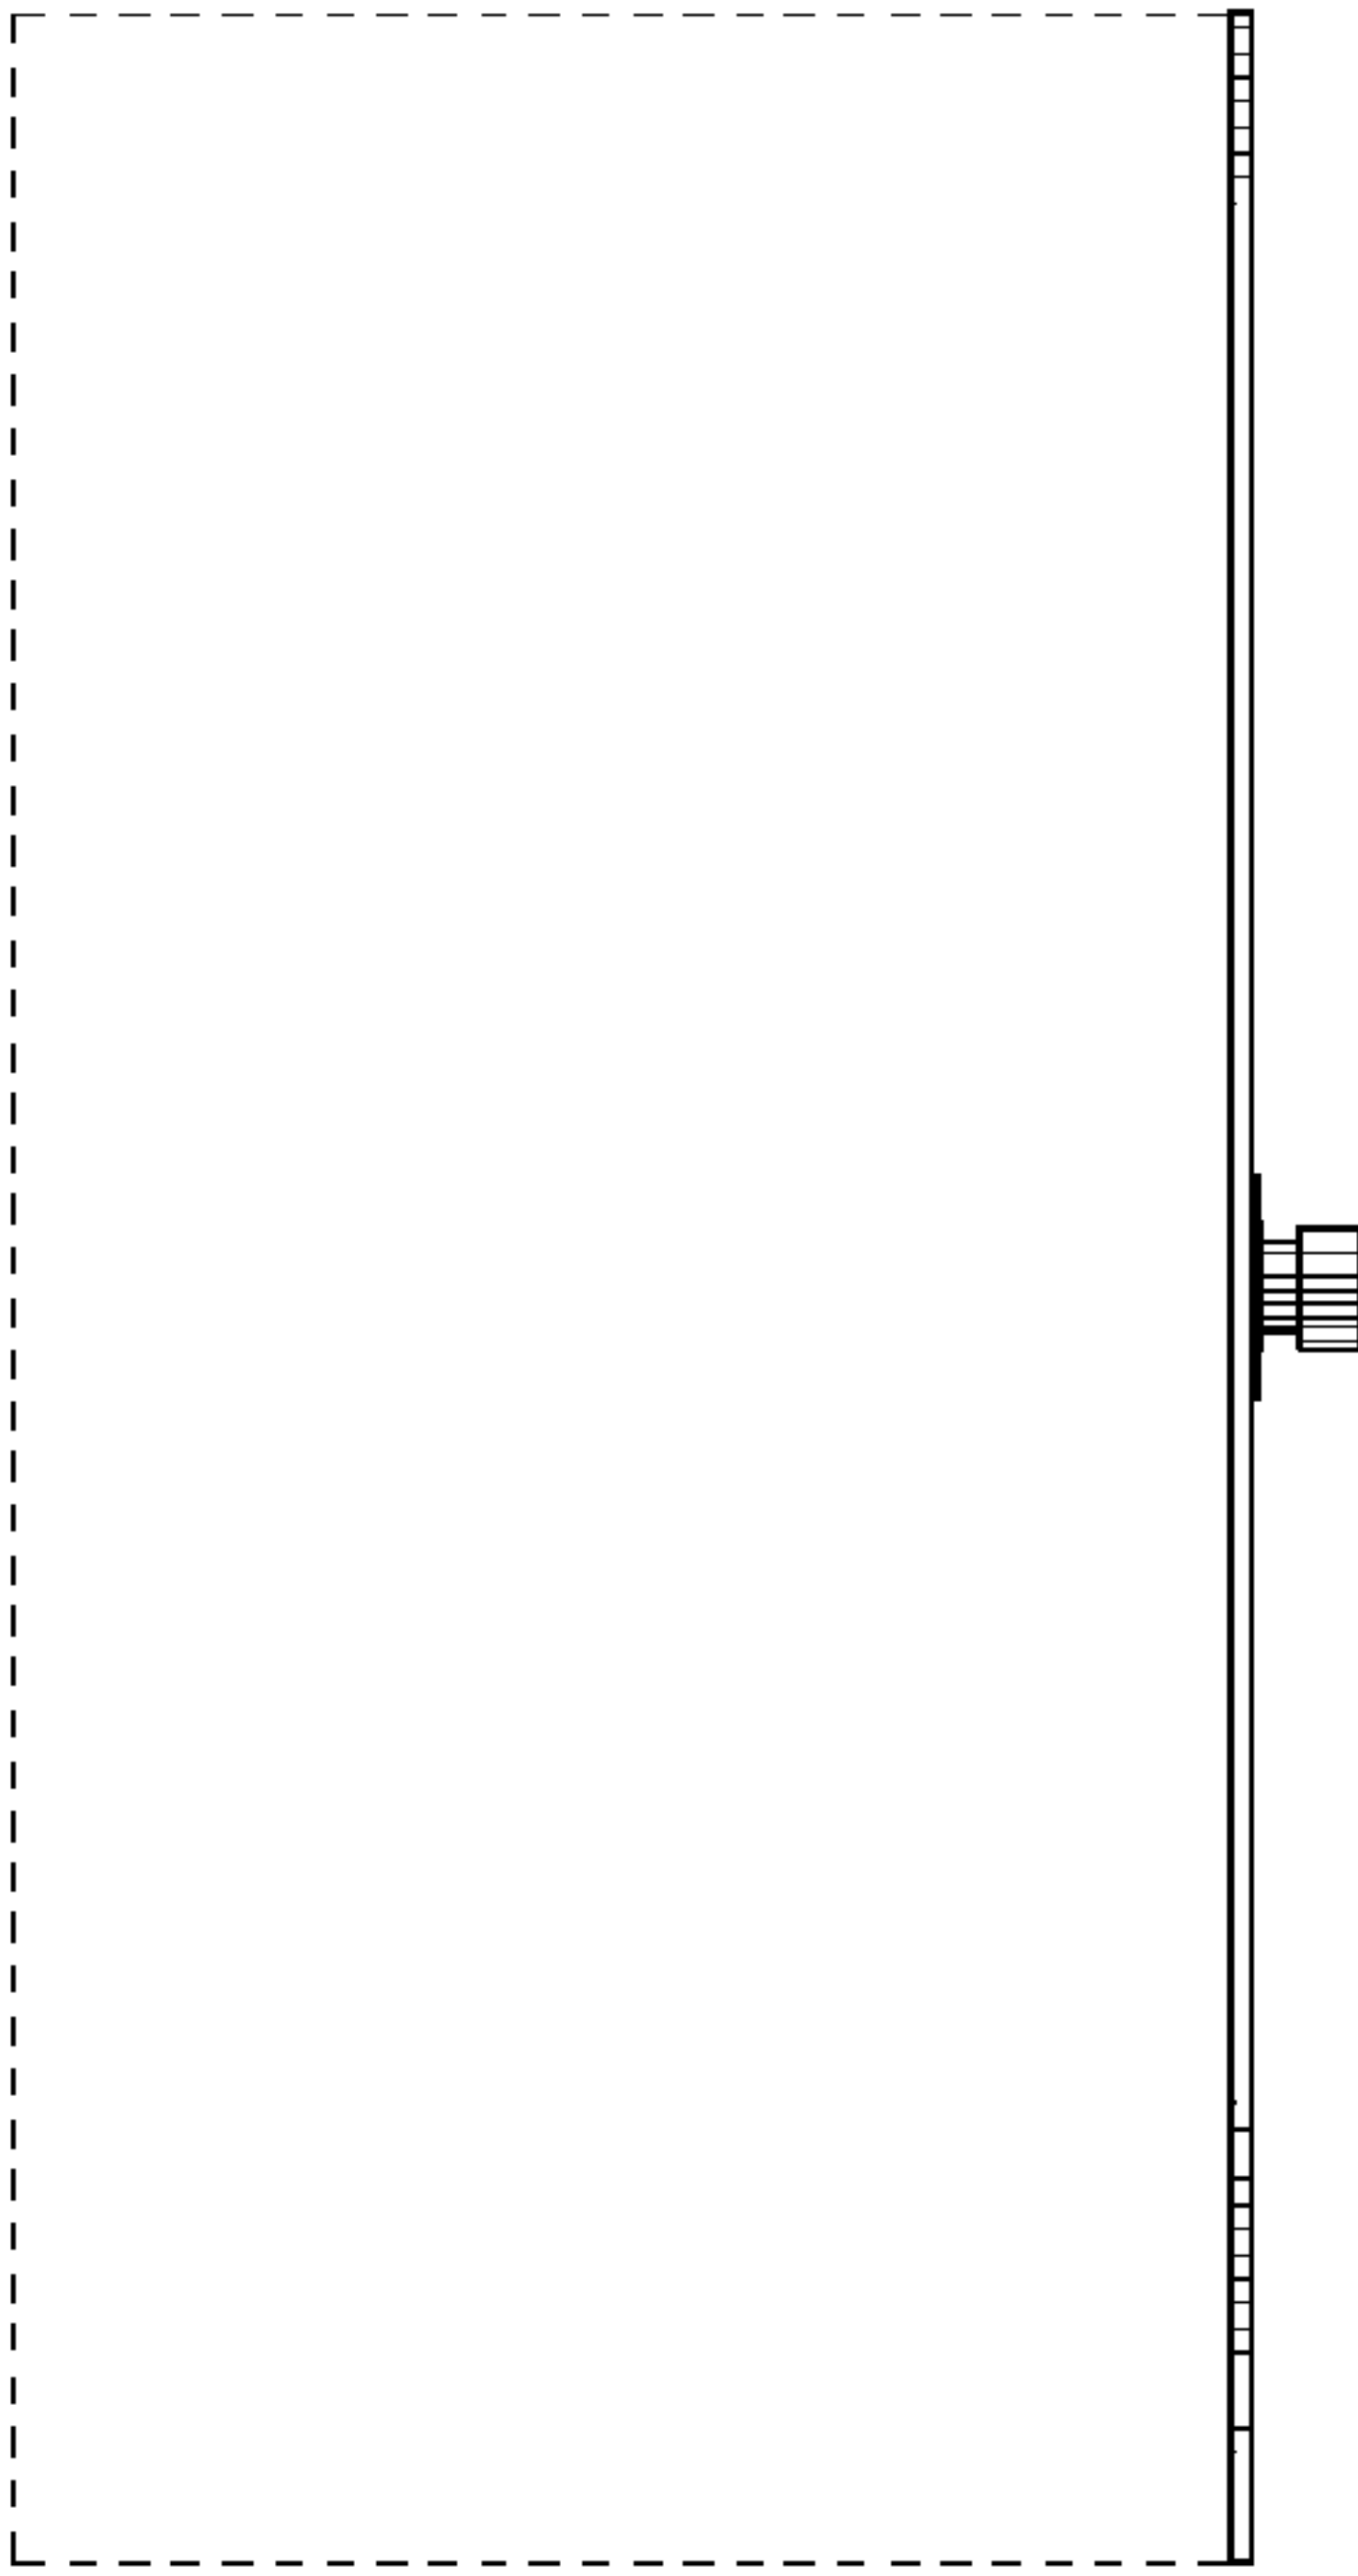


Fig. 3