

US00D667125S

(12) **United States Design Patent**  
**Fisher et al.**

(10) **Patent No.:** **US D667,125 S**

(45) **Date of Patent:** **\*\* Sep. 11, 2012**

(54) **ELECTRONIC READER FOR MEDICAL ENVIRONMENTS**

(76) Inventors: **Stanley Fisher**, Durham, NC (US);  
**Stephen S. Jackson**, Chapel Hill, NC (US)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/396,974**

(22) Filed: **Jul. 8, 2011**

**Related U.S. Application Data**

(60) Continuation of application No. 29/380,885, filed on Dec. 13, 2010, now Pat. No. Des. 641,481, and a division of application No. 29/359,700, filed on Apr. 14, 2010, now Pat. No. Des. 631,165.

(51) **LOC (9) Cl.** ..... **24-01**

(52) **U.S. Cl.** ..... **D24/186**

(58) **Field of Classification Search** ..... D24/185-186;  
D10/106, 109, 40, 70, 15; D13/158, 162,  
D13/164, 165, 168, 170, 177, 160, 154, 137.1,  
D13/137.2, 137.3, 137.4, 139.1, 139.2, 139.8,  
D13/139.3; 340/573.4, 555-556, 600; 250/353,  
250/349, 342, 370; 600/473; 439/105, 535;  
315/360; 363/146; 174/66

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D301,868 S \* 6/1989 Schwartz ..... D13/162  
D309,890 S \* 8/1990 Cheng ..... D13/165  
D310,063 S \* 8/1990 Cheng ..... D13/168  
D310,814 S \* 9/1990 Rosenbaum et al. .... D13/158  
D314,368 S \* 2/1991 Schwartz ..... D13/165  
D323,297 S \* 1/1992 Zeller ..... D10/15  
D324,670 S \* 3/1992 Ferraro ..... D13/137.4  
D325,370 S \* 4/1992 Belcher ..... D13/137.3  
D325,562 S \* 4/1992 Smith, Sr. .... D13/139.1  
D329,422 S \* 9/1992 Fujiyoshi ..... D13/139.1  
D354,943 S \* 1/1995 Williams et al. .... D13/137.1  
D357,460 S \* 4/1995 Lovett ..... D13/139.8  
D361,315 S \* 8/1995 Wedell et al. .... D13/160

D399,495 S \* 10/1998 Bachschmid ..... D13/177  
D401,555 S \* 11/1998 Tam ..... D13/137.3  
D405,760 S \* 2/1999 Yu ..... D13/139.3  
6,045,374 A \* 4/2000 Candeloro ..... 439/105  
6,049,281 A \* 4/2000 Osterweil ..... 340/573.4  
D431,027 S \* 9/2000 Armstrong ..... D13/162  
D435,523 S \* 12/2000 Ciornei et al. .... D13/164  
D436,082 S \* 1/2001 Jilani ..... D13/158  
D443,589 S \* 6/2001 Tong et al. .... D13/137.2  
D455,406 S \* 4/2002 Pinchuk ..... D13/165

(Continued)

**OTHER PUBLICATIONS**

Notice of Allowance for U.S. Appl. No. 29/359,700 mailed Sep. 16, 2010.

(Continued)

*Primary Examiner* — T. Chase Nelson

*Assistant Examiner* — Mark Cavanna

(74) *Attorney, Agent, or Firm* — K&L Gates LLP


(57) **CLAIM**

The ornamental design for electronic reader for medical environments, as shown and described.

**DESCRIPTION**

FIG. 1 is a front perspective view of another embodiment of the electronic reader showing our new design;  
FIG. 2 is a front view thereof (the rear view thereof is disclaimed);  
FIG. 3 is a side view thereof;  
FIG. 4 is an opposing side view;  
FIG. 5 is a top end view thereof;  
FIG. 6 is a bottom end view thereof; and,  
FIG. 7 is a front perspective environmental view thereof illustrating the electronic reader in an exemplary medical (e.g., hospital) use environment.  
The broken lines showing an example medical environment are included for the purpose of illustrating portions of the electronic reader for medical environments that form no part of the claimed design.

**1 Claim, 5 Drawing Sheets**

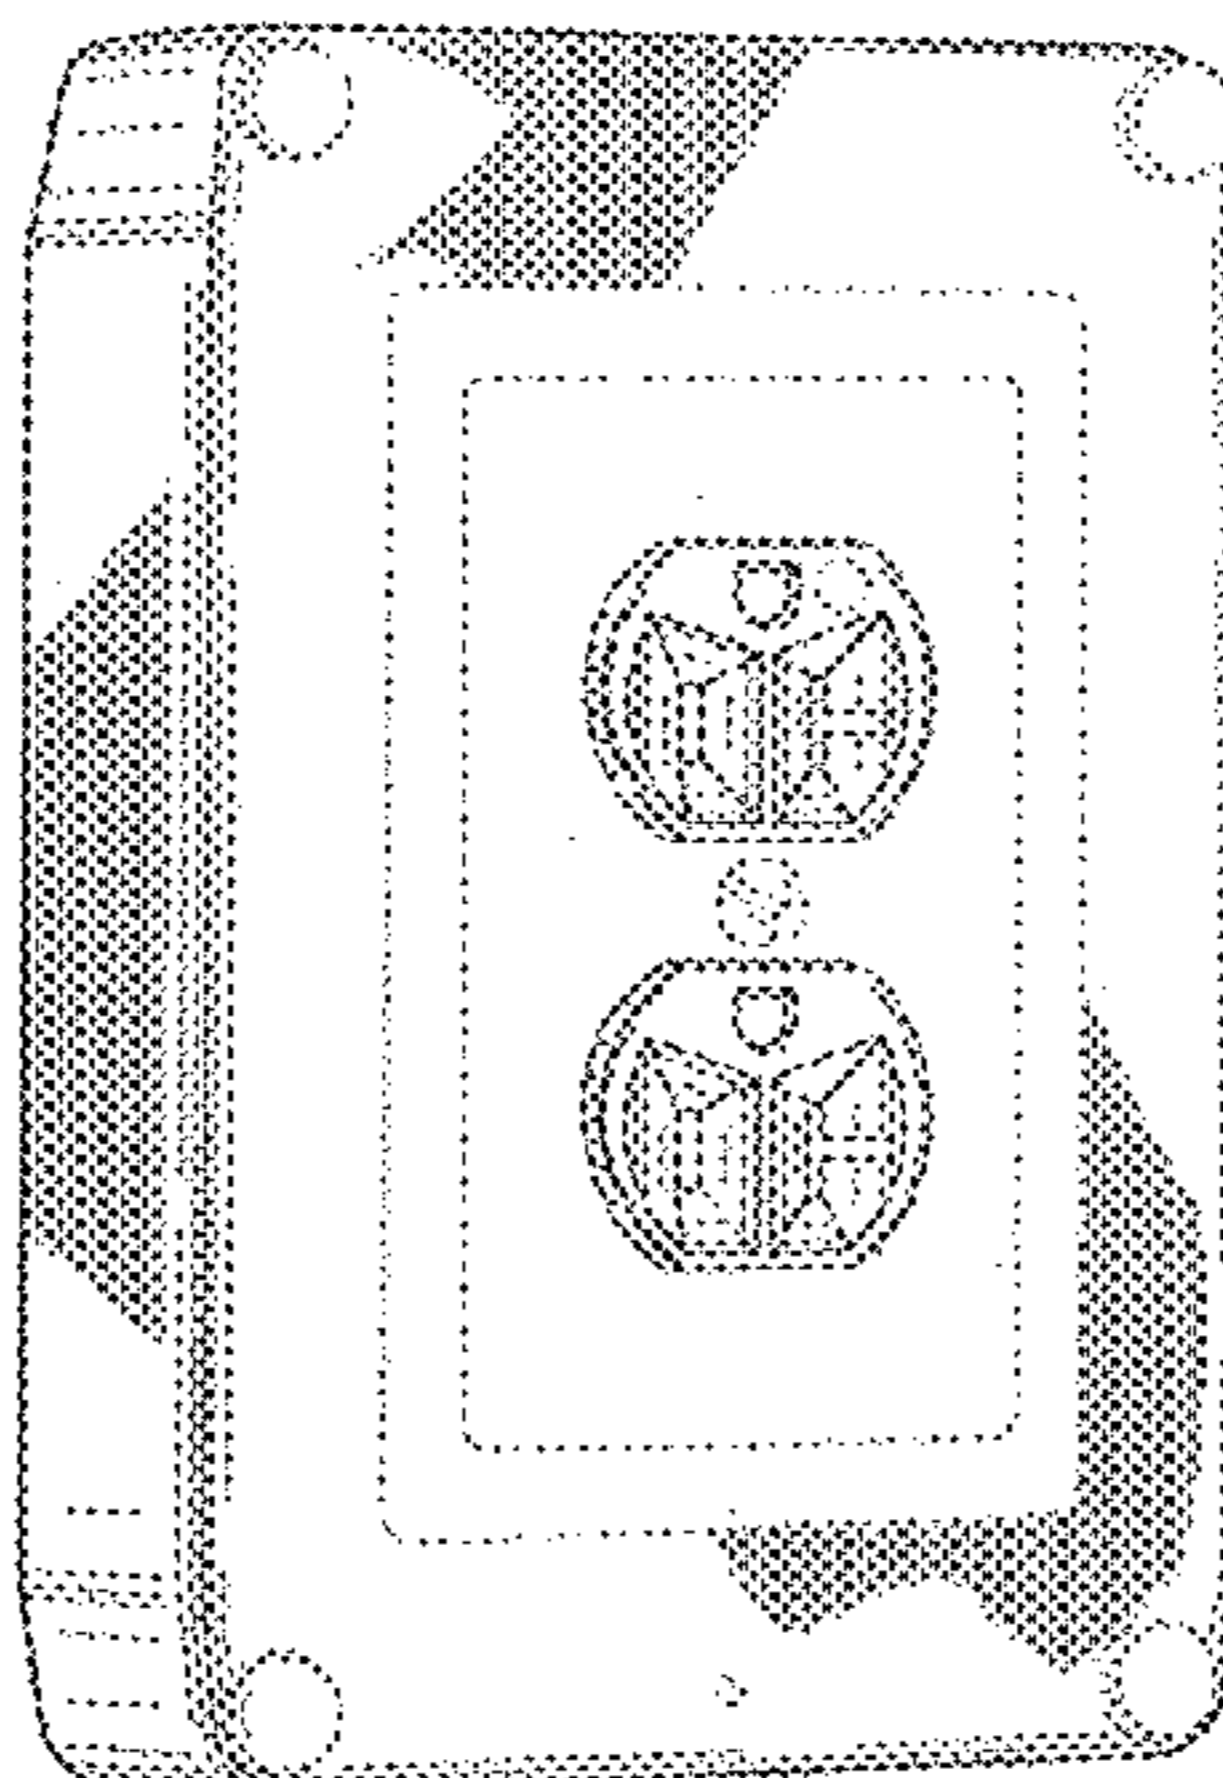

# US D667,125 S

Page 2

## U.S. PATENT DOCUMENTS

D486,126 S \* 2/2004 Aromin ..... D13/137.3  
D500,686 S \* 1/2005 Stekelenburg ..... D10/40  
D500,687 S \* 1/2005 Morrison et al. .... D10/40  
D514,067 S \* 1/2006 Lee ..... D13/137.2  
D523,397 S \* 6/2006 Maglionico et al. .... D13/137.2  
D535,204 S \* 1/2007 Bender et al. .... D10/106.8  
D543,939 S \* 6/2007 Burke ..... D13/137.2  
D547,272 S \* 7/2007 Ng et al. .... D13/137.2  
D565,984 S \* 4/2008 Lidong et al. .... D10/106.8  
D567,950 S \* 4/2008 Savage, Jr. .... D24/186  
D568,253 S \* 5/2008 Gorman ..... D13/154  
D581,870 S \* 12/2008 Zhou ..... D13/137.2  
D582,346 S \* 12/2008 Zhou ..... D13/137.2  
D583,688 S \* 12/2008 Guercio ..... D10/70  
D588,035 S \* 3/2009 Schmalz et al. .... D10/106.8  
D588,076 S \* 3/2009 Ollila ..... D13/168  
D590,352 S \* 4/2009 Jacoby et al. .... D13/164  
D595,229 S \* 6/2009 LaGrotta ..... D13/137.2  
D595,604 S \* 7/2009 Schmalz et al. .... D10/106.8  
D596,140 S \* 7/2009 Hollner ..... D13/164  
D603,346 S \* 11/2009 Murray et al. .... D13/162  
D608,302 S \* 1/2010 Liu ..... D13/164  
D610,554 S \* 2/2010 Lanfear et al. .... D13/162

D611,005 S \* 3/2010 Lanfear et al. .... D13/162  
D618,808 S 6/2010 Fisher et al.  
D631,165 S 1/2011 Fisher et al.  
D641,481 S 7/2011 Fisher et al.  
2002/0072272 A1 \* 6/2002 King ..... 439/535  
2003/0151938 A1 \* 8/2003 Liao ..... 363/146  
2004/0121648 A1 \* 6/2004 Voros ..... 439/535  
2005/0242753 A1 \* 11/2005 Morrison et al. .... 315/360  
2008/0289844 A1 \* 11/2008 Dutton, Jr. .... 174/66

## OTHER PUBLICATIONS

Notice of Allowance for U.S. Appl. No. 29/380,885 mailed Mar. 7, 2011.  
Non-Final Office Action for U.S. Appl. No. 29/396,972, mailed Oct. 27, 2011.  
Non-Final Office Action for U.S. Appl. No. 29/396,973, mailed Oct. 26, 2011.  
Ex Parte Quayle Action for U.S. Appl. No. 29/396,975, mailed Oct. 26, 2011.  
U.S. Appl. No. 29/396,972, filed Jul. 8, 2011.  
U.S. Appl. No. 29/396,973, filed Jul. 8, 2011.  
U.S. Appl. No. 29/396,975, filed Jul. 8, 2011.

\* cited by examiner

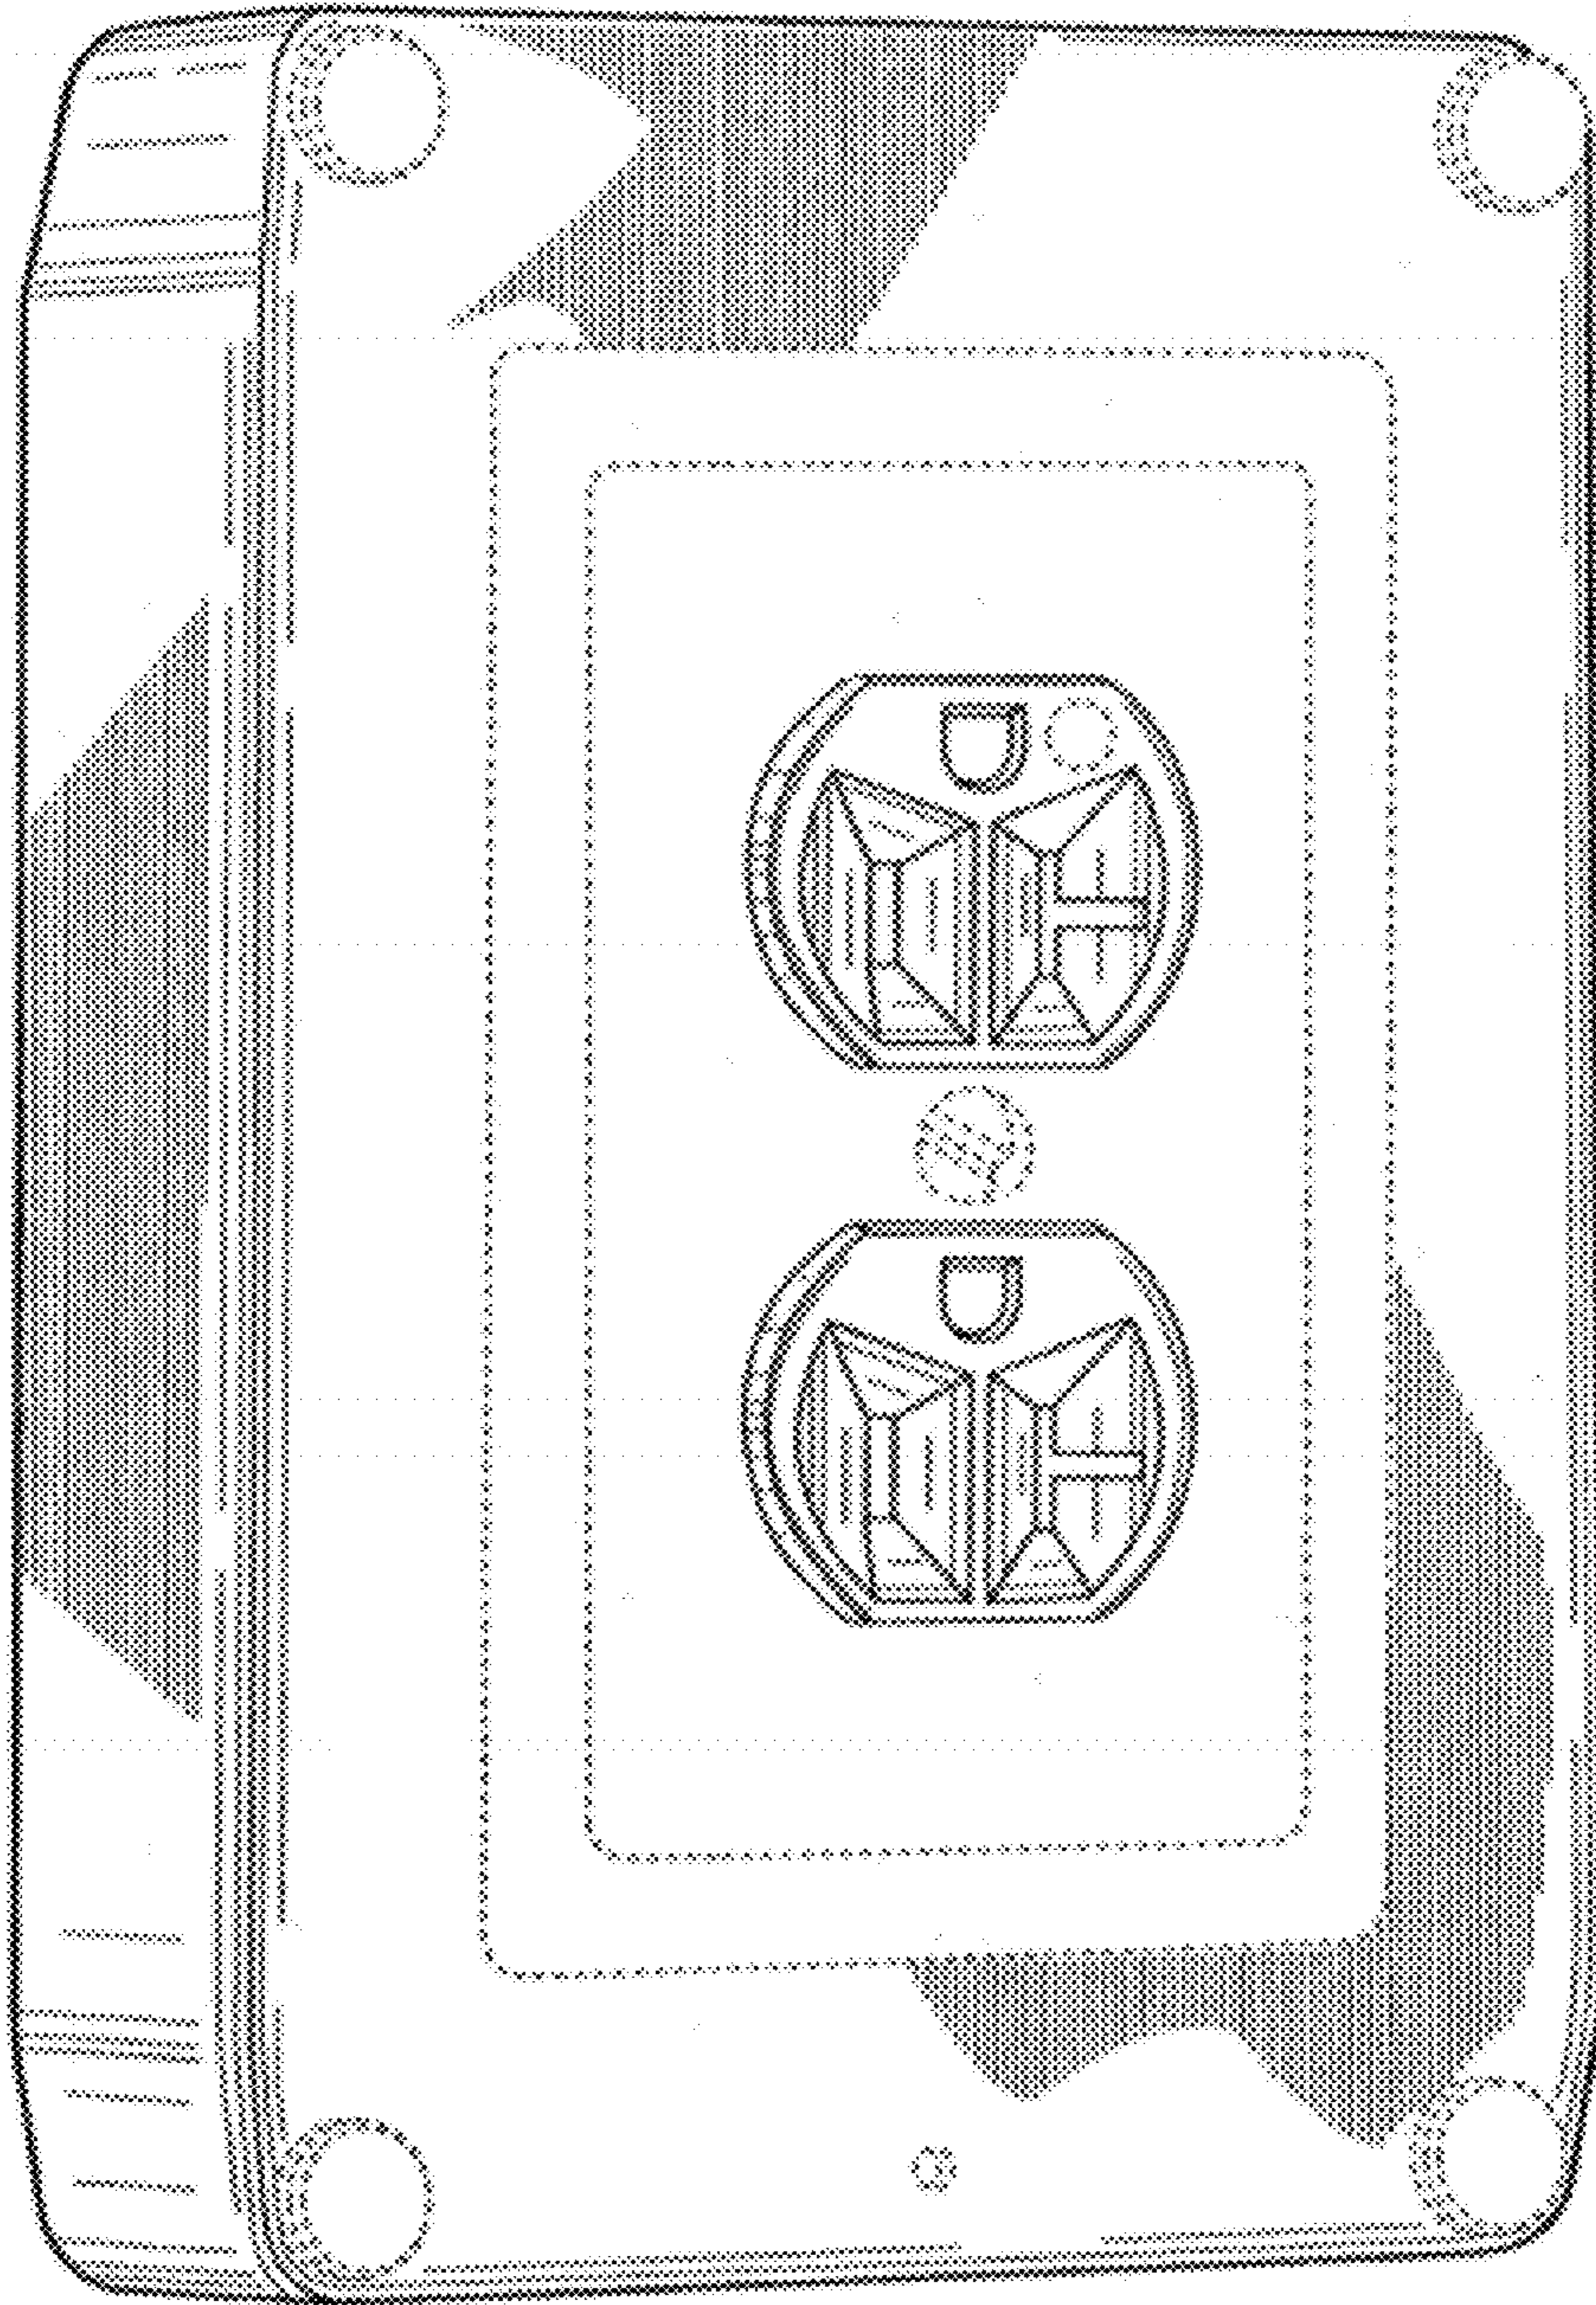


FIG. 1

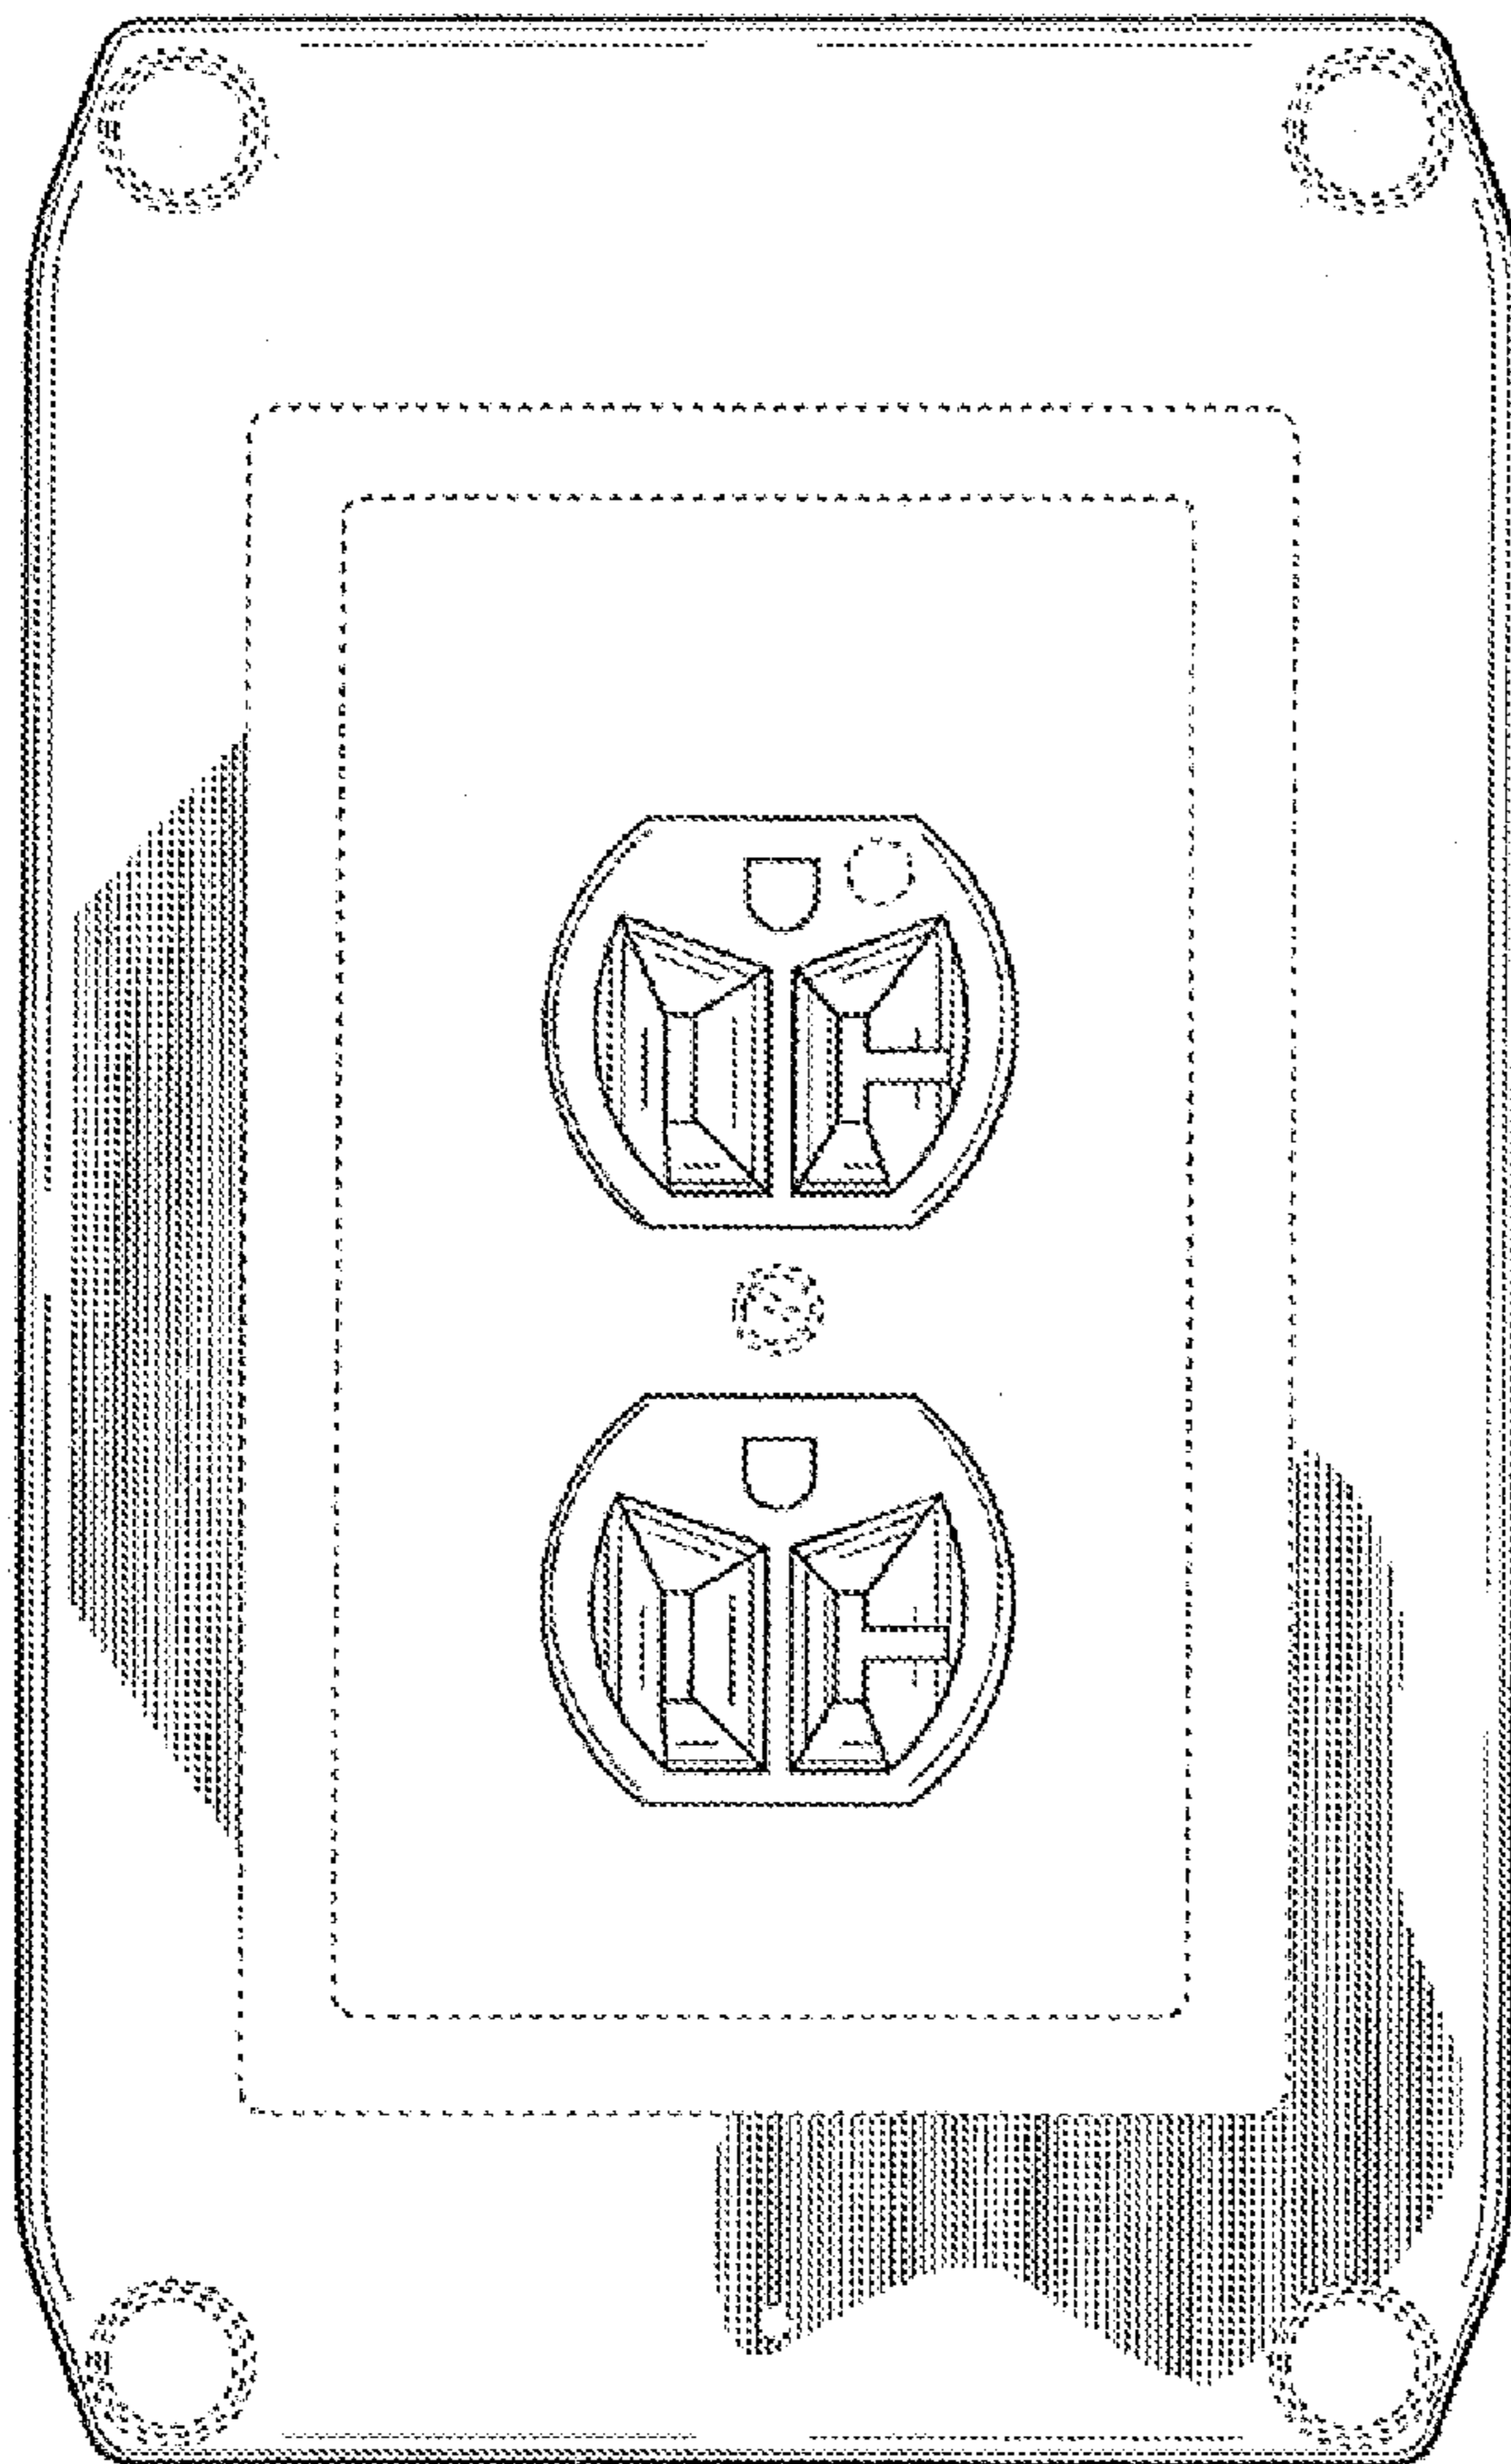


FIG. 2

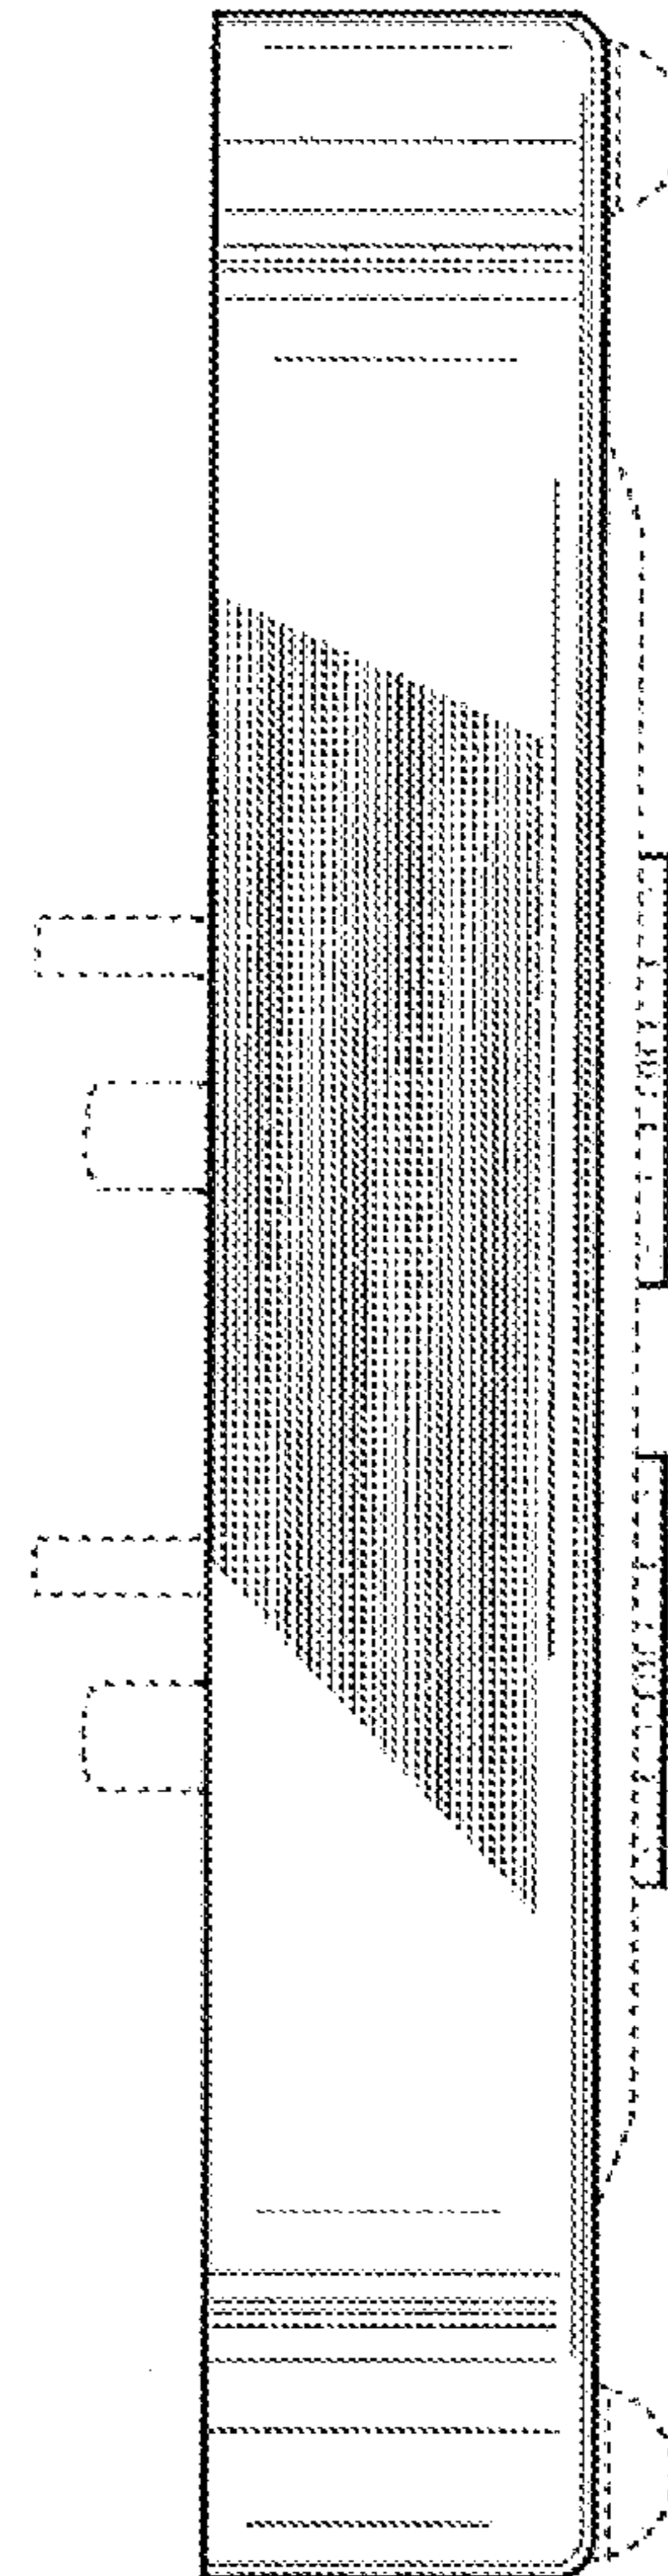


FIG. 3

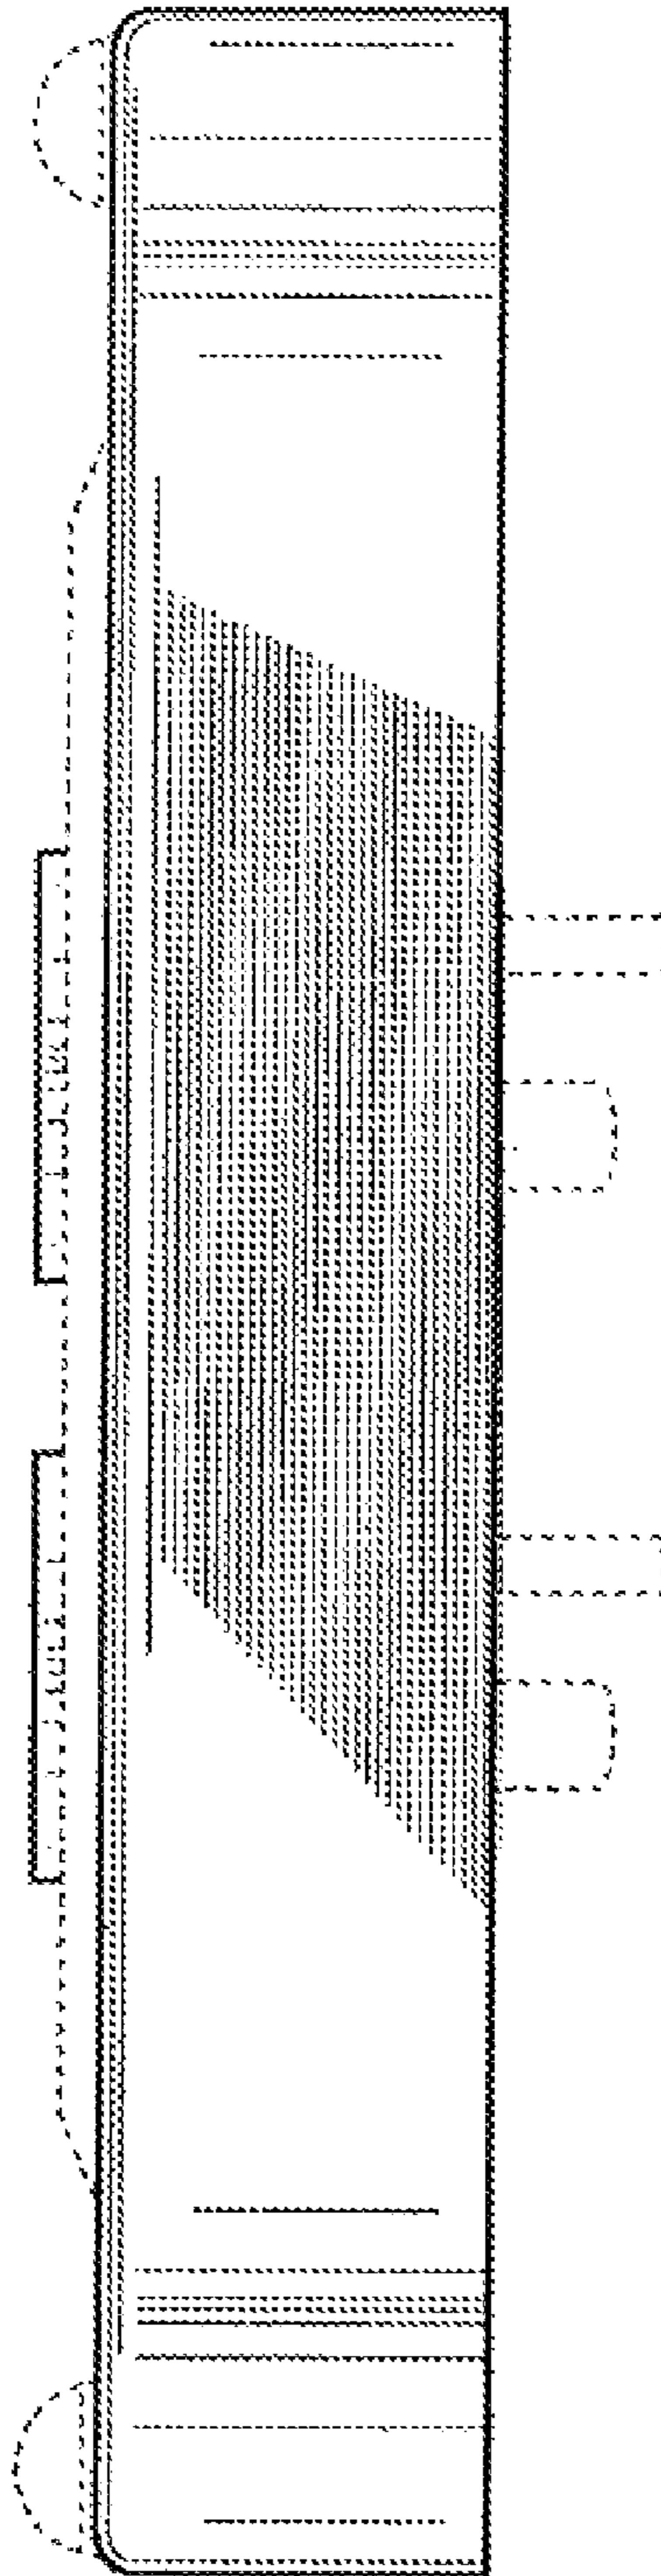


FIG. 4

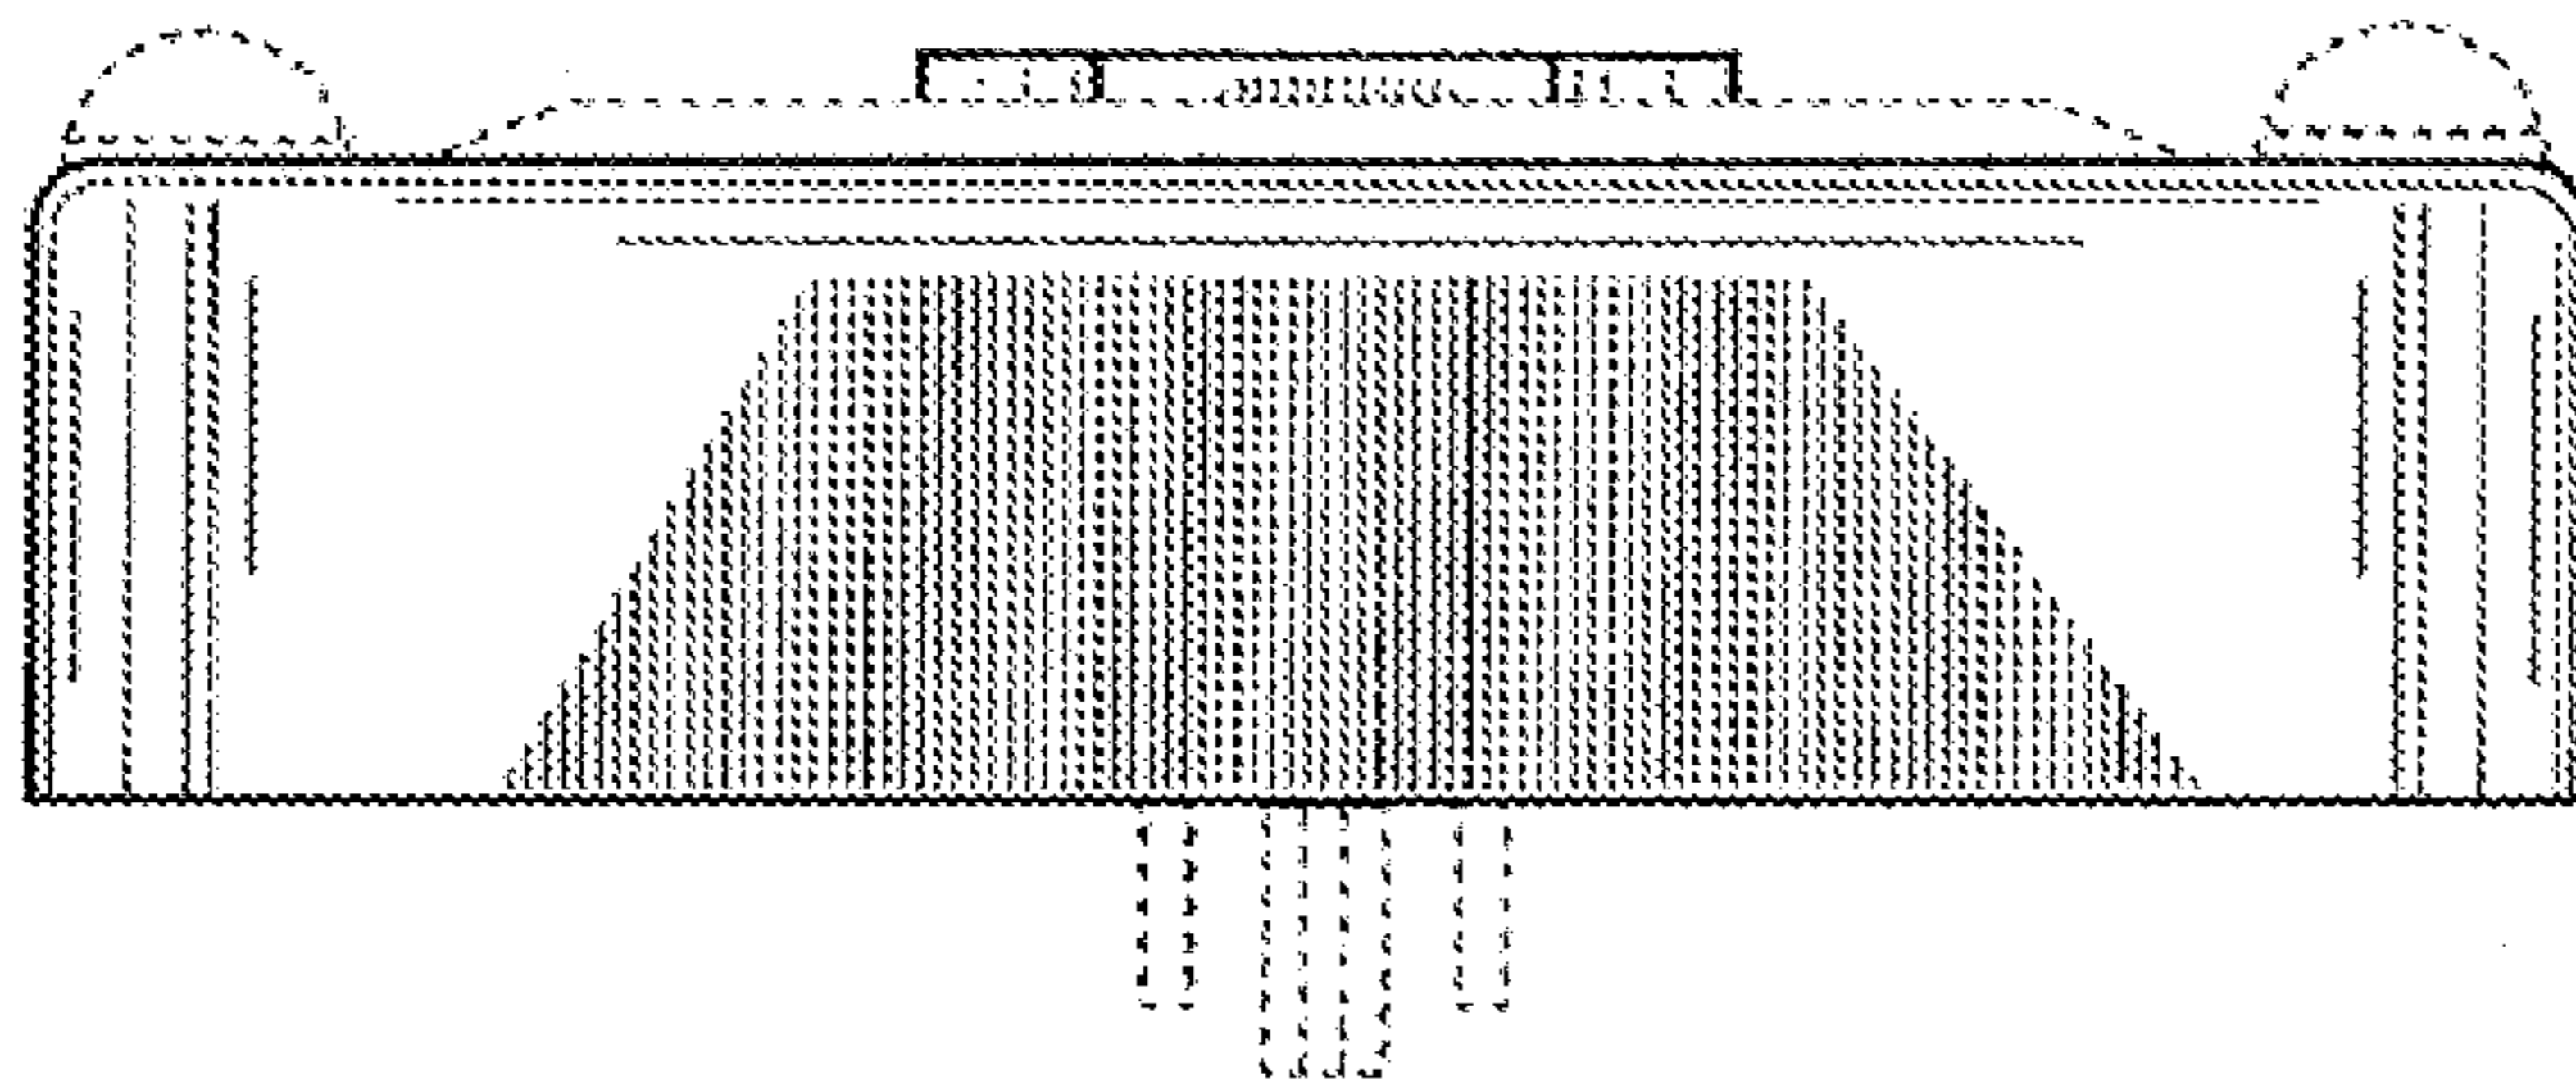


FIG. 5

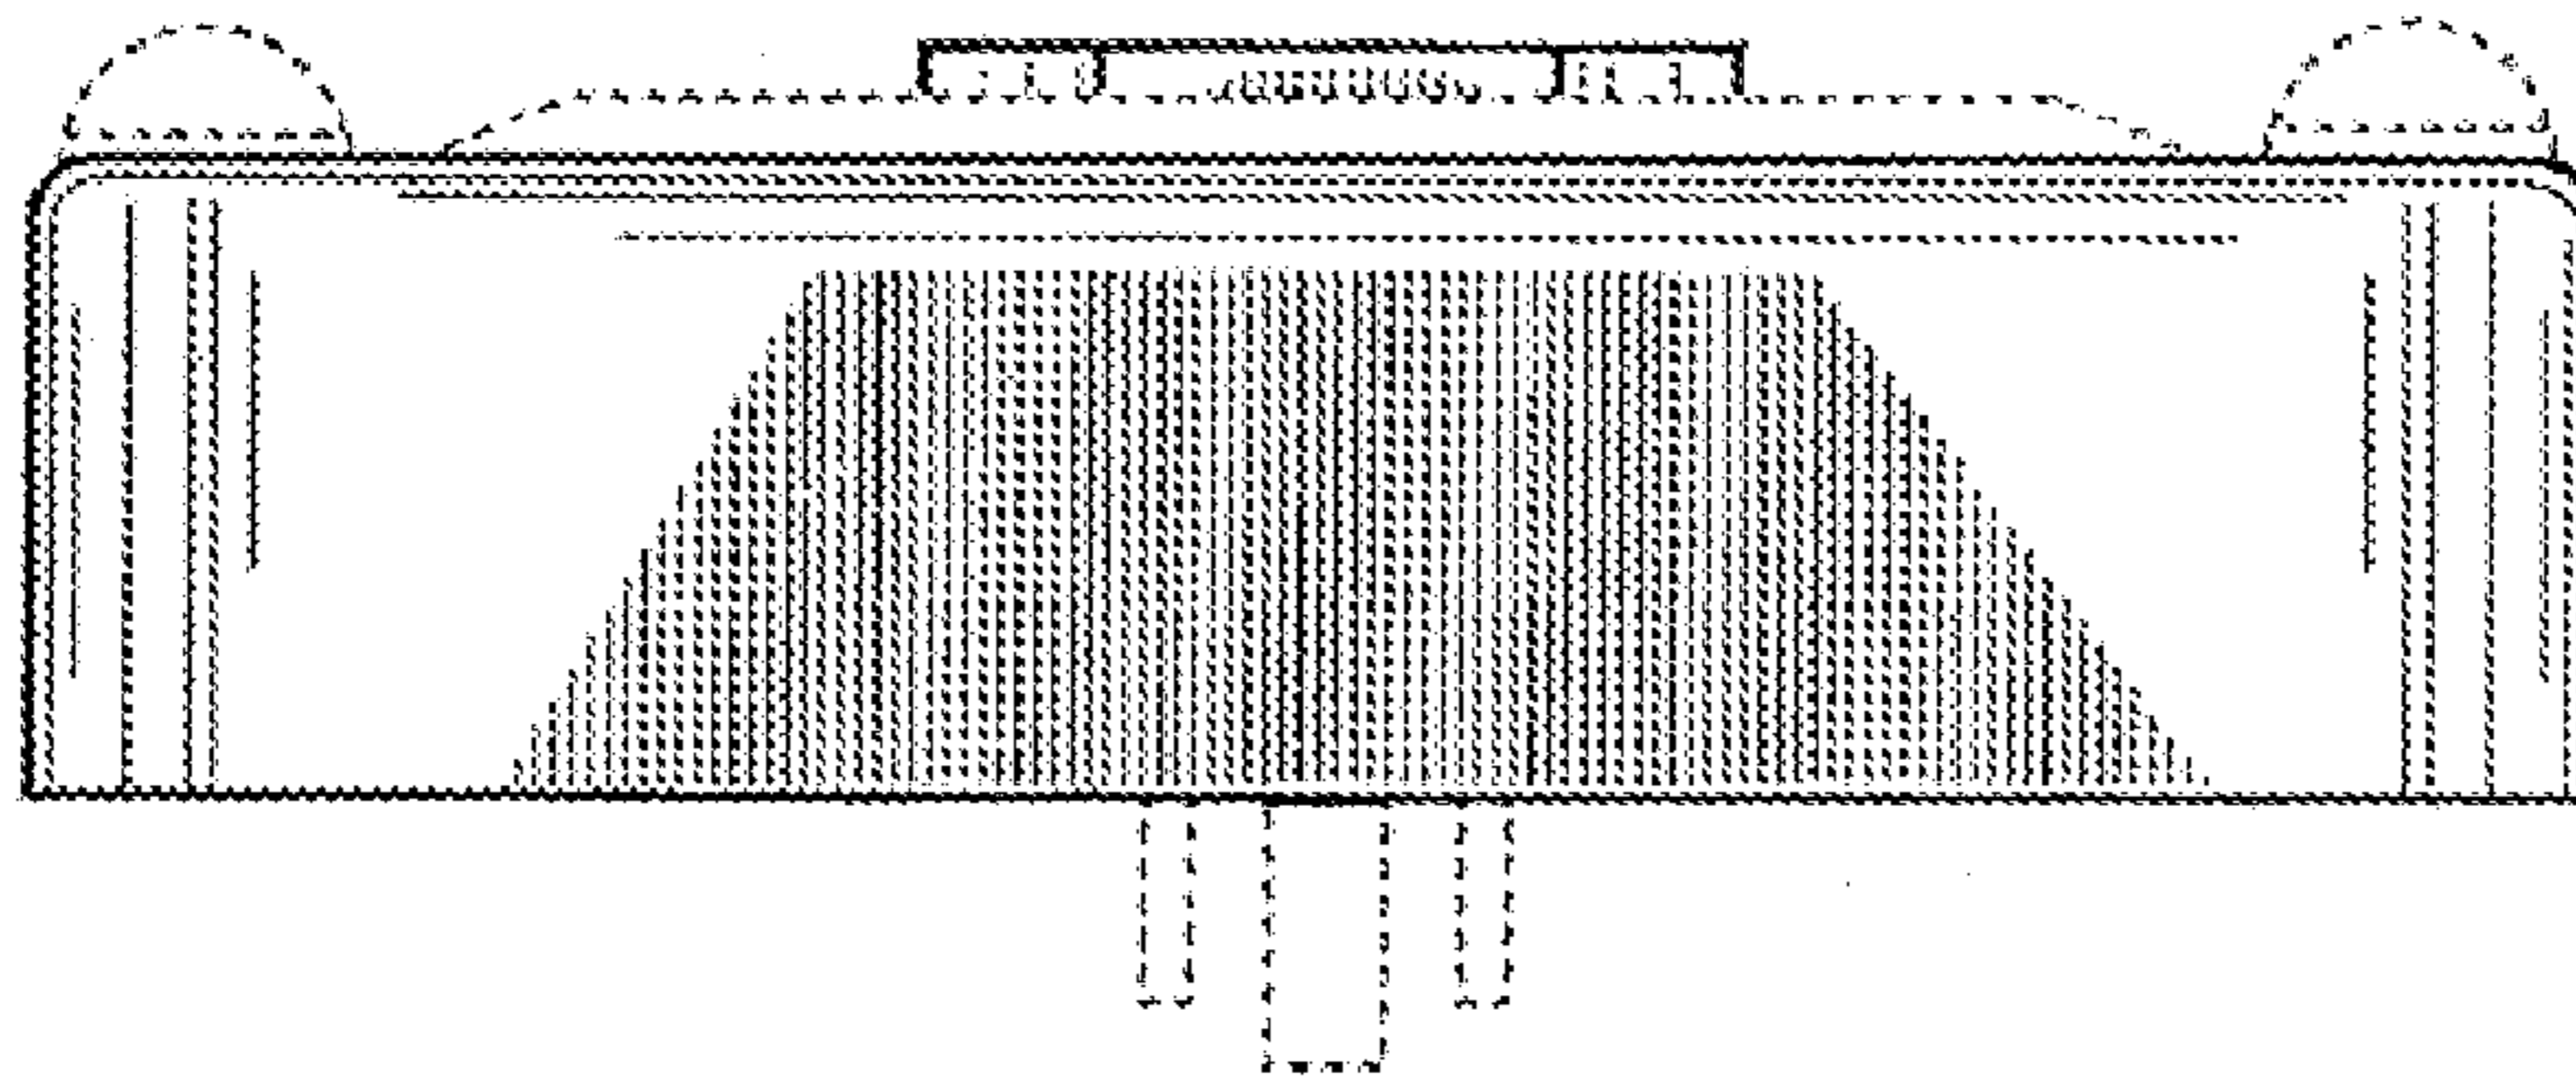


FIG. 6

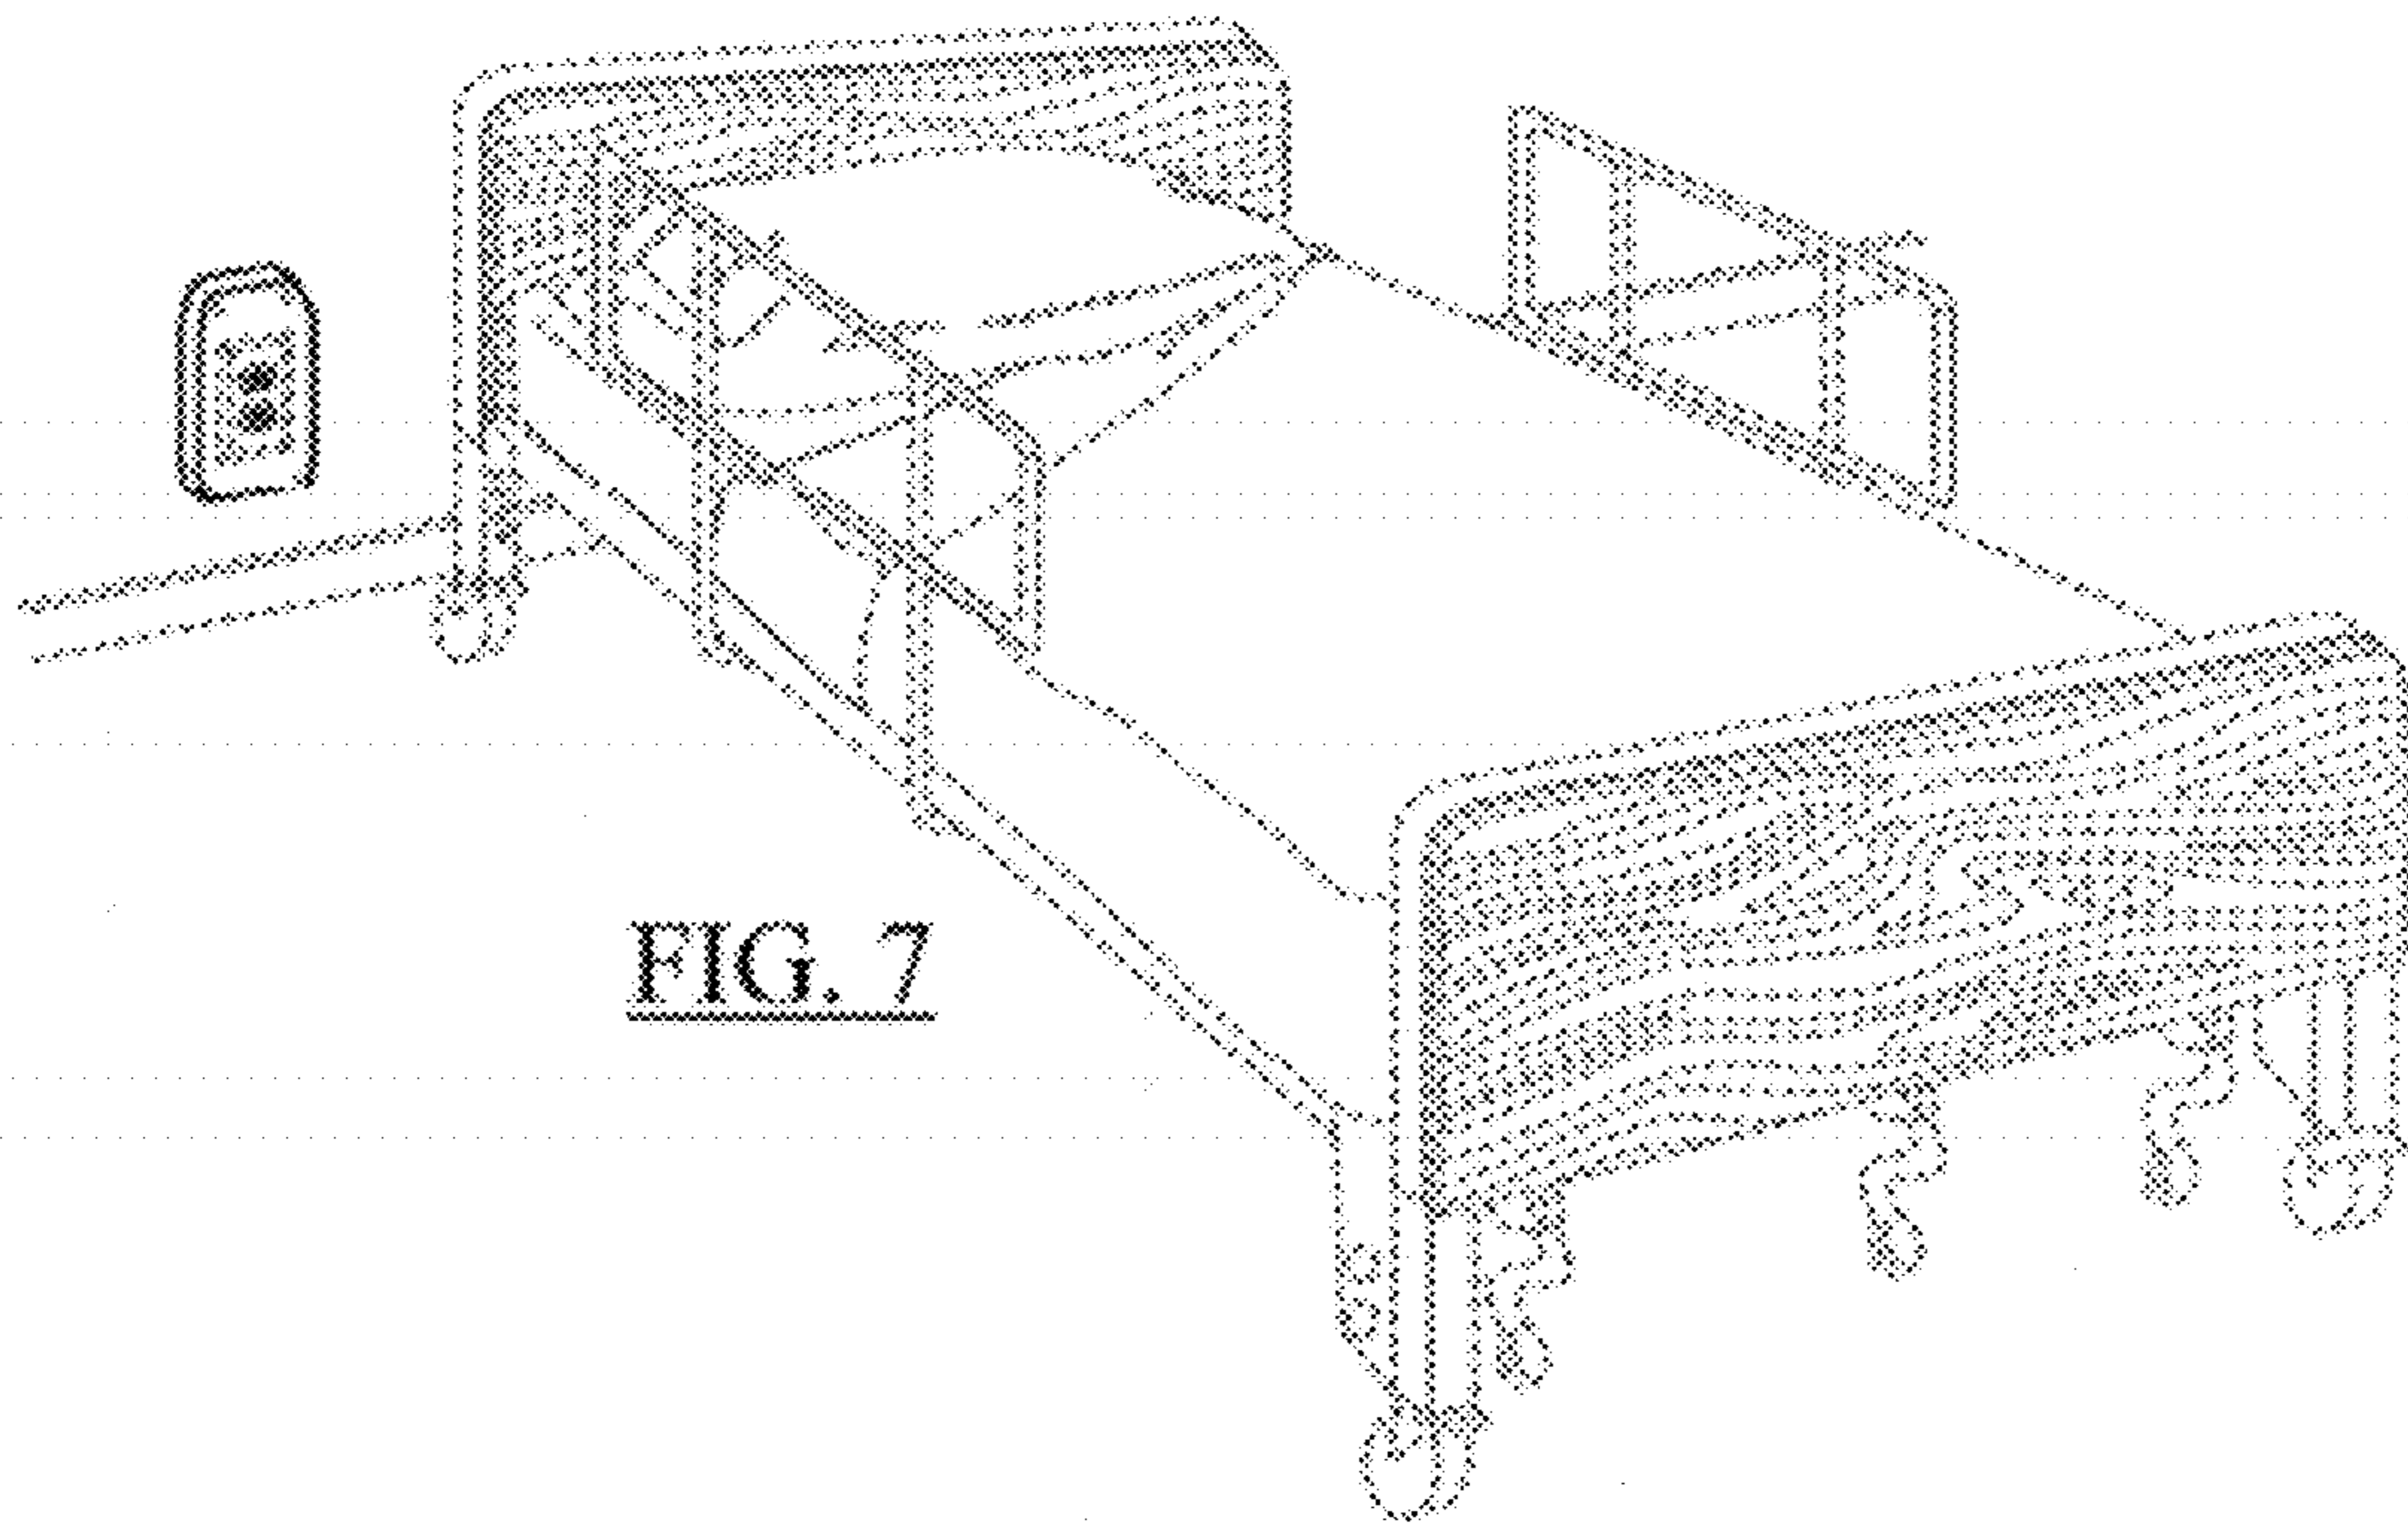


FIG. 7