

US00D668336S

(12) **United States Design Patent**
Yanagawa

(10) **Patent No.:** **US D668,336 S**

(45) **Date of Patent:** **** Oct. 2, 2012**

(54) **ELECTRODE NEEDLE FOR
HIGH-FREQUENCY THERAPY EQUIPMENT**

(75) Inventor: **Kiwamu Yanagawa**, Tokyo (JP)

(73) Assignee: **Kabushiki Kaisha Top**, Tokyo (JP)

(**) Term: **14 Years**

(21) Appl. No.: **29/391,552**

(22) Filed: **May 10, 2011**

(30) **Foreign Application Priority Data**

Nov. 11, 2010 (JP) 2010-027171

(51) **LOC (9) Cl.** **24-02**

(52) **U.S. Cl.** **D24/144; D24/130**

(58) **Field of Classification Search** D24/144,
D24/133, 146-147, 170, 145, 186-187, 112,
D24/129-130, 127; 606/31-35, 37-38, 41-42,
606/45-50, 167, 169; 600/567, 372; 604/528,
604/533, 523, 264, 272, 19, 22

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,198,319 A * 4/1940 Silverman 600/567
2,994,324 A * 8/1961 Lemos D24/144
3,058,225 A * 10/1962 Ward D24/147
4,892,105 A * 1/1990 Prass 600/554

5,011,473 A * 4/1991 Gattorna 604/528
5,971,980 A * 10/1999 Sherman 606/34
6,402,701 B1 * 6/2002 Kaplan et al. 600/567
D494,677 S * 8/2004 Garvin D24/130
7,655,003 B2 * 2/2010 Lorang et al. 606/32
2011/0118729 A1 * 5/2011 Heeren et al. 606/41
2011/0282340 A1 * 11/2011 Toth et al. 606/33

* cited by examiner

Primary Examiner — Wan Laymon

(74) *Attorney, Agent, or Firm* — Birch, Stewart, Kolasch & Birch, LLP

(57) **CLAIM**


The ornamental design for an electrode needle for high-frequency therapy equipment, as shown and described.

DESCRIPTION

FIG. 1 is a front elevational view of a electrode needle for high-frequency therapy equipment showing my new design, the rear view being symmetrical thereto;
FIG. 2 is a right side elevational view thereof;
FIG. 3 is left side elevational view thereof;
FIG. 4 is a top plan view thereof, the bottom view being symmetrical thereto;
FIG. 5 is an enlarged front elevational view thereof;
FIG. 6 is an enlarged left side elevational view thereof; and,
FIG. 7 is a reference drawing showing the use state of the invention.

The broken lines shown in FIGS. 1, 2, 4 and 7 represent portions of the electrode needle for high-frequency therapy equipment that form no part of the claimed design.

1 Claim, 4 Drawing Sheets

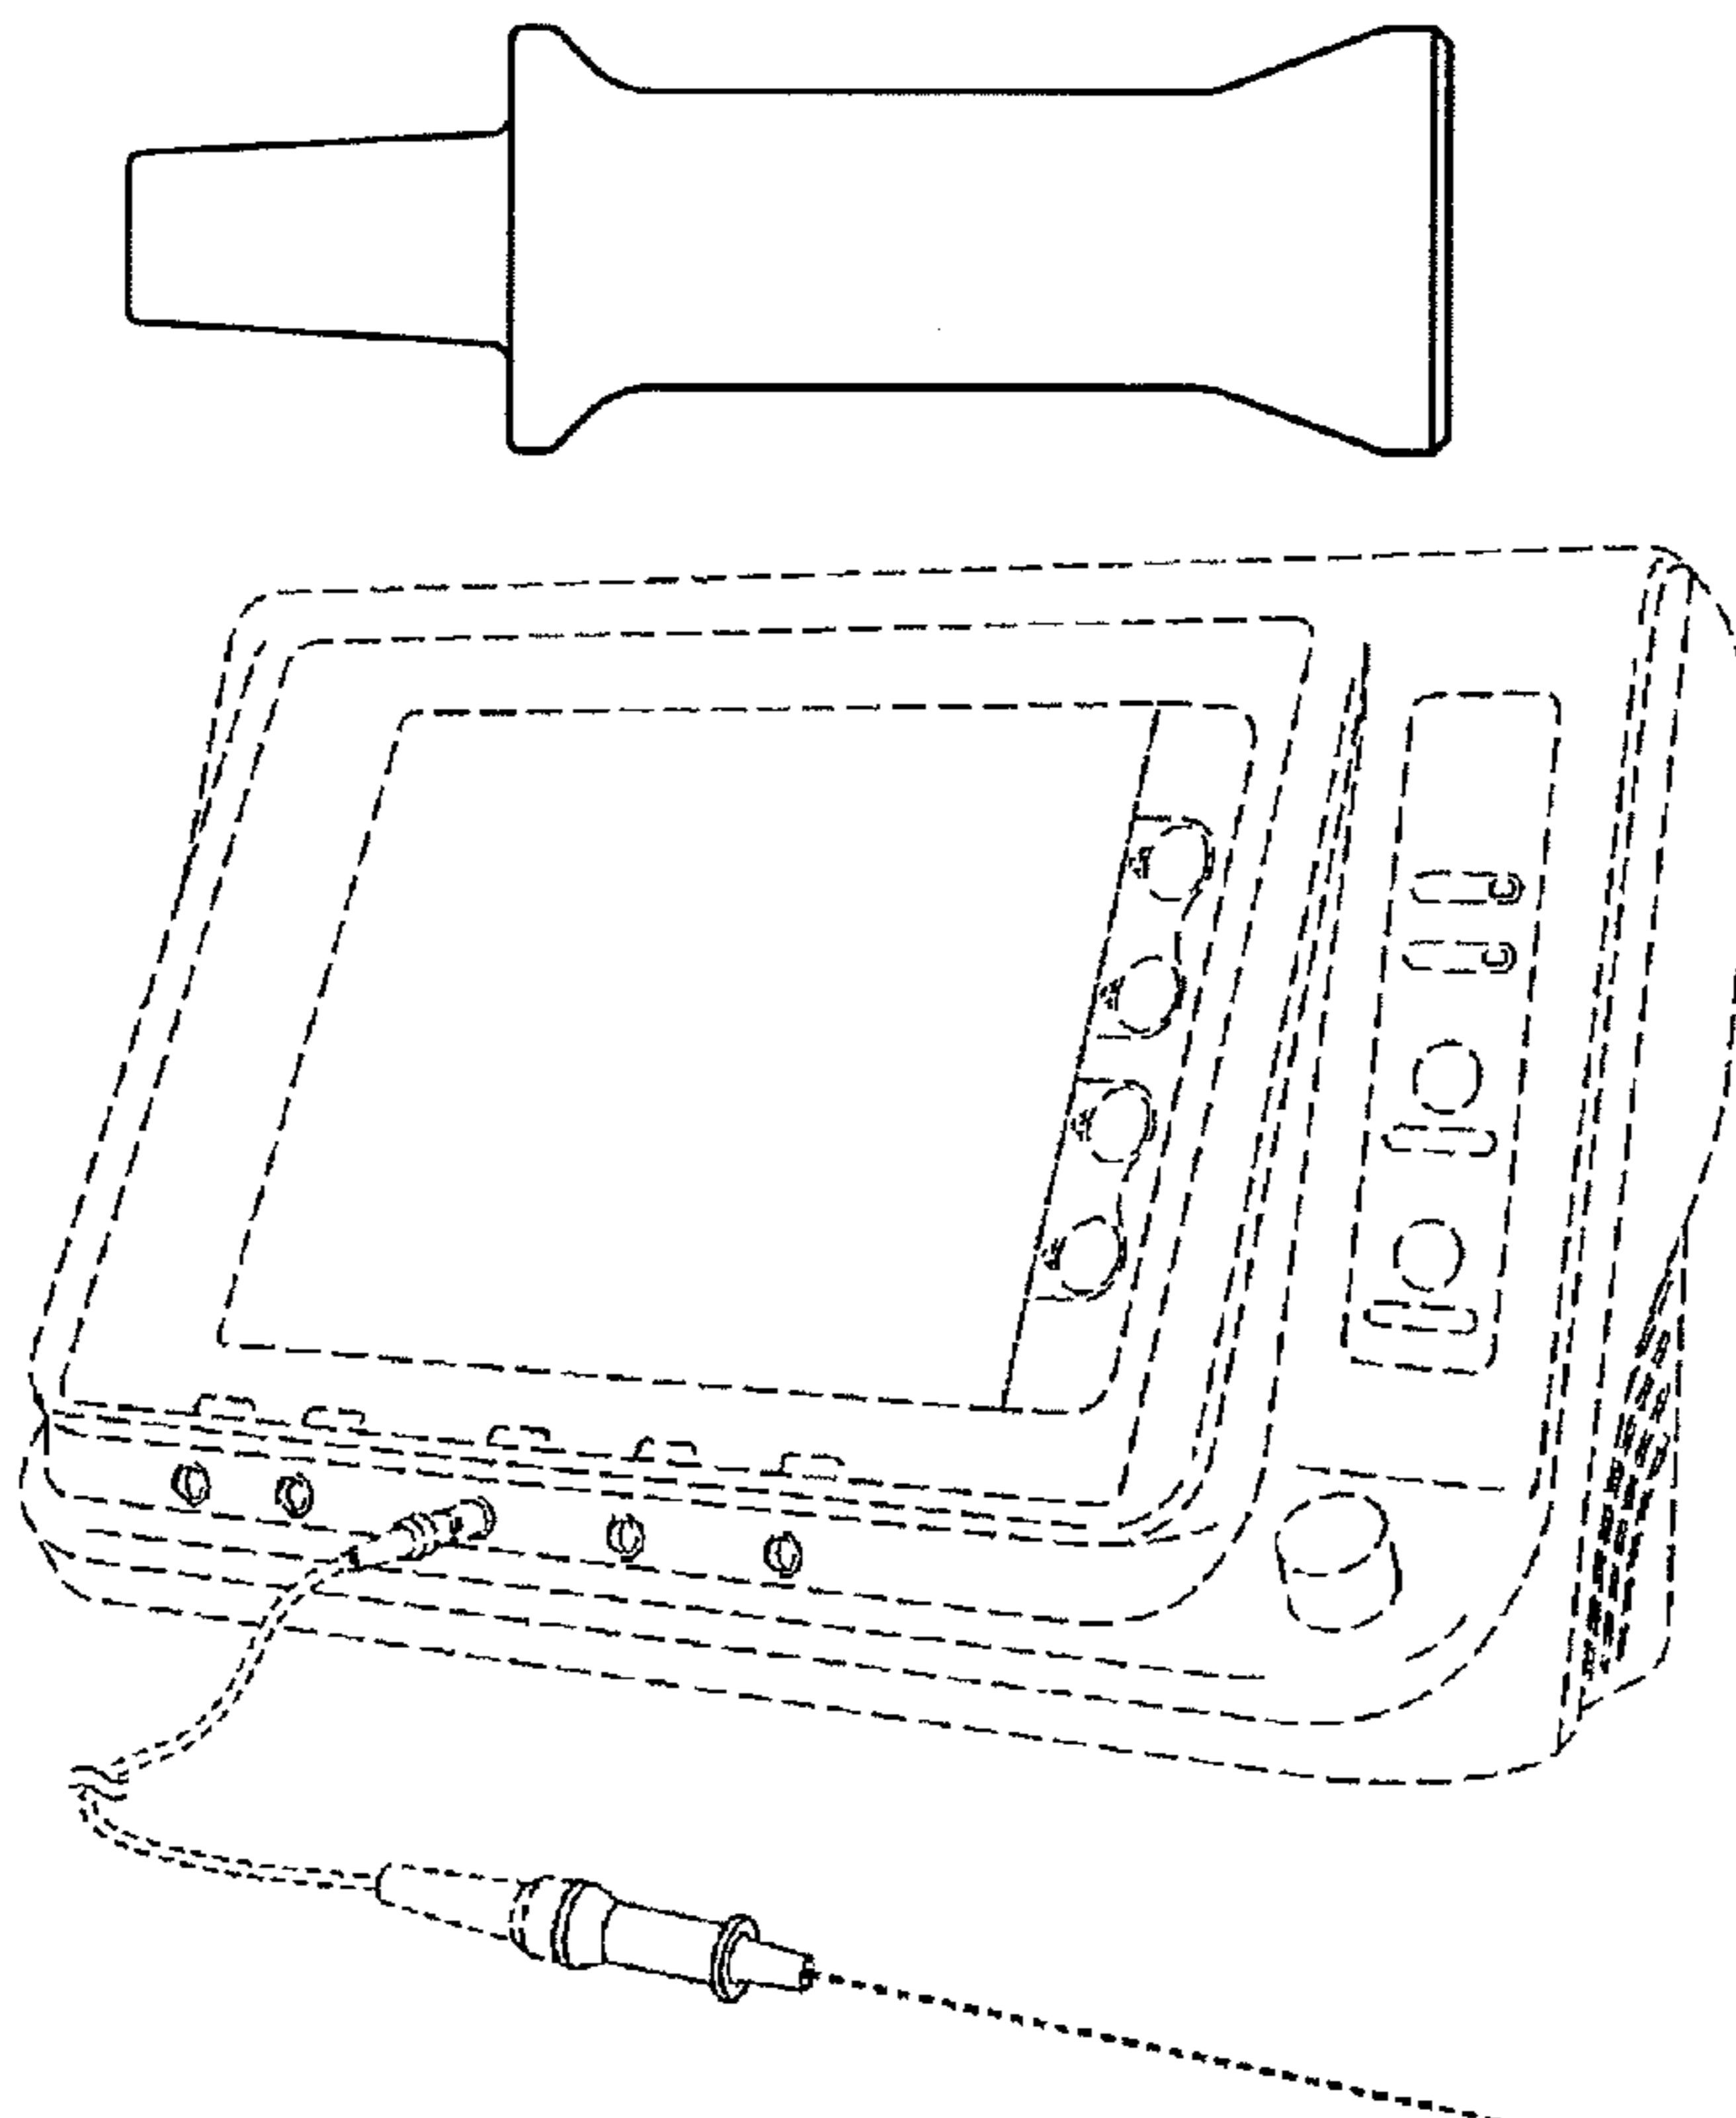

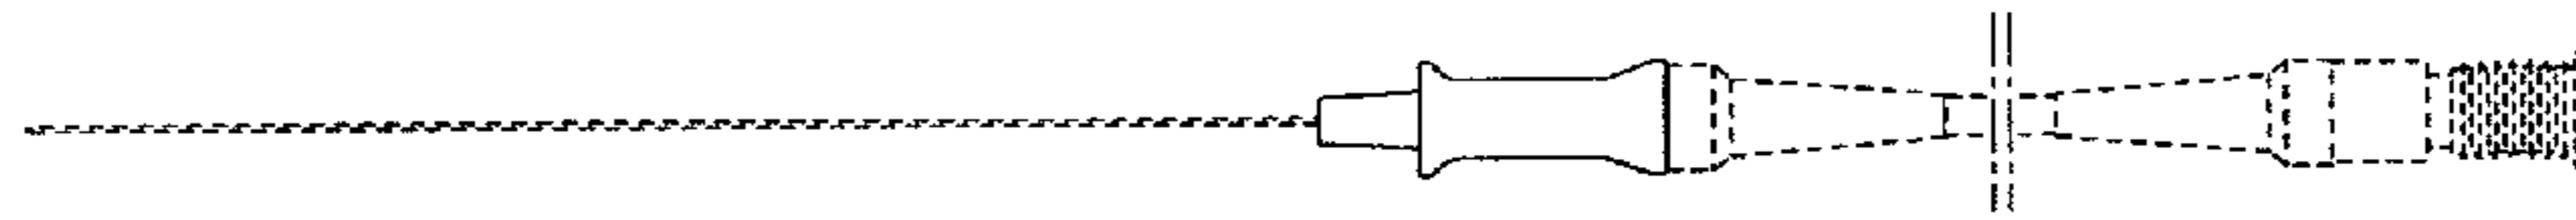


FIG. 1



FIG. 2



FIG. 3



FIG. 4

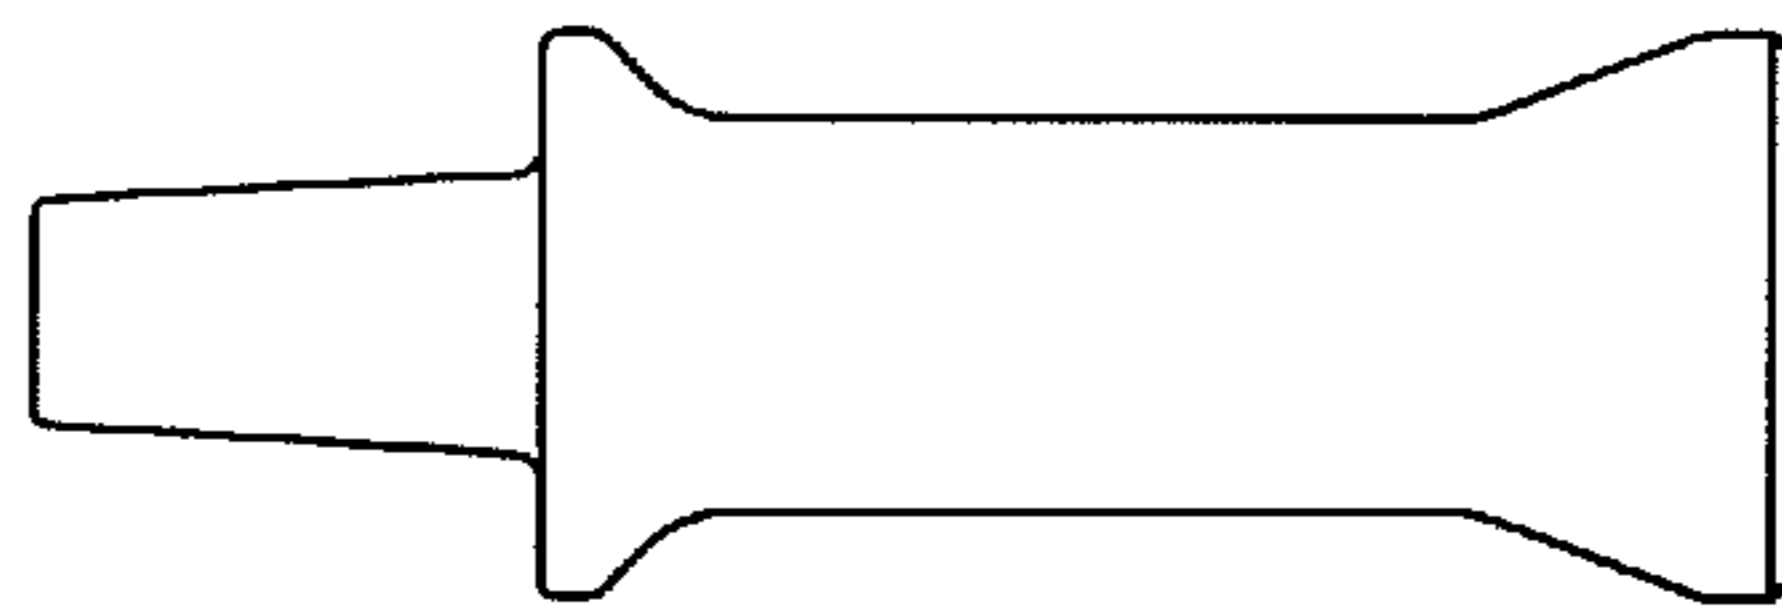


FIG. 5

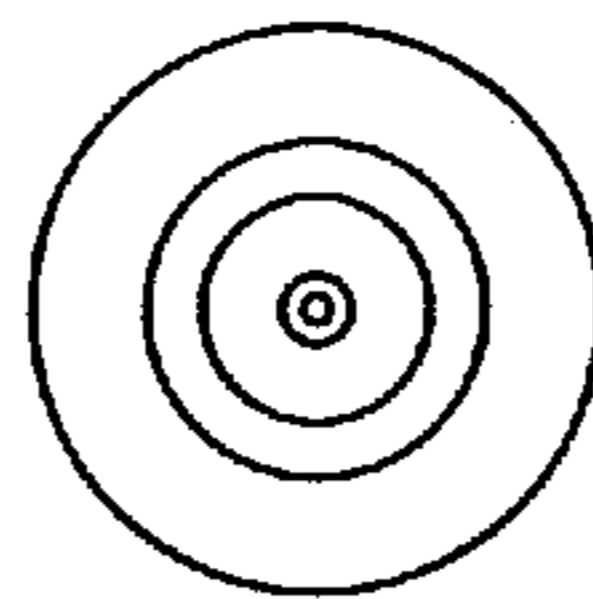


FIG. 6

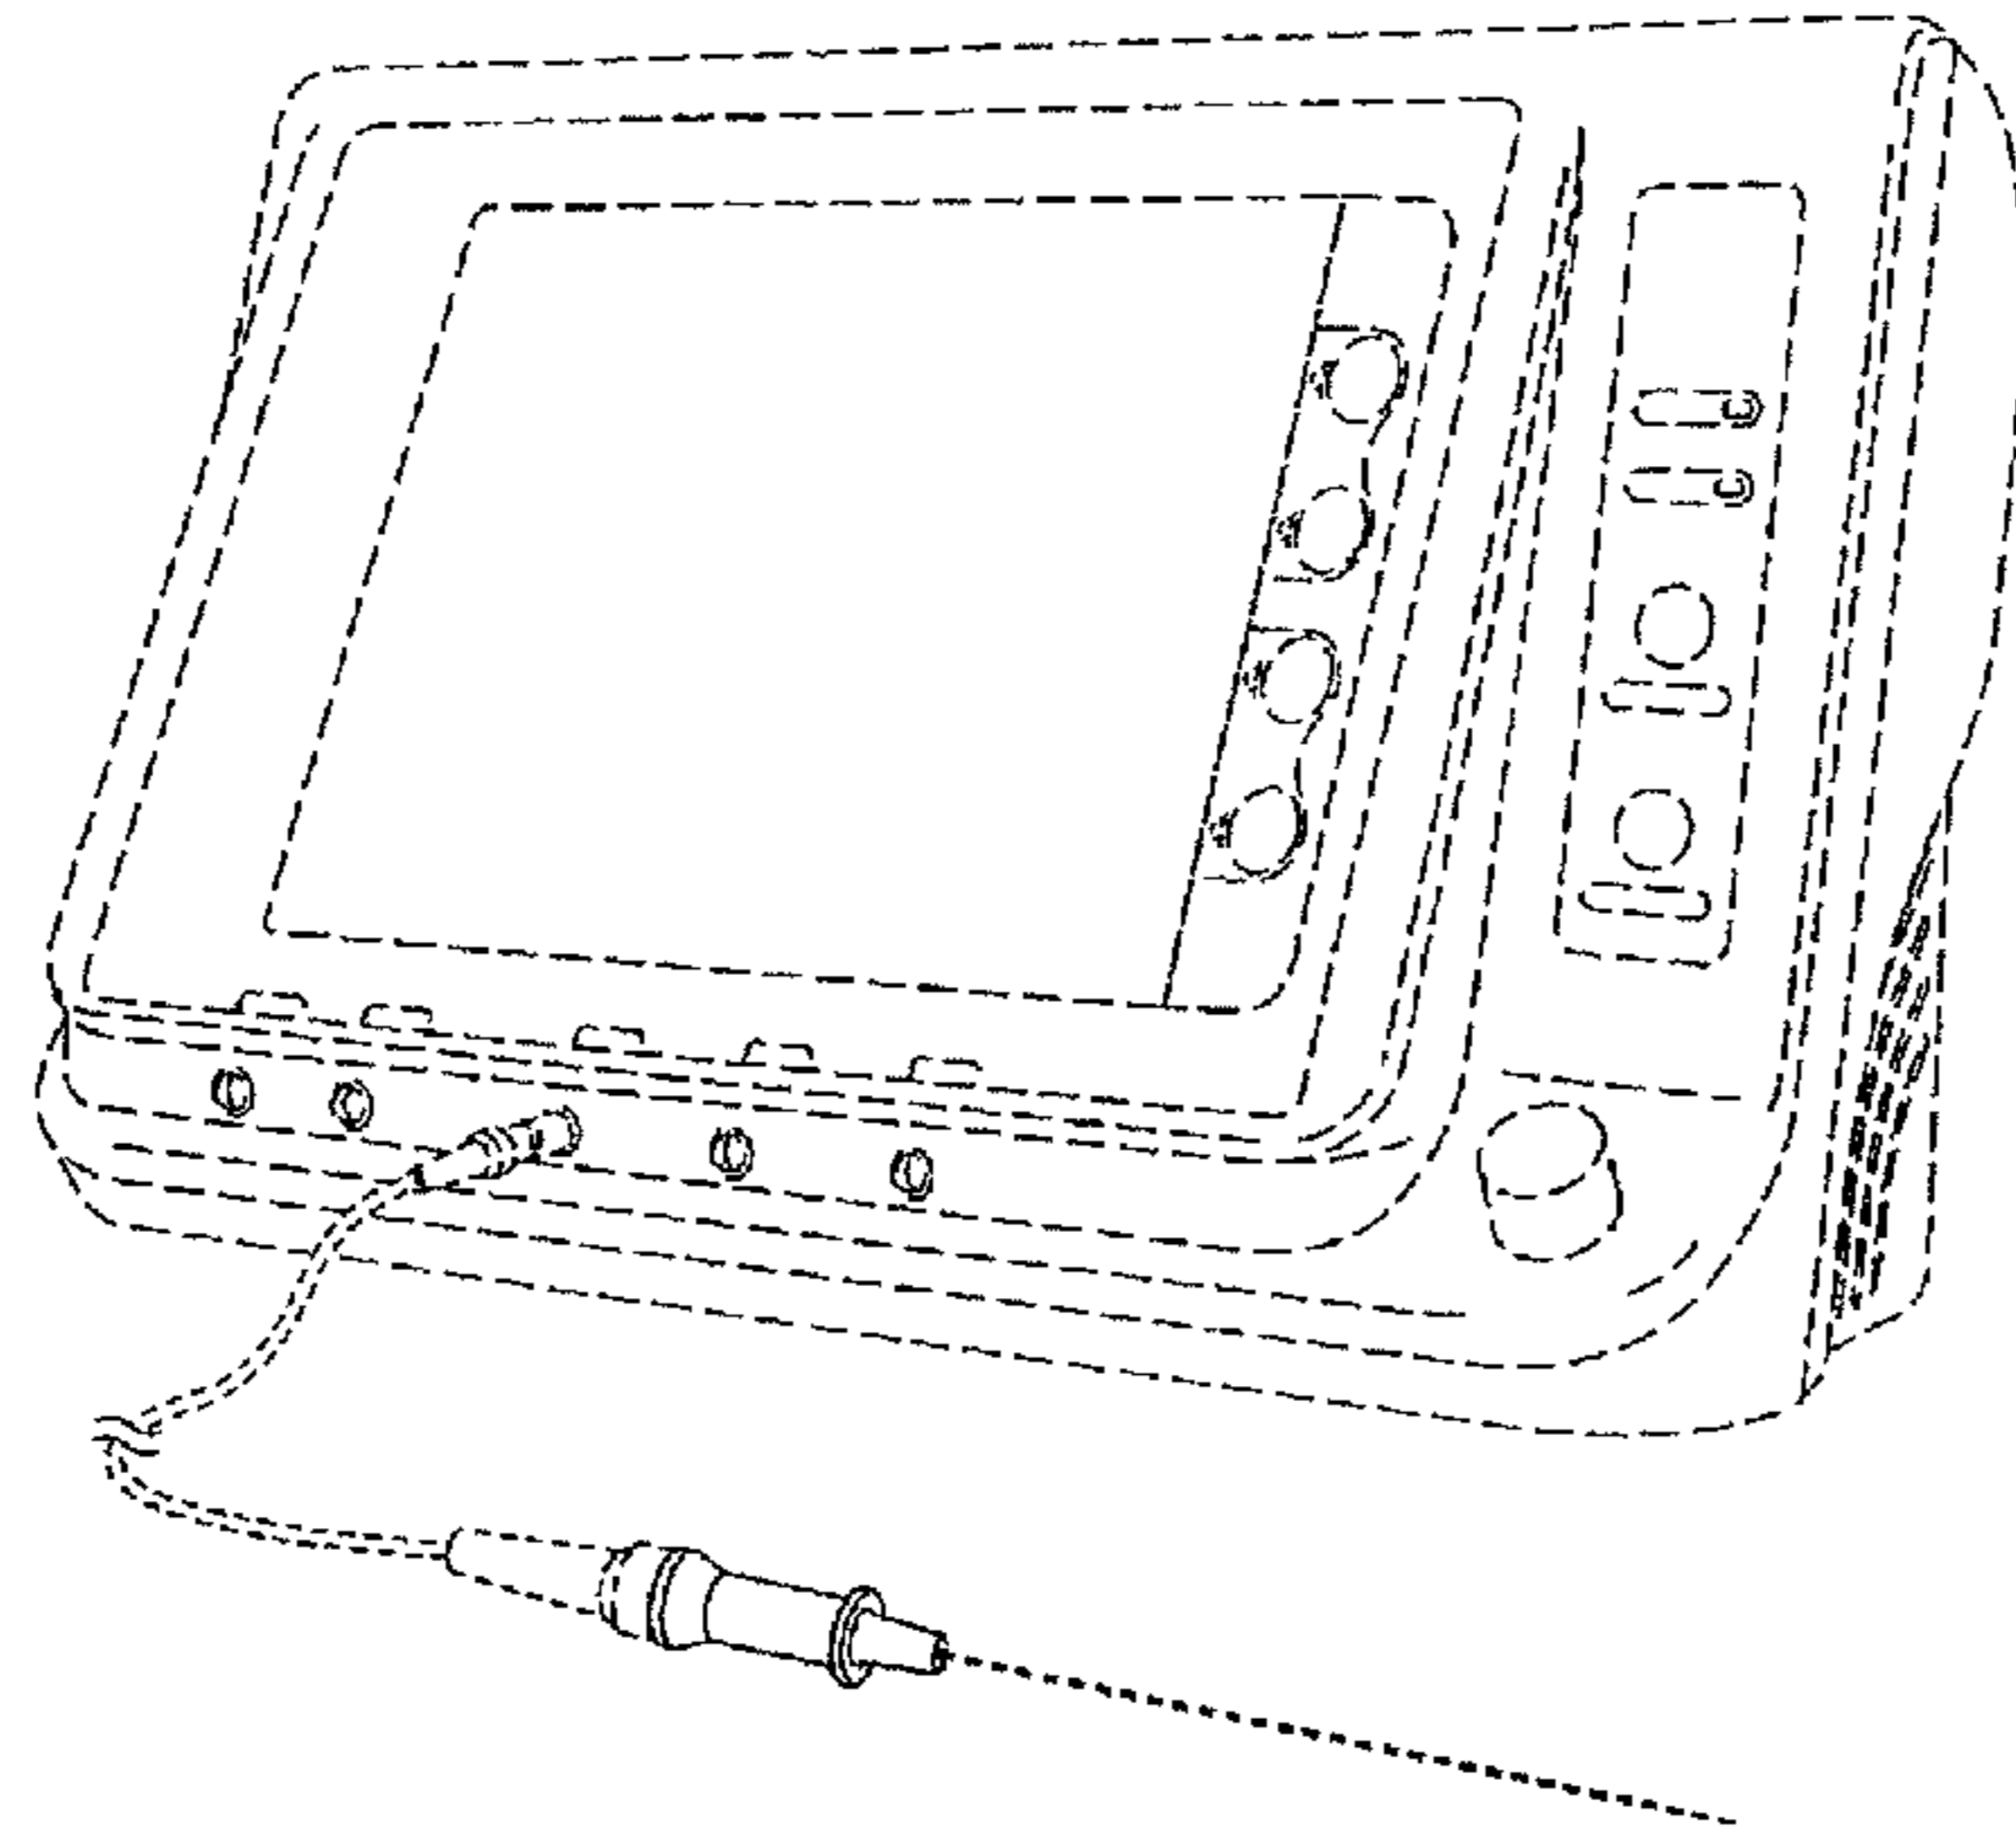


FIG. 7