



US00D670811S

(12) **United States Design Patent**
Fukuzawa

(10) **Patent No.:** **US D670,811 S**

(45) **Date of Patent:** **** Nov. 13, 2012**

(54) **BLOOD GLUCOSE LEVEL MEASURING
DEVICE**

7,841,993 B2 * 11/2010 Kojima et al. 600/583
D633,814 S * 3/2011 Nishiyama D10/81
2011/0034786 A1 * 2/2011 Cadio et al. 600/316

(75) Inventor: **Masahiro Fukuzawa**, Kyoto (JP)

(73) Assignee: **Arkray, Inc.** (JP)

(**) Term: **14 Years**

(21) Appl. No.: **29/387,702**

(22) Filed: **Mar. 16, 2011**

(30) **Foreign Application Priority Data**

Sep. 17, 2010 (JP) 2010-022513

(51) **LOC (9) Cl.** **24-01**

(52) **U.S. Cl.** **D24/169**

(58) **Field of Classification Search** D24/165-169,
D24/107, 186, 216, 223, 231, 232; D10/46,
D10/81; D14/341; 422/56, 58, 68.1; 600/316,
600/322, 347, 365, 368

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D406,895 S *	3/1999	Byrd et al.	D24/169
D499,805 S *	12/2004	D'Agostino	D24/169
D545,438 S *	6/2007	Huang et al.	D24/186
D548,347 S *	8/2007	Ichino et al.	D24/186
D562,458 S *	2/2008	Padain	D24/169
D566,706 S *	4/2008	Andre et al.	D14/341
D581,056 S *	11/2008	Kurokawa et al.	D24/186
D590,063 S *	4/2009	Garthoff et al.	D24/186
D595,415 S *	6/2009	Fukuzawa	D24/186
D622,394 S *	8/2010	Bielawa et al.	D24/169

FOREIGN PATENT DOCUMENTS

JP	D1222984 S	11/2004
JP	D1328968 S	5/2008
JP	D1353862 S	3/2009
JP	D1355469 S	4/2009
JP	D1397613 S	9/2010

OTHER PUBLICATIONS

Explanation of U.S. Appl. No. 29/387,702.

* cited by examiner

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Studebaker & Brackett PC;
Donald R. Studebaker

(57) **CLAIM**

The ornamental design for a blood glucose level measuring device, as shown and described.

DESCRIPTION

FIG. 1 is a top perspective view of the blood glucose level measuring device;

FIG. 2 is a bottom perspective view thereof;

FIG. 3 is a top view thereof;

FIG. 4 is a bottom view thereof;

FIG. 5 is a left side view thereof;


FIG. 6 is a right side view thereof;

FIG. 7 is a front view thereof; and,

FIG. 8 is a rear view thereof.

The broken lines in the FIGS. 4 and 5 are included for the purpose of illustrating portions of the blood glucose level measuring device that form no part of the claimed design.

1 Claim, 8 Drawing Sheets

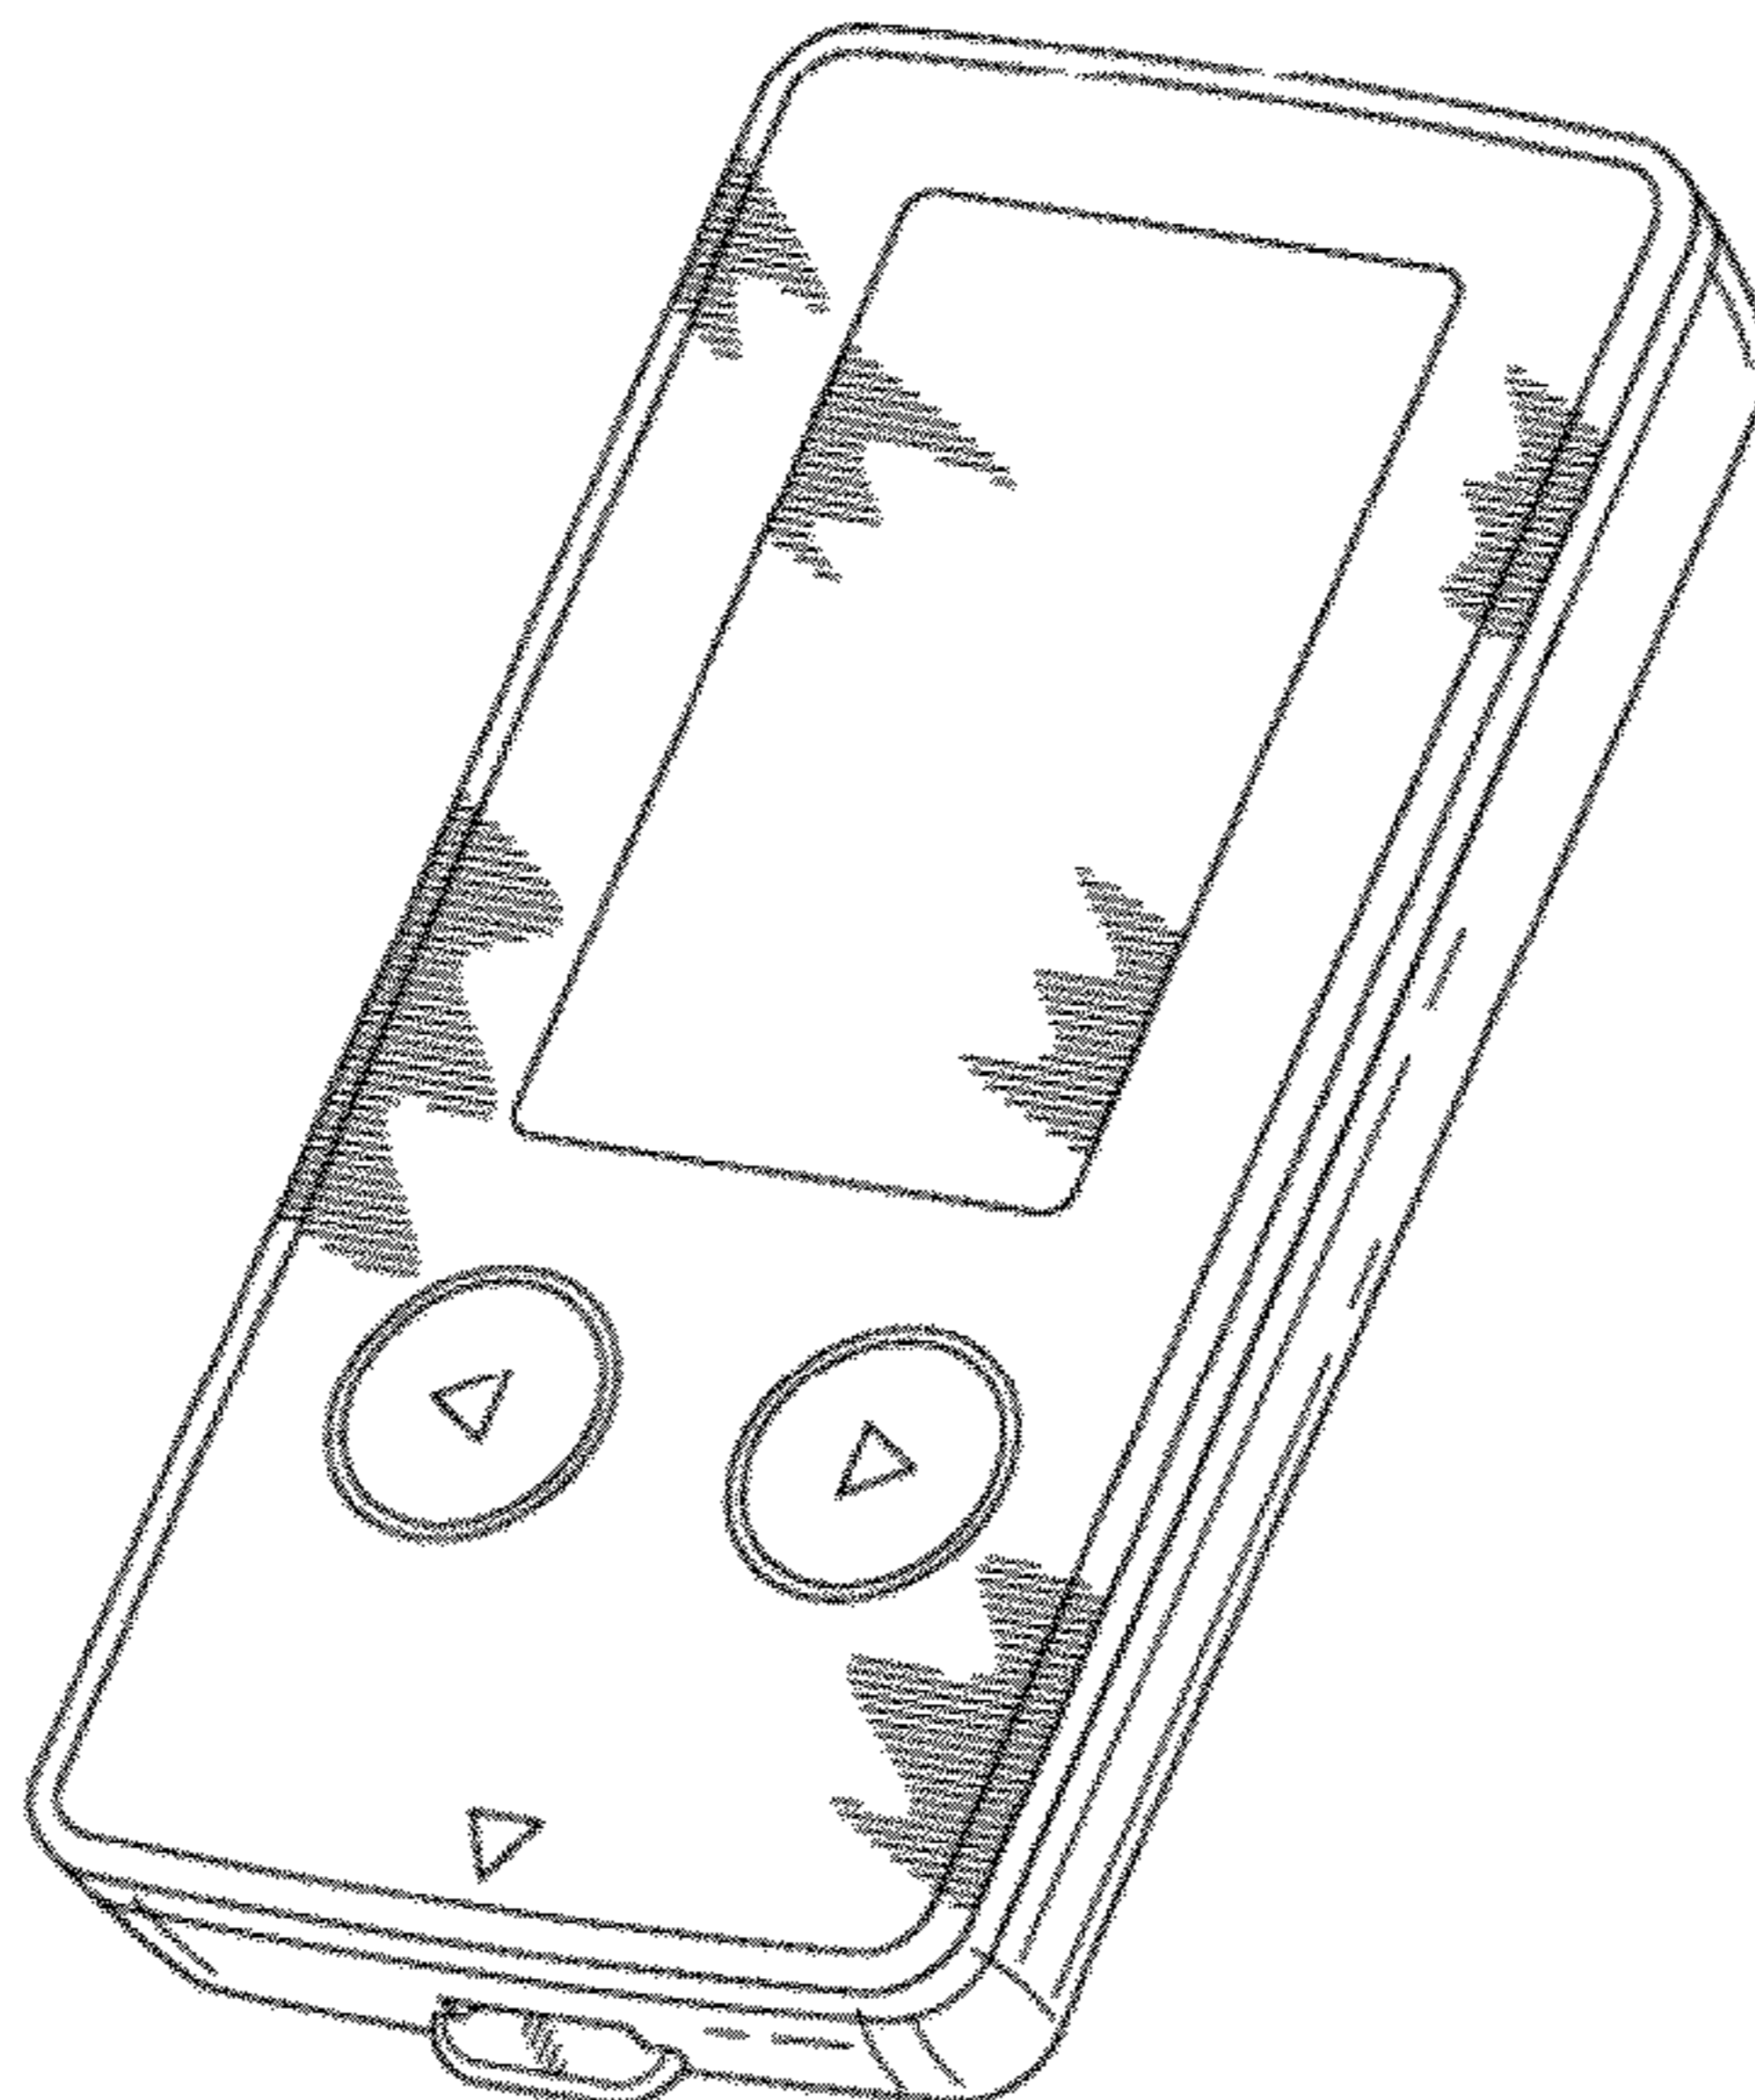

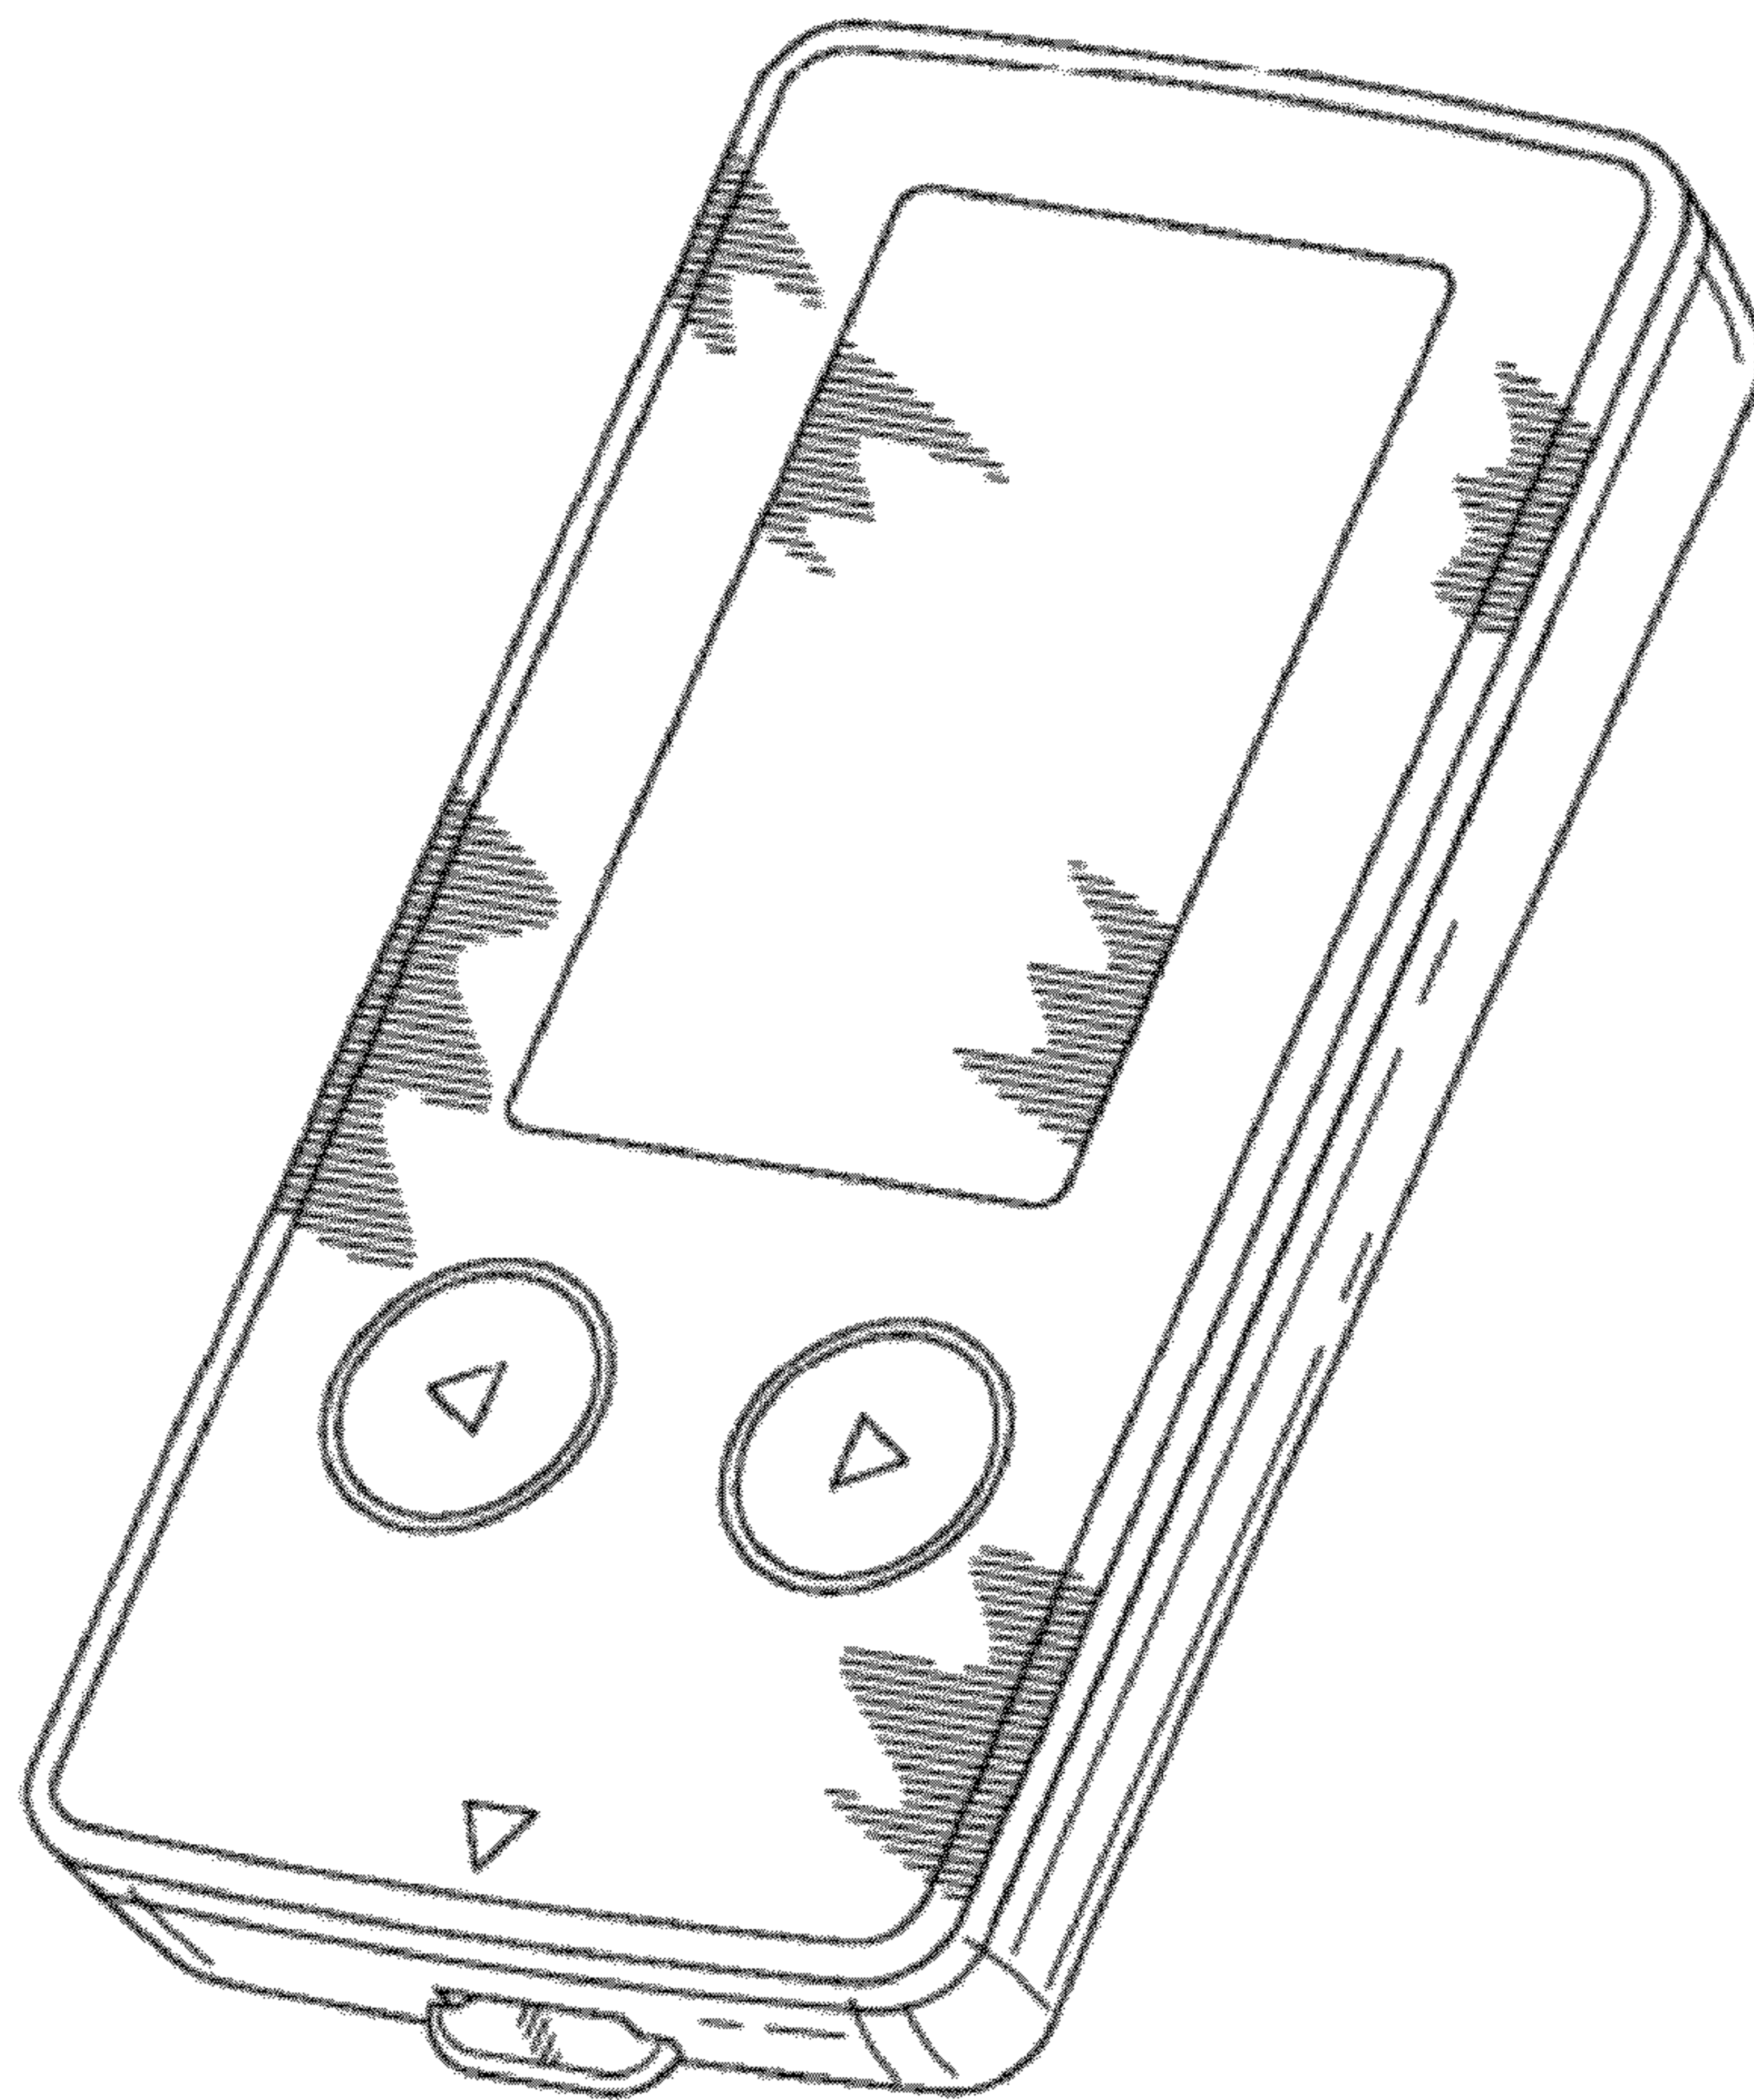


FIG. 1

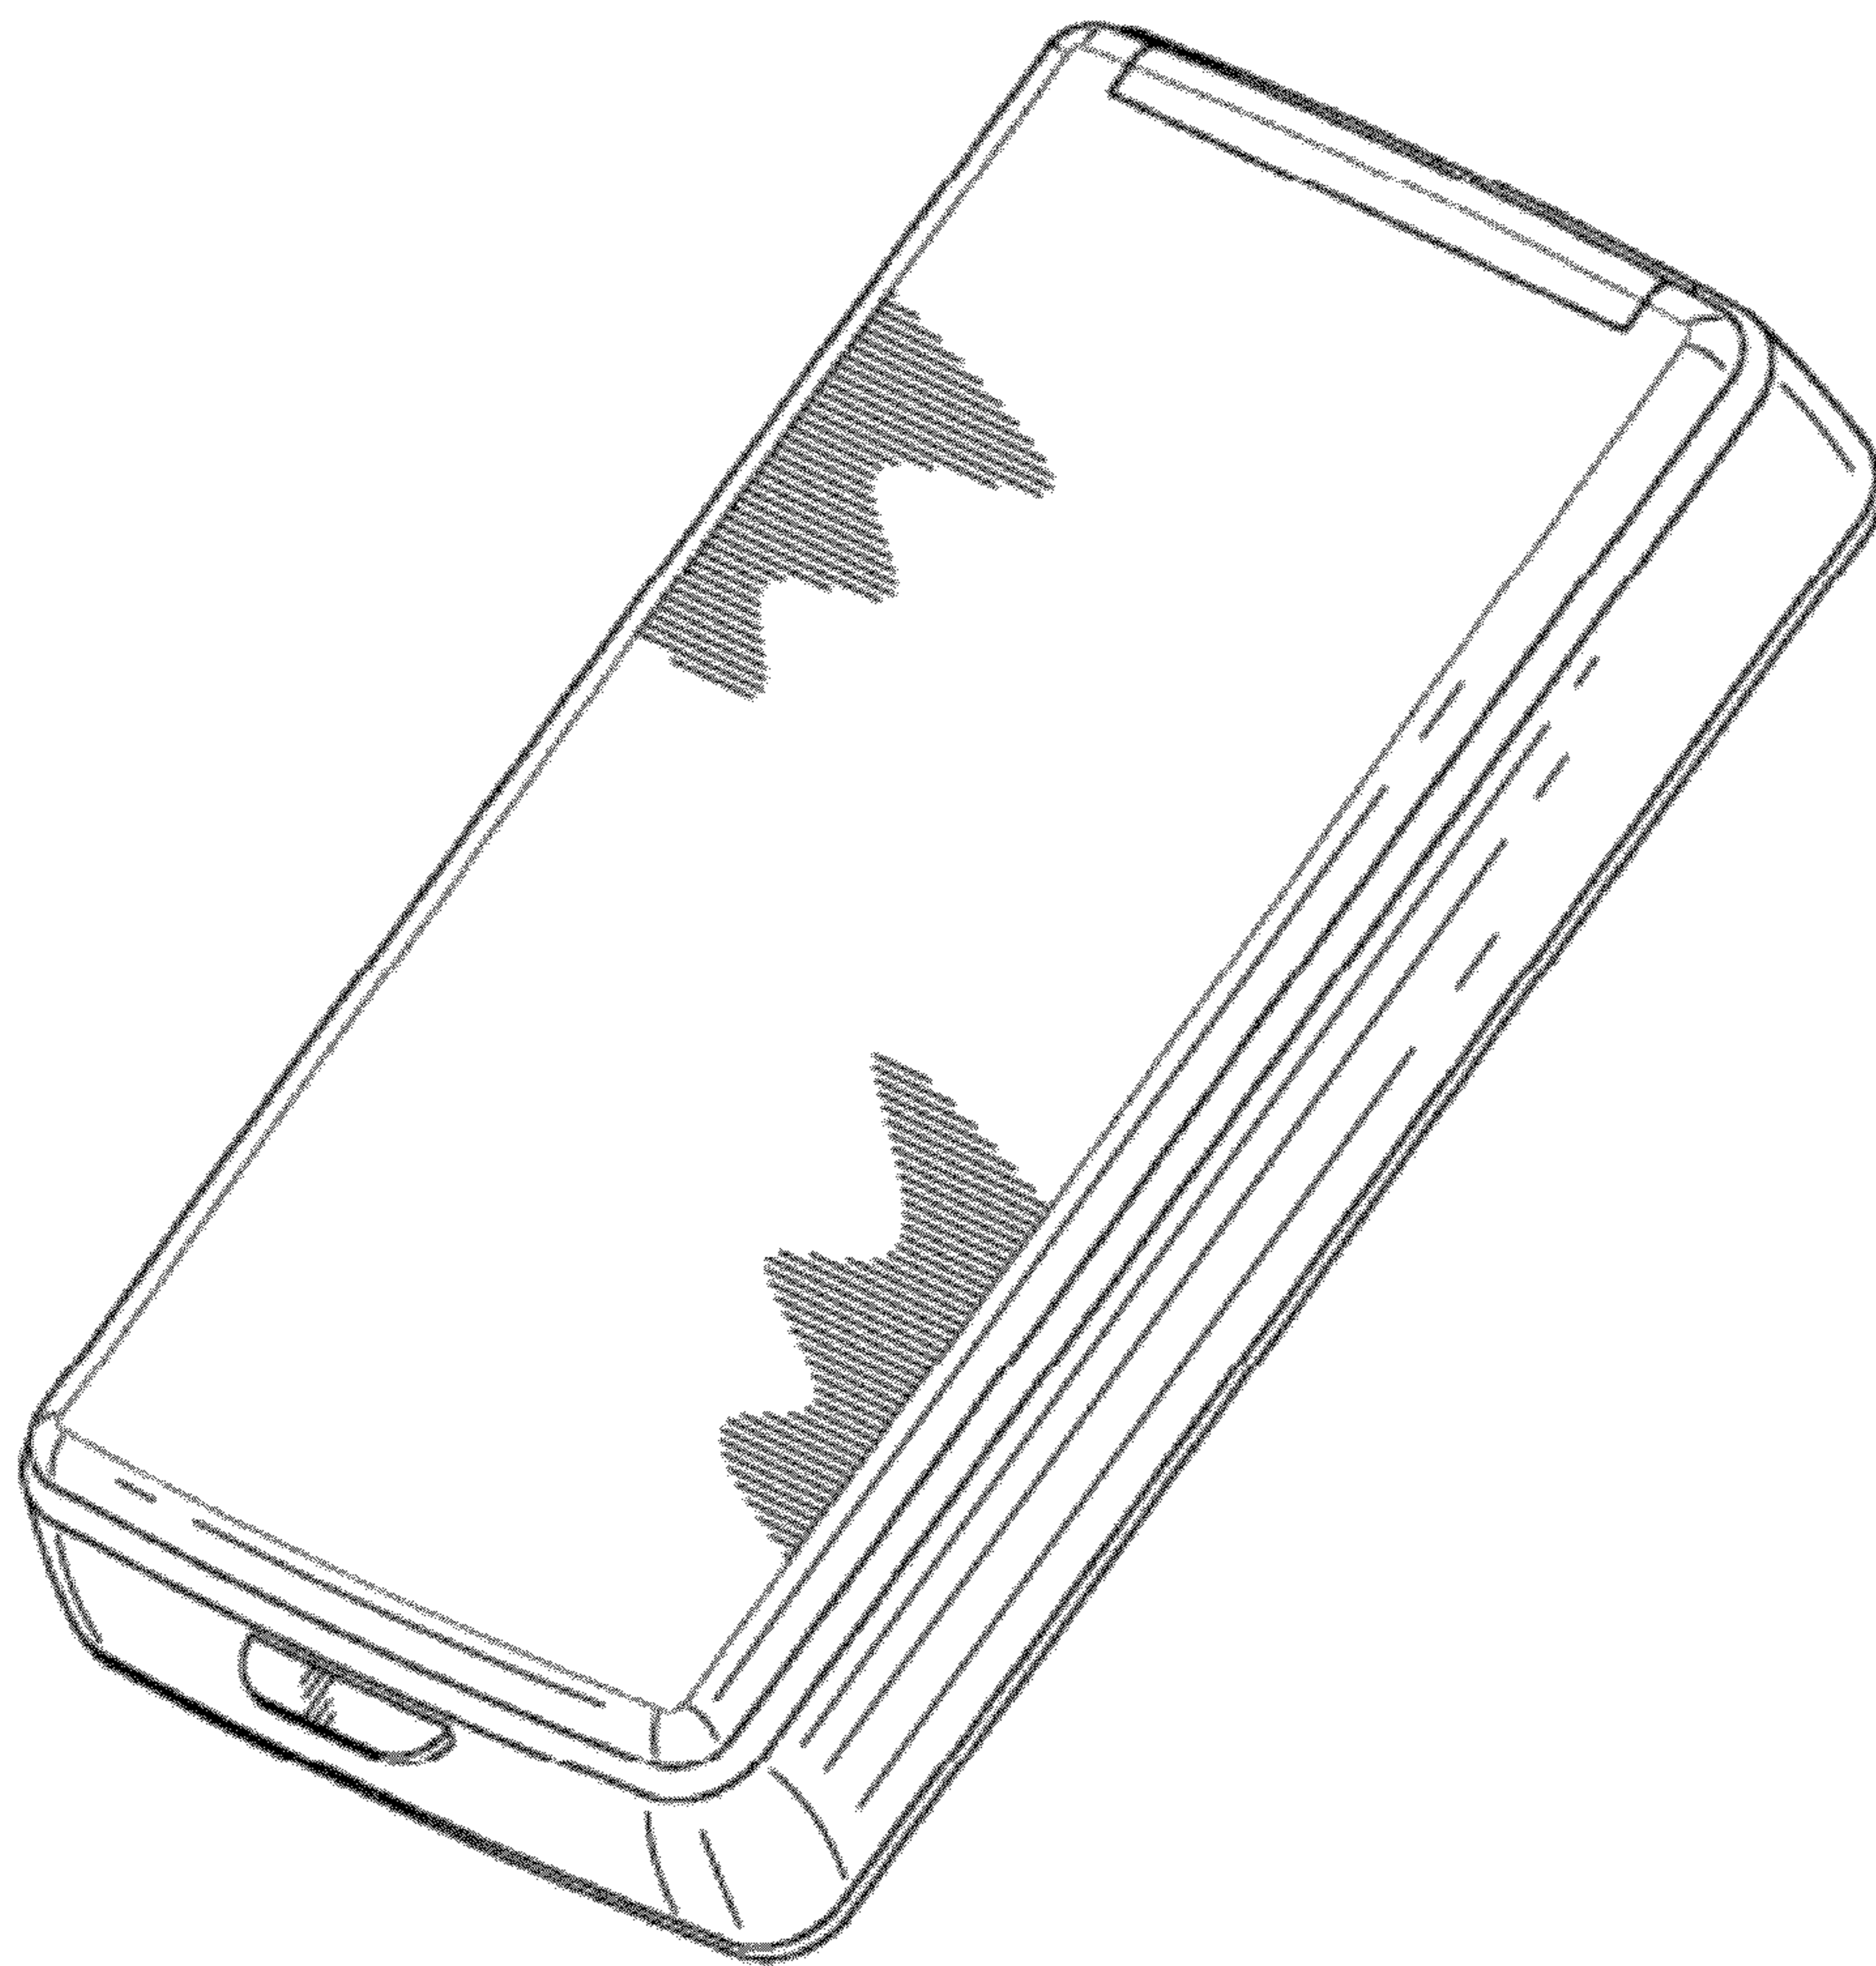


FIG. 2

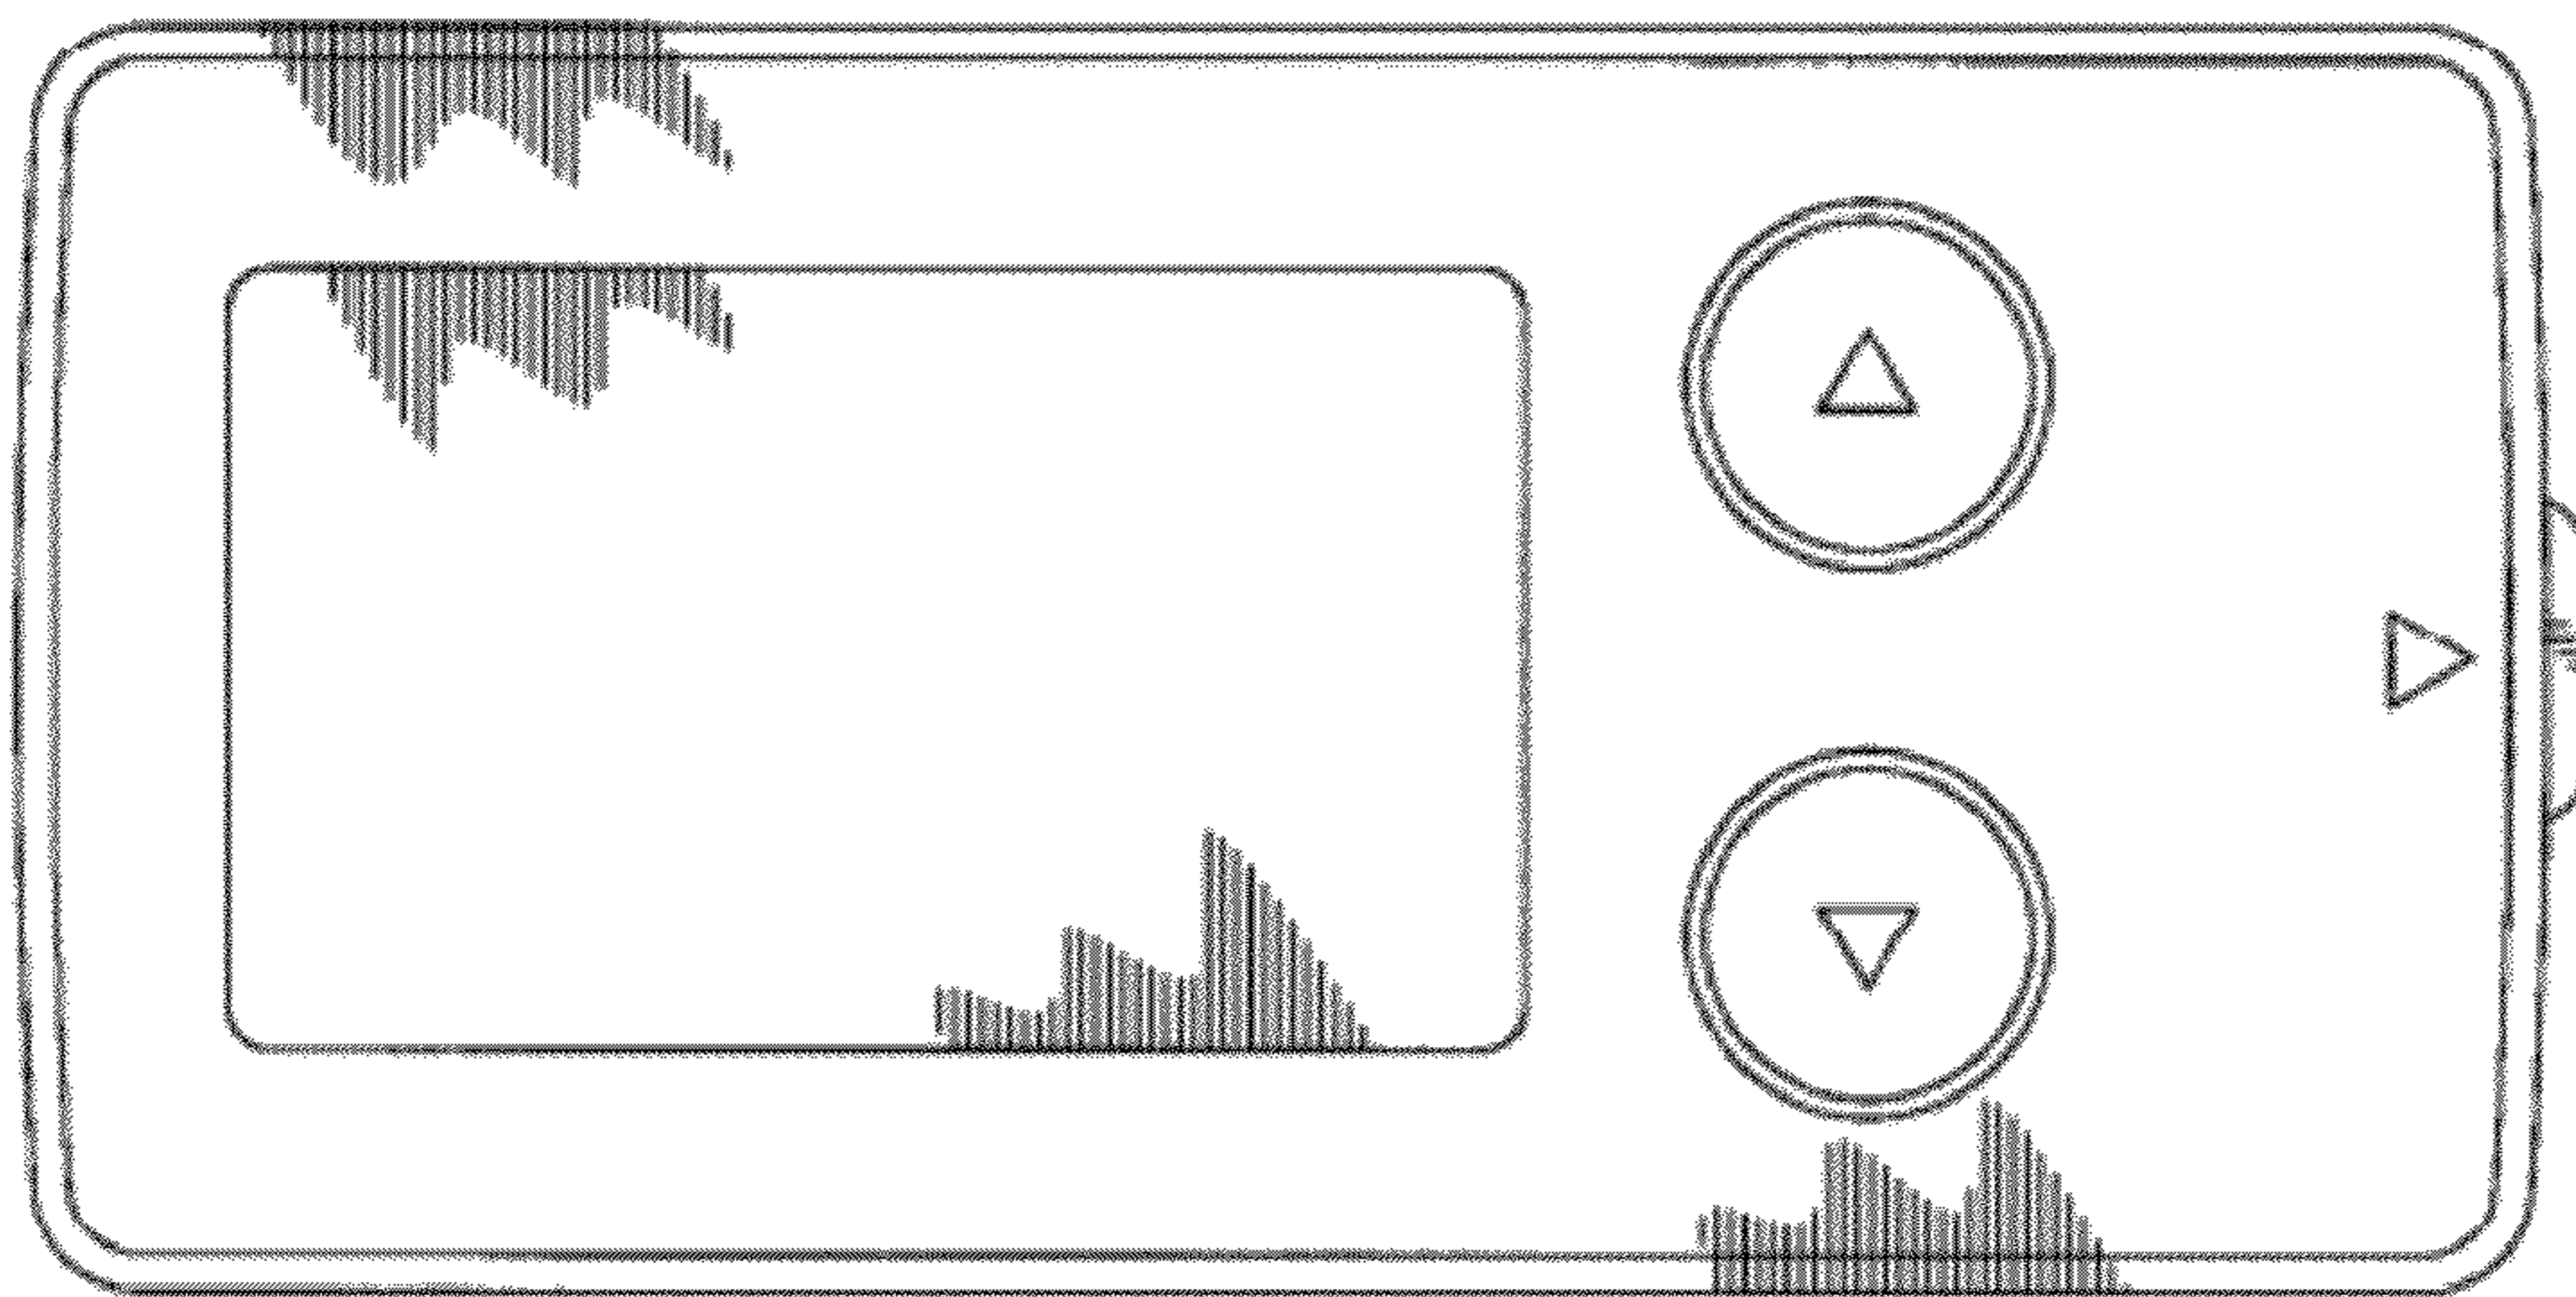


FIG. 3

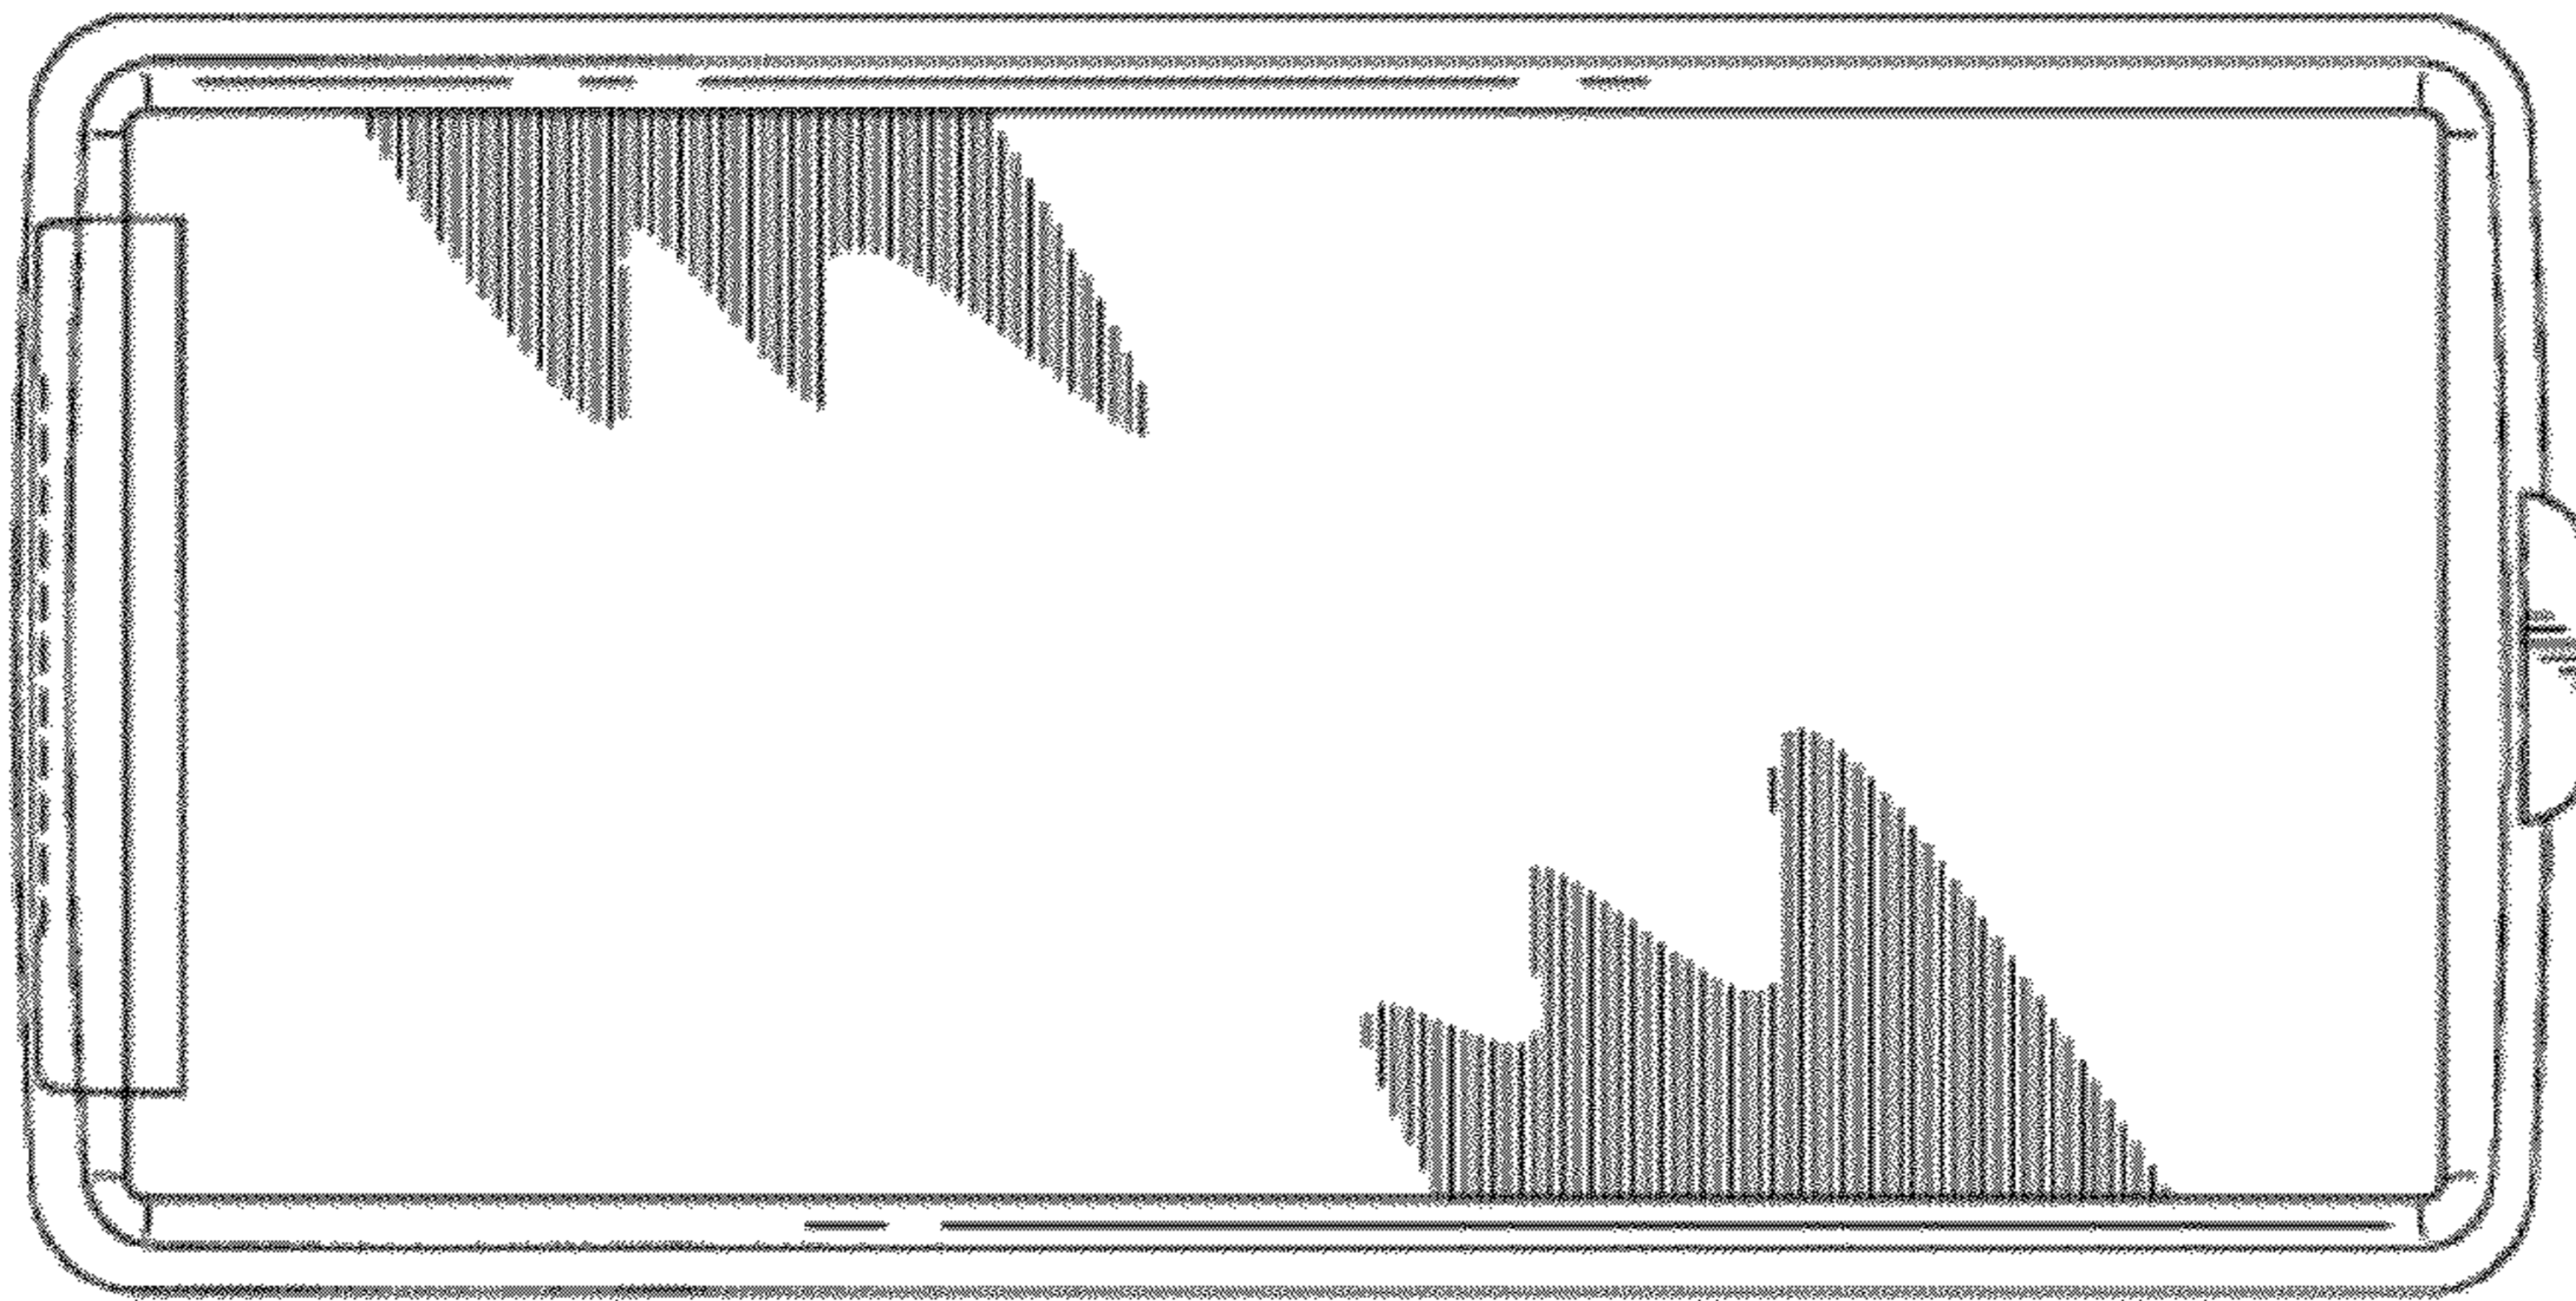


FIG. 4

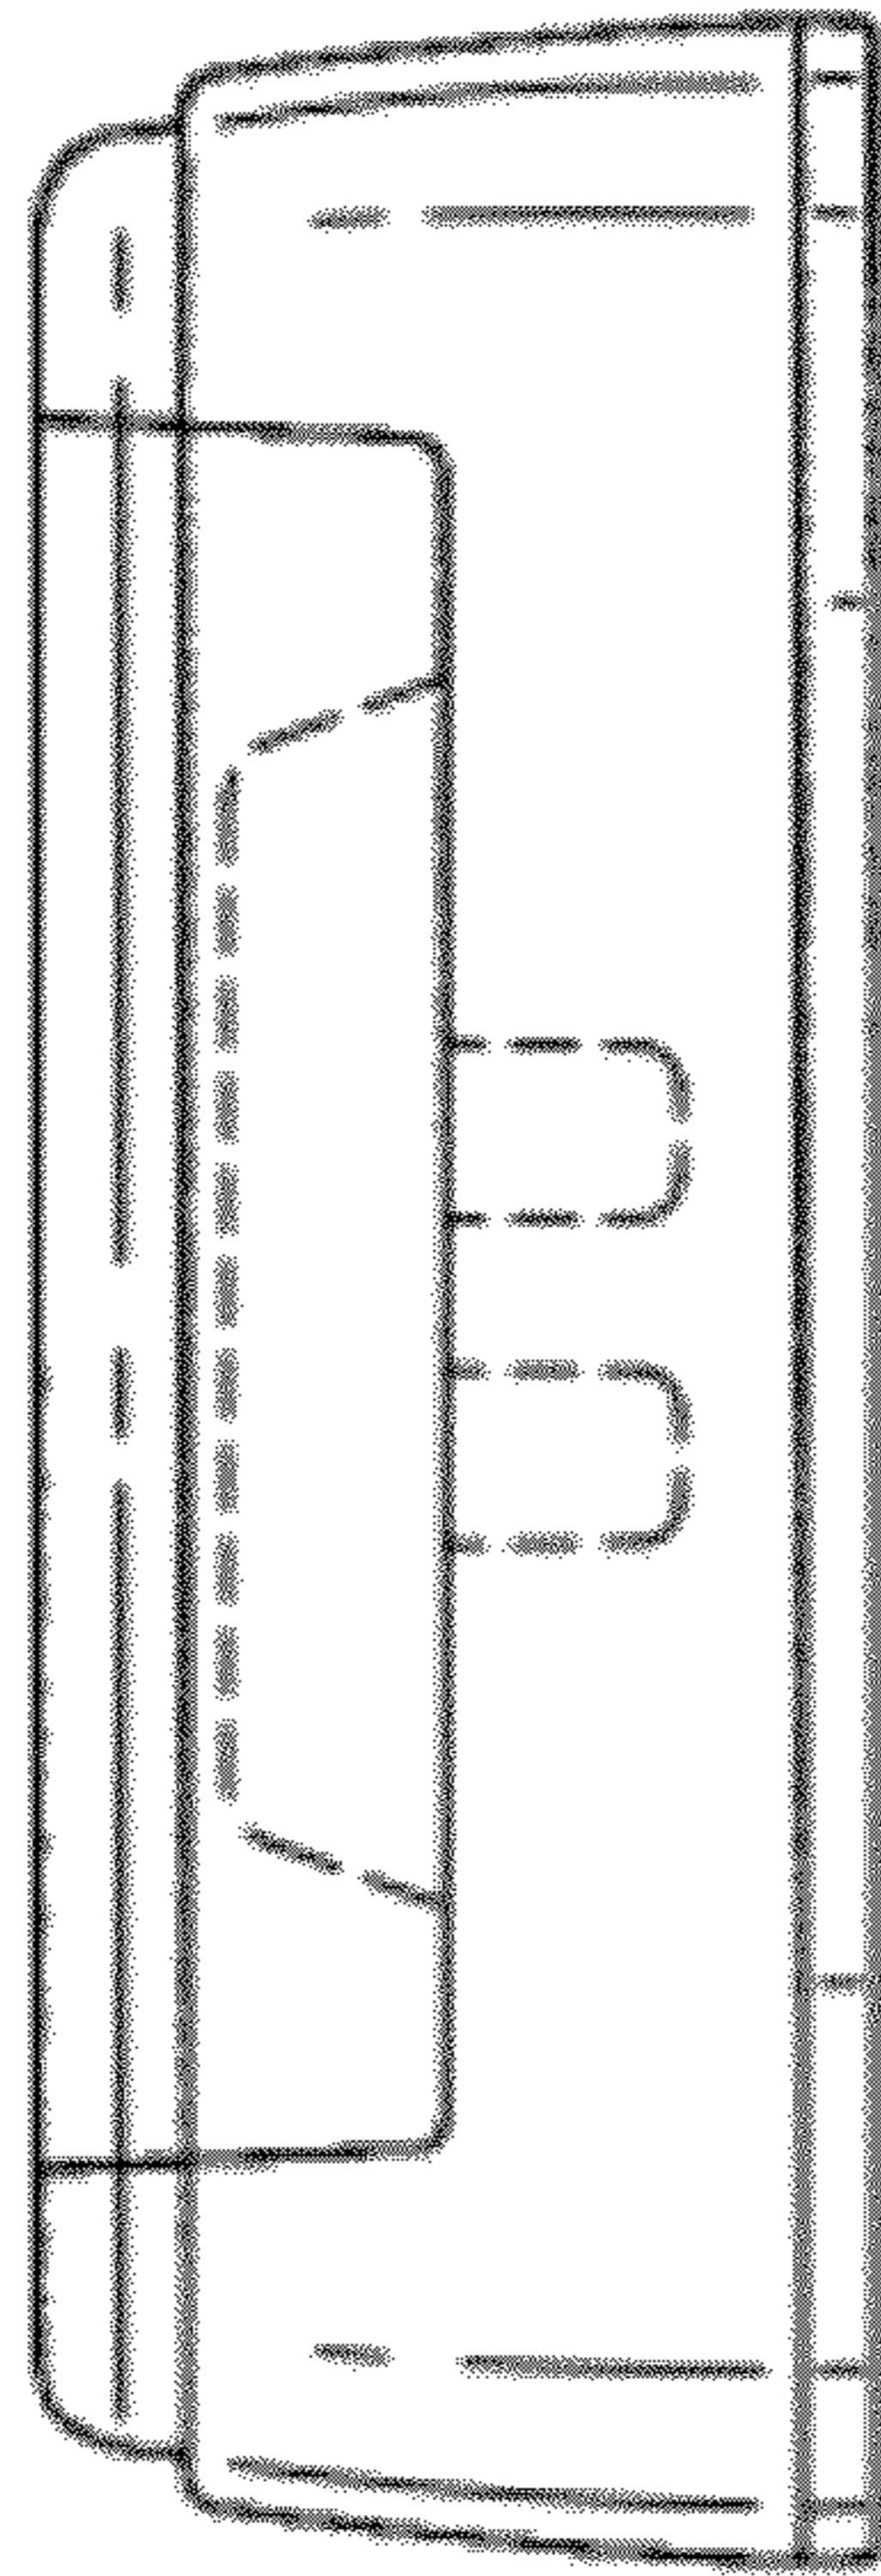


FIG. 5

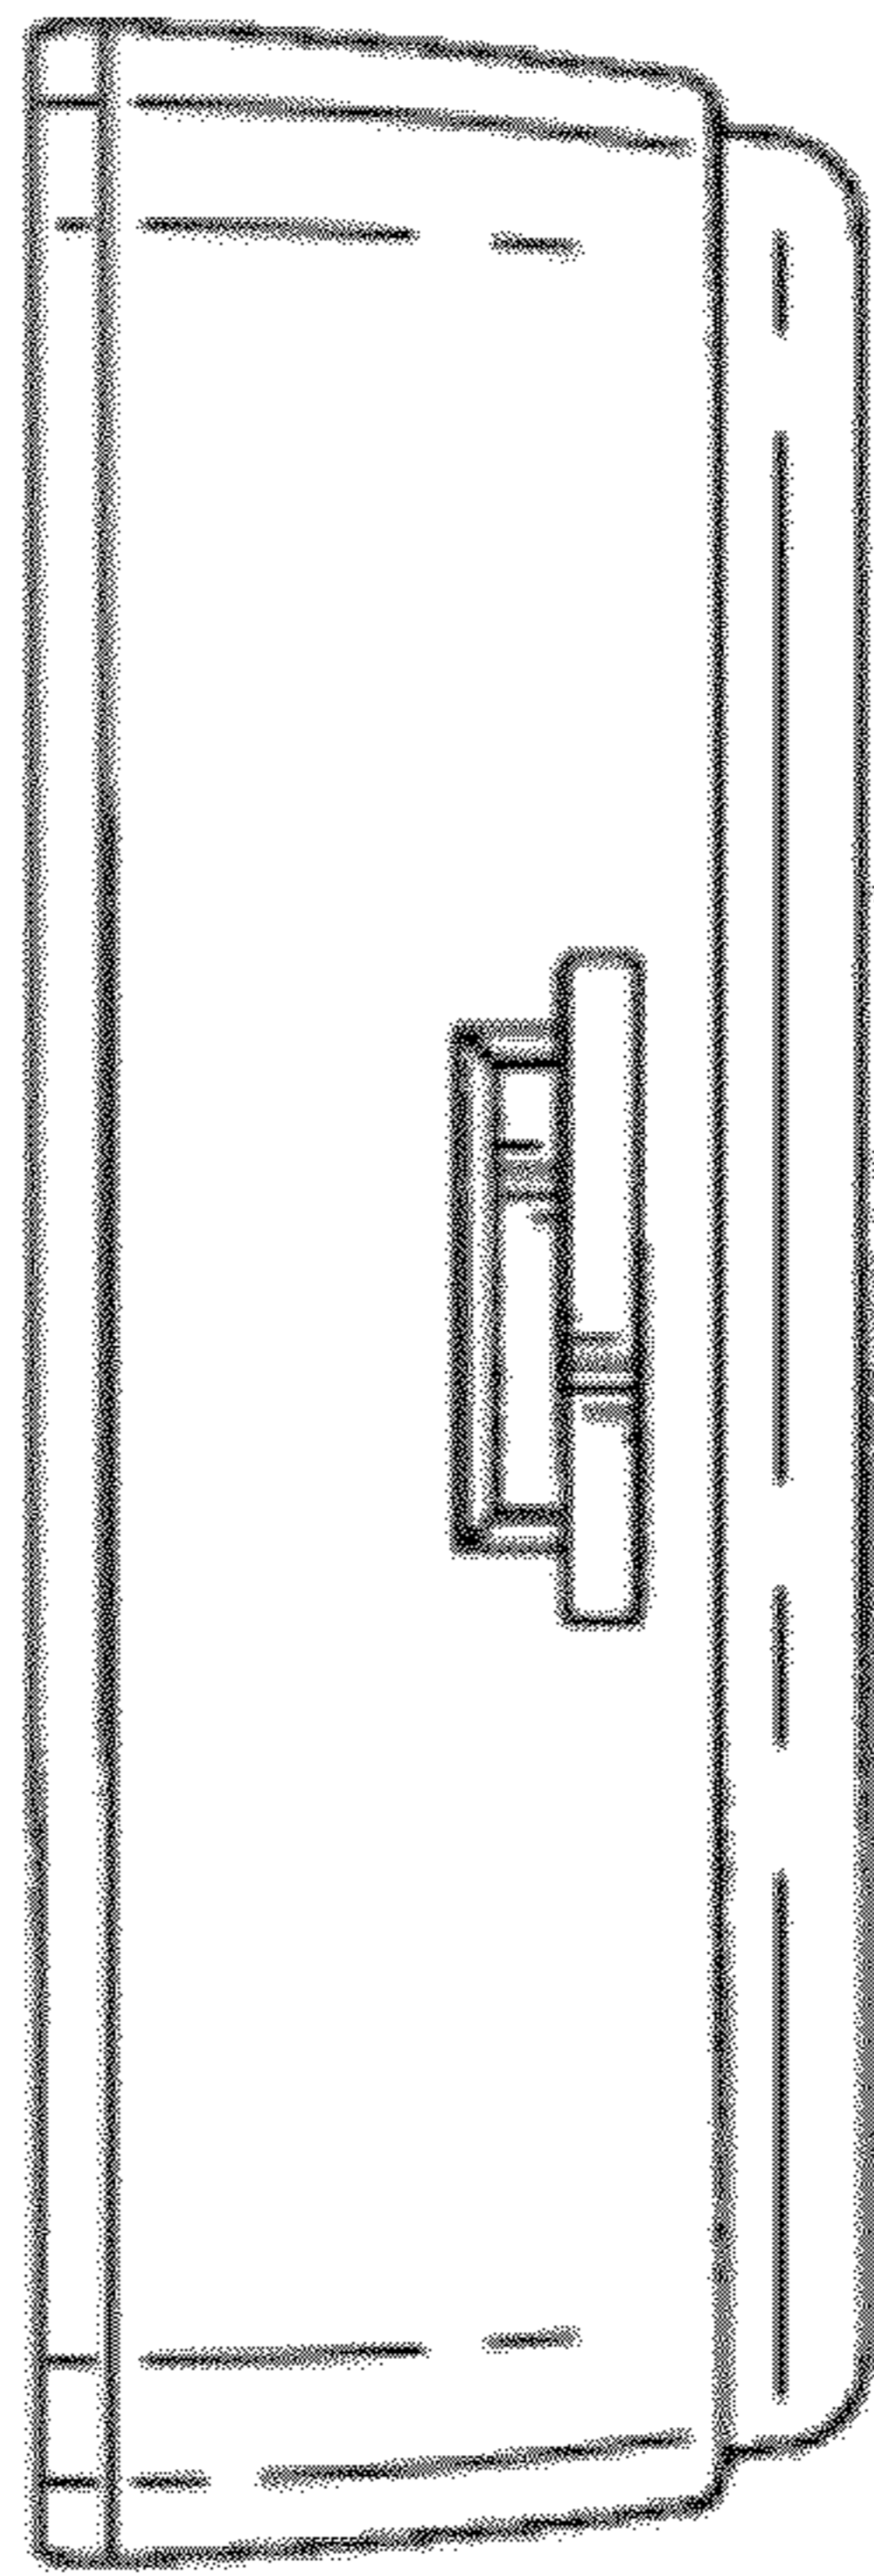


FIG. 6

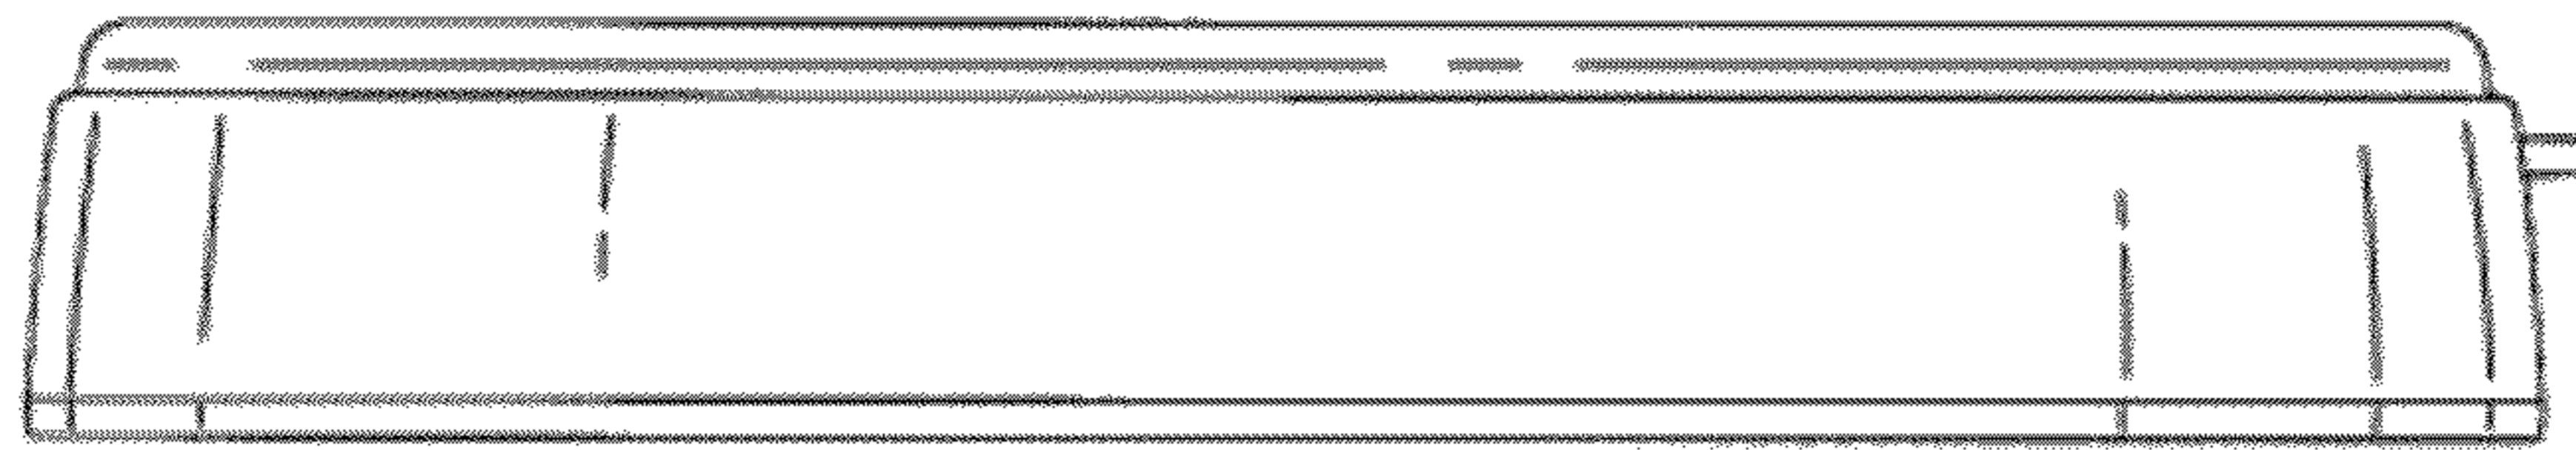


FIG. 7



FIG. 8