



US00D670811S

(12) **United States Design Patent**  
**Fukuzawa**

(10) **Patent No.:** **US D670,811 S**  
(45) **Date of Patent:** **\*\* Nov. 13, 2012**

(54) **BLOOD GLUCOSE LEVEL MEASURING DEVICE**

7,841,993 B2 \* 11/2010 Kojima et al. .... 600/583  
D633,814 S \* 3/2011 Nishiyama ..... D10/81  
2011/0034786 A1 \* 2/2011 Cadio et al. .... 600/316

(75) Inventor: **Masahiro Fukuzawa, Kyoto (JP)**

**FOREIGN PATENT DOCUMENTS**

(73) Assignee: **Arkray, Inc. (JP)**

JP D1222984 S 11/2004  
JP D1328968 S 5/2008  
JP D1353862 S 3/2009  
JP D1355469 S 4/2009  
JP D1397613 S 9/2010

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/387,702**

**OTHER PUBLICATIONS**

(22) Filed: **Mar. 16, 2011**

Explanation of U.S. Appl. No. 29/387,702.

(30) **Foreign Application Priority Data**

\* cited by examiner

Sep. 17, 2010 (JP) ..... 2010-022513

*Primary Examiner* — Anhdao Doan

(51) **LOC (9) Cl.** ..... **24-01**

(74) *Attorney, Agent, or Firm* — Studebaker & Brackett PC;  
Donald R. Studebaker

(52) **U.S. Cl.** ..... **D24/169**

(58) **Field of Classification Search** ..... D24/165–169,  
D24/107, 186, 216, 223, 231, 232; D10/46,  
D10/81; D14/341; 422/56, 58, 68.1; 600/316,  
600/322, 347, 365, 368

(57) **CLAIM**

The ornamental design for a blood glucose level measuring device, as shown and described.

See application file for complete search history.

**DESCRIPTION**

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D406,895 S \* 3/1999 Byrd et al. .... D24/169  
D499,805 S \* 12/2004 D'Agostino ..... D24/169  
D545,438 S \* 6/2007 Huang et al. .... D24/186  
D548,347 S \* 8/2007 Ichino et al. .... D24/186  
D562,458 S \* 2/2008 Padain ..... D24/169  
D566,706 S \* 4/2008 Andre et al. .... D14/341  
D581,056 S \* 11/2008 Kurokawa et al. .... D24/186  
D590,063 S \* 4/2009 Garthoff et al. .... D24/186  
D595,415 S \* 6/2009 Fukuzawa ..... D24/186  
D622,394 S \* 8/2010 Bielawa et al. .... D24/169

FIG. 1 is a top perspective view of the blood glucose level measuring device;

FIG. 2 is a bottom perspective view thereof;

FIG. 3 is a top view thereof;

FIG. 4 is a bottom view thereof;

FIG. 5 is a left side view thereof;


FIG. 6 is a right side view thereof;

FIG. 7 is a front view thereof; and,

FIG. 8 is a rear view thereof.

The broken lines in the FIGS. 4 and 5 are included for the purpose of illustrating portions of the blood glucose level measuring device that form no part of the claimed design.

**1 Claim, 8 Drawing Sheets**

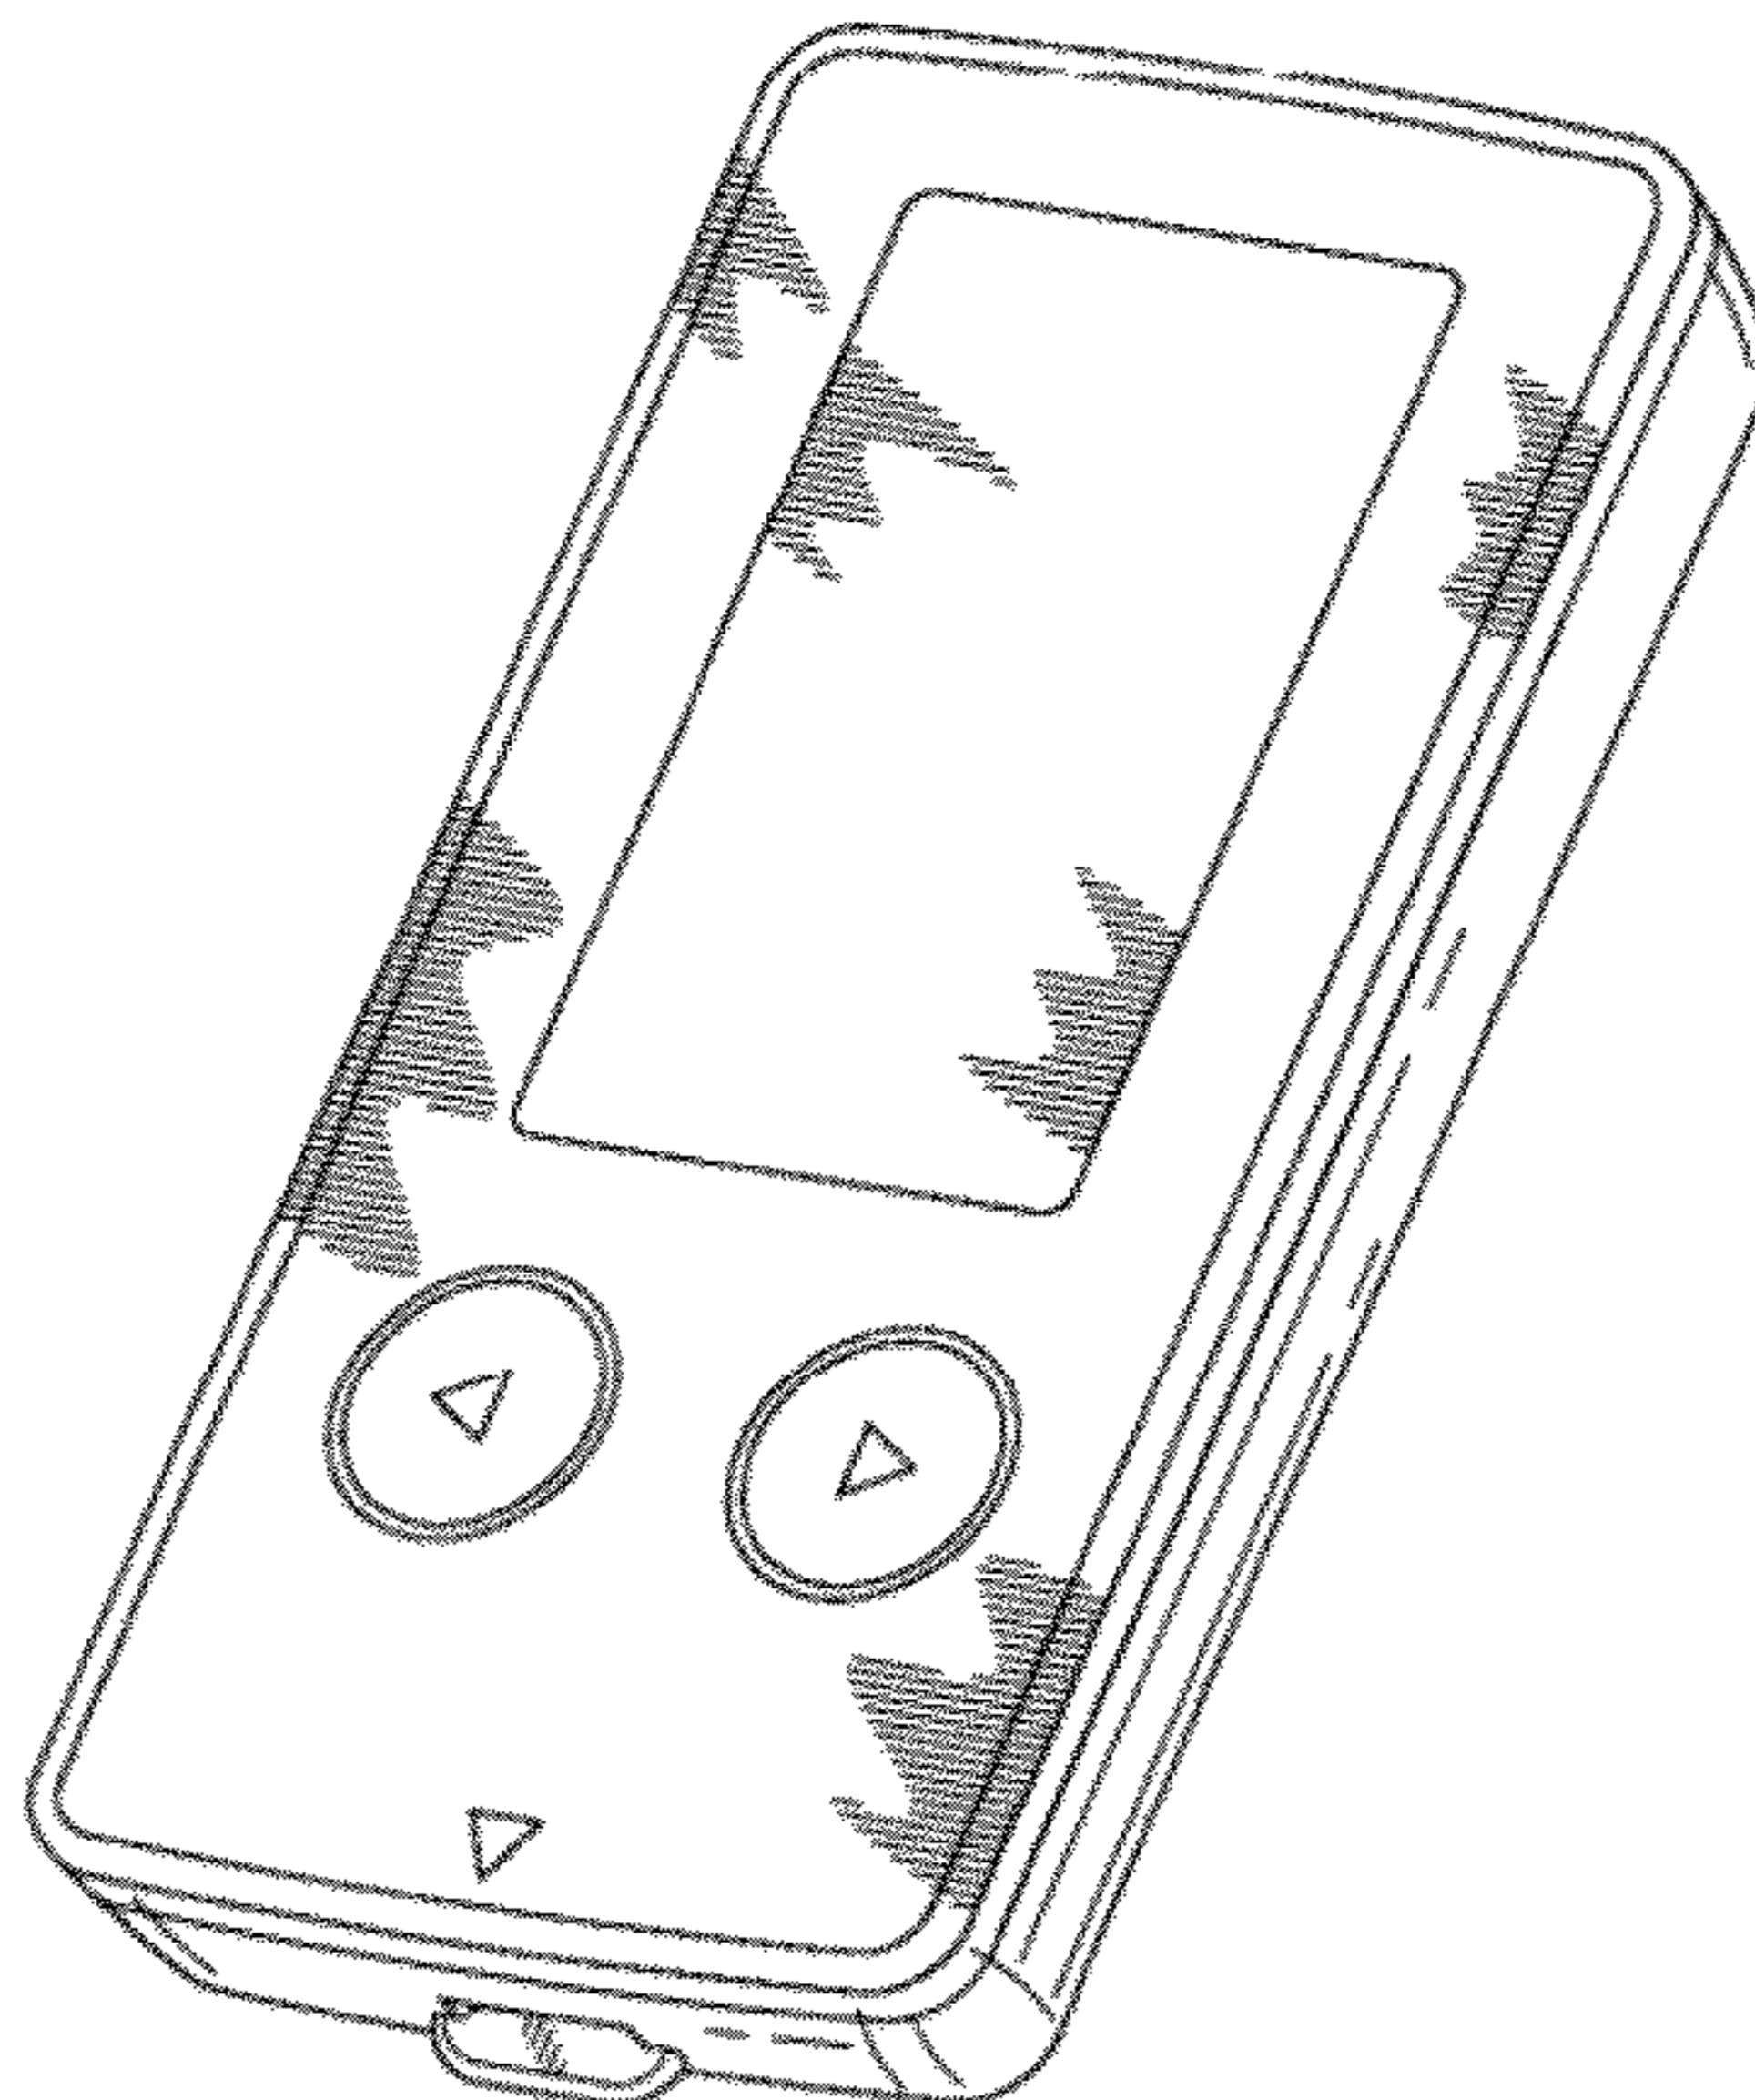

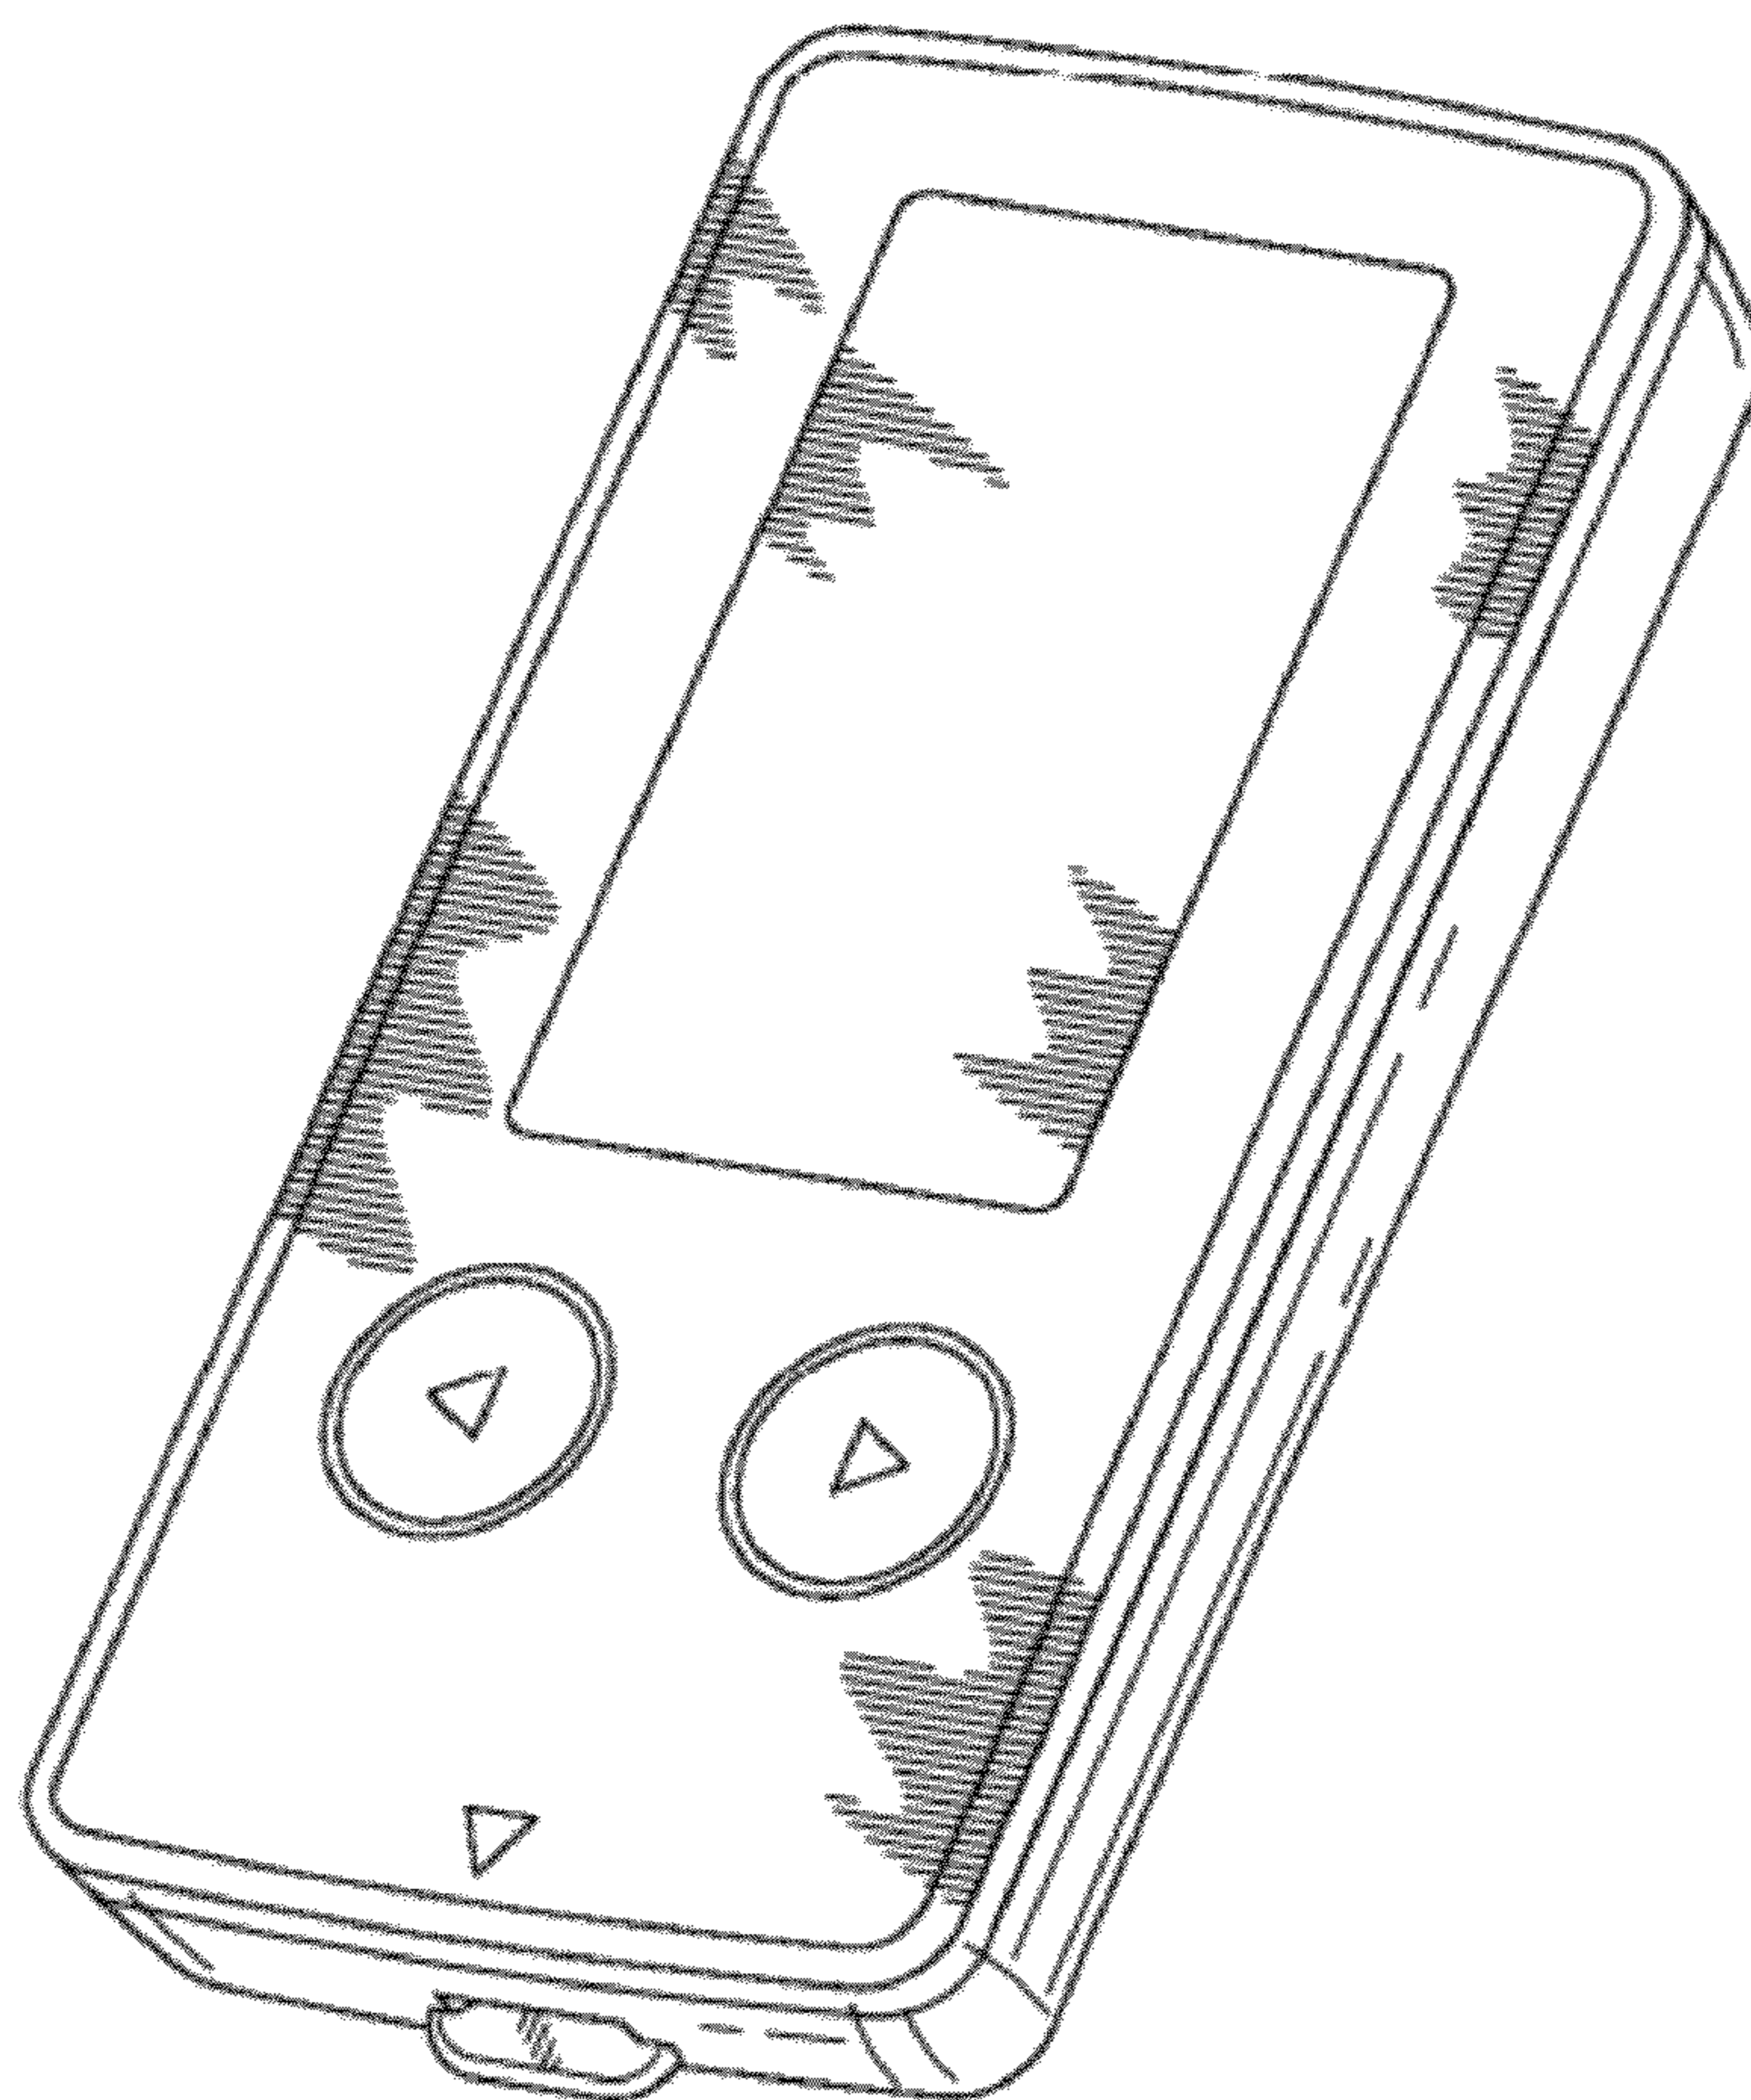


FIG. 1

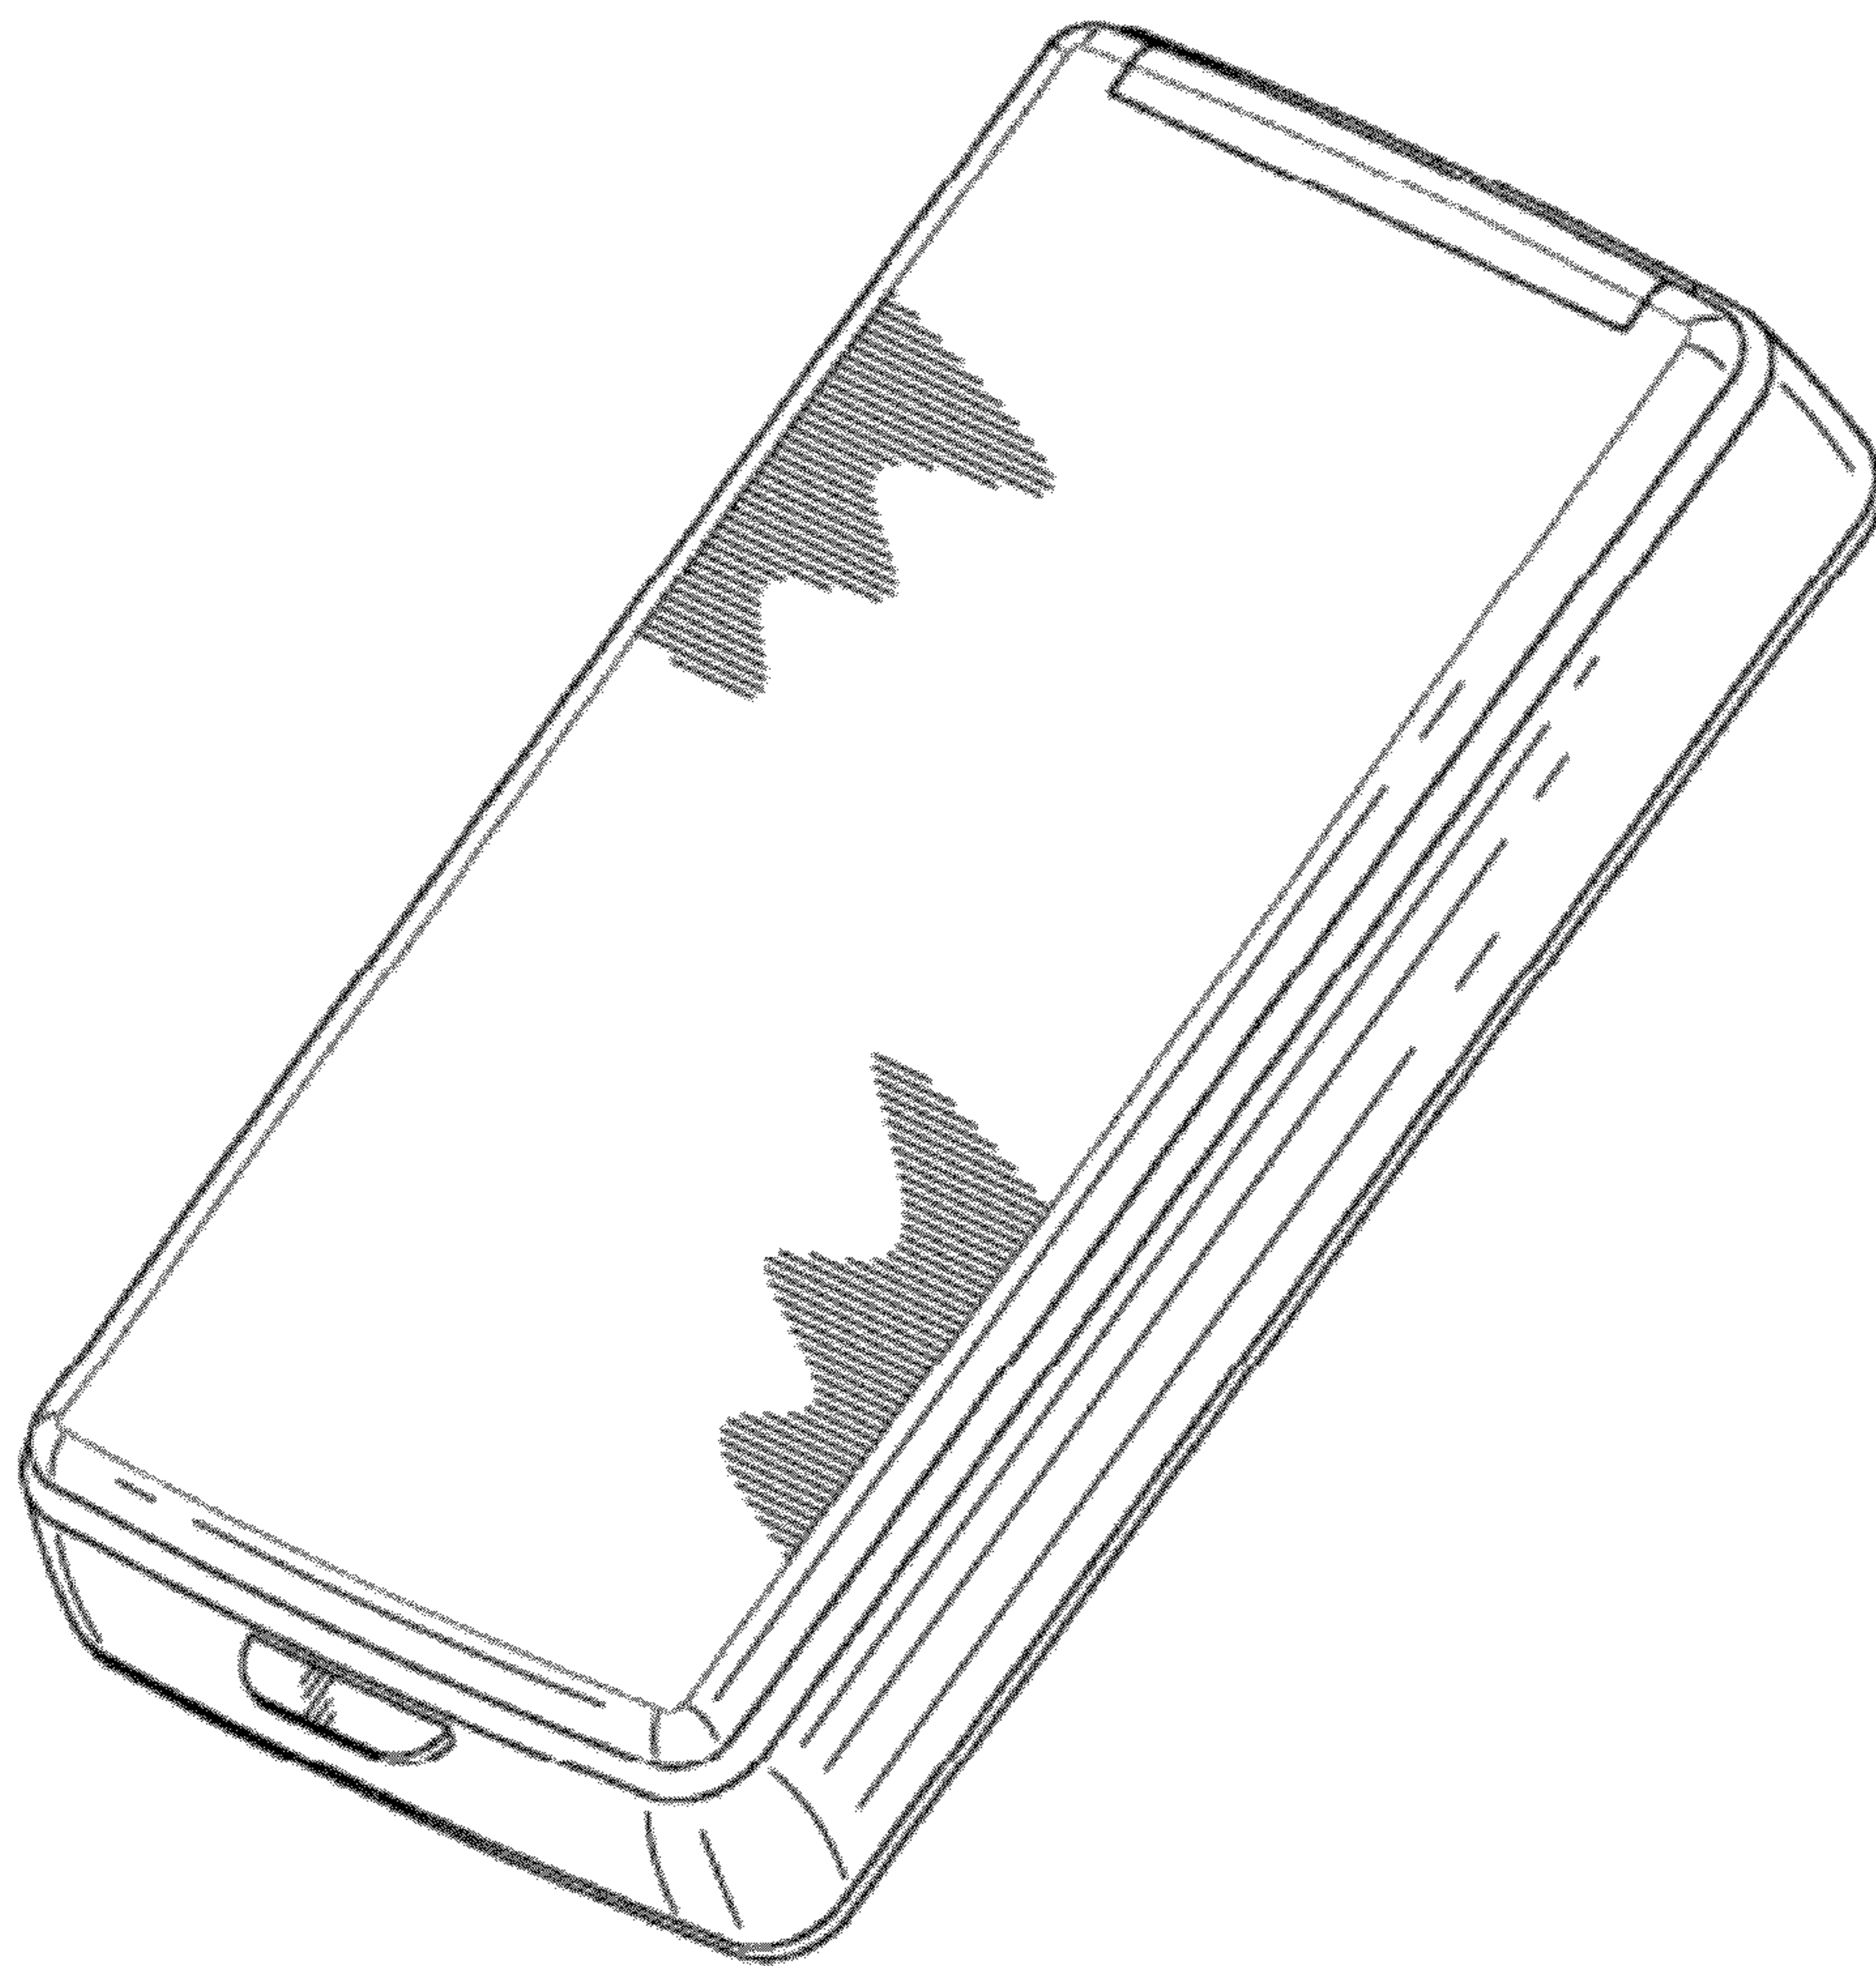


FIG. 2

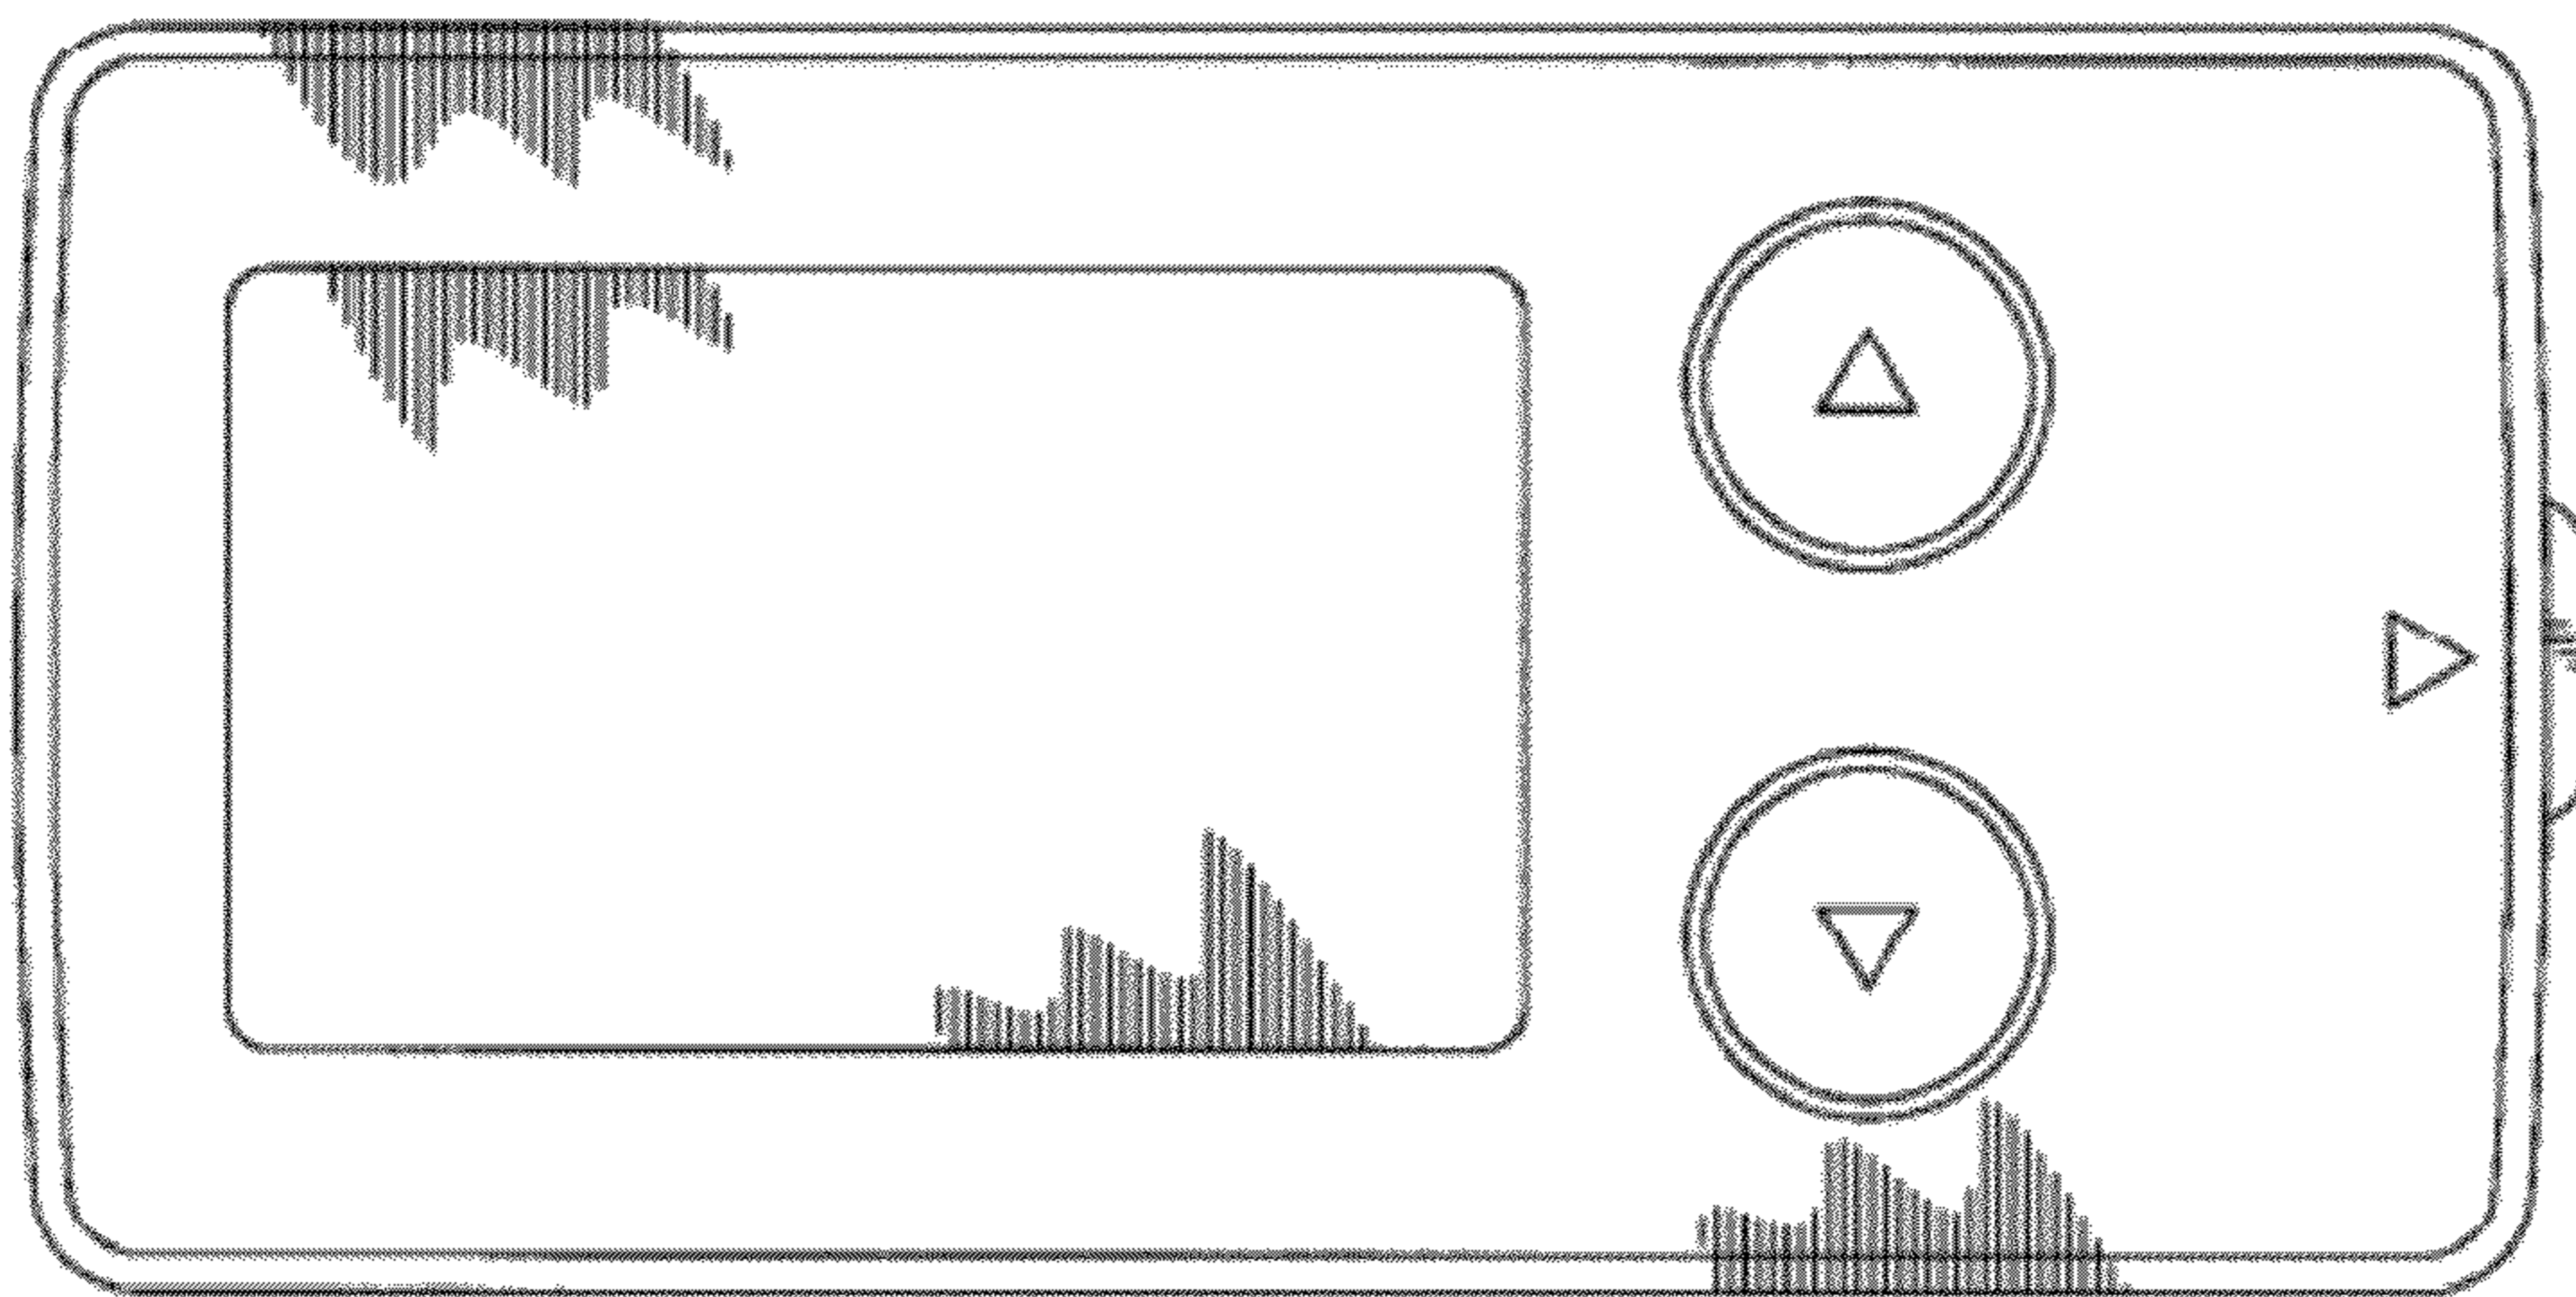


FIG. 3

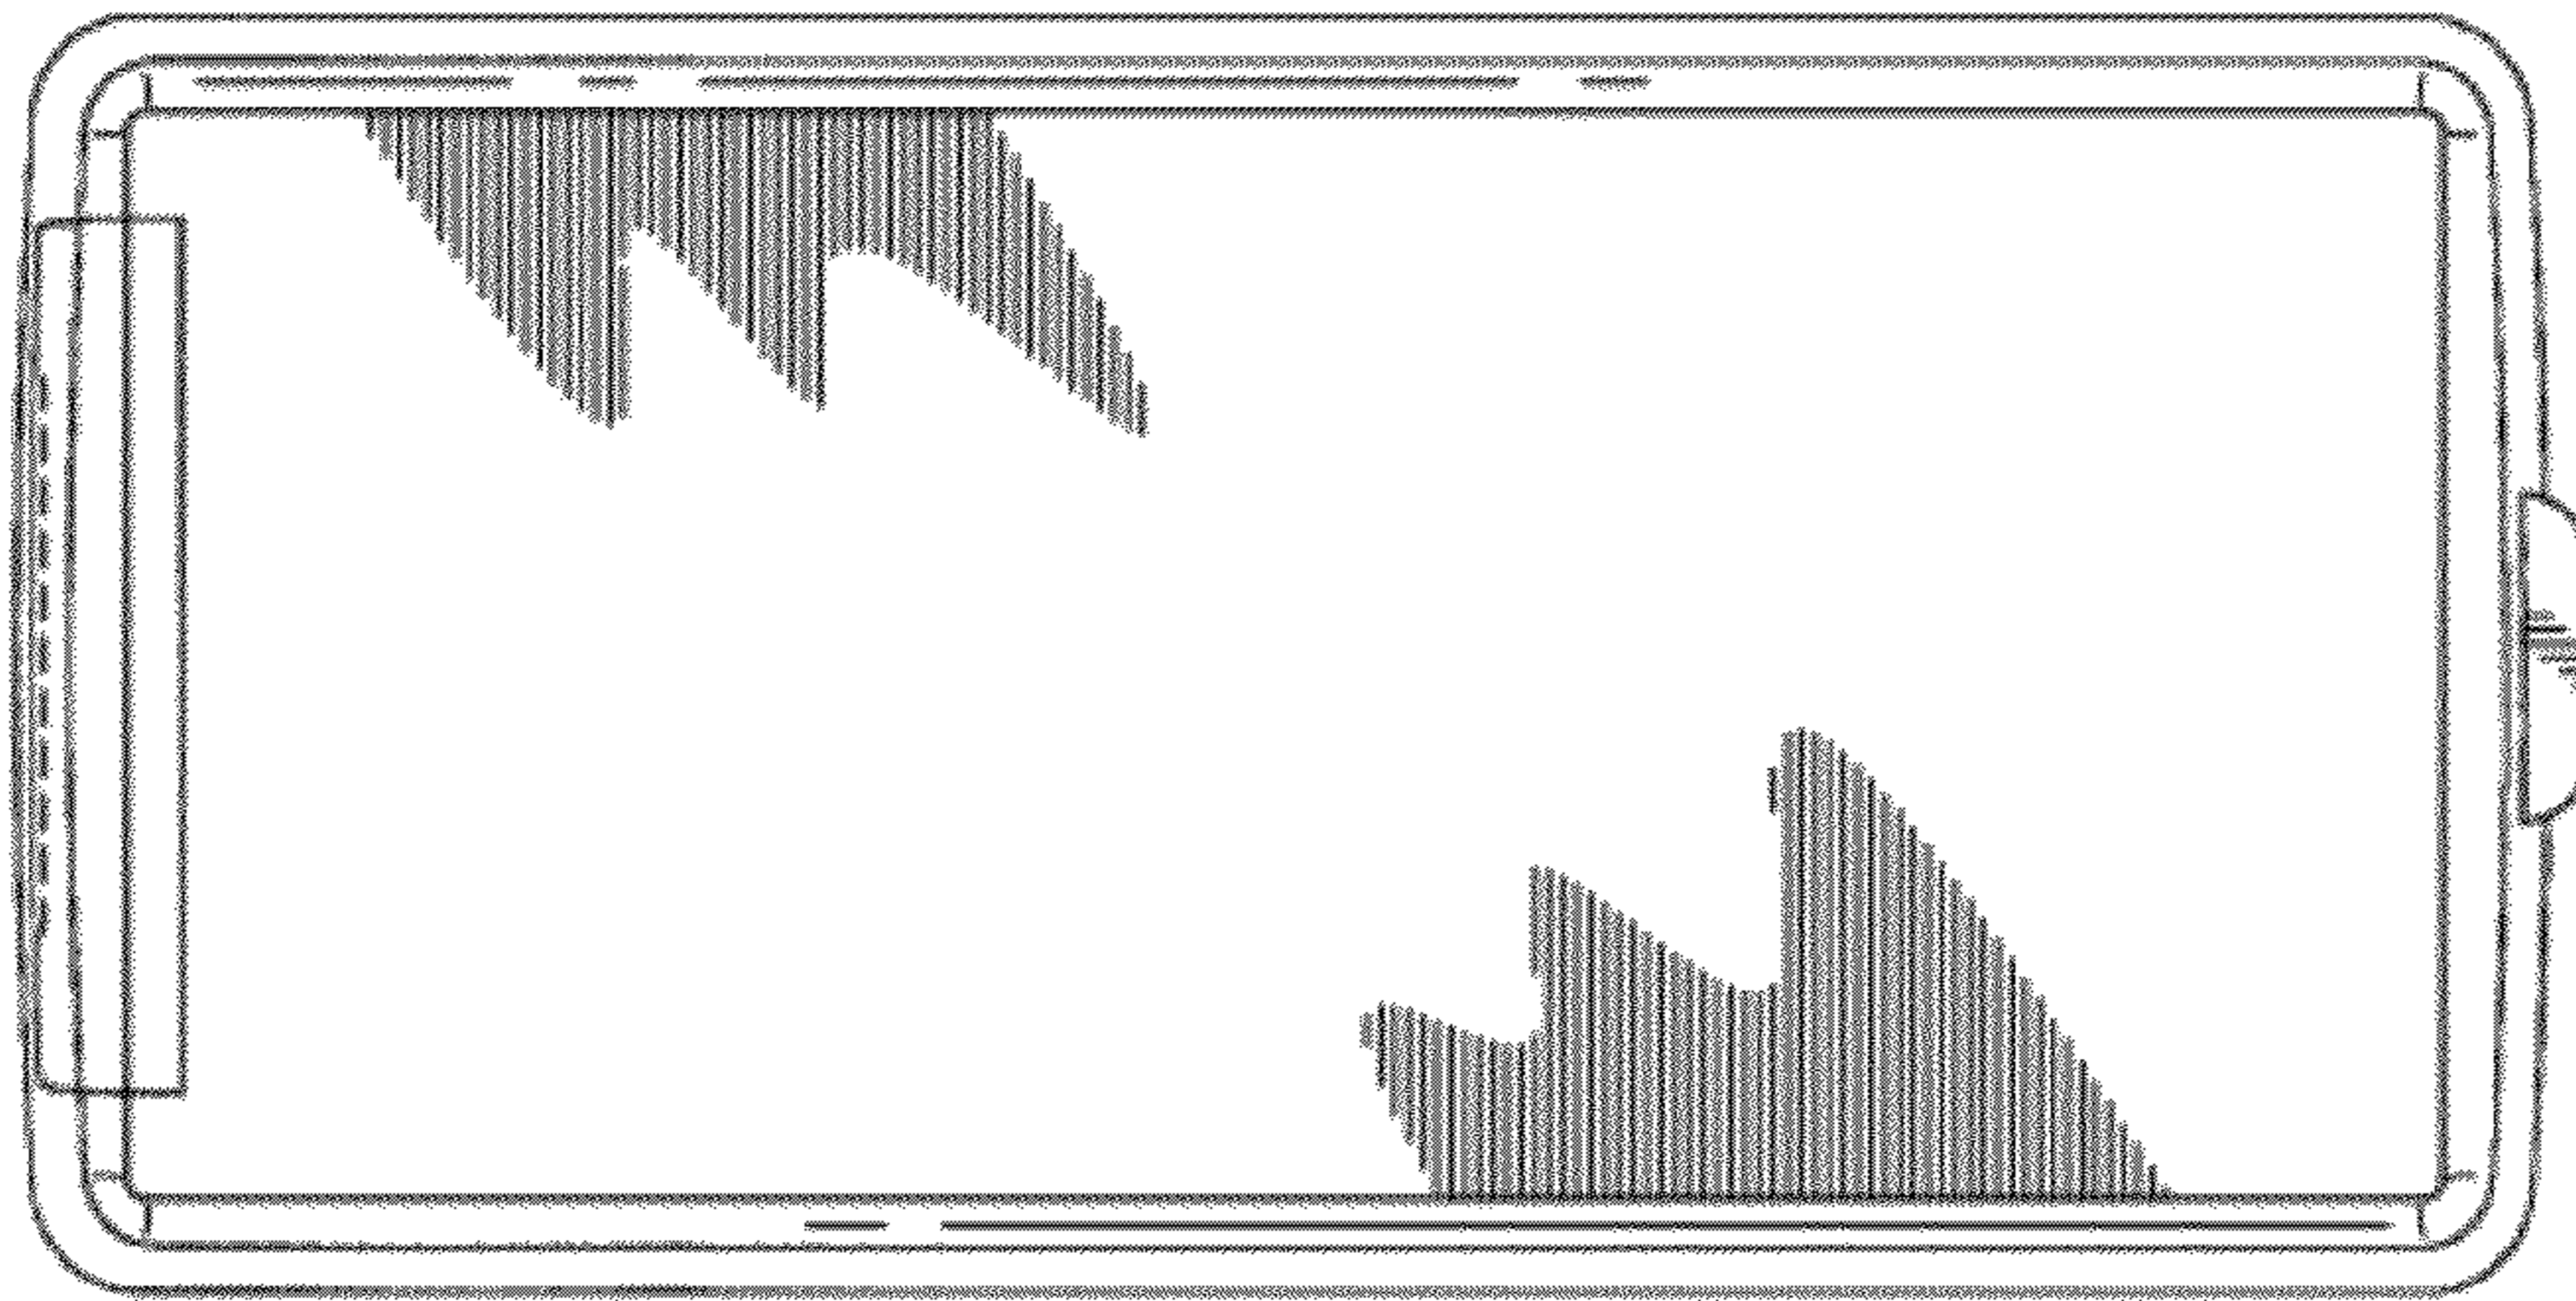


FIG. 4

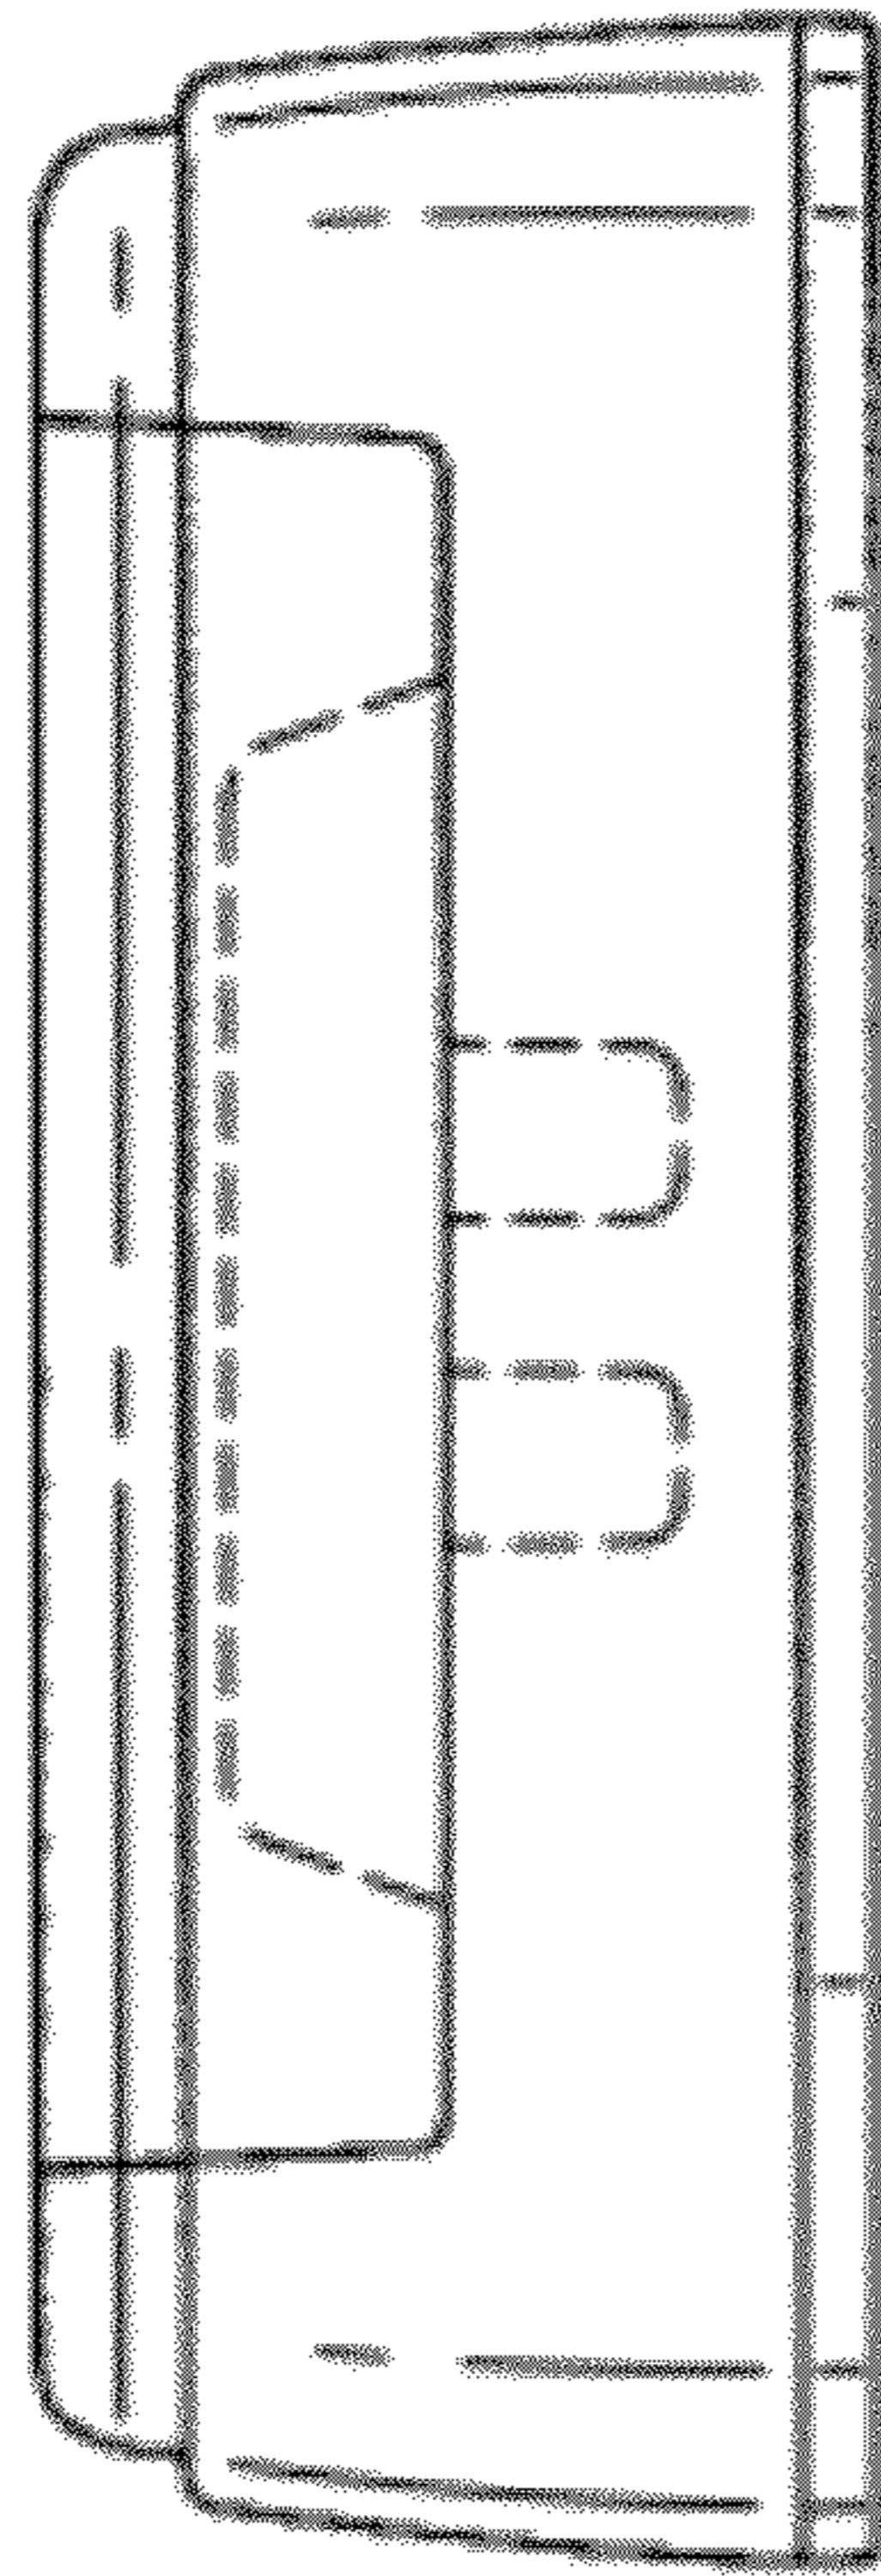


FIG. 5

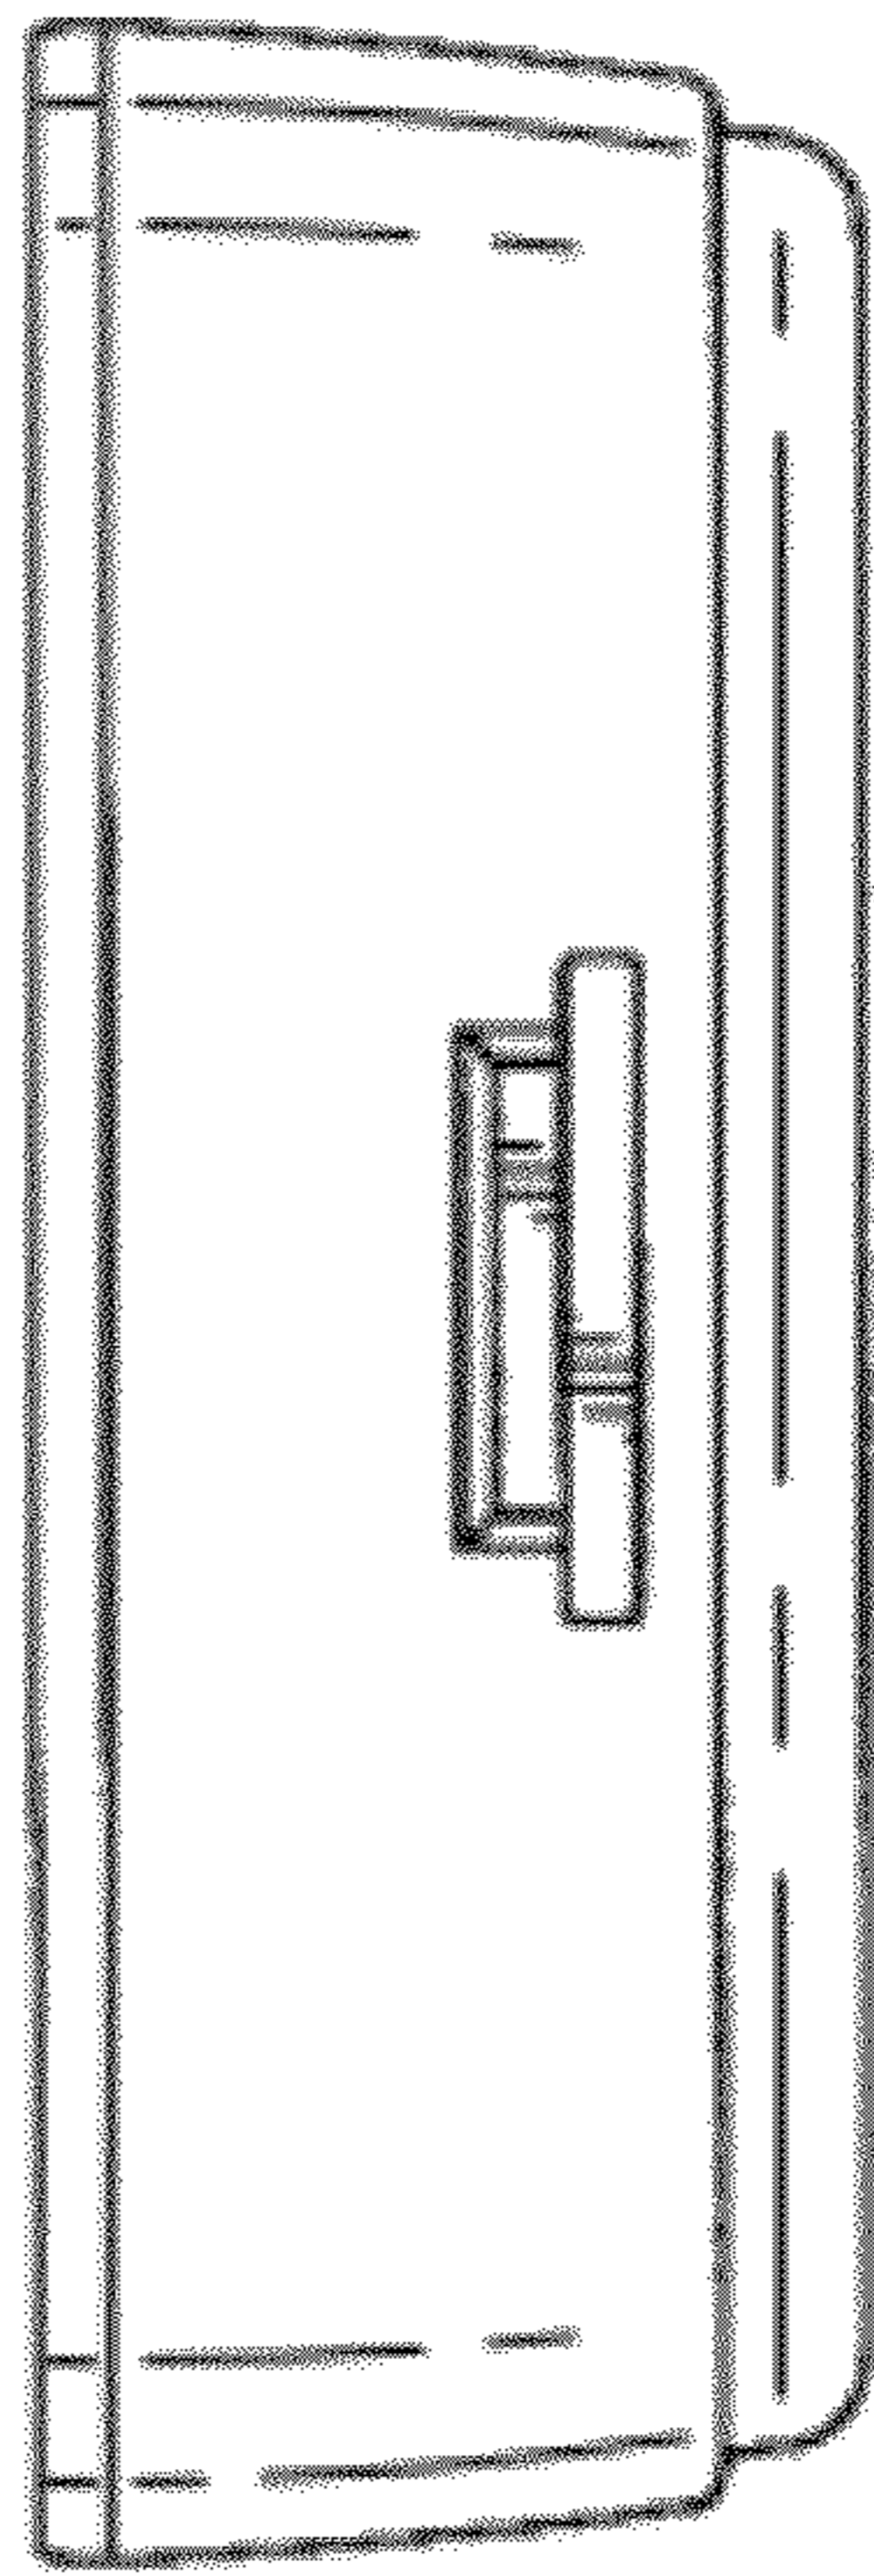


FIG. 6

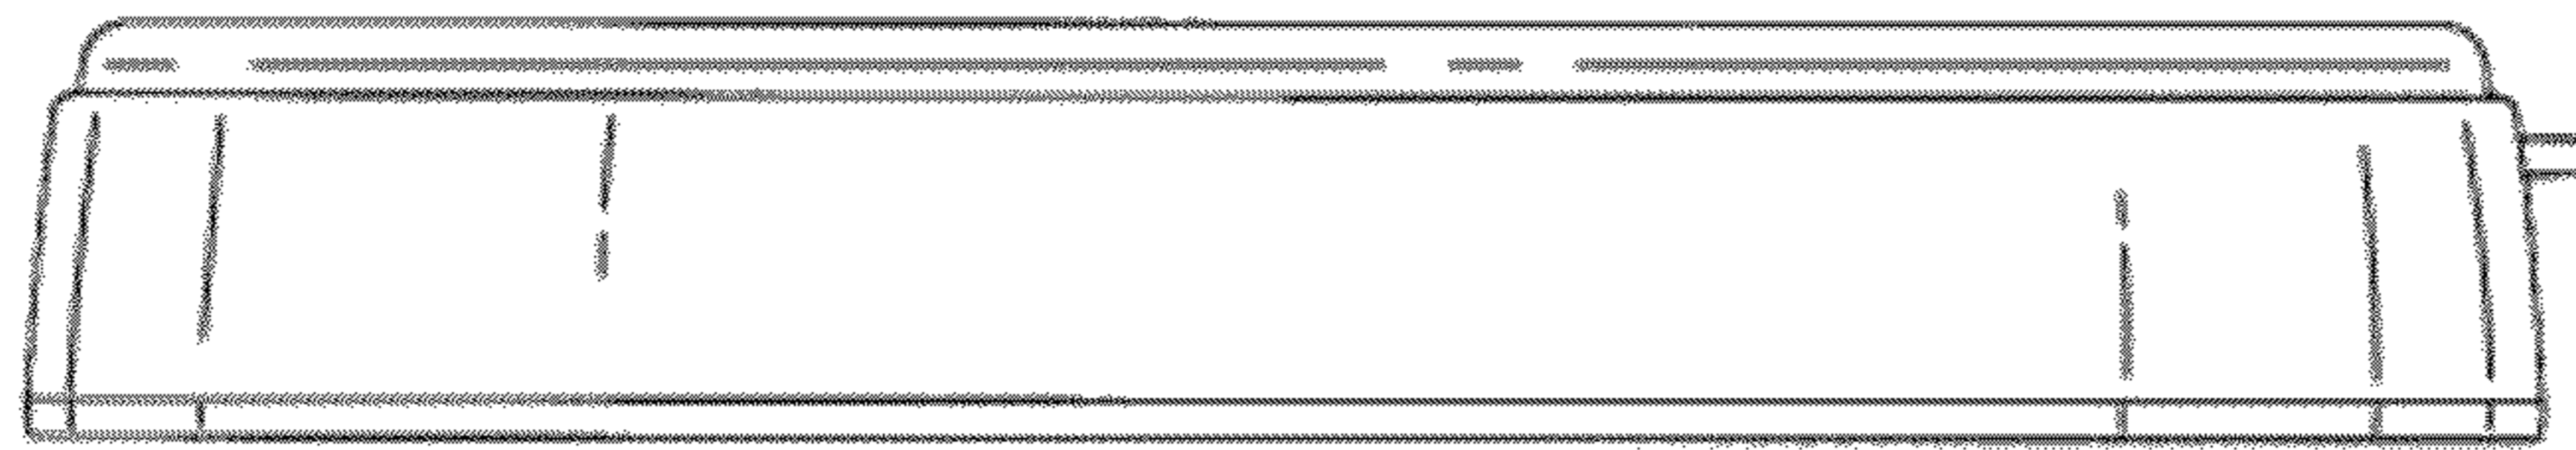


FIG. 7





FIG. 8