



US00D671125S

(12) **United States Design Patent**
Hansen et al.

(10) **Patent No.:** **US D671,125 S**

(45) **Date of Patent:** **** Nov. 20, 2012**

(54) **DISPLAY SCREEN WITH A GRAPHICAL USER INTERFACE**

(75) Inventors: **Bryan Scott Hansen**, Mead, CO (US);
Yu Jung Pinto, Boulder, CO (US);
Tracy Eliasson, Boulder, CO (US);
Greg Lund, Boulder, CO (US); **Corinne Johnson**, Denver, CO (US)

(73) Assignee: **Nellcor Puritan Bennett LLC**, Boulder, CO (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/369,153**

(22) Filed: **Sep. 2, 2010**

(51) **LOC (9) Cl.** **14-04**

(52) **U.S. Cl.** **D14/485**

(58) **Field of Classification Search** D14/485-495;
715/700, 703, 715, 716, 717, 718, 719, 727,
715/728, 730, 732, 739, 740, 752, 758, 762,
715/763, 771, 772, 773, 779, 780, 804, 808,
715/809, 810, 822, 823, 825, 828, 832, 833,
715/834, 835, 837, 838, 839, 841, 842, 843,
715/845, 846, 847, 848, 851, 860, 861, 864,
715/840, 961, 962, 963, 965, 966, 967, 968,
715/975; 379/106.02

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,972,331 A 11/1990 Chance
5,020,540 A 6/1991 Chamoun
5,122,974 A 6/1992 Chance
5,783,821 A 7/1998 Costello
5,999,852 A 12/1999 Elabbady
6,322,515 B1 11/2001 Goor et al.
6,615,065 B1 9/2003 Barrett et al.
D498,240 S * 11/2004 Amaitis et al. D14/486
6,839,580 B2 1/2005 Zonios et al.

6,839,581 B1 1/2005 El-Solh et al.
7,025,730 B2 4/2006 Cho et al.
D529,041 S * 9/2006 Melander et al. D14/492
D533,875 S * 12/2006 Miles et al. D14/495
7,246,618 B2 7/2007 Habashi
7,349,731 B2 3/2008 Jiang
D570,359 S * 6/2008 Sriver D14/486
D570,371 S * 6/2008 Melander et al. D14/492
D575,298 S * 8/2008 Chen et al. D14/486
D575,792 S * 8/2008 Benson D14/486
D600,716 S * 9/2009 LaManna et al. D14/492
D614,634 S * 4/2010 Nilsen D14/486
D619,609 S * 7/2010 Meziere D14/486
D632,699 S * 2/2011 Judy et al. D14/486
D633,510 S * 3/2011 MacBeth et al. D14/486
D640,264 S * 6/2011 Fujii et al. D14/486
D647,102 S * 10/2011 Tokunaga et al. D14/485

(Continued)

FOREIGN PATENT DOCUMENTS

WO WO2005096170 10/2005
WO WO2006067725 A2 6/2006
WO WO2006085120 8/2006
WO WO2008134813 11/2008

OTHER PUBLICATIONS

Active Matrix ePaper Displays; Innovating Display Solutions; SiPix.

(Continued)

Primary Examiner — Angela J Lee


(57) **CLAIM**

The ornamental design for a display screen with a graphical user interface, as shown and described.

DESCRIPTION

The FIGURE is a front view of a display screen with a graphical user interface showing our new design. The outer edge of the portion of the display screen is understood to be congruent with the outer edge of the user interface.

1 Claim, 1 Drawing Sheet

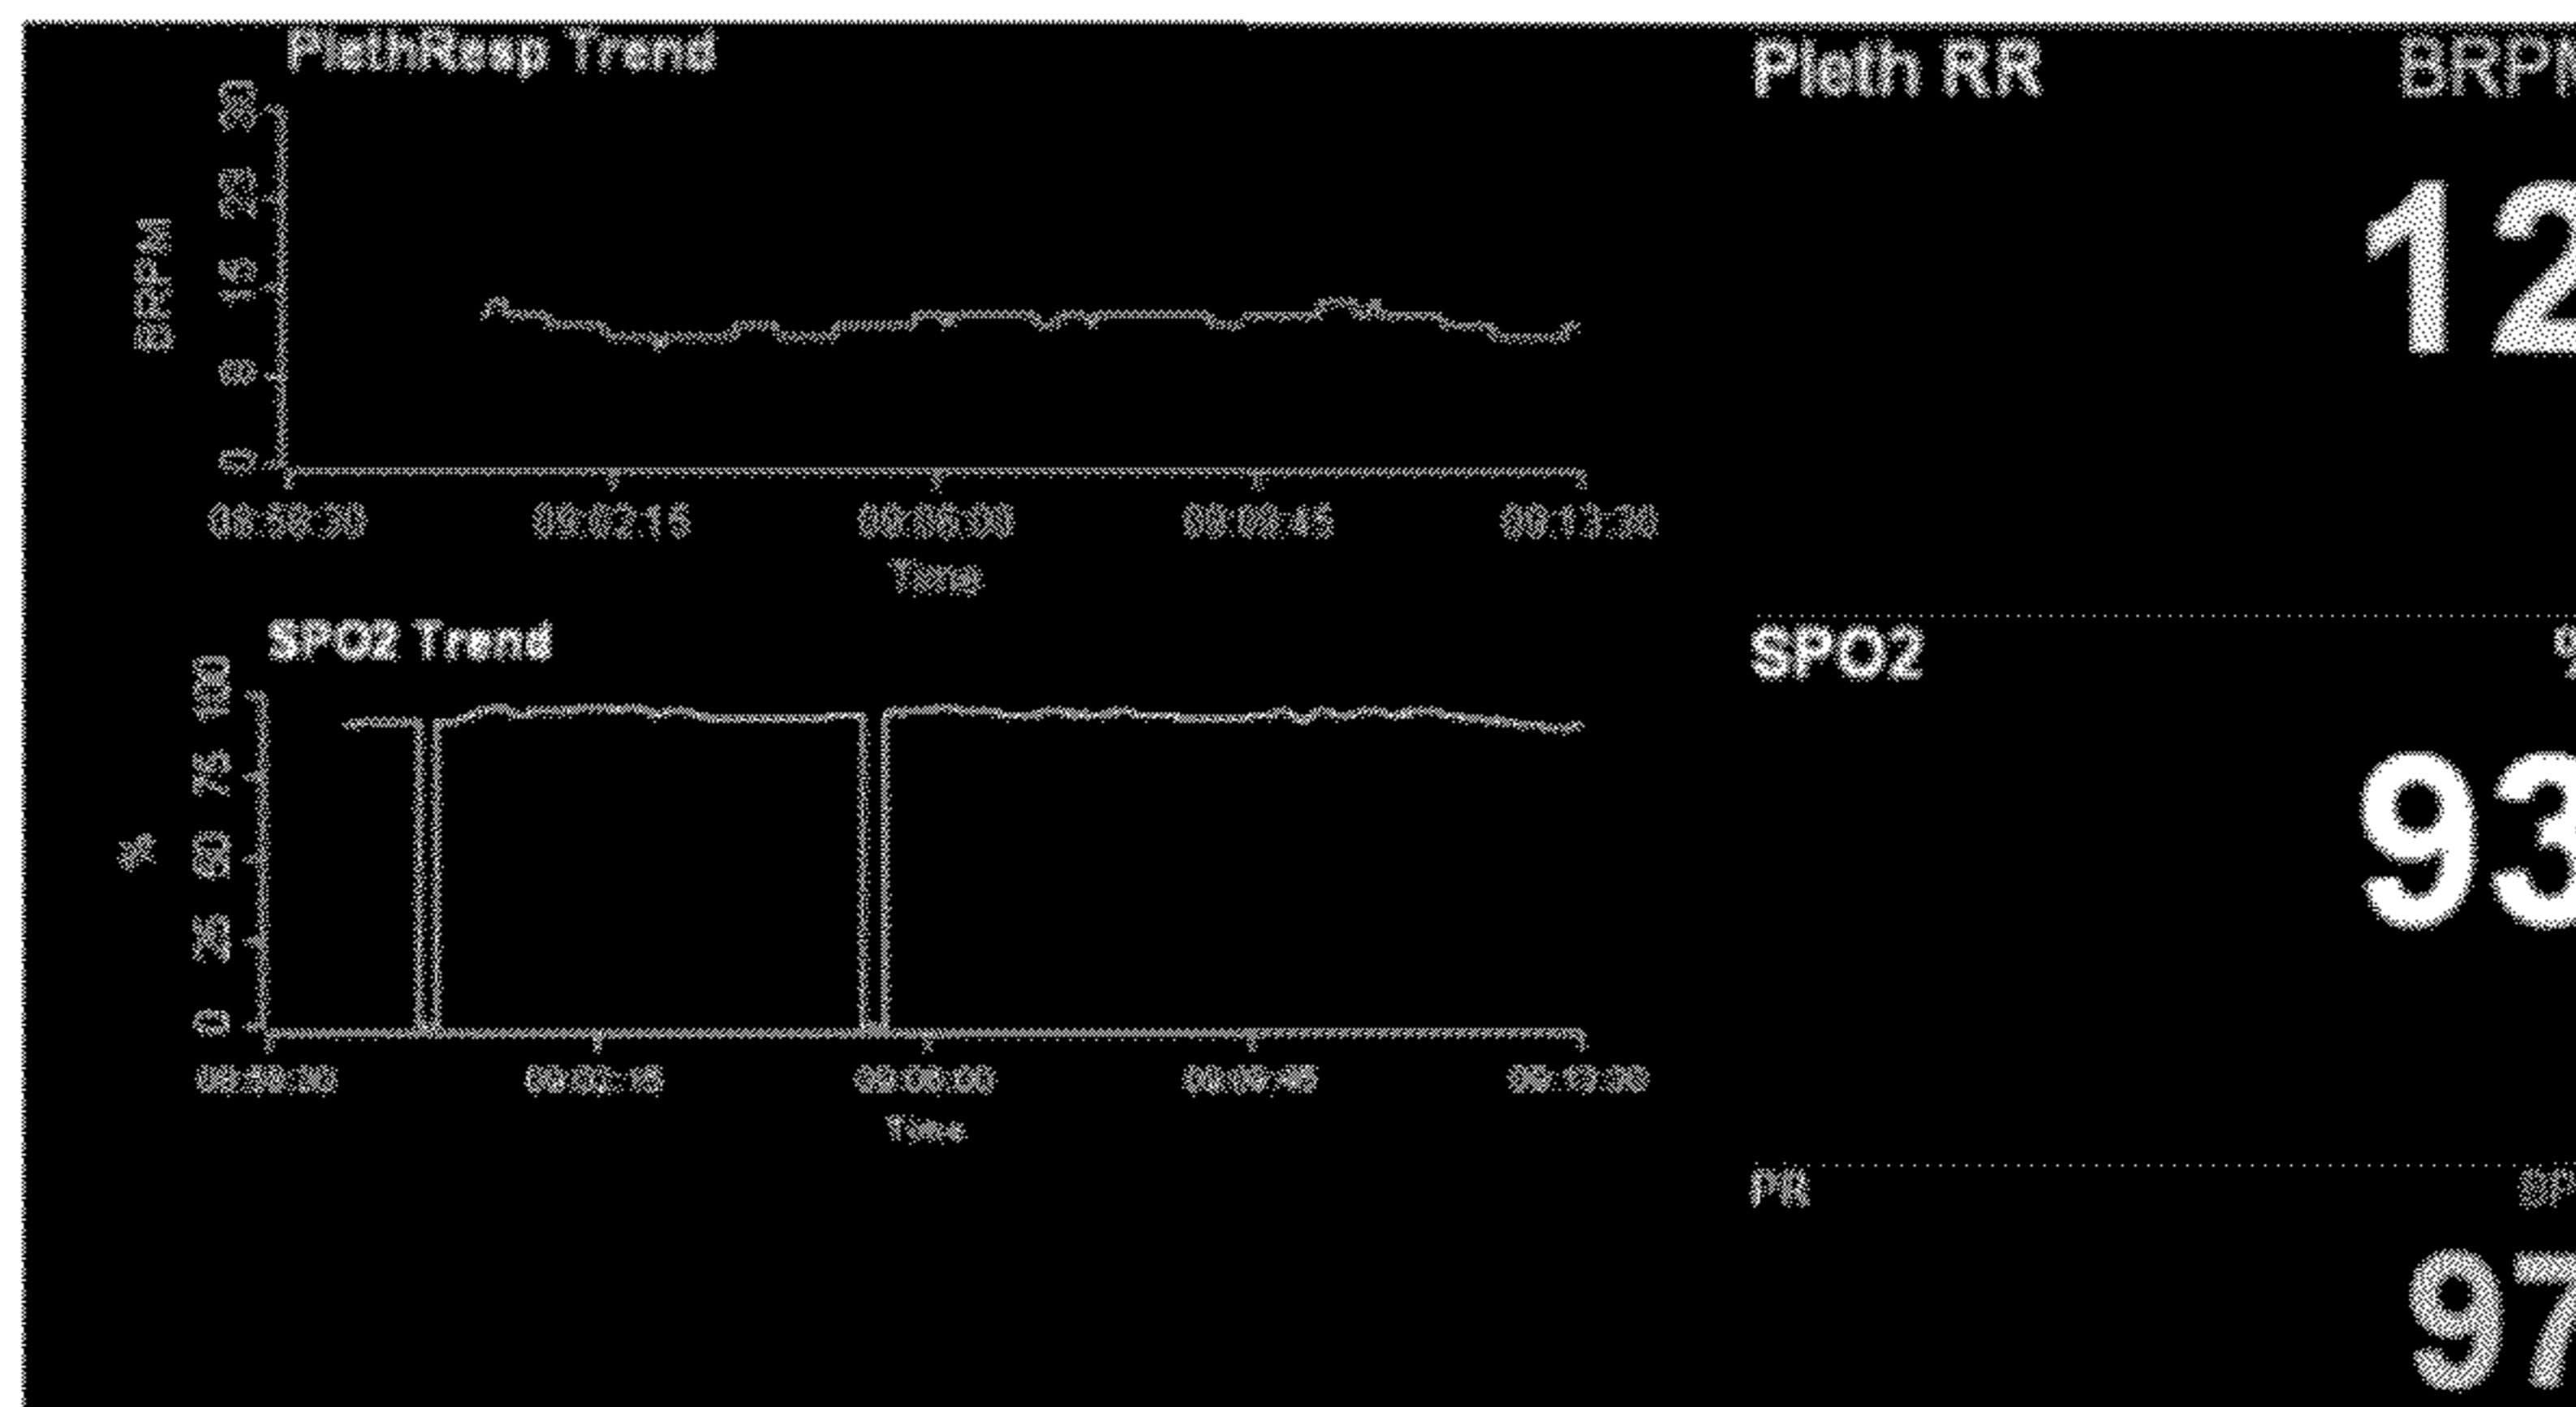

U.S. PATENT DOCUMENTS

2005/0137481	A1	6/2005	Sheard et al.	
2006/0063992	A1	3/2006	Yu et al.	
2006/0063993	A1	3/2006	Yu et al.	
2006/0167367	A1	7/2006	Stanczak et al.	
2006/0212316	A1	9/2006	Jackson et al.	
2006/0287590	A1	12/2006	McEowen	
2007/0118045	A1	5/2007	Naghavi et al.	
2008/0000477	A1	1/2008	Huster et al.	
2008/0004513	A1	1/2008	Walker et al.	
2008/0045832	A1	2/2008	McGrath	
2008/0081963	A1	4/2008	Naghavi et al.	
2008/0146890	A1	6/2008	LeBoeuf et al.	
2008/0198361	A1	8/2008	Kaushal et al.	
2008/0295839	A1	12/2008	Habashi	
2010/0107103	A1*	4/2010	Wallaert et al.	715/771
2010/0107109	A1*	4/2010	Filbeck et al.	715/777
2010/0162111	A1*	6/2010	Amundson et al.	715/702
2011/0029865	A1*	2/2011	Gilland et al.	715/702
2011/0071420	A1*	3/2011	St. Pierre et al.	600/549
2011/0138323	A1*	6/2011	Skidmore et al.	715/800

OTHER PUBLICATIONS

Electronic Paper Displays; E Ink Corporation; 2005.
 First-Generation Electronic Paper Display from Philips, Sony and E Ink to be Used in New Electronic Reading Devices; E Ink Corporation; 2005.

Plastic Logic; <http://www.plasticlogic.com/product.html> ; 2000.
 Segmented ePaper Displays; Innovating Display Solutions; SiPix.
 Crilly, Paul B., et al.; "An Integrated Pulse Oximeter System for Telemedicine Applications," IEEE Instrumentation and Measurement Technology Conference, Ottawa, Canada; May 19-21, 1997; pp. 102-104.
 Lutter, Norbert O., et al.; "False Alarm Rates of Three Third-Generation Pulse Oximeters in PACU, ICU and IABP Patients," *Anesth Analg*, vol. 94, pp. S69-S75 (2002).
 Östmark, Ake, et al.; "Mobile Medical Applications Made Feasible Through Use of EIS Platforms," IMTC—Instrumentation and Measurement Technology Conference, Vail, Colorado; May 20-22, 2003; pp. 292-295.
 Rhee, Sokwoo, et al.; "Design of a Artifact-Free Wearable Plethysmographic Sensor," *Proceedings of the First joint BMES/EMBS Conference*, Oct. 13-16, 1999, Atlanta, Georgia, p. 786.
 Warren, Steve, et al.; "A Distributed Infrastructure for Veterinary Telemedicine," *Proceedings of the 25th Annual International Conference of the IEEE EMBS*, Cancun, Mexico; Sep. 17-21, 2003; pp. 1394-1397.
 Yang, Boo-Ho, et al.; "A Twenty-Four Hour Tele-Nursing System Using a Ring Sensor," *Proceedings of the 1998 IEEE International Conference on Robotics & Automation*, Leaven, Belgium, May 1998; pp. 387-392.

* cited by examiner

