



US00D673269S

(12) **United States Design Patent**  
**El-Mohtar**

(10) **Patent No.:** **US D673,269 S**

(45) **Date of Patent:** **\*\* Dec. 25, 2012**

(54) **COLLAPSIBLE STETHOSCOPE**

(75) Inventor: **Kody El-Mohtar**, Albany, NY (US)

(73) Assignee: **Albany Medical College**, Albany, NY (US)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/414,262**

(22) Filed: **Feb. 27, 2012**

(51) **LOC (9) Cl.** ..... **24-02**

(52) **U.S. Cl.** ..... **D24/134**

(58) **Field of Classification Search** ..... D24/134;  
181/131, 132

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,715,296	A *	8/1955	Pettit	446/418
3,032,030	A	5/1962	Han	
3,086,610	A	4/1963	Haas	
D284,790	S	7/1986	Moore	
6,006,856	A *	12/1999	Skubal et al.	181/131
D589,144	S *	3/2009	Bagha et al.	D24/134
7,575,094	B1	8/2009	Rosenberg	
7,636,445	B2	12/2009	Yoshimine	
2001/0030077	A1	10/2001	Watson	
2003/0192736	A1 *	10/2003	Werblud	181/131

\* cited by examiner

*Primary Examiner* — Bridget L Eland

(74) *Attorney, Agent, or Firm* — Heslin Rothenberg Farley & Mesiti P.C.

(57) **CLAIM**

The ornamental design for a collapsible stethoscope, as shown and described.


**DESCRIPTION**

FIG. 1 is a perspective view of a collapsible stethoscope showing my new design;  
 FIG. 2 is a front elevational view of the design of FIG. 1;  
 FIG. 3 is a rear elevational view of the design of FIG. 1;  
 FIG. 4 is a left side elevational view of the design of FIG. 1, where the right side elevational view is a mirror image thereof;  
 FIG. 5 is a top view of the design of FIG. 1;  
 FIG. 6 is a bottom view of the design of FIG. 1; and,  
 FIG. 7 is a perspective view of the design of FIG. 1 in an extended state.

The outer most broken lines showing a digital display output and the diaphragm represent the bounds of the claimed design while the connecting hinge, ear buds, portion of the listening tube, and all other broken lines are directed to environment and are for illustrative purposes only; the broken lines form no part of the claimed design.

The broken lines shown in the drawings illustrates portions of the collapsible stethoscope, and form no part of the claimed design.

**1 Claim, 5 Drawing Sheets**

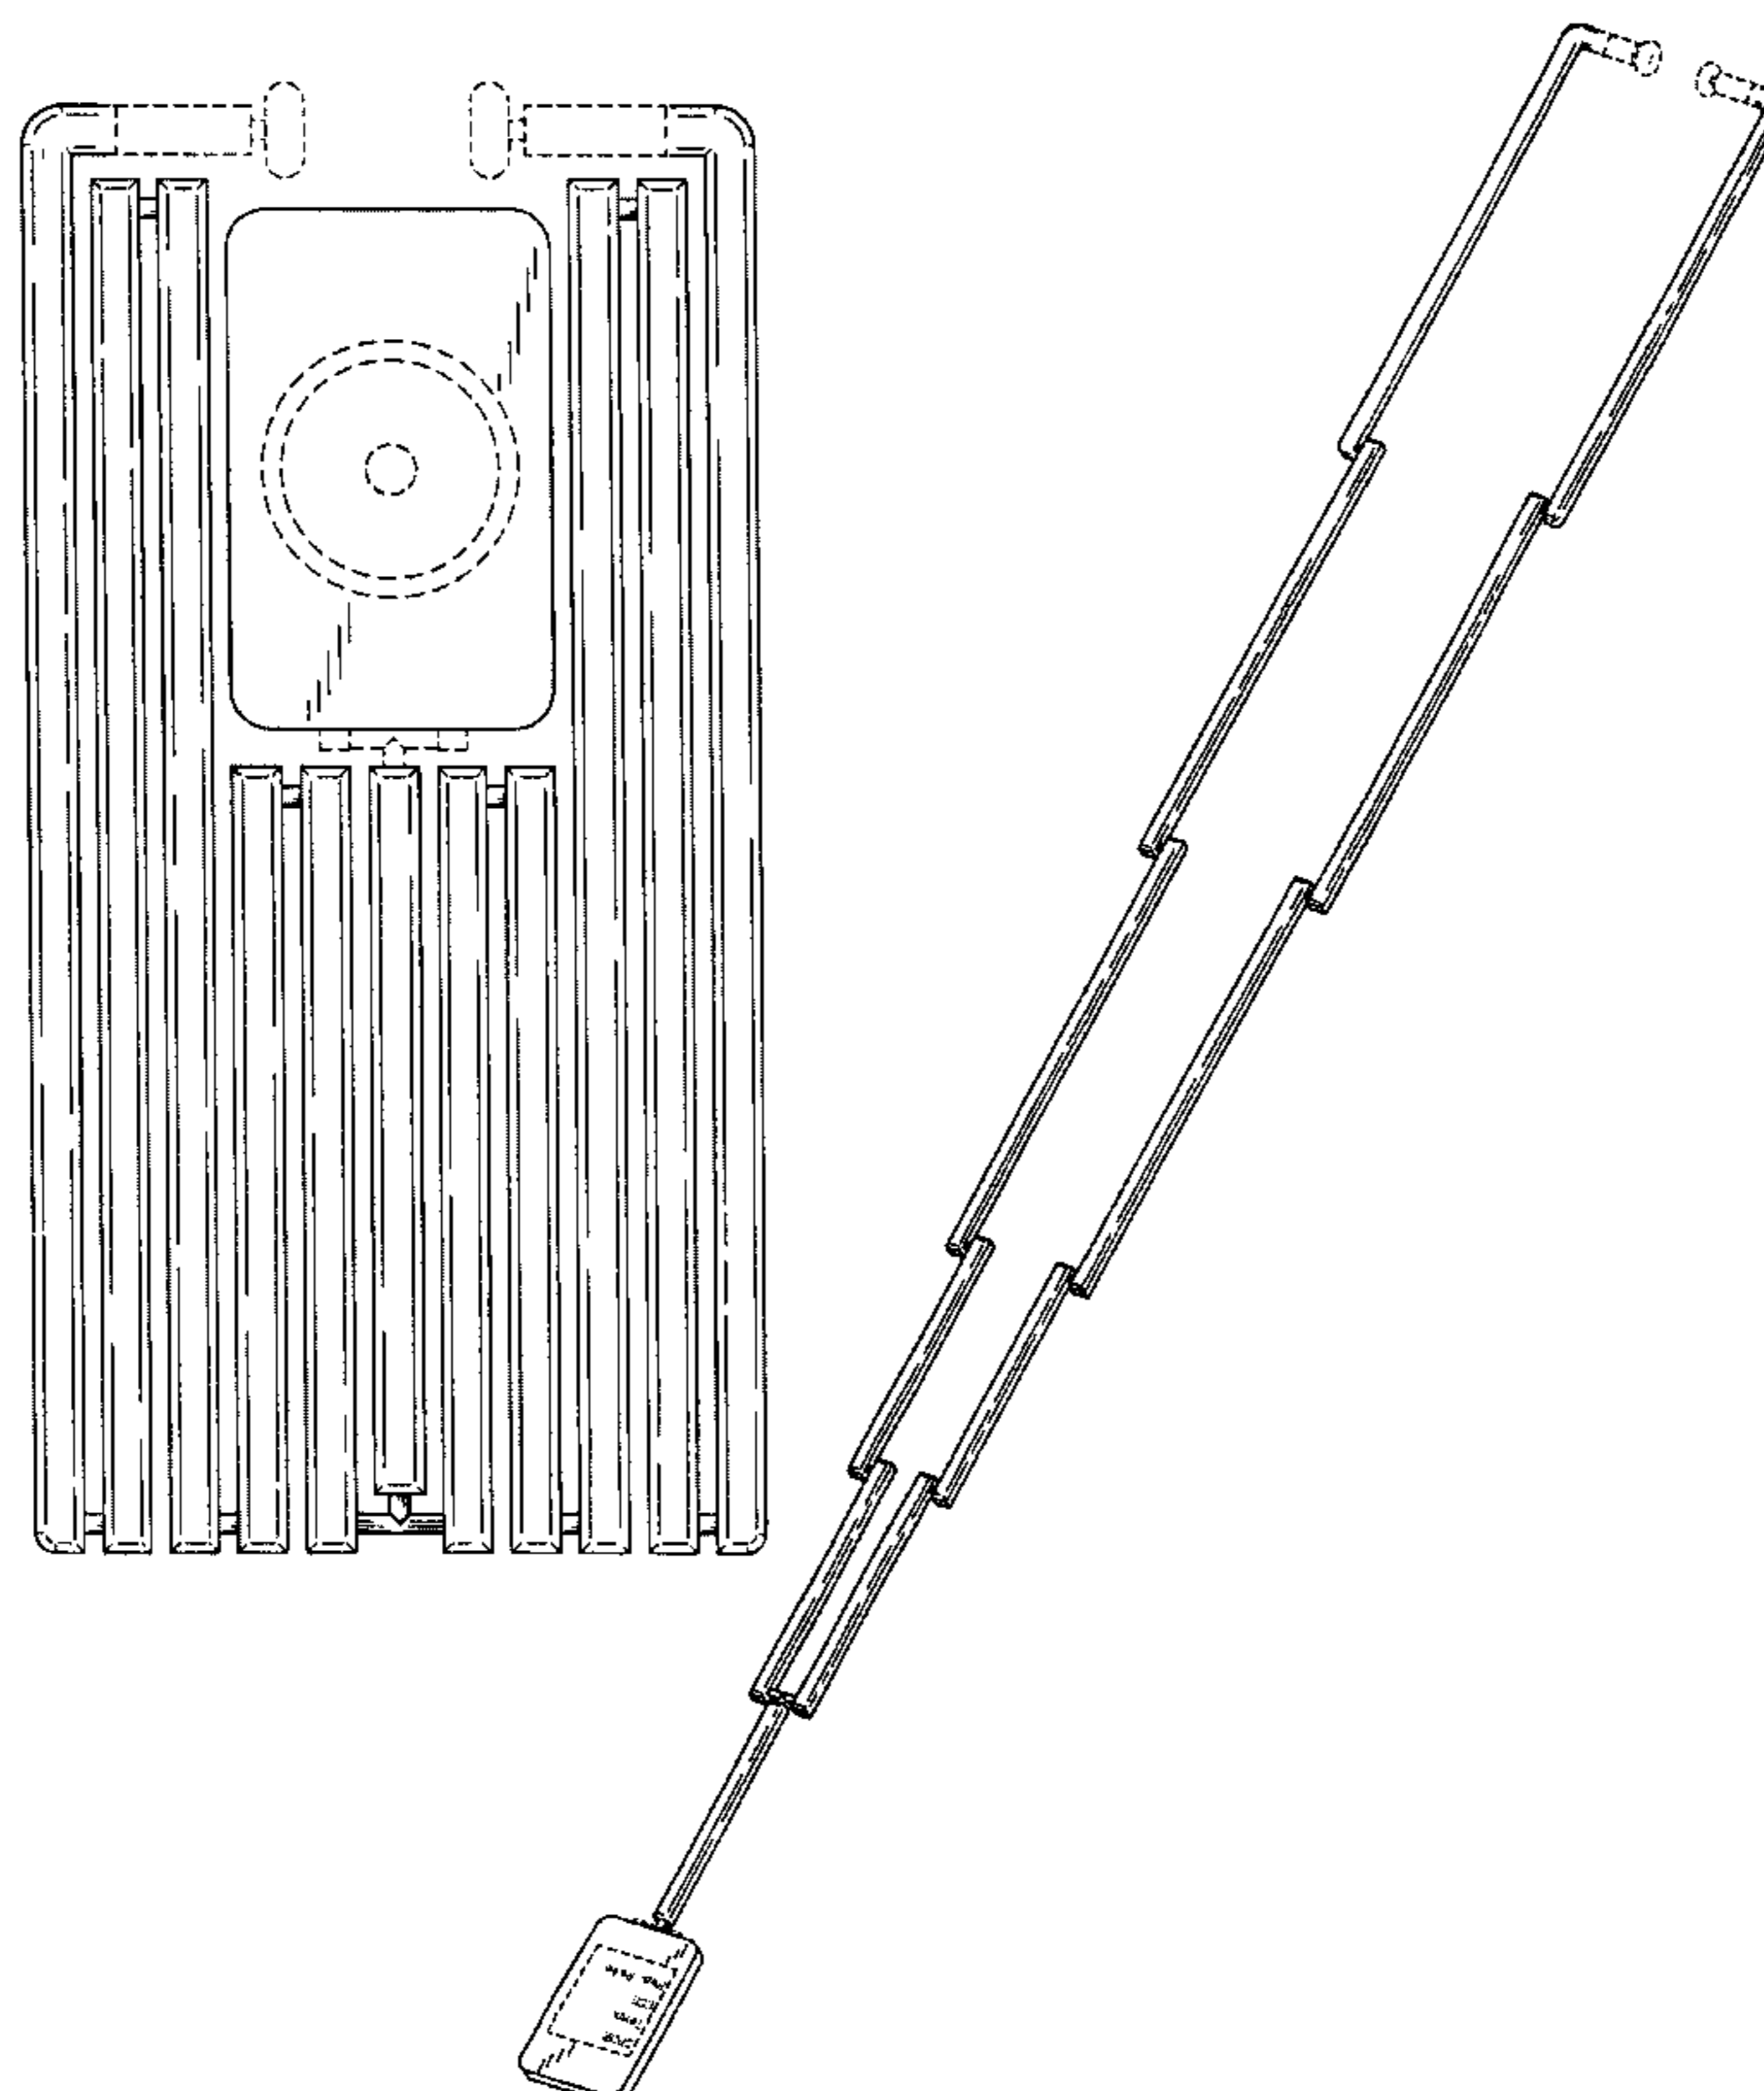

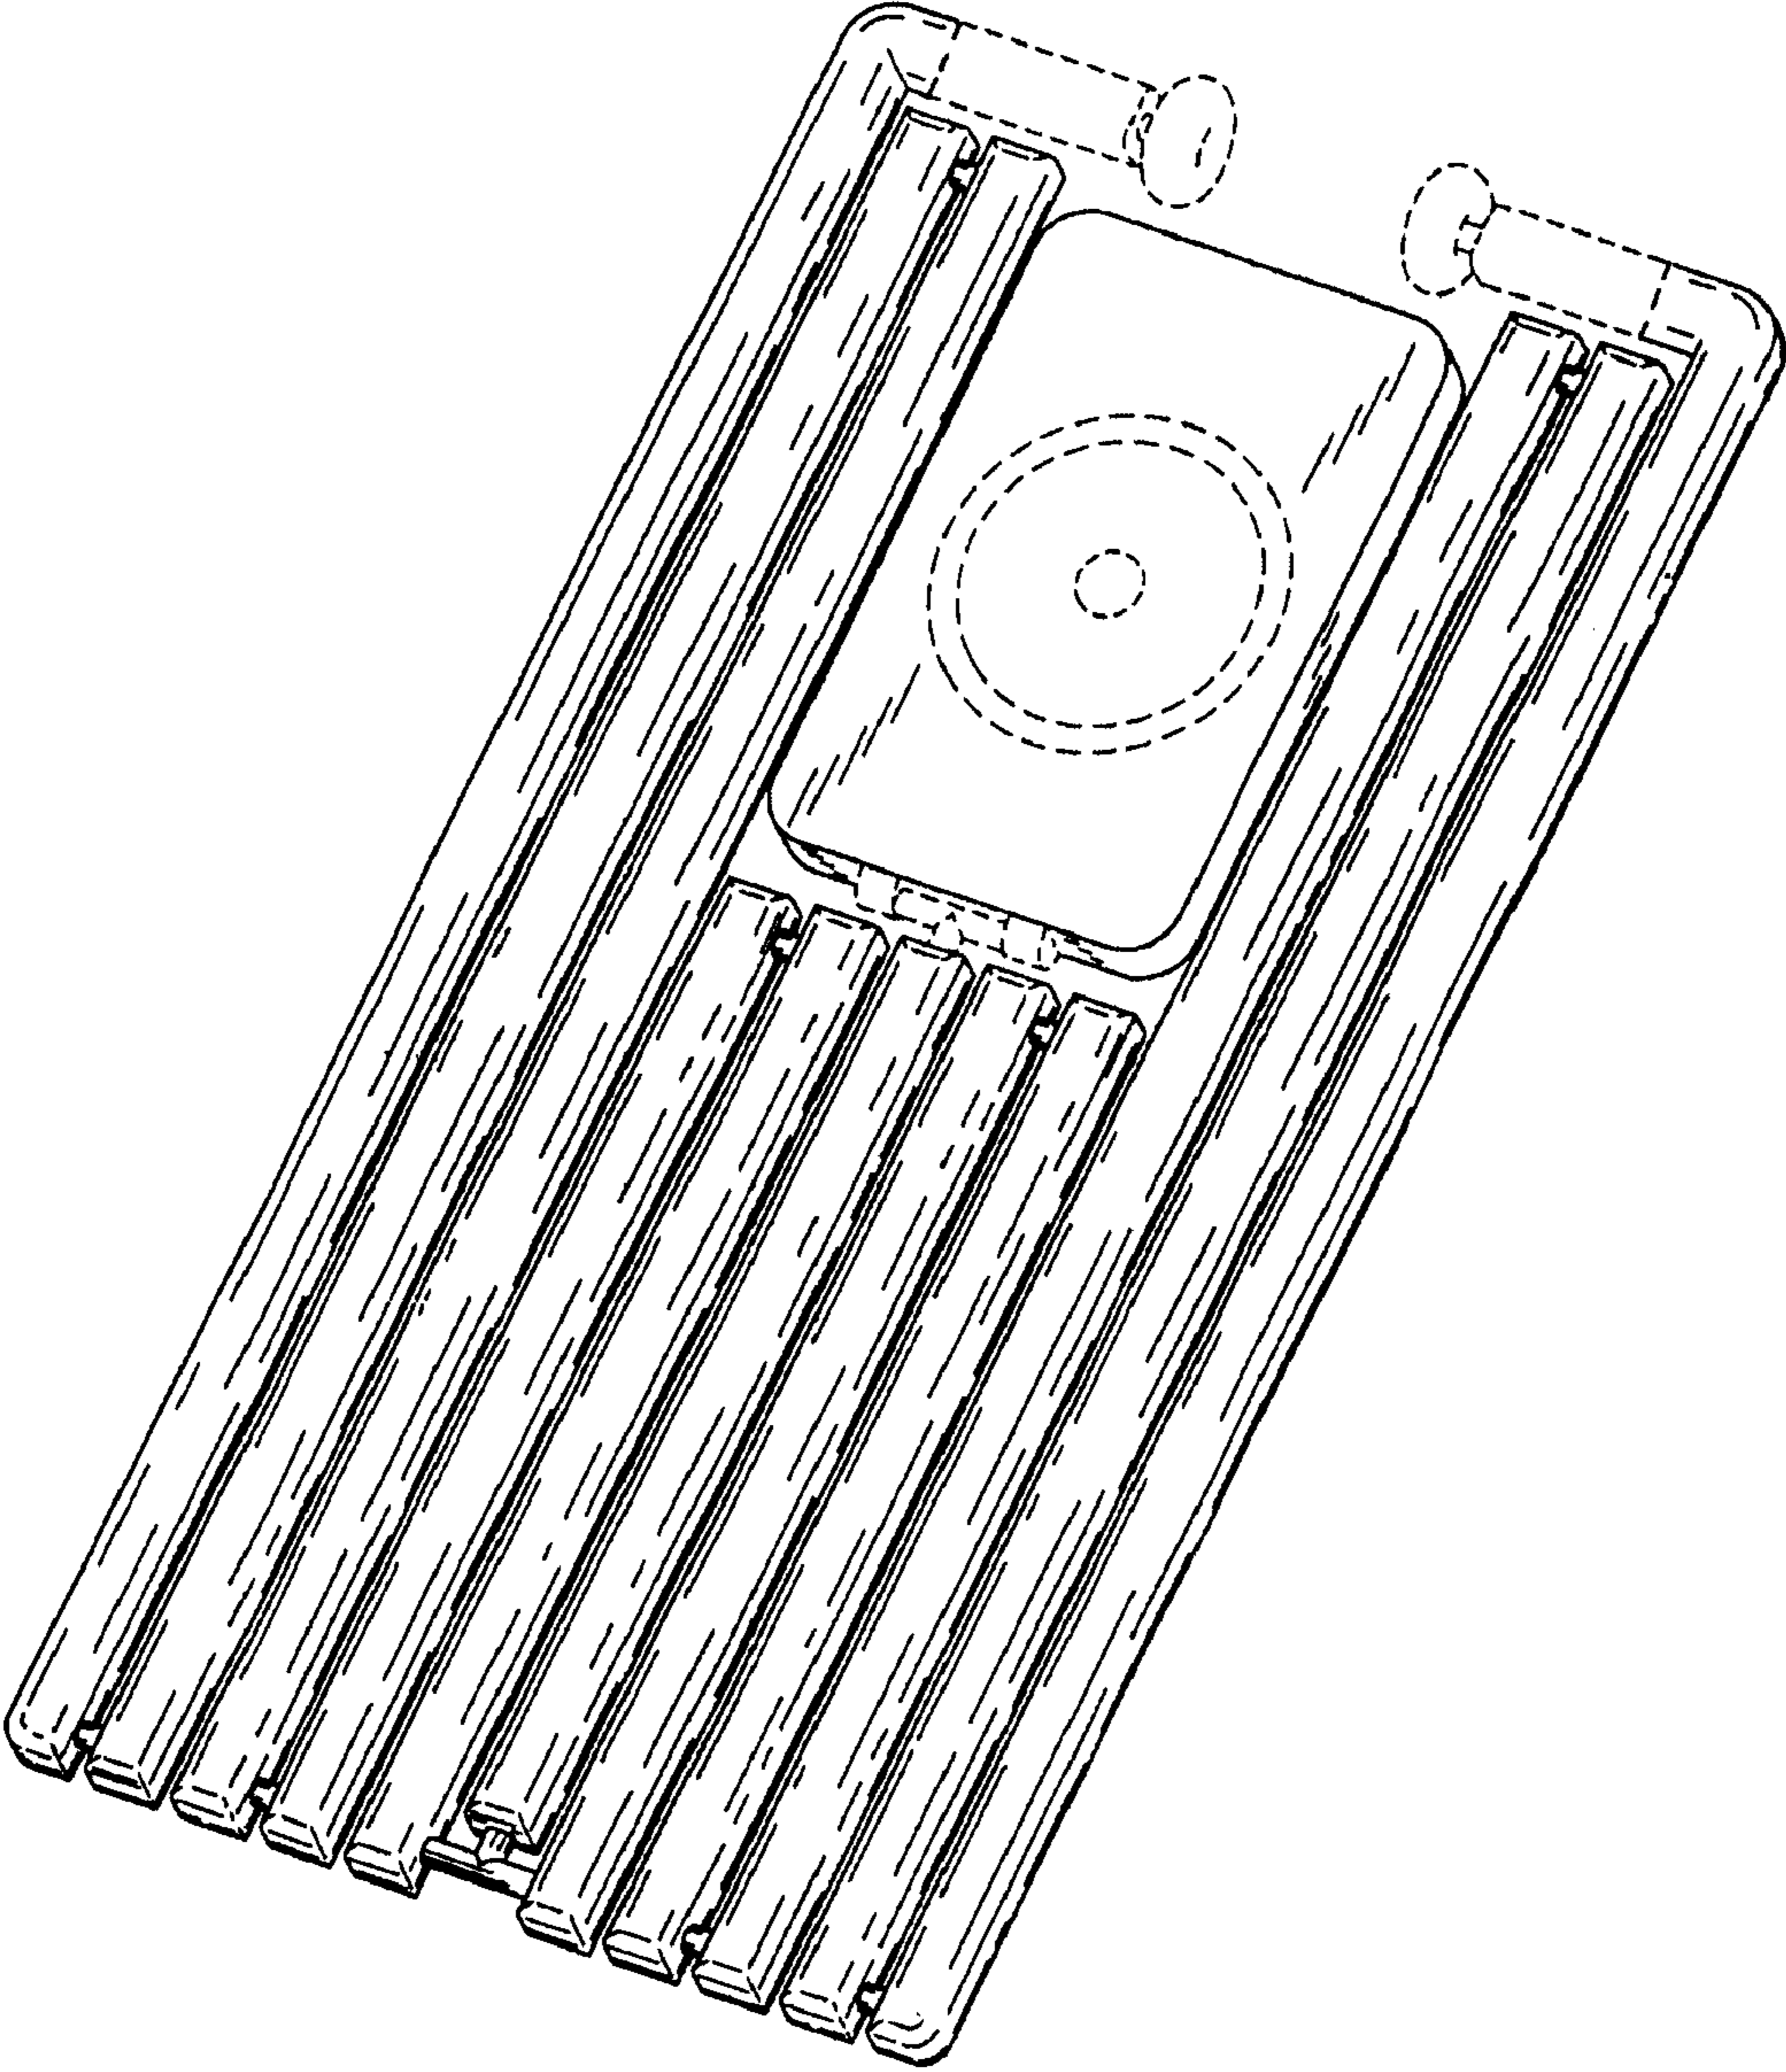


FIG. 1

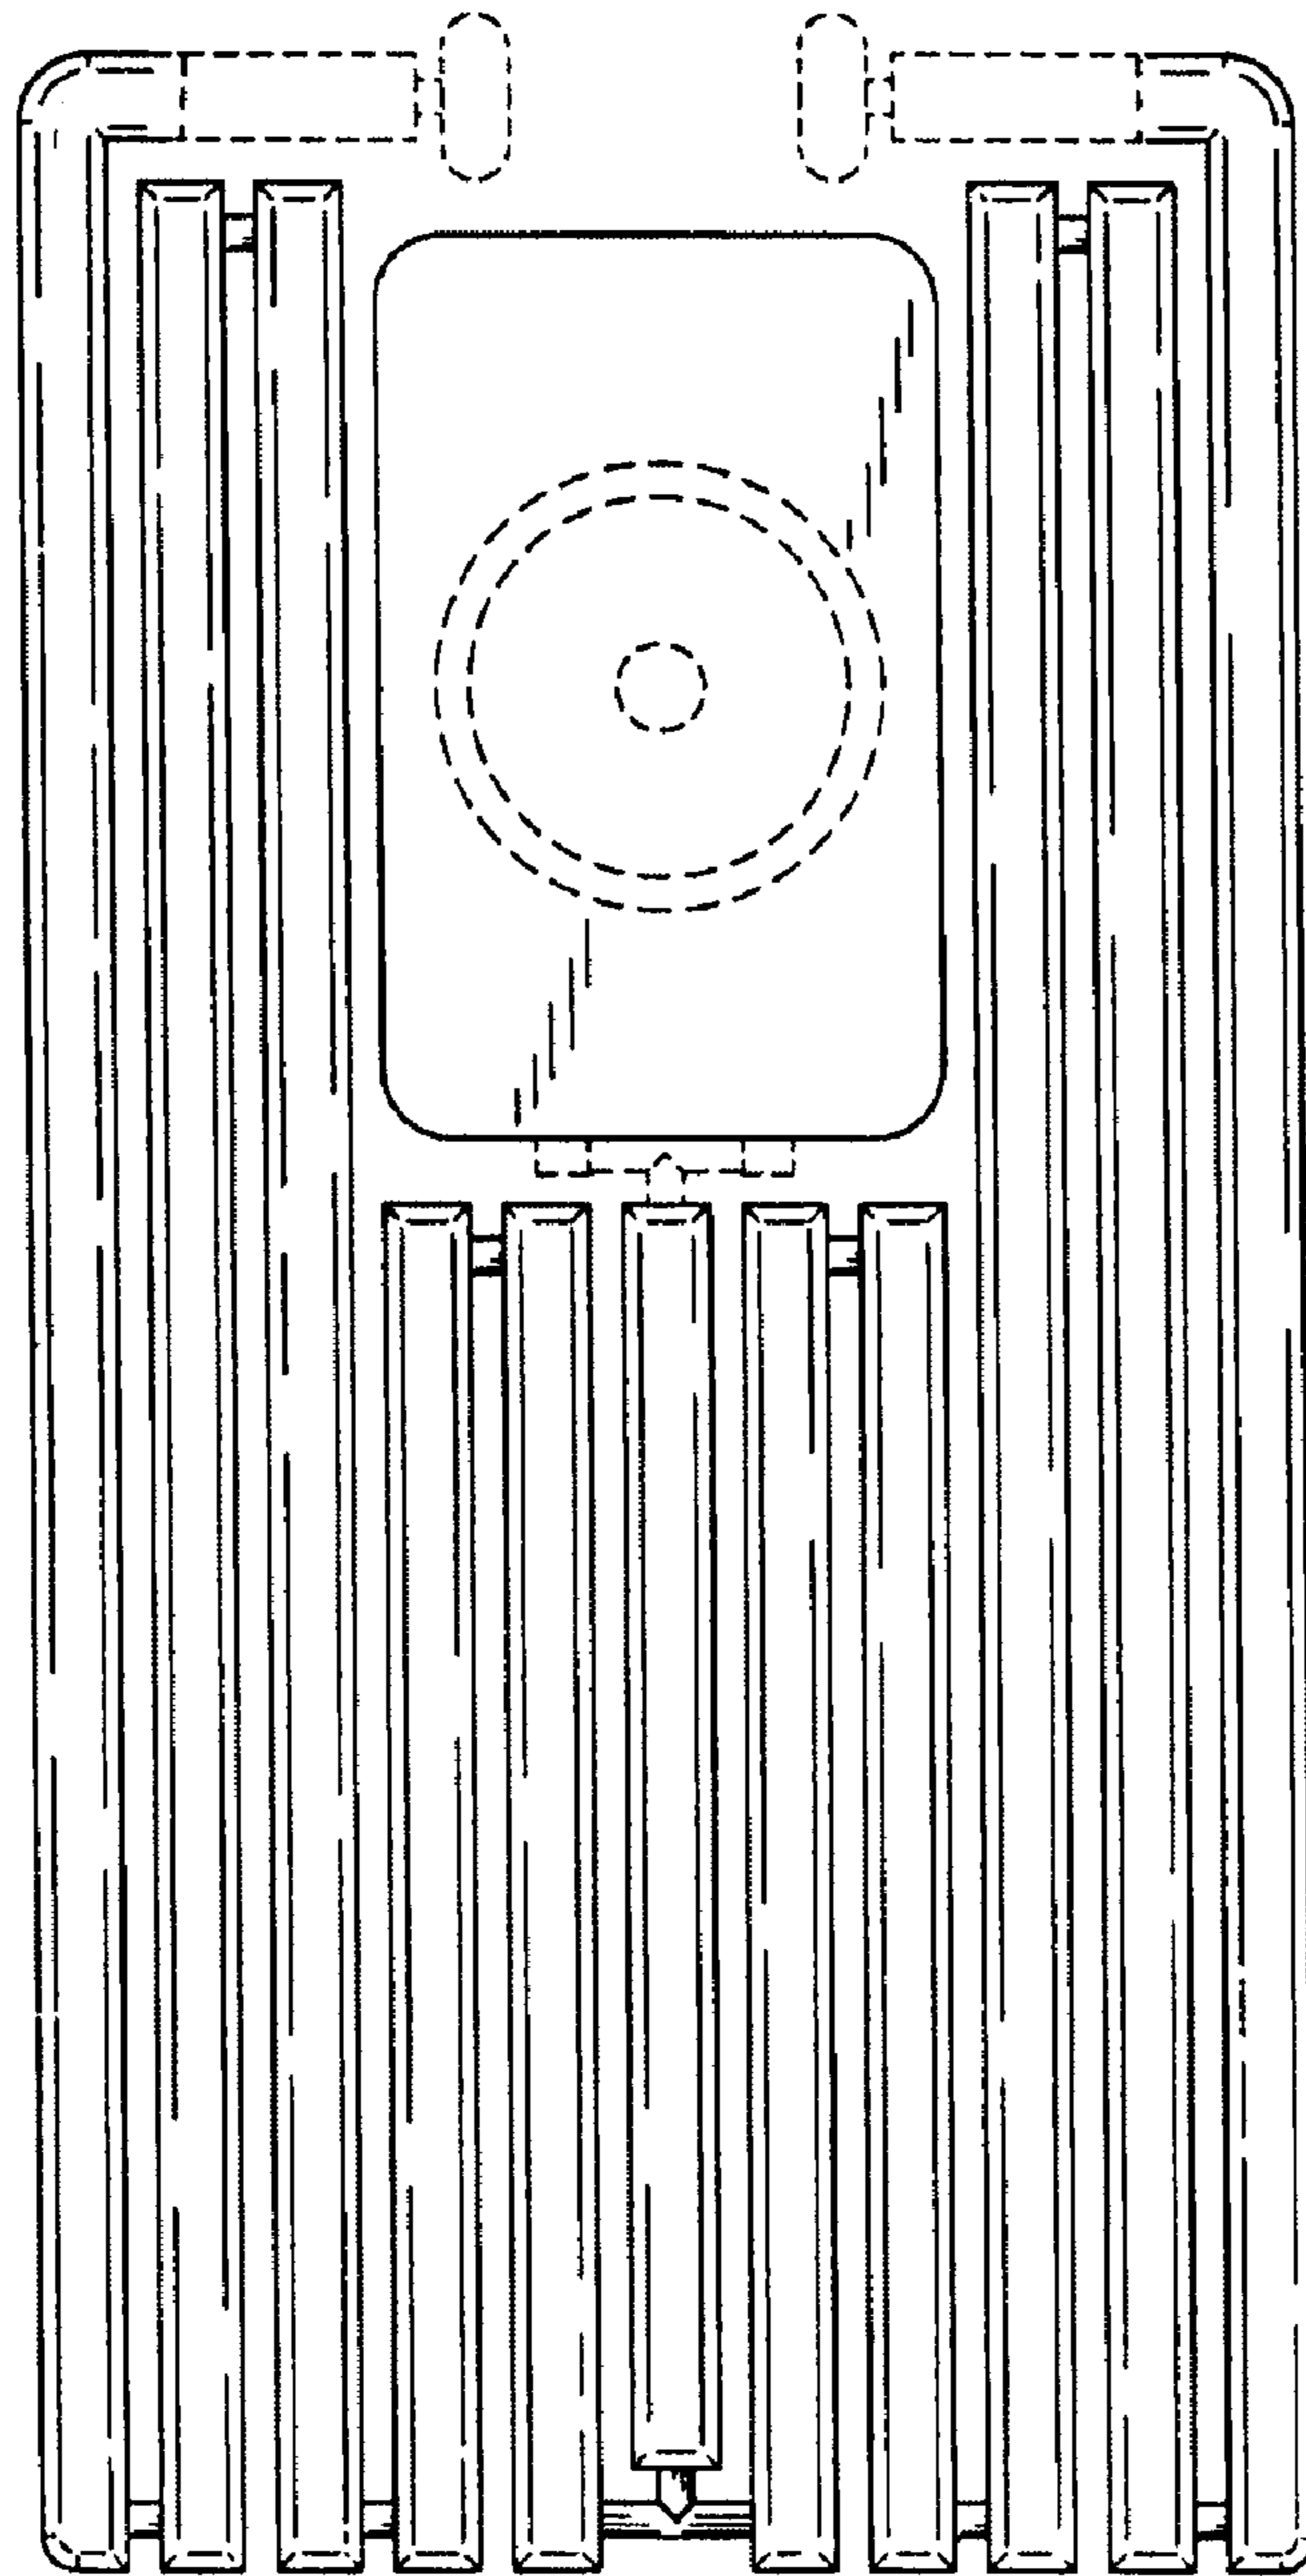


FIG. 2

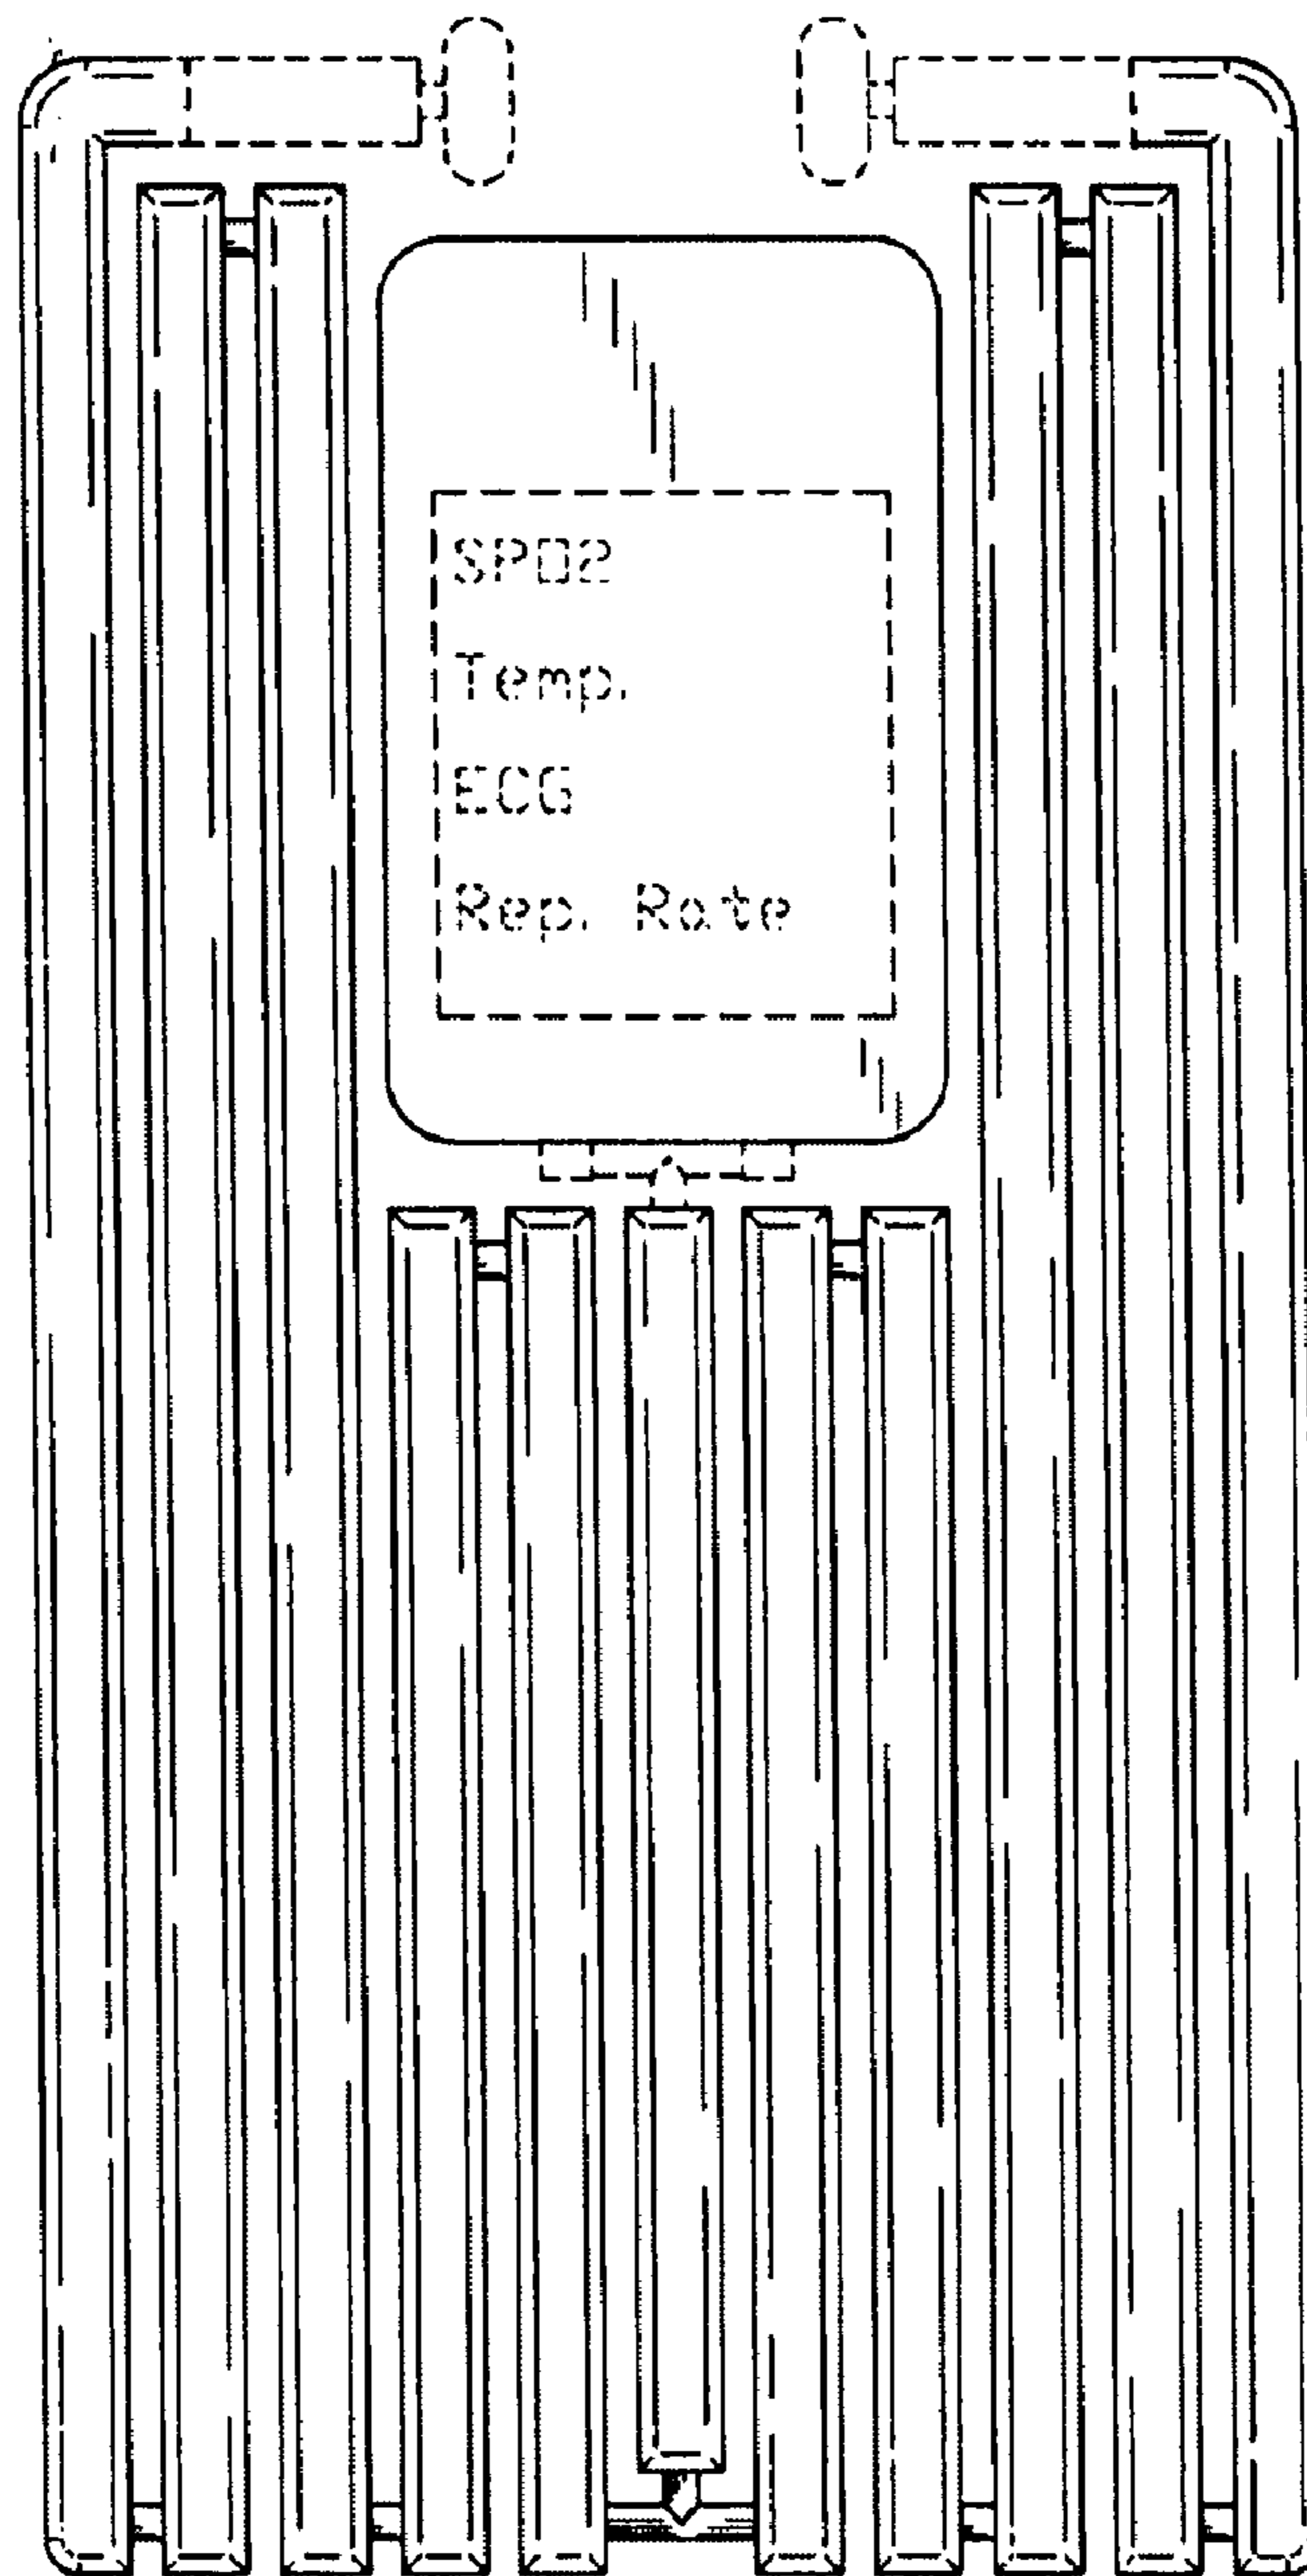


FIG. 3



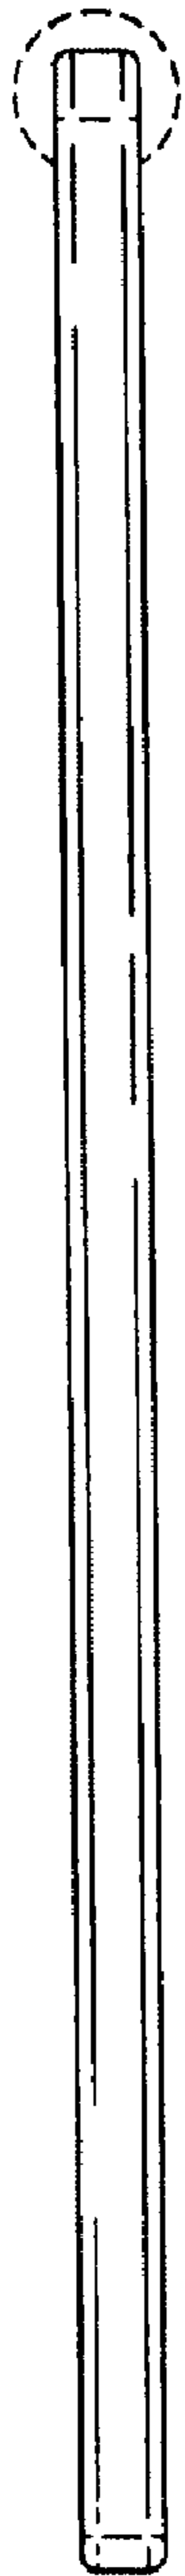


FIG. 4

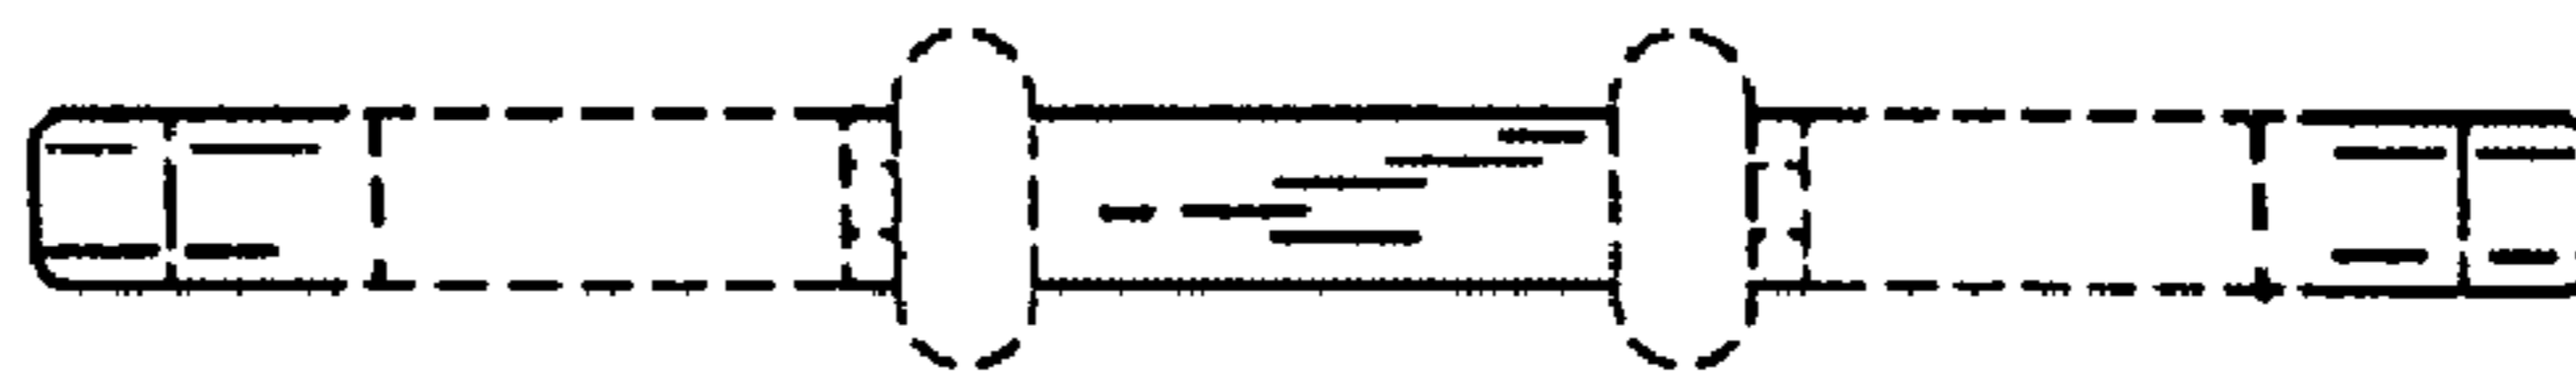


FIG. 5



FIG. 6

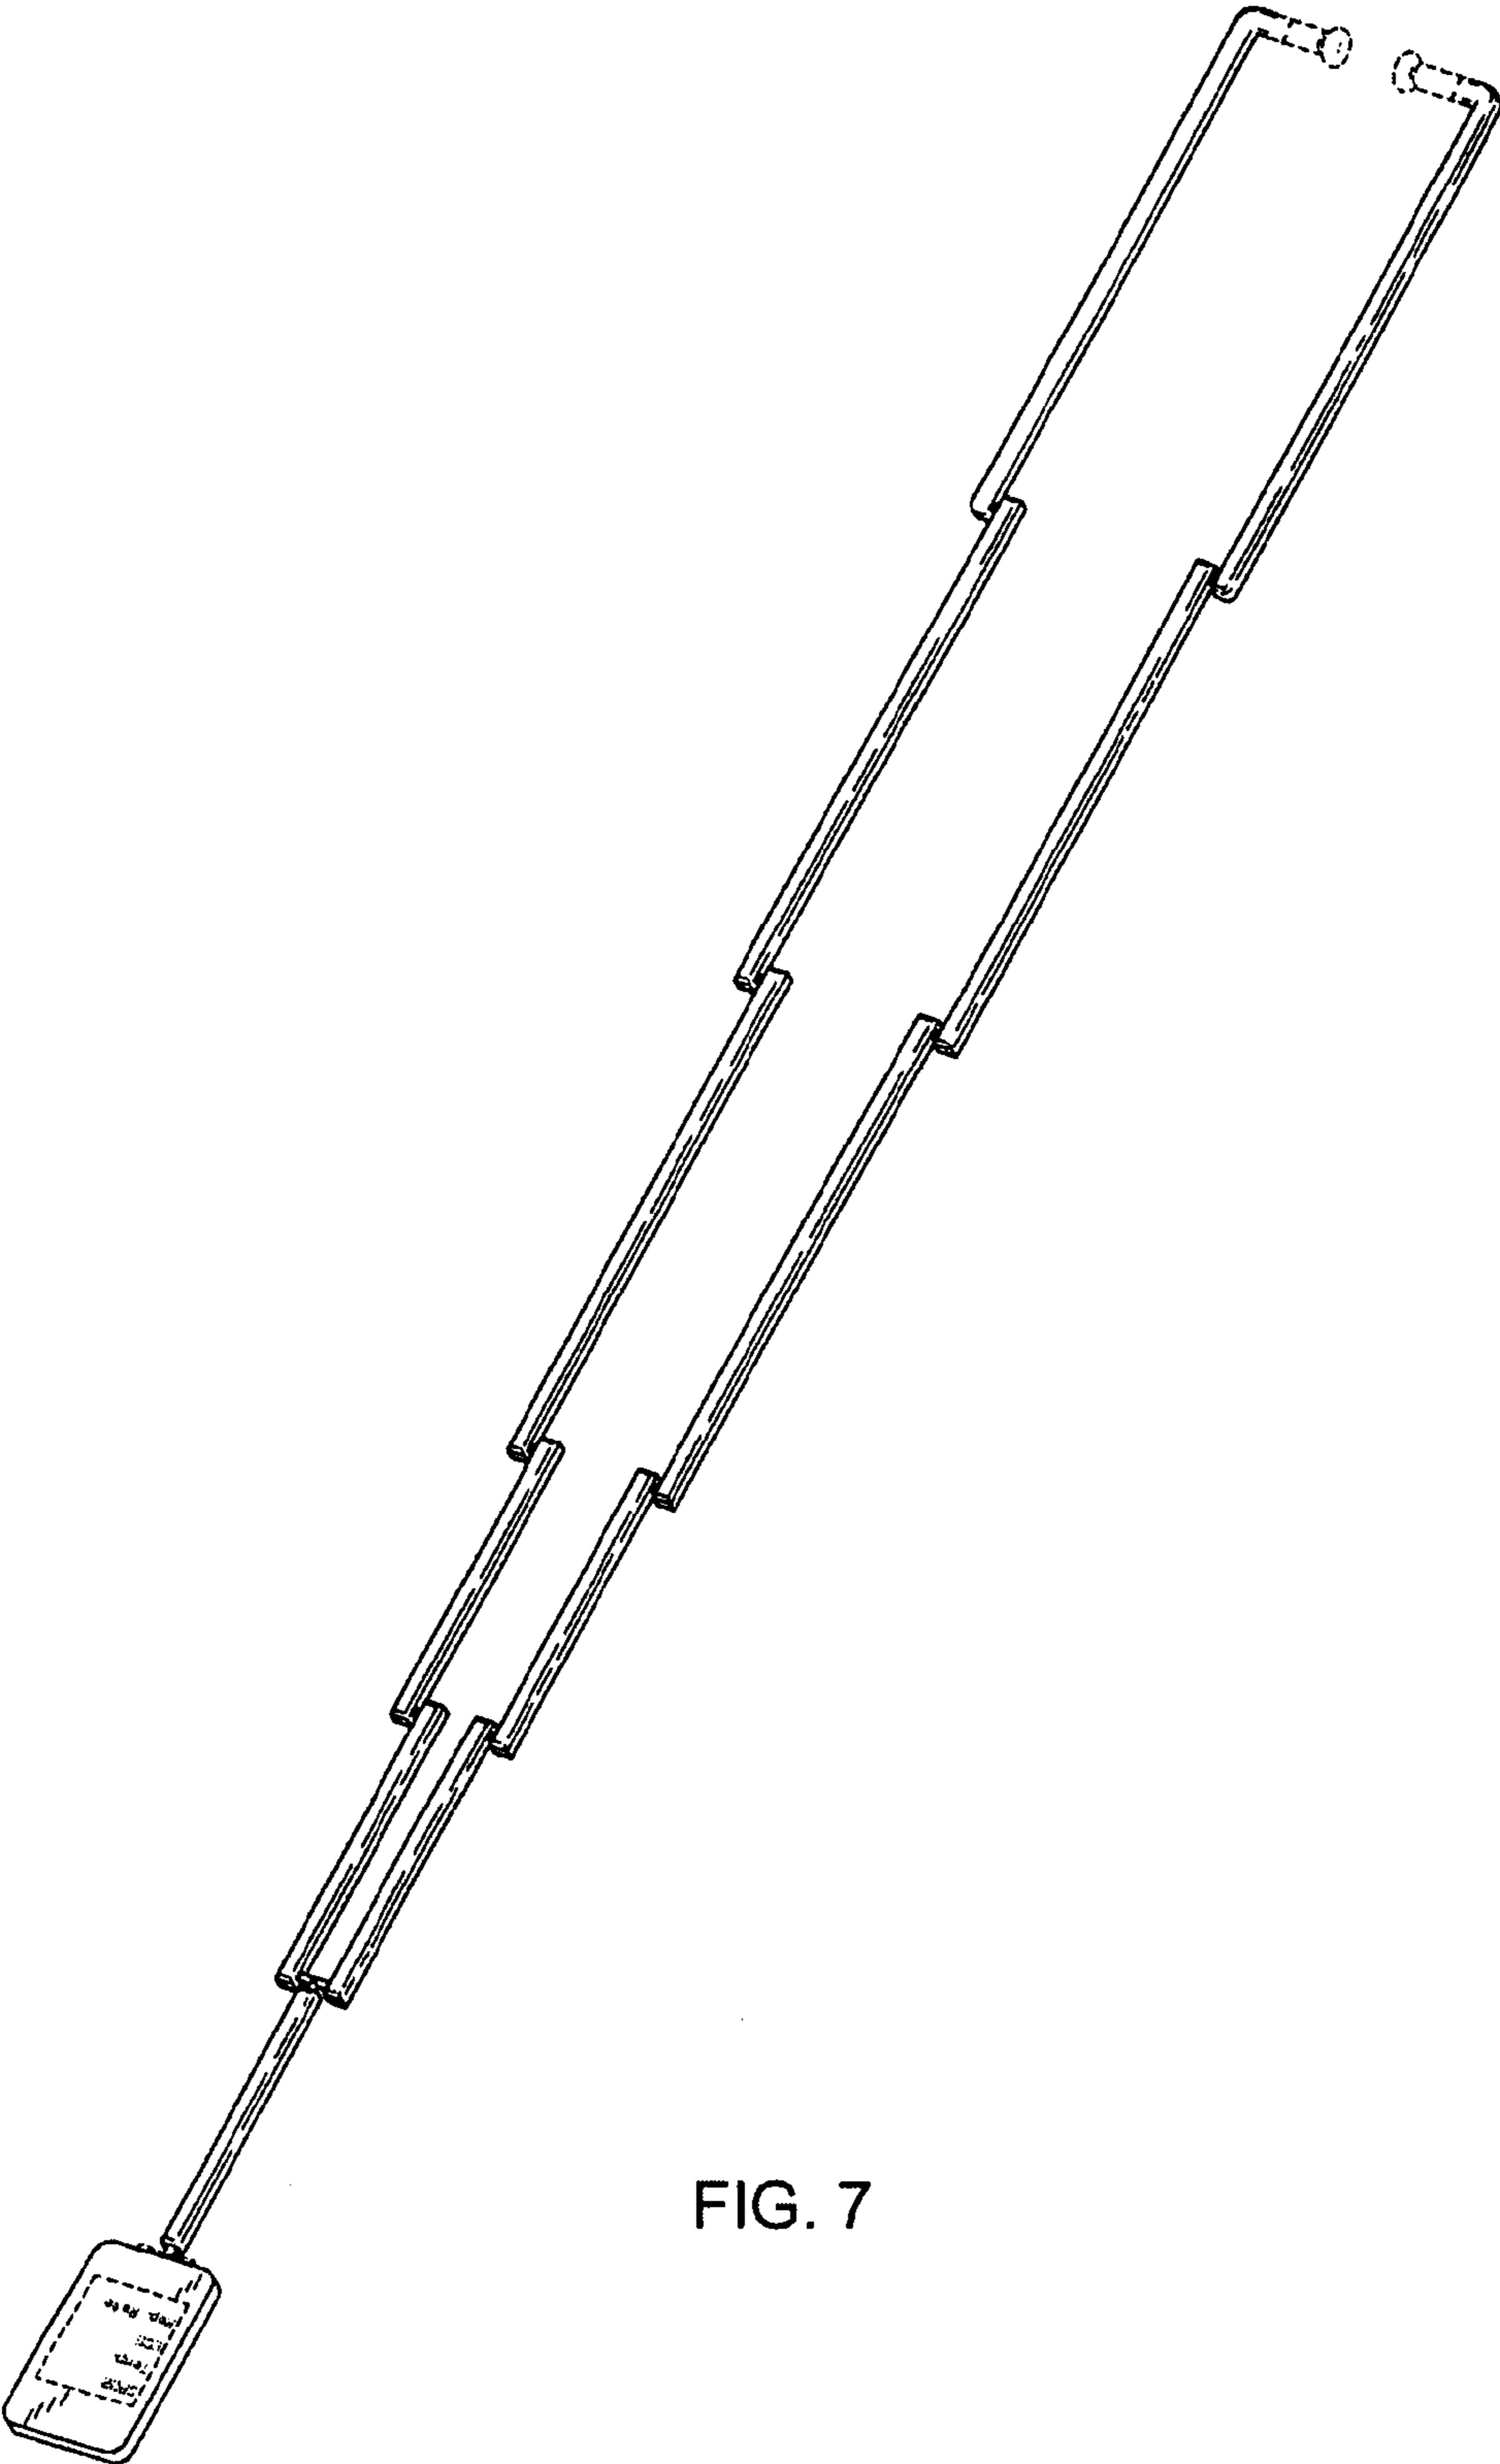


FIG. 7