



US00D675322S

(12) **United States Design Patent**
Jamison et al.

(10) **Patent No.:** **US D675,322 S**
(45) **Date of Patent:** **** Jan. 29, 2013**

(54) **EXAMINATION SYSTEM INCLUDING AN INSTRUMENT STAND AND EXAMINATION CHAIR**

(75) Inventors: **Chris M. Jamison**, West Chester, OH (US); **H. Ray Wright**, Loudon, TN (US); **Antonio Belton**, Richton Park, IL (US); **Dominik J. Beck**, Menlo Park, CA (US)

(73) Assignee: **Reliance Medical Products, Inc.**, Mason, OH (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/404,330**

(22) Filed: **Oct. 19, 2011**

(51) **LOC (9) Cl.** **24-01**

(52) **U.S. Cl.** **D24/178; D24/172**

(58) **Field of Classification Search** D24/172, D24/176-179, 183-185; D6/334, 336, 360-361, D6/501-502, 335, 367, 500; D10/46; 248/127; 297/330, 391, 411.2, 445.1, 447.2, 452.28, 297/452.29; 351/245, 200, 244, 246; 433/33
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,491,242	A	12/1949	Alexander
2,874,689	A	2/1959	Gavelek
3,198,574	A	8/1965	Hayashi et al.
3,259,355	A	7/1966	Slouka
D206,532	S	12/1966	Gardella
D206,585	S	1/1967	Gardella
3,436,046	A	4/1969	Valeska
3,486,789	A	12/1969	Taylor et al.
3,578,379	A	5/1971	Taylor et al.
3,873,152	A	3/1975	Garas
D235,274	S	6/1975	Armbruster
D236,299	S	8/1975	Long
D268,149	S	3/1983	Case
4,415,204	A	11/1983	Cavrak
4,657,217	A	4/1987	Kiesel et al.
D292,526	S	10/1987	Nakayama
4,741,506	A	5/1988	Schwaegerle

(Continued)

OTHER PUBLICATIONS

Topcon IS-2500 Instrument Stand. Cal Coast Ophthalmic Instruments, Inc. Copyright 2005. [Retrieved on Sep. 12, 2012]. Retrieved from the Internet: <URL: <http://www.calcoastophthalmic.com/products/stands/topcon IS2500/>>.*

(Continued)

Primary Examiner — Wan Laymon

(74) *Attorney, Agent, or Firm* — Wood, Herron & Evans, L.L.P.

(57) **CLAIM**

The ornamental design for an examination system including an instrument stand and examination chair, as shown and described.

DESCRIPTION

FIG. 1 is a front perspective view of the examination system including an instrument stand and examination chair according to the invention.

FIG. 2 is a front view of the examination system including an instrument stand and examination chair according to the invention.

FIG. 3 is a left side view of the examination system including an instrument stand and examination chair according to the invention.


FIG. 4 is a right side view of the examination system including an instrument stand and examination chair according to the invention. FIG. 5 is a rear view of the examination system including an instrument stand and examination chair according to the invention.

FIG. 6 is a top view of the examination system including an instrument stand and examination chair according to the invention; and,

FIG. 7 is a bottom view of the examination system including an instrument stand and examination chair according to the invention.

Any elements shown in dash-dot lines form no part of the claimed invention in this application, and are instead included to show environmental aspects of the claimed invention.

1 Claim, 7 Drawing Sheets

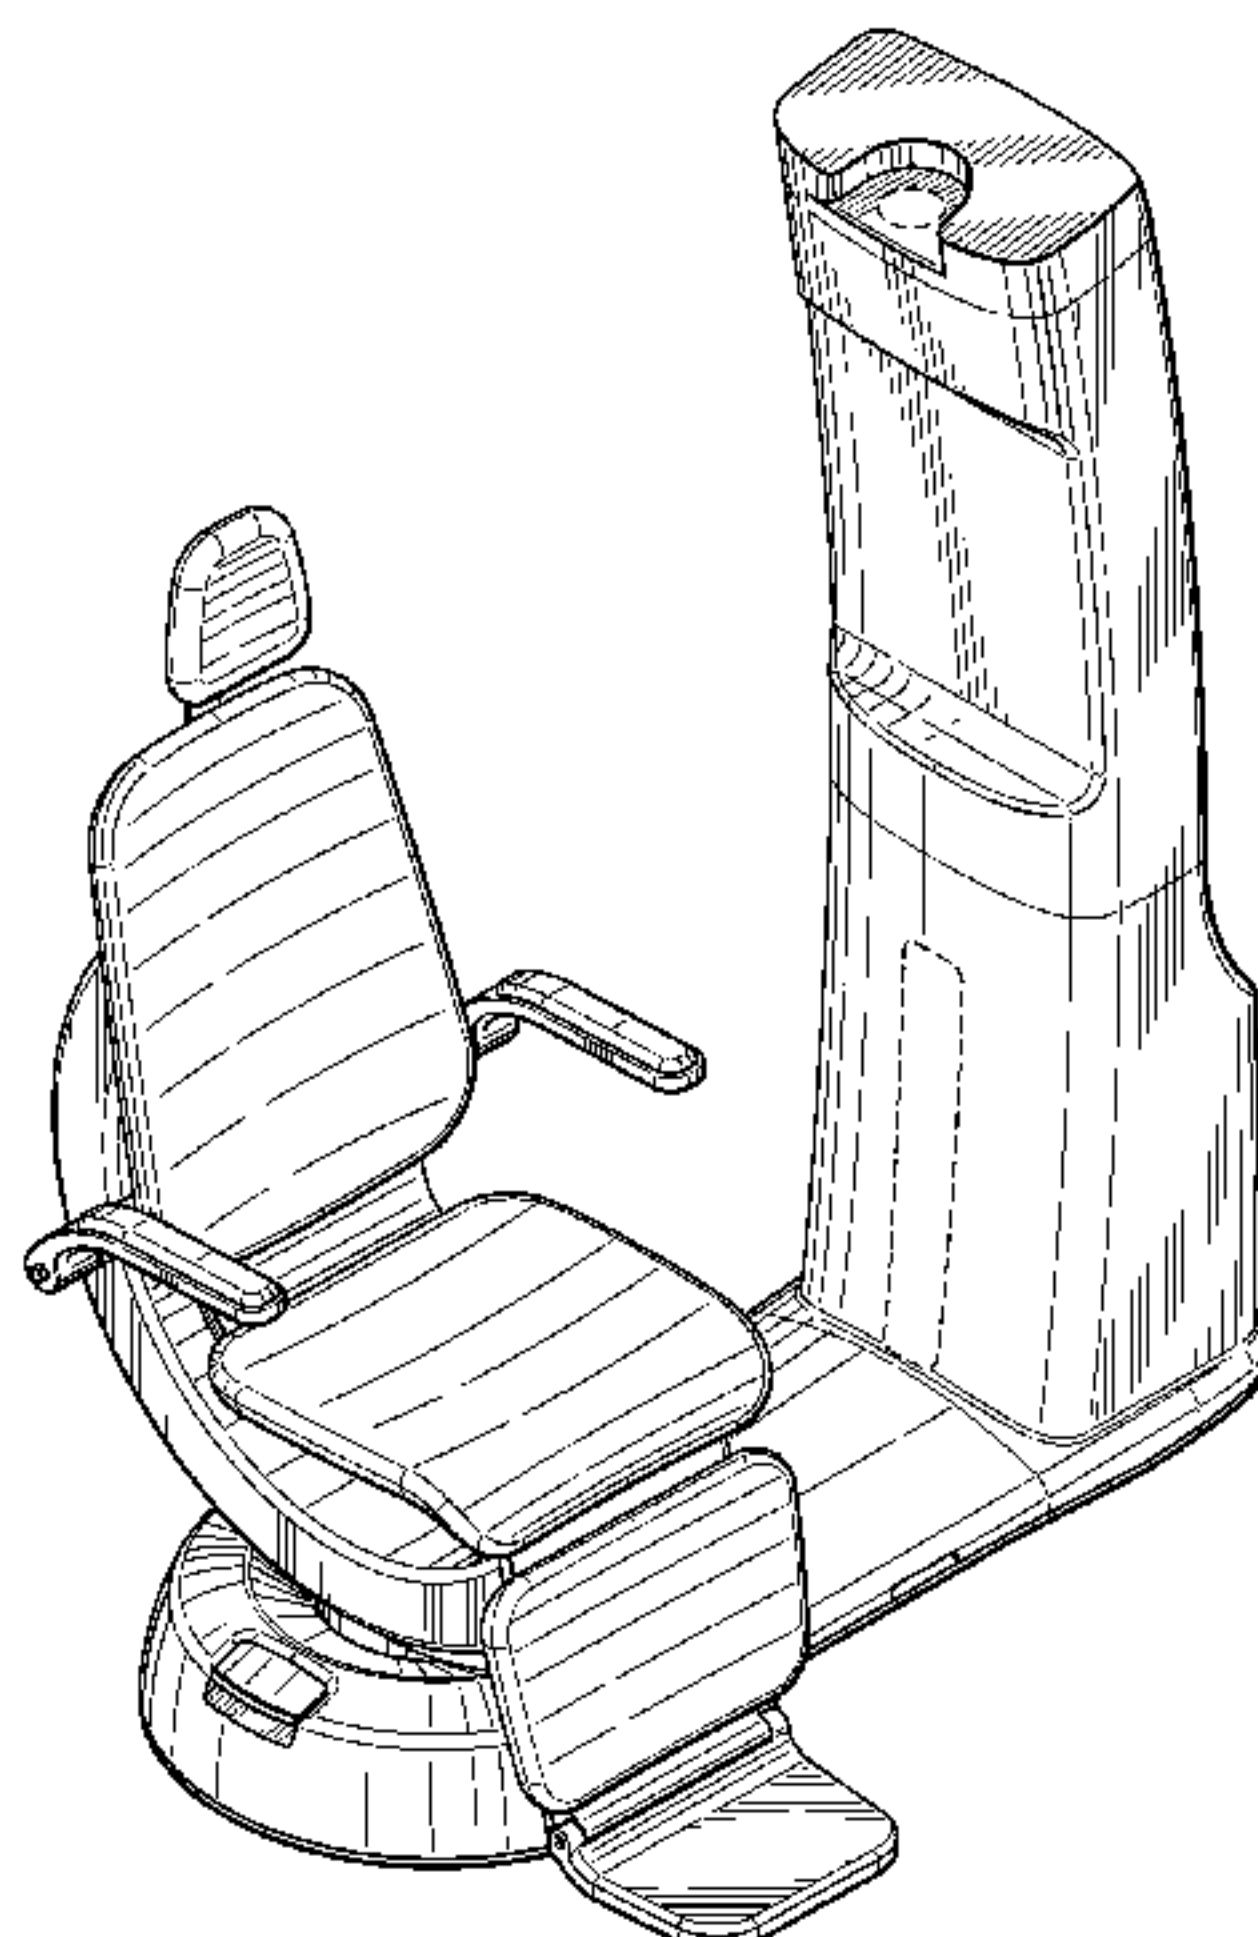

U.S. PATENT DOCUMENTS

D300,657 S 4/1989 Simpkins et al.
4,852,941 A 8/1989 Jones
4,910,386 A 3/1990 Johnson
D321,097 S 10/1991 Jones et al.
5,313,961 A 5/1994 McKee
5,348,375 A 9/1994 Steininger
D352,106 S 11/1994 Fanney et al.
D353,201 S 12/1994 Crook et al.
D354,176 S 1/1995 Schwaegerle et al.
D354,177 S 1/1995 Schwaegerle et al.
5,399,007 A 3/1995 Marconet
D361,674 S 8/1995 Carter, Sr.
5,461,965 A 10/1995 Schwaegerle
5,467,002 A 11/1995 Brooks
5,480,212 A 1/1996 Marconet
5,520,363 A 5/1996 Burton et al.
5,580,023 A 12/1996 Burton et al.
D378,315 S 3/1997 Schwaegerle et al.
5,624,159 A 4/1997 Celoni et al.
D379,409 S 5/1997 Schwaegerle et al.
5,645,313 A 7/1997 Best et al.
D384,154 S * 9/1997 Malmen et al. D24/178
5,696,574 A 12/1997 Schwaegerle
5,717,480 A 2/1998 Brooks et al.
5,777,344 A 7/1998 Hayashi
D397,259 S 8/1998 Chatani et al.
D407,379 S 3/1999 Schwaegerle
5,907,387 A 5/1999 Schwaegerle
D412,621 S 8/1999 Smith et al.
D412,801 S 8/1999 Smith et al.
5,992,934 A 11/1999 Gehrig et al.
D418,339 S 1/2000 Smith et al.
D418,686 S 1/2000 Smith et al.
D419,343 S 1/2000 Smith et al.
D420,233 S 2/2000 Smith et al.
D423,262 S 4/2000 Smith et al.
D424,200 S 5/2000 Smith
D424,337 S 5/2000 Smith et al.
D425,341 S 5/2000 Smith et al.
D425,735 S 5/2000 Smith et al.
D425,991 S 5/2000 Smith et al.
D426,715 S 6/2000 Smith et al.

6,095,649 A 8/2000 Brooks et al.
6,106,065 A 8/2000 Carroll
D433,588 S 11/2000 Smith et al.
6,264,329 B1 7/2001 Brooks et al.
D456,080 S 4/2002 Karlsson
D456,158 S 4/2002 Van Severen
6,382,725 B1 5/2002 Carroll
D458,378 S 6/2002 Bevington
6,575,575 B2 6/2003 O'Brien et al.
6,721,976 B2 4/2004 Schwaegerle
6,736,360 B1 5/2004 Buczek
6,761,454 B2 * 7/2004 Lai et al. 351/216
D503,233 S 3/2005 Smith
D504,515 S 4/2005 Smith
6,886,199 B1 5/2005 Schwaegerle
D506,257 S 6/2005 Smith
6,928,676 B1 8/2005 Schwaegerle
D509,079 S 9/2005 Natuzzi
D509,371 S 9/2005 Natuzzi
D512,507 S 12/2005 Smith
D514,701 S 2/2006 Smith
D531,318 S 10/2006 Morral Gispert
D533,368 S 12/2006 Natuzzi
7,207,531 B2 4/2007 Piontkowski
7,401,921 B2 7/2008 Baker et al.
7,467,871 B2 12/2008 Lawhorn et al.
D602,269 S 10/2009 Jamison et al.
7,670,003 B2 3/2010 Kendrick
D621,050 S 8/2010 Jamison et al.
7,954,950 B2 * 6/2011 Dreher et al. 351/246
2011/0147546 A1 6/2011 Monsalve et al.

OTHER PUBLICATIONS

Ophthalmic Chair And Instrument Stand Model 1500. Protech Ophthalmics. Copyright 2012. [Retrieved on Sep. 12, 2012]. Retrieved from the Internet: <URL: <http://www.eyedoctorsupply.com/servlet/the-140/Ophthalmic-Chair-And-Instrument/Detail>>.*
Topcon CSIII Chair and Stand. Vision Systems Inc. [Retrieved on Sep. 12, 2012]. Retrieved from the Internet: <URL: <http://www.patternless.com/topcon-csiii-chair-and-stand/>>.*

* cited by examiner

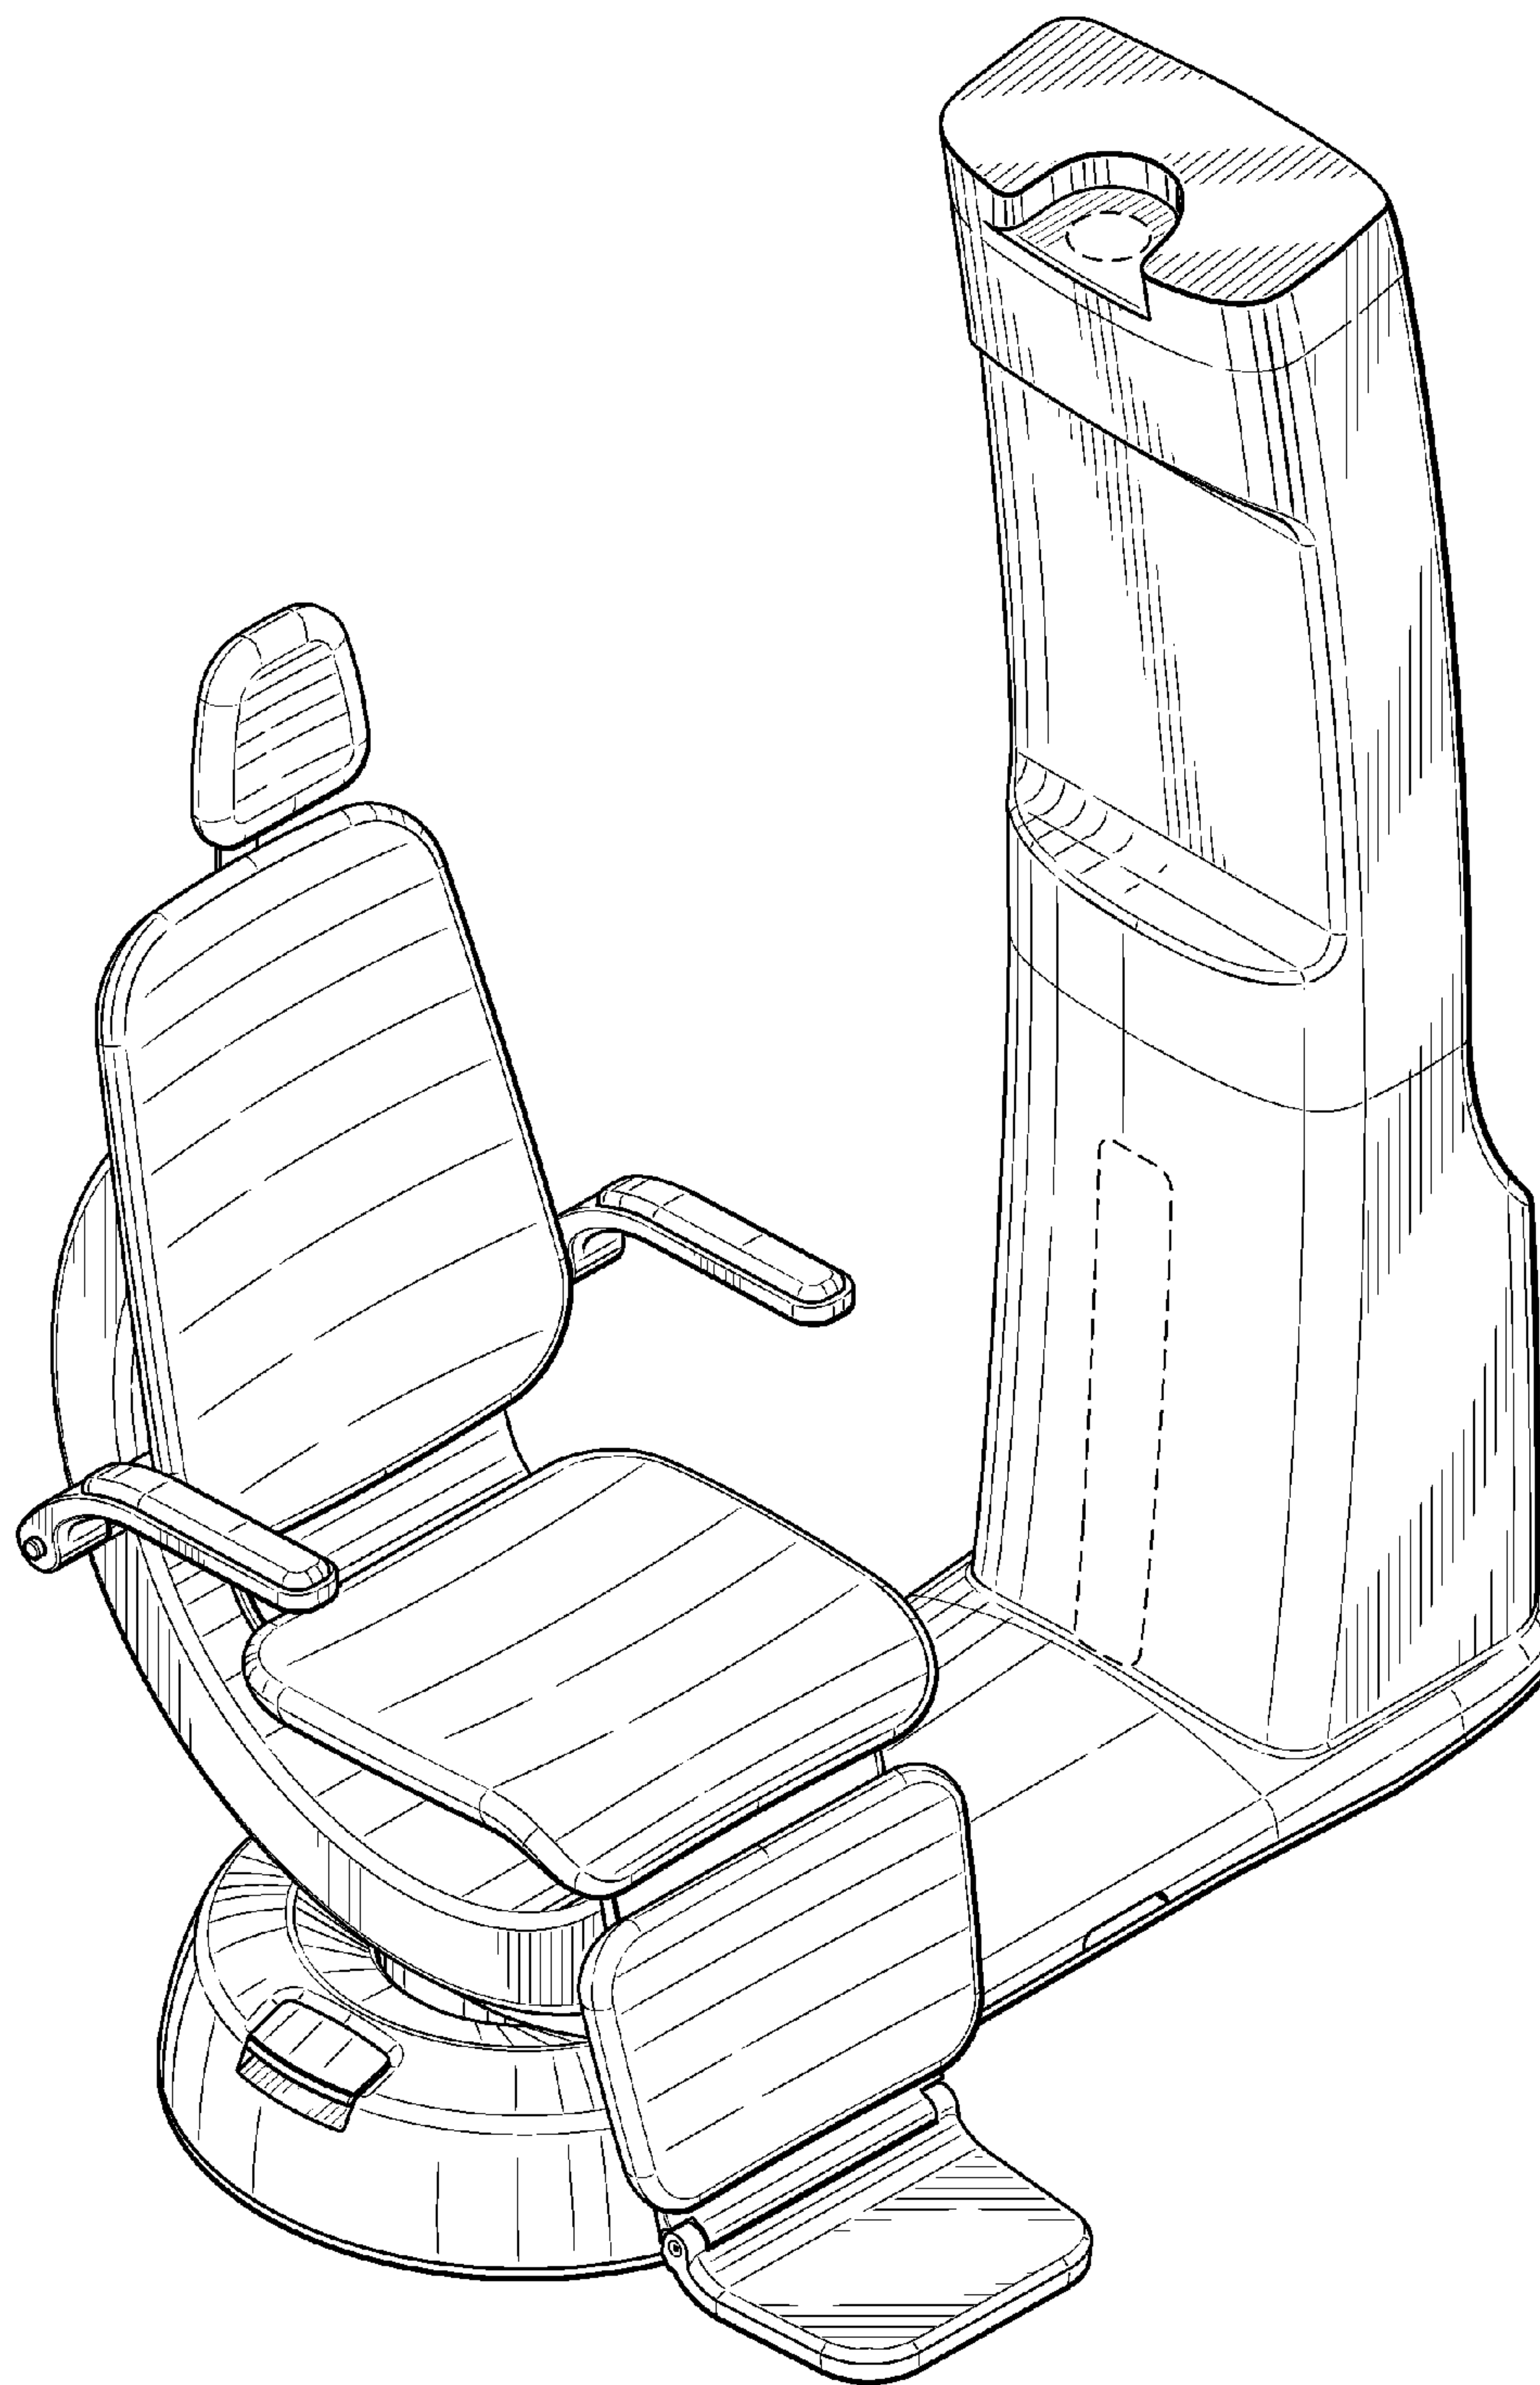


FIG. 1

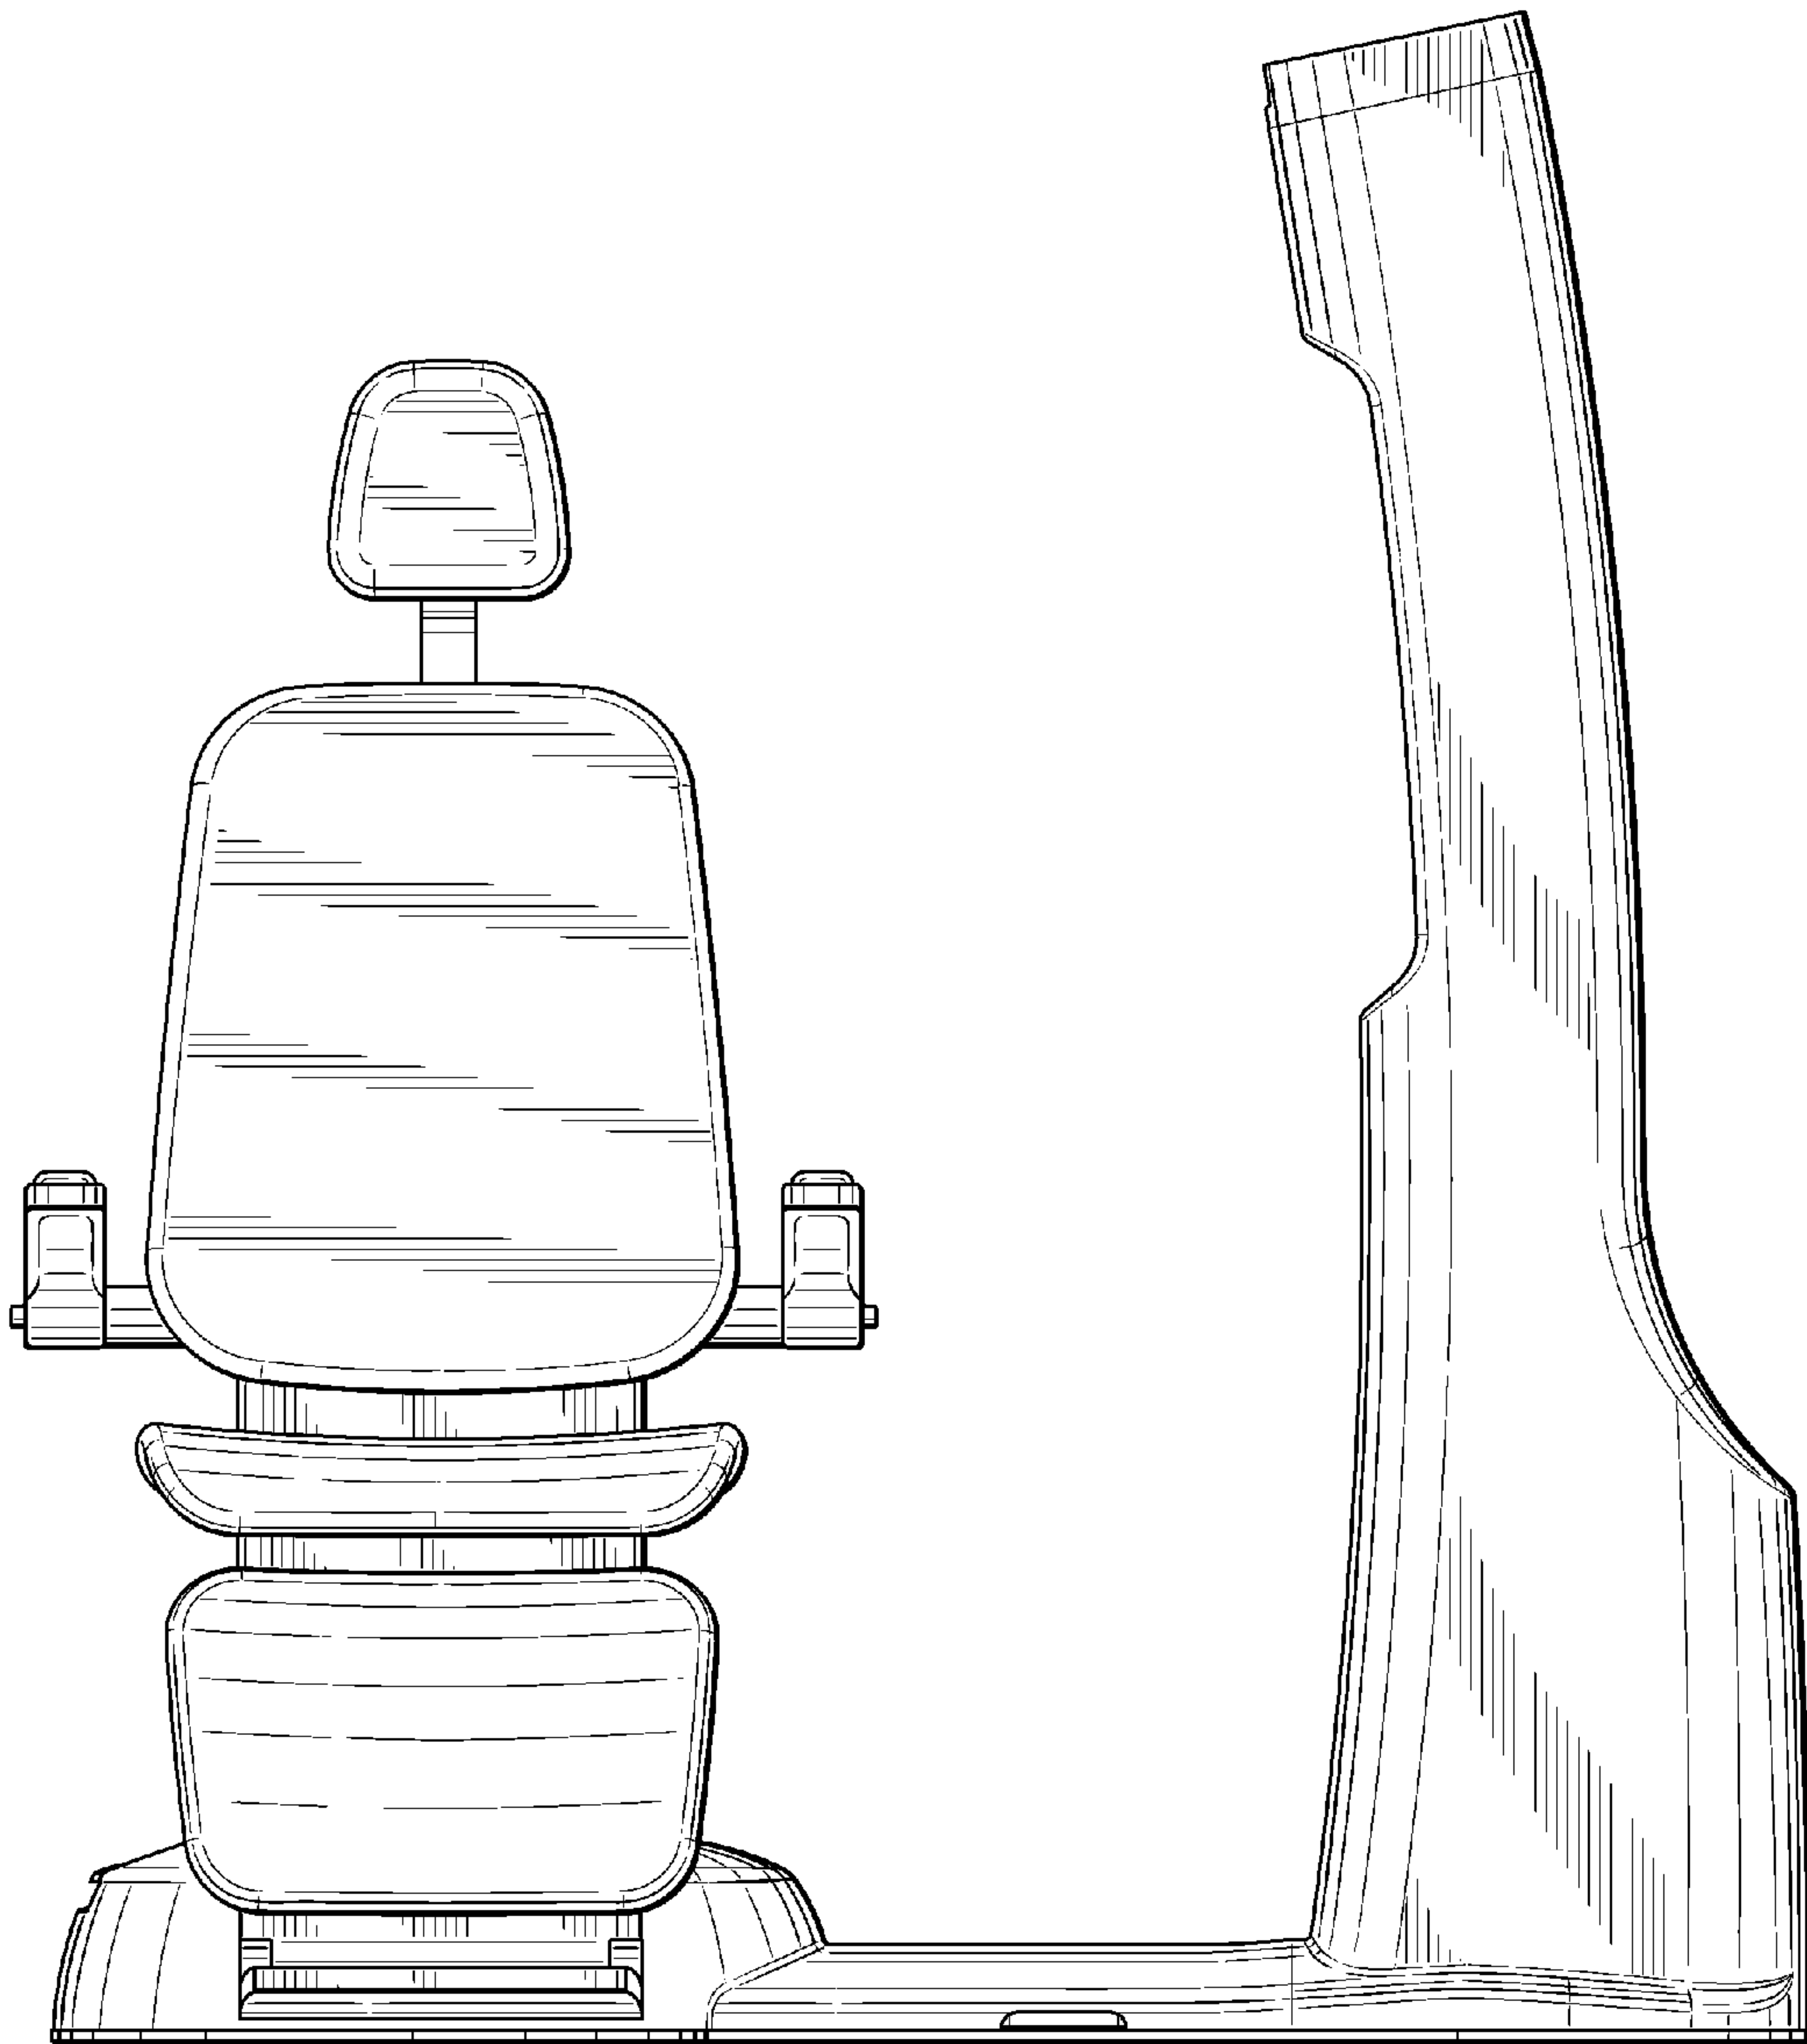


FIG. 2

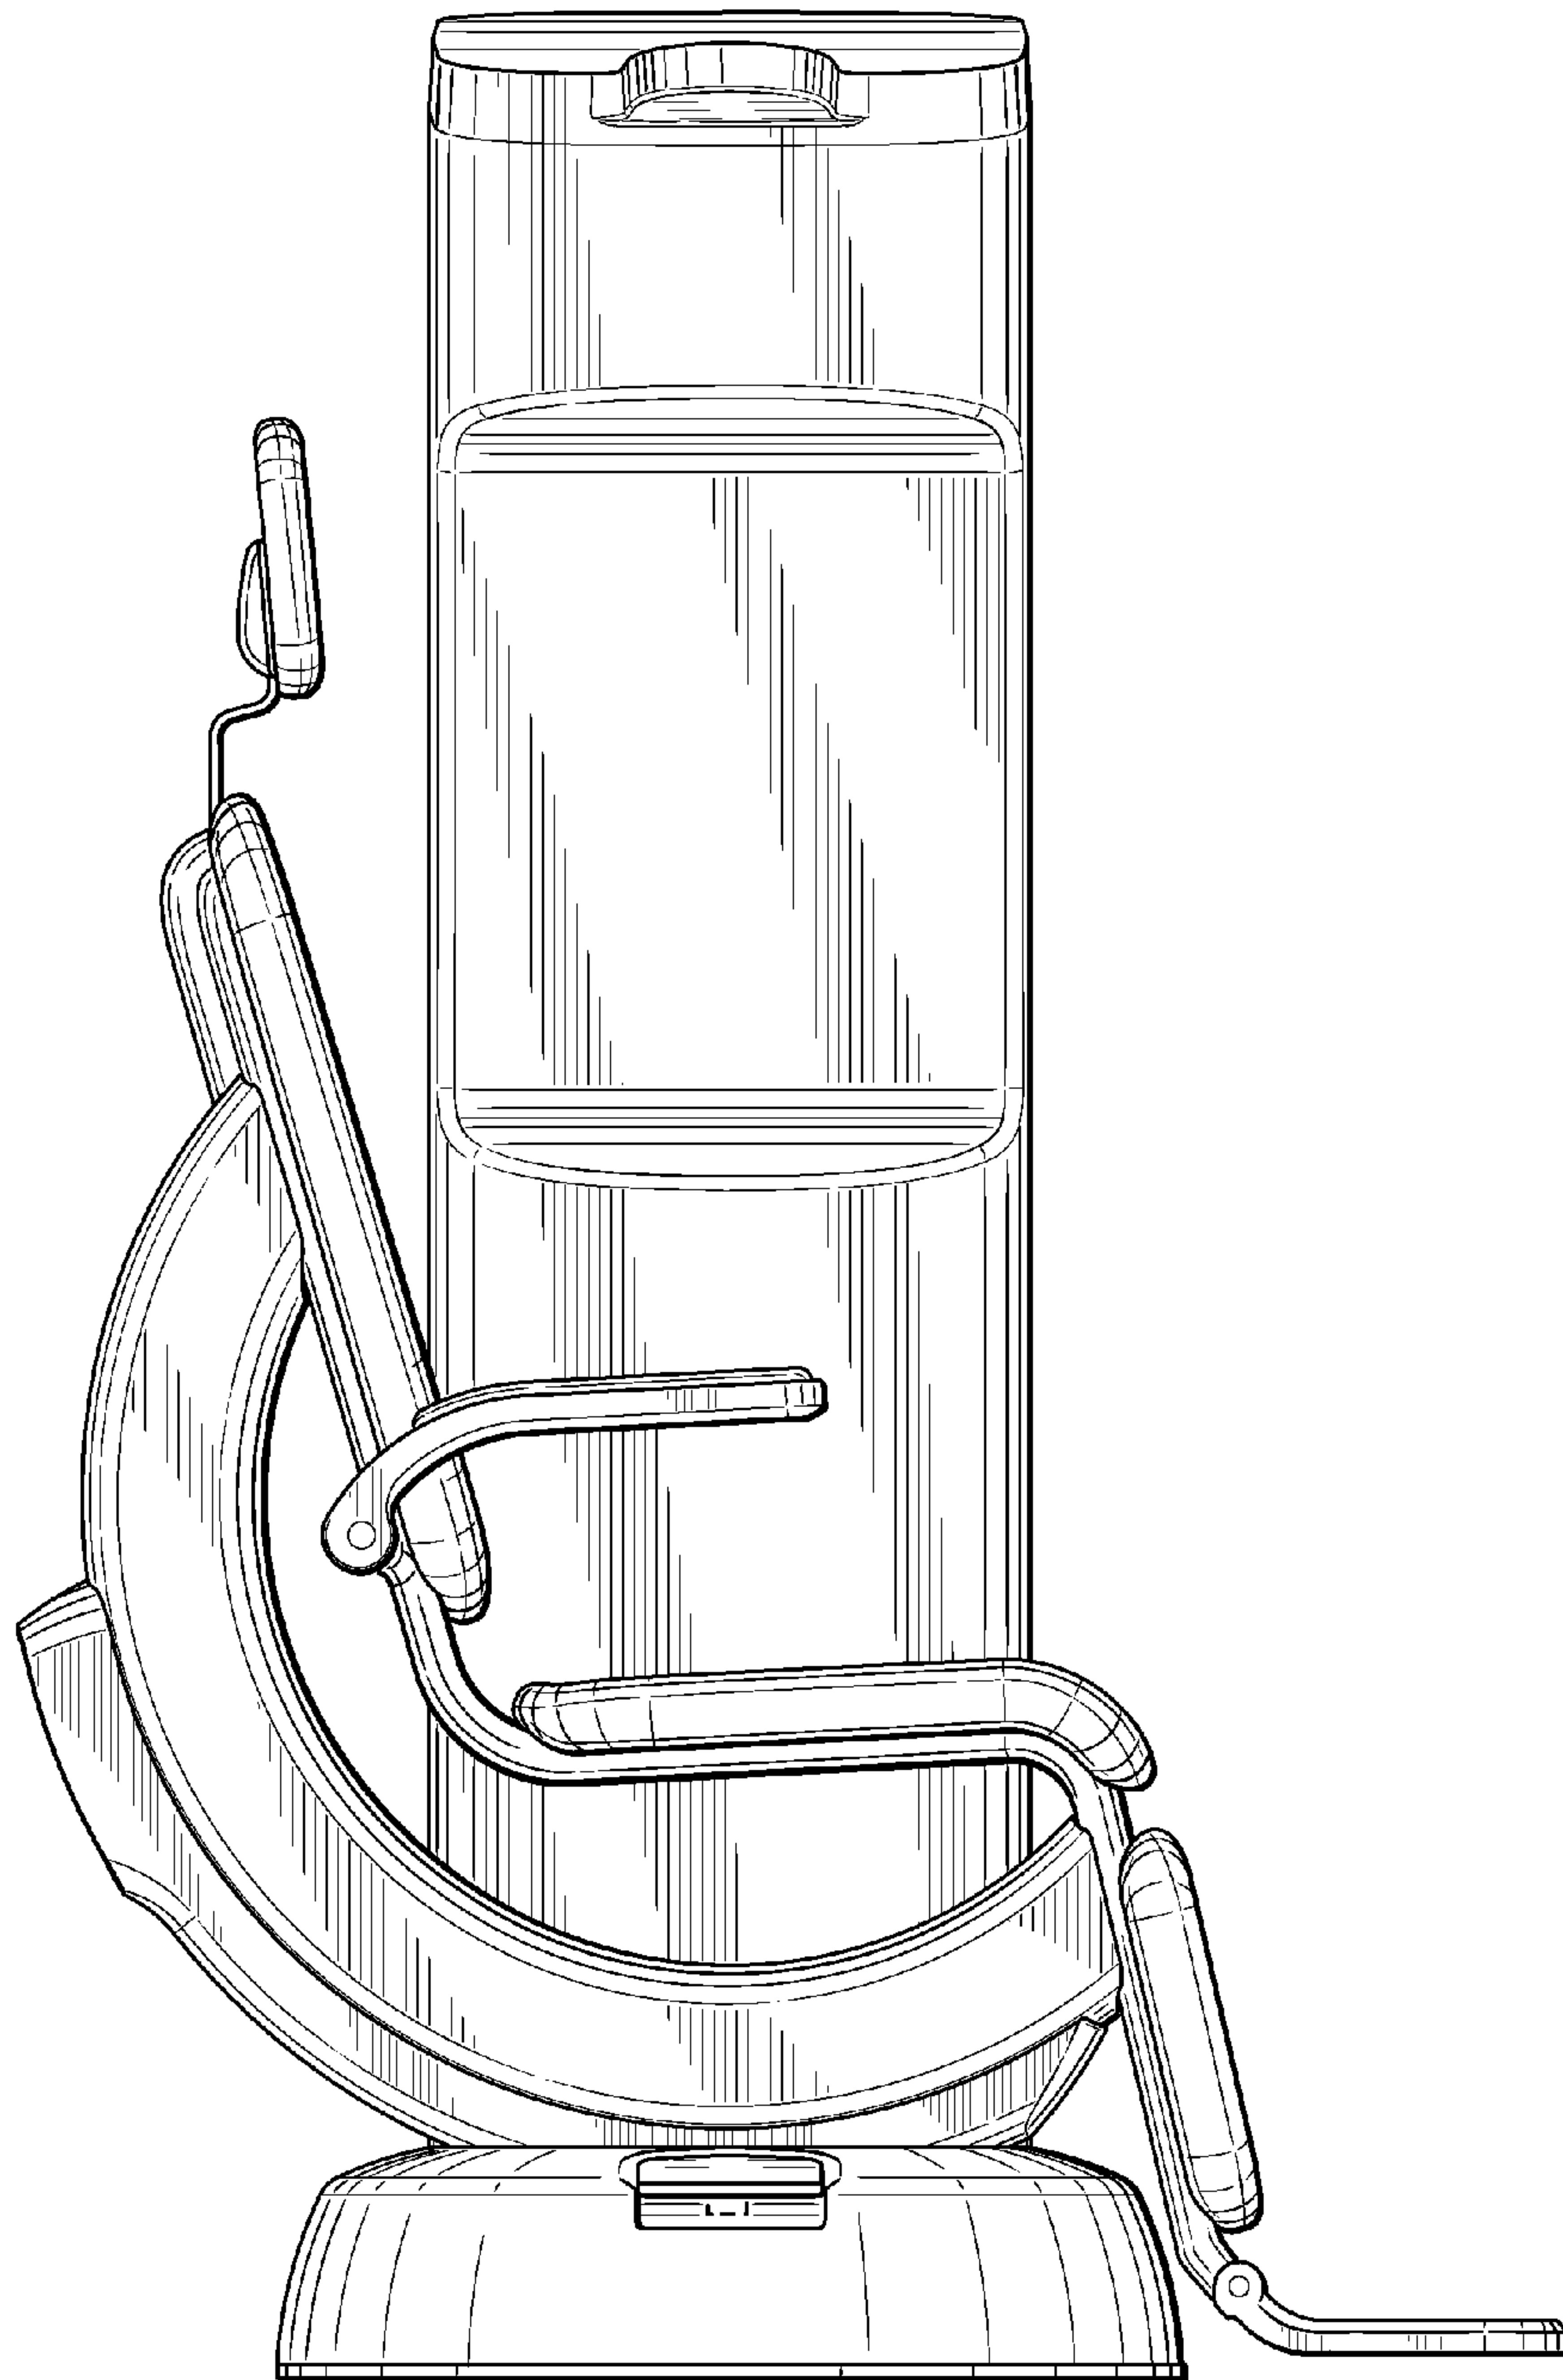


FIG. 3

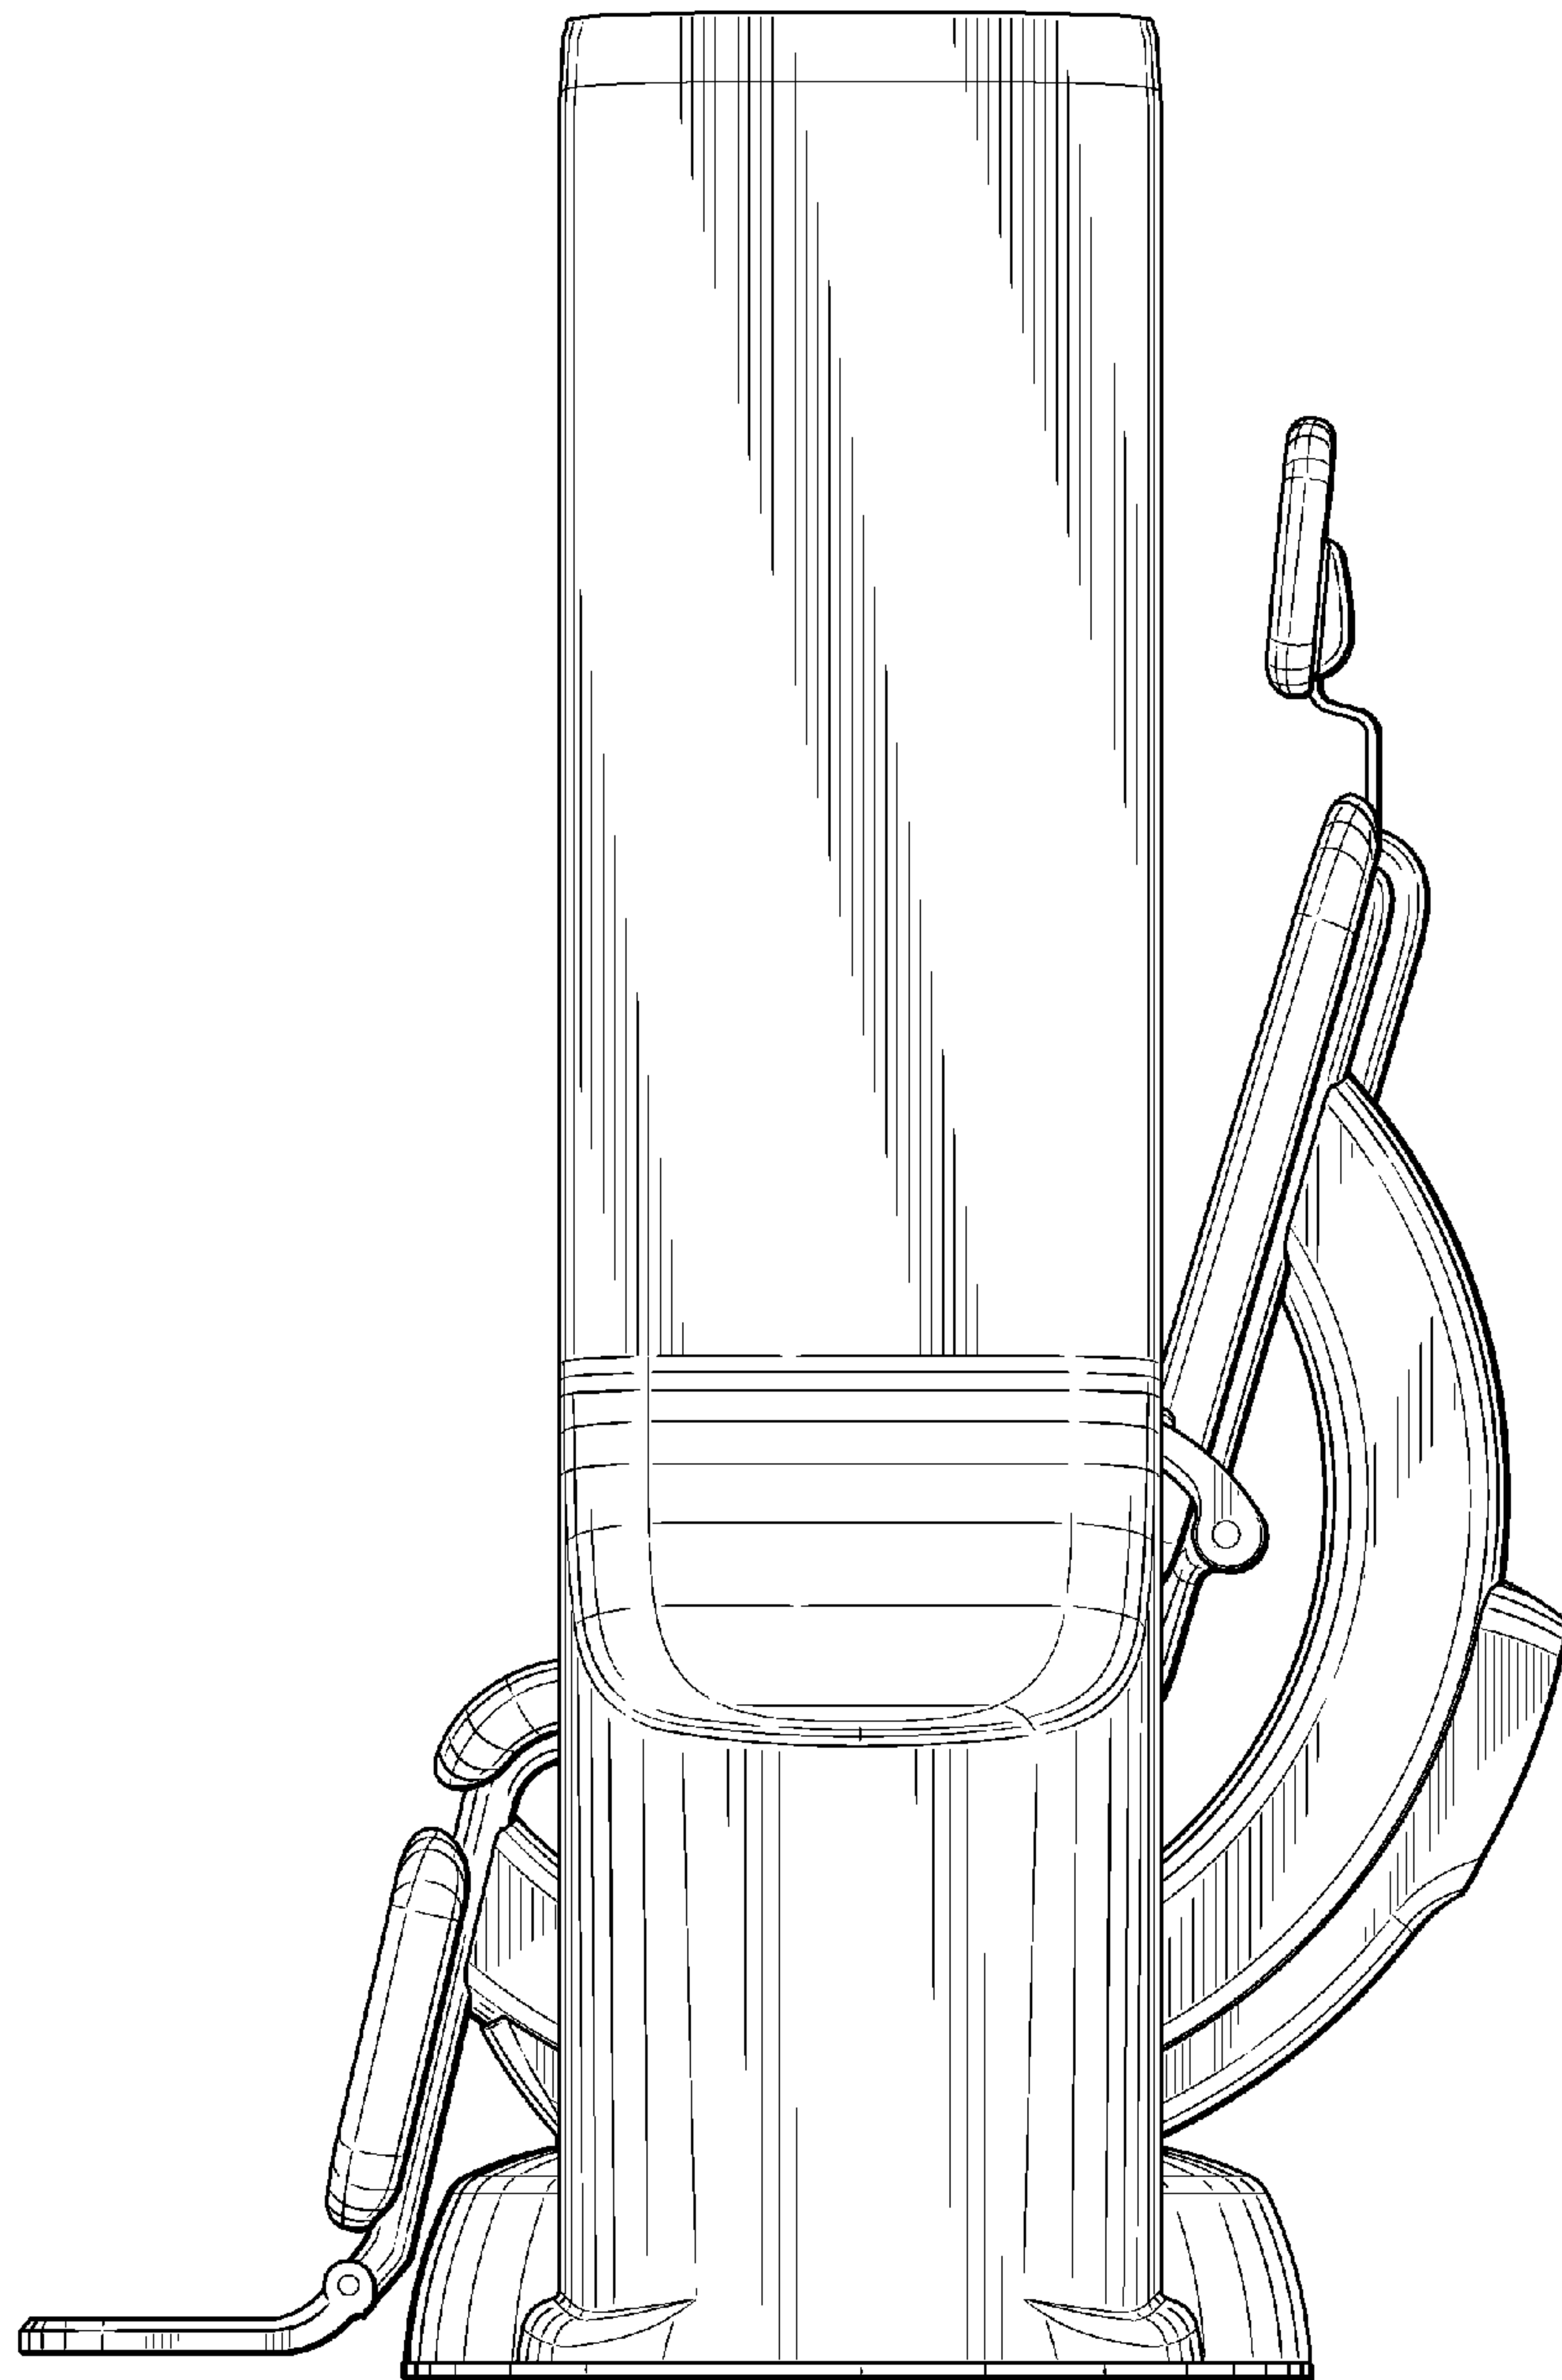


FIG. 4

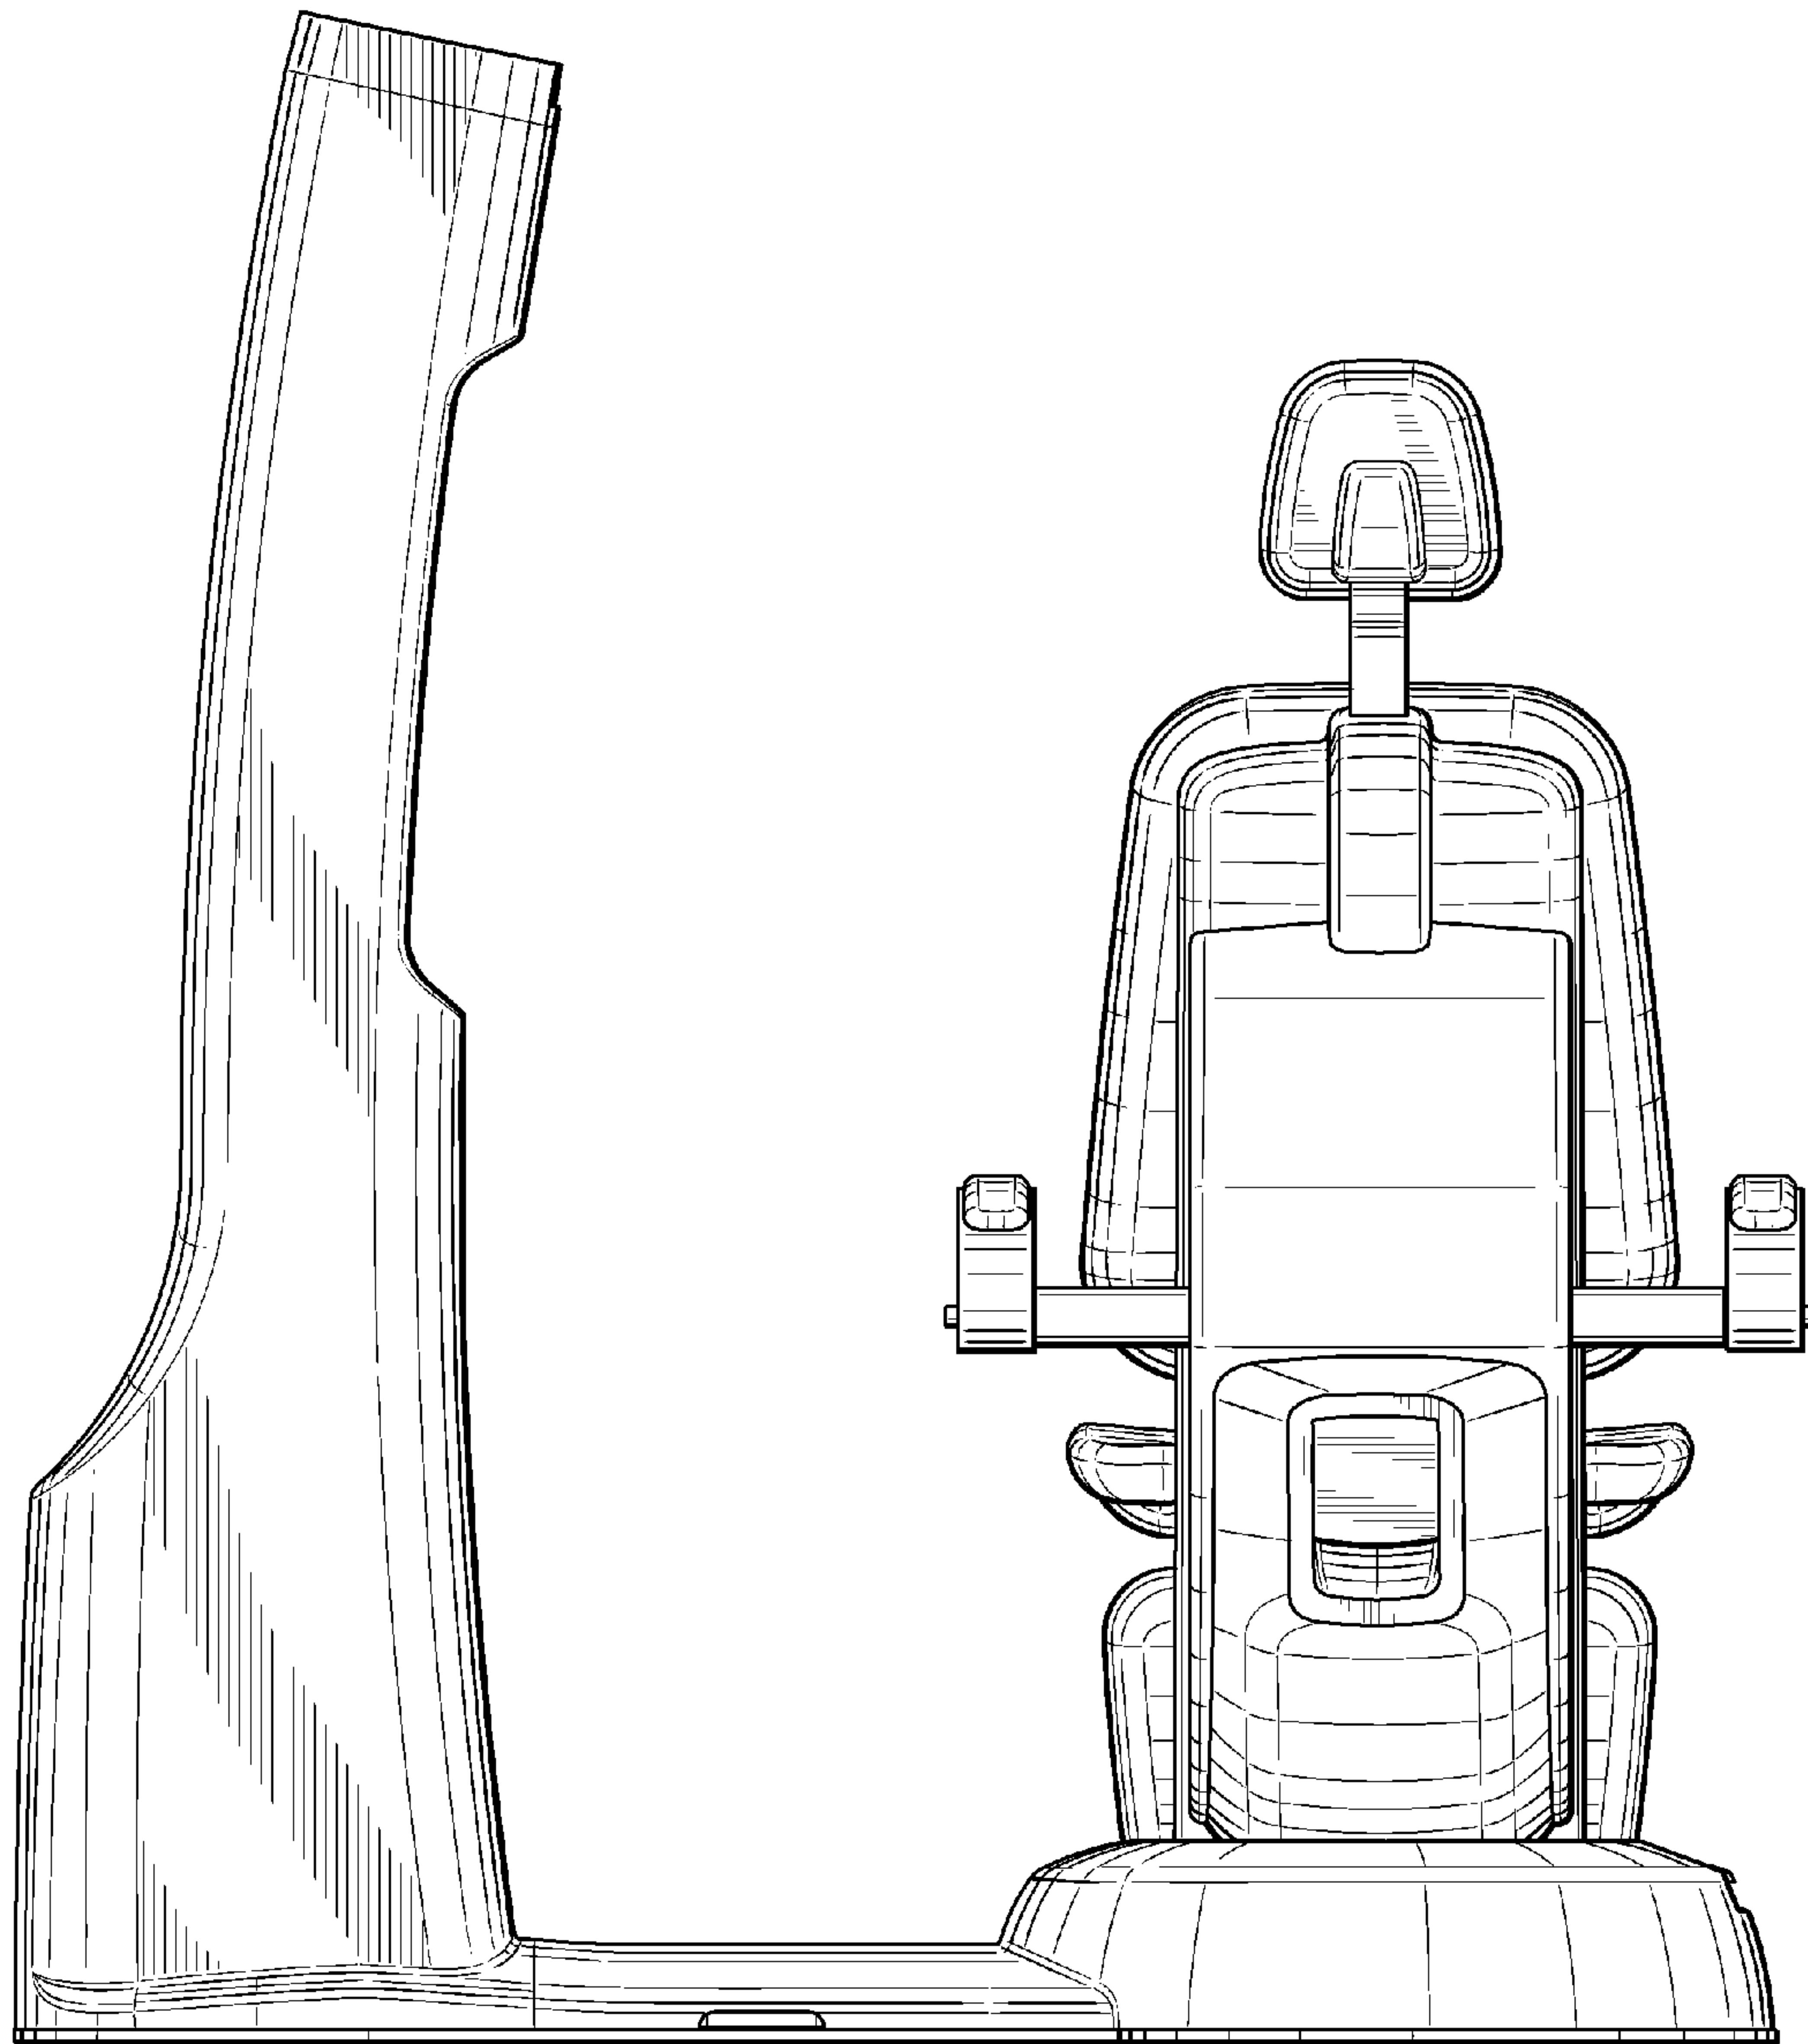


FIG. 5

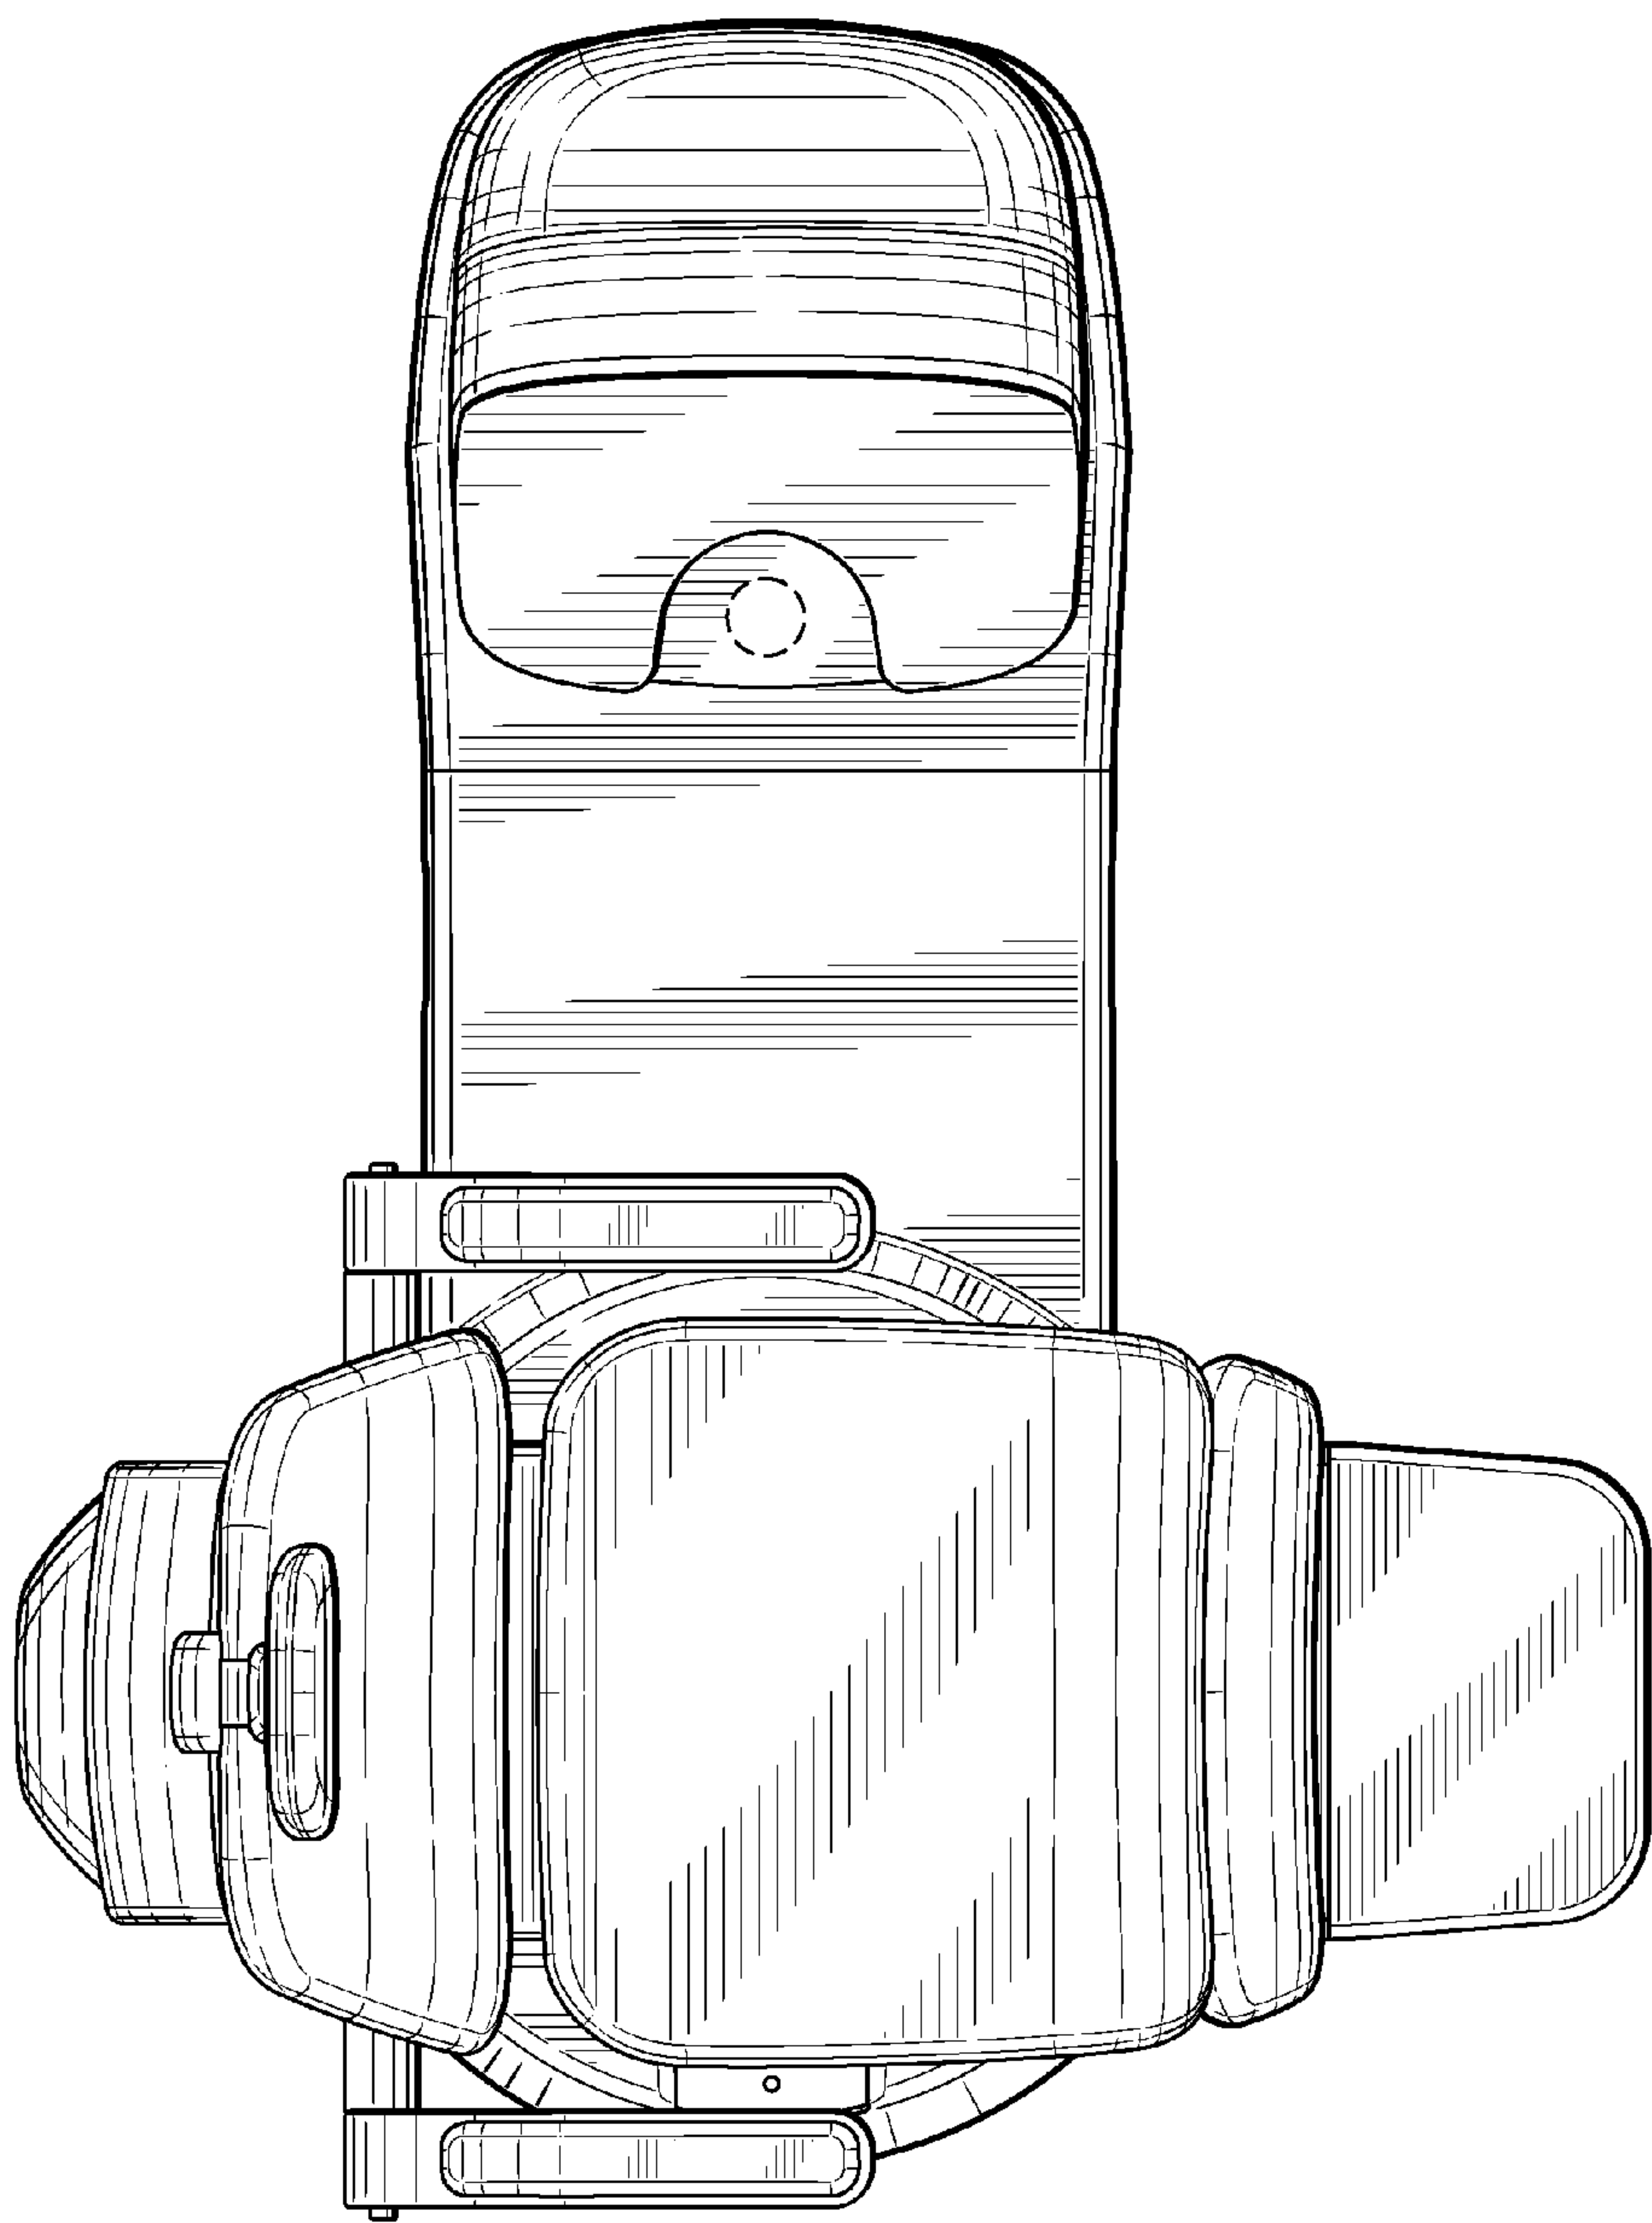


FIG. 6

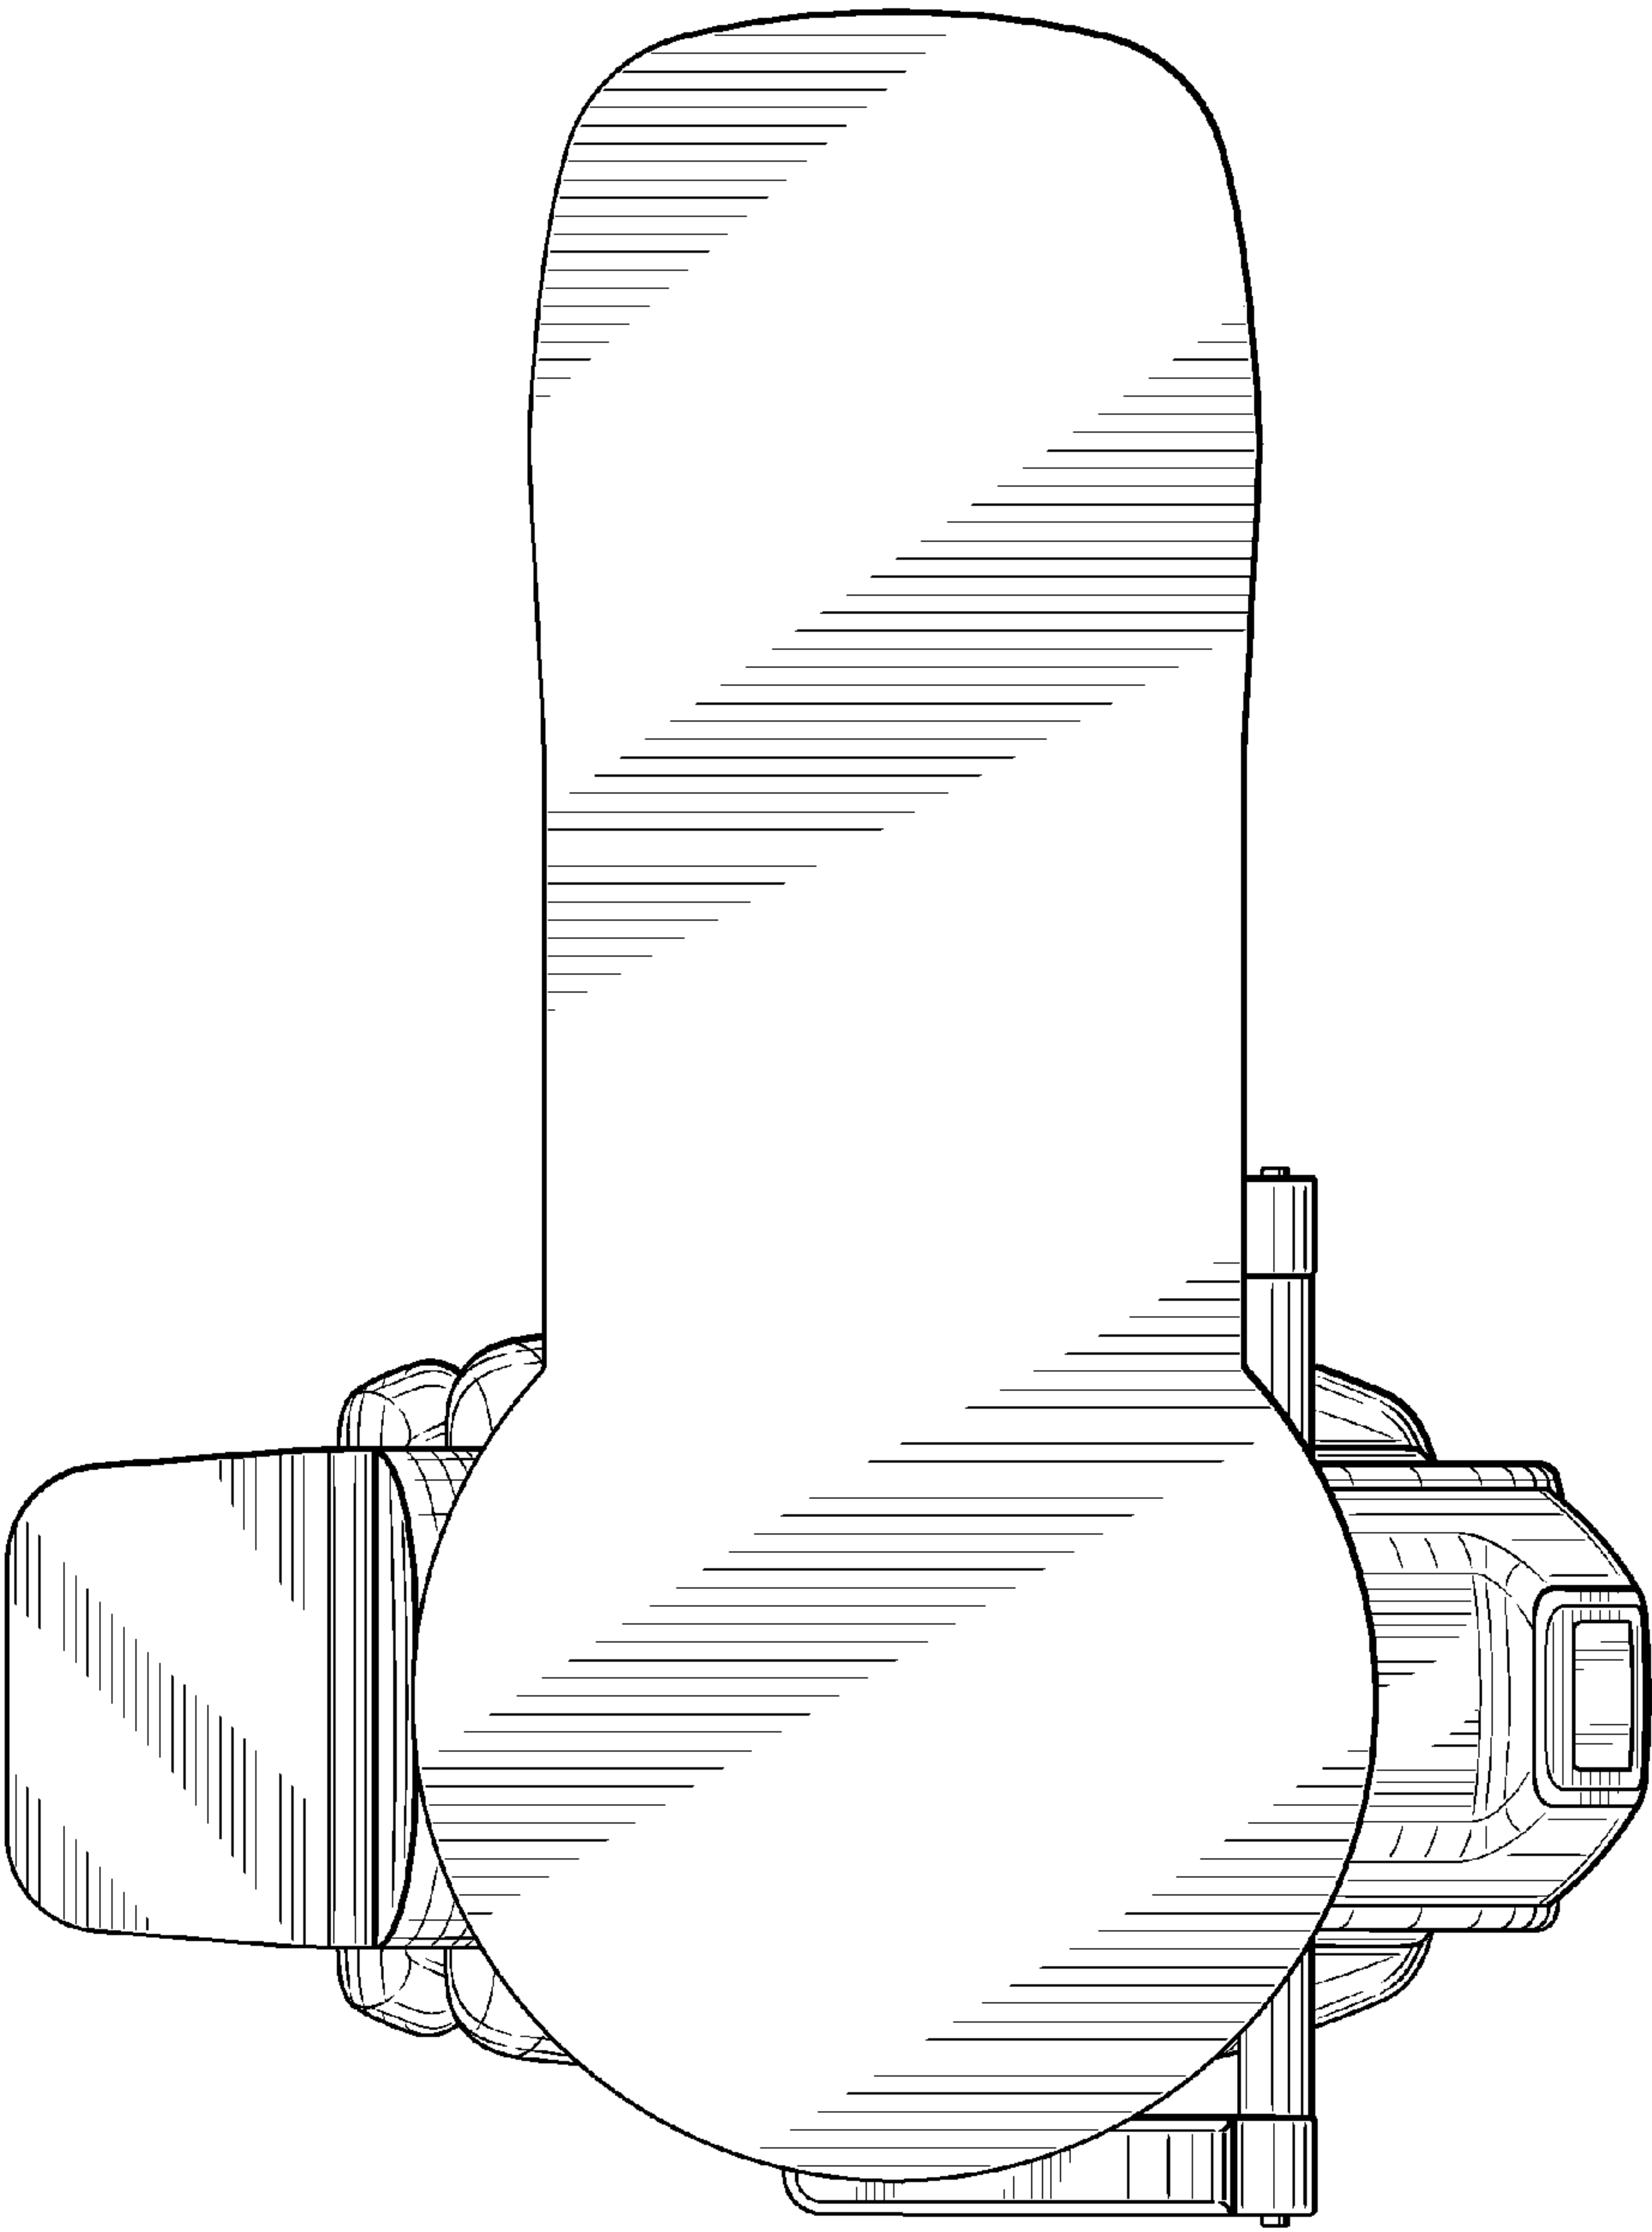


FIG. 7