



US00D676570S

(12) **United States Design Patent**
Chance et al.

(10) **Patent No.:** **US D676,570 S**

(45) **Date of Patent:** **** Feb. 19, 2013**

(54) **LATERAL FLOW ASSAY DEVICE**
(75) Inventors: **Suzette Chance**, Richfield, WI (US);
Gian Paolo Visentin, Waukesha, WI
(US); **Keith Kopitzke**, Fallbrook, CA
(US); **John Zeis**, San Marcos, CA (US)

D390,667 S * 2/1998 Nazareth D24/223
D432,244 S * 10/2000 Anderson et al. D24/223
6,277,650 B1 * 8/2001 Nazareth et al. 422/68.1
6,669,908 B2 * 12/2003 Weyker et al. 422/68.1
D655,424 S * 3/2012 Castanon et al. D24/225
D660,978 S * 5/2012 Wagner et al. D24/223
D668,779 S * 10/2012 Khan et al. D24/225

(73) Assignee: **Gen-Probe Incorporated**, San Diego,
CA (US)

* cited by examiner

(**) Term: **14 Years**

Primary Examiner — Anhdao Doan

(21) Appl. No.: **29/420,588**

(74) *Attorney, Agent, or Firm* — Yan Leychkis; Jeffrey E.
Landes

(22) Filed: **May 10, 2012**

(51) **LOC (9) Cl.** **24-01**

(52) **U.S. Cl.** **D24/223**

(58) **Field of Classification Search** D24/216–217,
D24/219, 223–226, 227, 229–231, 232, 107,
D24/121–123; D10/81; 422/408, 430, 500,
422/502, 503, 68.1; 436/163, 164, 169
See application file for complete search history.

(57) **CLAIM**

The ornamental design for a lateral flow assay device, as
shown and described.

DESCRIPTION


FIG. 1 is a perspective view of a lateral flow assay device,
showing the new design;
FIG. 2 is a left elevational view thereof;
FIG. 3 is a right elevational view thereof;
FIG. 4 is a rear elevational view thereof;
FIG. 5 is a front elevational view thereof;
FIG. 6 is a top plan view thereof; and,
FIG. 7 is a bottom plan view thereof.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D342,575 S * 12/1993 Ashihara et al. D24/224
D383,549 S * 9/1997 Arnett et al. D24/223

1 Claim, 3 Drawing Sheets

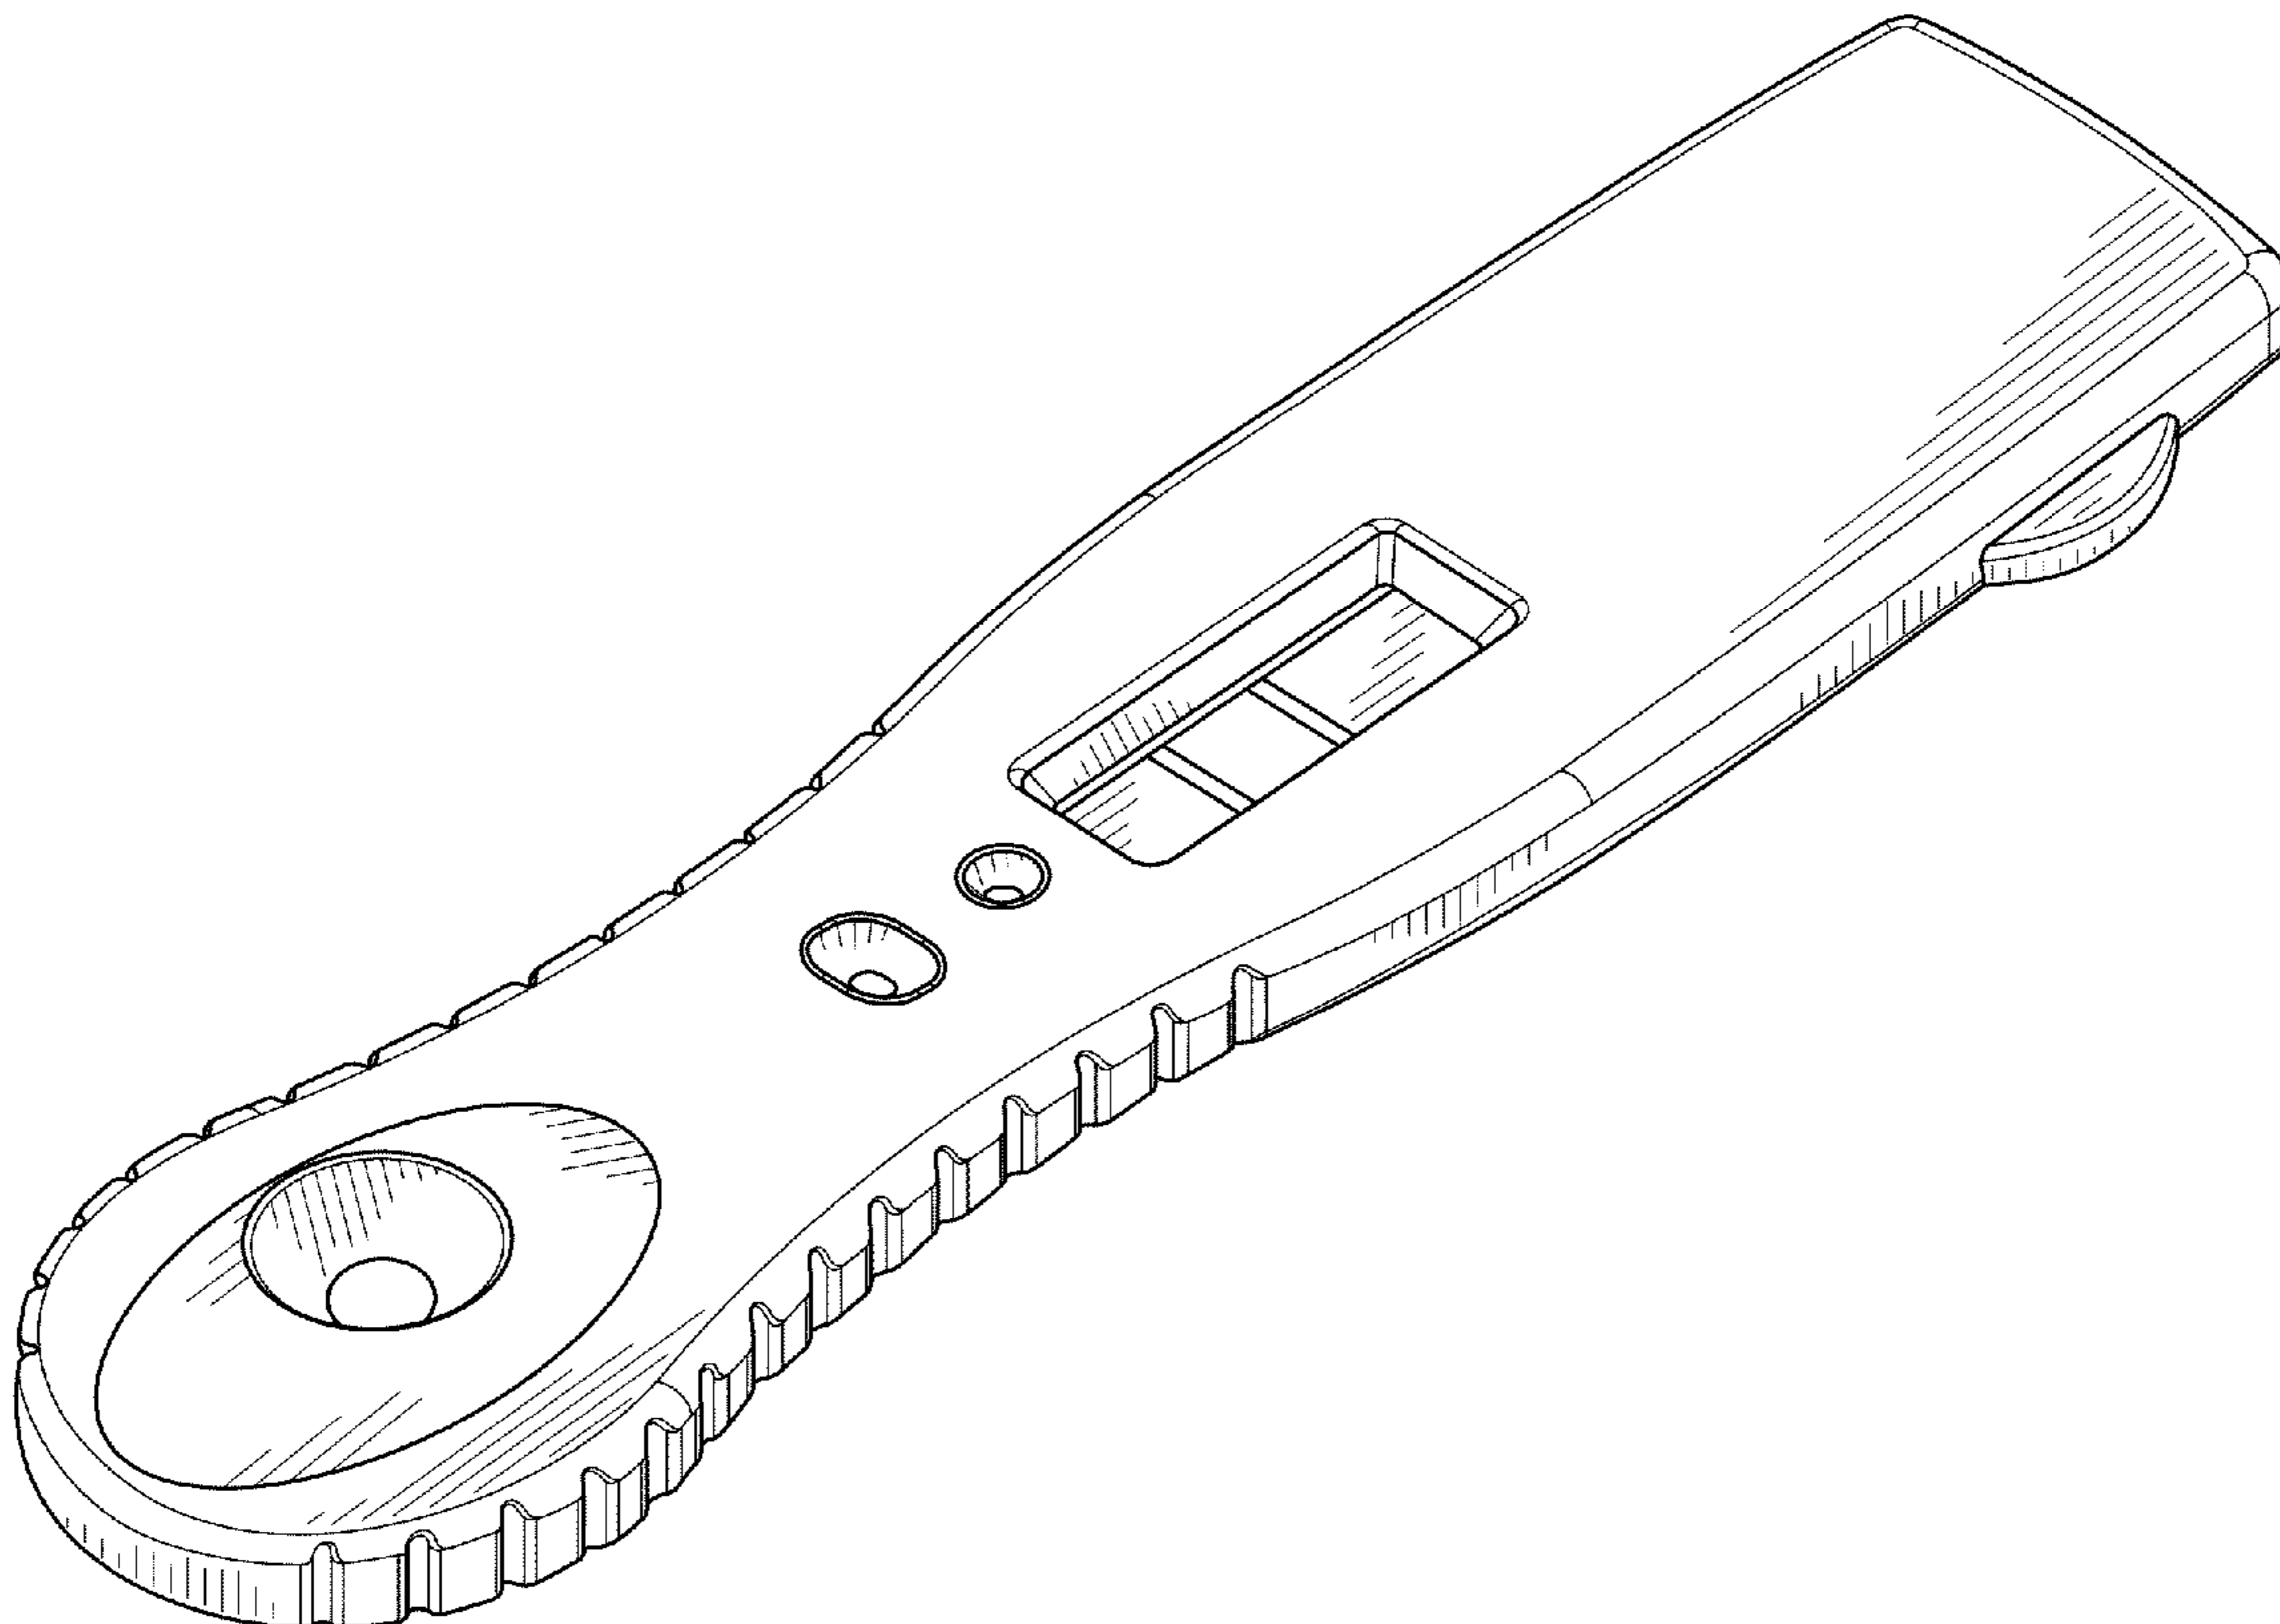

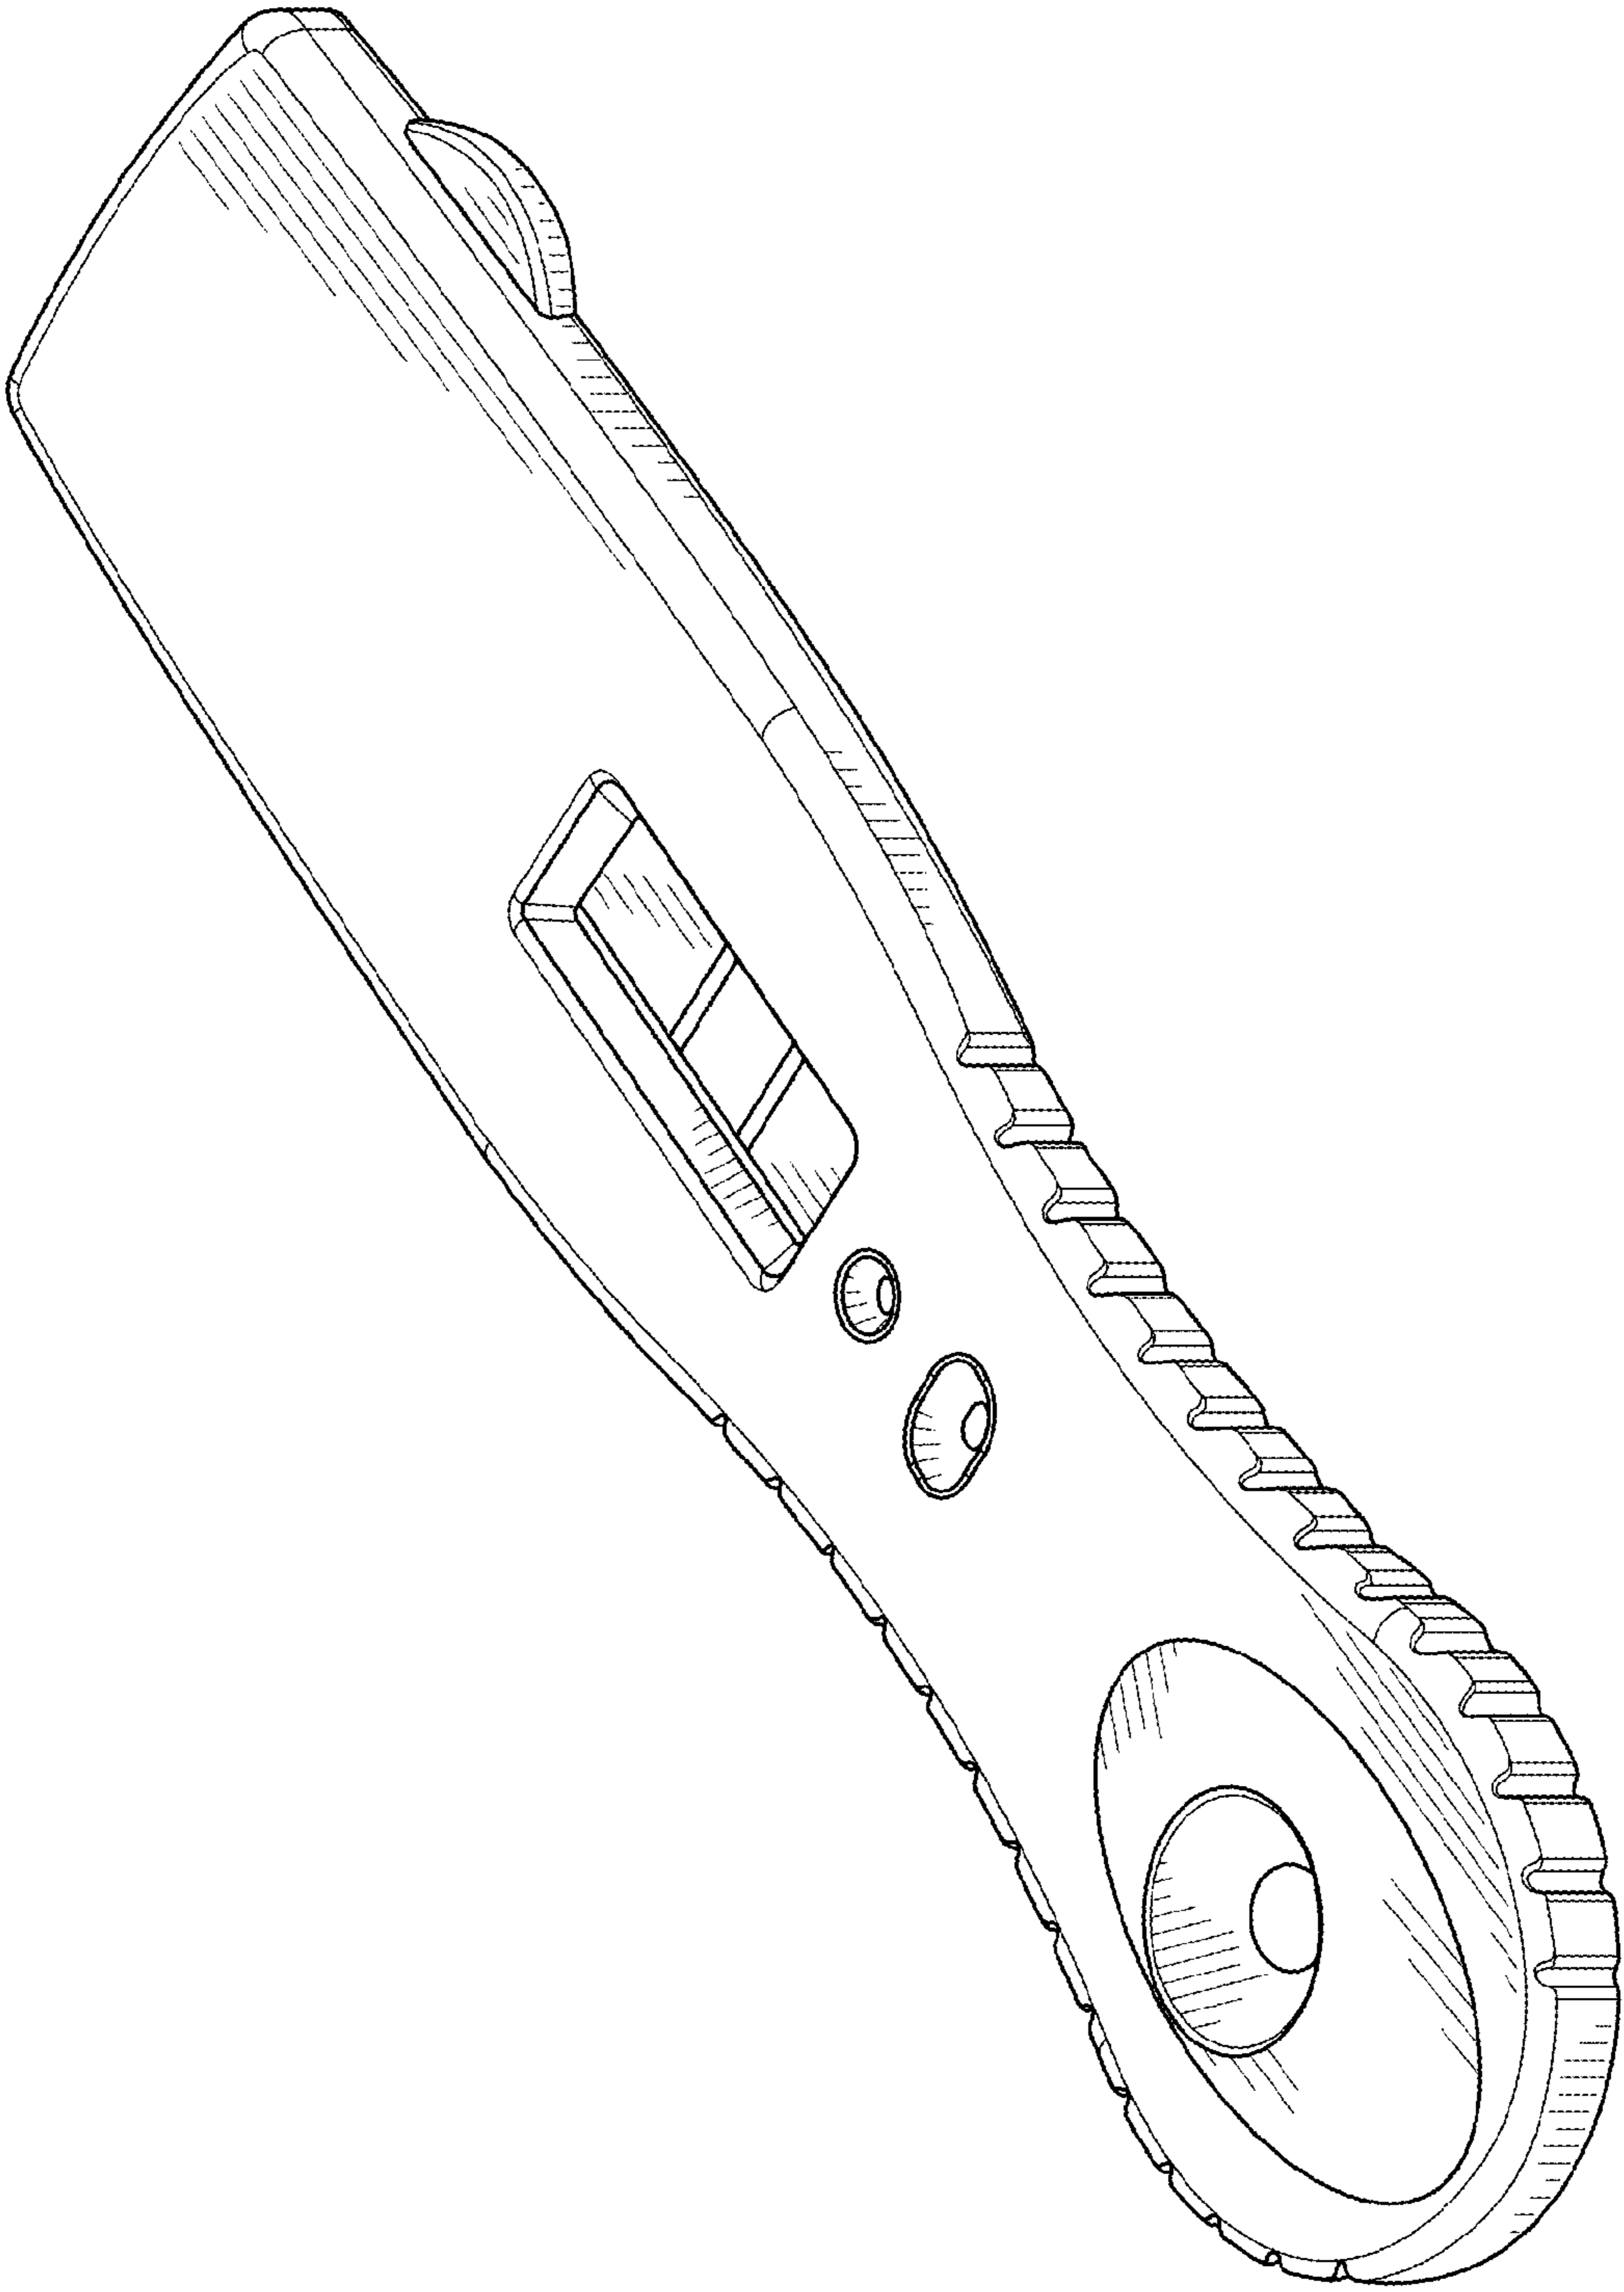


FIG. 1

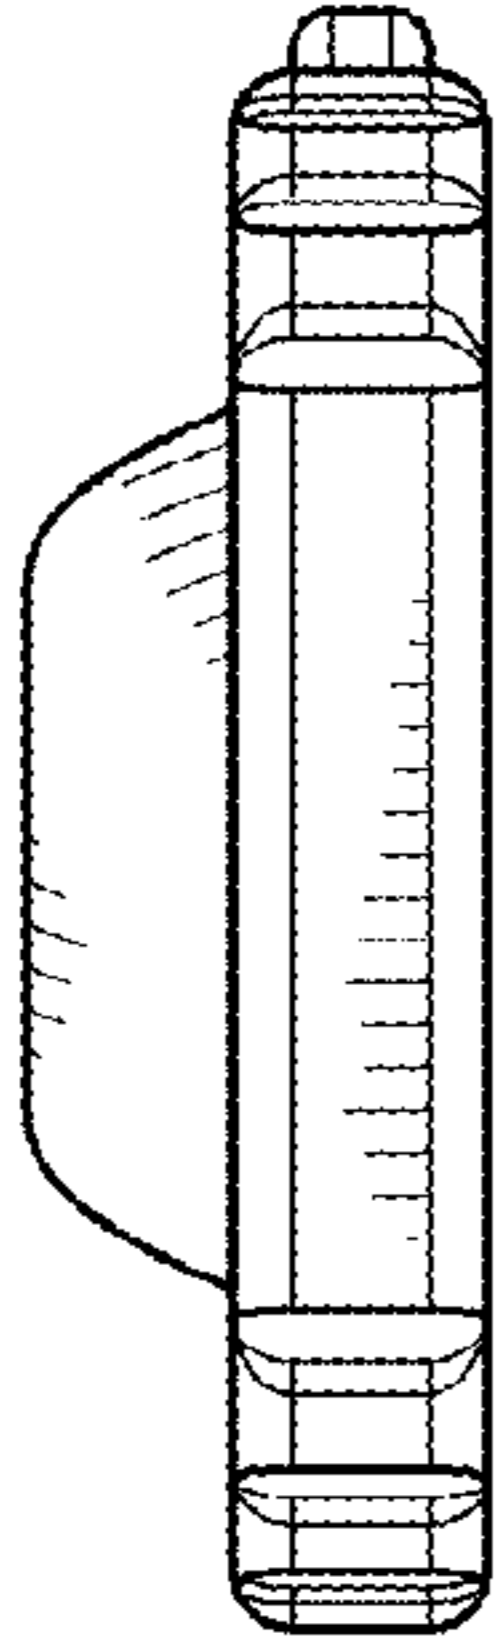


FIG. 2

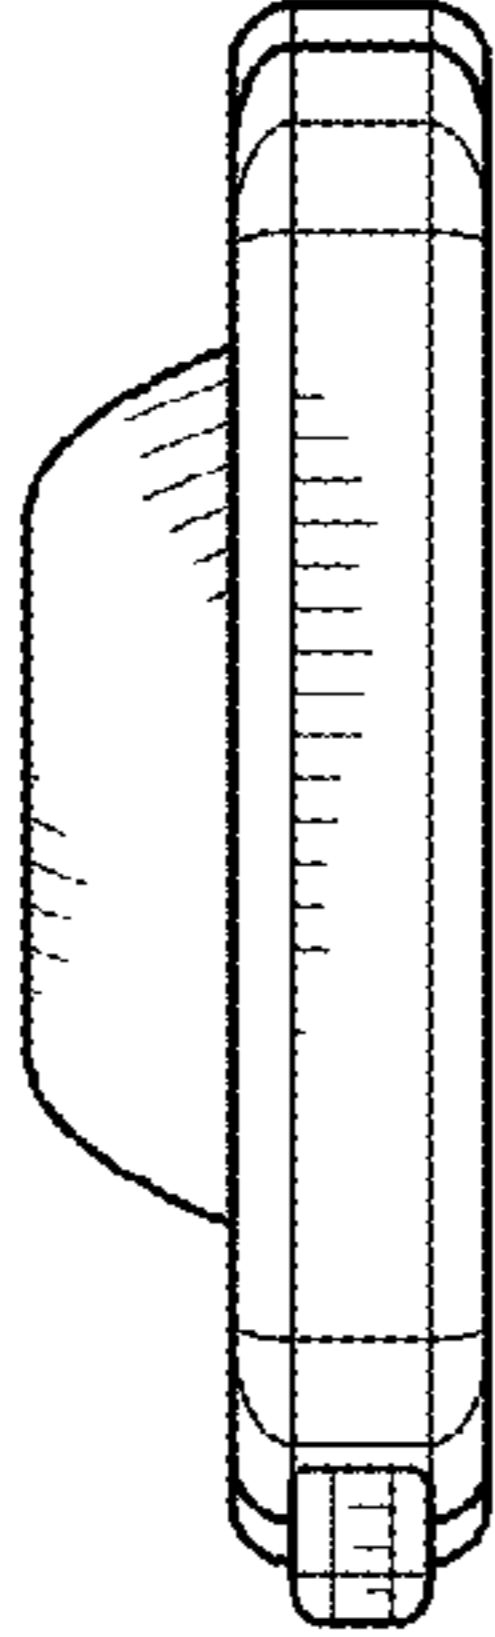


FIG. 3

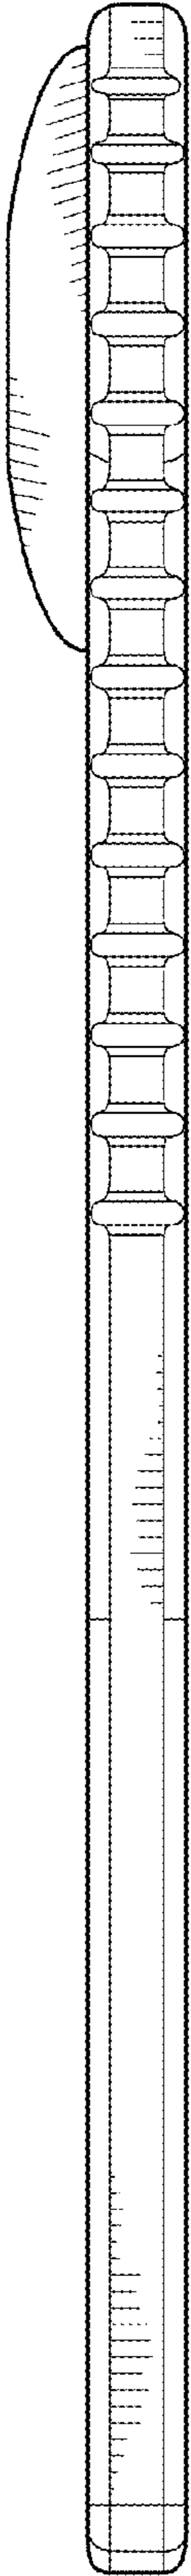


FIG. 4

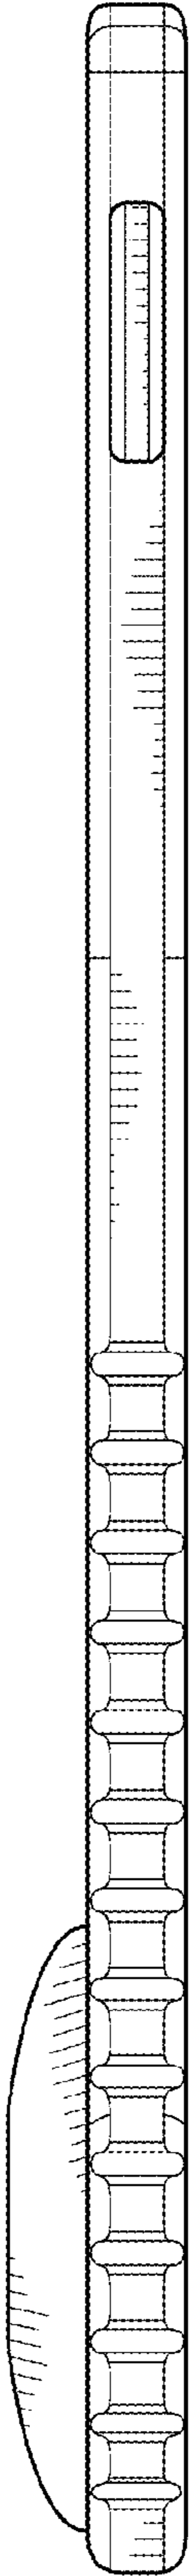


FIG. 5

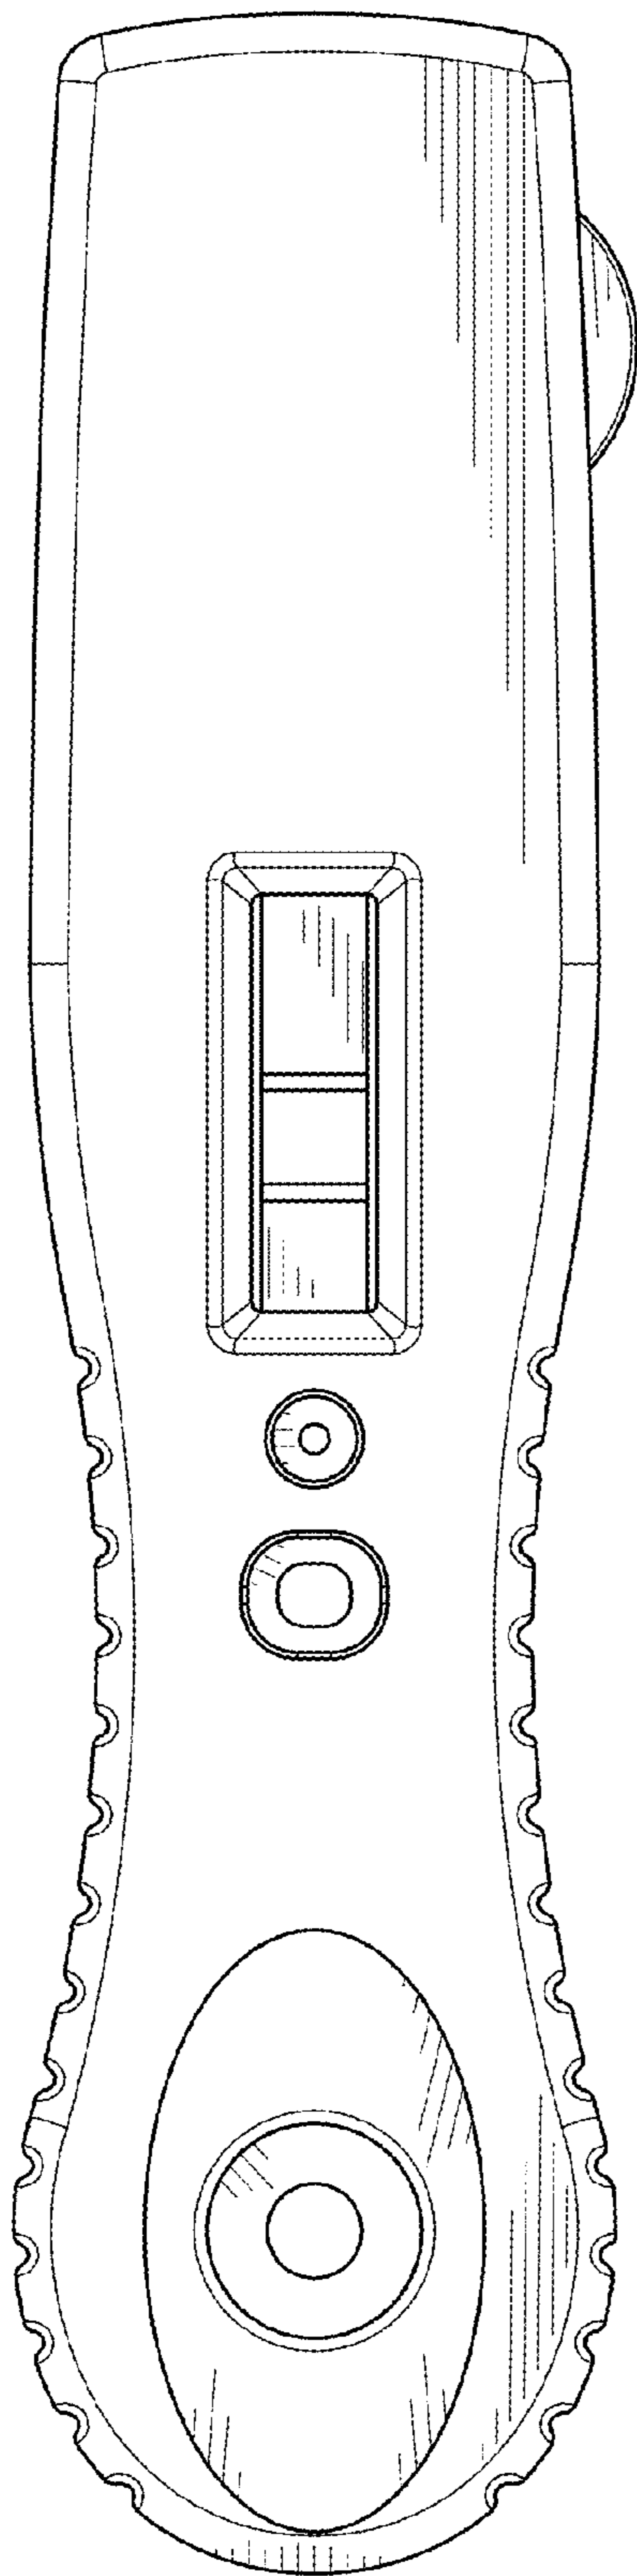


FIG. 6

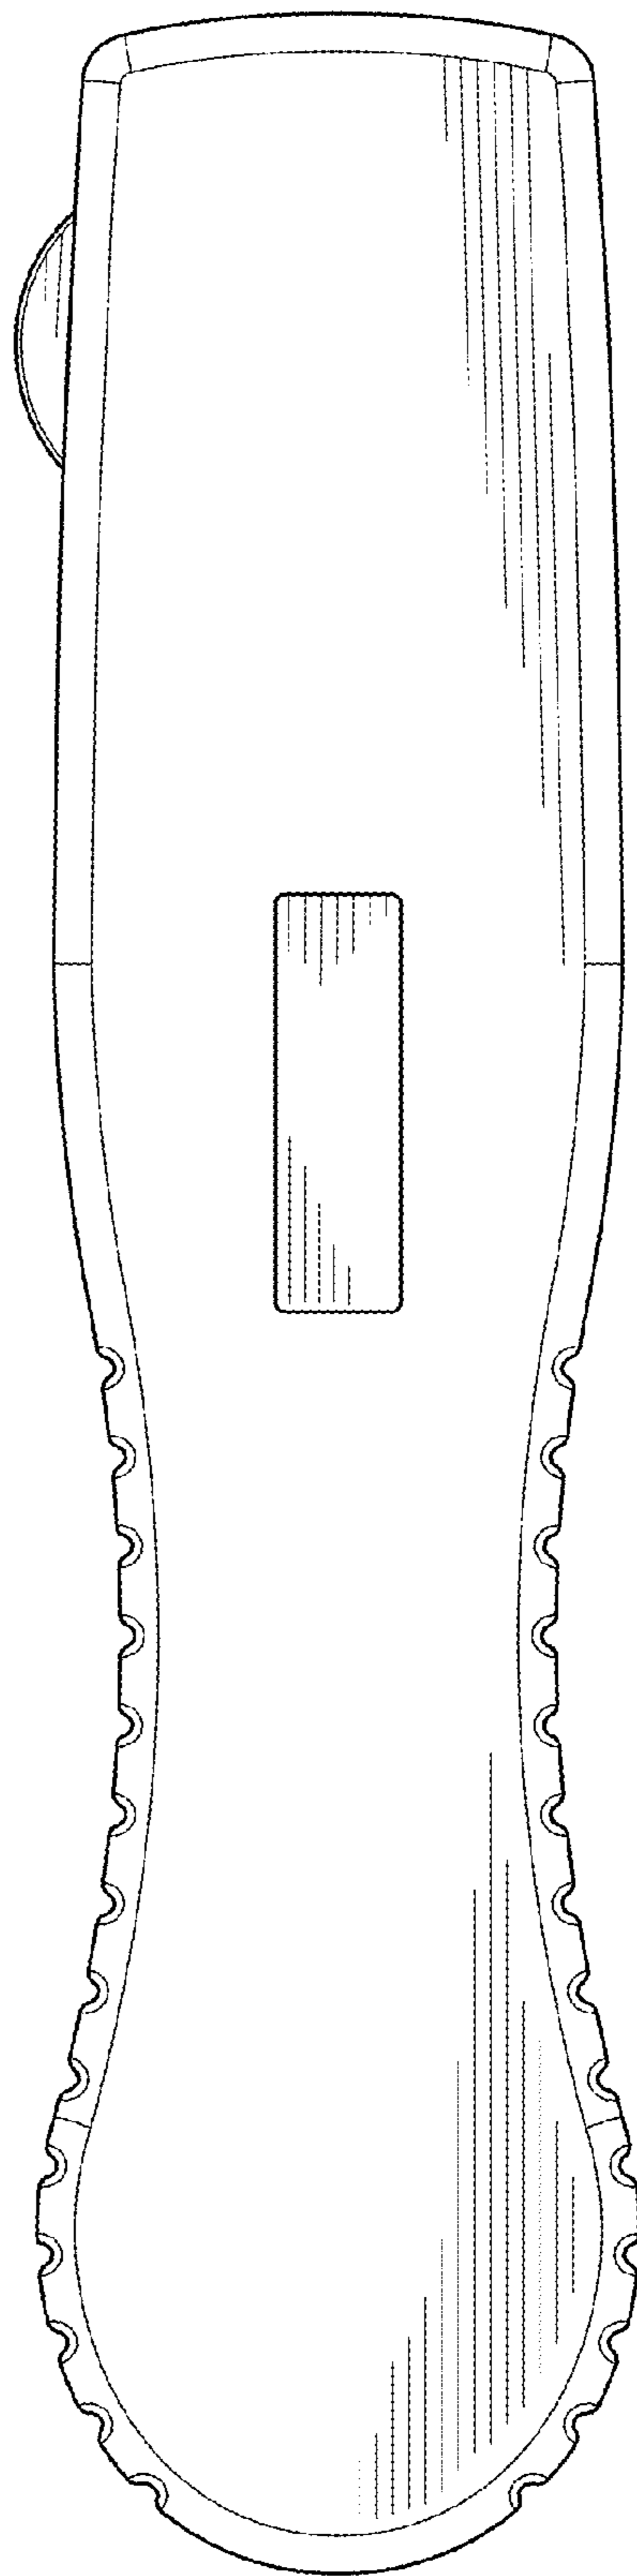


FIG. 7