



US00D678530S

(12) **United States Design Patent**
Khan et al.

(10) **Patent No.:** **US D678,530 S**
(45) **Date of Patent:** **** Mar. 19, 2013**

(54) **DIAGNOSTIC CARTRIDGE READER**

(75) Inventors: **Macksoud Khan**, Palo Alto, CA (US);
Zachary M. Ruef, San Francisco, CA
(US); **Keagan Rowley**, Boulder, CO
(US)

(73) Assignee: **MBio Diagnostics, Inc.**, Boulder, CO
(US)

(**) Term: **14 Years**

(21) Appl. No.: **29/393,971**

(22) Filed: **Jun. 10, 2011**

(51) **LOC (9) Cl.** **24-01**

(52) **U.S. Cl.** **D24/186**

(58) **Field of Classification Search** D24/107,
D24/111, 164–165, 167, 186, 216, 231, 232,
D24/200, 172; 600/301, 481, 483–485, 509,
600/513, 519, 544; D10/81, 104

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D334,237 S *	3/1993	Collister et al.	D24/186
D400,673 S *	11/1998	Kheiri et al.	D24/107
D404,140 S *	1/1999	Meguro	D24/232
D427,315 S *	6/2000	Saltzstein et al.	D24/186
D446,306 S *	8/2001	Ochi et al.	D24/186
D477,084 S *	7/2003	Menezes et al.	D24/172
D489,816 S *	5/2004	Ross	D24/107
D490,516 S *	5/2004	Takahashi et al.	D24/107
D503,807 S *	4/2005	Ryan	D24/200
D536,793 S *	2/2007	Assad et al.	D24/185

D573,051 S *	7/2008	Alden et al.	D10/81
D584,975 S *	1/2009	Haberstroh	D10/81
D597,216 S *	7/2009	McGuigan et al.	D24/216
D598,551 S *	8/2009	Miwa et al.	D24/186
D609,343 S *	2/2010	Omaki	D24/165
D609,344 S *	2/2010	Hara	D24/165
D647,209 S *	10/2011	Muller et al.	D24/216
D651,319 S *	12/2011	Hara	D24/165

* cited by examiner

Primary Examiner — T. Chase Nelson

Assistant Examiner — Mark Cavanna

(74) *Attorney, Agent, or Firm* — Lathrop & Gage LLP

(57) **CLAIM**

The ornamental design for a diagnostic cartridge reader, as shown and described.

DESCRIPTION

FIG. 1 is a front perspective view of the diagnostic cartridge reader, showing the new design;

FIG. 2 is a front elevation of the diagnostic cartridge reader;

FIG. 3 is a side elevation of the diagnostic cartridge reader, an opposing side elevation of the diagnostic cartridge reader being a mirror image thereof;

FIG. 4 is a top plan view of the diagnostic cartridge reader;



FIG. 5 is a rear elevation of the diagnostic cartridge reader;

FIG. 6 is a bottom plan view of the diagnostic cartridge reader; and,

FIG. 7 is a rear perspective view of the diagnostic cartridge reader.

In all of FIGS. 1 through 7, dashed lines indicate environmental structure that forms no part of the claimed design.

1 Claim, 7 Drawing Sheets

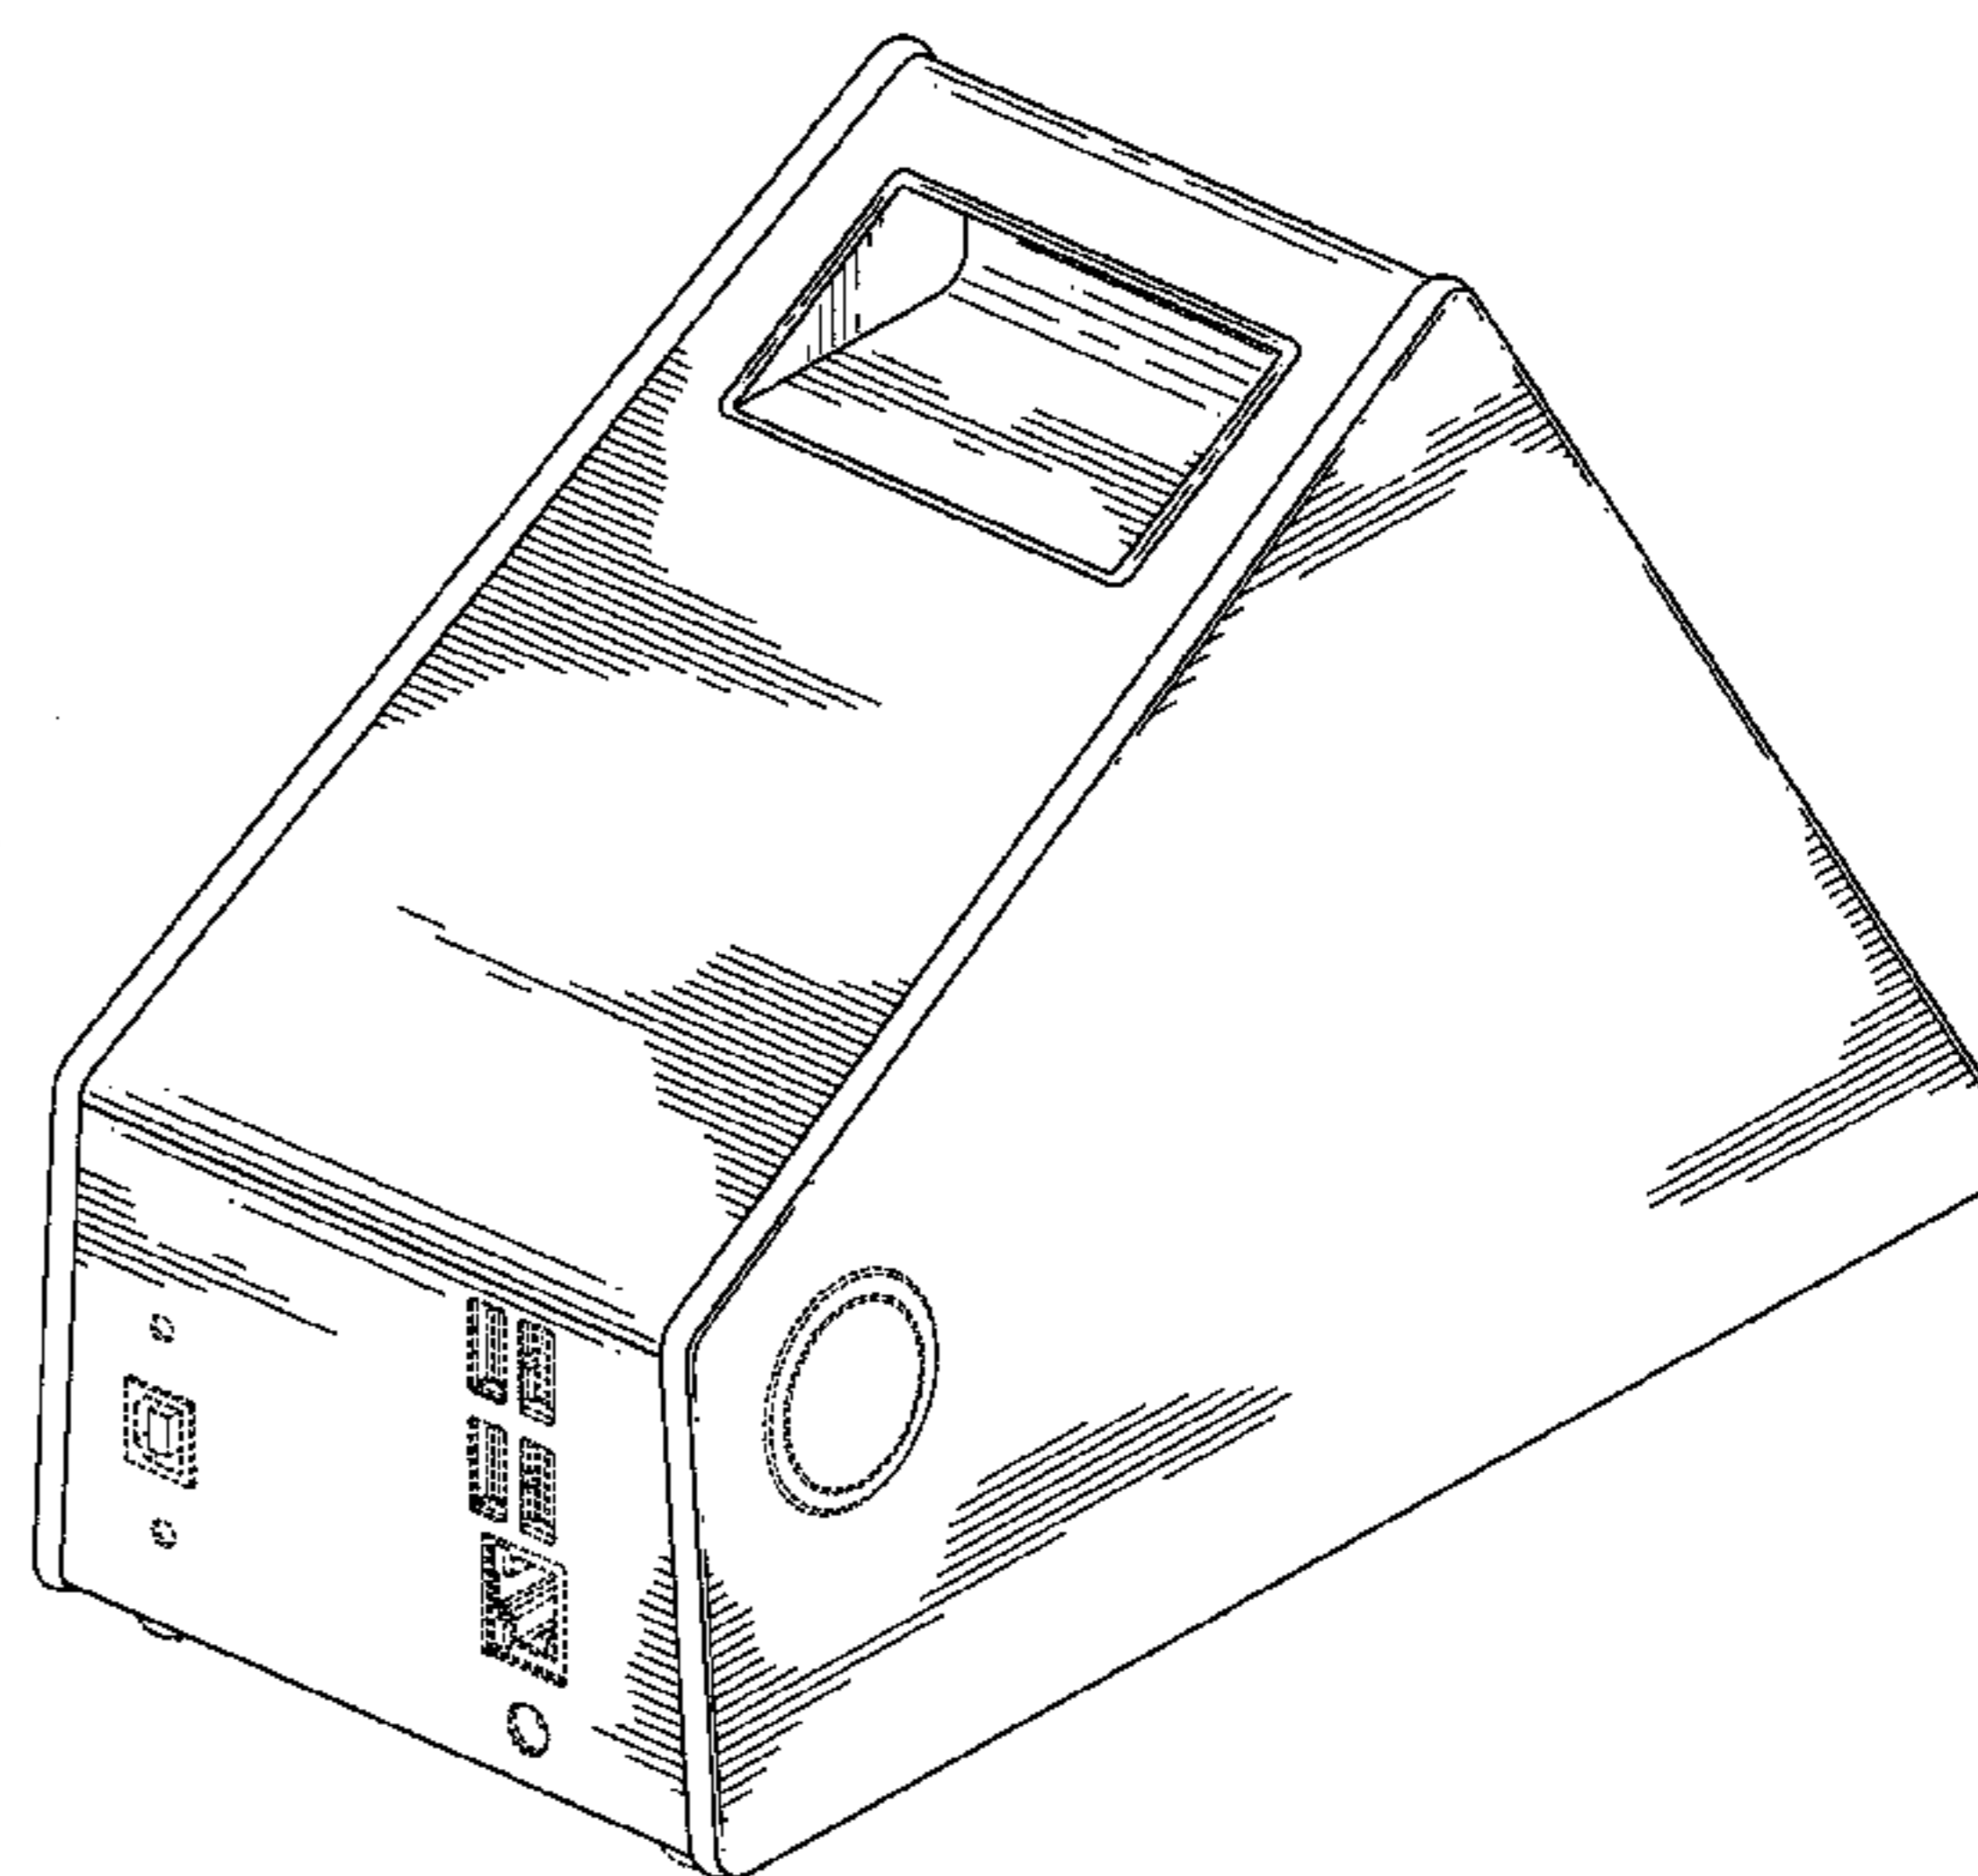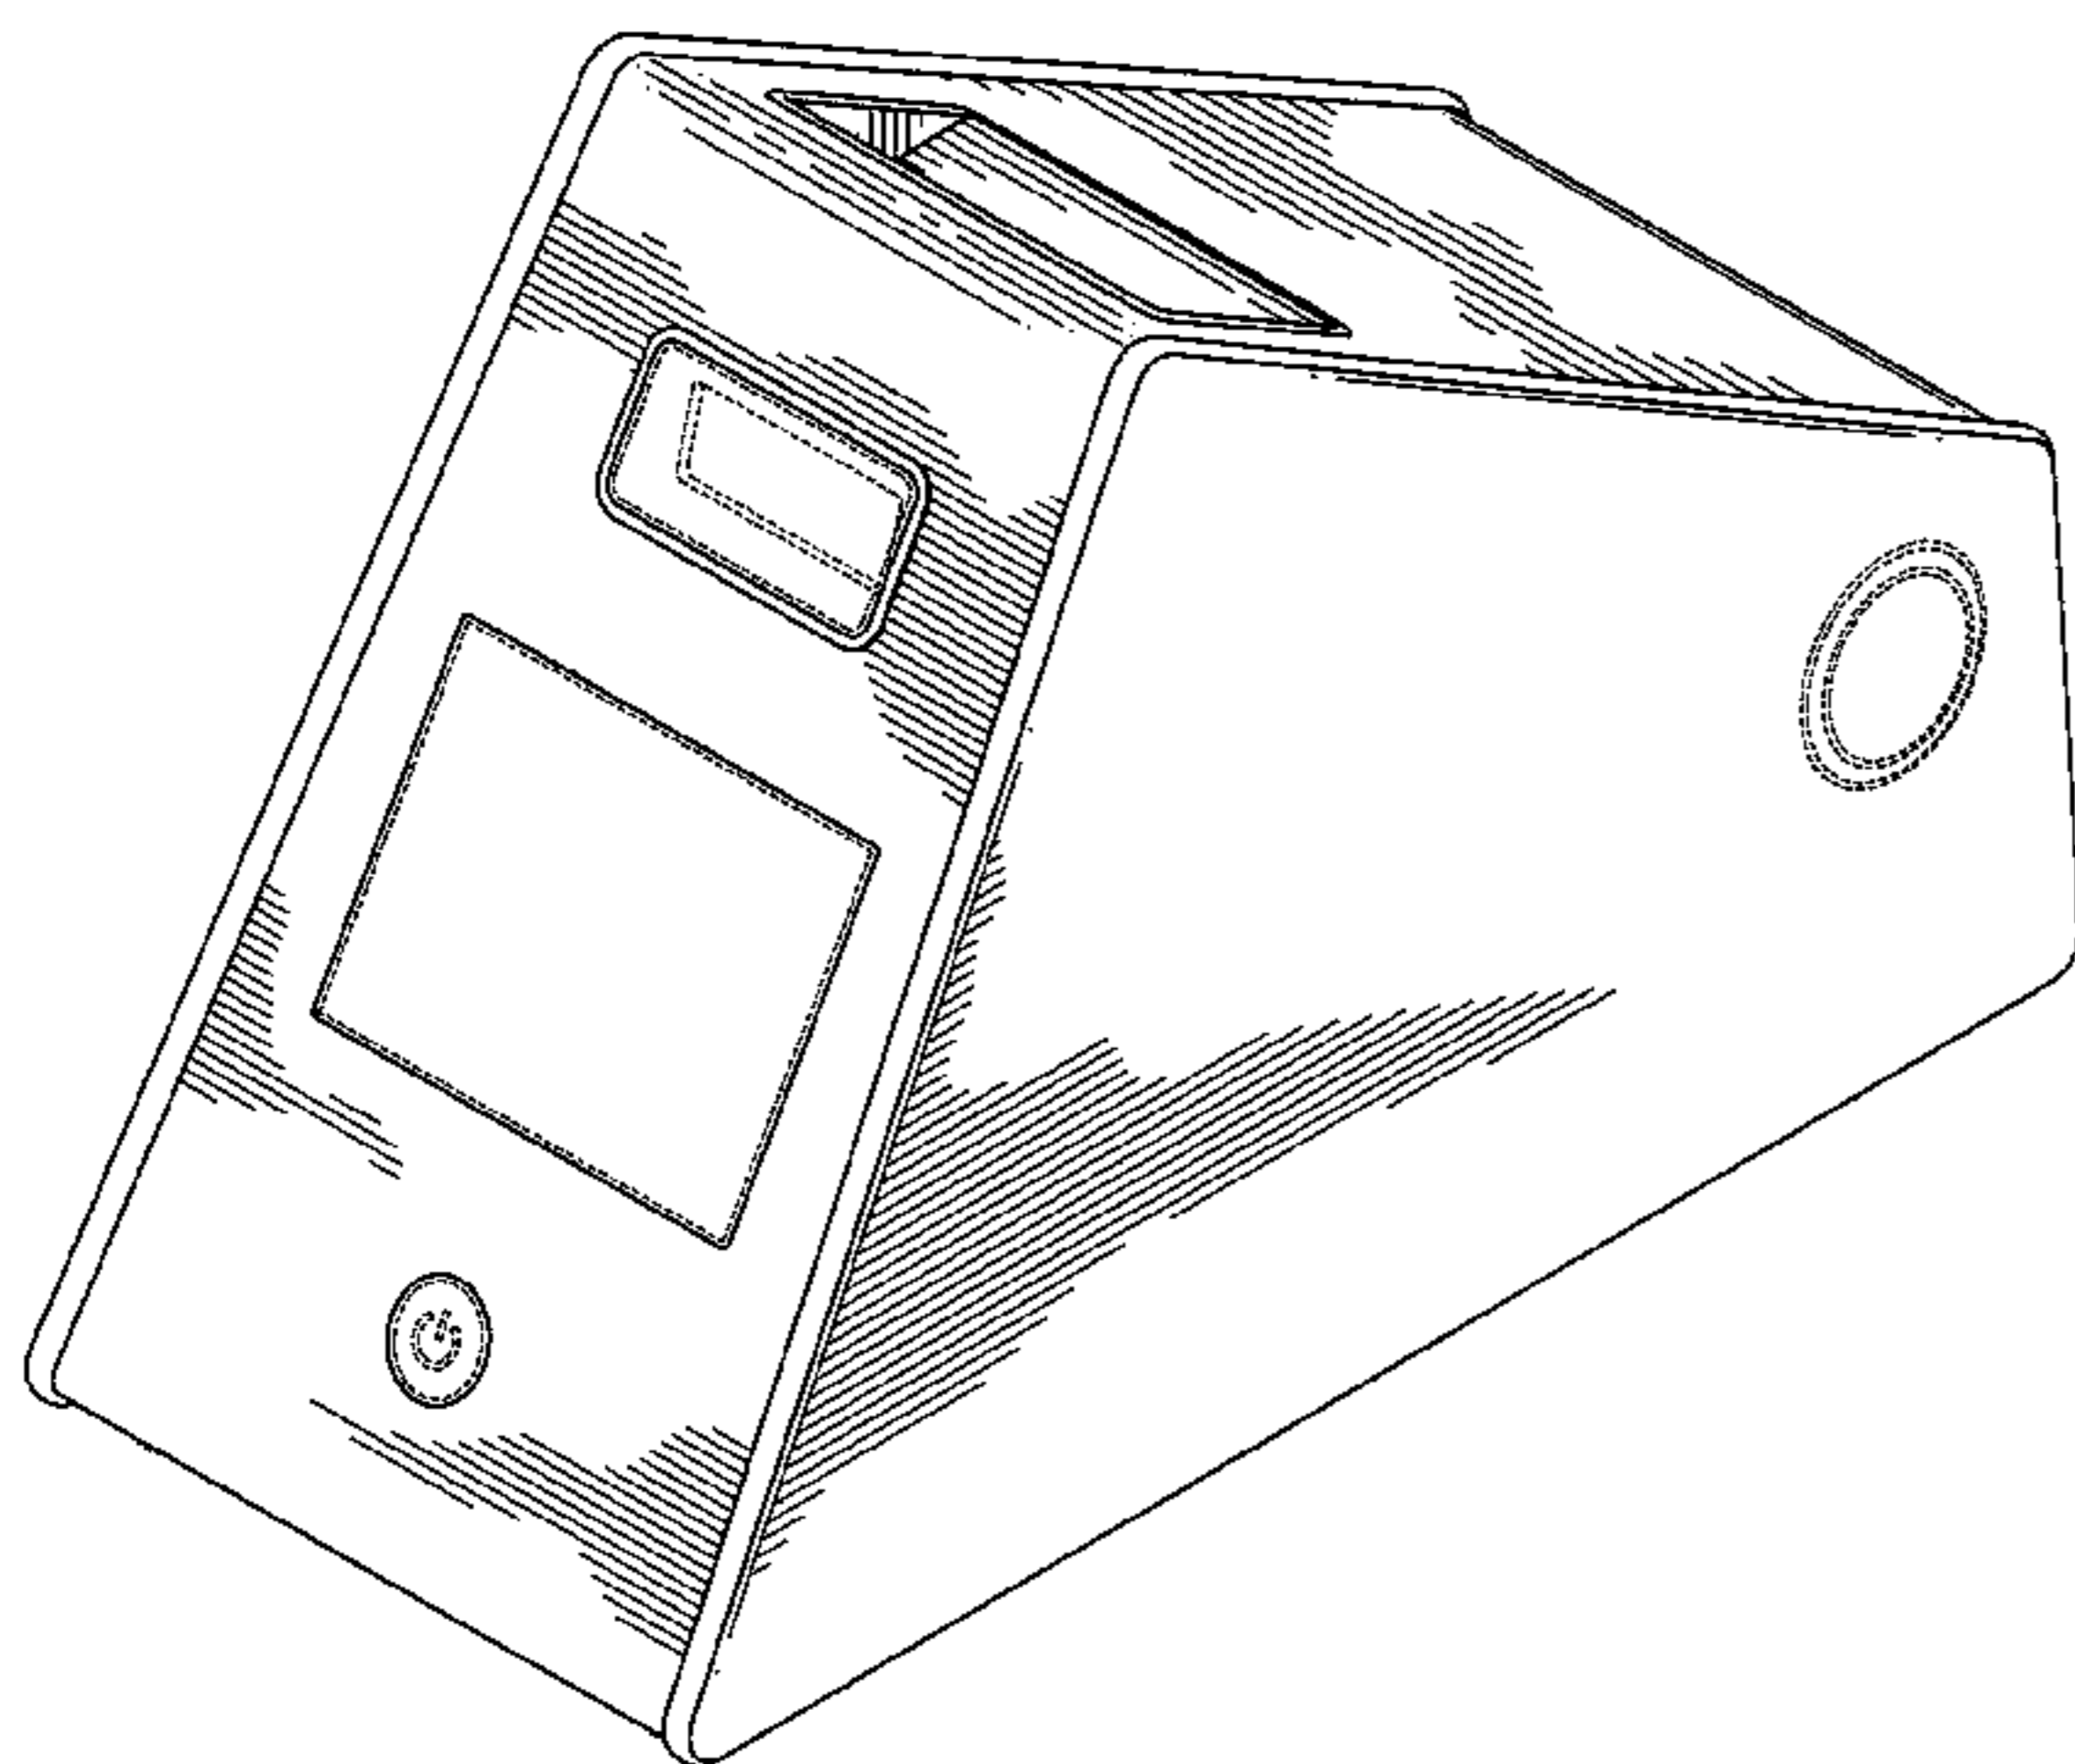

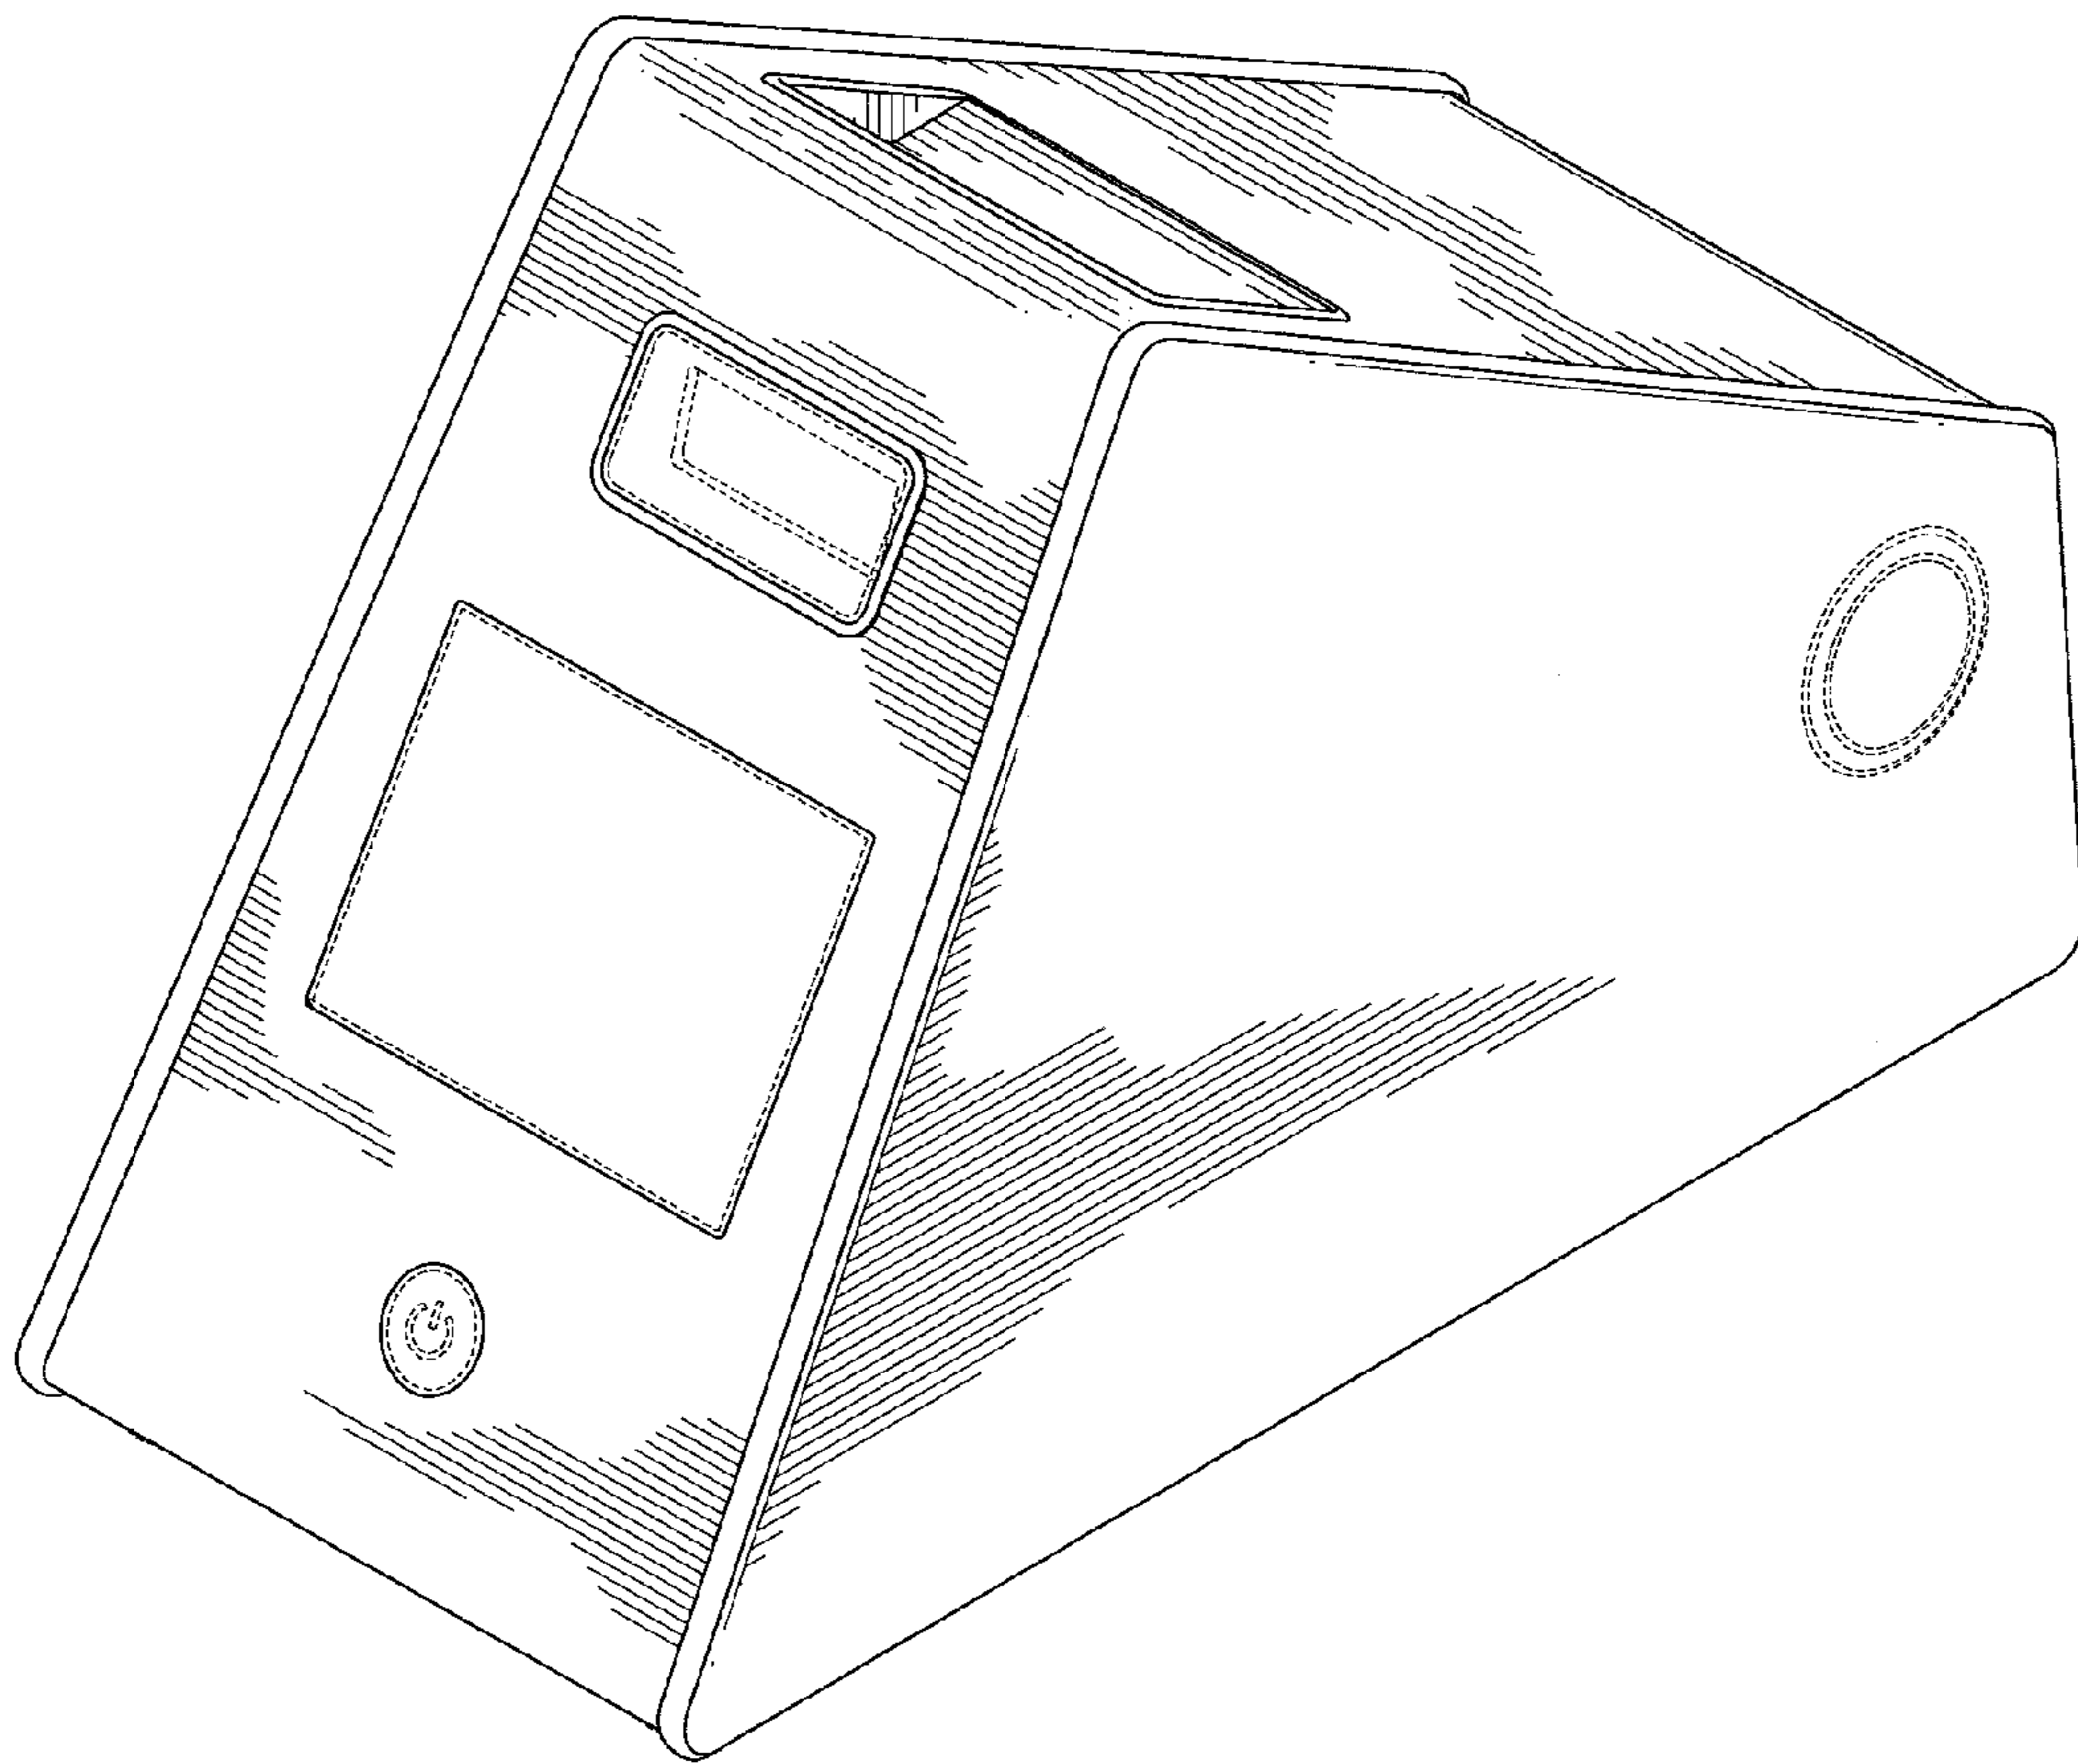


FIG. 1

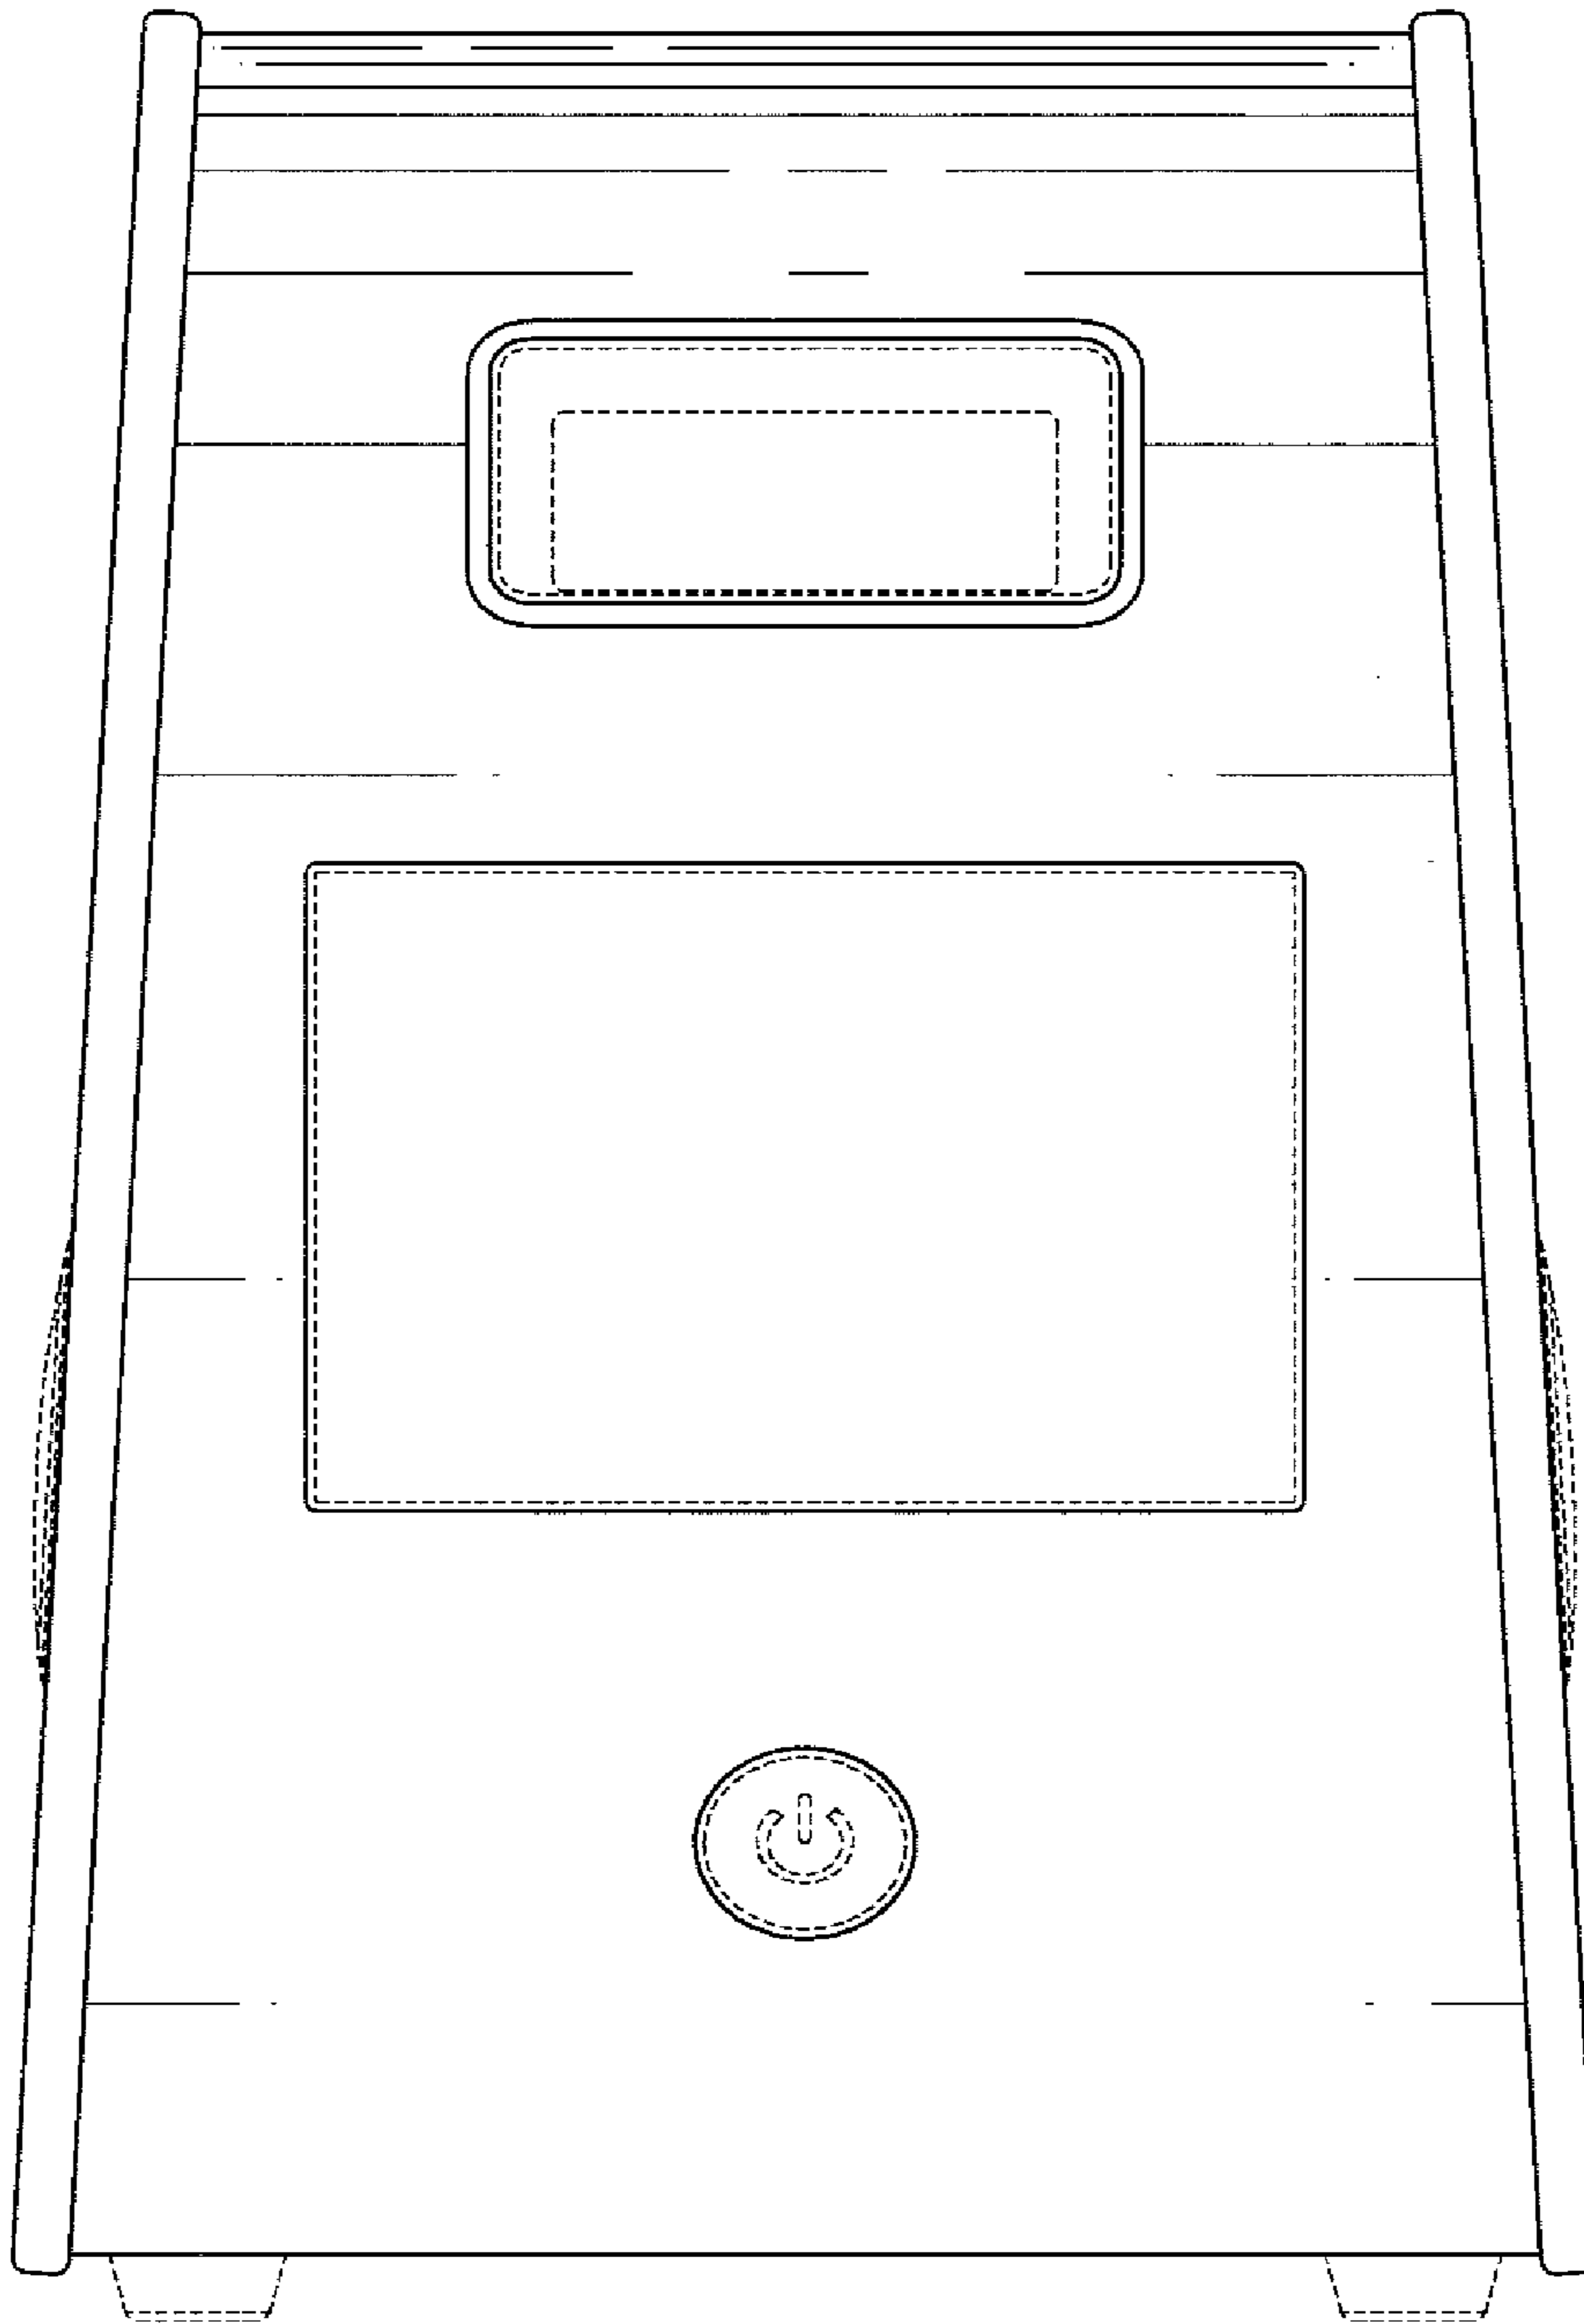


FIG. 2

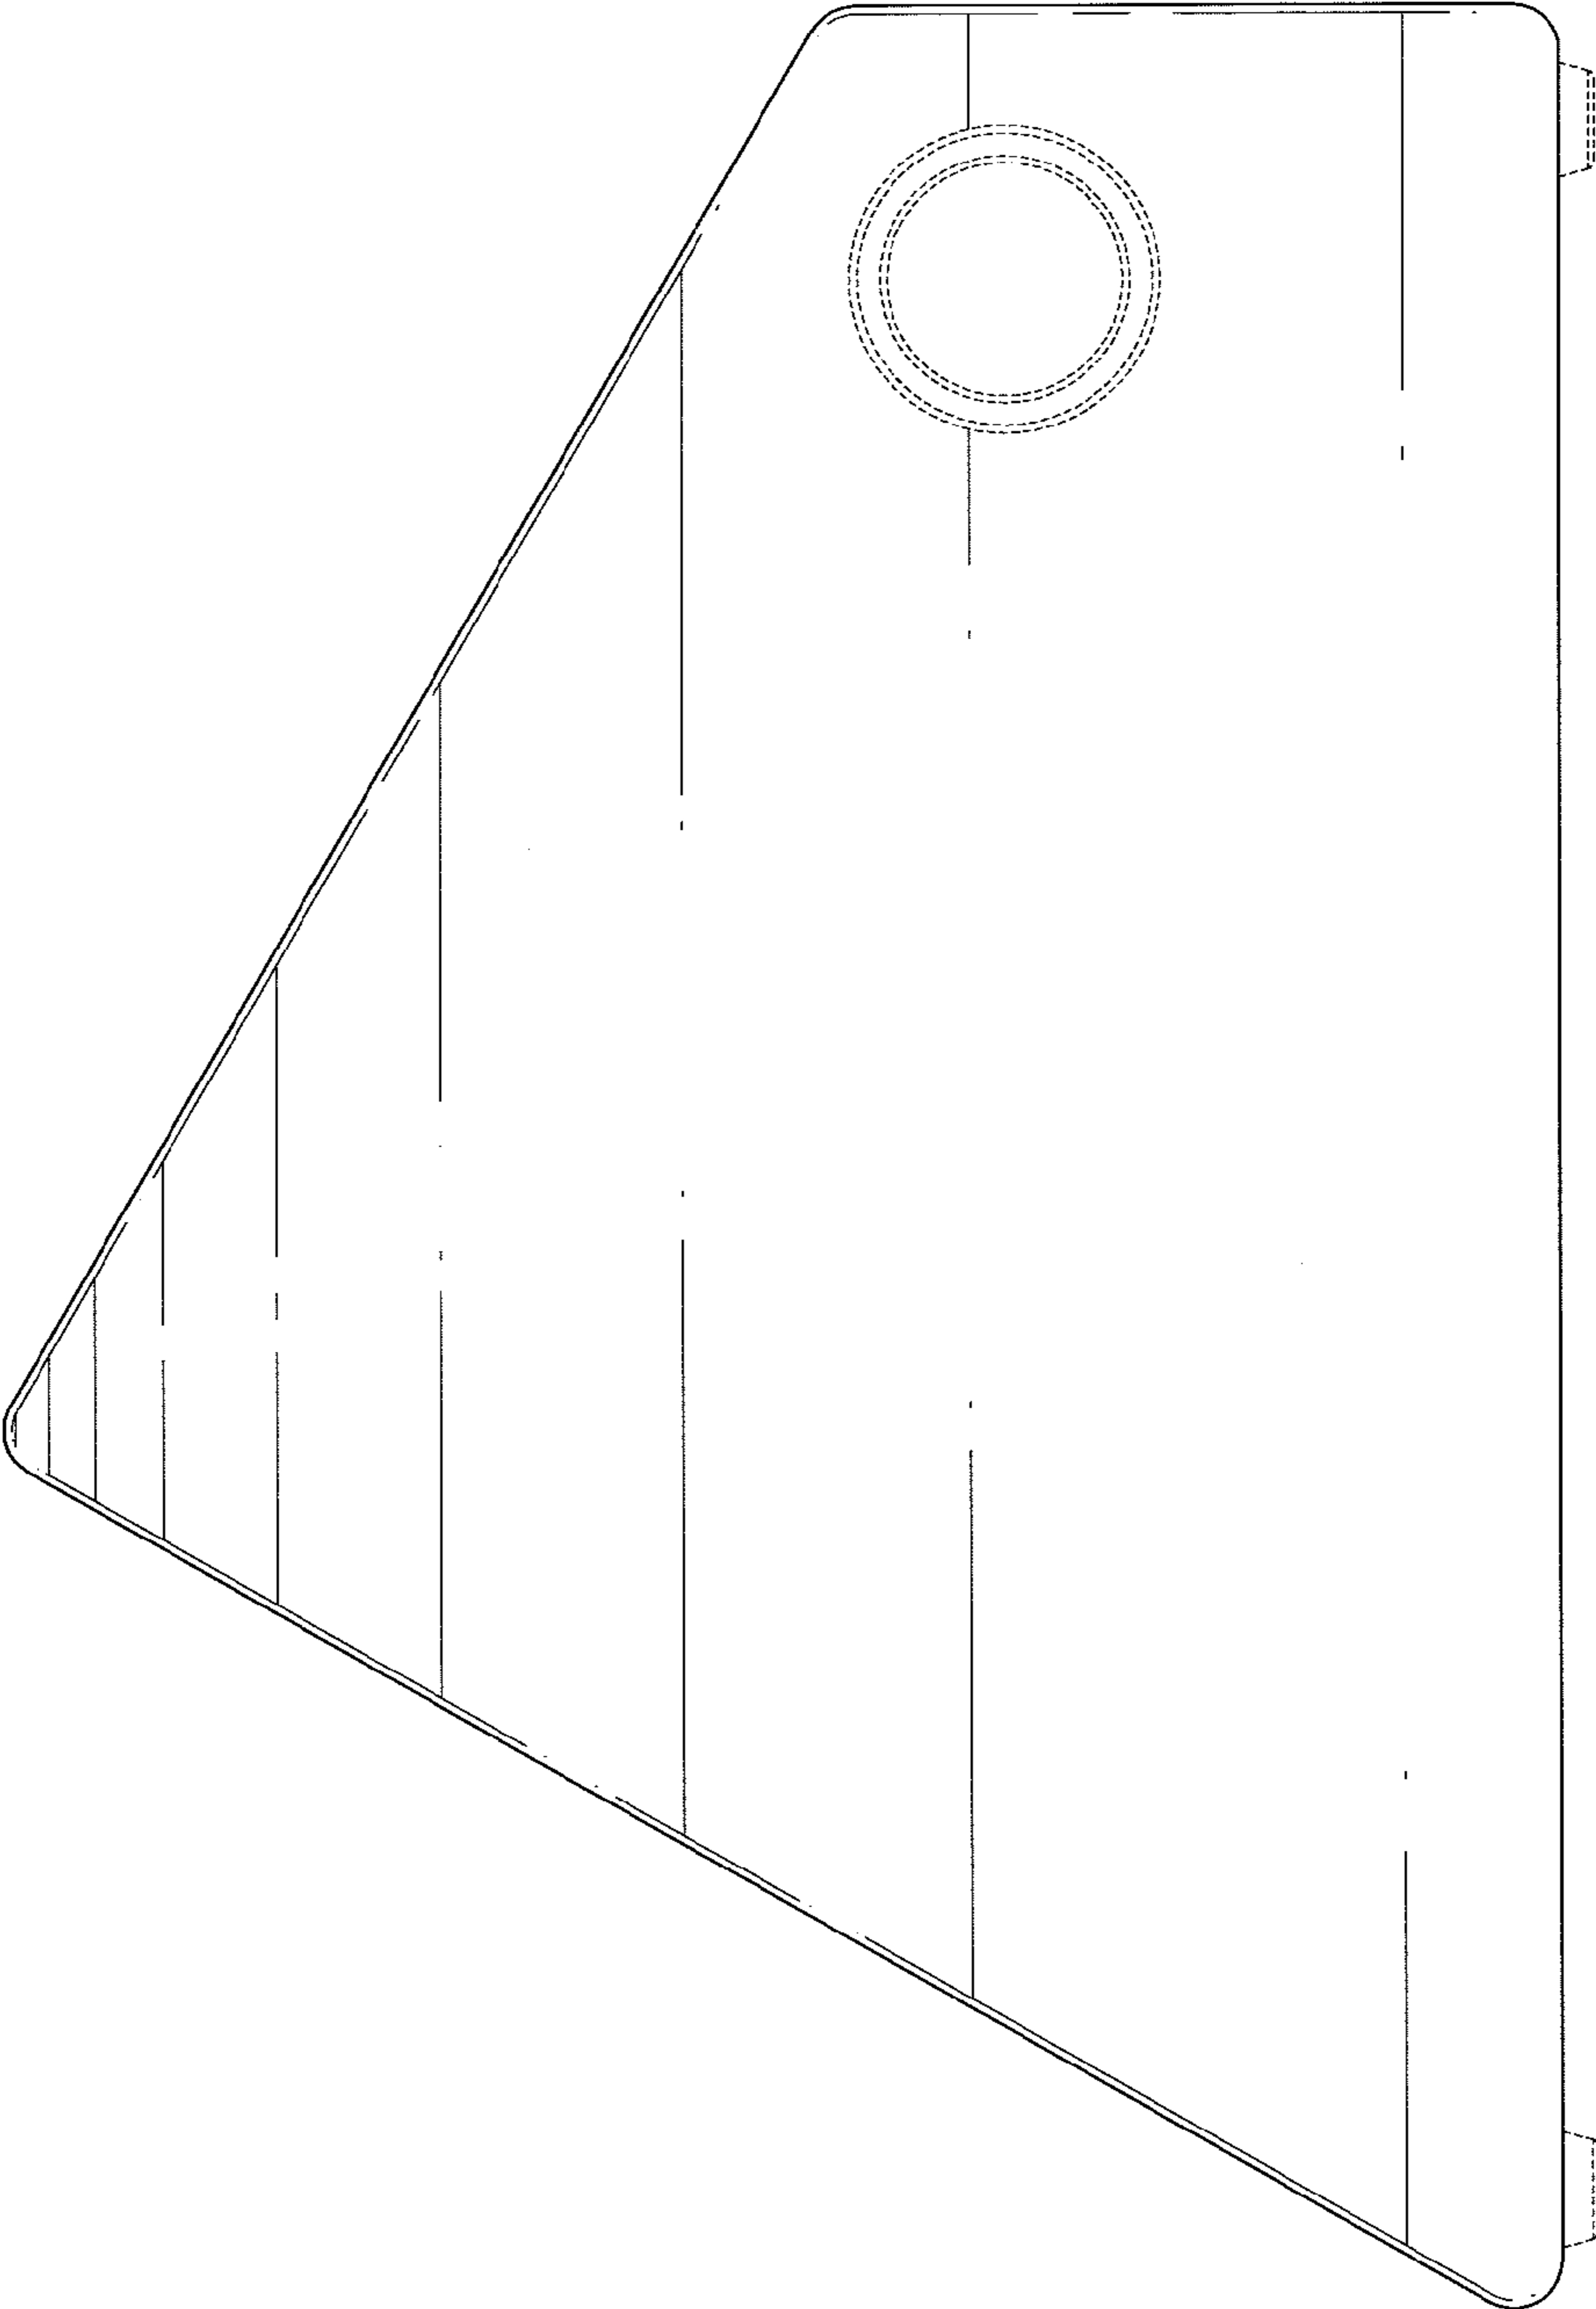


FIG. 3

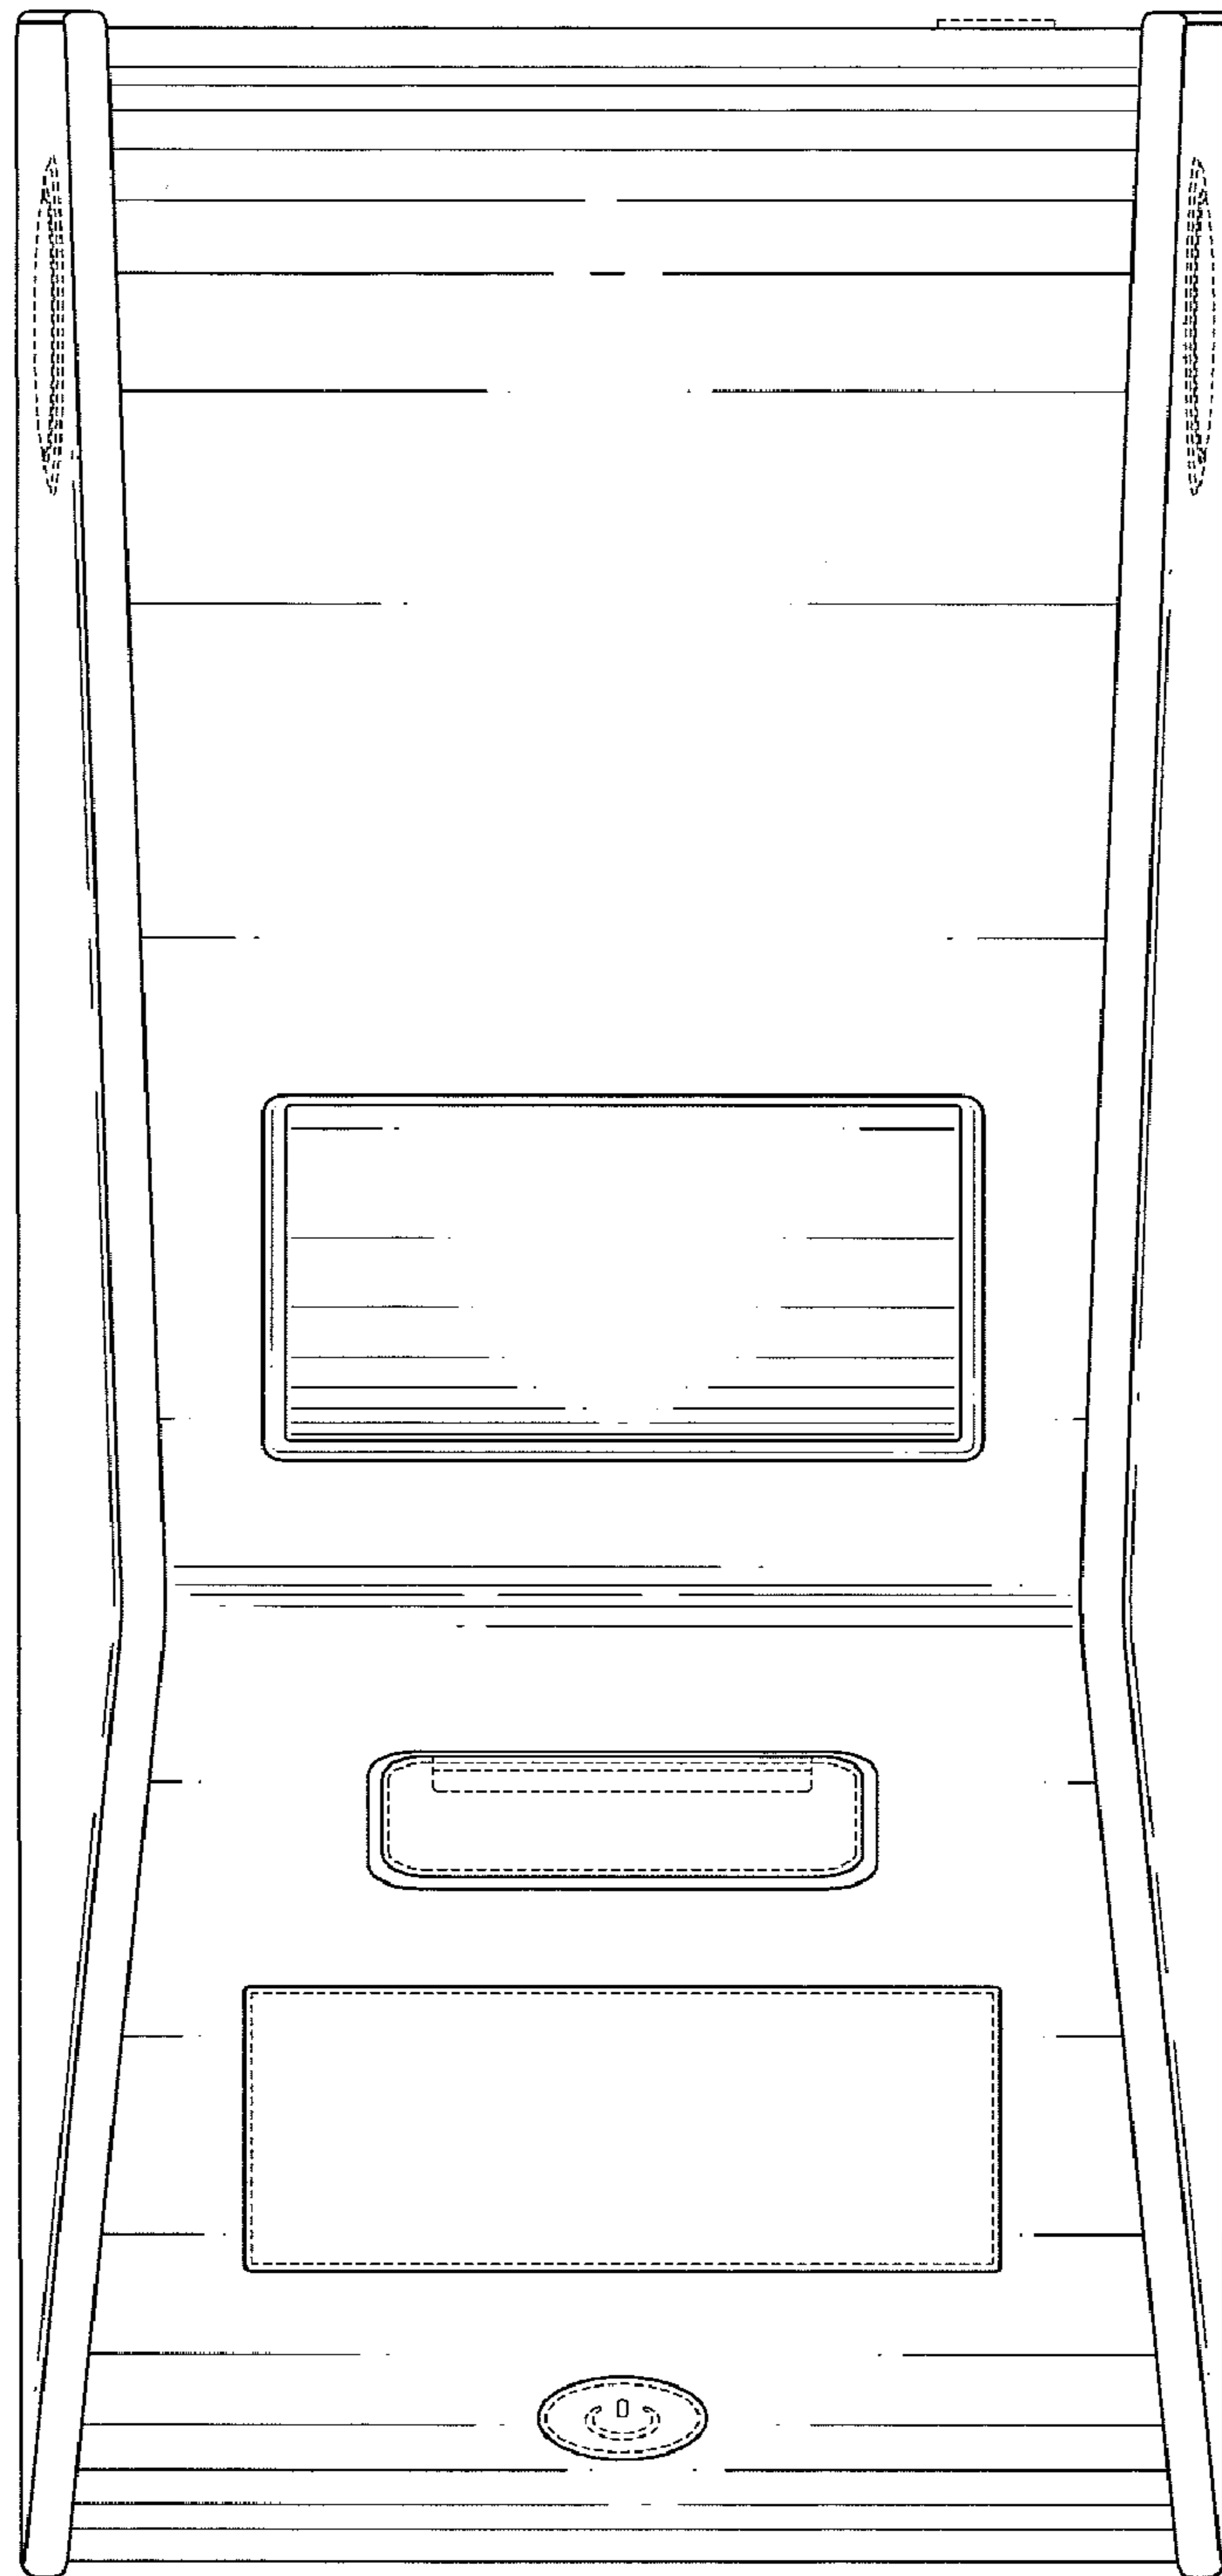


FIG. 4

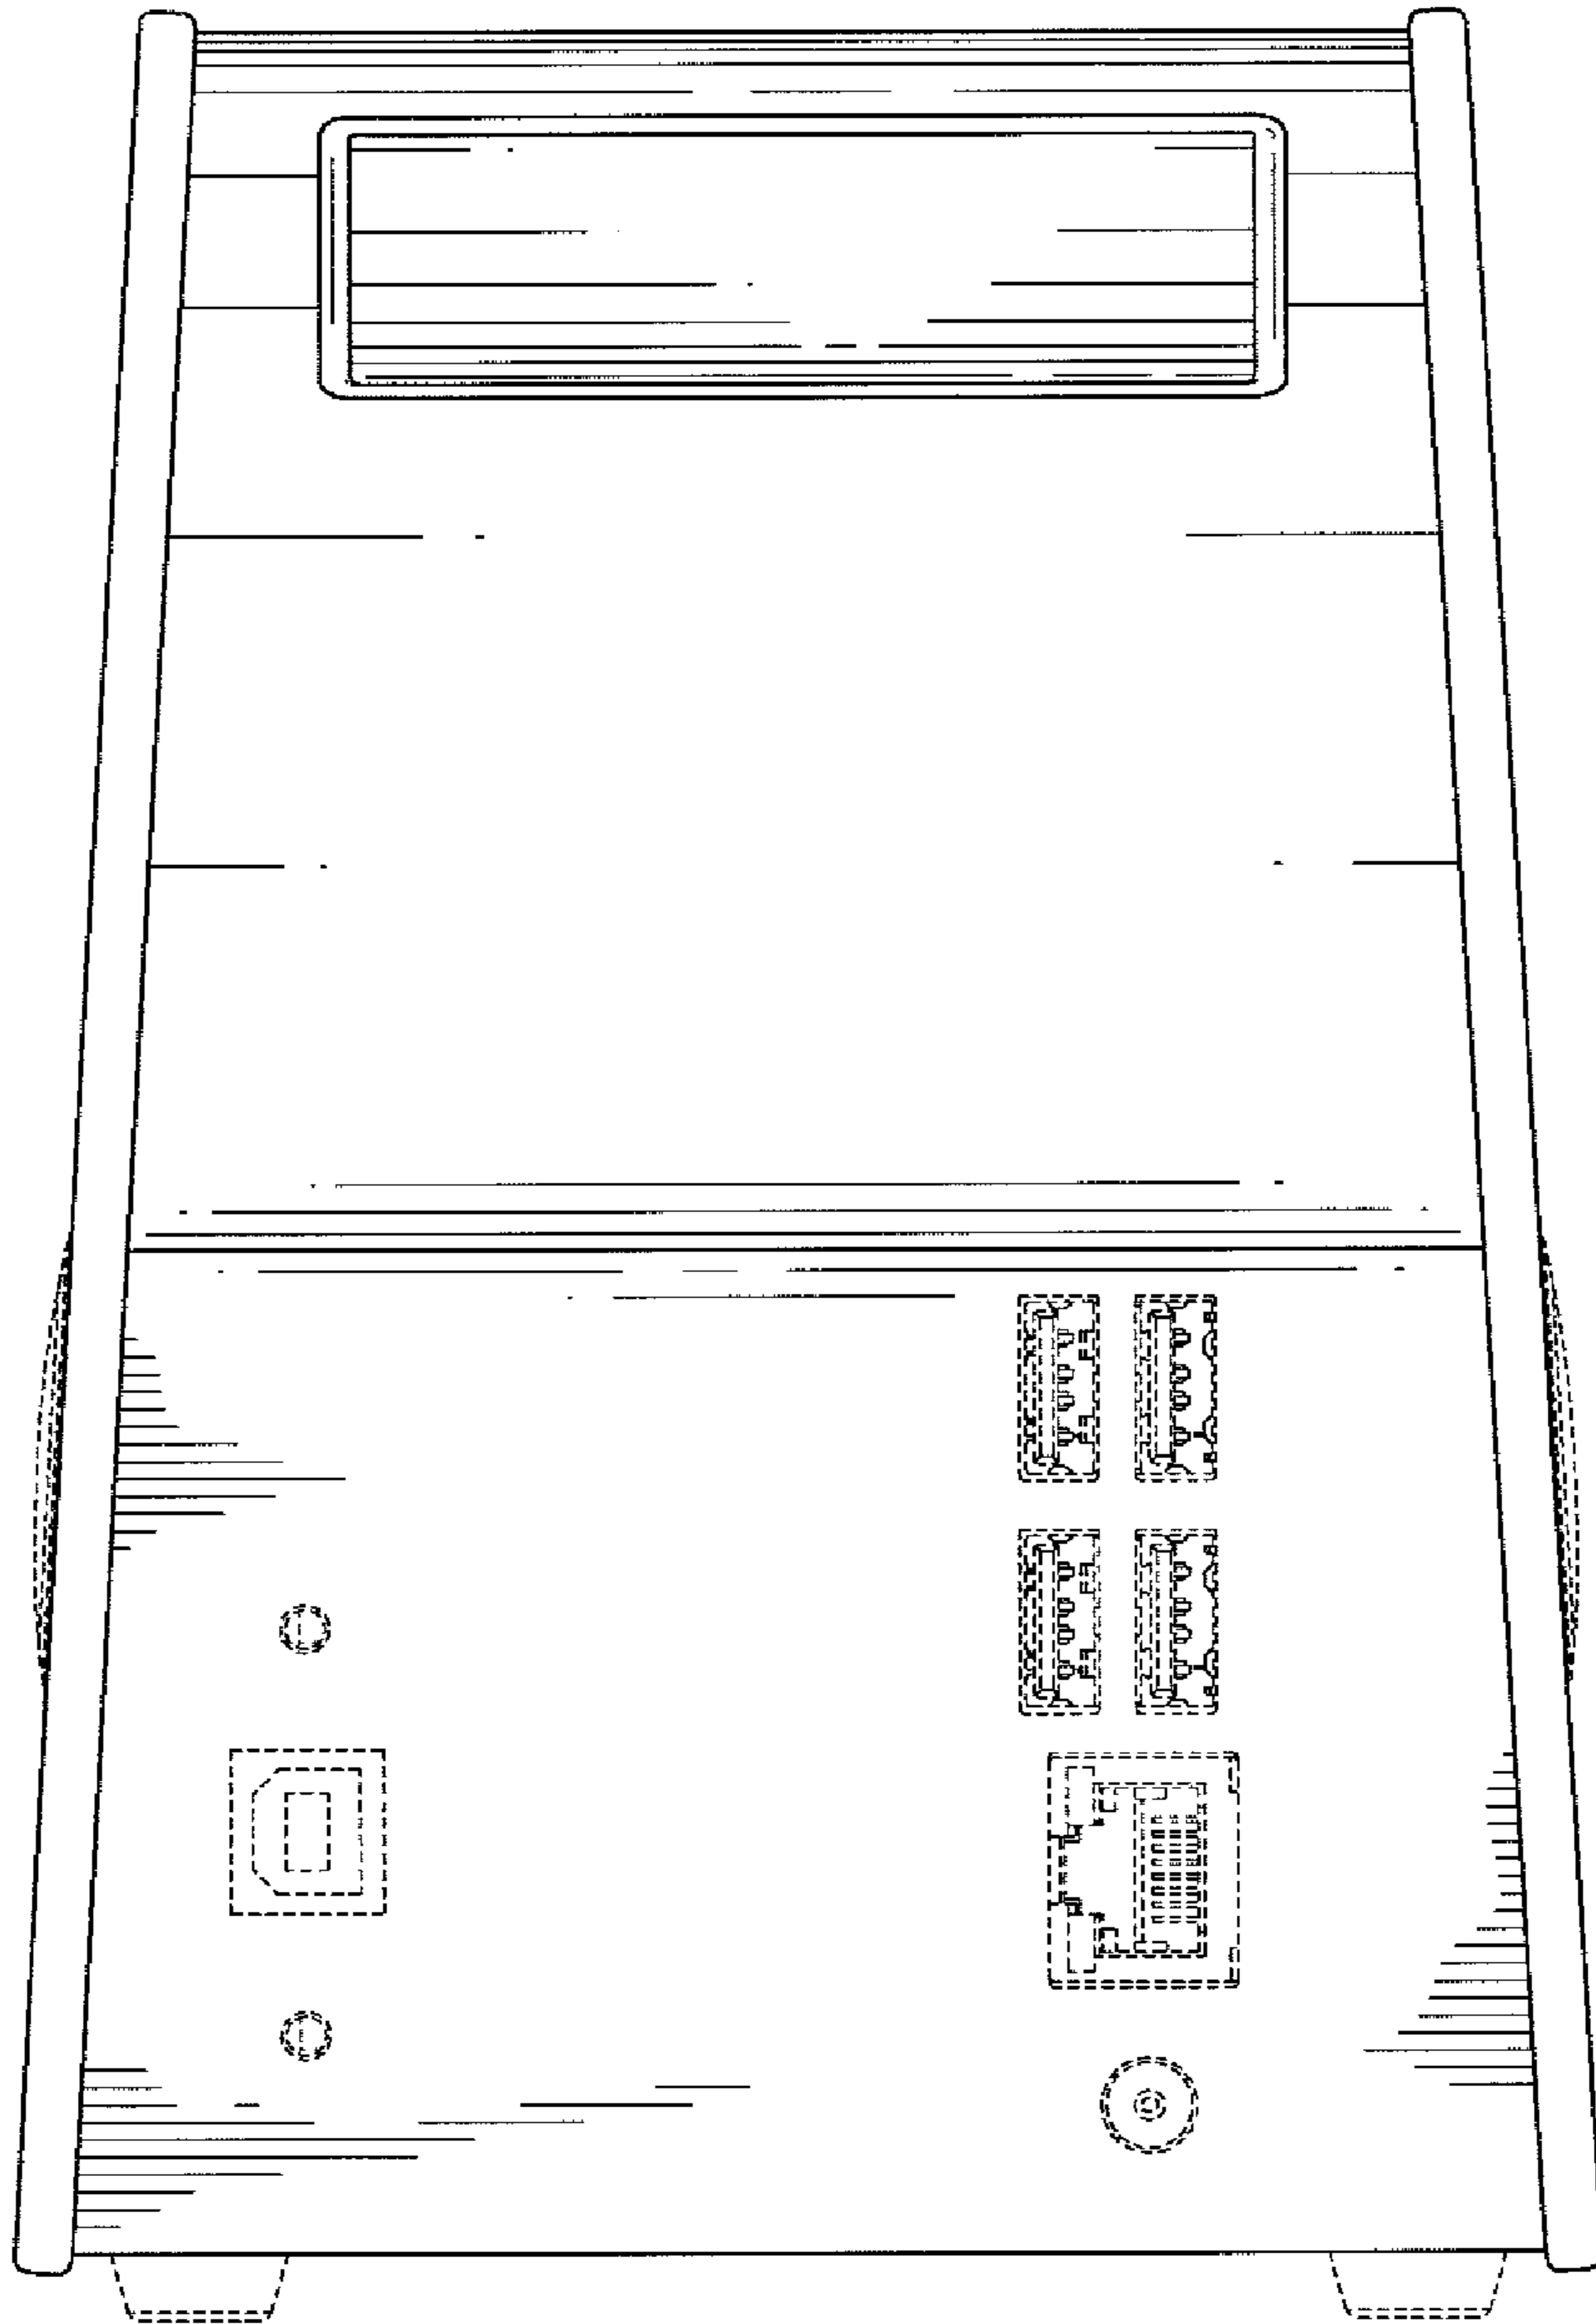


FIG. 5

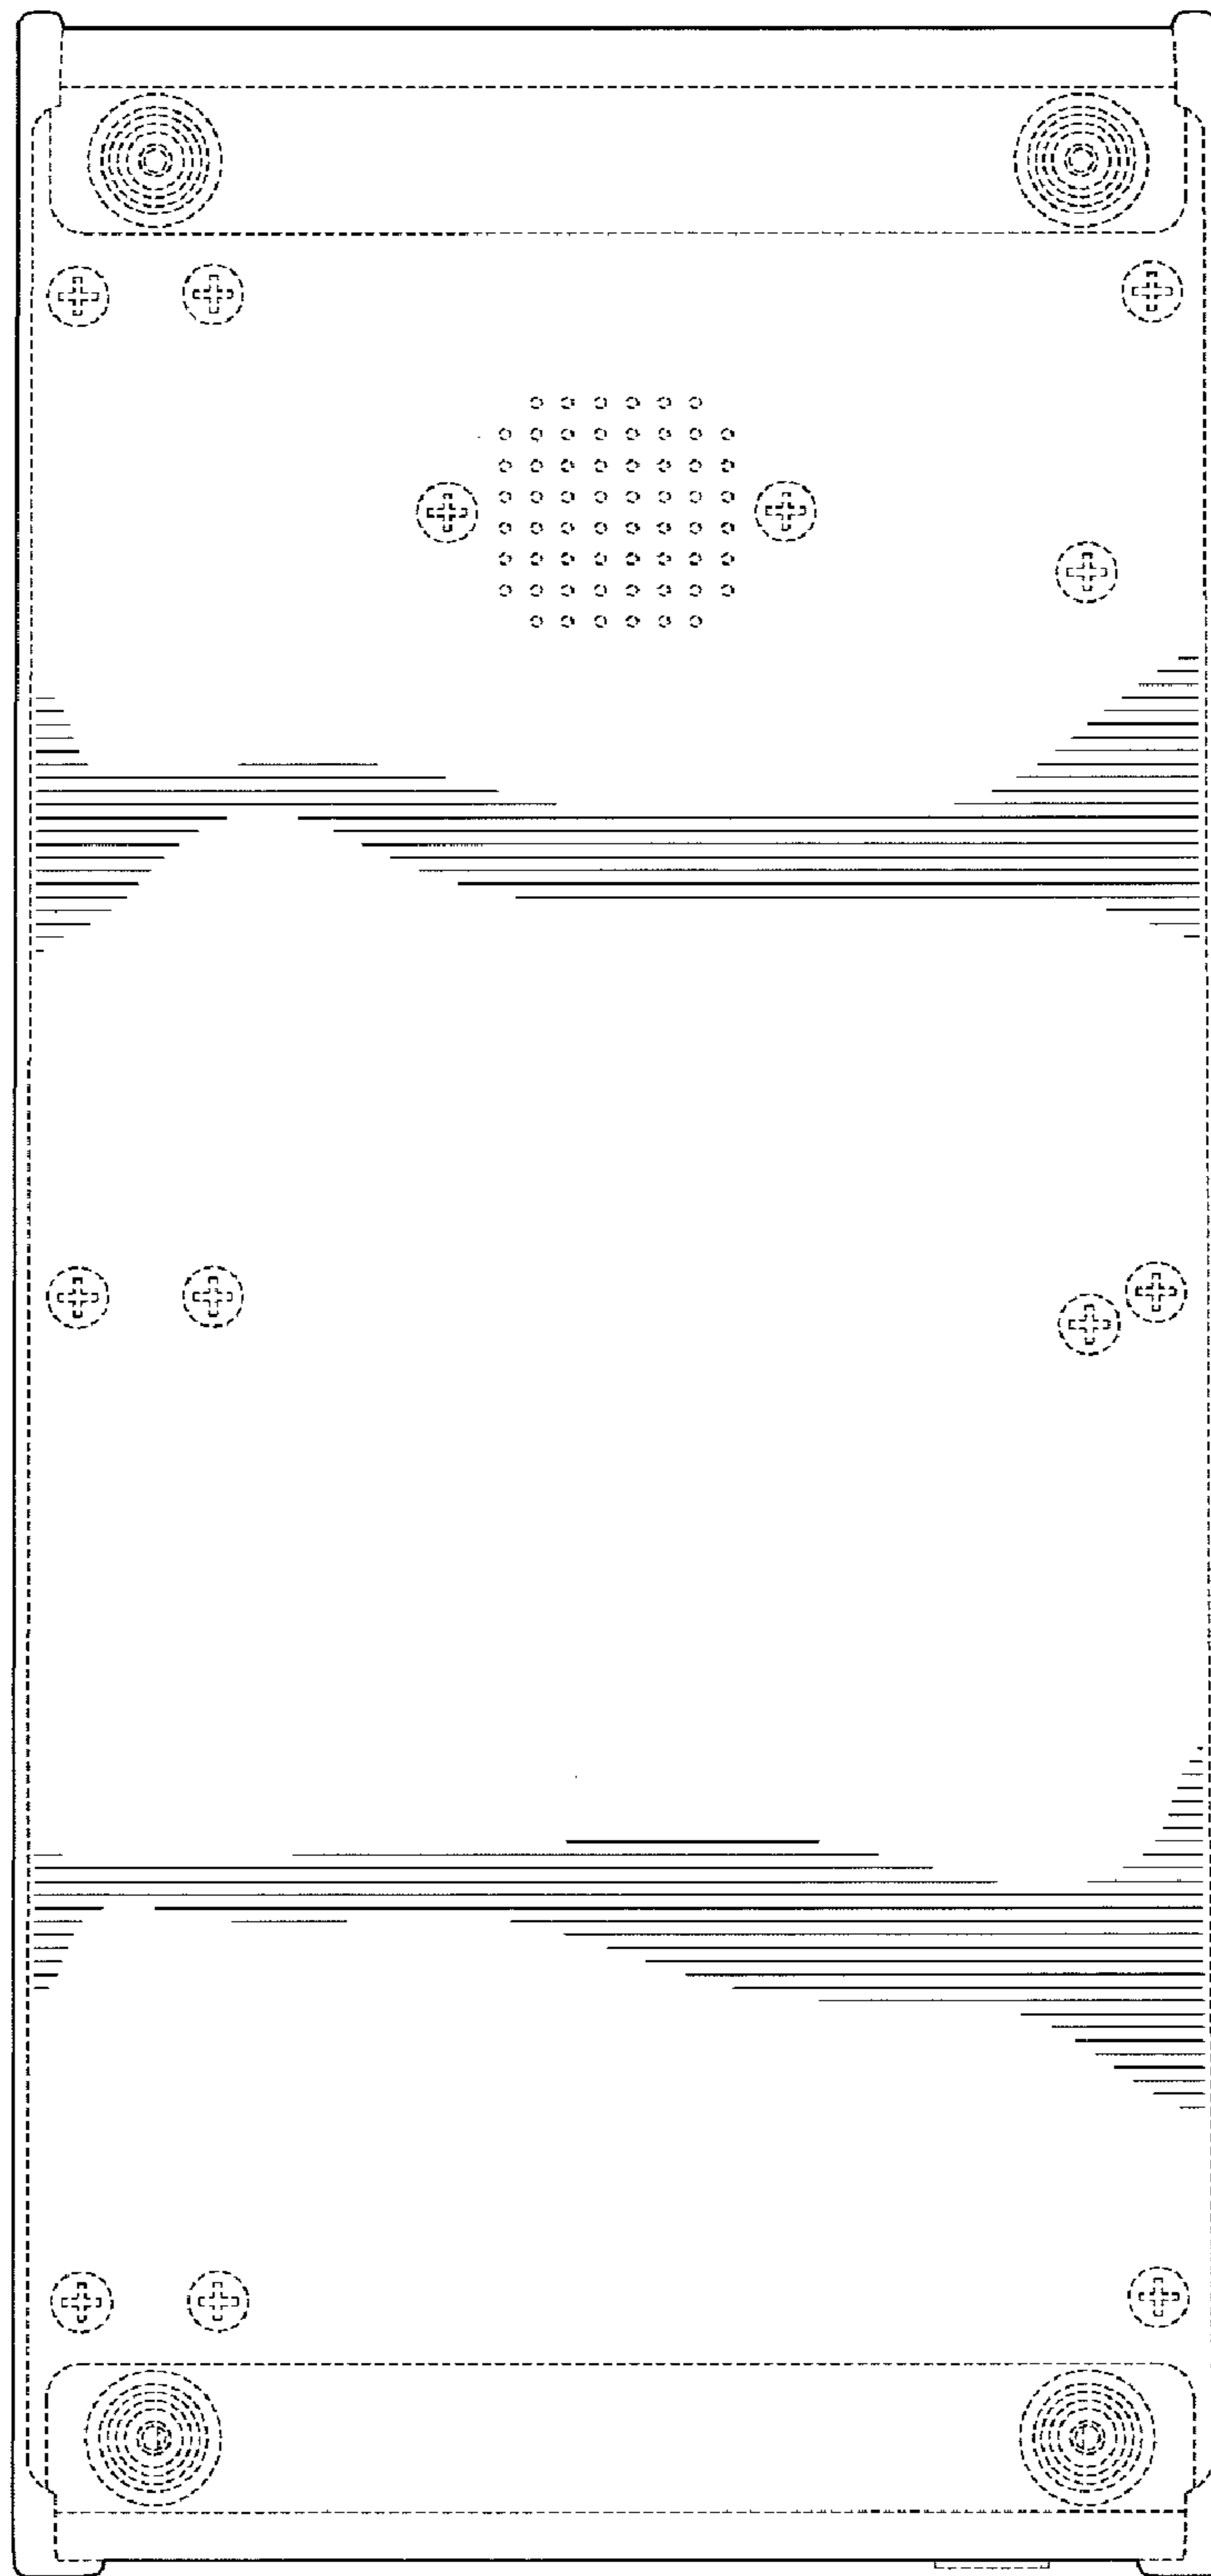


FIG. 6

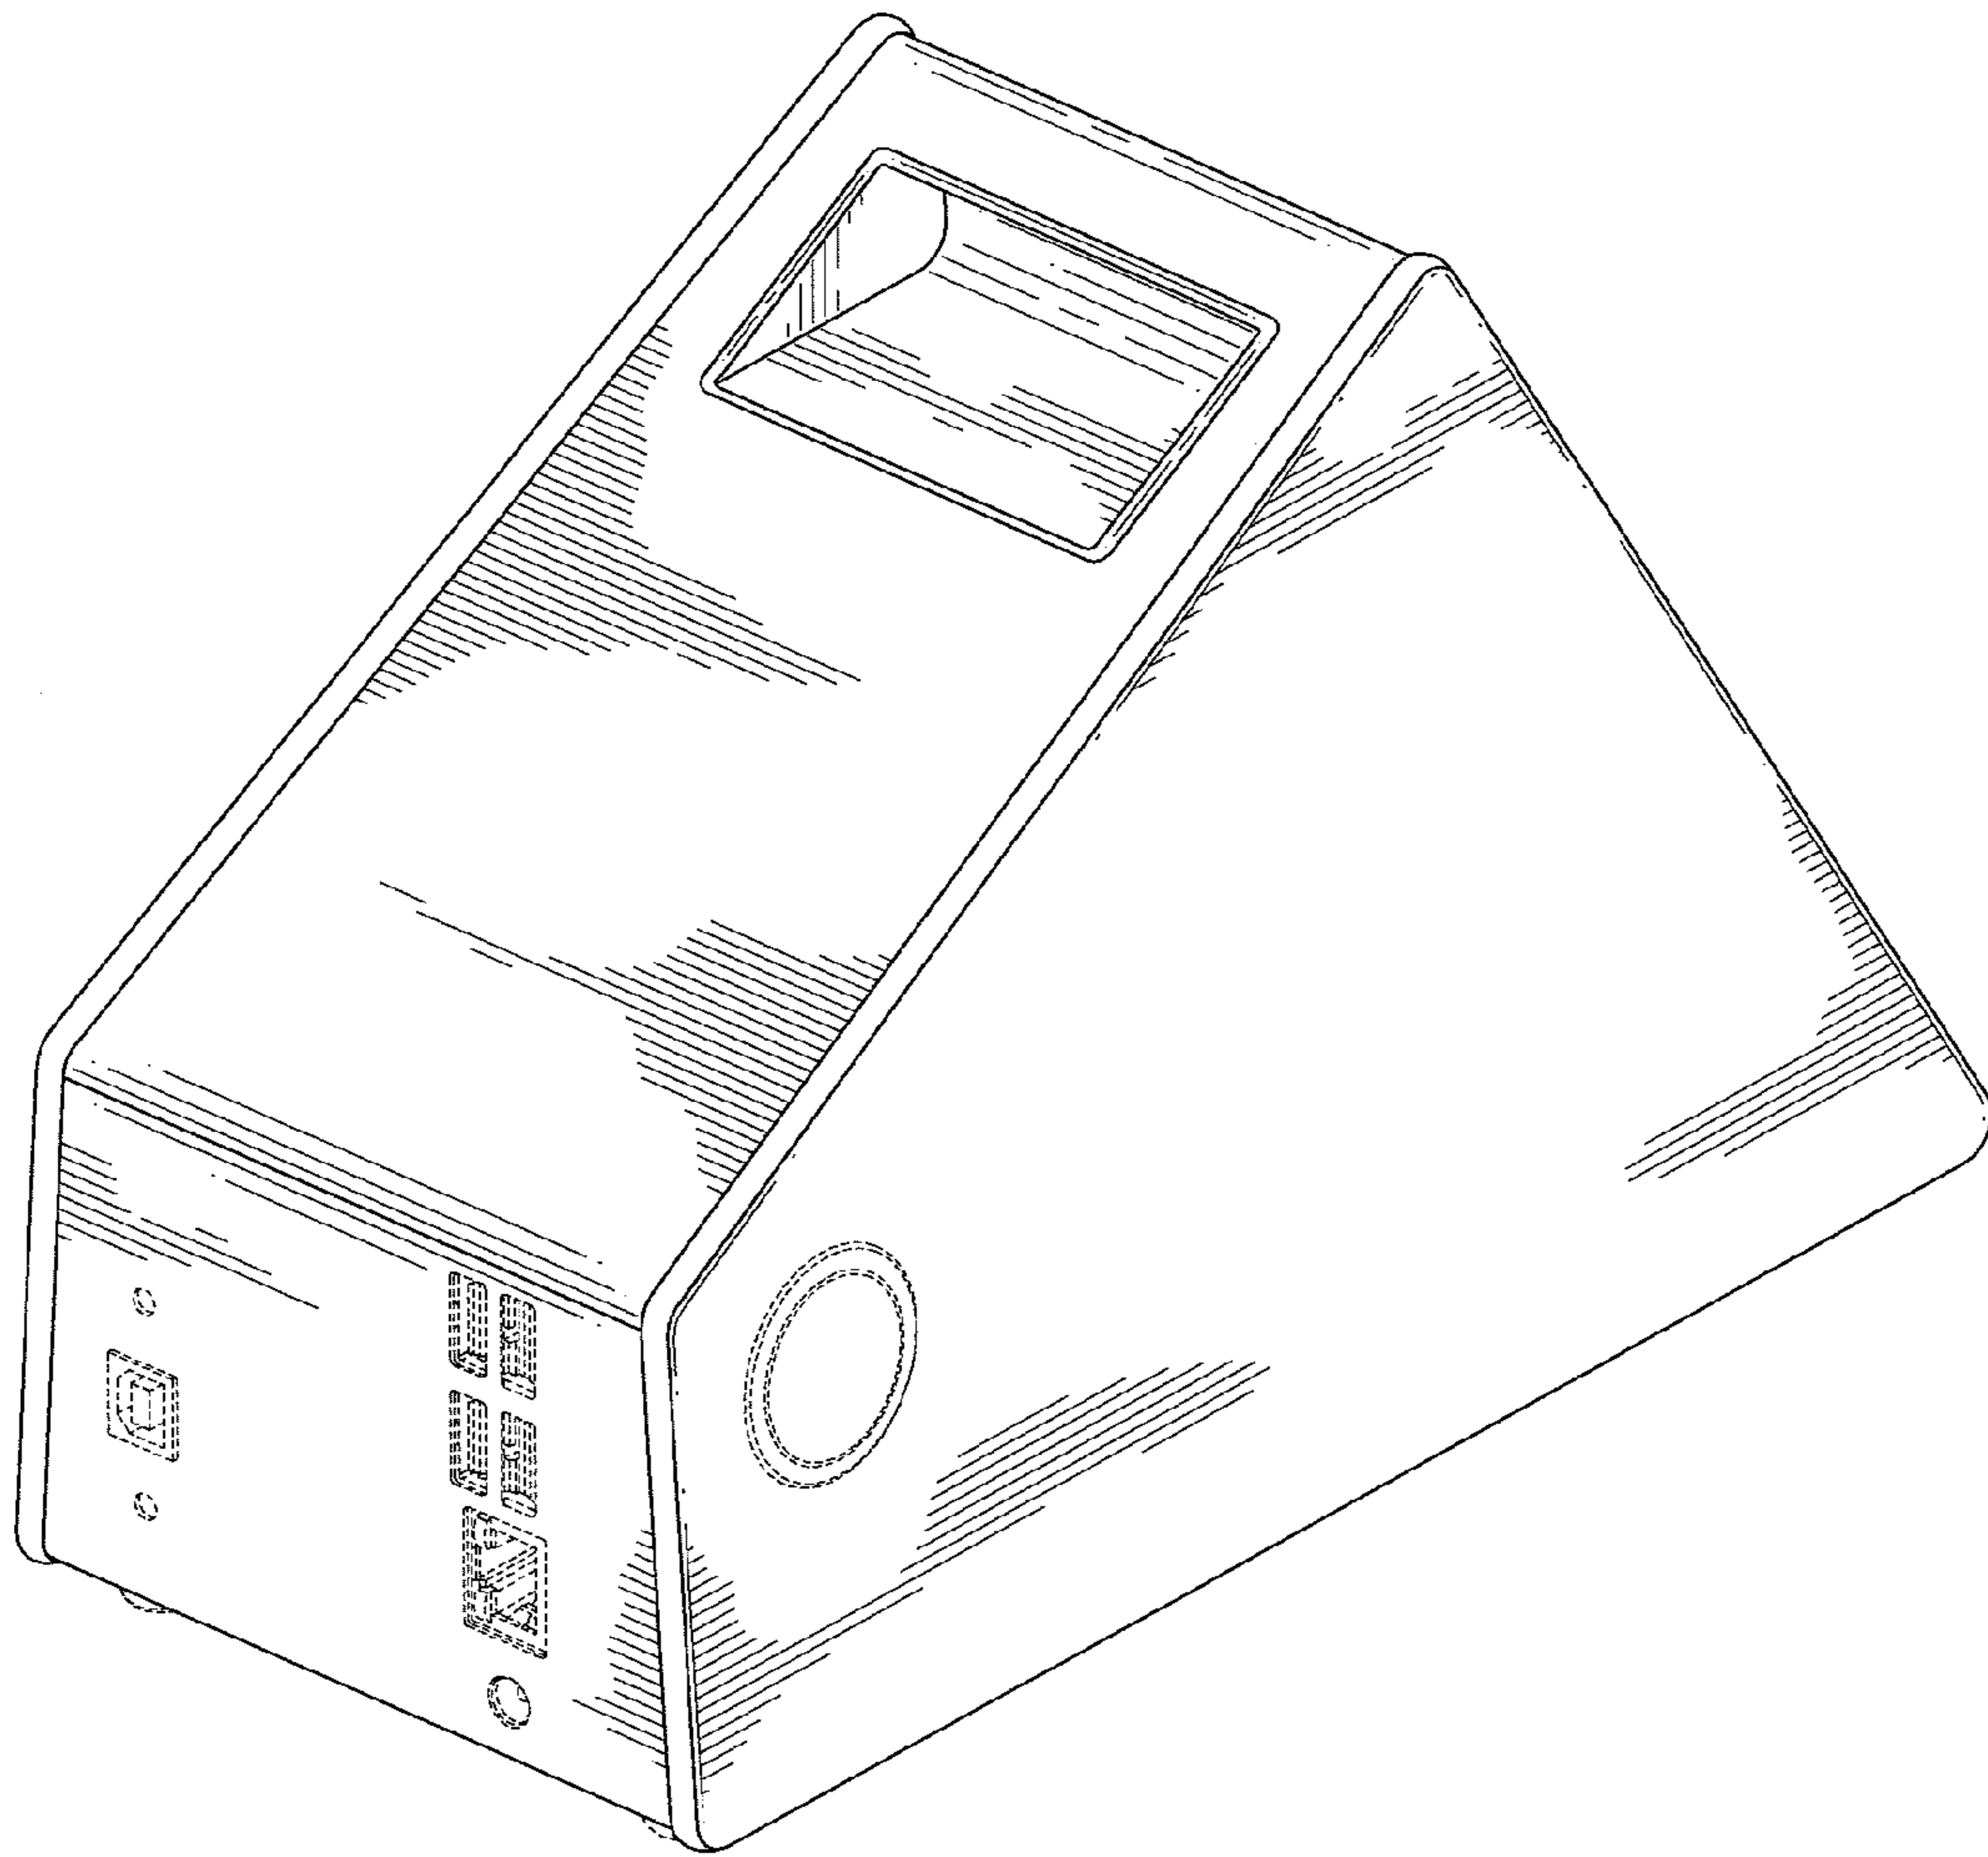


FIG. 7