



US00D678532S

(12) **United States Design Patent**  
**Powers et al.**

(10) **Patent No.:** **US D678,532 S**  
(45) **Date of Patent:** **\*\* Mar. 19, 2013**

(54) **PEDIATRIC MODE KEY FOR AN EXTERNAL DEFIBRILLATOR HAVING AN ELECTRODE PAD PLACEMENT OVERLAY**

(75) Inventors: **Daniel J. Powers**, Issaquah, WA (US);  
**Kurt Fischer**, Lynnwood, WA (US)

(73) Assignee: **Koninklijke Philips Electronics N.V.**,  
Eindhoven (NL)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/398,241**

(22) Filed: **Jul. 28, 2011**

**Related U.S. Application Data**

(63) Continuation-in-part of application No. 11/721,549,  
filed on Jun. 13, 2007.

(51) **LOC (9) Cl.** ..... **24-01**

(52) **U.S. Cl.** ..... **D24/187**

(58) **Field of Classification Search** ..... D24/167-168,  
D24/186-187, 200, 232; D13/182; 600/372-384,  
600/391-397, 386; 607/62, 109, 121, 139,  
607/149, 152, 153; D8/347-348; D9/707;  
D14/435-436; D10/106.9

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D291,121 S *	7/1987	Jones et al.	.....	D24/167
D332,045 S *	12/1992	Moore	.....	D8/347
D414,266 S *	9/1999	Pastrick et al.	.....	D24/168
D433,922 S *	11/2000	Hatada et al.	.....	D8/347
D450,708 S *	11/2001	Hsu	.....	D14/435
D453,338 S *	2/2002	Pentz et al.	.....	D14/436

D462,966 S *	9/2002	Pentz et al.	.....	D14/436
D473,234 S *	4/2003	Hussaini et al.	.....	D14/435
D498,848 S *	11/2004	Vaisnys et al.	.....	D24/187
D502,182 S *	2/2005	Mitchell et al.	.....	D14/436
D514,951 S *	2/2006	Vaisnys et al.	.....	D9/707
D534,414 S *	1/2007	Stifle et al.	.....	D8/347
D557,588 S *	12/2007	Stifle et al.	.....	D8/347
D621,689 S *	8/2010	Sedley	.....	D8/347
D631,370 S *	1/2011	Vaisnys et al.	.....	D9/707
D637,298 S *	5/2011	Vaisnys et al.	.....	D24/187
D649,486 S *	11/2011	Daniels et al.	.....	D10/106.9

\* cited by examiner

*Primary Examiner* — T. Chase Nelson

*Assistant Examiner* — Mark Cavanna

(57) **CLAIM**

The ornamental design for a pediatric mode key for an external defibrillator having an electrode pad placement overlay, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of a pediatric mode key for an external defibrillator having an electrode pad placement overlay showing our new design.

FIG. 2 is a front elevational view thereof;

FIG. 3 is a rear elevational view thereof;

FIG. 4 is a right side elevational view thereof;


FIG. 5 is a left side elevational view thereof;

FIG. 6 is a top plan view thereof; and,

FIG. 7 is a bottom plan view thereof.

The broken lines shown in FIG. 3 and FIG. 7 are included for the purpose of illustrating unclaimed portions of the pediatric mode key for an external defibrillator having an electrode pad placement overlay that form no part of the claimed design.

**1 Claim, 3 Drawing Sheets**

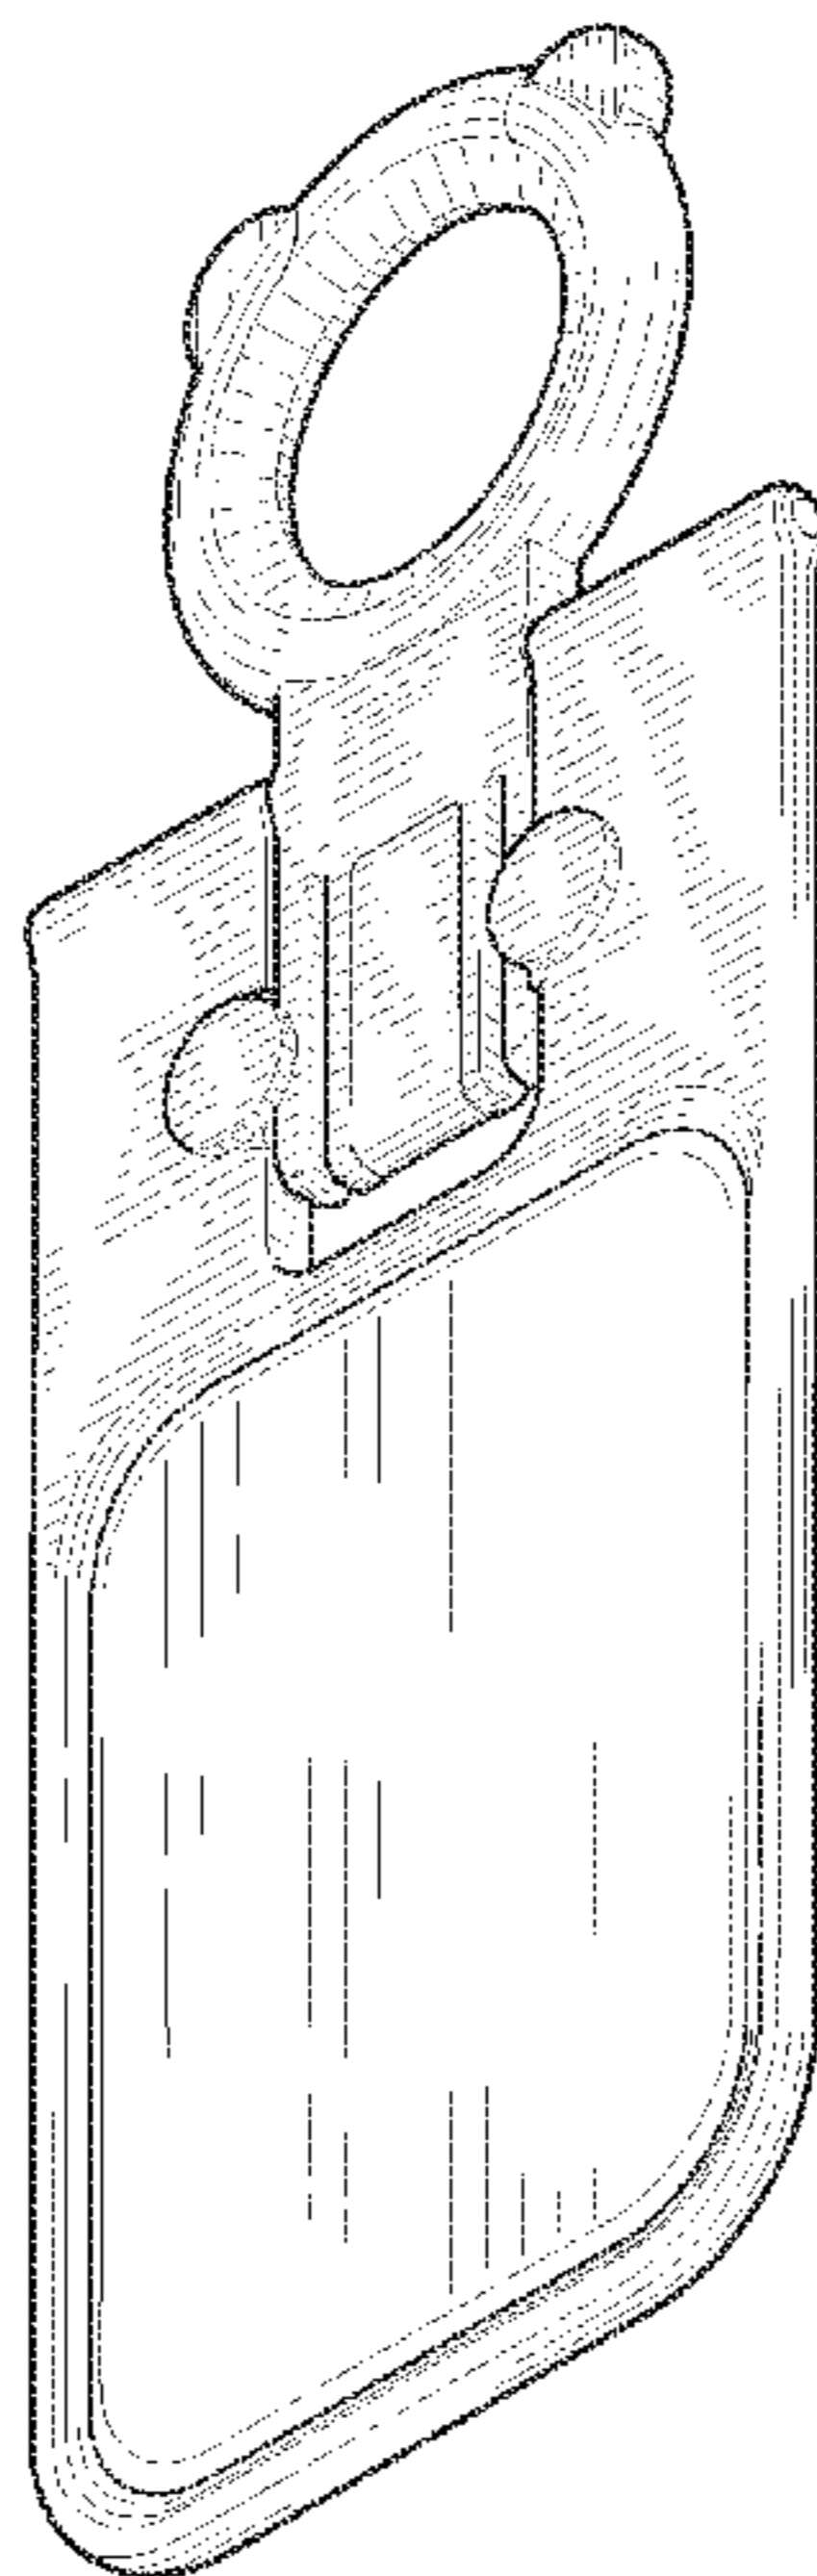

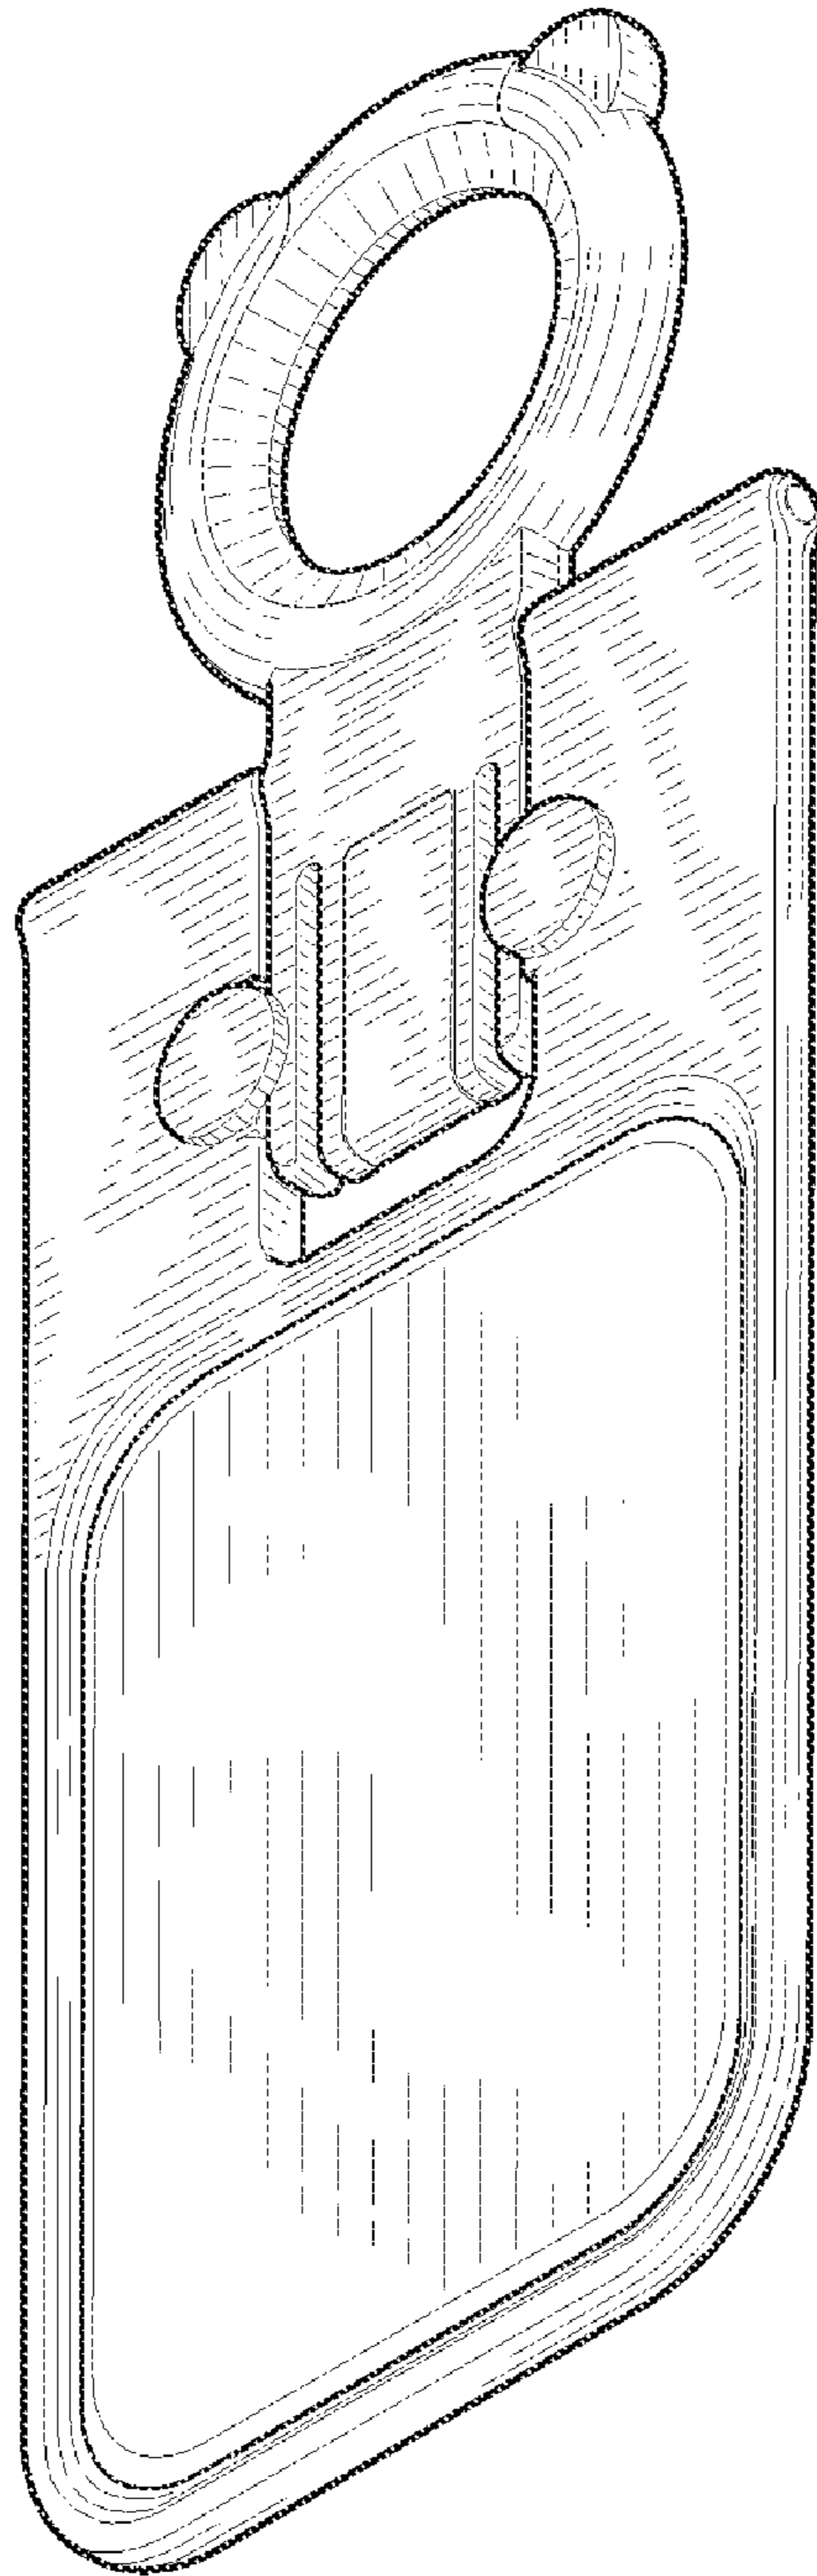


FIG. 1

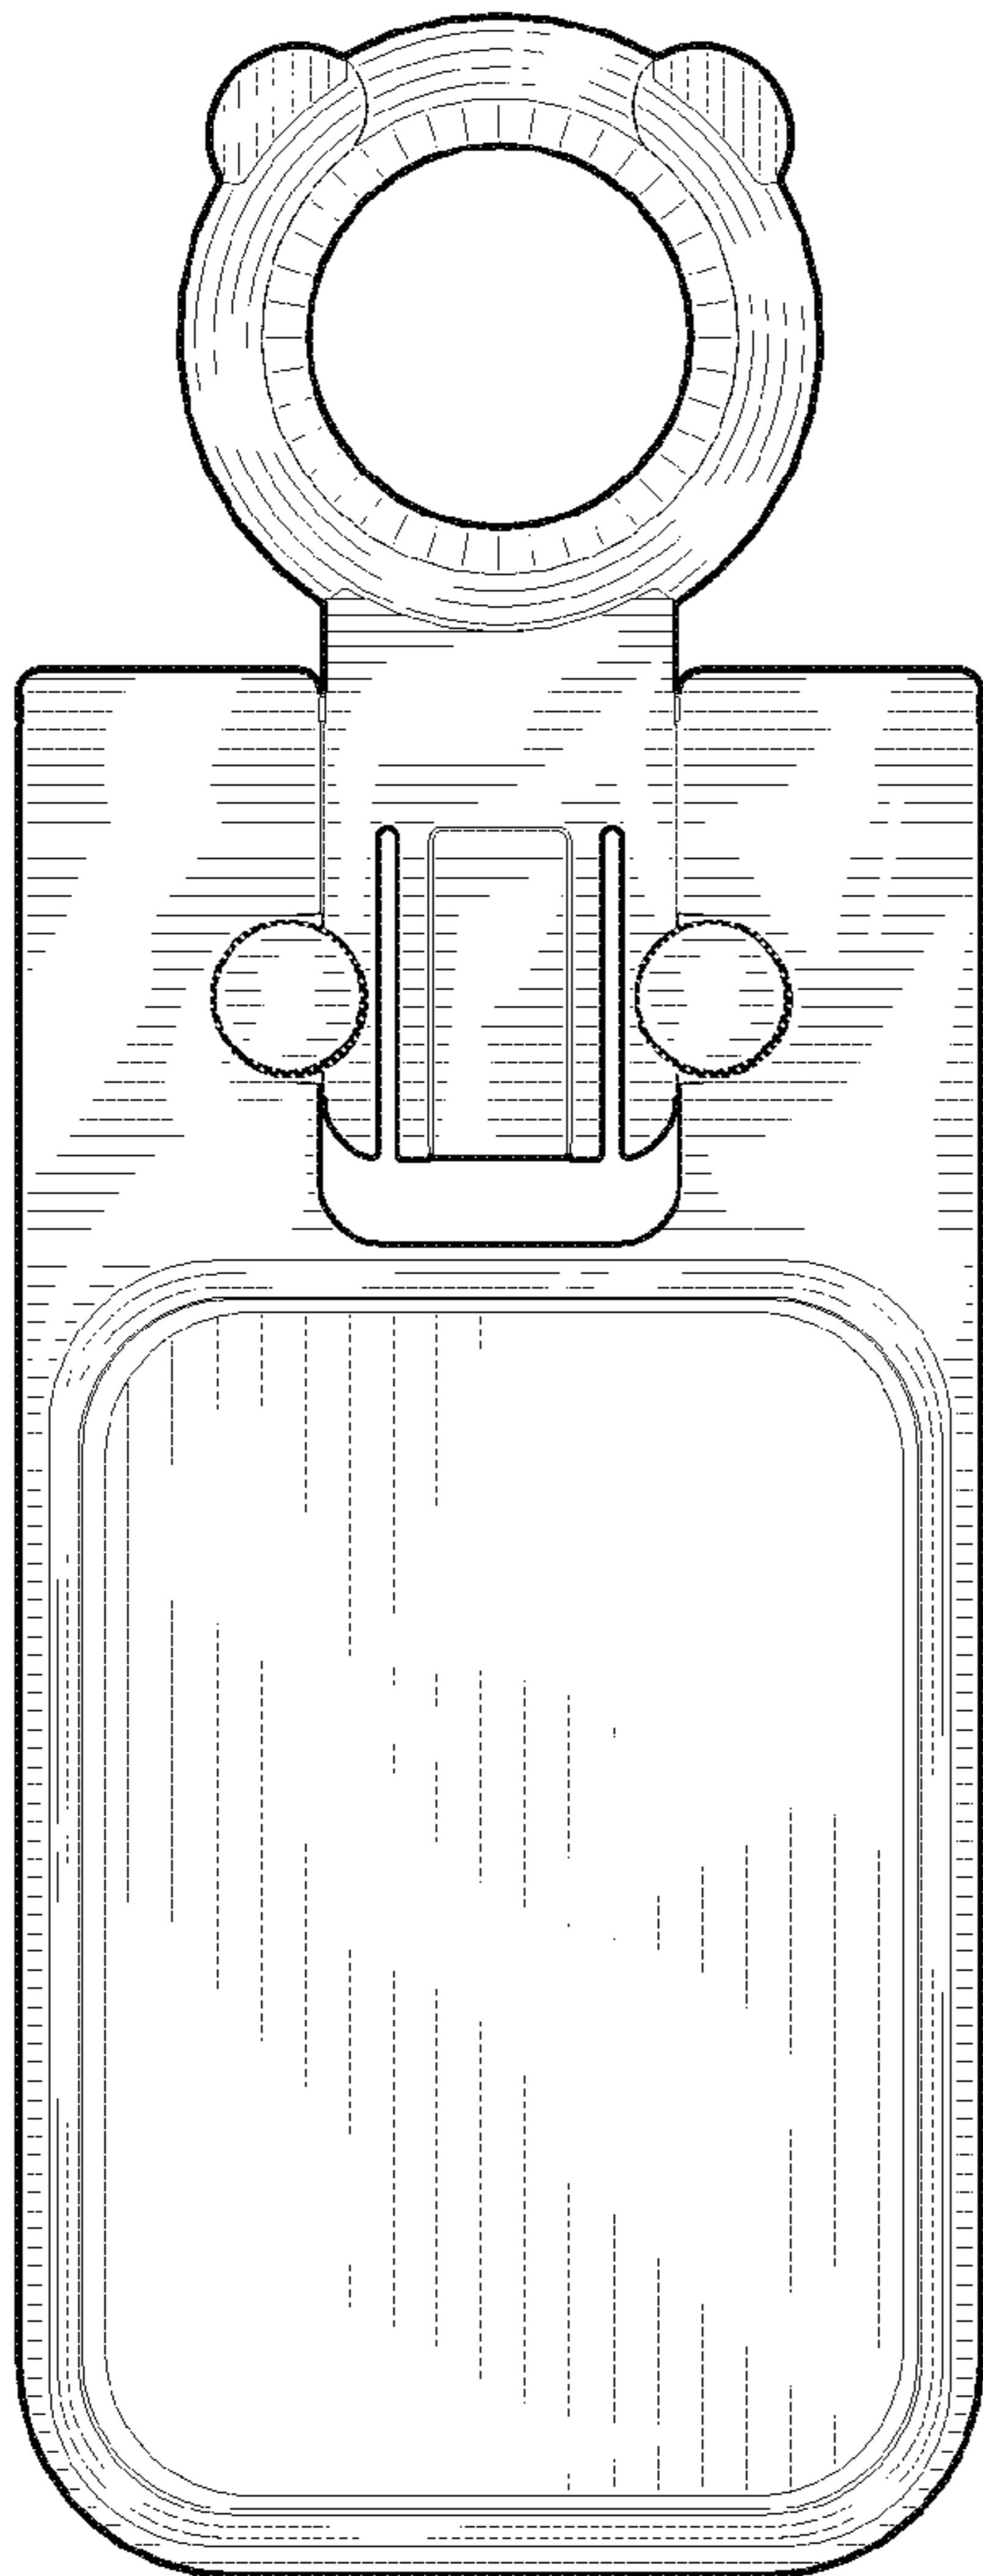


FIG. 2

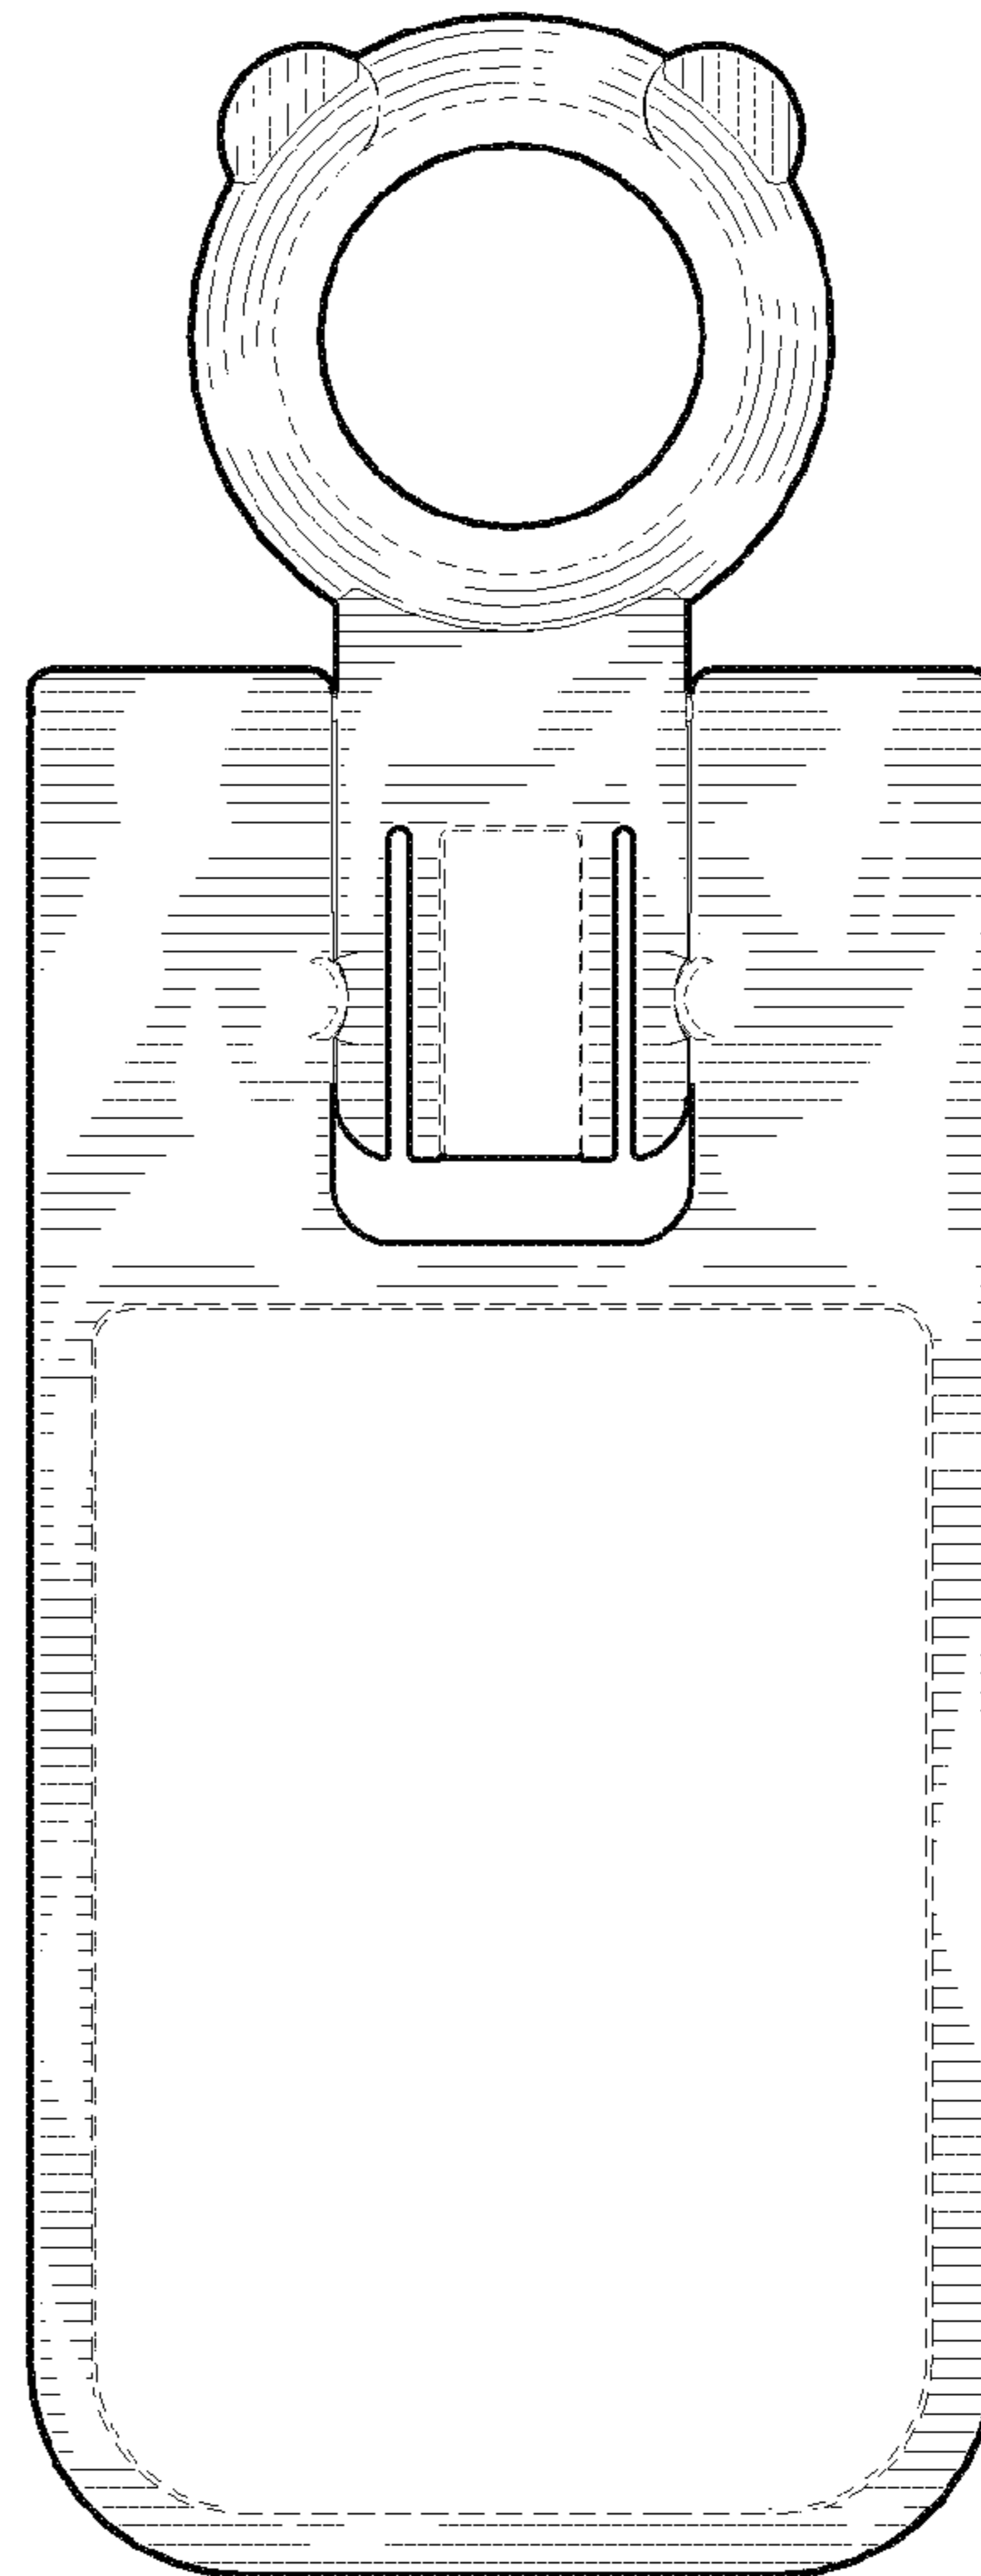


FIG. 3

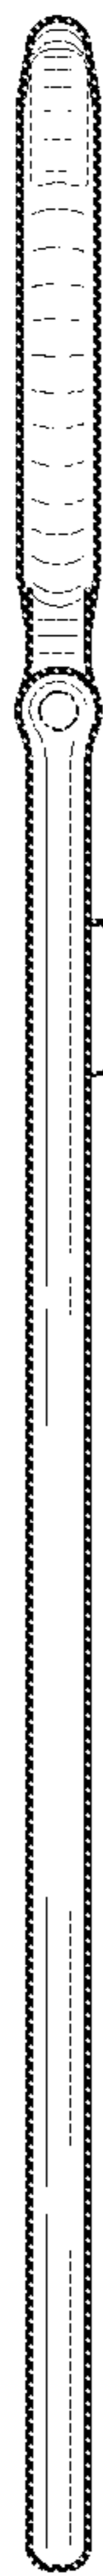


FIG. 4

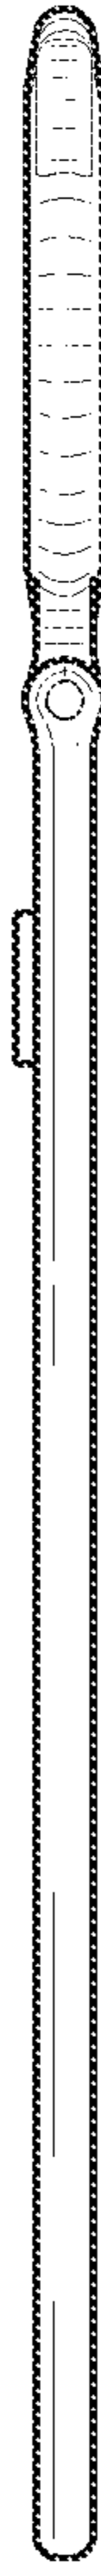


FIG. 5

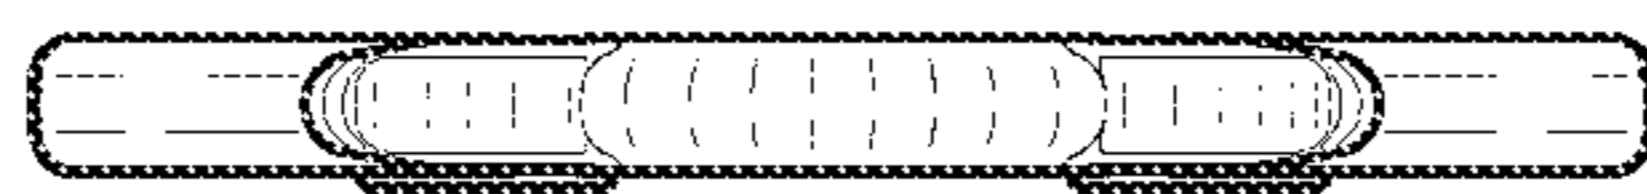


FIG. 6



FIG. 7