



US00D678532S

(12) **United States Design Patent**  
**Powers et al.**

(10) **Patent No.:** **US D678,532 S**  
(45) **Date of Patent:** **\*\* Mar. 19, 2013**

(54) **PEDIATRIC MODE KEY FOR AN EXTERNAL DEFIBRILLATOR HAVING AN ELECTRODE PAD PLACEMENT OVERLAY**

(75) Inventors: **Daniel J. Powers**, Issaquah, WA (US);  
**Kurt Fischer**, Lynnwood, WA (US)

(73) Assignee: **Koninklijke Philips Electronics N.V.**,  
Eindhoven (NL)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/398,241**

(22) Filed: **Jul. 28, 2011**

**Related U.S. Application Data**

(63) Continuation-in-part of application No. 11/721,549,  
filed on Jun. 13, 2007.

(51) **LOC (9) Cl.** ..... **24-01**

(52) **U.S. Cl.** ..... **D24/187**

(58) **Field of Classification Search** ..... D24/167-168,  
D24/186-187, 200, 232; D13/182; 600/372-384,  
600/391-397, 386; 607/62, 109, 121, 139,  
607/149, 152, 153; D8/347-348; D9/707;  
D14/435-436; D10/106.9

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D291,121 S \* 7/1987 Jones et al. .... D24/167  
D332,045 S \* 12/1992 Moore ..... D8/347  
D414,266 S \* 9/1999 Pastrick et al. .... D24/168  
D433,922 S \* 11/2000 Hatada et al. .... D8/347  
D450,708 S \* 11/2001 Hsu ..... D14/435  
D453,338 S \* 2/2002 Pentz et al. .... D14/436

D462,966 S \* 9/2002 Pentz et al. .... D14/436  
D473,234 S \* 4/2003 Hussaini et al. .... D14/435  
D498,848 S \* 11/2004 Vaisnys et al. .... D24/187  
D502,182 S \* 2/2005 Mitchell et al. .... D14/436  
D514,951 S \* 2/2006 Vaisnys et al. .... D9/707  
D534,414 S \* 1/2007 Stifle et al. .... D8/347  
D557,588 S \* 12/2007 Stifle et al. .... D8/347  
D621,689 S \* 8/2010 Sedley ..... D8/347  
D631,370 S \* 1/2011 Vaisnys et al. .... D9/707  
D637,298 S \* 5/2011 Vaisnys et al. .... D24/187  
D649,486 S \* 11/2011 Daniels et al. .... D10/106.9

\* cited by examiner

*Primary Examiner* — T. Chase Nelson

*Assistant Examiner* — Mark Cavanna

(57) **CLAIM**

The ornamental design for a pediatric mode key for an external defibrillator having an electrode pad placement overlay, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of a pediatric mode key for an external defibrillator having an electrode pad placement overlay showing our new design.

FIG. 2 is a front elevational view thereof;

FIG. 3 is a rear elevational view thereof;

FIG. 4 is a right side elevational view thereof;


FIG. 5 is a left side elevational view thereof;

FIG. 6 is a top plan view thereof; and,

FIG. 7 is a bottom plan view thereof.

The broken lines shown in FIG. 3 and FIG. 7 are included for the purpose of illustrating unclaimed portions of the pediatric mode key for an external defibrillator having an electrode pad placement overlay that form no part of the claimed design.

**1 Claim, 3 Drawing Sheets**

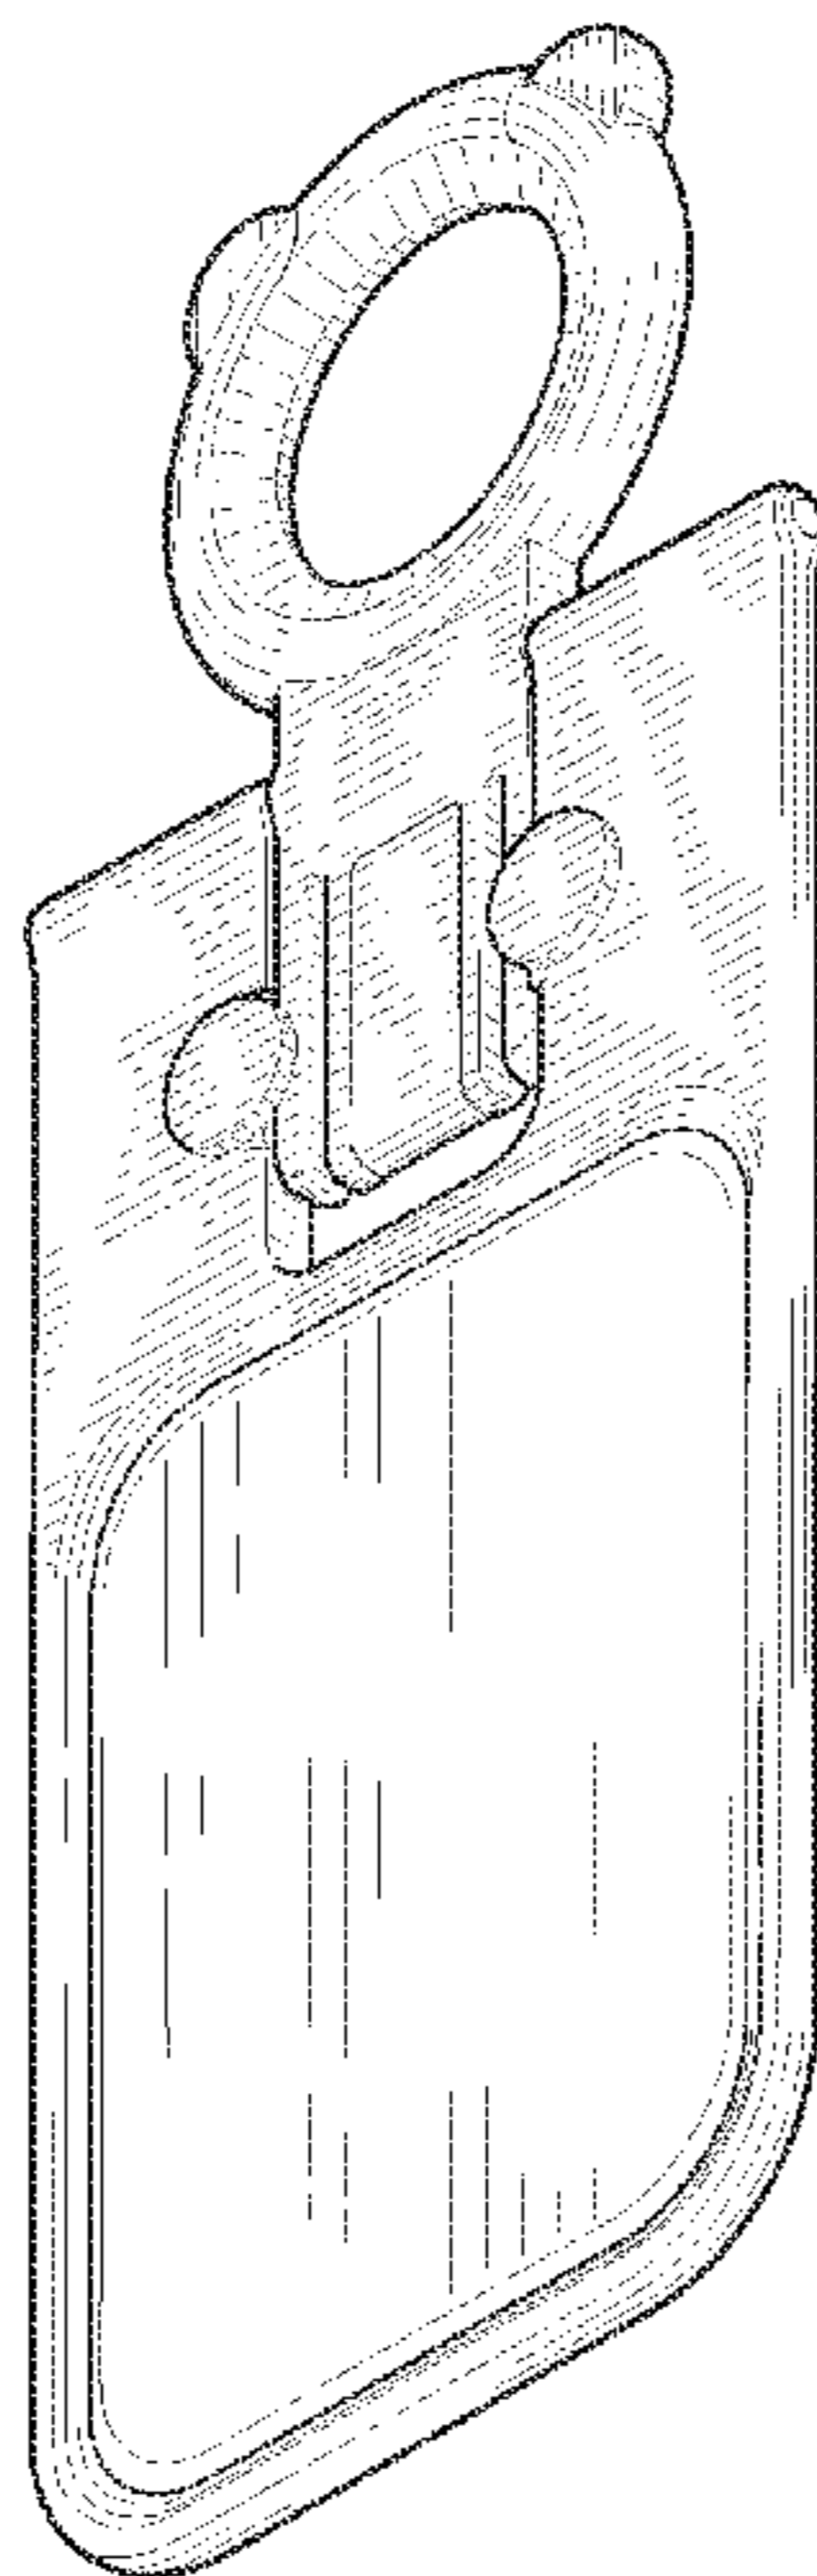

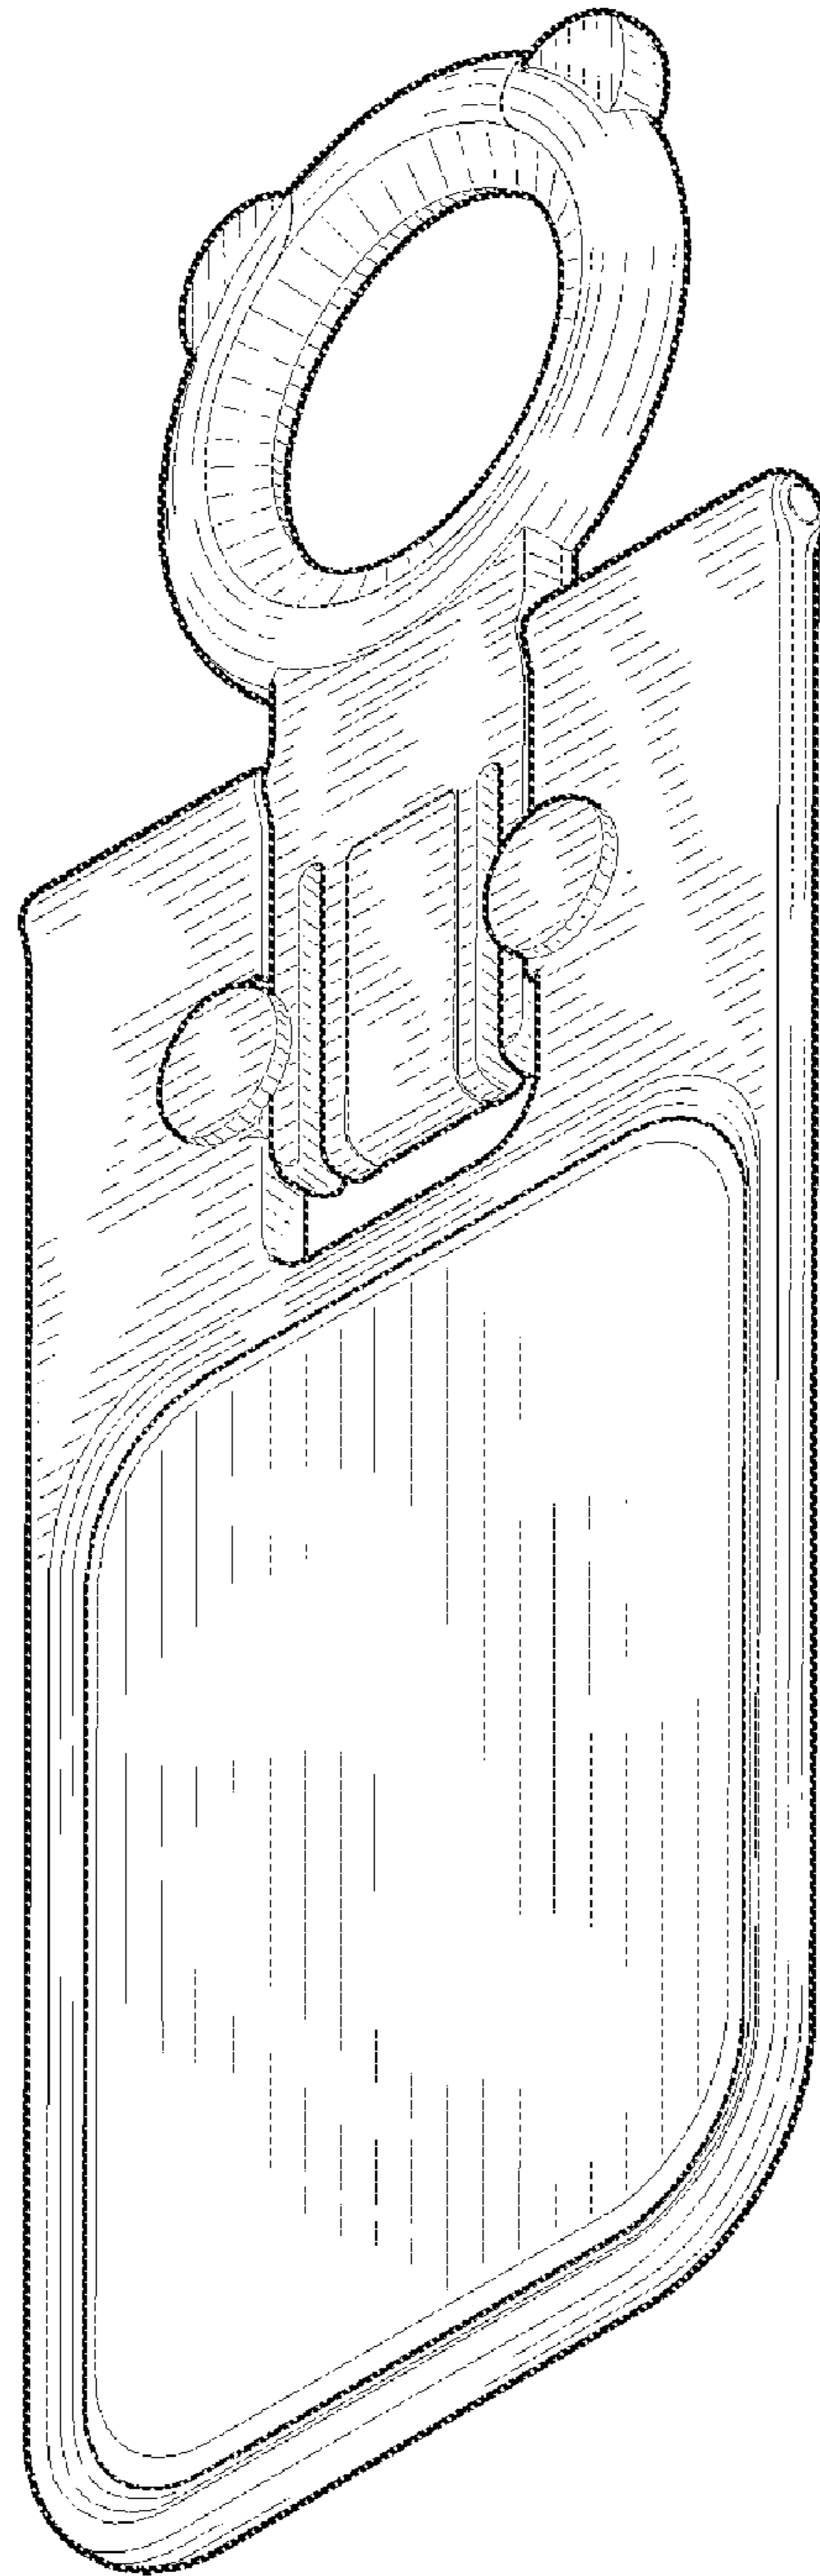


FIG. 1

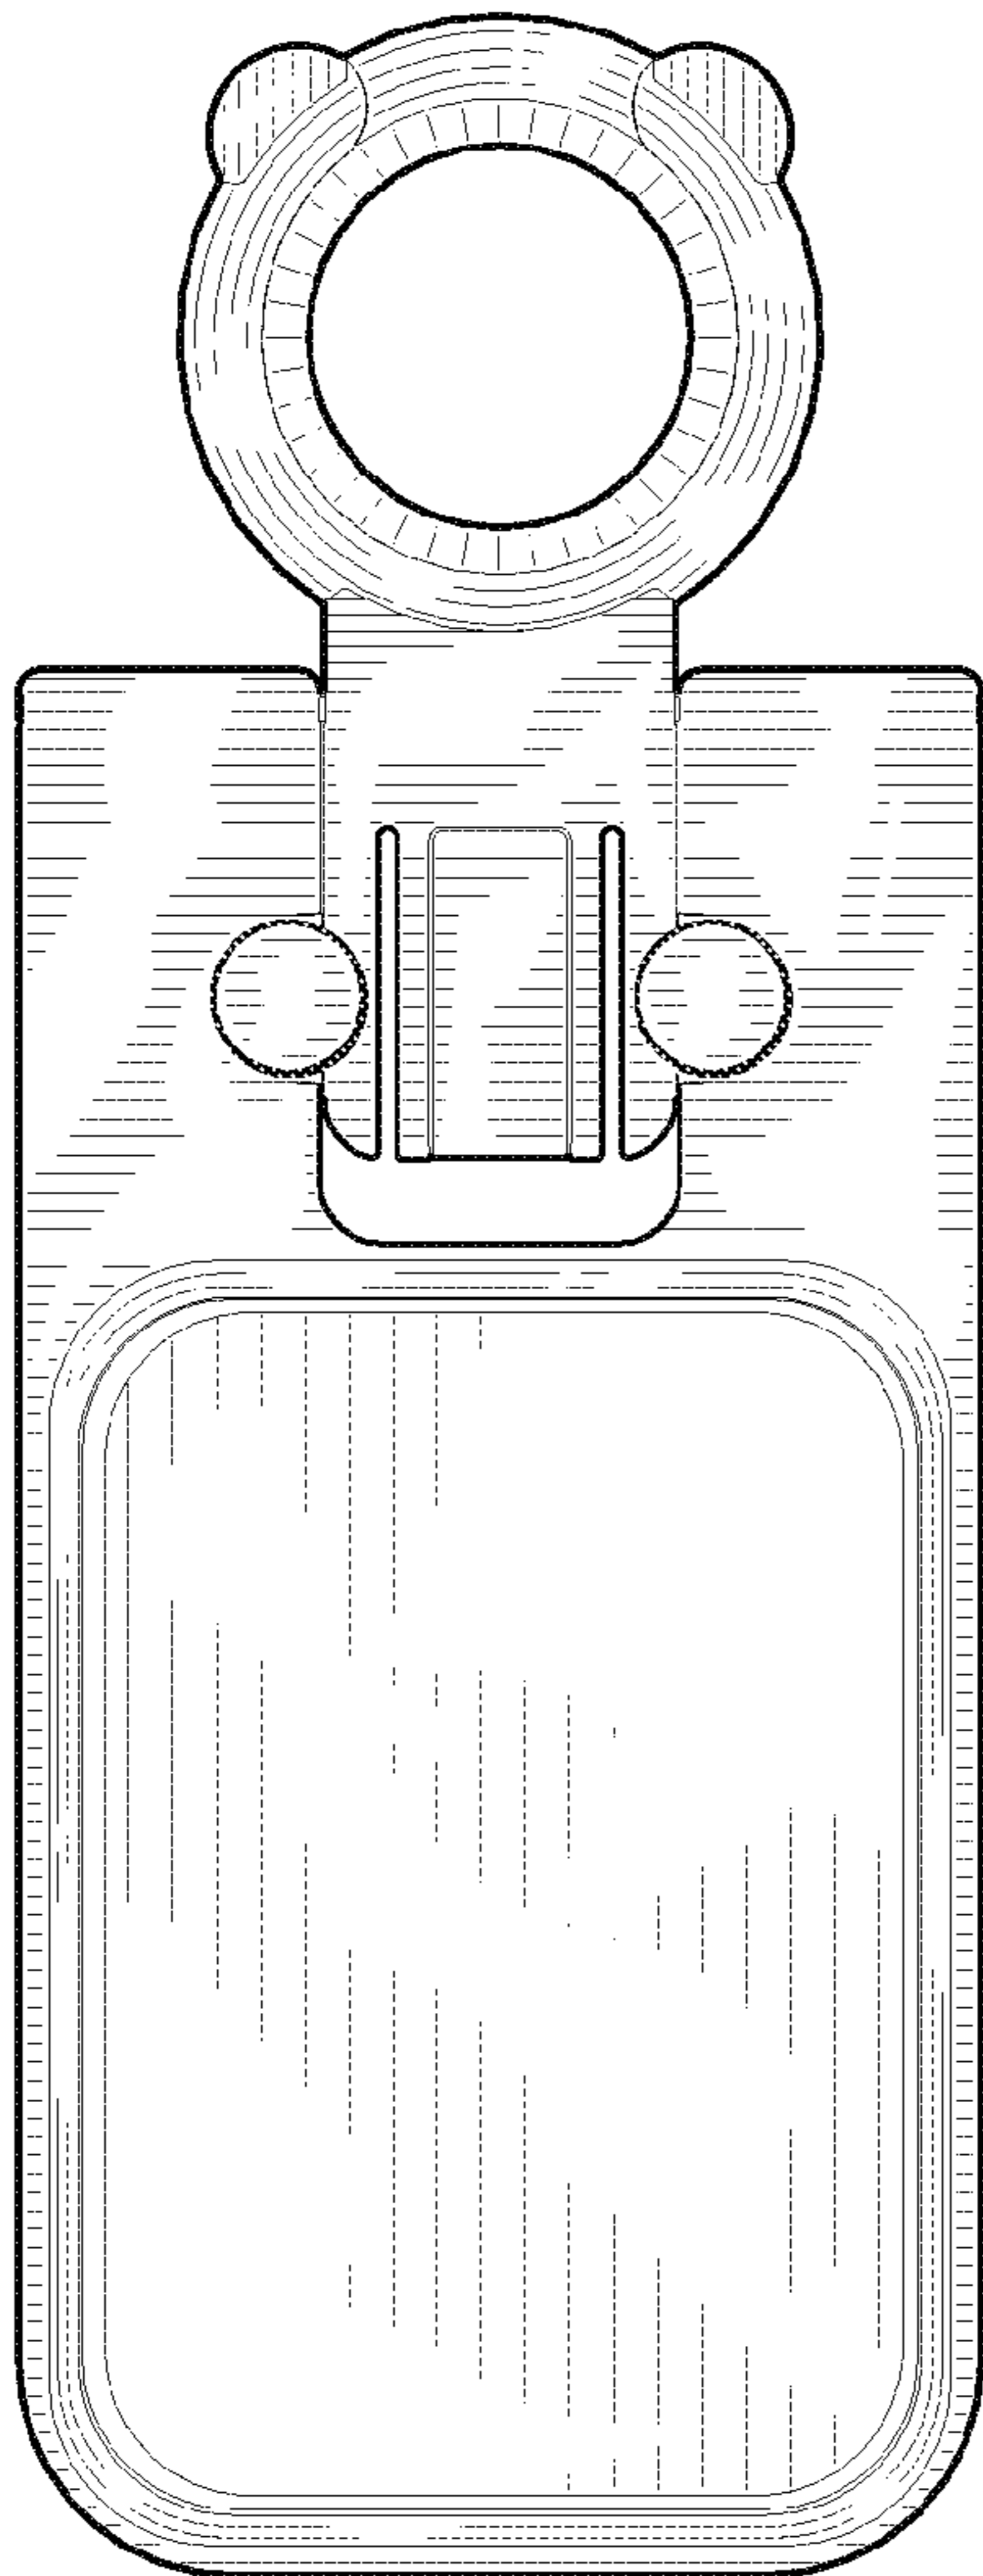


FIG. 2

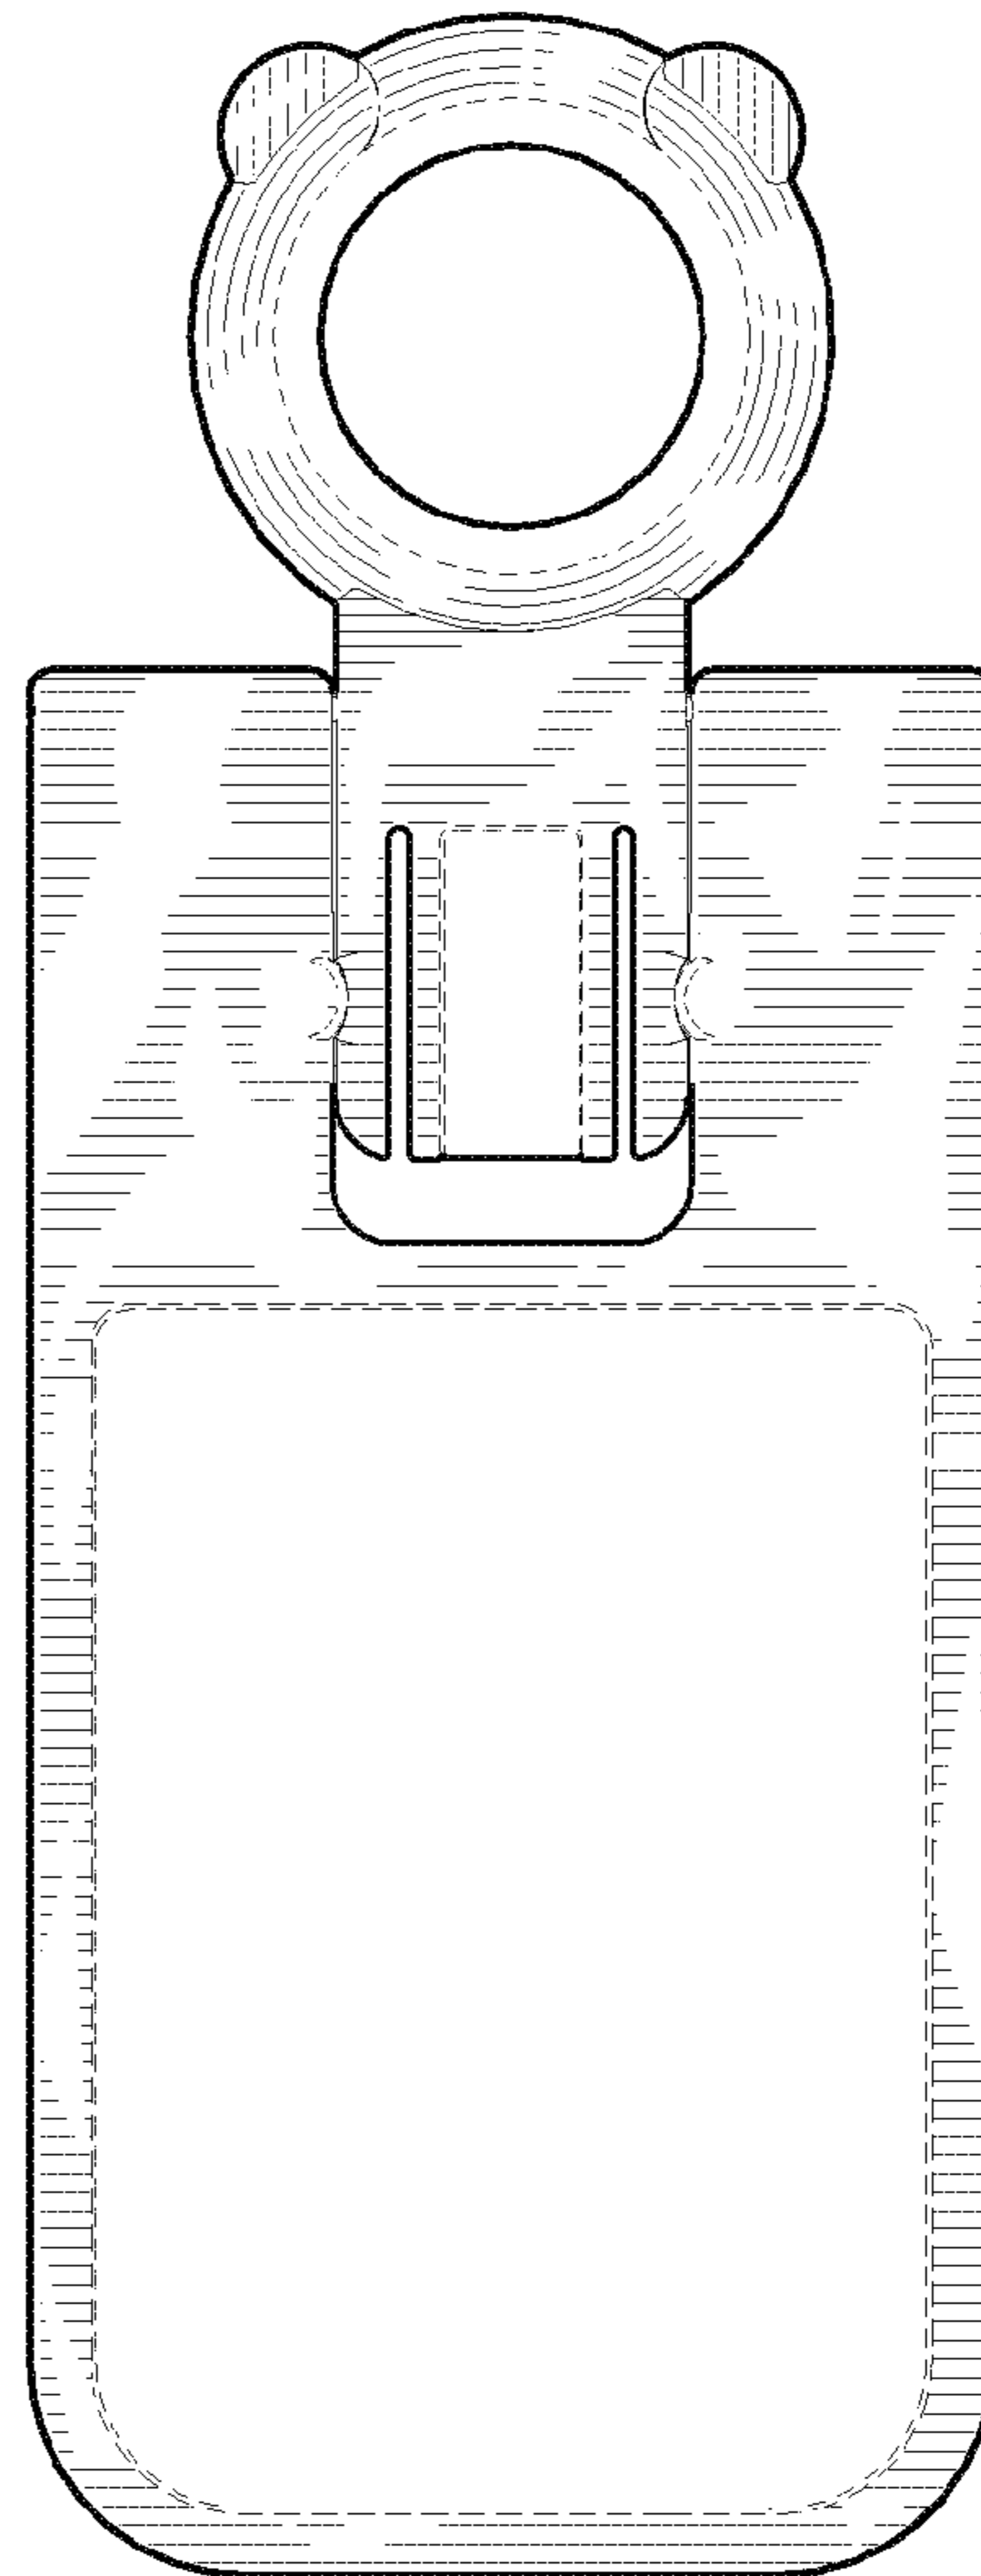


FIG. 3

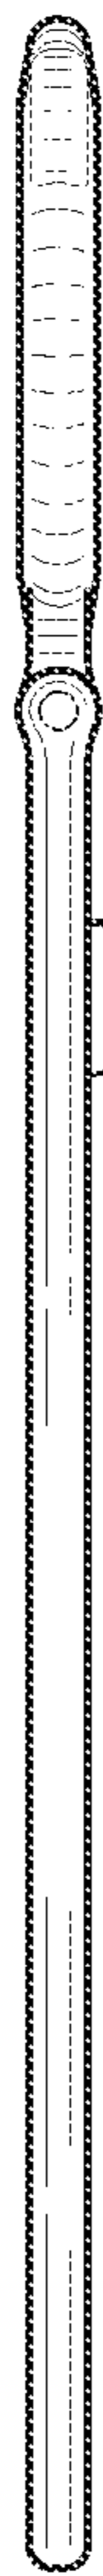


FIG. 4

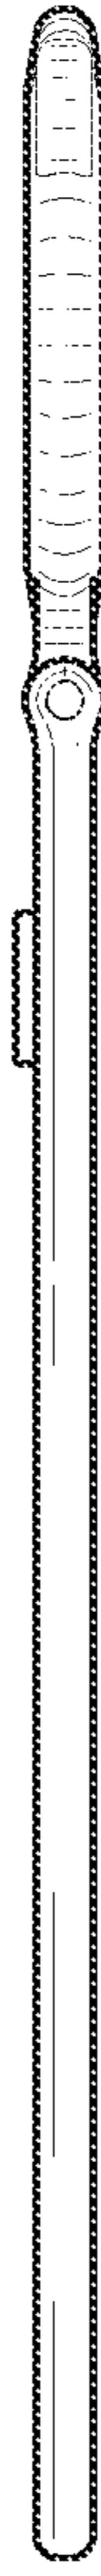


FIG. 5

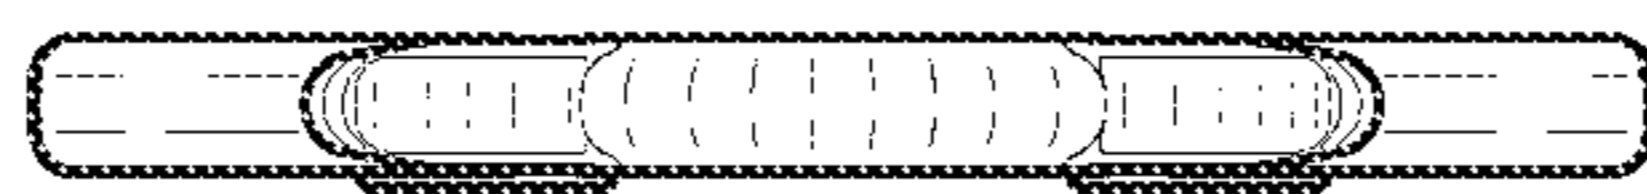


FIG. 6



FIG. 7