



US00D679818S

(12) **United States Design Patent**
Prpa

(10) **Patent No.:** **US D679,818 S**

(45) **Date of Patent:** **** Apr. 9, 2013**

(54) **IMPLANT TRACKING DEVICE**

(76) Inventor: **Branko Prpa**, Kenosha, WI (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/417,289**

(22) Filed: **Apr. 2, 2012**

(51) **LOC (9) Cl.** **24-02**

(52) **U.S. Cl.** **D24/186**

(58) **Field of Classification Search** D24/127,
D24/133, 186-187, 200, 206-207, 214, 231-232;
600/49, 300, 301, 368, 372, 481, 529, 544,
600/554, 561; 607/4, 5, 9, 30, 48, 60; 128/846,
128/888, 899, 903-904; D10/46-47, 70,
D10/104.1, 57; 206/16

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D245,513	S	*	8/1977	Kopel	D10/57
5,155,624	A		10/1992	Flagler		
5,288,986	A		2/1994	Pine et al.		
D346,977	S		5/1994	Fiske		
D356,044	S		3/1995	Clements		
5,423,334	A		6/1995	Jordan		
5,554,841	A		9/1996	Kost et al.		
D374,829	S		10/1996	Yue		
5,631,456	A		5/1997	Kost et al.		
5,653,938	A		8/1997	Faries et al.		
D403,421	S	*	12/1998	Cody et al.	D24/186
5,879,621	A		3/1999	Faries, Jr. et al.		
D410,399	S		6/1999	De Torfino		
D418,226	S	*	12/1999	Cody et al.	D24/187
6,026,328	A		2/2000	Peckham et al.		
6,026,331	A		2/2000	Feldberg et al.		
6,032,195	A		2/2000	Reber et al.		
D459,245	S		6/2002	Power		
D459,246	S		6/2002	Power et al.		
D497,559	S		10/2004	Johnson		
D512,656	S		12/2005	Yeung		
D513,706	S		1/2006	Johnson		
D583,261	S		12/2008	Johnson et al.		
D596,299	S		7/2009	Han et al.		

7,611,010	B2		11/2009	Gammons		
D614,980	S		5/2010	Junes		
D614,981	S		5/2010	Junes		
D616,991	S		6/2010	Kitayama		
7,813,809	B2		10/2010	Strother et al.		
D629,525	S	*	12/2010	Ladwig et al.	D24/187
D630,756	S		1/2011	Kitayama		
D642,690	S		8/2011	Altmann et al.		
D658,298	S	*	4/2012	Prpa	D24/186

(Continued)

FOREIGN PATENT DOCUMENTS

WO 2011033540 3/2011

OTHER PUBLICATIONS

Application Brief, Symbol DS6707-DP: Improve patient safety and workforce productivity through real-time accurate inventory counts in the operating room and beyond; motorola.com; Jan. 1, 2008.

(Continued)

Primary Examiner — T. Chase Nelson

Assistant Examiner — Mark Cavanna

(74) *Attorney, Agent, or Firm* — Whyte Hirschboeck Dudek S.C.; James A. Joyce


(57) **CLAIM**

The ornamental design for an implant tracking device, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of an implant tracking device showing my new design;
FIG. 2 is a front elevation view thereof;
FIG. 3 is a top plan view thereof;
FIG. 4 is a side elevation view thereof;
FIG. 5 is a back elevation view thereof; and,
FIG. 6 is a bottom plan view thereof.
The broken lines are included for the purpose of illustrating portions of the implant tracking device that form no part of the claimed design.

1 Claim, 3 Drawing Sheets

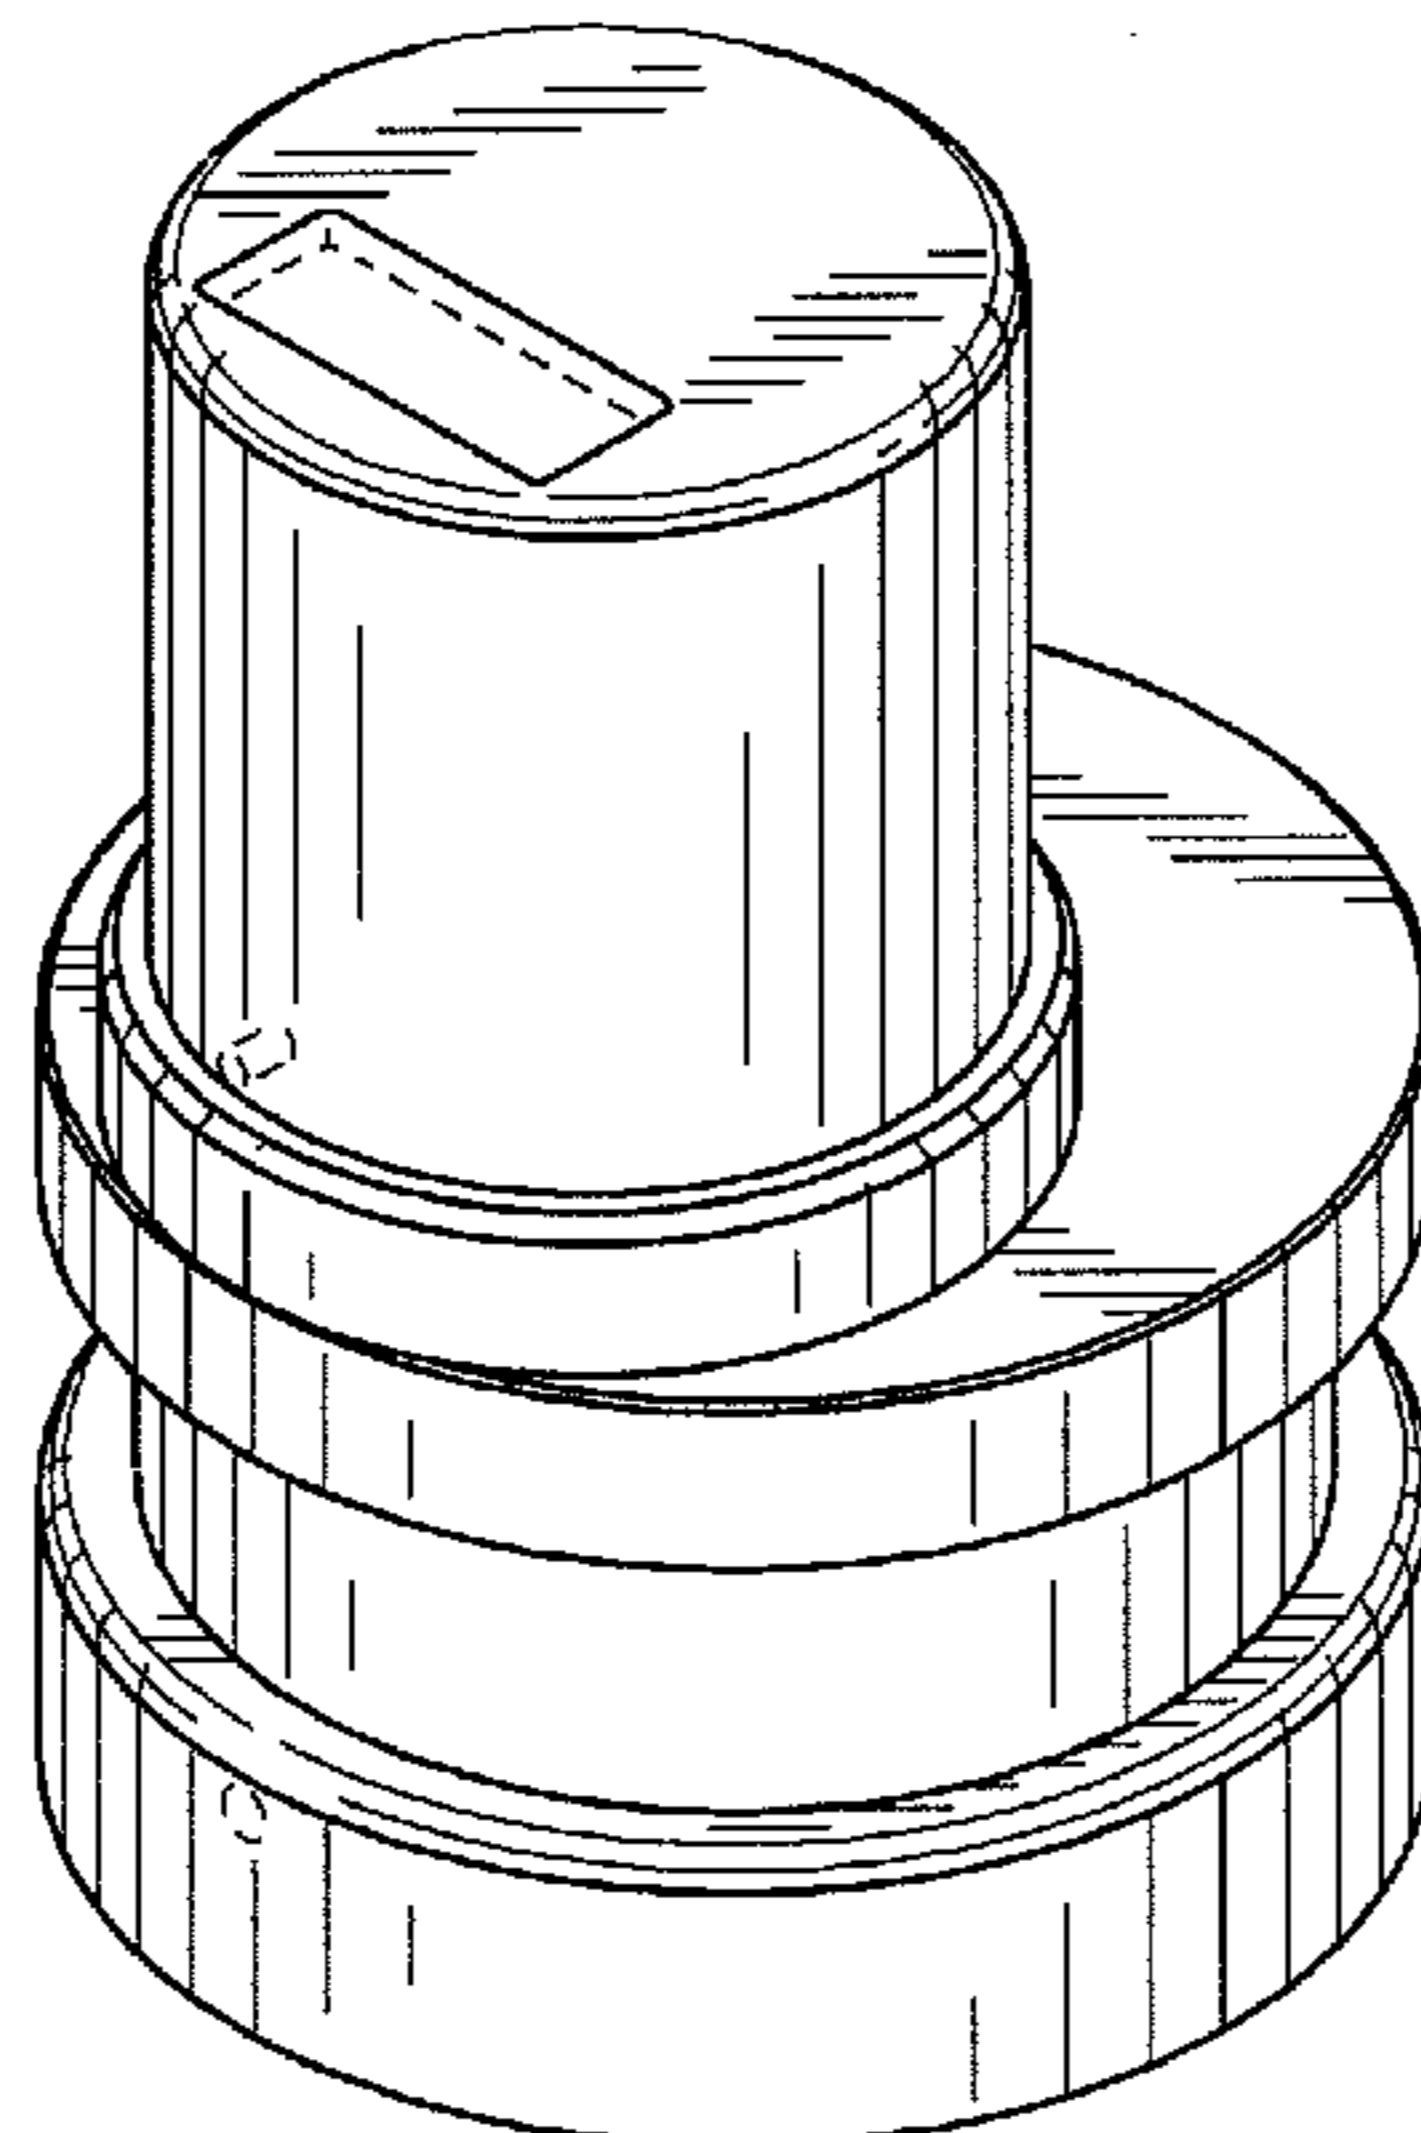

US D679,818 S

Page 2

U.S. PATENT DOCUMENTS

2005/0203384 A1 9/2005 Sati et al.
2006/0256400 A1 11/2006 Carnevali
2006/0291533 A1 12/2006 Faries et al.
2008/0015590 A1 1/2008 Sanders et al.
2009/0247999 A1 10/2009 Tuan et al.
2009/0317002 A1 12/2009 Dein
2010/0076306 A1 3/2010 Daigneault et al.
2011/0023343 A1 2/2011 Turner et al.
2011/0060386 A1 3/2011 Woods et al.
2011/0114514 A1 5/2011 Bagozzi et al.

OTHER PUBLICATIONS

Cognex, "Dataman logistics barcode readers", www.cognex.com/dataman500/. Jan. 1, 2012.

International Search Report and Written Opinion for PCT App. No. PCT/US2012/039980 mailed on Aug. 22, 2012.

* cited by examiner

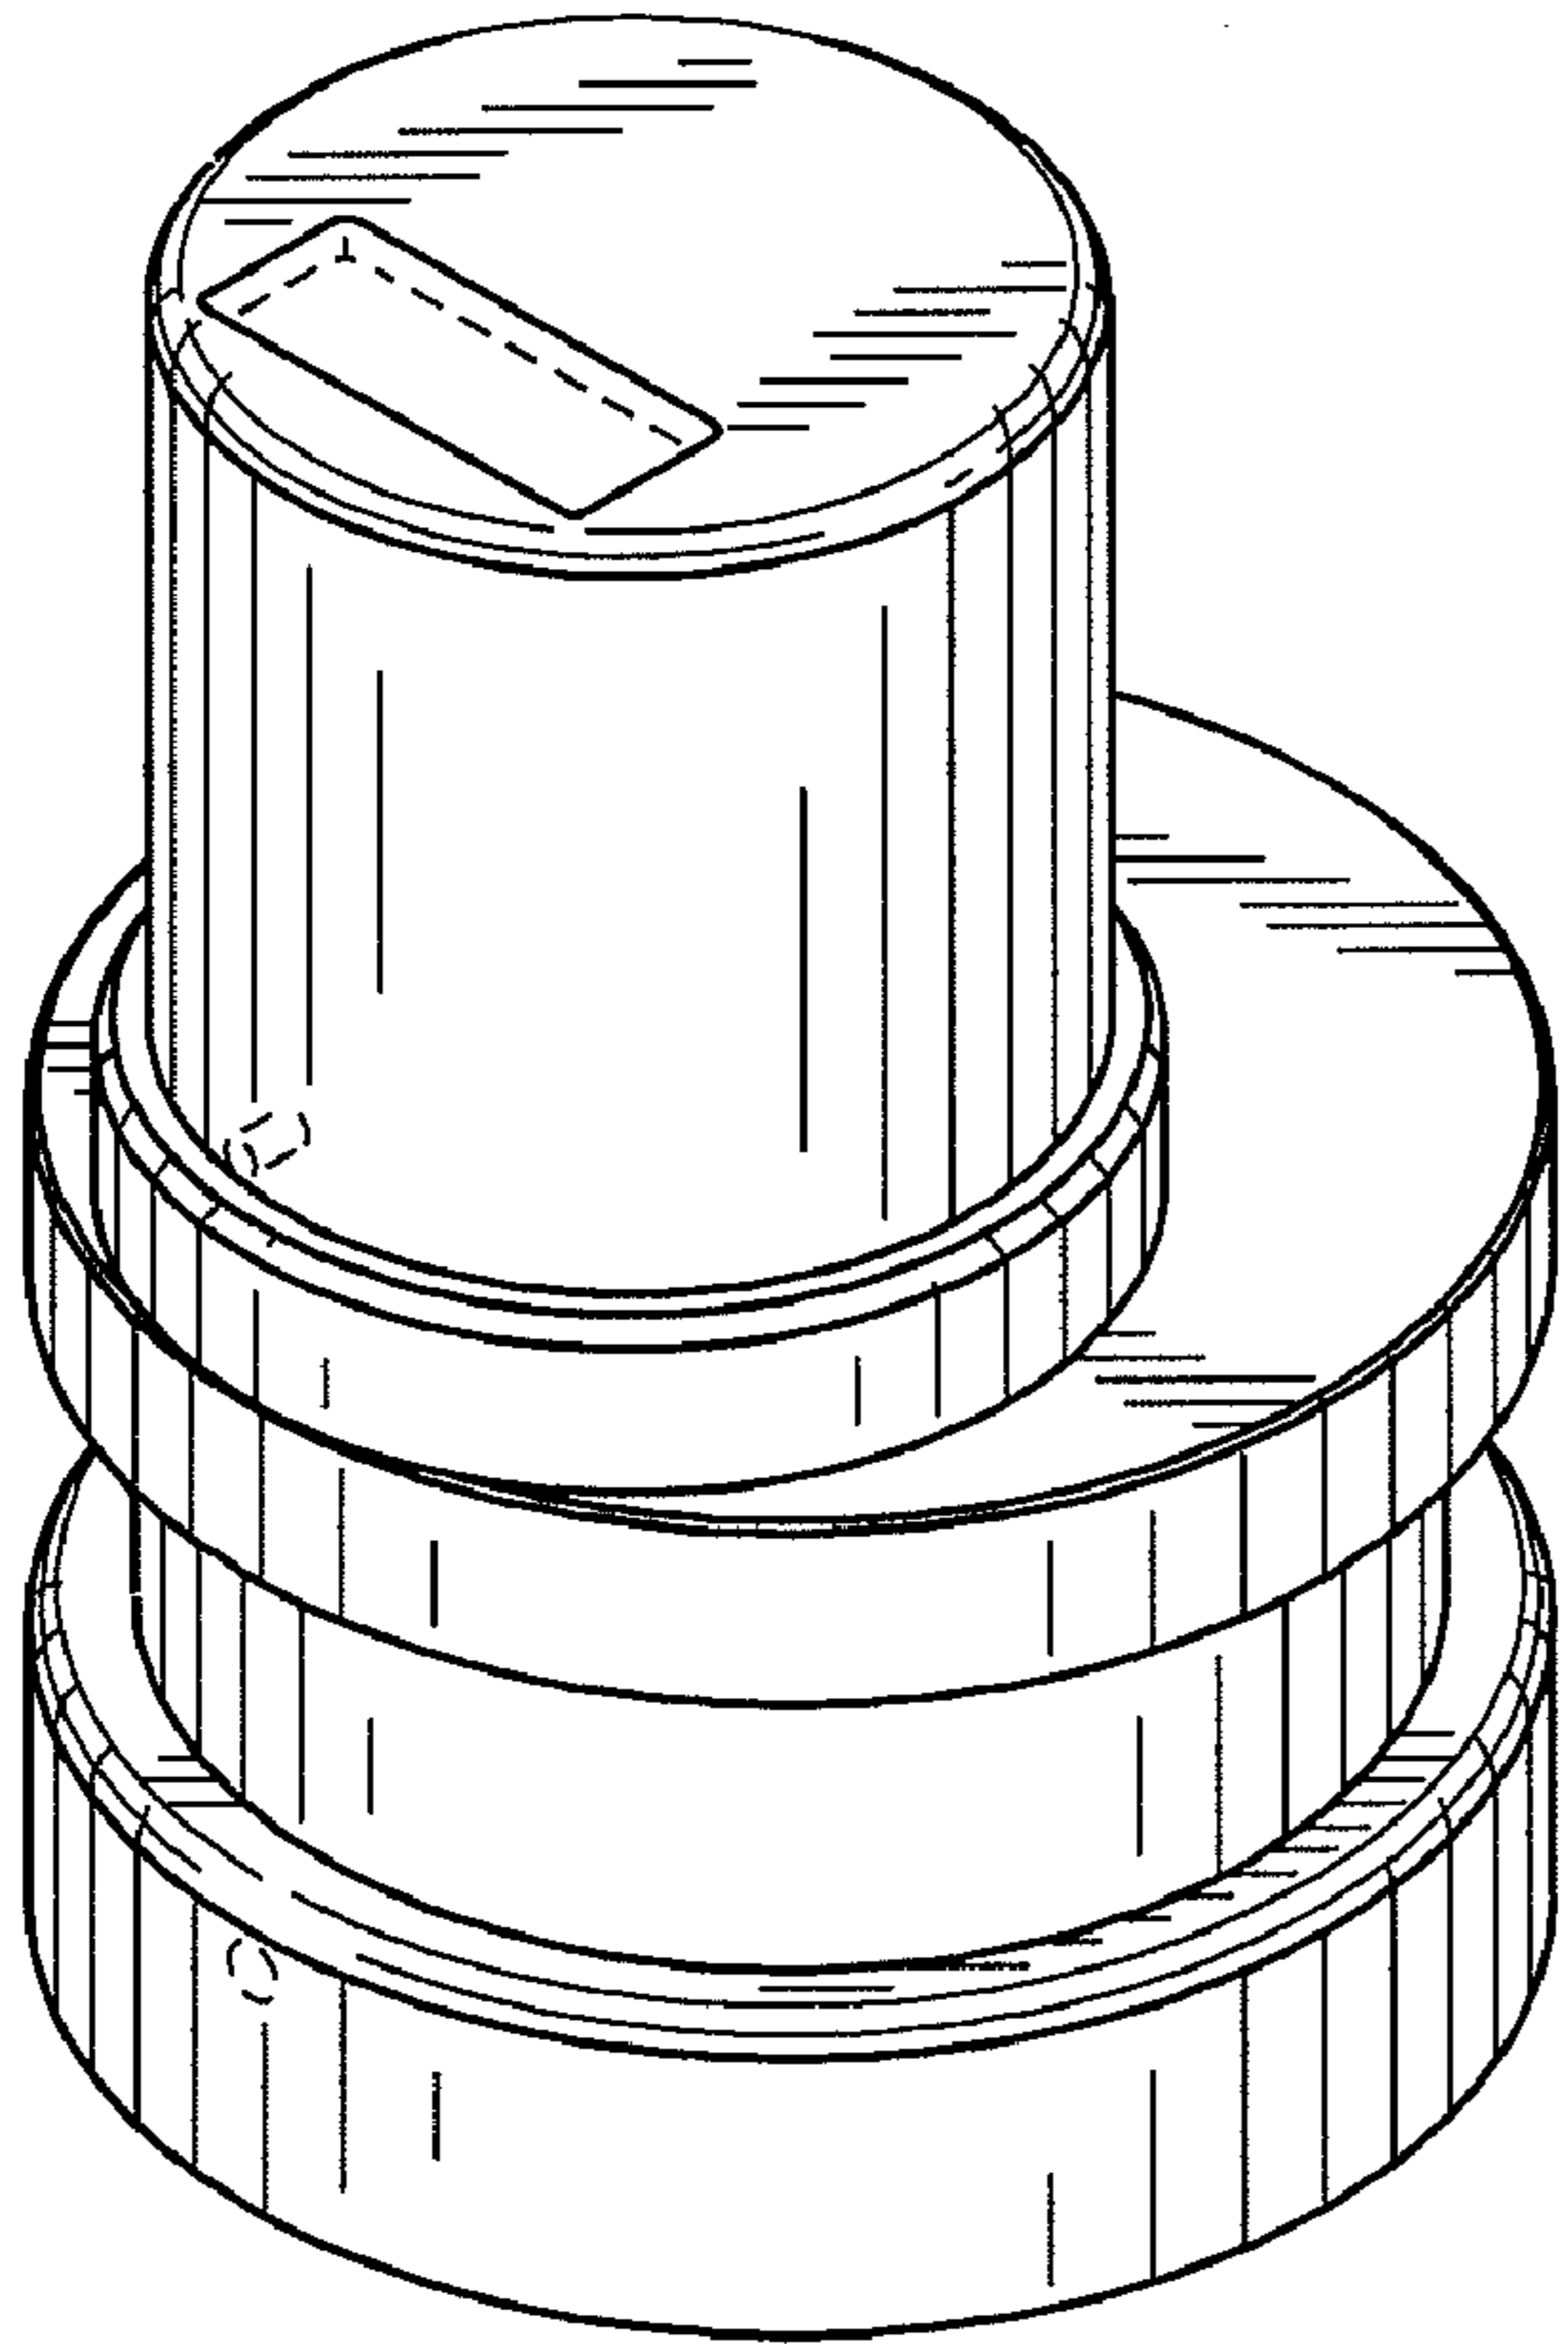


FIG. 1

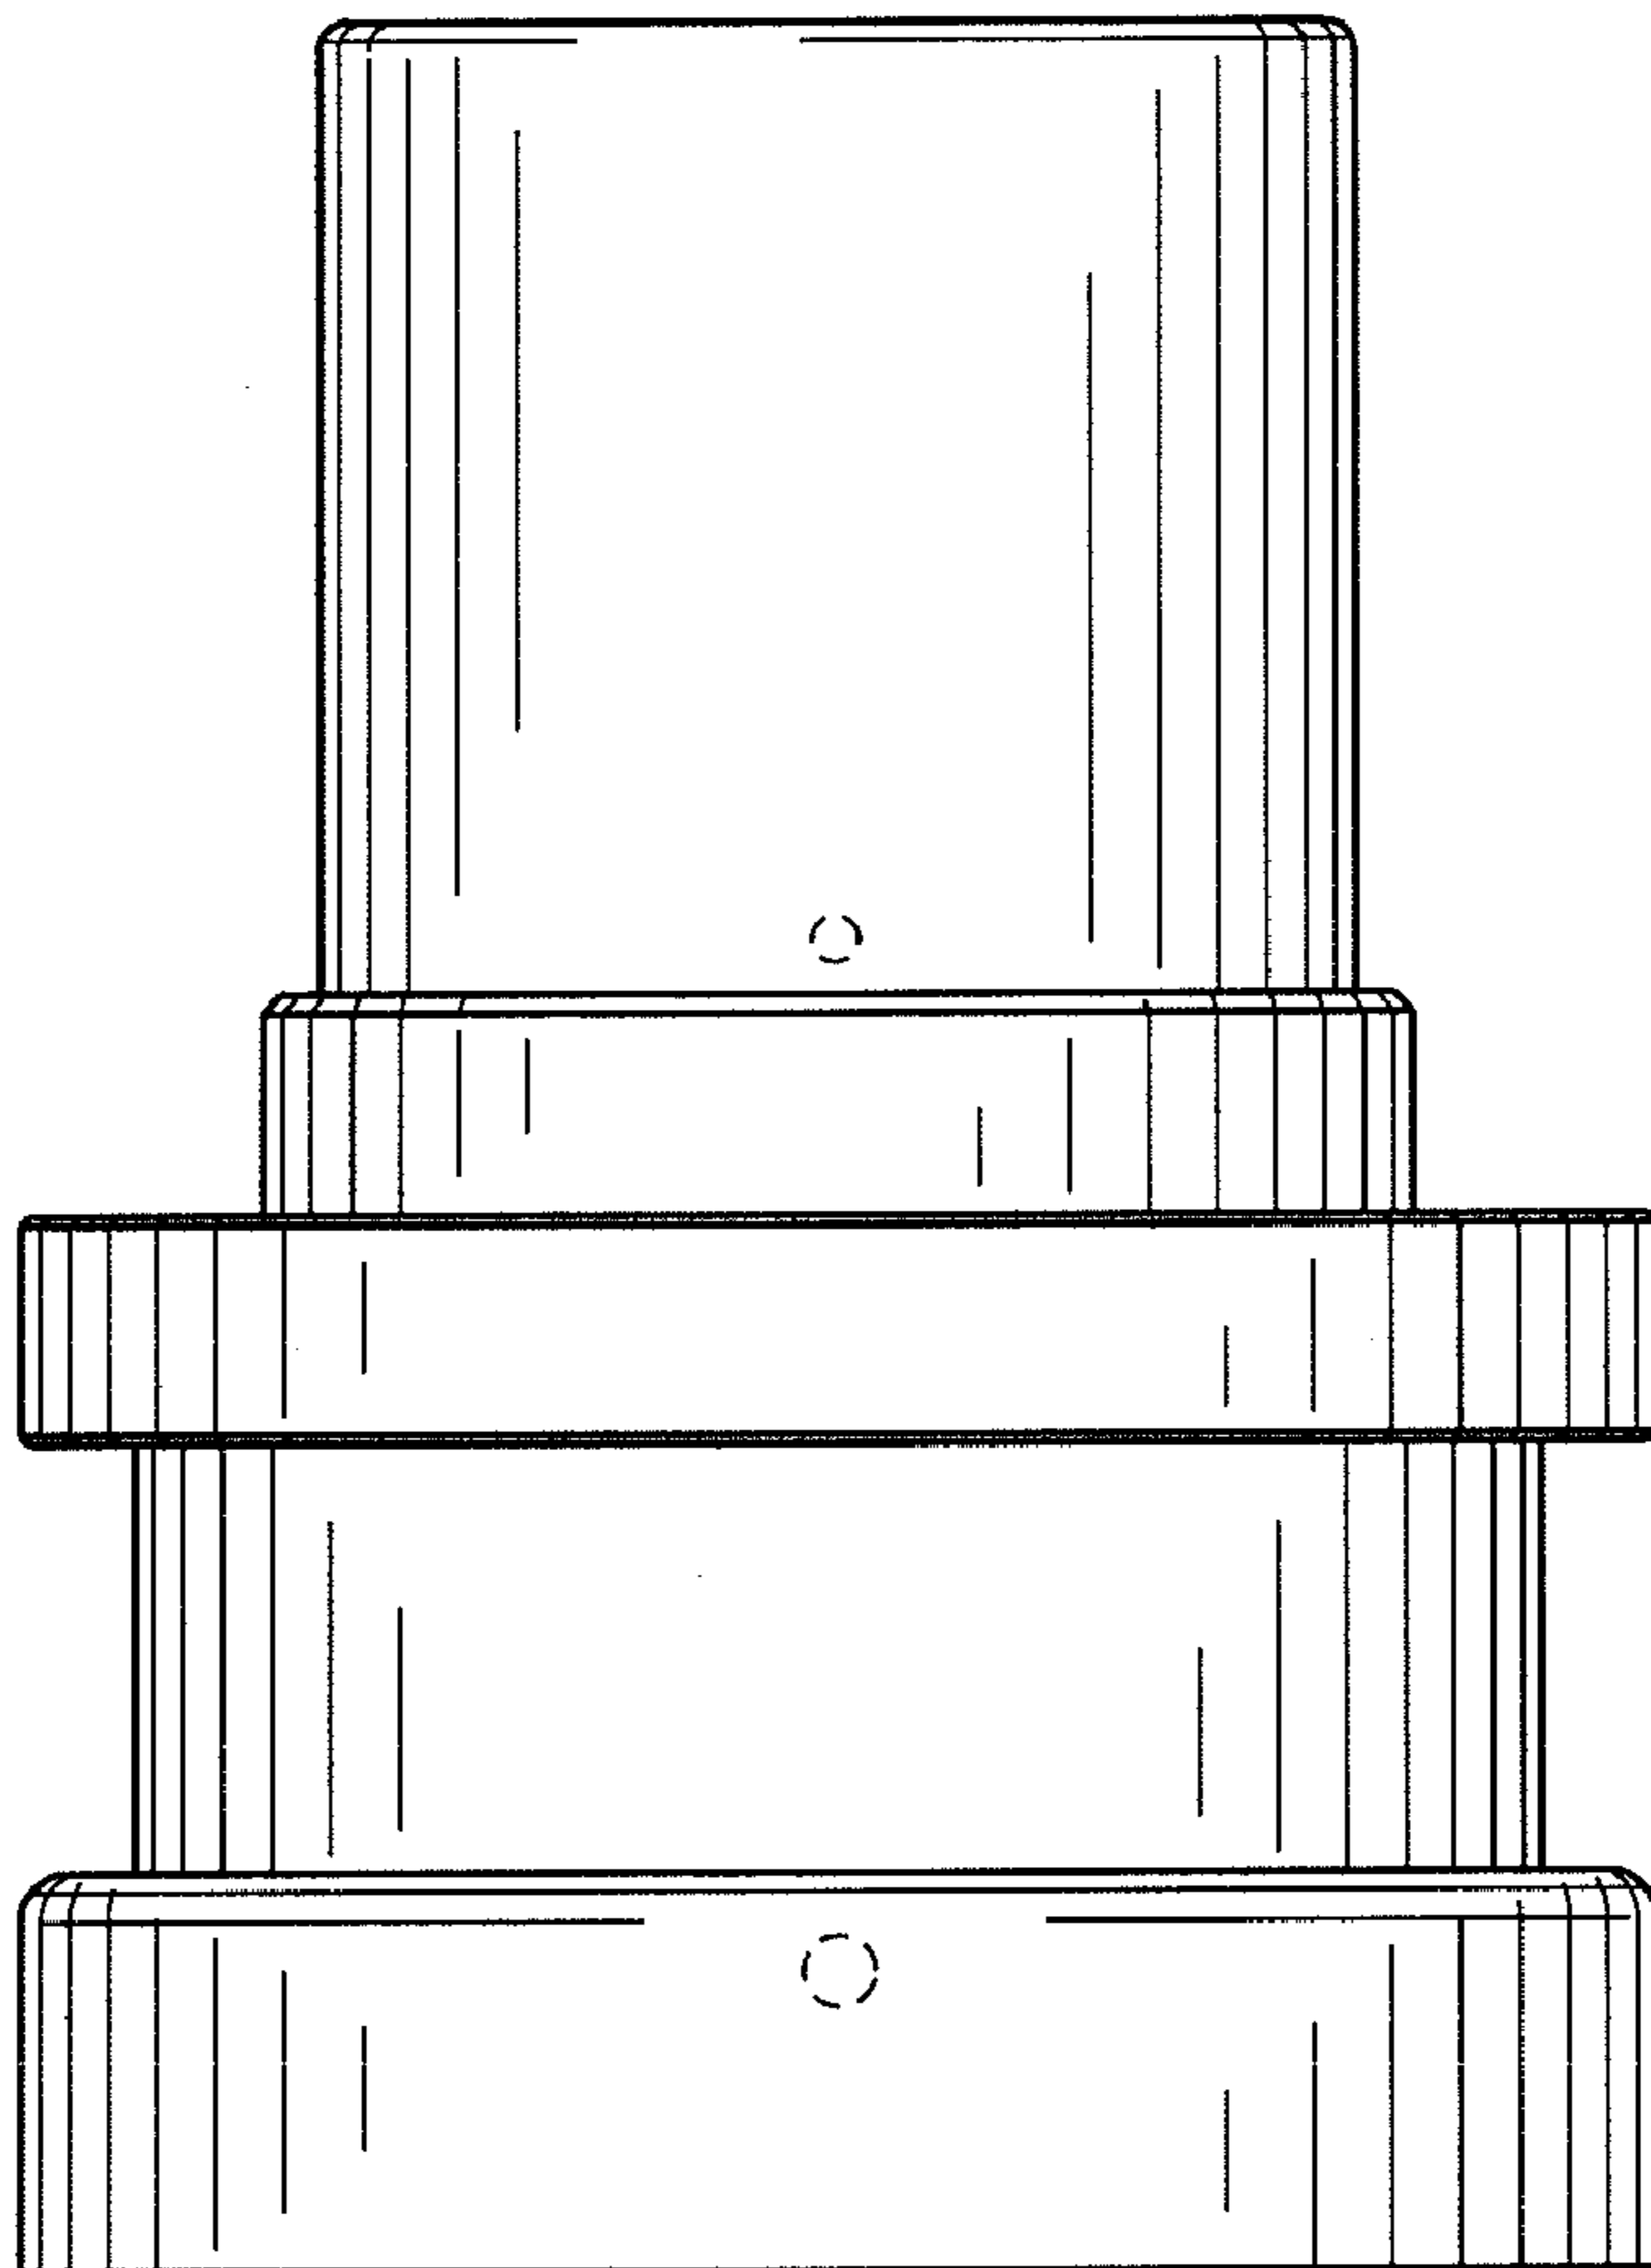


FIG. 2

FIG. 3

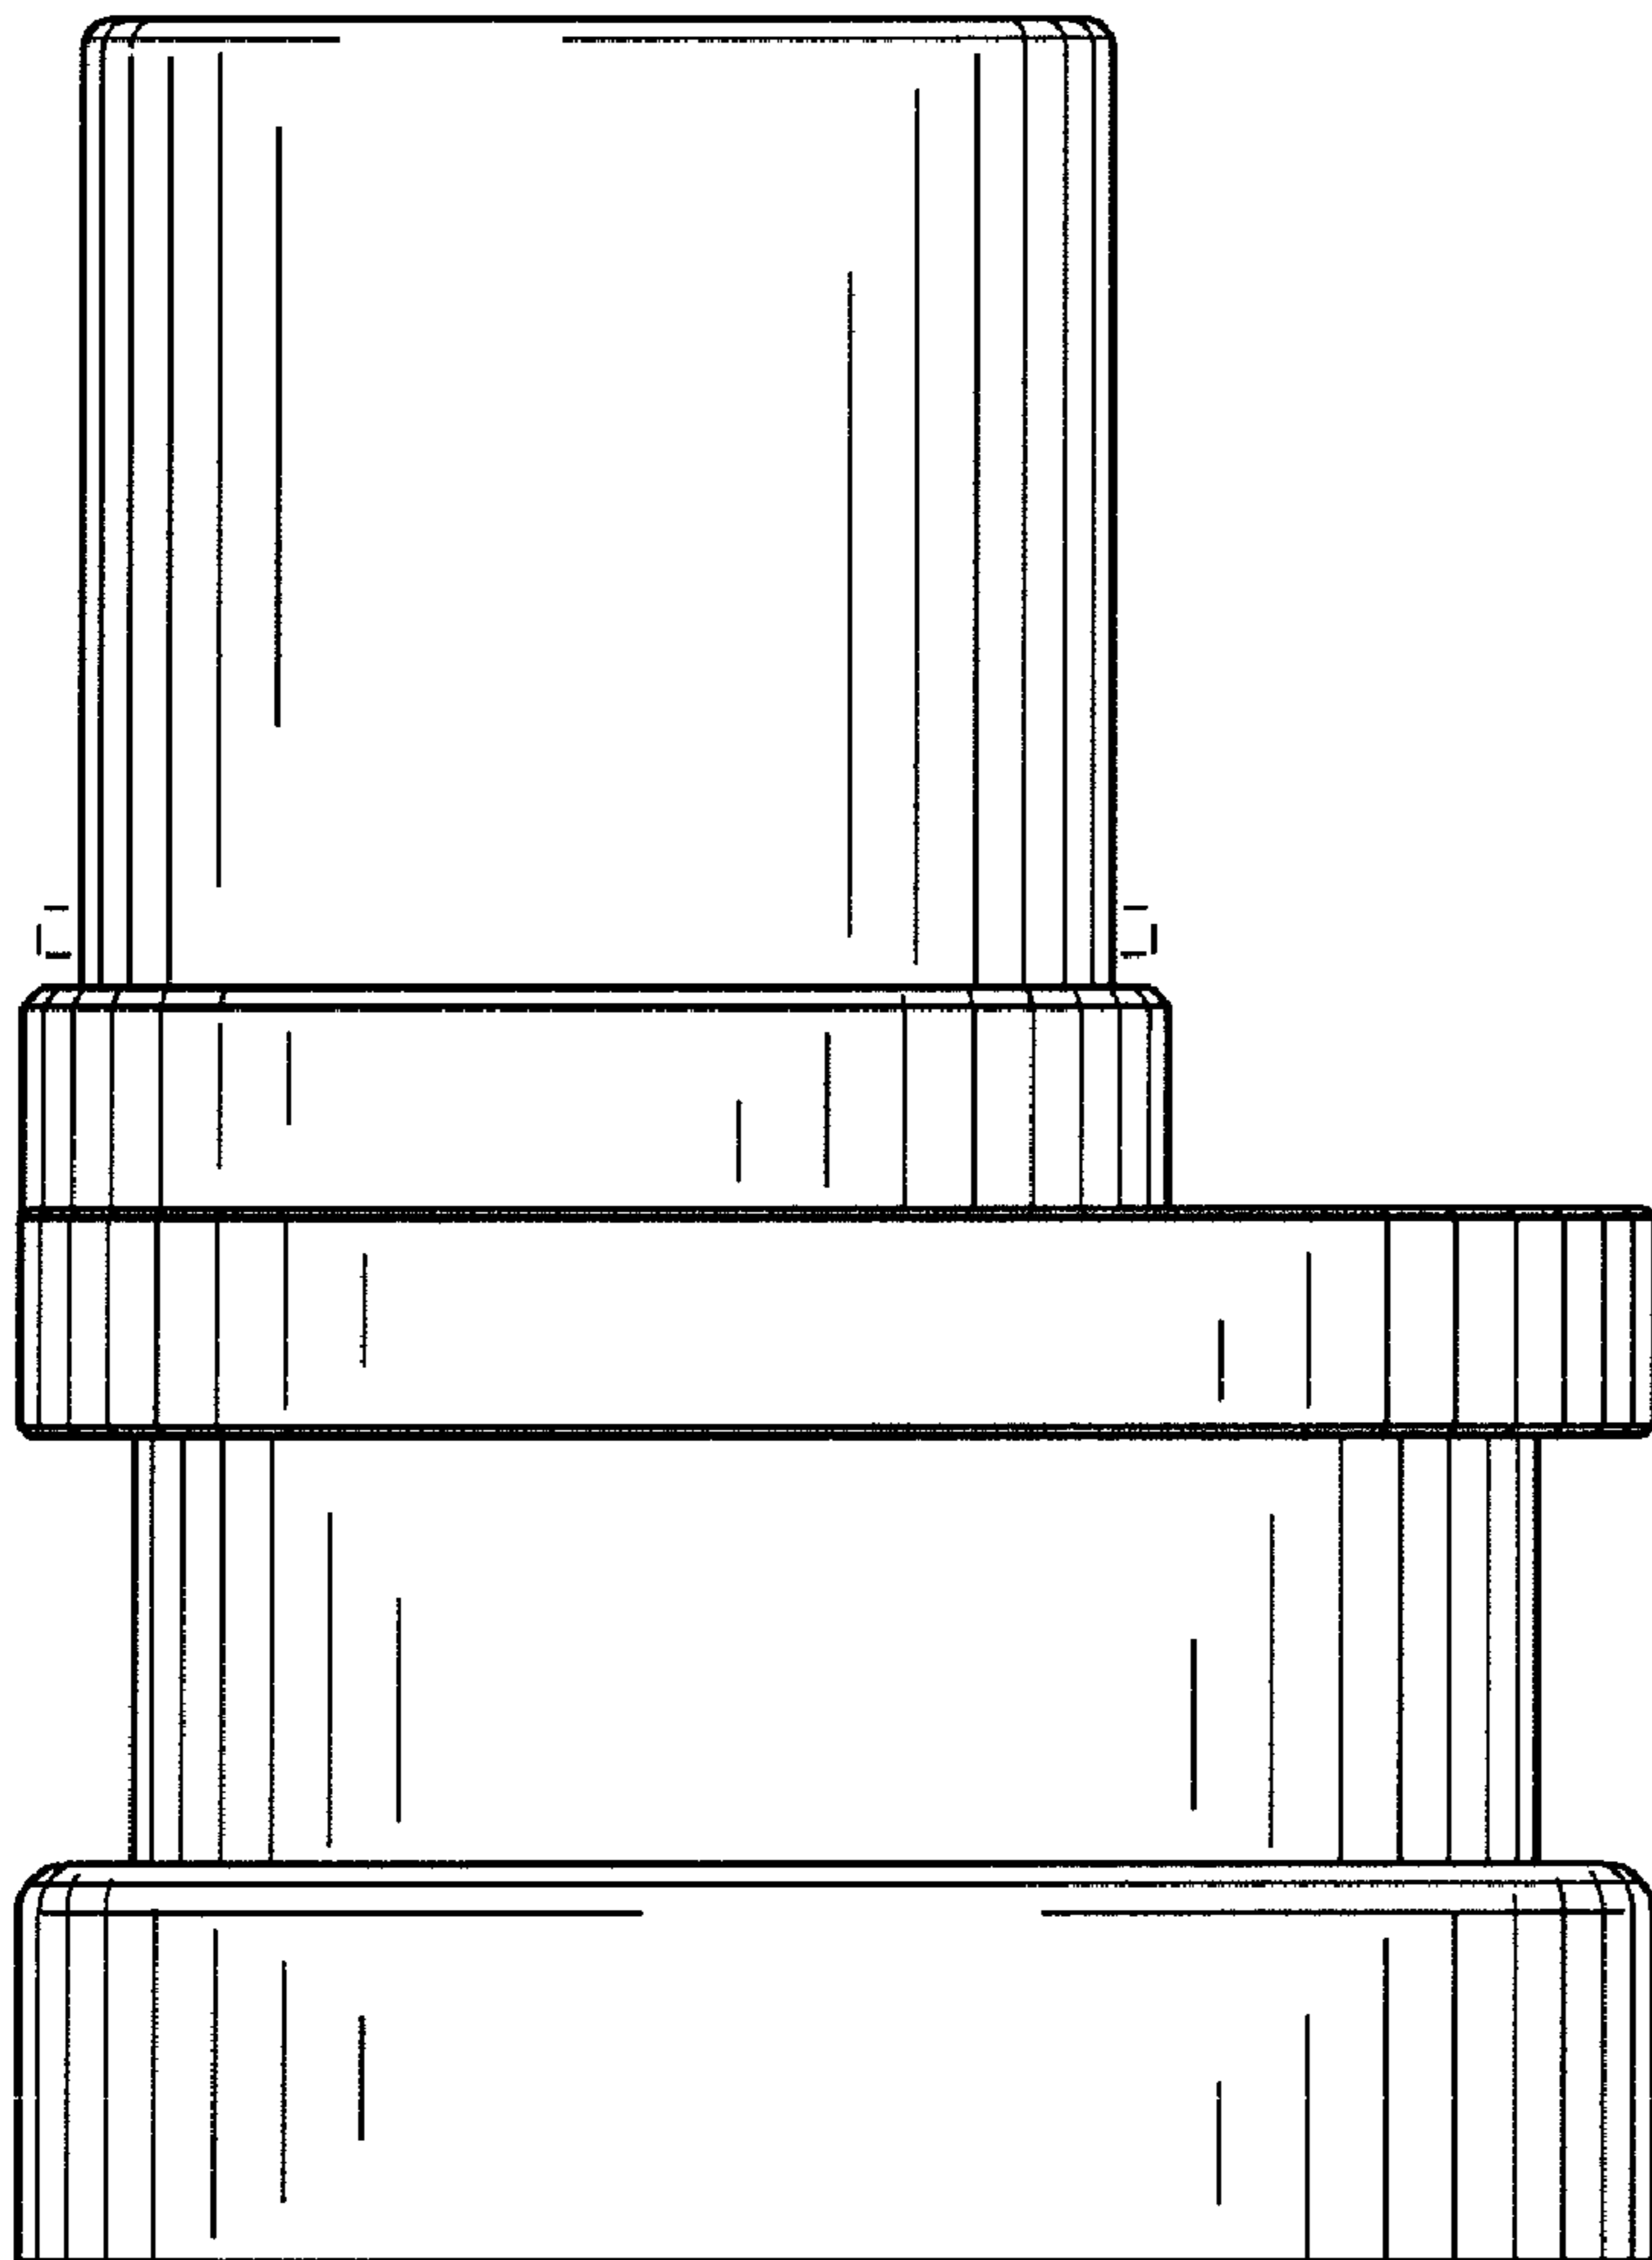
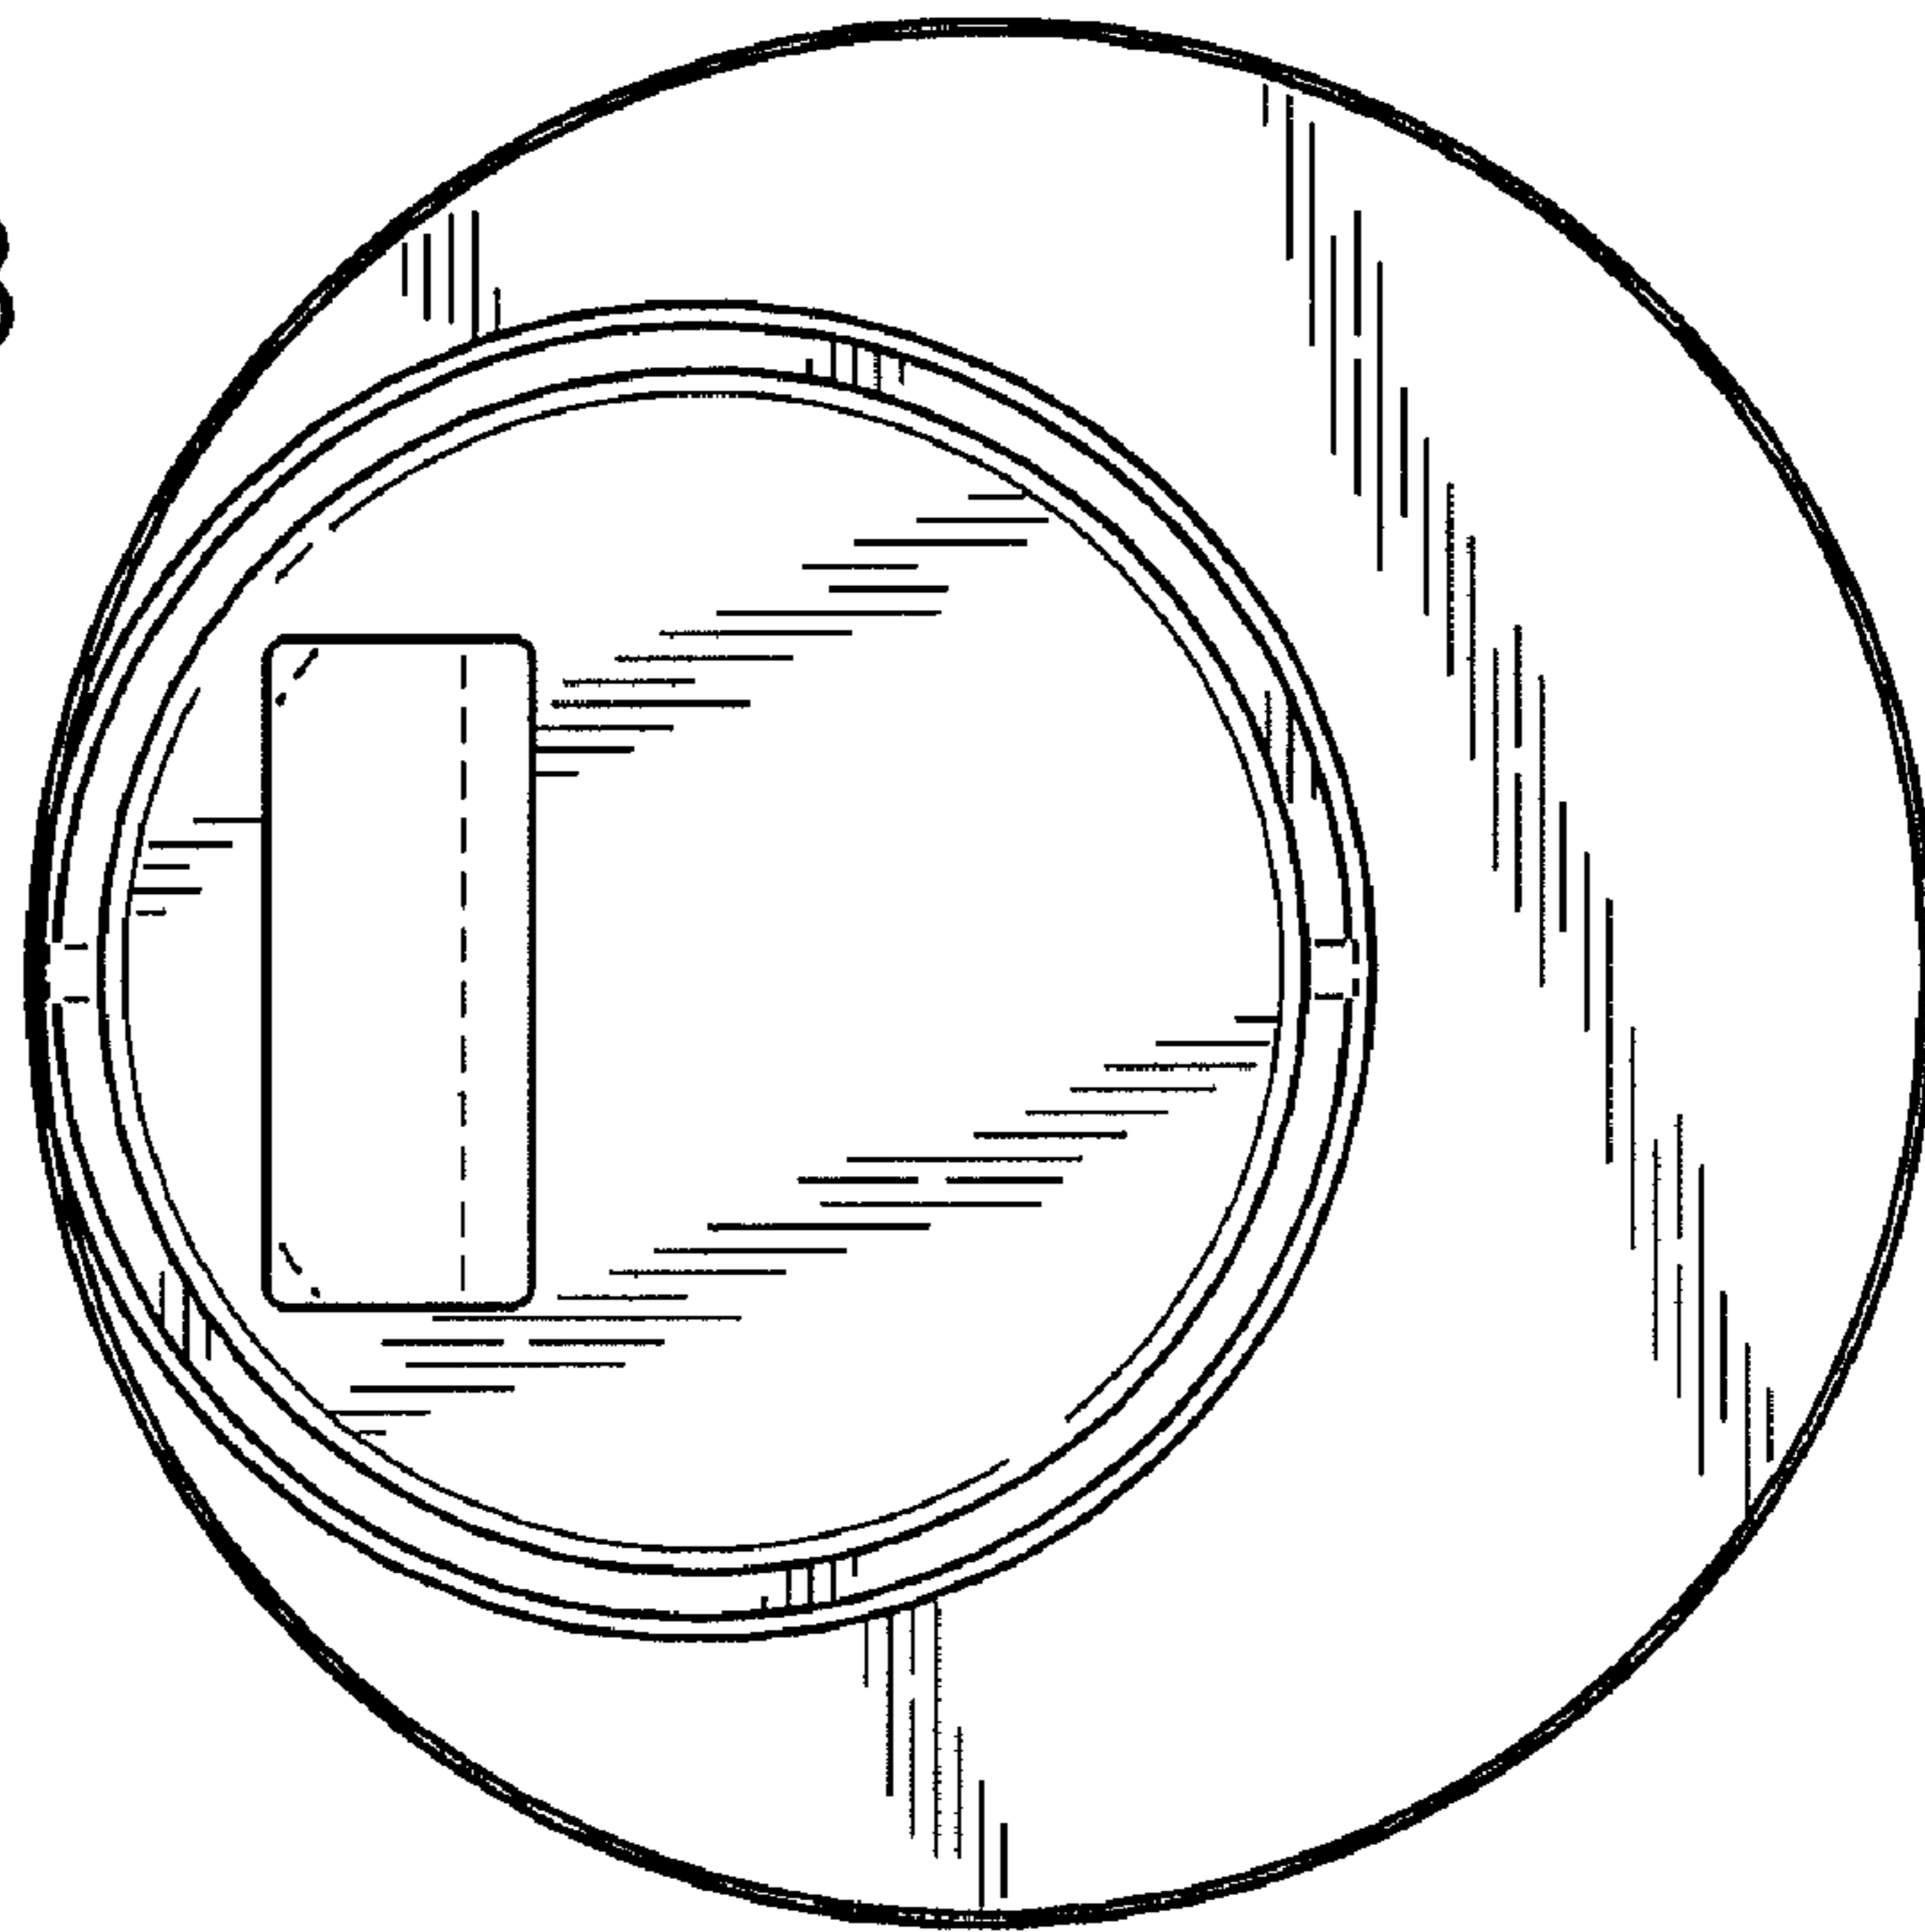


FIG. 4

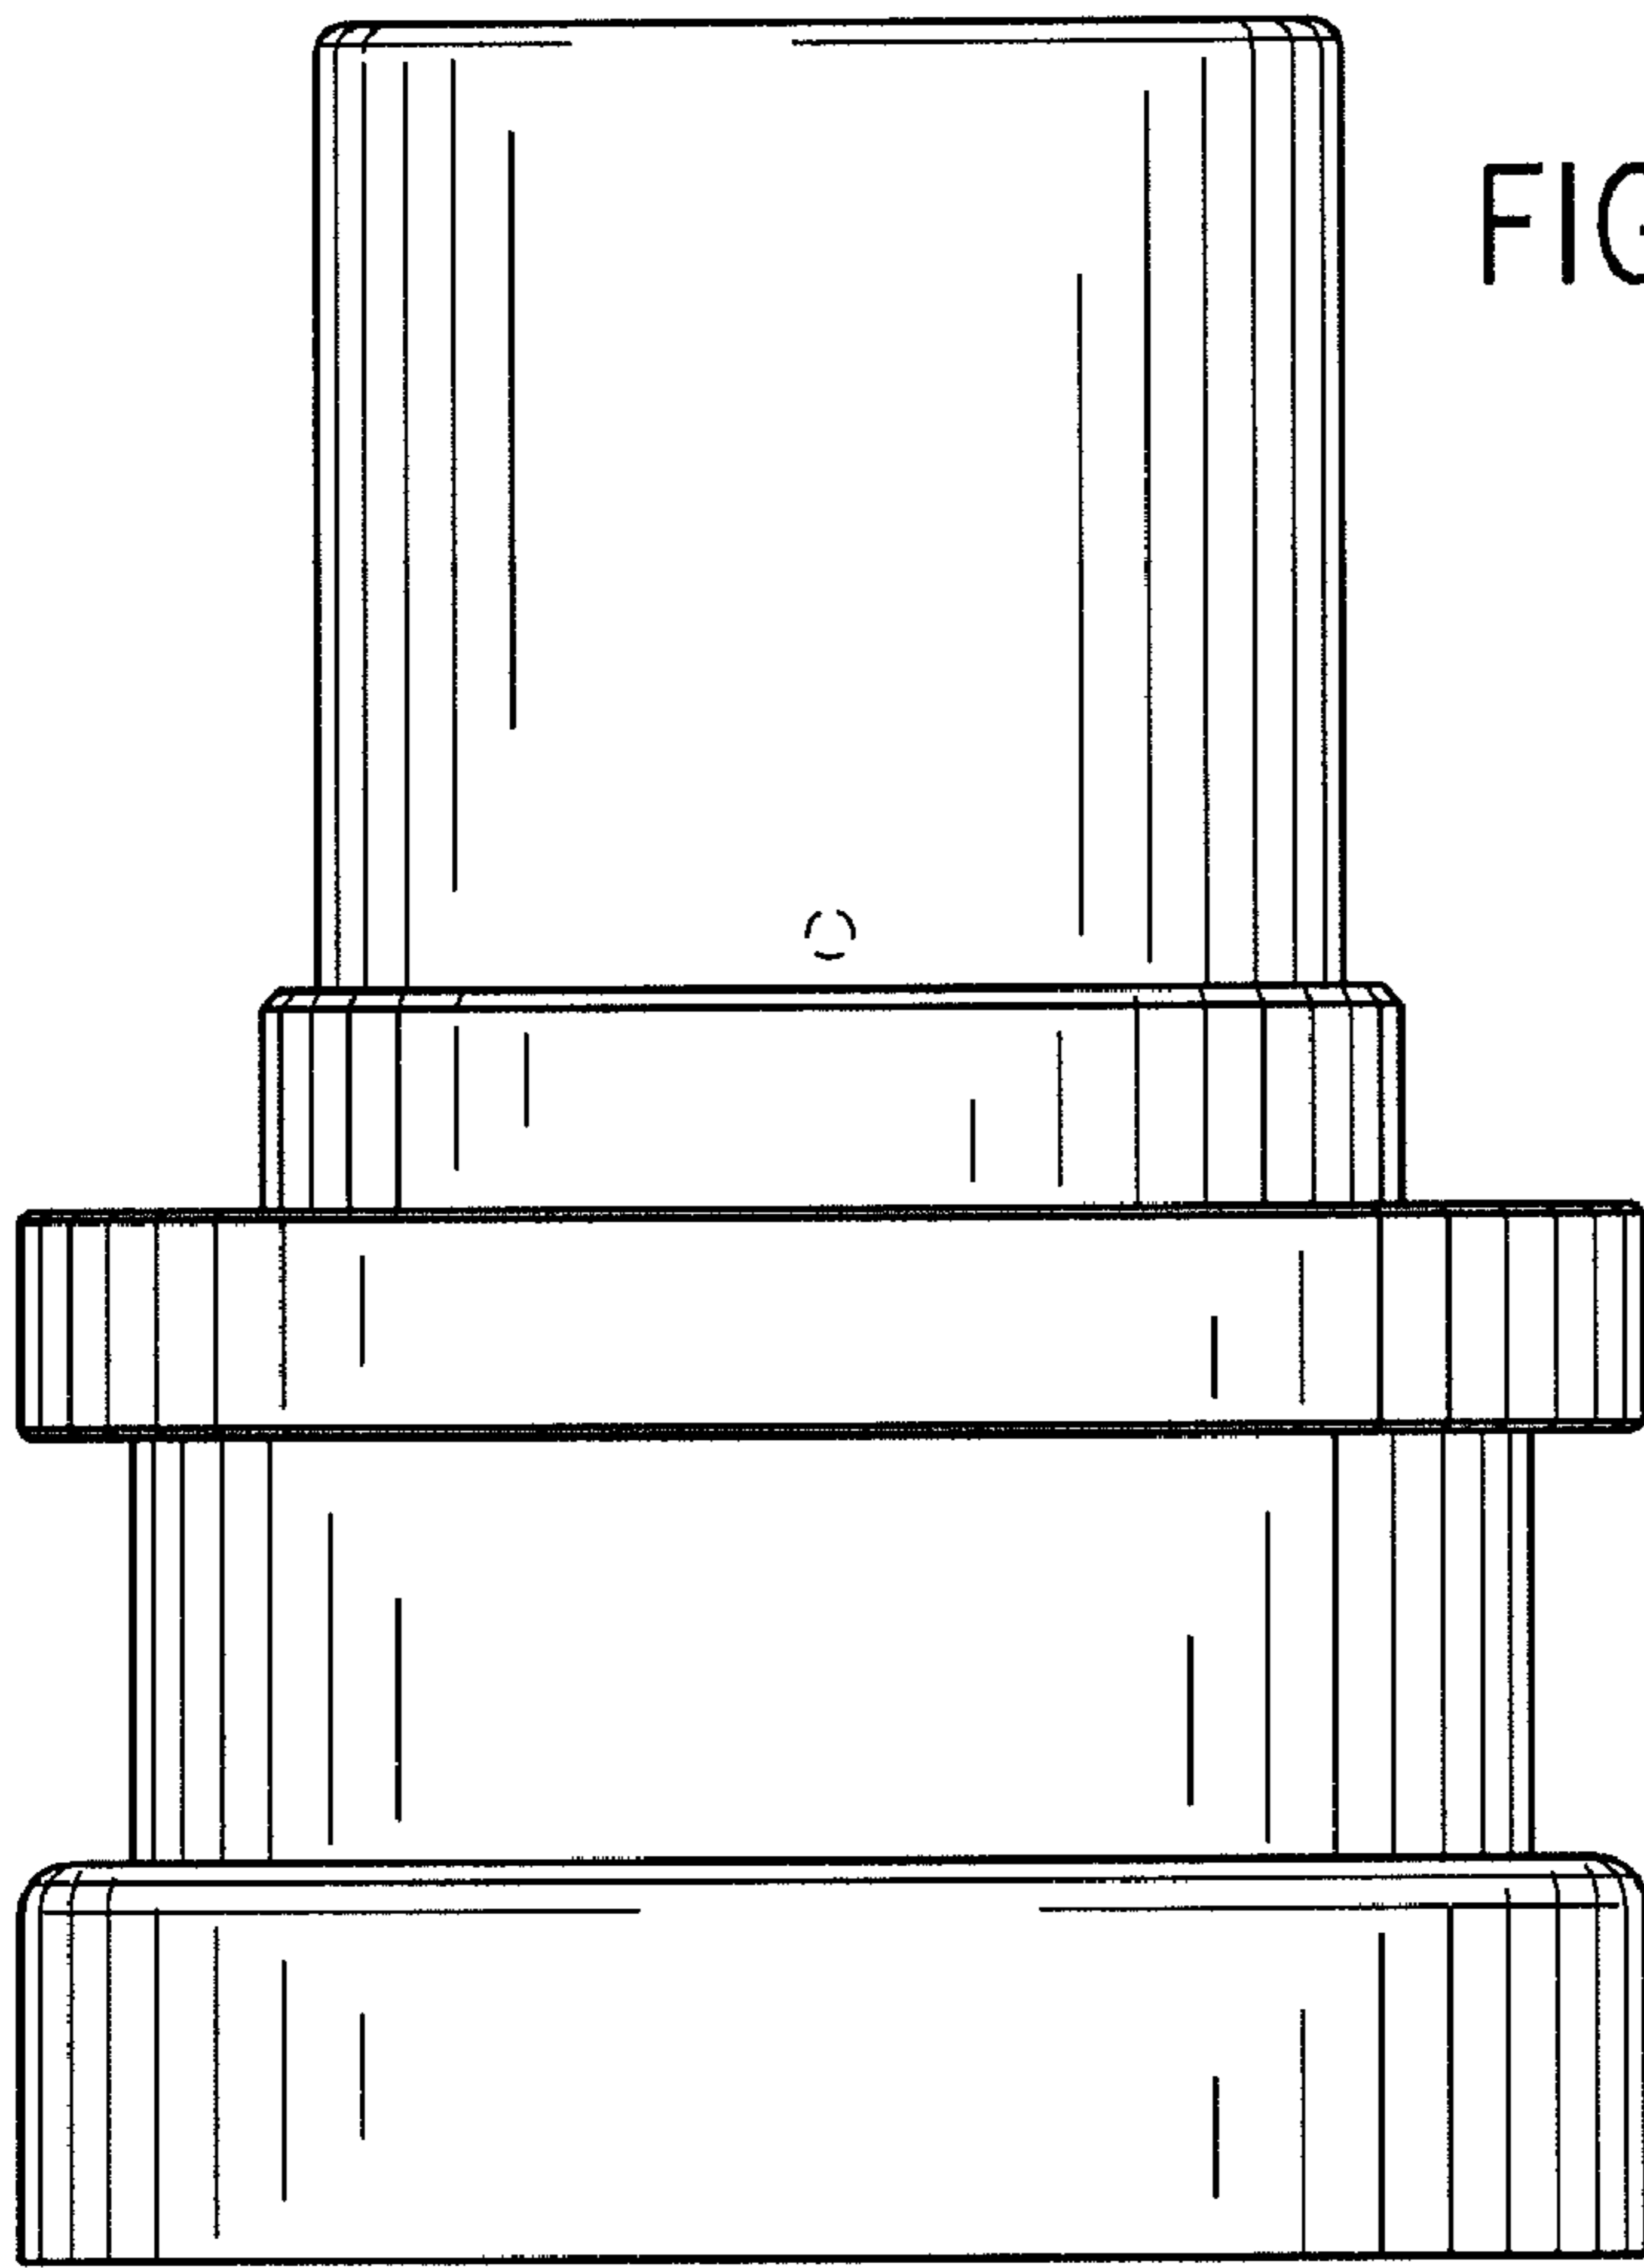


FIG. 5

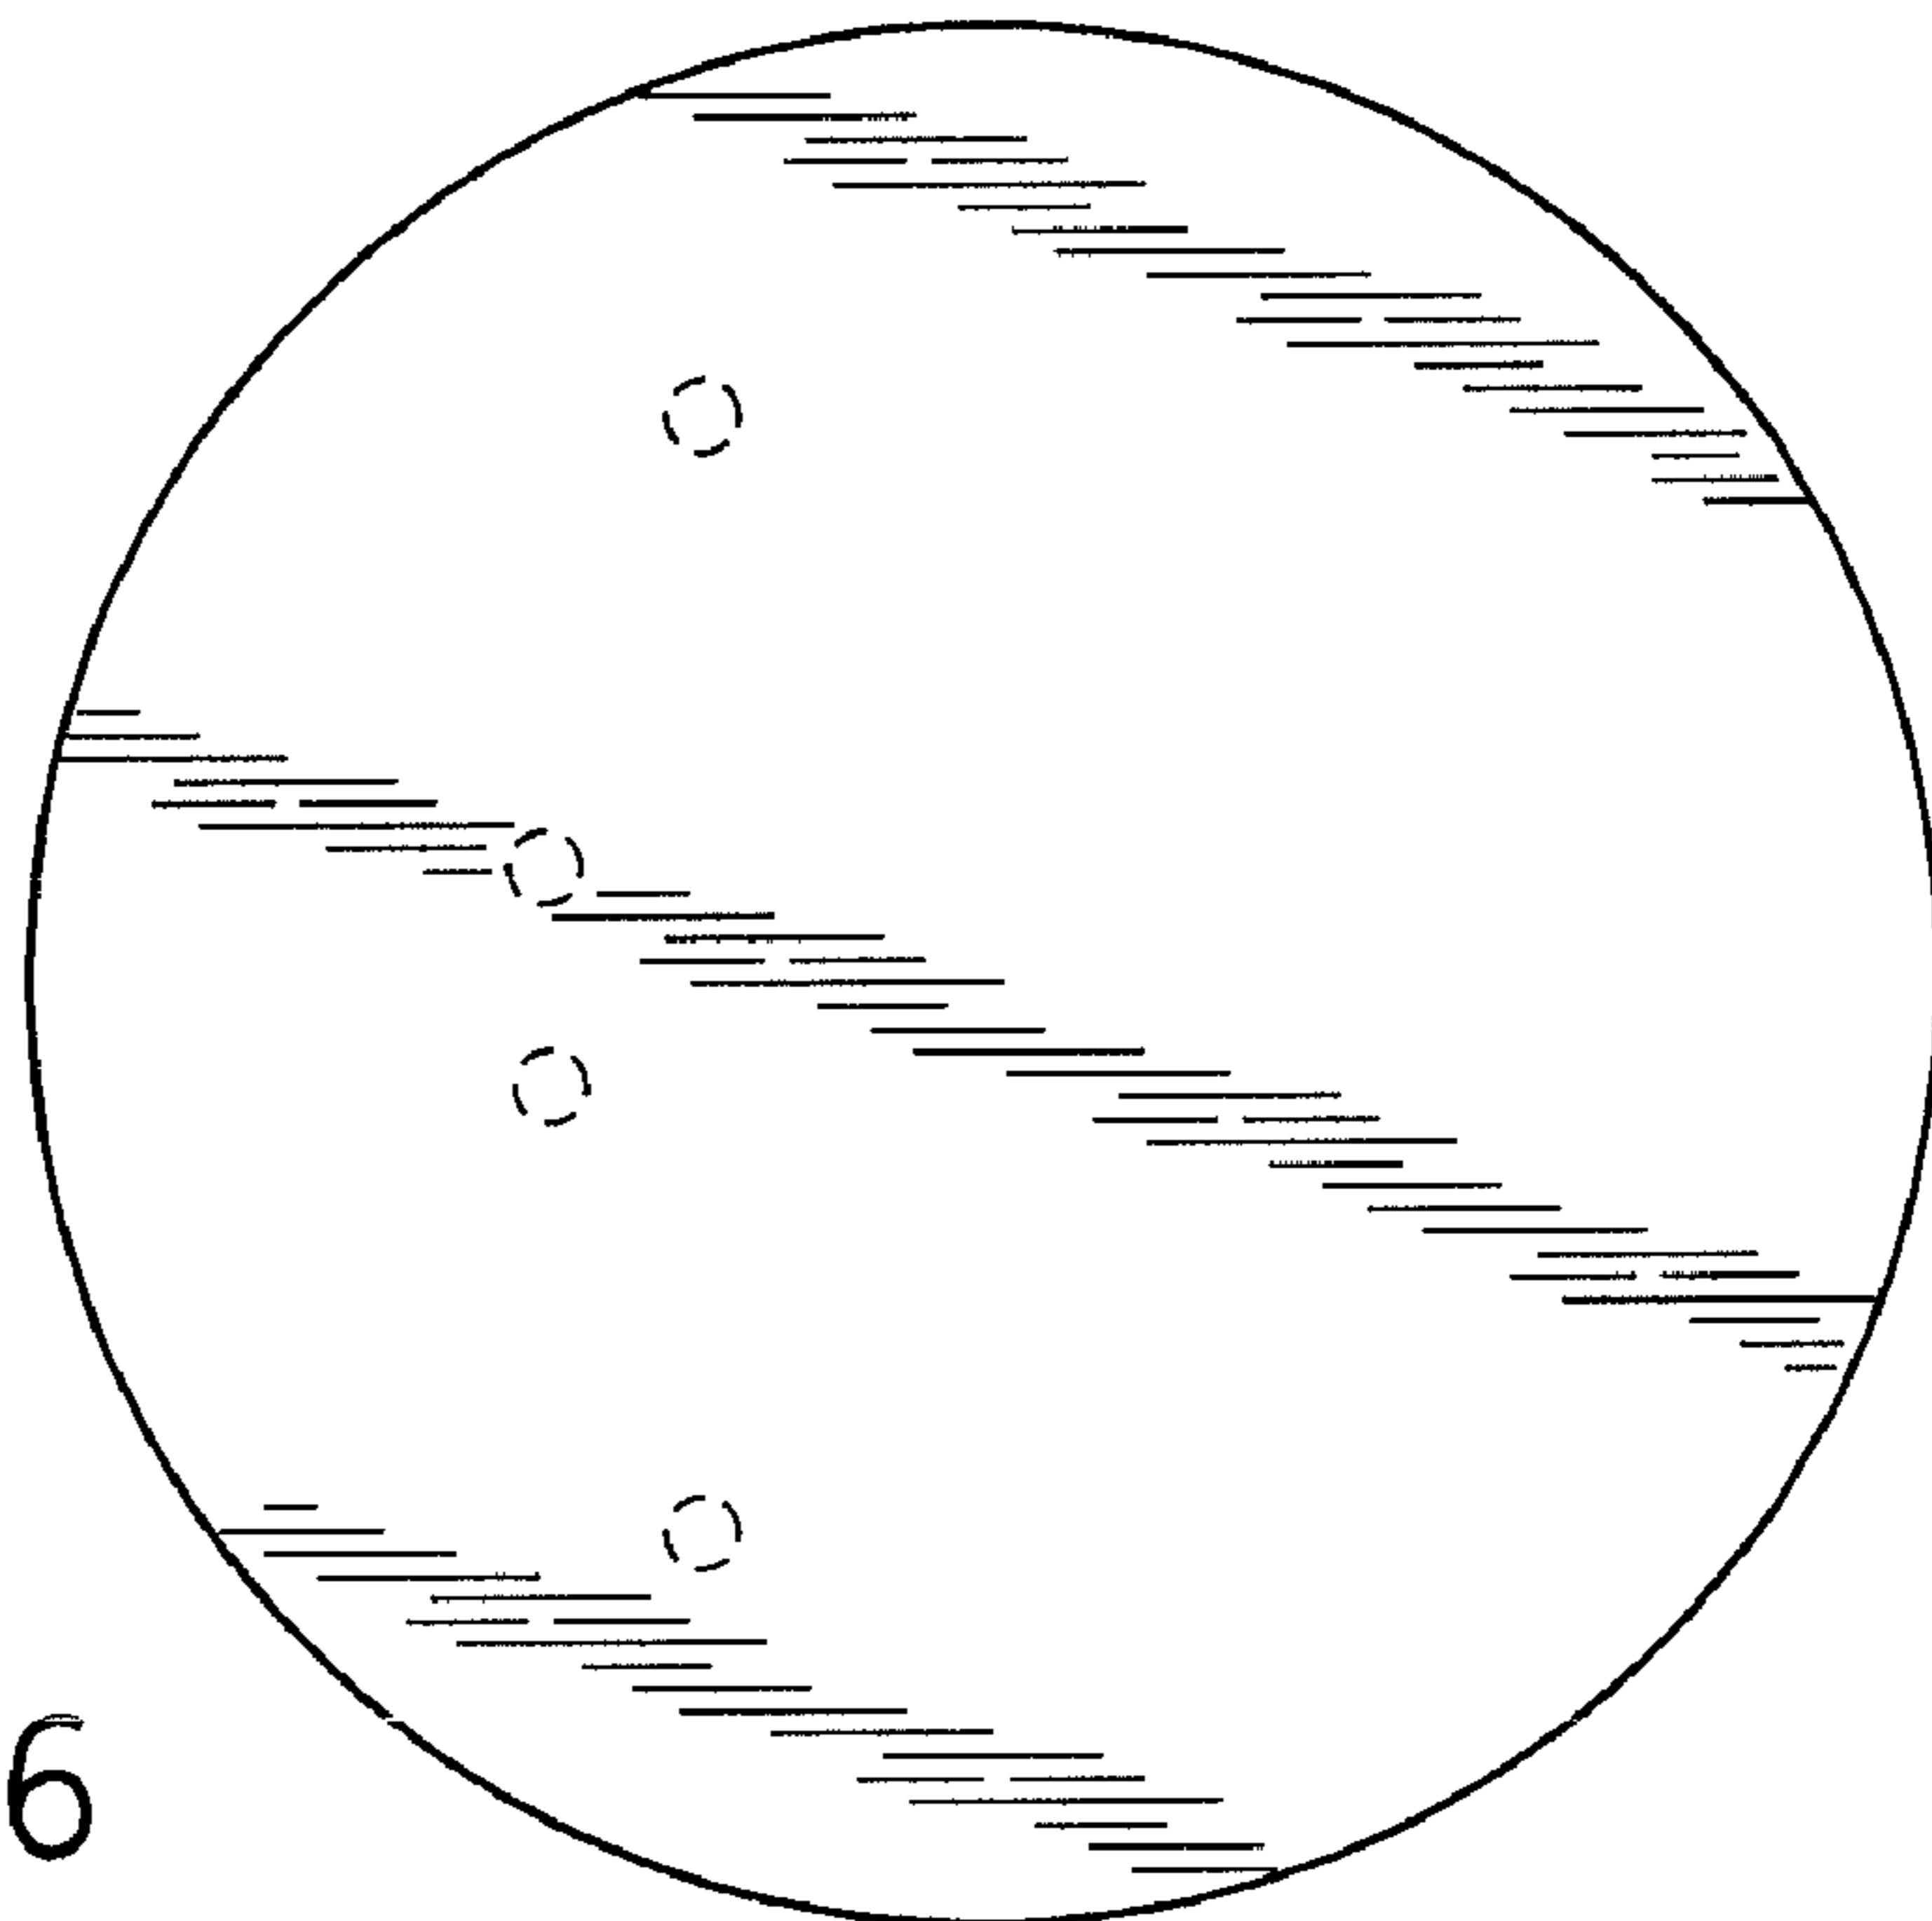


FIG. 6