



US00D680223S

(12) **United States Design Patent**
Jamison et al.

(10) **Patent No.:** **US D680,223 S**
(45) **Date of Patent:** **** Apr. 16, 2013**

(54) **EXAMINATION CHAIR**

(75) Inventors: **Chris M. Jamison**, West Chester, OH
(US); **H. Ray Wright**, Loudon, TN
(US); **Antonio Belton**, Richton Park, IL
(US); **Dominik J. Beck**, Menlo Park, CA
(US)

(73) Assignee: **Reliance Medical Products, Inc.**,
Mason, OH (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/404,346**

(22) Filed: **Oct. 19, 2011**

(51) **LOC (9) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/178; D6/336**

(58) **Field of Classification Search** D24/172,
D24/176–179, 183–185; D6/334, 336, 360–361,
D6/501–502, 335, 367, 500; D10/46; 248/127;
297/330, 391, 411.2, 445.1, 447.2, 452.28,
297/452.29; 351/245, 200, 244, 246; 433/33
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,491,242	A	12/1949	Alexander	
D180,350	S *	5/1957	Armbruster	D6/360
2,874,689	A	2/1959	Gavelek	
D194,673	S *	2/1963	Watlington	D6/360
3,198,574	A	8/1965	Hayashi et al.	
3,259,355	A	7/1966	Slouka	
D206,532	S	12/1966	Gardella	
D206,585	S *	1/1967	Gardella	D6/361
3,414,324	A *	12/1968	Taylor et al.	297/330
3,436,046	A	4/1969	Valeska	
3,486,789	A	12/1969	Taylor et al.	
3,578,379	A	5/1971	Taylor et al.	
3,873,152	A	3/1975	Garas	
D235,274	S	6/1975	Armbruster	

D236,299	S	8/1975	Long	
D263,434	S *	3/1982	Miller	D6/360
D268,149	S	3/1983	Case	
4,415,203	A *	11/1983	Cawley	297/391
4,415,204	A	11/1983	Cavrak	
4,657,217	A	4/1987	Kiesel et al.	
D292,526	S	10/1987	Nakayama	
4,741,506	A	5/1988	Schwaegerle	
D300,657	S	4/1989	Simpkins et al.	

(Continued)

OTHER PUBLICATIONS

Topcon IS-2500 Instrument Stand. Cal Coast Ophthalmic Instruments, Inc. Copyright 2005. [Retrieved on Sep. 12, 2012]. Retrieved from the Internet: <URL: <http://www.calcoastophthalmic.com/products/stands/topcon IS2500/>>.*

(Continued)

Primary Examiner — Wan Laymon

(74) *Attorney, Agent, or Firm* — Wood, Herron & Evans, L.L.P.

(57) **CLAIM**

The ornamental design for an examination chair, as shown and described.

DESCRIPTION

FIG. 1 is a front perspective view of the examination chair according to the invention.

FIG. 2 is a front elevational view thereof.

FIG. 3 is a left side elevational view thereof.

FIG. 4 is a right side elevational view thereof.



FIG. 5 is a rear elevational view thereof.

FIG. 6 is a top view thereof; and,

FIG. 7 is a bottom view thereof.

Any elements shown in broken lines form no part of the claimed invention in this application, and are instead included to show environmental aspects of the claimed invention.

1 Claim, 6 Drawing Sheets

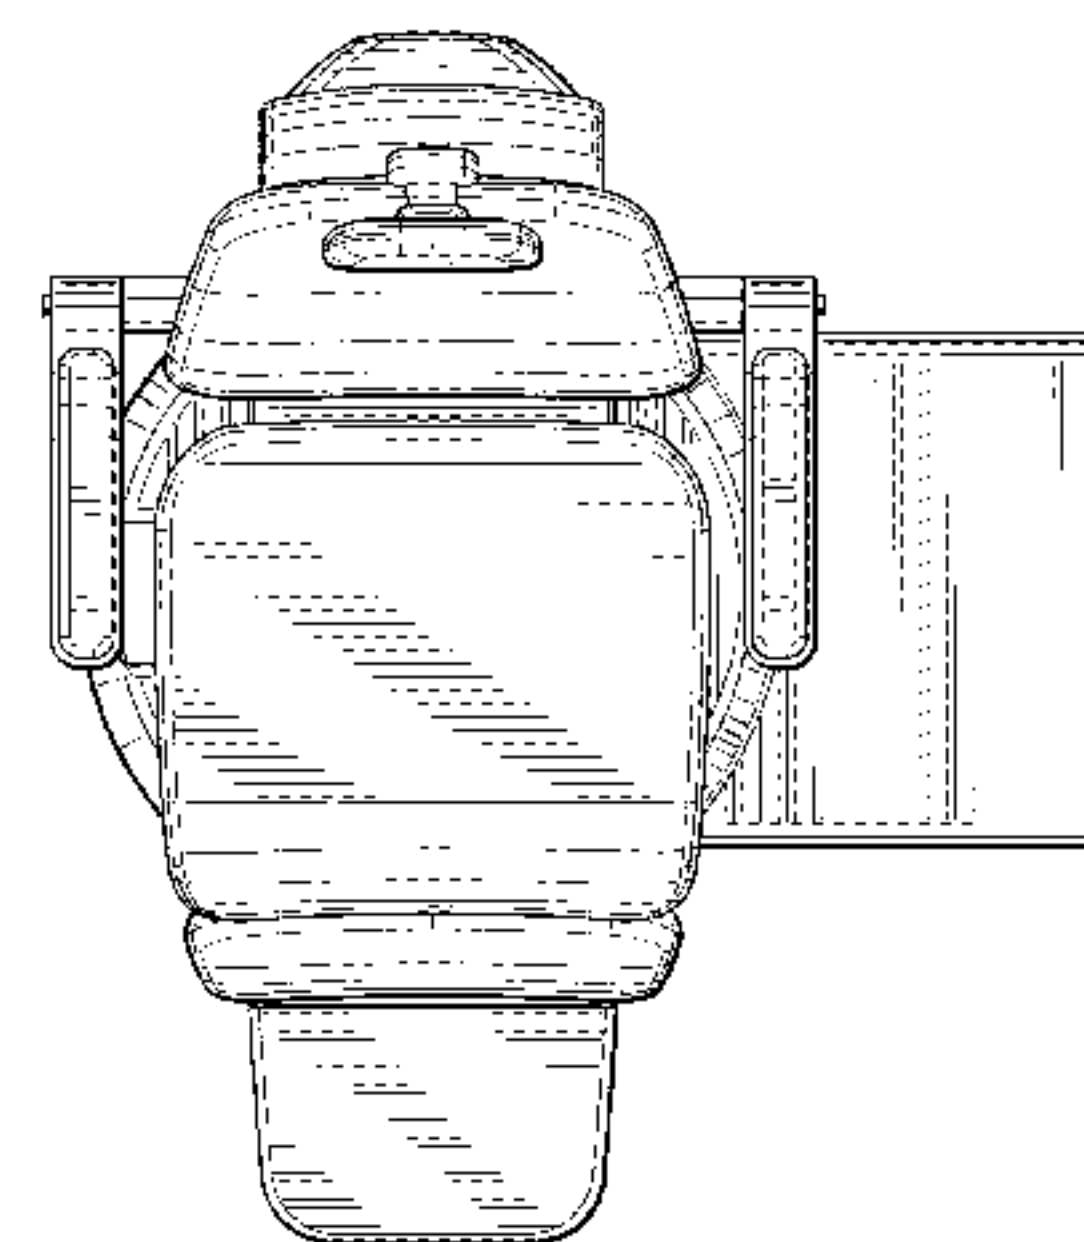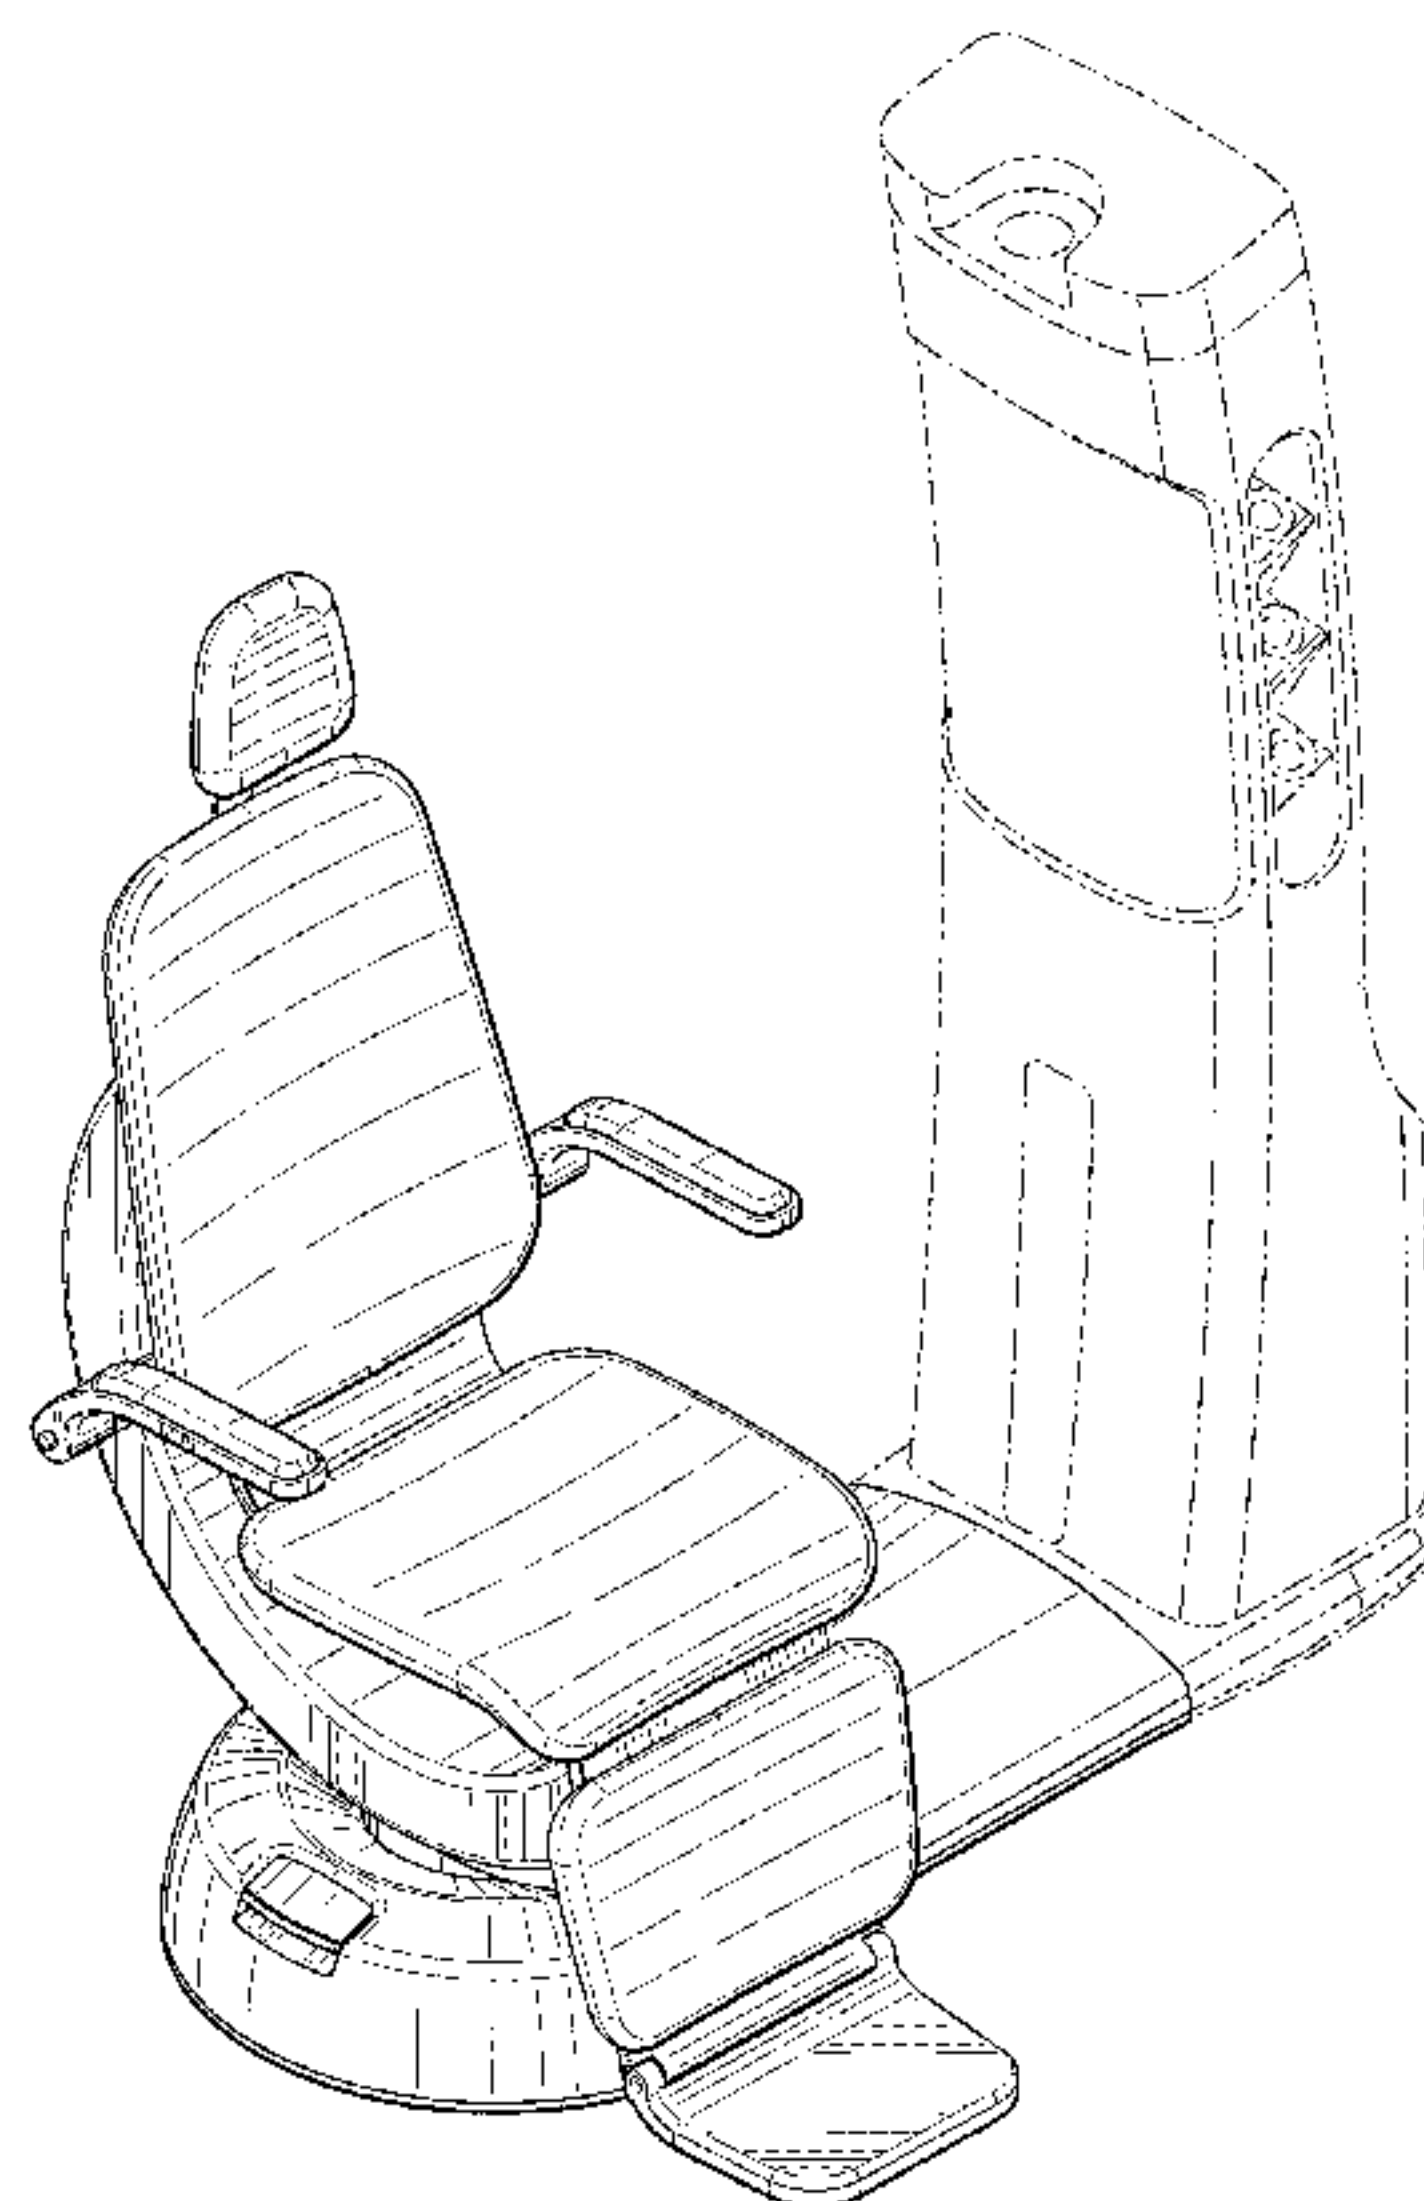

U.S. PATENT DOCUMENTS

4,852,941 A 8/1989 Jones
4,910,386 A 3/1990 Johnson
D321,097 S 10/1991 Jones et al.
D333,736 S * 3/1993 Nordstrom D6/367
5,313,961 A 5/1994 McKee
5,348,375 A 9/1994 Steininger
D352,106 S 11/1994 Fanney et al.
D353,201 S 12/1994 Crook et al.
D354,176 S 1/1995 Schwaegerle et al.
D354,177 S 1/1995 Schwaegerle et al.
5,399,007 A 3/1995 Marconet
D361,674 S 8/1995 Carter, Sr.
5,461,965 A 10/1995 Schwaegerle
5,467,002 A 11/1995 Brooks
5,480,212 A 1/1996 Marconet
5,520,363 A 5/1996 Burton et al.
5,580,023 A 12/1996 Burton et al.
D378,315 S 3/1997 Schwaegerle et al.
5,624,159 A 4/1997 Celoni et al.
D379,409 S 5/1997 Schwaegerle et al.
5,645,313 A 7/1997 Best et al.
5,696,574 A 12/1997 Schwaegerle
5,717,480 A 2/1998 Brooks et al.
5,777,344 A 7/1998 Hayashi
D397,259 S 8/1998 Chatani et al.
D407,379 S 3/1999 Schwaegerle
5,907,387 A 5/1999 Schwaegerle
D412,621 S 8/1999 Smith et al.
D412,801 S 8/1999 Smith et al.
5,992,934 A 11/1999 Gehrig et al.
D418,339 S 1/2000 Smith et al.
D418,686 S 1/2000 Smith et al.
D419,343 S 1/2000 Smith et al.
D420,233 S 2/2000 Smith et al.
D423,262 S 4/2000 Smith et al.
D424,200 S 5/2000 Smith
D424,337 S 5/2000 Smith et al.
D425,341 S 5/2000 Smith et al.
D425,735 S 5/2000 Smith et al.
D425,991 S 5/2000 Smith et al.

D426,715 S 6/2000 Smith et al.
6,095,649 A 8/2000 Brooks et al.
6,106,065 A 8/2000 Carroll
D433,588 S 11/2000 Smith et al.
6,264,329 B1 7/2001 Brooks et al.
D456,080 S 4/2002 Karlsson
D456,158 S 4/2002 Van Severen
6,382,725 B1 5/2002 Carroll
D458,378 S 6/2002 Bevington
6,575,575 B2 6/2003 O'Brien et al.
6,721,976 B2 4/2004 Schwaegerle
6,736,360 B1 5/2004 Buczek
D503,233 S 3/2005 Smith
D504,515 S 4/2005 Smith
6,886,199 B1 5/2005 Schwaegerle
D506,257 S 6/2005 Smith
6,928,676 B1 8/2005 Schwaegerle
D509,079 S 9/2005 Natuzzi
D509,371 S 9/2005 Natuzzi
D512,507 S 12/2005 Smith
D514,701 S 2/2006 Smith
D531,318 S 10/2006 Morral Gispert
D533,368 S 12/2006 Natuzzi
7,207,531 B2 4/2007 Piontkowski
7,401,921 B2 7/2008 Baker et al.
7,467,871 B2 12/2008 Lawhorn et al.
D602,269 S 10/2009 Jamison et al.
7,670,003 B2 3/2010 Kendrick
D621,050 S 8/2010 Jamison et al.
2011/0147546 A1 6/2011 Monsalve et al.

OTHER PUBLICATIONS

Ophthalmic Chair and Instrument Stand Model 1500. Protech Ophthalmics. Copyright 2012. [Retrieved on Sep. 12, 2012]. Retrieved from the Internet: <URL: <http://www.eyedoctorsupply.com/servlet/the-140/Ophthalmic-Chair-And-Instrument/Detail>>.*
Topcon CSIII Chair and Stand. Vision Systems Inc. [Retrieved on Sep. 12, 2012]. Retrieved from the Internet: <URL: <http://www.patternless.com/topcon-csiii-chair-and-stand/>>.*

* cited by examiner



FIG. 1

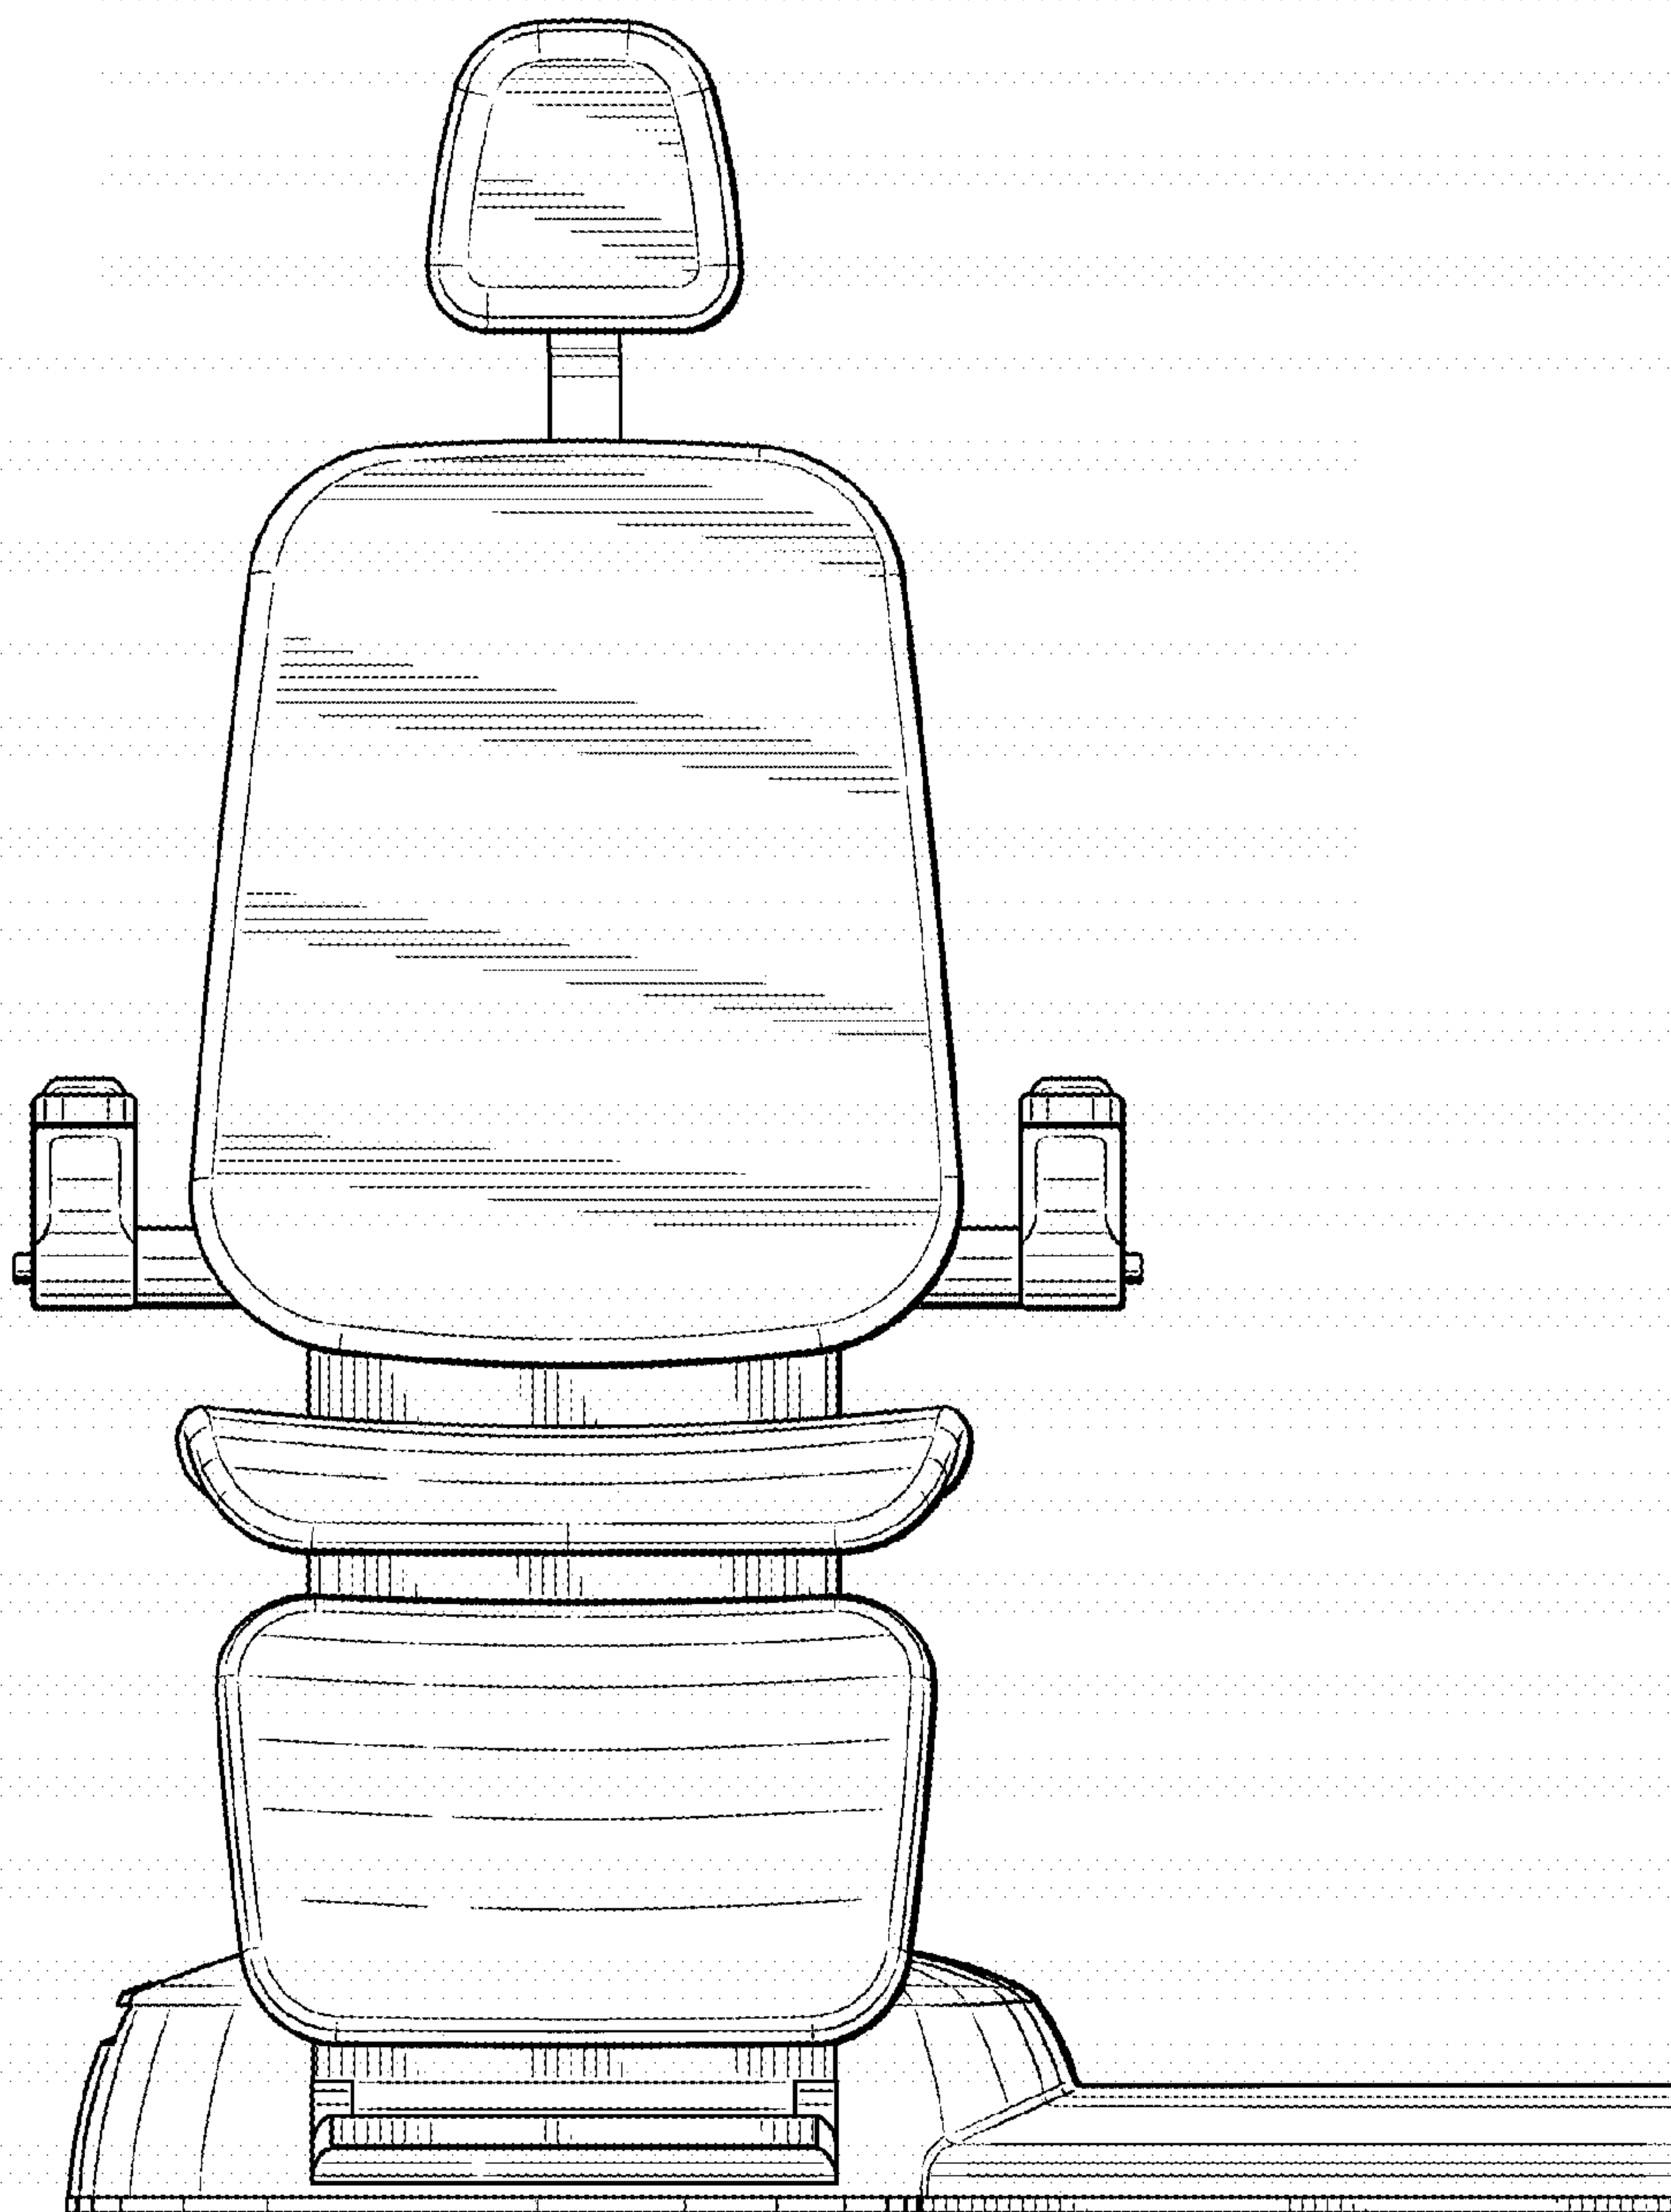


FIG. 2

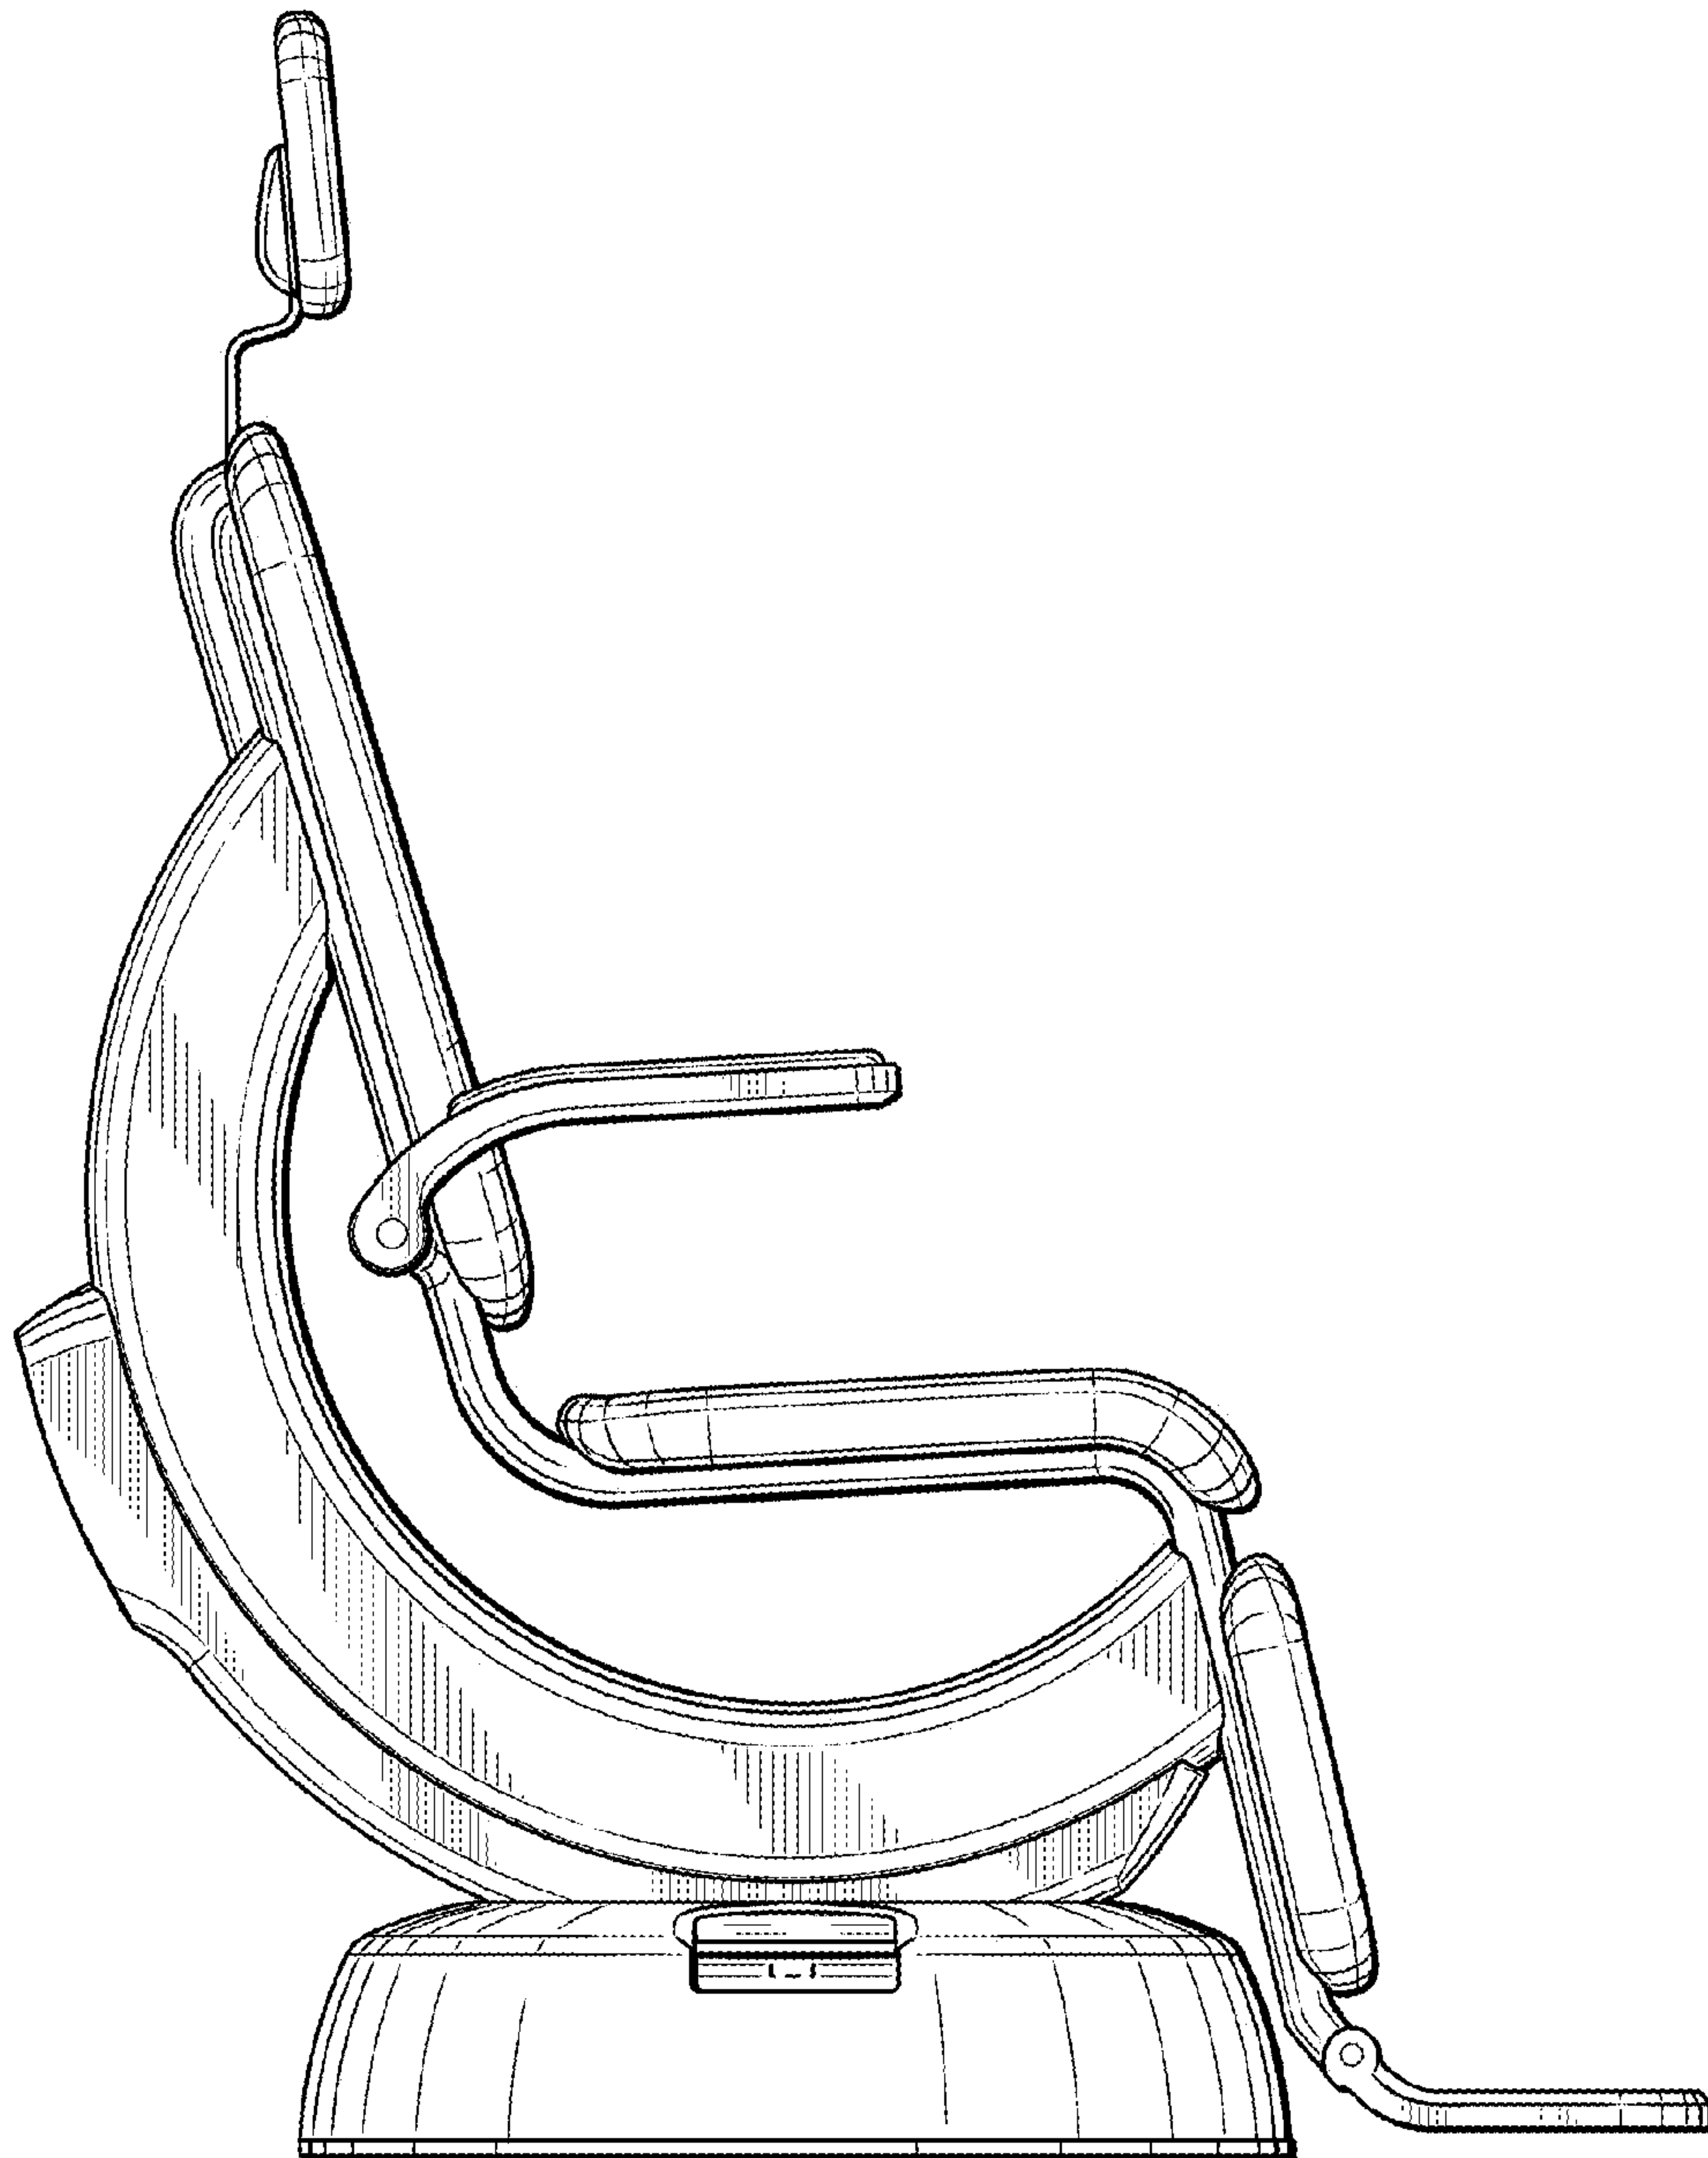


FIG. 3

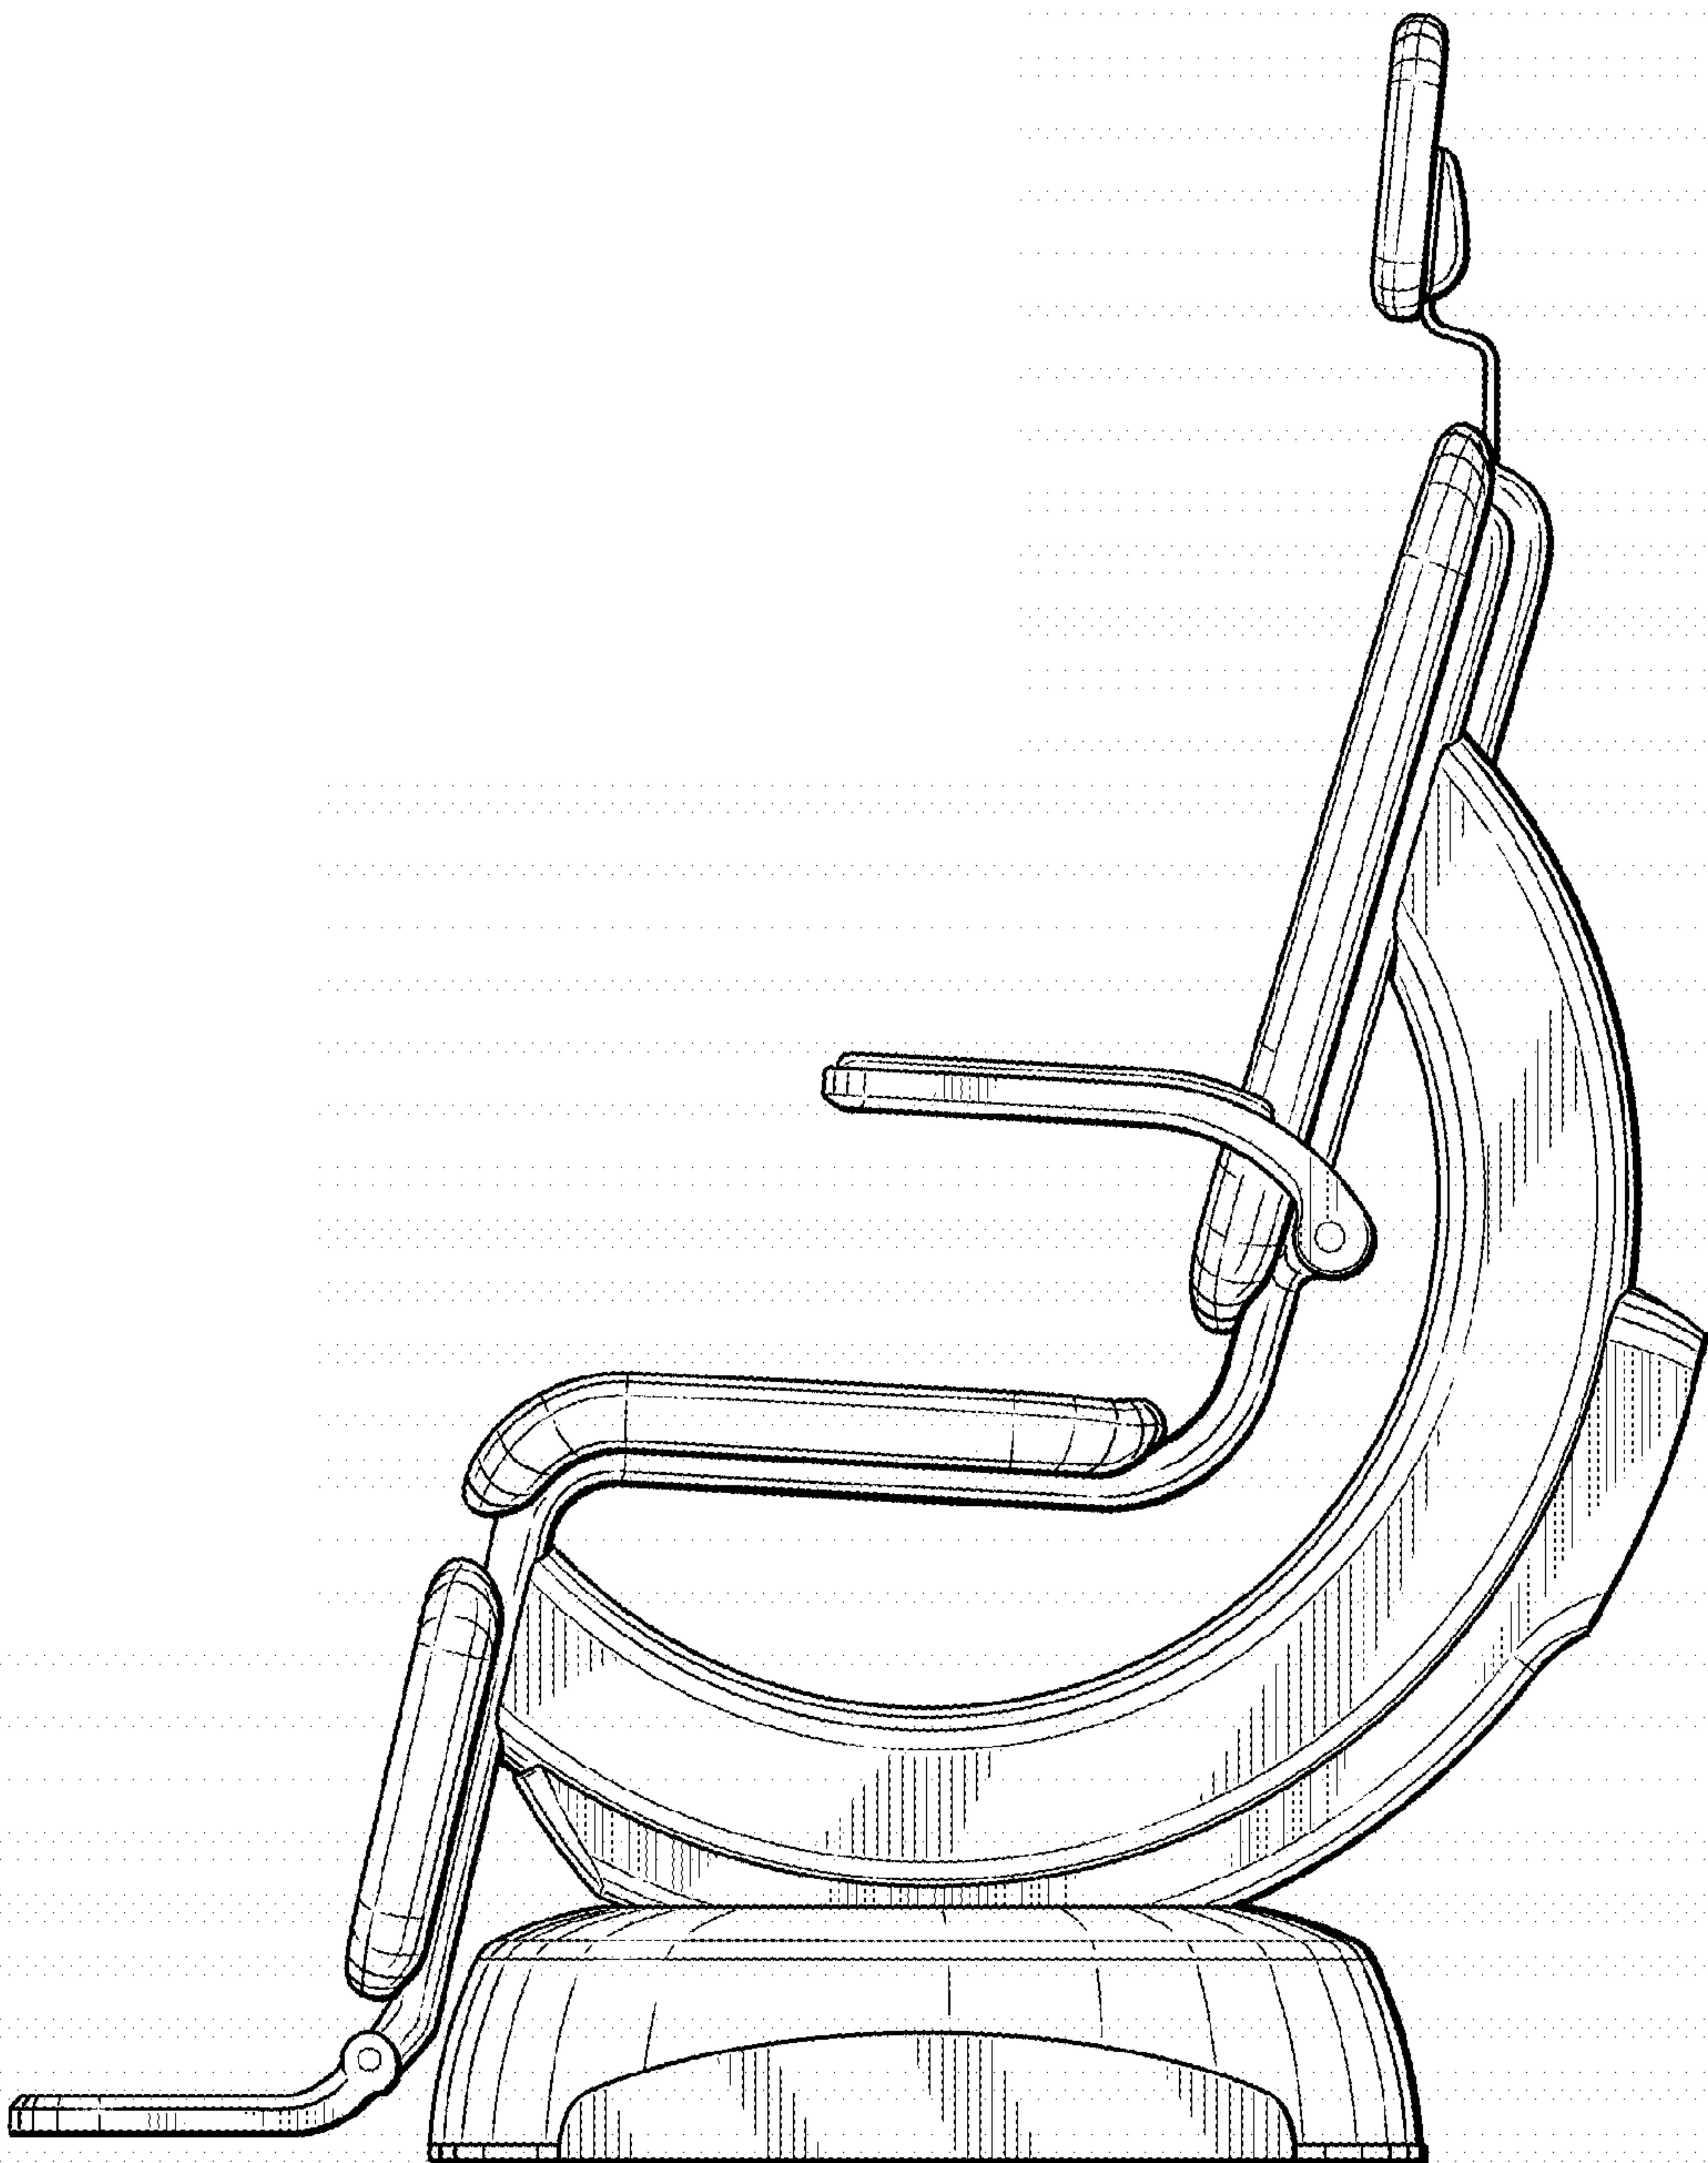


FIG. 4

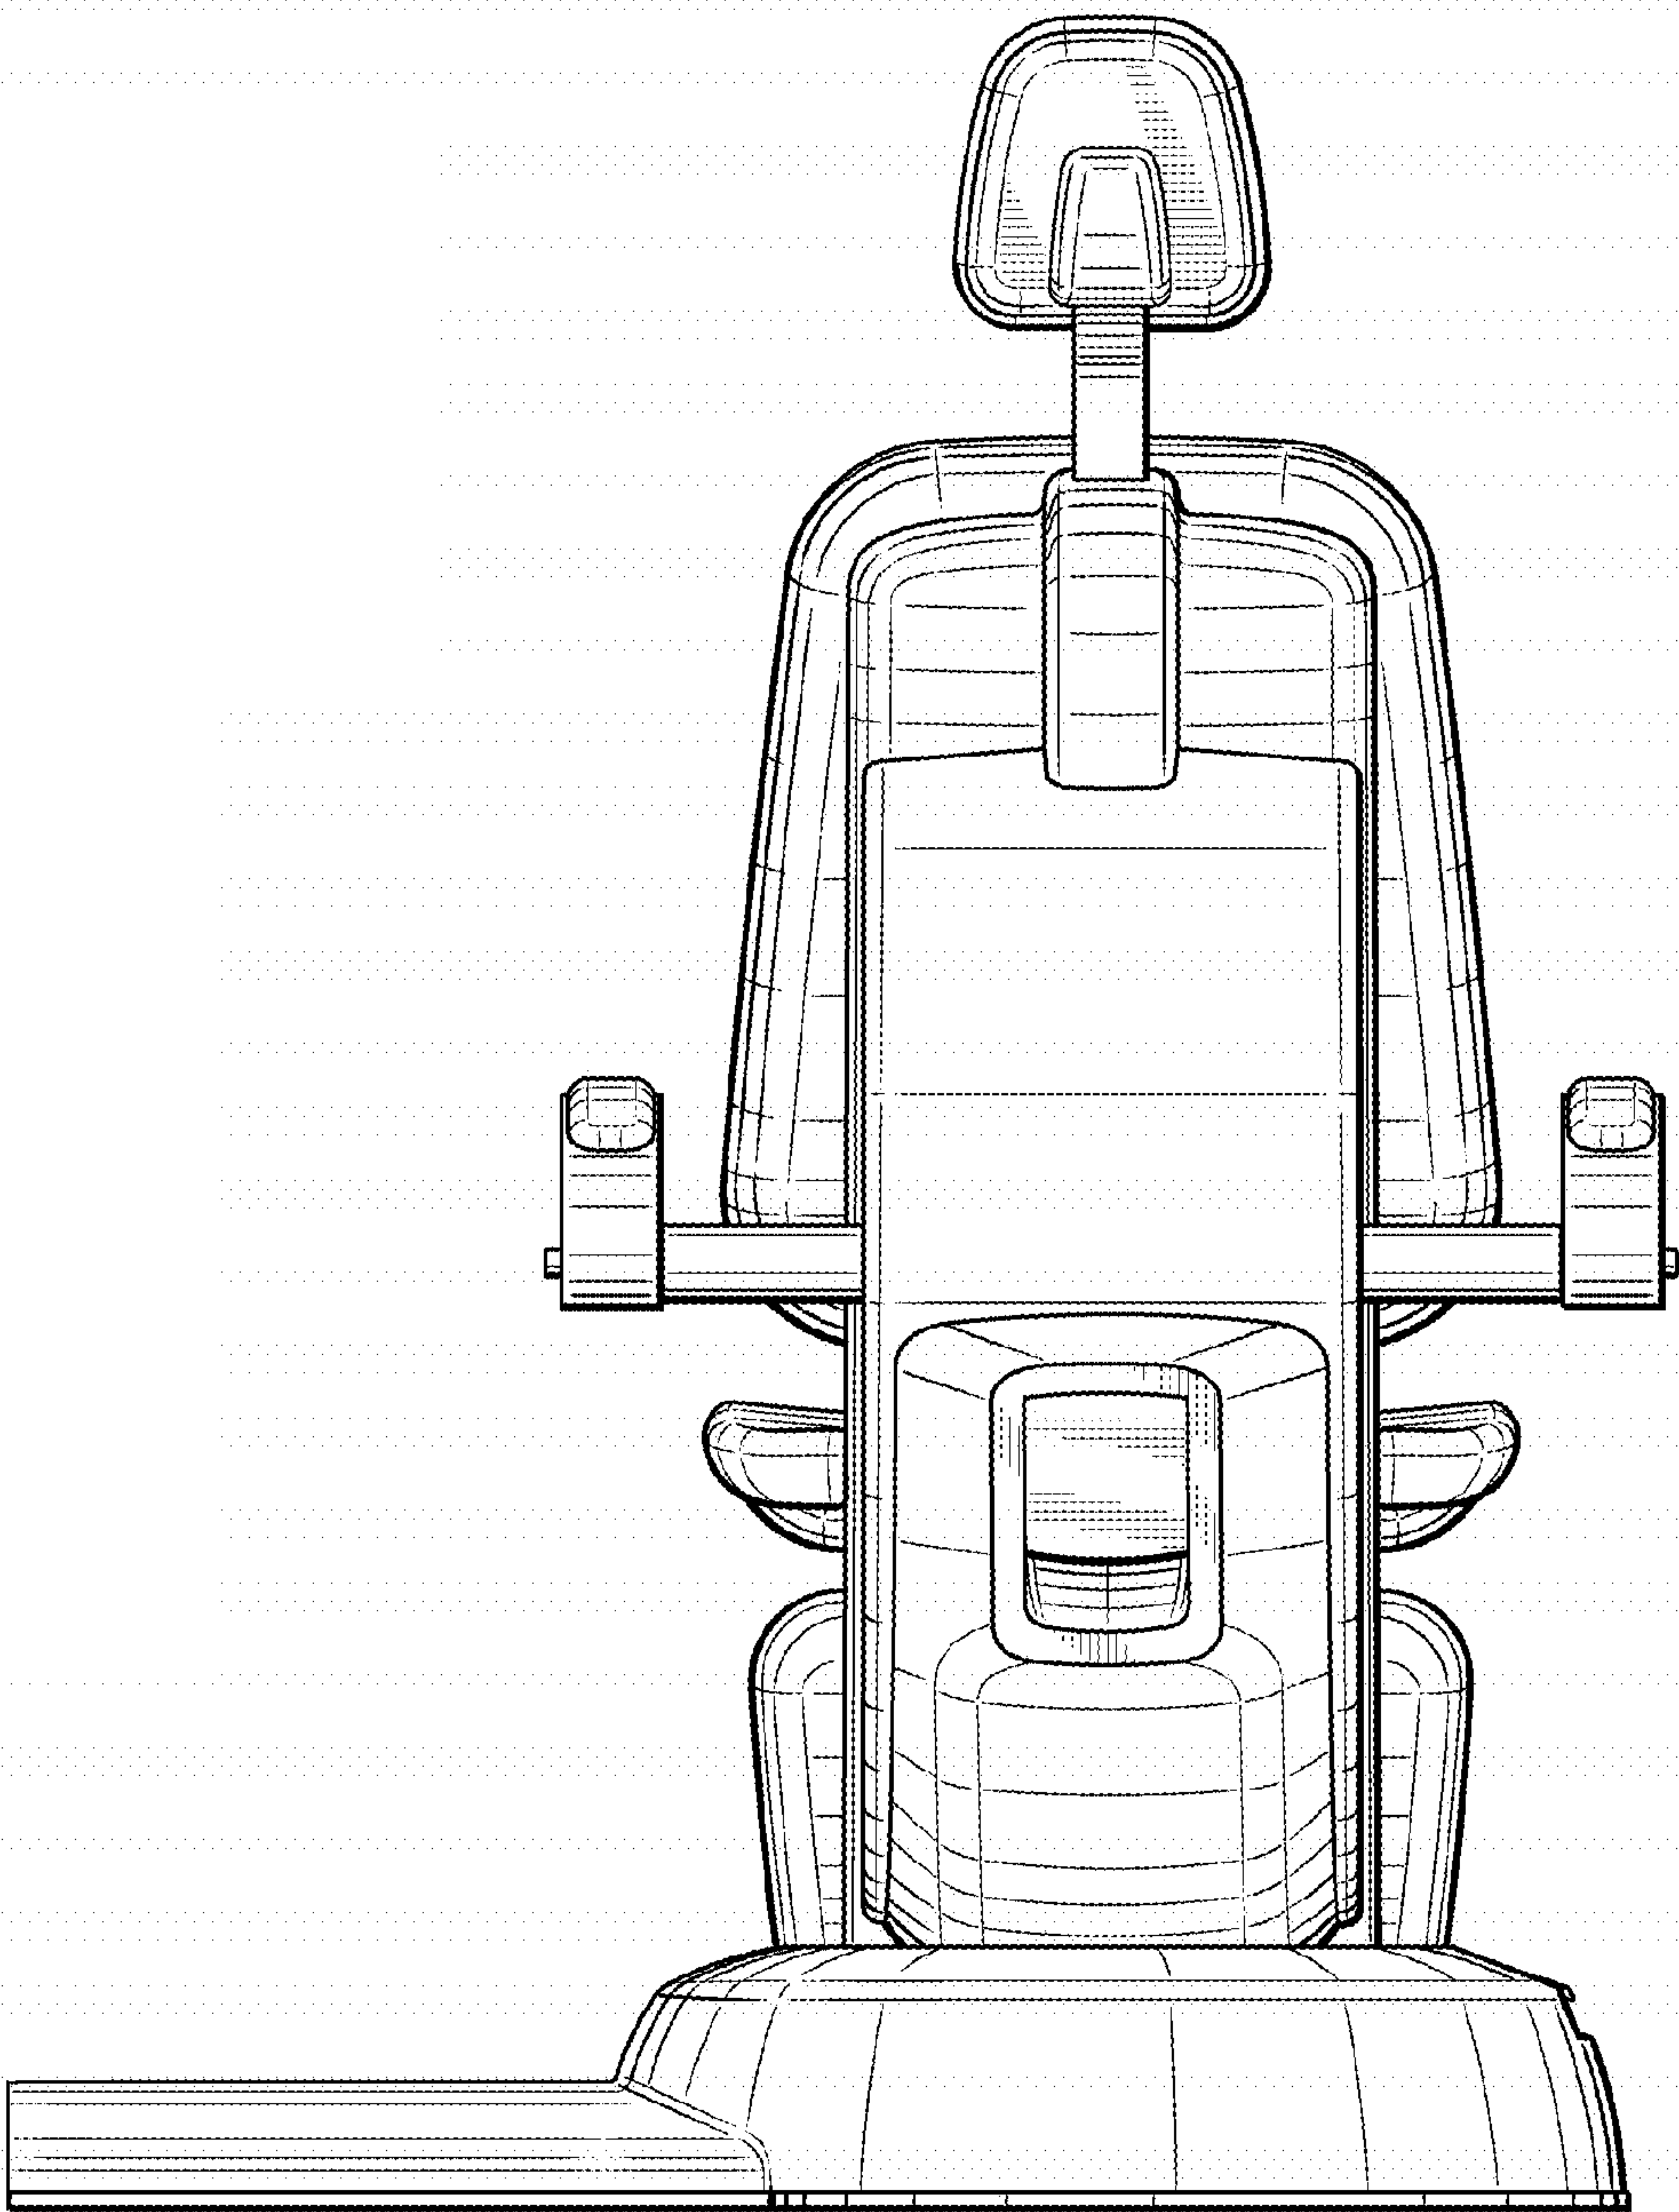


FIG. 5

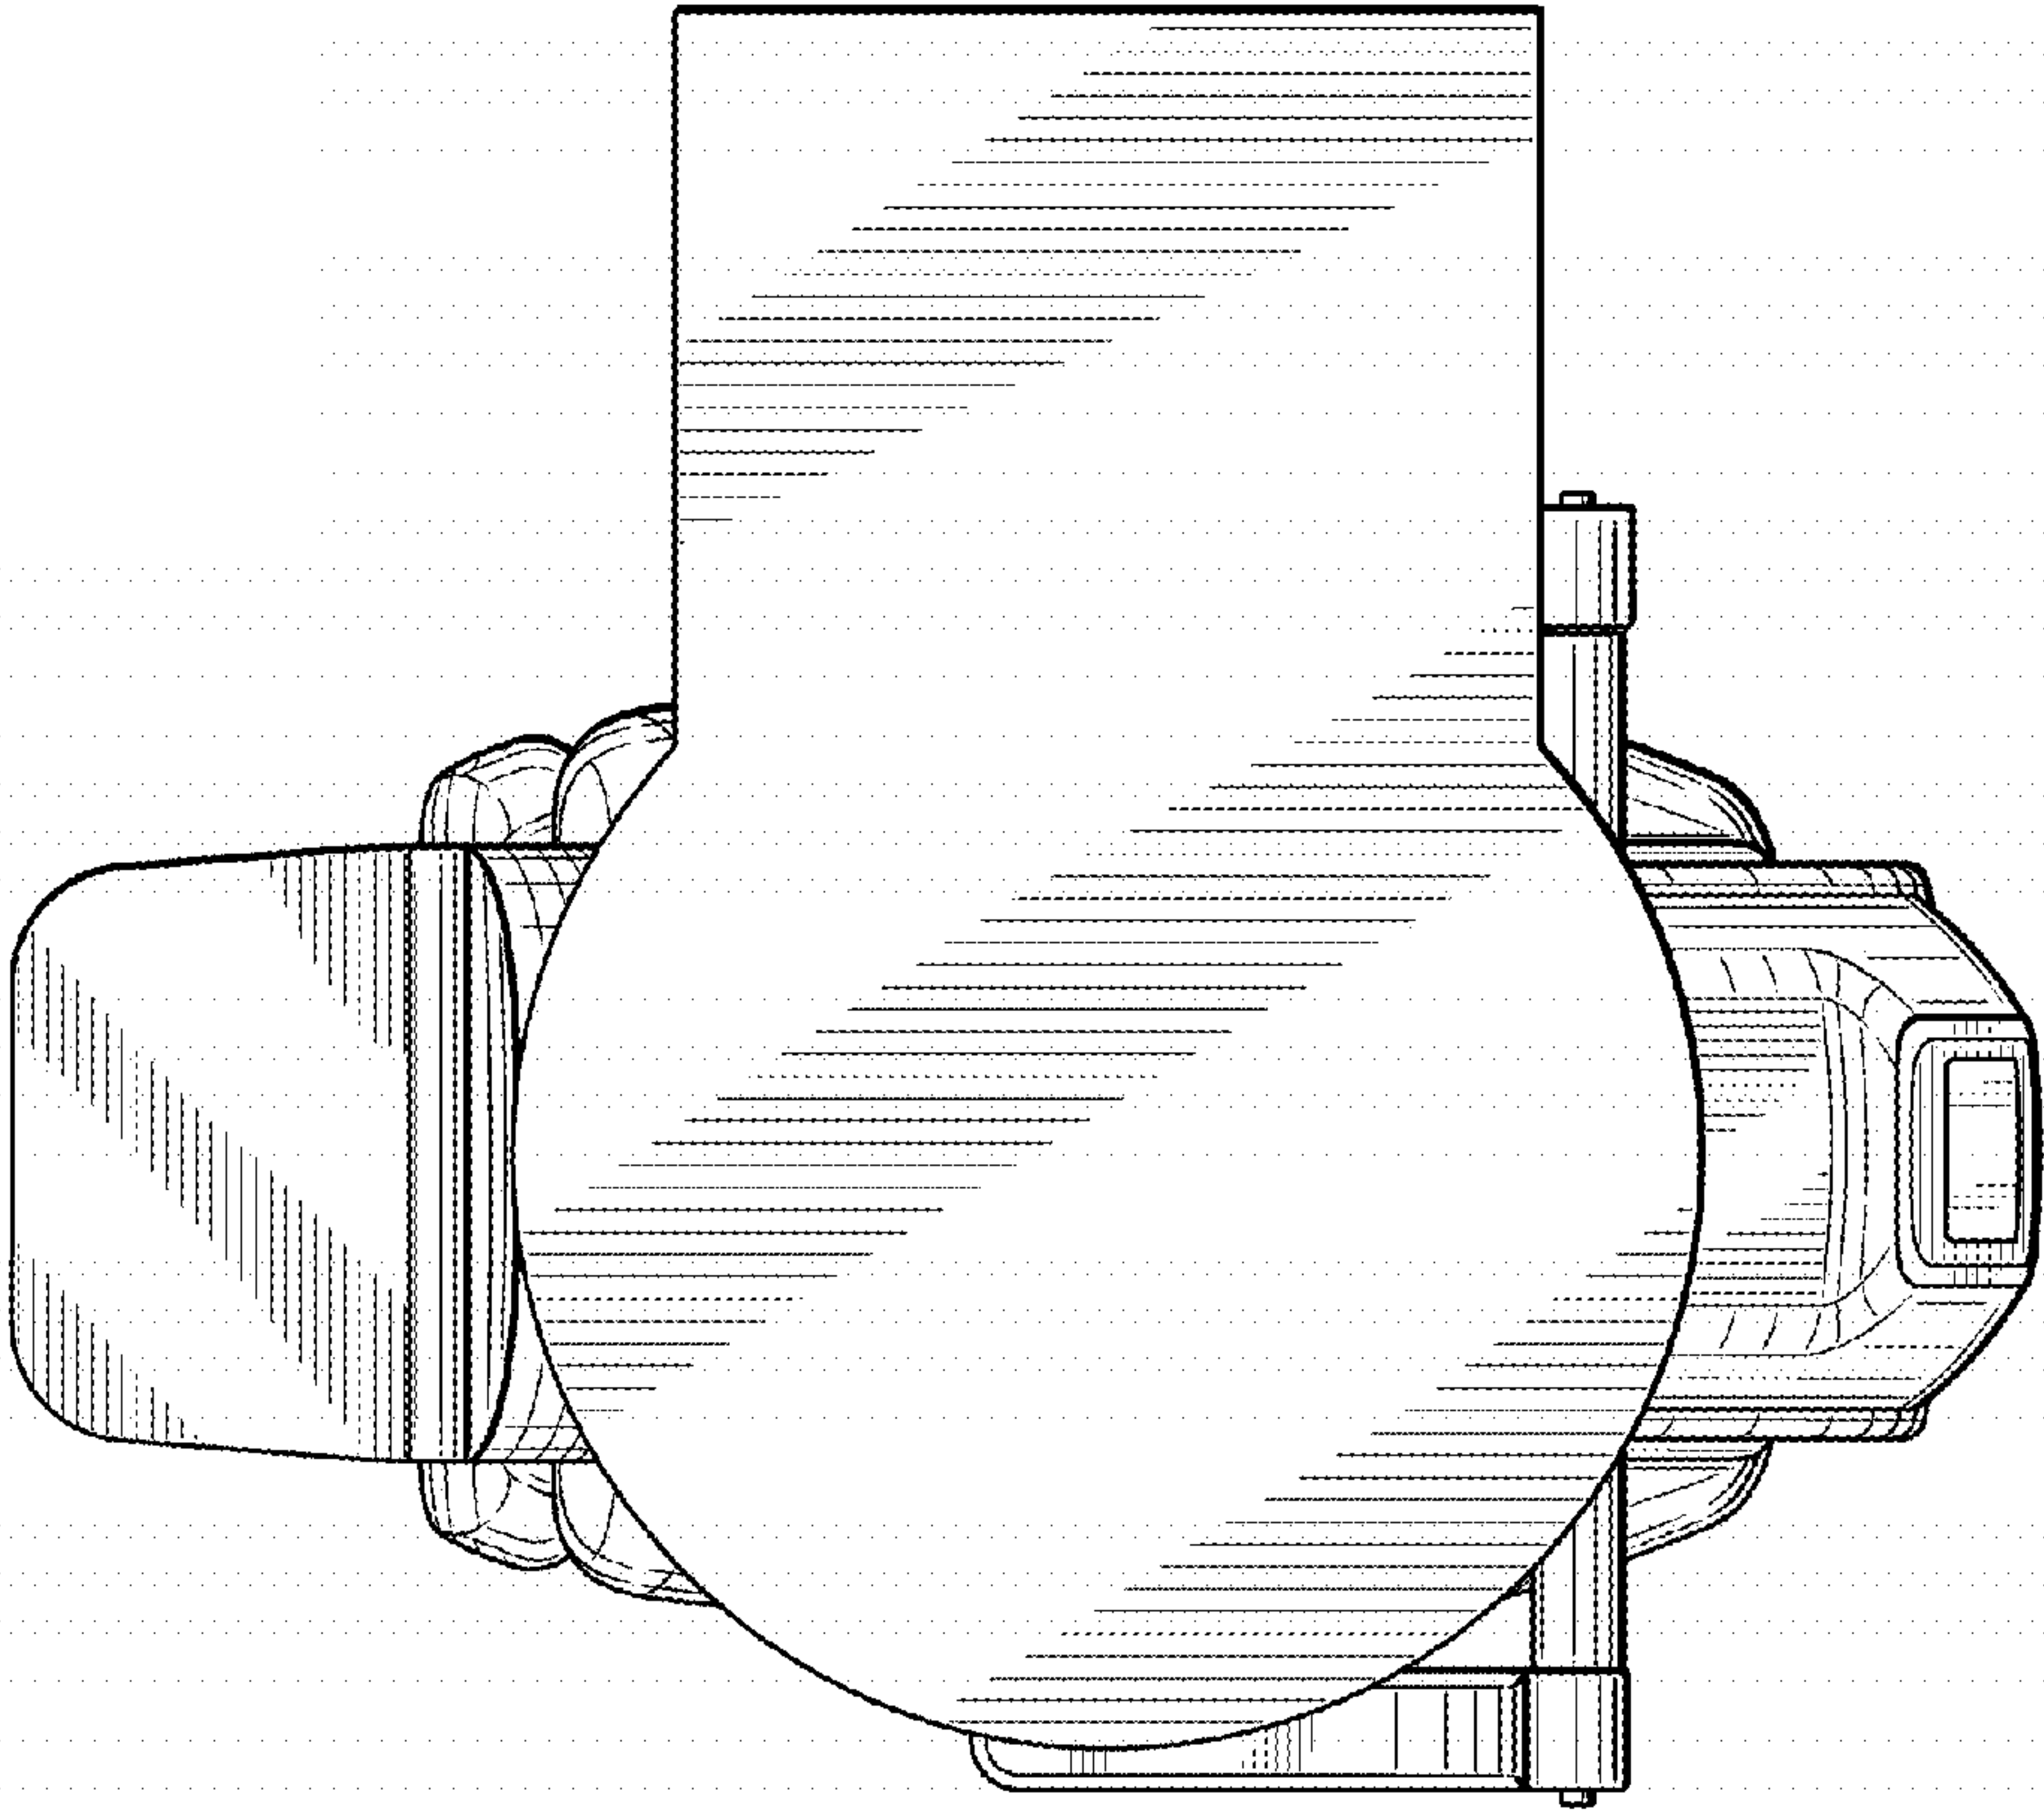


FIG. 7

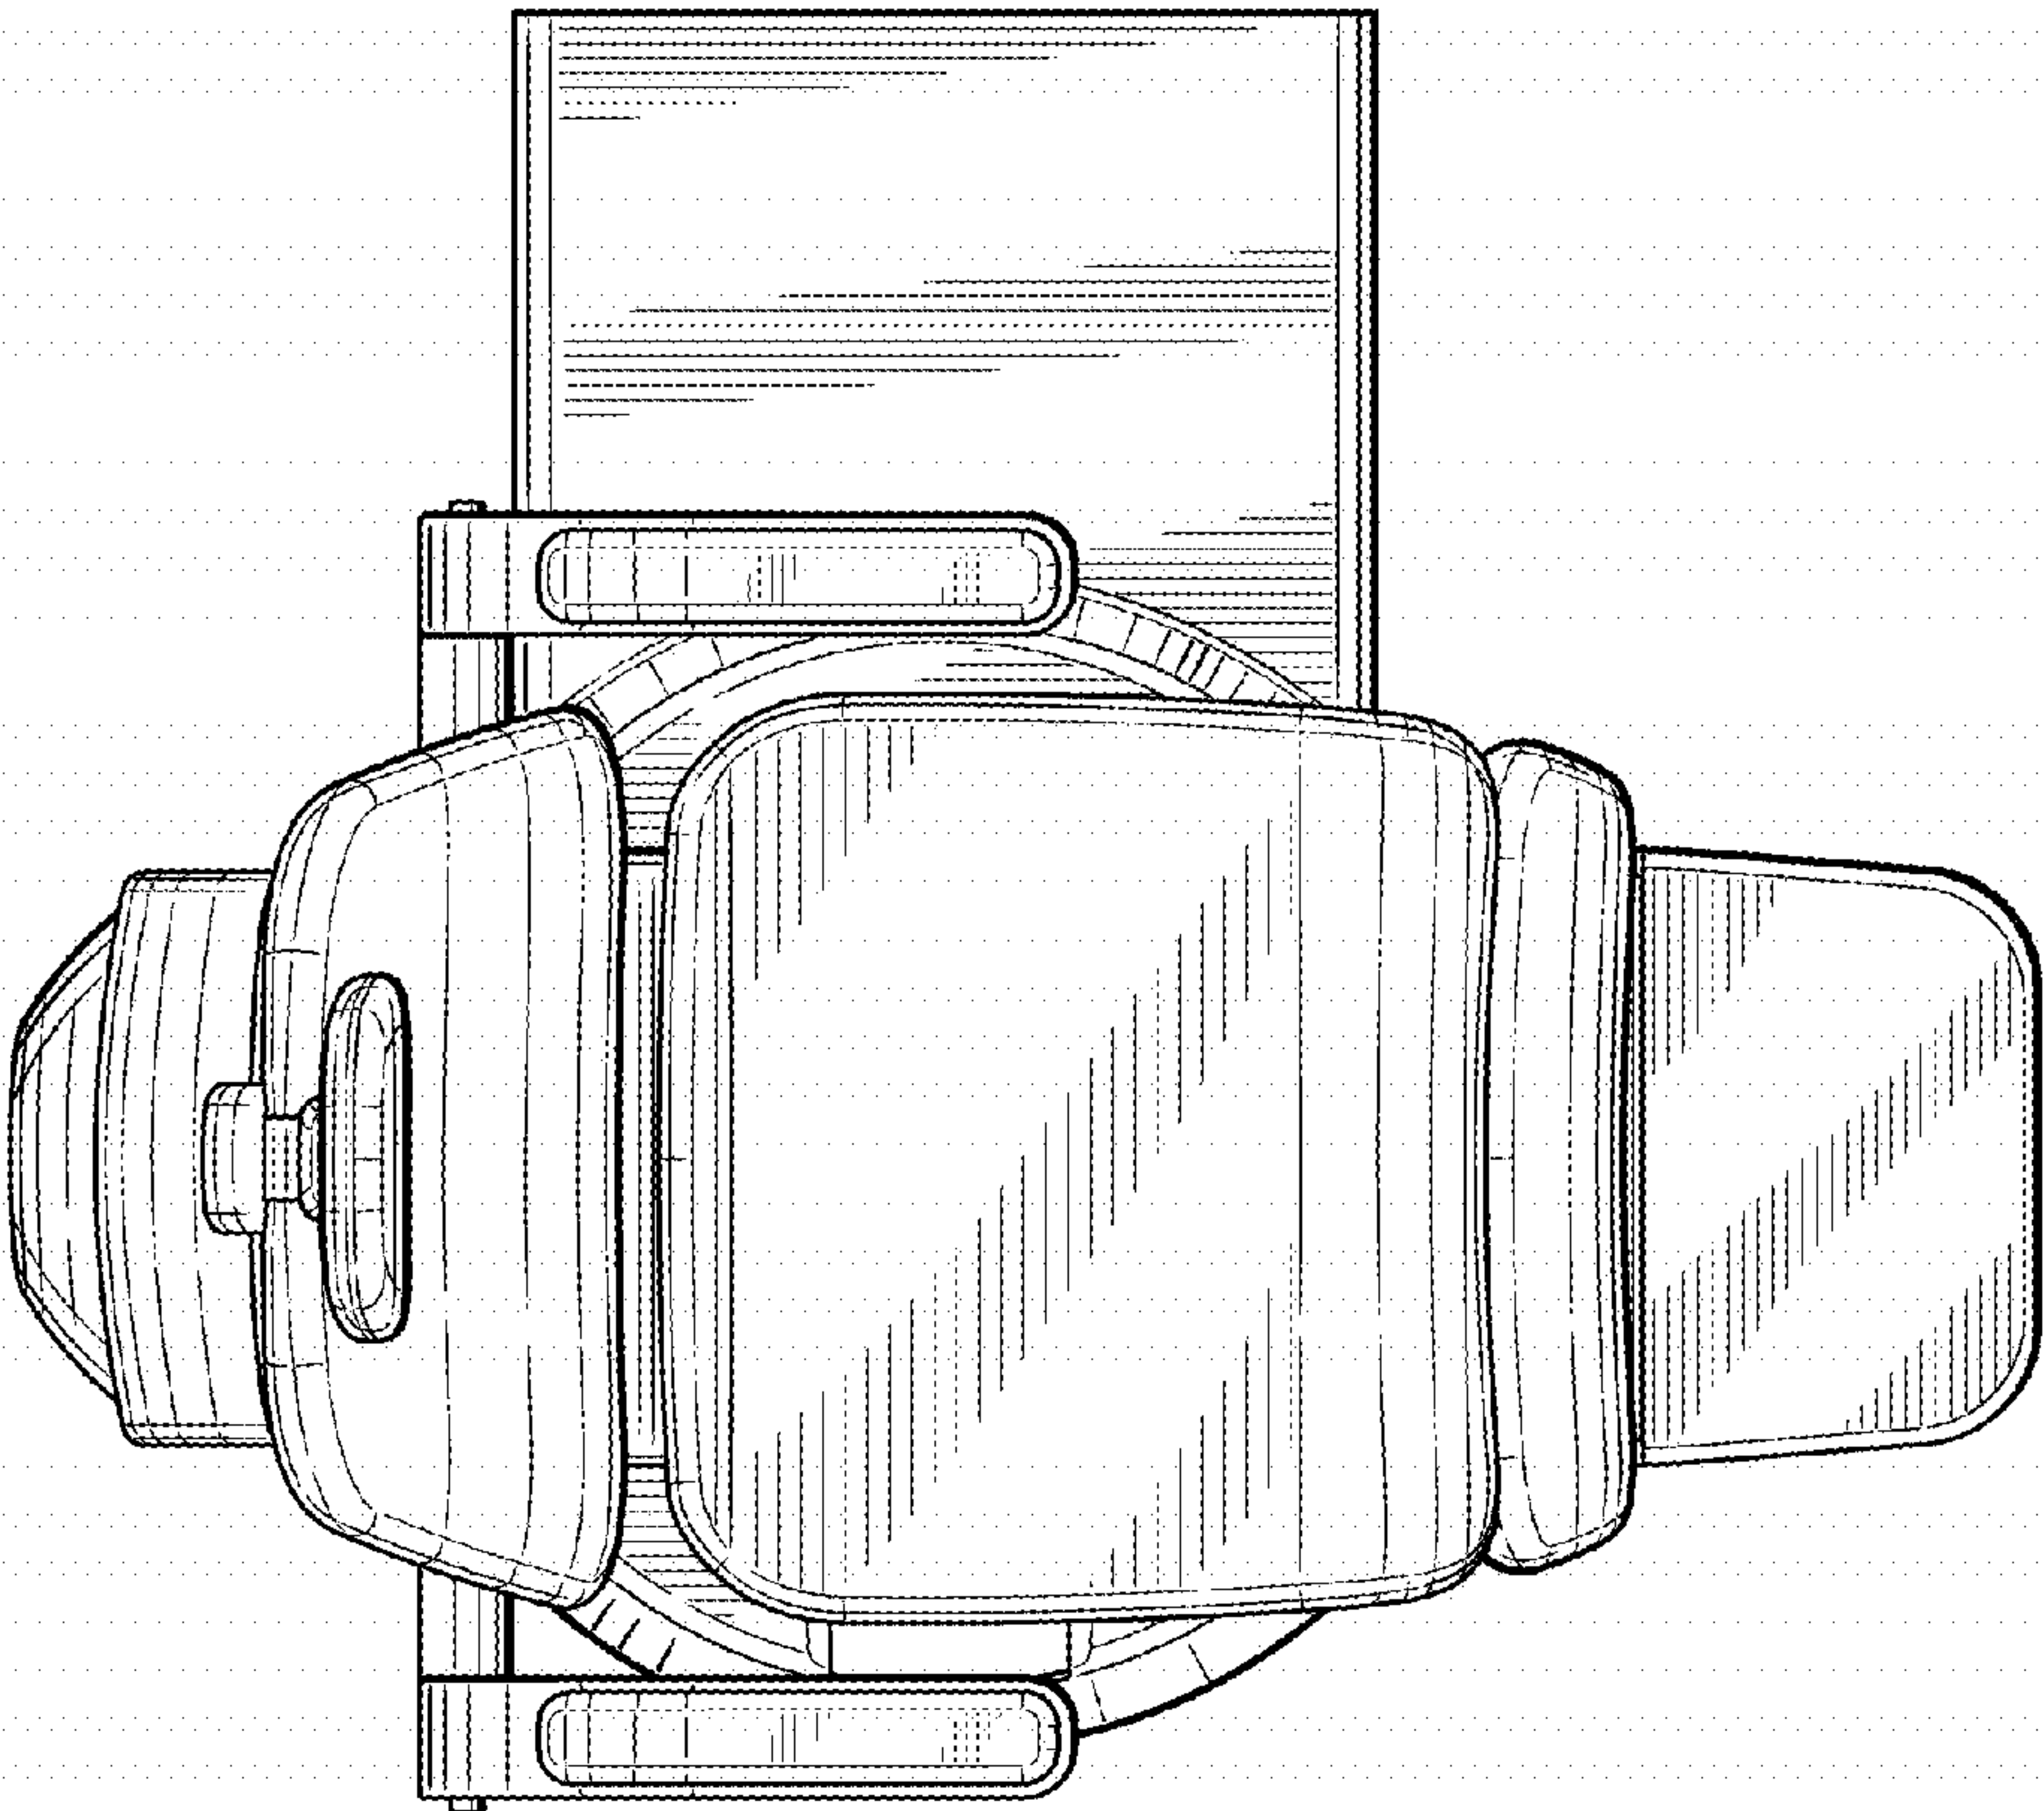


FIG. 6