



US00D682432S

(12) **United States Design Patent**
Khan et al.

(10) **Patent No.:** **US D682,432 S**
(45) **Date of Patent:** **** *May 14, 2013**

(54) **DIAGNOSTIC CARTRIDGE READER**

(75) Inventors: **Macksoud Khan**, Palo Alto, CA (US);
Zachary M. Ruef, San Francisco, CA
(US); **Keagan Rowley**, Boulder, CO
(US)

(73) Assignee: **MBio Diagnostics, Inc.**, Boulder, CO
(US)

(*) Notice: This patent is subject to a terminal disclaimer.

(**) Term: **14 Years**

(21) Appl. No.: **29/416,269**

(22) Filed: **Mar. 20, 2012**

Related U.S. Application Data

(63) Continuation of application No. 29/393,971, filed on
Jun. 10, 2011.

(51) **LOC (9) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/186**

(58) **Field of Classification Search** D24/107,
D24/111, 164–165, 167, 186, 216, 231, 232,
D24/200, 172; 600/301, 481, 483–485, 509,
600/513, 519, 544; D10/81, 104
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D334,237 S * 3/1993 Collister et al. D24/186
D400,673 S * 11/1998 Kheiri et al. D24/107
D404,140 S * 1/1999 Meguro D24/232
D427,315 S * 6/2000 Saltzstein et al. D24/186
D446,306 S * 8/2001 Ochi et al. D24/186

D477,084 S * 7/2003 Menezes et al. D24/172
D489,816 S * 5/2004 Ross D24/107
D490,516 S * 5/2004 Takahashi et al. D24/107
D503,807 S * 4/2005 Ryan D24/200
D536,793 S * 2/2007 Assad et al. D24/185
D573,051 S * 7/2008 Alden et al. D10/81
D584,975 S * 1/2009 Haberstroh D10/81
D597,216 S * 7/2009 McGuigan et al. D24/216
D598,551 S * 8/2009 Miwa et al. D24/186
D609,343 S * 2/2010 Omaki D24/165
D609,344 S * 2/2010 Hara D24/165
D647,209 S * 10/2011 Muller et al. D24/216
D651,319 S * 12/2011 Hara D24/165

* cited by examiner

Primary Examiner — T. Chase Nelson

Assistant Examiner — Mark Cavanna

(74) *Attorney, Agent, or Firm* — Lathrop & Gage LLP

(57) **CLAIM**

The ornamental design for a diagnostic cartridge reader, as
shown and described.

DESCRIPTION

FIG. 1 is a front perspective view of the diagnostic cartridge
reader, showing the new design;

FIG. 2 is a front elevation of the diagnostic cartridge reader;
FIG. 3 is a side elevation of the diagnostic cartridge reader, an
opposing side elevation of the diagnostic cartridge reader
being a mirror image thereof;

FIG. 4 is atop plan view of the diagnostic cartridge reader;



FIG. 5 is a rear elevation of the diagnostic cartridge reader;

FIG. 6 is a bottom plan view of the diagnostic cartridge
reader; and,

FIG. 7 is a rear perspective view of the diagnostic cartridge
reader.

In all of FIGS. 1 through 7, dashed lines indicate environmen-
tal structure that forms no part of the claimed design.

1 Claim, 7 Drawing Sheets

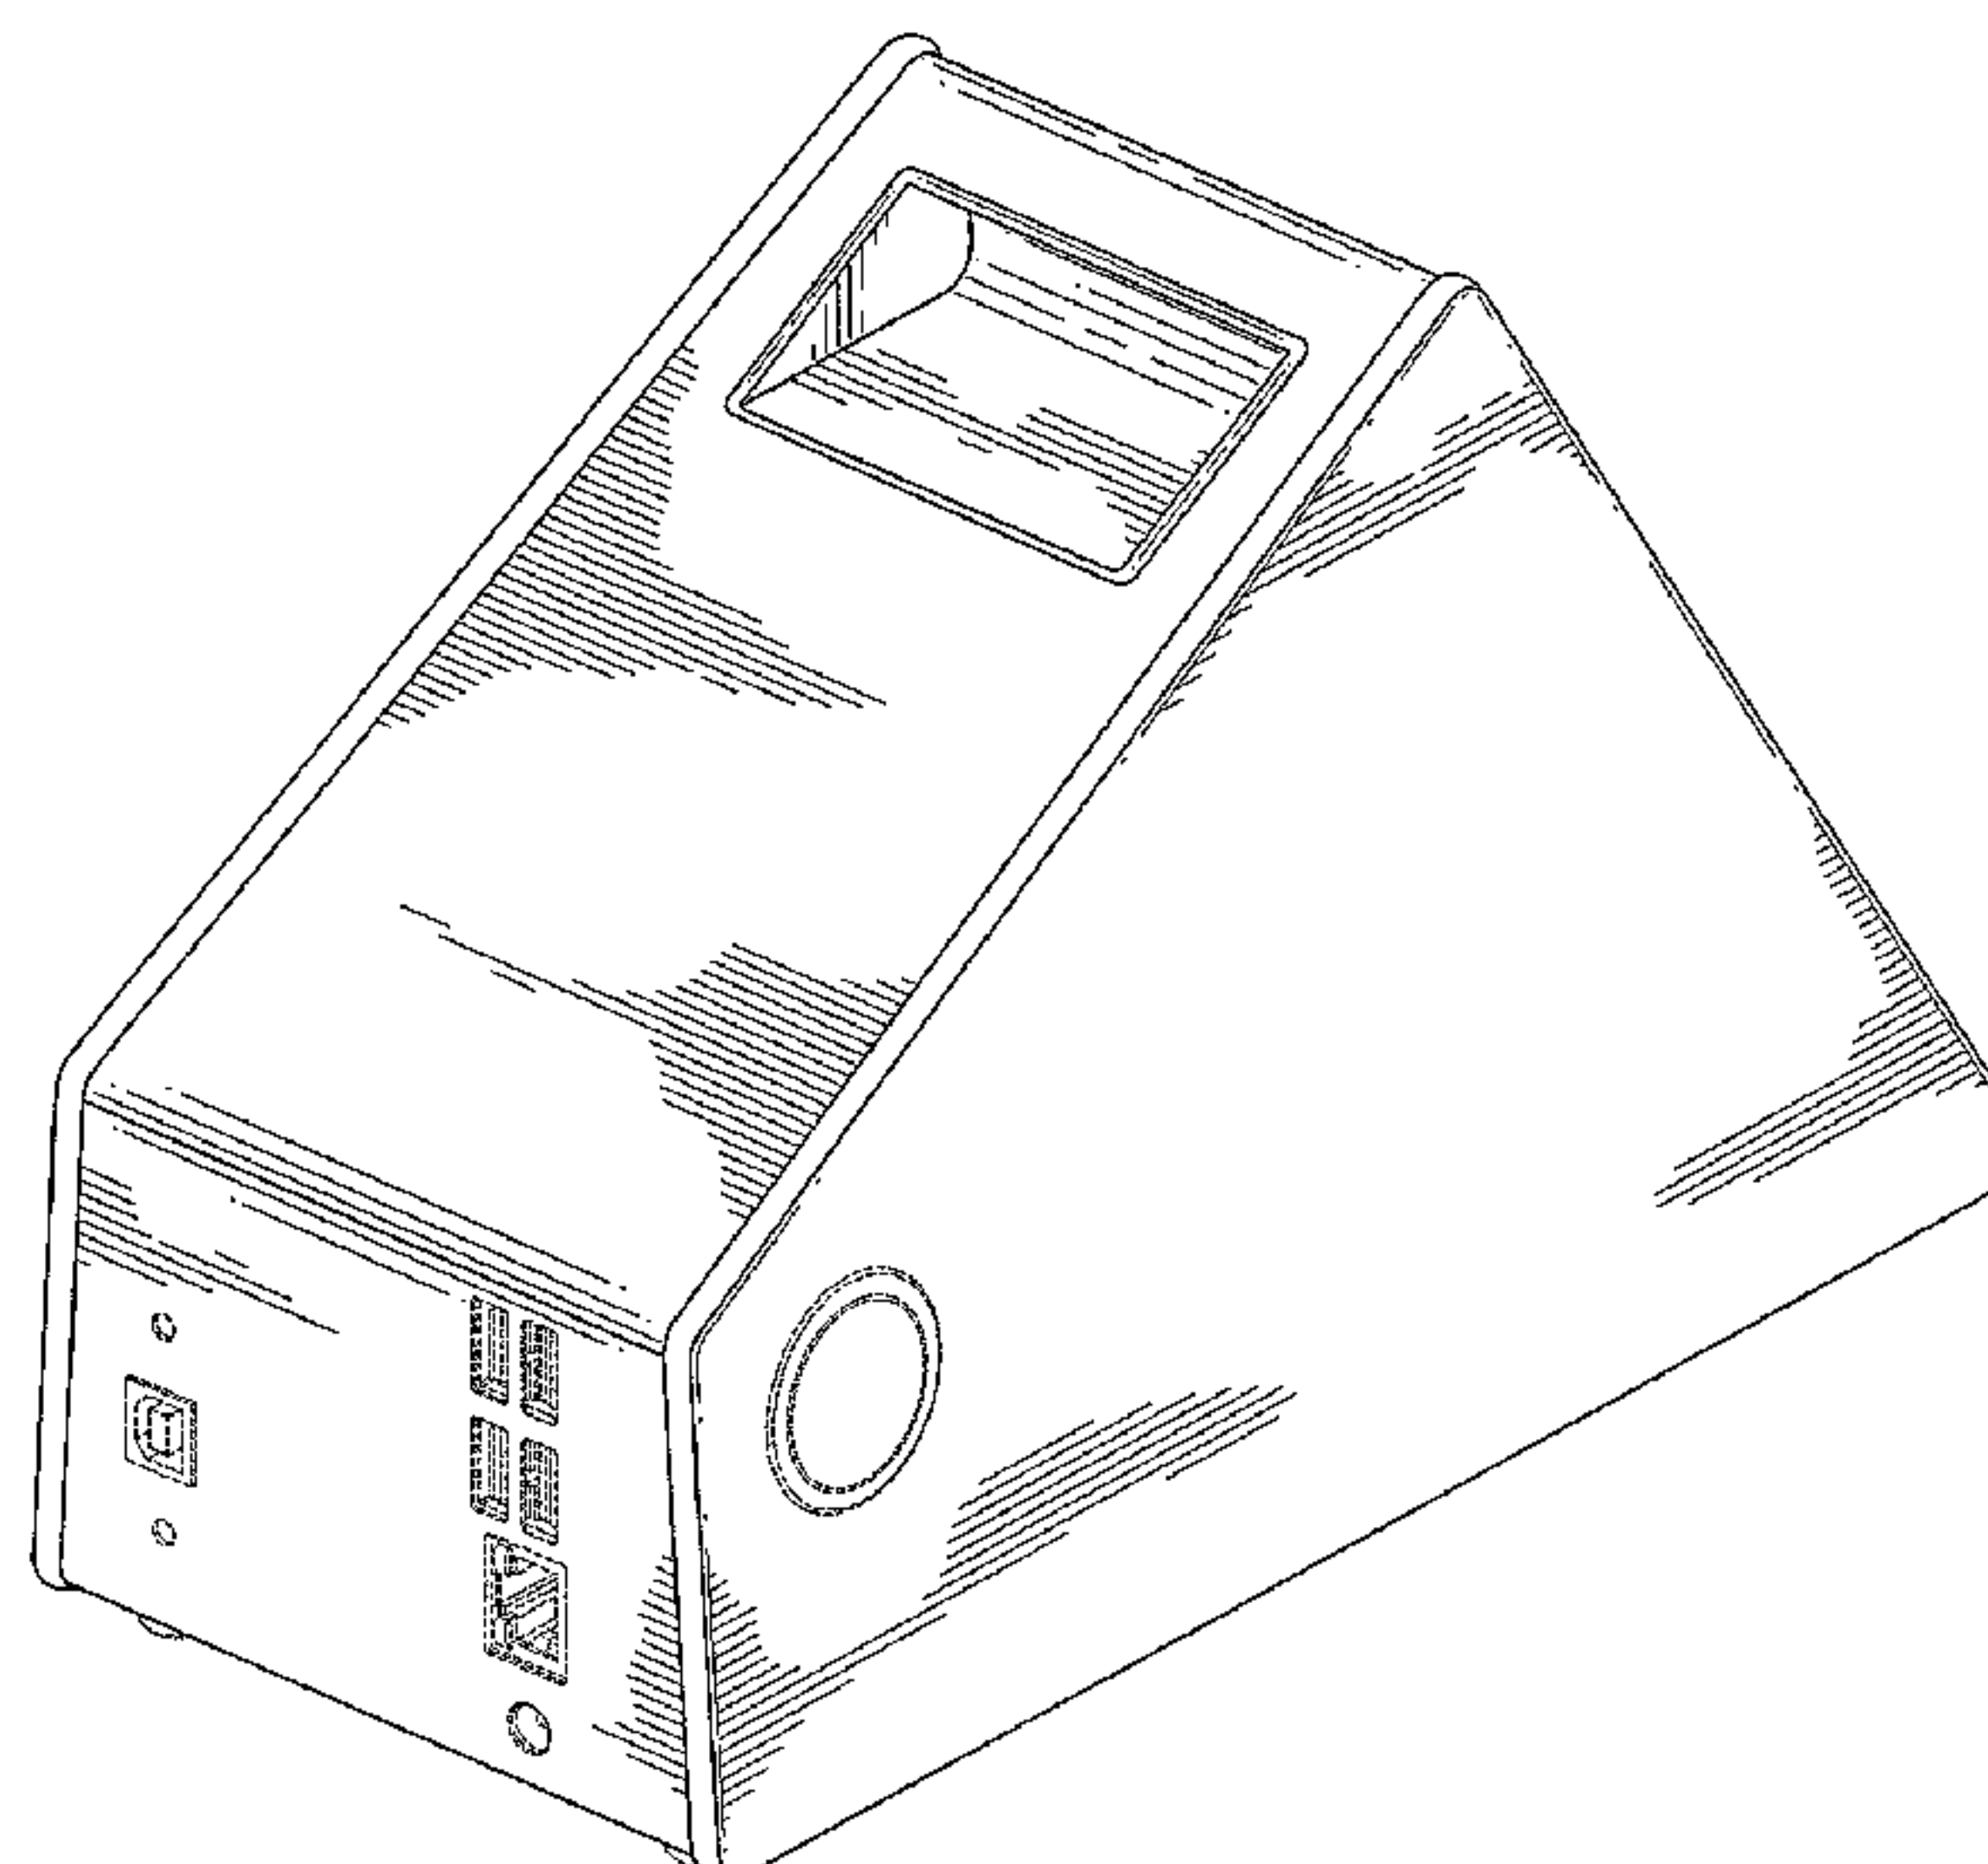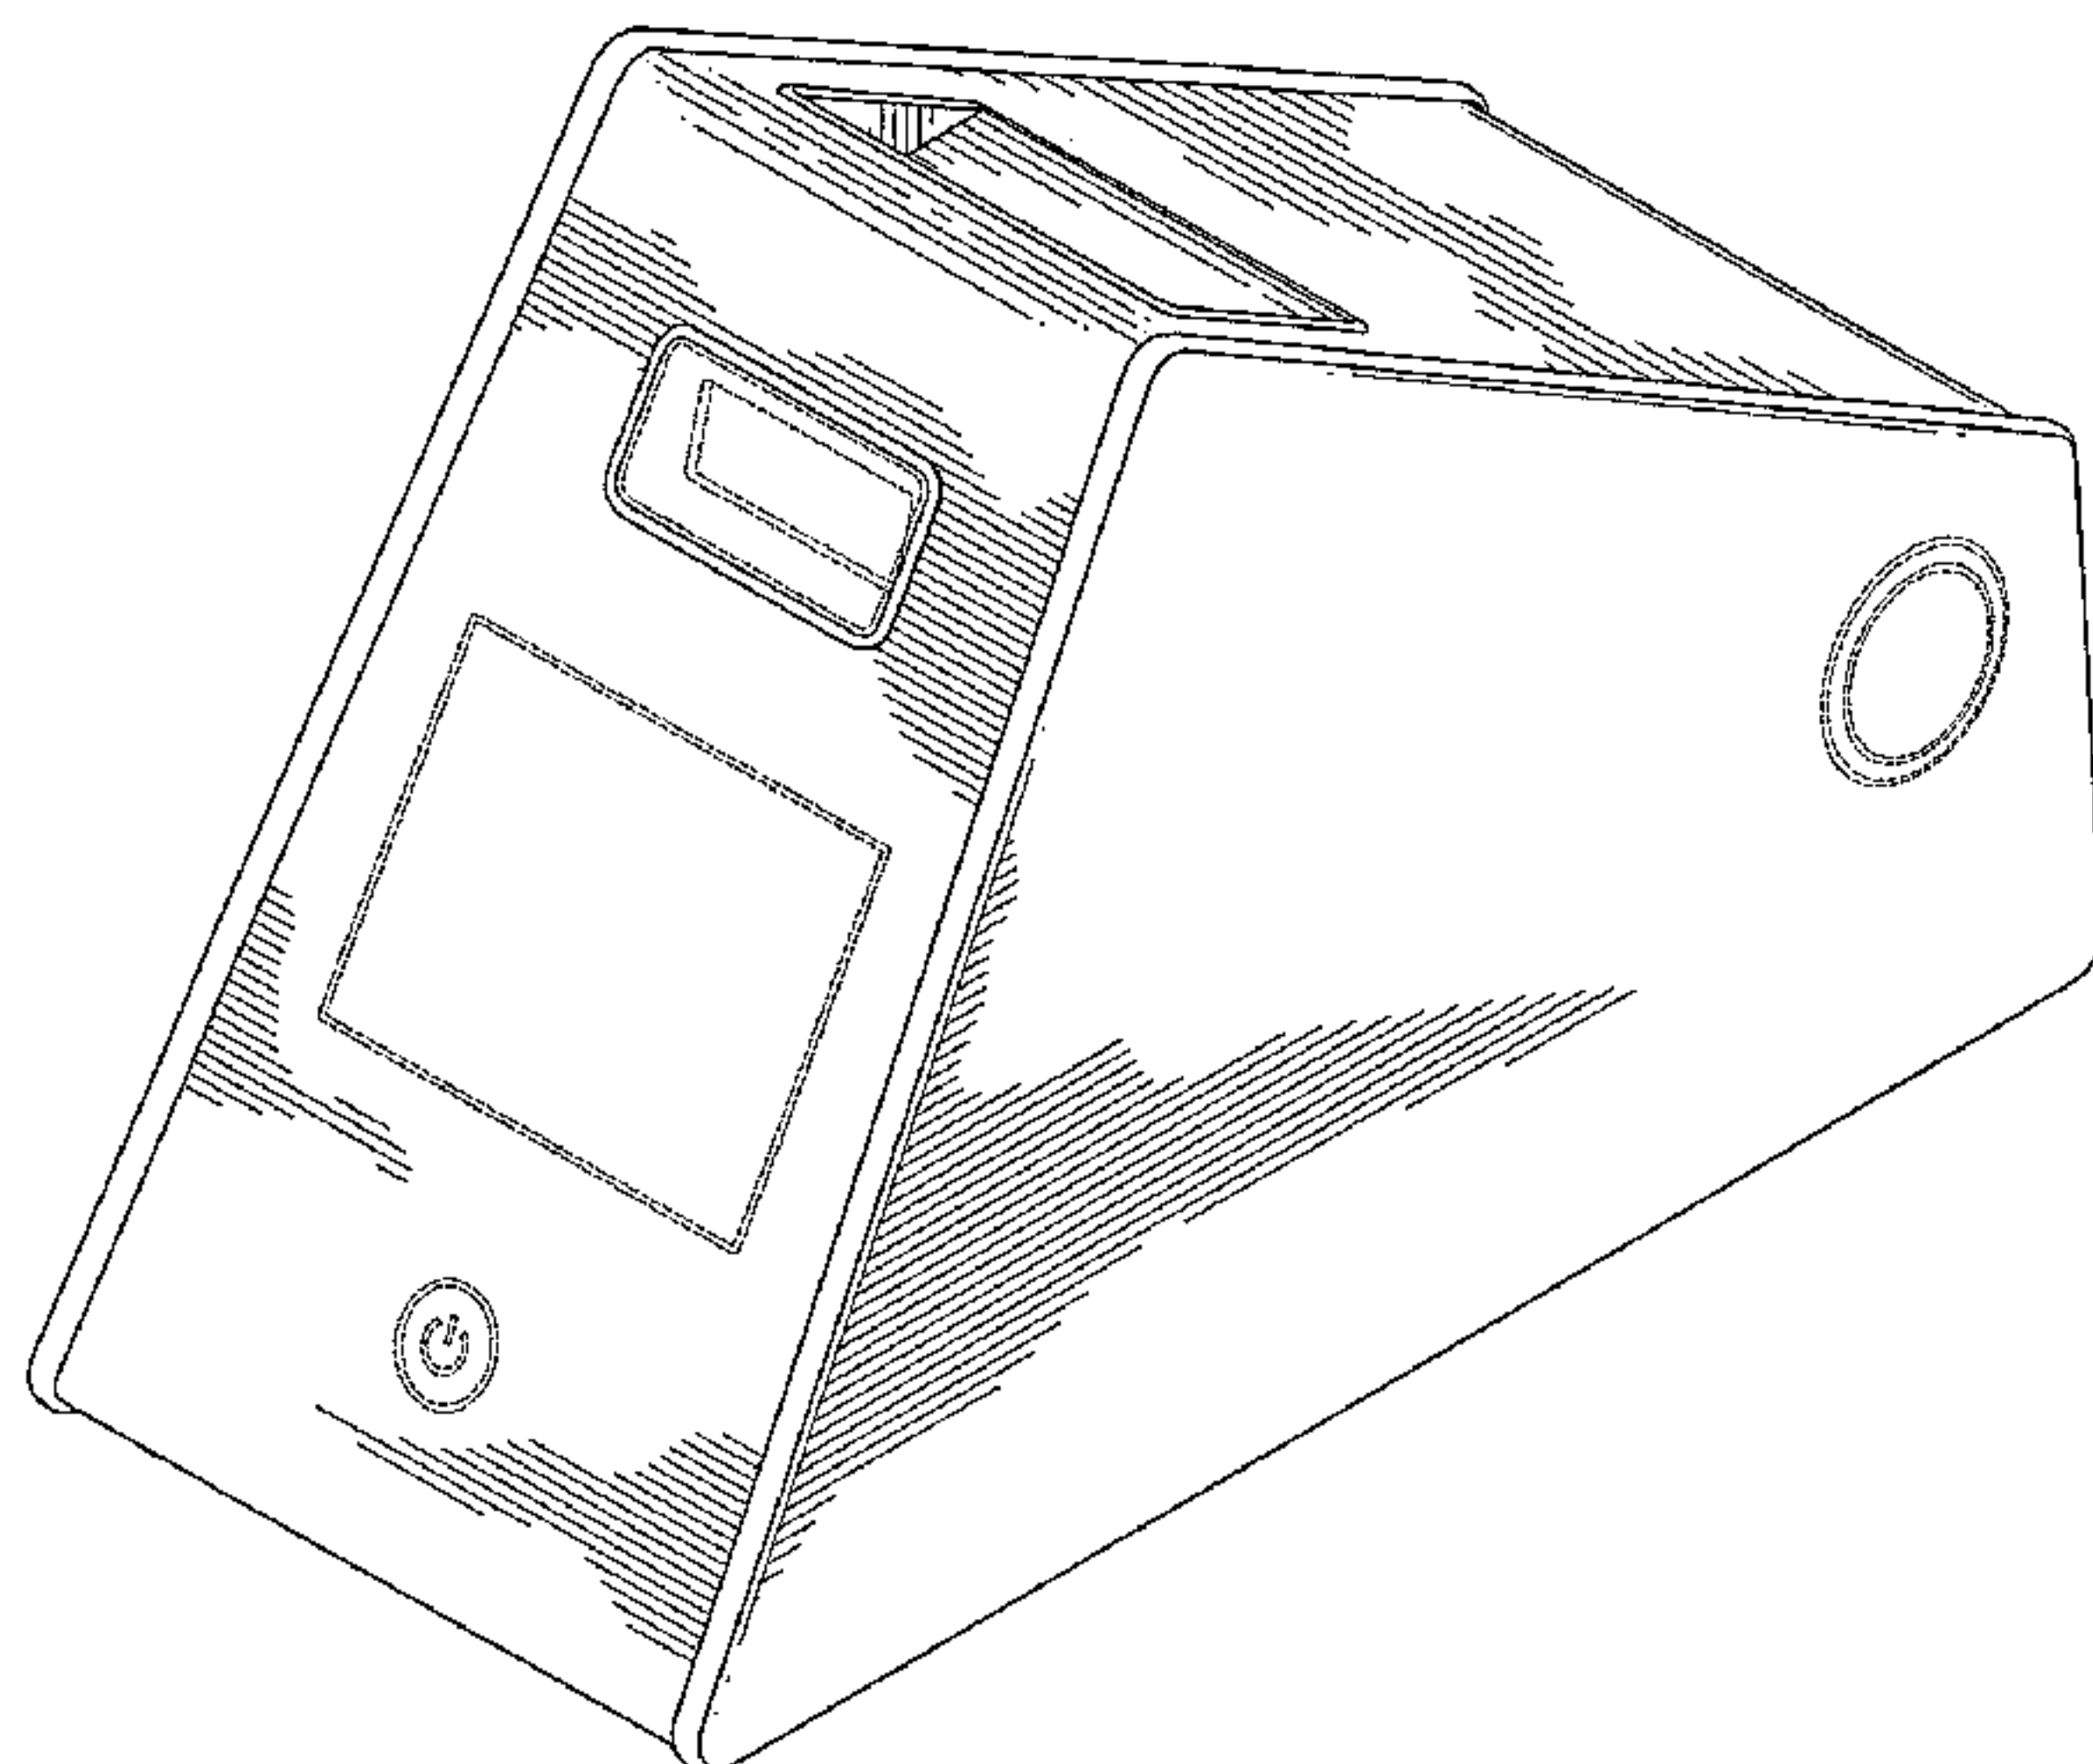

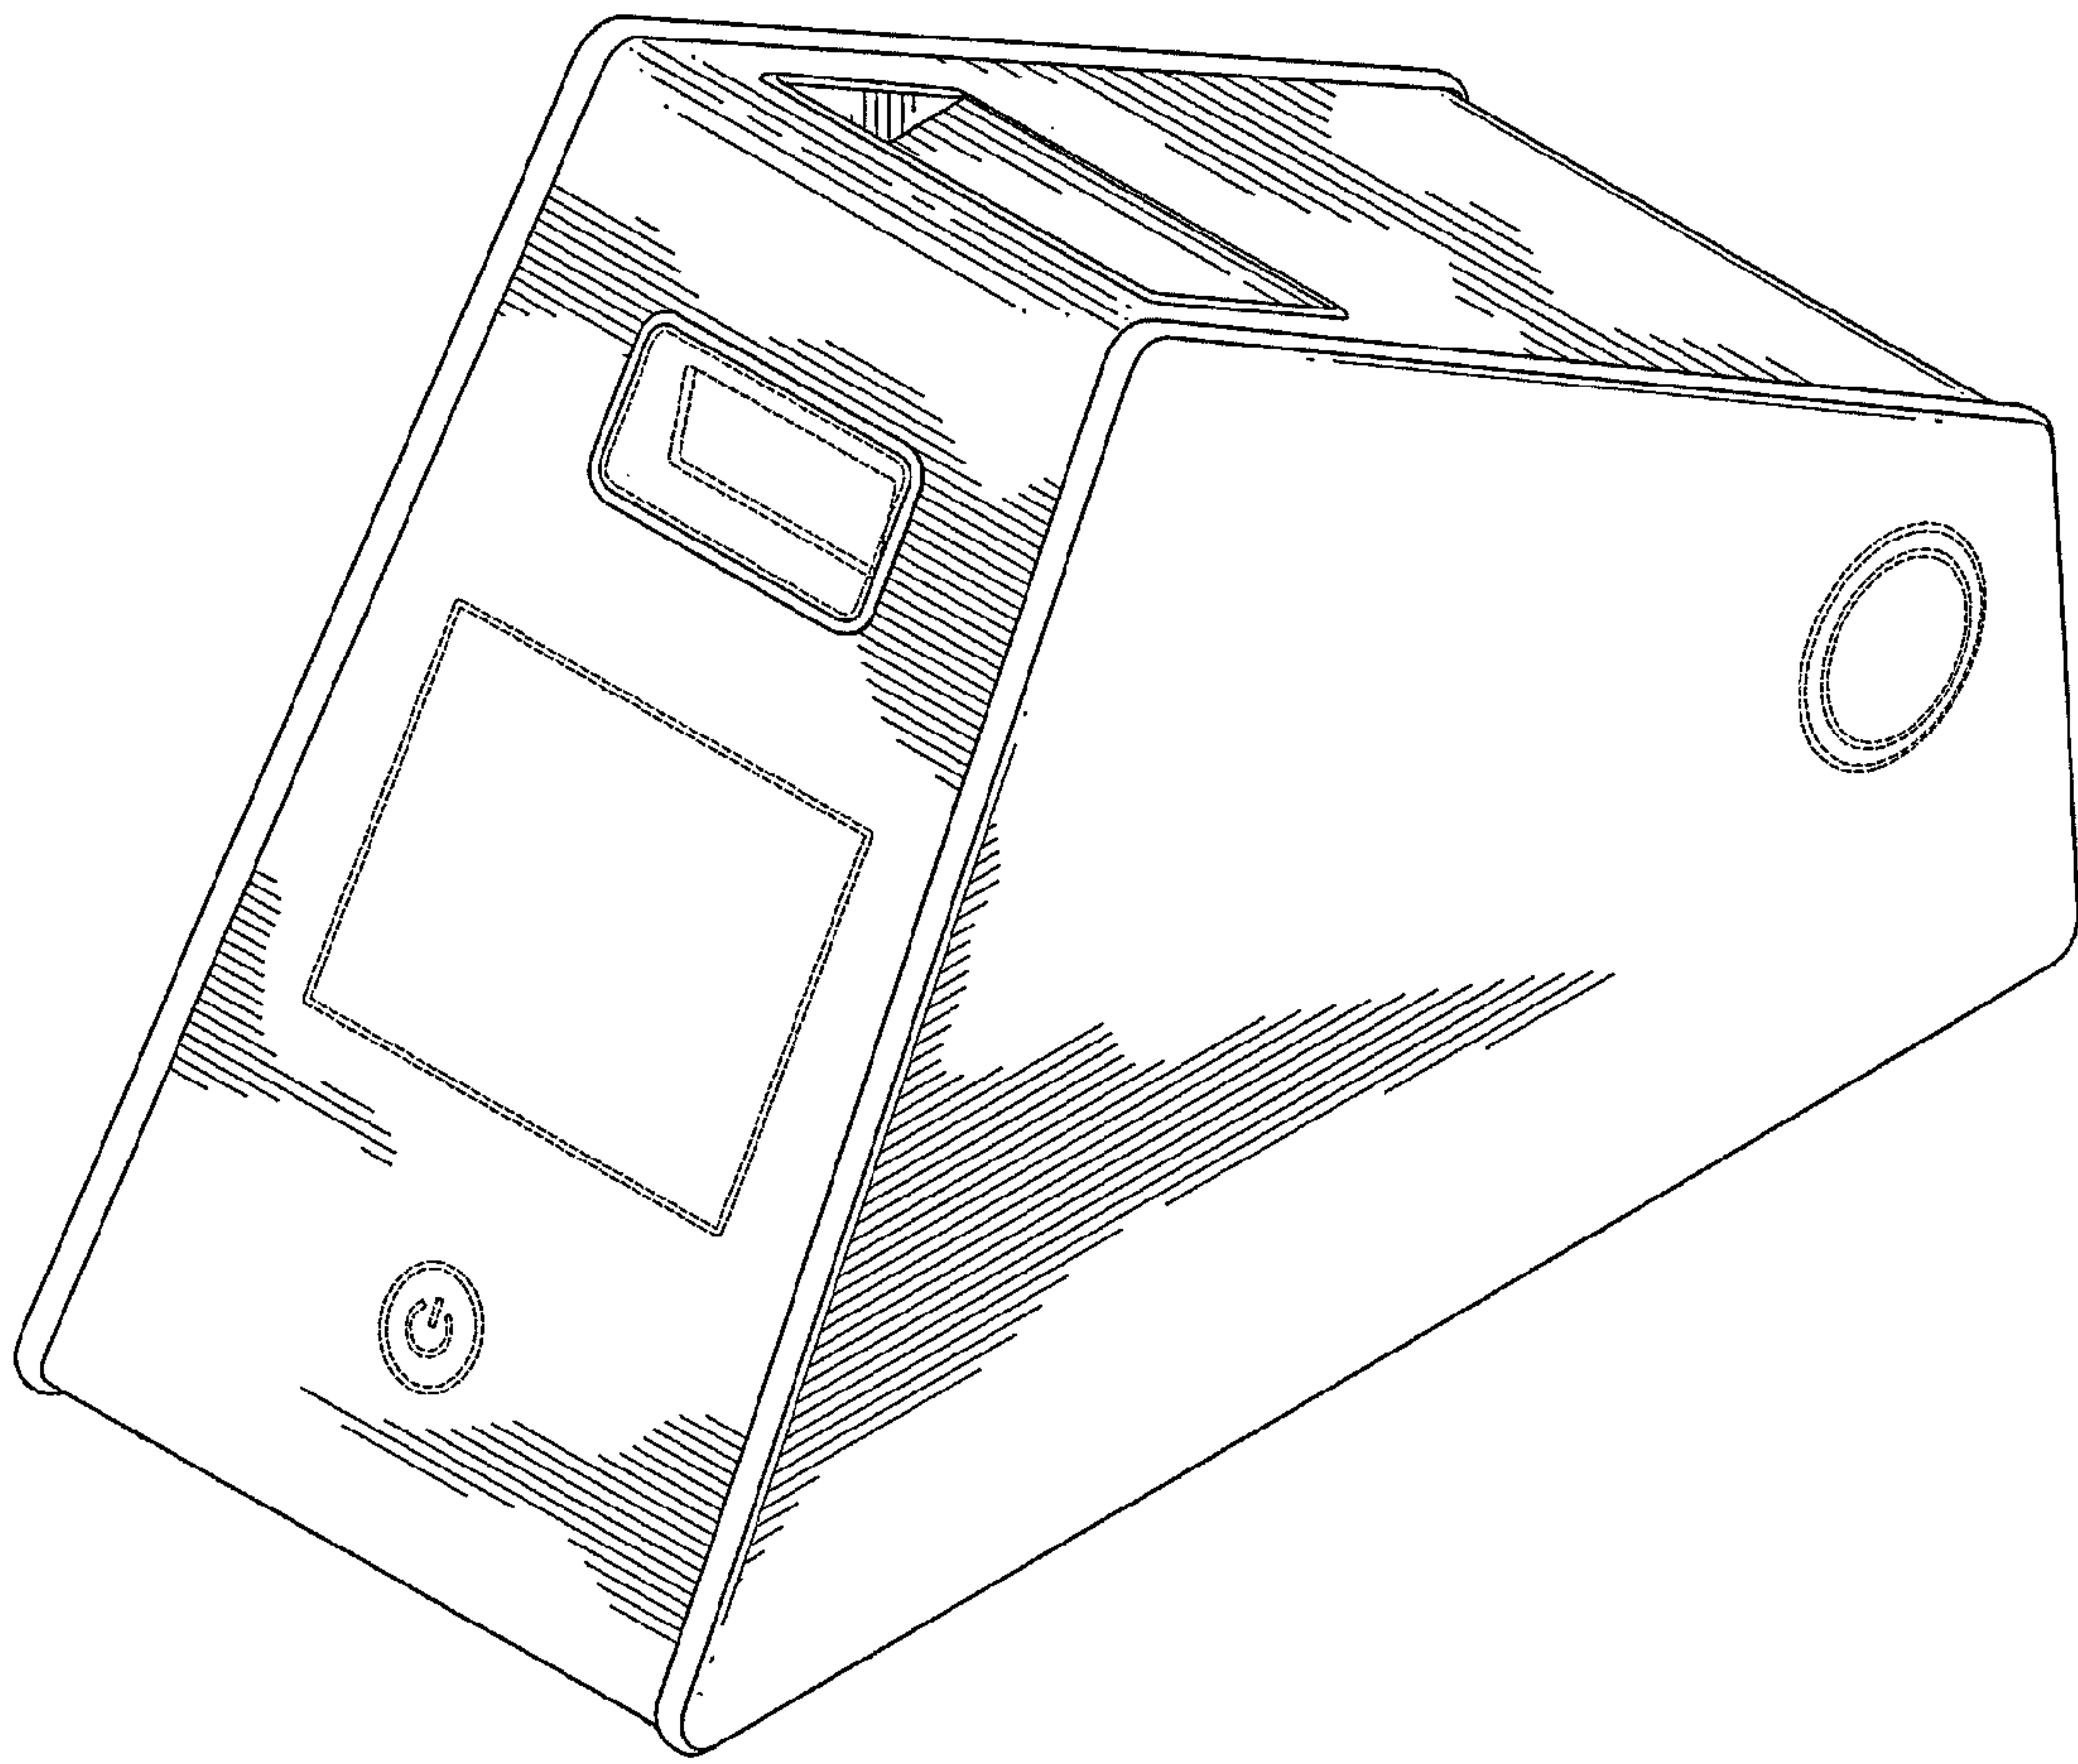


FIG. 1

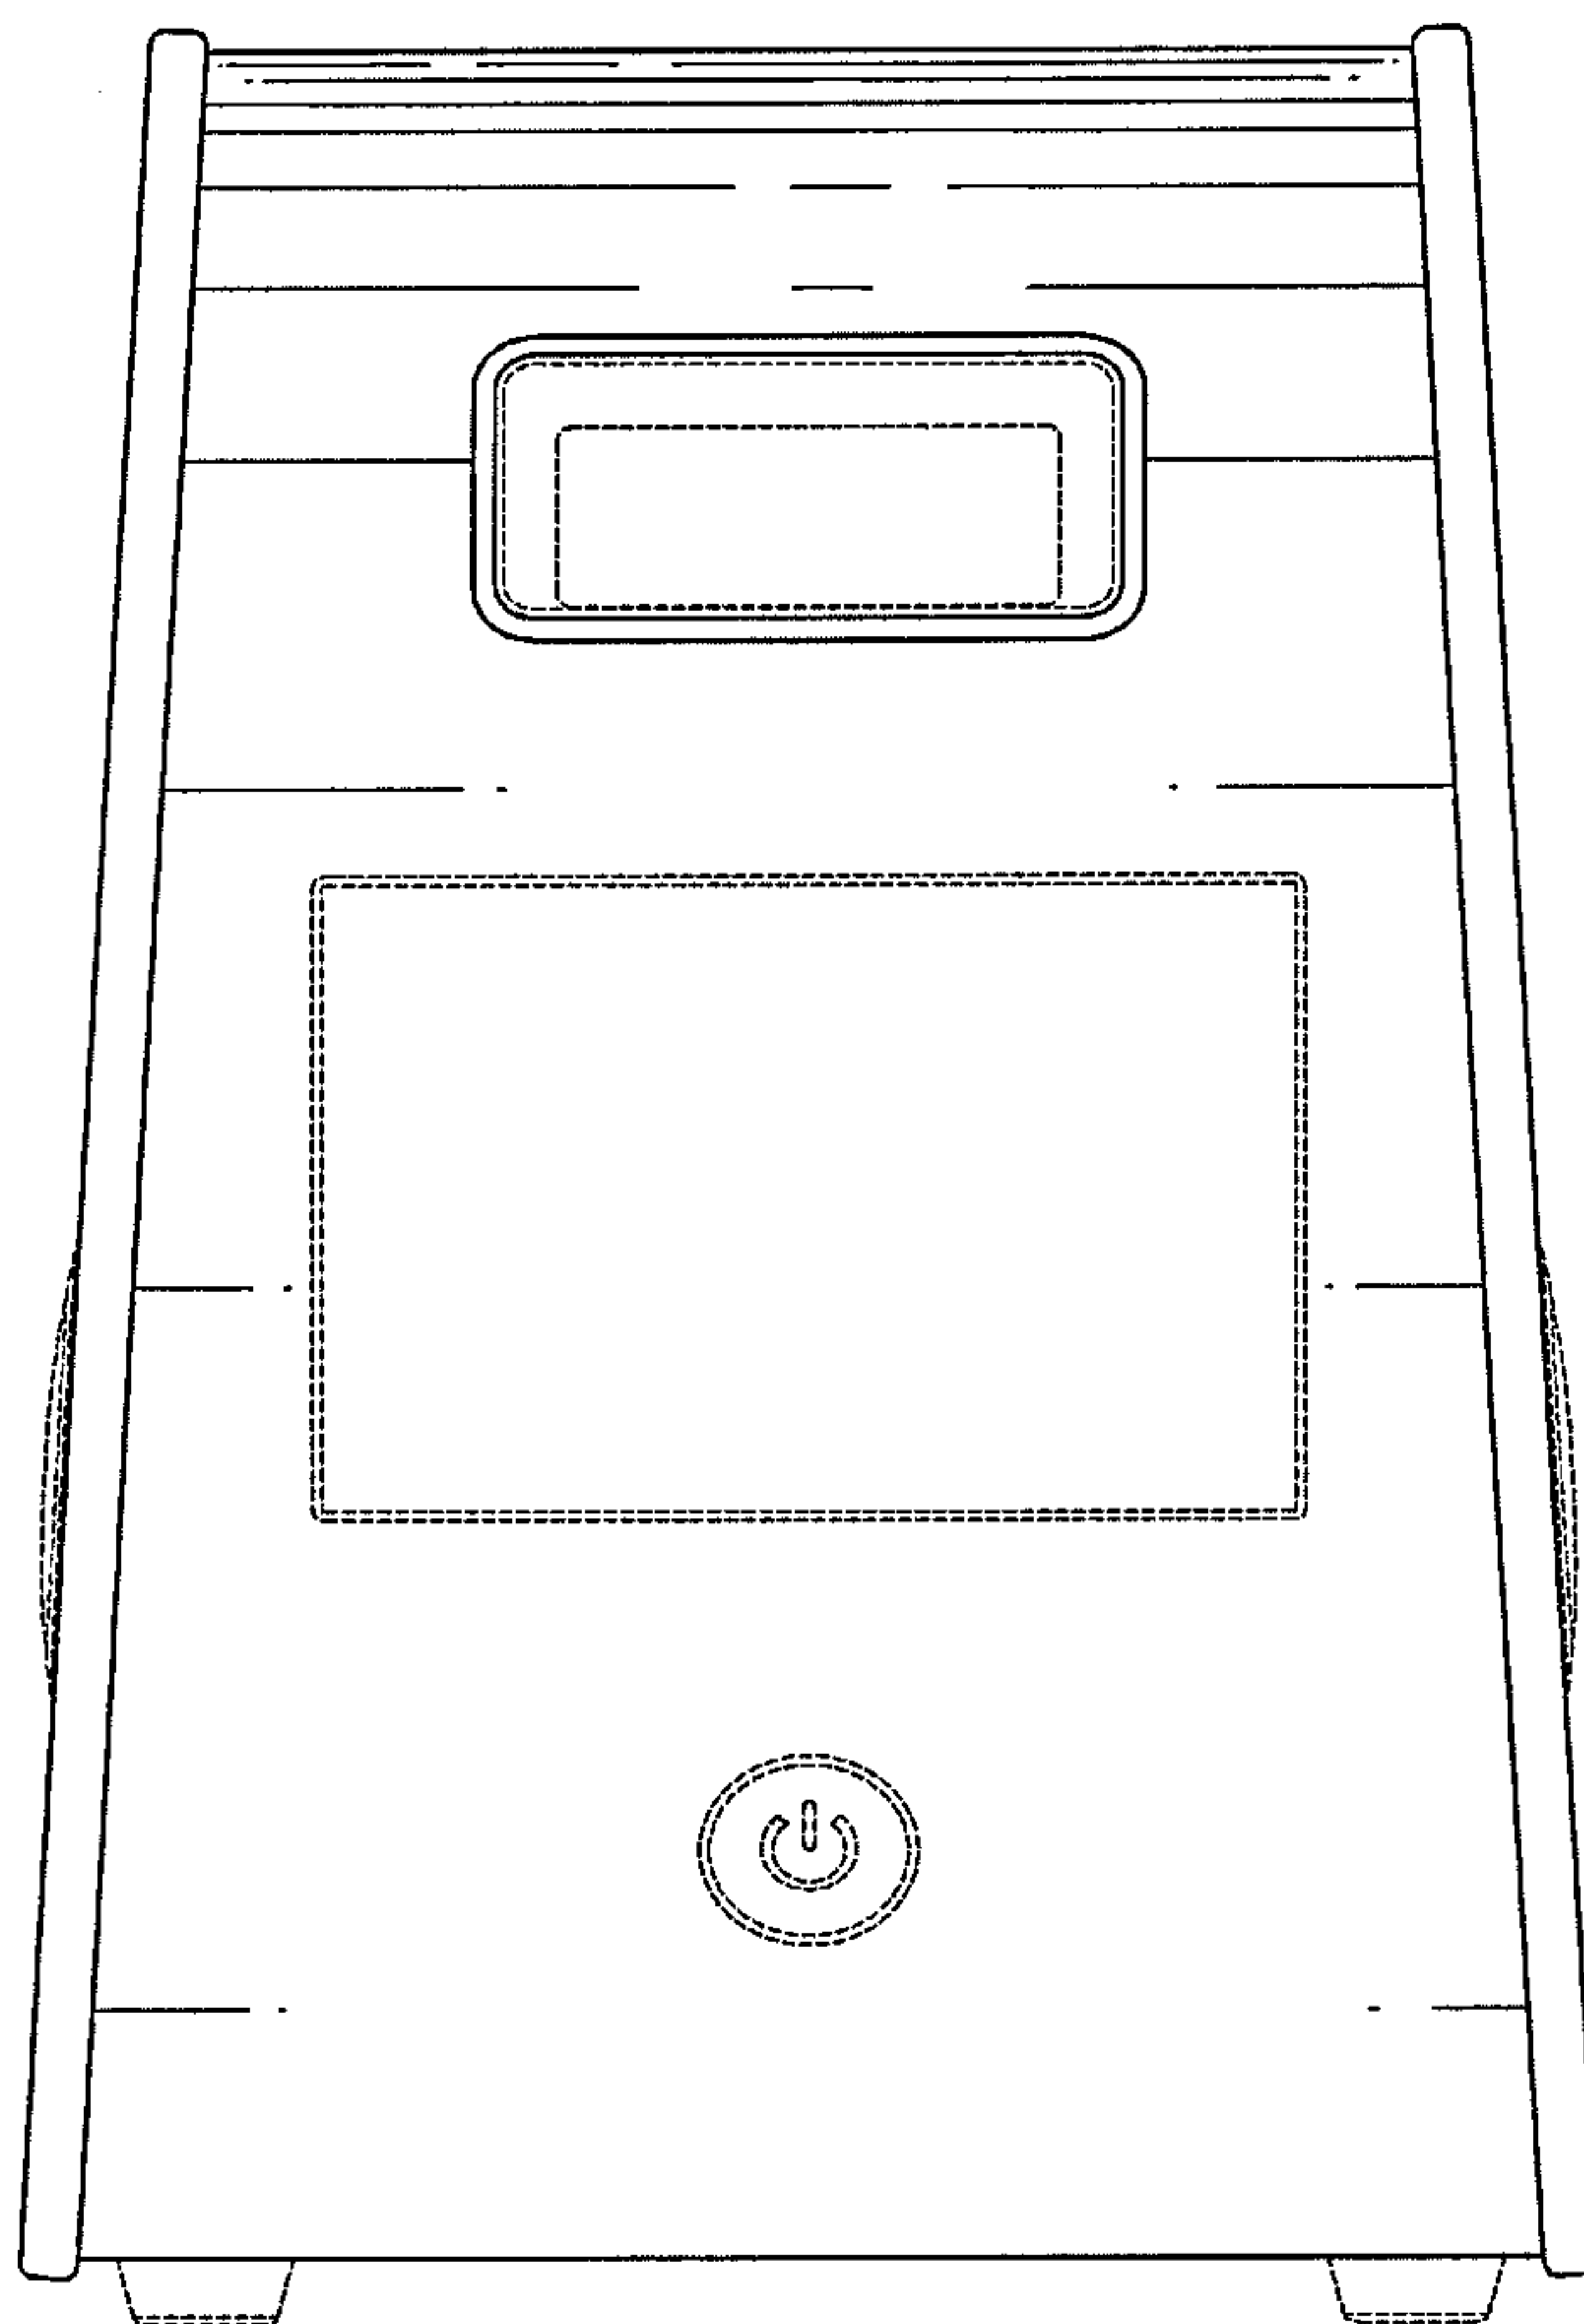


FIG. 2

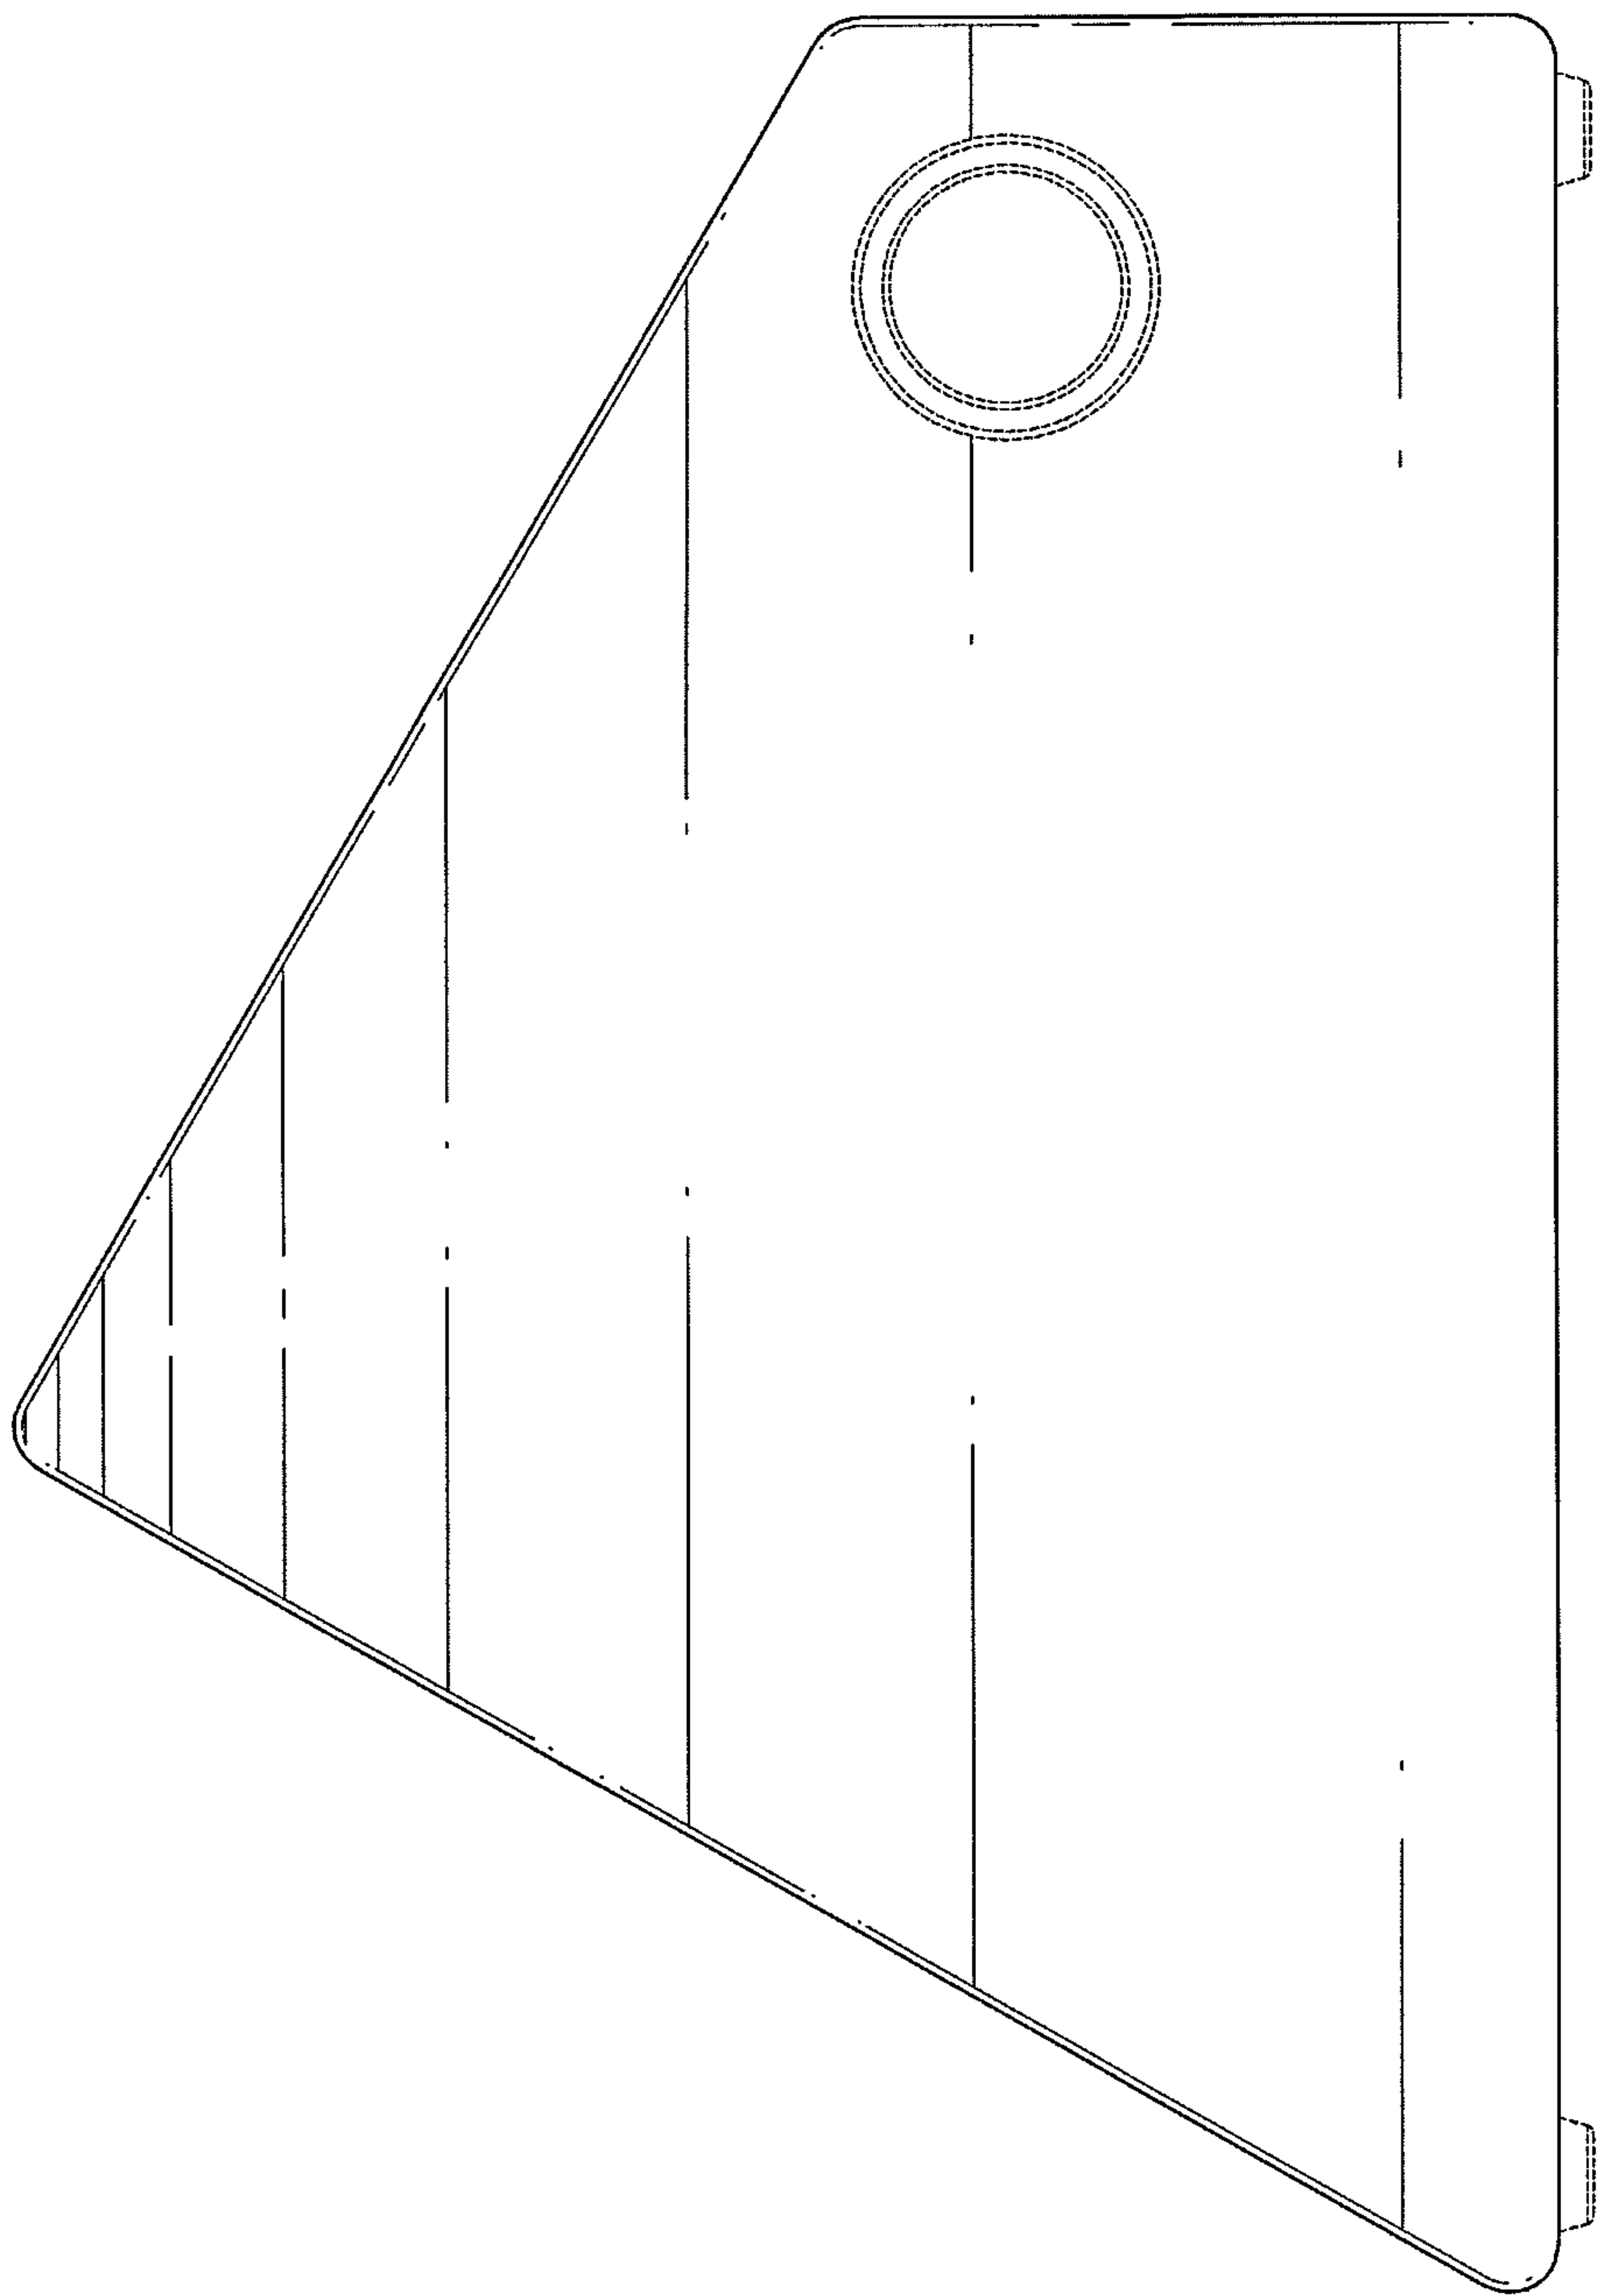


FIG. 3

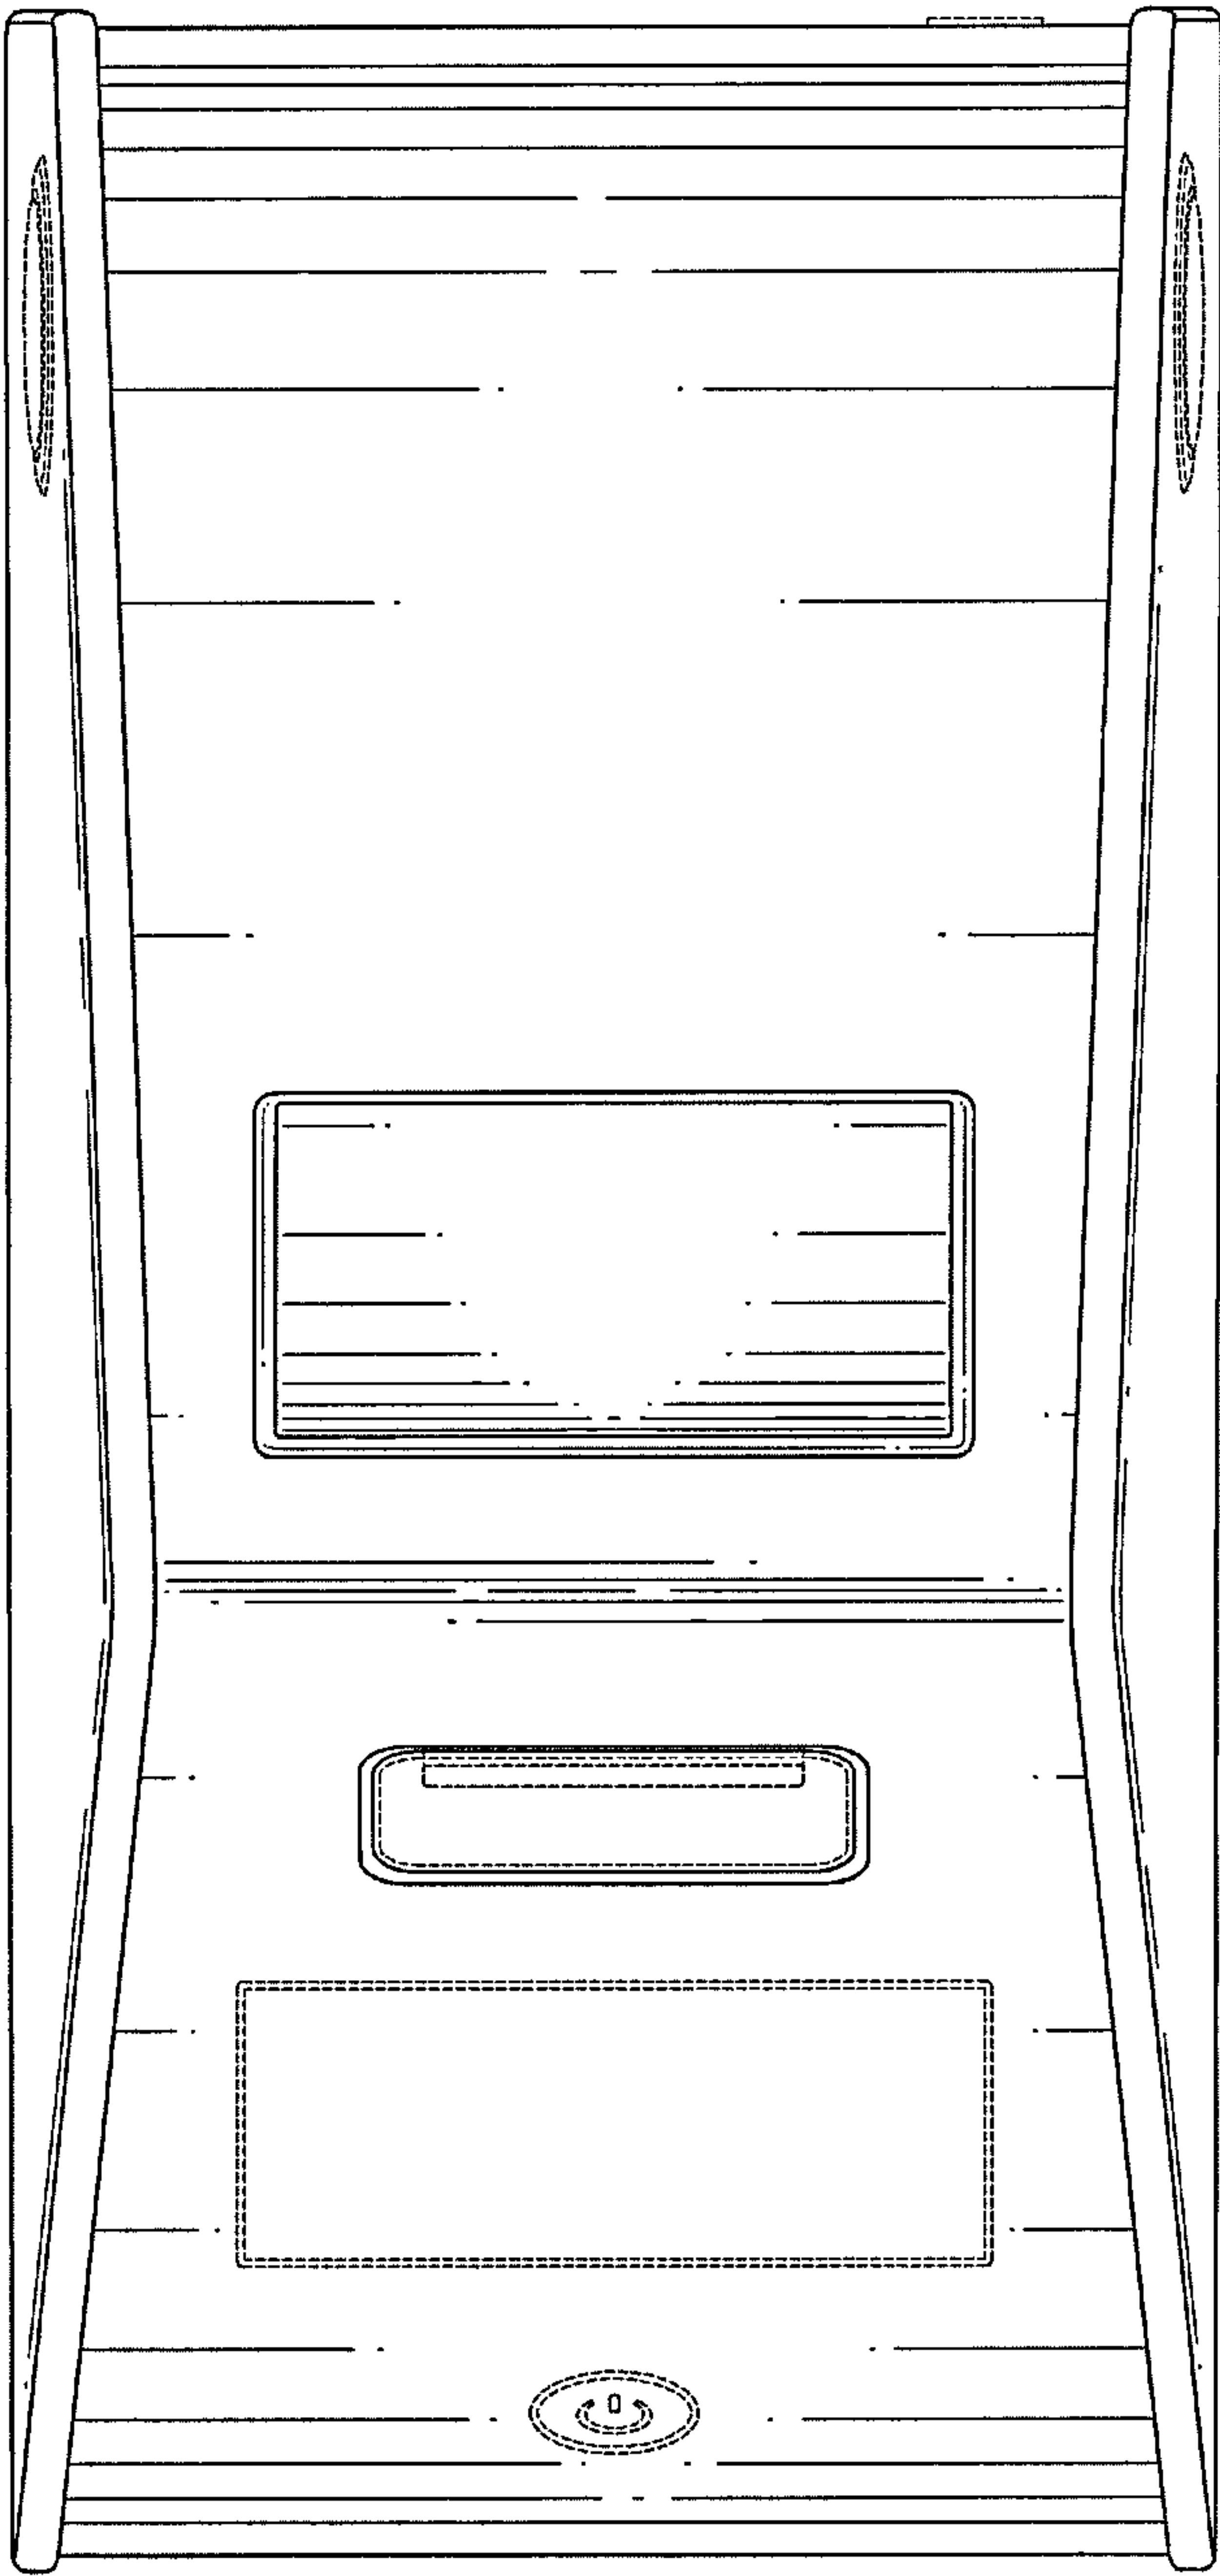


FIG.4

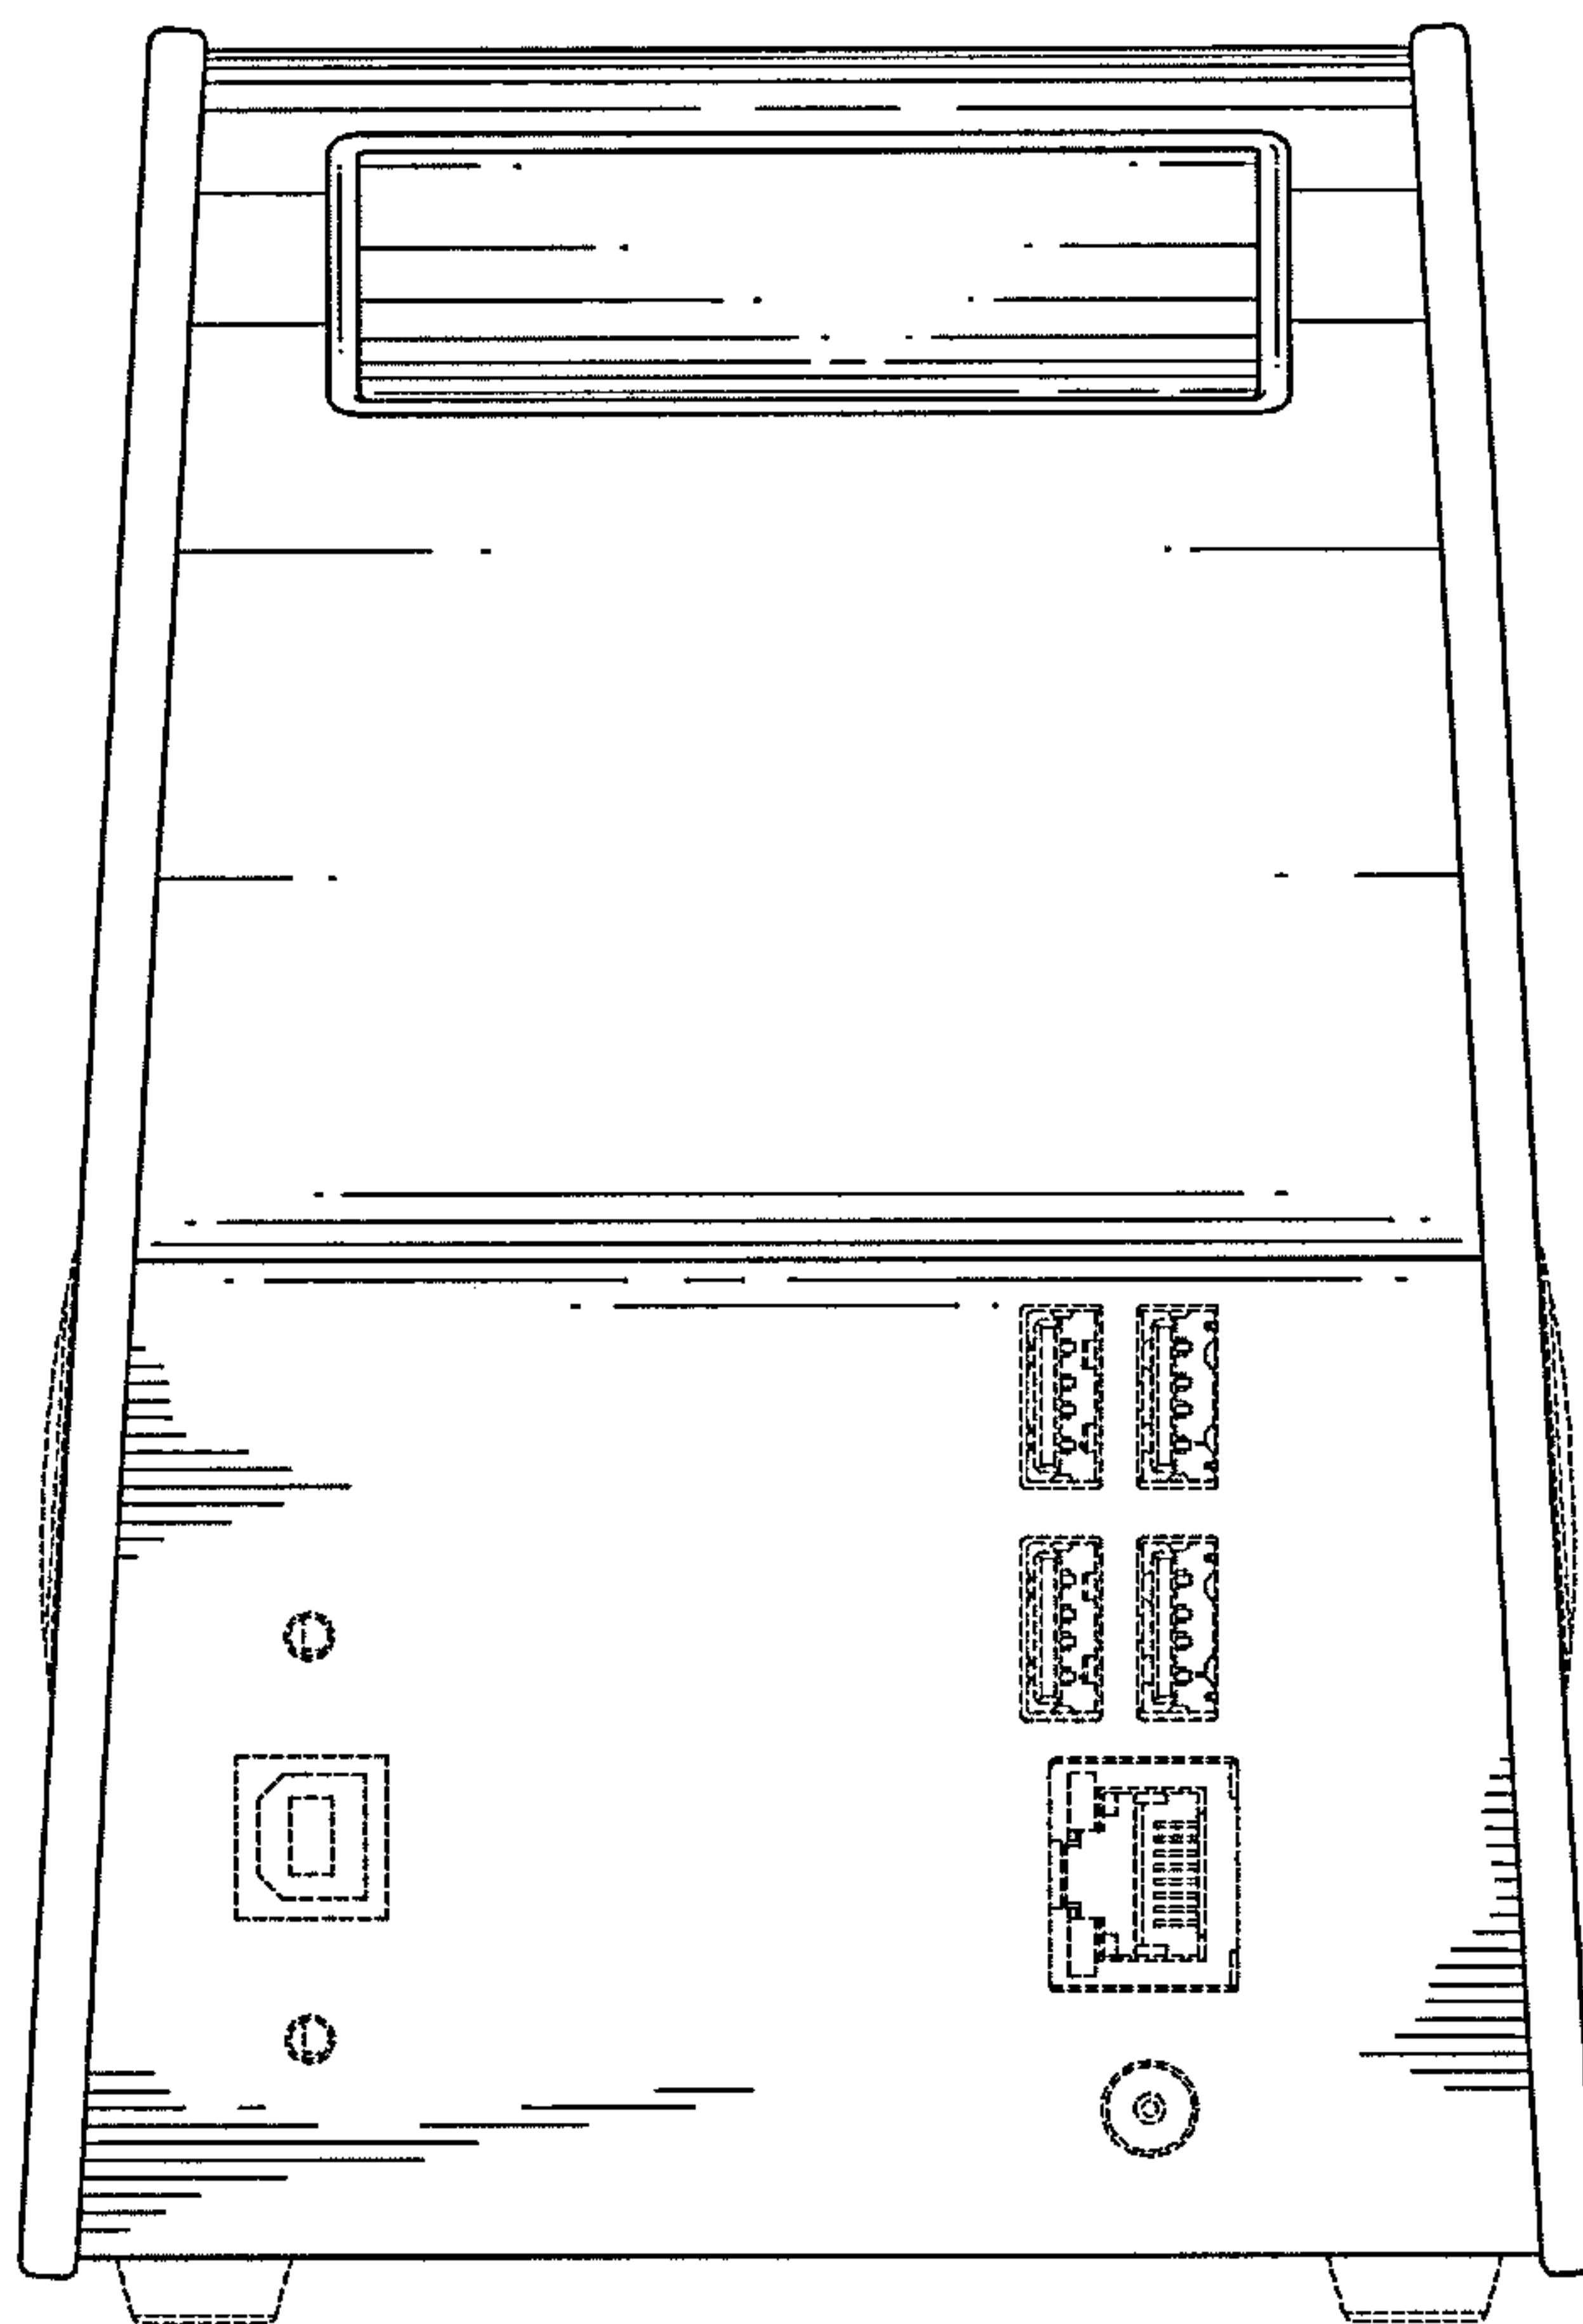


FIG. 5

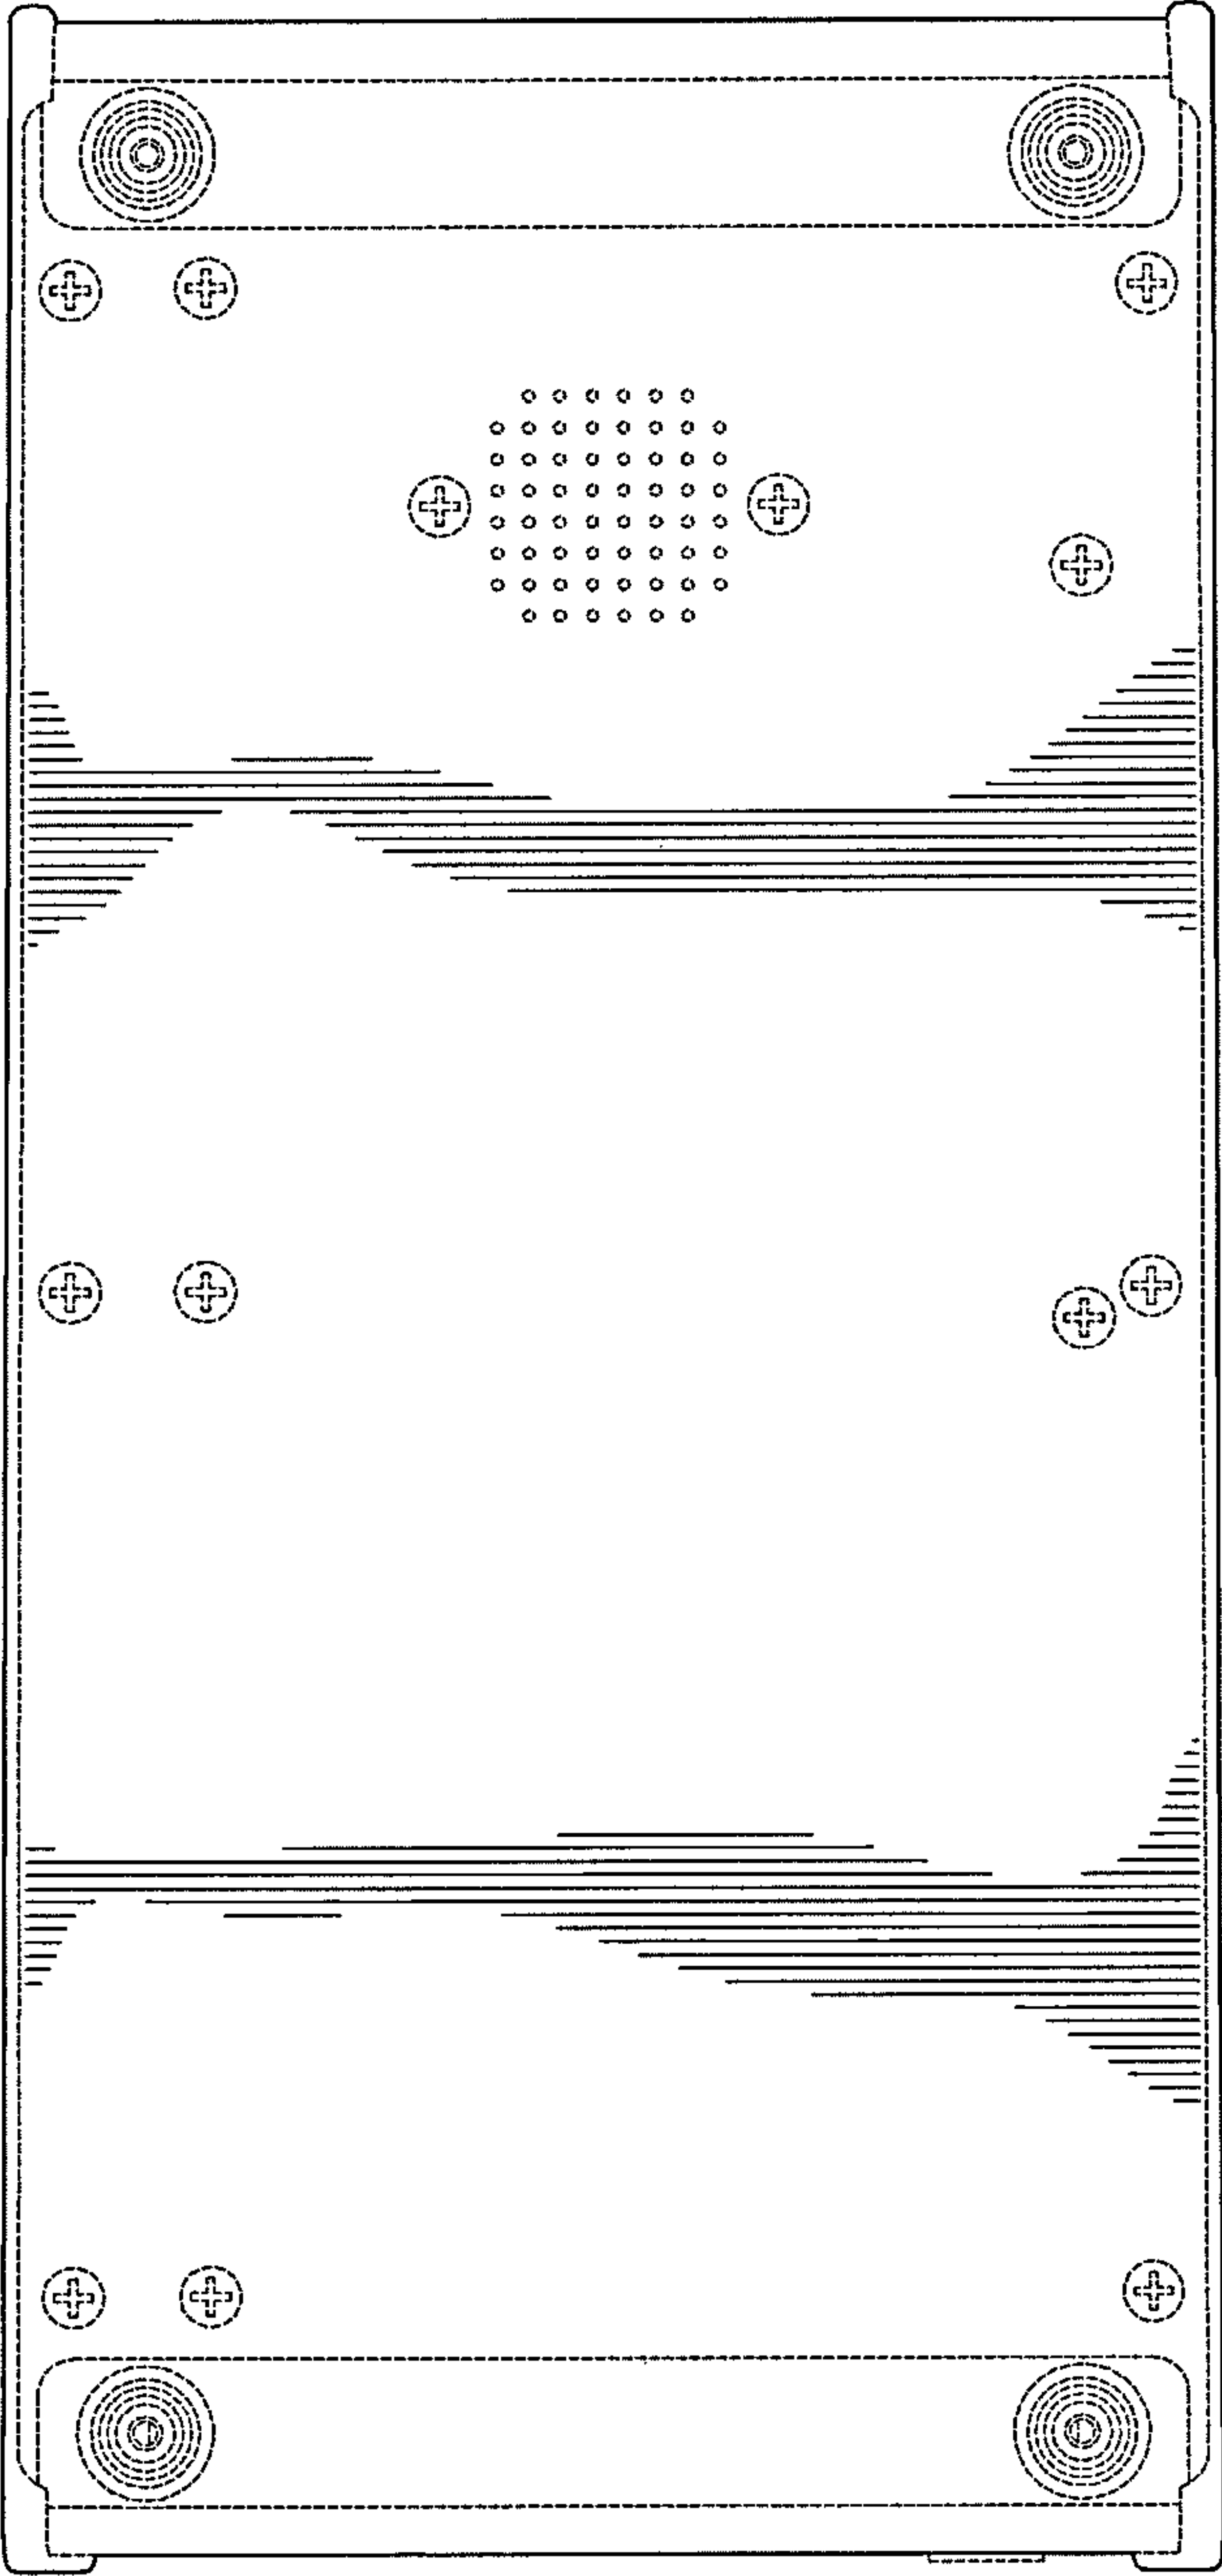


FIG. 6

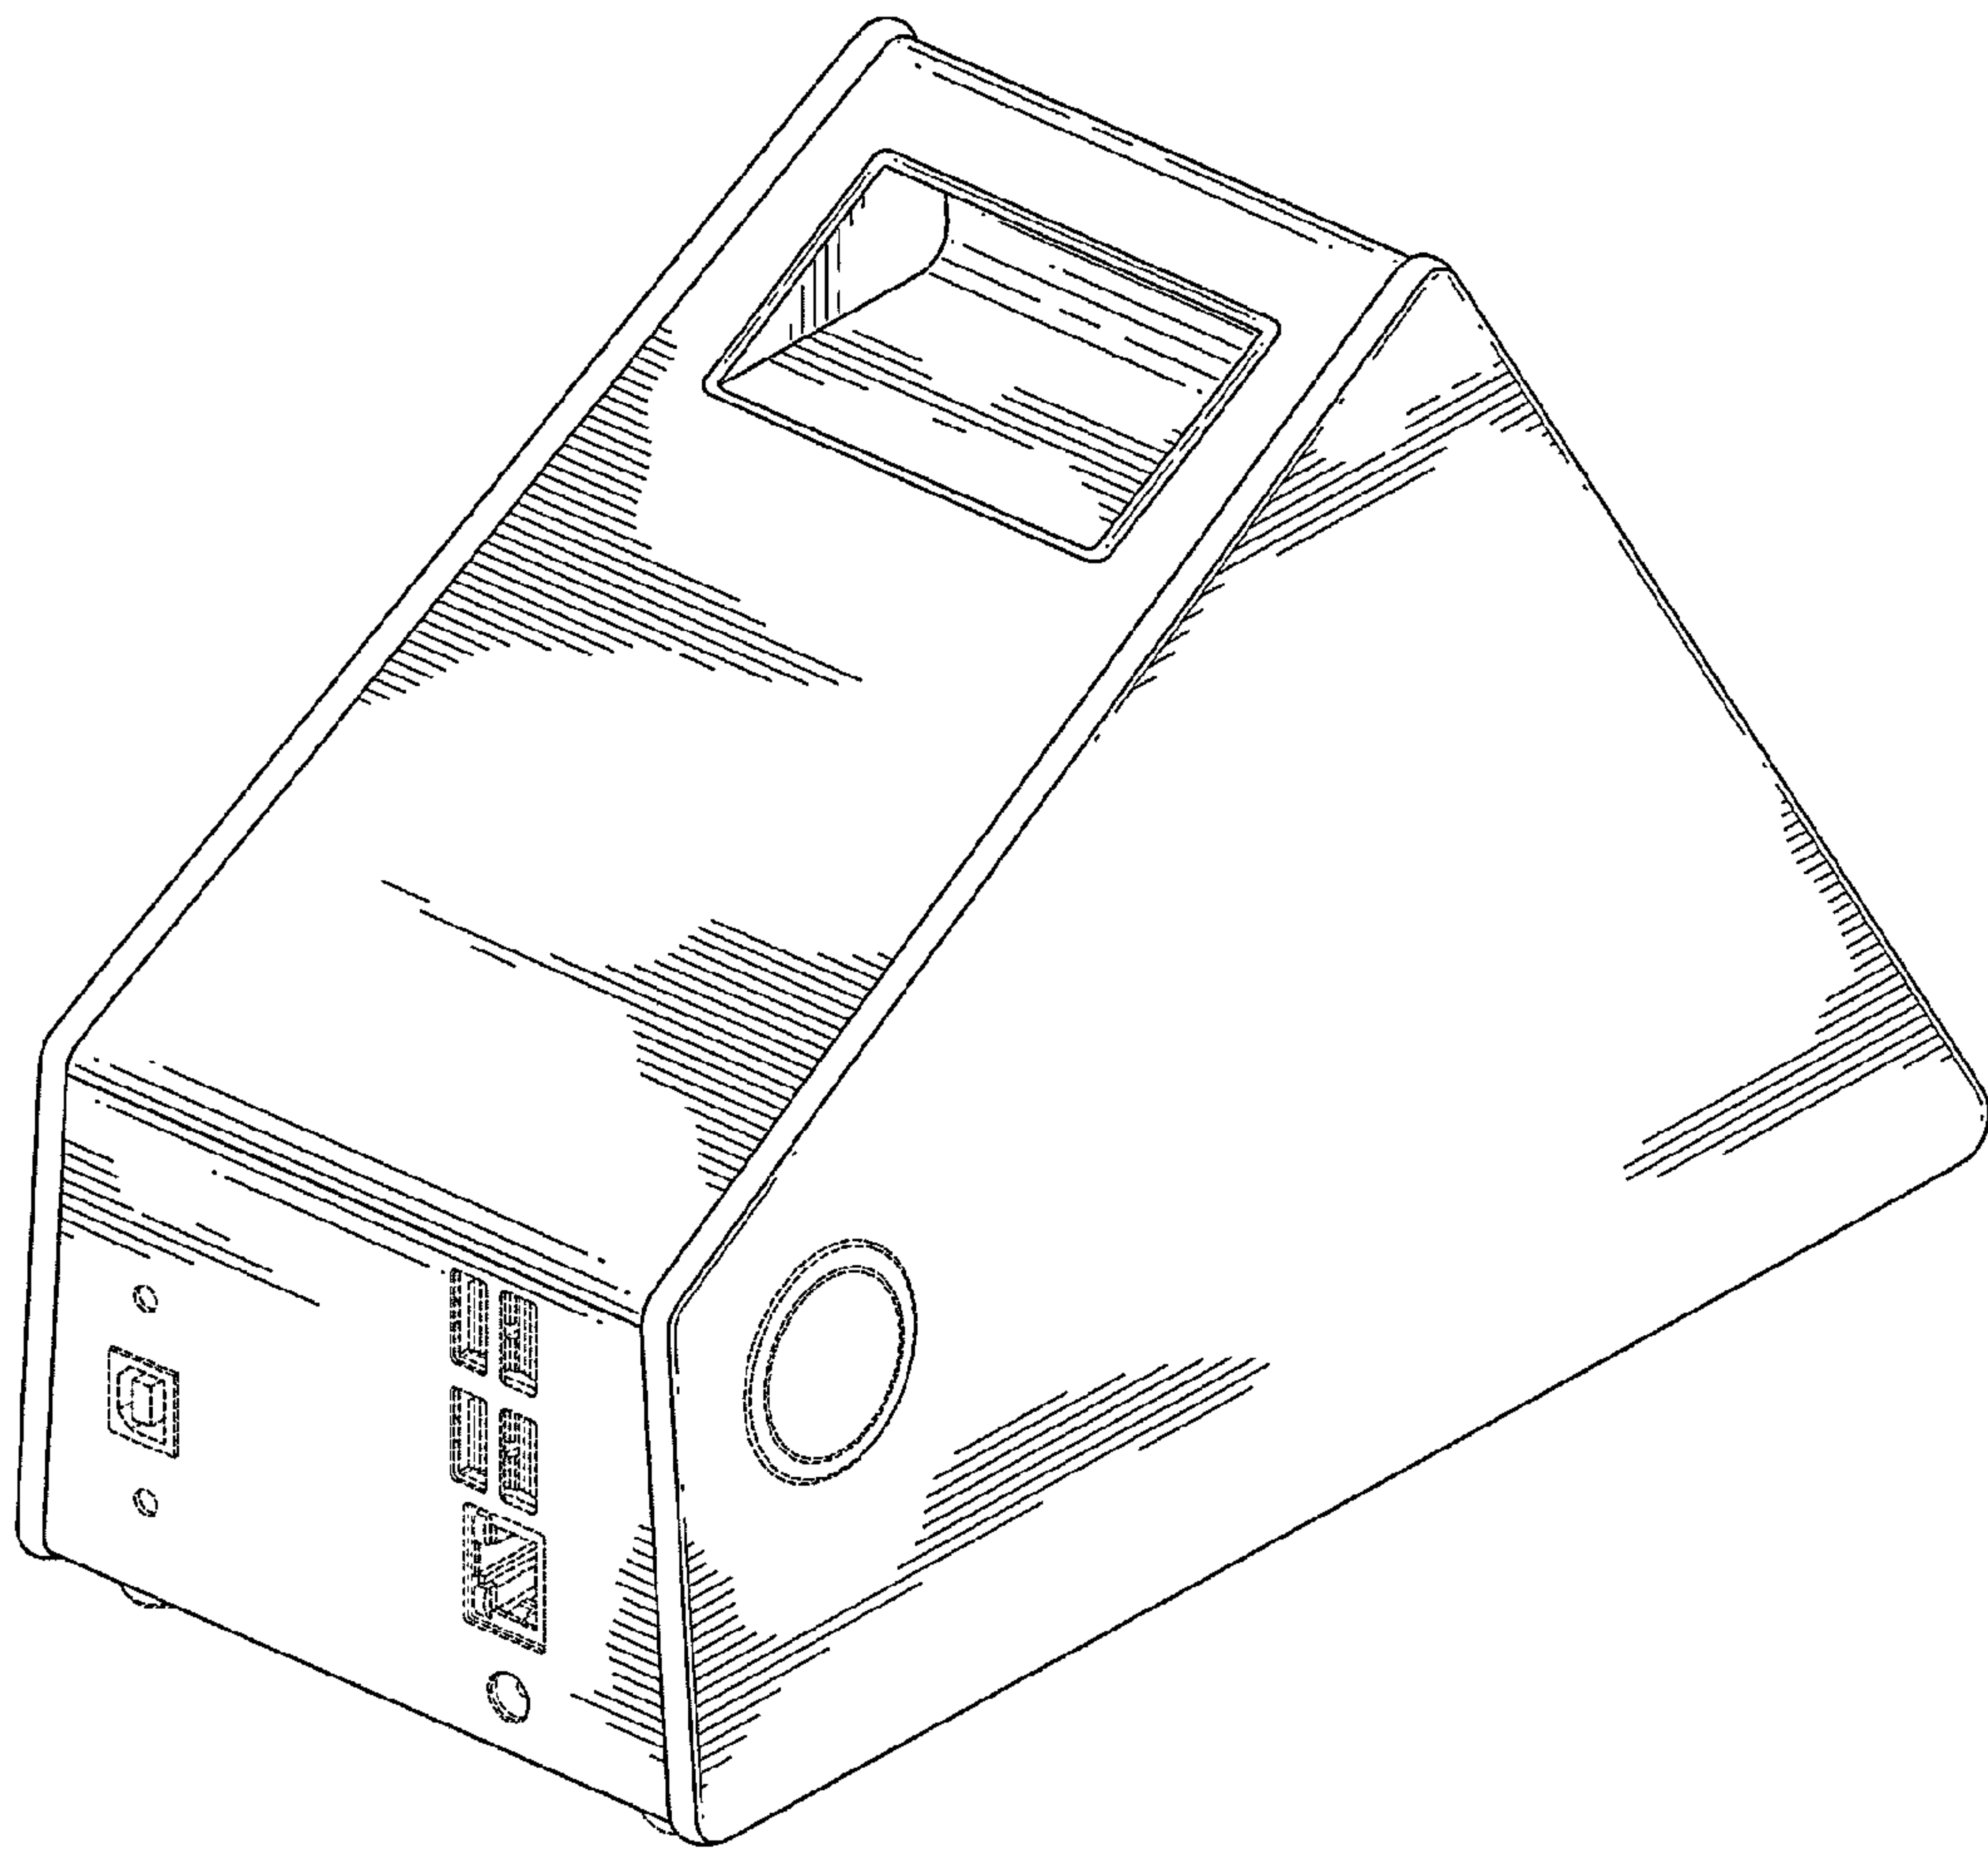


FIG.7