



US00D683851S

(12) **United States Design Patent**
Greenhalgh

(10) **Patent No.:** **US D683,851 S**
(45) **Date of Patent:** **** *Jun. 4, 2013**

(54) **MEDICAL POWDER DELIVERY
INSTRUMENT**

(75) Inventor: **Paul Greenhalgh**, Buckinghamshire
(GB)

(73) Assignee: **ProFibrix B.V.** (NL)

(*) Notice: This patent is subject to a terminal disclaimer.

(**) Term: **14 Years**

(21) Appl. No.: **29/394,931**

(22) Filed: **Jun. 23, 2011**

(30) **Foreign Application Priority Data**

Dec. 23, 2010 (EP) 001798257

(51) **LOC (9) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/133**

(58) **Field of Classification Search**

USPC D24/110, 110.4, 110.5, 108, 109,
D24/107, 133, 112-114, 137, 144, 147, 130;
128/203.15, 200.2, 200.14-200.23,
203.12-203.24; 604/30, 32, 33, 35, 247,
604/110, 249; 222/633, 635, 631, 632, 604,
222/34, 39, 36, 43

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,950,564 A * 8/1960 Bonine 222/631
4,253,468 A * 3/1981 Lehmbeck 600/539
D300,438 S * 3/1989 Berghash et al. D21/411
D331,281 S * 11/1992 Levine D24/110

(Continued)

FOREIGN PATENT DOCUMENTS

DE 619625 C 10/1935
FR 2863503 A1 6/2005
WO 2005037443 A2 4/2005
WO 2010070333 A2 6/2010

OTHER PUBLICATIONS

Cooper, N., Profibrix Enters Phase III Clinical Trials. [on-line]. Team-consulting.com web site, posted on Jun. 15, 2012. [Retrieved on Aug. 6, 2012]. Retrieved from the Internet. <URL: rdms-mpep-vip.uspto.gov/RDMS/detail/manual/MPEP/E8r8/d0e18.xml#/manual/MPEP/E8r8/d0e73852.xml>.*

(Continued)

Primary Examiner — Ian Simmons

Assistant Examiner — Eleni H Aldridge

(74) *Attorney, Agent, or Firm* — Young Basile

(57) **CLAIM**

The ornamental design for the medical powder delivery instrument, as shown and described.

DESCRIPTION

FIG. 1 is a rear and left perspective view of a medical powder delivery instrument showing my new design;

FIG. 2 is a top plan view of the medical powder delivery instrument of FIG. 1;

FIG. 3 is a bottom plan view of the medical powder delivery instrument of FIG. 1;

FIG. 4 is a front elevation view of the medical powder delivery instrument of FIG. 1;


FIG. 5 is a rear elevation view of the medical powder delivery instrument of FIG. 1;

FIG. 6 is a left elevation view of the medical powder delivery instrument of FIG. 1; and,

FIG. 7 is a right elevation view of the medical powder delivery instrument of FIG. 1.

The broken line showing inside the nozzle is included for the purpose of illustrating environmental structure and forms no part of the claimed design.

1 Claim, 7 Drawing Sheets

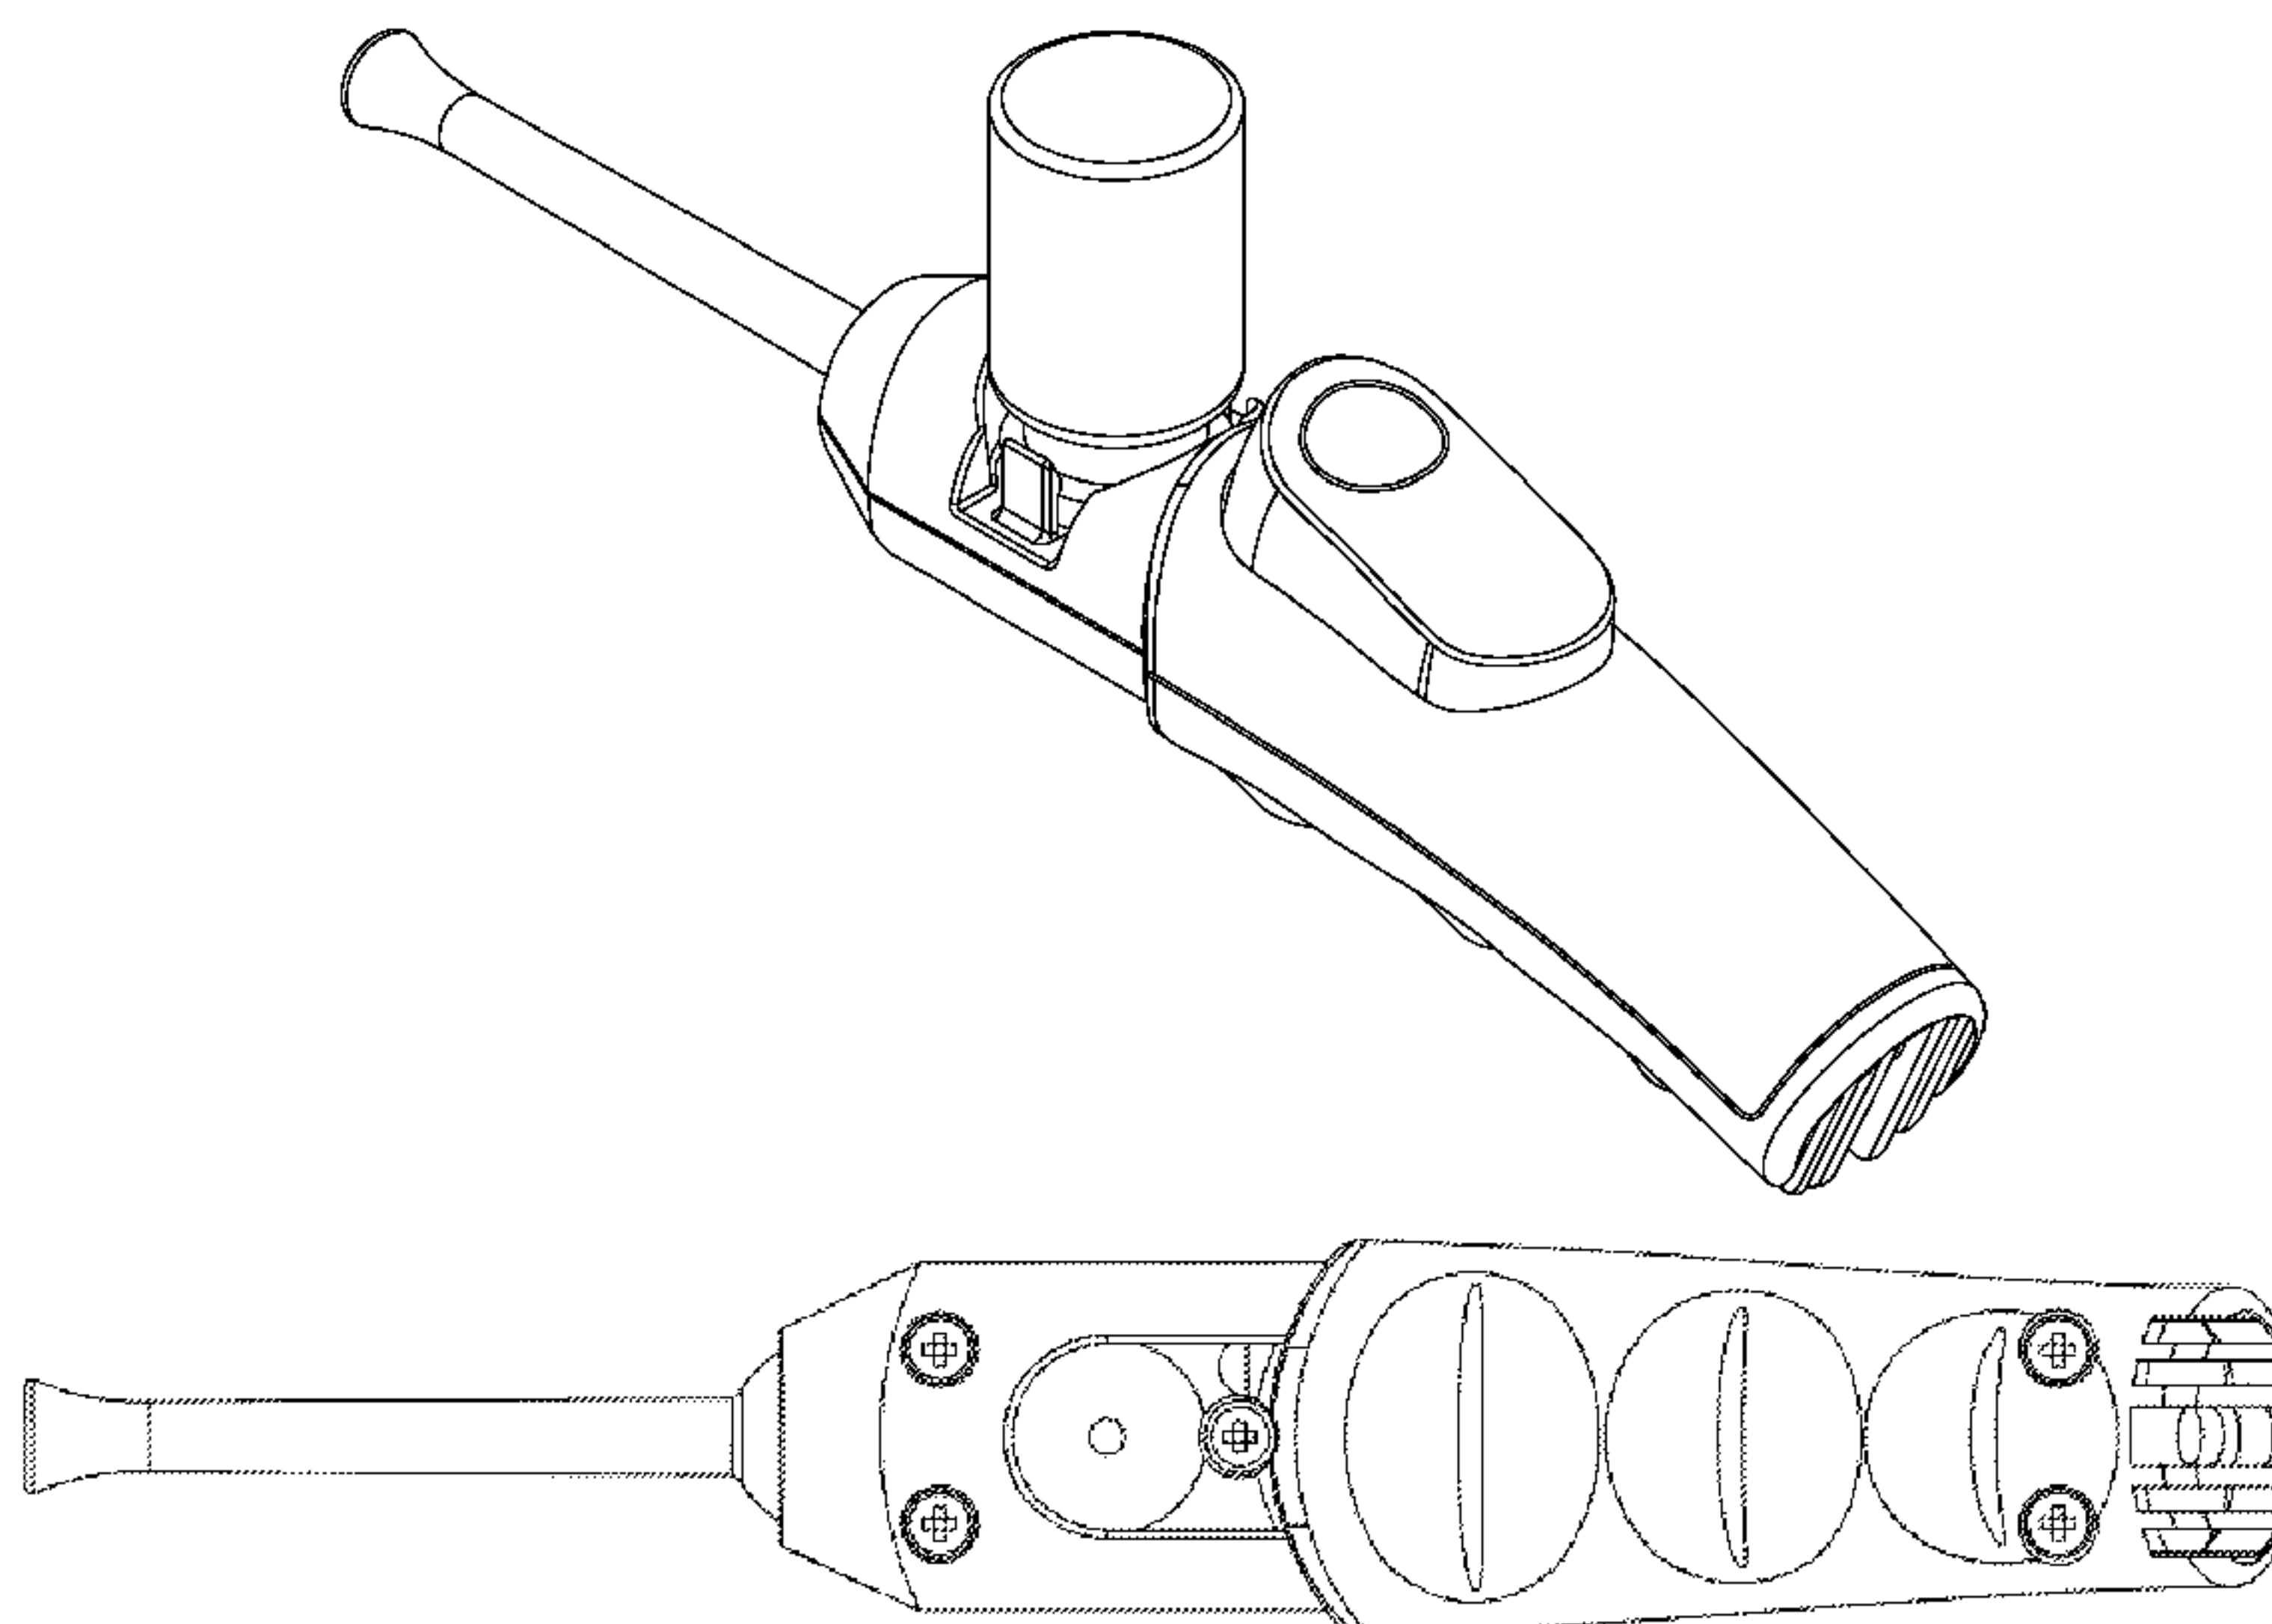

U.S. PATENT DOCUMENTS

D341,760 S * 11/1993 Armbruster et al. D8/68
5,522,380 A * 6/1996 Dwork 128/200.23
6,024,129 A 2/2000 Schima
D473,598 S * 4/2003 Izen et al. D21/411
6,539,939 B2 * 4/2003 Rubin 128/203.15
D533,274 S * 12/2006 Visconti et al. D24/133
D536,444 S * 2/2007 Bacher et al. D24/133
D607,558 S * 1/2010 Abry et al. D24/113
D628,692 S 12/2010 Greenhalgh
2011/0230820 A1 9/2011 Lillis et al.
2012/0080457 A1 * 4/2012 Lovinger et al. 222/633

OTHER PUBLICATIONS

Dry Powder Haemostat Delivery Device. [on-line]. Team-consulting.
com website, no posting date. [Retrieved on Aug. 6, 2012]. Retrieved
from the Internet. <URL: [www.team-consulting.com/case_studies/
dry-powder-haemostat-delivery-device](http://www.team-consulting.com/case_studies/dry-powder-haemostat-delivery-device)>.*

* cited by examiner

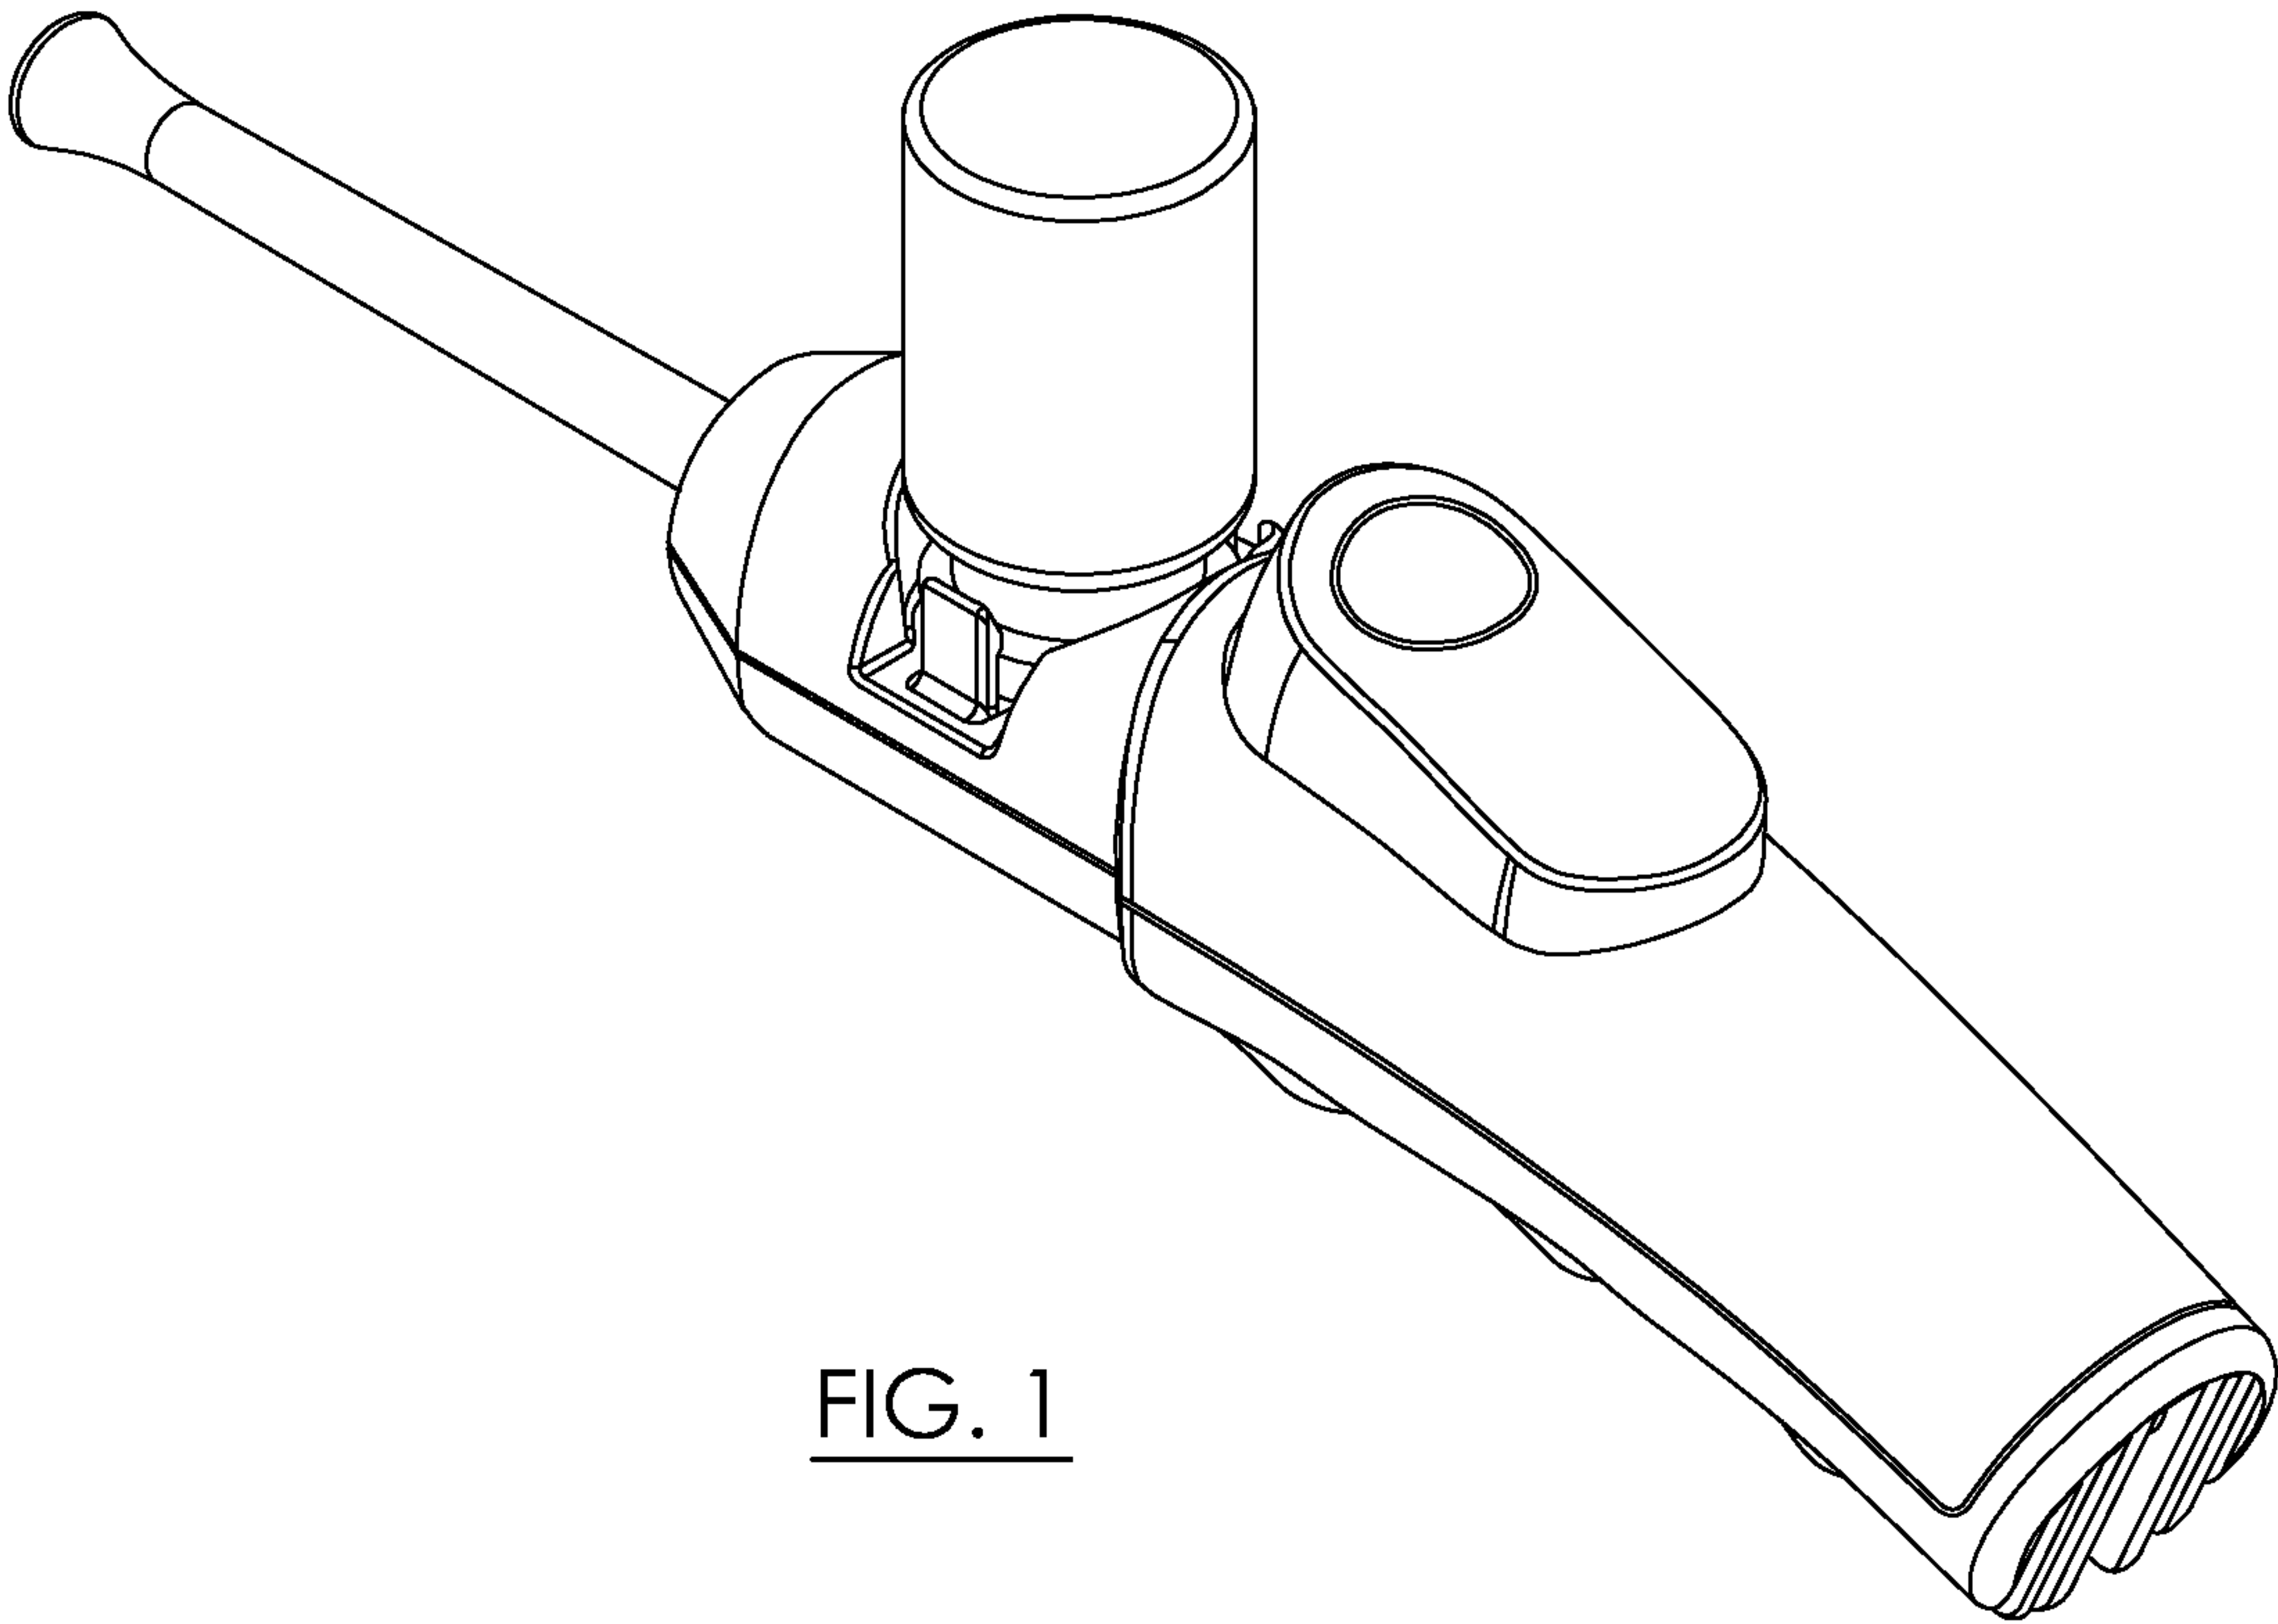


FIG. 1

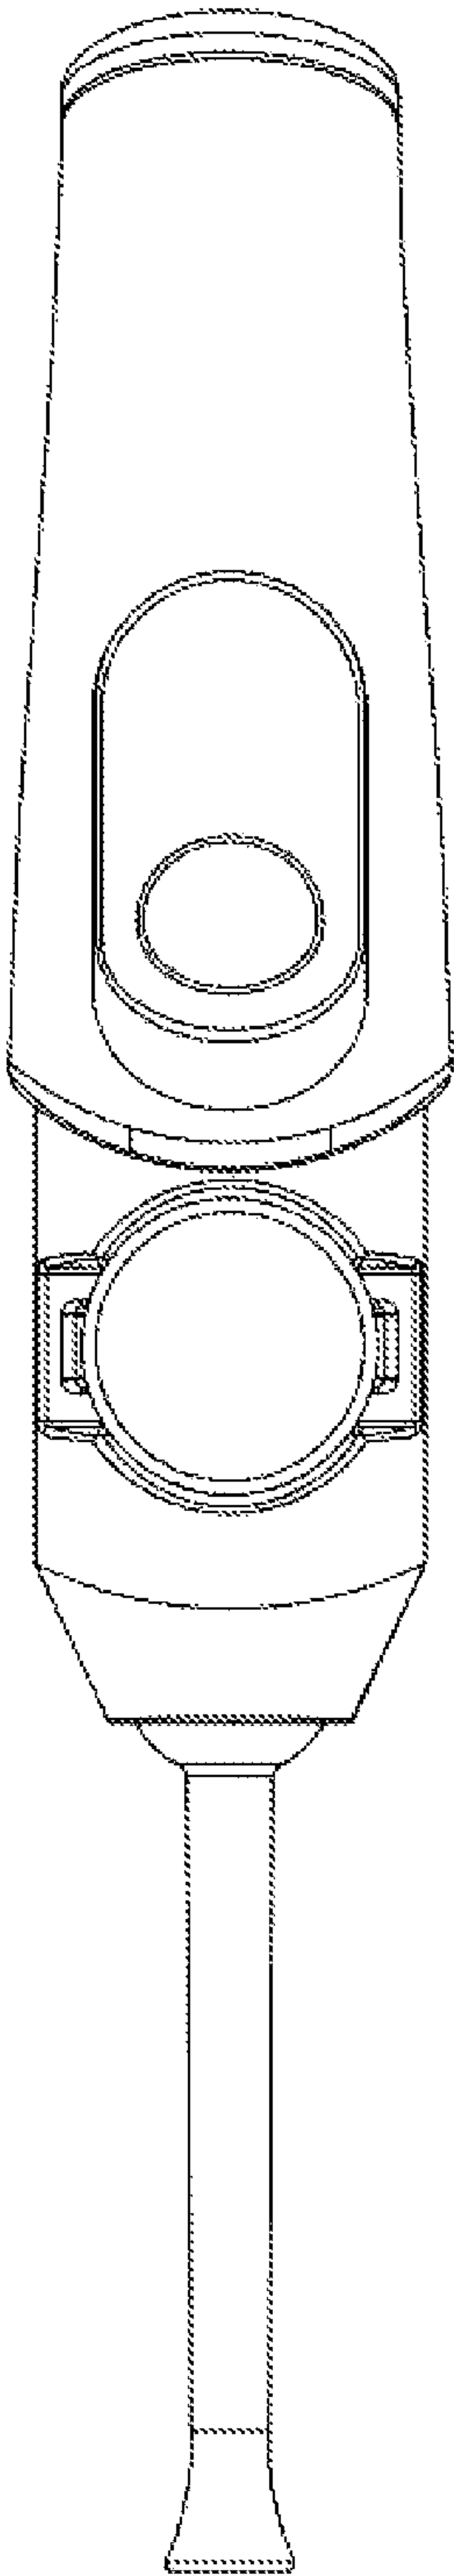


FIG. 2

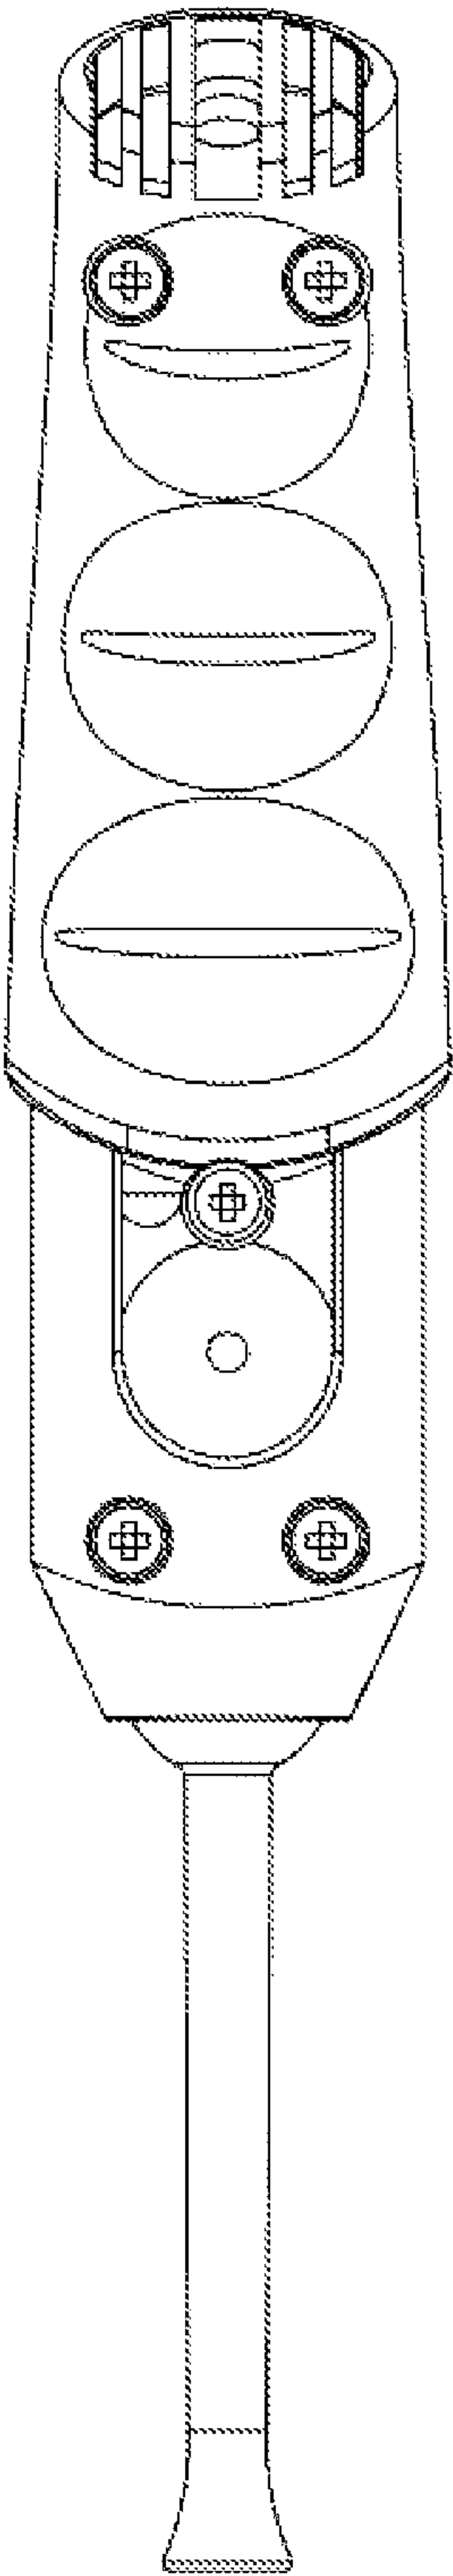


FIG. 3

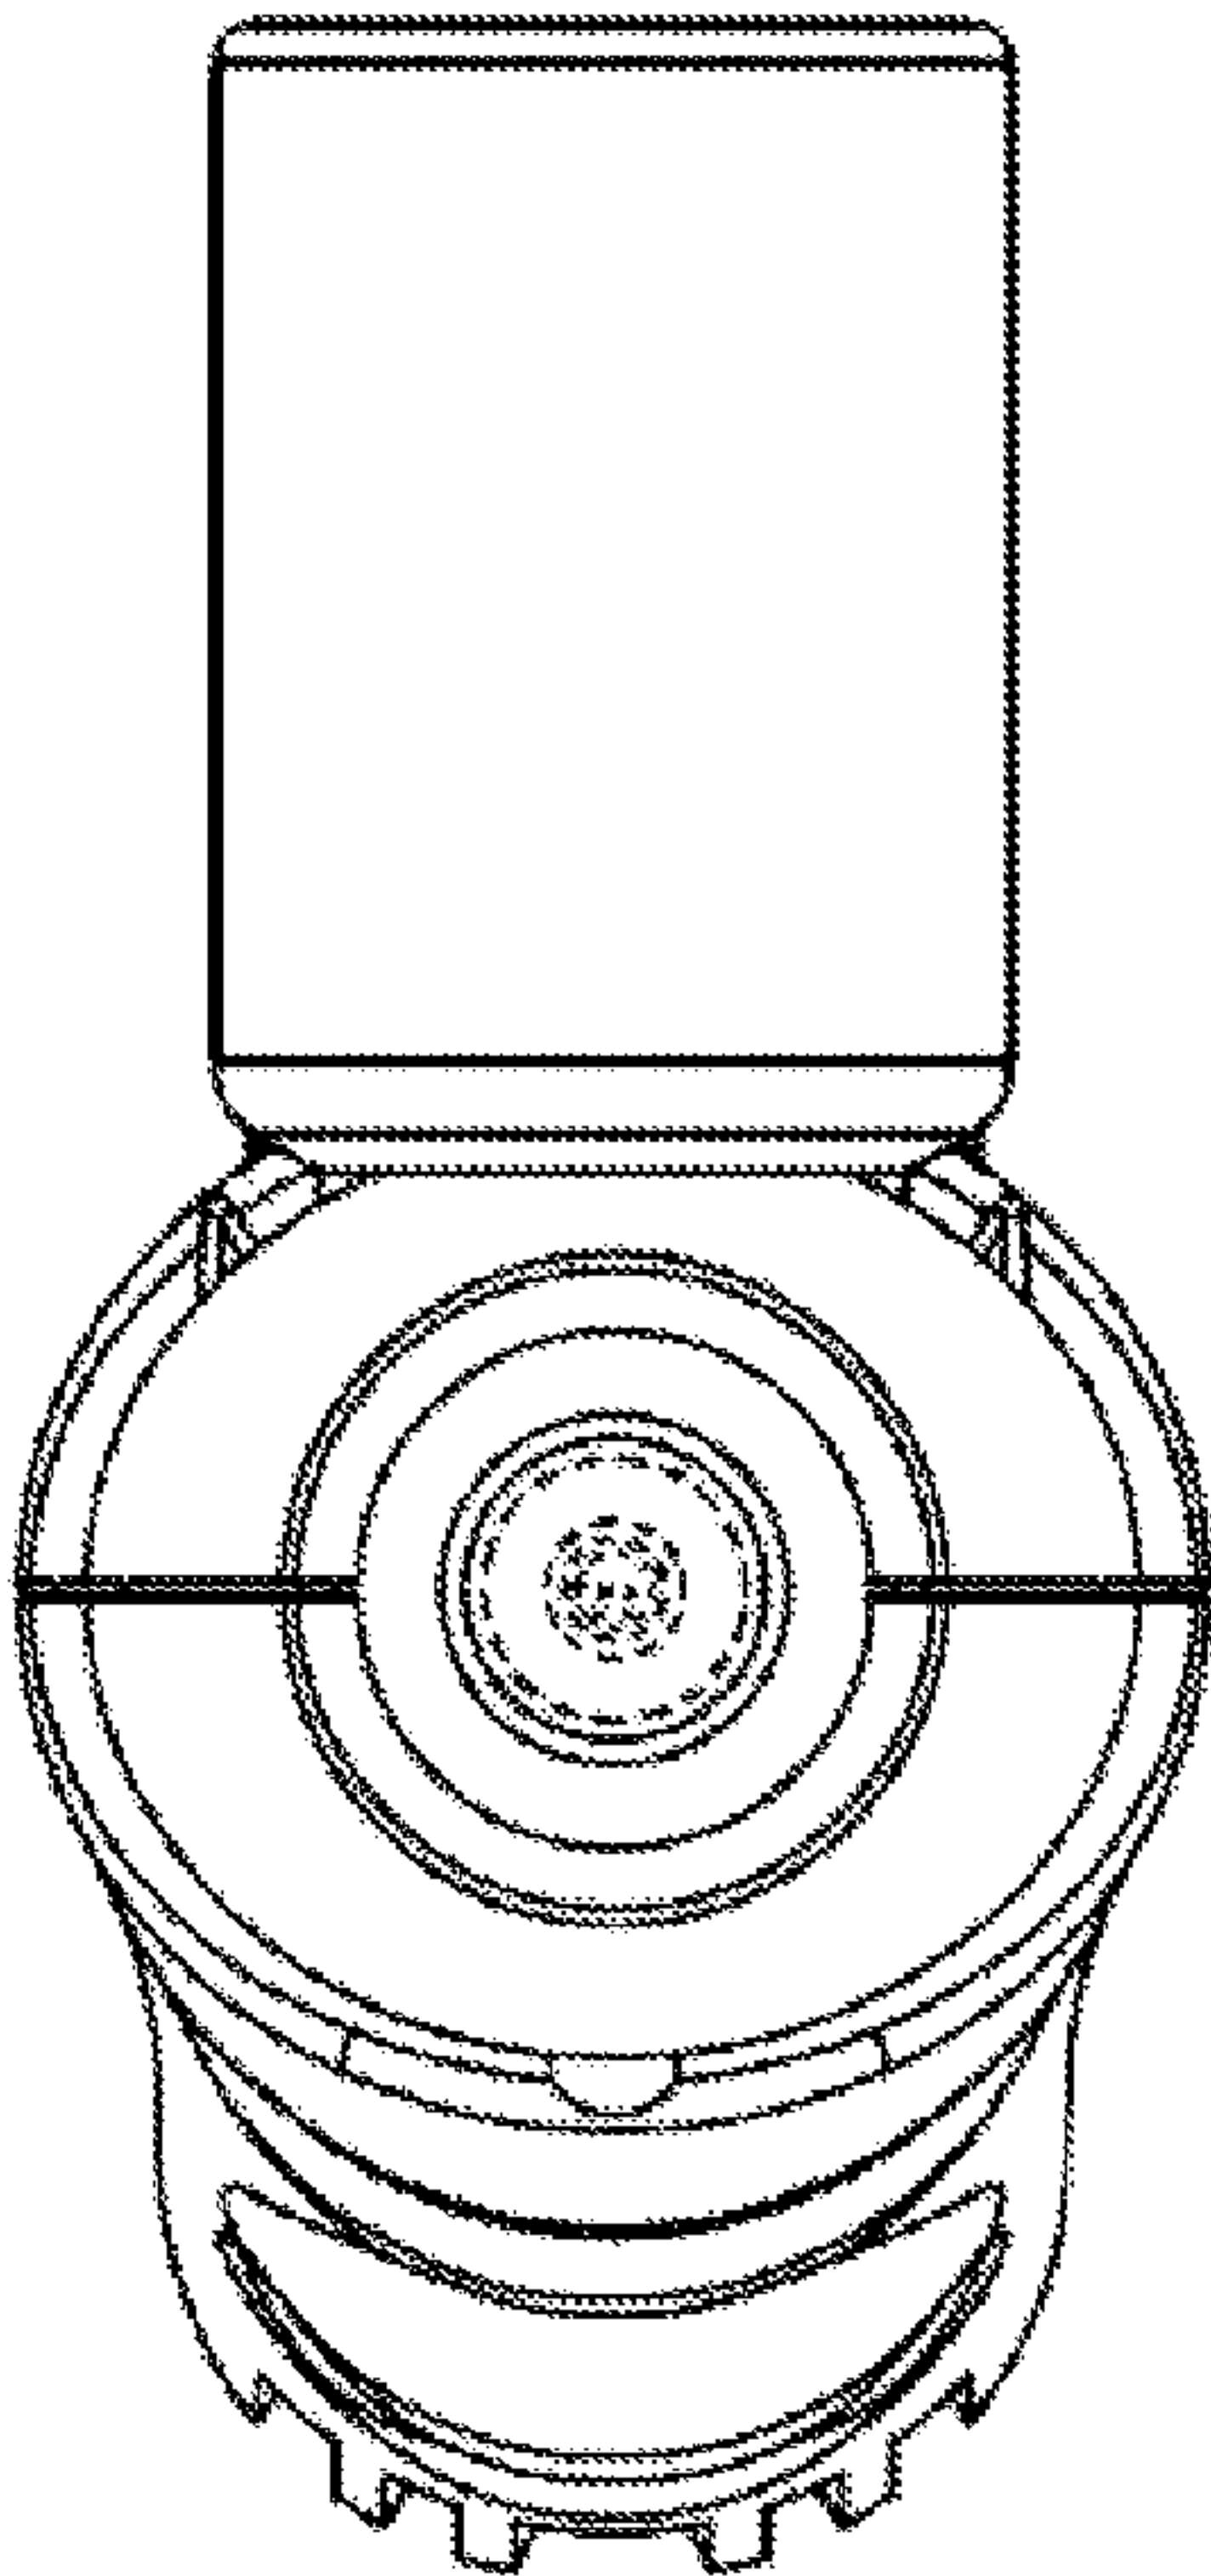


FIG. 4

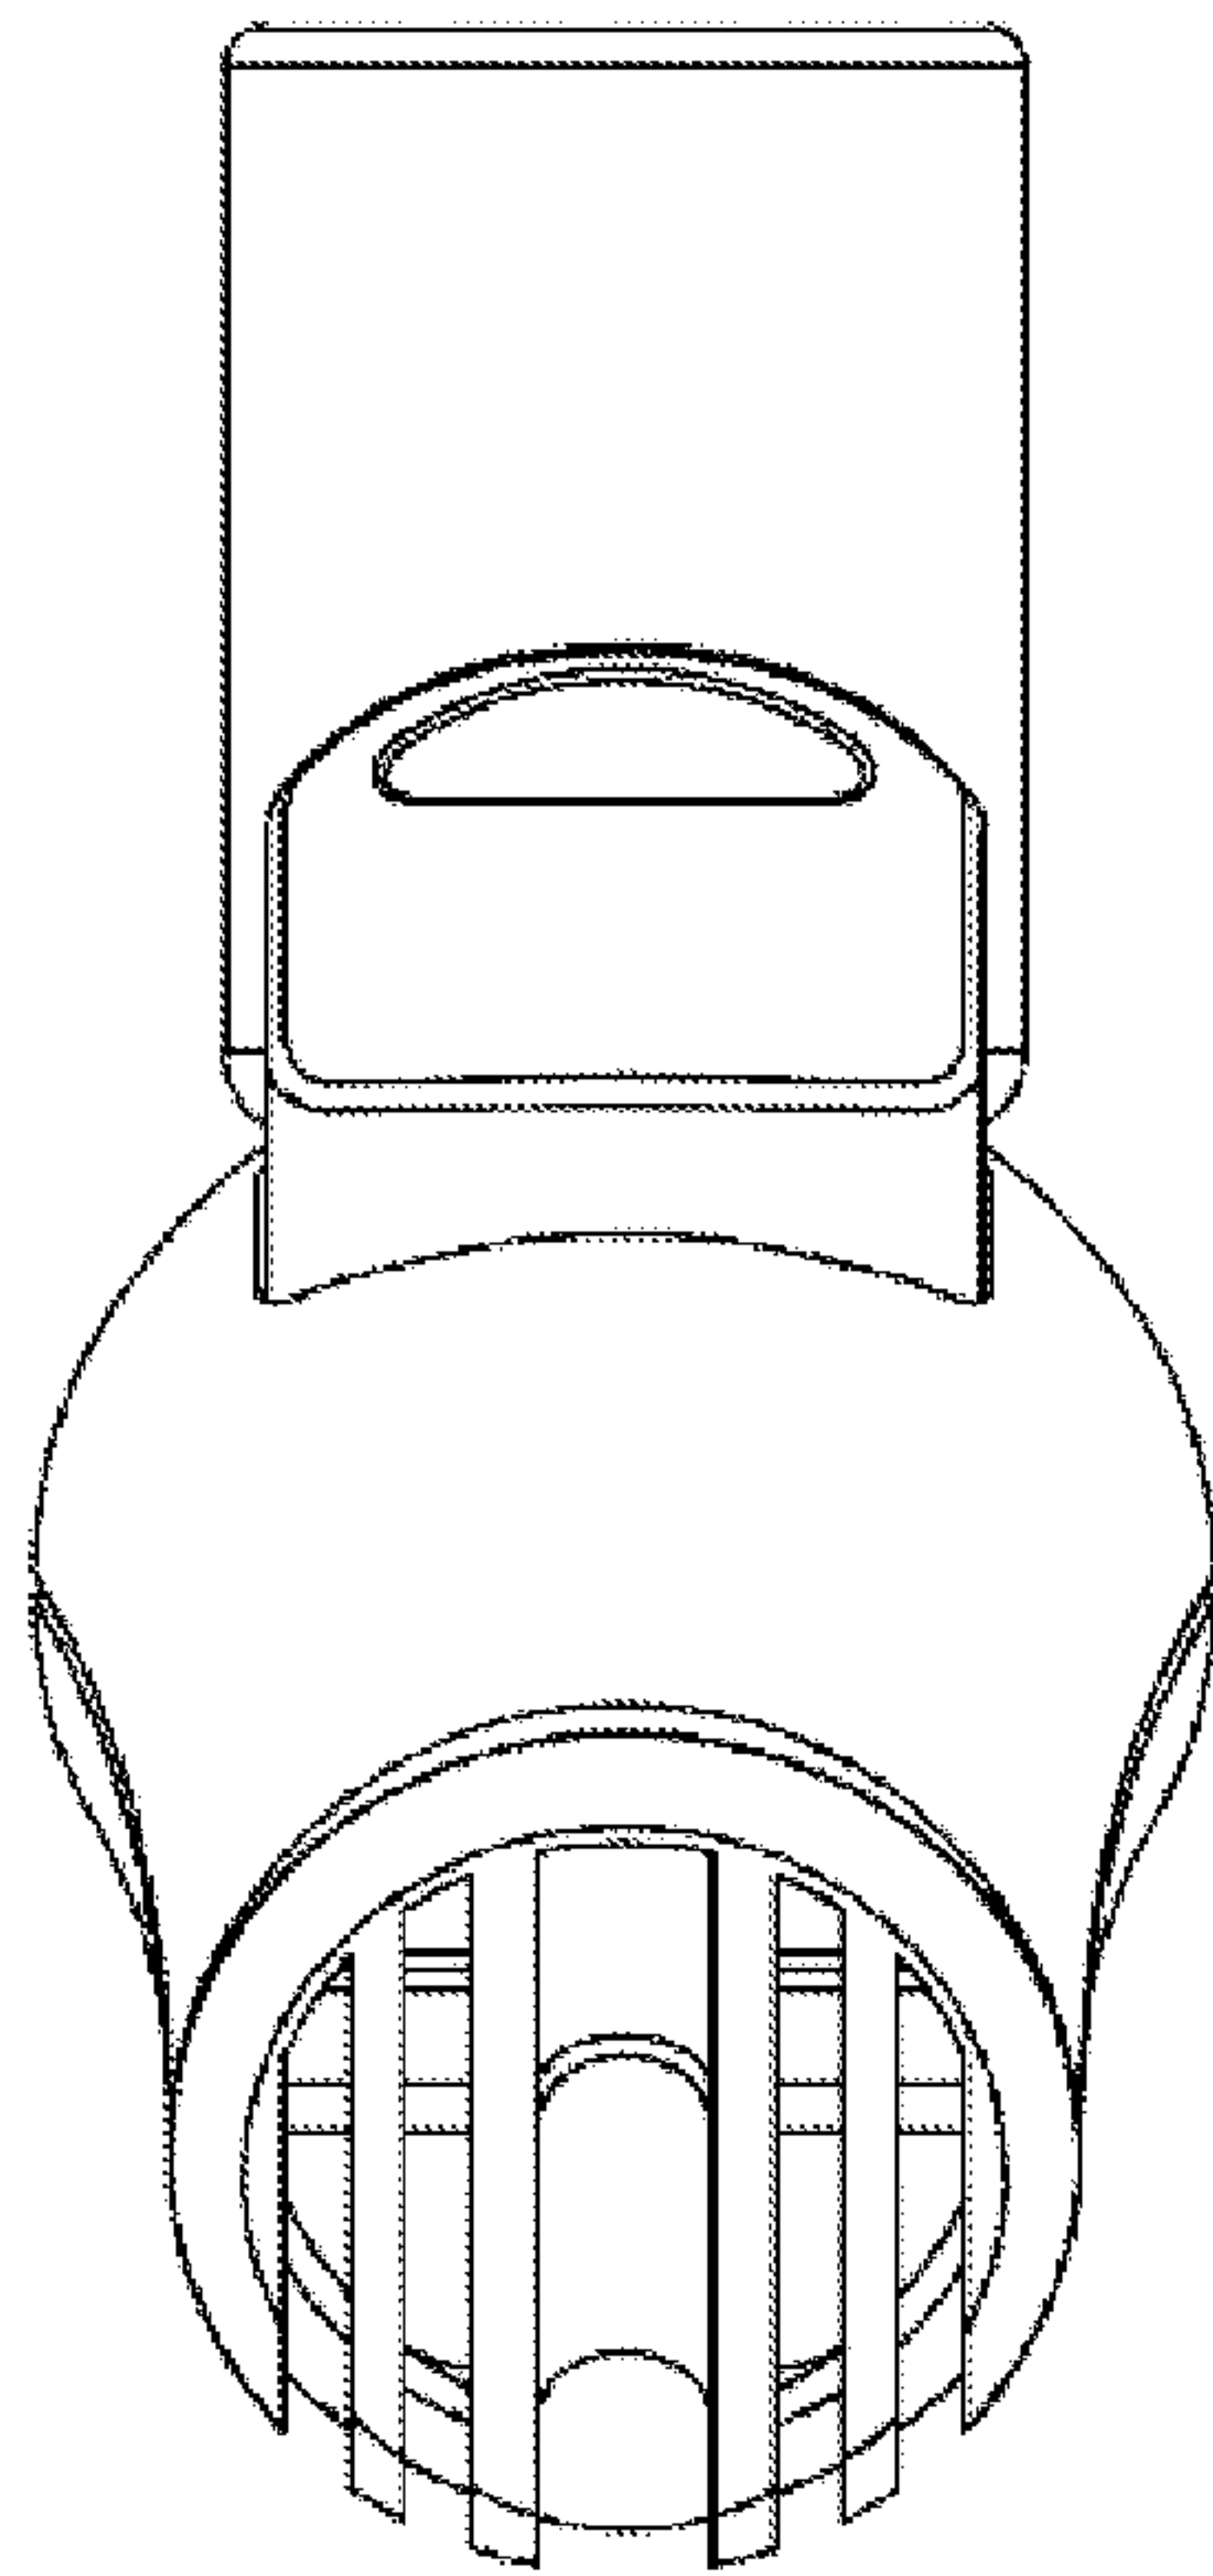


FIG. 5

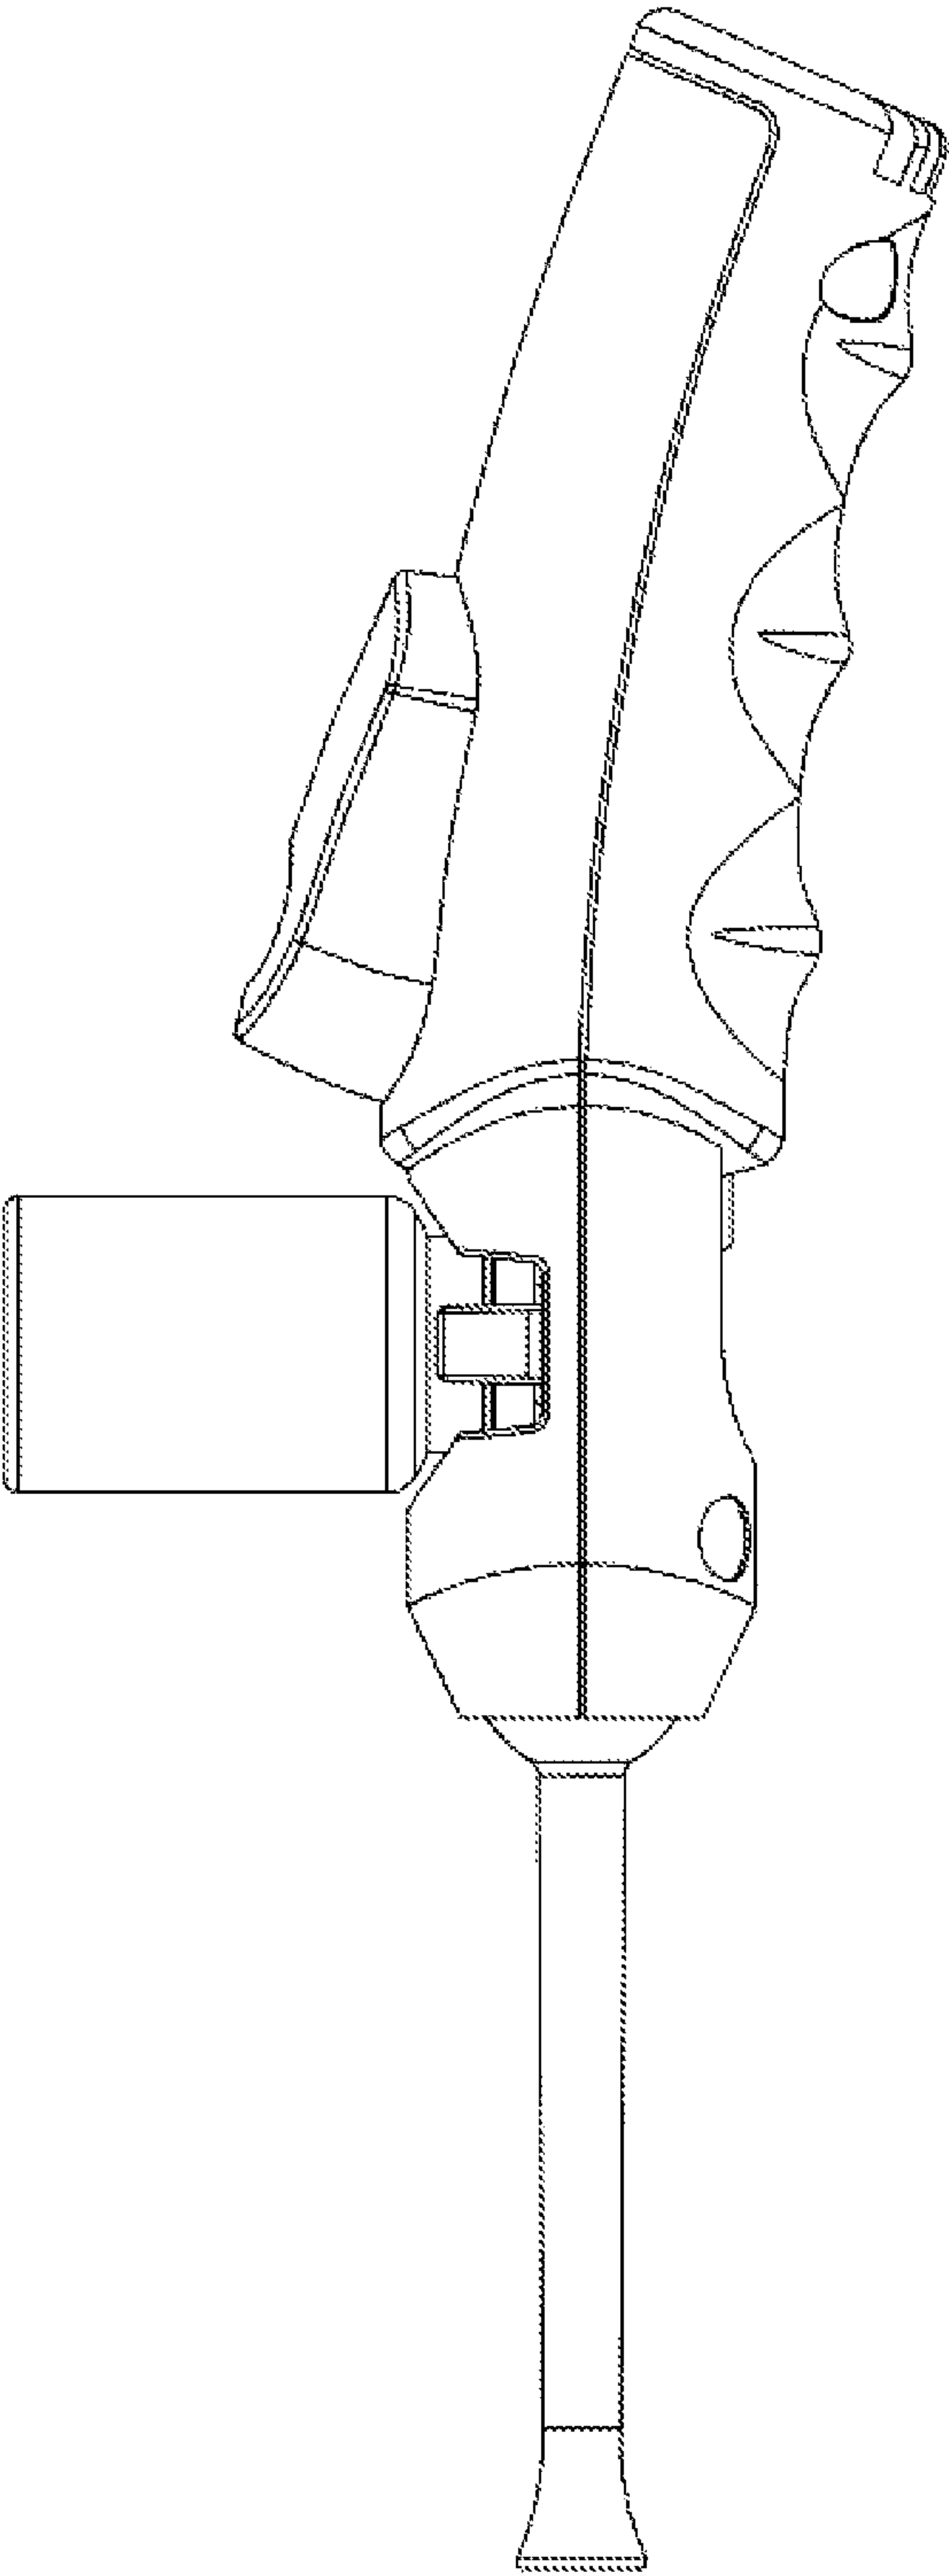


FIG. 6

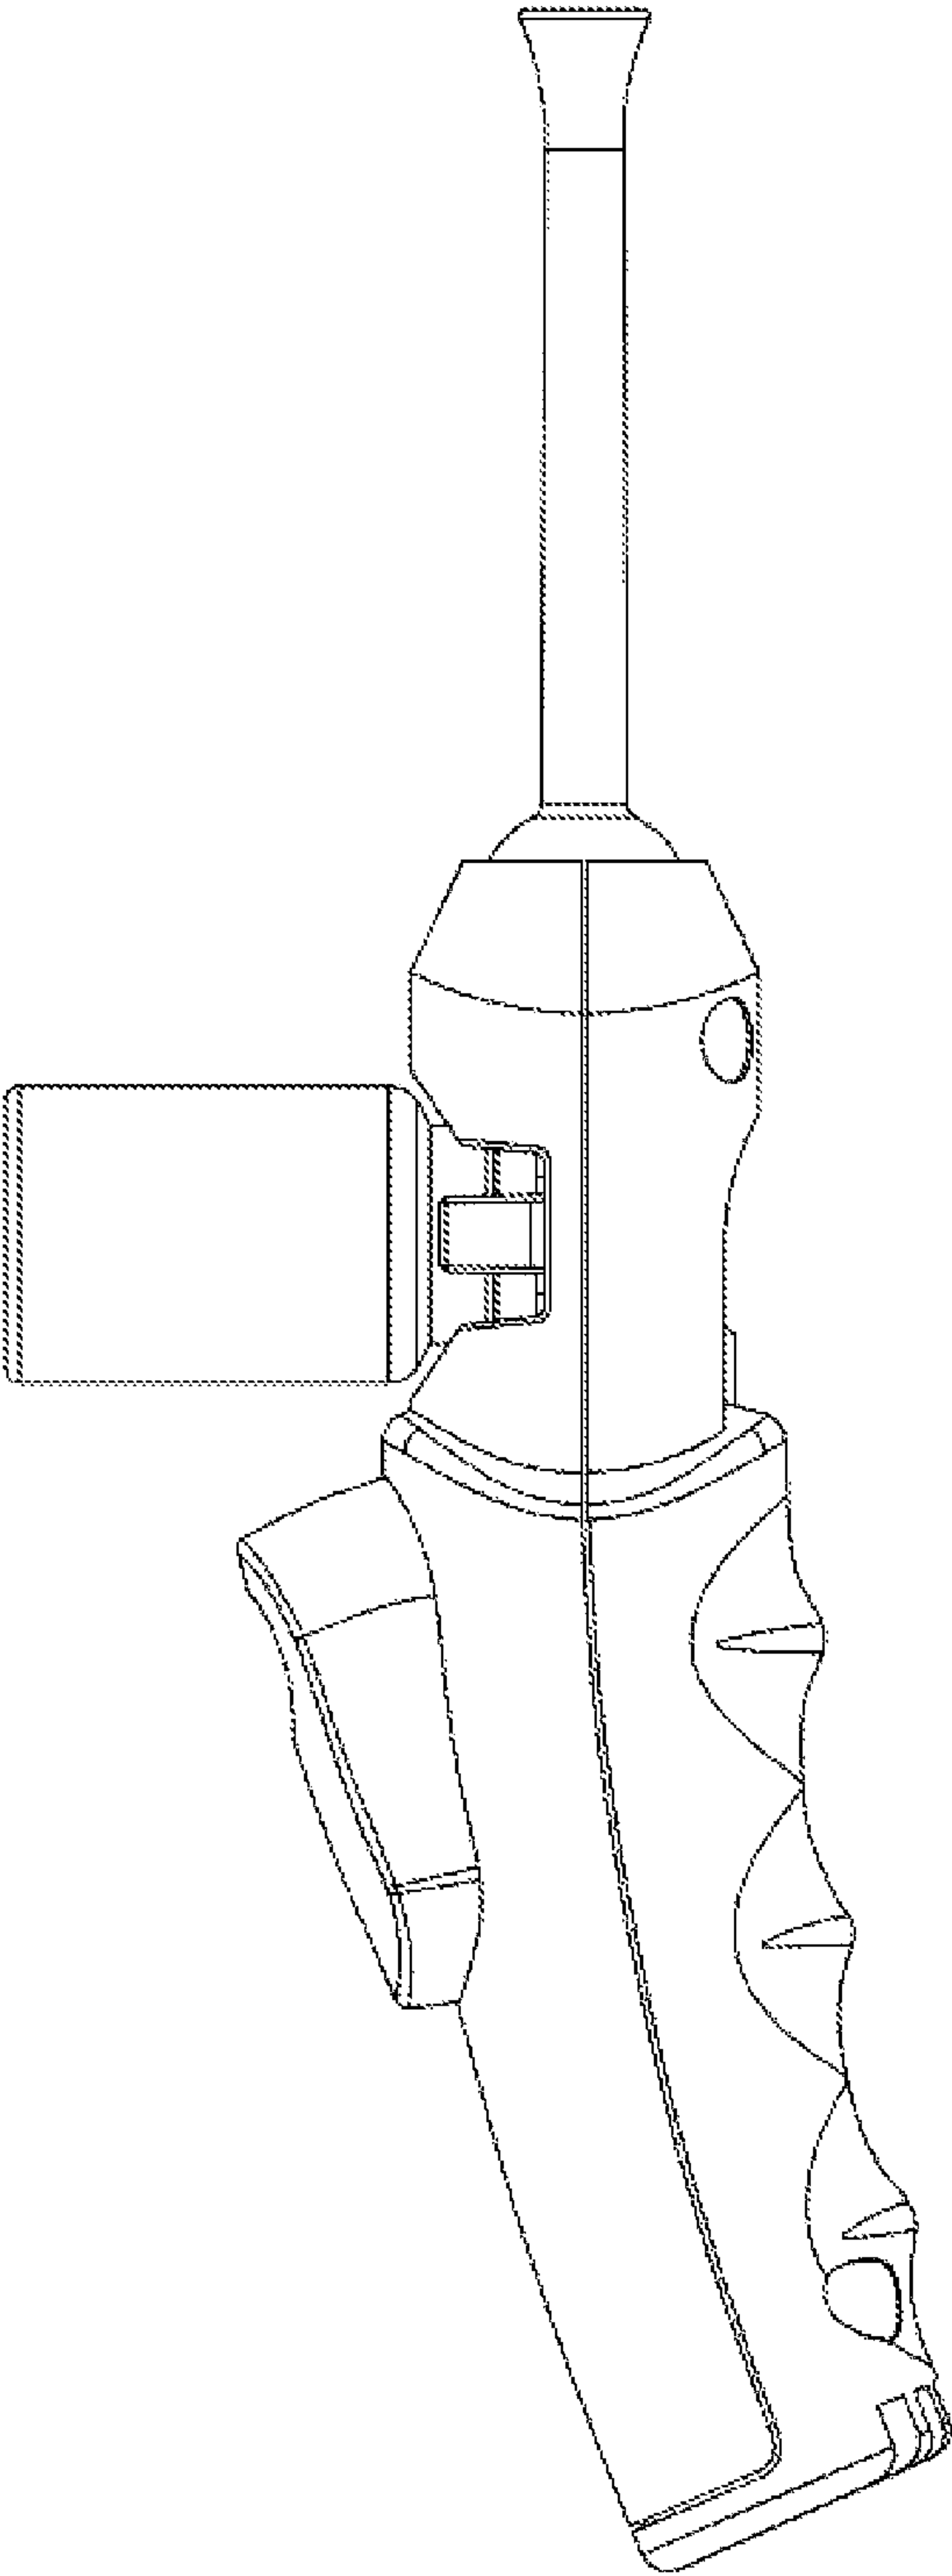


FIG. 7