

US00D685469S

(12) **United States Design Patent**  
**Cole et al.**

(10) **Patent No.:** **US D685,469 S**  
(45) **Date of Patent:** **\*\* Jul. 2, 2013**

(54) **STETHOSCOPE CLEANING ASSEMBLY  
CARTRIDGE**

4,210,974 A 7/1980 Stoltzman  
4,449,976 A 5/1984 Kamen  
4,701,968 A 10/1987 Stoltzman  
4,871,046 A 10/1989 Turner  
4,953,999 A 9/1990 Rivers

(75) Inventors: **Michael R. Cole**, Stratham, NH (US);  
**Mathew Cardinali**, Portsmouth, NH  
(US); **James M. Sellers**, Eliot, ME (US);  
**Michael Perlman**, Davie, FL (US);  
**Keith Rubin**, Fort Lauderdale, FL (US)

(Continued)

**FOREIGN PATENT DOCUMENTS**

CN 148125 A 3/2004  
CN 101674898 3/2010

(Continued)

**OTHER PUBLICATIONS**

Dix, et al., "Environmental Surface Cleaning First Defense Against  
Infectious Agents." [http://www.vpico.com/articlemanager/  
printerfriendly.aspx?article=60960](http://www.vpico.com/articlemanager/printerfriendly.aspx?article=60960); Dec. 2, 2006; 7 pg.

(Continued)

(\*\*) Term: **14 Years**  
(21) Appl. No.: **29/410,631**  
(22) Filed: **Jan. 10, 2012**

**Related U.S. Application Data**

(63) Continuation of application No. 29/310,258, filed on  
Aug. 5, 2008, now Pat. No. Des. 652,142, which is a  
continuation-in-part of application No. 12/079,077,  
filed on Mar. 24, 2008, now Pat. No. 7,503,335, which  
is a continuation-in-part of application No.  
11/728,207, filed on Mar. 23, 2007, now Pat. No.  
7,406,973.

*Primary Examiner* — Wan Laymon

(74) *Attorney, Agent, or Firm* — Malloy & Malloy, P.L.

(51) **LOC (9) Cl.** ..... **24-02**  
(52) **U.S. Cl.**  
USPC ..... **D24/134**  
(58) **Field of Classification Search**  
USPC .. D24/134–135, 140; 181/131–137; 600/528;  
134/100.1, 133, 166 R; 221/221, 222; 401/17,  
401/22, 27, 136  
See application file for complete search history.

(57)

**CLAIM**

The ornamental design for a stethoscope cleaning assembly  
cartridge, as shown and described.

**DESCRIPTION**


FIG. 1 is a front perspective view of a stethoscope cleaning  
assembly cartridge showing our design;  
FIG. 2 is a front view thereof;  
FIG. 3 is a left side view thereof;  
FIG. 4 is a top view thereof view thereof;  
FIG. 5 is a right side view thereof;  
FIG. 6 is a bottom view thereof; and  
FIG. 7 is a rear view thereof; and,  
FIG. 8 is a rear perspective thereof.  
The broken lines in the drawings are for illustrative purposes  
only and form no part of the claimed design.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

2,604,650 A 7/1952 Mottelson  
4,002,009 A 1/1977 Tolosa et al.

**1 Claim, 6 Drawing Sheets**

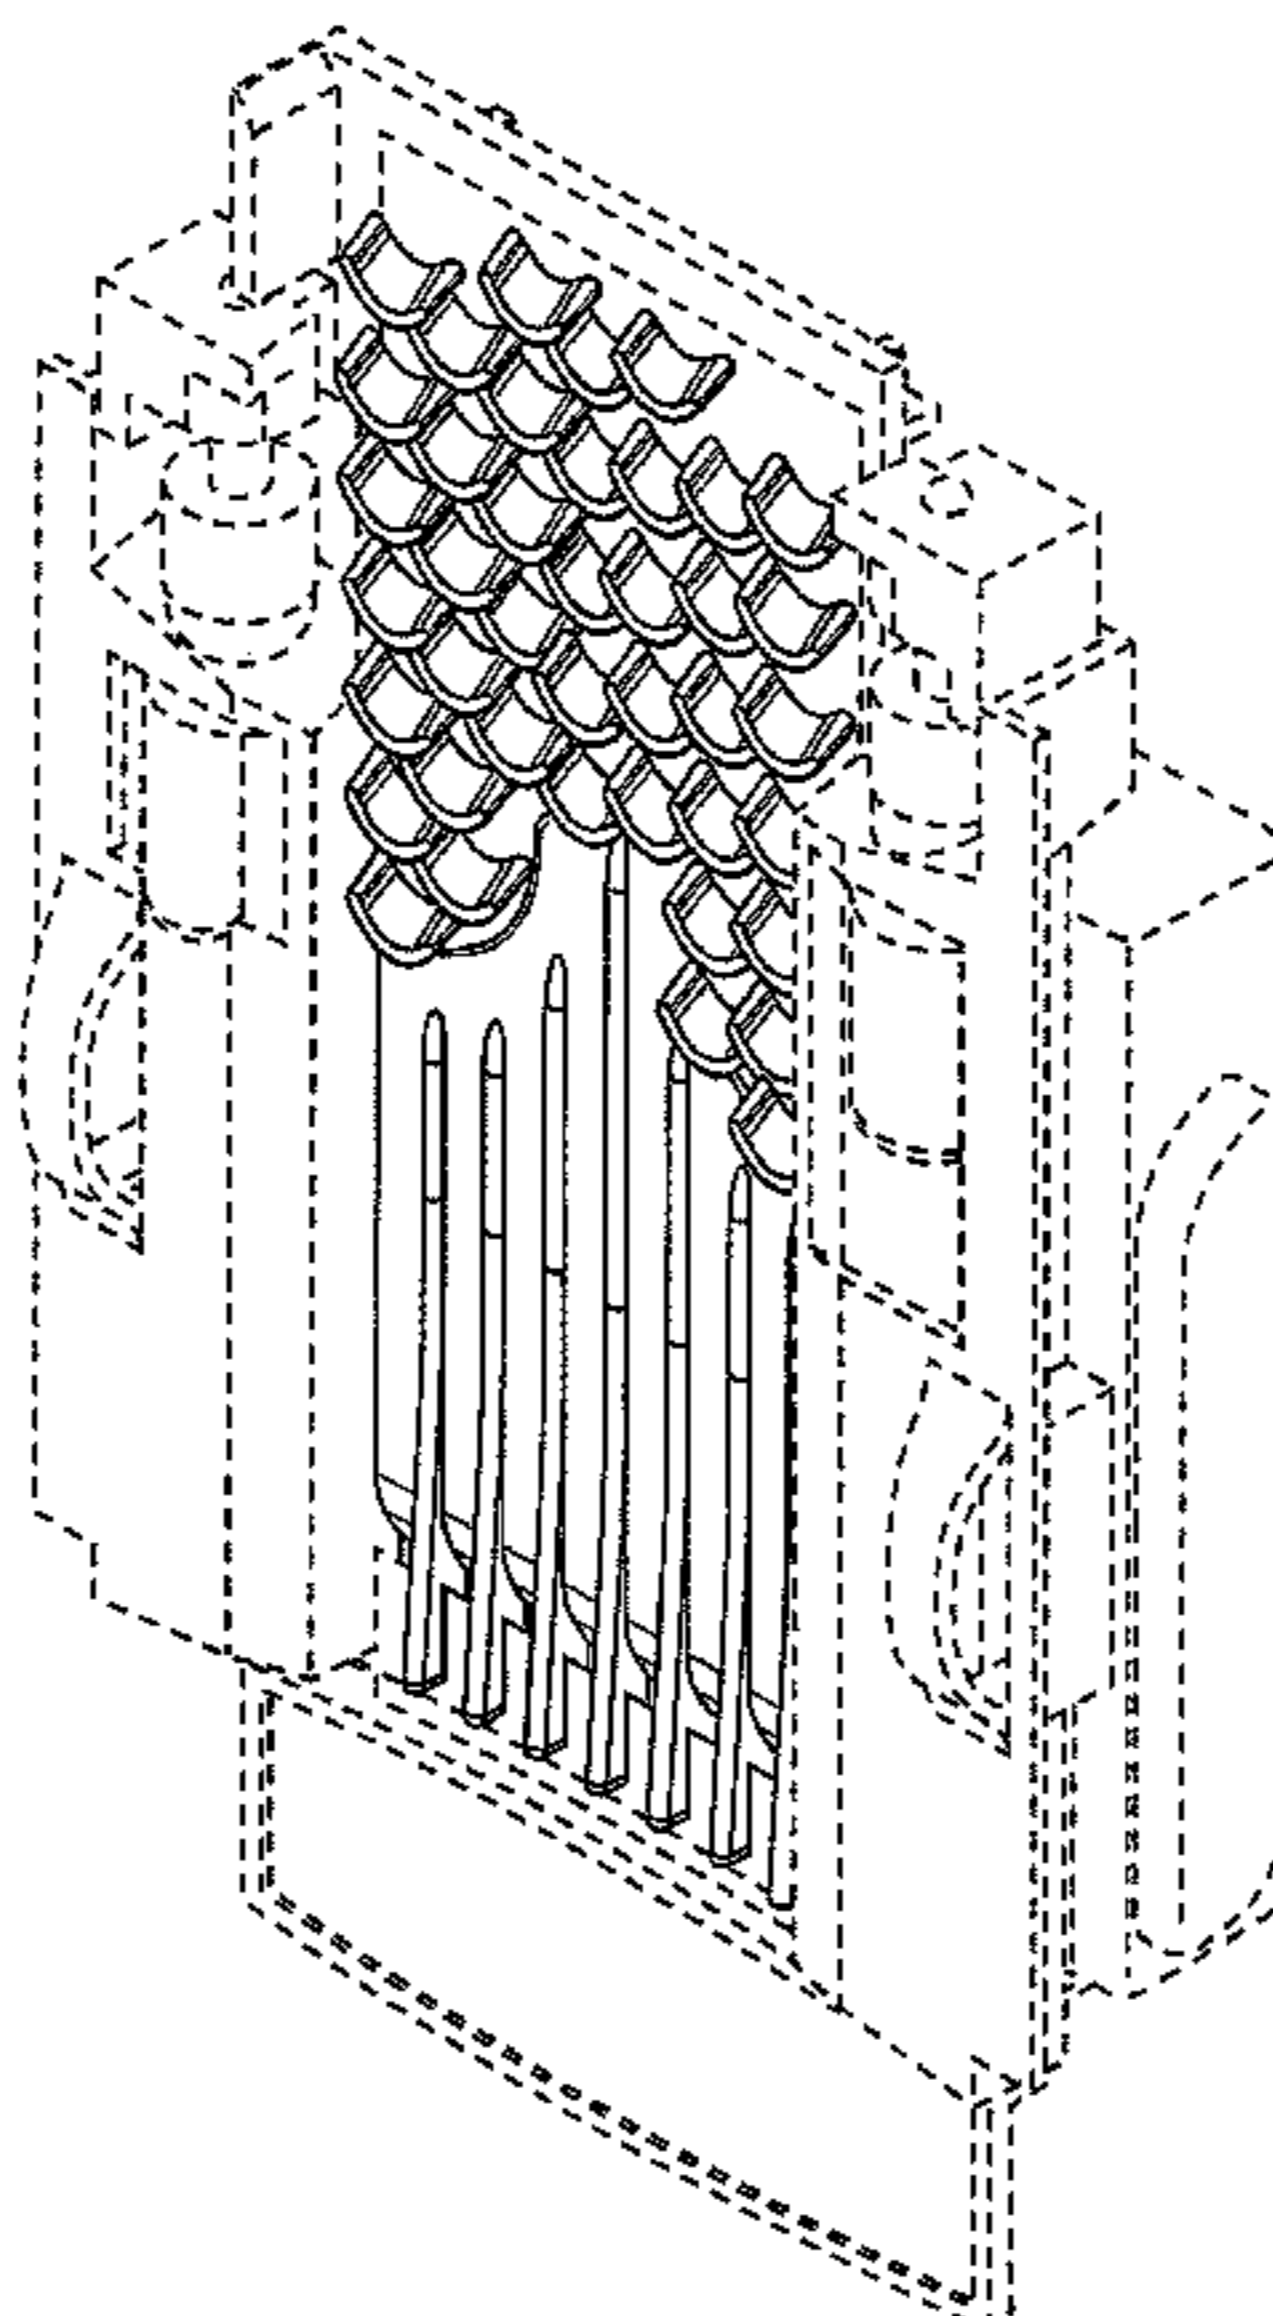

U.S. PATENT DOCUMENTS

5,048,549 A \* 9/1991 Hethcoat ..... 134/122 R  
 5,114,670 A 5/1992 Duffey  
 5,185,532 A \* 2/1993 Zabsky et al. .... 422/24  
 5,448,025 A \* 9/1995 Stark et al. .... 181/131  
 5,466,897 A \* 11/1995 Ross et al. .... 181/131  
 D375,161 S 10/1996 Hart  
 5,641,464 A 6/1997 Briggs, III et al.  
 5,686,706 A \* 11/1997 Wurzbarger ..... 181/131  
 5,692,657 A \* 12/1997 Kilo et al. .... 181/131  
 5,808,244 A 9/1998 Knight et al.  
 5,813,992 A 9/1998 Henwood  
 5,865,551 A \* 2/1999 Lalli et al. .... 401/139  
 5,892,233 A \* 4/1999 Clement ..... 181/131  
 5,925,021 A 7/1999 Castellano et al.  
 6,018,835 A 2/2000 Schonfeld  
 6,019,187 A 2/2000 Appavu  
 D425,353 S 5/2000 Foy  
 6,206,134 B1 3/2001 Stark et al.  
 D445,185 S 7/2001 Najmi  
 6,461,568 B1 10/2002 Eckhardt  
 6,467,568 B1 10/2002 Kemper  
 6,484,918 B1 11/2002 Lefebvre  
 6,575,917 B2 6/2003 Giroux et al.  
 6,643,998 B1 11/2003 Curtis et al.  
 7,117,971 B1 10/2006 Cornacchia  
 7,182,117 B2 2/2007 Abe et al.  
 7,258,125 B2 8/2007 Holbrook  
 7,282,186 B2 10/2007 Lake, Jr. et al.  
 7,287,426 B2 10/2007 Frank  
 7,406,973 B1 8/2008 Perlman et al.  
 7,424,929 B1 9/2008 Martinez  
 7,469,769 B1 12/2008 Hmayakyan et al.  
 7,503,335 B2 3/2009 Perlman et al.  
 7,614,478 B2 11/2009 Hmayakyan et al.  
 7,636,445 B2 12/2009 Yoshimine  
 D621,935 S 8/2010 Cole et al.  
 7,866,908 B2 \* 1/2011 Perlman et al. .... 134/166 R  
 7,942,597 B2 \* 5/2011 Perlman et al. .... 221/222  
 8,057,117 B2 \* 11/2011 Perlman et al. .... 134/166 R  
 D652,142 S 1/2012 Cole et al.  
 2002/0146343 A1 10/2002 Jenkins et al.  
 2002/0198564 A1 12/2002 Pichon et al.  
 2004/0258560 A1 12/2004 Lake, Jr. et al.  
 2005/0214185 A1 9/2005 Castaneda  
 2005/0236579 A1 10/2005 Jenkins et al.  
 2005/0254992 A1 11/2005 Jenkins et al.  
 2007/0080017 A1 4/2007 Stickley  
 2007/0256753 A1 11/2007 Riley  
 2007/0261185 A1 11/2007 Guney et al.

2008/0019889 A1 1/2008 Rogers et al.  
 2008/0131332 A1 6/2008 Nguyen et al.  
 2009/0144918 A1 \* 6/2009 Perlman et al. .... 15/97.1  
 2009/0273477 A1 11/2009 Barnhill  
 2010/0116300 A1 \* 5/2010 Perlman et al. .... 134/133  
 2010/0116841 A1 \* 5/2010 Perlman et al. .... 221/222  
 2011/0197921 A1 8/2011 Rubin et al.  
 2012/0117792 A1 \* 5/2012 Perlman et al. .... 29/700  
 2012/0125377 A1 \* 5/2012 Perlman et al. .... 134/100.1

FOREIGN PATENT DOCUMENTS

CN 101678131 A 3/2010  
 EP 2131967 A0 12/2009  
 EP 2155265 A0 2/2010  
 JP 2010522058 3/2010  
 JP 2010522062 7/2010  
 WO WO 02/094326 A1 11/2002  
 WO WO 2008/118311 A2 10/2008  
 WO WO 2008/118401 A2 10/2008  
 WO WO 2011/103090 A1 8/2011

OTHER PUBLICATIONS

Virgo Publishing., "A Clean Sweep: Surface Cleaning in the Healthcare Environment." <http://www.vpico.com/articlemanager/printerfriendly.aspx?article=60253>; Dec. 1, 2004; 3 pg.  
 McCaughey., "Coming Clean—New York Times." <http://www.nytimes.com/2005/06/06/opinion/06mccaughey.html?ei=5088&en=d591e517f...>; Dec. 2, 2006; 1 pg.  
 Sharmila et al., "Stethoscope and Nosocomial Infection," Indian Journal of Pediatrics, 2000; 67 (3): 197-199.  
 Marinella, et al., "The Stethoscopy: A Potential Source of Nosocomial Infection?," vol. 157(7), Apr. 14, 1997, pp. 786-790, Mar. 30, 2006.  
 Jones, et al., "Stethoscopes: A Potential Vector of Infection?" Annals of Emergency Medicine. 26:3 Sep. 1995; 296-299.  
 CDC, "Contact Precautions from the Guidelines for Isolation Precautions in Hospitals (Jan. 1996)." [http://www.cdc.gov/ncidod/dhqp/gl\\_isolation\\_contact.html](http://www.cdc.gov/ncidod/dhqp/gl_isolation_contact.html); Dec. 2, 2006; 2 pg.  
 CDC, "Standard Precautions from the Guidelines for Isolation Precautions in Hospitals (Jan. 1996)." [http://www.cdc.gov/ncidod/dhqp/gl\\_isolation\\_standar.html](http://www.cdc.gov/ncidod/dhqp/gl_isolation_standar.html); Dec. 2, 2006; 2 pg.  
 Schneider, "Report of the Council on Science and Public Health—CSAPH's Sunet Review of 1996 House Policies".  
 "American Medical Association Proceedings of the House of Delegates," 50th Interim Meeting, Dec. 8-11, 1996. Resolution 501. Policy H-440. 908.

\* cited by examiner



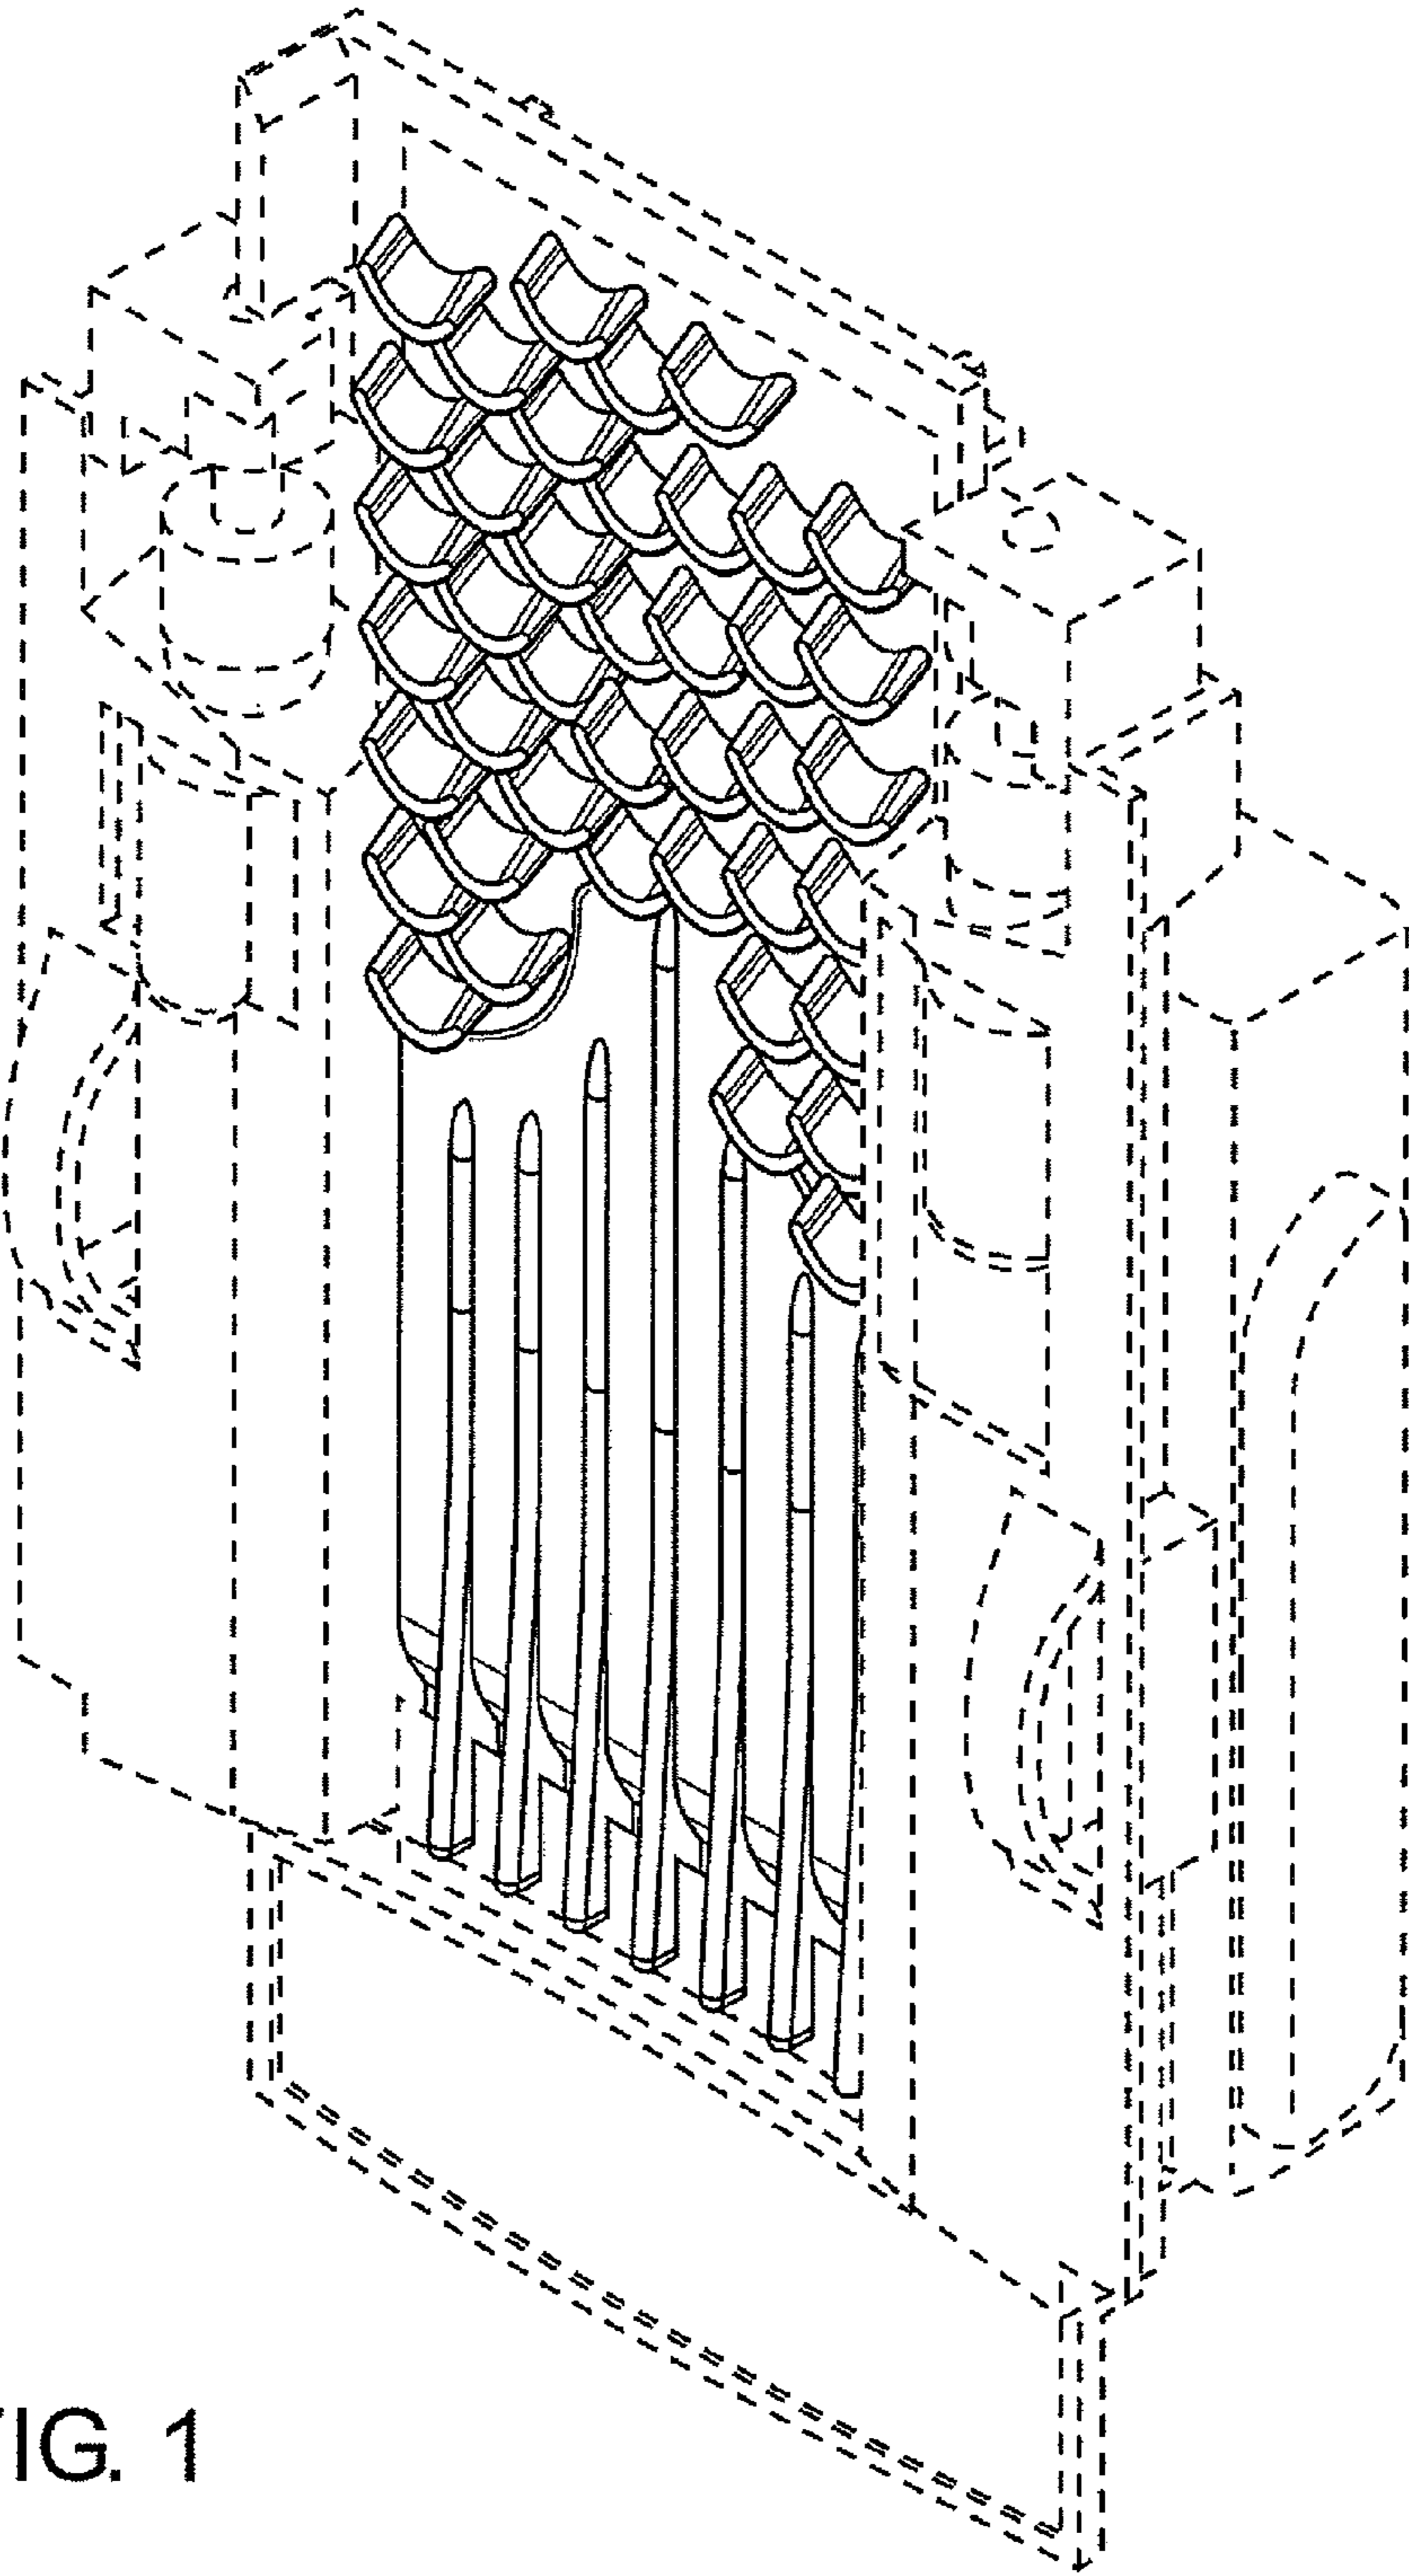


FIG. 1

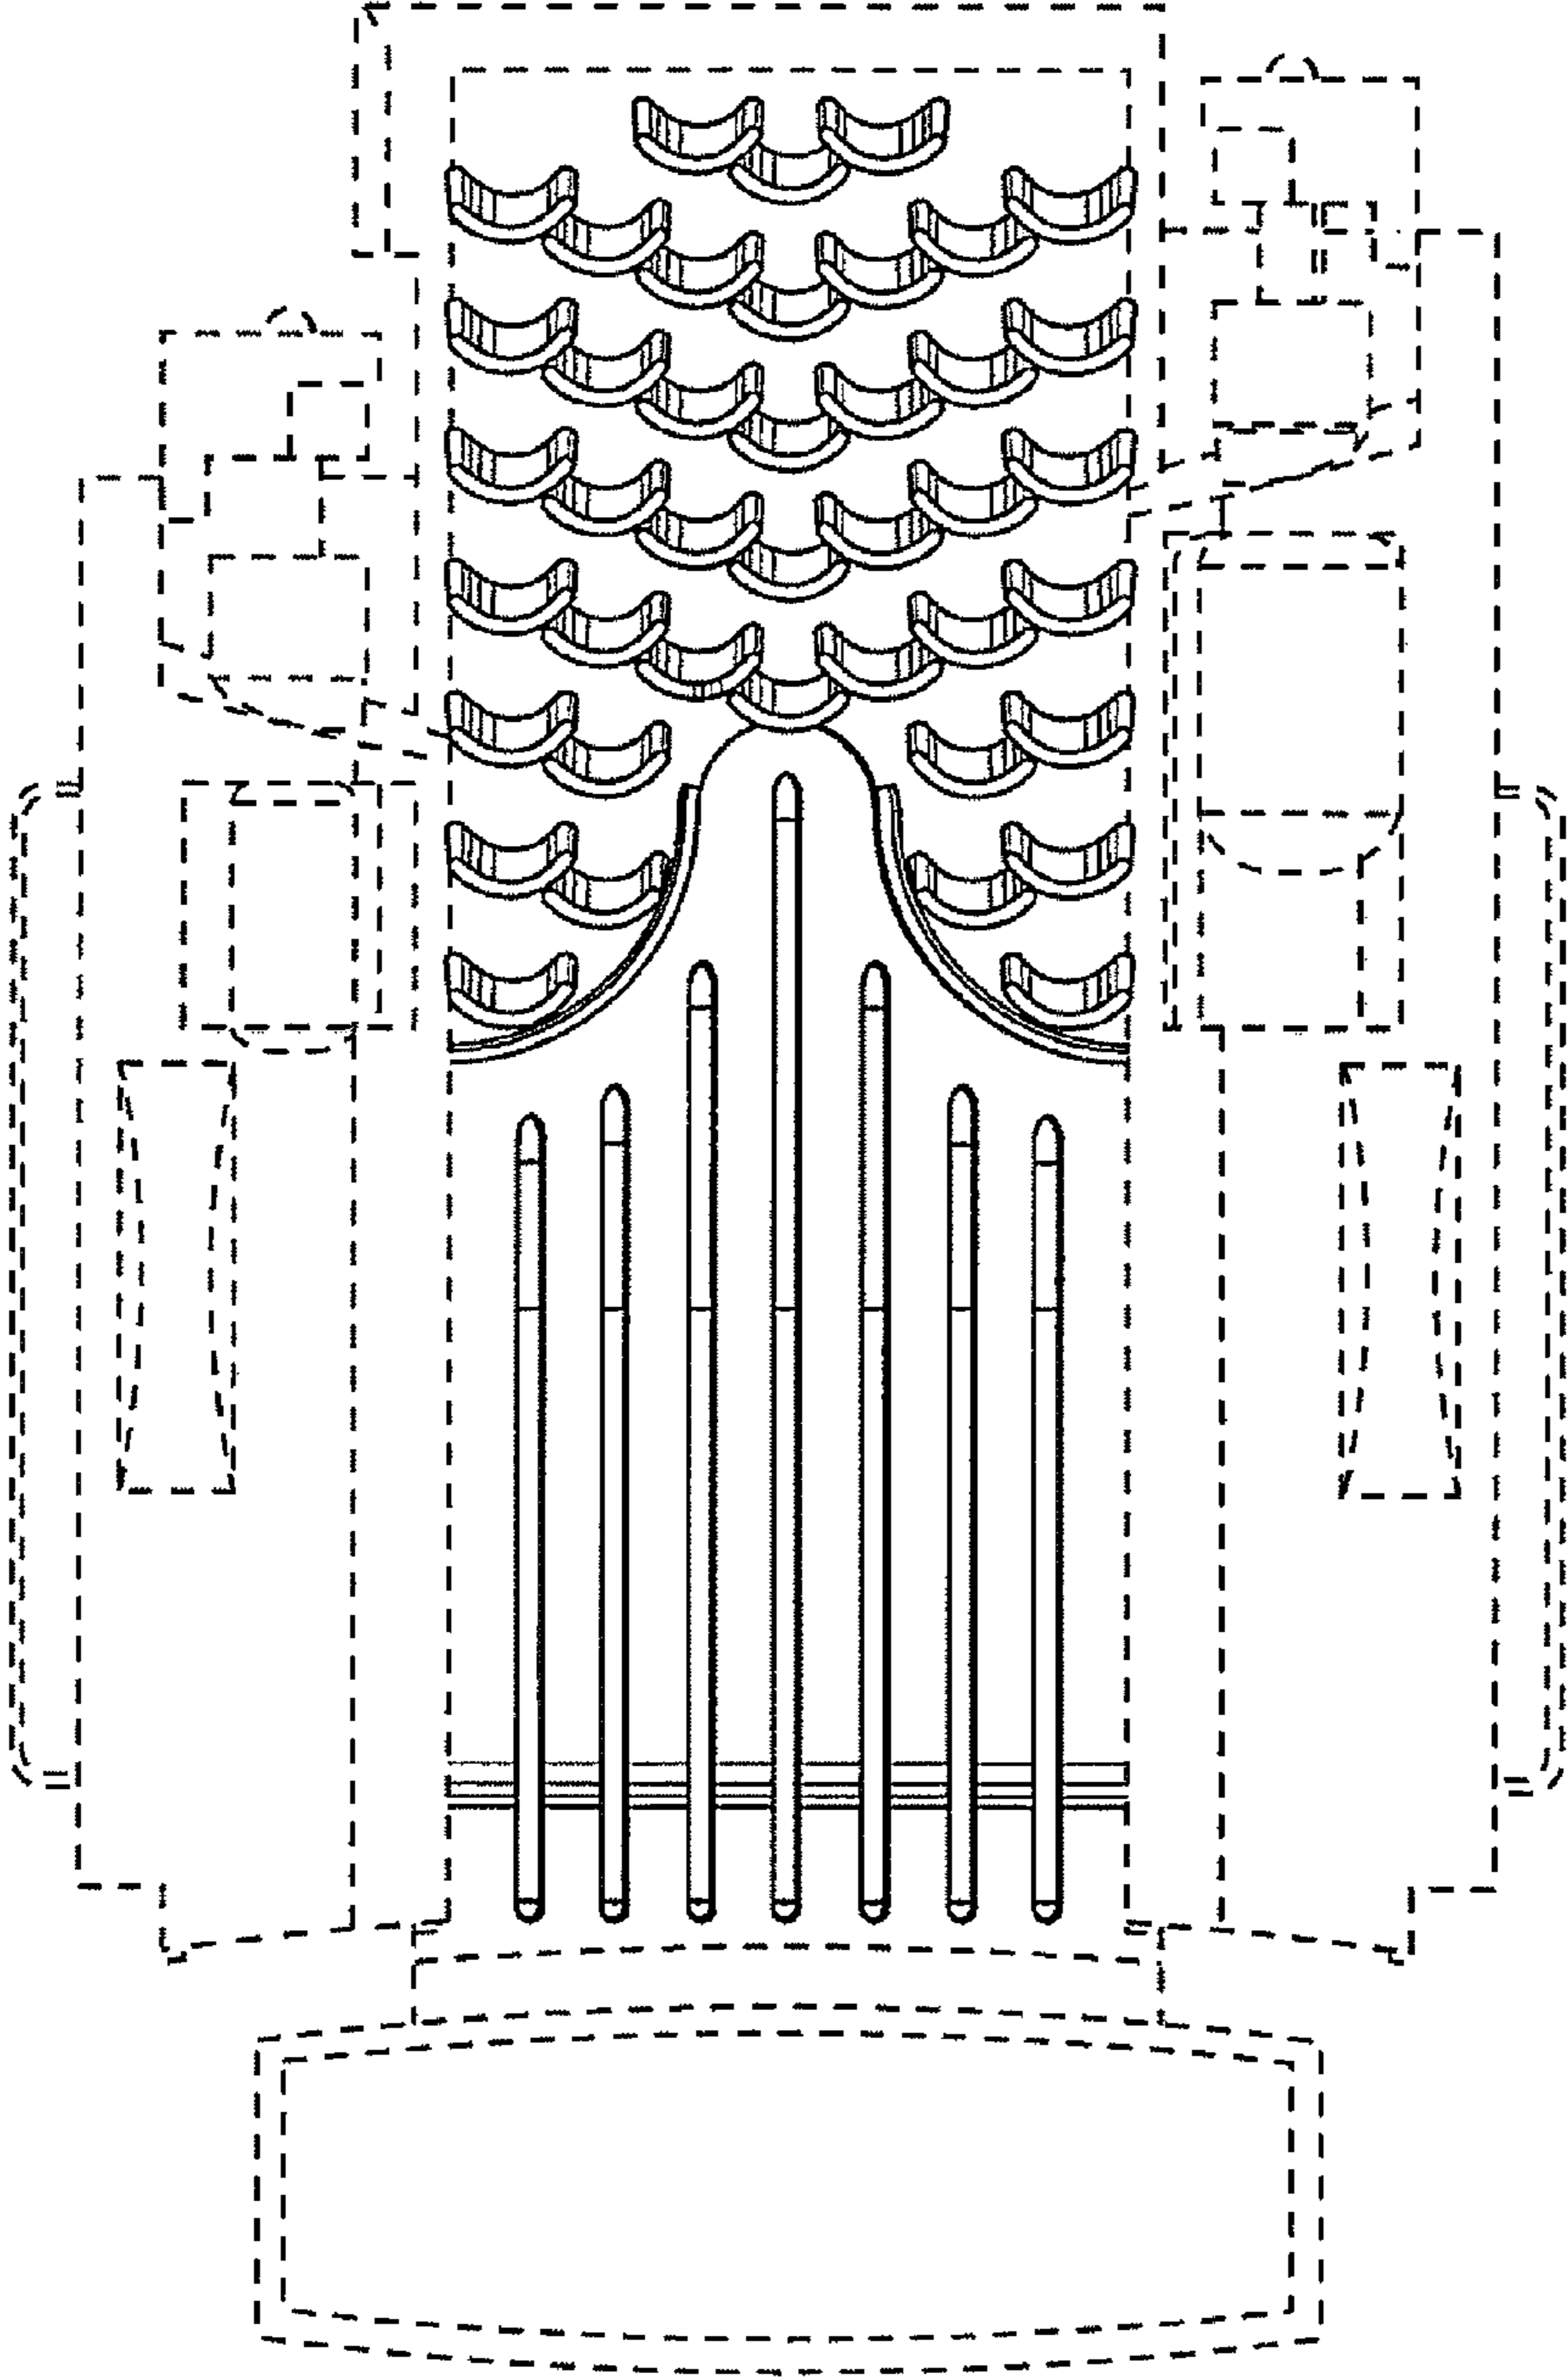


FIG. 2

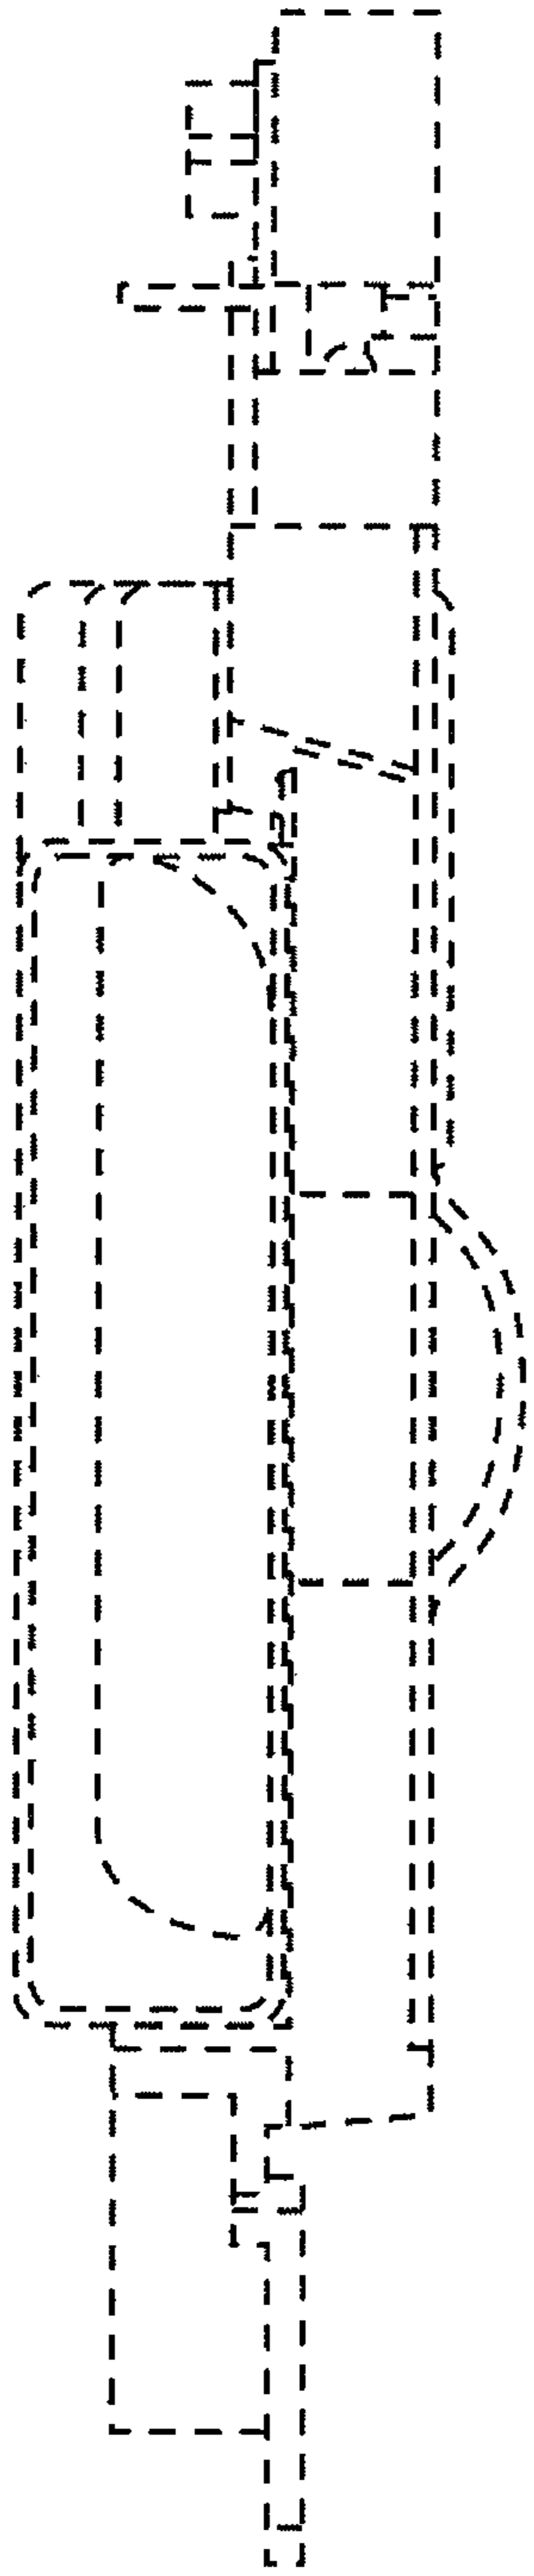


FIG. 3

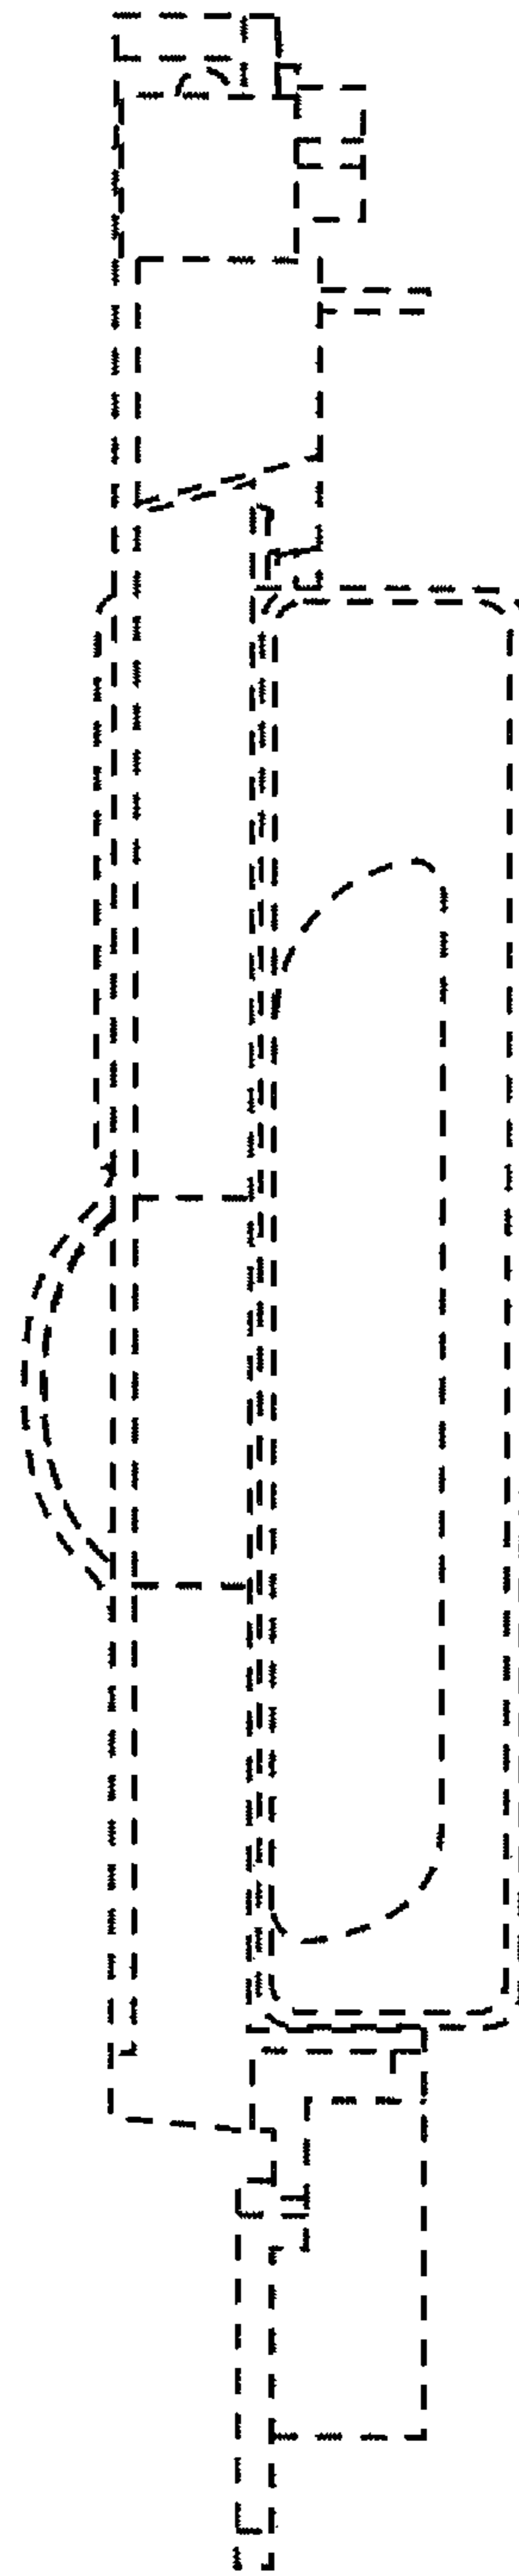


FIG. 5

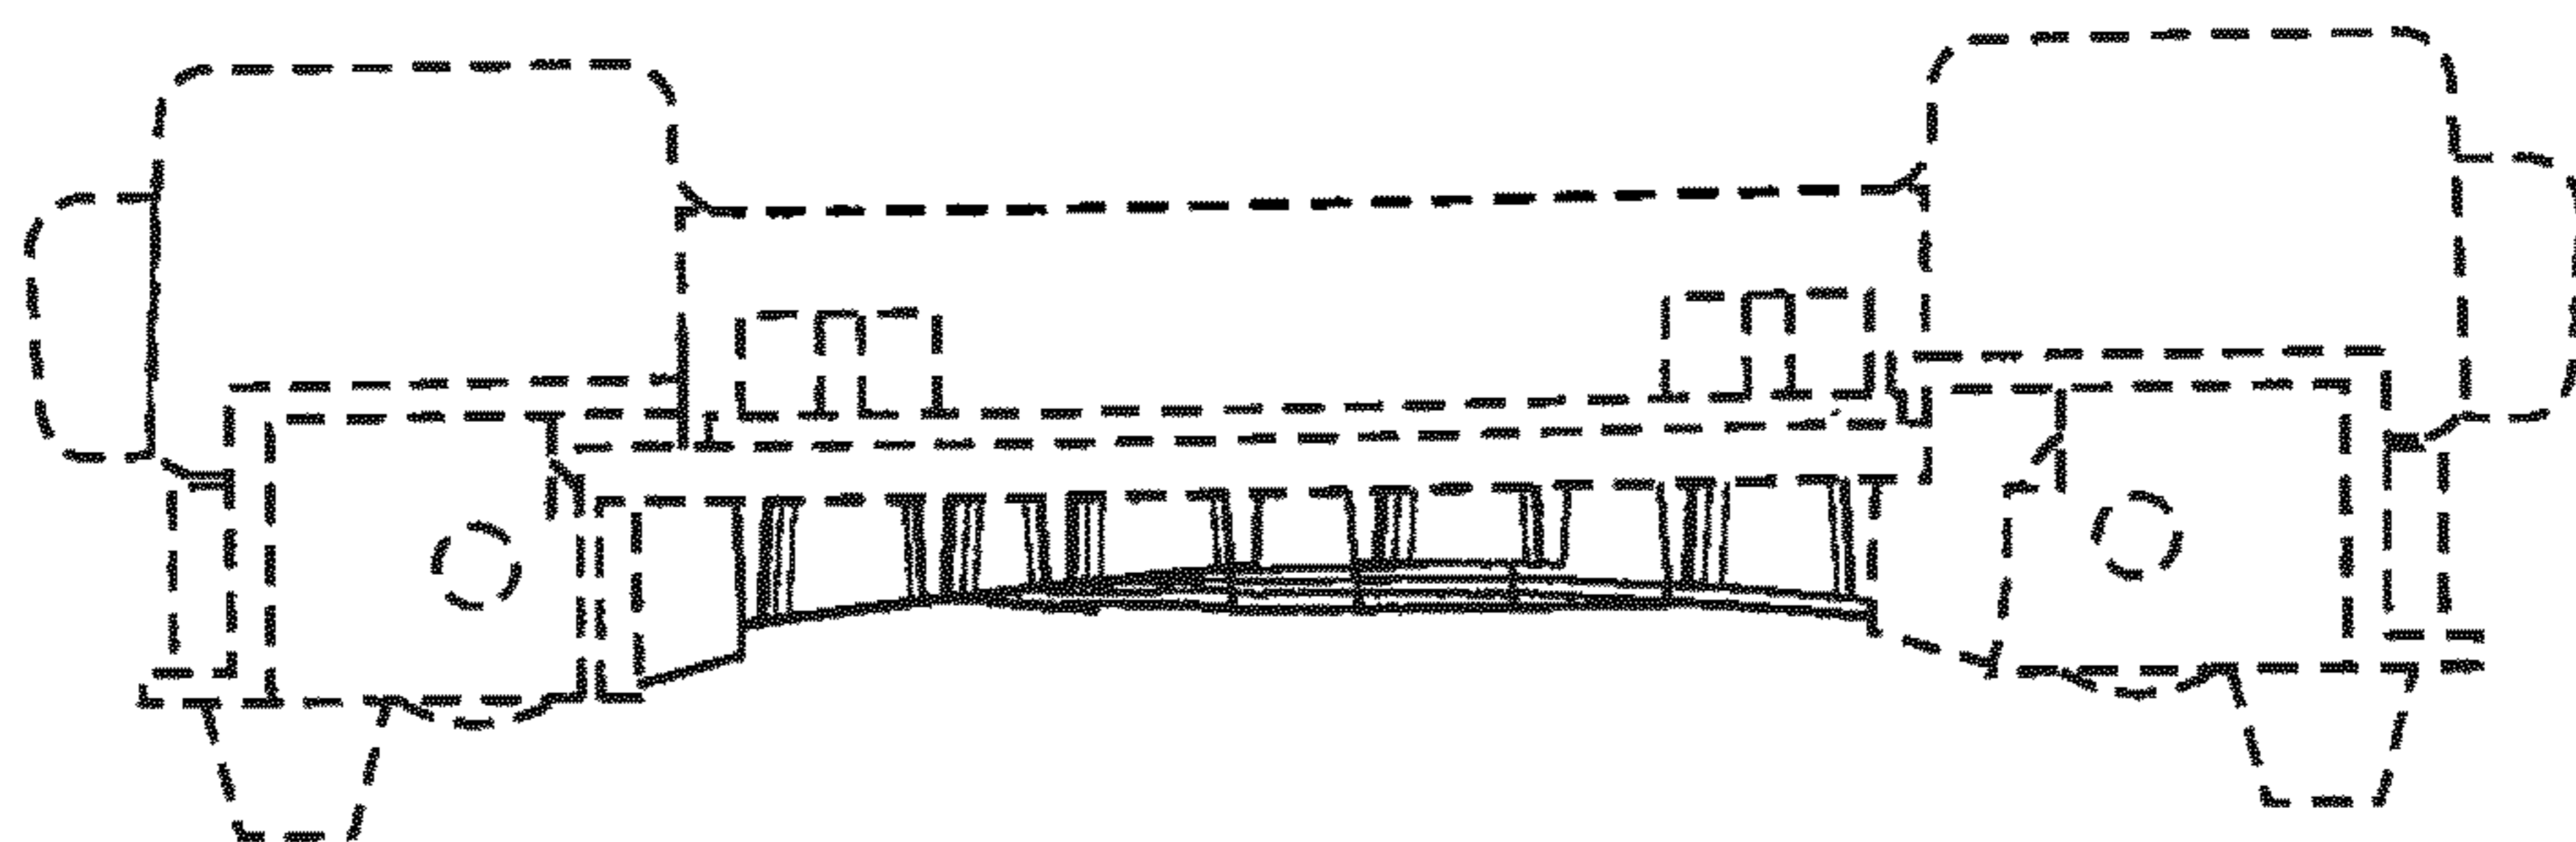


FIG. 4

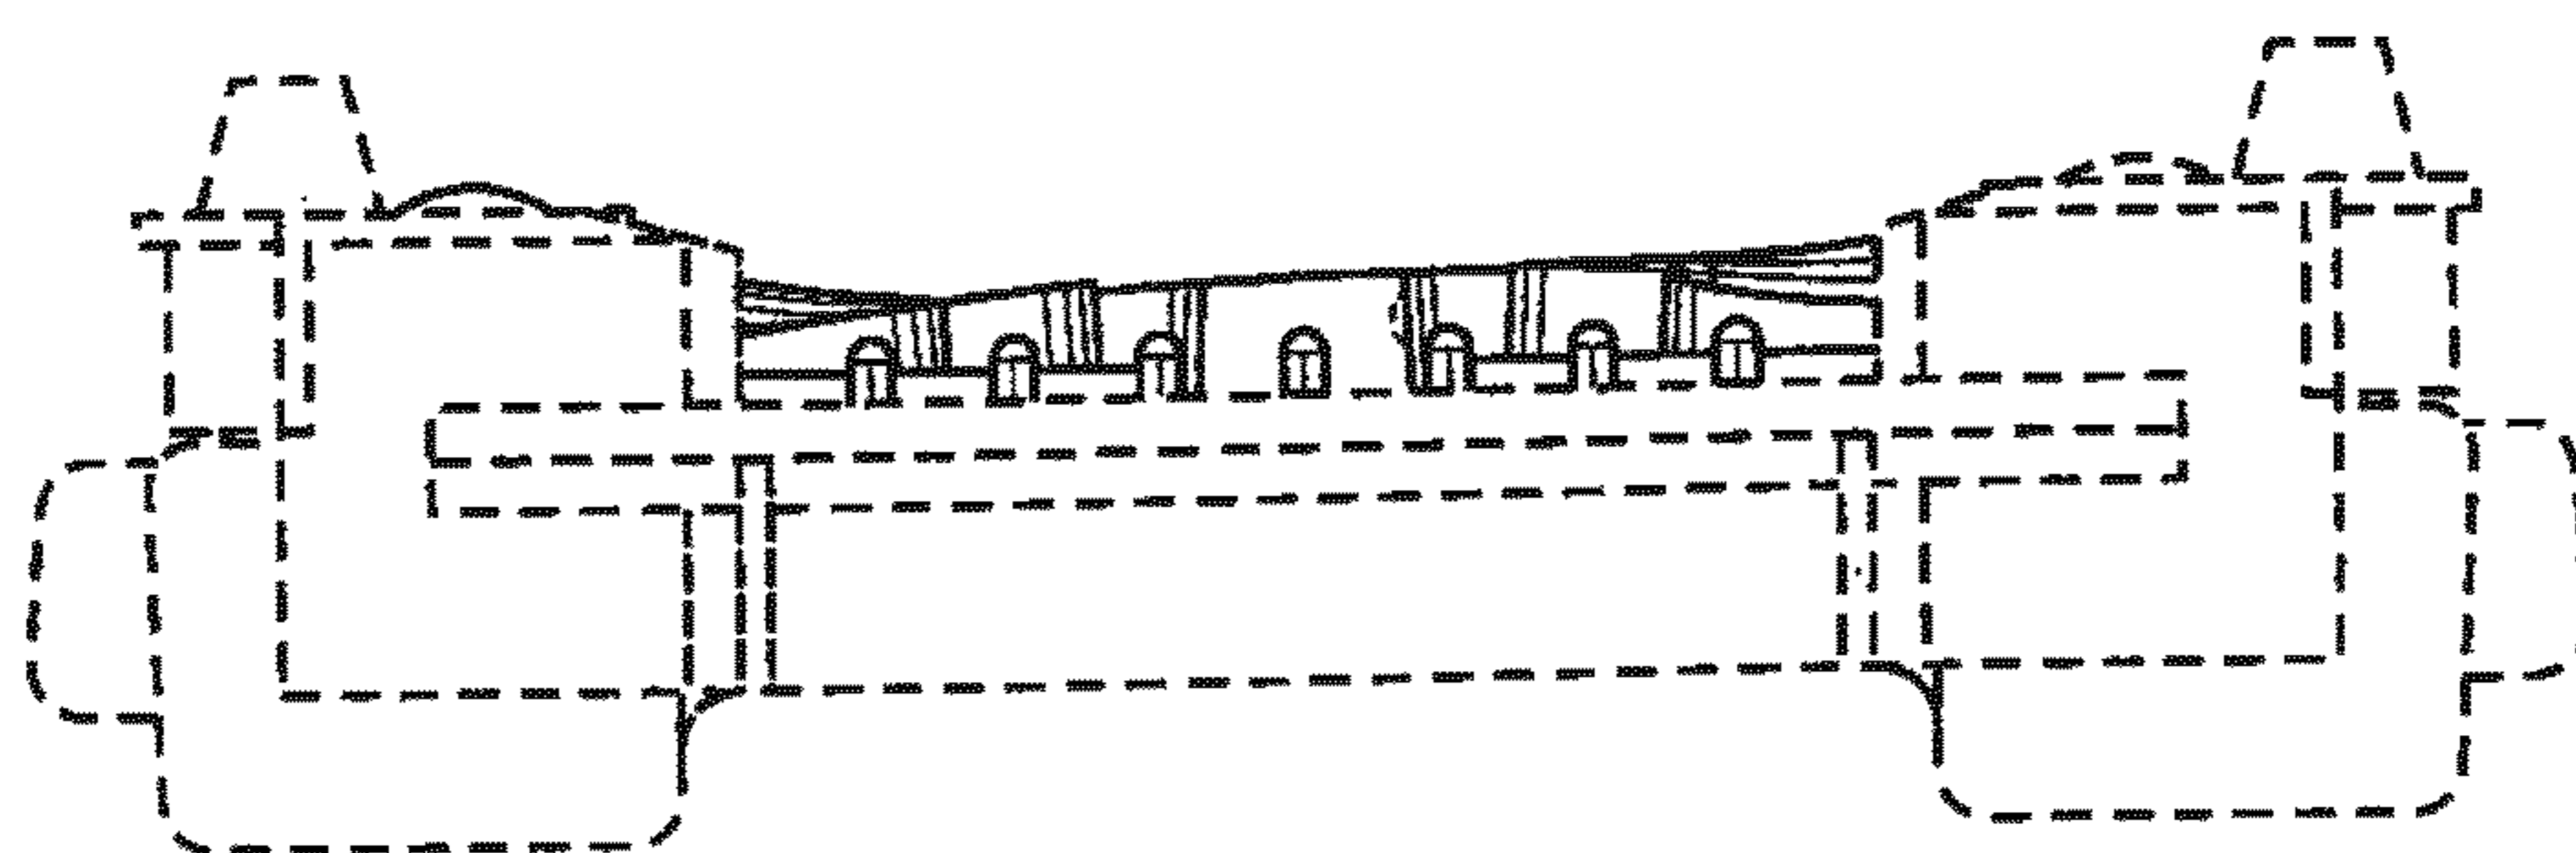


FIG. 6

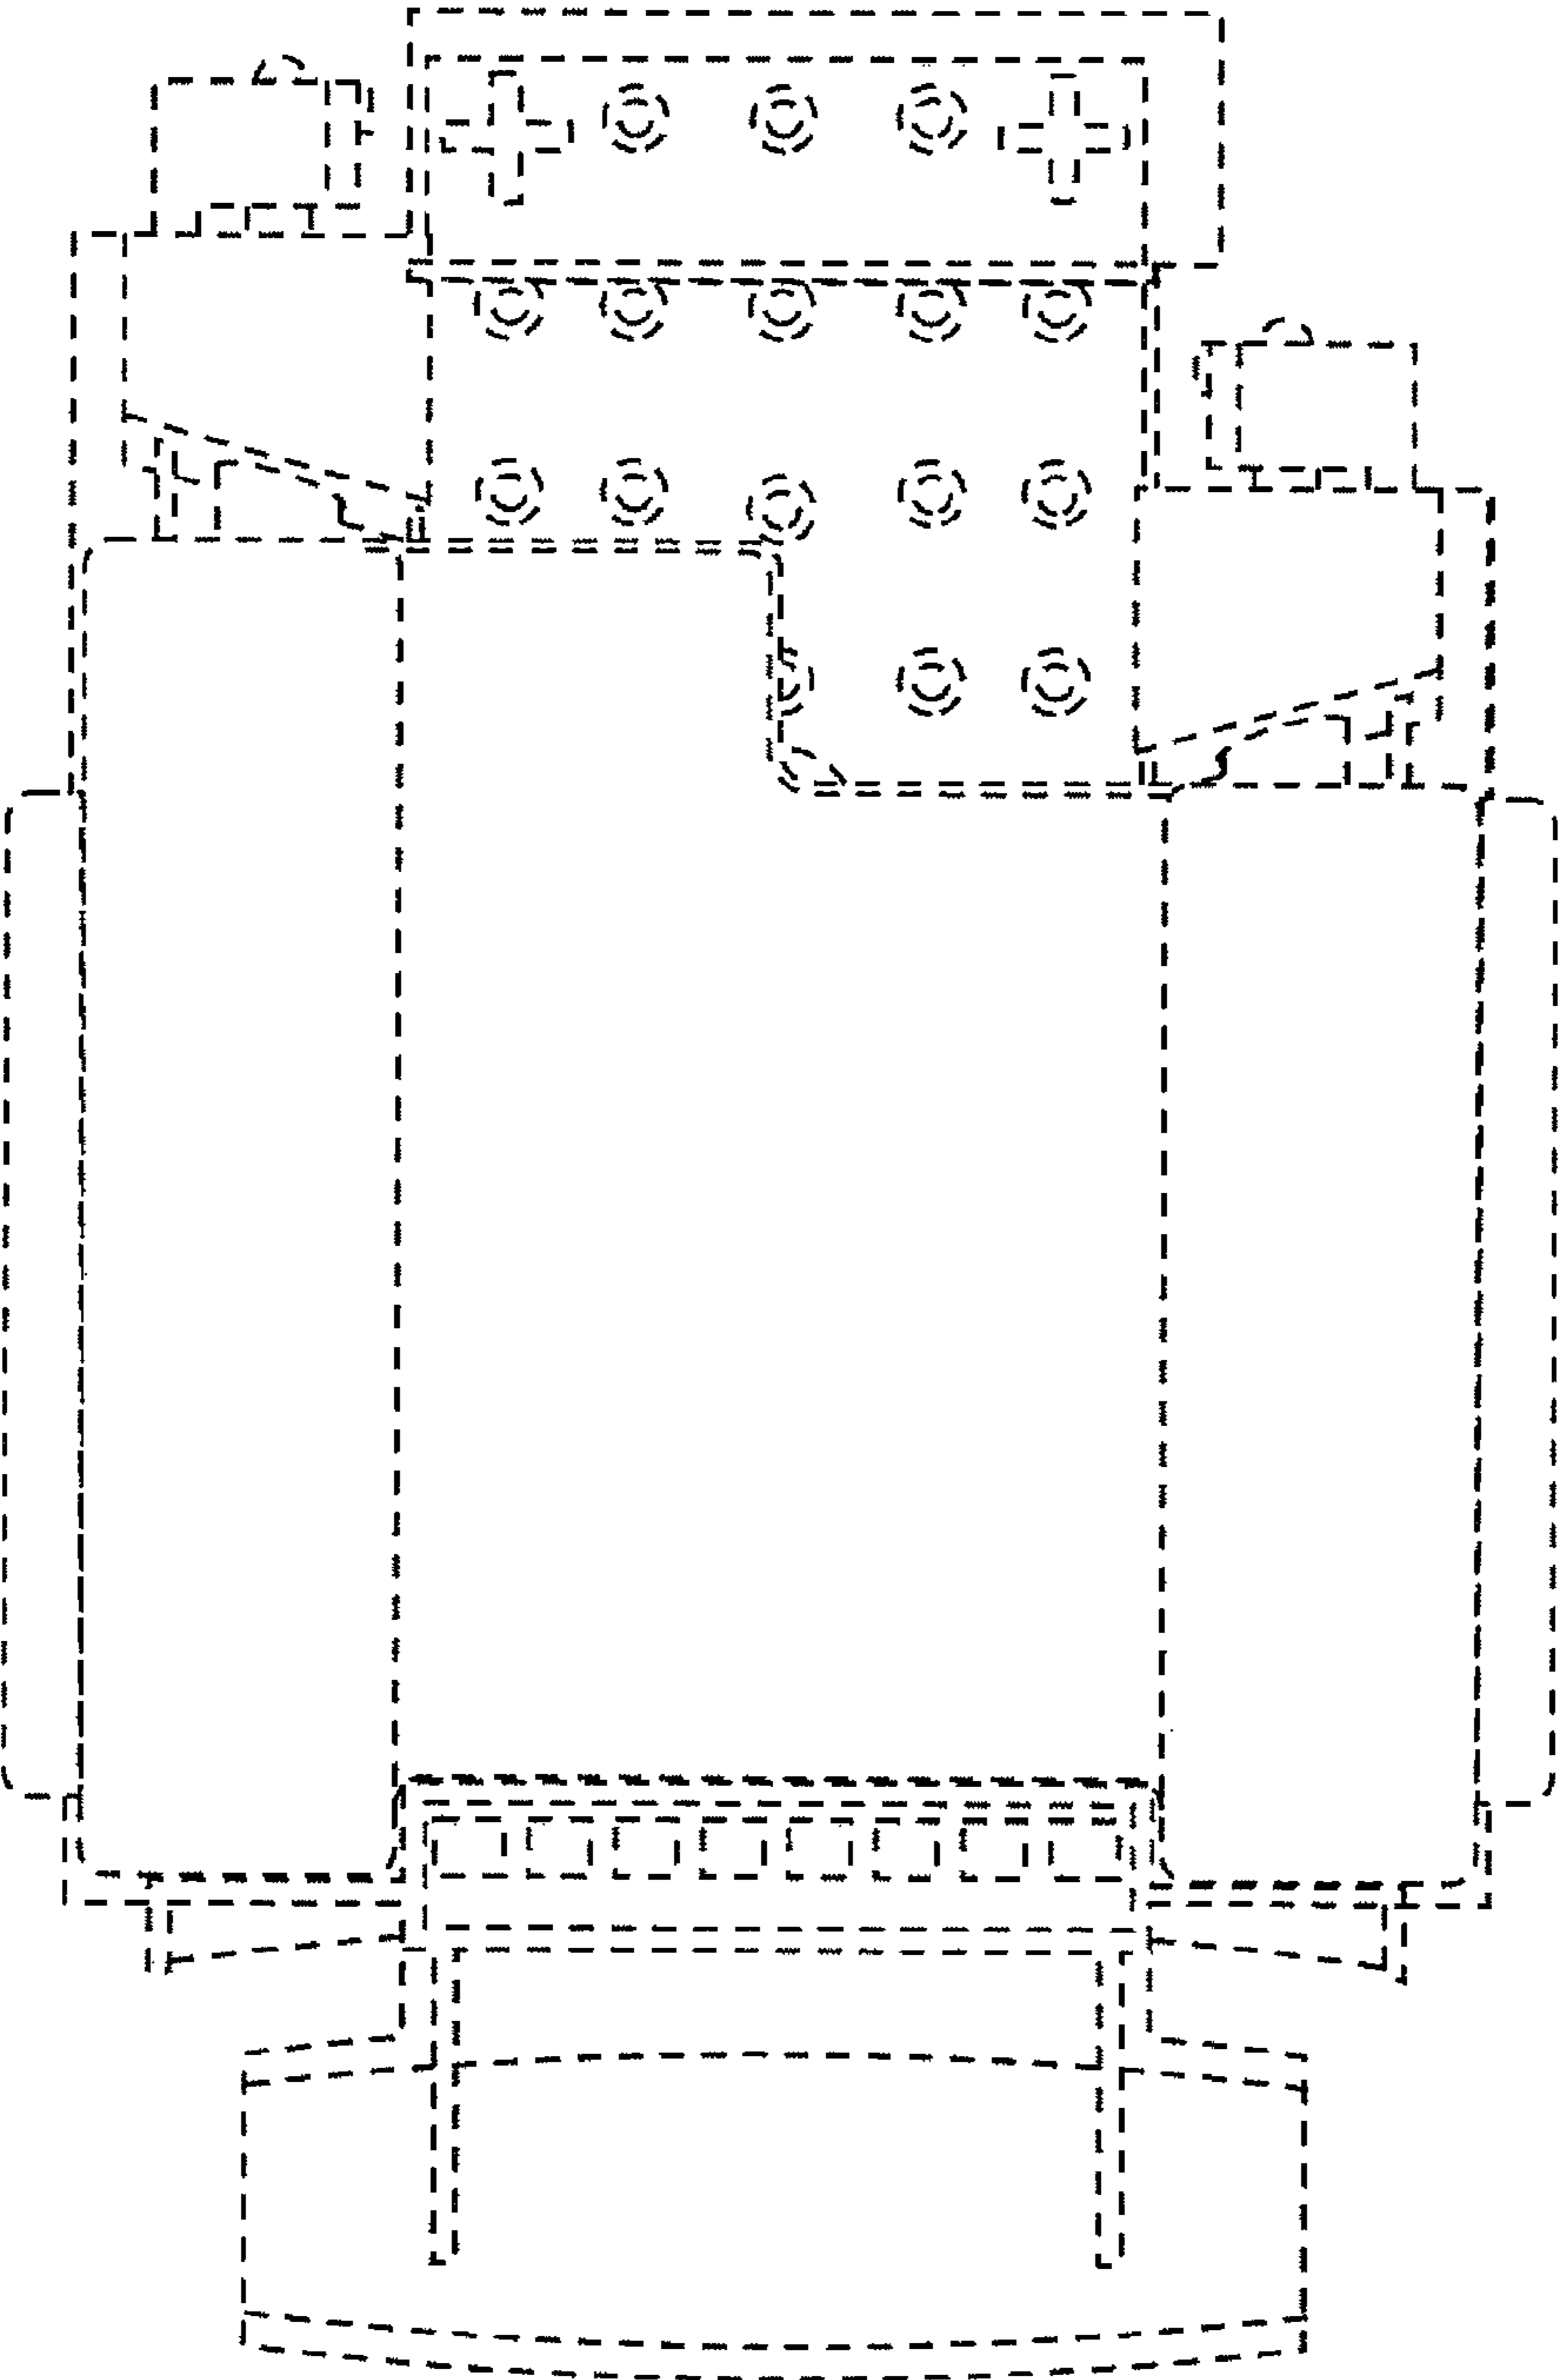


FIG. 7



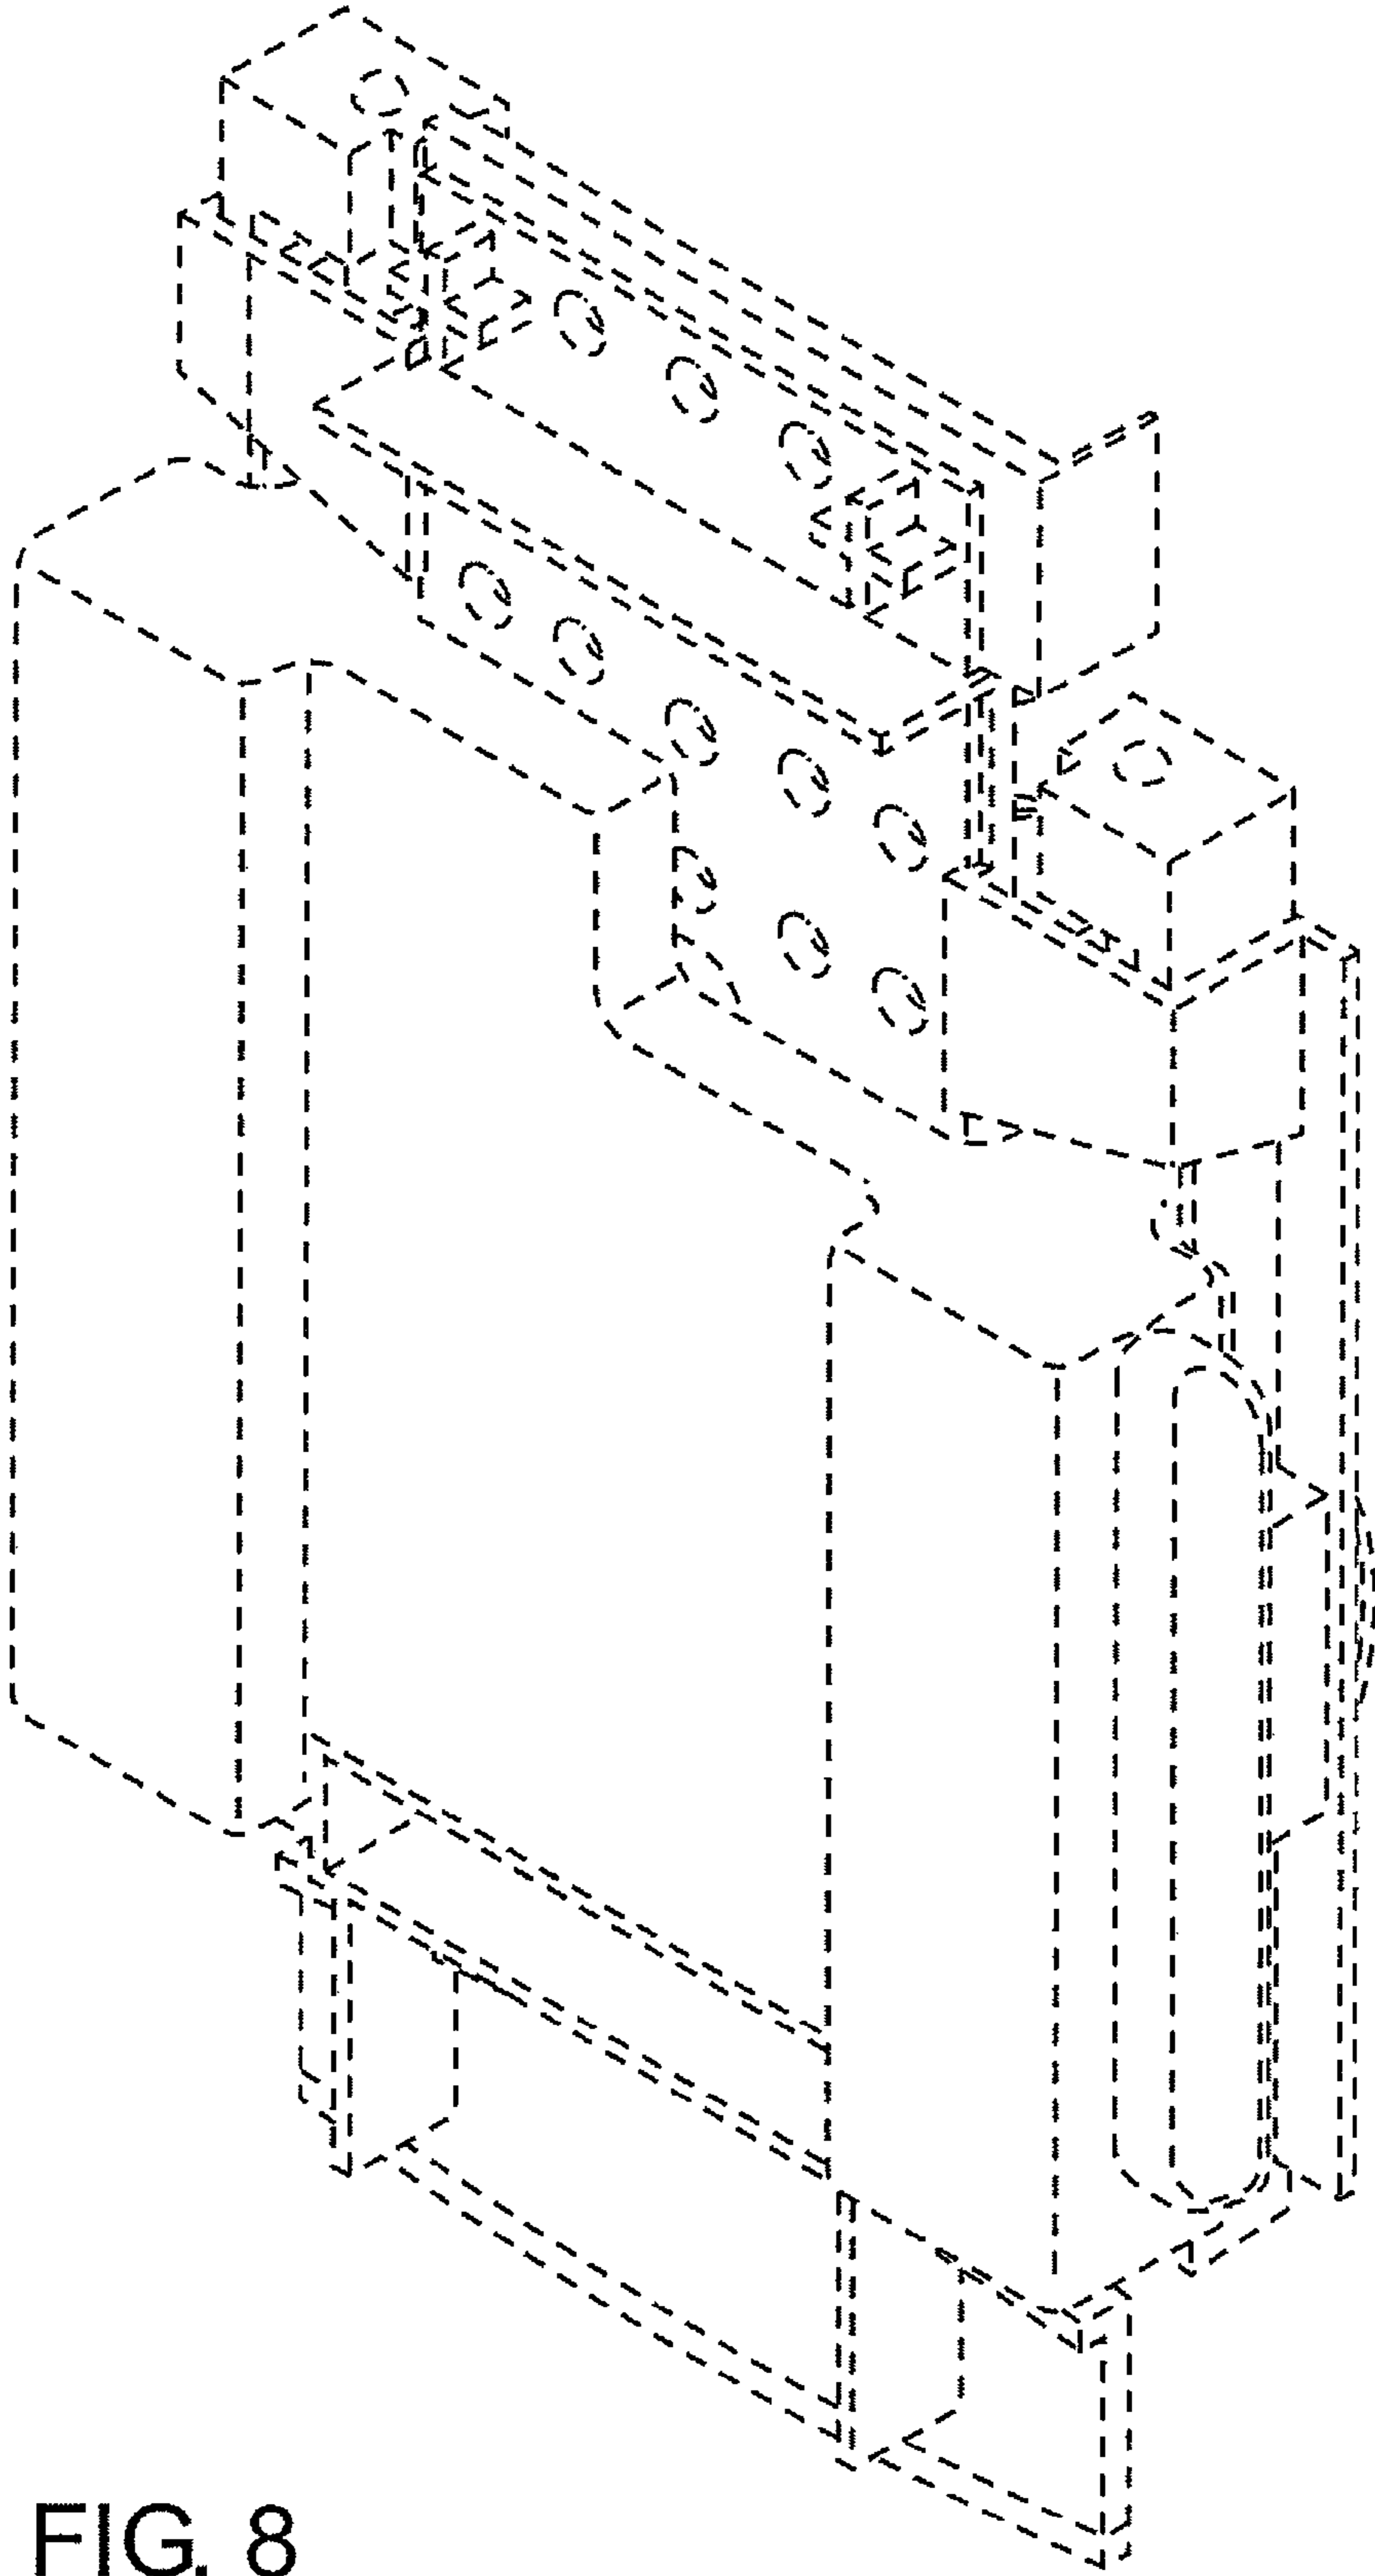


FIG. 8