

US00D685493S

(12) **United States Design Patent**
Sato et al.

(10) **Patent No.:** **US D685,493 S**
(45) **Date of Patent:** **** Jul. 2, 2013**

(54) **SAMPLE TUBE HOLDER STOCKER FOR CLINICAL LABORATORY AUTOMATION SYSTEM**

D653,766 S * 2/2012 Oonuma et al. D24/216
D655,823 S * 3/2012 Oonuma et al. D24/216
D658,776 S 5/2012 Oonuma et al.

* cited by examiner

(75) Inventors: **Yoko Sato**, Fuchu (JP); **Mitsuru Oonuma**, Tokyo (JP); **Hiroaki Sakai**, Kasama (JP); **Naoto Tsujimura**, Hitachinaka (JP)

Primary Examiner — Anhdao Doan
(74) *Attorney, Agent, or Firm* — Antonelli, Terry, Stout & Kraus, LLP.

(73) Assignee: **Hitachi High-Technologies Corporation**, Tokyo (JP)

(57) **CLAIM**
We claim the ornamental design for a sample tube holder stocker for clinical laboratory automation system, as shown and described.

(**) Term: **14 Years**

(21) Appl. No.: **29/411,274**

DESCRIPTION

(22) Filed: **Jan. 19, 2012**

(30) **Foreign Application Priority Data**

Sep. 30, 2011 (JP) 2011-022524

(51) **LOC (9) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/216**

(58) **Field of Classification Search**
USPC D24/216, 217, 219, 231, 232, 107,
D24/169, 186; D10/81; 422/62-65, 67; 436/43,
436/45, 47
See application file for complete search history.


FIG. 1 is a front, top and right side perspective view of a sample tube holder stocker for clinical laboratory automation system showing our new design;
FIG. 2 is a front elevational view thereof;
FIG. 3 is a rear elevational view thereof;
FIG. 4 is a left side elevational view thereof;
FIG. 5 is a right side elevational view thereof;
FIG. 6 is a top plan view thereof; and,
FIG. 7 is a bottom plan view thereof;
FIG. 8 is a right side elevational view thereof showing in an opened position;
FIG. 9 is a cross sectional view taken along the lines 9-9 of FIG. 2; and,
FIG. 10 is a cross sectional view taken along the lines 10-10 of FIG. 5.
The broken lines in the drawing views are included for the purpose of illustrating portions of the sample tube holder stocker for clinical laboratory automation system that form no part of the claimed design.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D380,551 S * 7/1997 Ohnuma et al. D24/186
6,521,183 B1 * 2/2003 Burri et al. 422/65
D631,976 S * 2/2011 Oonuma et al. D24/216
D637,730 S * 5/2011 Oonuma et al. D24/216

1 Claim, 8 Drawing Sheets

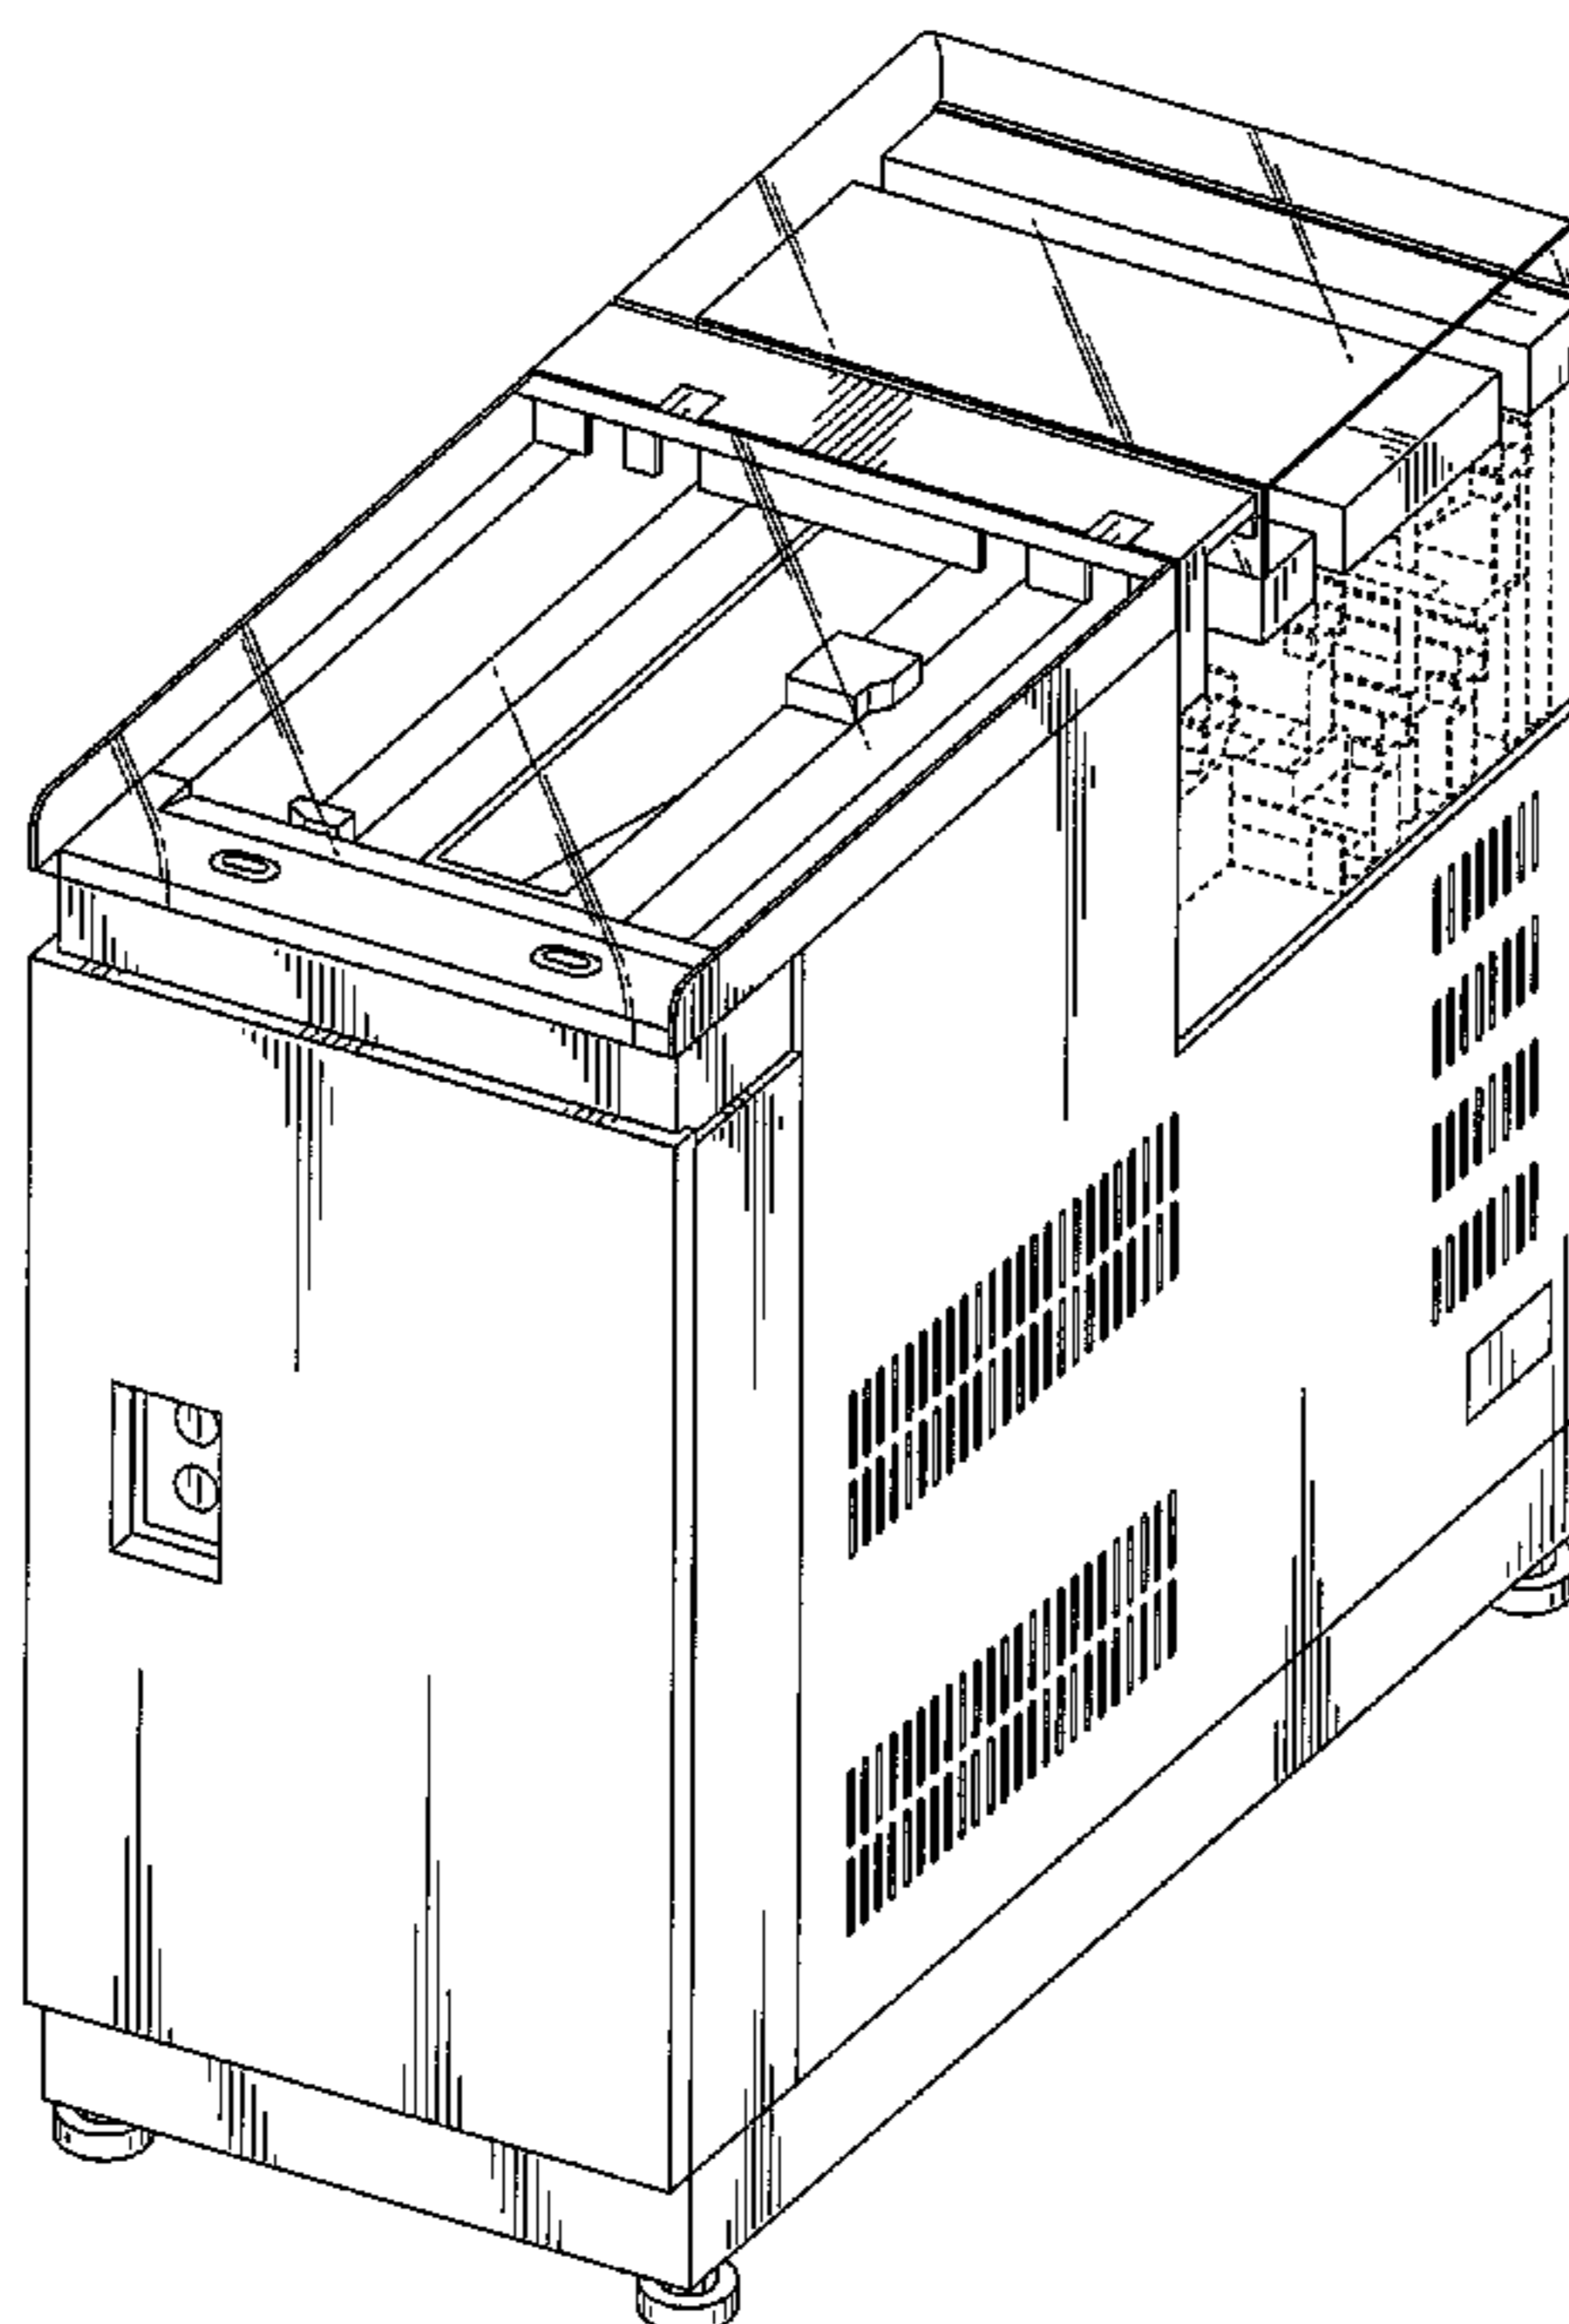


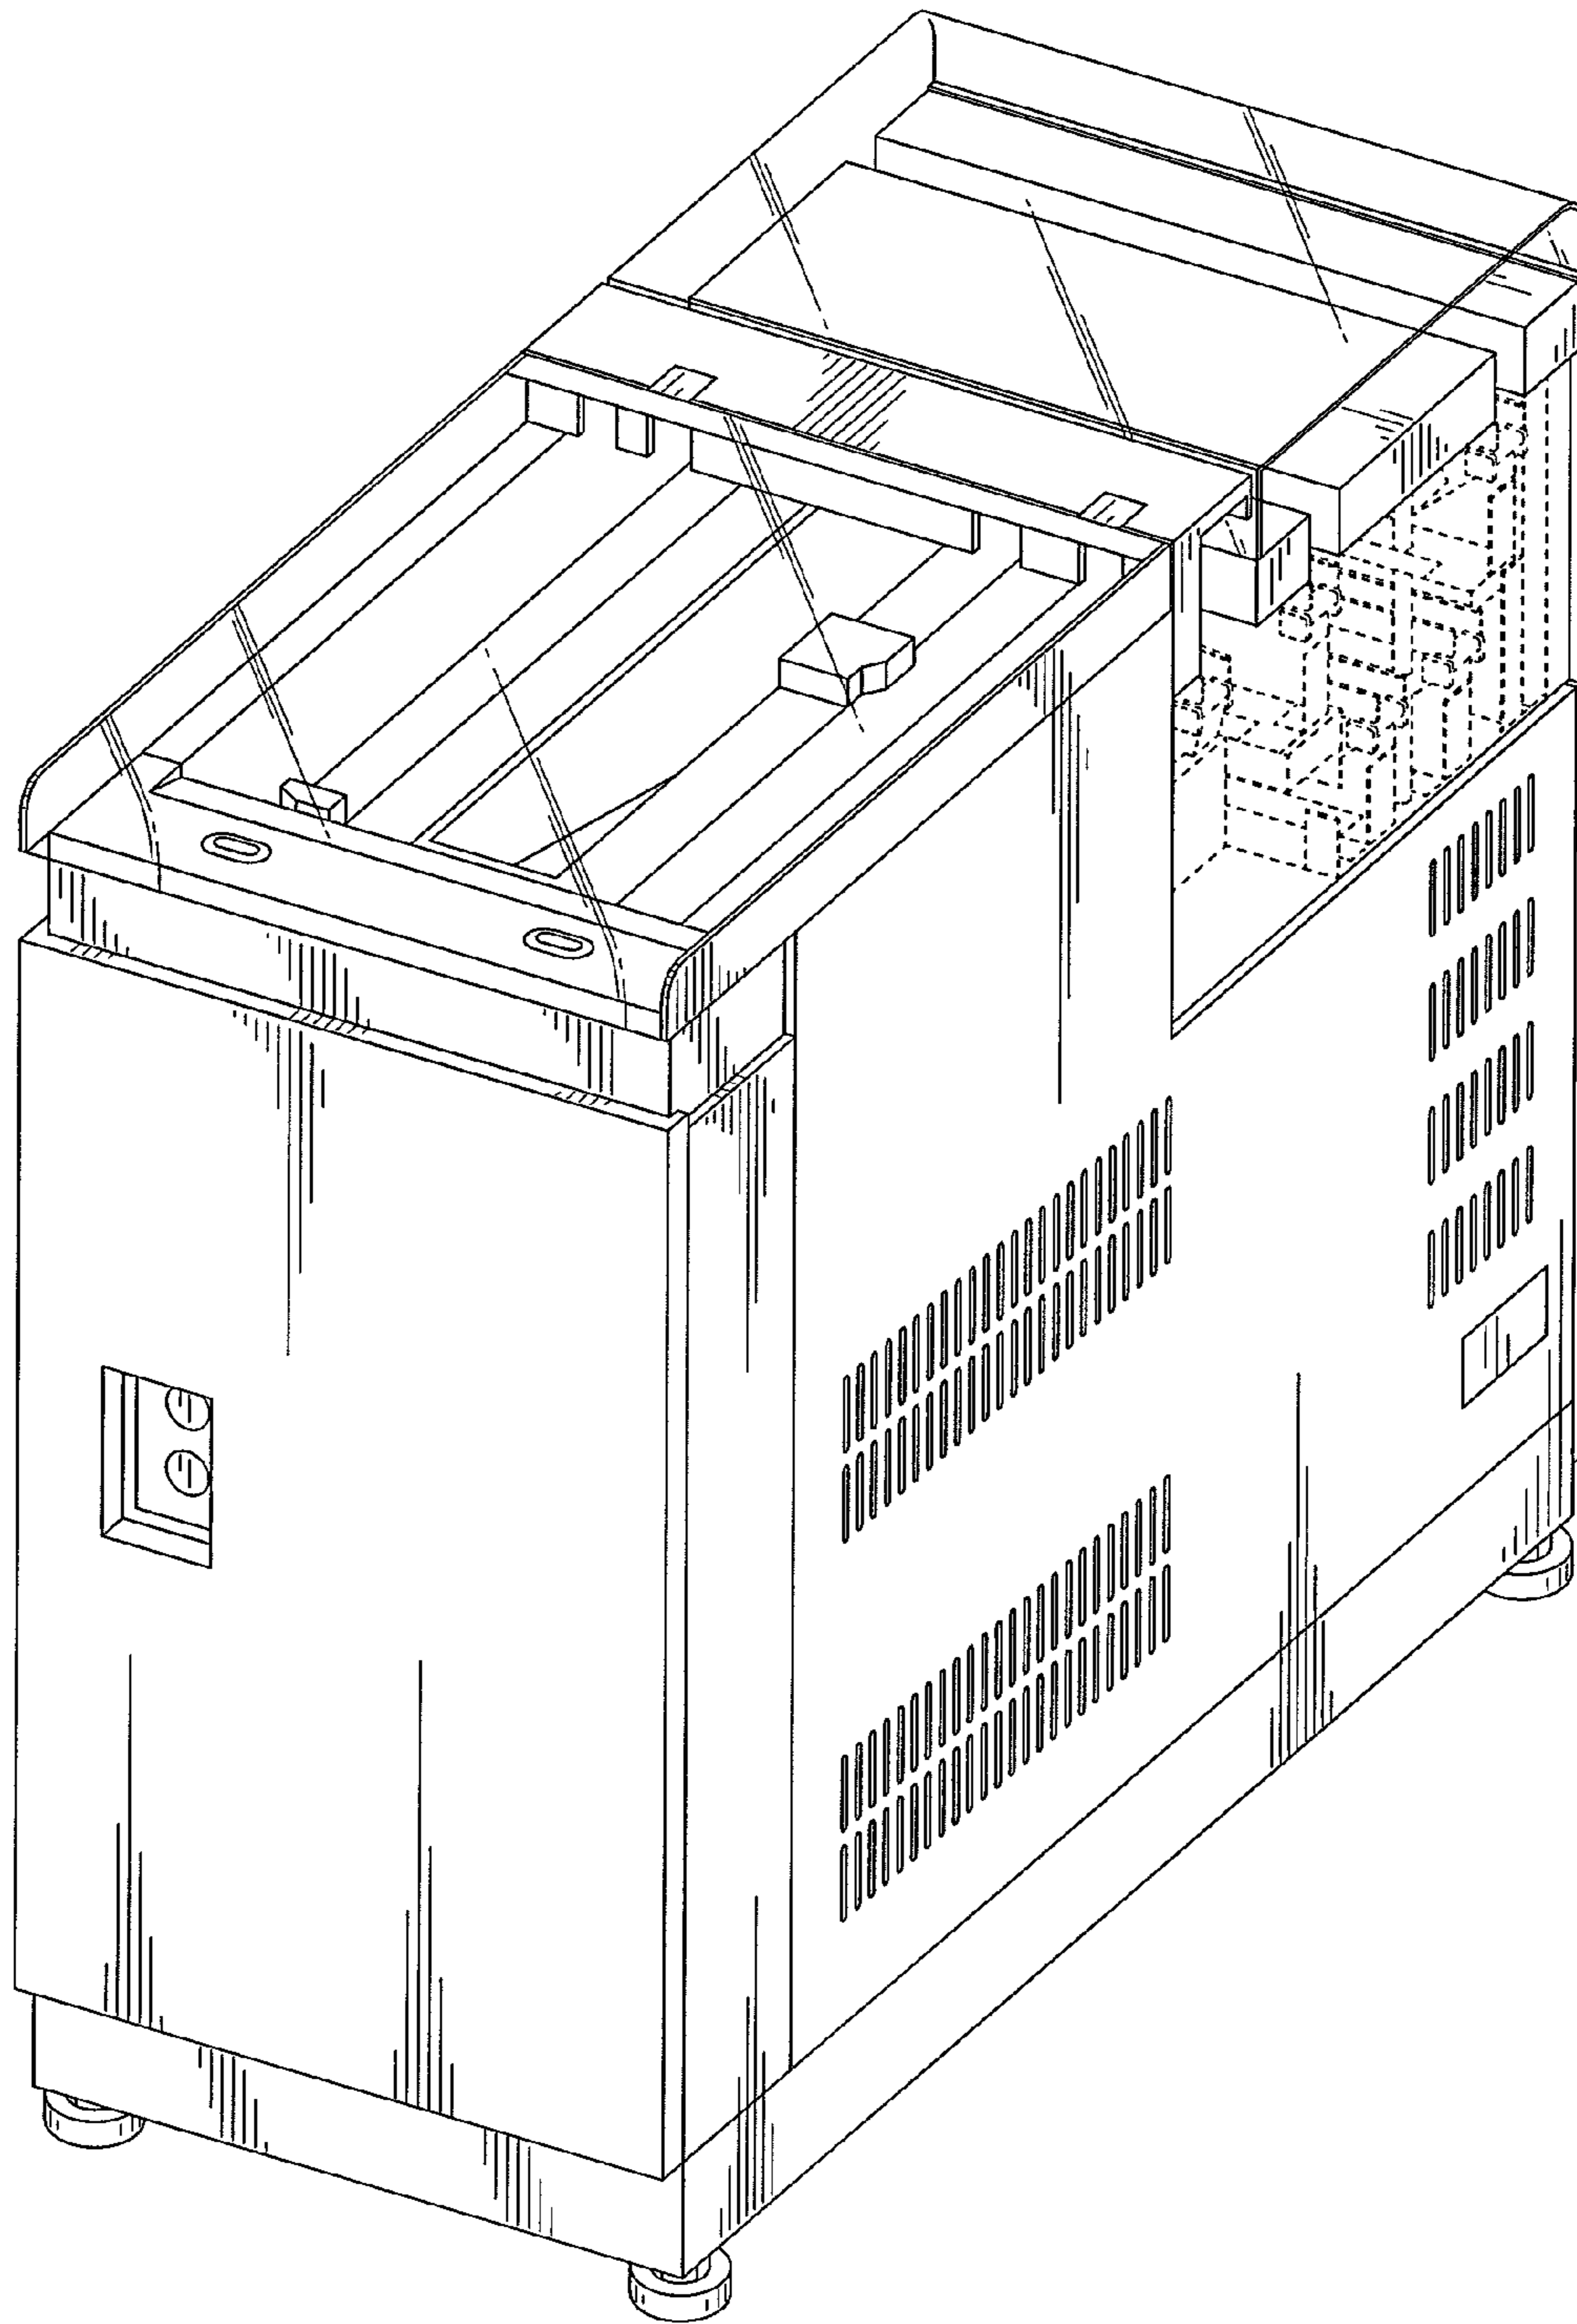


FIG. 1

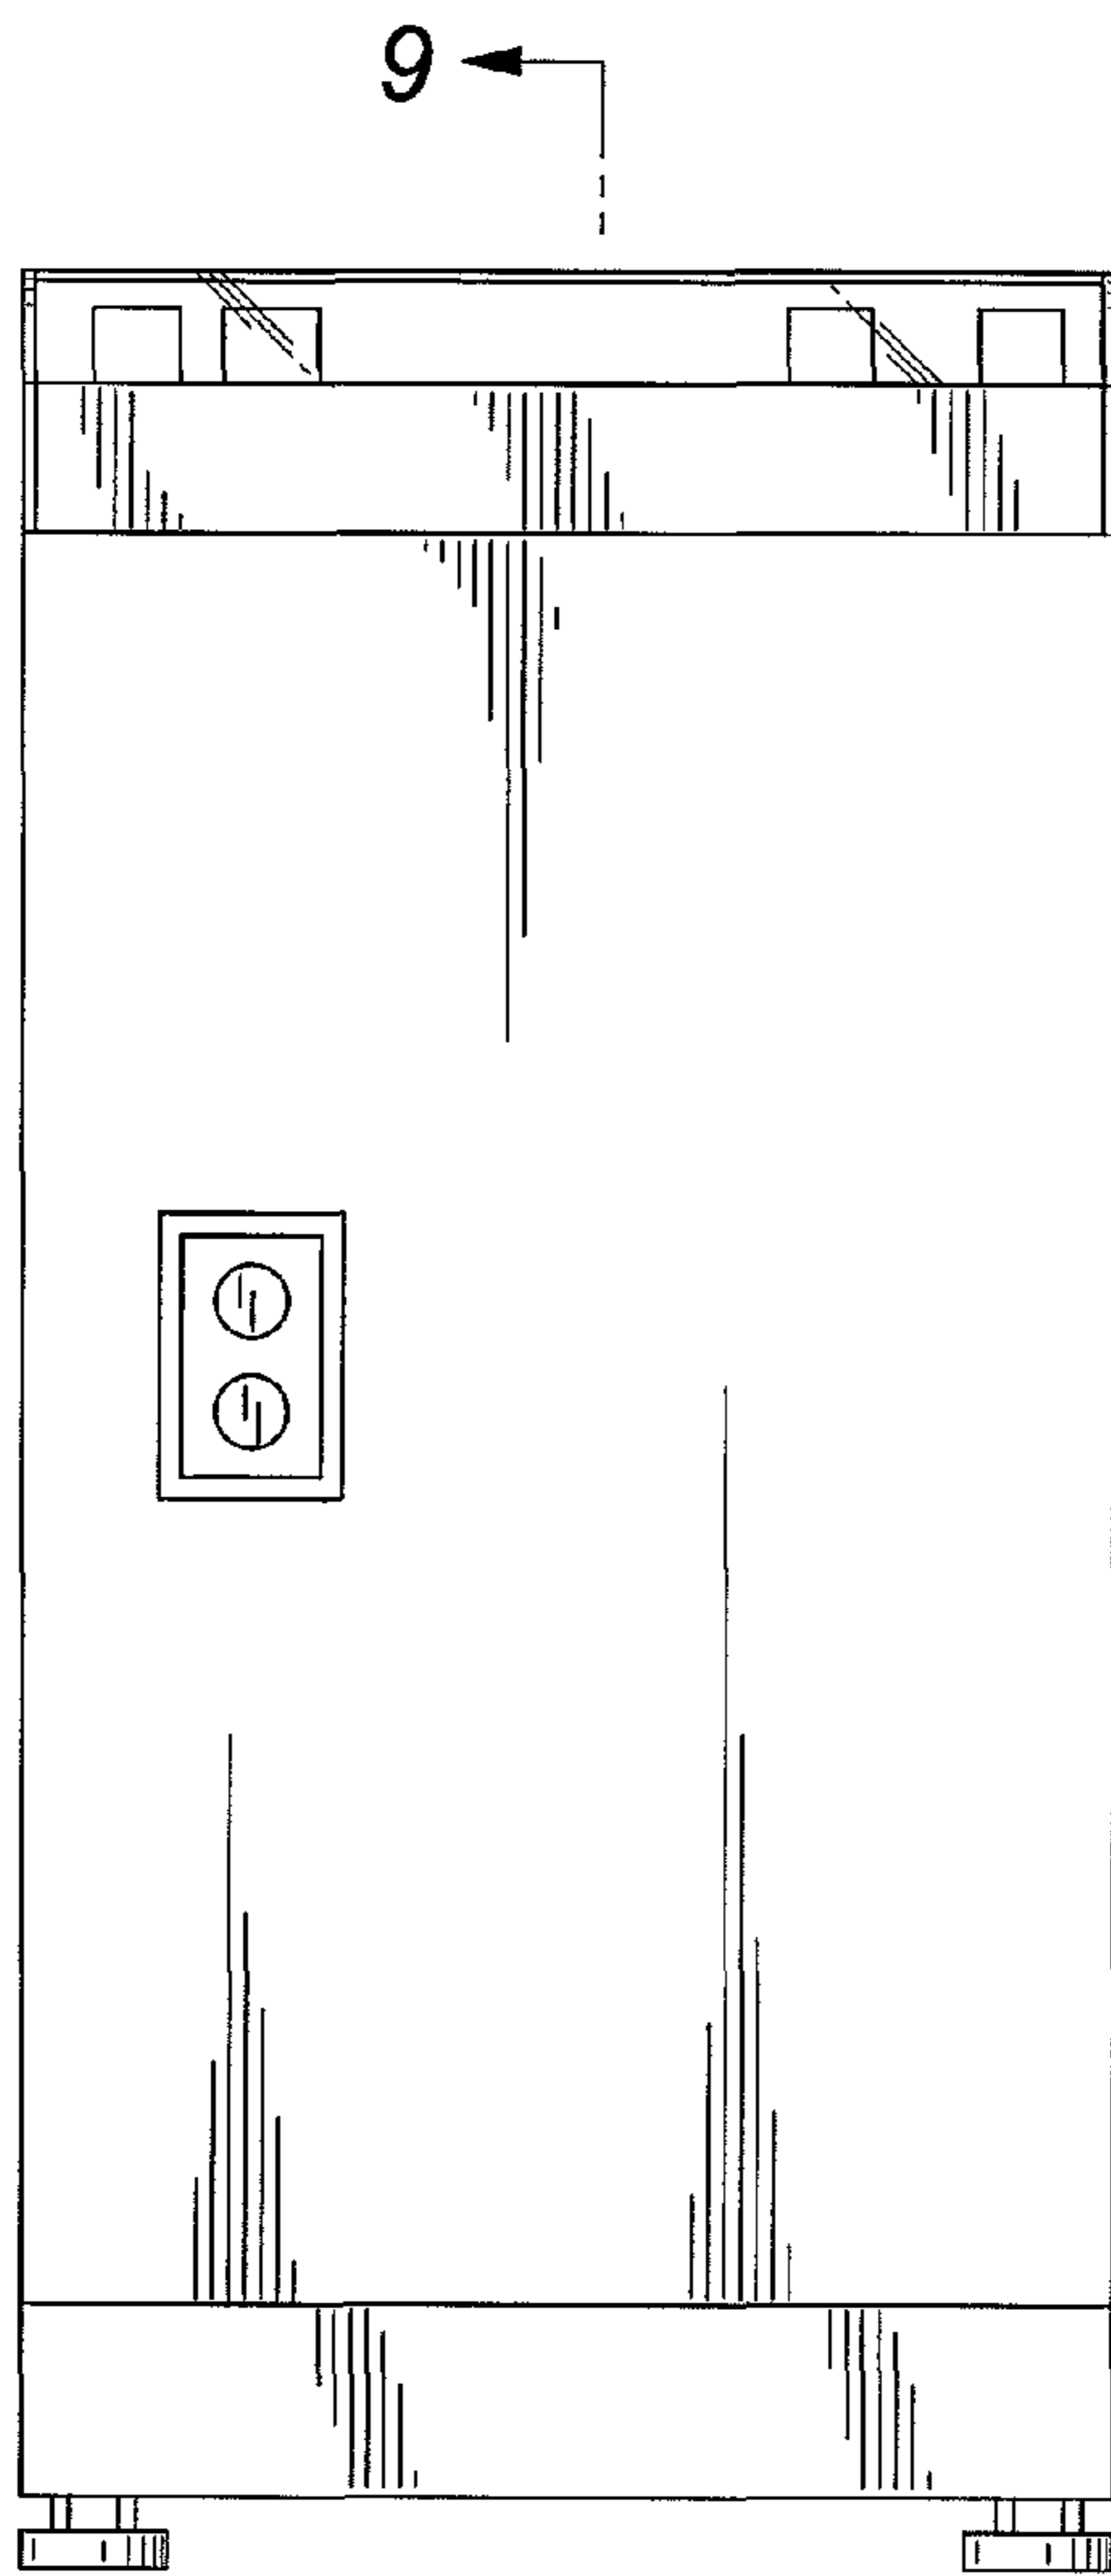

9
FIG. 2

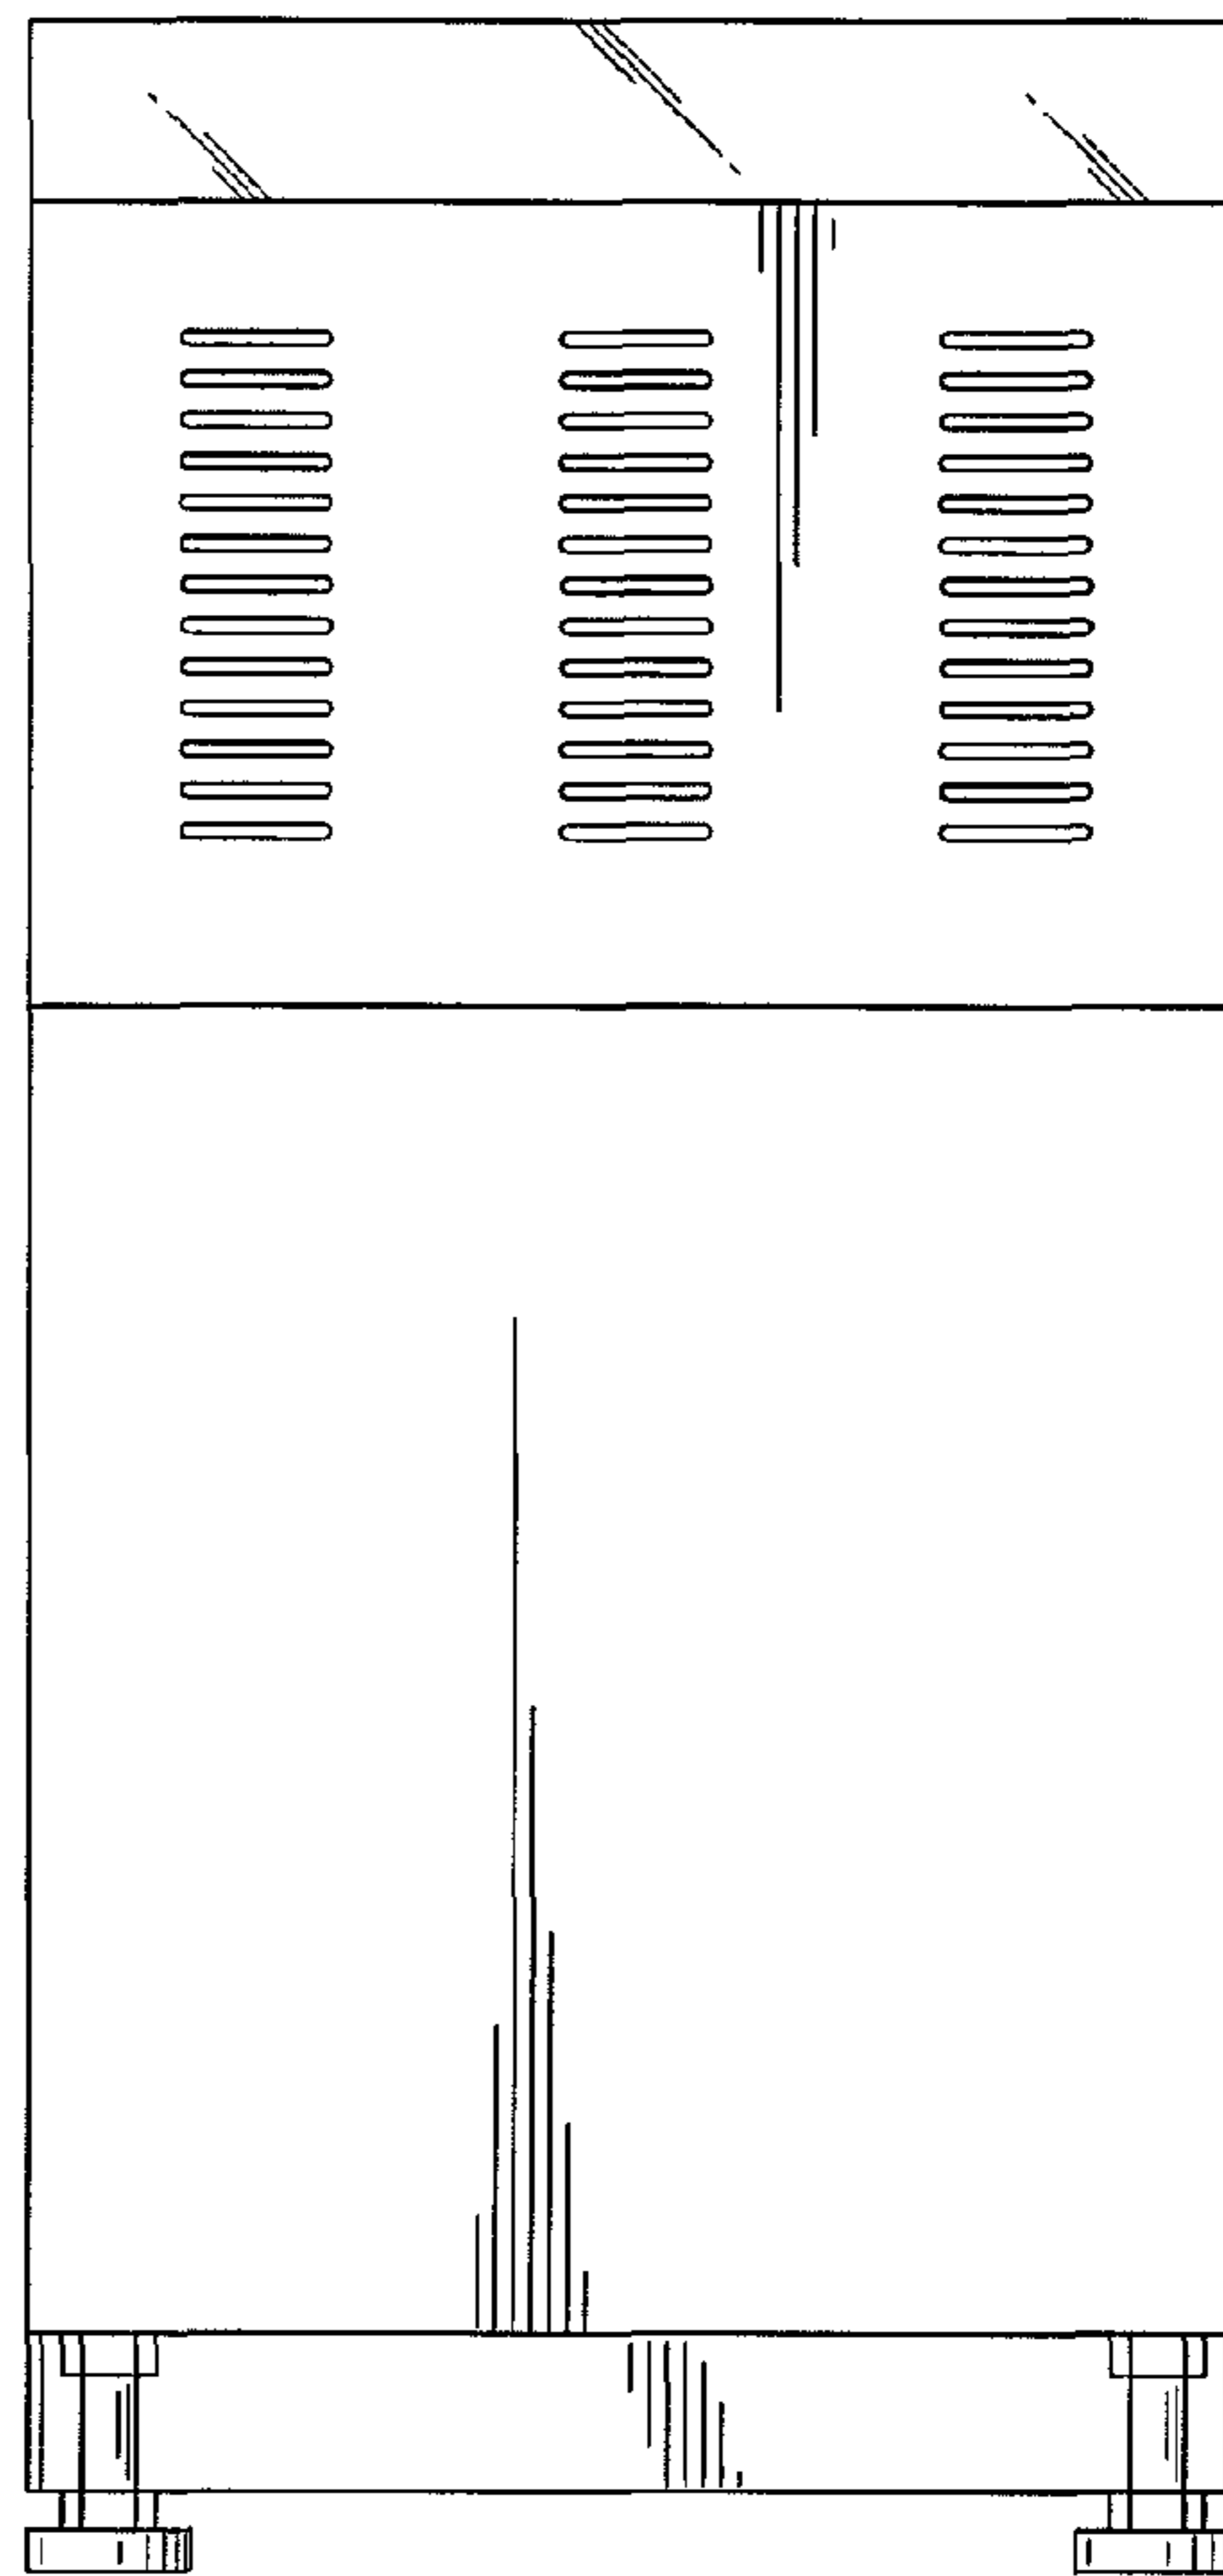


FIG. 3

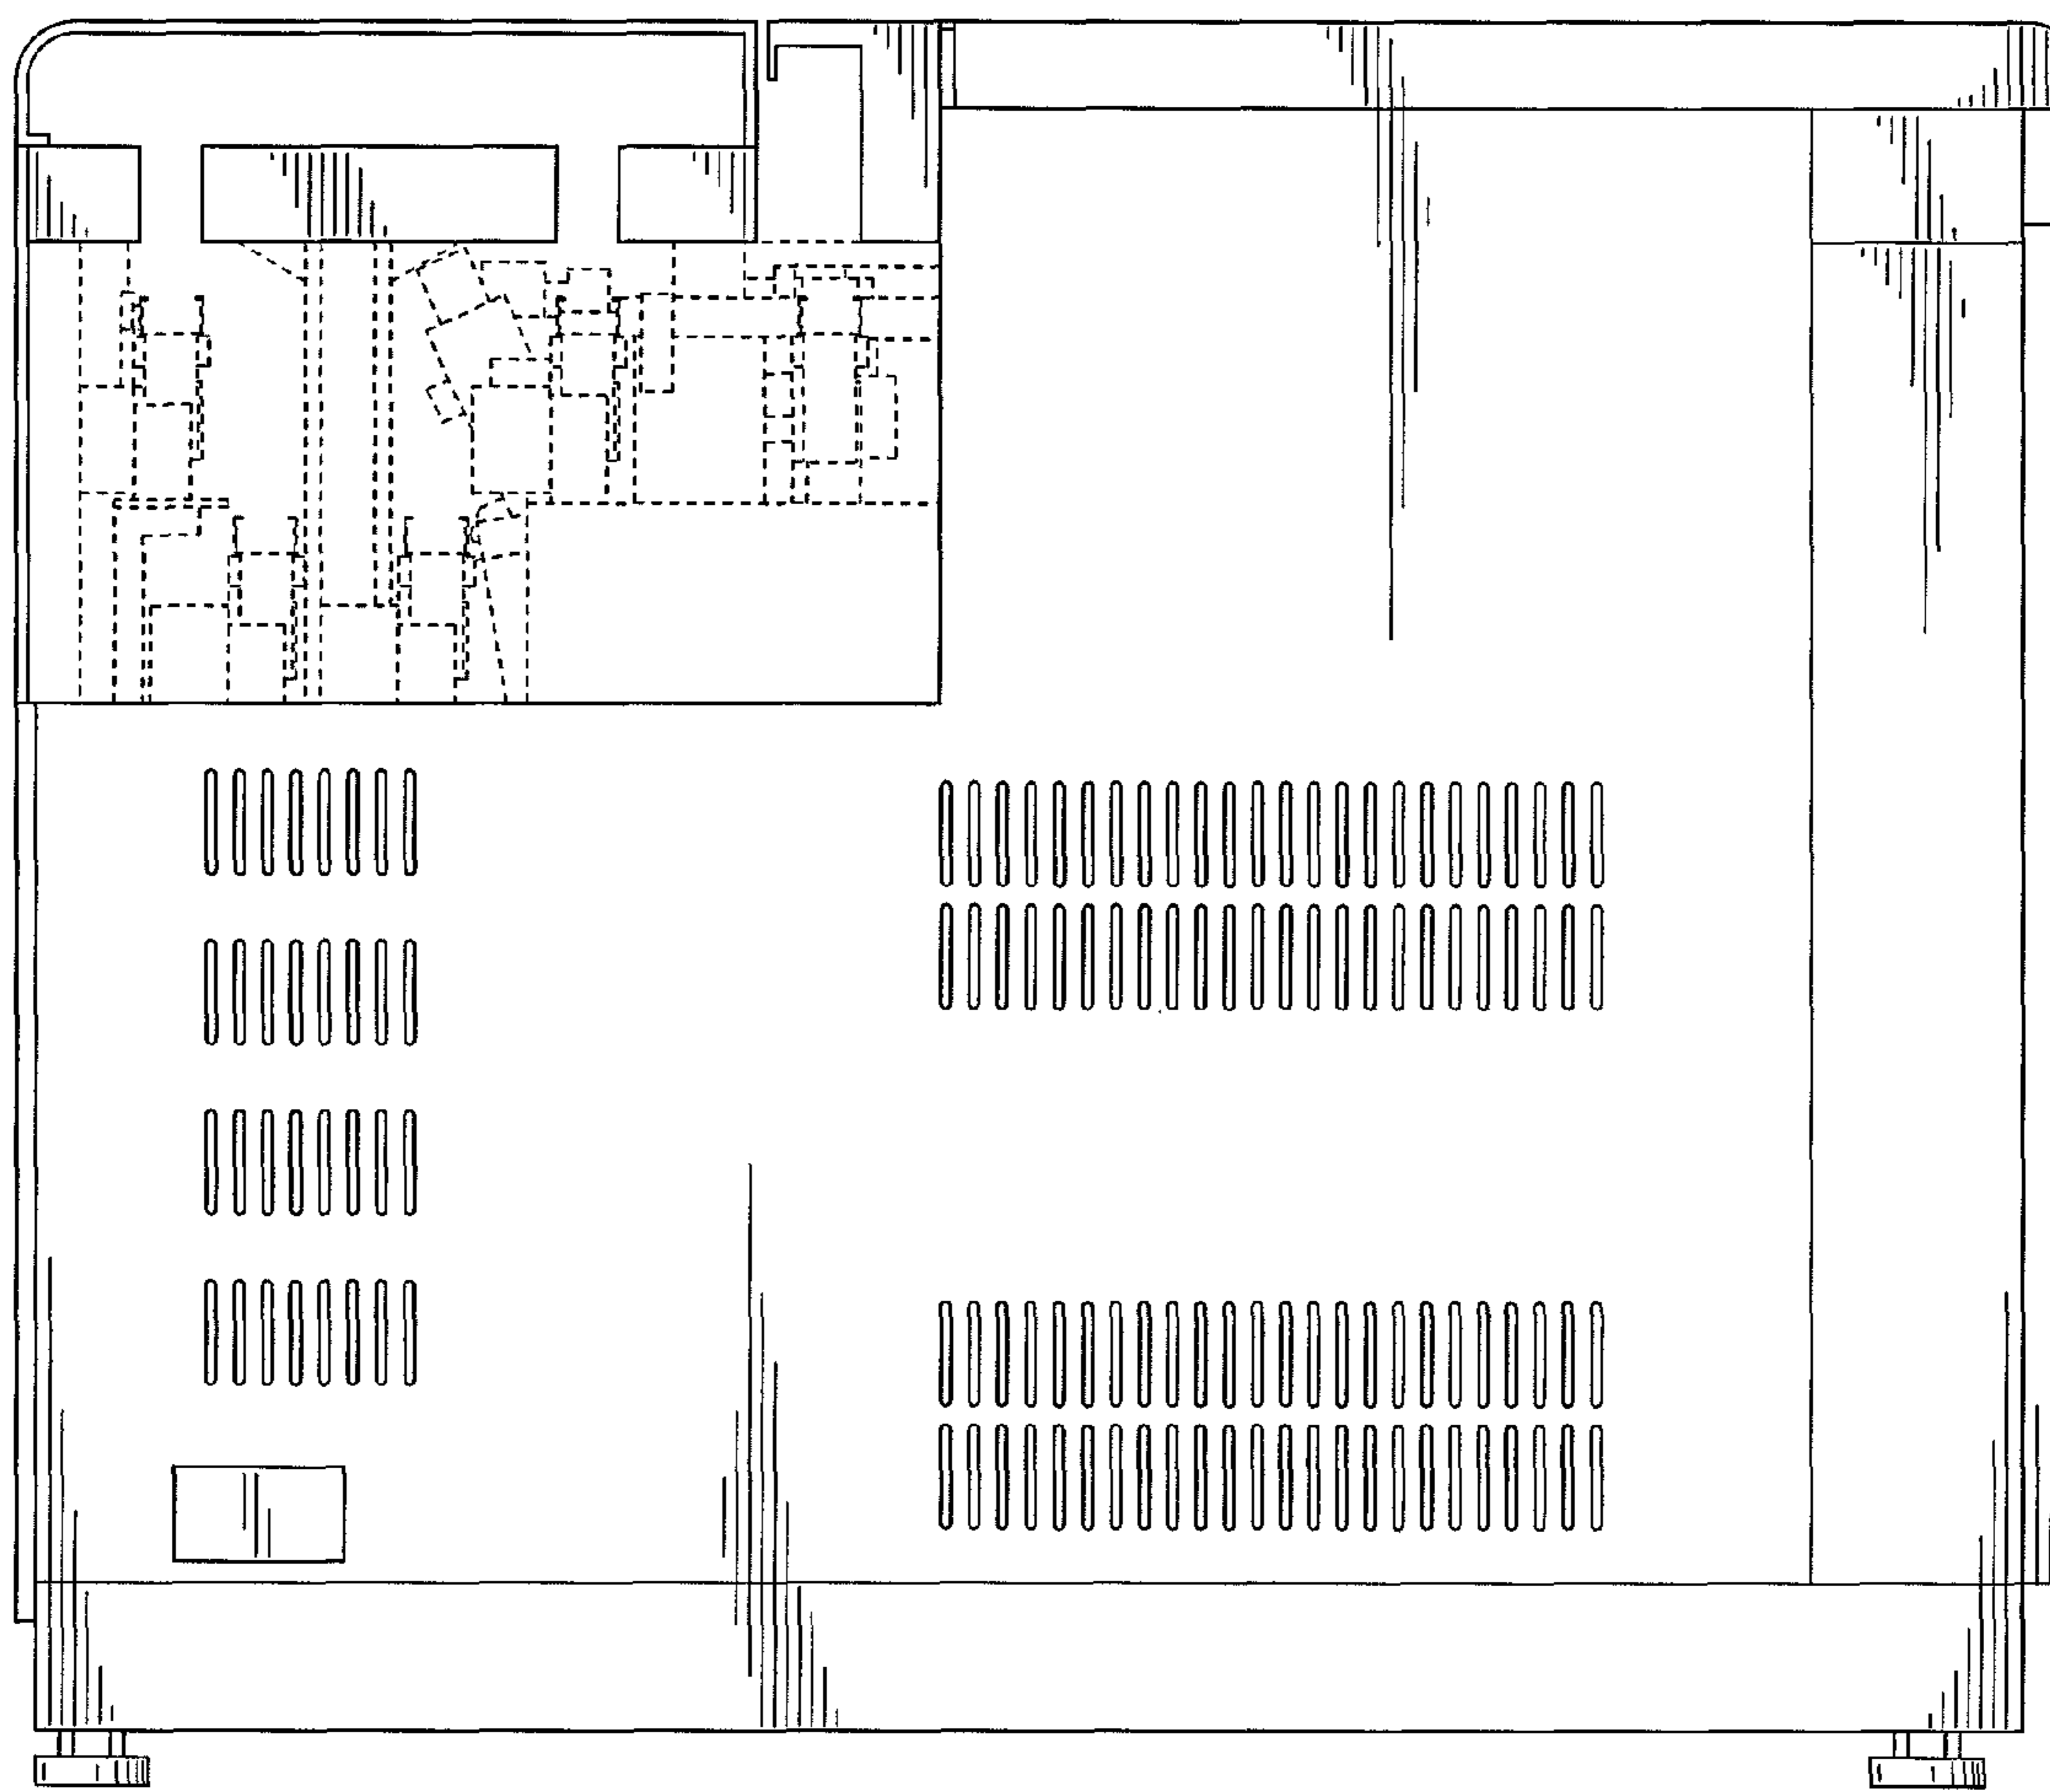


FIG. 4

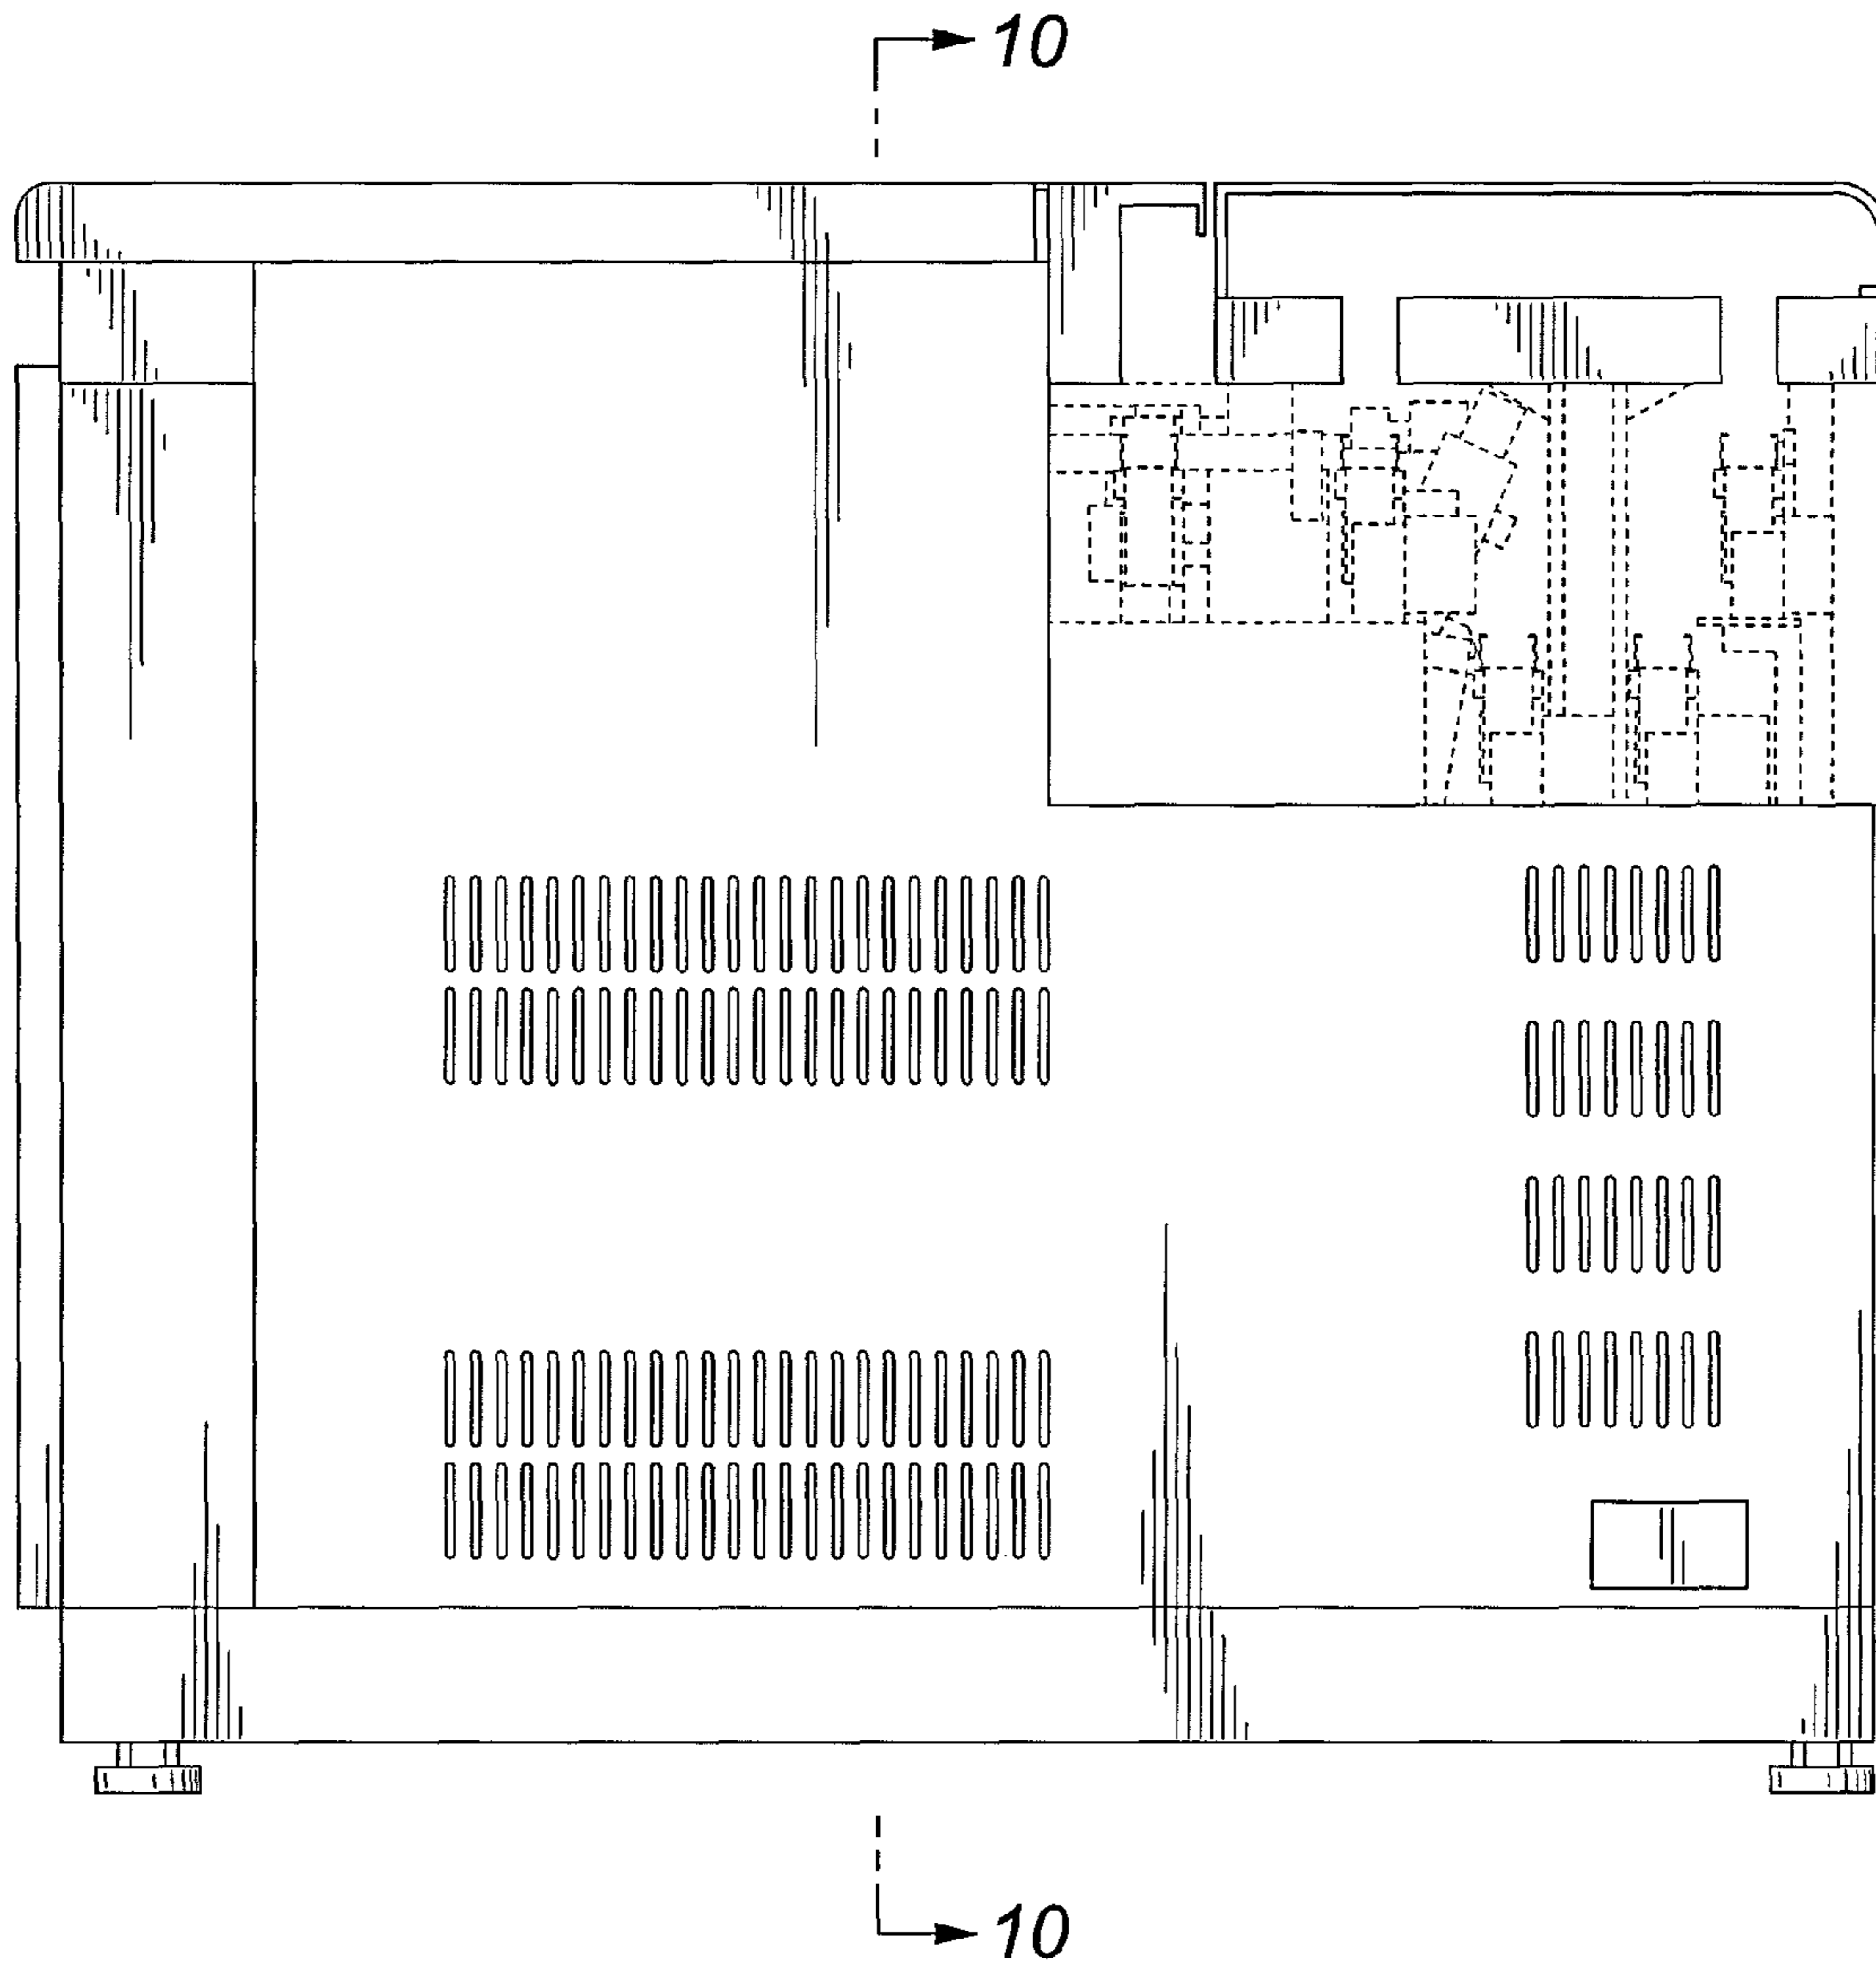


FIG. 5

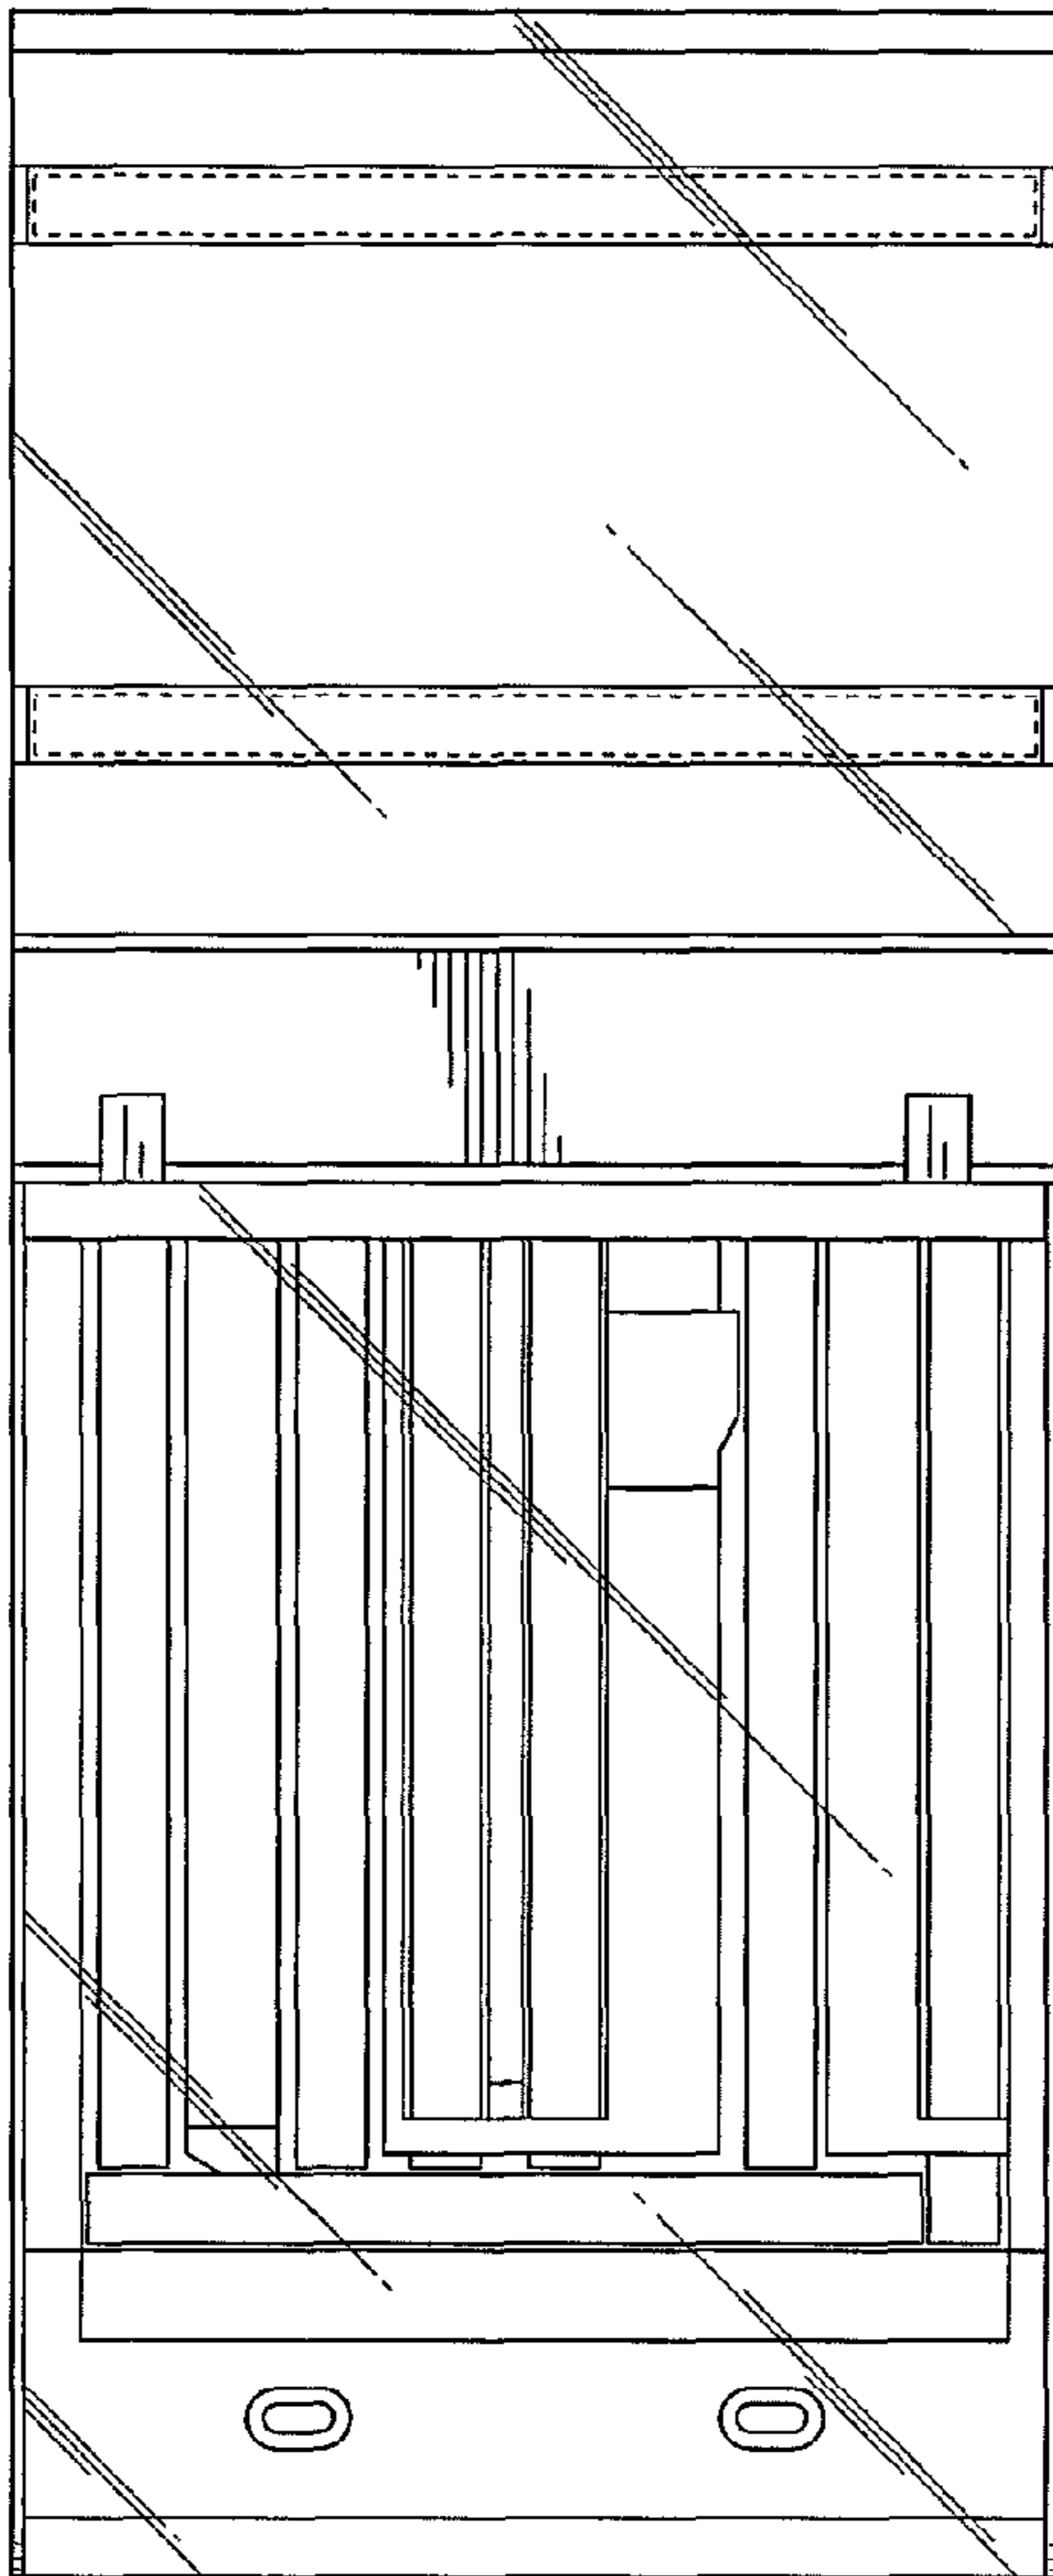


FIG. 6

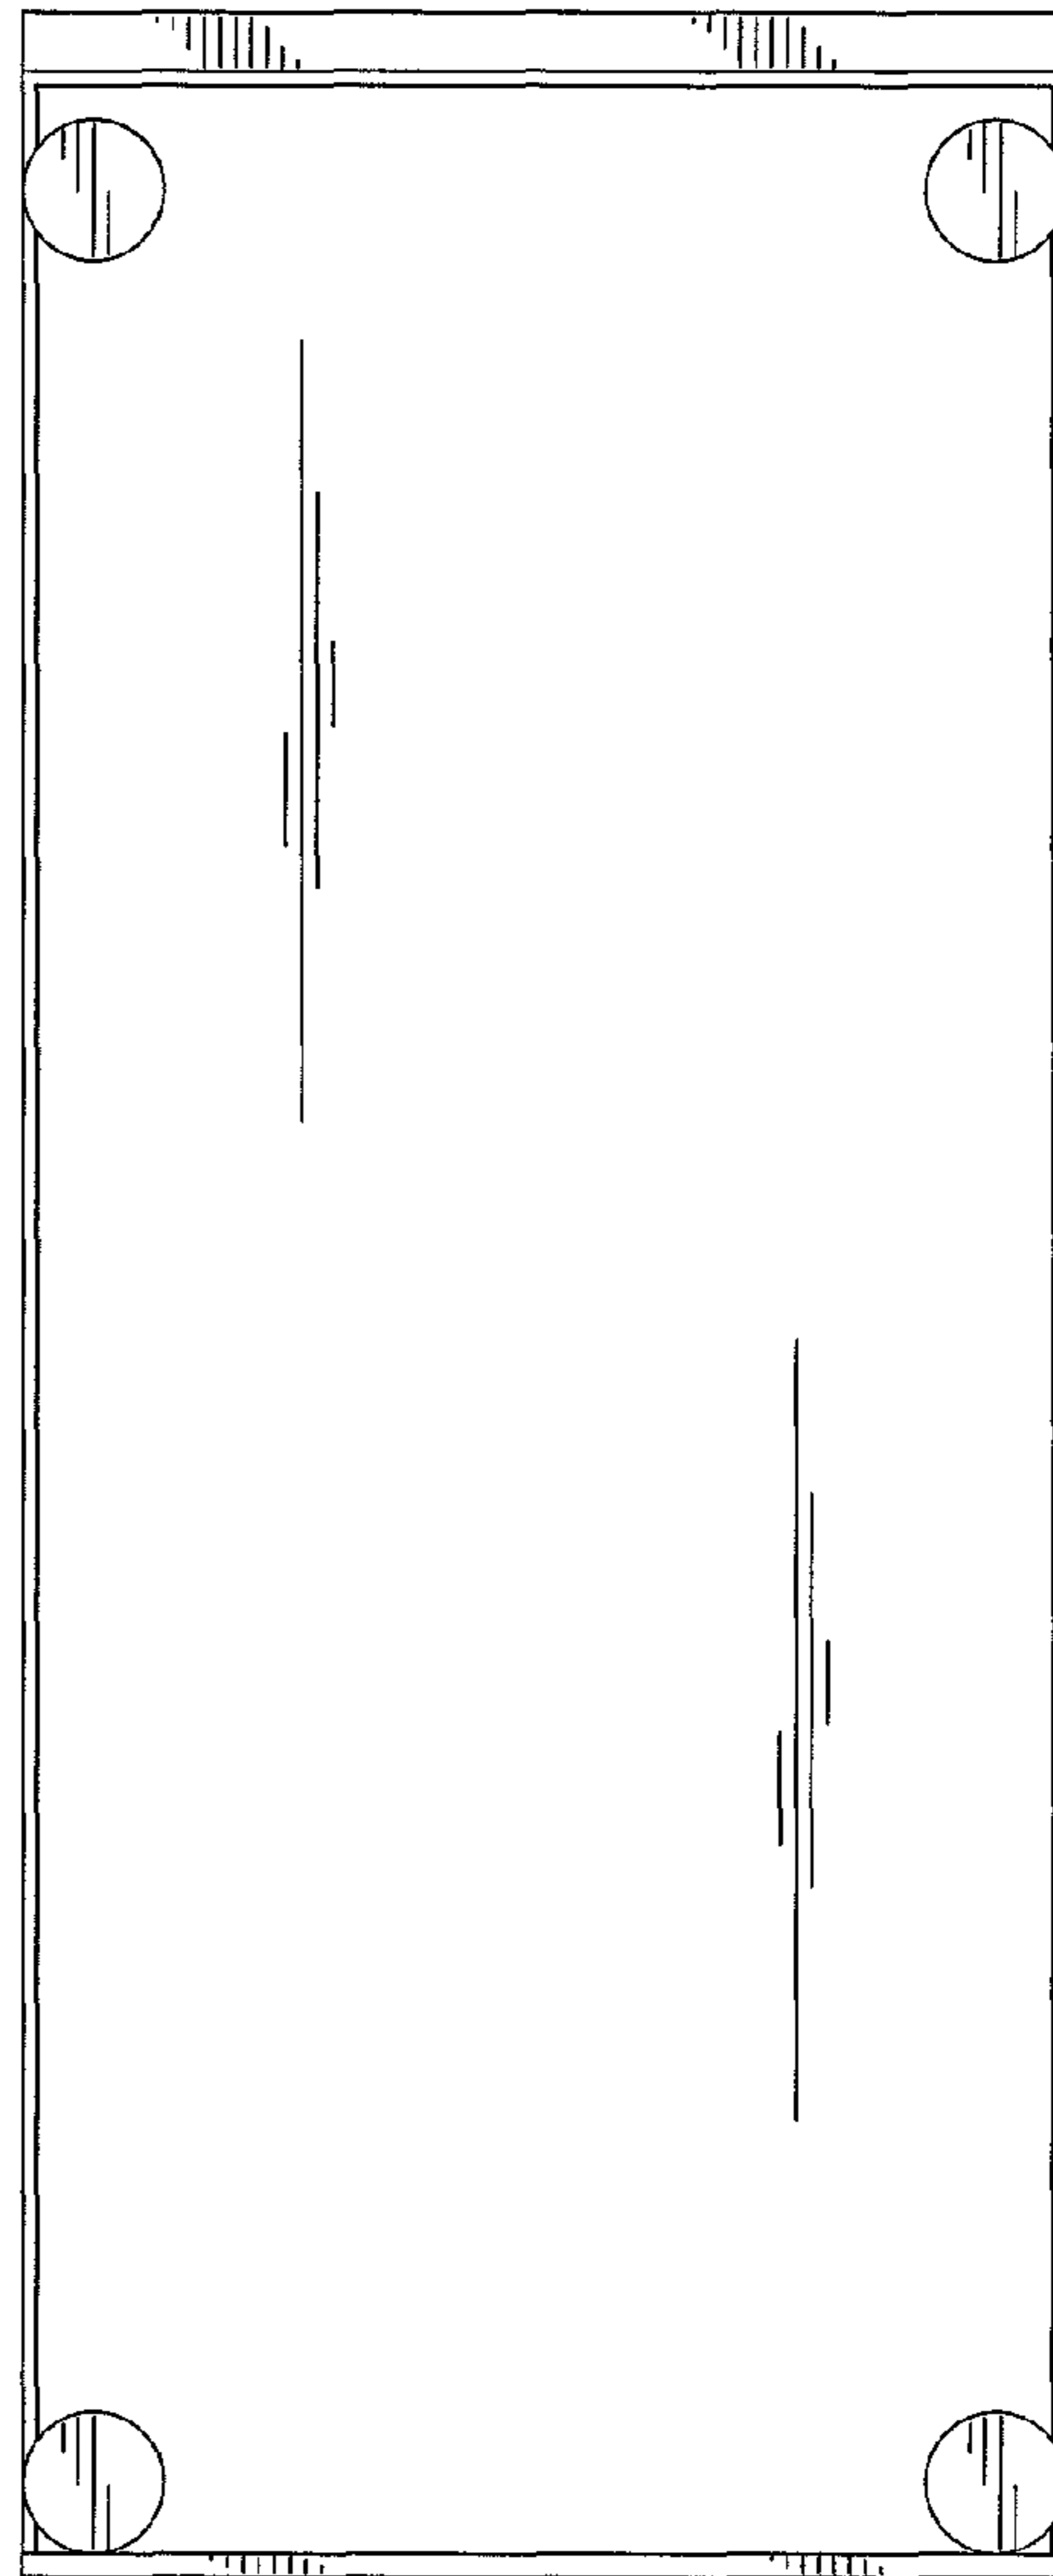


FIG. 7

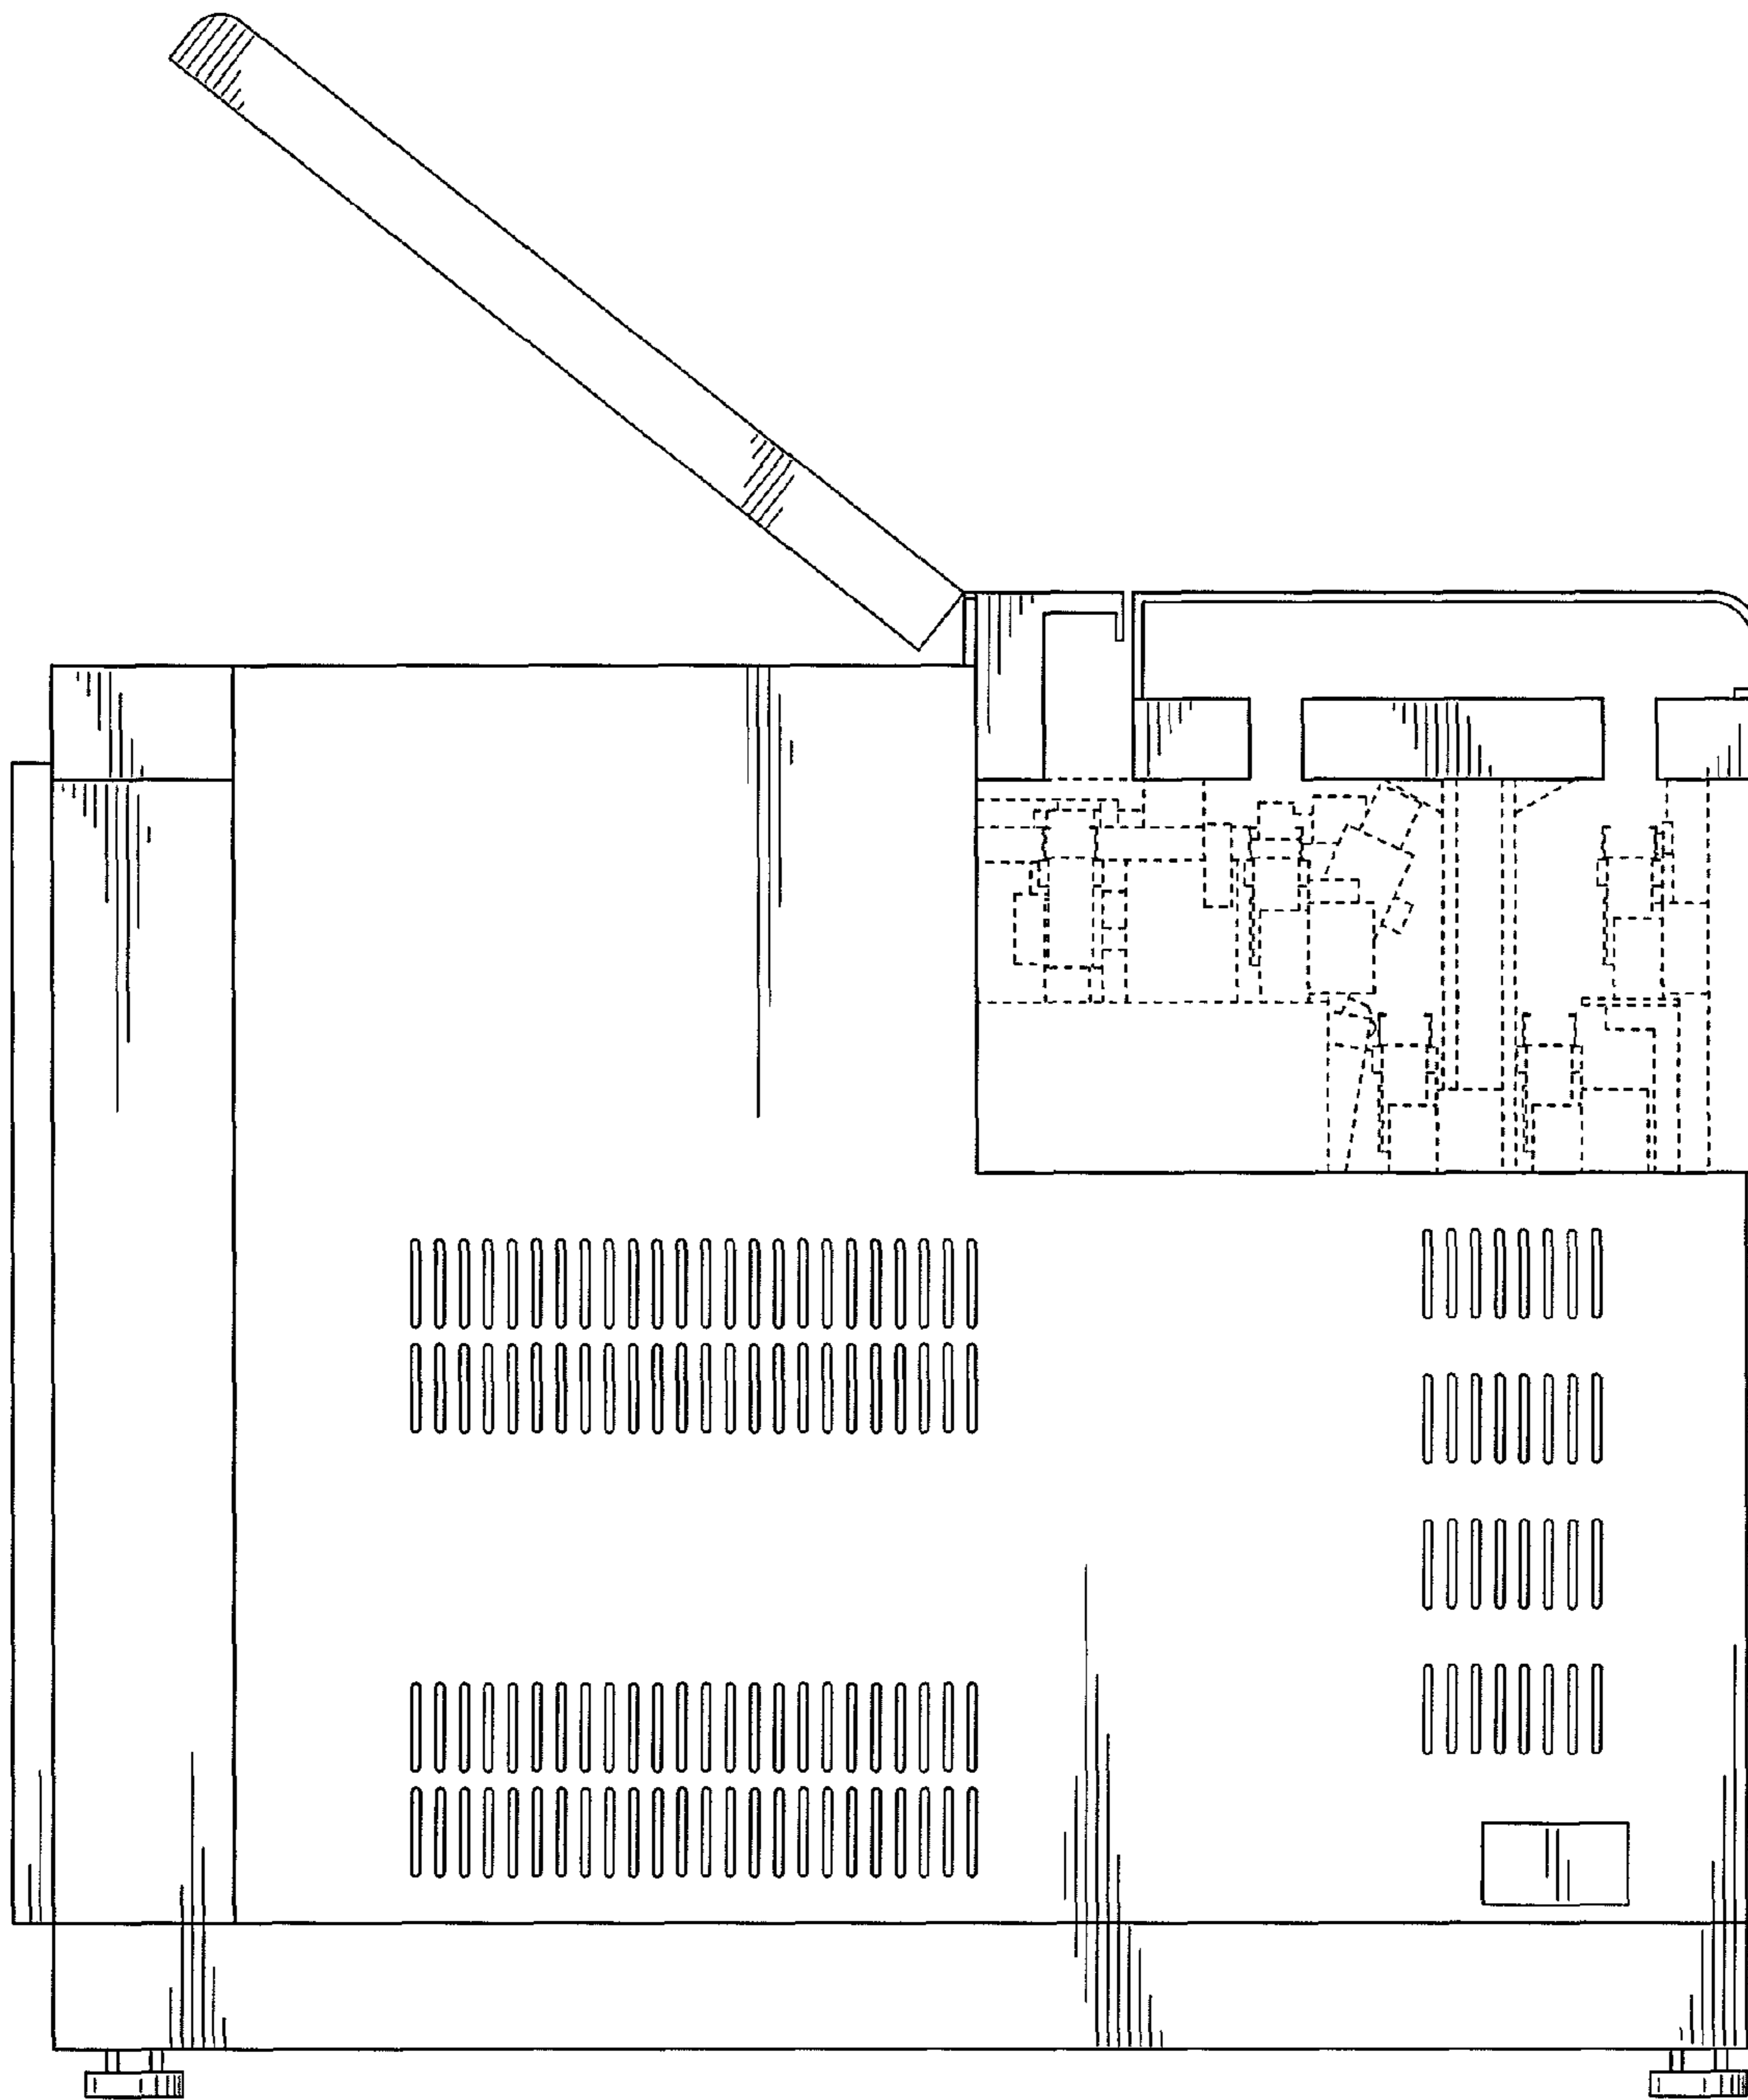


FIG. 8

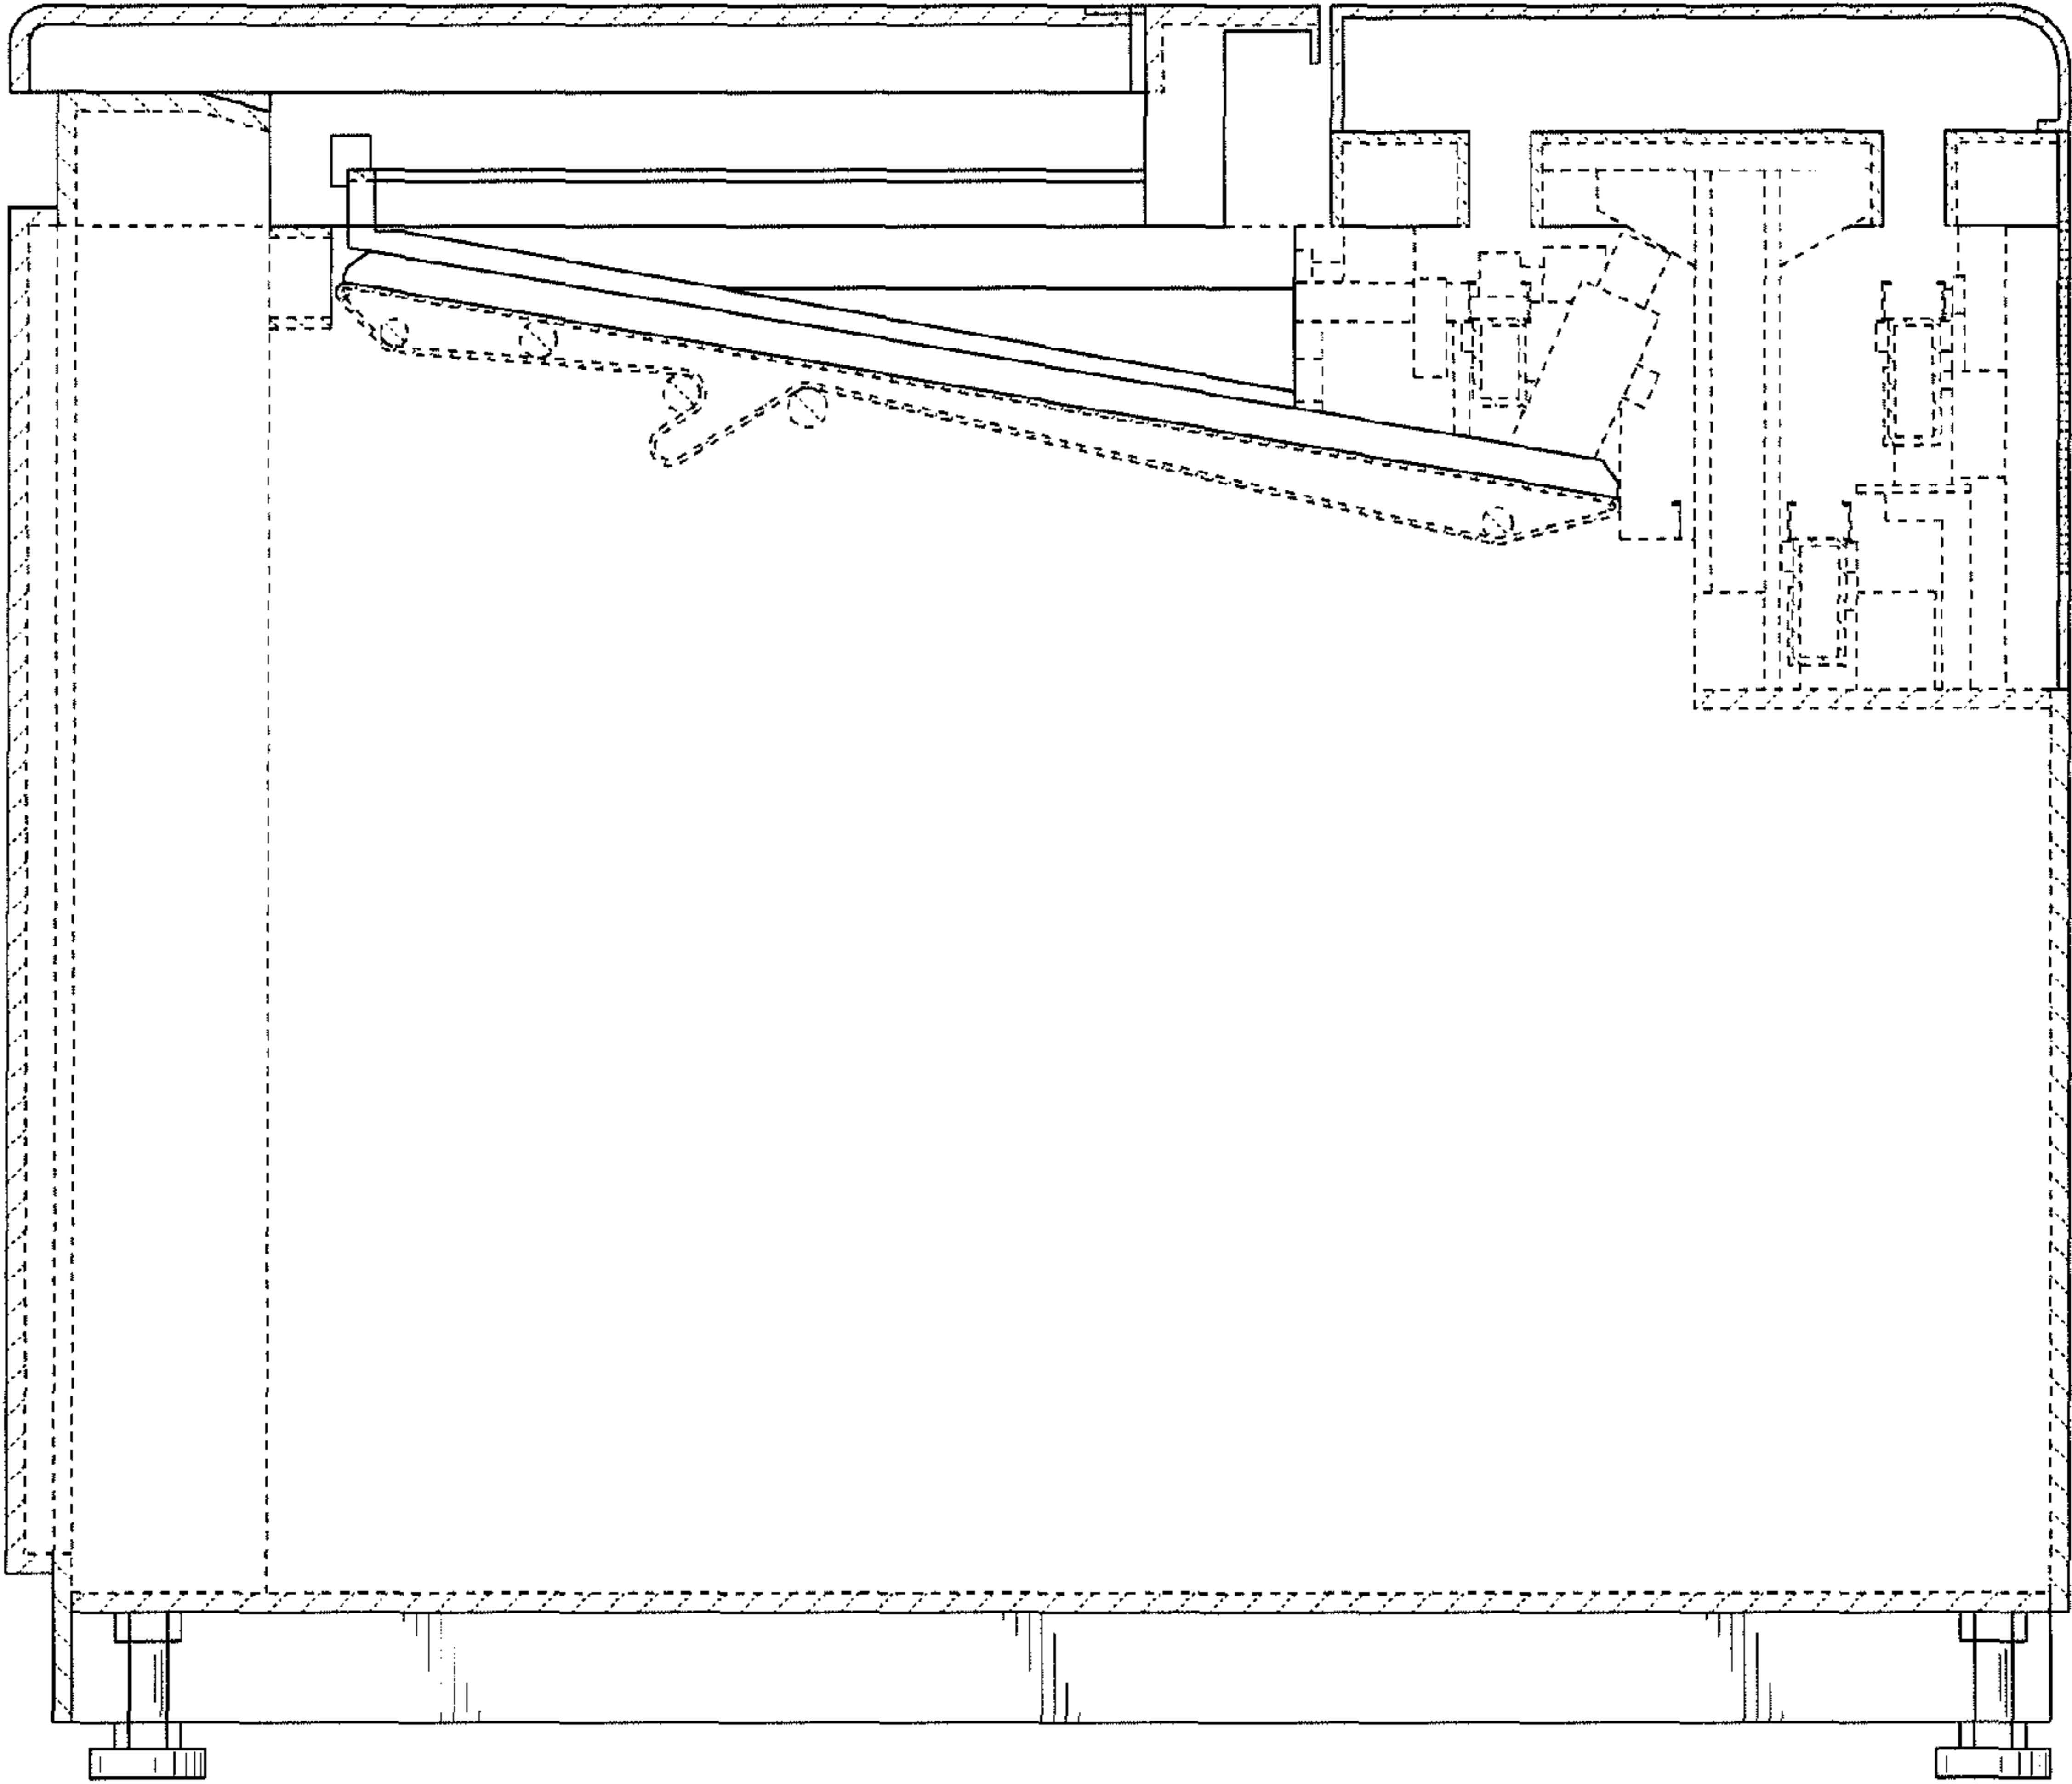


FIG. 9

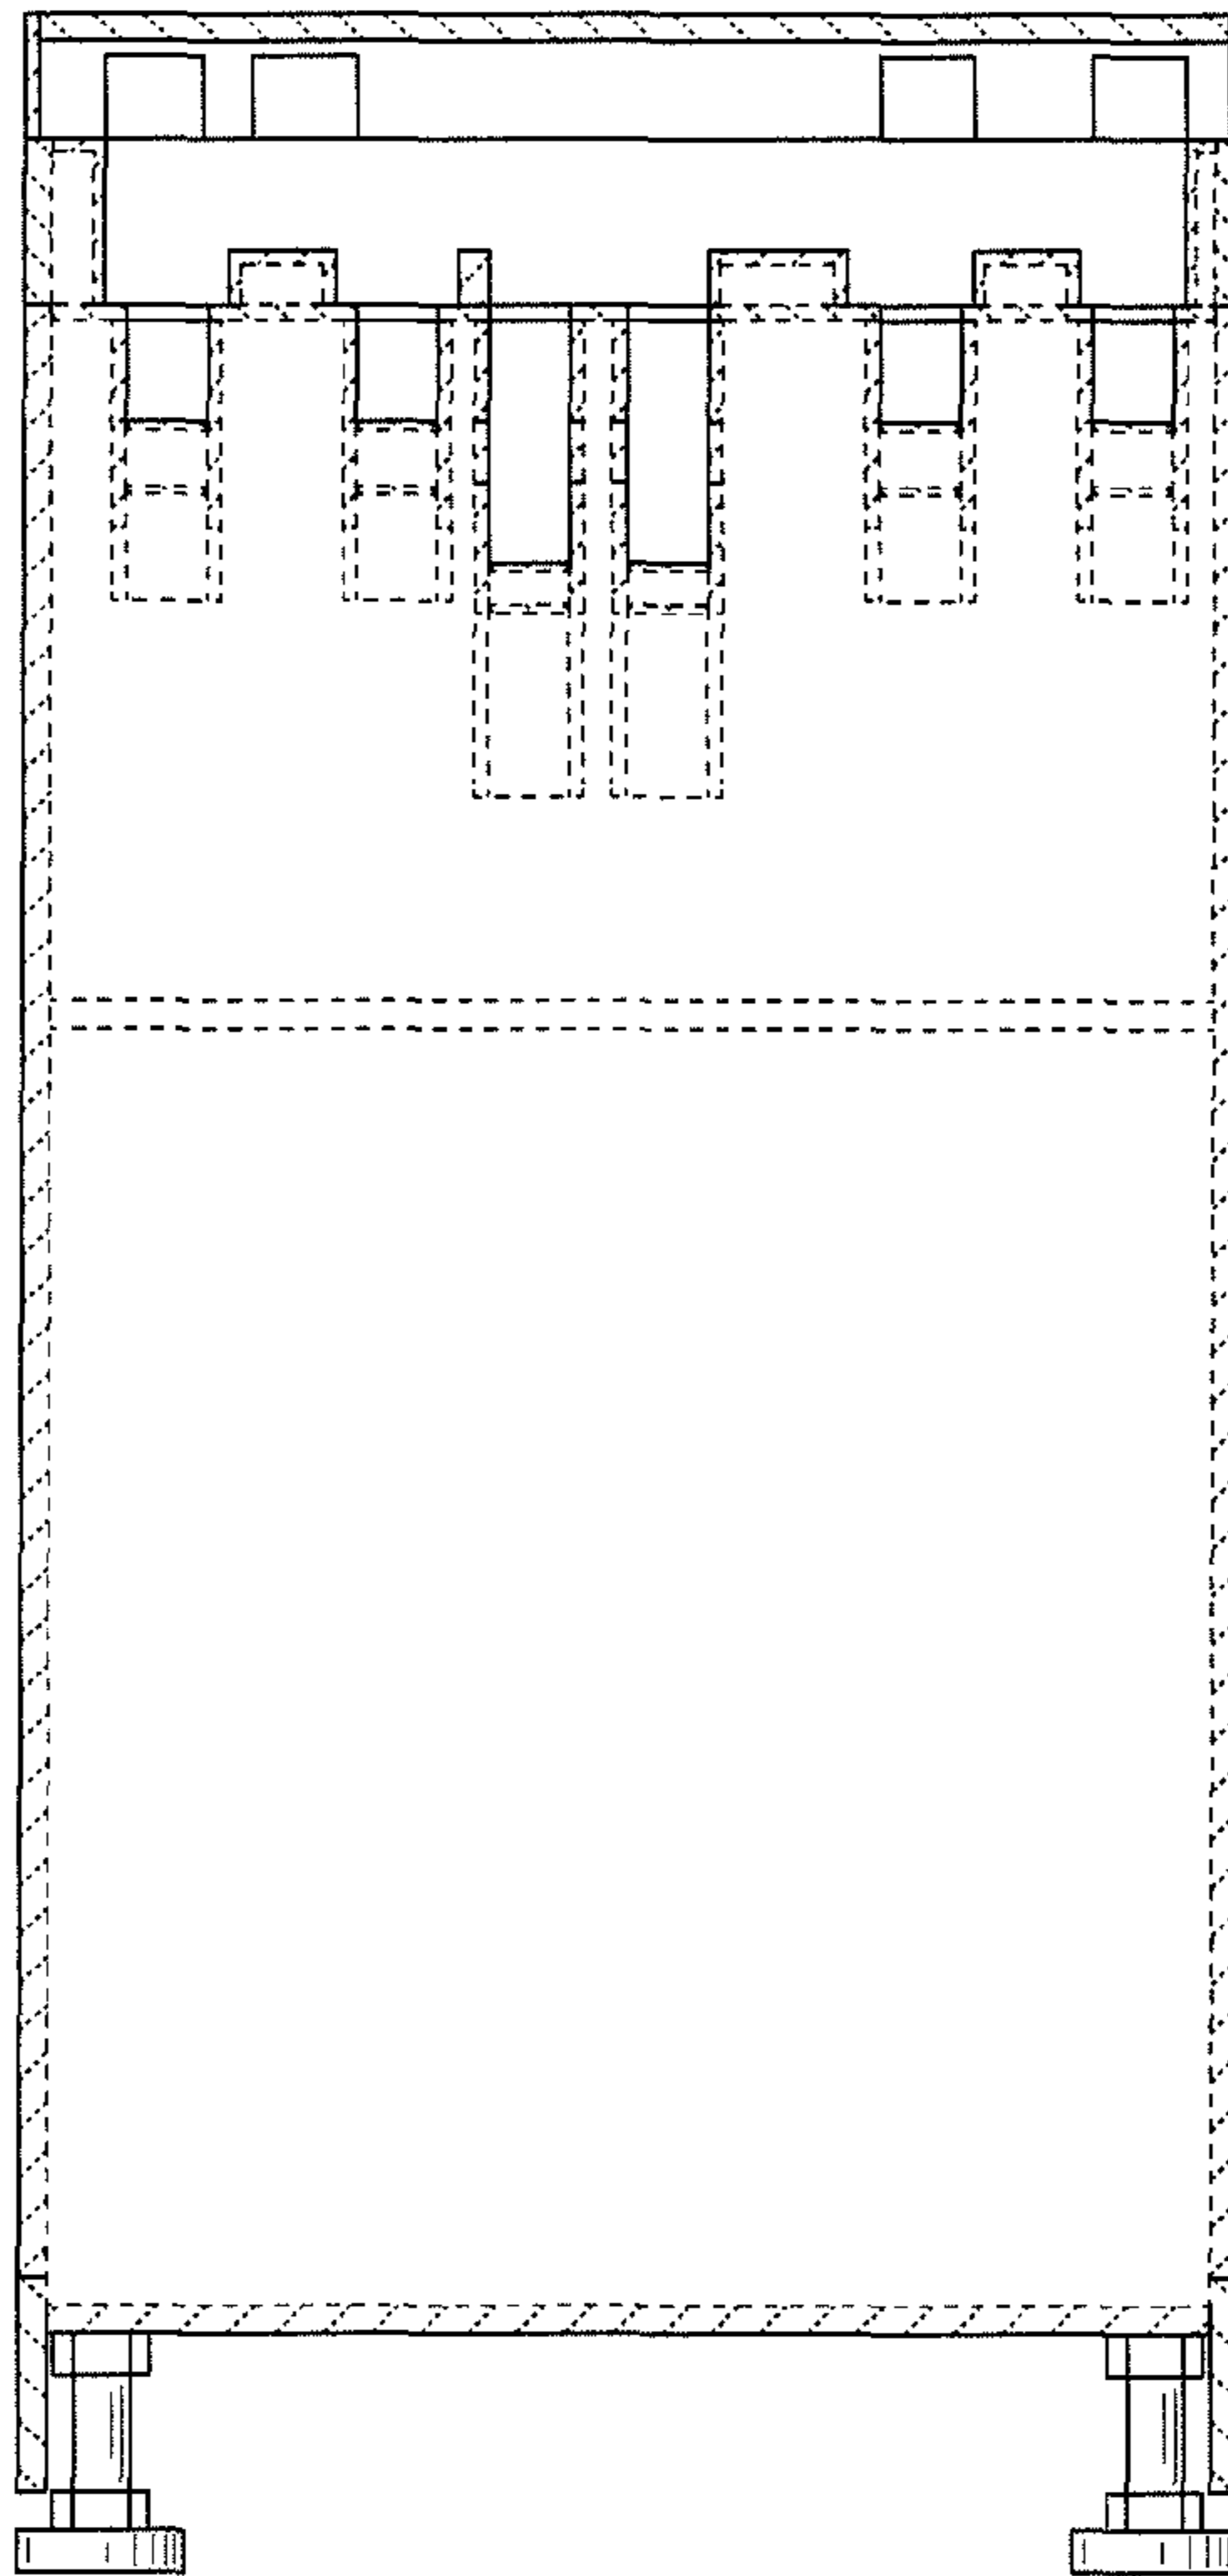


FIG. 10