



US00D688383S

(12) **United States Design Patent**  
**Manabe**

(10) **Patent No.:** **US D688,383 S**  
(45) **Date of Patent:** **\*\* Aug. 20, 2013**

(54) **STIMULATION DEVICE**

(71) Applicant: **Takashi Manabe**, Chiba (JP)

(72) Inventor: **Takashi Manabe**, Chiba (JP)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/436,871**

(22) Filed: **Nov. 9, 2012**

(51) **LOC (9) Cl.** ..... **28-03**

(52) **U.S. Cl.**  
USPC ..... **D24/215**

(58) **Field of Classification Search**  
USPC ..... D24/200, 211, 212, 213, 214, 215;  
601/114, 120, 121, 124, 125, 130, 131, 134,  
601/135, 136, 137

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,690,603	A *	11/1997	Kain	600/38
6,254,555	B1 *	7/2001	Sevier et al.	601/135
D495,424	S *	8/2004	Nan	D24/215
D530,823	S *	10/2006	Sevier et al.	D24/214
D536,097	S *	1/2007	Nan	D24/215
D592,758	S *	5/2009	Kain	D24/215
D596,307	S *	7/2009	Stewart	D24/214
D603,052	S *	10/2009	Bauer et al.	D24/215
D630,762	S *	1/2011	Elliott	D24/215
D630,764	S *	1/2011	Elliott	D24/215
D636,887	S *	4/2011	Nan	D24/215

\* cited by examiner

Primary Examiner — Sandra Snapp

(74) *Attorney, Agent, or Firm* — Ladas & Parry LLP

(57) **CLAIM**

I claim the ornamental design for a stimulation device, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of the stimulation device in accordance with a first embodiment of the present invention. FIG. 2 is a front end elevational view of the stimulation device of FIG. 1.

FIG. 3 is a rear end elevational view of the stimulation device of FIG. 1.

FIG. 4 is an elevational view from one side of the stimulation device of FIG. 1.

FIG. 5 is an elevational view from the other side of the stimulation device of FIG. 1.

FIG. 6 is a top plan view of the stimulation device of FIG. 1.

FIG. 7 is a bottom plan view of the stimulation device of FIG. 1.

FIG. 8 is a perspective view of the stimulation device in accordance with a second embodiment of the present invention.

FIG. 9 is a front end elevational view of the stimulation device of FIG. 8.

FIG. 10 is a rear end elevational view of the stimulation device of FIG. 8.


FIG. 11 is an elevational view from one side of the stimulation device of FIG. 8.

FIG. 12 is an elevational view from the other side of the stimulation device of FIG. 8.

FIG. 13 is a top plan view of the stimulation device of FIG. 8; and,


FIG. 14 is a bottom plan view of the stimulation device of FIG. 8.

**1 Claim, 14 Drawing Sheets**

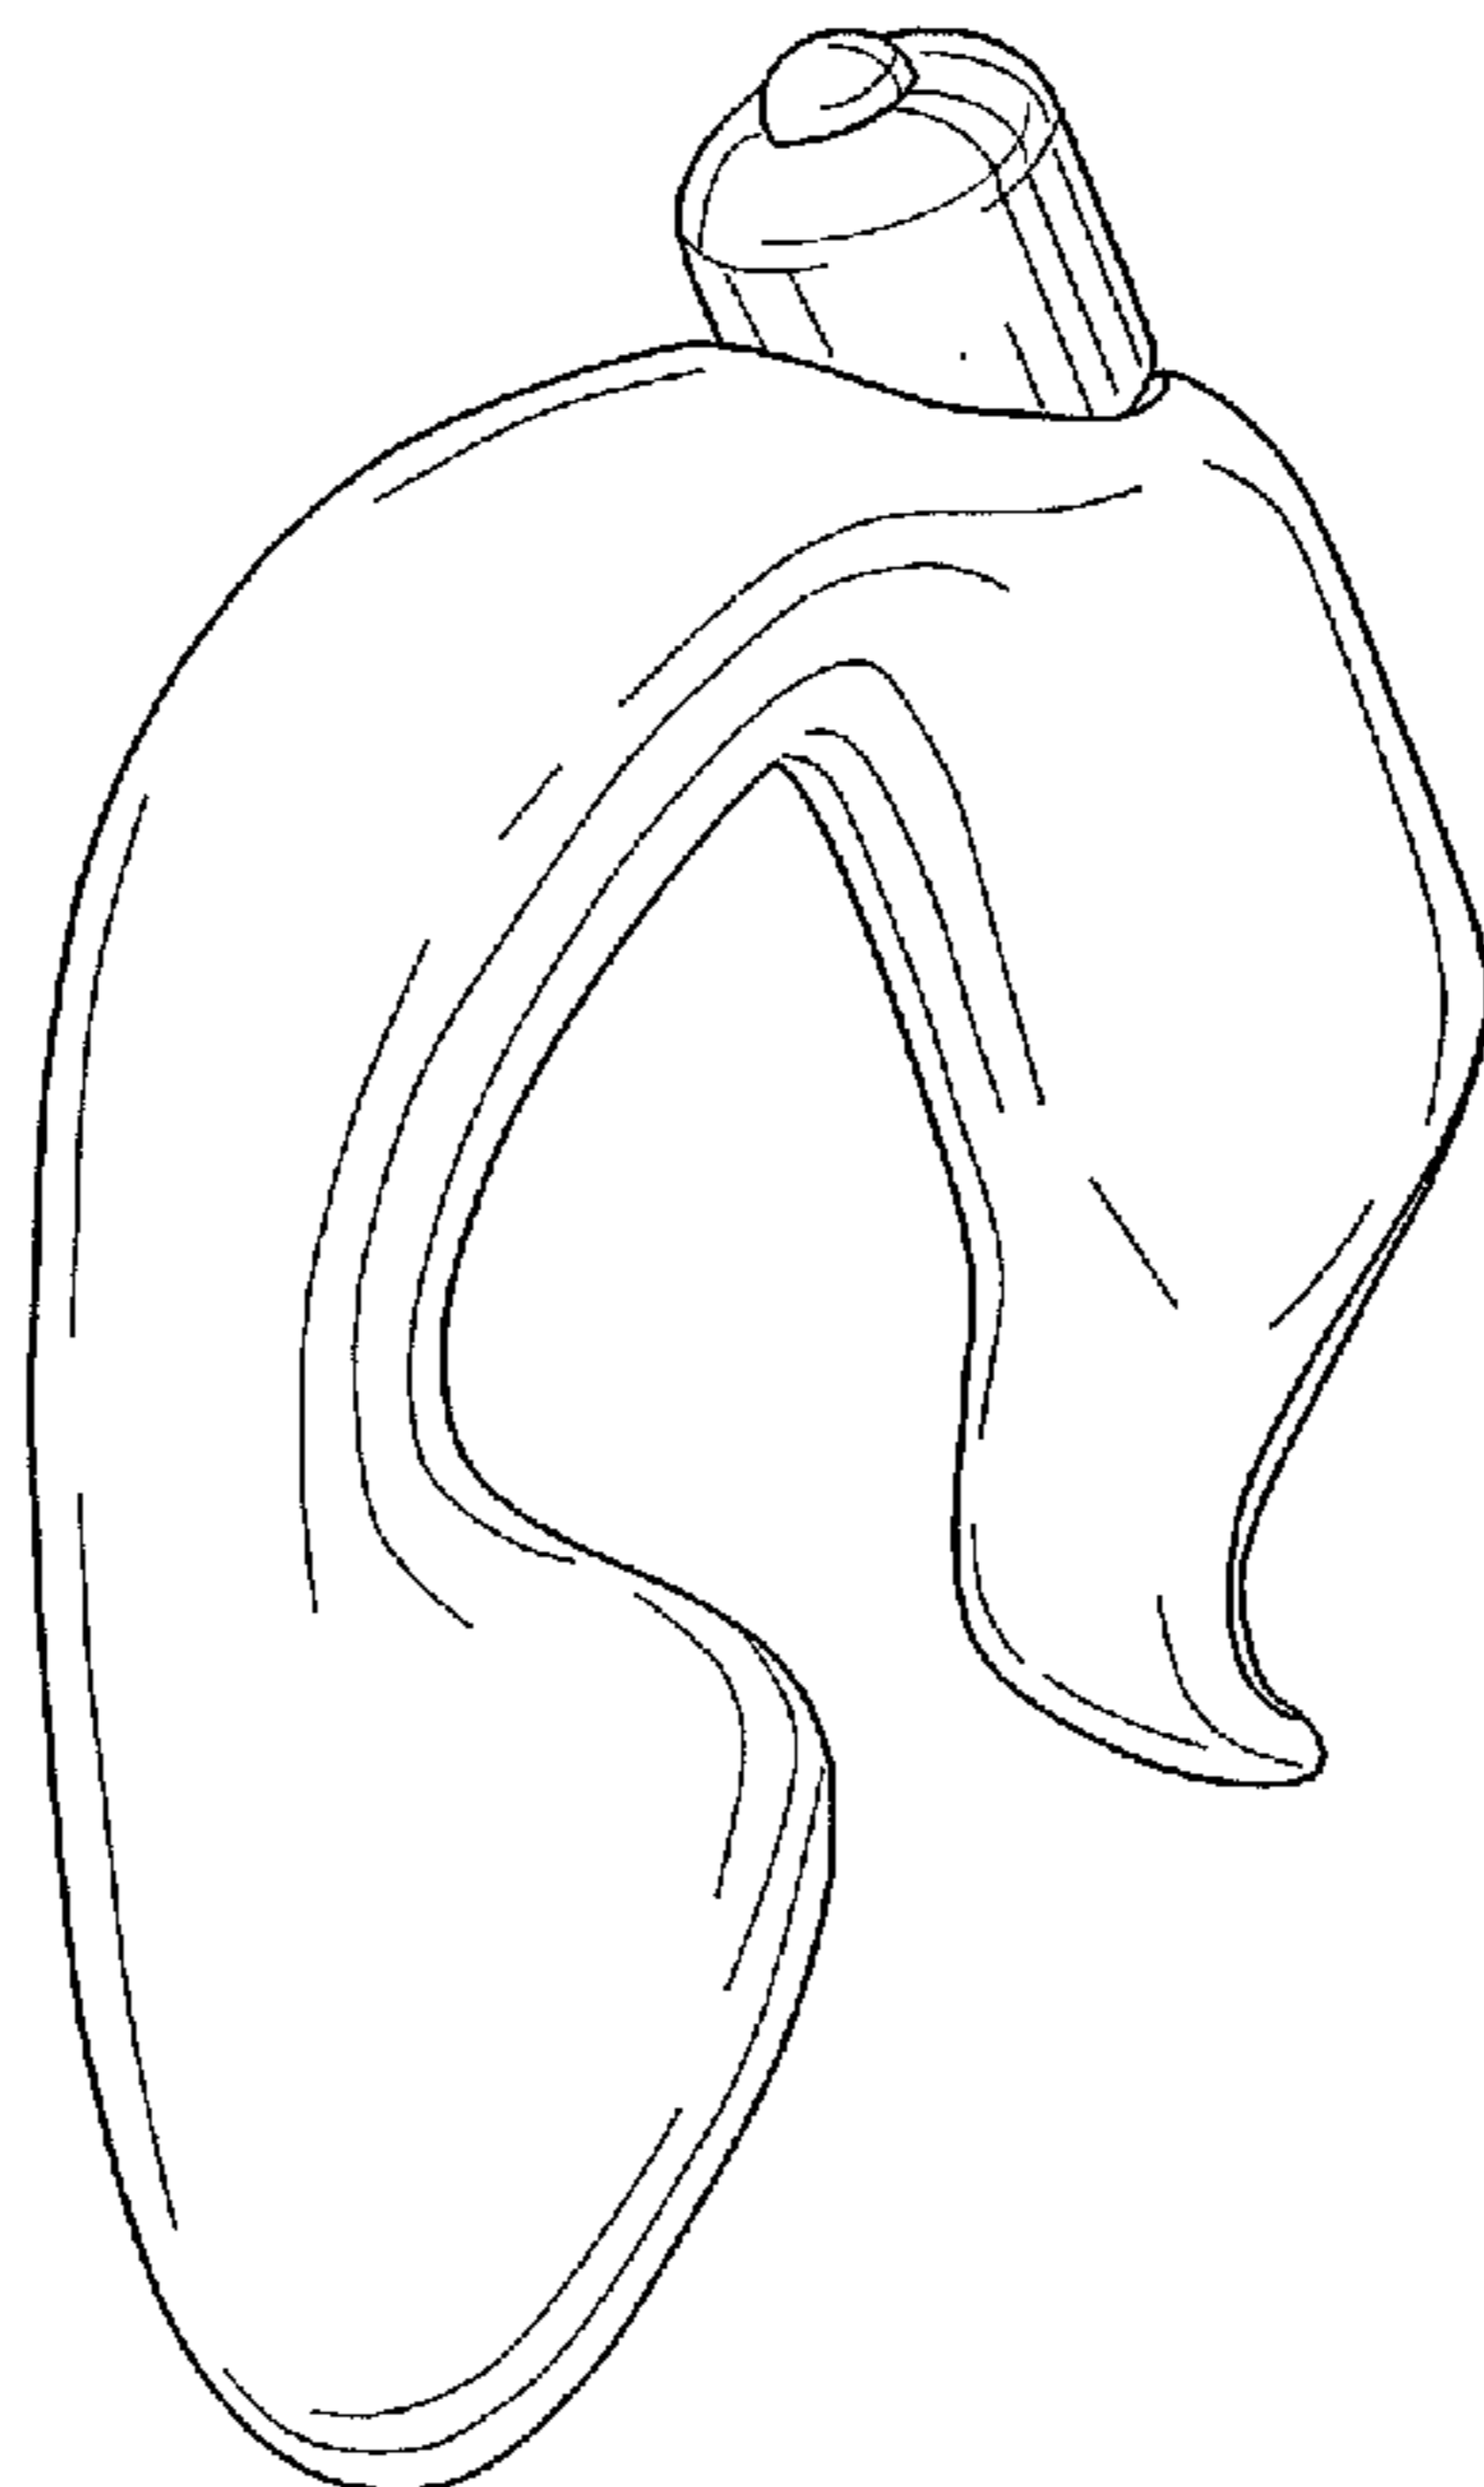





**FIG. 1**

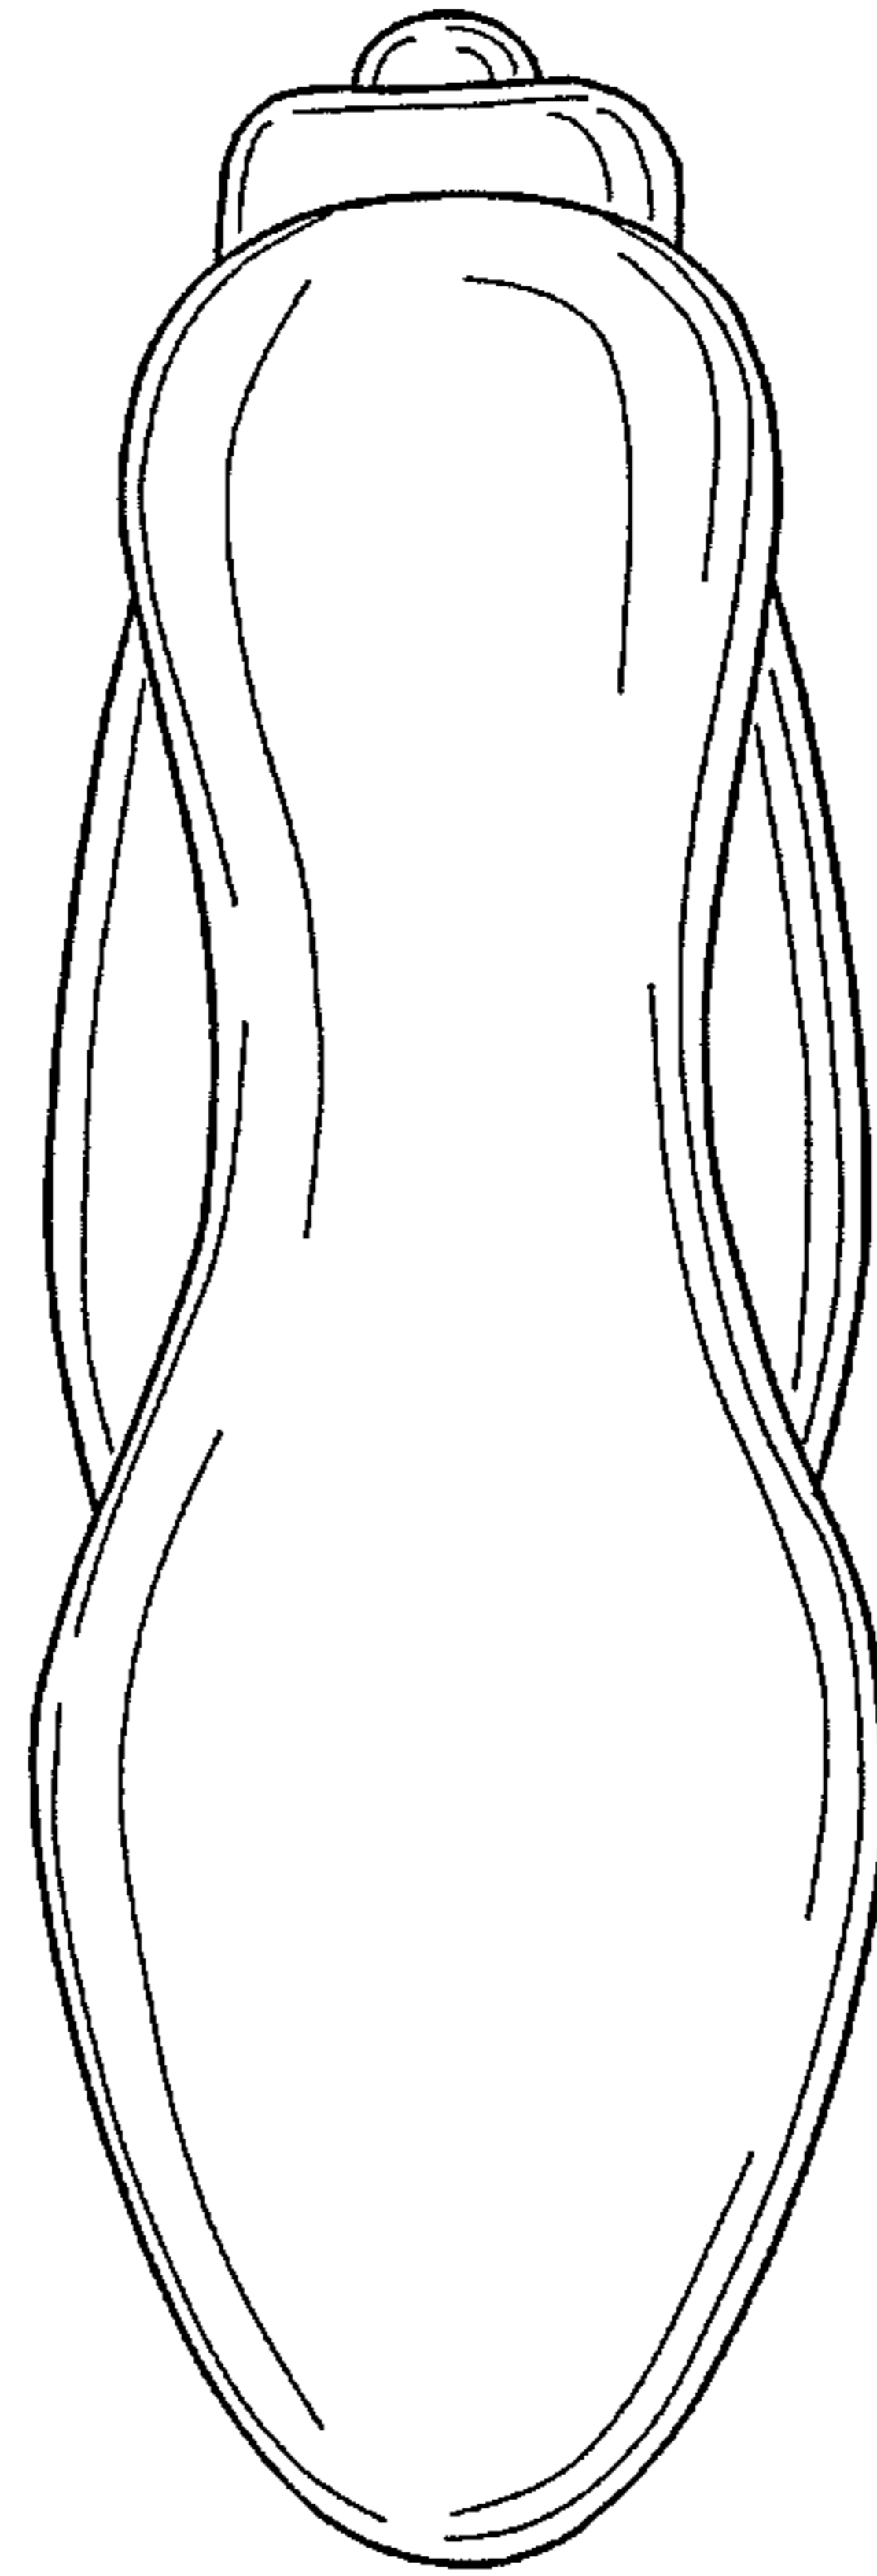

**FIG. 2**

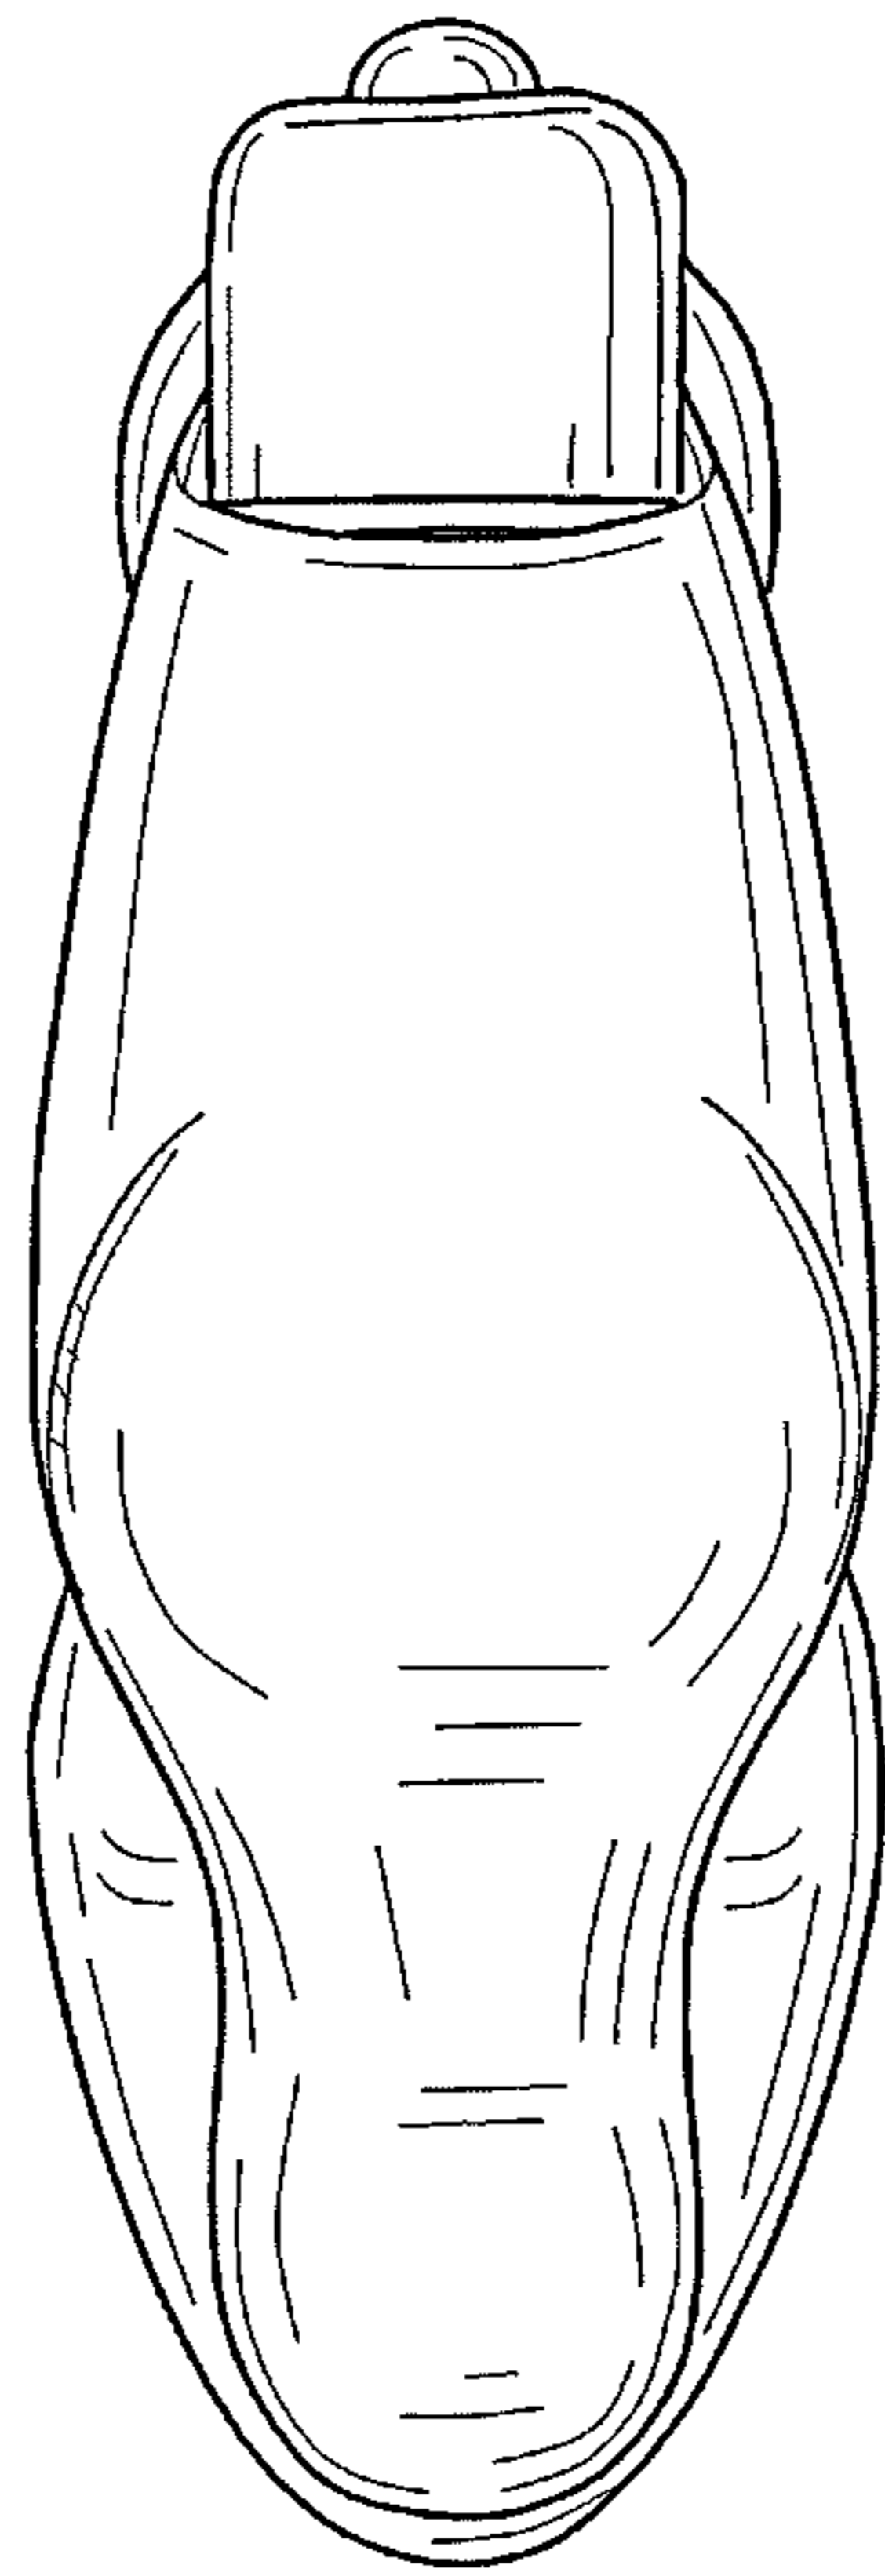

**FIG. 3**

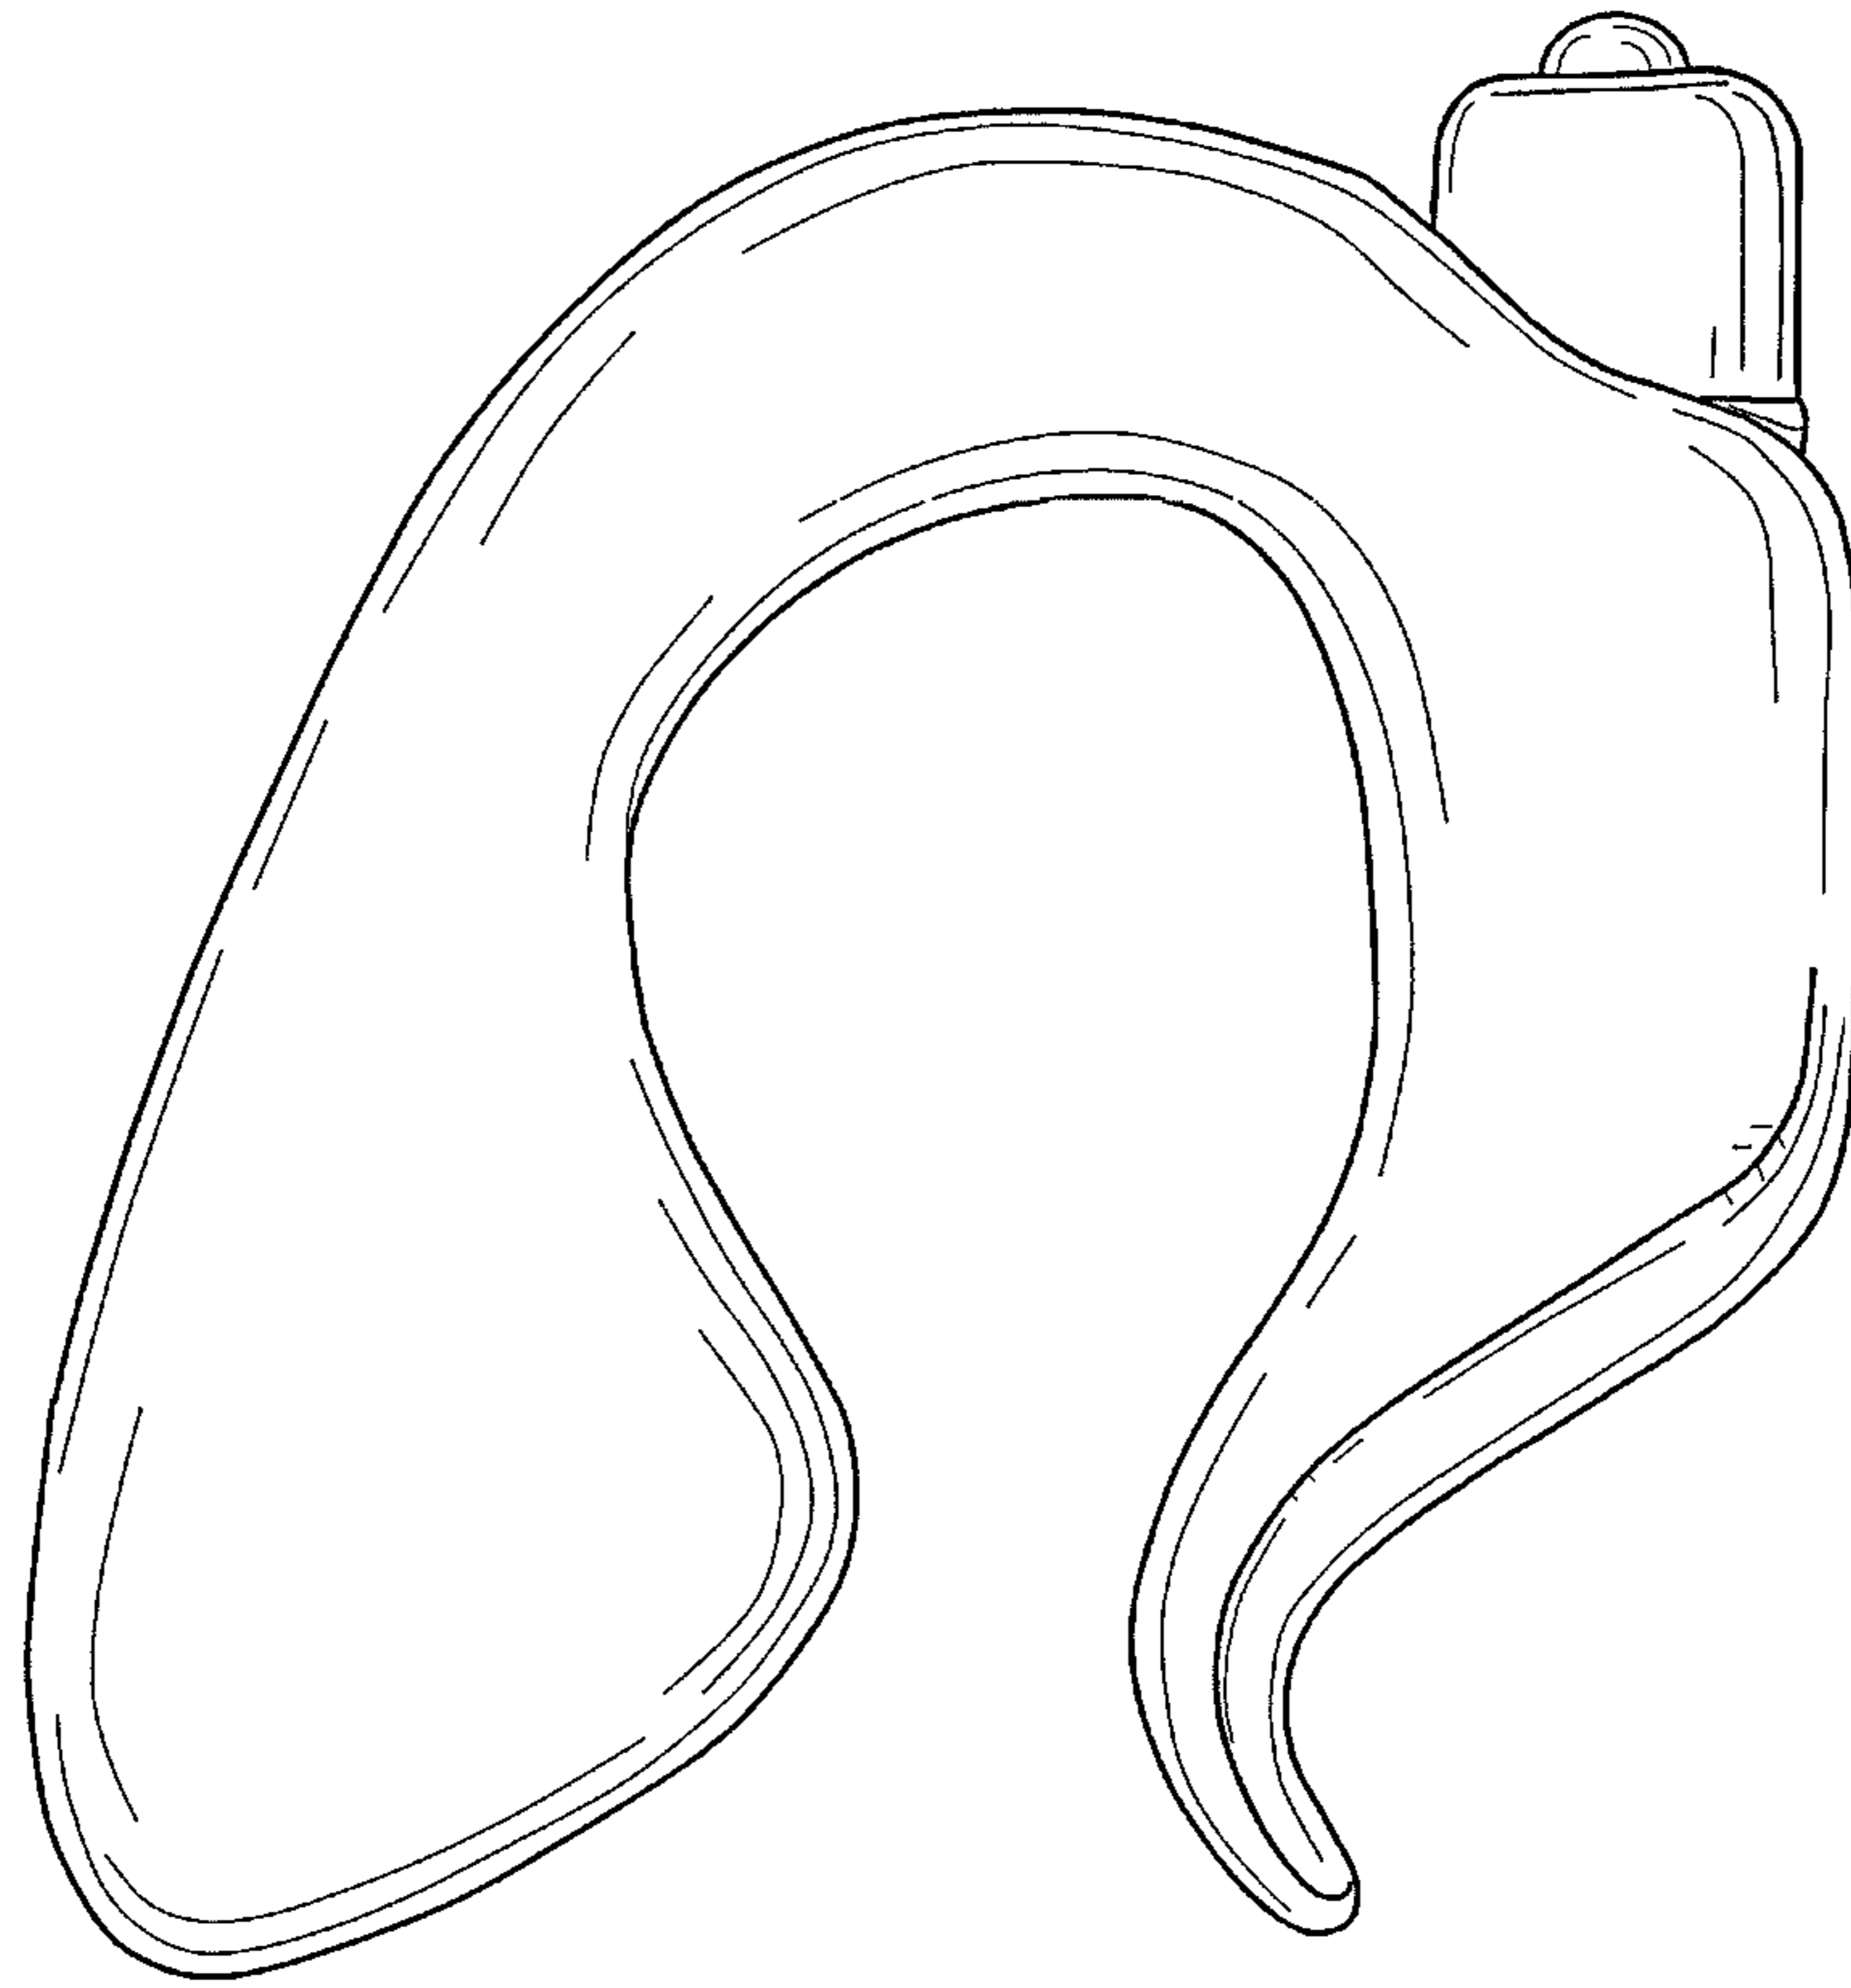

**FIG. 4**



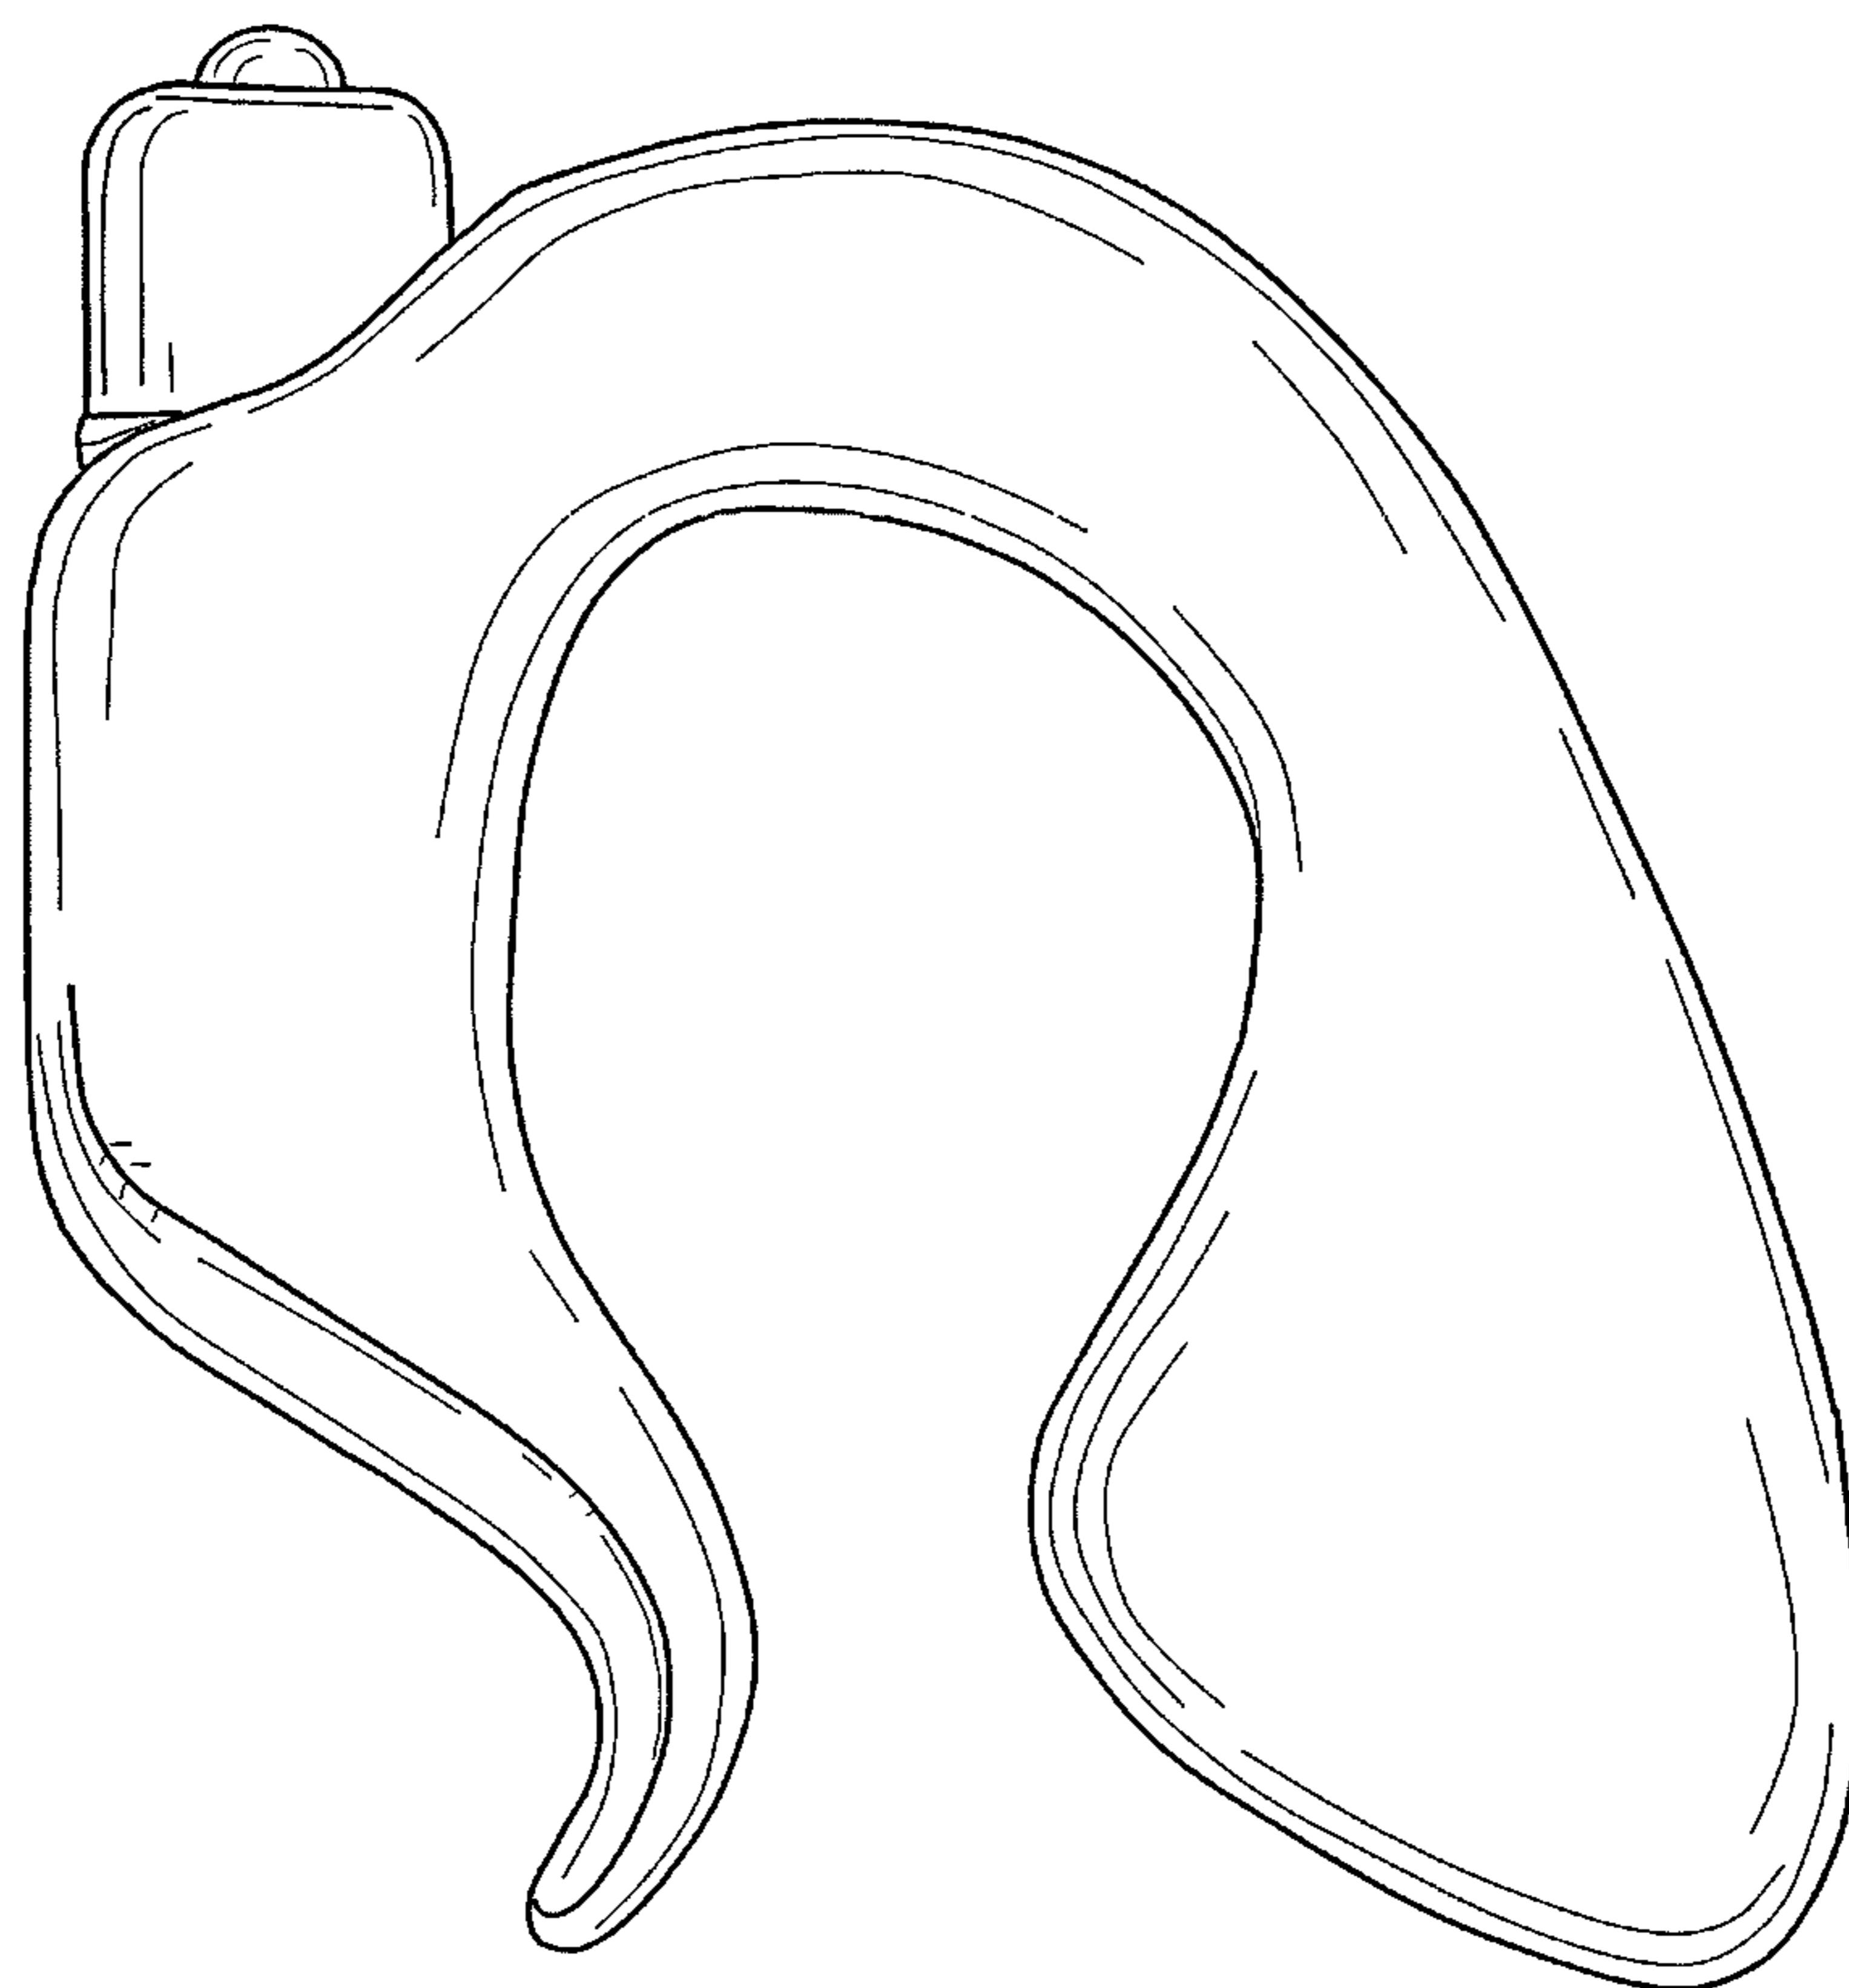


FIG. 5

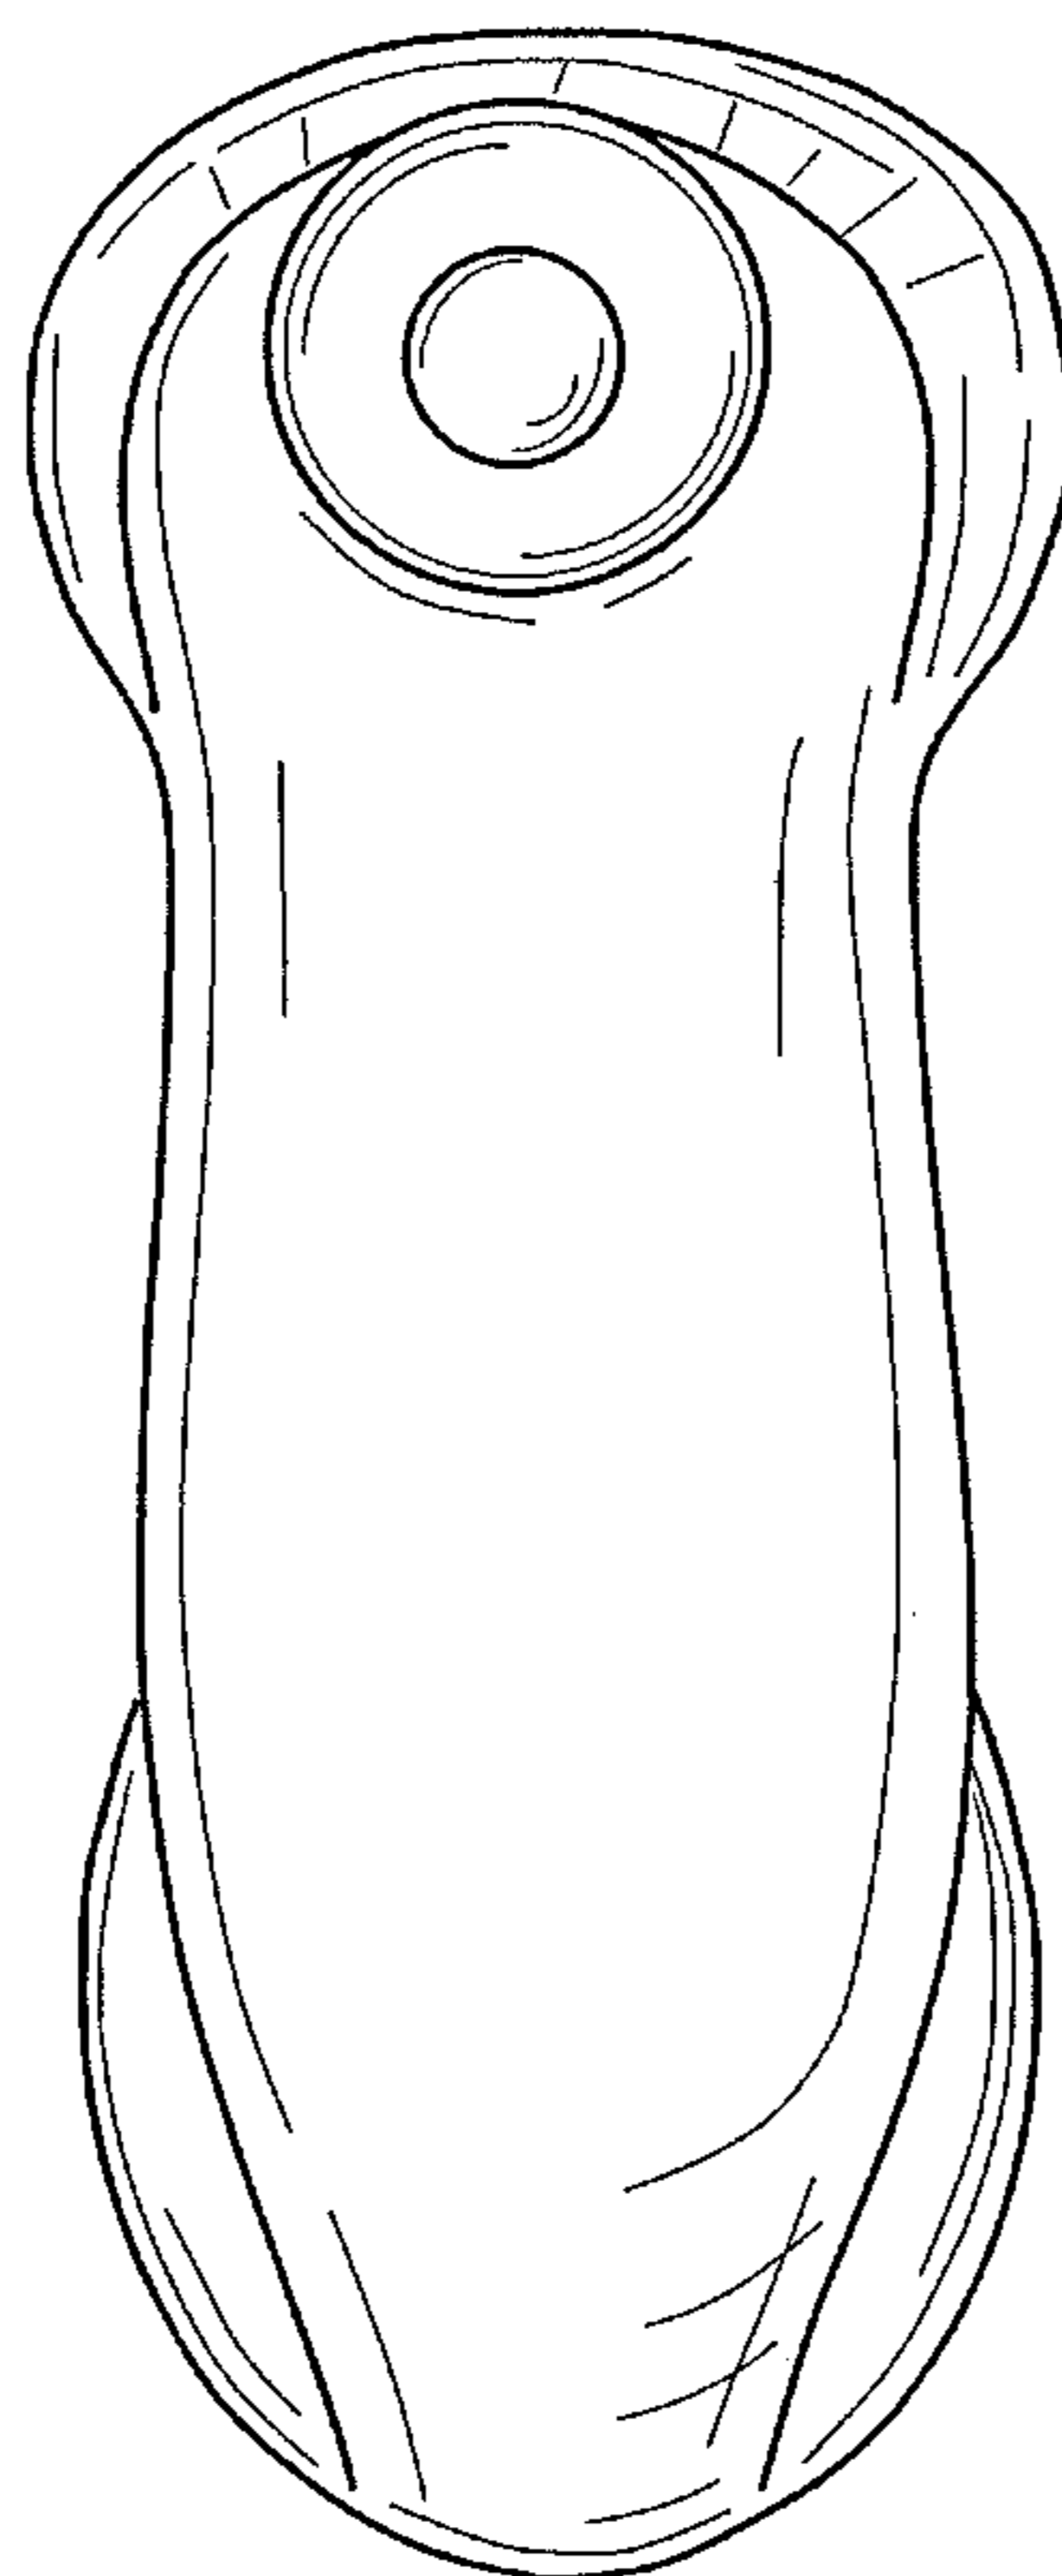

**FIG. 6**

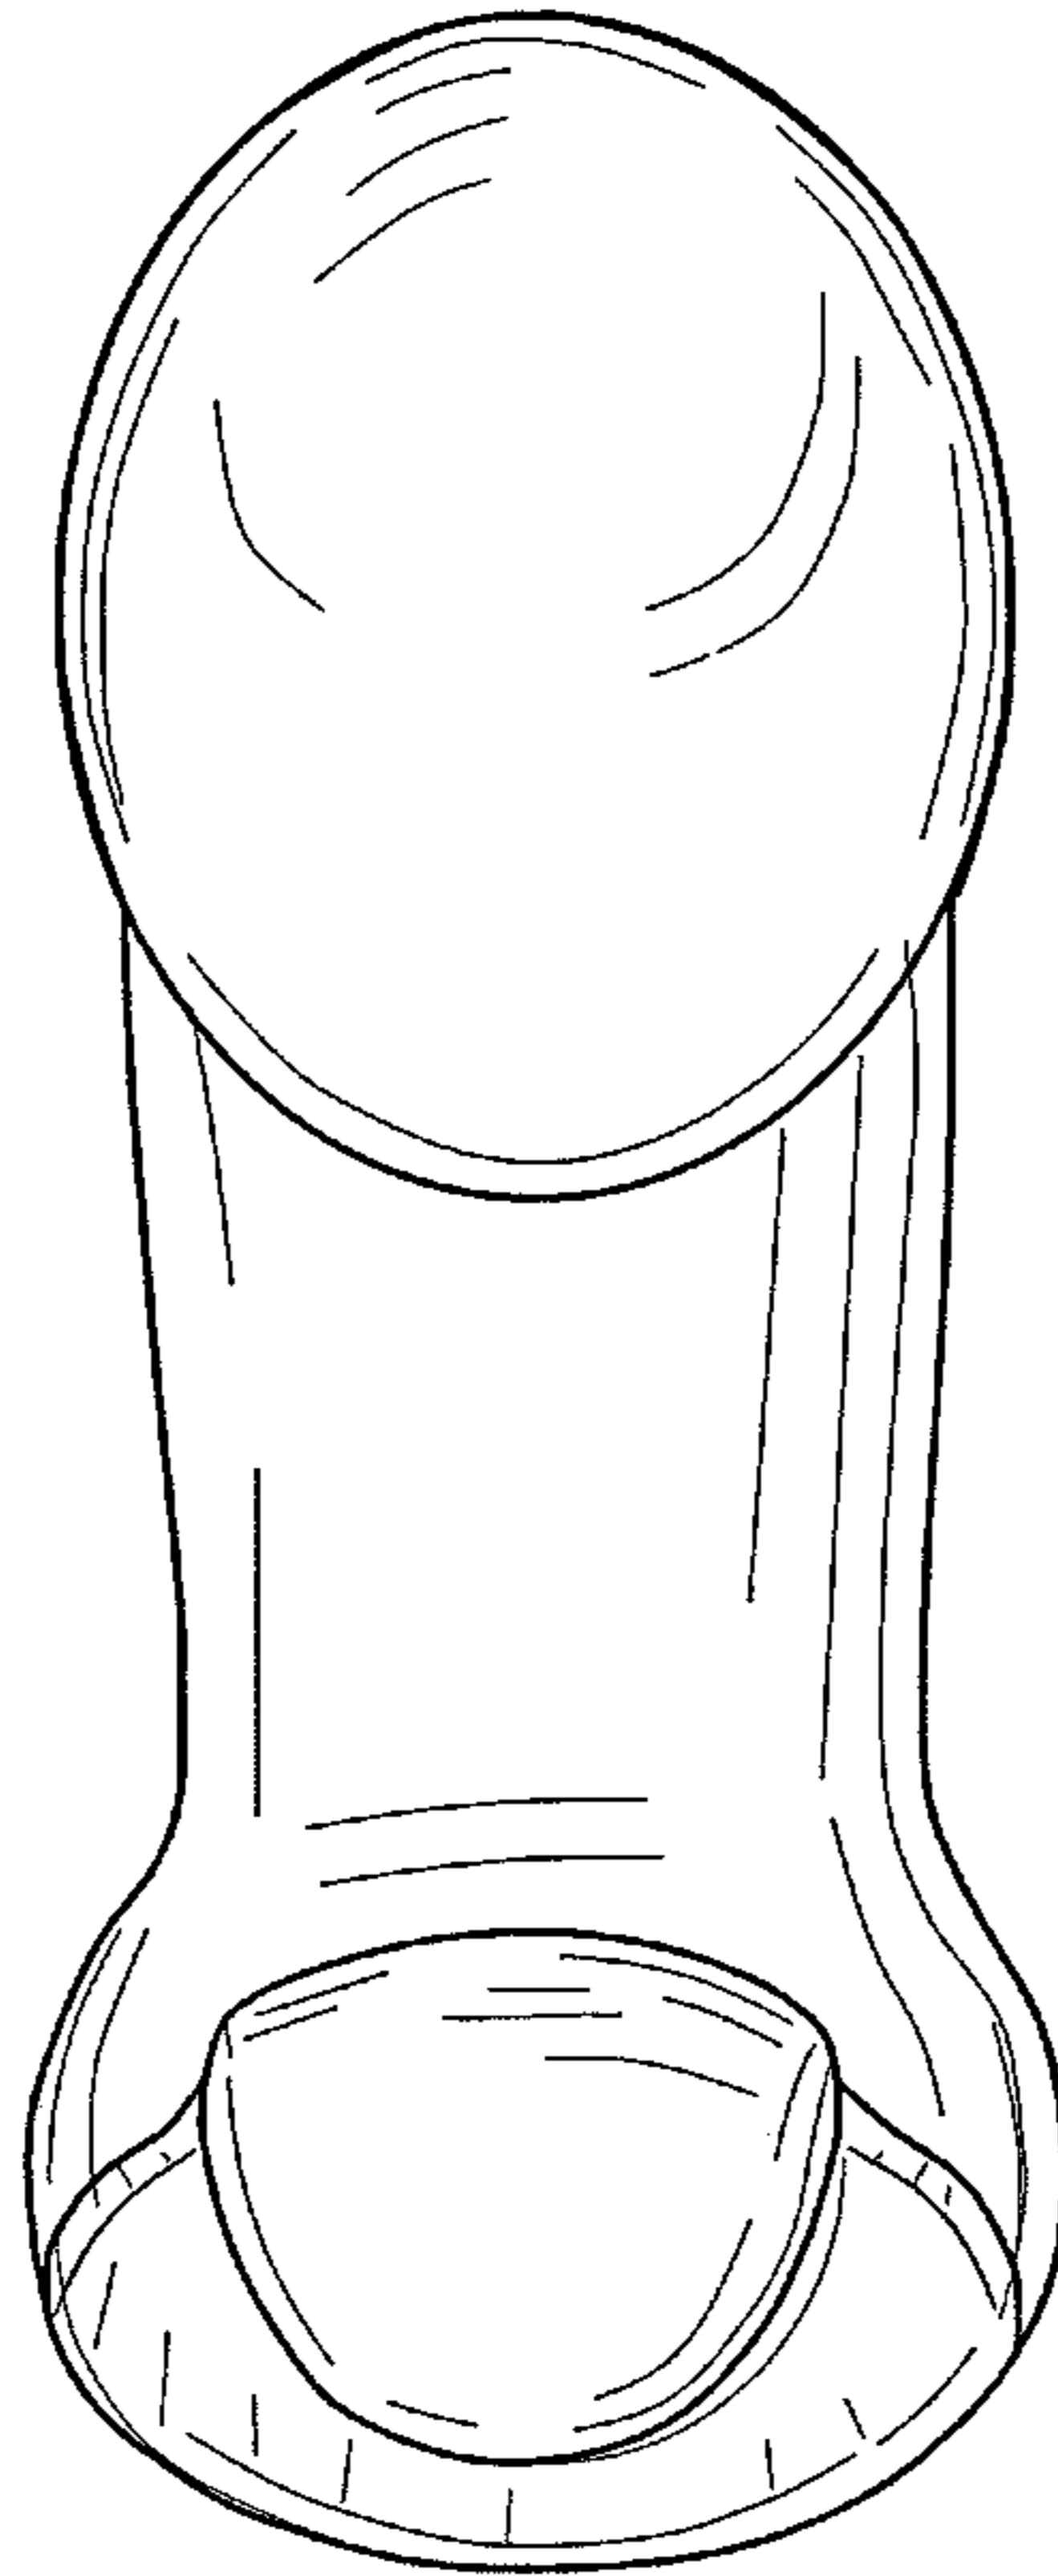


**FIG. 7**






**FIG. 8**

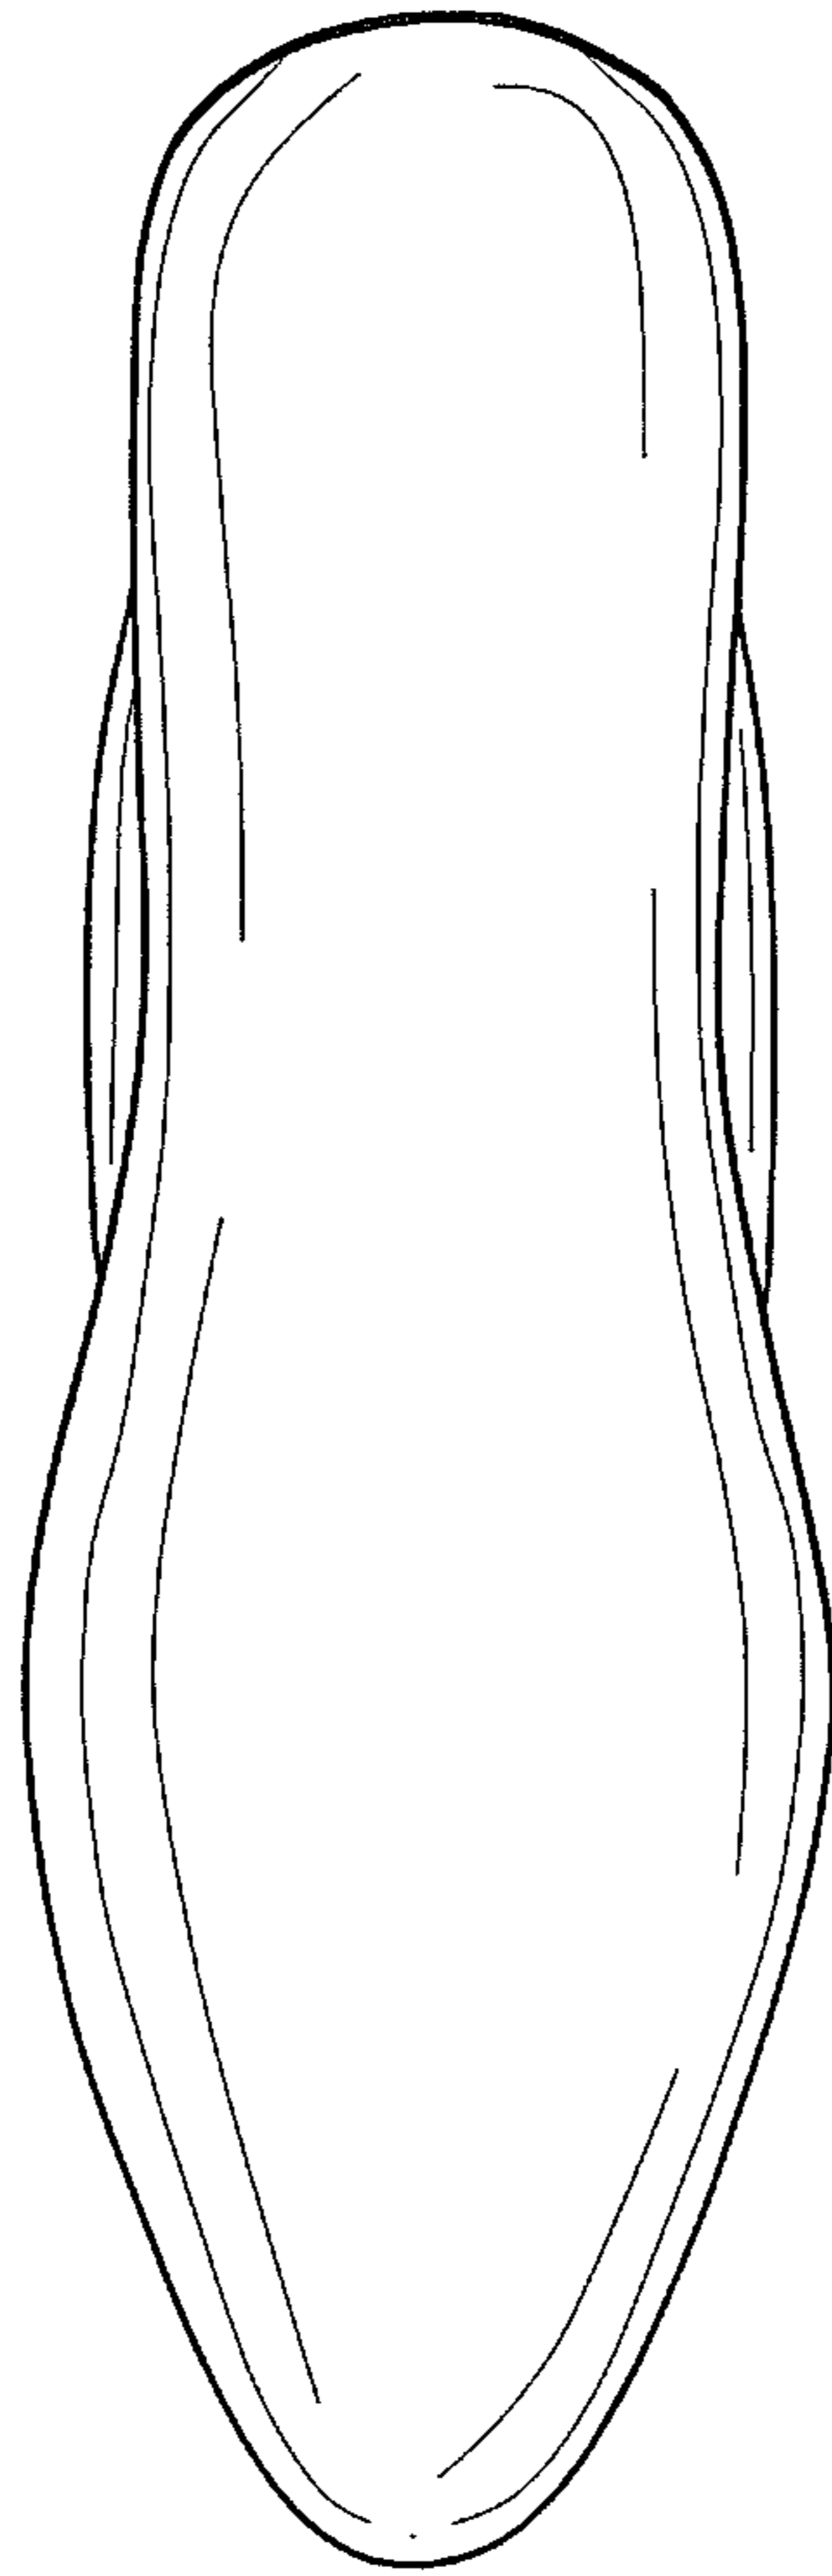

**FIG. 9**

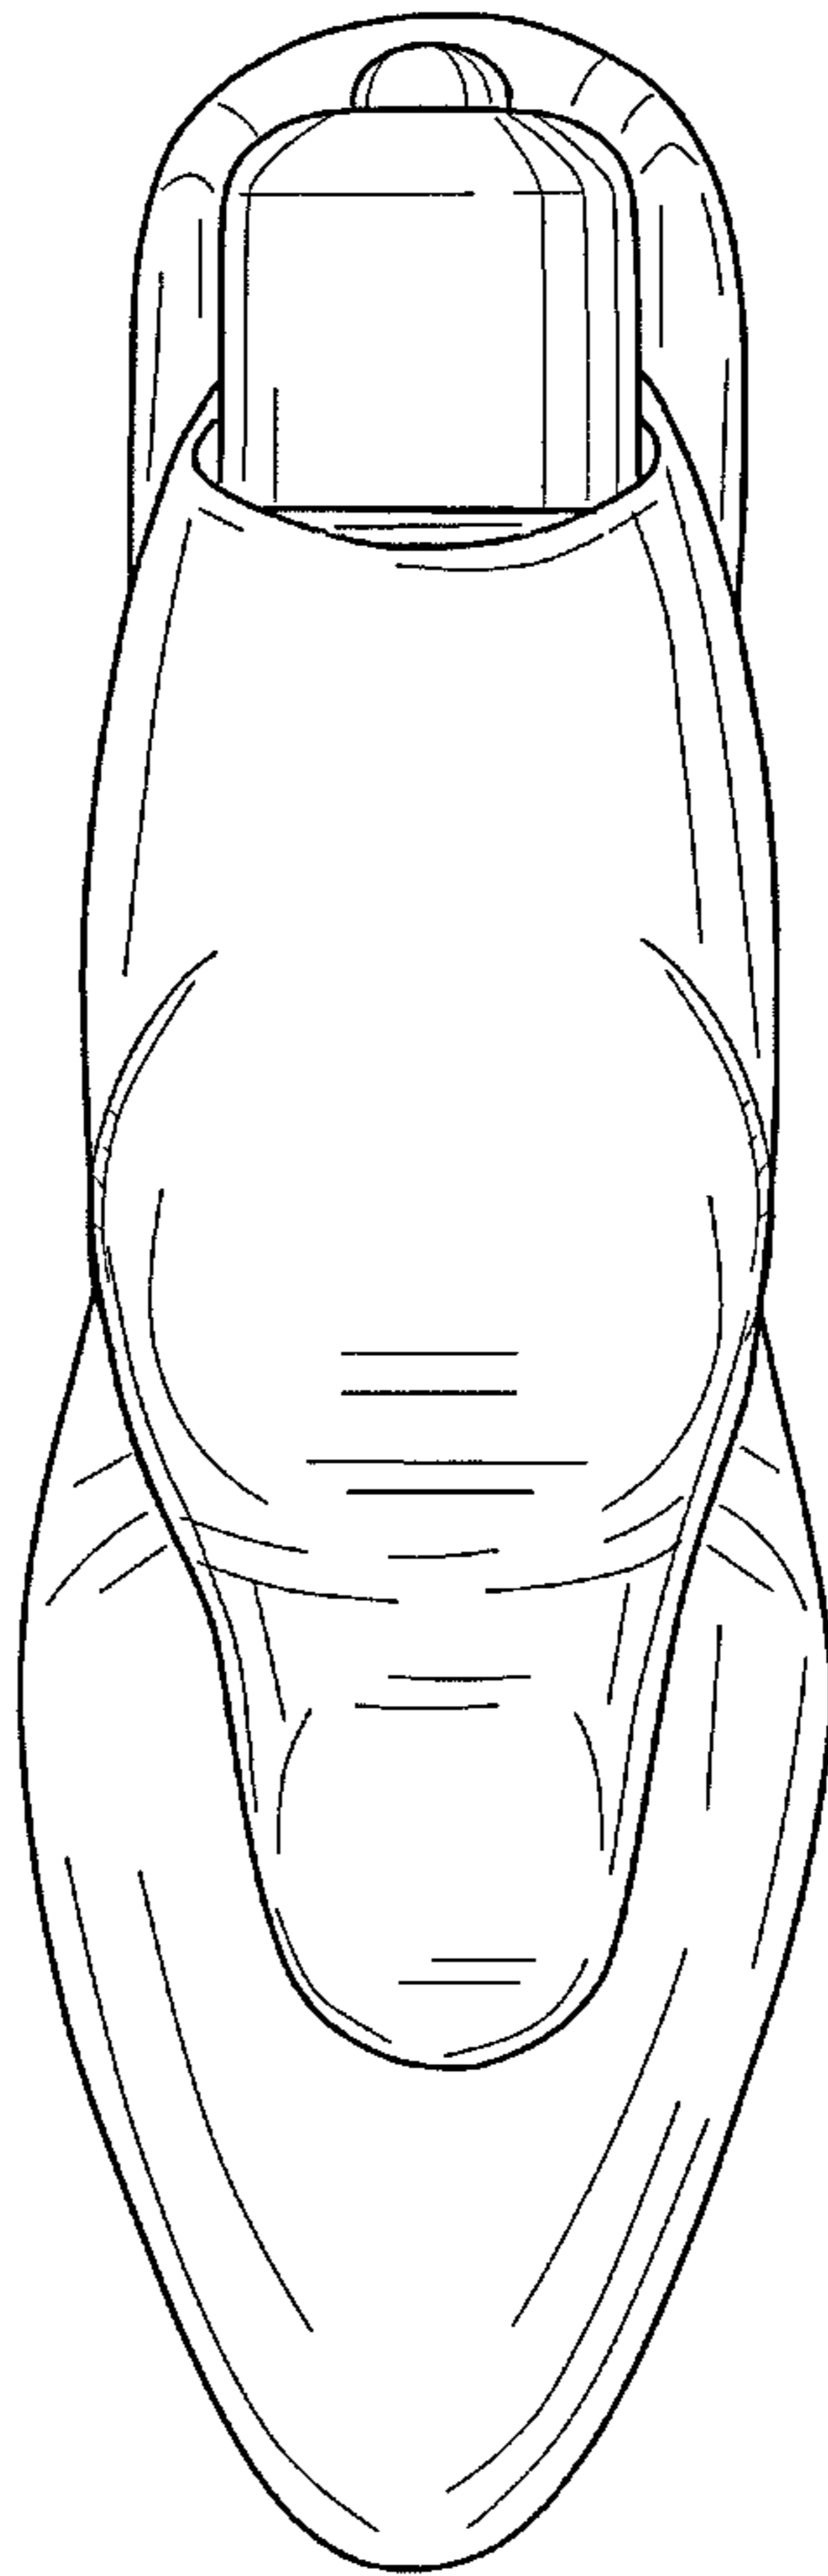

**FIG. 10**

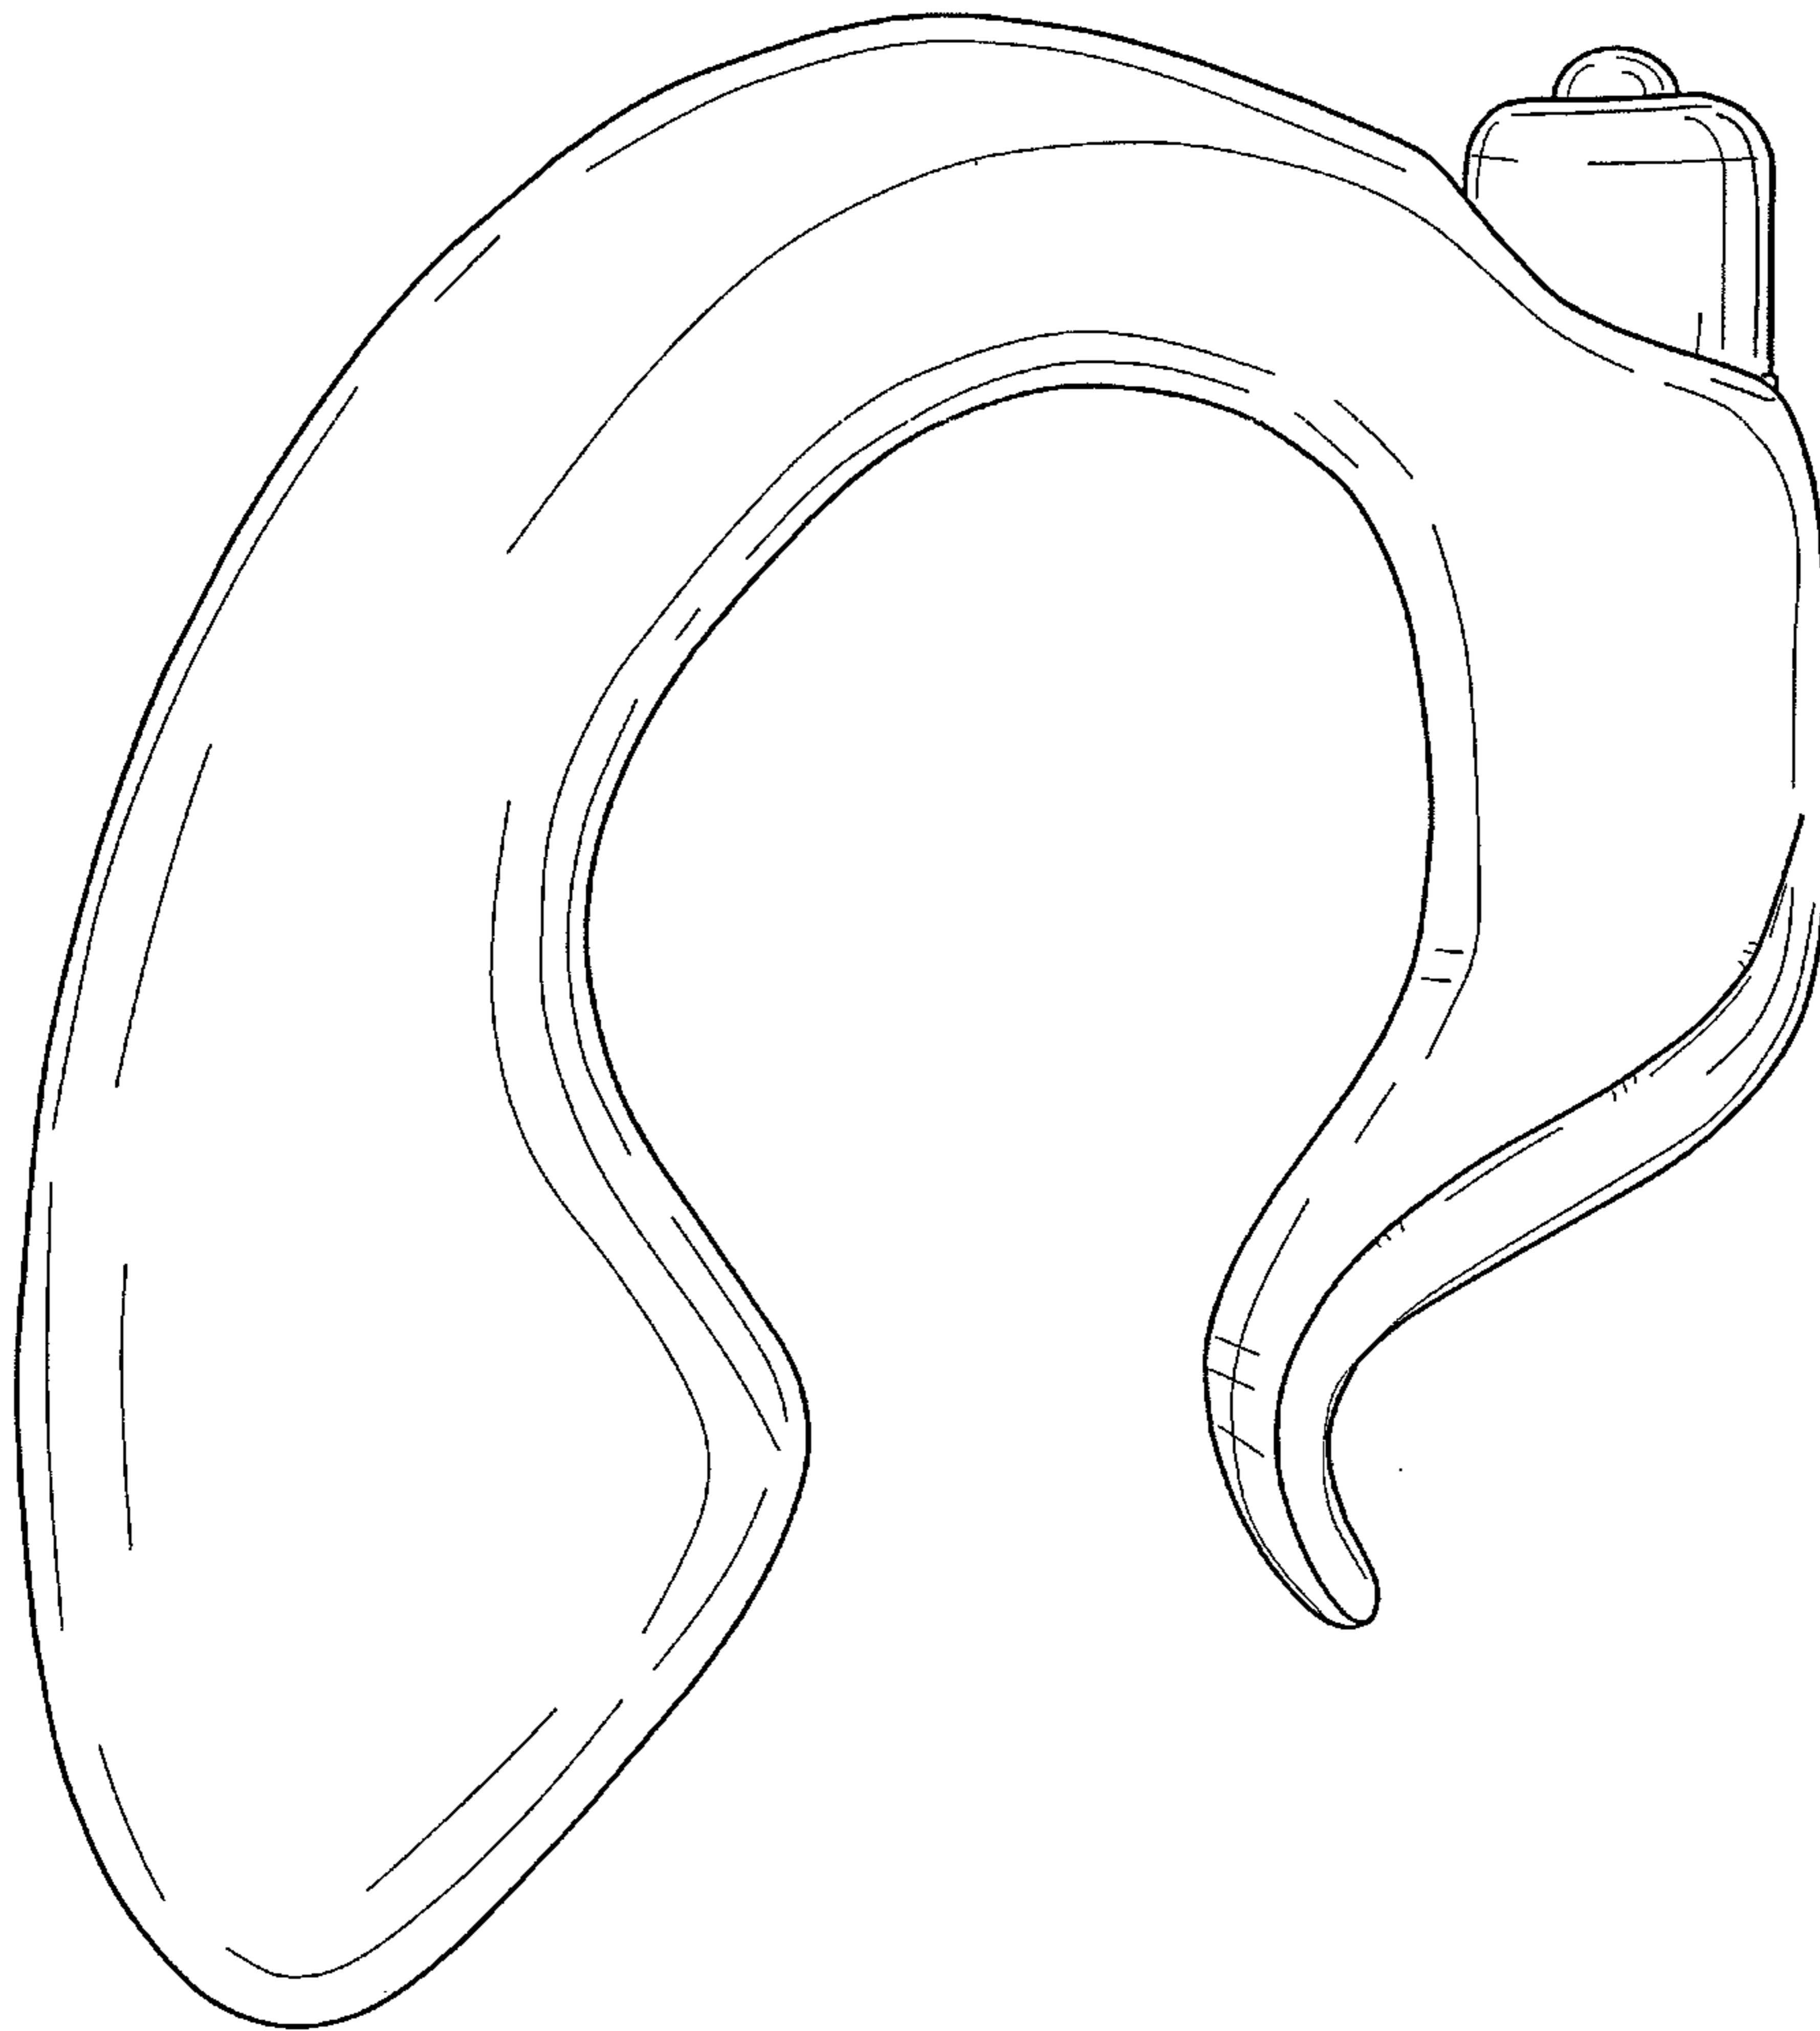


FIG. 11



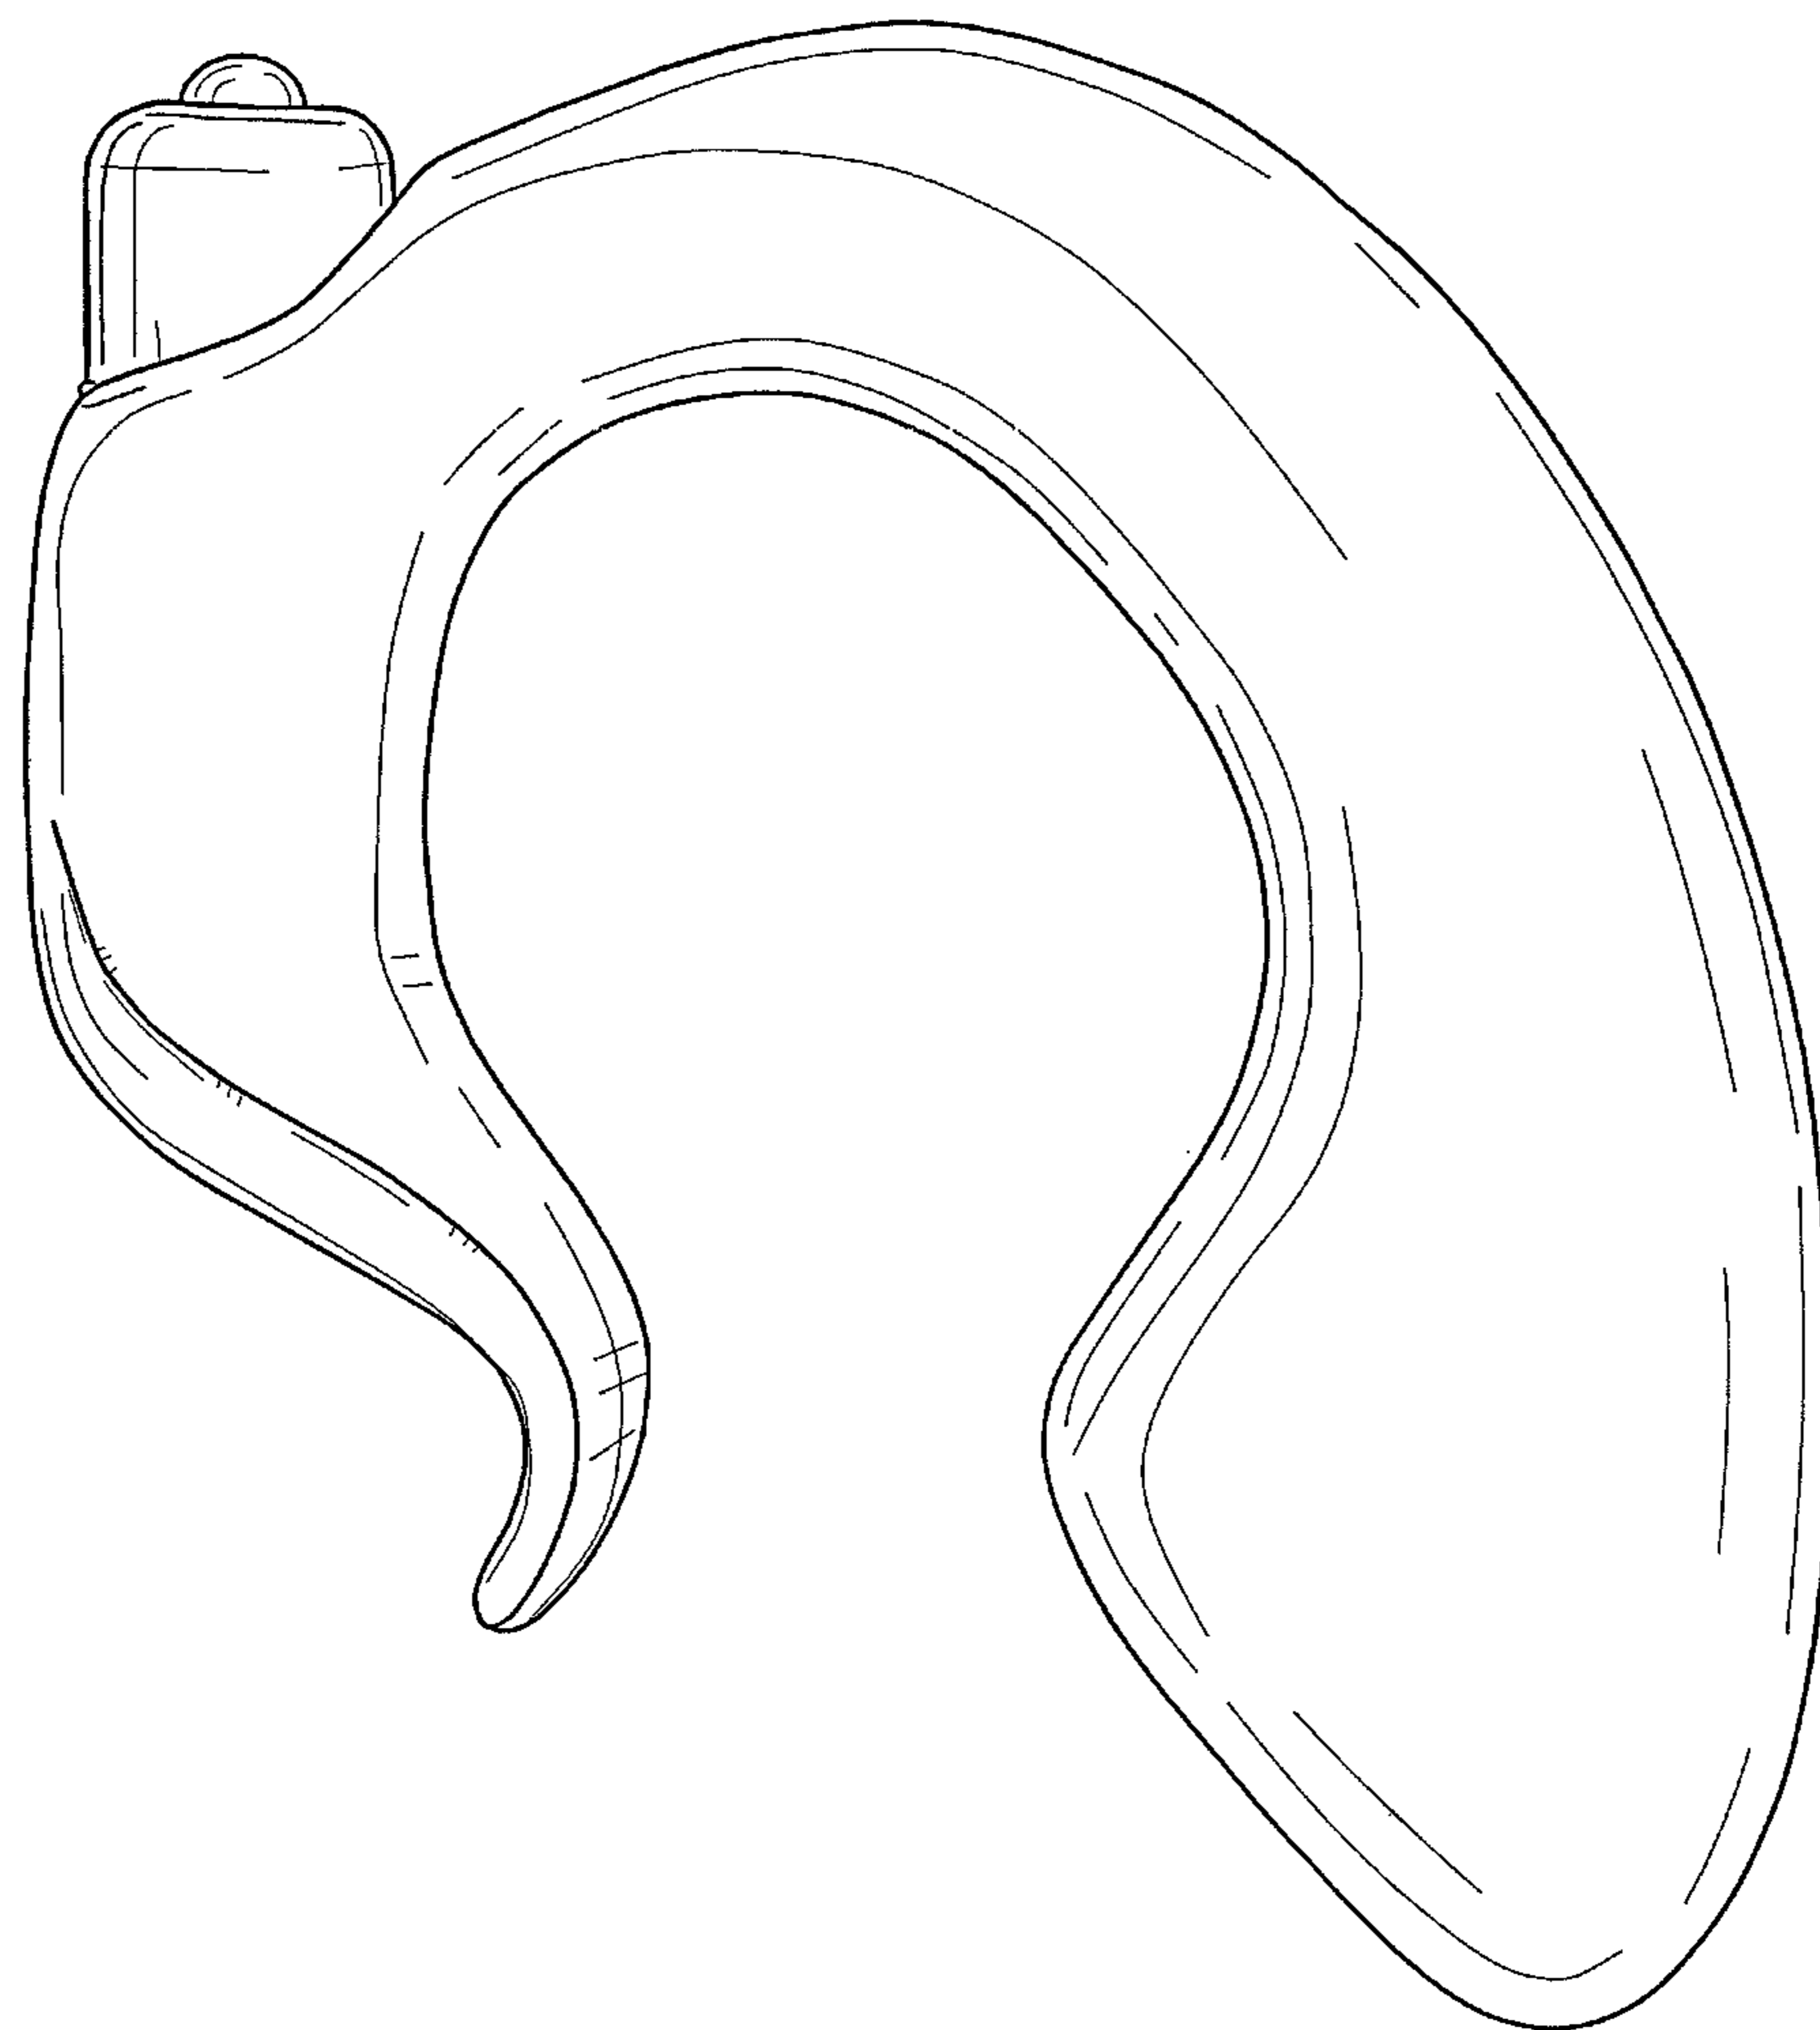


FIG. 12

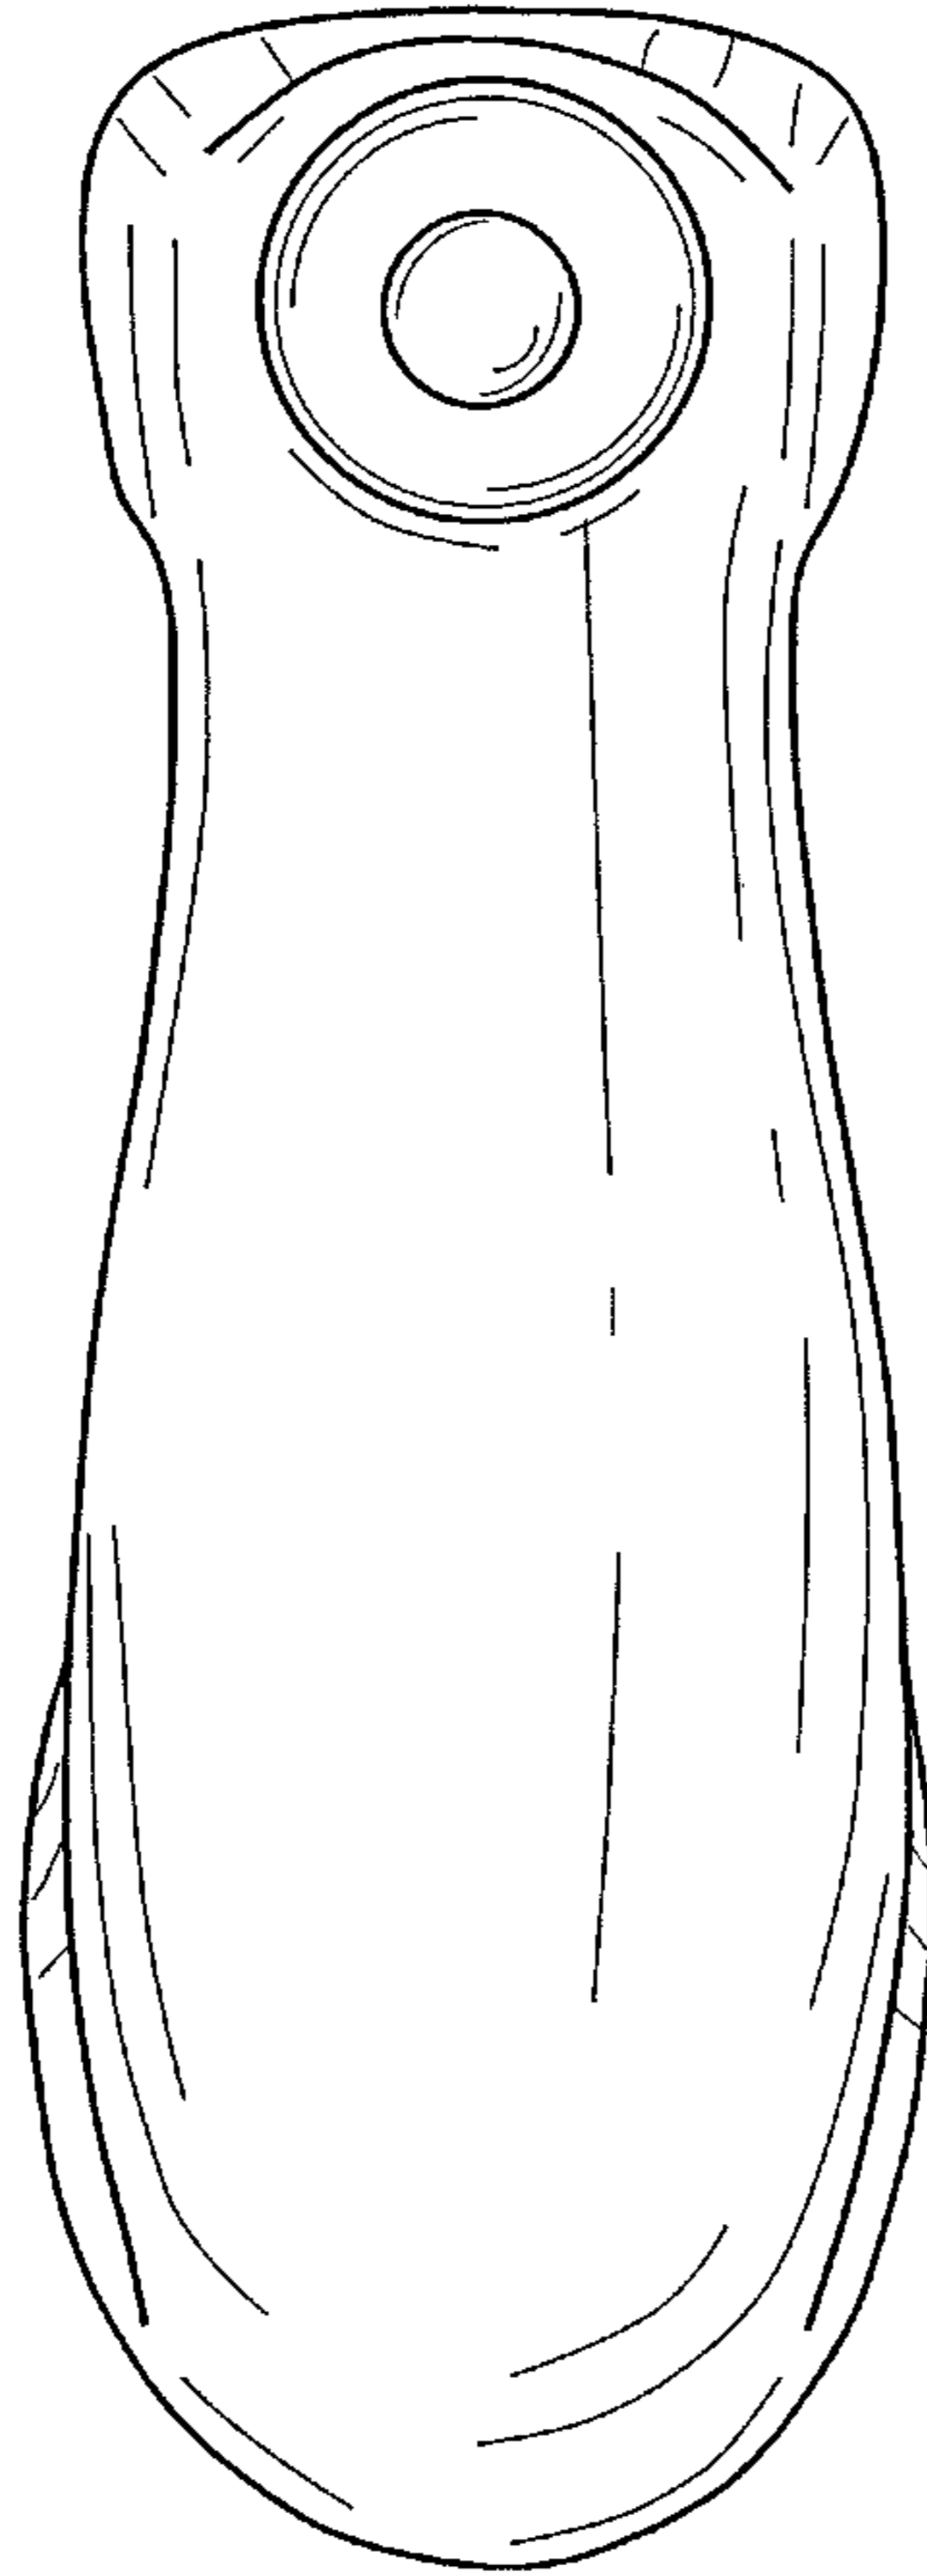

**FIG. 13**

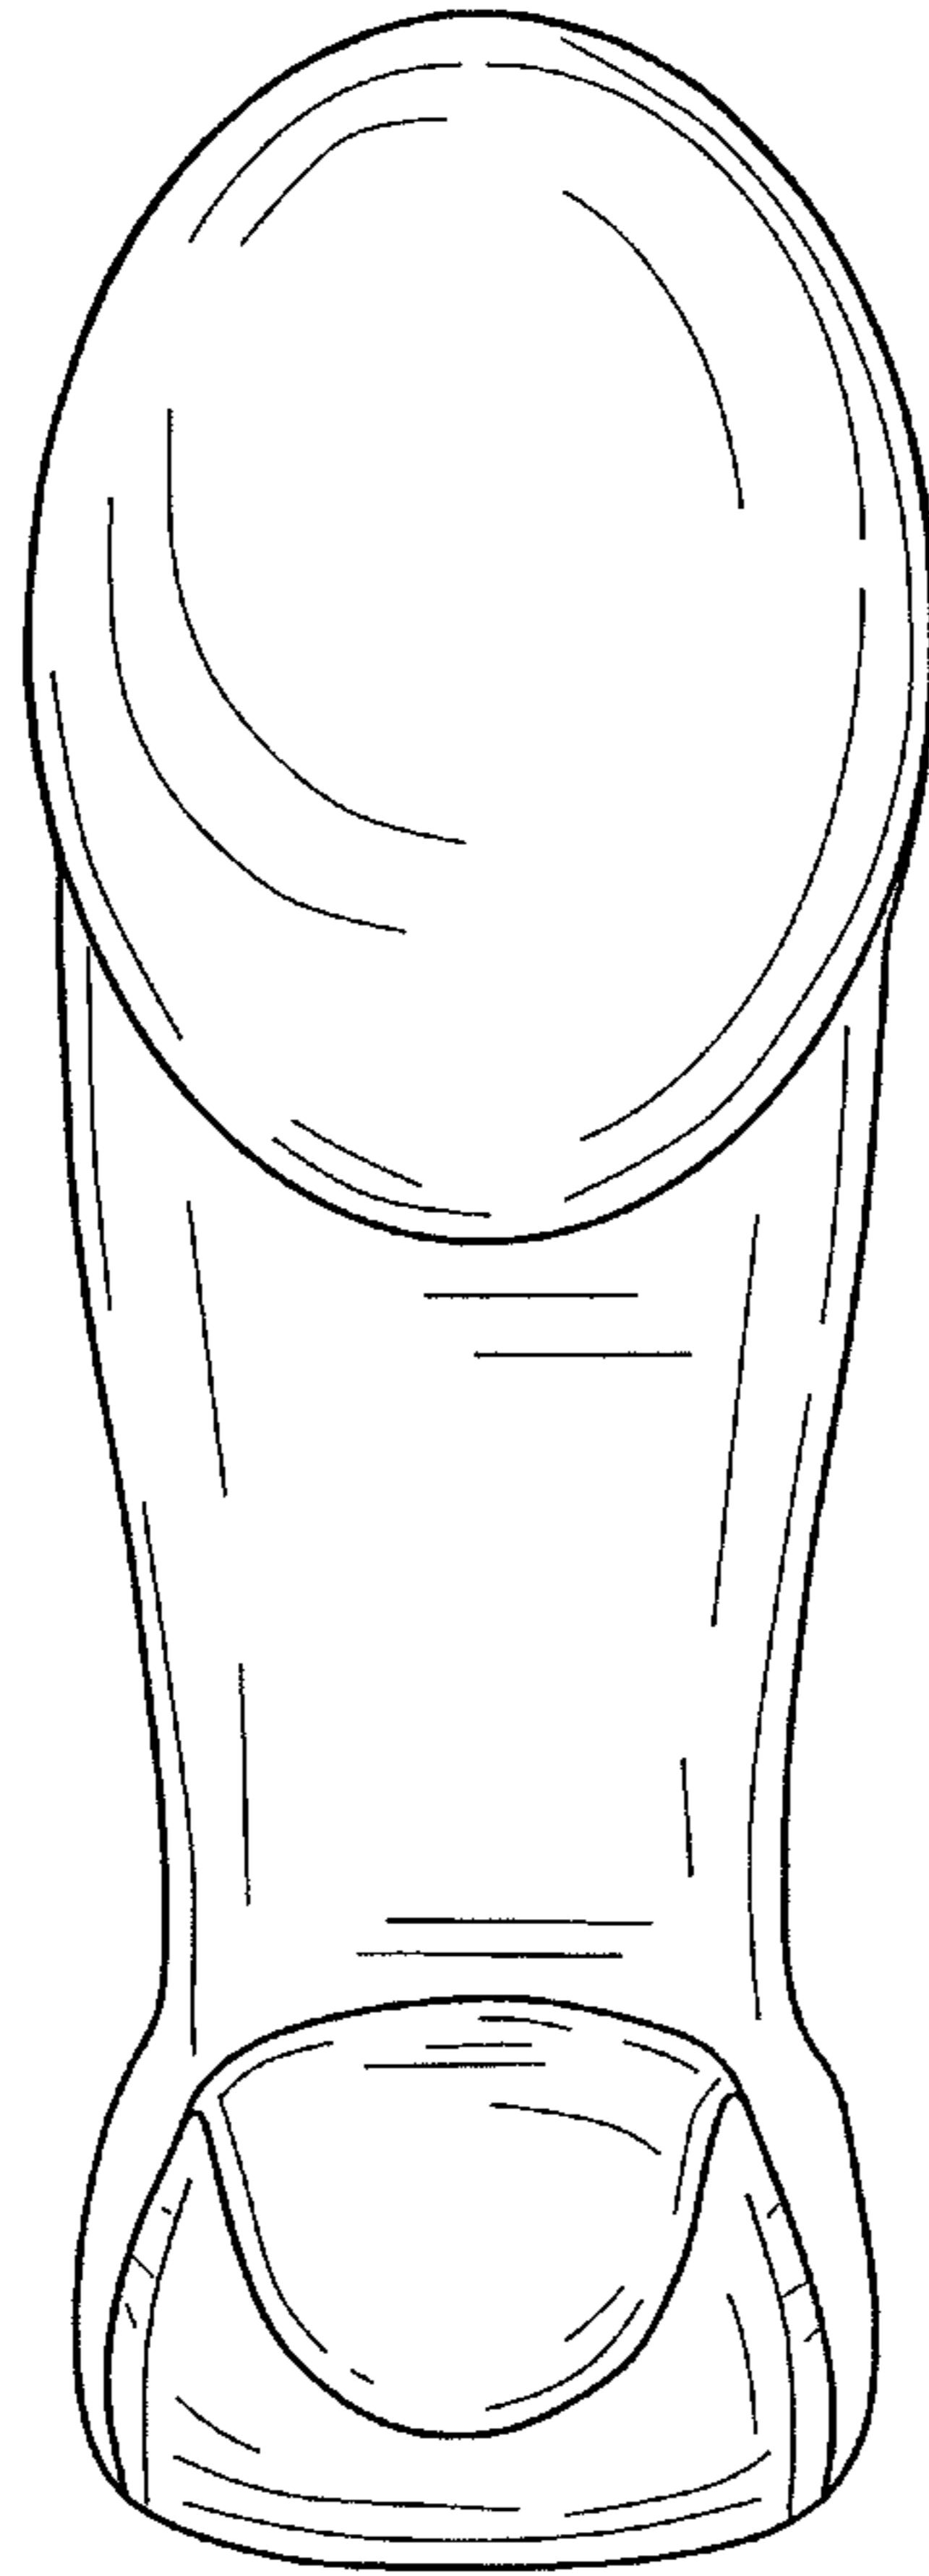

**FIG. 14**