



US00D689189S

(12) **United States Design Patent**  
**Dunn et al.**

(10) **Patent No.:** **US D689,189 S**

(45) **Date of Patent:** **\*\* \*Sep. 3, 2013**

(54) **MEDICAL DEVICE**

(75) Inventors: **Timothy Christian Dunn**, San Francisco, CA (US); **Wesley Scott Harper**, Alameda, CA (US); **Annie C. Tan**, Redwood City, CA (US)

(73) Assignee: **Abbott Diabetes Care Inc.**, Alameda, CA (US)

(\*) Notice: This patent is subject to a terminal disclaimer.

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/368,833**

(22) Filed: **Aug. 30, 2010**

(51) **LOC (9) Cl.** ..... **24-01**

(52) **U.S. Cl.**  
USPC ..... **D24/169**

(58) **Field of Classification Search**  
USPC ..... D24/165-169, 107, 186, 216, 223, D24/231, 232; D10/46, 81; D14/341; 422/56, 422/58, 68.1; 600/316, 322, 347, 365, 368  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D406,895 S \* 3/1999 Byrd et al. .... D24/169  
D423,102 S \* 4/2000 Mertenat ..... D24/169  
D440,312 S \* 4/2001 Bertrand et al. .... D24/169  
D473,310 S \* 4/2003 Schlagheck et al. .... D24/169

D495,418 S \* 8/2004 Rounds et al. .... D24/169  
D502,655 S \* 3/2005 Huang ..... D10/81  
D545,438 S \* 6/2007 Huang et al. .... D24/186  
D546,218 S \* 7/2007 Grasso et al. .... D10/81  
D546,454 S \* 7/2007 Gutmann et al. .... D24/169  
D546,456 S \* 7/2007 May ..... D24/186  
D585,135 S \* 1/2009 Mori et al. .... D24/169  
D610,688 S \* 2/2010 Donars et al. .... D24/169  
D622,394 S \* 8/2010 Bielawa et al. .... D24/169  
D650,079 S \* 12/2011 Presta et al. .... D24/169  
2010/0053851 A1 \* 3/2010 Bernstein et al. .... 361/679.01  
2010/0068795 A1 \* 3/2010 Shinohara et al. .... 435/287.1

\* cited by examiner

*Primary Examiner* — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Jackson & Co., LLP

(57) **CLAIM**

The ornamental design for a medical device, as shown and described.

**DESCRIPTION**

FIG. 1 is a front view of a medical device in accordance with the new design;

FIG. 2 is a bottom perspective view of the medical device;

FIG. 3 is a top perspective view of the medical device;


FIG. 4 is a back view of the medical device;

FIG. 5 is a right-side perspective view of the medical device; and,

FIG. 6 is a left-side perspective view of the medical device.

The broken lines in the drawing views are included for the purpose of illustrating portions of the medical device that form no part of the claimed design.

**1 Claim, 4 Drawing Sheets**

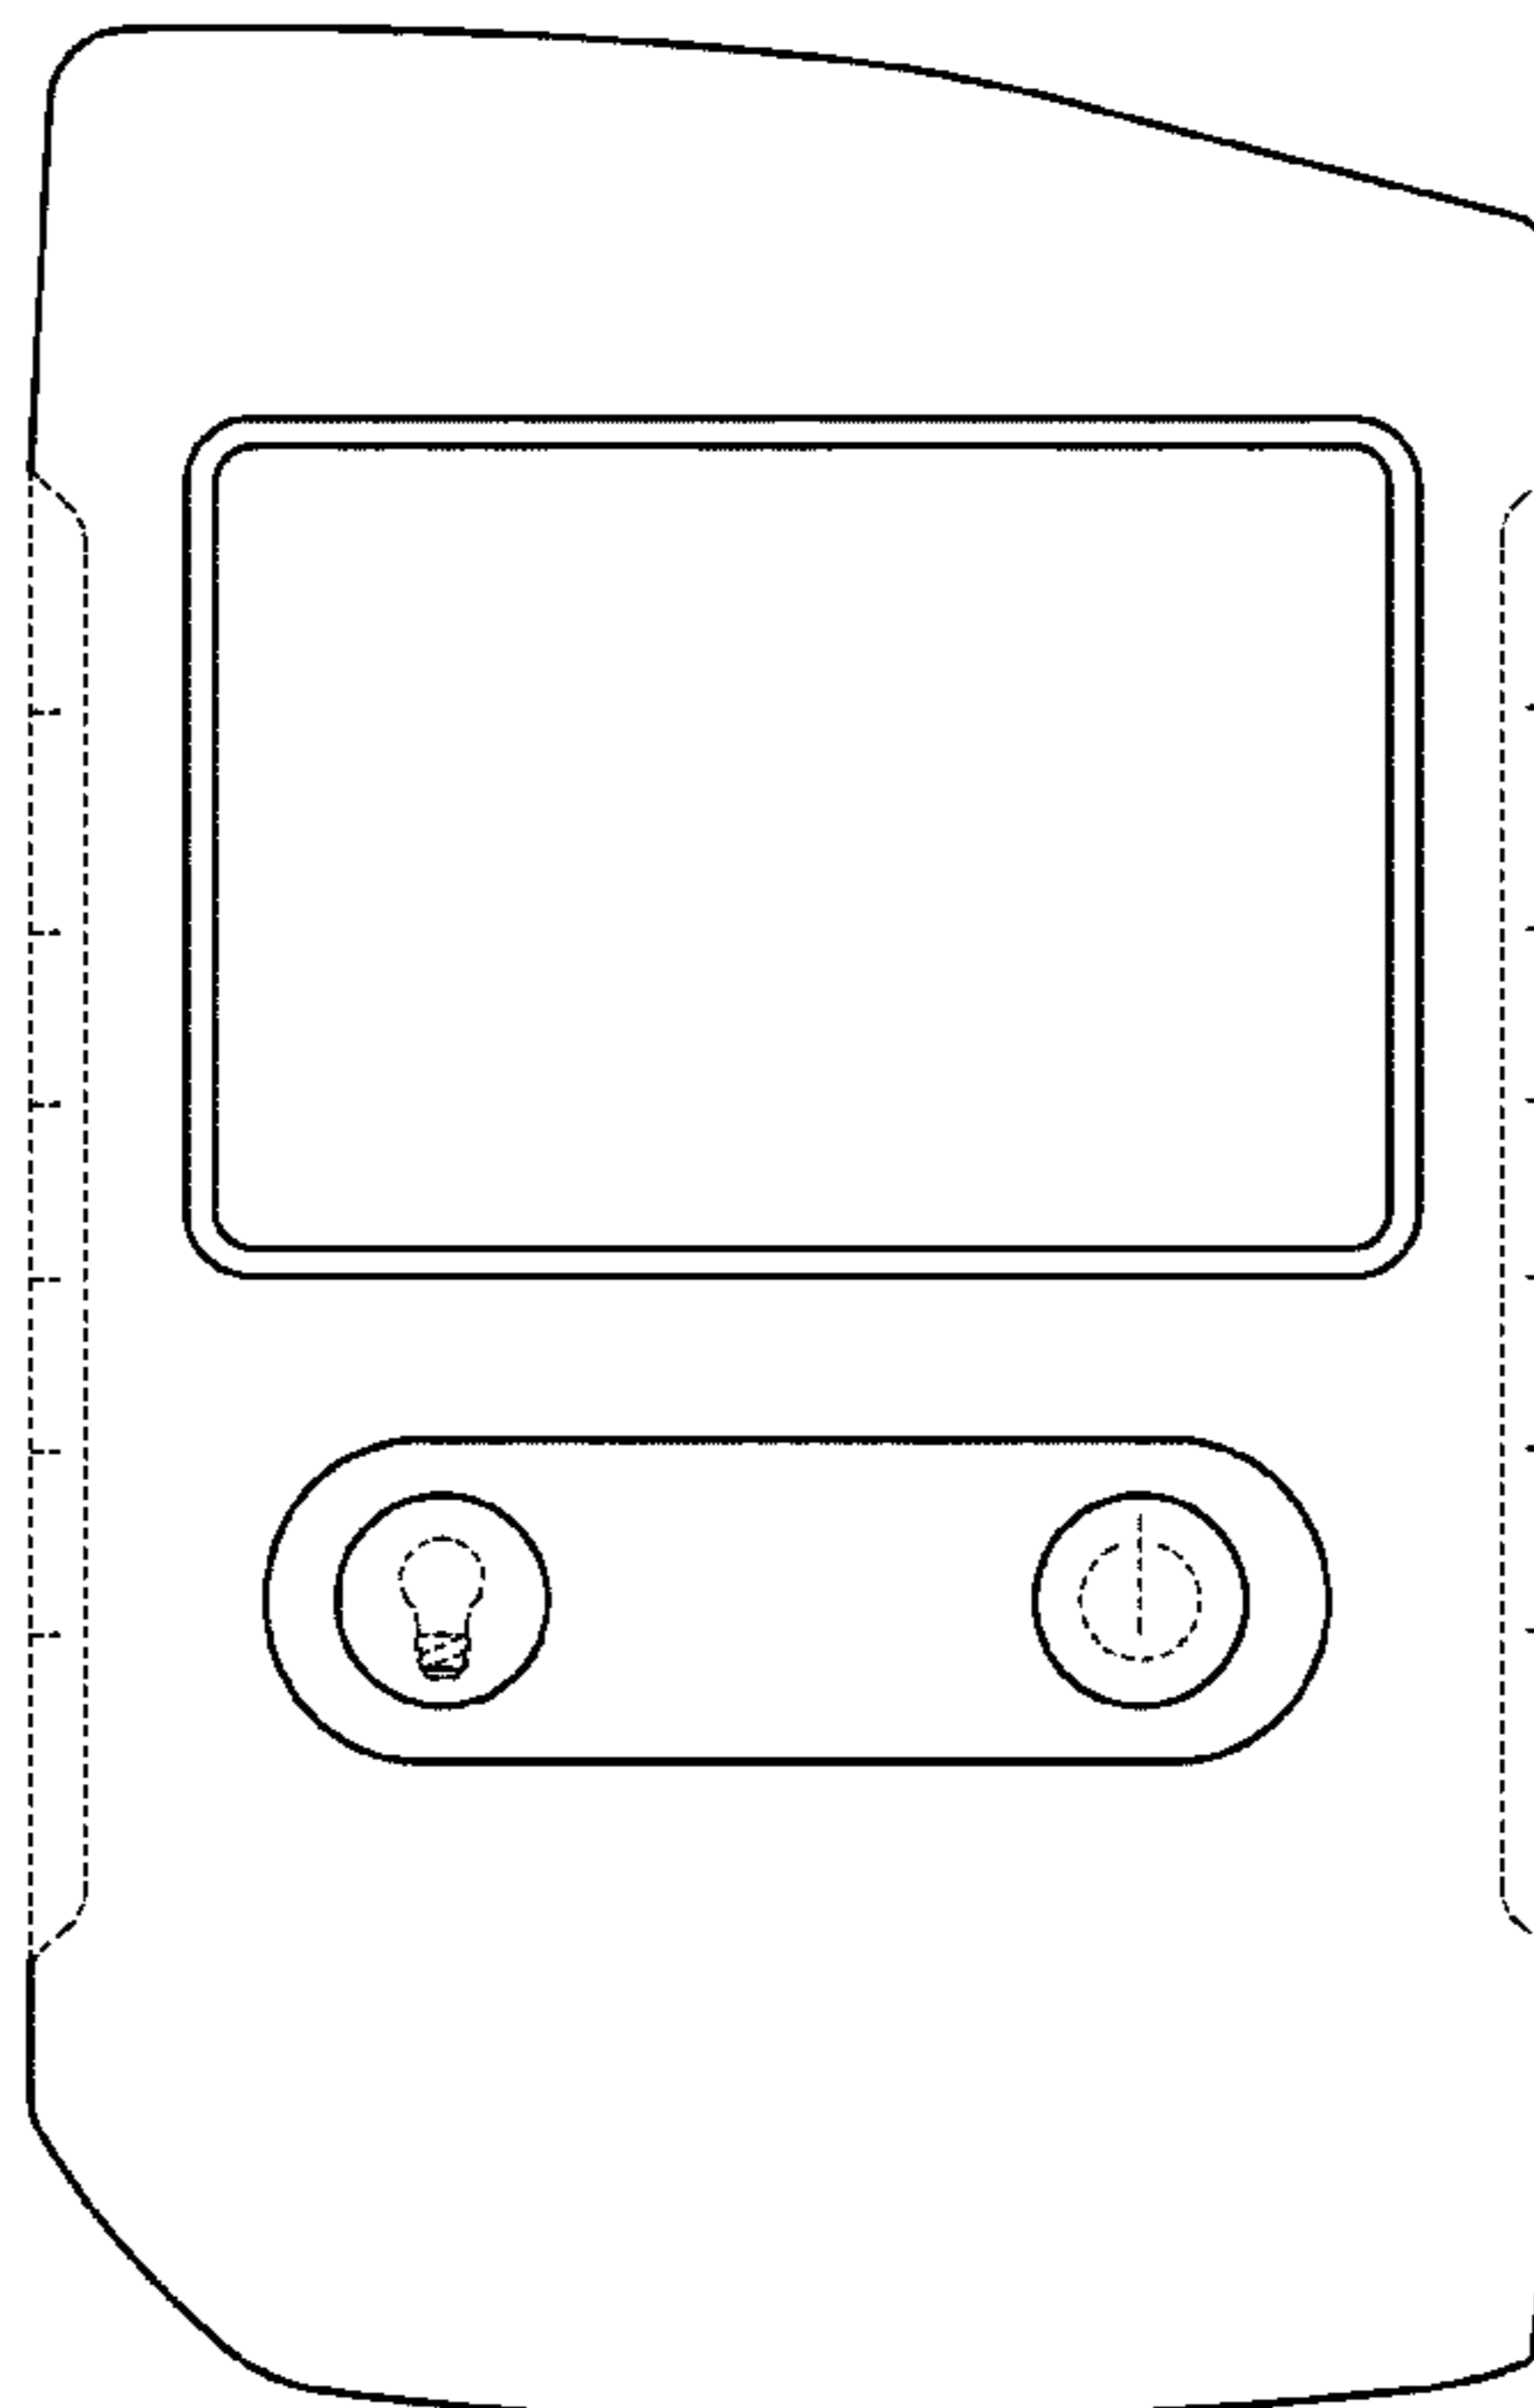

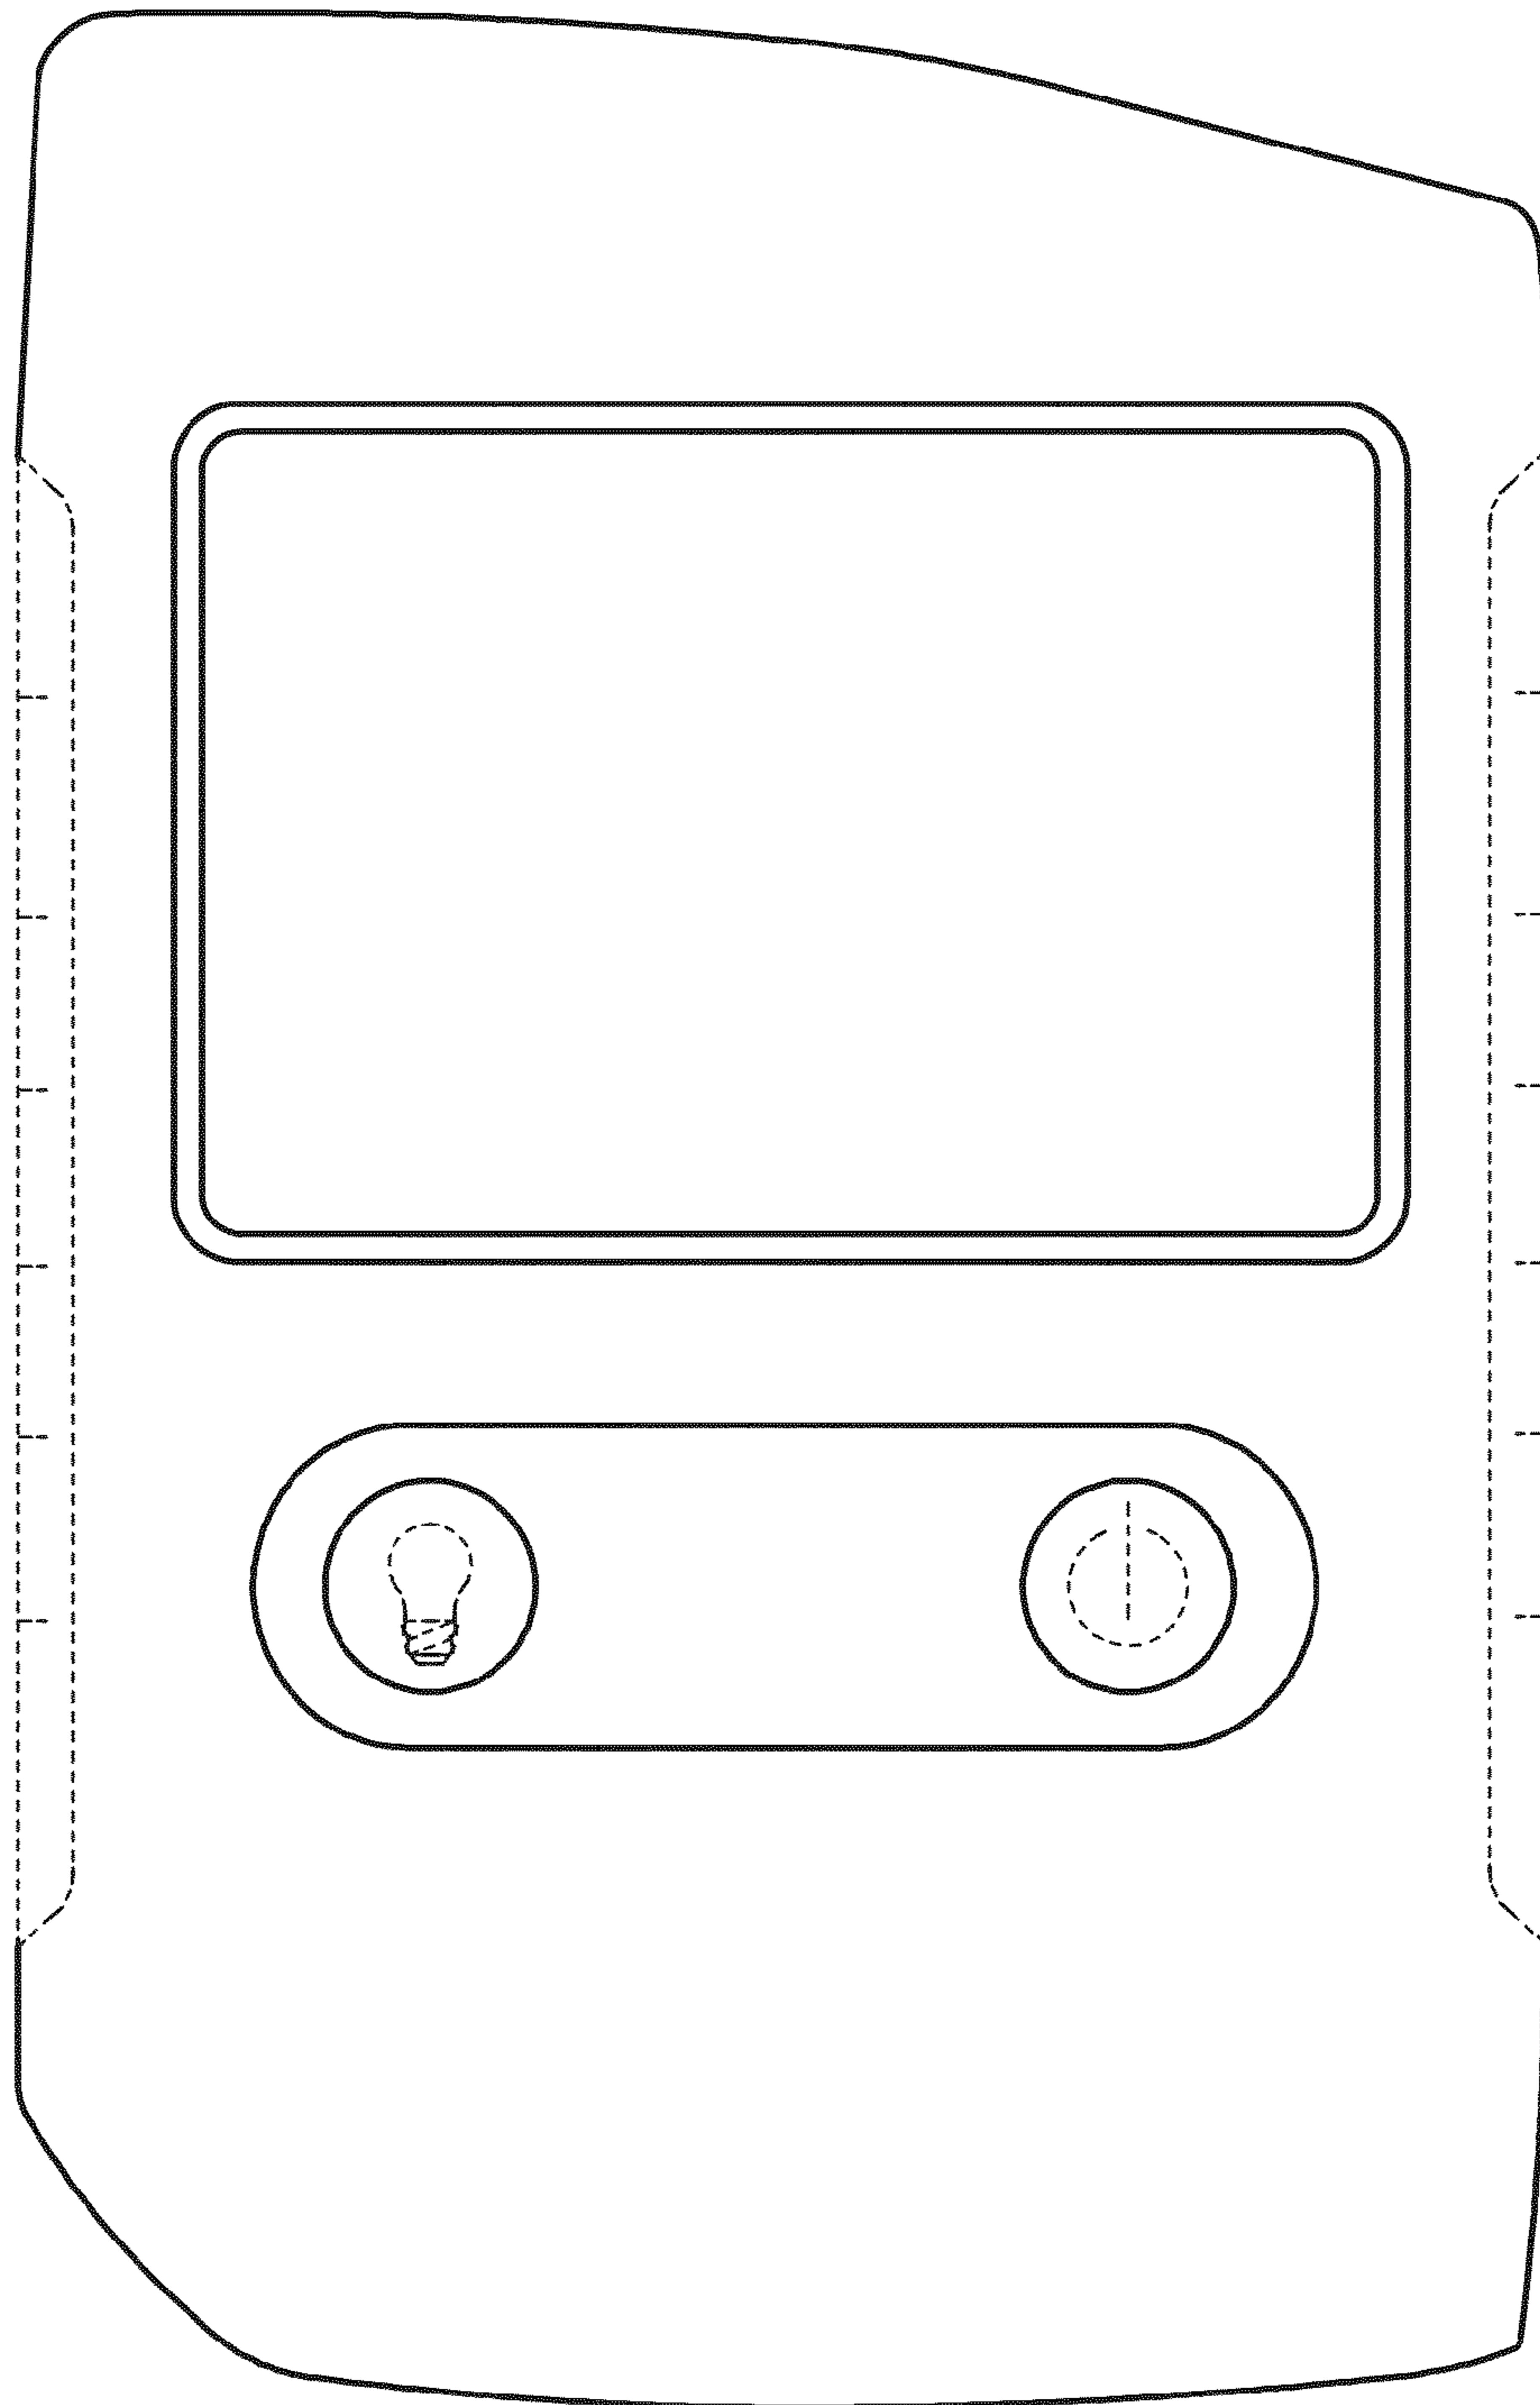


FIG. 1

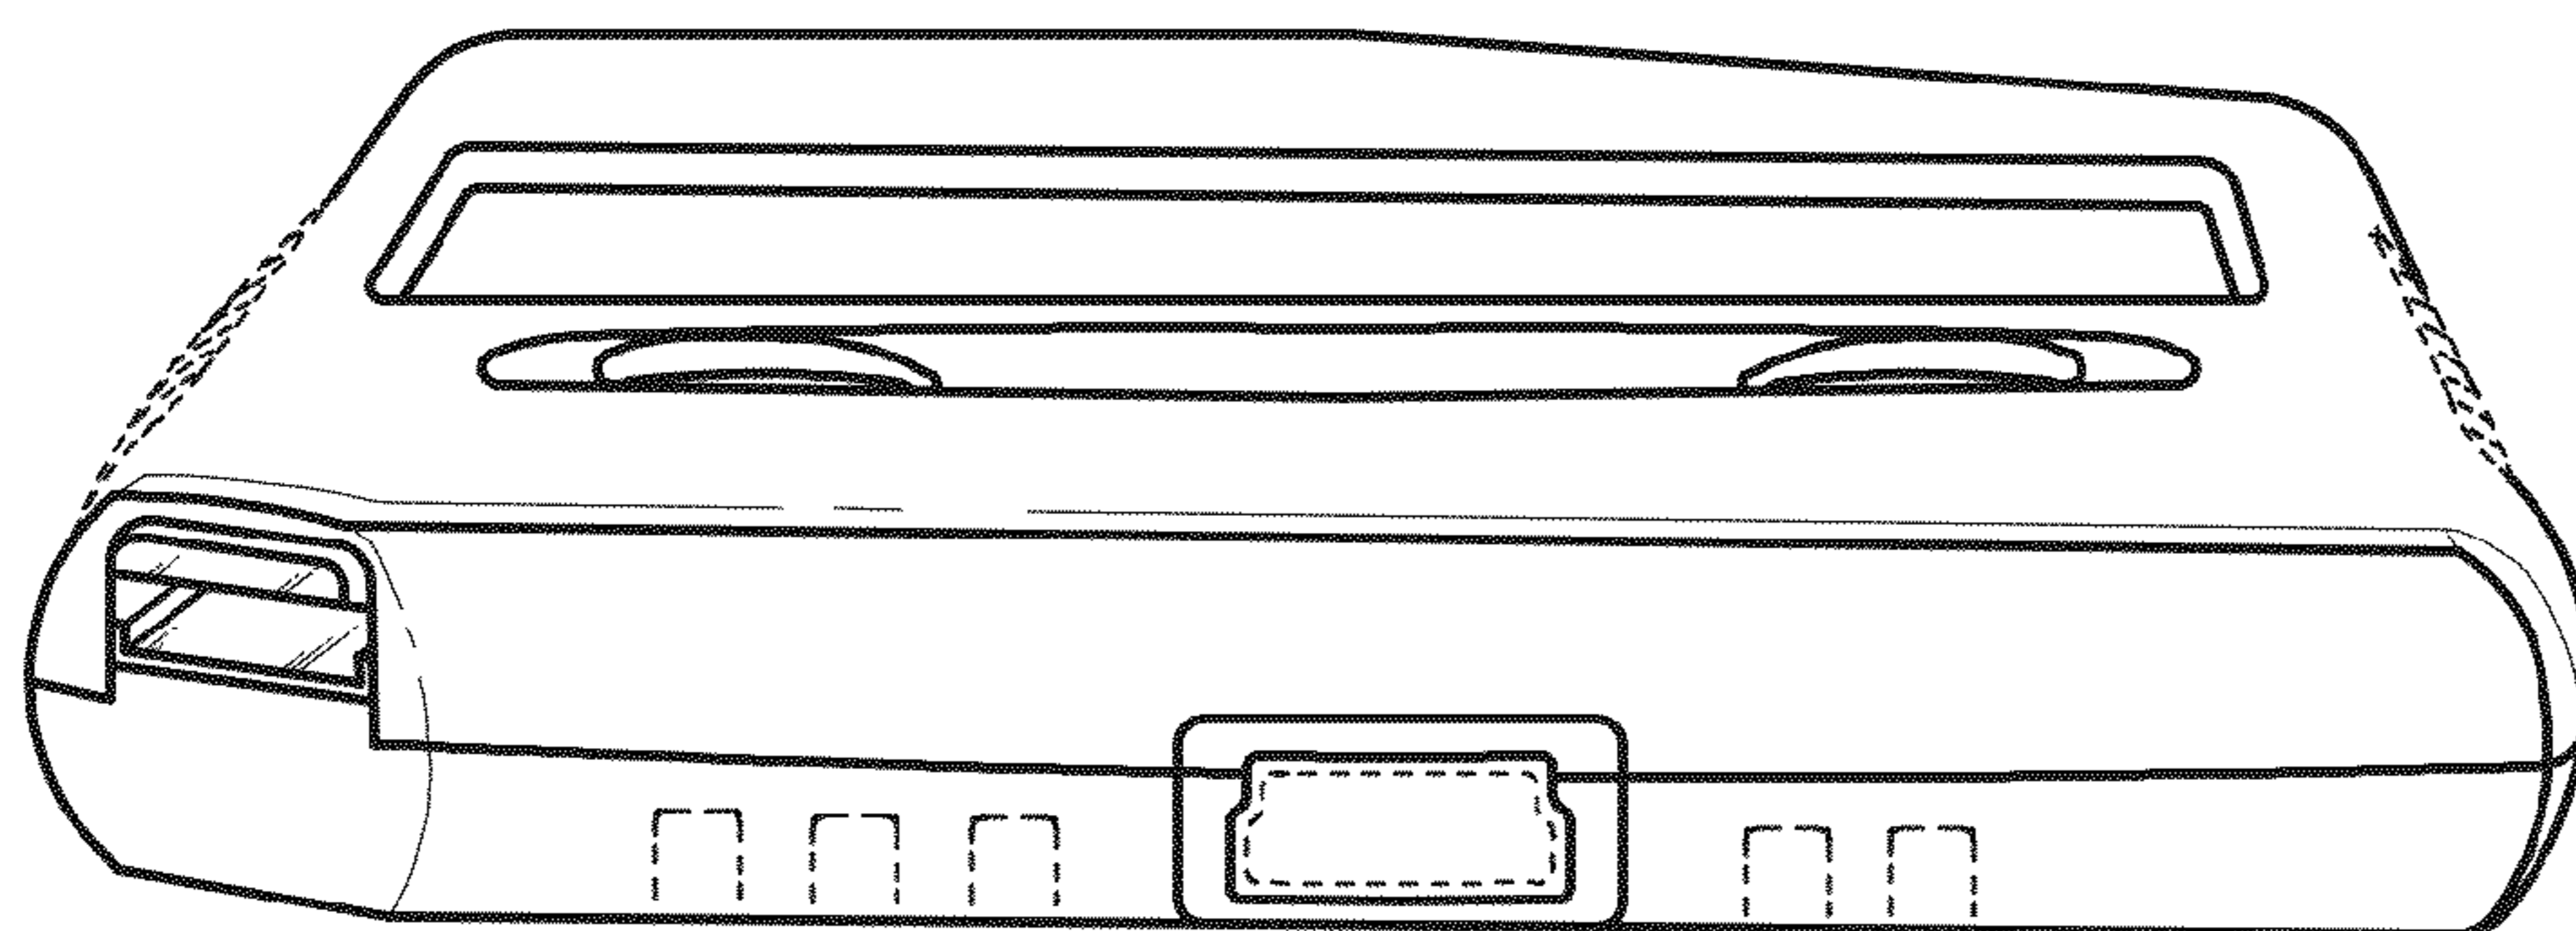


FIG. 2

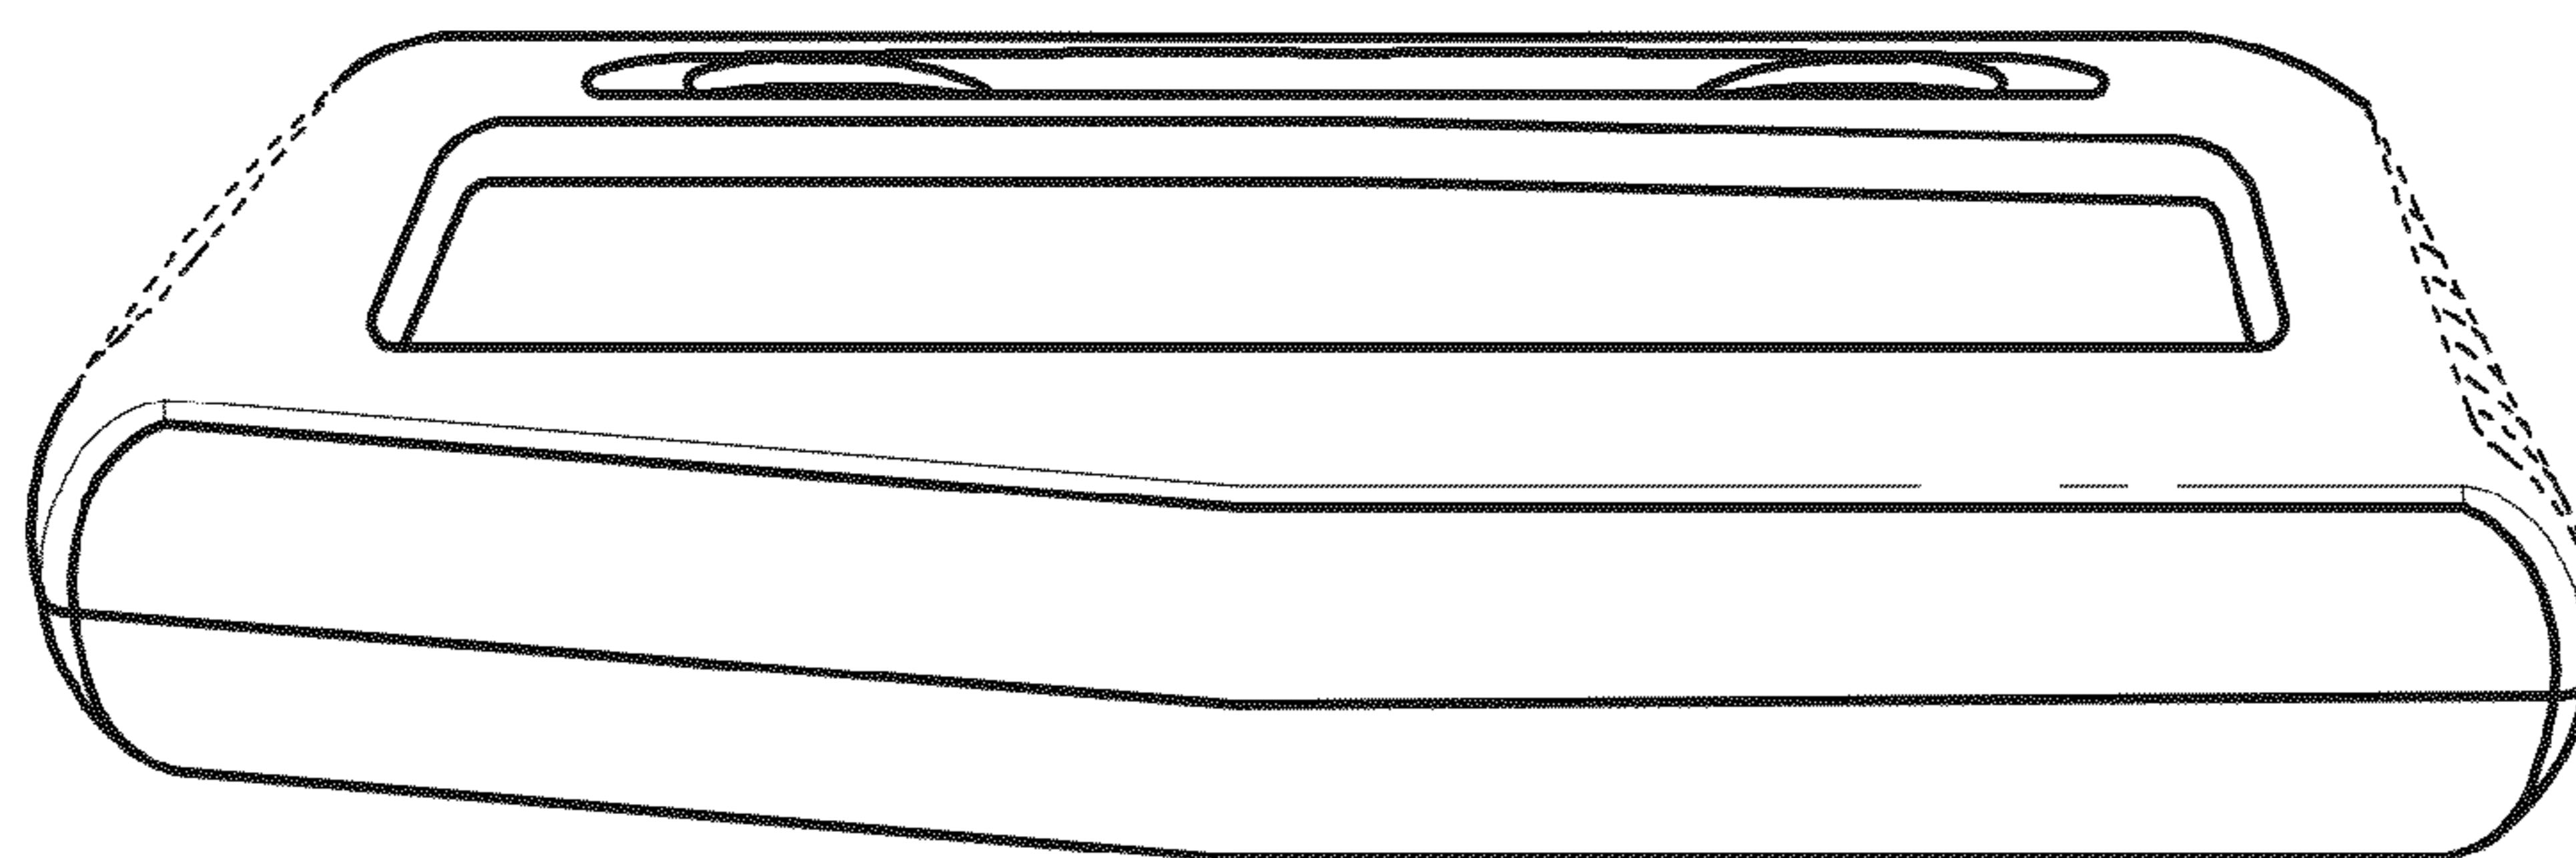


FIG. 3

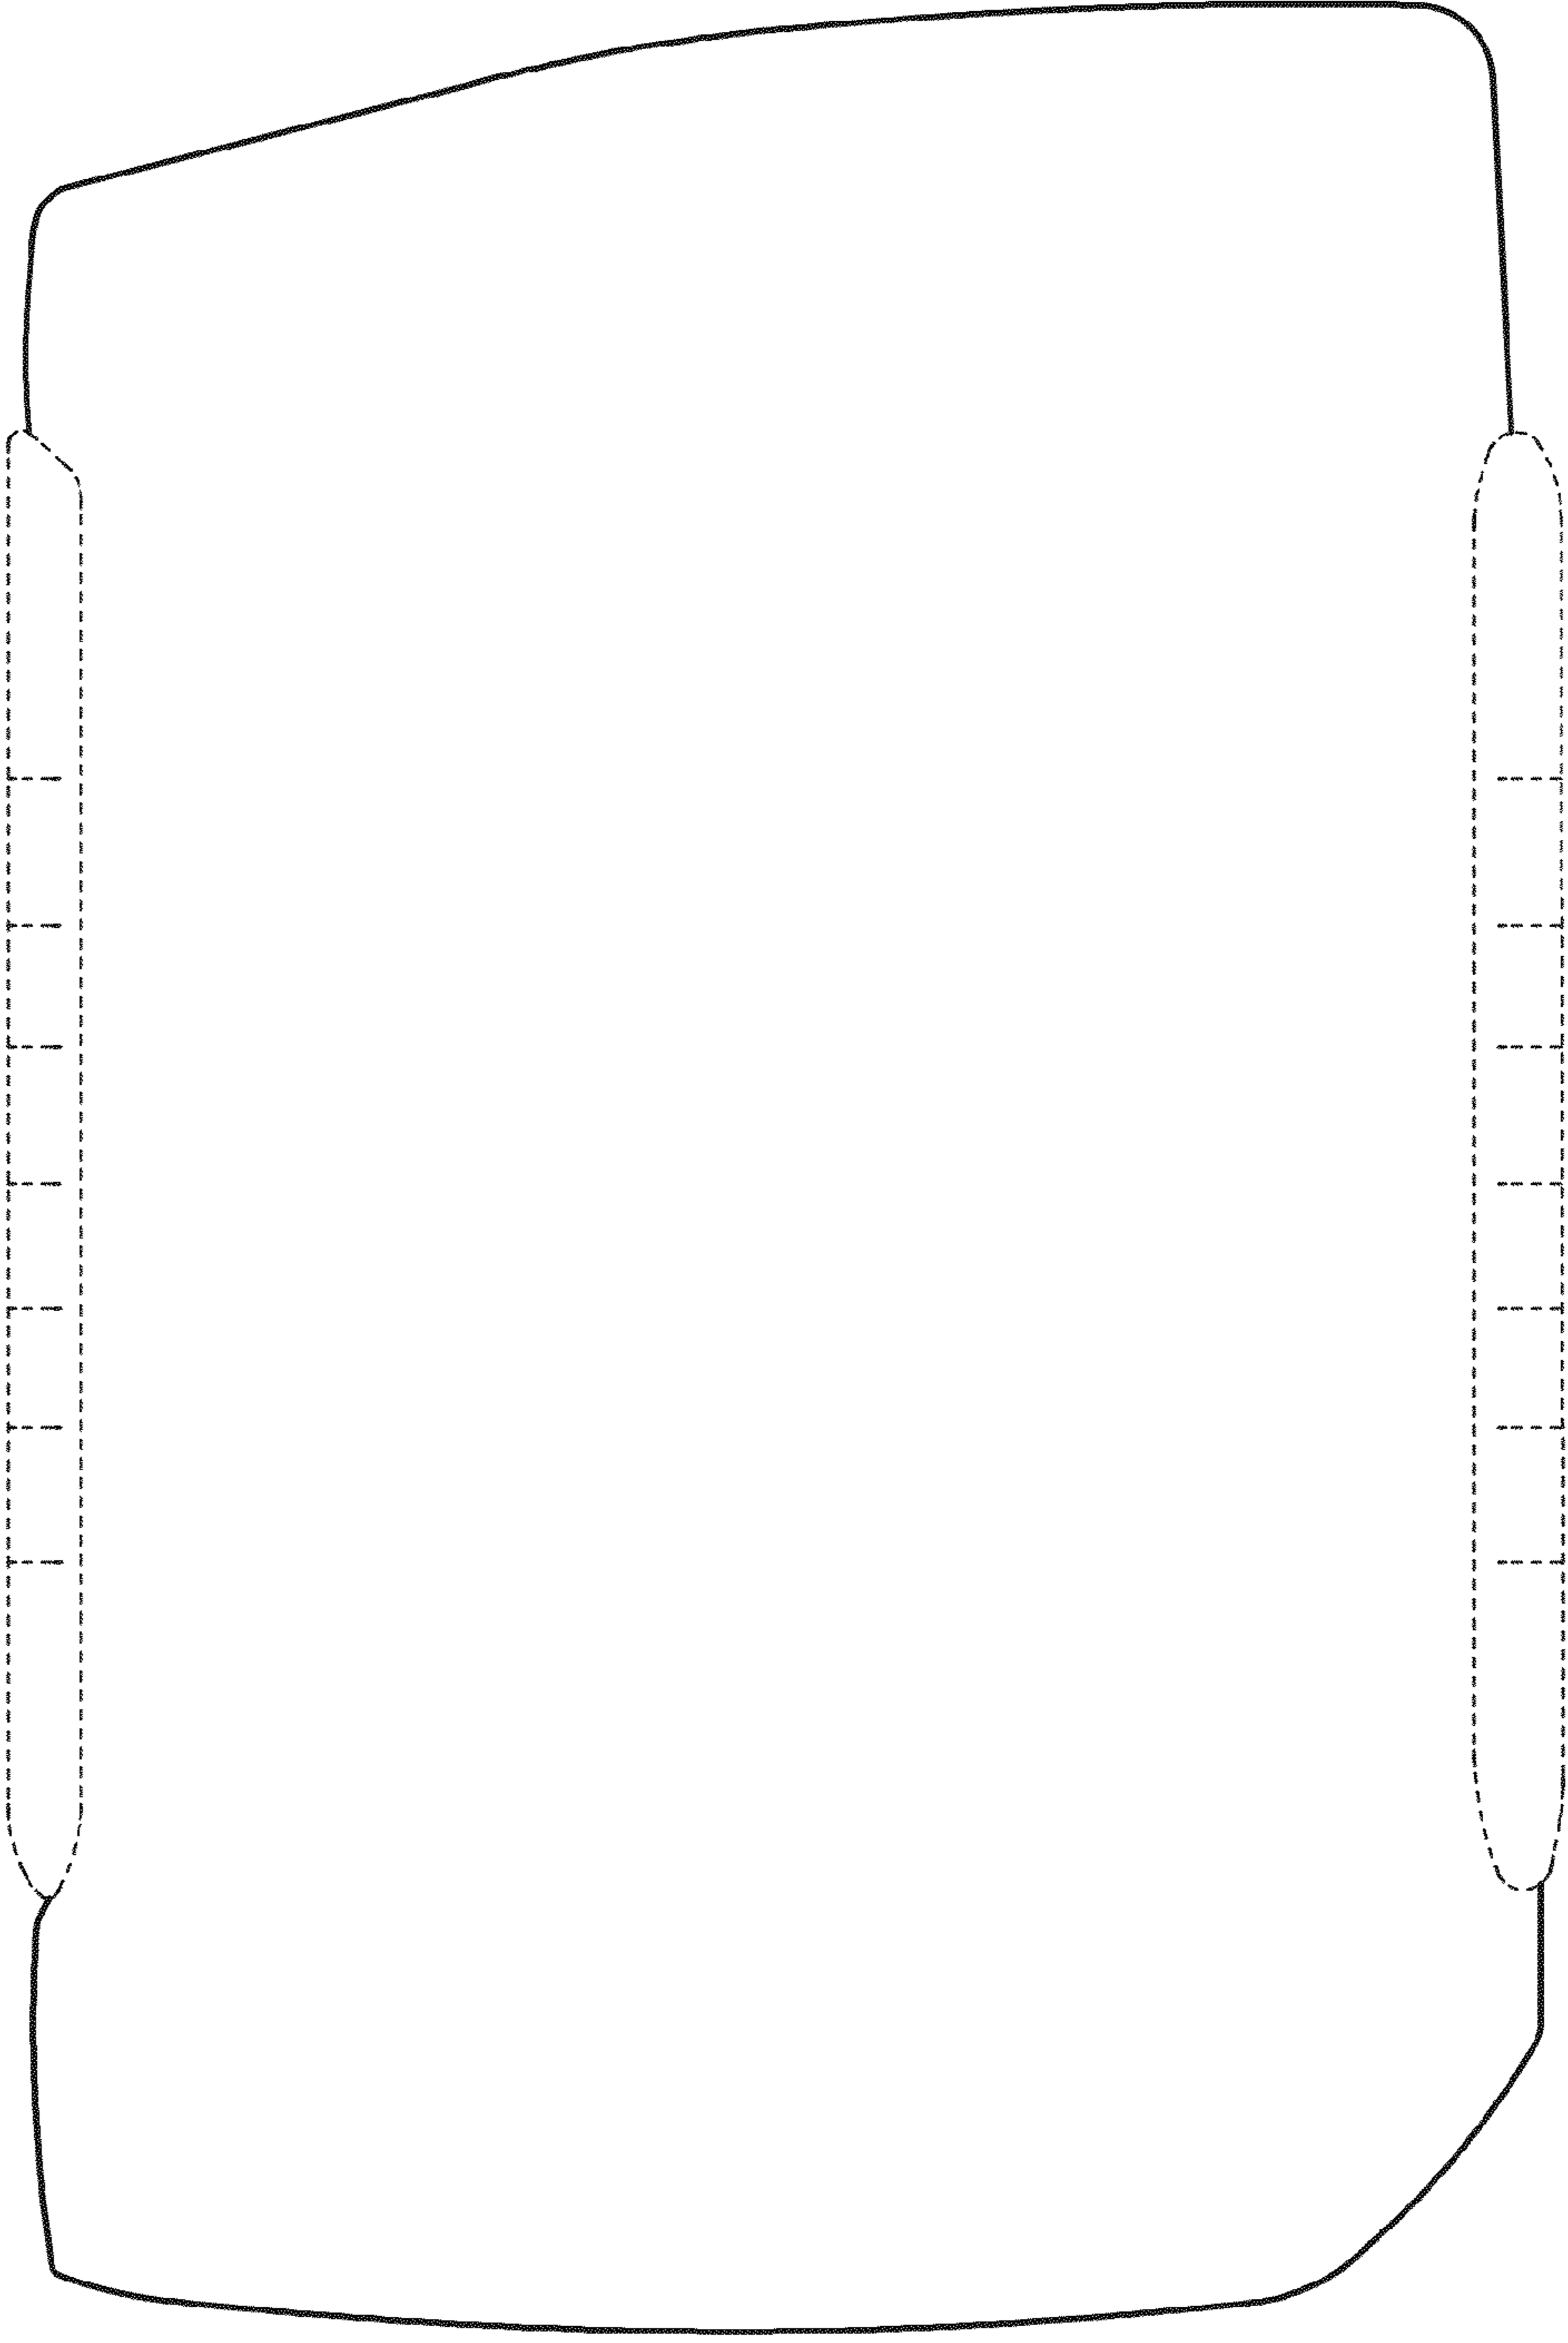


FIG. 4

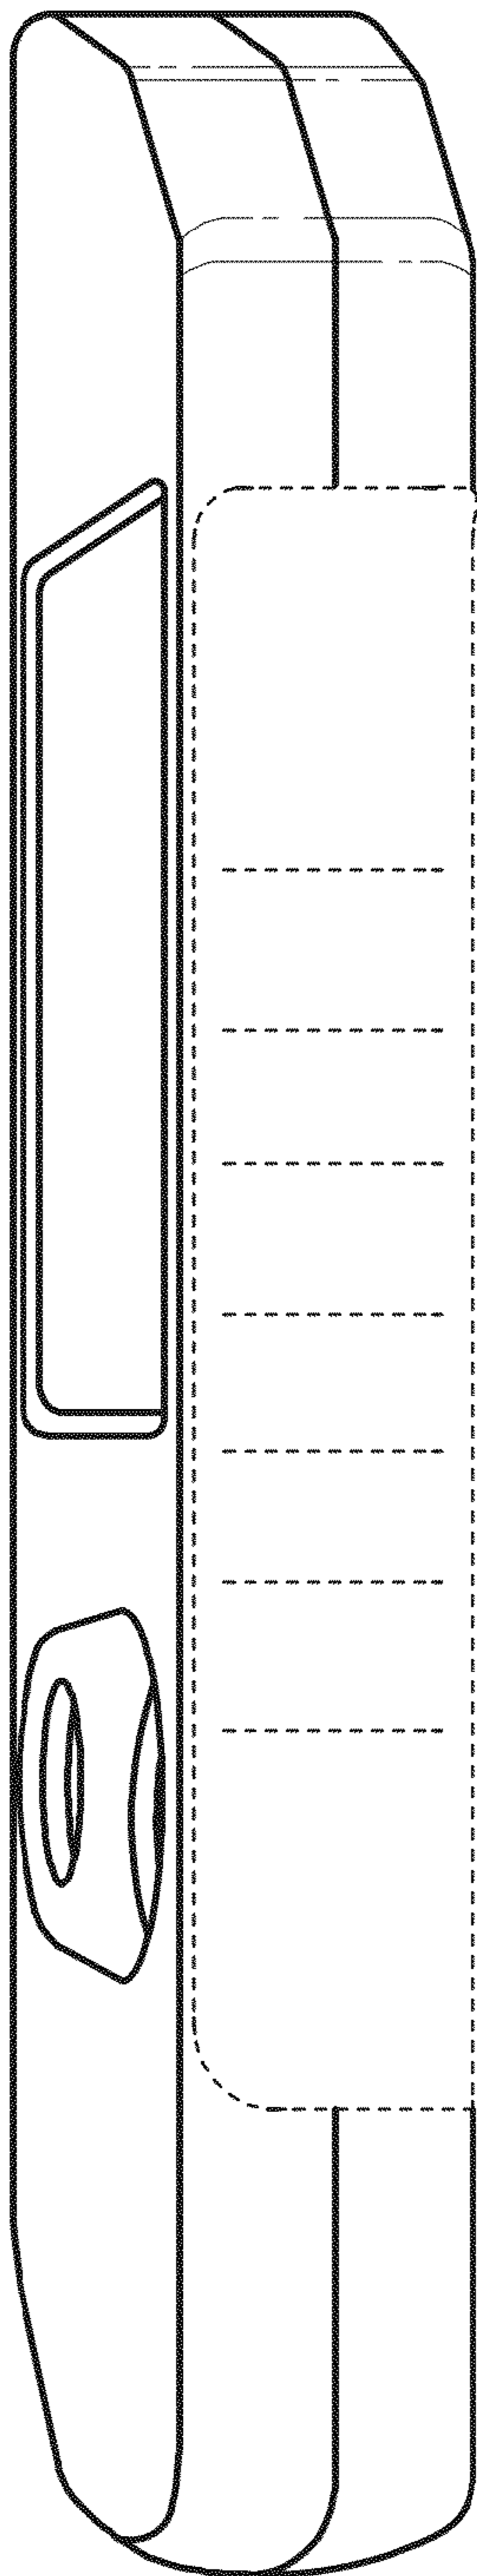


FIG. 5

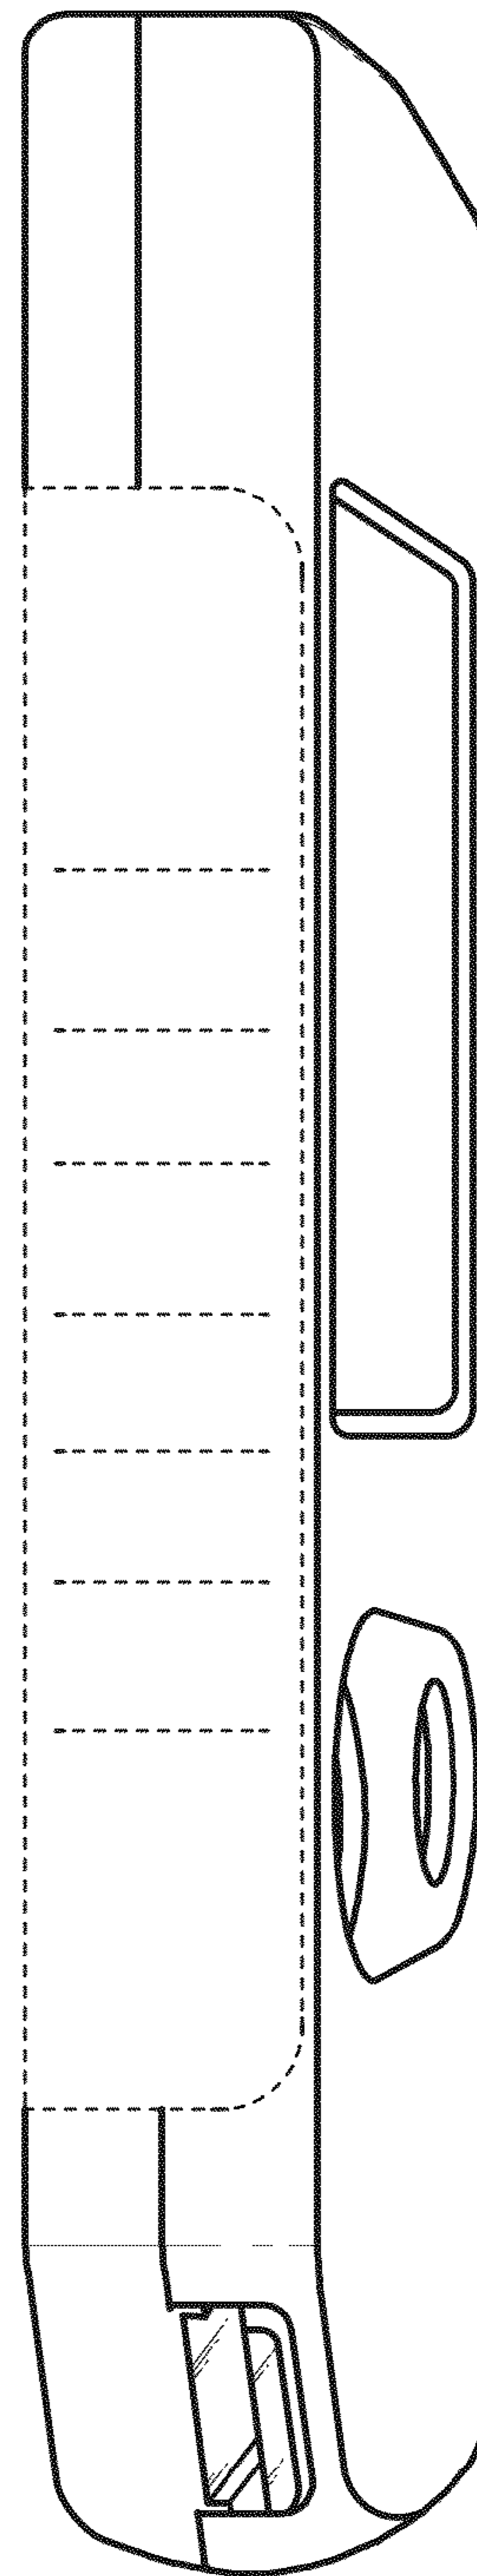


FIG. 6