



US00D689506S

(12) **United States Design Patent**  
**Yanagawa**

(10) **Patent No.:** **US D689,506 S**

(45) **Date of Patent:** **\*\* Sep. 10, 2013**

(54) **HIGH FREQUENCY THERAPY EQUIPMENT WITH GRAPHICAL USER INTERFACE**

(75) Inventor: **Kiwamu Yanagawa**, Tokyo (JP)

(73) Assignee: **Kabushiki Kaisha Top**, Tokyo (JP)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/391,554**

(22) Filed: **May 10, 2011**

(30) **Foreign Application Priority Data**

Nov. 11, 2010 (JP) ..... 2010-027180

(51) **LOC (9) Cl.** ..... **14-04**

(52) **U.S. Cl.**  
USPC ..... **D14/486**

(58) **Field of Classification Search**  
USPC ..... D14/485, 486, 487, 488, 489, 490,  
D14/491, 492, 493, 494, 495; 709/217, 218,  
709/219, 220, 223, 224; 715/205, 833, 834,  
715/835, 863, 865, 810; 68/139, 20  
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,456,682	A *	10/1995	Edwards et al.	.....	606/31
D376,207	S *	12/1996	Buczek et al.	.....	D24/172
D396,108	S *	7/1998	Garito et al.	.....	D24/144
D468,322	S *	1/2003	Walker et al.	.....	D14/486
D481,123	S *	10/2003	Hayamizu	.....	D24/138
D491,667	S *	6/2004	Kimmell et al.	.....	D24/170
D526,654	S *	8/2006	McDougall et al.	.....	D14/485
7,226,447	B2 *	6/2007	Uchida et al.	.....	606/34
D562,337	S *	2/2008	Keohane	.....	D14/487
D562,338	S *	2/2008	Keohane	.....	D14/487
D585,903	S *	2/2009	Yamaoka	.....	D14/485

D593,114	S *	5/2009	Vakkalanka	.....	D14/486
D593,117	S *	5/2009	Lettau	.....	D14/488
D599,905	S *	9/2009	Matsushita	.....	D24/138
D614,191	S *	4/2010	Takano et al.	.....	D14/486
D614,192	S *	4/2010	Takano et al.	.....	D14/486
D617,332	S *	6/2010	Loken et al.	.....	D14/485
D631,160	S *	1/2011	Schurg et al.	.....	D24/144
D632,698	S *	2/2011	Judy et al.	.....	D14/486
D648,342	S *	11/2011	Pearson et al.	.....	D14/486
D656,946	S *	4/2012	Judy et al.	.....	D14/486
D658,667	S *	5/2012	Cho et al.	.....	D14/486
D659,151	S *	5/2012	Loken et al.	.....	D14/485
D661,313	S *	6/2012	Nenoki	.....	D14/487
D670,386	S *	11/2012	Yanagawa	.....	D24/144
D679,284	S *	4/2013	Rounding et al.	.....	D14/486
2005/0165819	A1 *	7/2005	Kudoh et al.	.....	707/101

\* cited by examiner

*Primary Examiner* — Kevin Rudzinski


(74) *Attorney, Agent, or Firm* — Birch, Stewart, Kolasch & Birch, LLP

(57) **CLAIM**  
The ornamental design for an high frequency therapy equipment with graphical user interface, as shown and described.

**DESCRIPTION**

FIG. 1 is a front elevational view of a high frequency therapy equipment with graphical user interface showing my new design;  
FIG. 2 is a rear elevational view thereof;  
FIG. 3 is right side elevational view thereof;  
FIG. 4 is a left side elevational view thereof; and,  
FIG. 5 is a top plan view thereof.  
The bottom surface forms no part of the claimed design.  
The portions shown in broken lines form no part of the claimed design.

**1 Claim, 3 Drawing Sheets**

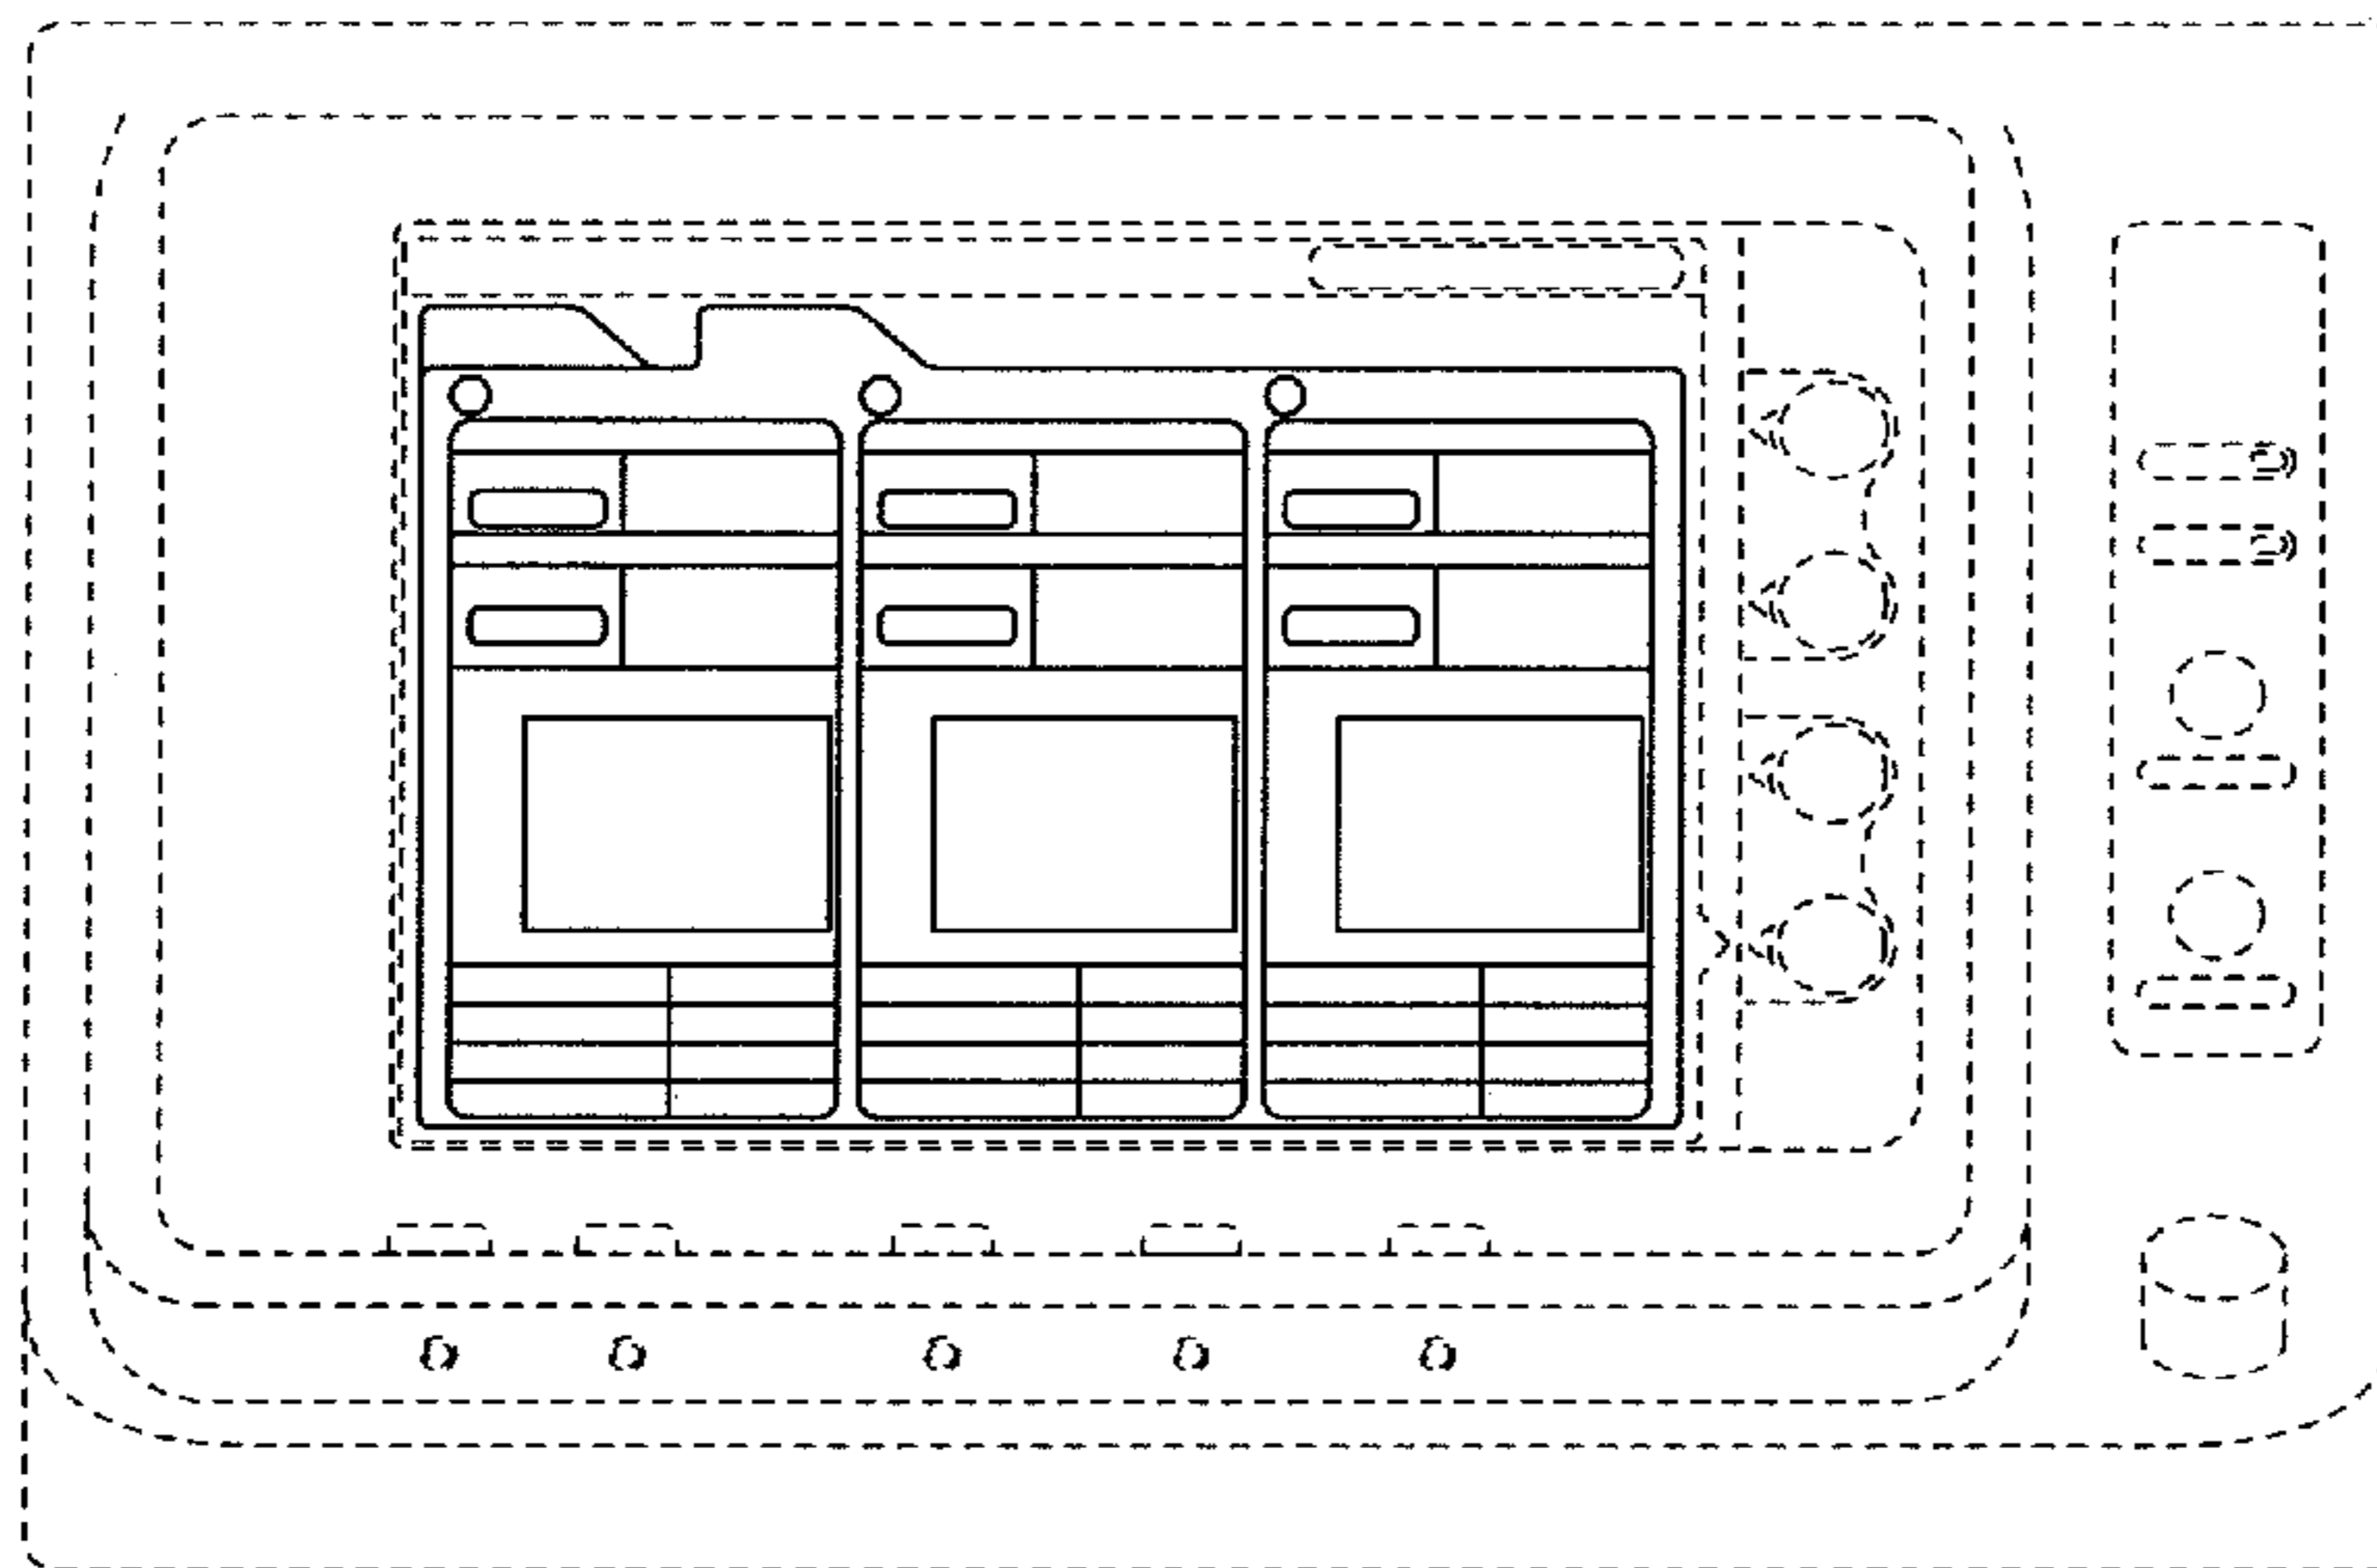

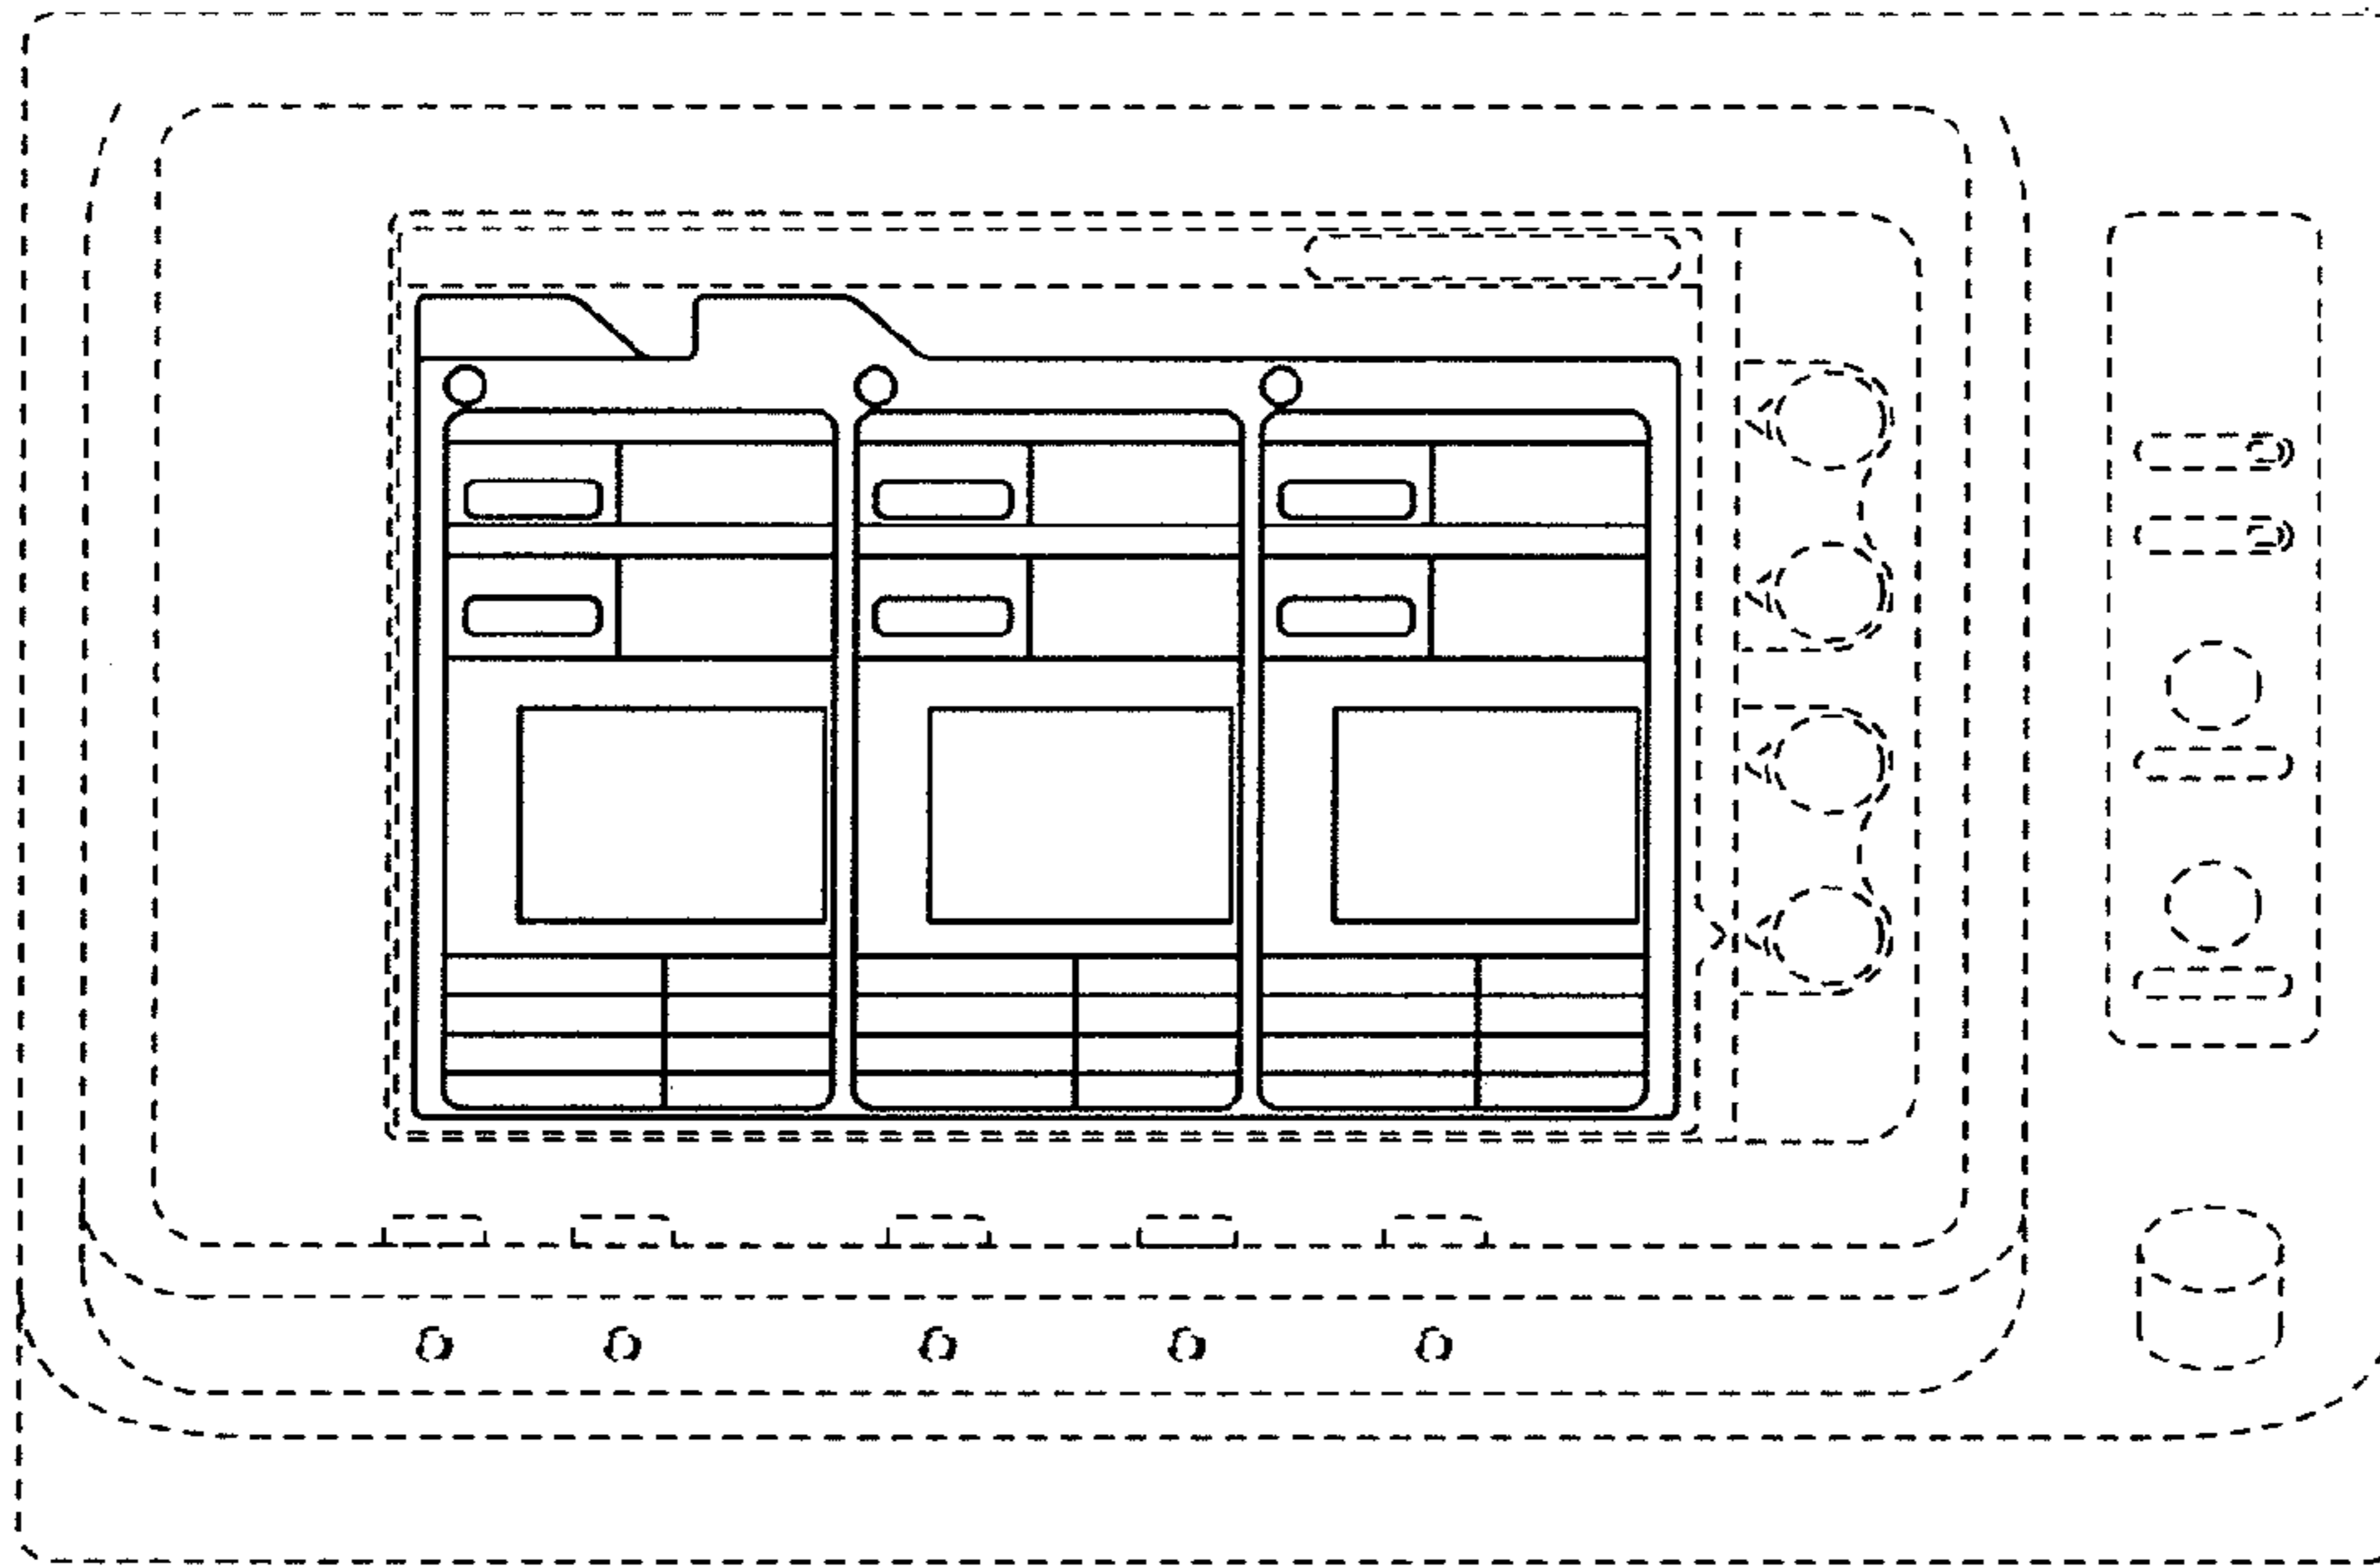


FIG. 1

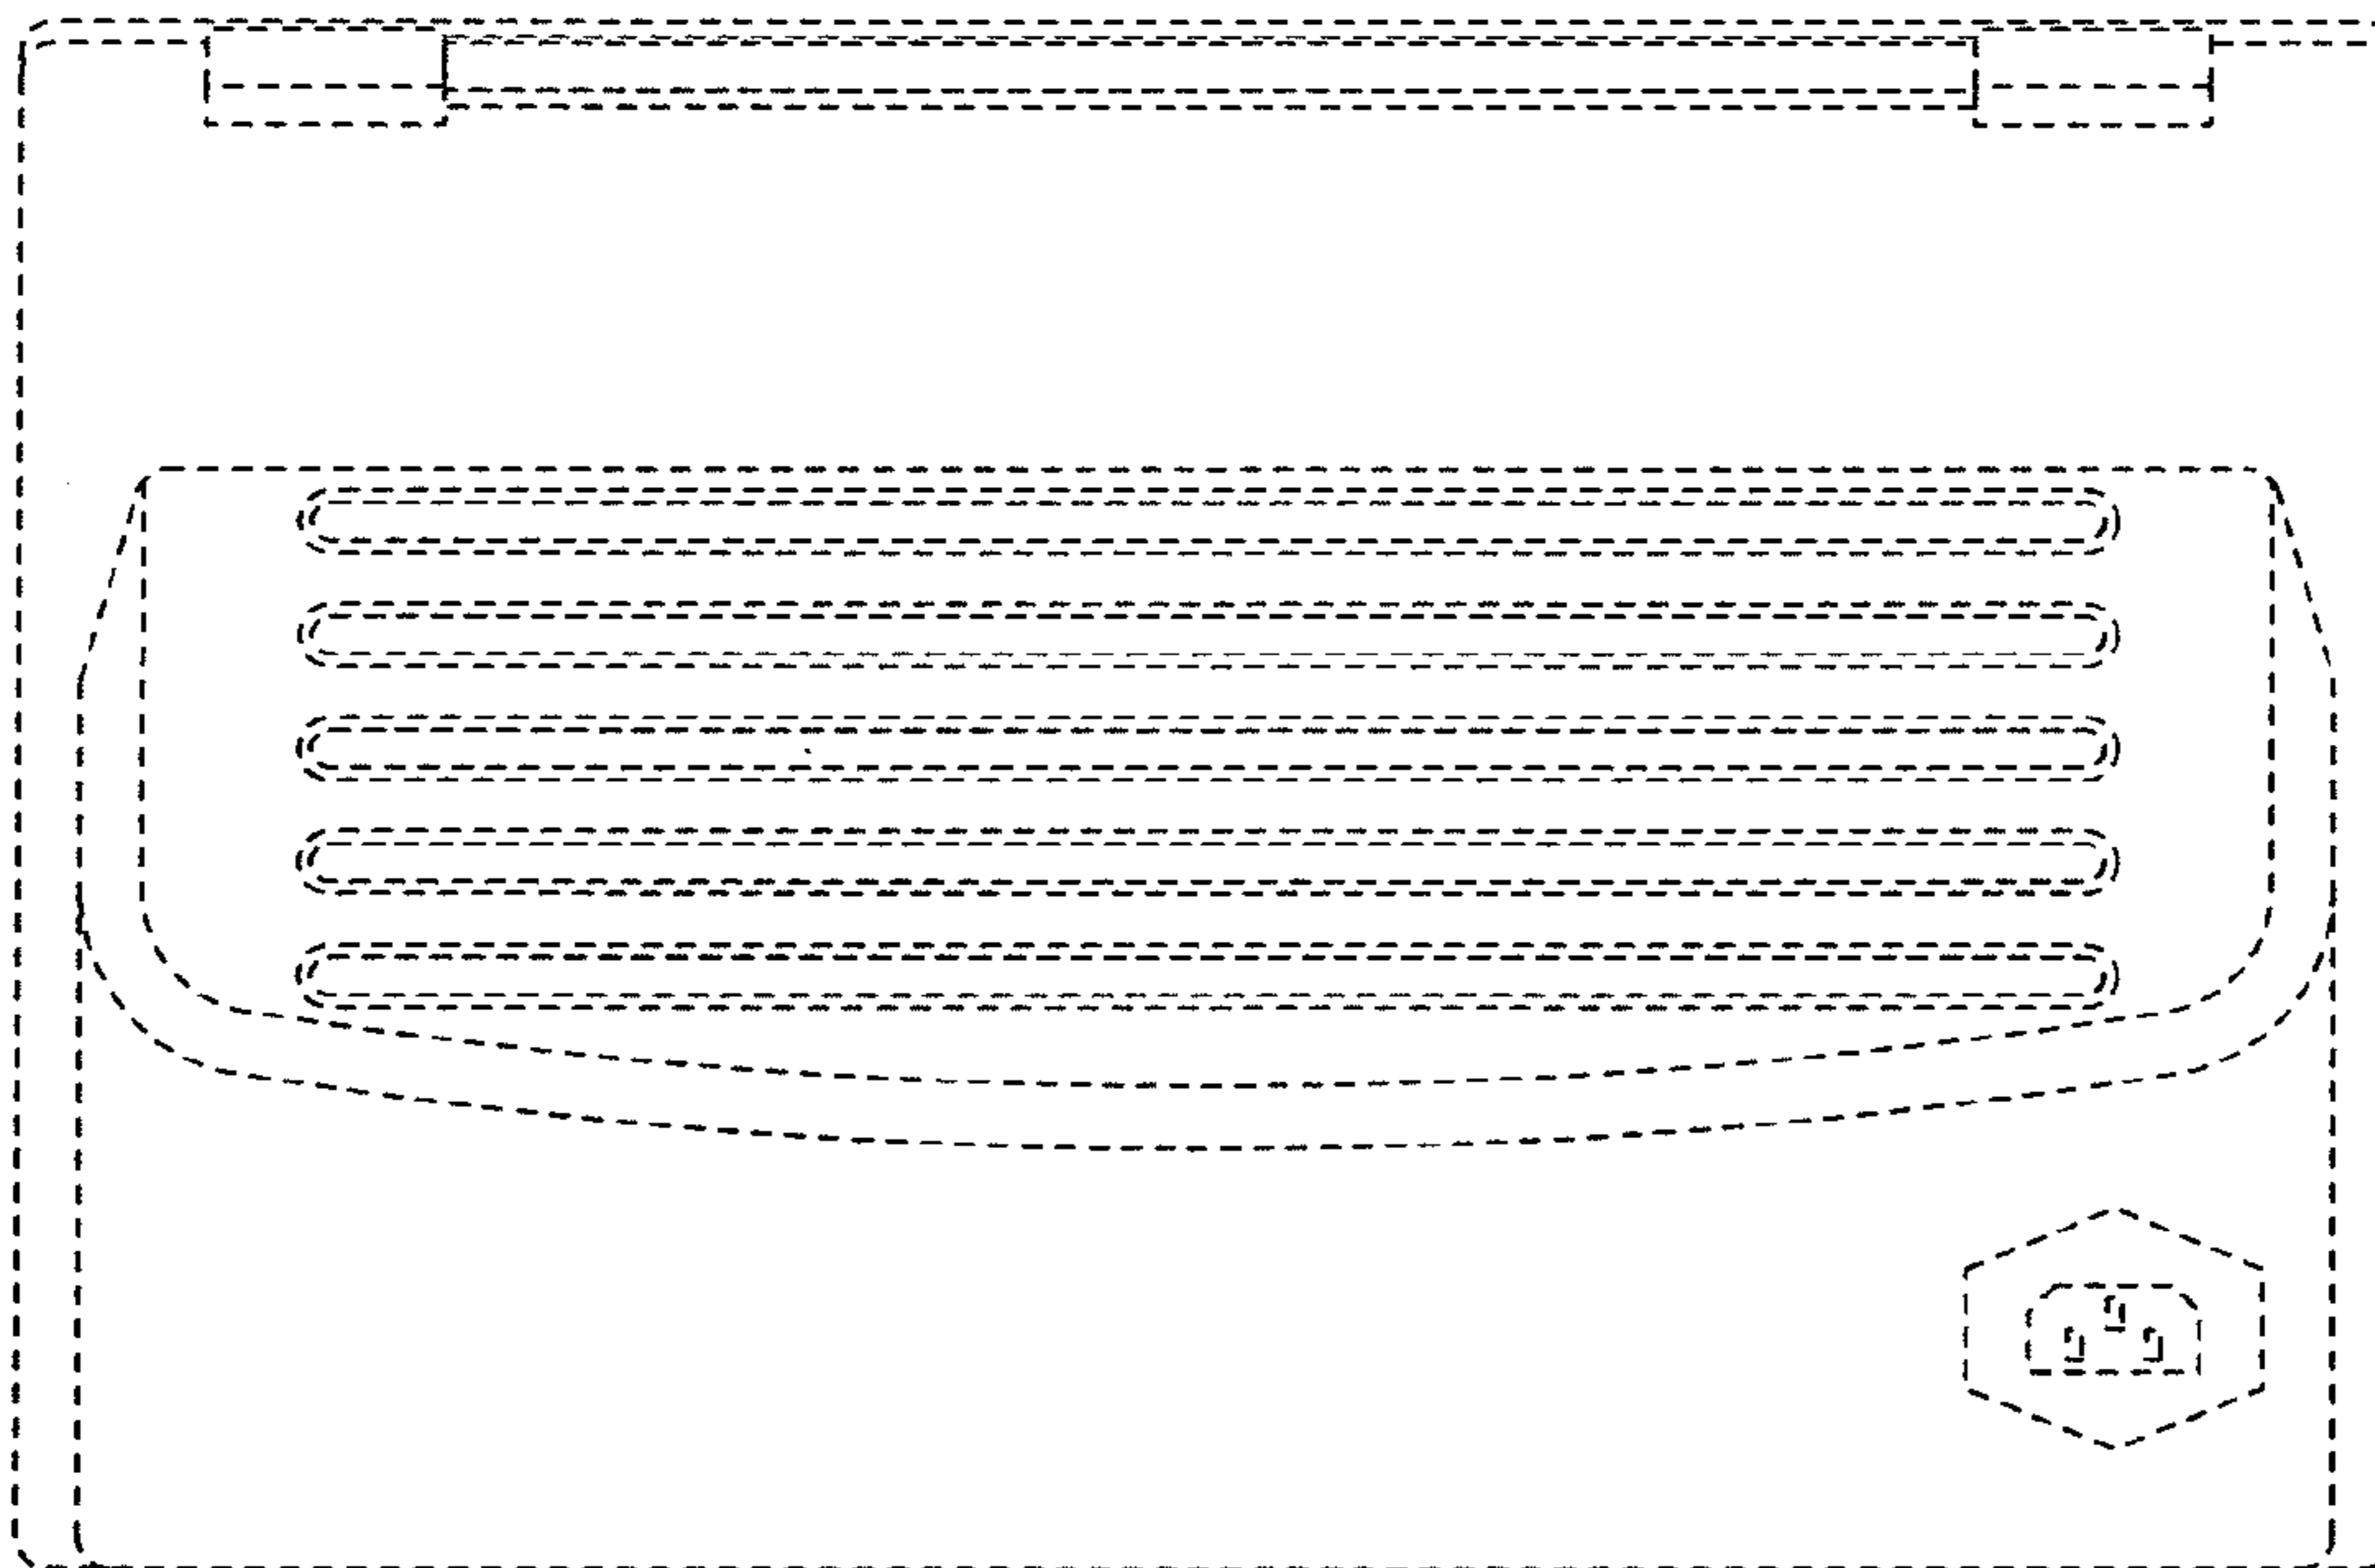
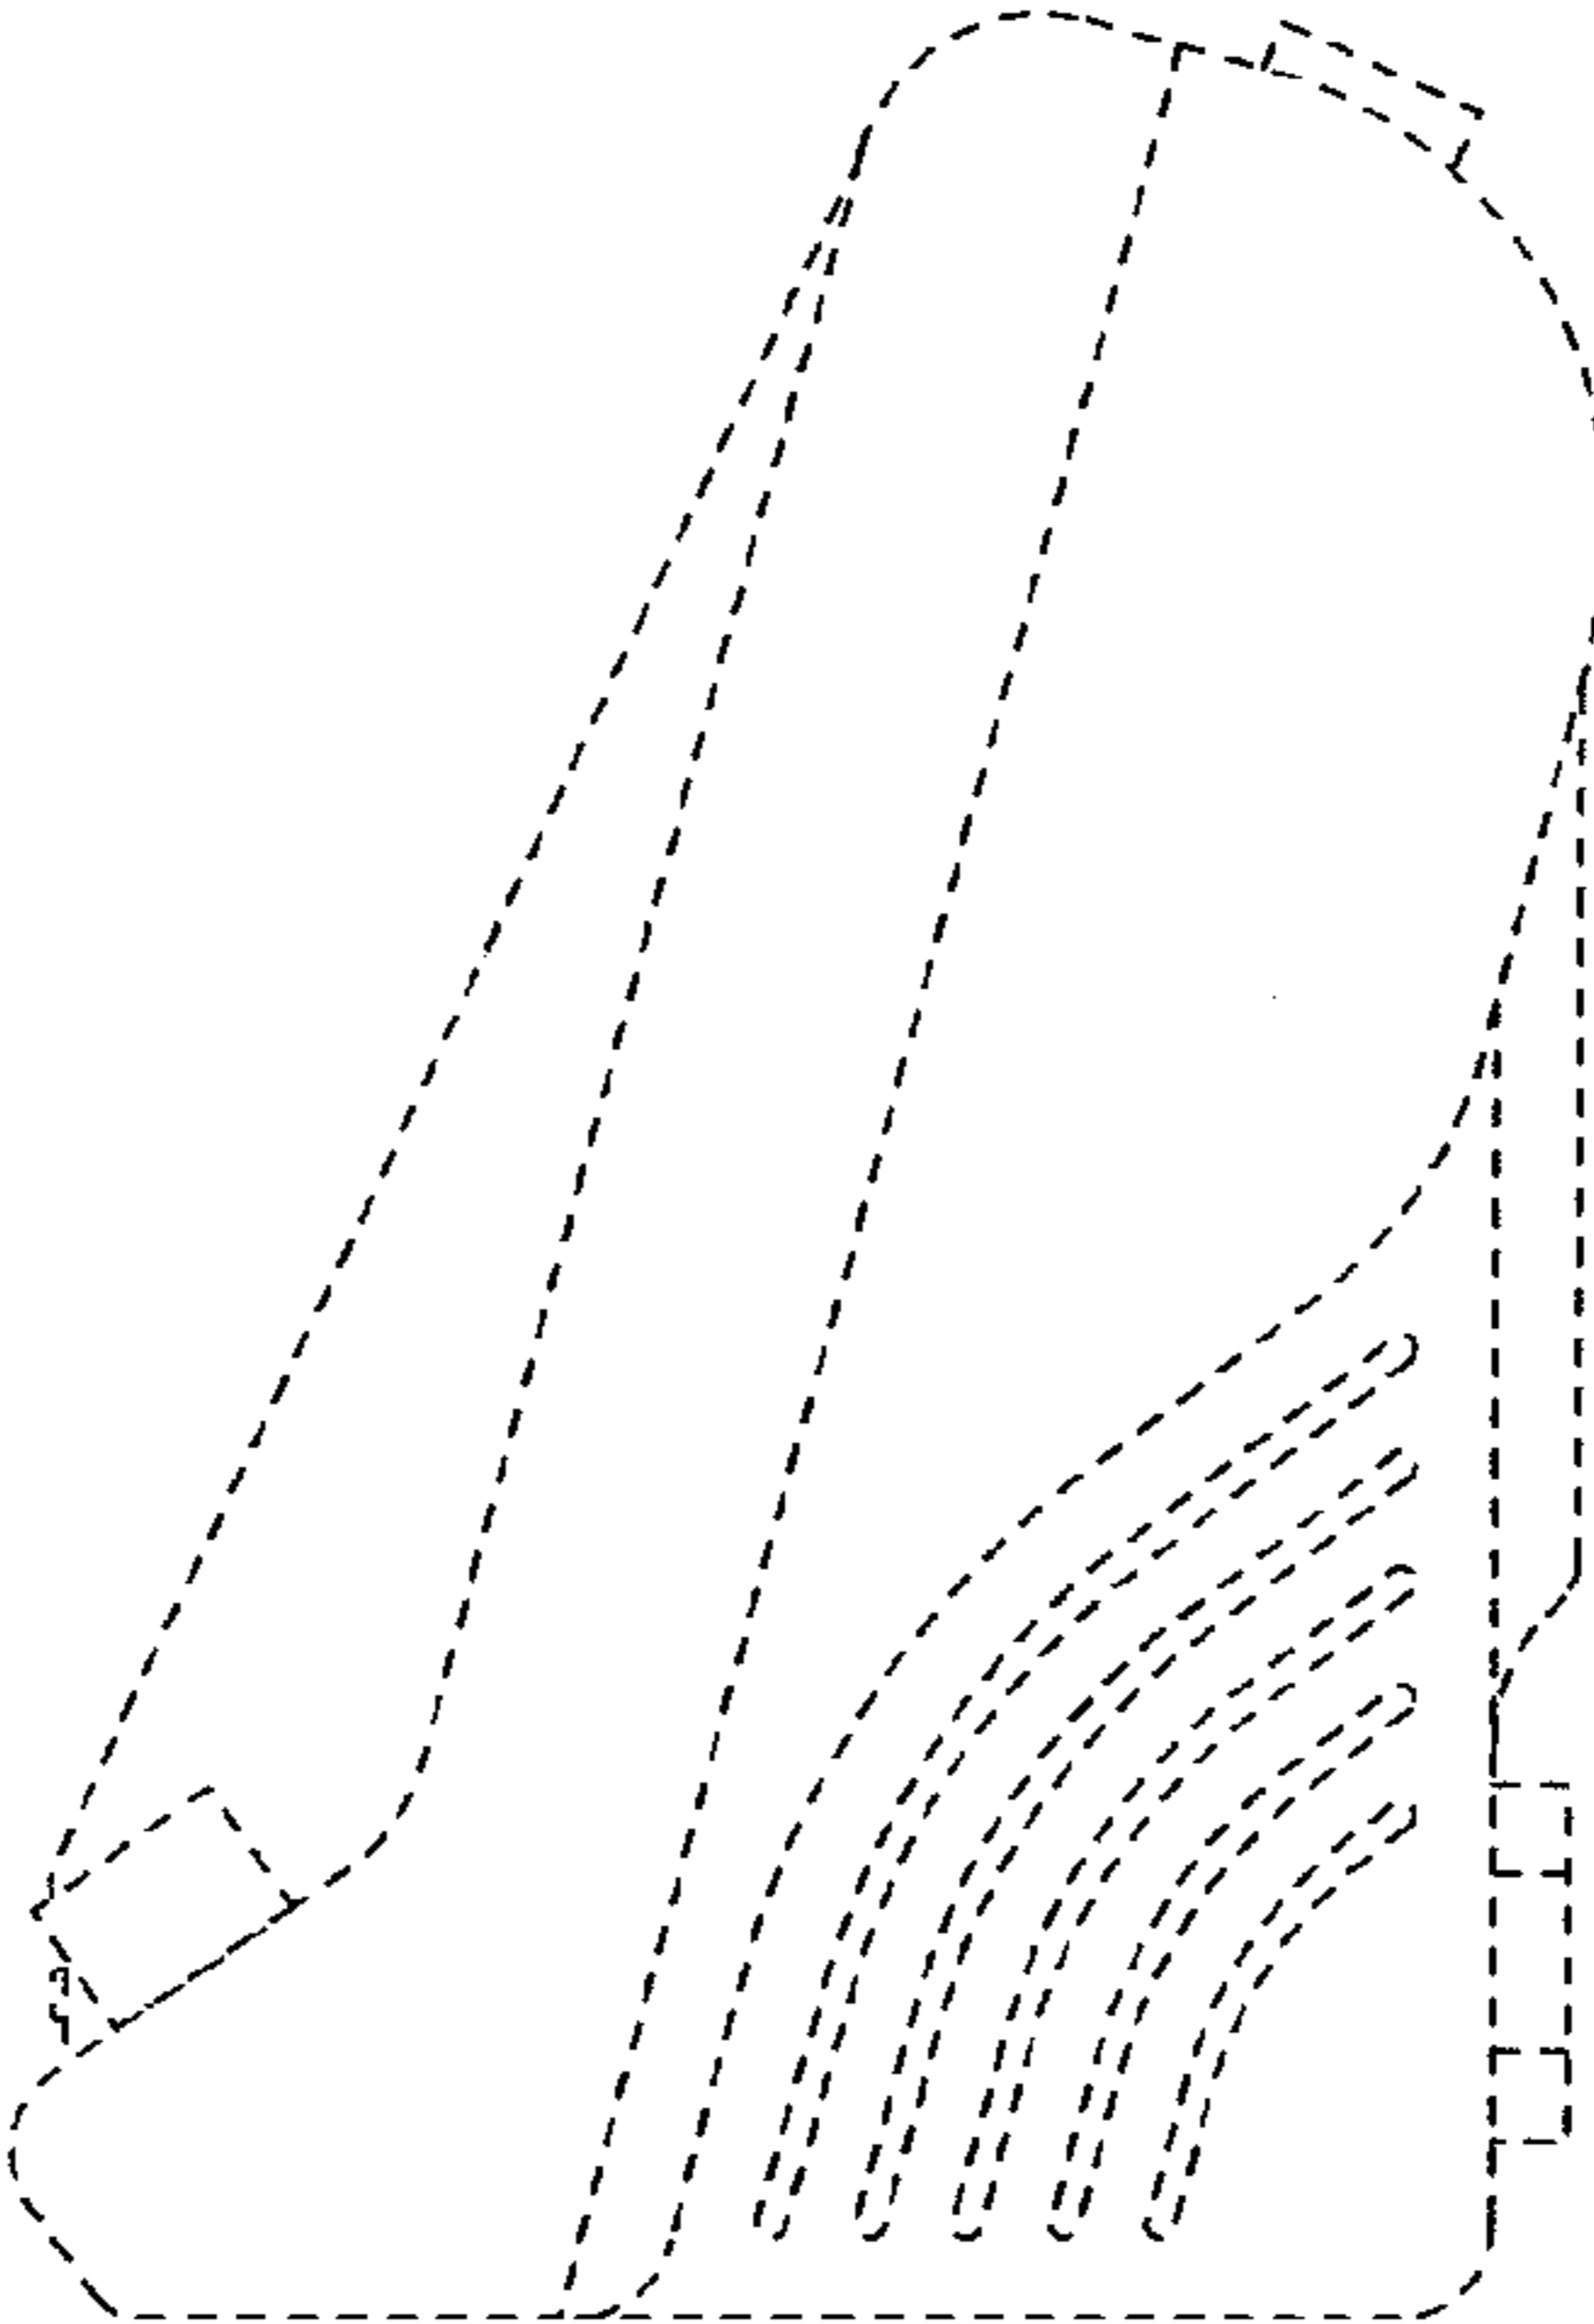
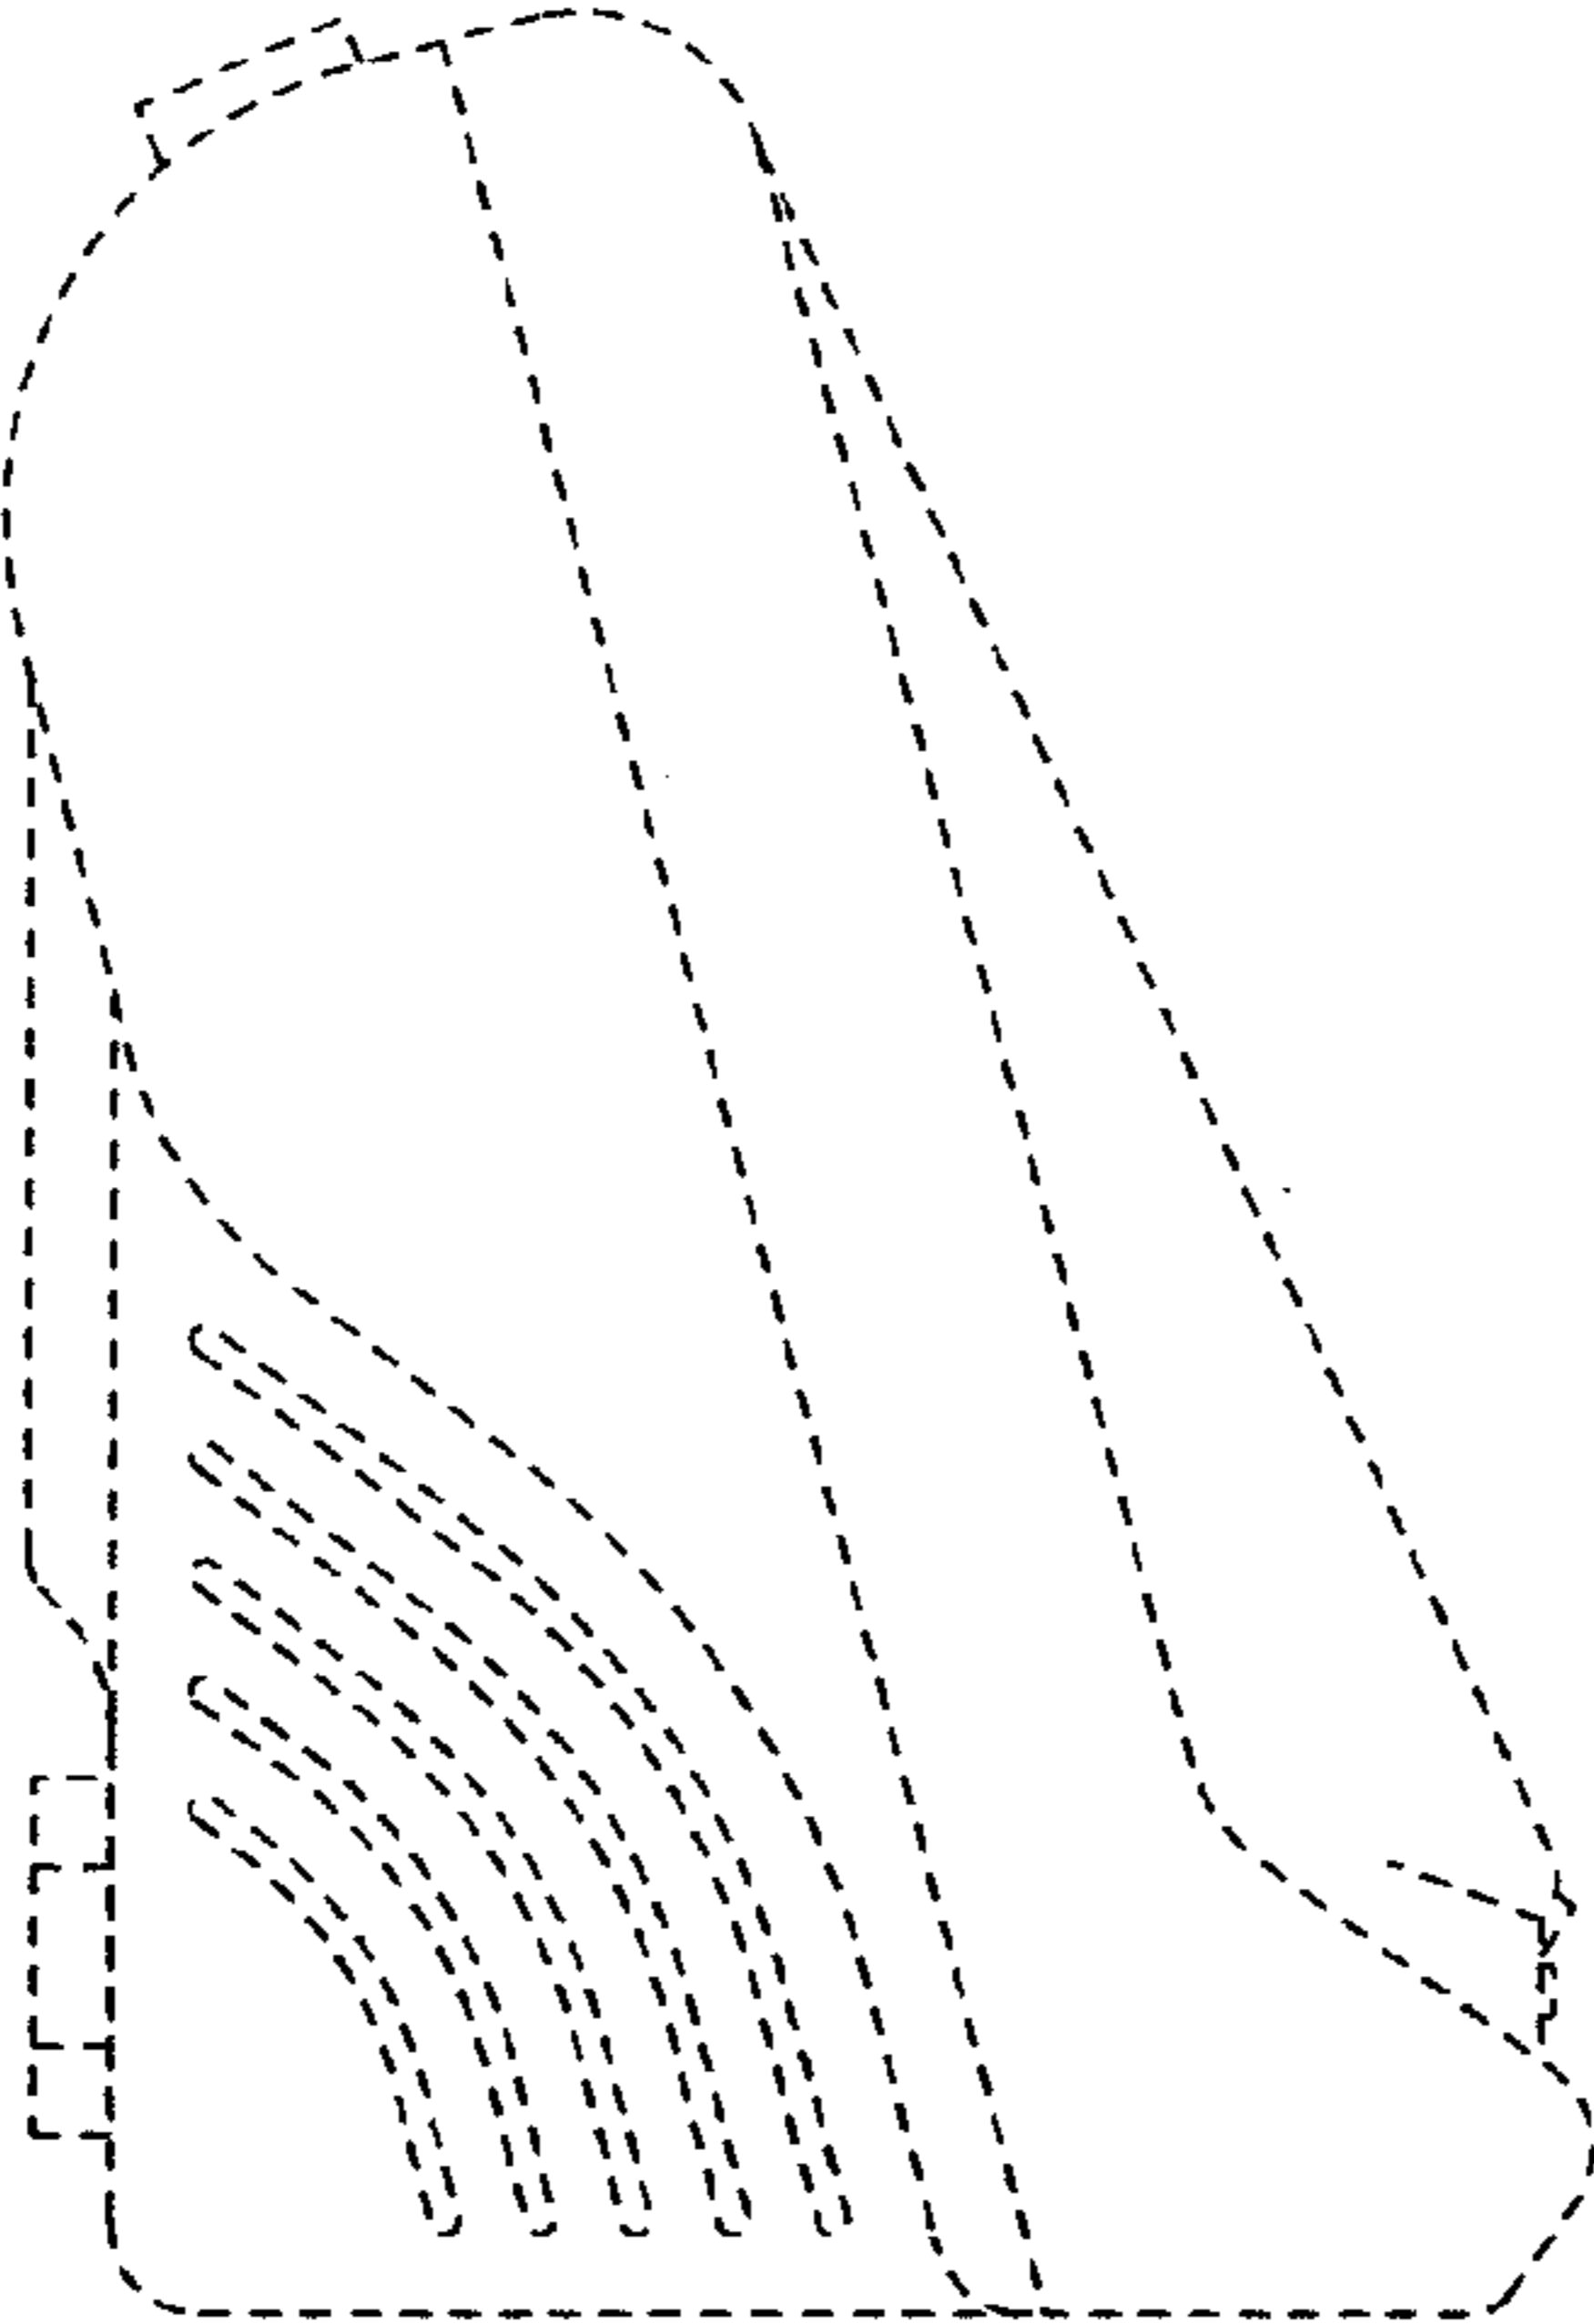


FIG. 2



**FIG. 3**



**FIG. 4**

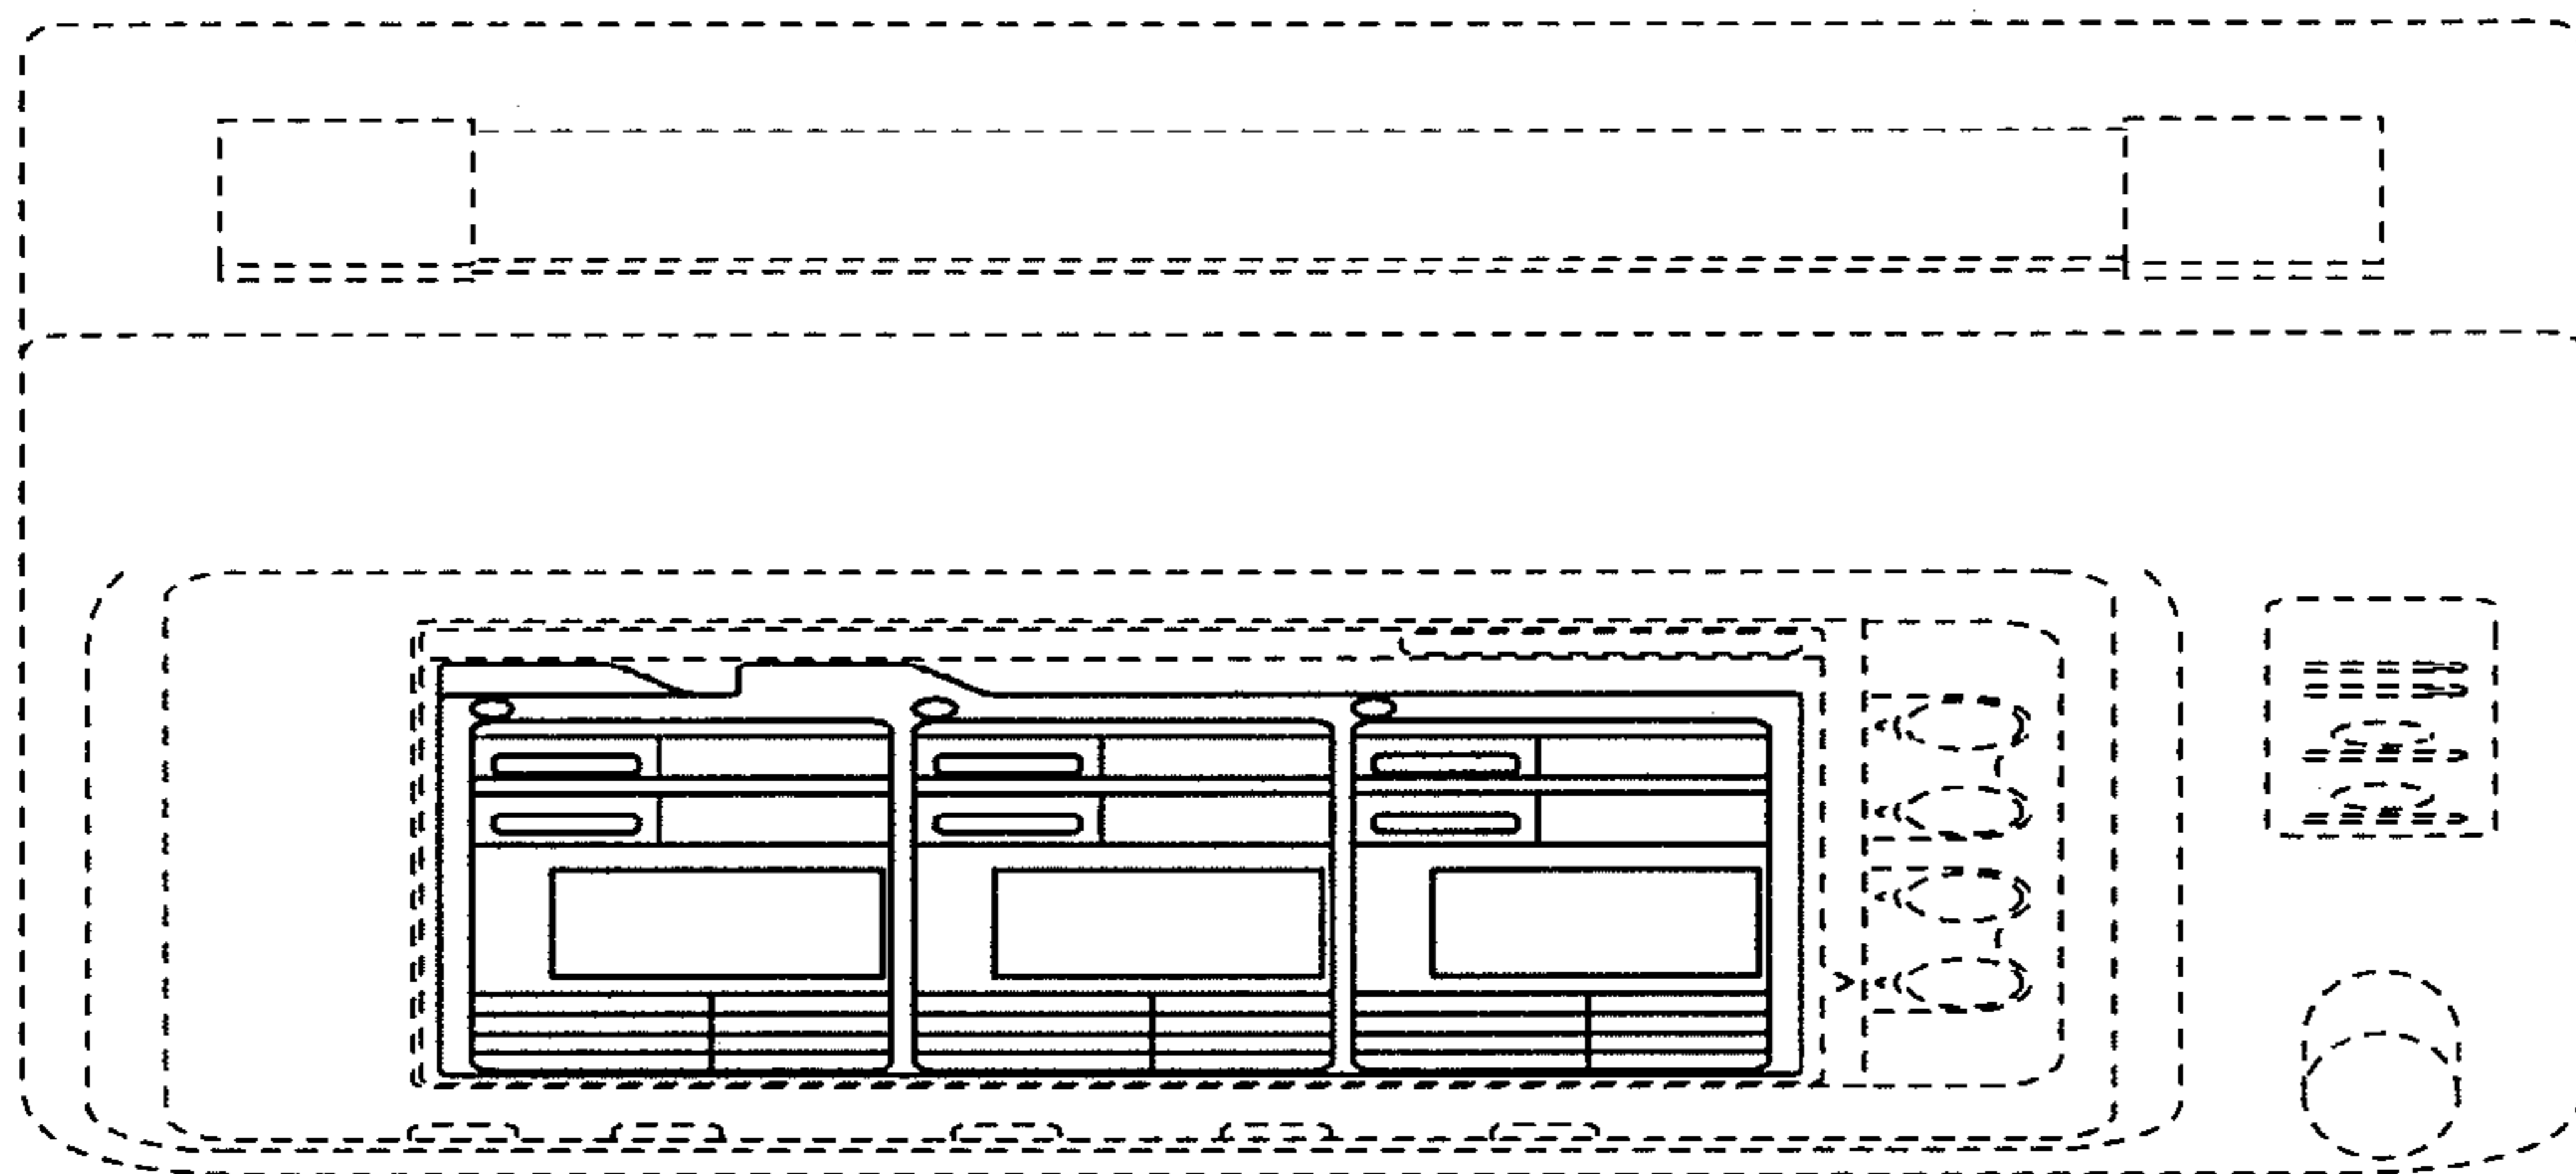


FIG. 5