



US00D689621S

(12) **United States Design Patent**  
**Morrow et al.**(10) **Patent No.:** **US D689,621 S**  
(45) **Date of Patent:** **\*\* Sep. 10, 2013**(54) **LABORATORY INSTRUMENT HOUSING**(75) Inventors: **James D. Morrow**, Oak Park, IL (US);  
**Bruce R. Boeke**, Ames, IA (US)(73) Assignee: **Advanced Analytical Technologies,  
Inc.**, Ames, IA (US)(\*\*) Term: **14 Years**(21) Appl. No.: **29/421,549**(22) Filed: **Mar. 15, 2012****Related U.S. Application Data**(63) Continuation-in-part of application No. 29/389,556,  
filed on Apr. 13, 2011, now abandoned.(51) **LOC (9) Cl.** ..... **24-02**(52) **U.S. Cl.**USPC ..... **D24/232**(58) **Field of Classification Search**USPC ..... D24/231–232, 185–186, 216, 229;  
D10/81; D6/436, 445–446, 510; 422/62,  
422/65–66, 63, 80–81, 89

See application file for complete search history.

(56) **References Cited****U.S. PATENT DOCUMENTS**

D207,537	S	5/1967	Parks
D207,582	S	5/1967	Perrine
D215,275	S	9/1969	Oye
D233,511	S	11/1974	Condon et al.
D319,102	S	* 8/1991	Futatsuka et al. .... D24/232
D347,478	S	5/1994	Pinkney
D368,143	S	* 3/1996	Willows et al. .... D24/232

D421,653	S	3/2000	Purcell
D454,399	S	3/2002	Doms et al.
D542,931	S	* 5/2007	Pukall et al. .... D24/232
D571,480	S	6/2008	Beck et al.
7,834,278	B1	11/2010	Zeiss et al.
D634,442	S	3/2011	Tajima et al.
D652,947	S	* 1/2012	Philipak et al. .... D24/216
D670,401	S	* 11/2012	Tsuda et al. .... D24/216

\* cited by examiner

*Primary Examiner* — Wan Laymon(74) *Attorney, Agent, or Firm* — McKee, Voorhees & Sease,  
P.L.C.**(57) CLAIM**We claim the ornamental design for a laboratory instrument  
housing, as shown and described.**DESCRIPTION**FIG. 1 is a left-front perspective view of a laboratory instru-  
ment housing.

FIG. 2 is a right-front perspective view.

FIG. 3 is a front view.

FIG. 4 is a back view.

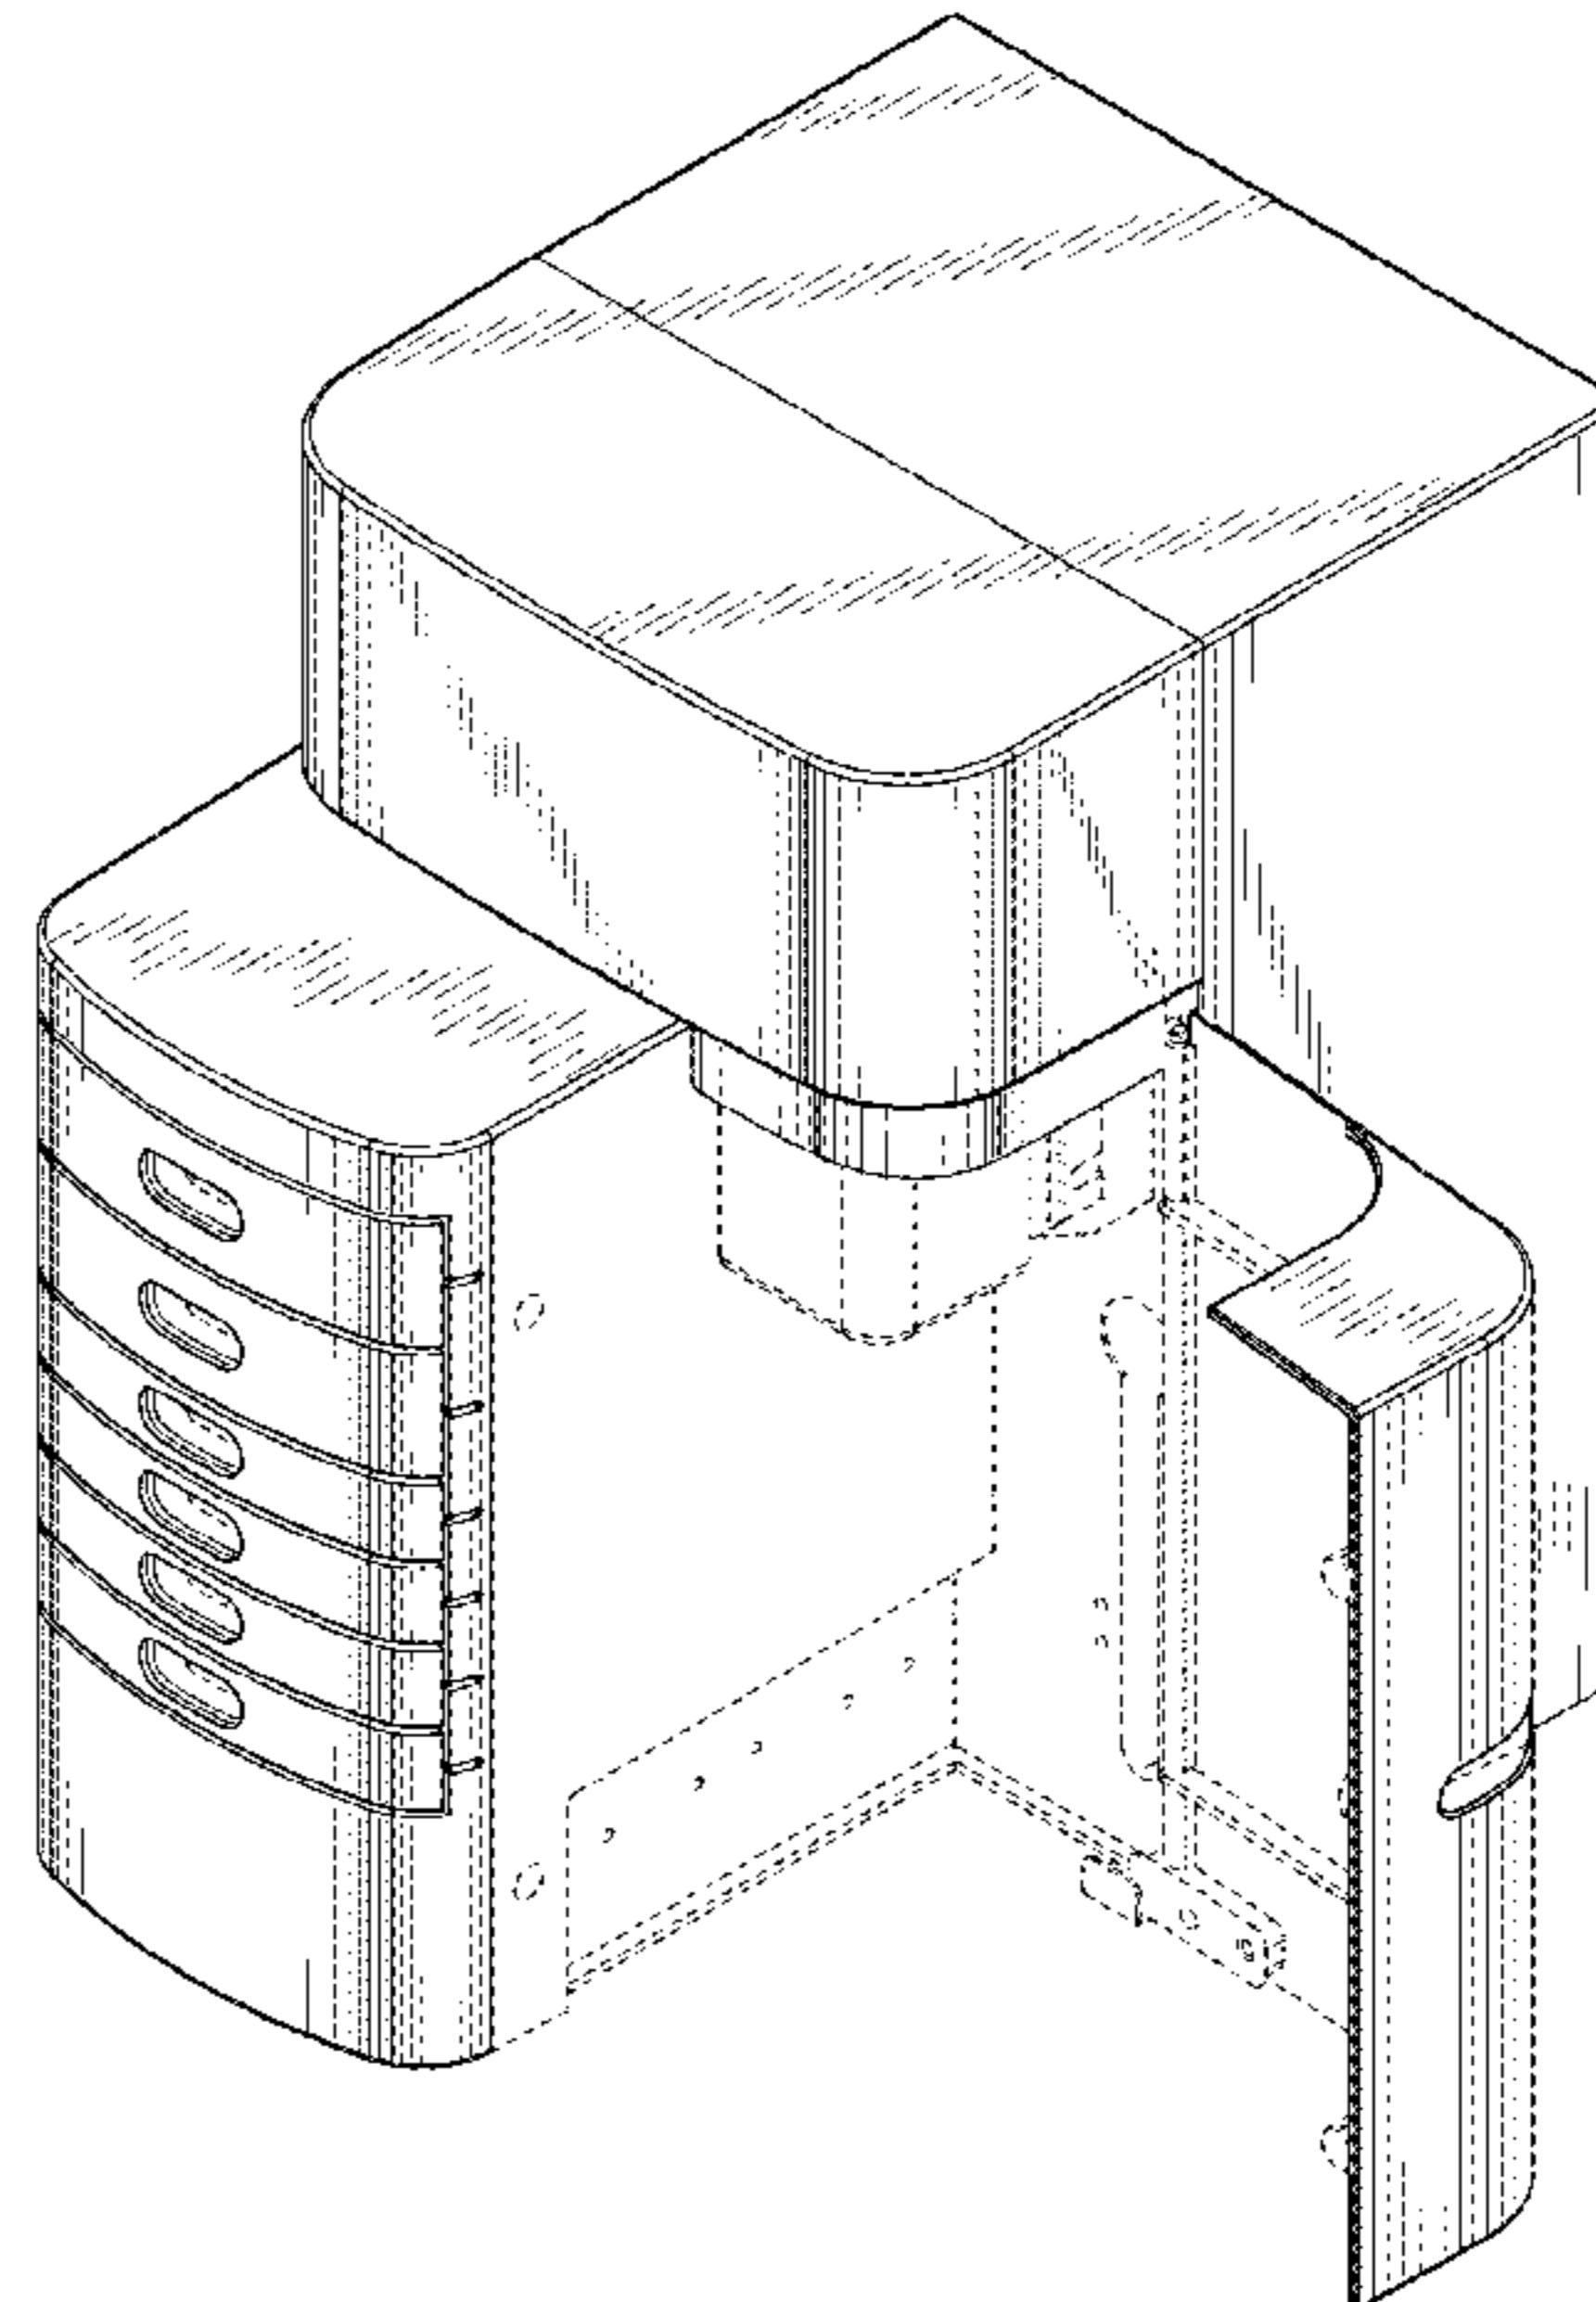
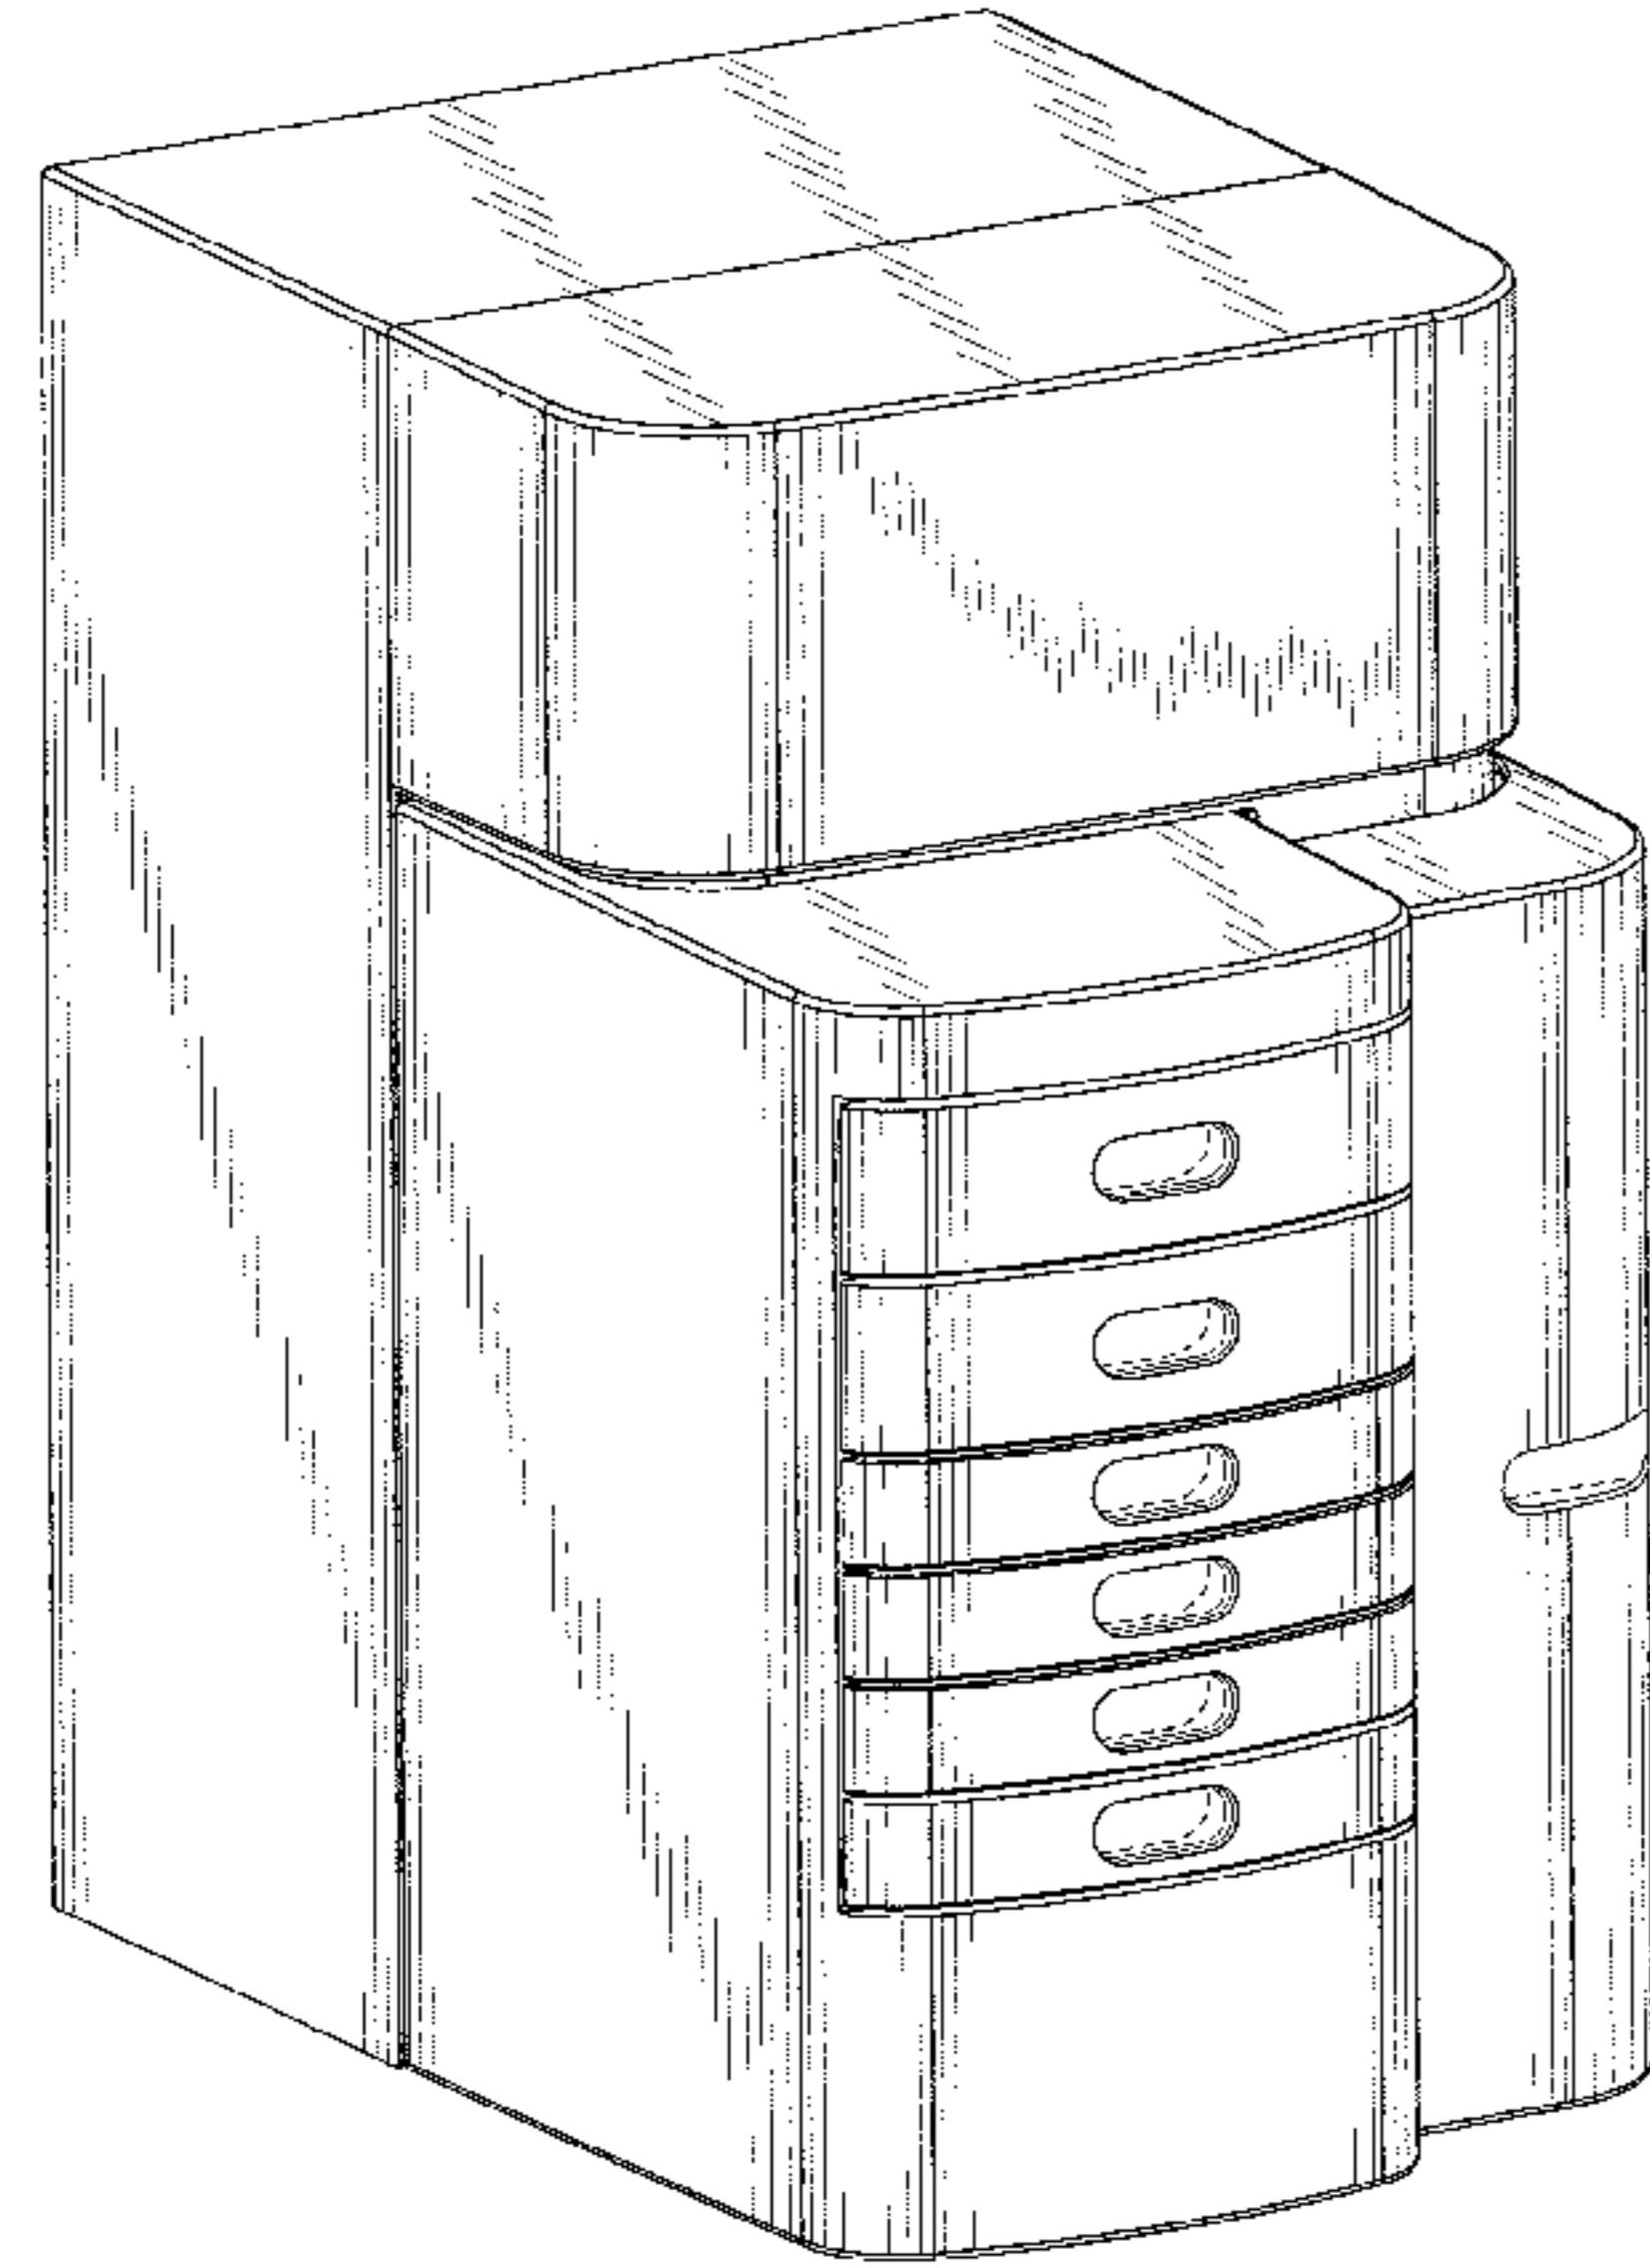
FIG. 5 is a left side view


FIG. 6 is a right side view.

FIG. 7 is a bottom view.


FIG. 8 is a right perspective view with a drawer in an open  
position.FIG. 9 is a left perspective view with the door shown in the  
open position; and,

FIG. 10 is a top view.


The broken lines shown in the figures represent portions of  
the laboratory instrument housing that form no part of the  
claimed design.**1 Claim, 10 Drawing Sheets**

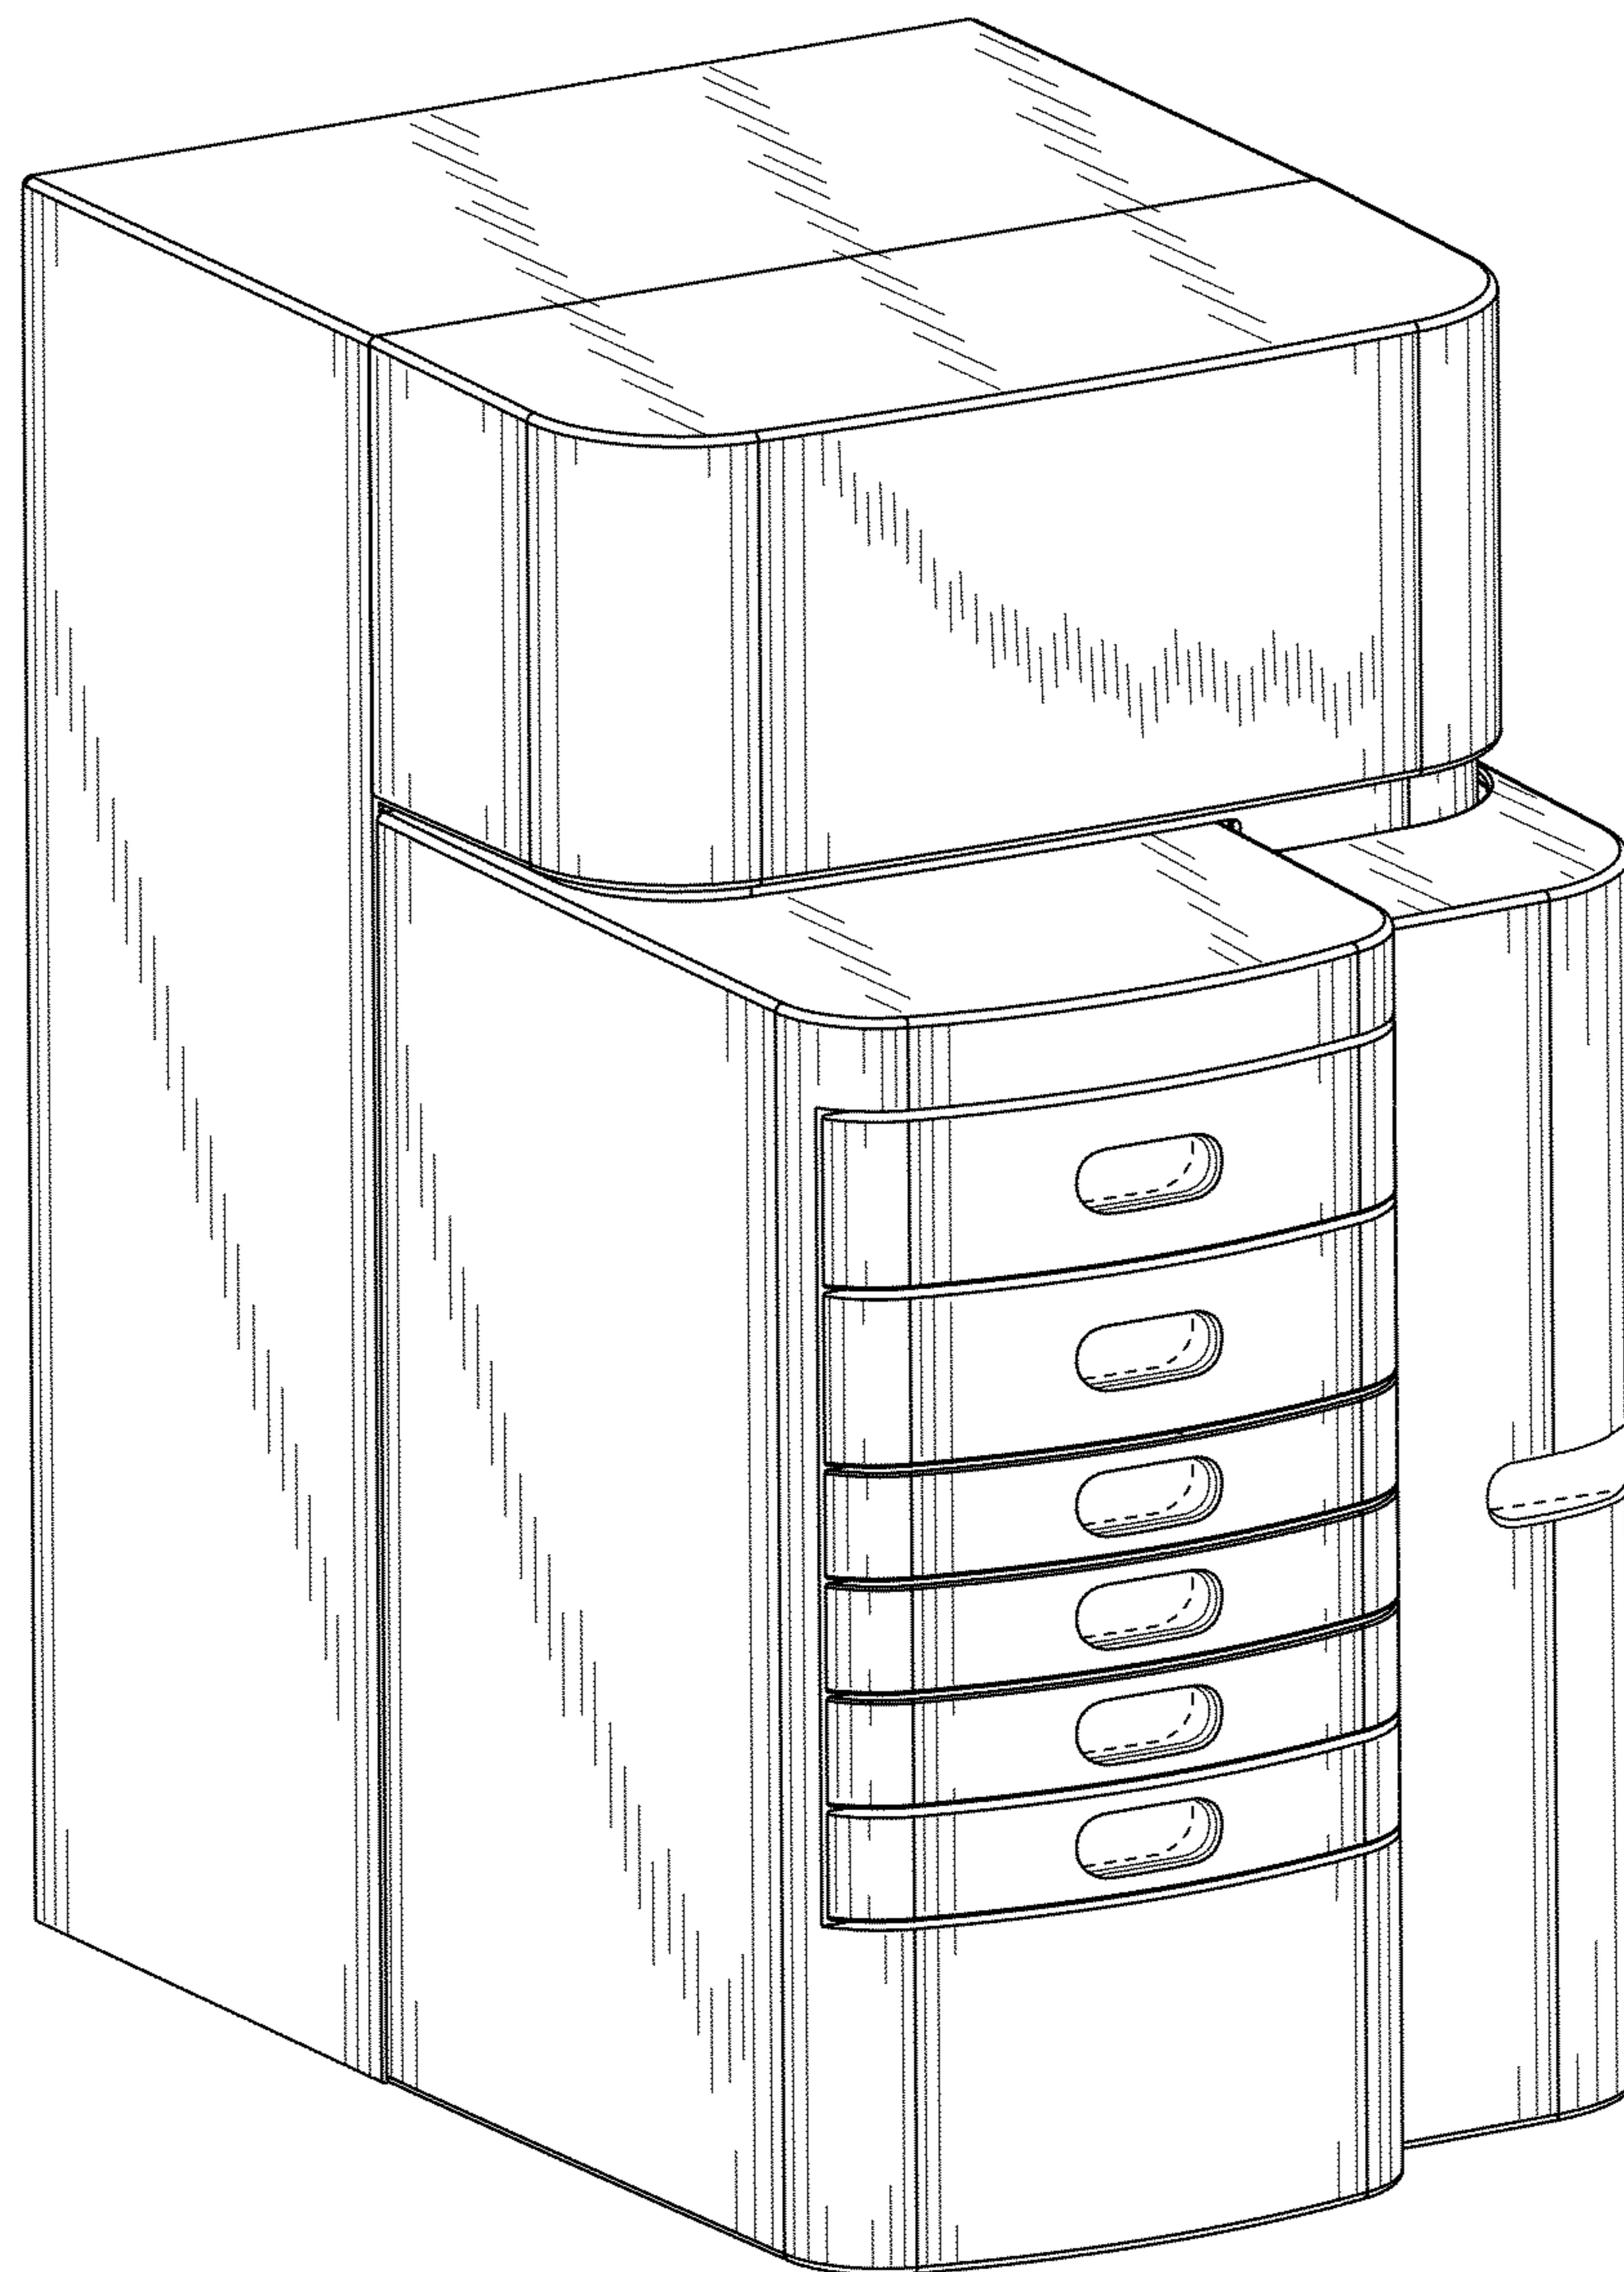


**FIG. 1**

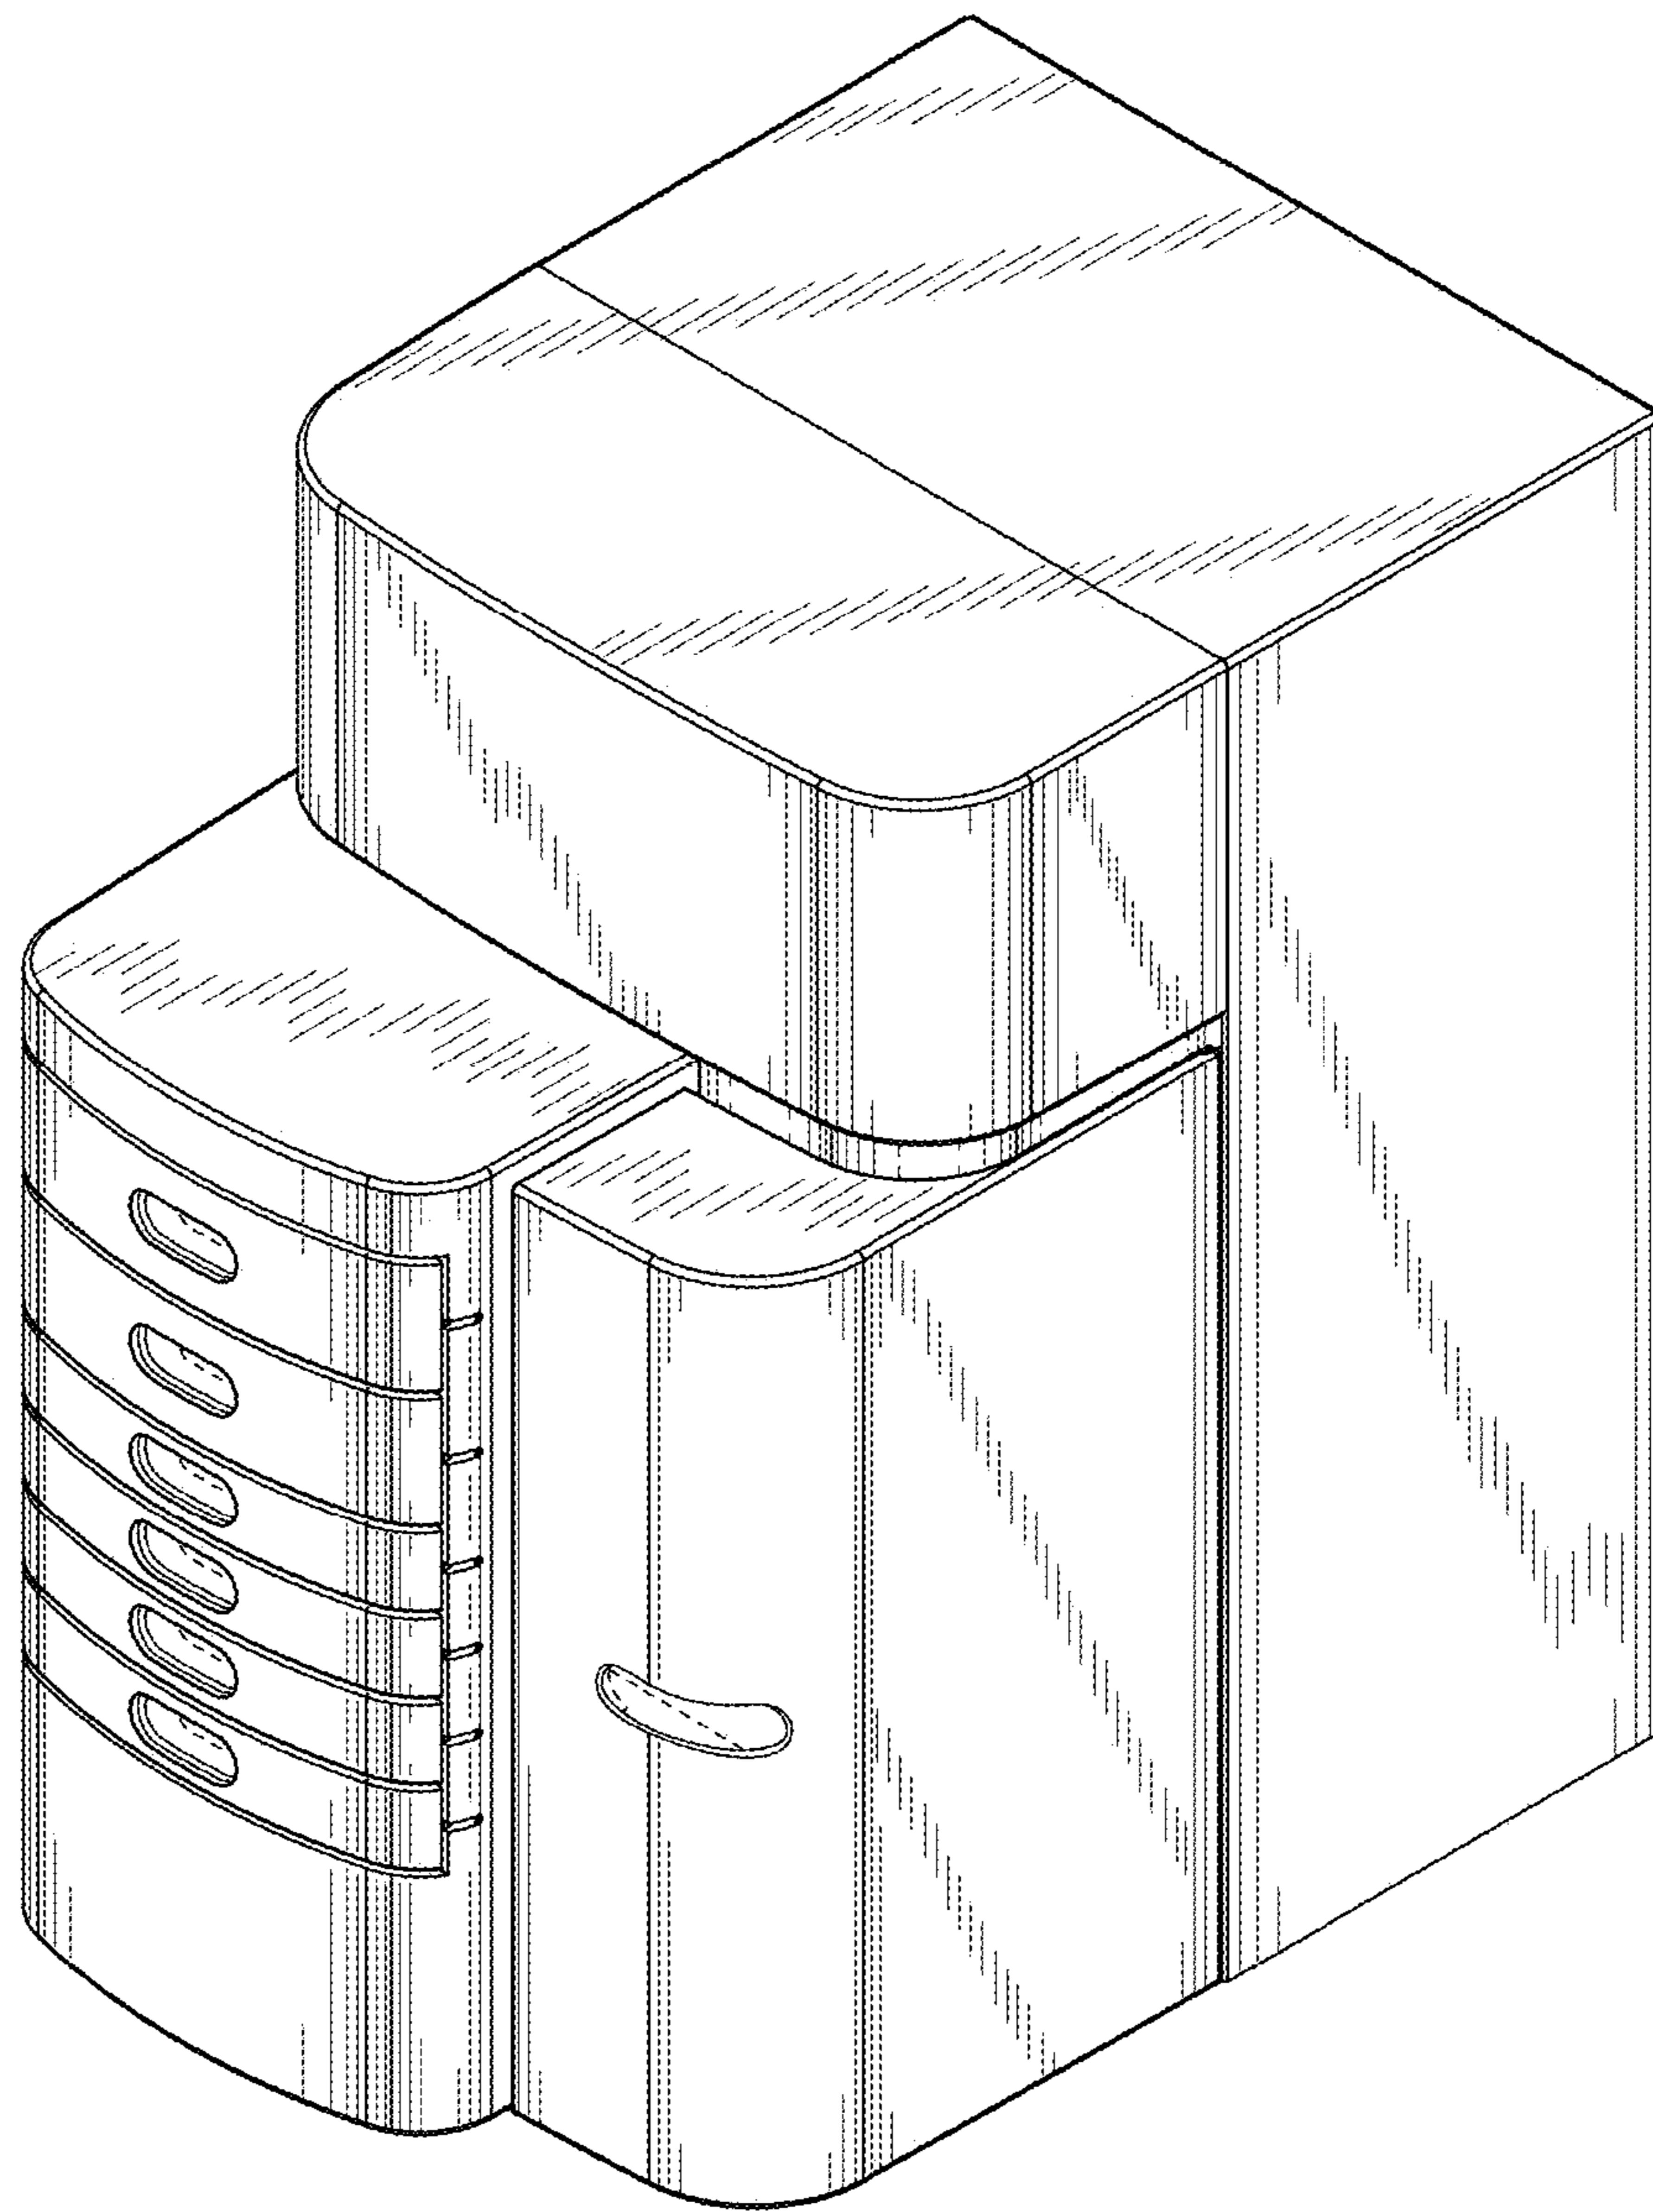


**FIG. 2**

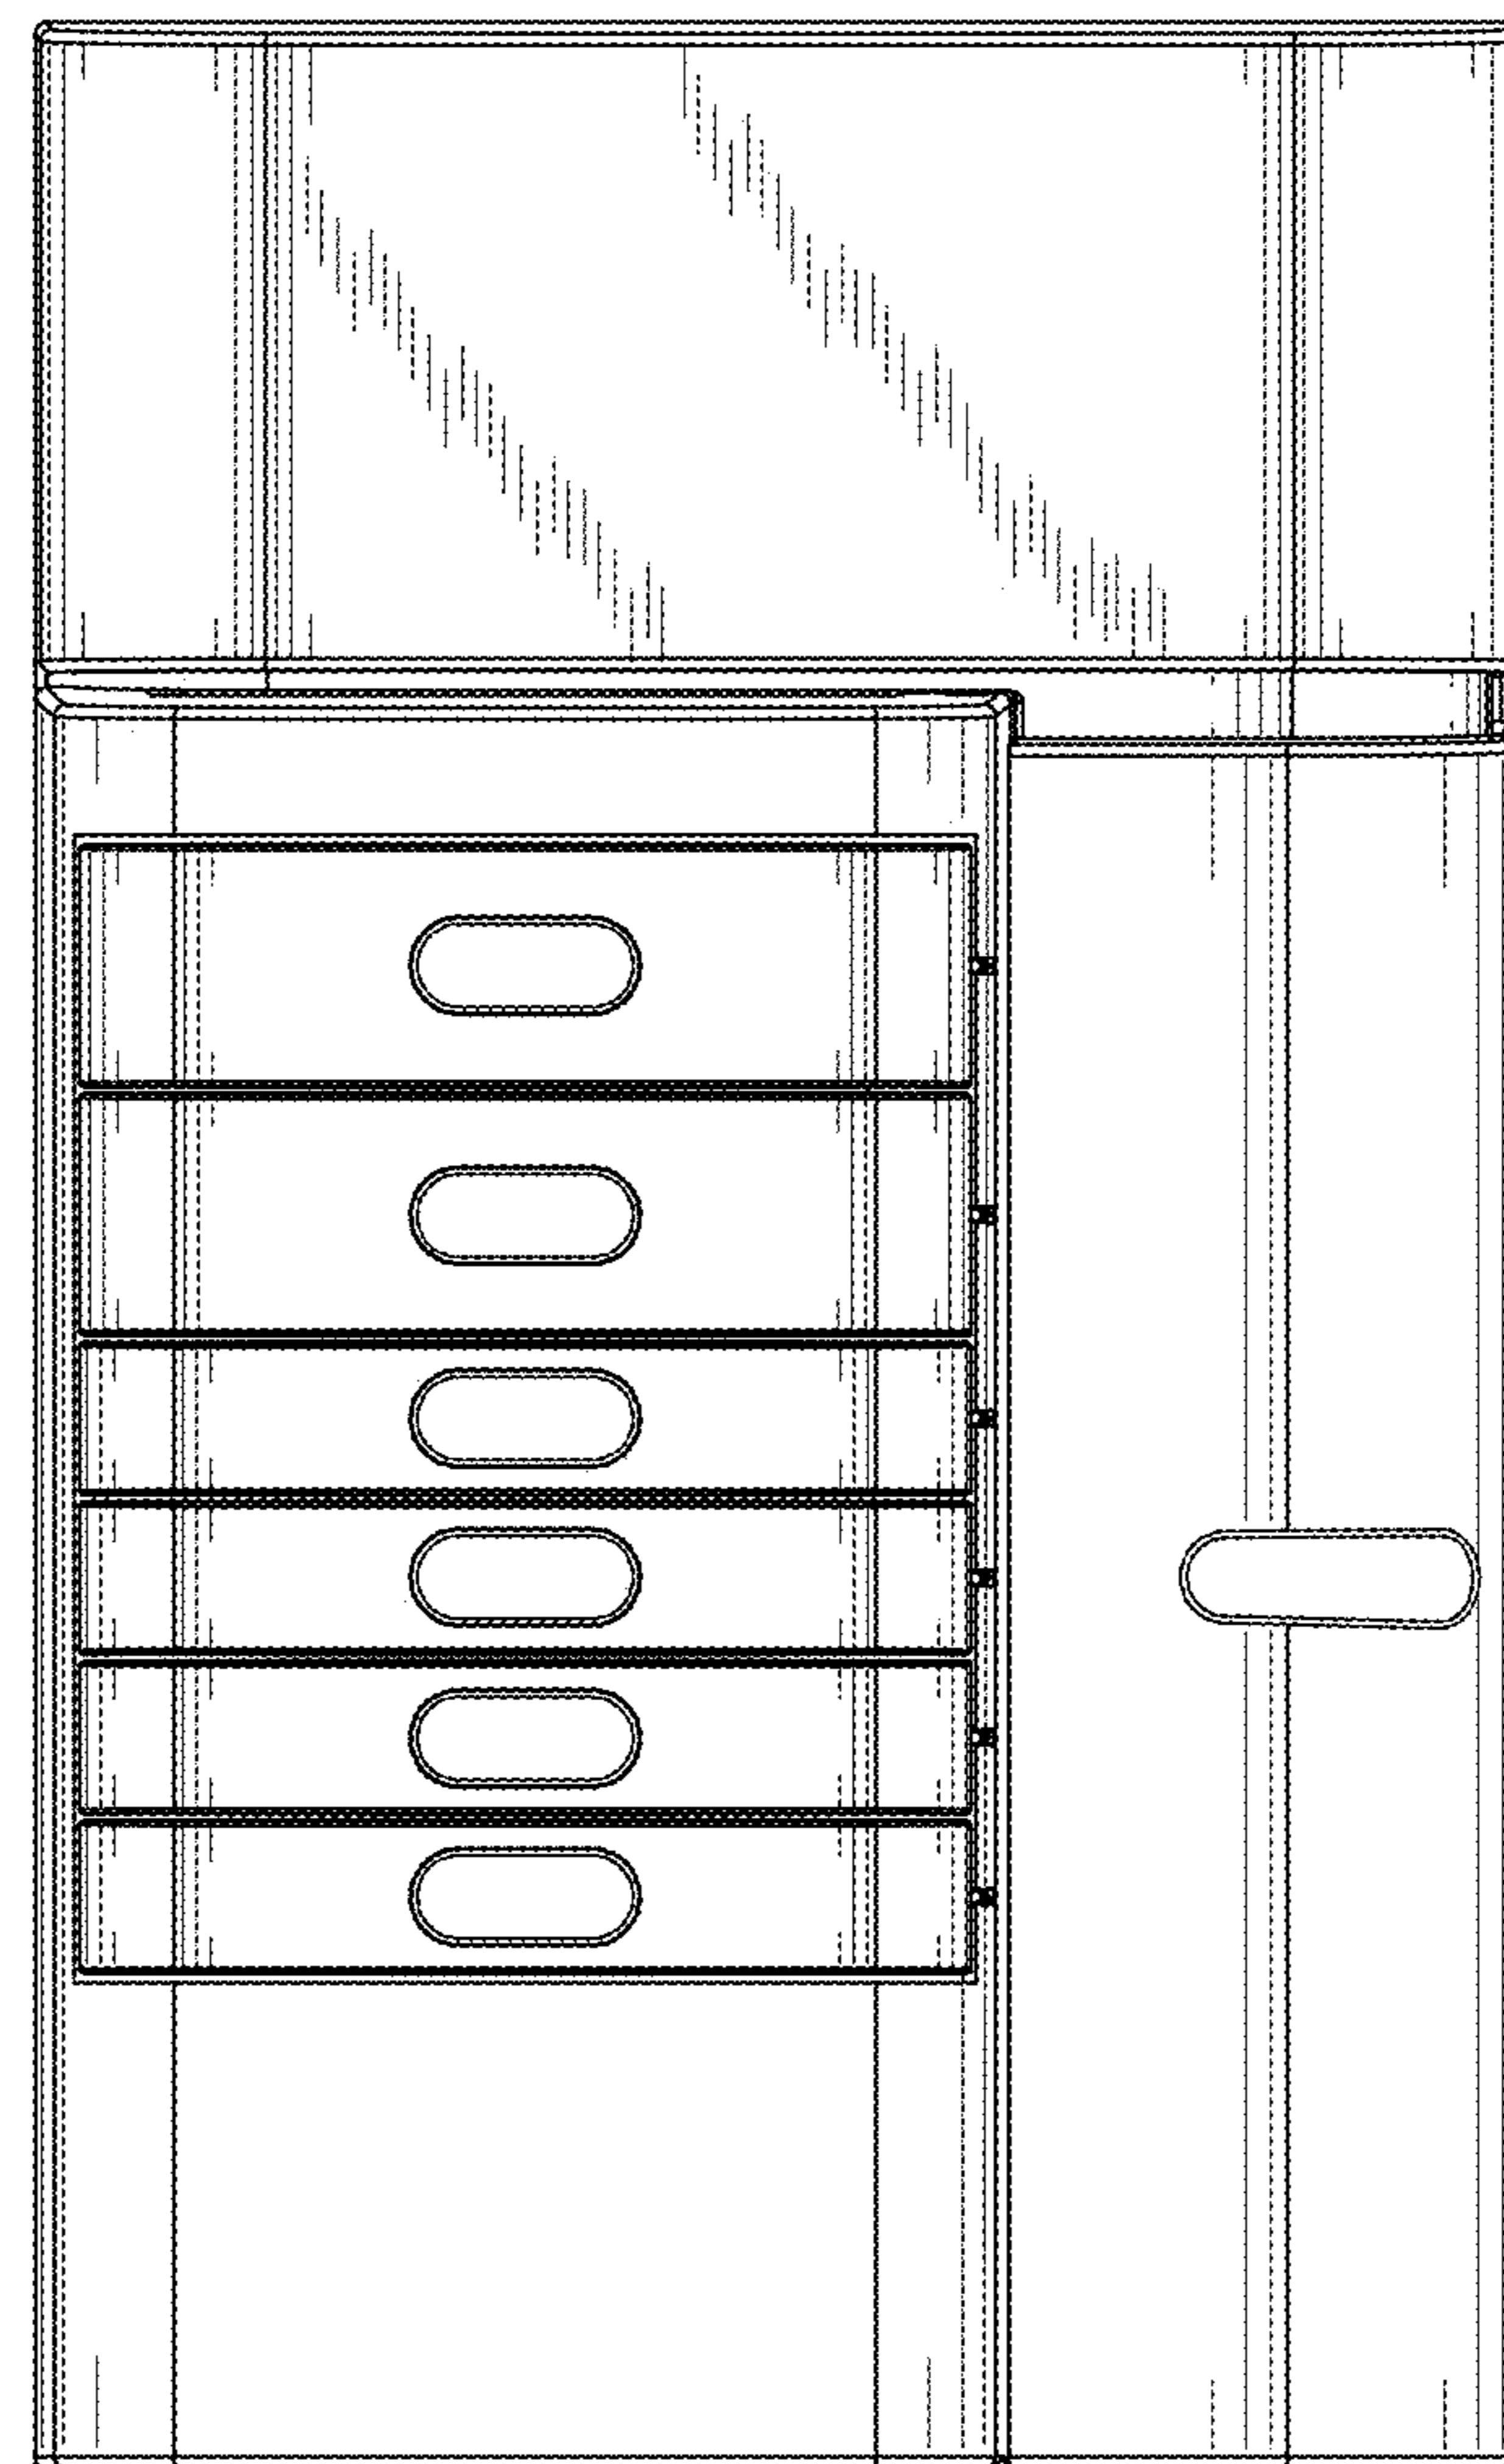


**FIG. 3**

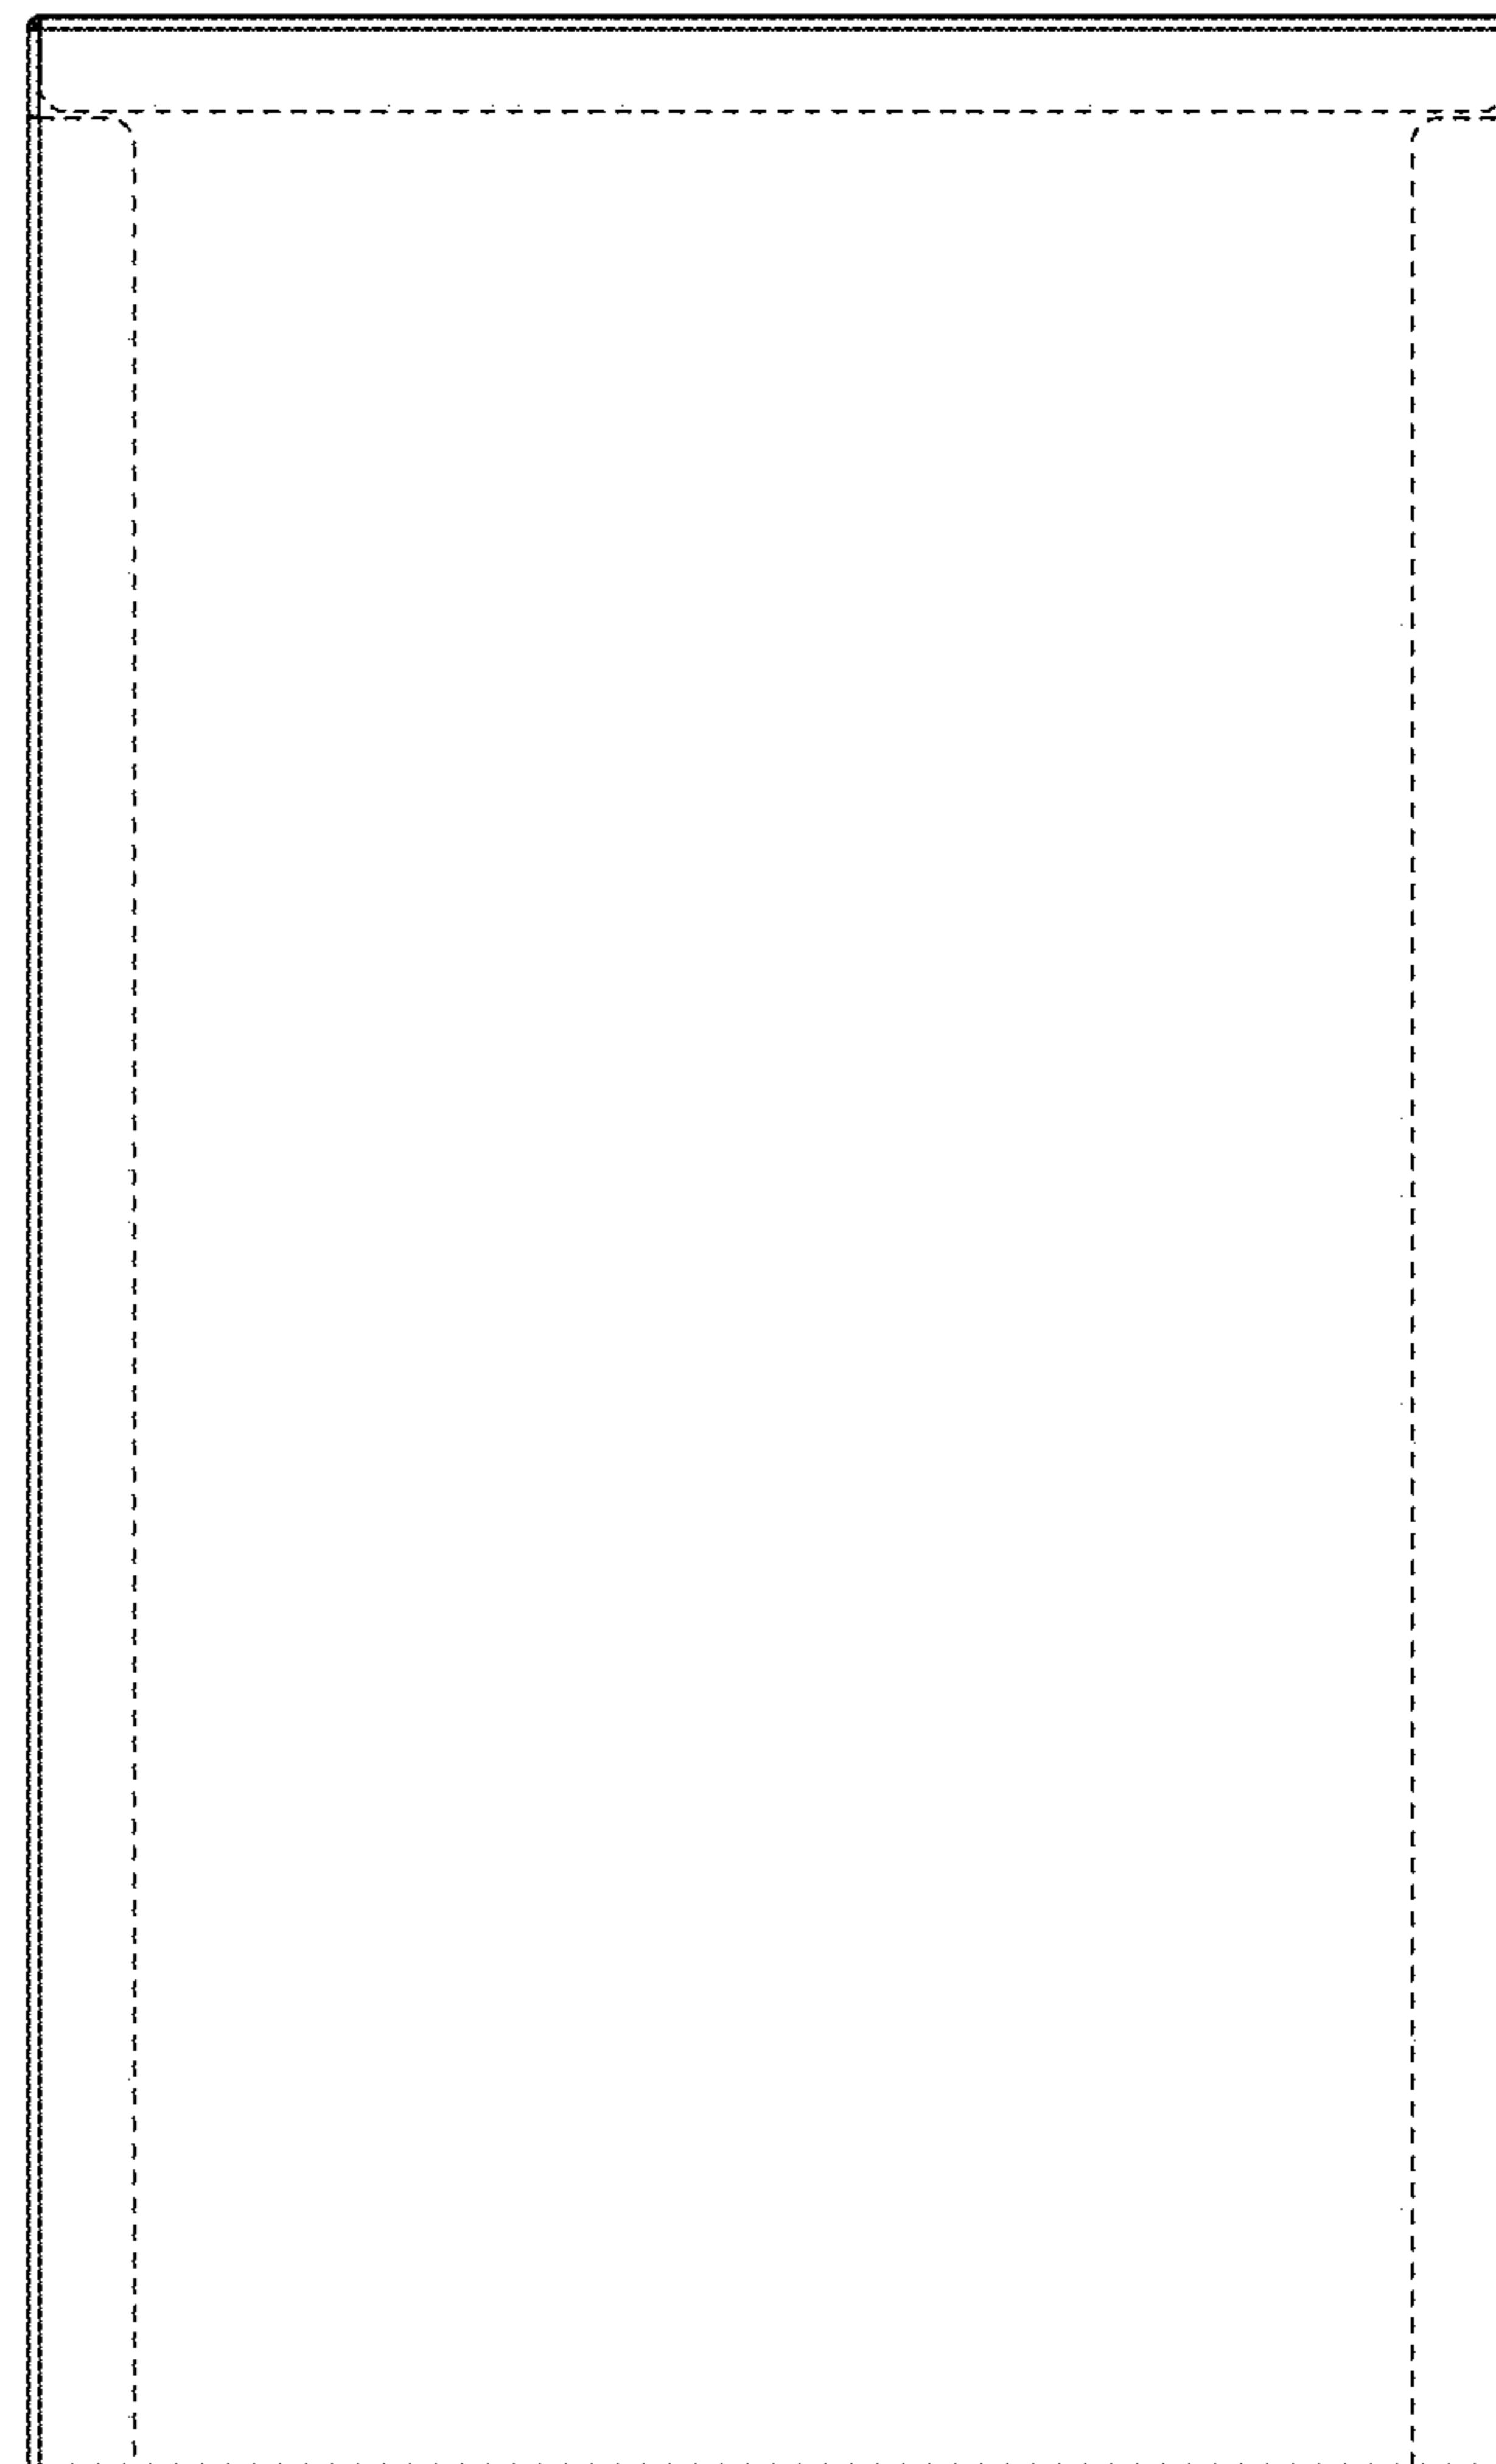


**FIG. 4**

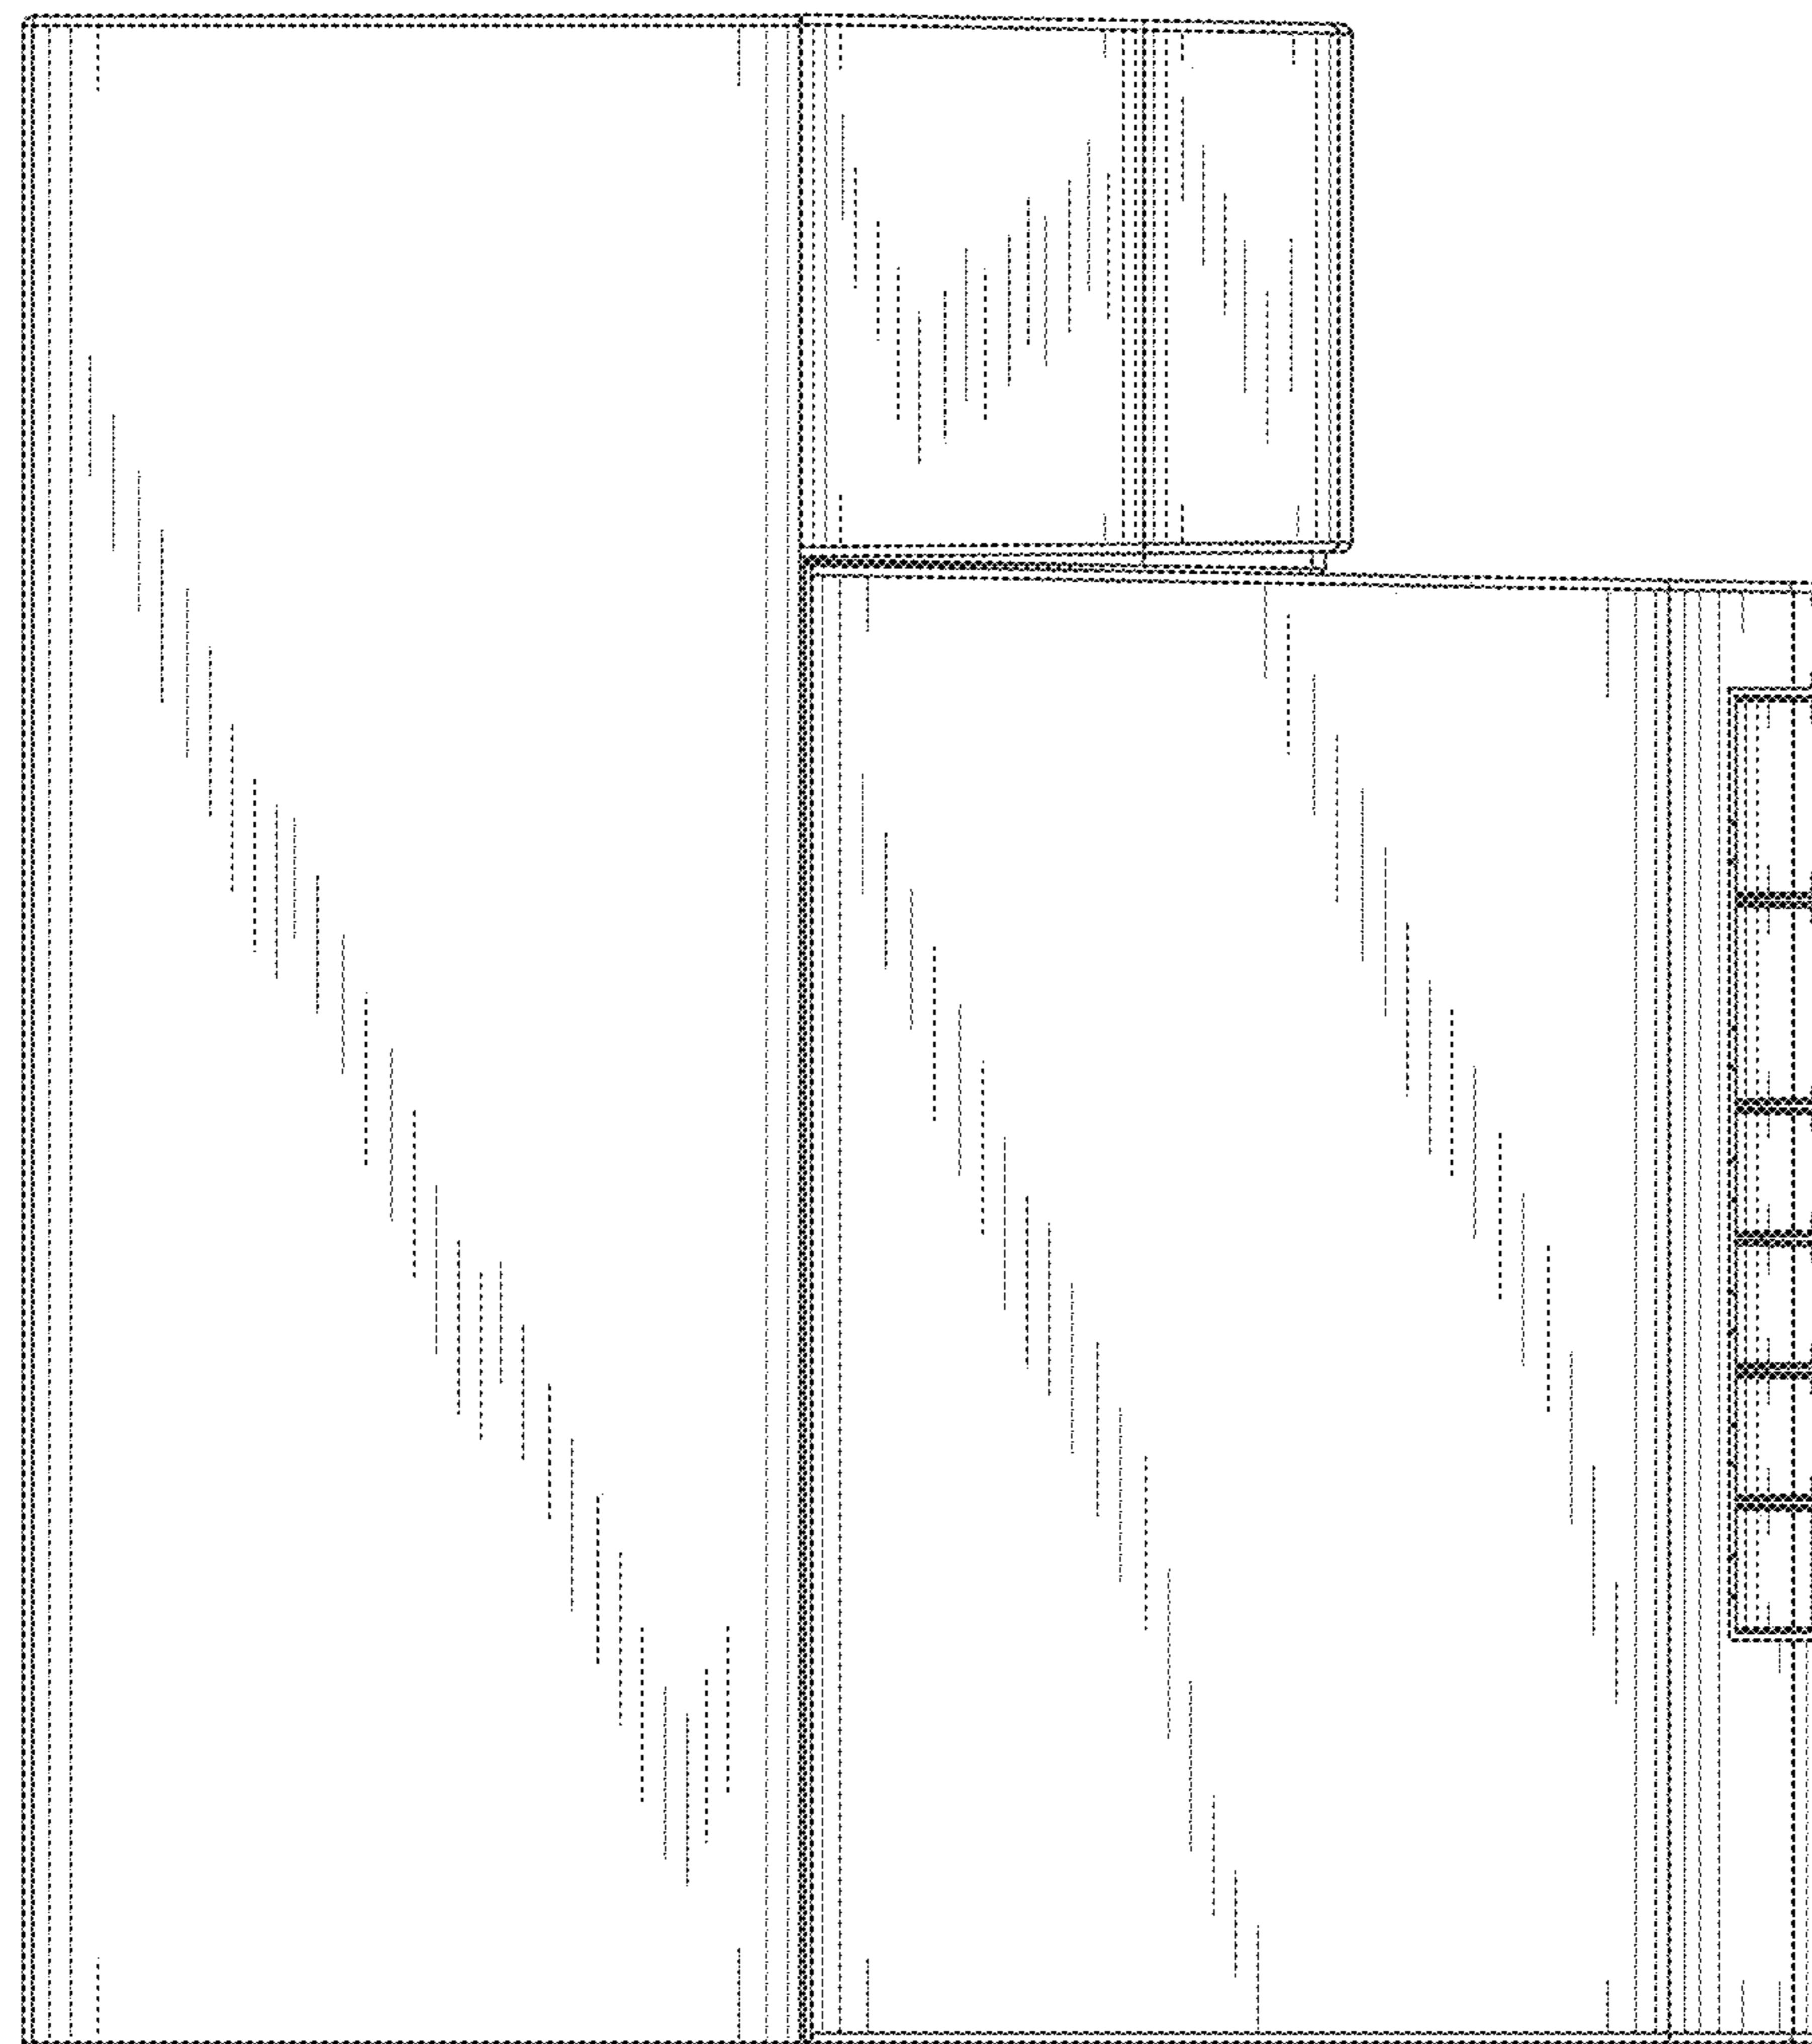


**FIG. 5**

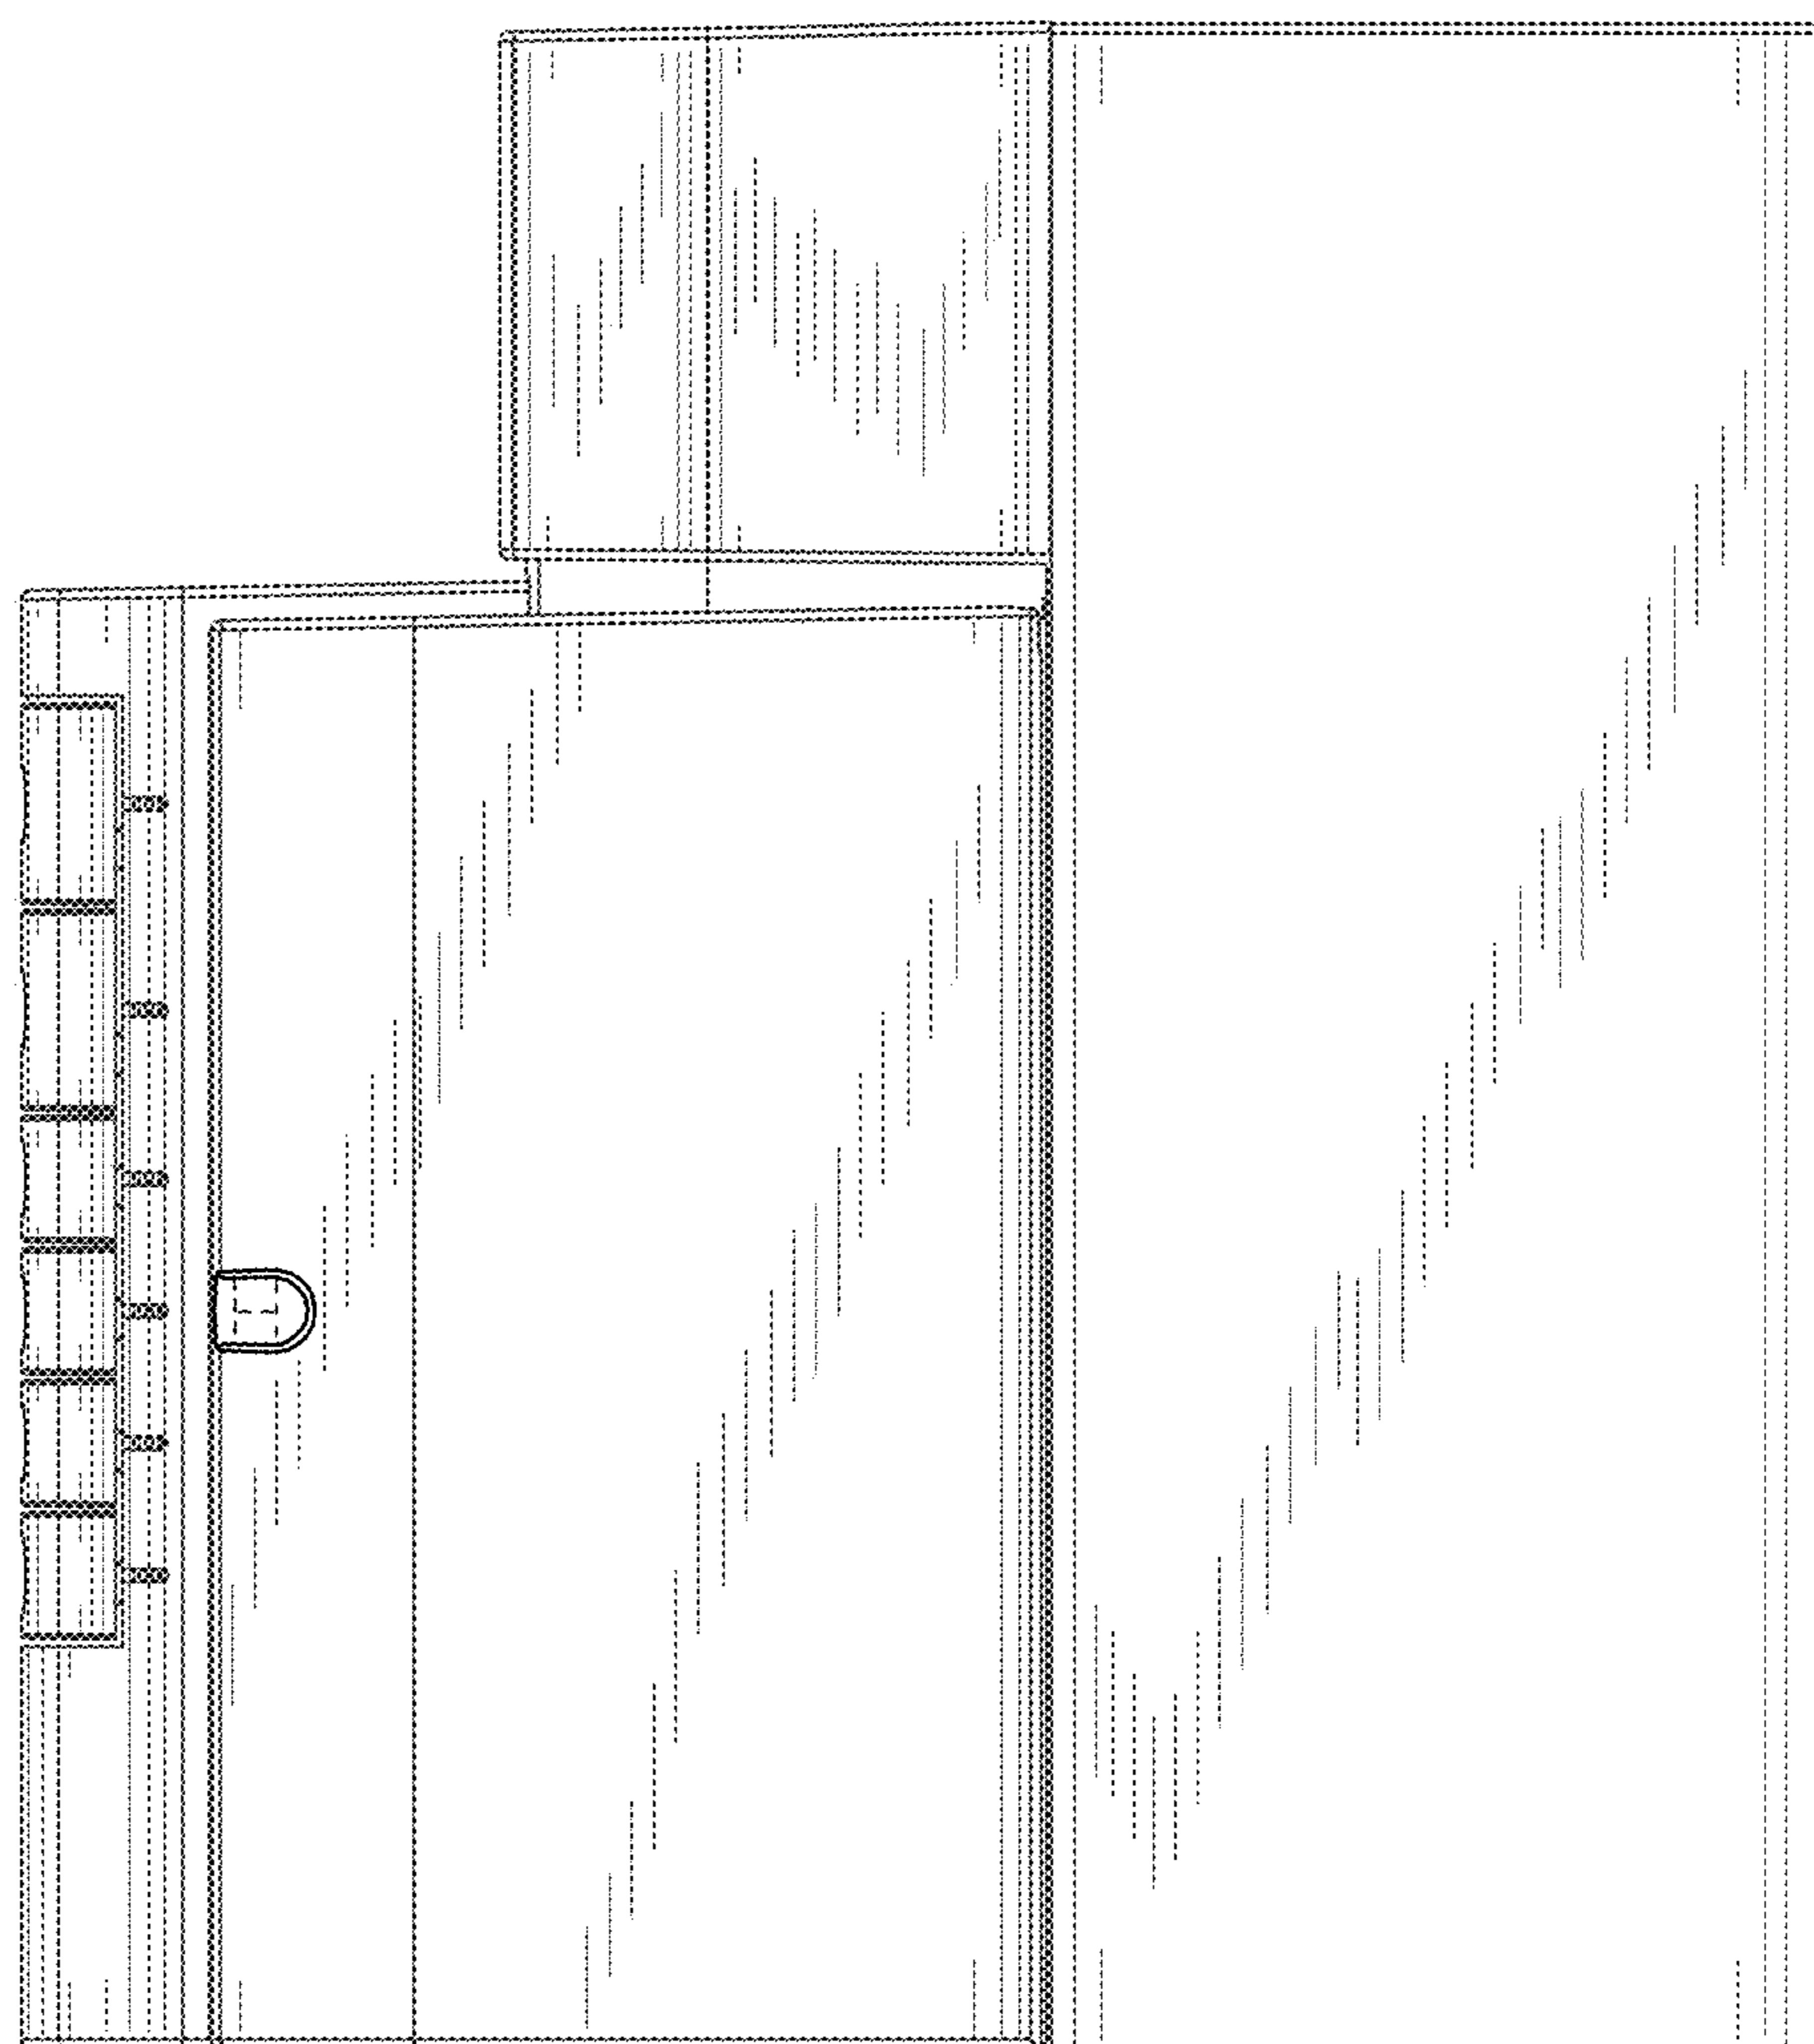

**FIG. 6**

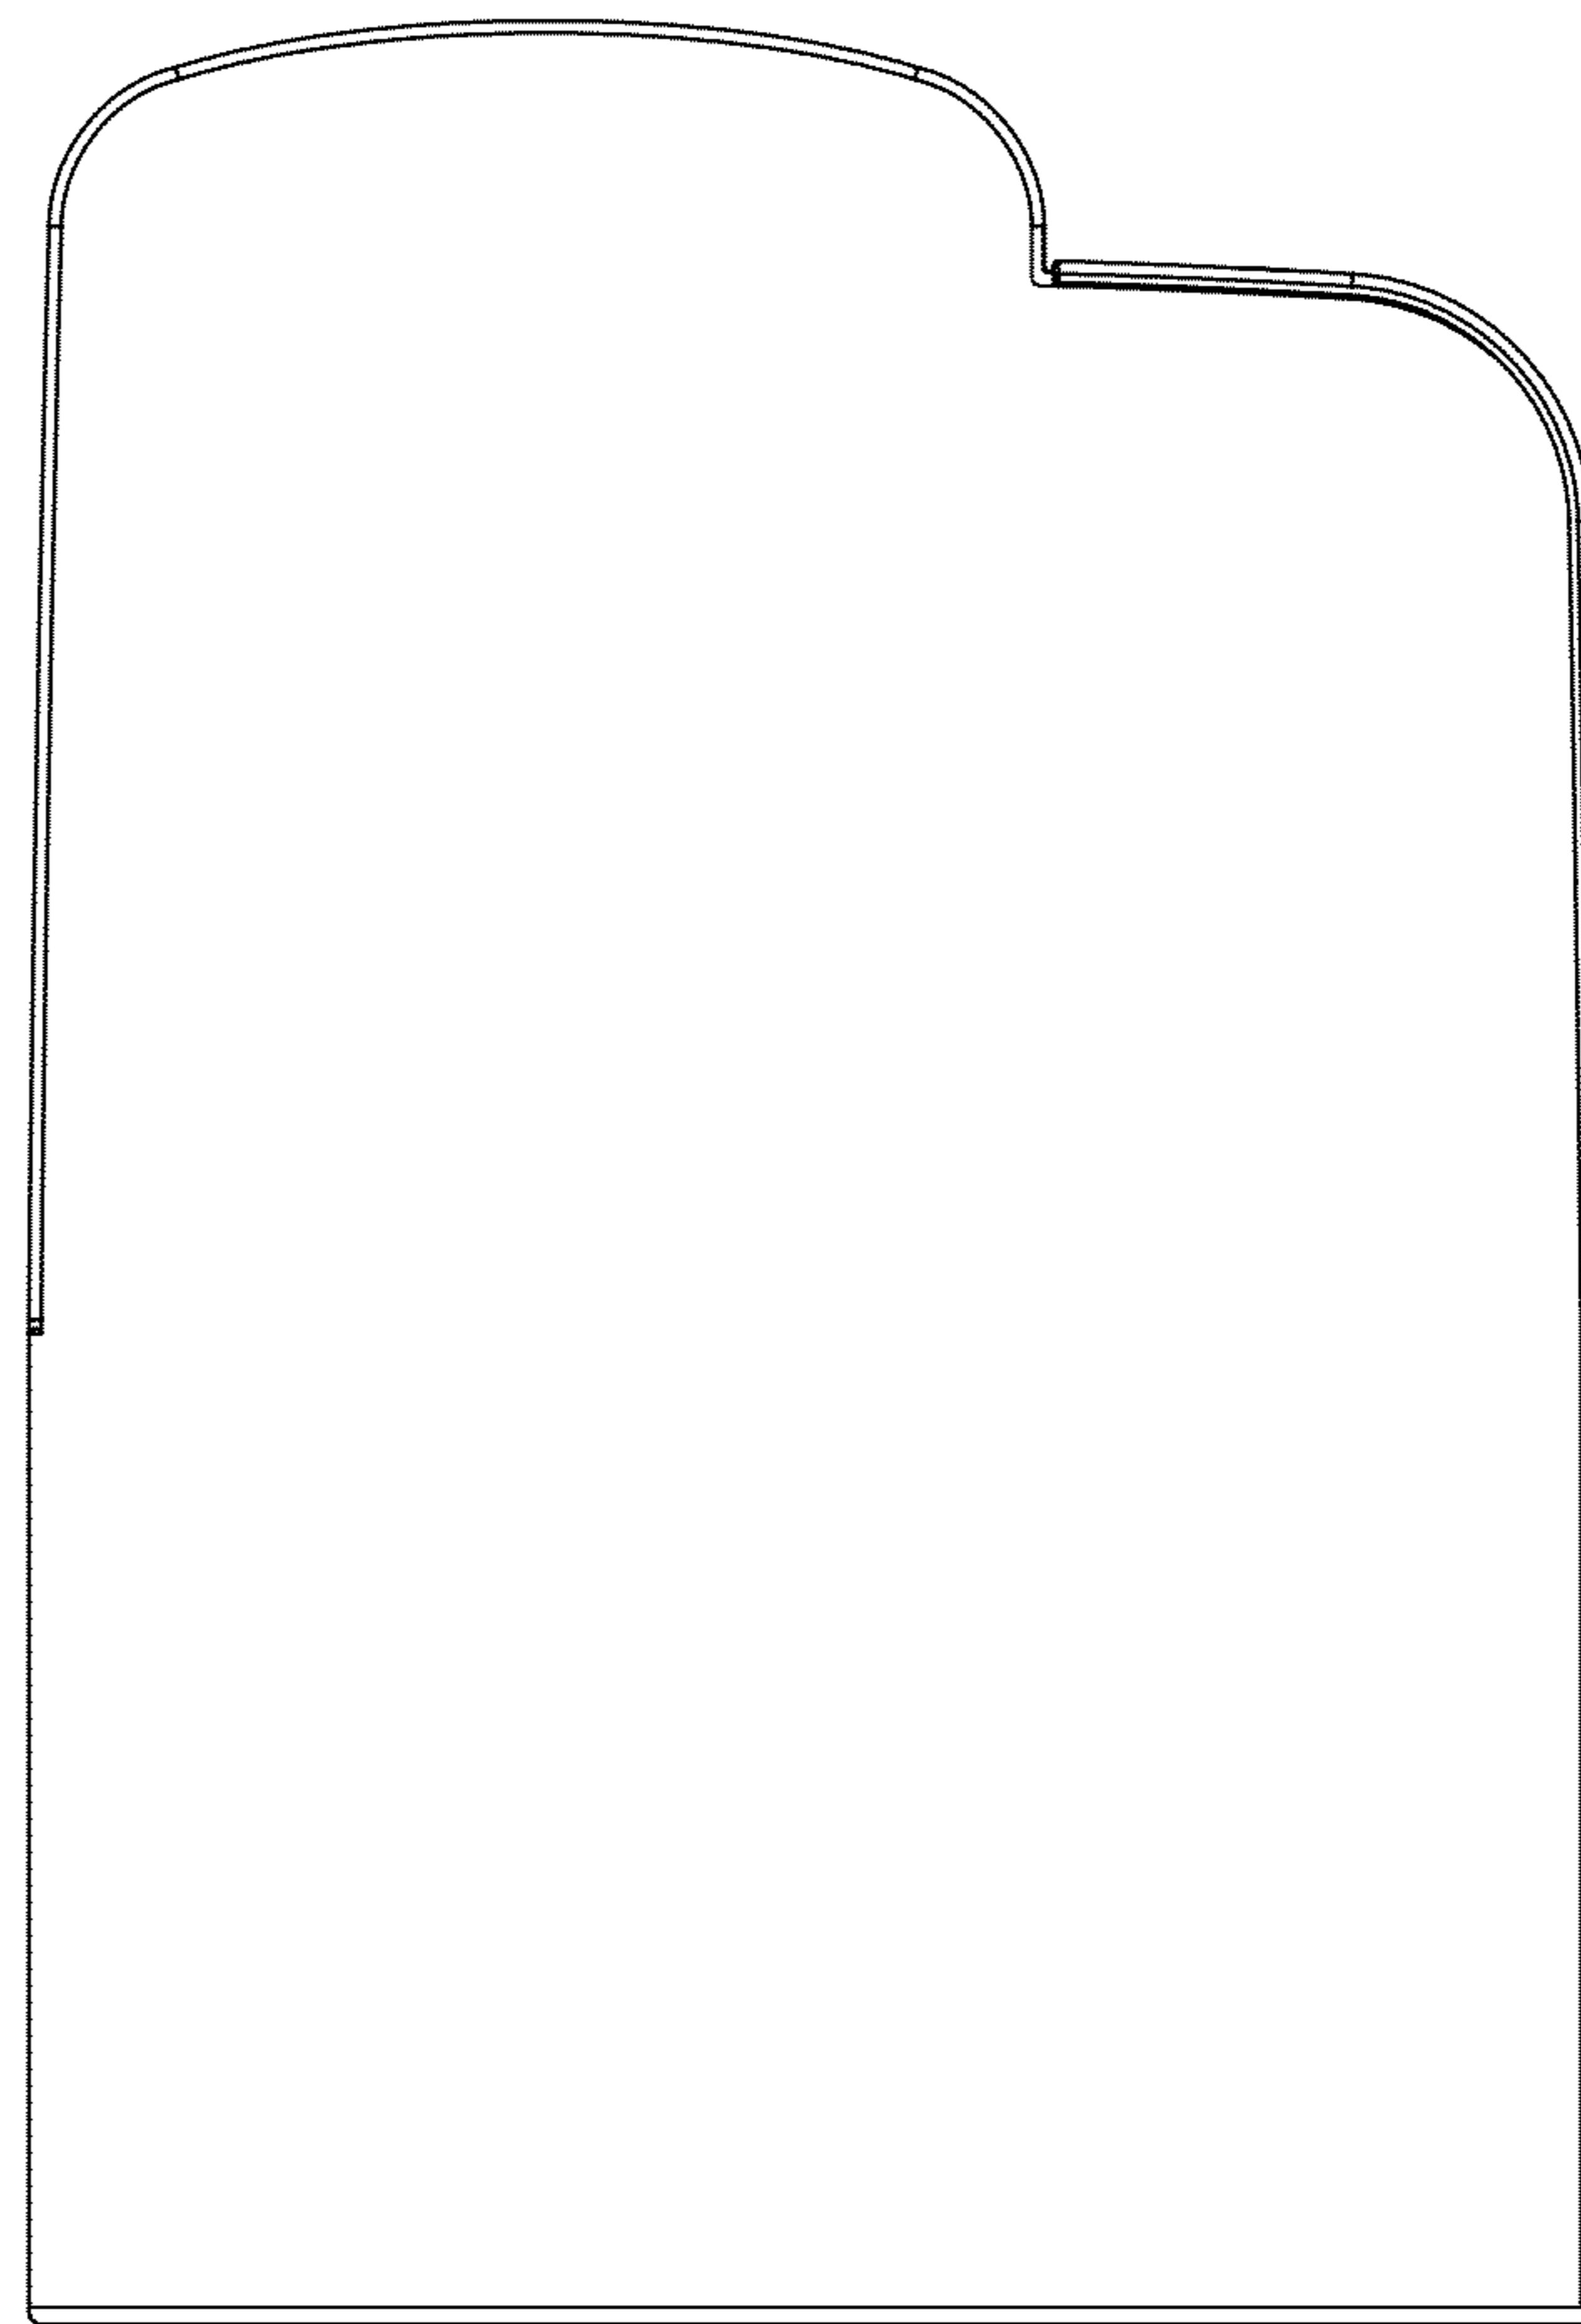

**FIG. 7**

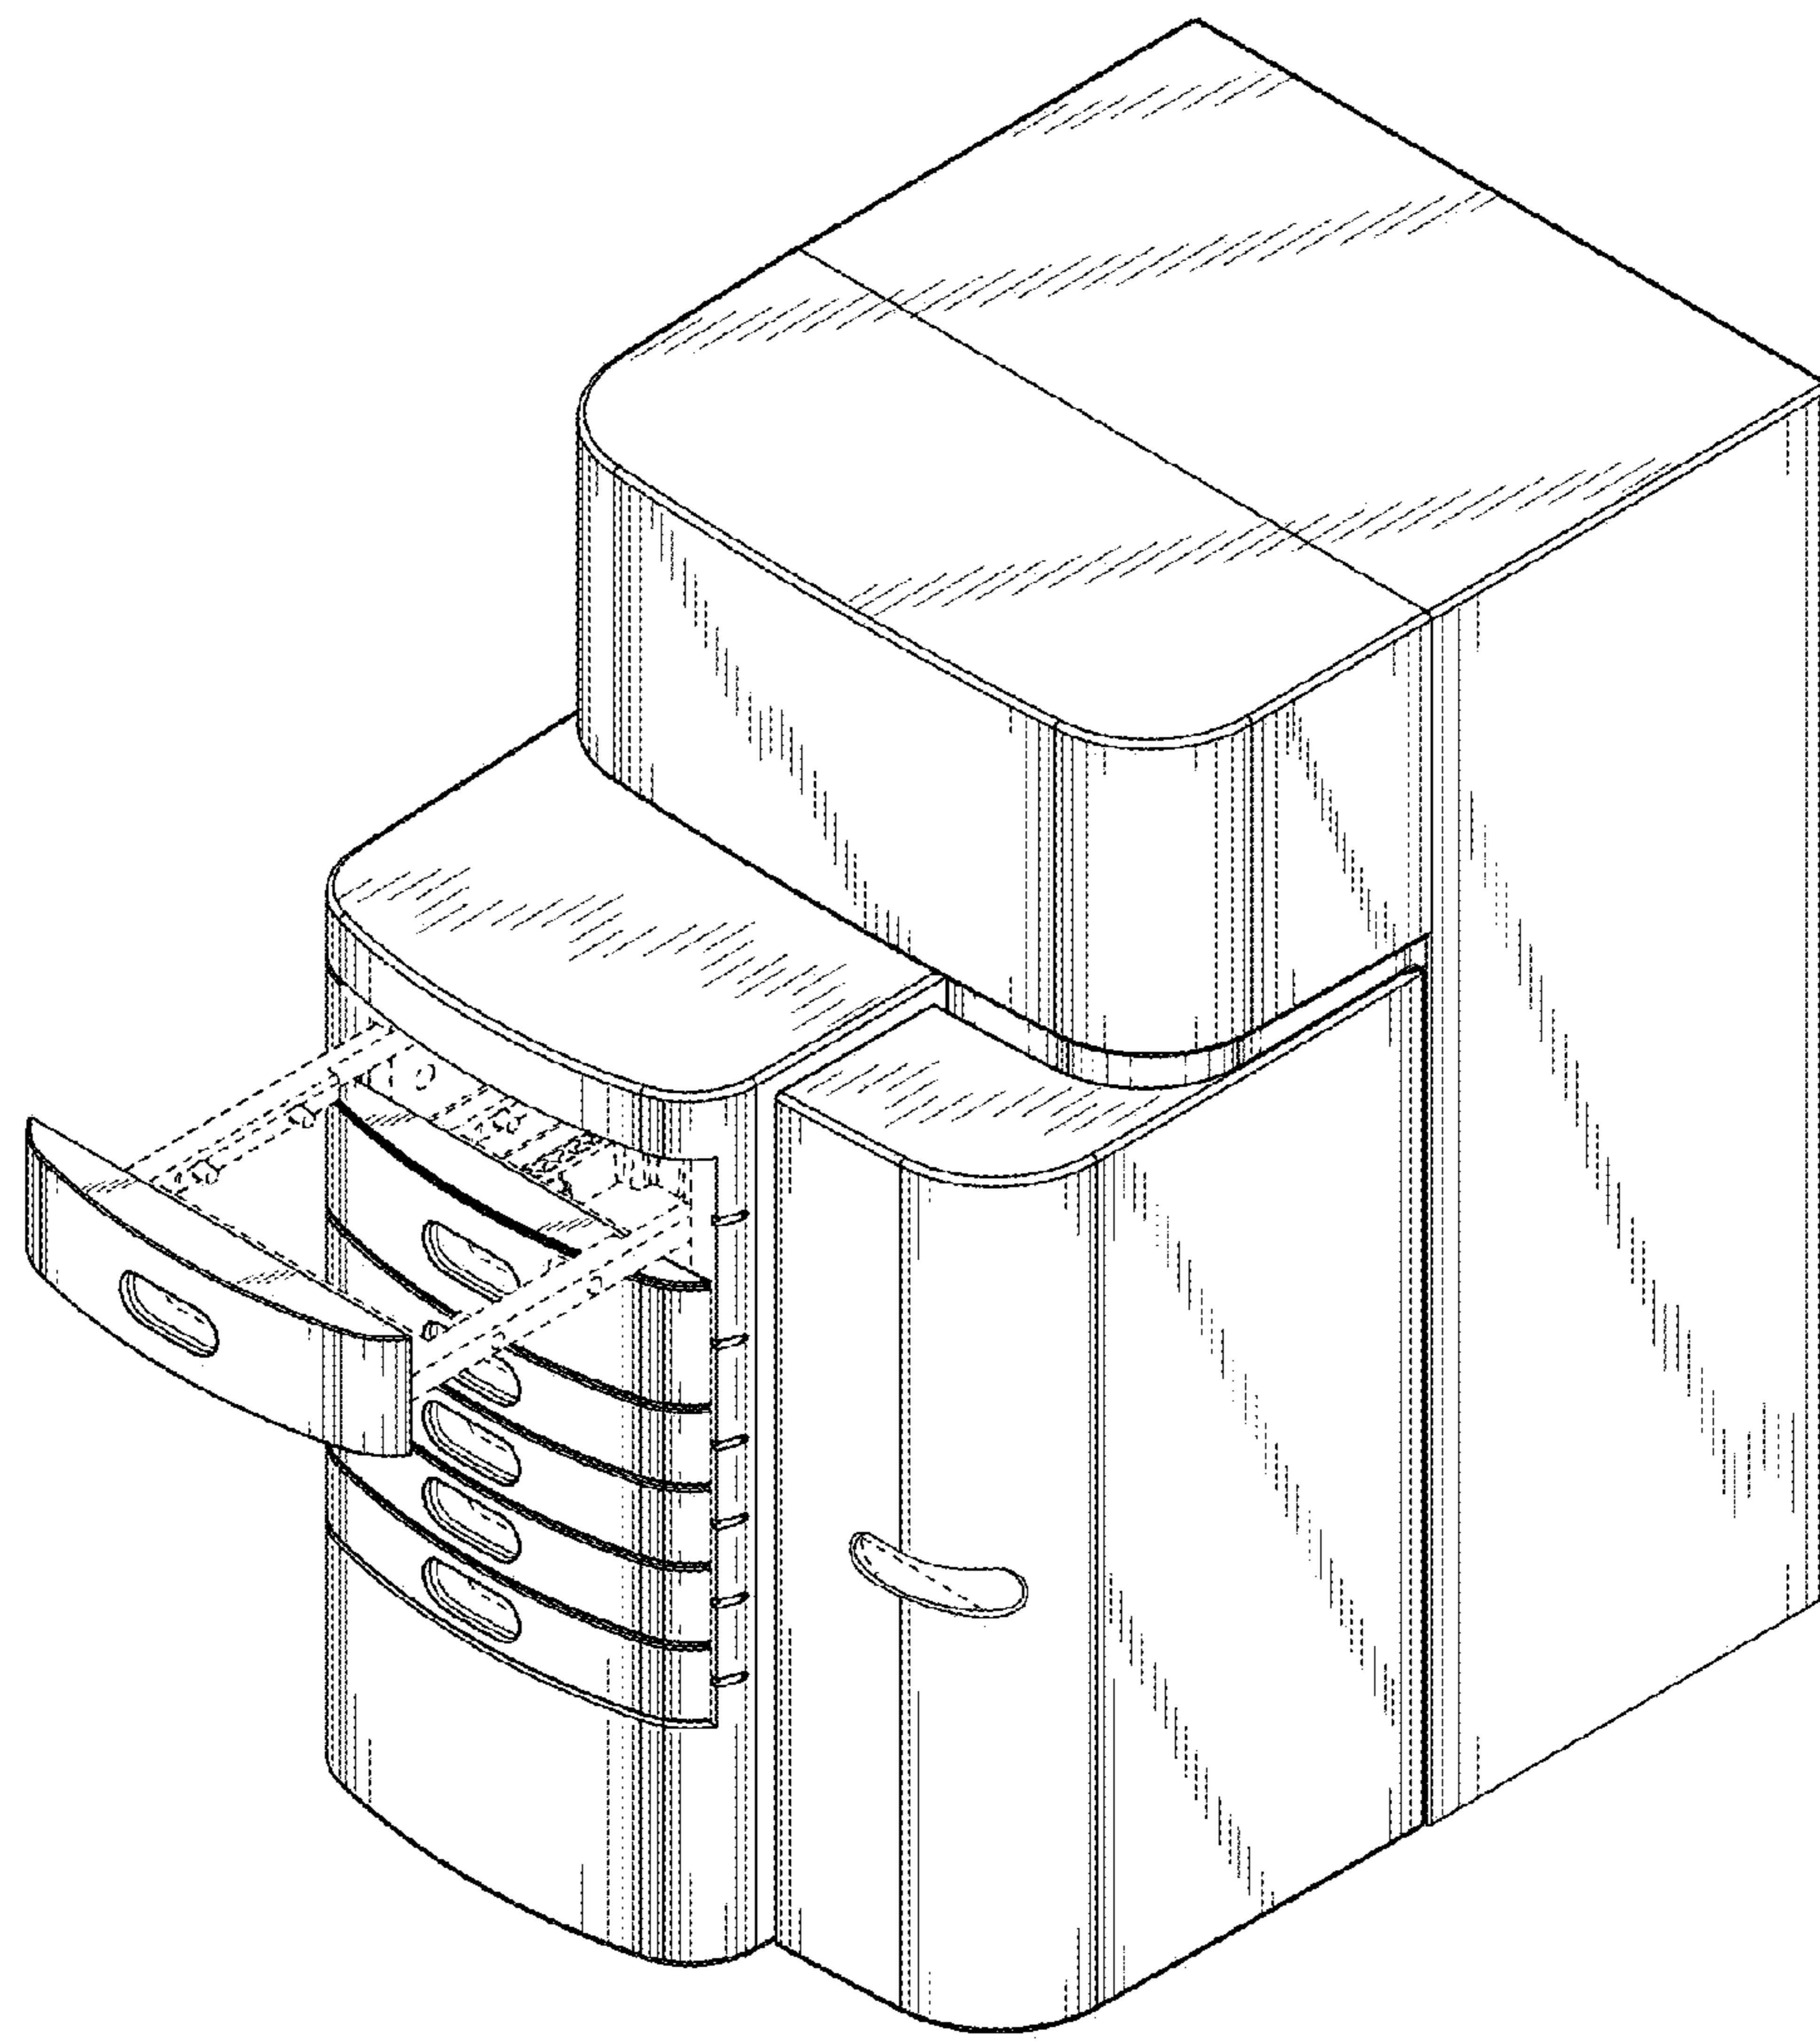

**FIG. 8**


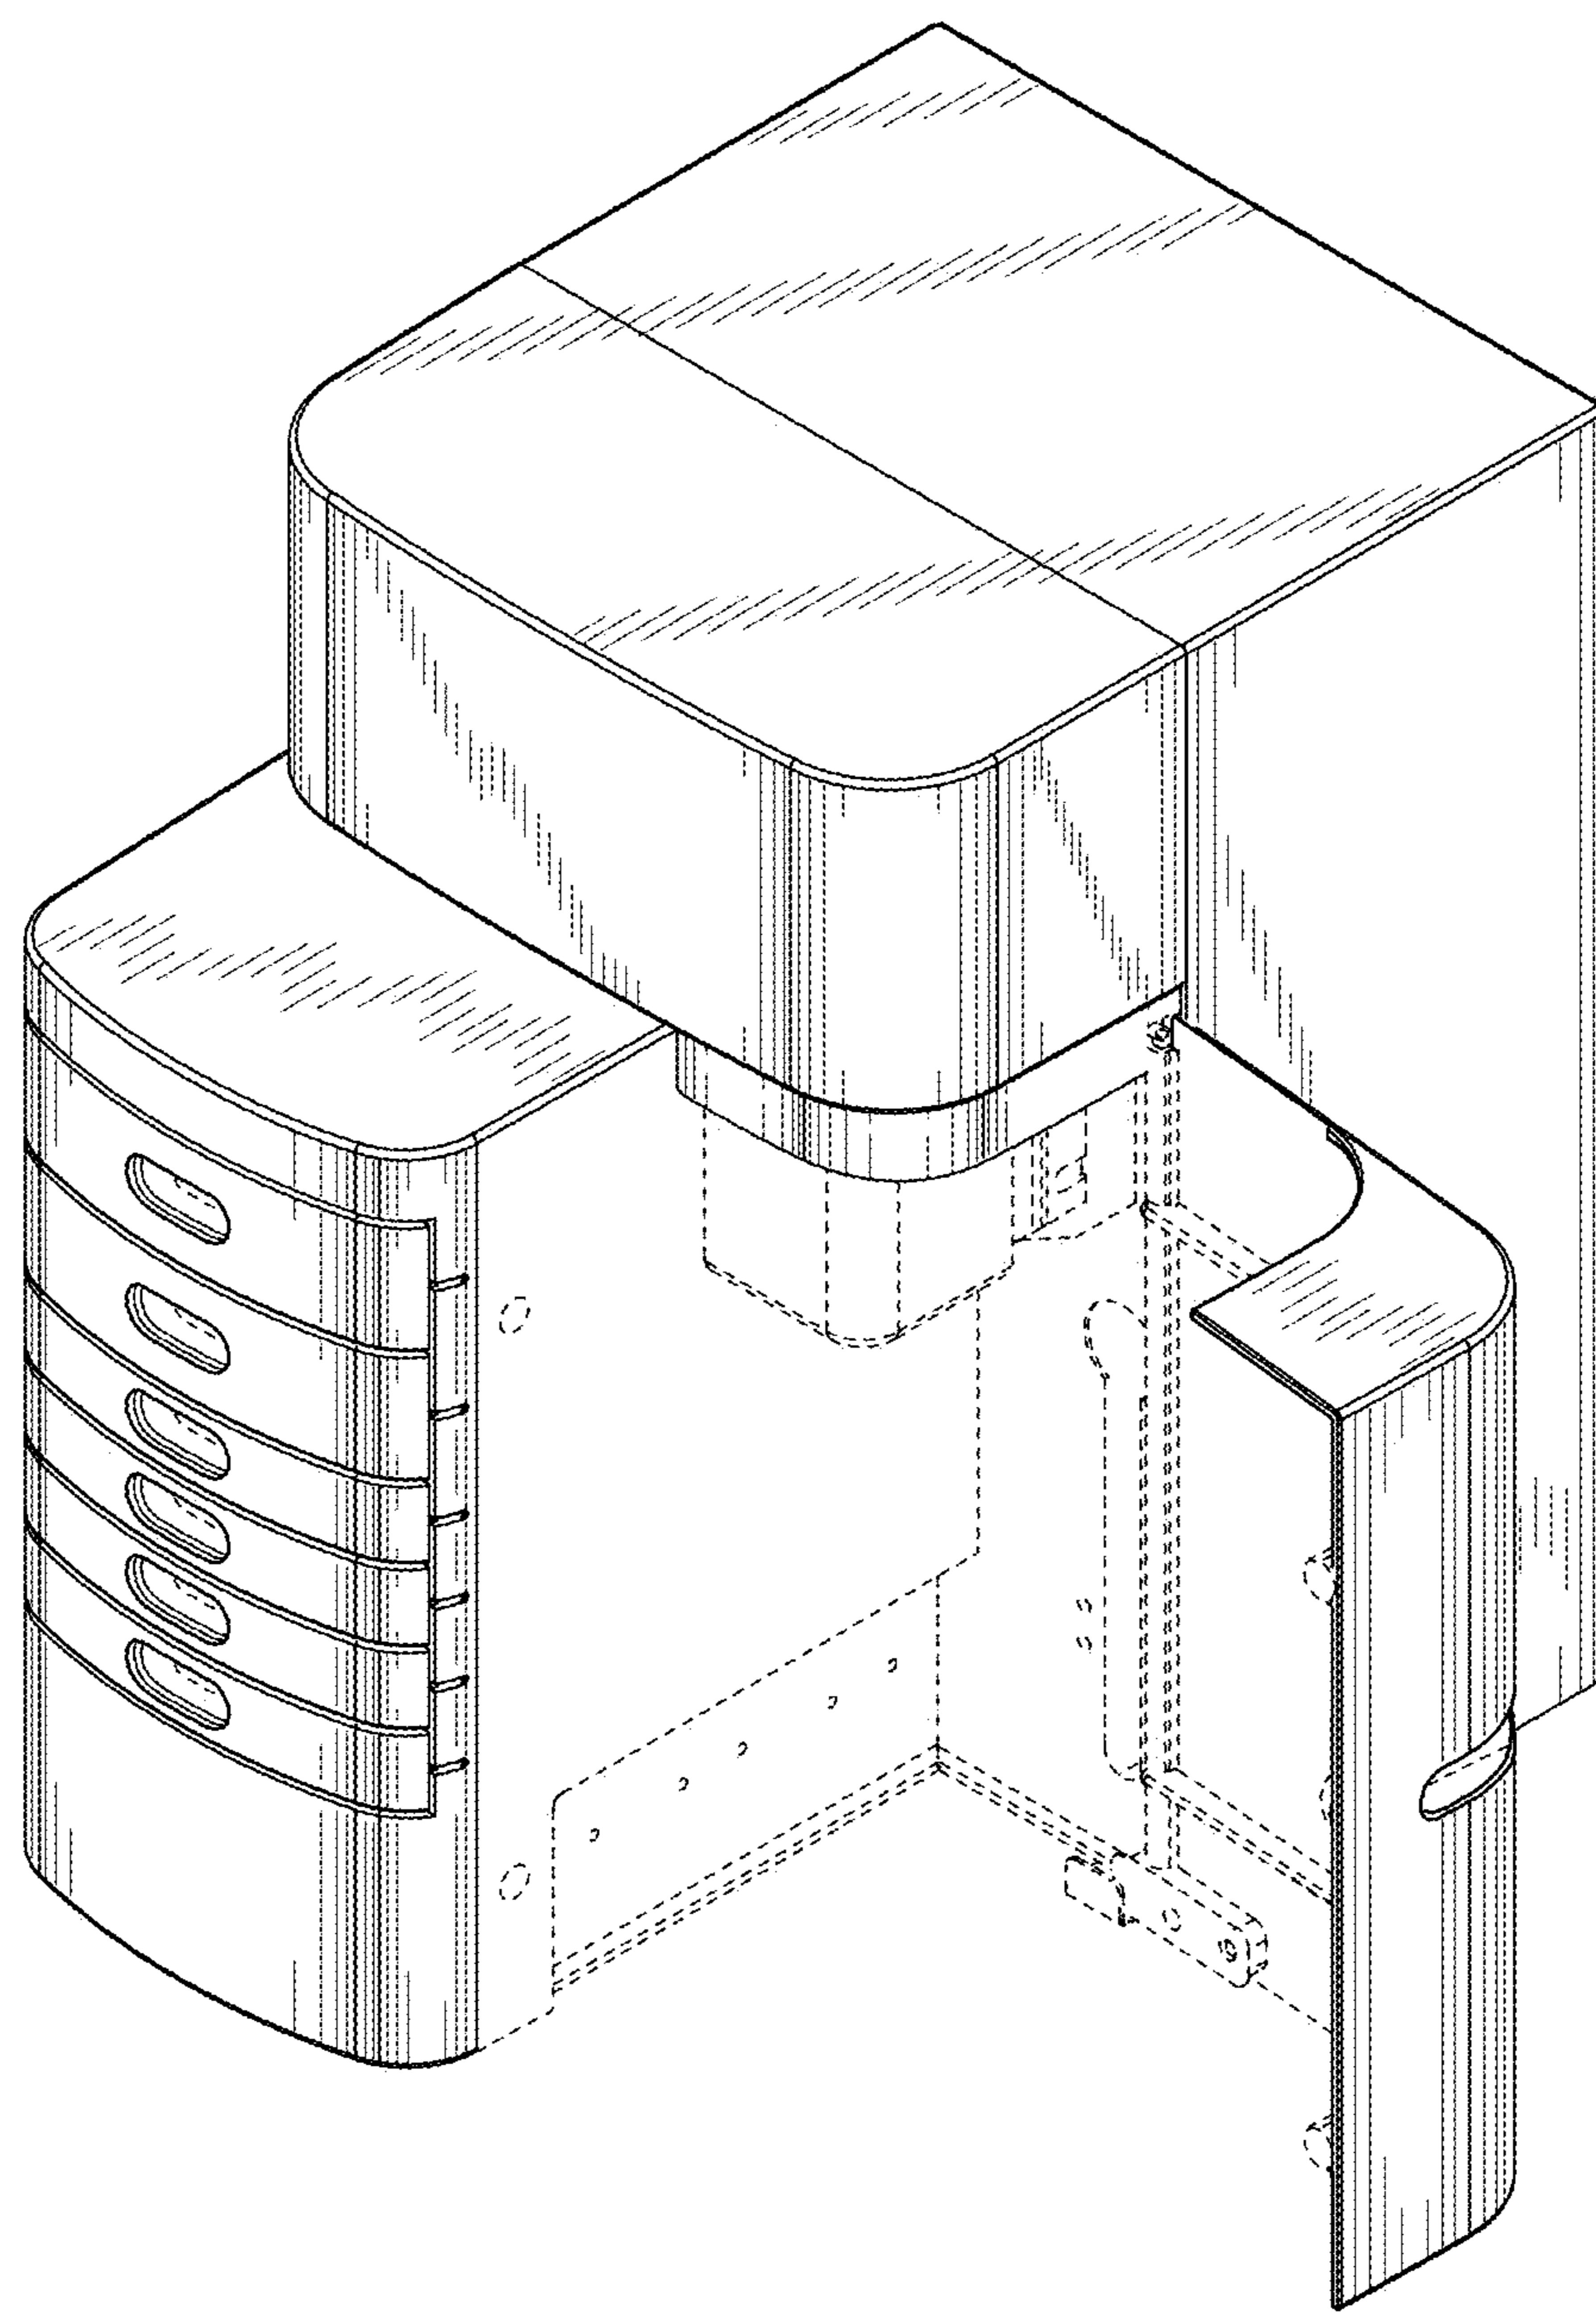


FIG. 9

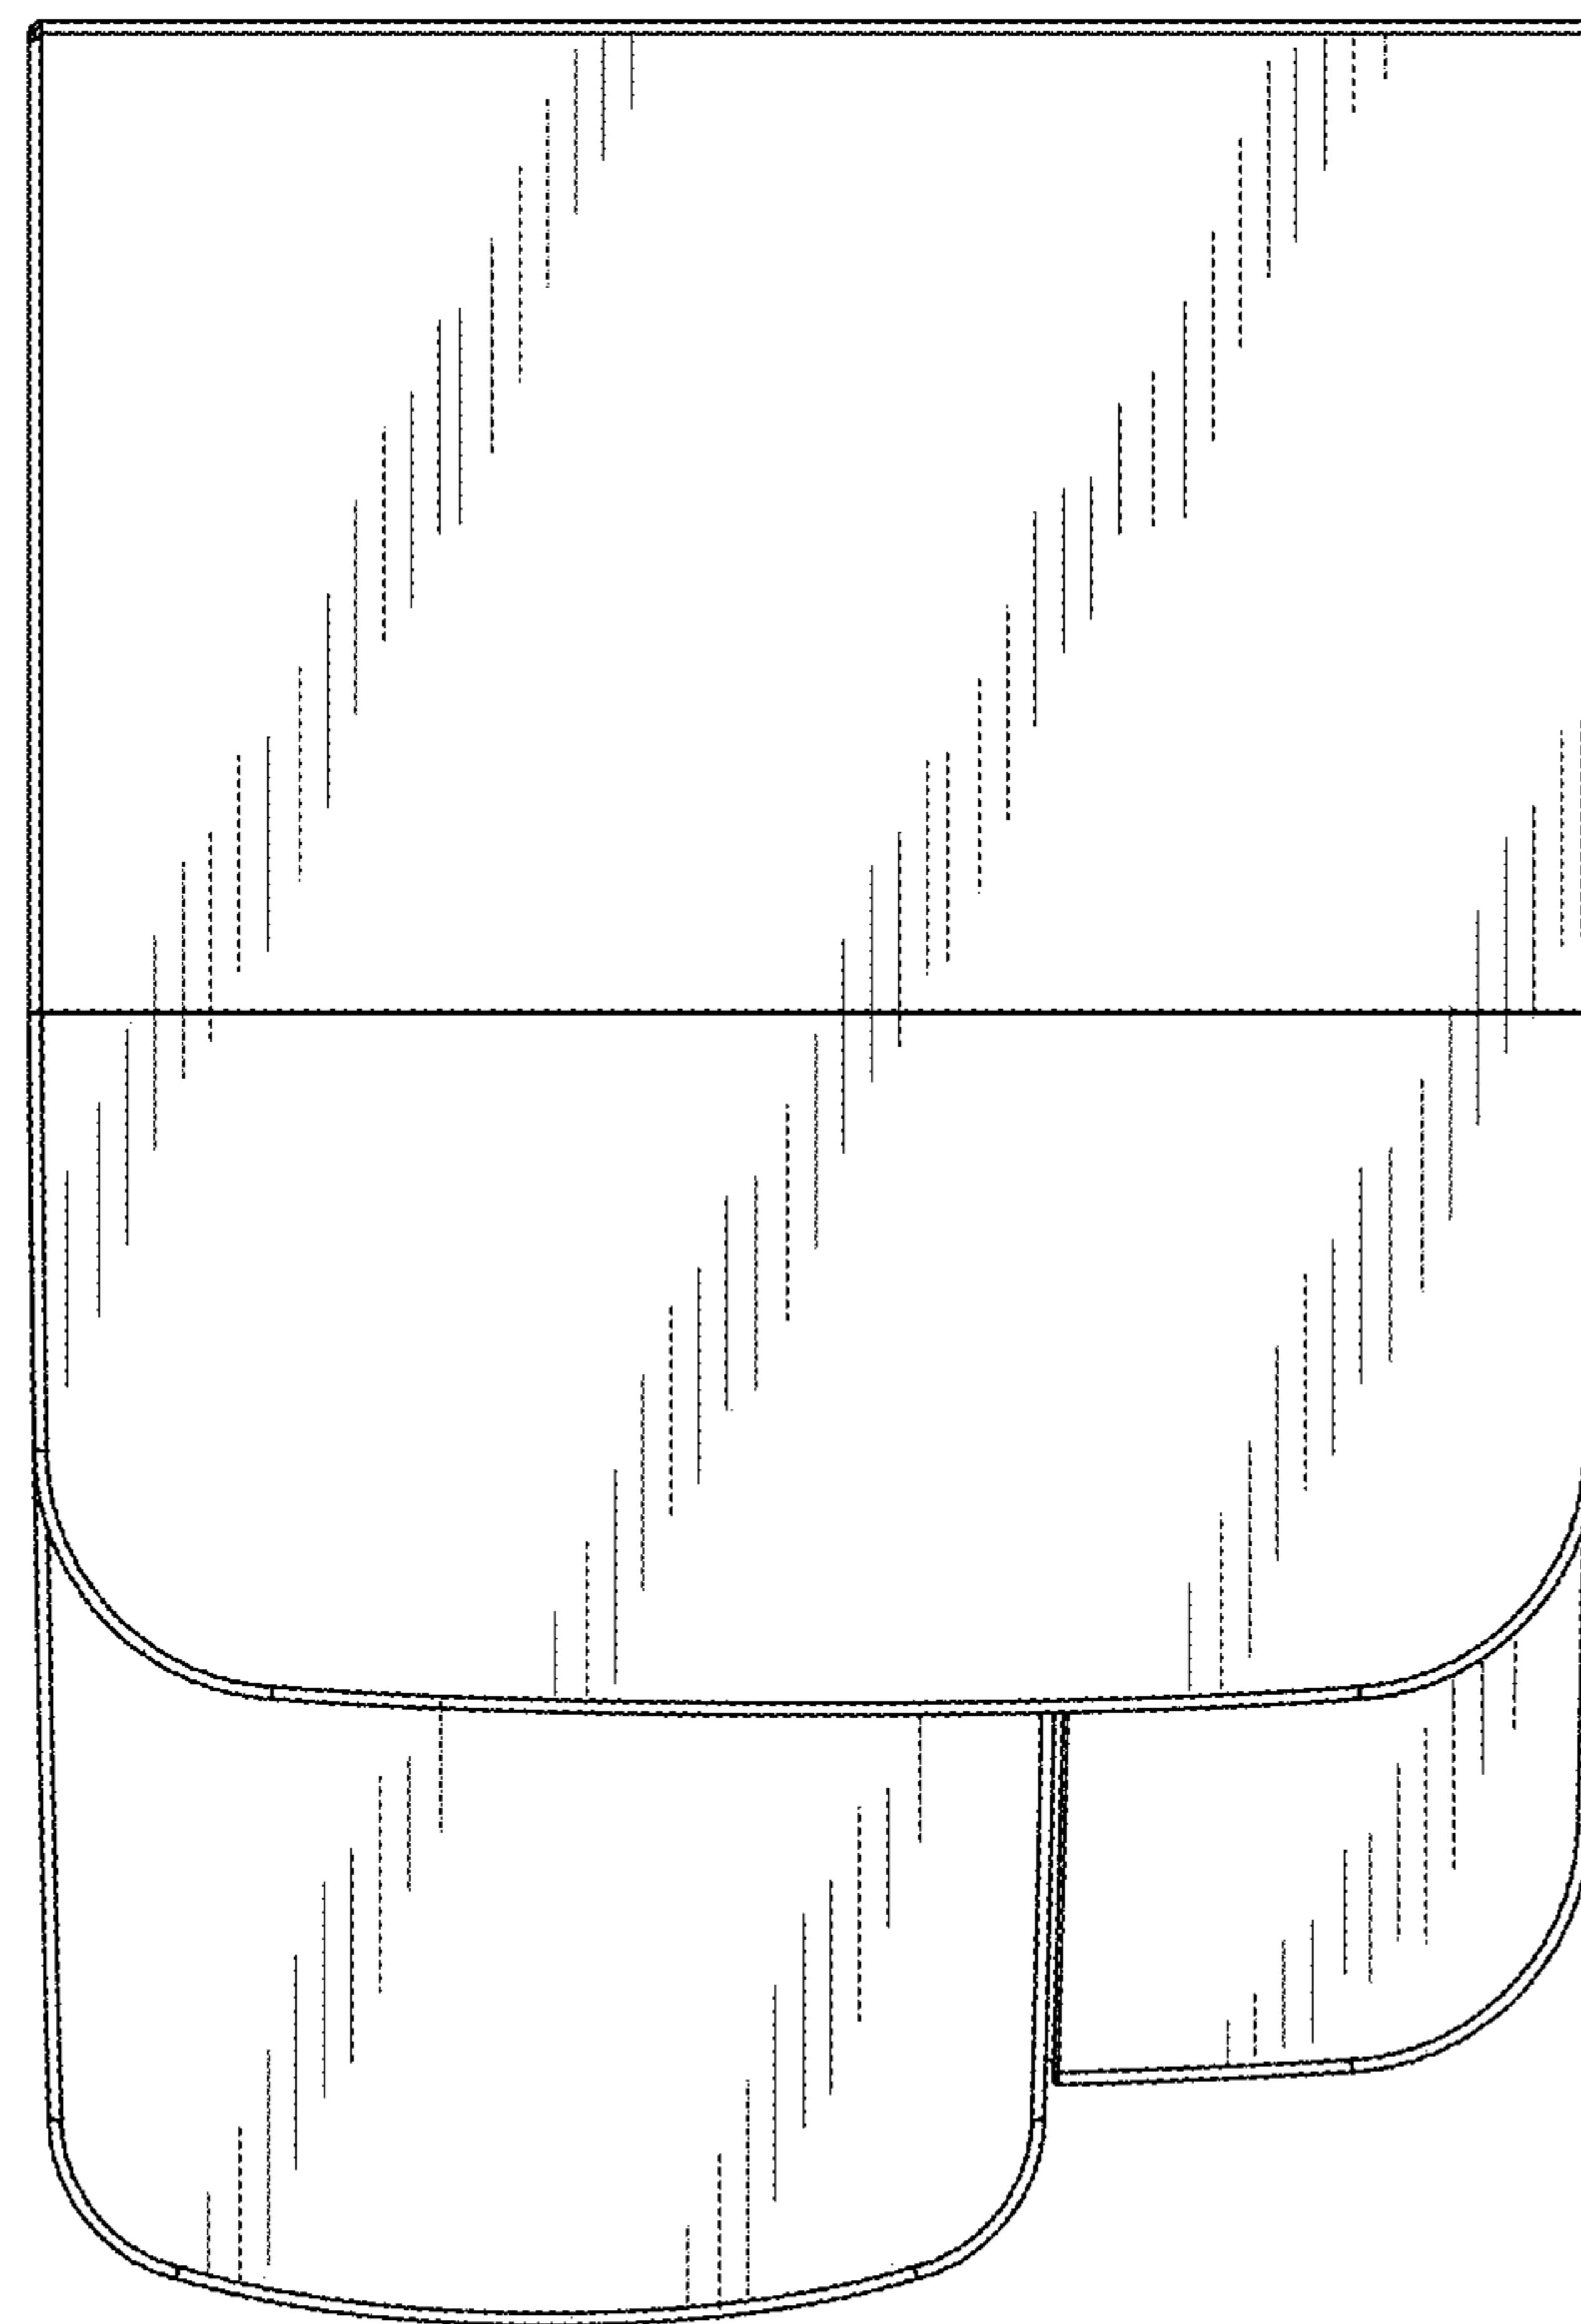

**FIG. 10**