



US00D690808S

(12) **United States Design Patent**
Laxmanan

(10) **Patent No.:** **US D690,808 S**

(45) **Date of Patent:** **** Oct. 1, 2013**

(54) **CRYOSURGICAL PROBE**

(75) Inventor: **Janarthanan Laxmanan**, Tamil Nadu (IN)

(73) Assignee: **Endocare, Inc.**, Austin, TX (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/424,626**

(22) Filed: **Jun. 13, 2012**

(51) **LOC (9) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/133**

(58) **Field of Classification Search**
USPC D24/133, 137, 138, 143, 144, 145,
D24/146, 147, 148, 149; D8/51, 57, 107;
606/1, 20-31
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,951,152	A	4/1976	Crandell et al.	
4,207,897	A	6/1980	Lloyd et al.	
D344,903	S	3/1994	Gampp et al.	
5,674,218	A	10/1997	Rubinsky et al.	
D406,337	S *	3/1999	Baust et al.	D24/133
D414,865	S	10/1999	Baust et al.	
6,475,212	B2	11/2002	Dobak et al.	
D497,206	S	10/2004	Damasco et al.	
D538,936	S *	3/2007	Bohmel et al.	D24/152
D623,739	S *	9/2010	Vernooij et al.	D24/133
2002/0165549	A1 *	11/2002	Owusu-Akyaw et al.	606/80
2006/0264920	A1 *	11/2006	Duong	606/21
2008/0306475	A1 *	12/2008	Lentz et al.	606/23

FOREIGN PATENT DOCUMENTS

DE 40305915-0001 * 1/2004

* cited by examiner

Primary Examiner — Bridget L Eland

(74) *Attorney, Agent, or Firm* — Lawrence N. Ginsberg


(57) **CLAIM**

The ornamental design for a cryosurgical probe, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a cryosurgical probe, showing my new design;
 FIG. 2 is a side view thereof;
 FIG. 3 is a top view thereof shown removed from its environment in order to show aspects of the design that are not otherwise apparent;
 FIG. 4 is a bottom view thereof shown removed from its environment in order to show aspects of the design that are not otherwise apparent;
 FIG. 5 is a front view thereof shown removed from its environment in order to show aspects of the design that are not otherwise apparent; and,
 FIG. 6 is a rear view thereof shown removed from its environment in order to show aspects of the design that are not otherwise apparent.
 Portions of the cryosurgical probe shown in broken lines are directed to environment; the broken lines form no part of the claimed design.

1 Claim, 4 Drawing Sheets

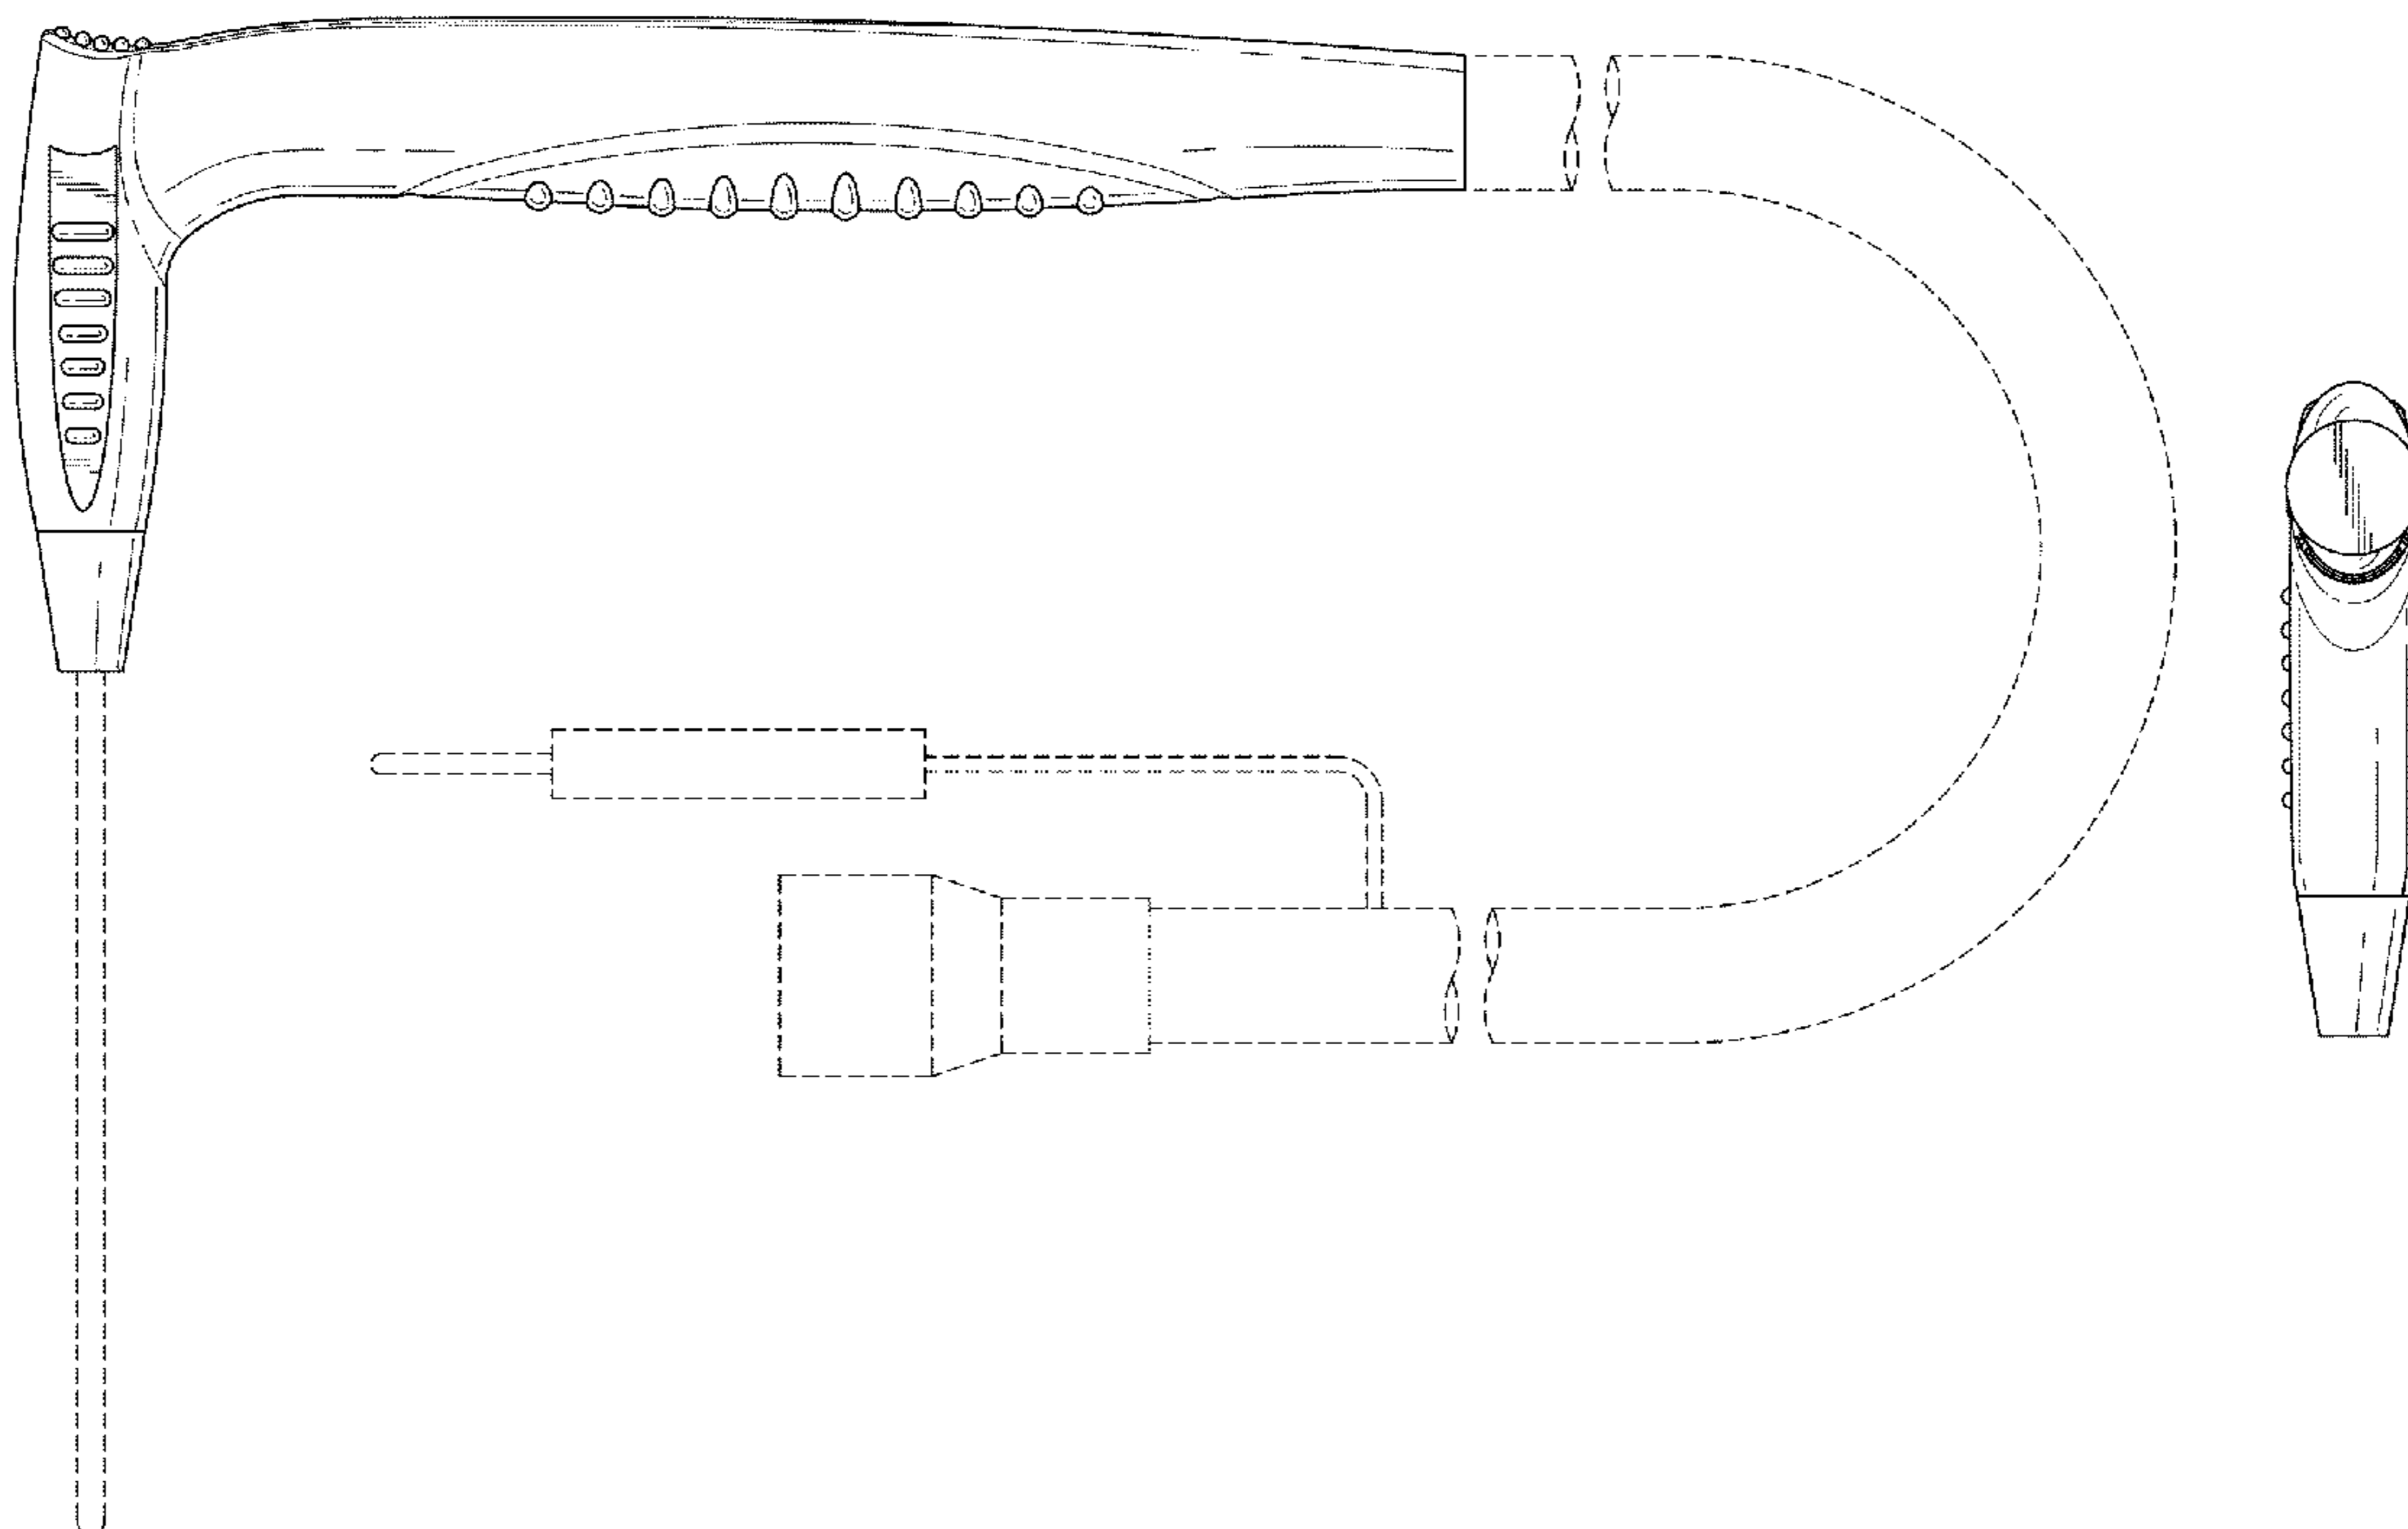

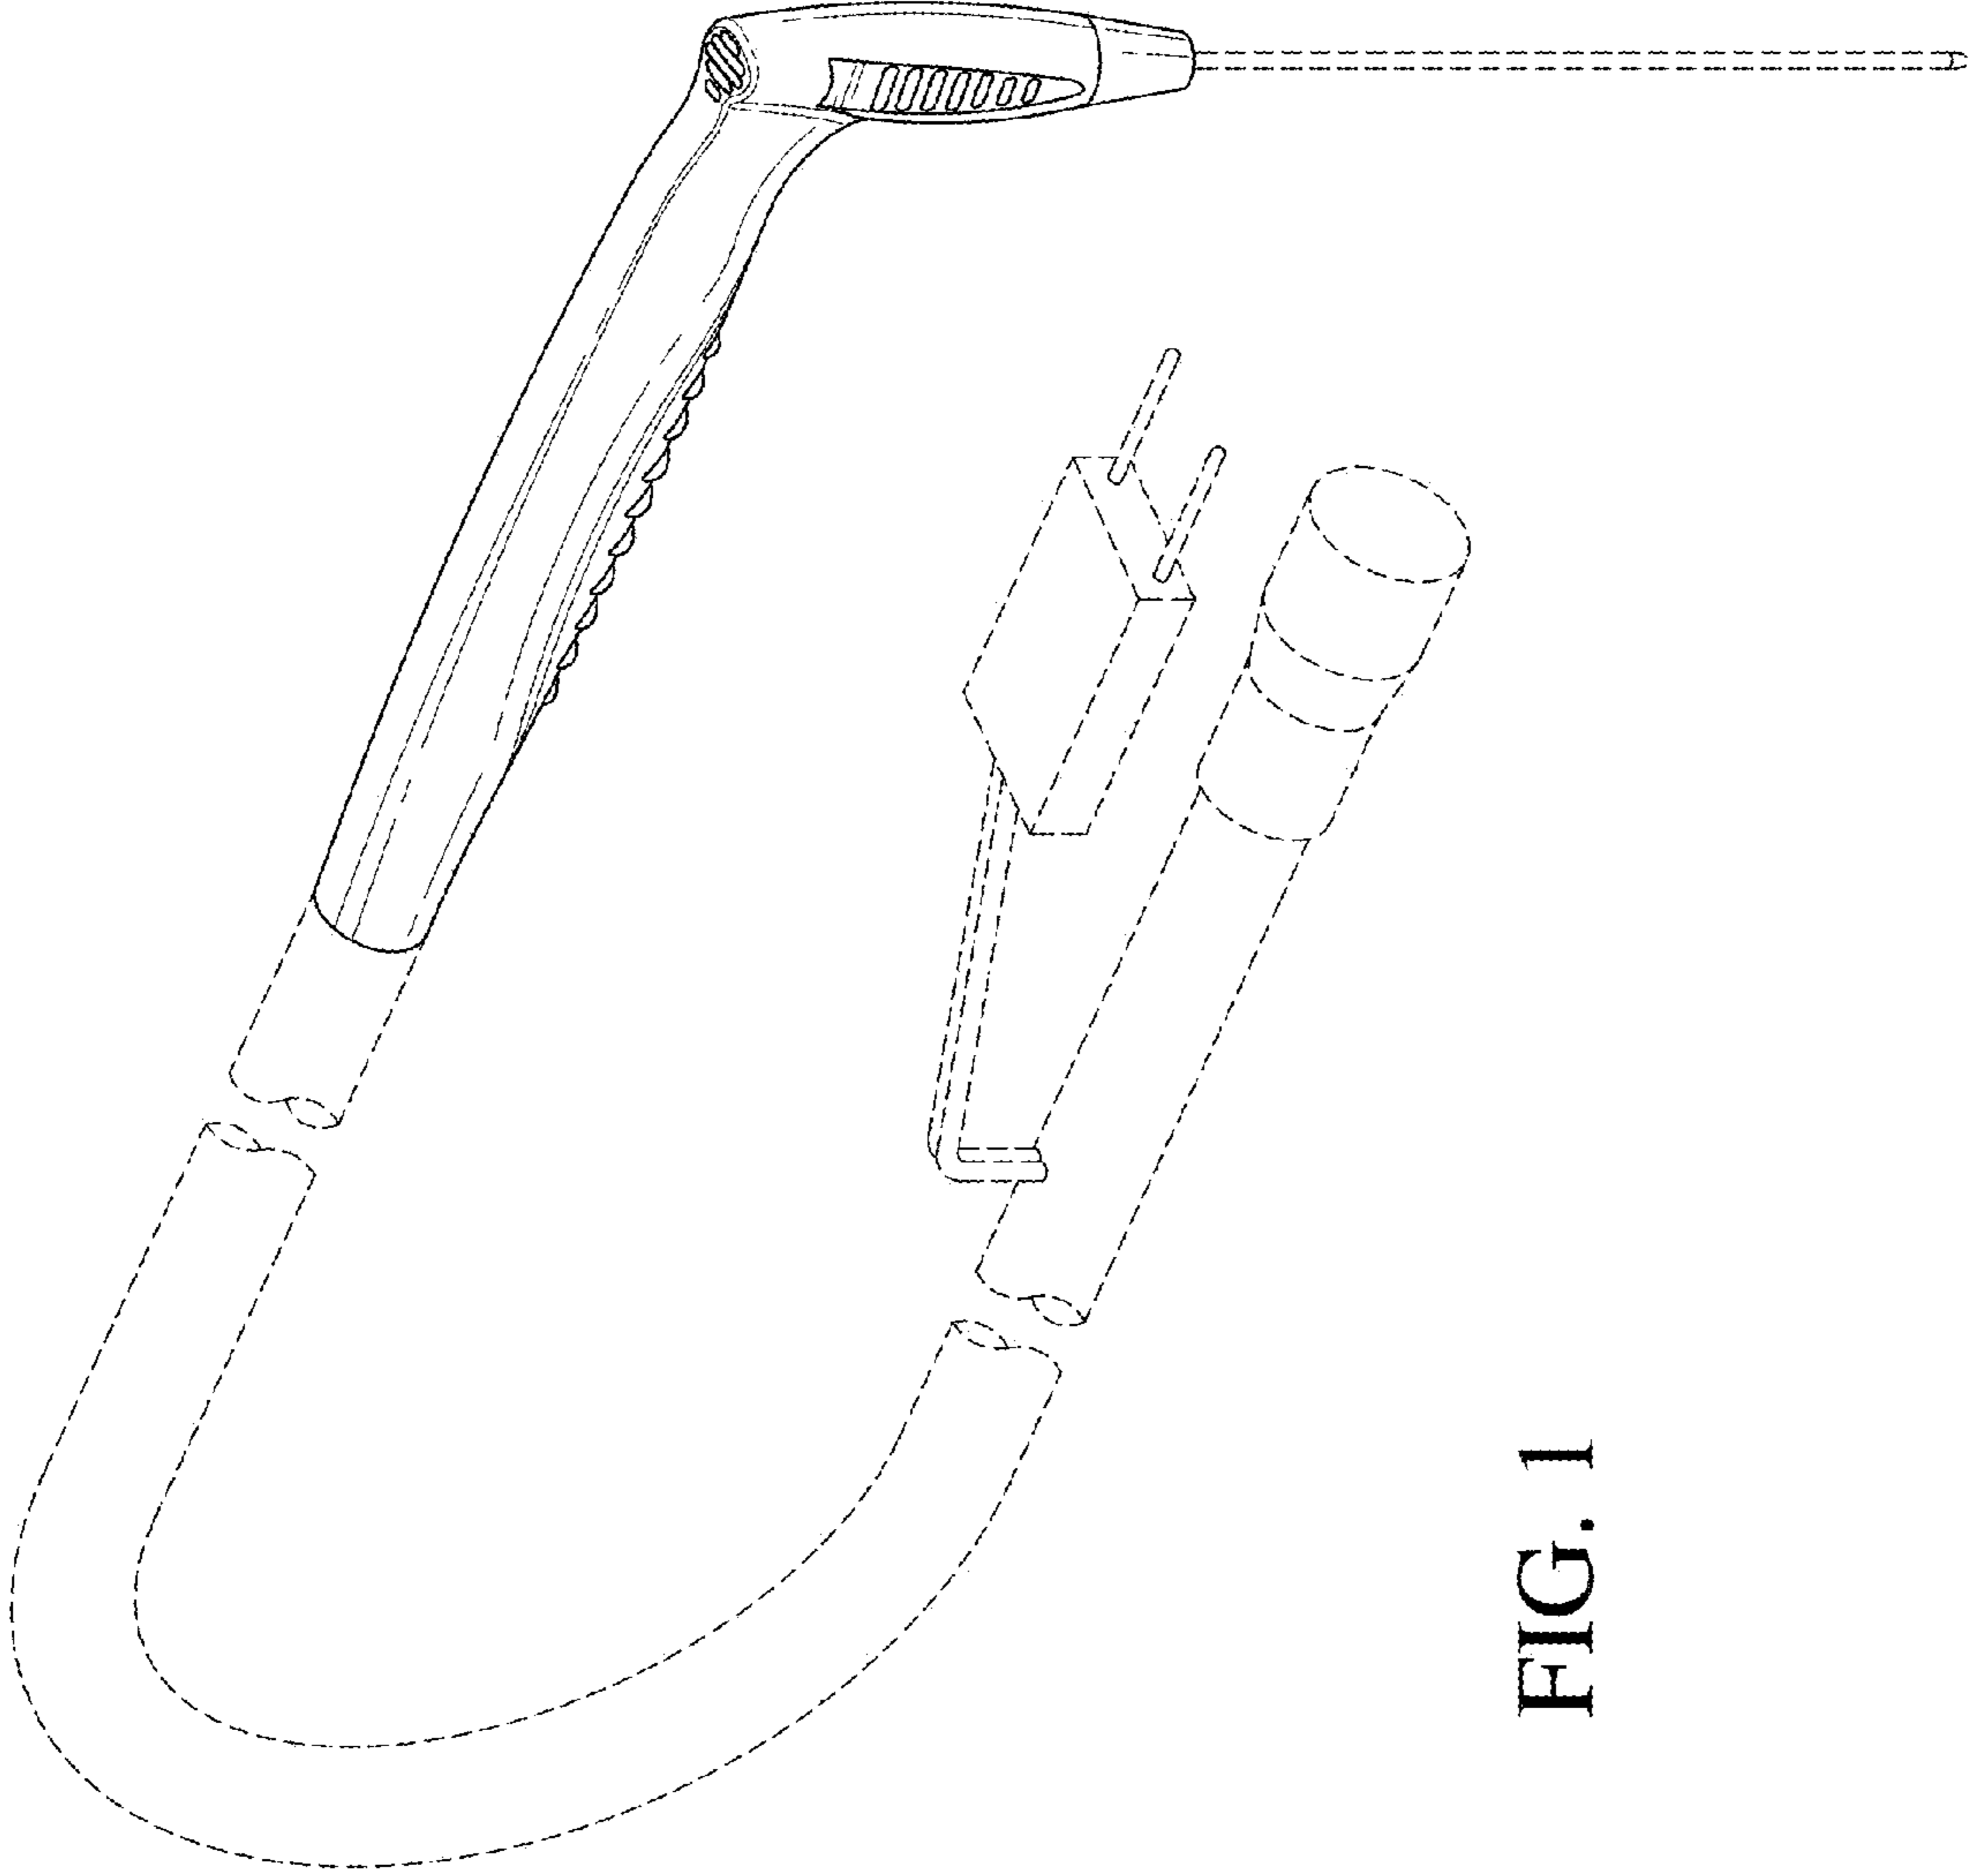


FIG. 1

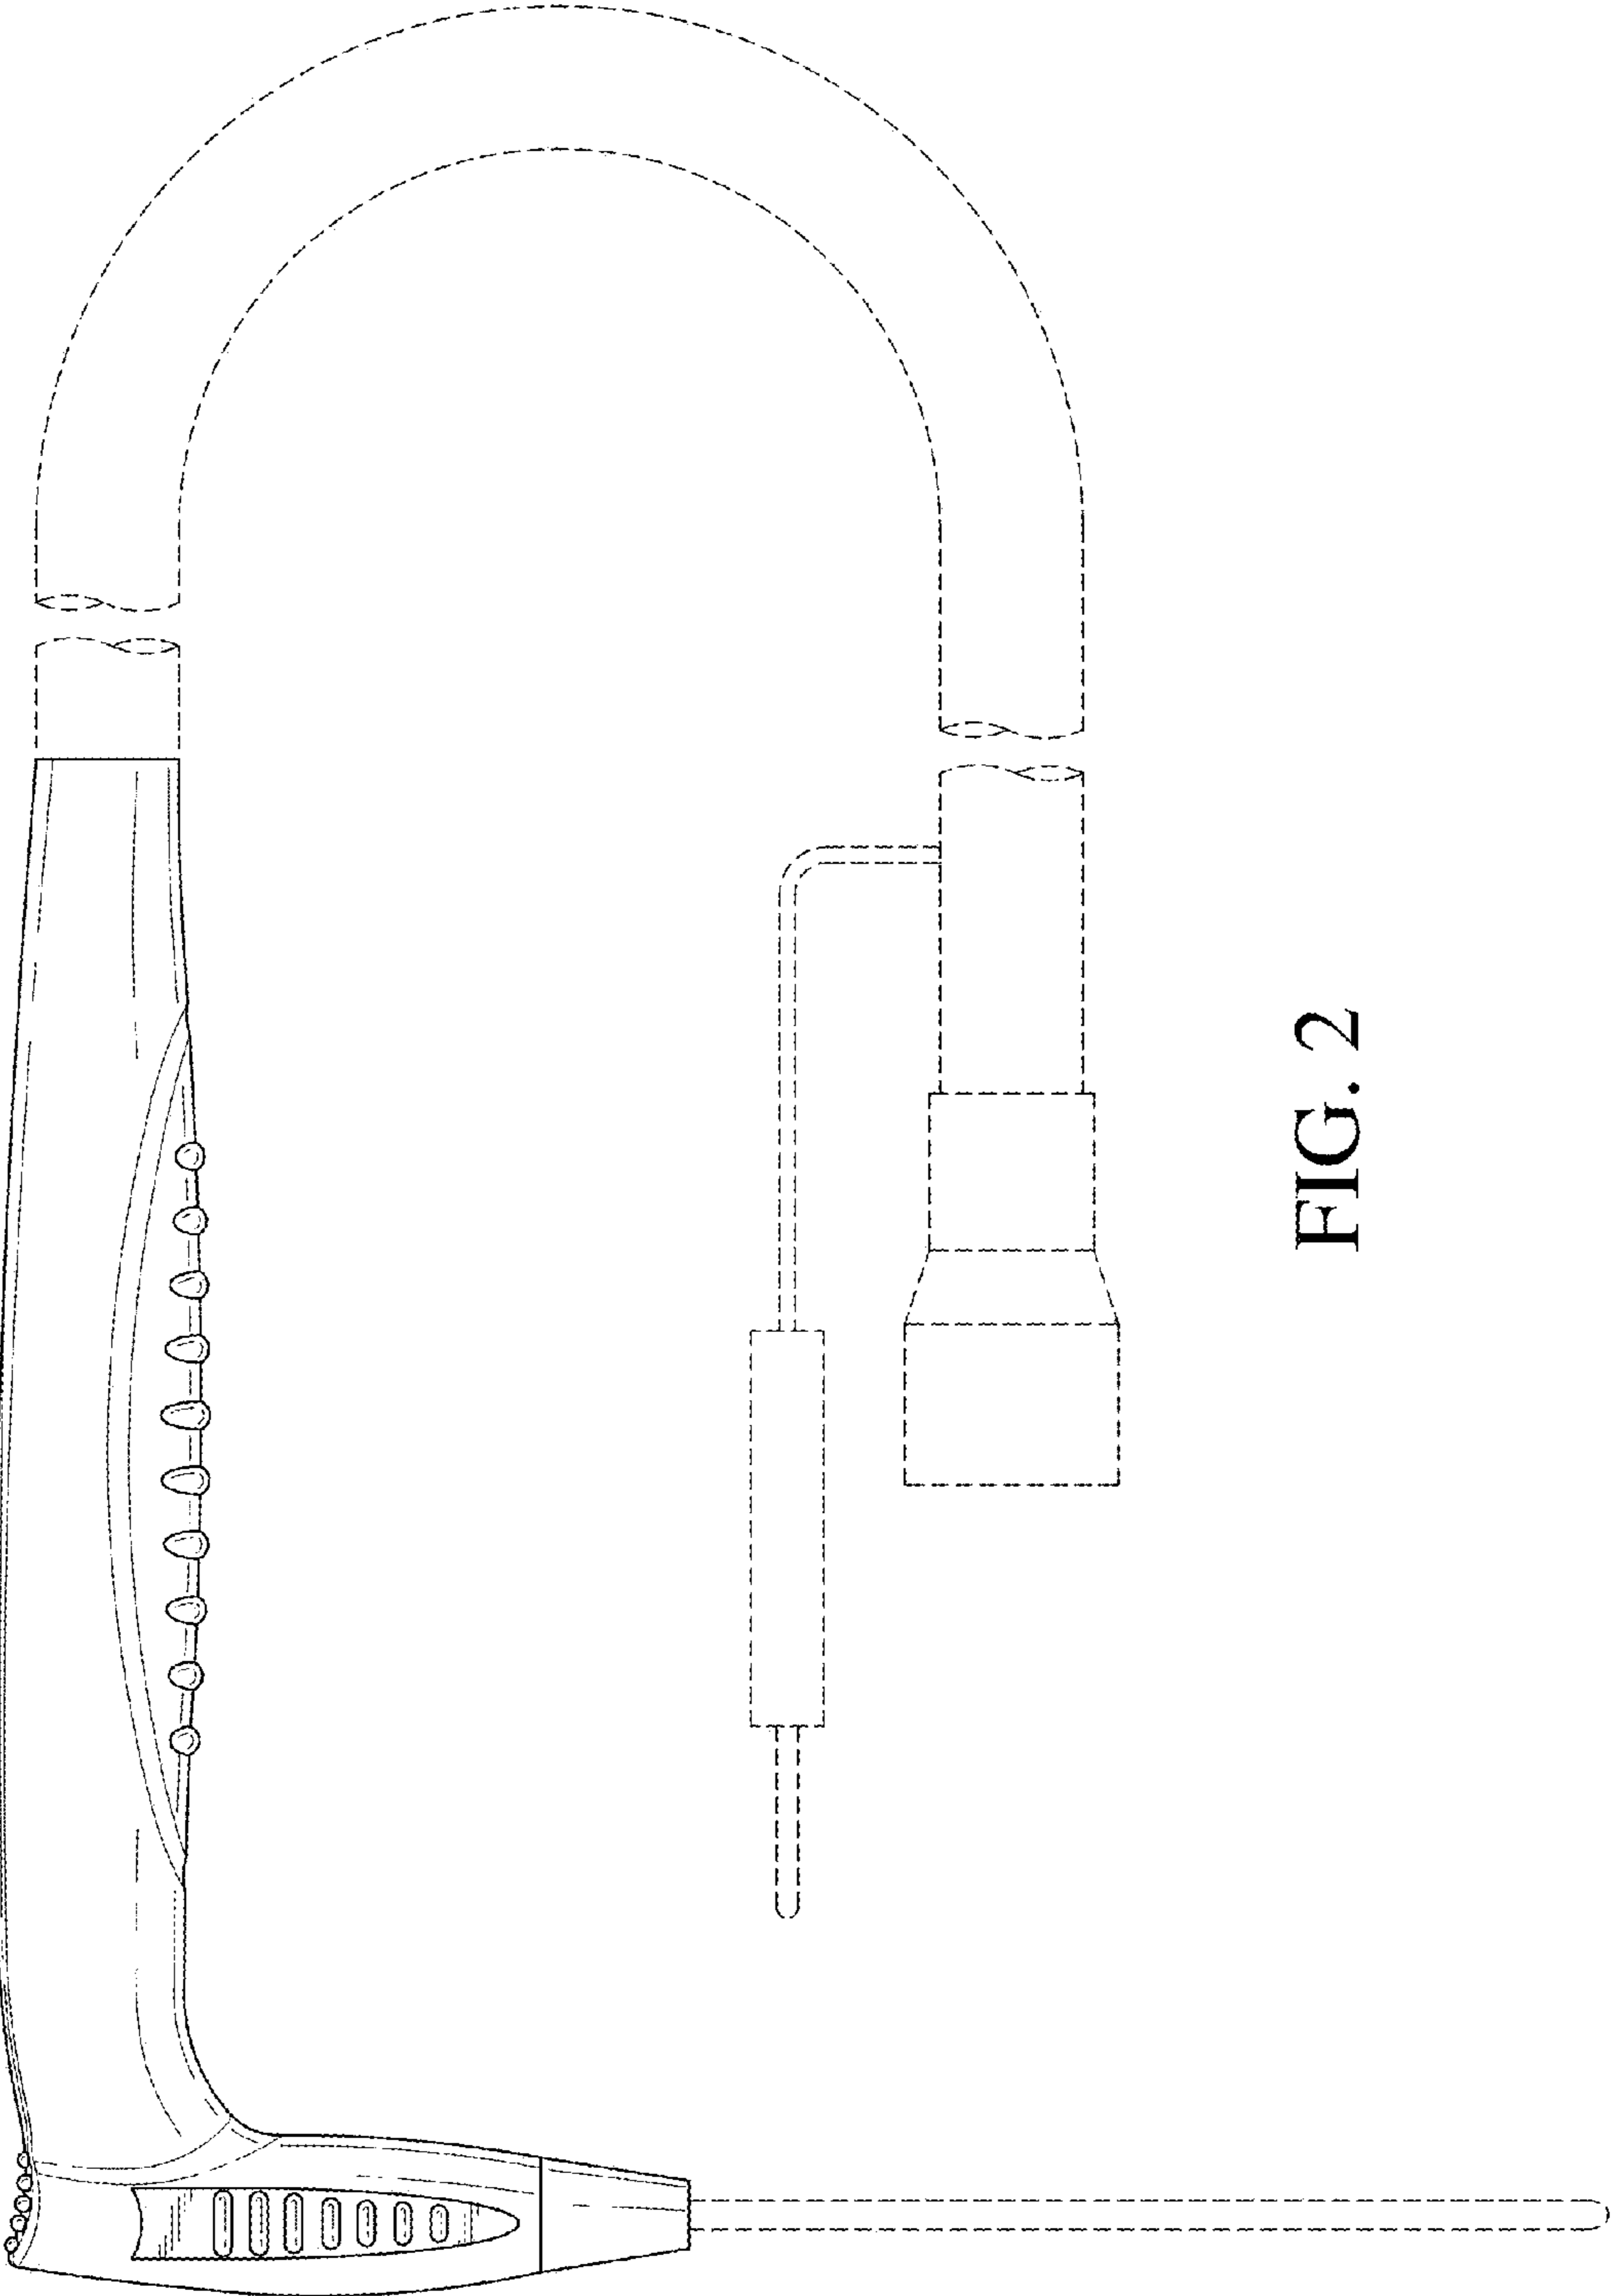


FIG. 2

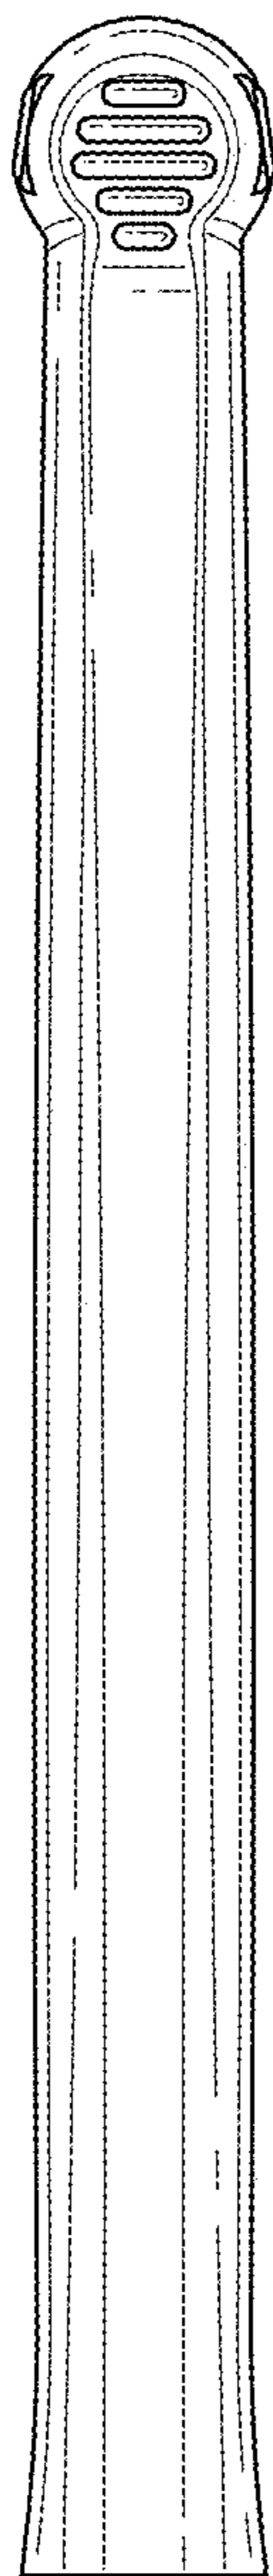


FIG. 3

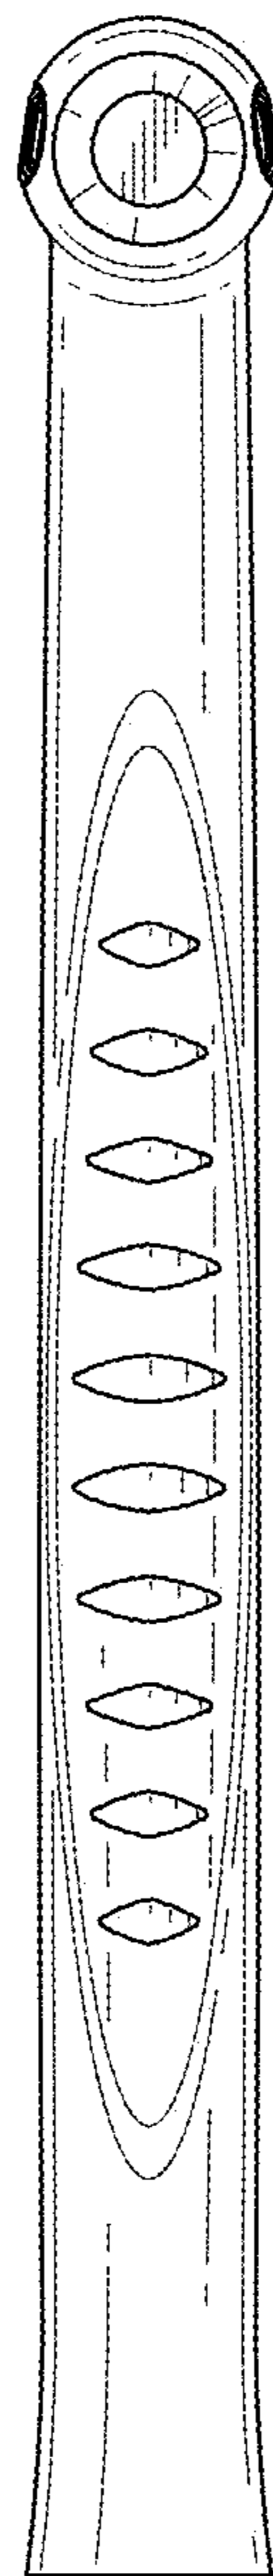


FIG. 4

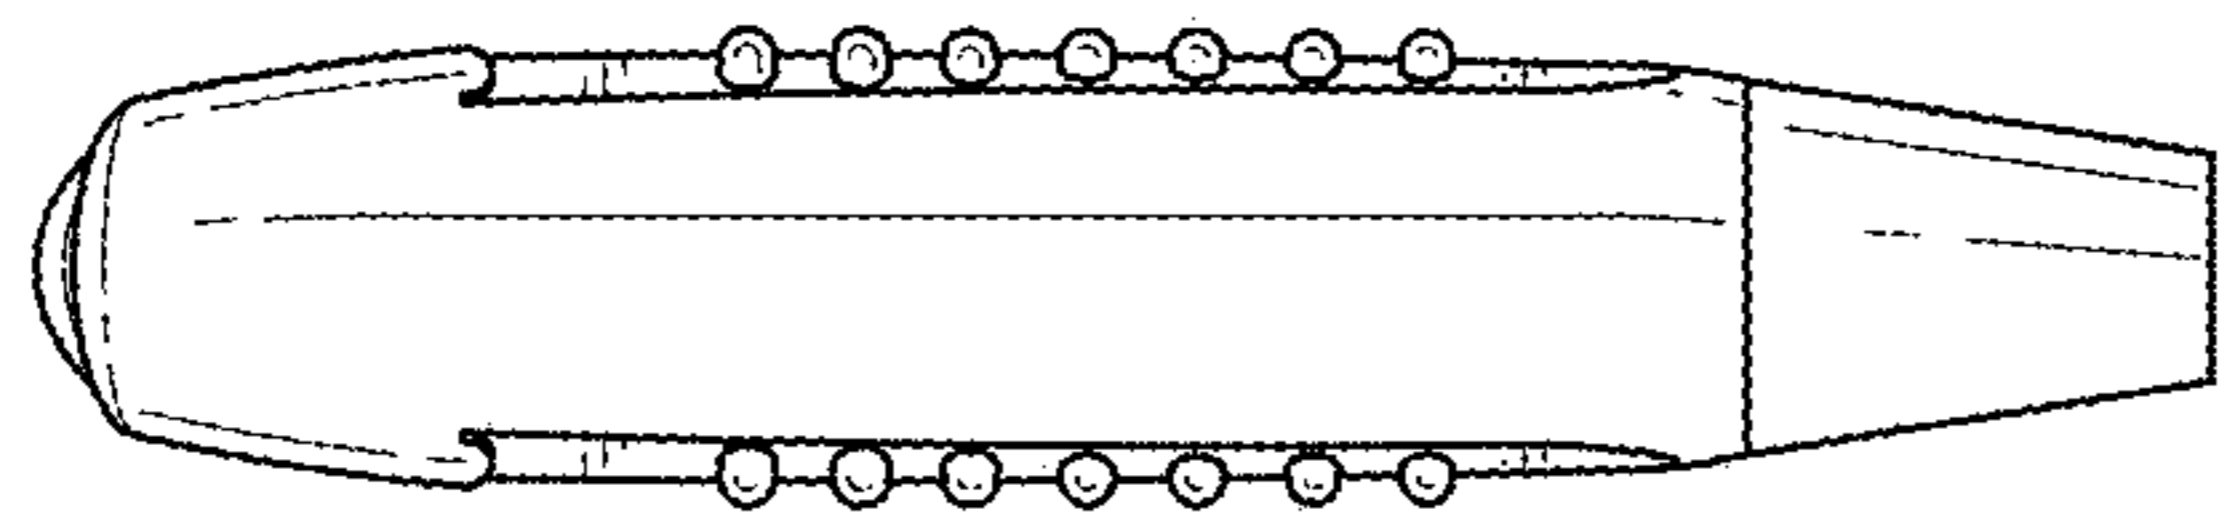


FIG. 6

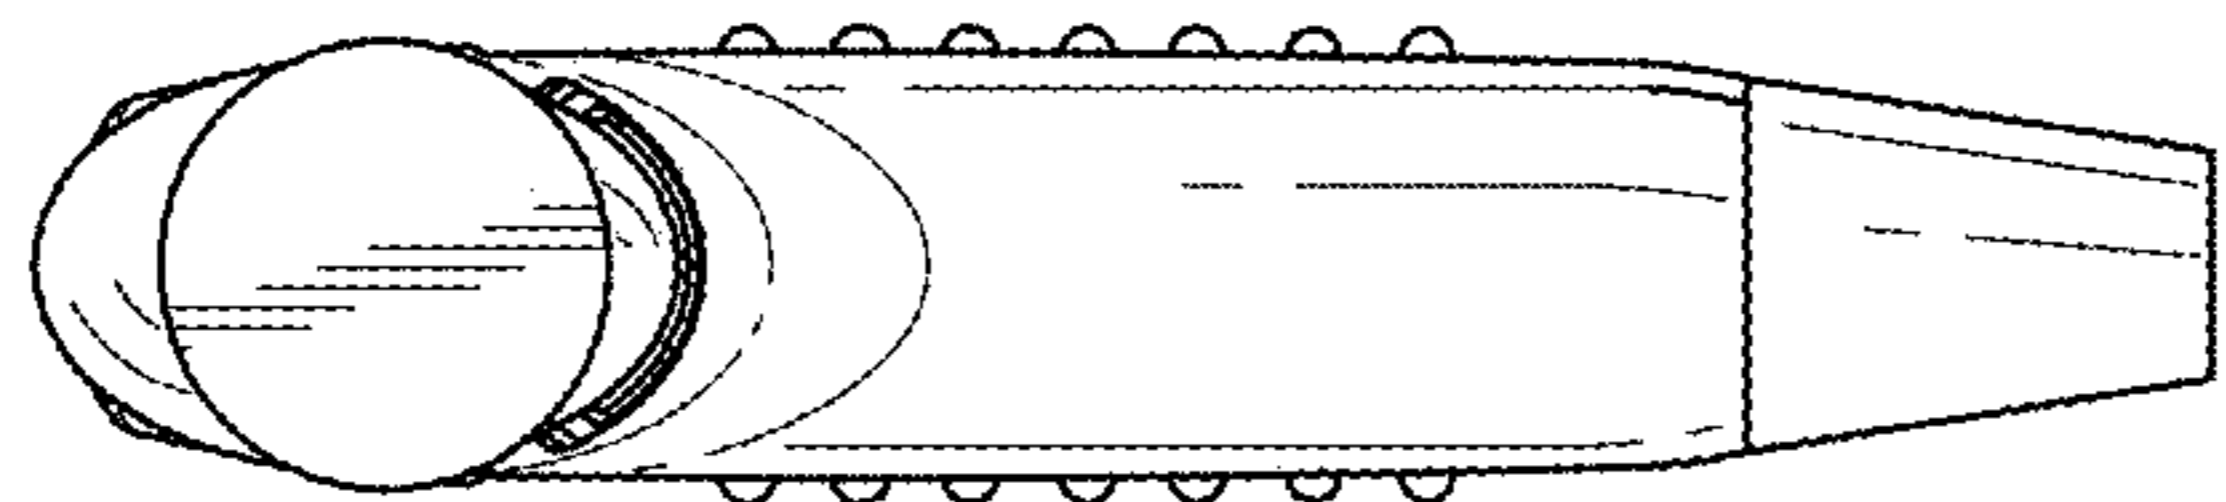


FIG. 5